

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
 Data File : VU063435.D
 Acq On : 24 Jun 2025 13:22
 Operator : MD/SY
 Sample : Q2377-03
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB01-061925

Quant Time: Jun 24 14:14:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jun 24 05:06:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.107	96	40746	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	13337	0.892	ug/l	0.00
Spiked Amount 1.000			Recovery	=	89.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	13889	0.924	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063435.D
Acq On : 24 Jun 2025 13:22
Operator : MD/SY
Sample : Q2377-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB01-061925

Quant Time: Jun 24 14:14:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jun 24 05:06:50 2025
Response via : Initial Calibration




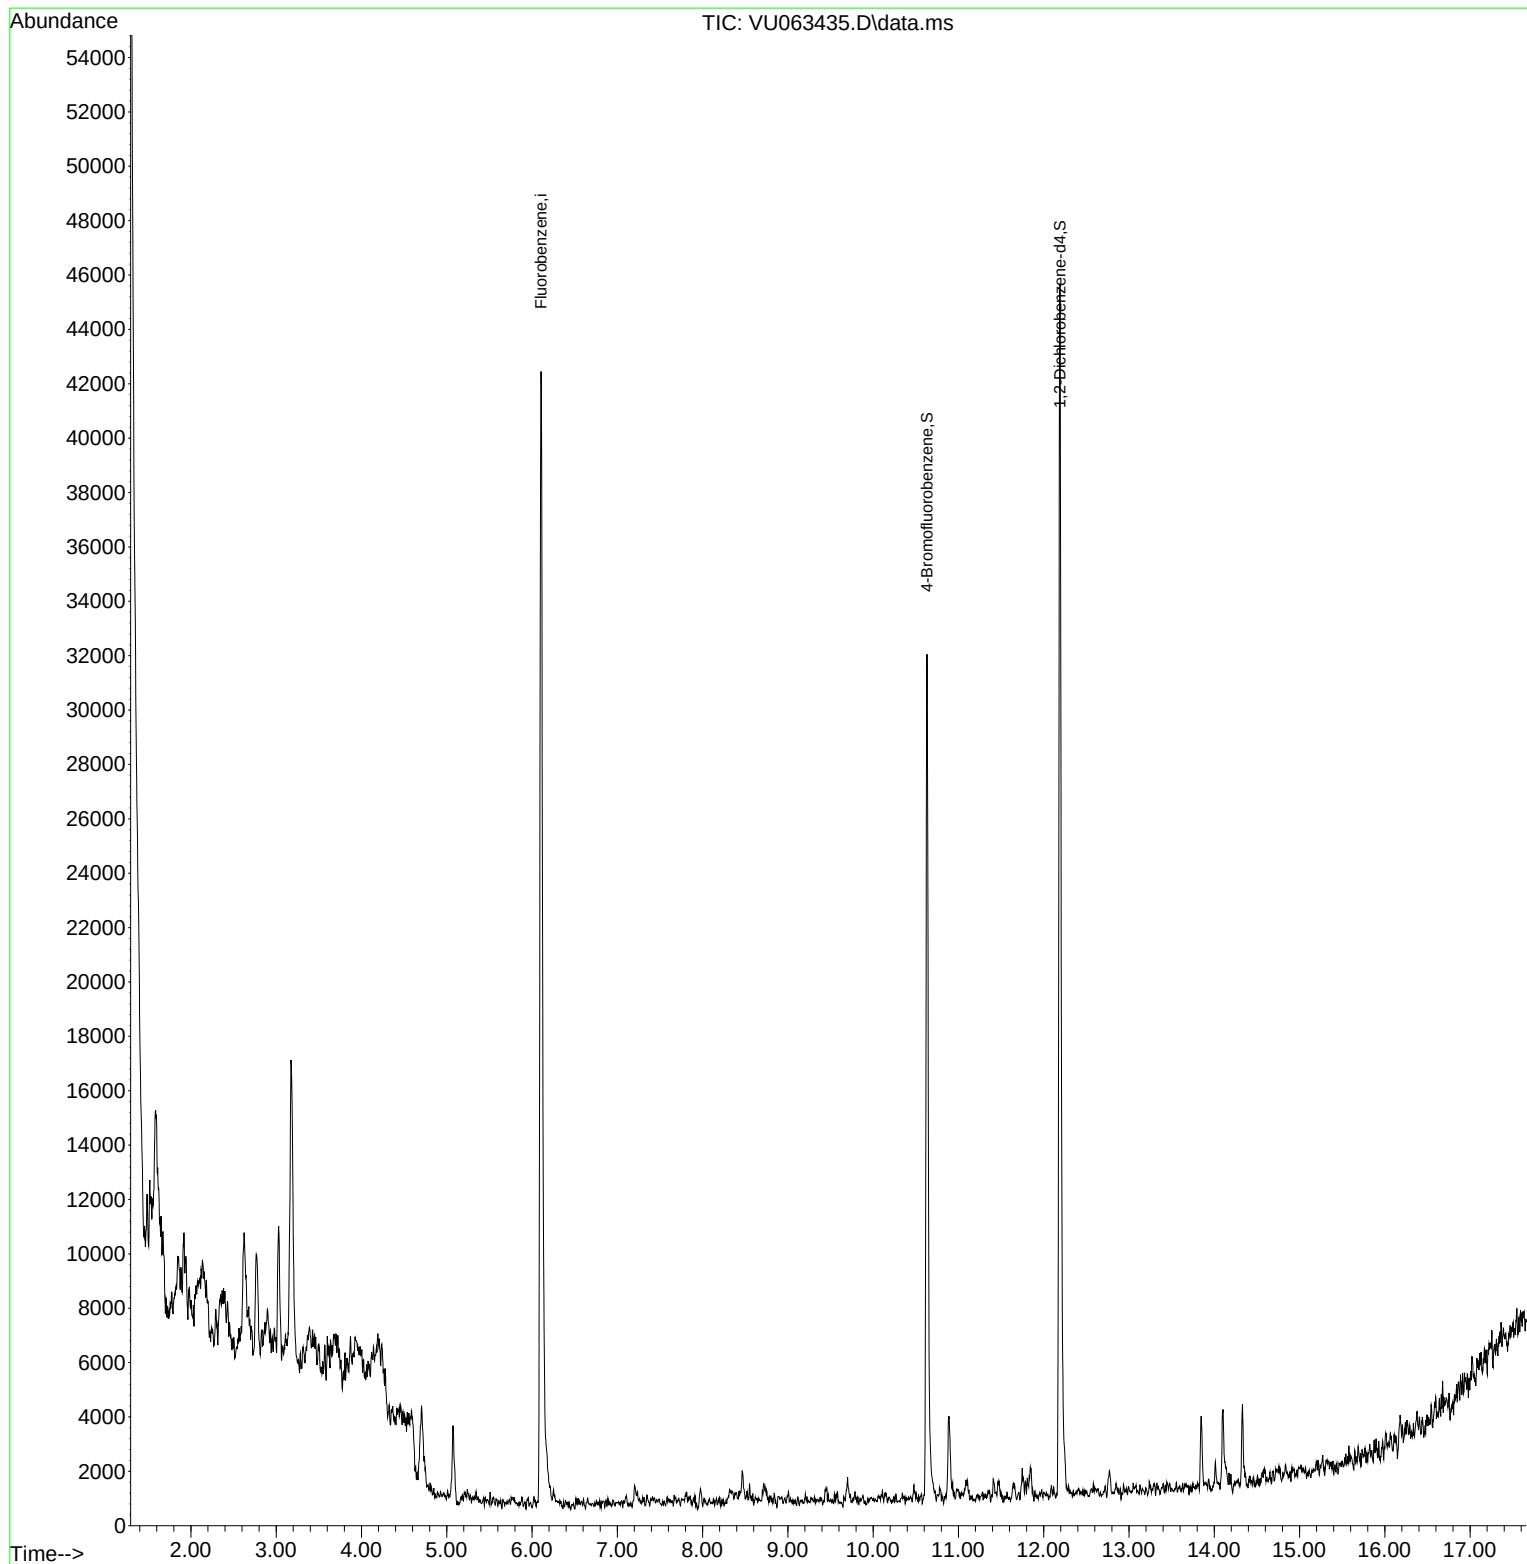


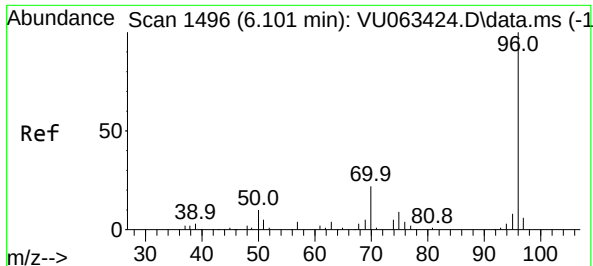

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1496
Delta R.T. 0.006 min
Lab File: VU063435.D
Acq: 24 Jun 2025 13:22




Instrument :
MSVOA_U
ClientSampleId :
TB01-061925


Tgt Ion: 96	Resp: 40746
Ion Ratio	Lower Upper
96	100
70	22.9 16.4 24.6
95	9.6 6.2 9.2#
97	7.1 0.0 0.0#

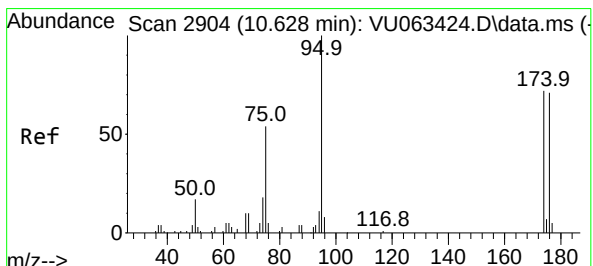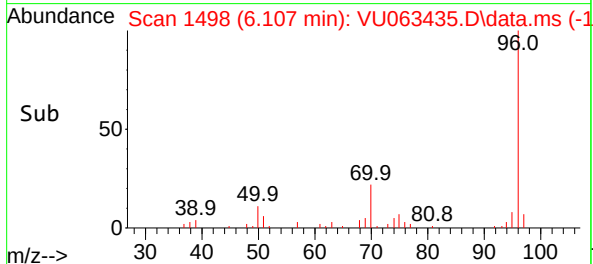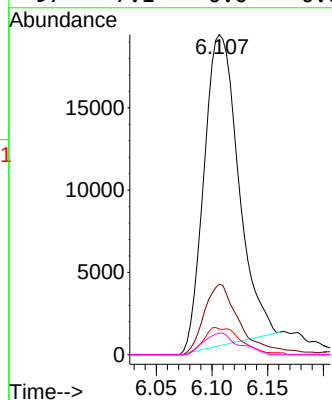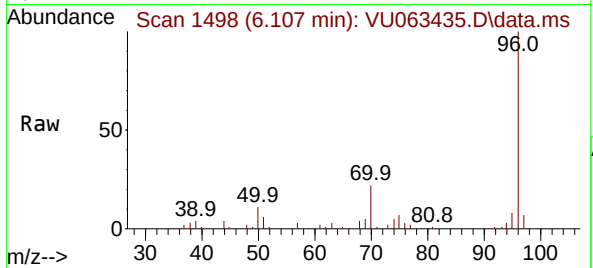

#57
4-Bromofluorobenzene
Concen: 0.892 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.002 min
Lab File: VU063435.D
Acq: 24 Jun 2025 13:22


Tgt Ion: 95	Resp: 13337
Ion Ratio	Lower Upper
95	100
174	73.1 59.4 89.2
176	74.7 57.8 86.6

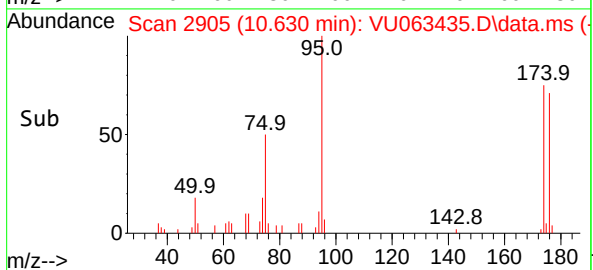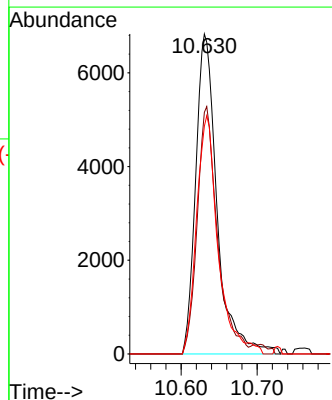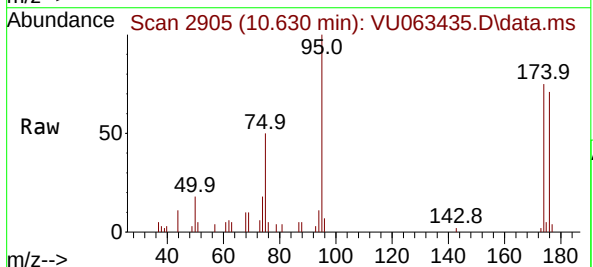

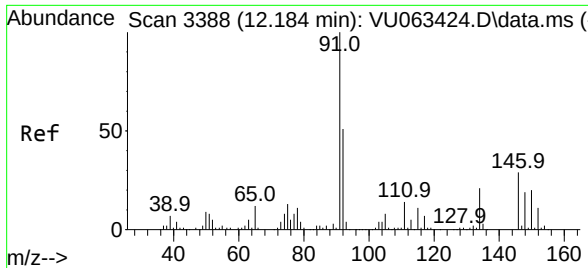

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.924 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VU063435.D
 Acq: 24 Jun 2025 13:22

Instrument :
 MSVOA_U
 ClientSampleId :
 TB01-061925

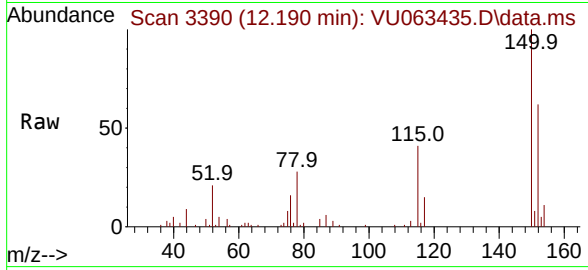

Tgt Ion:	152	Resp:	13889
Ion	Ratio	Lower	Upper
152	100		
115	62.6	0.0	327.6
150	159.6	0.0	664.4

