


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062025\
Data File : VX046783.D
Acq On : 20 Jun 2025 14:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Title : SW846 8260
Last Update : Wed Jun 18 03:09:16 2025

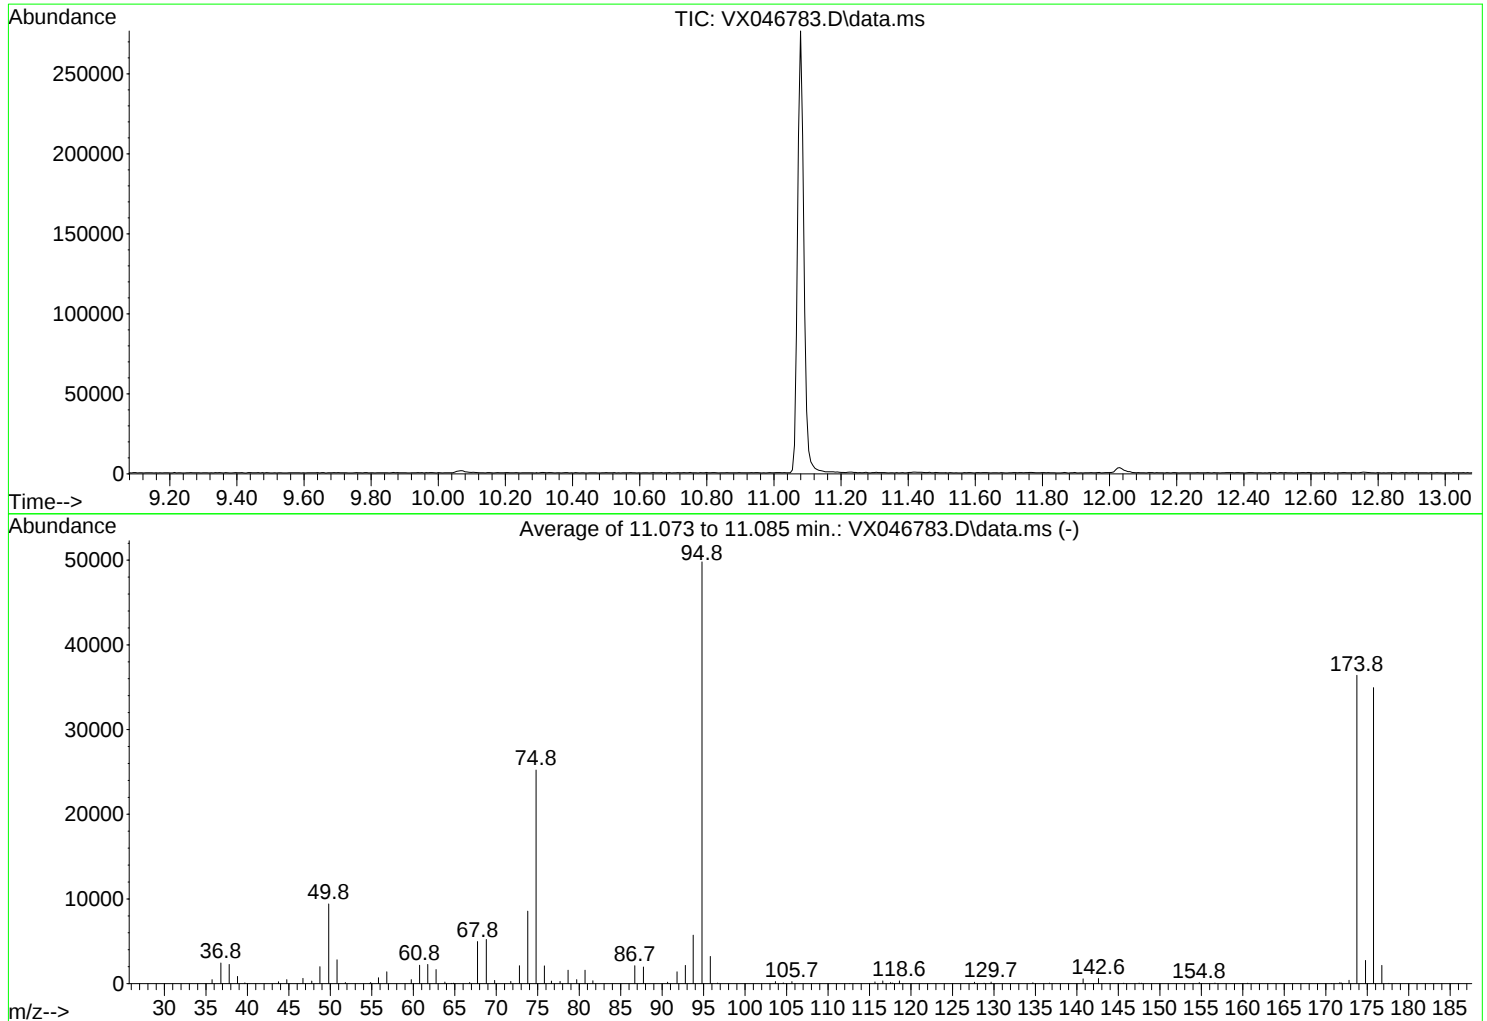

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	9401	PASS
75	95	30	60	50.7	25227	PASS
95	95	100	100	100.0	49805	PASS
96	95	5	9	6.5	3214	PASS
173	174	0.00	2	1.1	406	PASS
174	95	50	100	73.1	36405	PASS
175	174	5	9	7.5	2744	PASS
176	174	95	101	96.0	34952	PASS
177	176	5	9	6.2	2154	PASS