


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062325\
Data File : VL042662.D
Acq On : 23 Jun 2025 07:57
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 30 02:01:56 2025

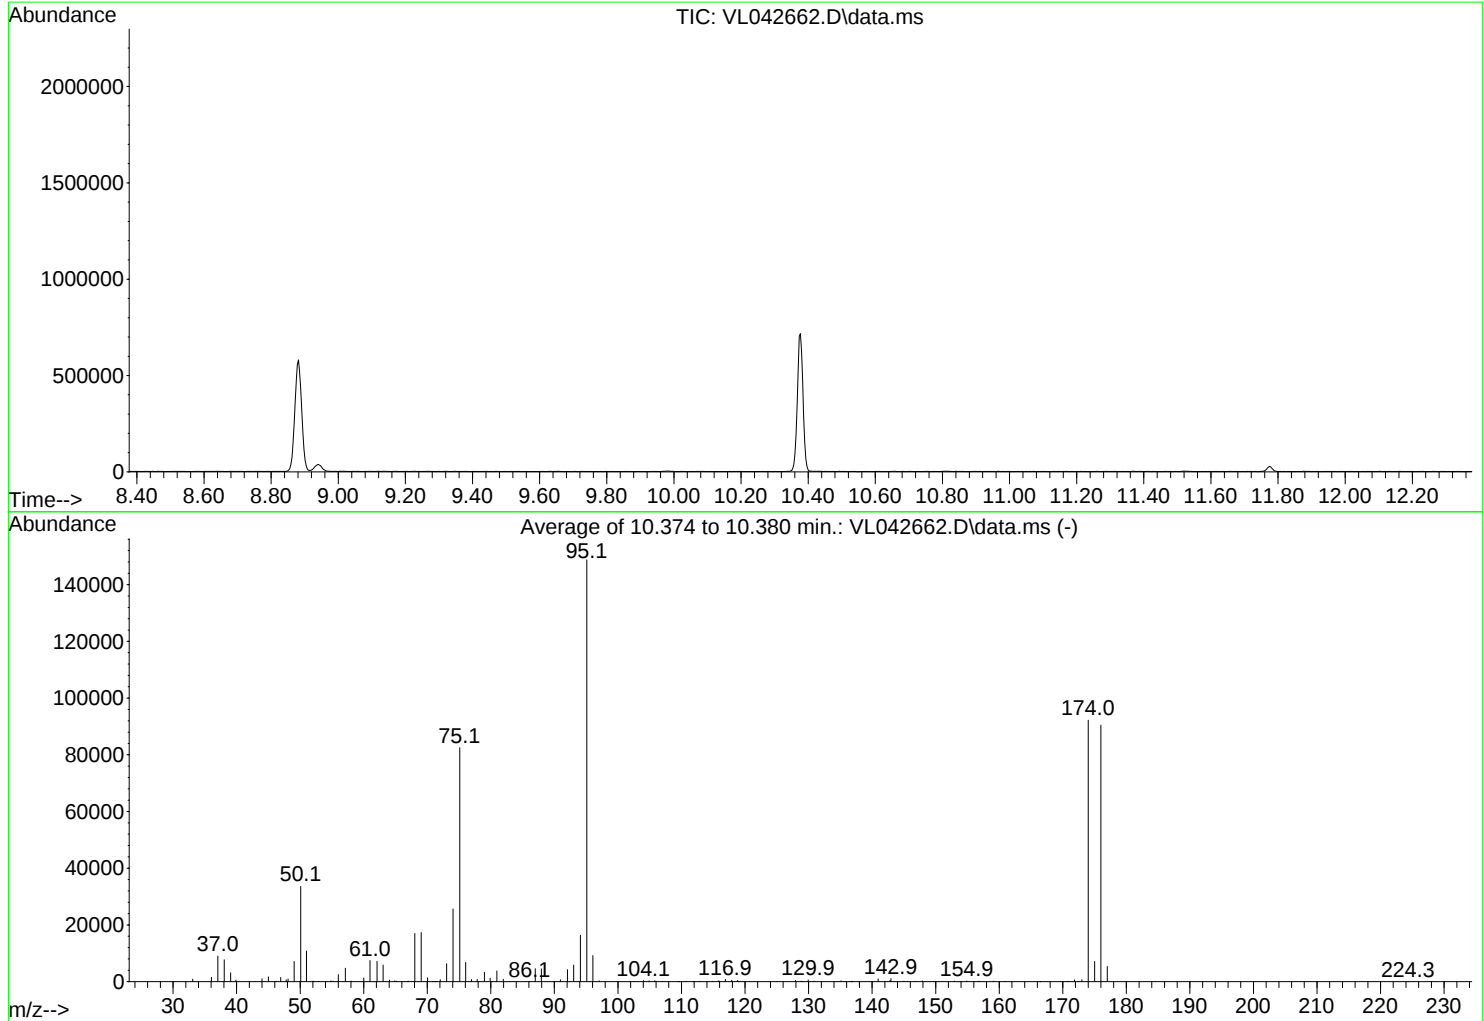

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.6	33587	PASS
75	95	30	66	55.5	82515	PASS
95	95	100	100	100.0	148757	PASS
96	95	5	9	6.2	9198	PASS
173	174	0.00	2	0.7	689	PASS
174	95	50	120	62.0	92200	PASS
175	174	4	9	7.7	7104	PASS
176	174	93	101	98.1	90432	PASS
177	176	5	9	6.0	5391	PASS

Average of 10.374 to 10.380 min.: VL042662.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	917	47.80	655	56.00	2477	67.05	191
36.05	1543	48.10	939	57.10	4745	68.05	1697
37.05	9049	49.05	7096	58.05	237	69.05	1730
38.05	7728	50.10	33587	60.00	1284	70.05	133
39.05	3093	51.00	10778	61.00	7459	70.80	17
39.90	591	52.00	122	62.10	7153	71.20	18
43.00	62	52.10	178	63.05	5896	72.05	676
44.00	1020	52.90	73	64.05	572	73.05	6336
45.00	1679	54.15	59	64.90	294	74.05	25627
46.20	181	54.85	303	65.20	166	75.10	82515
46.95	1496	55.20	156	66.90	128	76.05	6781

Average of 10.374 to 10.380 min.: VL042662.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	720	92.05	4233	106.95	141	118.80	407
77.85	777	93.05	5884	107.80	47	119.00	156
79.00	3346	94.10	16344	109.50	17	123.90	102
79.90	1228	95.10	148757	110.85	77	125.05	64
80.95	3796	96.05	9198	111.90	18	127.95	401
81.95	843	97.05	281	112.85	108	128.85	182
82.95	41	102.55	65	114.85	138	129.10	47
86.10	94	104.05	416	115.80	273	129.95	608
87.00	4595	104.90	264	116.00	186	130.85	199
87.95	4497	105.80	372	116.90	786	134.60	52
90.95	699	106.00	151	117.90	516	135.10	286

Average of 10.374 to 10.380 min.: VL042662.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
135.75	47	145.00	150	156.80	176	175.00	7104
136.45	55	145.60	99	159.10	183	176.00	90432
136.70	31	146.00	124	160.90	126	177.00	5391
136.95	130	146.80	107	166.40	18	177.95	112
139.70	39	147.90	272	169.70	37	224.35	46
140.00	40	149.70	83	170.15	72		
140.95	943	150.00	45	170.70	53		
142.00	198	152.95	145	170.95	112		
142.80	429	153.80	20	171.85	651		
142.95	1069	154.90	228	173.00	689		
144.00	108	156.00	37	174.00	92200		