


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061925\  
Data File : BF142787.D  
Acq On : 19 Jun 2025 16:37  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061925.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Jun 20 05:06:14 2025

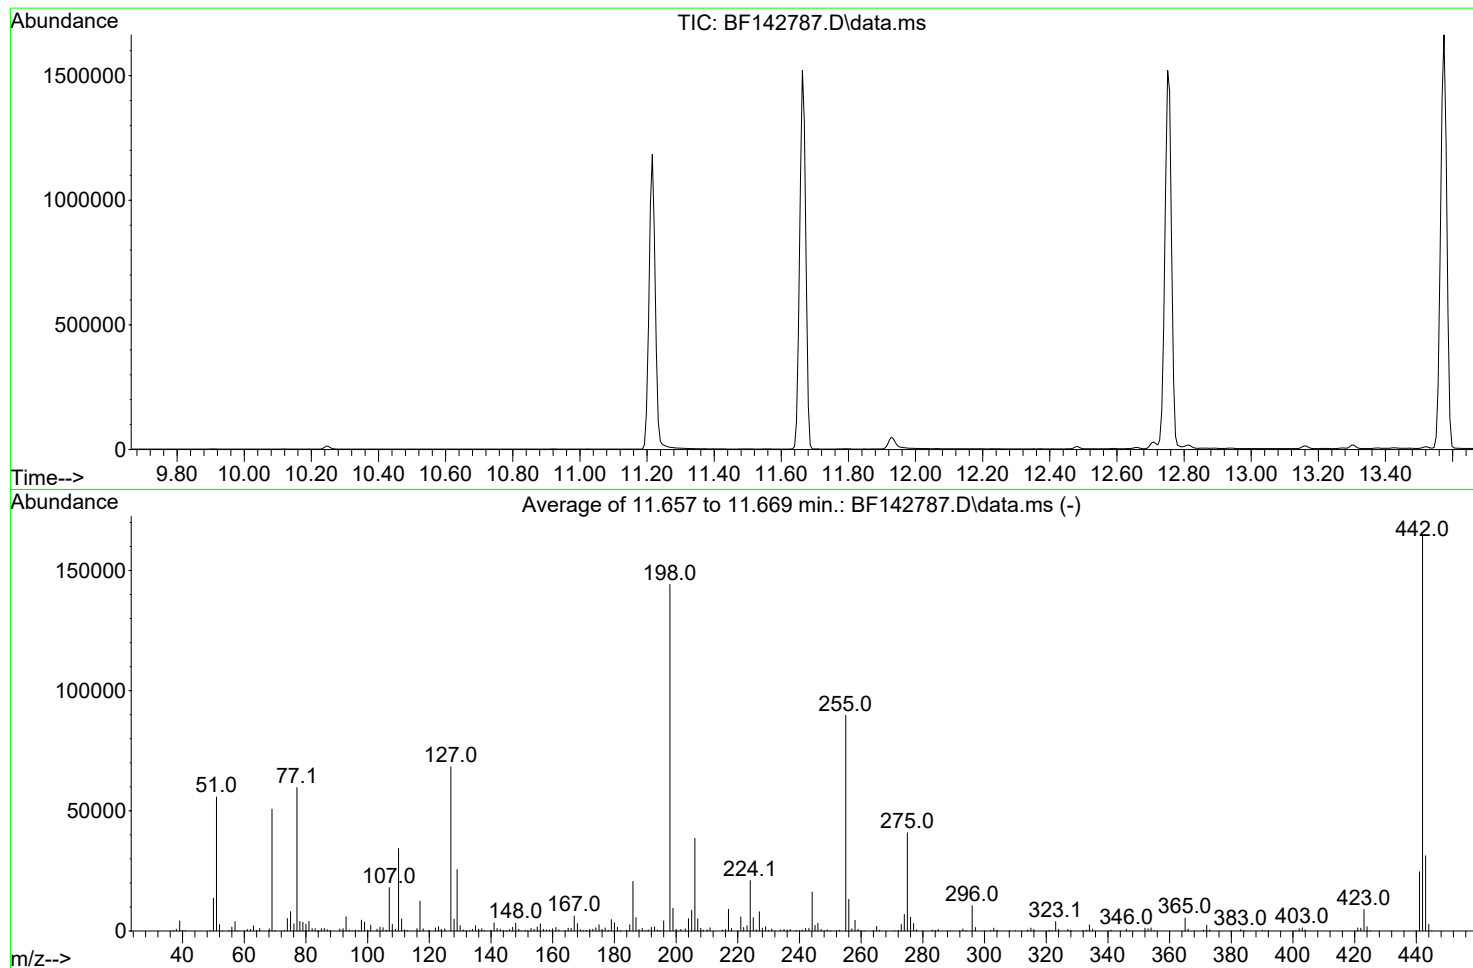

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.8   | 926    | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 50712  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 243    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 144192 | PASS      |
| 199    | 198     | 5      | 9      | 6.6   | 9464   | PASS      |
| 365    | 198     | 1      | 100    | 3.7   | 5372   | PASS      |
| 441    | 443     | 0.01   | 150    | 78.8  | 24649  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 164283 | PASS      |
| 443    | 442     | 15     | 24     | 19.1  | 31296  | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/19/2025     | BNA_F            | <u>BF142787.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 429715           | 13.574             |
| DDD           | 7712             | 13.304             |
| DDE           | 717              | 12.939             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 8429          | 438144           | 1.92               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061925\  
Data File : BF142787.D  
Acq On : 19 Jun 2025 16:37  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 20 05:38:32 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 20 05:06:14 2025  
Response via : Initial Calibration

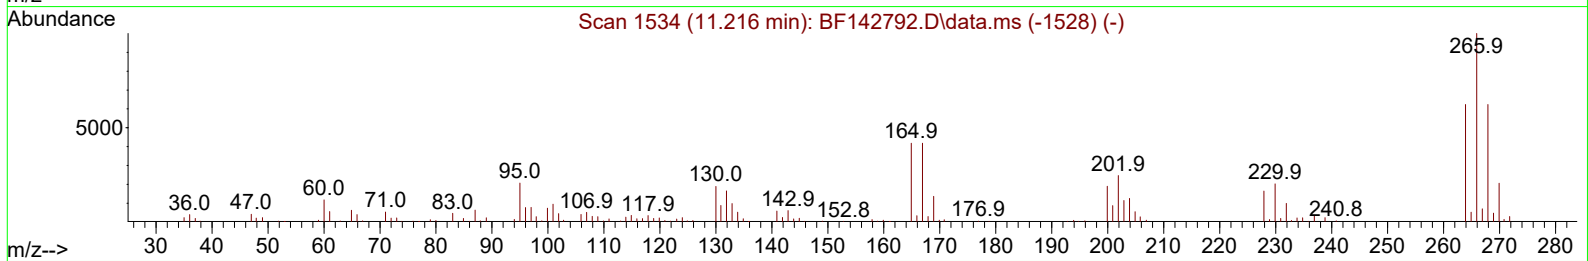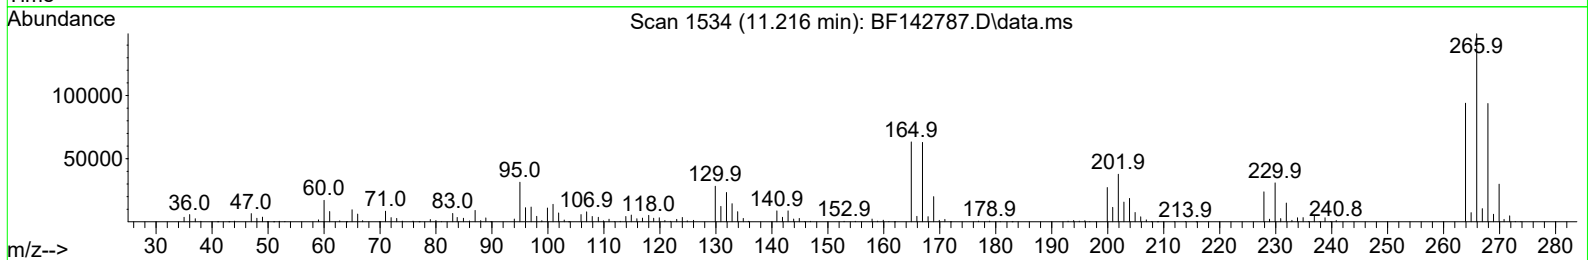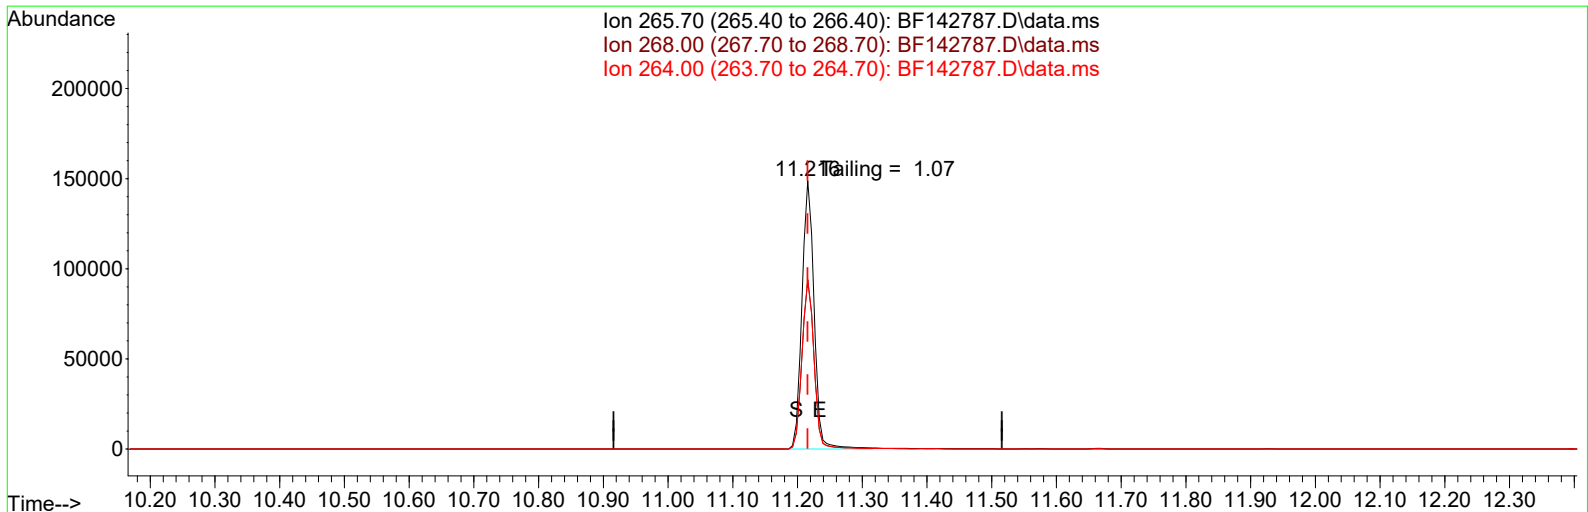

TIC: BF142787.D\data.ms

**(70) Pentachlorophenol (C)**

**11.216min (+ 0.000) 37164.56 ng**




**response 195787**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.30  | 62.94  |
| 264.00 | 62.40  | 63.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF061925\  
Data File : BF142787.D  
Acq On : 19 Jun 2025 16:37  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 20 05:38:32 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 20 05:06:14 2025  
Response via : Initial Calibration

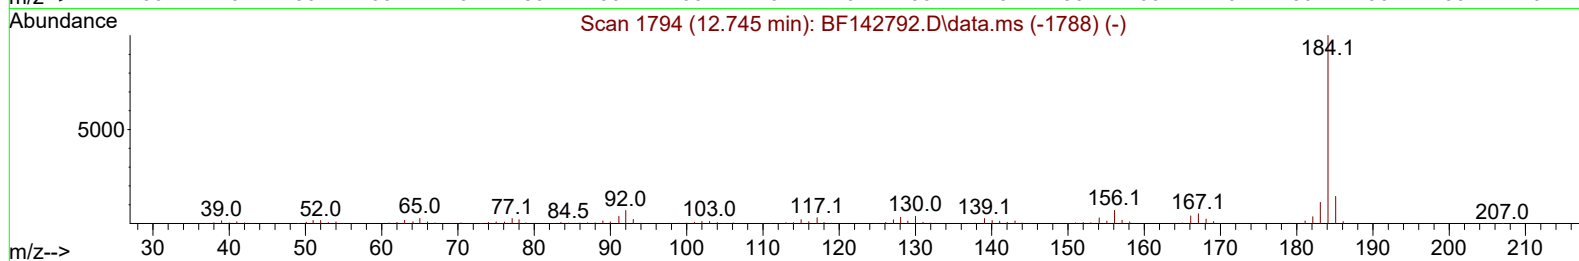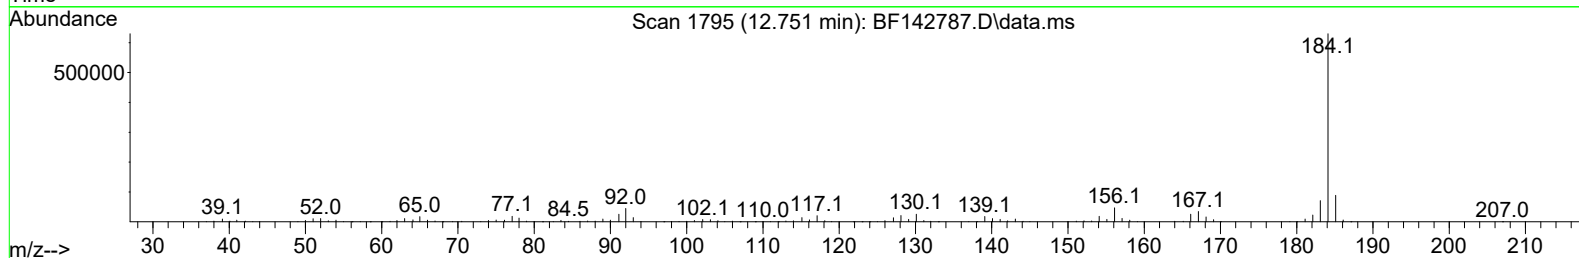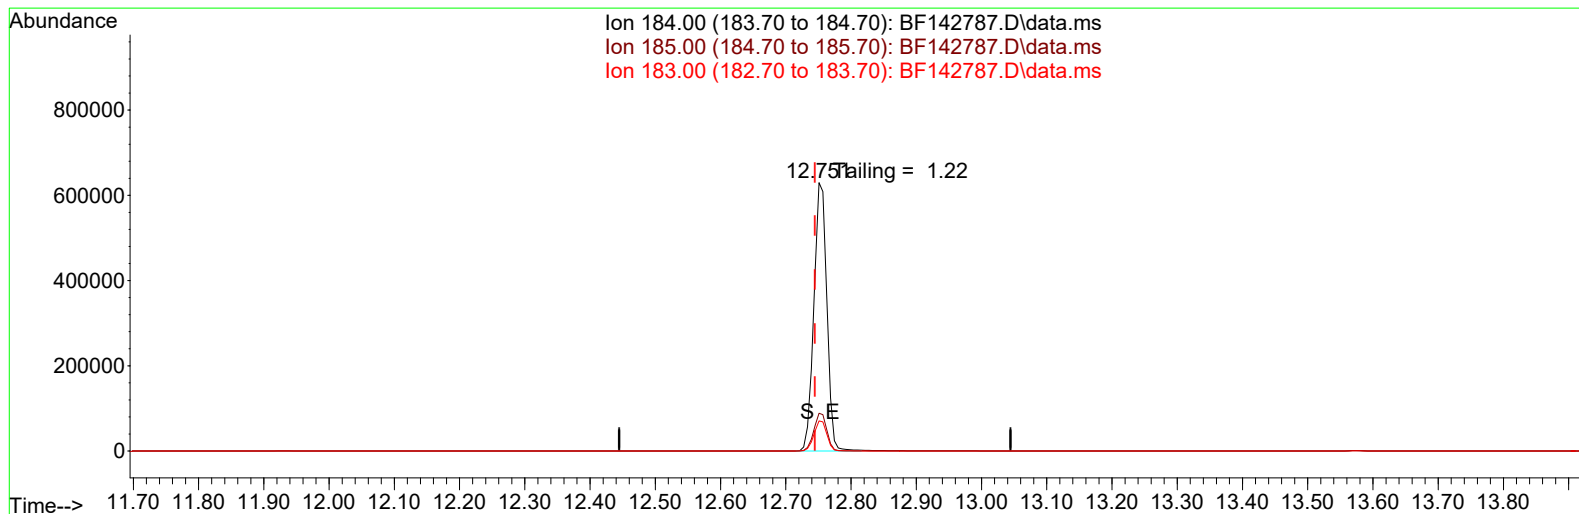

TIC: BF142787.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 874127

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 14.11  |
| 183.00 | 11.20  | 11.25  |
| 0.00   | 0.00   | 0.00   |