

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062425\
 Data File : VN087159.D
 Acq On : 24 Jun 2025 16:11
 Operator : JC\MD
 Sample : Q2402-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OBSI

Quant Time: Jun 25 04:20:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	181938	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	387109	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	336293	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	160118	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	148885	61.120	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	= 122.240%		
35) Dibromofluoromethane	8.177	113	115149	50.194	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 100.380%		
50) Toluene-d8	10.565	98	479901	52.842	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	= 105.680%		
62) 4-Bromofluorobenzene	12.847	95	166768	49.425	ug/l	0.00
Spiked Amount	50.000	Range 77 - 121	Recovery	= 98.860%		
Target Compounds						
						Qvalue
3) Chloromethane	2.401	50	1849	0.789	ug/l	99
16) Acetone	4.459	43	3501	2.710	ug/l	98
40) Benzene	8.612	78	9158	0.819	ug/l	93
52) Toluene	10.629	92	3923	0.574	ug/l	96
68) m/p-Xylenes	12.070	106	2339	0.478	ug/l	95
84) 1,2,4-Trimethylbenzene	13.476	105	3960	0.410	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062425\
Data File : VN087159.D
Acq On : 24 Jun 2025 16:11
Operator : JC\MD
Sample : Q2402-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OBSI

Quant Time: Jun 25 04:20:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 07 02:12:50 2025
Response via : Initial Calibration




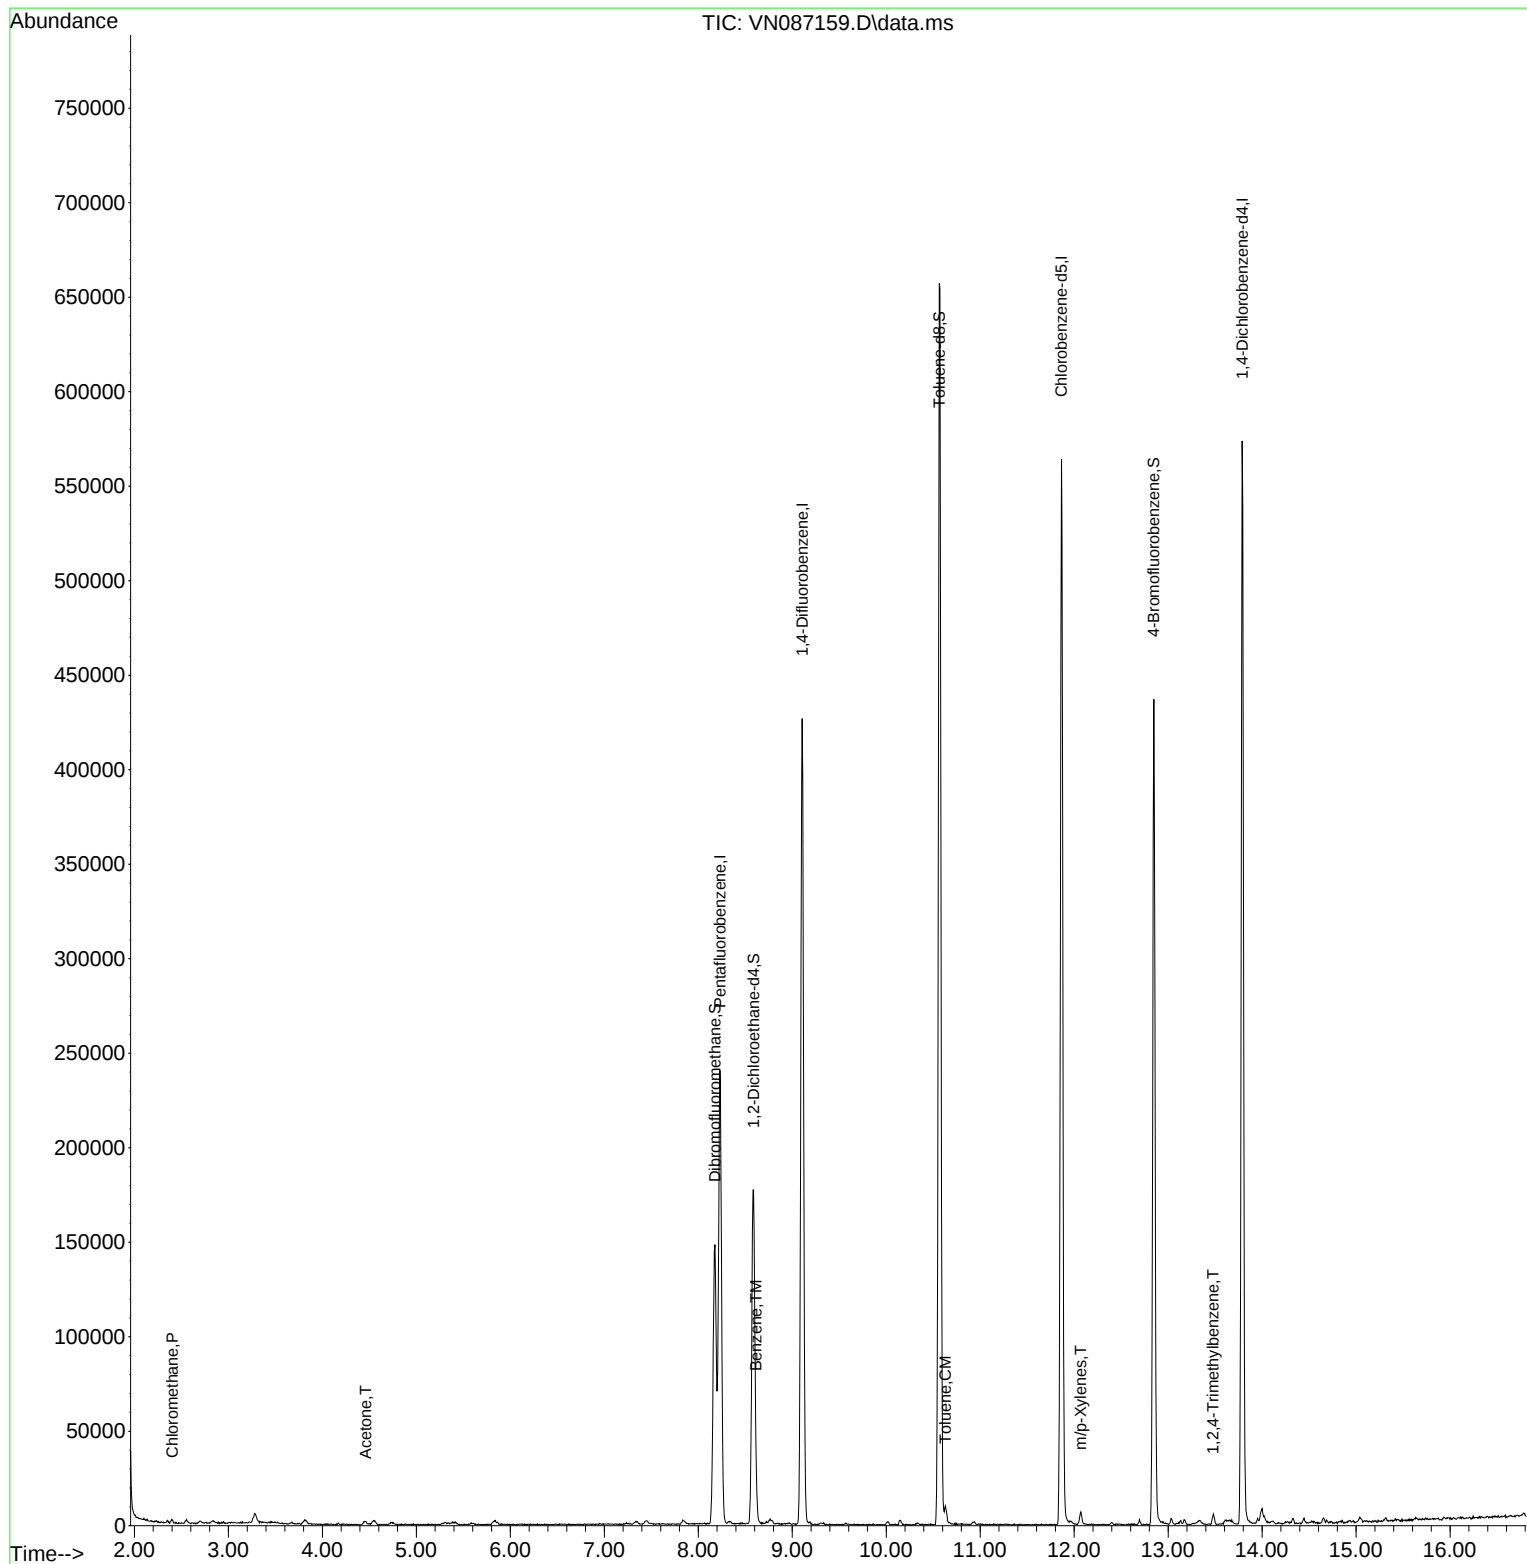




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1068
Delta R.T. -0.006 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11




Instrument :
MSVOA_N
ClientSampleId :
OBSI


Tgt Ion:168 Resp: 181938
Ion Ratio Lower Upper
168 100
99 61.7 49.1 73.7

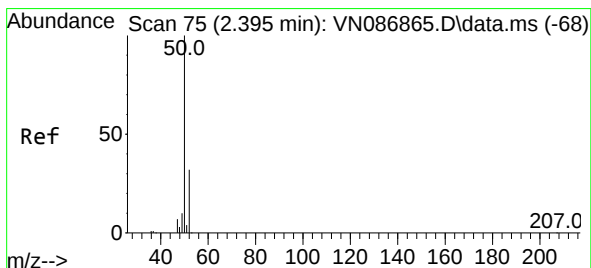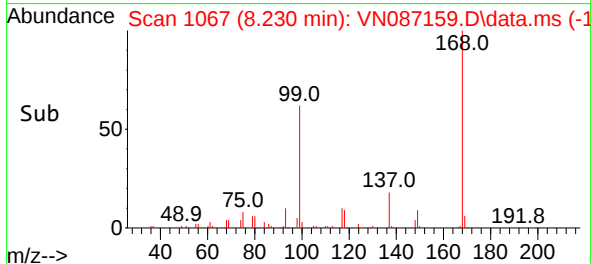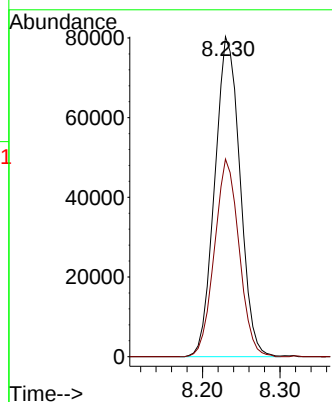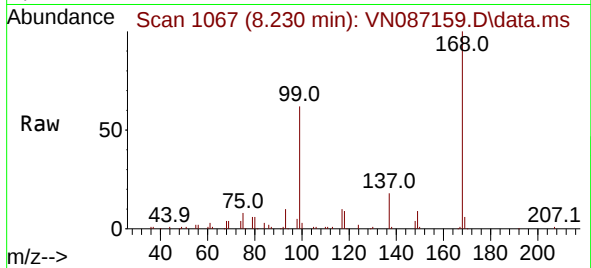

#3
Chloromethane
Concen: 0.789 ug/l
RT: 2.401 min Scan# 76
Delta R.T. 0.006 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11

Tgt Ion: 50 Resp: 1849
Ion Ratio Lower Upper
50 100
52 31.7 25.7 38.5


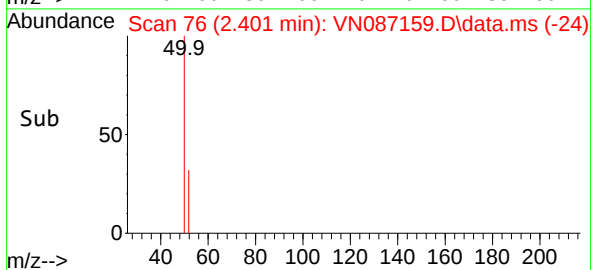
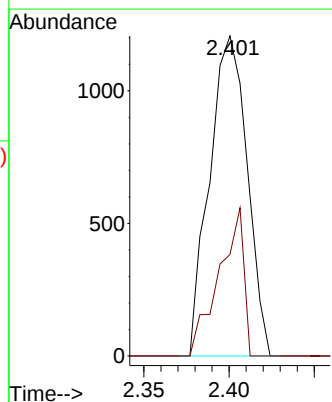
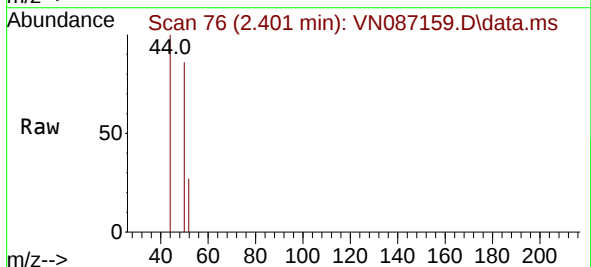


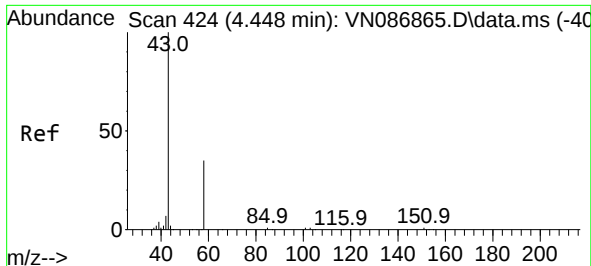

#16
Acetone
Concen: 2.710 ug/l
RT: 4.459 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11




Instrument :
MSVOA_N
ClientSampleId :
OBSI


Tgt Ion: 43 Resp: 3501
Ion Ratio Lower Upper
43 100
58 34.0 28.0 42.0

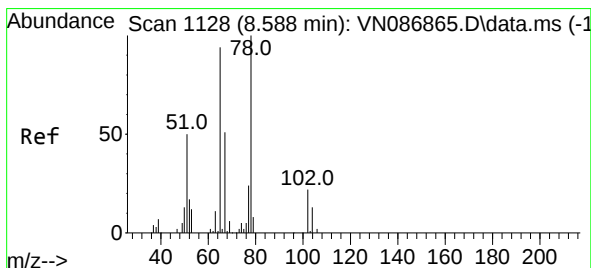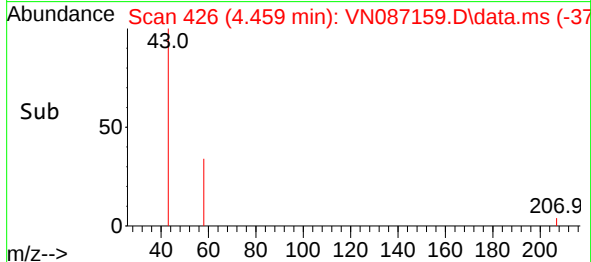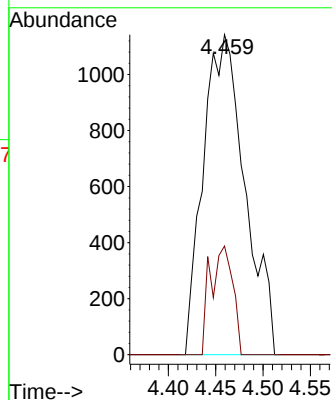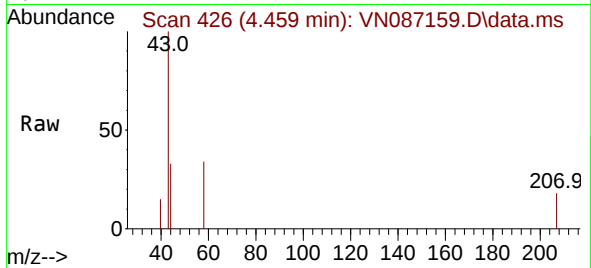

#33
1,2-Dichloroethane-d4
Concen: 61.120 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11

Tgt Ion: 65 Resp: 148885
Ion Ratio Lower Upper
65 100
67 53.5 0.0 105.6


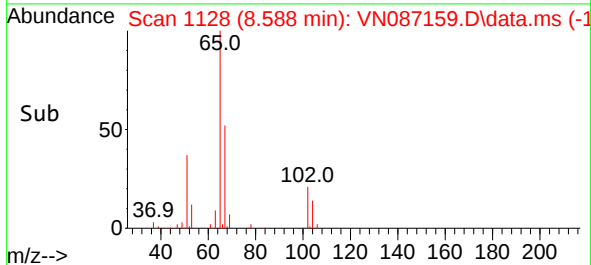
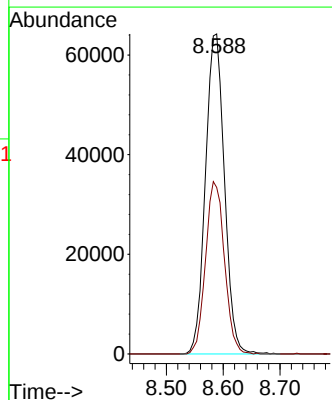
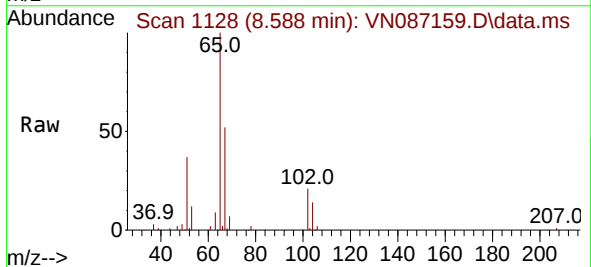


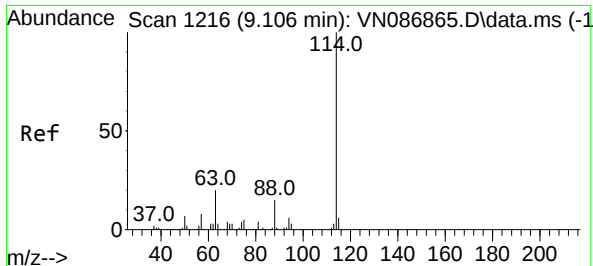

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11




Instrument :
MSVOA_N
ClientSampleId :
OBSI


Tgt Ion:114 Resp: 387109
Ion Ratio Lower Upper
114 100
63 21.0 0.0 39.6
88 15.1 0.0 30.2

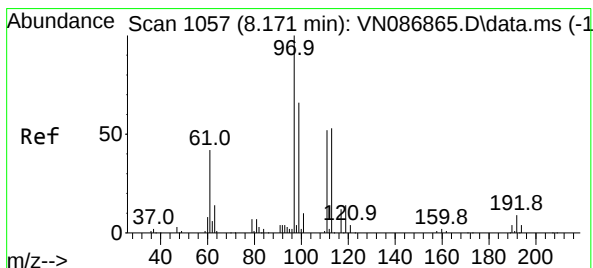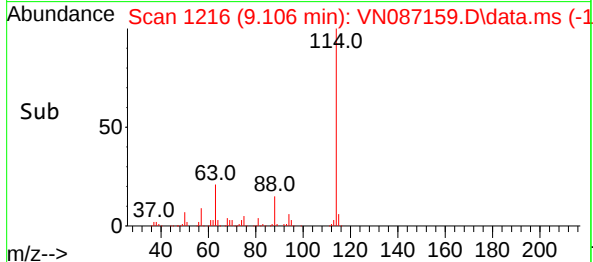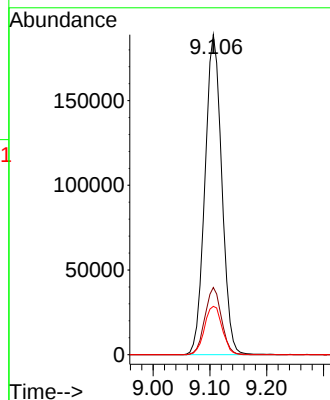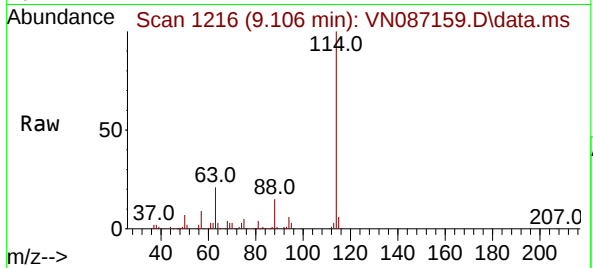

#35
Dibromofluoromethane
Concen: 50.194 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. 0.006 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11

Tgt Ion:113 Resp: 115149
Ion Ratio Lower Upper
113 100
111 102.8 84.2 126.2
192 17.1 14.2 21.4


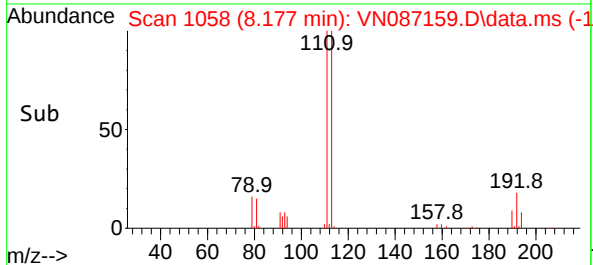
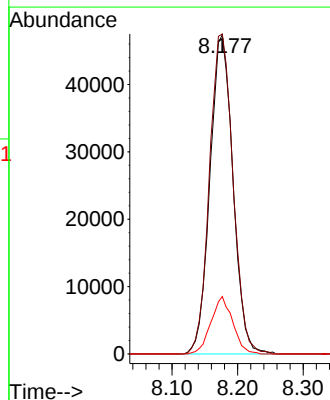
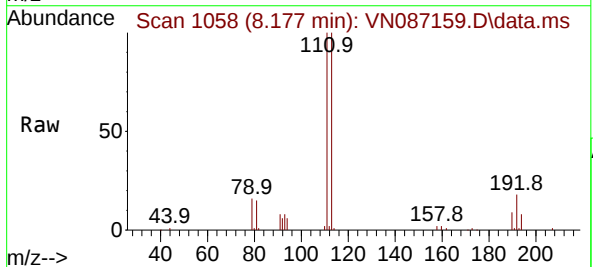


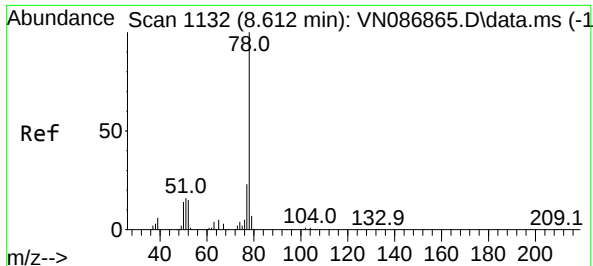

#40
Benzene
Concen: 0.819 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. -0.000 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11




Instrument :
MSVOA_N
ClientSampleId :
OBSI


Tgt Ion: 78 Resp: 9158
Ion Ratio Lower Upper
78 100
77 20.0 18.7 28.1

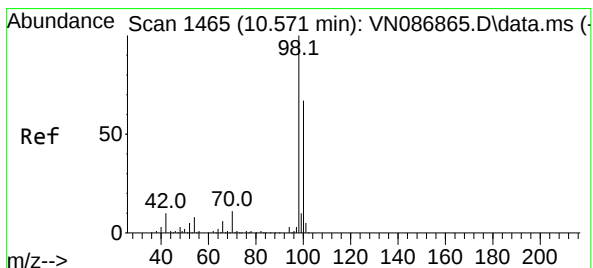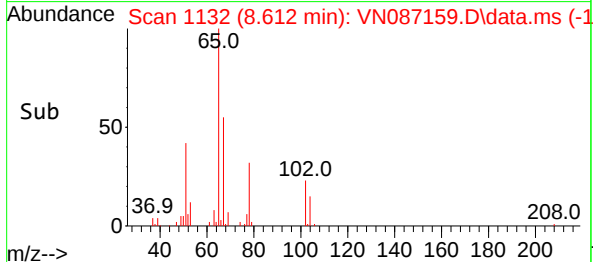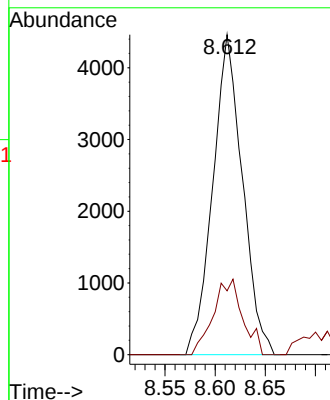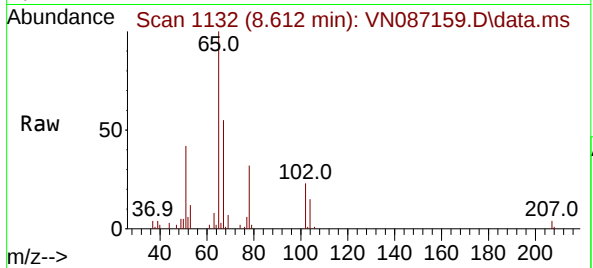

#50
Toluene-d8
Concen: 52.842 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11

Tgt Ion: 98 Resp: 479901
Ion Ratio Lower Upper
98 100
100 64.8 53.4 80.0

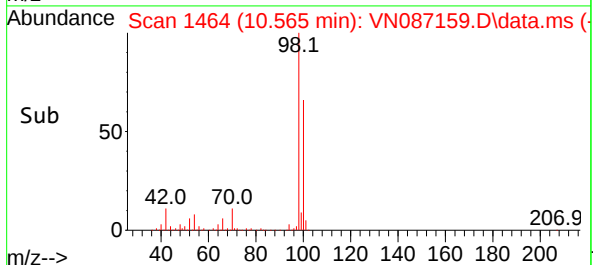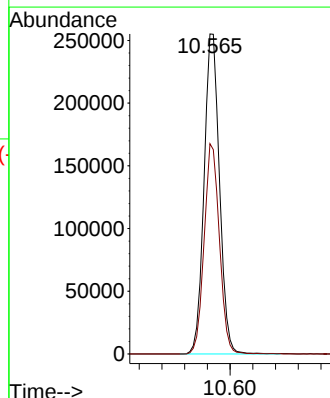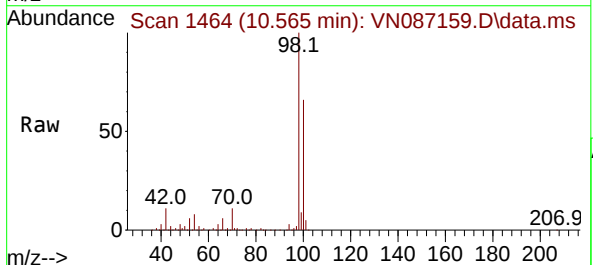

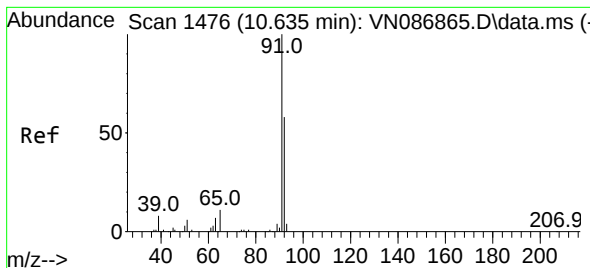

#52

Toluene

Concen: 0.574 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. -0.006 min

Lab File: VN087159.D

Acq: 24 Jun 2025 16:11

Instrument :

MSVOA_N

ClientSampleId :





OBSI

Tgt Ion: 92 Resp: 3923

Ion Ratio Lower Upper

92 100

91 175.9 136.5 204.7

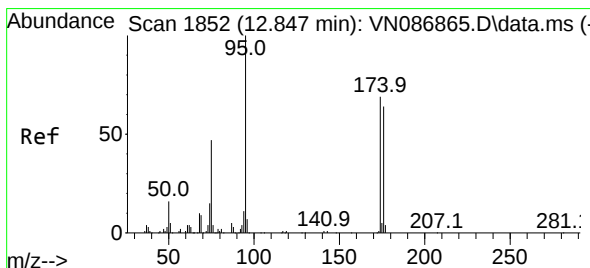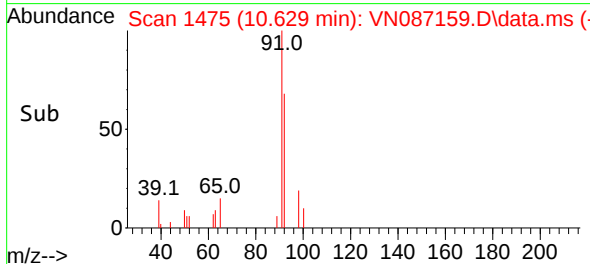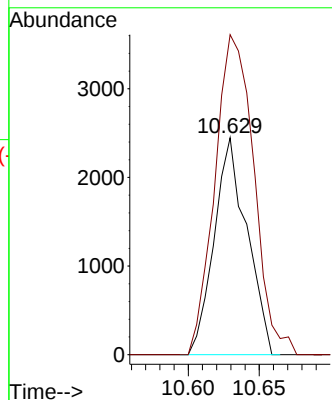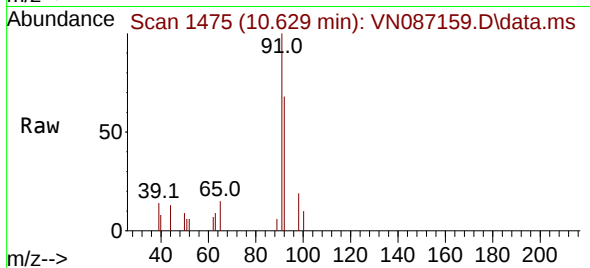

#62

4-Bromofluorobenzene

Concen: 49.425 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.000 min

Lab File: VN087159.D

Acq: 24 Jun 2025 16:11




Tgt Ion: 95 Resp: 166768


Ion Ratio Lower Upper

95 100

174 70.5 0.0 141.8

176 67.5 0.0 132.6


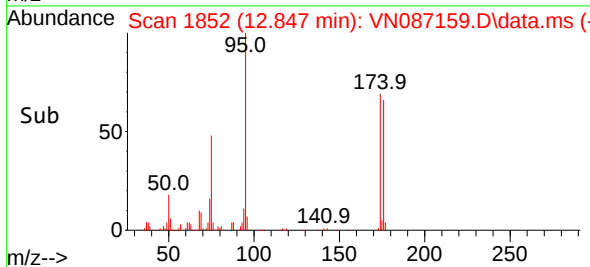
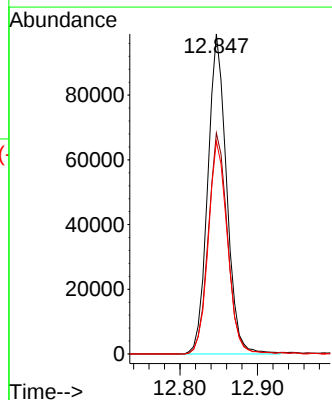
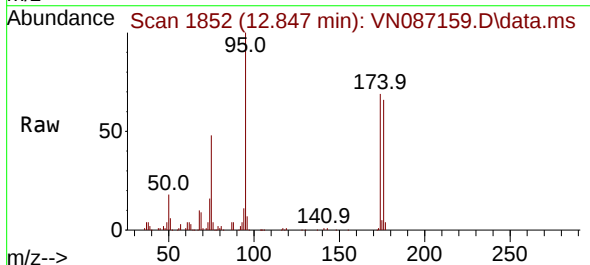


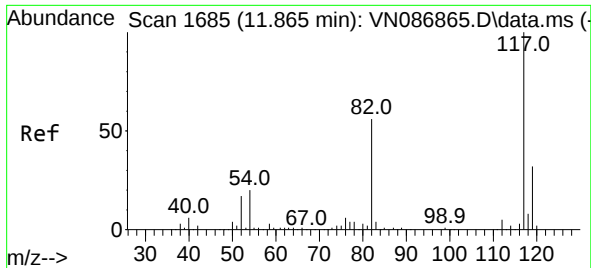

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11




Instrument :
MSVOA_N
ClientSampleId :
OBSI


Tgt Ion:117 Resp: 336293
Ion Ratio Lower Upper
117 100
82 56.8 44.6 67.0
119 32.5 25.5 38.3

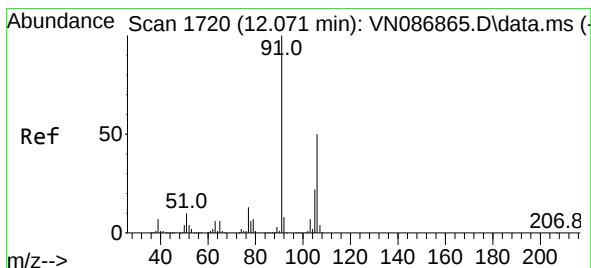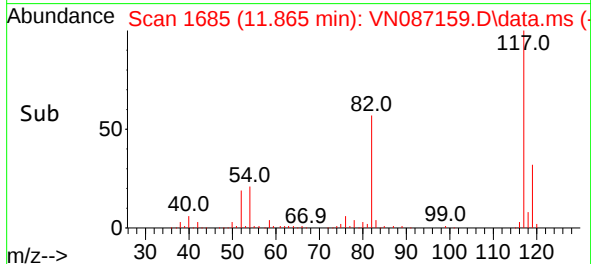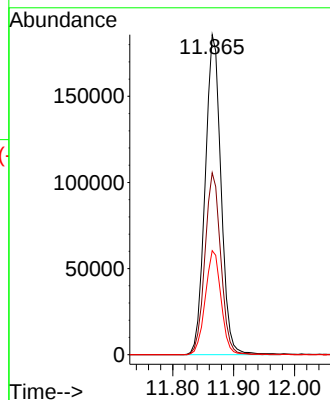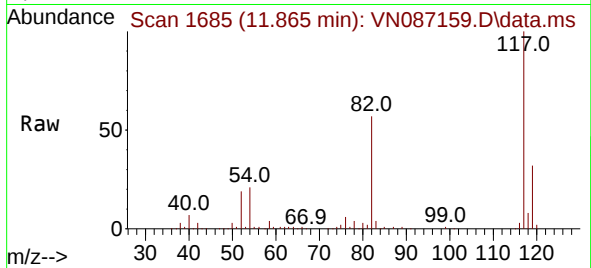

#68
m/p-Xylenes
Concen: 0.478 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.000 min
Lab File: VN087159.D
Acq: 24 Jun 2025 16:11

Tgt Ion:106 Resp: 2339
Ion Ratio Lower Upper
106 100
91 206.9 159.4 239.0


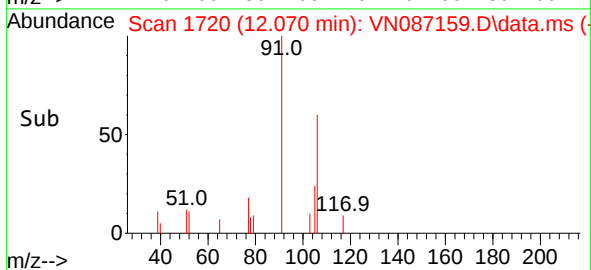
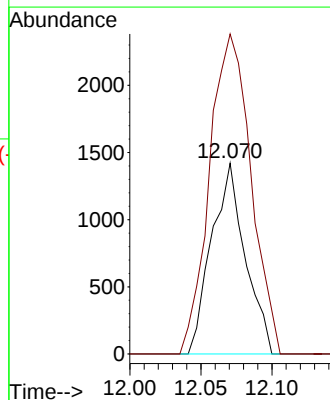
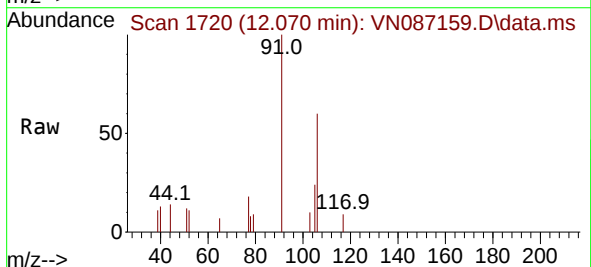


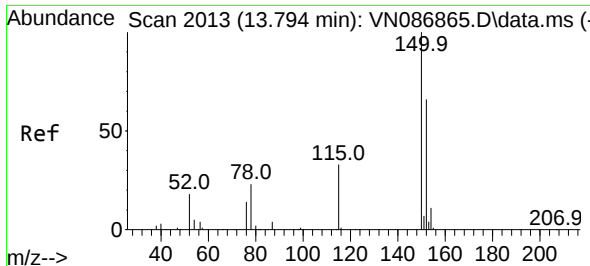

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.788 min Scan# 2013
 Delta R.T. -0.006 min
 Lab File: VN087159.D
 Acq: 24 Jun 2025 16:11

Instrument :
 MSVOA_N
 ClientSampleId :
 OBSI

Tgt Ion:152 Resp: 160118
 Ion Ratio Lower Upper
 152 100
 115 63.4 30.1 90.5
 150 160.5 0.0 345.0

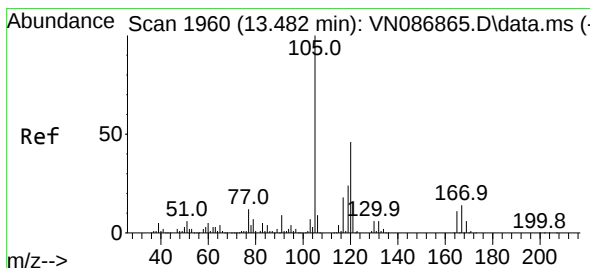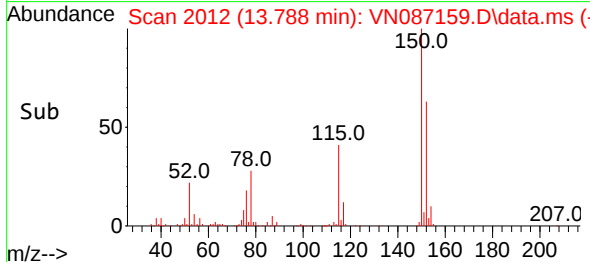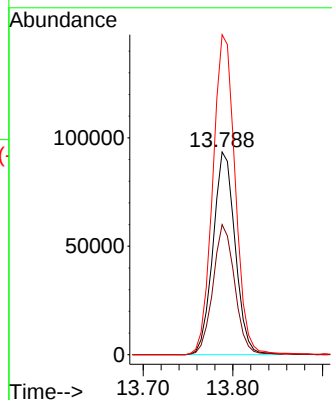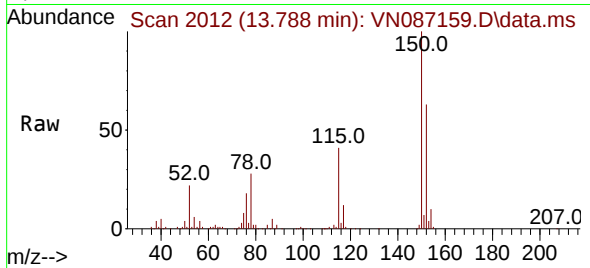

#84
 1,2,4-Trimethylbenzene
 Concen: 0.410 ug/l
 RT: 13.476 min Scan# 1959
 Delta R.T. -0.006 min
 Lab File: VN087159.D
 Acq: 24 Jun 2025 16:11

Tgt Ion:105 Resp: 3960
 Ion Ratio Lower Upper
 105 100
 120 45.7 23.2 69.6

