


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062525\
Data File : BF142833.D
Acq On : 25 Jun 2025 12:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

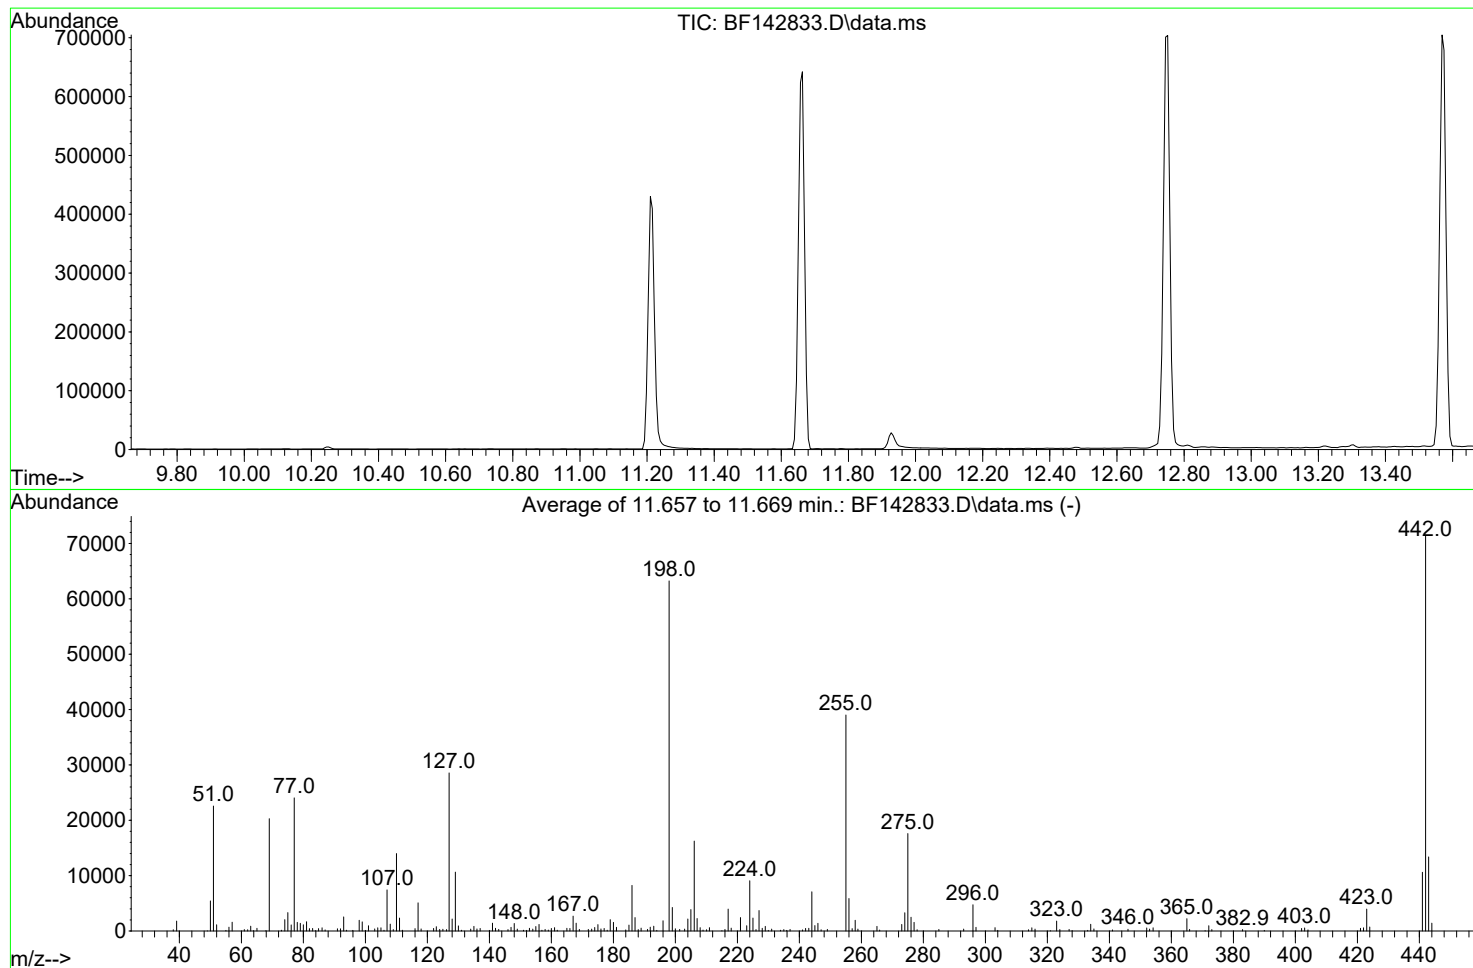

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.4	72	PASS
69	69	100	100	100.0	20307	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63235	PASS
199	198	5	9	6.7	4266	PASS
365	198	1	100	3.5	2228	PASS
441	443	0.01	150	79.2	10603	PASS
442	442	100	100	100.0	71325	PASS
443	442	15	24	18.8	13383	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/25/2025	BNA_F	<u>BF142833.D</u>
Compound Name	Response	Retention Time
DDT	182439	13.574
DDD	2979	13.304
DDE	207	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3186	185625	1.72

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062525\
Data File : BF142833.D
Acq On : 25 Jun 2025 12:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 13:51:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

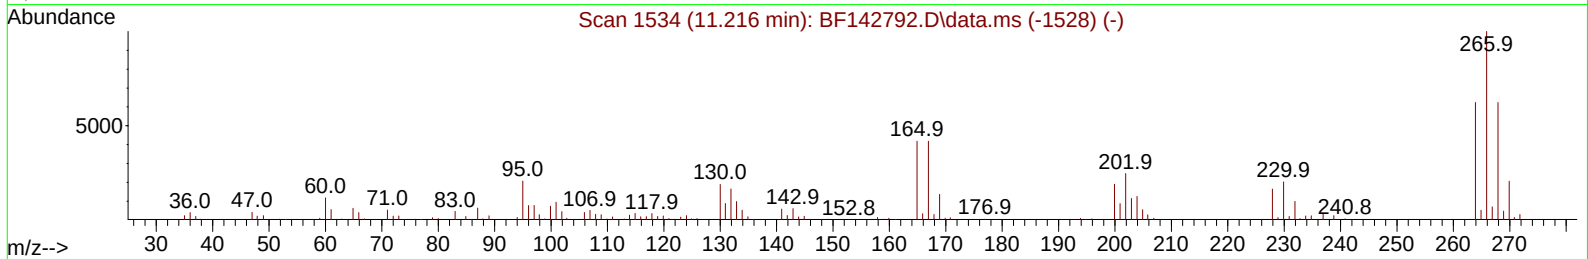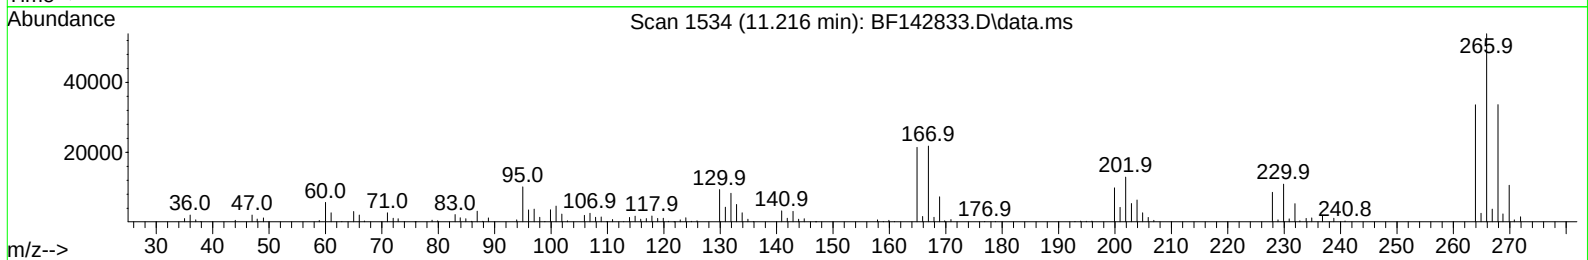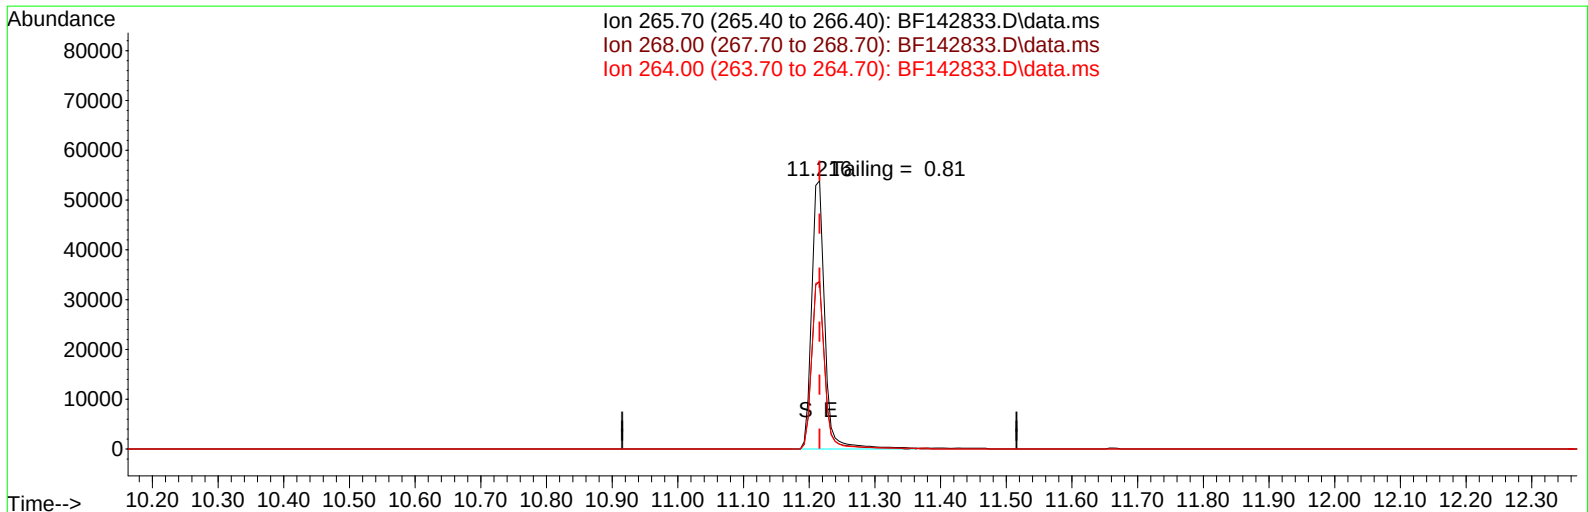

TIC: BF142833.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 32756.87 ng




response 75756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.42
264.00	62.40	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062525\
Data File : BF142833.D
Acq On : 25 Jun 2025 12:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 13:51:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

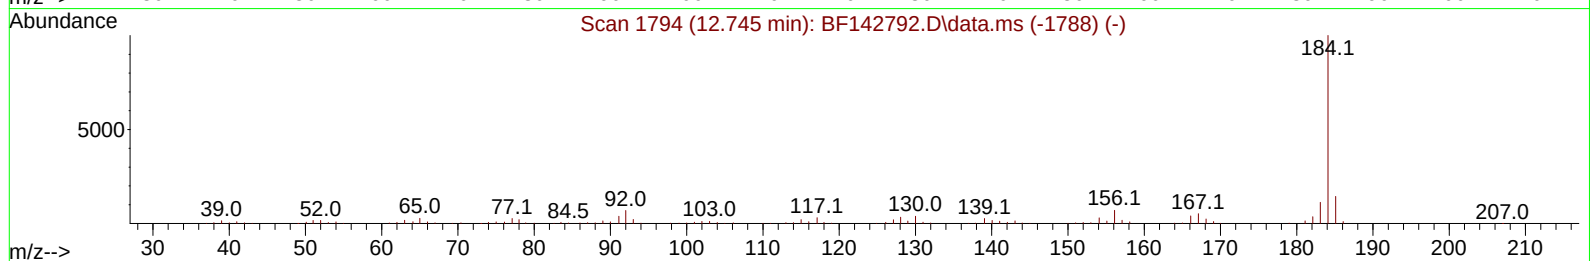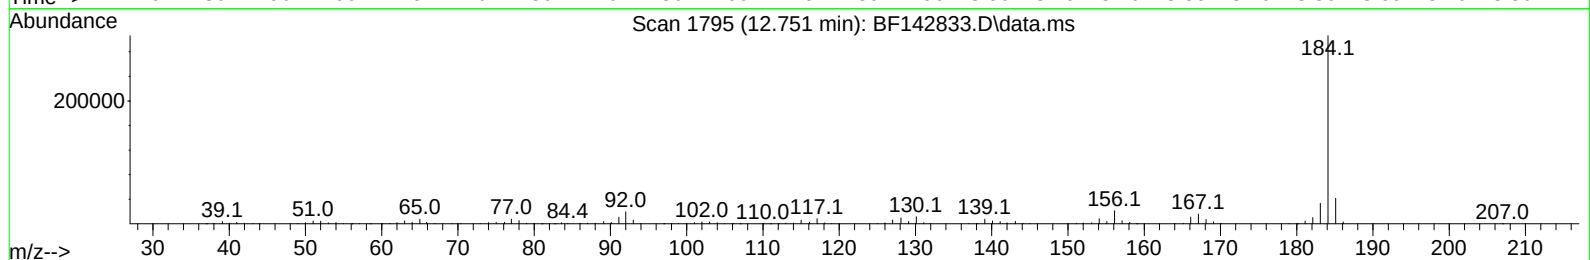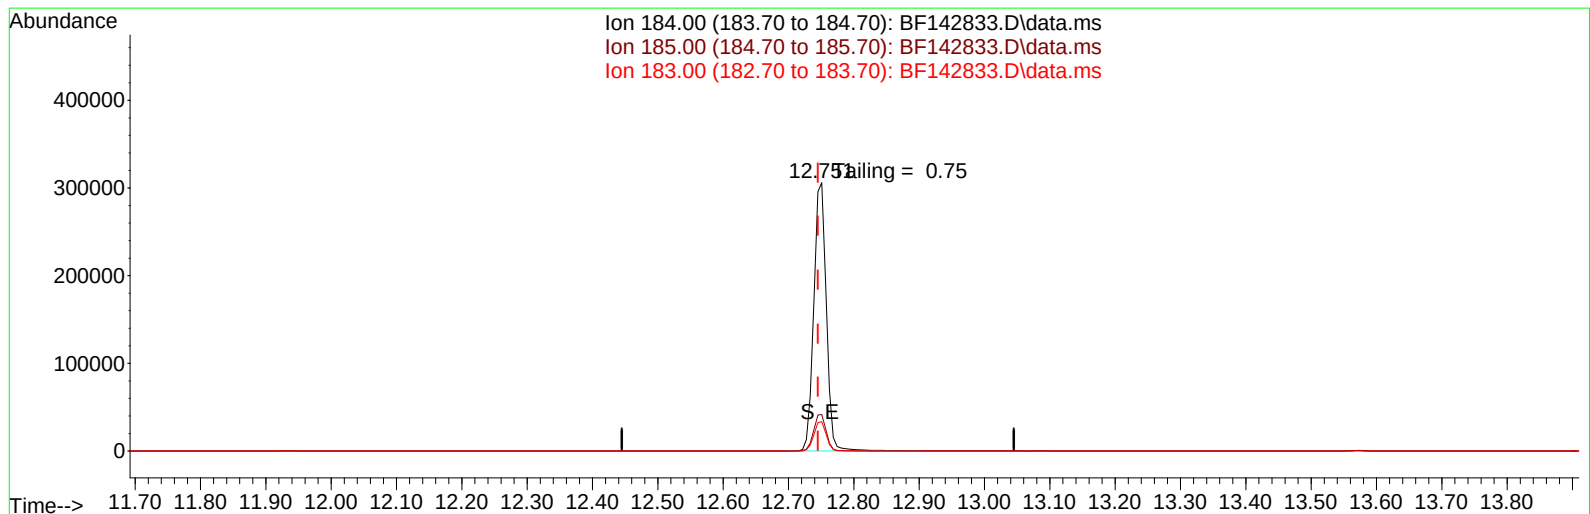

TIC: BF142833.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 410200

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.59
183.00	11.20	10.93
0.00	0.00	0.00