


Fluoride (Anions)

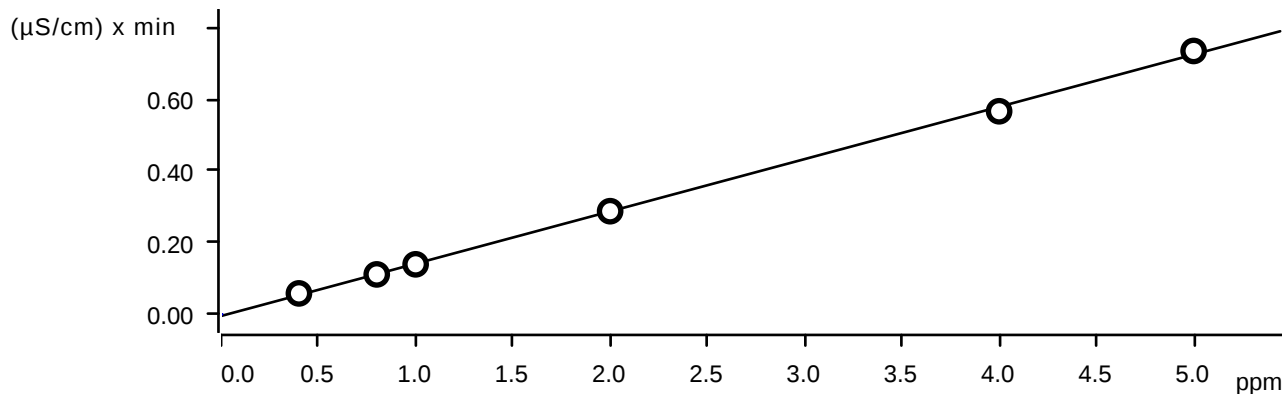


Function: $A = -4.55276E-3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

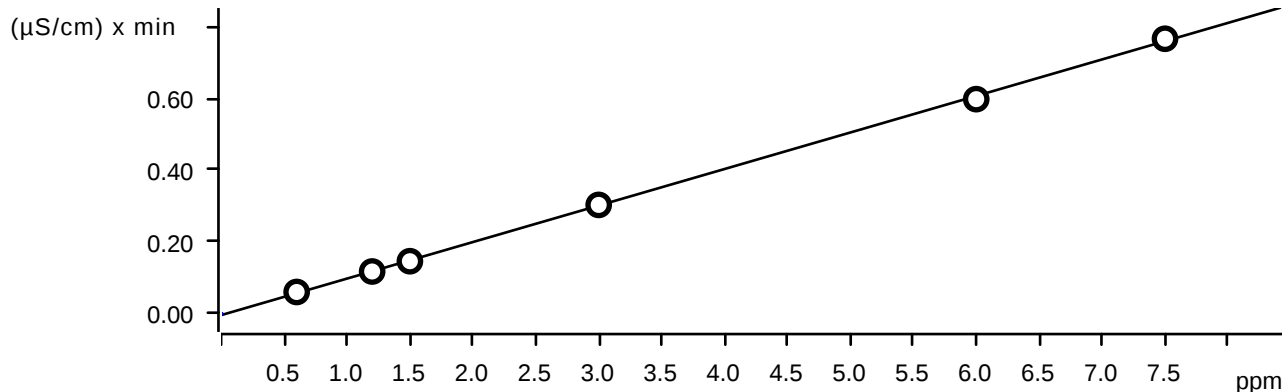

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

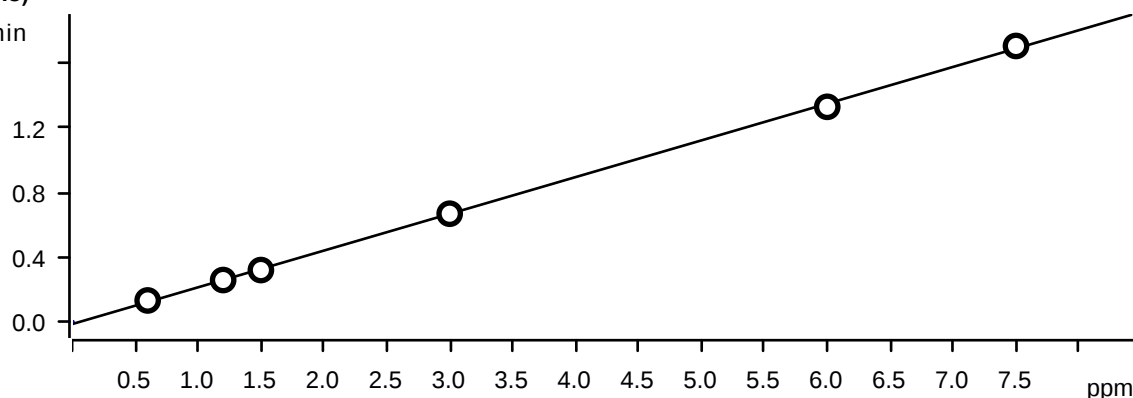Function: $A = -0.0166933 + 0.0227623 \times Q$


Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

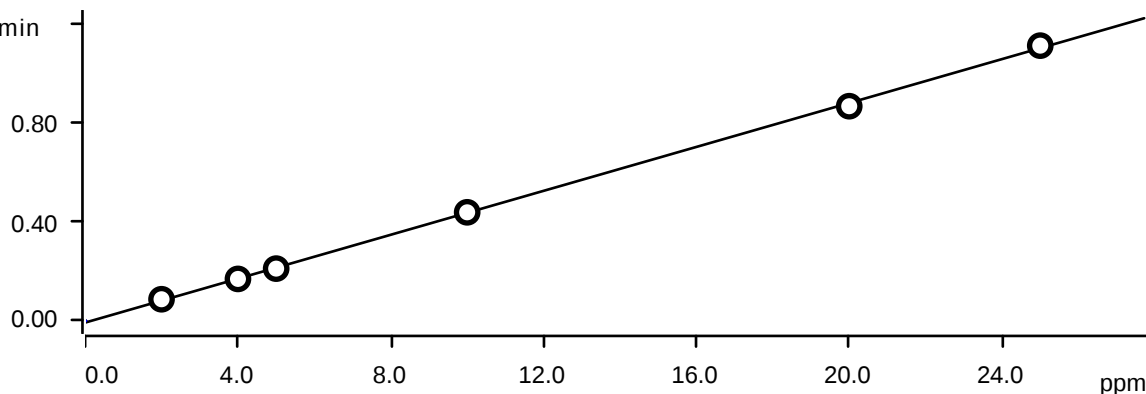

Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$


Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

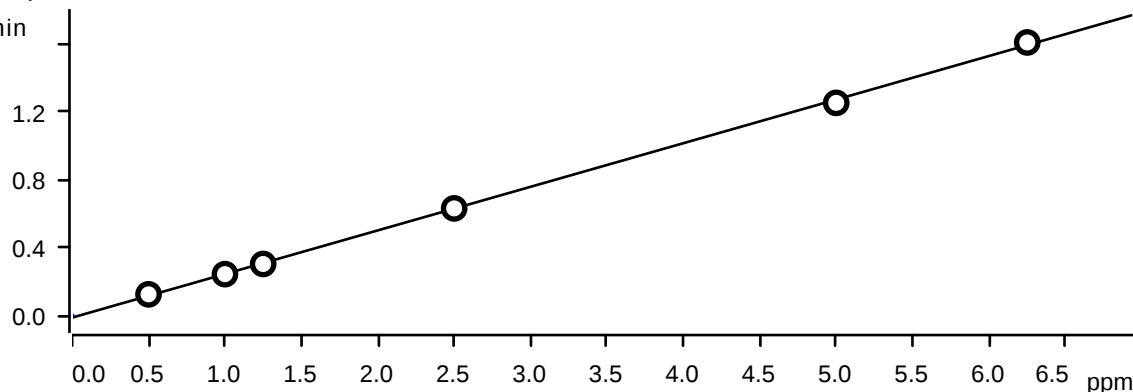


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

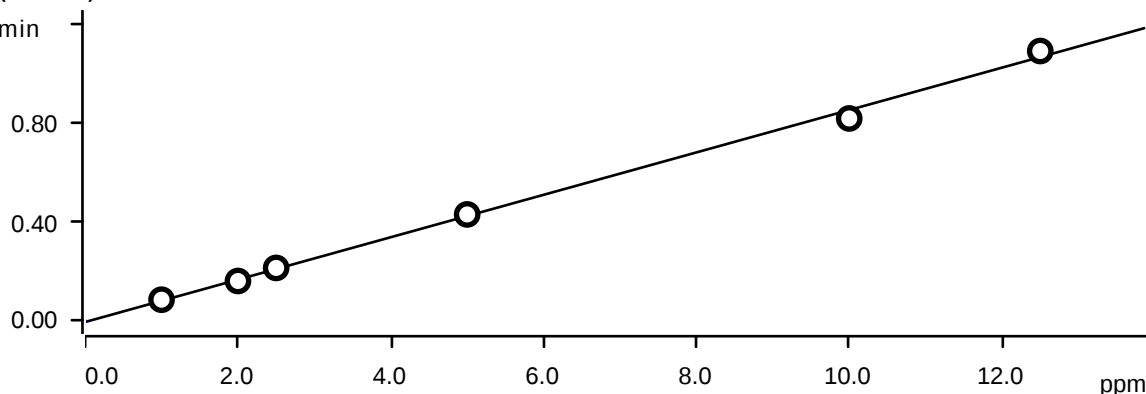
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

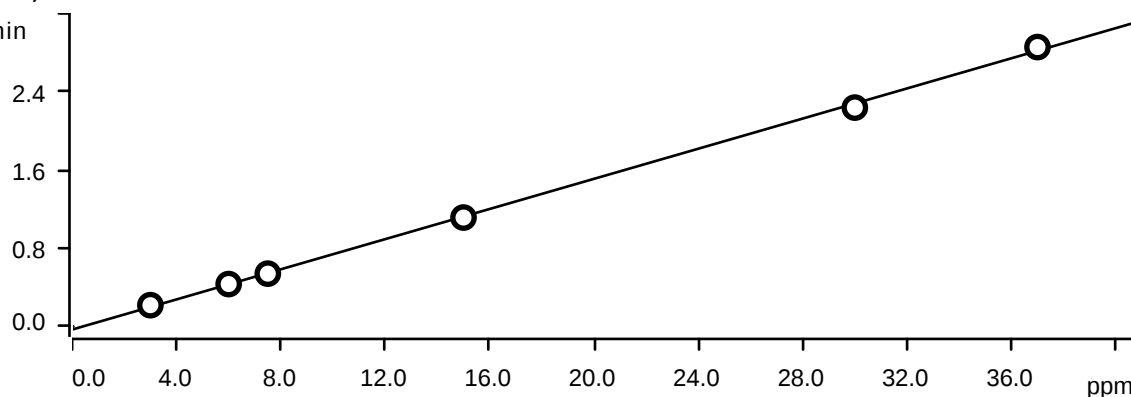 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-06-23 15:17:36 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

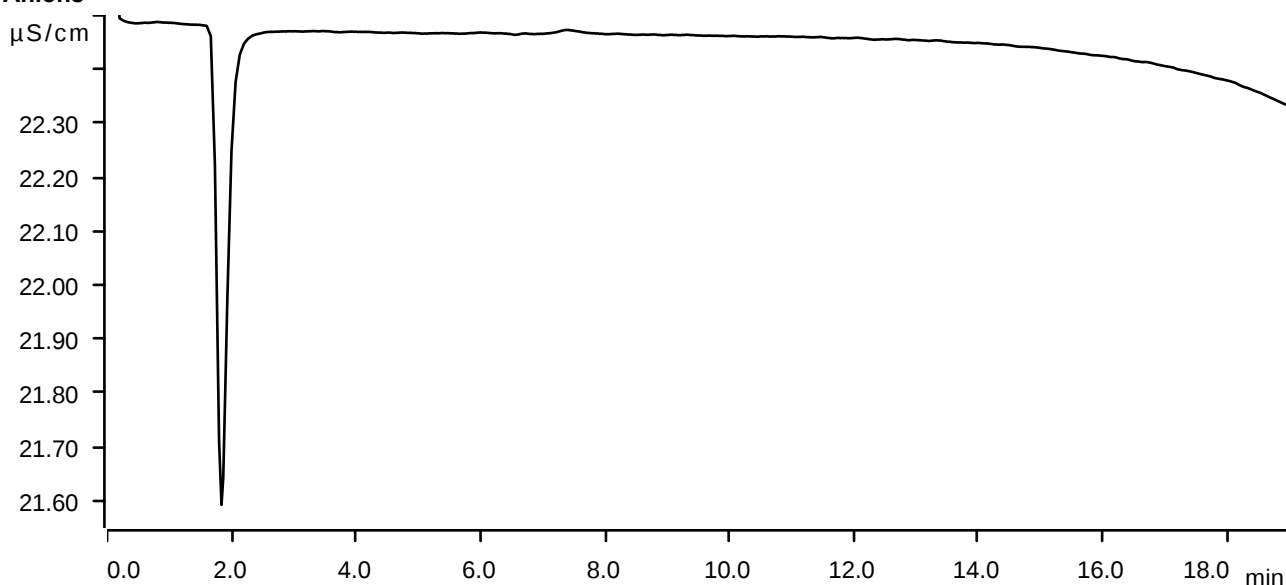
Anions

Sample data

Ident STD2
 Sample type Standard 2
 Determination start 2025-06-23 15:38:59 UTC-4
 Method IC1-062325
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.54 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

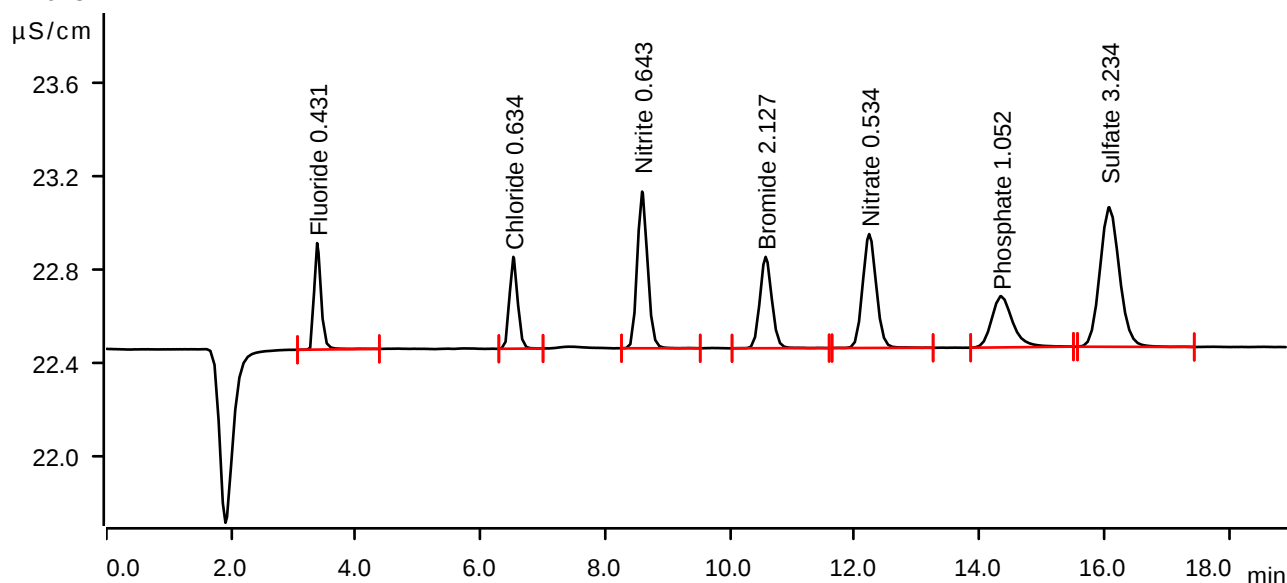Anions

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.380	0.0584	0.457	0.431	Fluoride
2	6.525	0.0599	0.394	0.634	Chloride
3	8.590	0.1297	0.673	0.643	Nitrite
4	10.570	0.0870	0.392	2.127	Bromide
5	12.230	0.1239	0.489	0.534	Nitrate
6	14.343	0.0862	0.220	1.052	Phosphate
7	16.078	0.2176	0.600	3.234	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-06-23 16:00:23 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

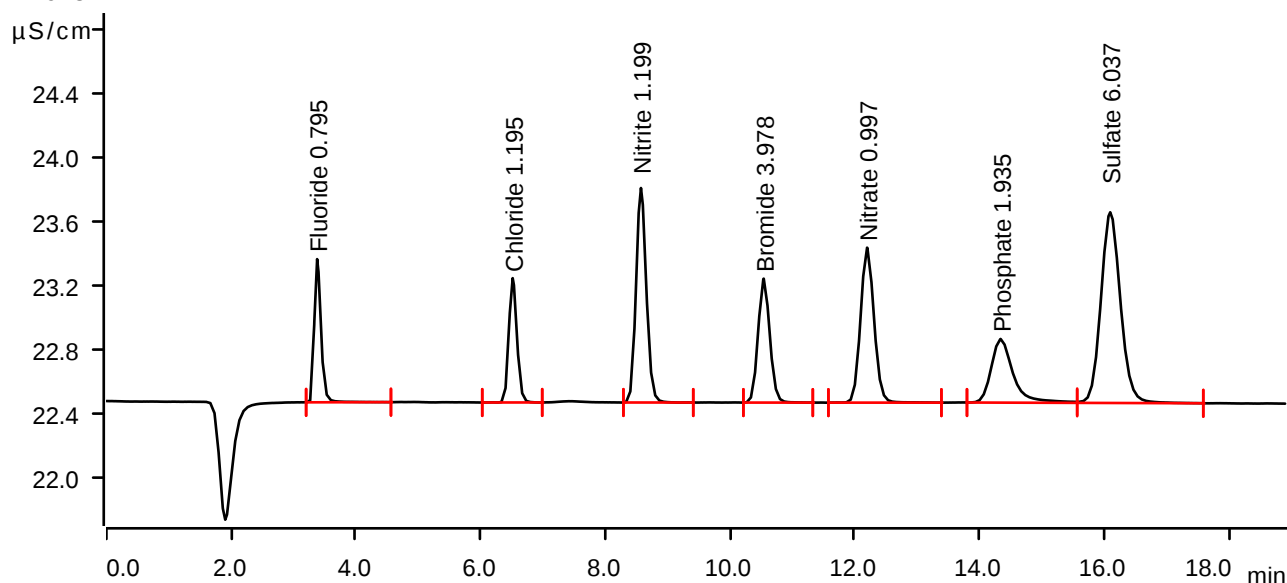

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.380	0.1114	0.894	0.795	Fluoride
2	6.515	0.1170	0.776	1.195	Chloride
3	8.572	0.2561	1.340	1.199	Nitrite
4	10.540	0.1688	0.774	3.978	Bromide
5	12.197	0.2428	0.968	0.997	Nitrate
6	14.338	0.1616	0.398	1.935	Phosphate
7	16.095	0.4335	1.191	6.037	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-06-23 16:21:47 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

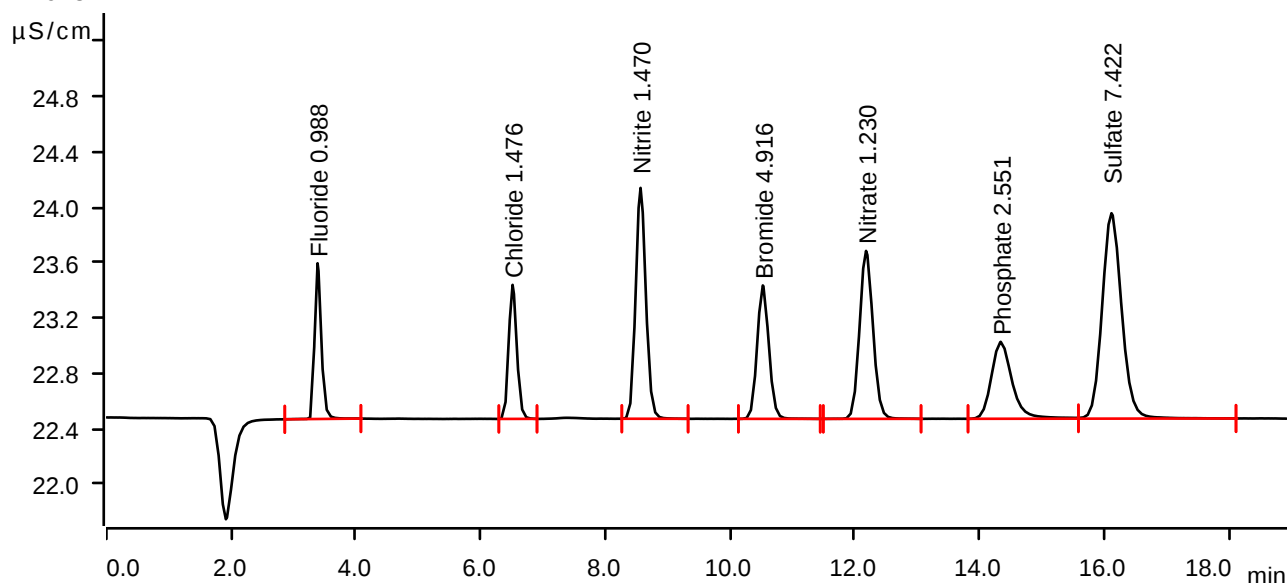

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.1394	1.124	0.988	Fluoride
2	6.513	0.1456	0.968	1.476	Chloride
3	8.565	0.3180	1.668	1.470	Nitrite
4	10.525	0.2103	0.964	4.916	Bromide
5	12.180	0.3026	1.213	1.230	Nitrate
6	14.340	0.2142	0.555	2.551	Phosphate
7	16.115	0.5402	1.484	7.422	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-06-23 16:43:01 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

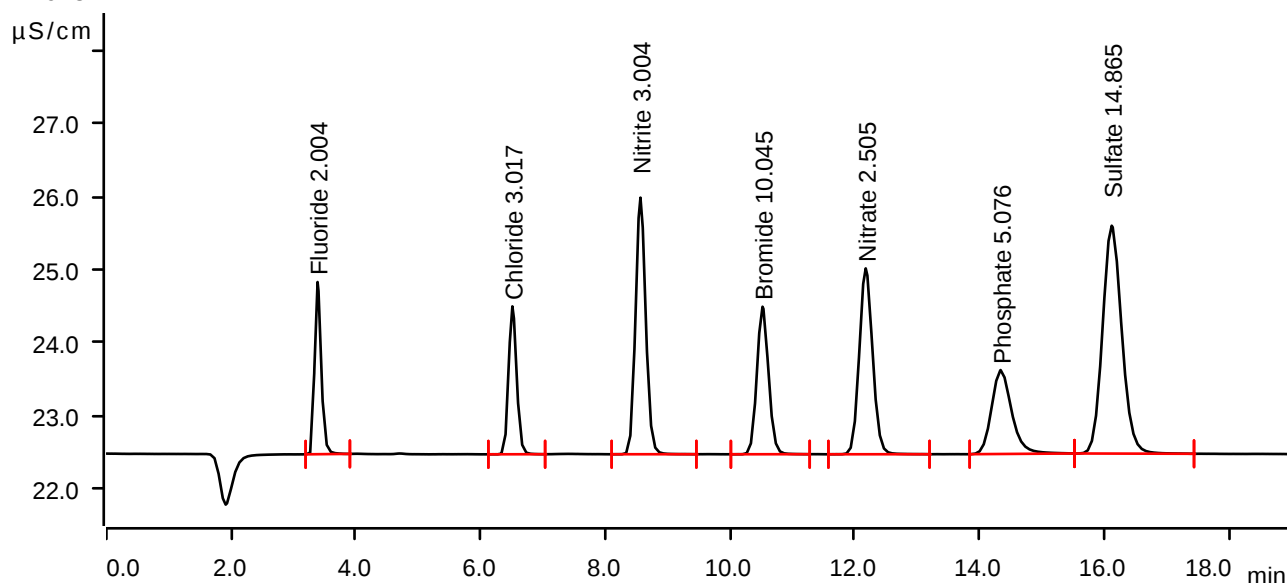

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.2876	2.353	2.004	Fluoride
2	6.510	0.3026	2.021	3.017	Chloride
3	8.563	0.6671	3.507	3.004	Nitrite
4	10.520	0.4371	2.016	10.045	Bromide
5	12.175	0.6299	2.540	2.505	Nitrate
6	14.338	0.4297	1.146	5.076	Phosphate
7	16.118	1.1136	3.114	14.865	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-06-23 17:04:27 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

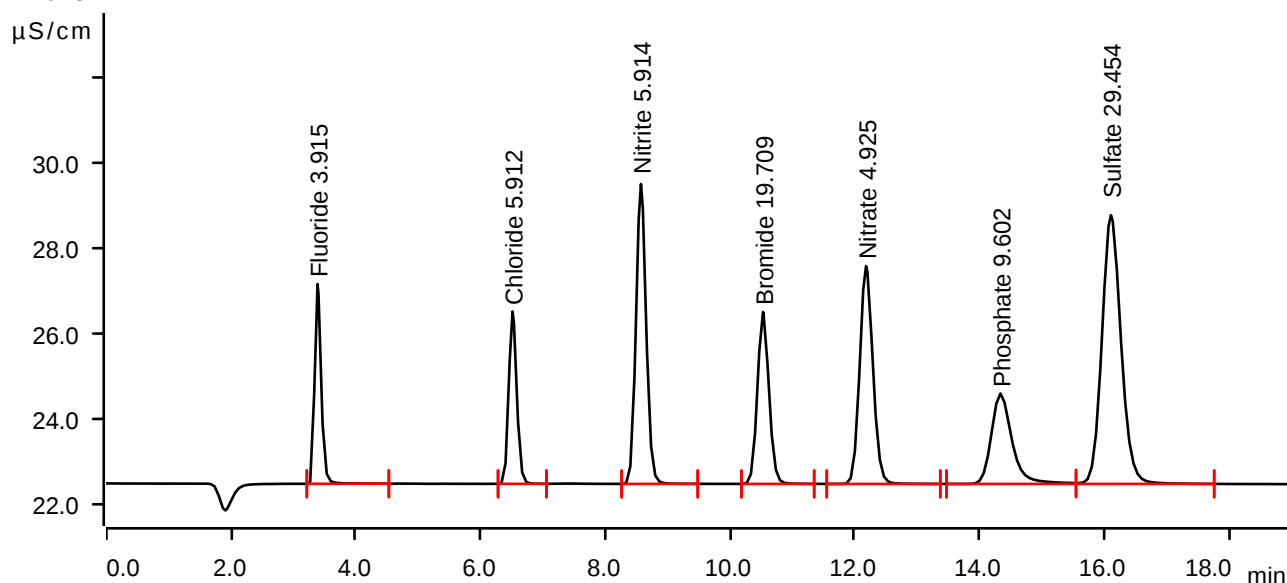

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.5661	4.679	3.915	Fluoride
2	6.513	0.5975	4.037	5.912	Chloride
3	8.572	1.3294	7.024	5.914	Nitrite
4	10.528	0.8644	4.027	19.709	Bromide
5	12.180	1.2509	5.103	4.925	Nitrate
6	14.335	0.8161	2.118	9.602	Phosphate
7	16.107	2.2375	6.295	29.454	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-06-23 17:25:53 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

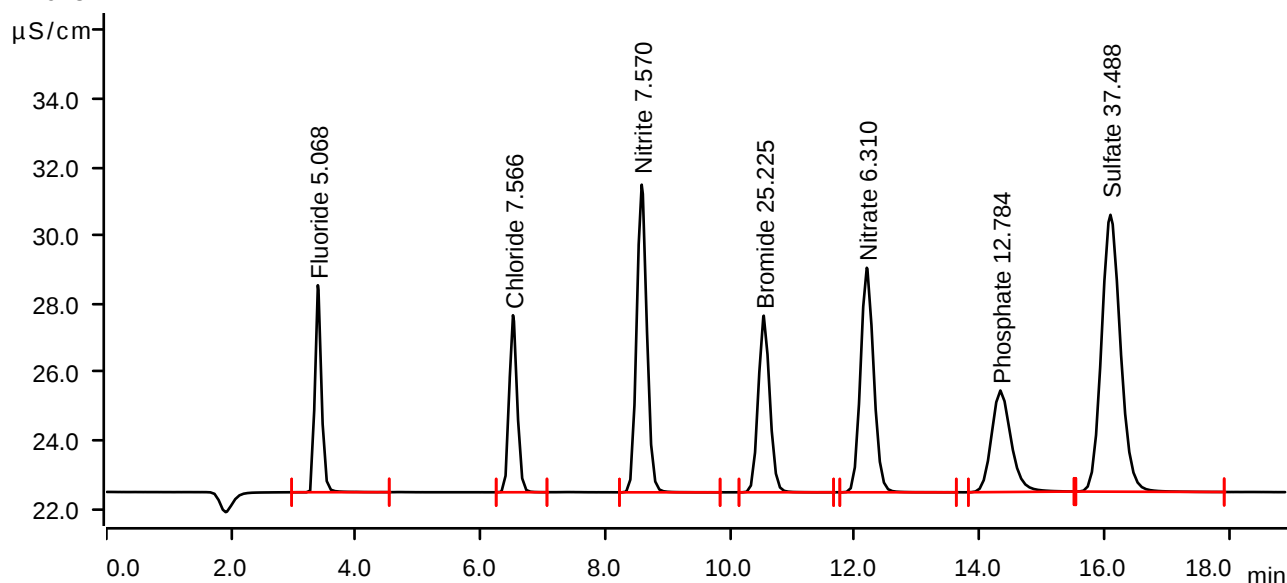

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.392	0.7342	6.060	5.068	Fluoride
2	6.520	0.7659	5.183	7.566	Chloride
3	8.583	1.7064	9.009	7.570	Nitrite
4	10.540	1.1083	5.172	25.225	Bromide
5	12.192	1.6065	6.575	6.310	Nitrate
6	14.333	1.0878	2.972	12.784	Phosphate
7	16.098	2.8564	8.108	37.488	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-06-23 17:47:21 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

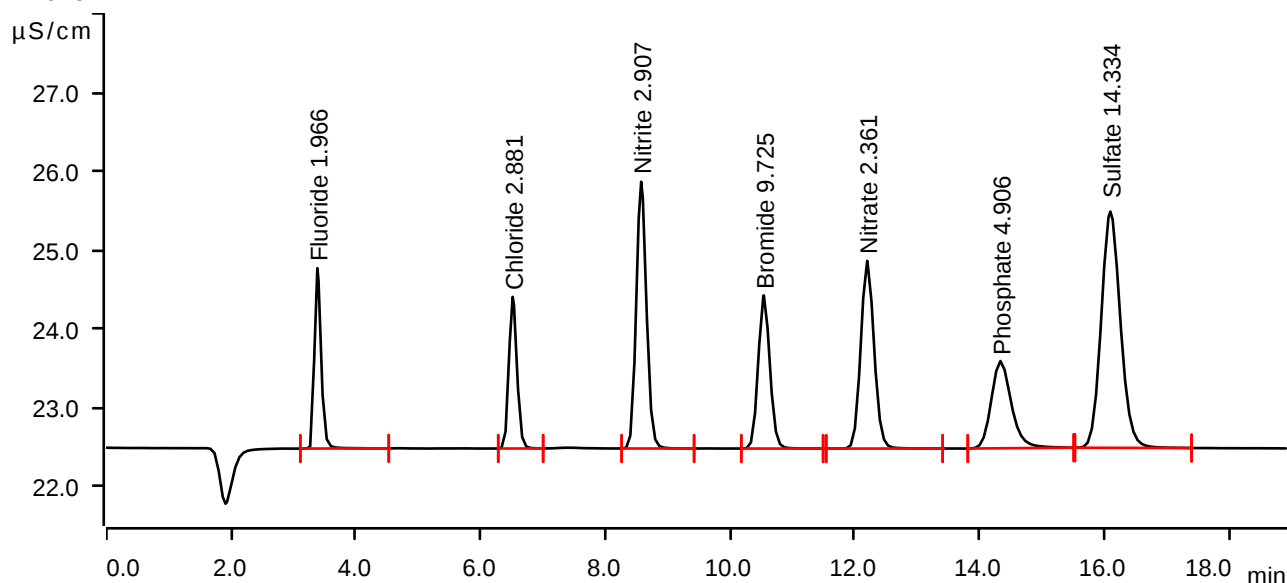


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.2821	2.288	1.966	Fluoride
2	6.515	0.2887	1.924	2.881	Chloride
3	8.575	0.6450	3.385	2.907	Nitrite
4	10.542	0.4229	1.943	9.725	Bromide
5	12.198	0.5928	2.382	2.361	Nitrate
6	14.335	0.4152	1.107	4.906	Phosphate
7	16.097	1.0727	2.998	14.334	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-06-23 18:08:49 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

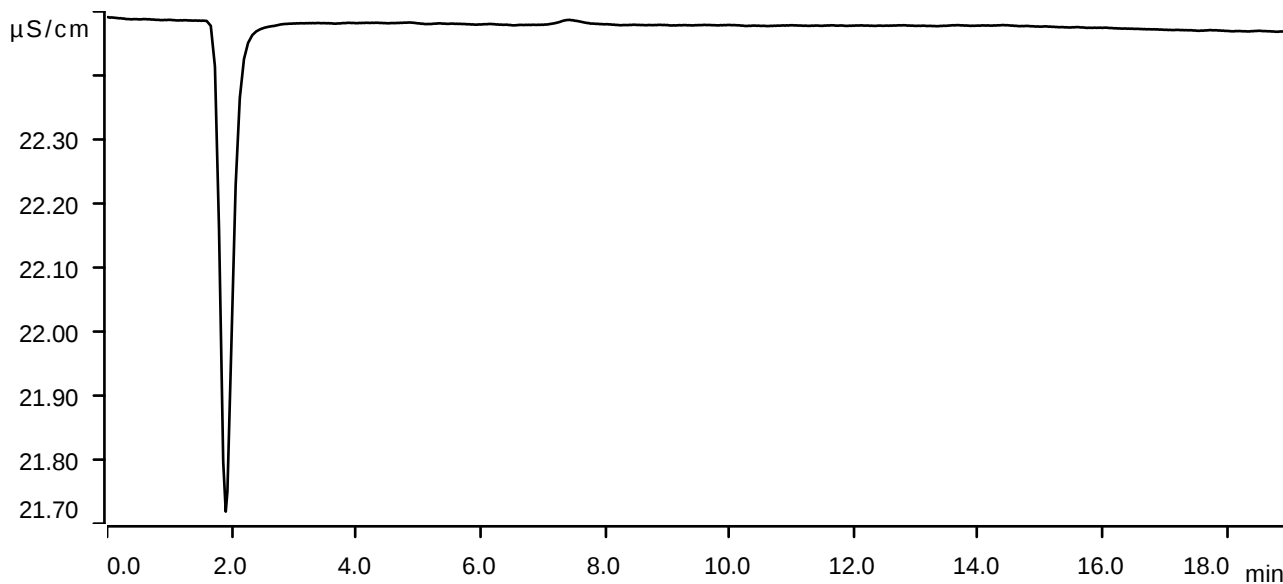Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-26 08:45:13 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C


Anions

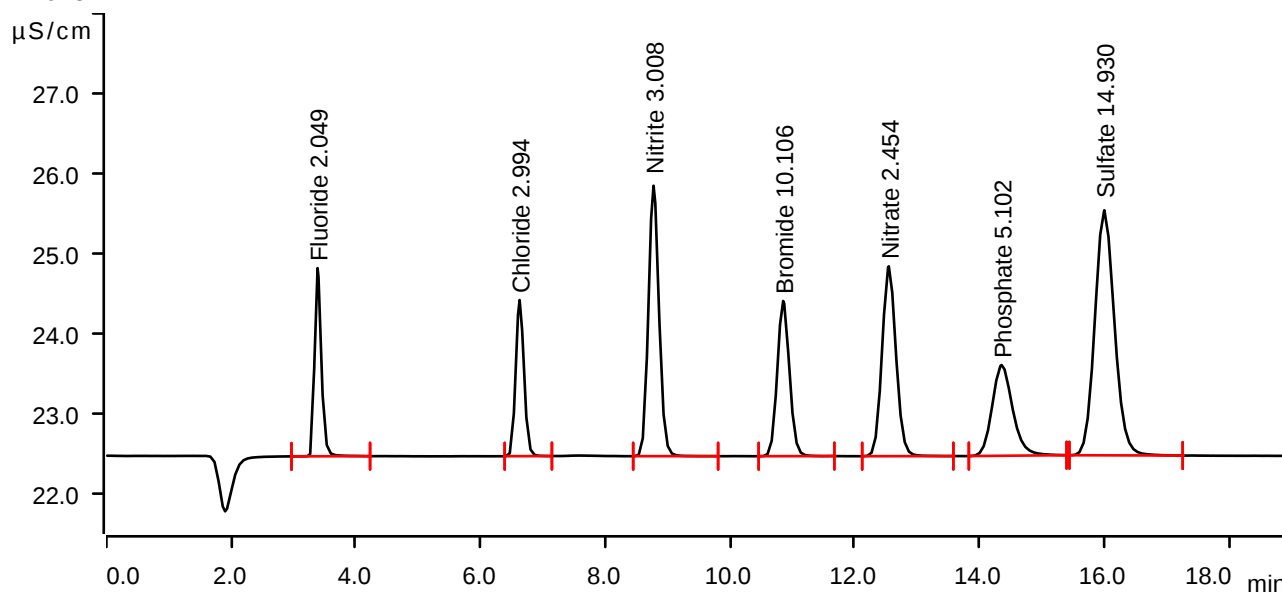

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.387	0.2942	2.351	2.049	Fluoride
2	6.627	0.3003	1.951	2.994	Chloride
3	8.773	0.6679	3.379	3.008	Nitrite
4	10.852	0.4398	1.939	10.106	Bromide
5	12.545	0.6168	2.372	2.454	Nitrate
6	14.353	0.4319	1.134	5.102	Phosphate
7	15.998	1.1186	3.062	14.930	Sulfate

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

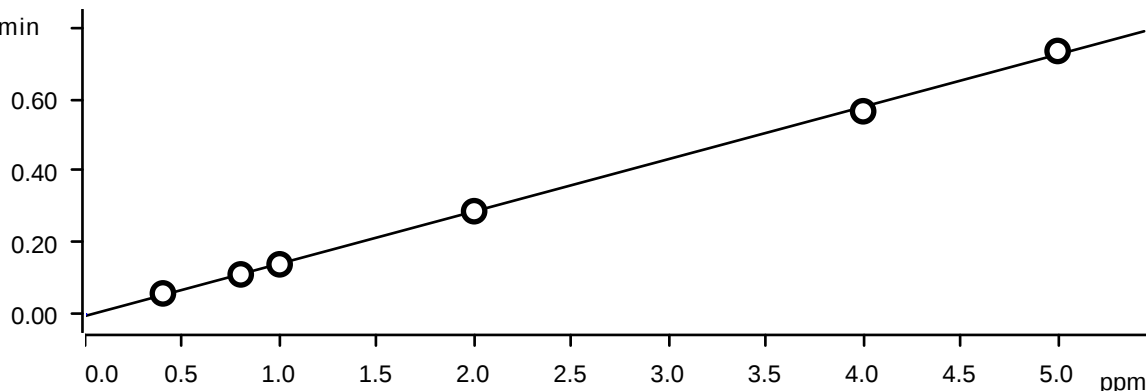

Function: $A = -4.55276\text{E-}3 + 0.0145788 \times Q$


Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

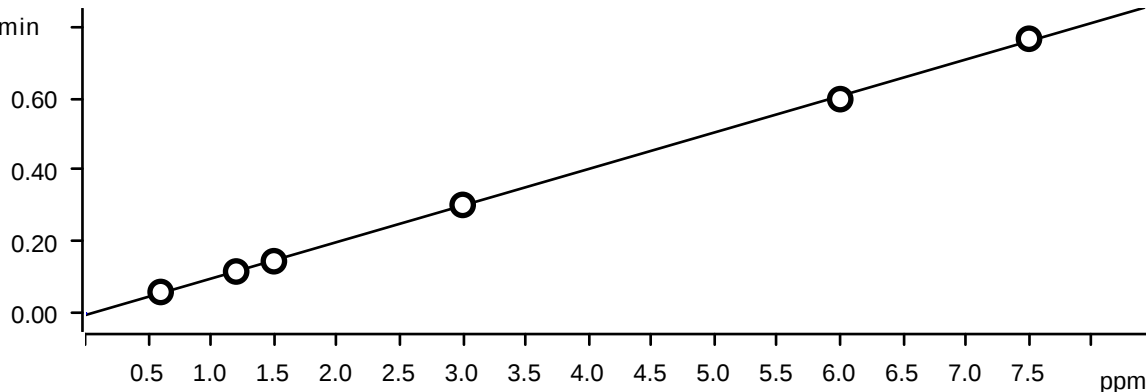

Function: $A = -4.66825\text{E-}3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

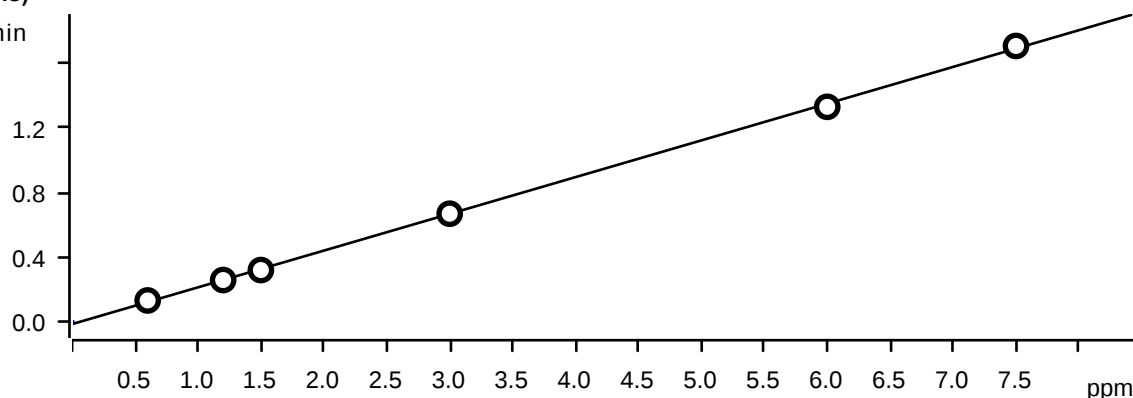
Function: $A = -0.0166933 + 0.0227623 \times Q$

Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

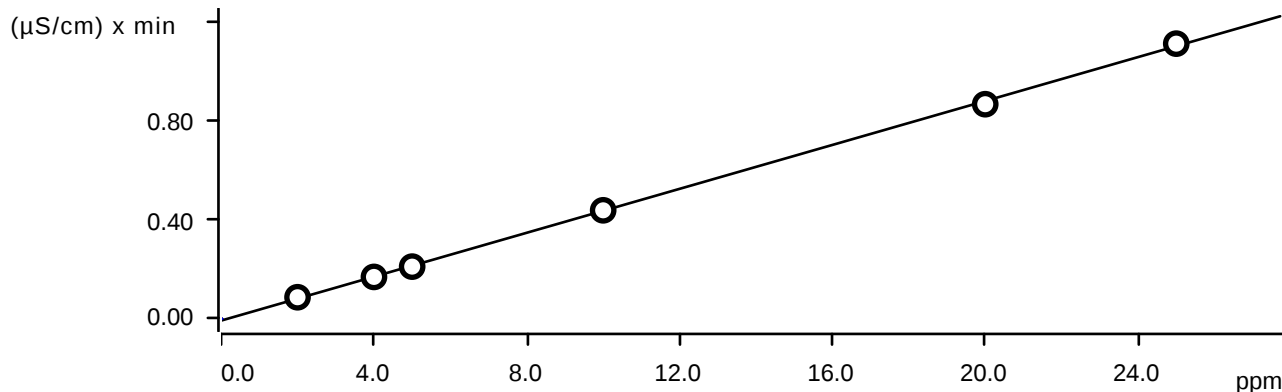


Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$

Relative standard deviation 1.851347 %

Correlation coefficient 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

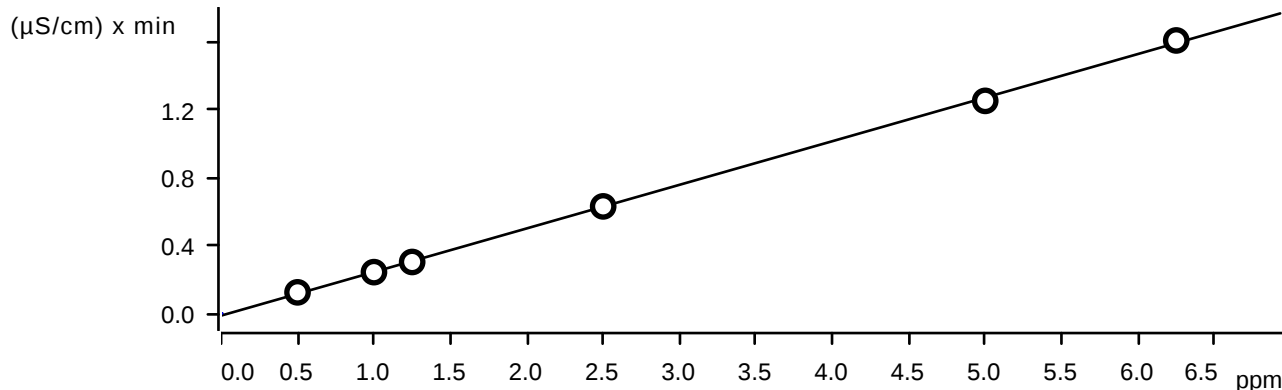


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

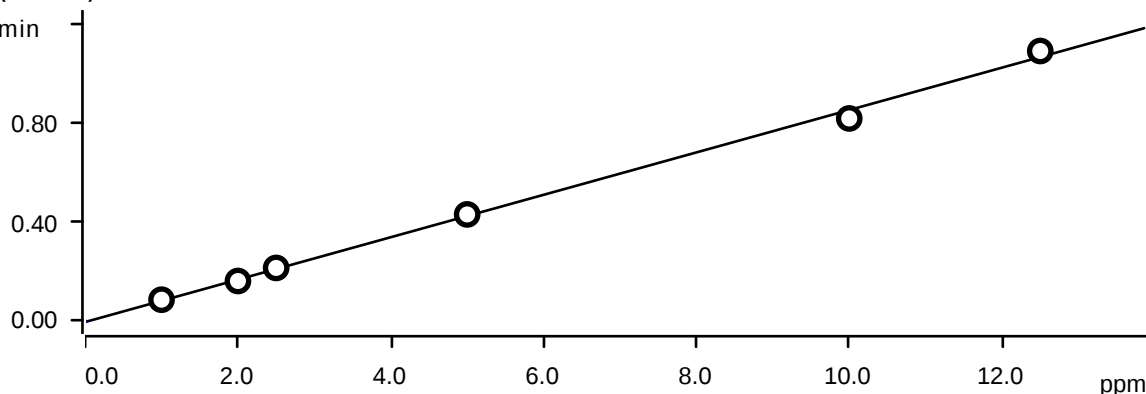
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

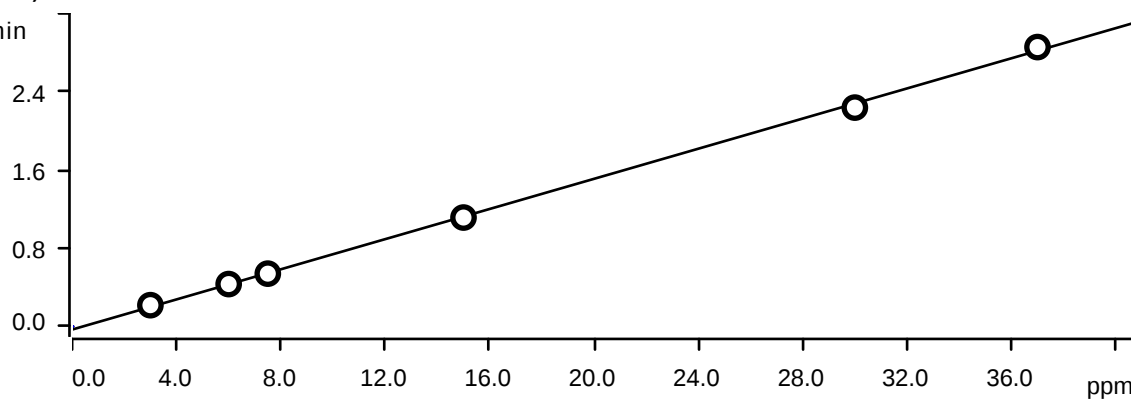 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used

Sample data


Ident CCB
Sample type Sample
Determination start 2025-06-26 09:06:43 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

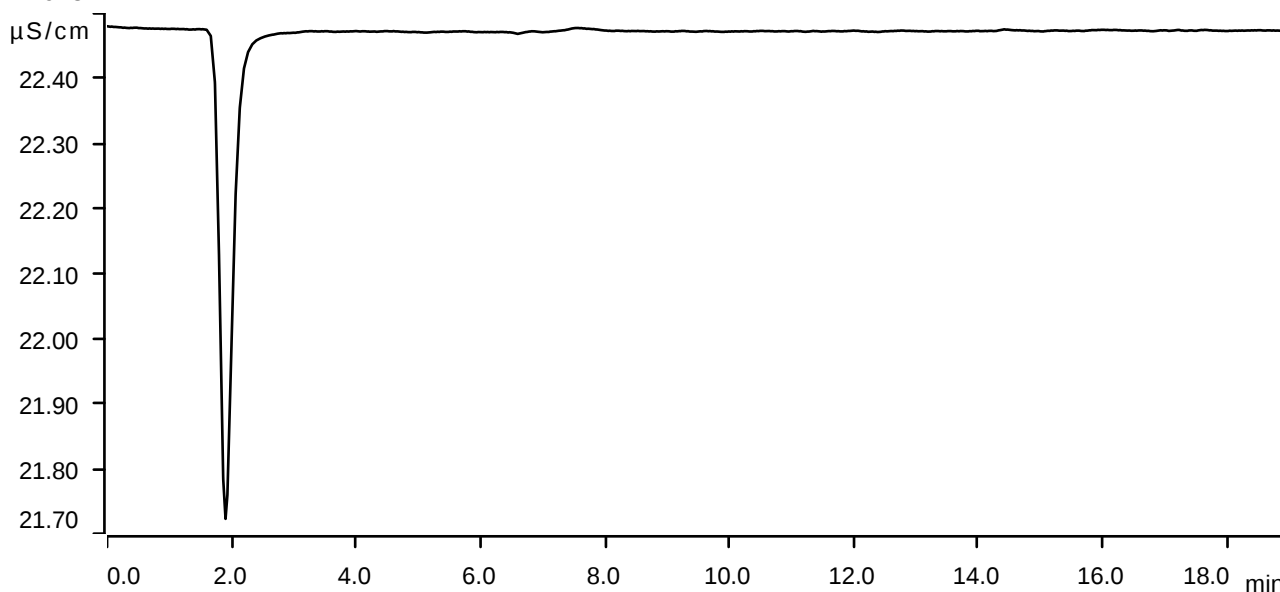Anions

Fluoride (Anions)

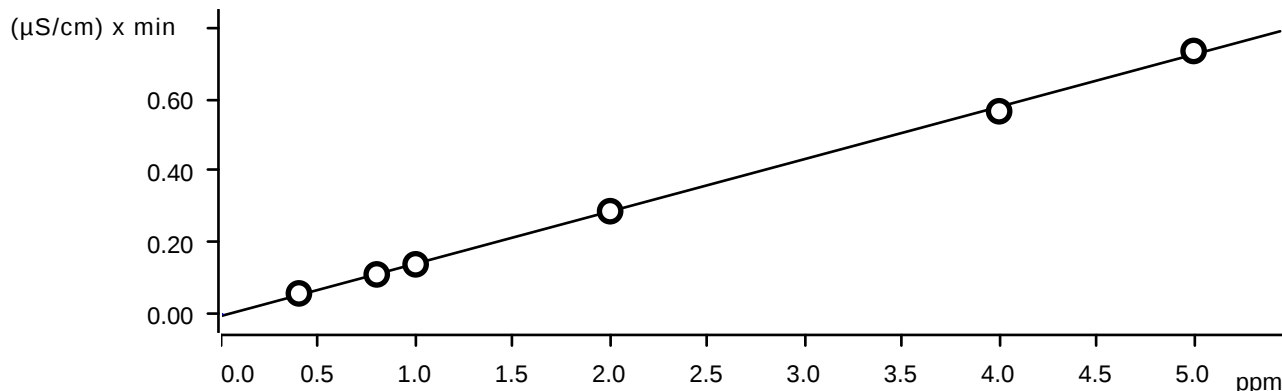


Function: $A = -4.55276E-3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

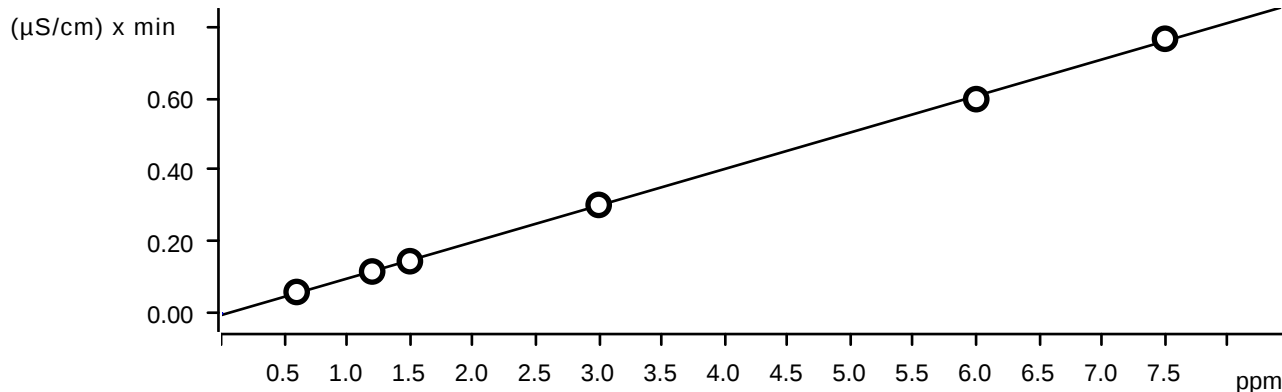

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

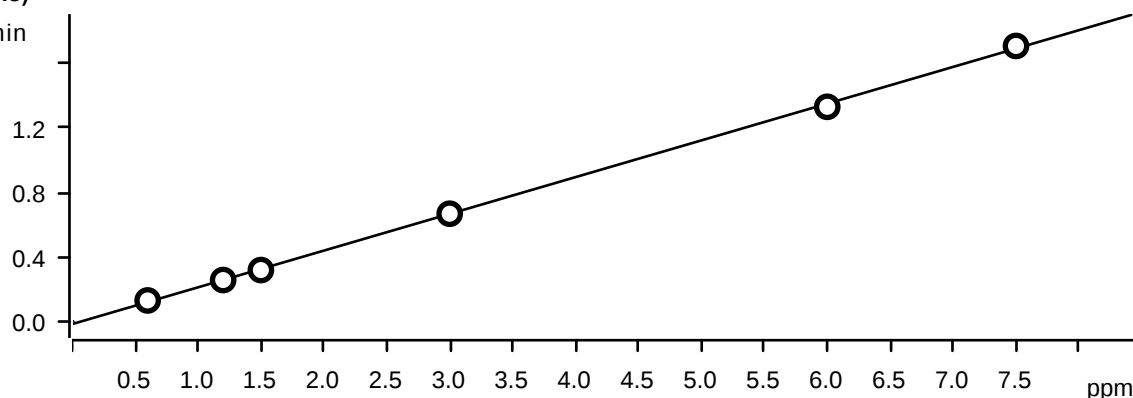
Function: $A = -0.0166933 + 0.0227623 \times Q$

Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

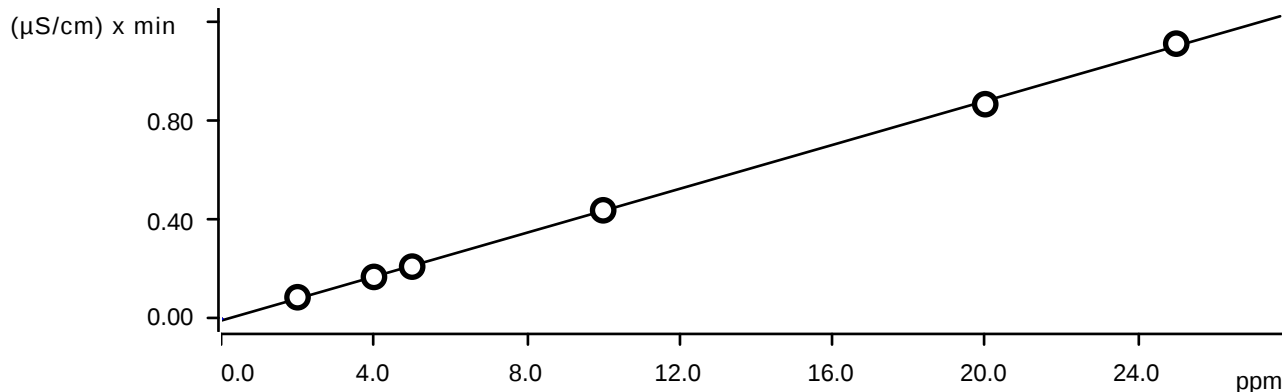


Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$

Relative standard deviation 1.851347 %

Correlation coefficient 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

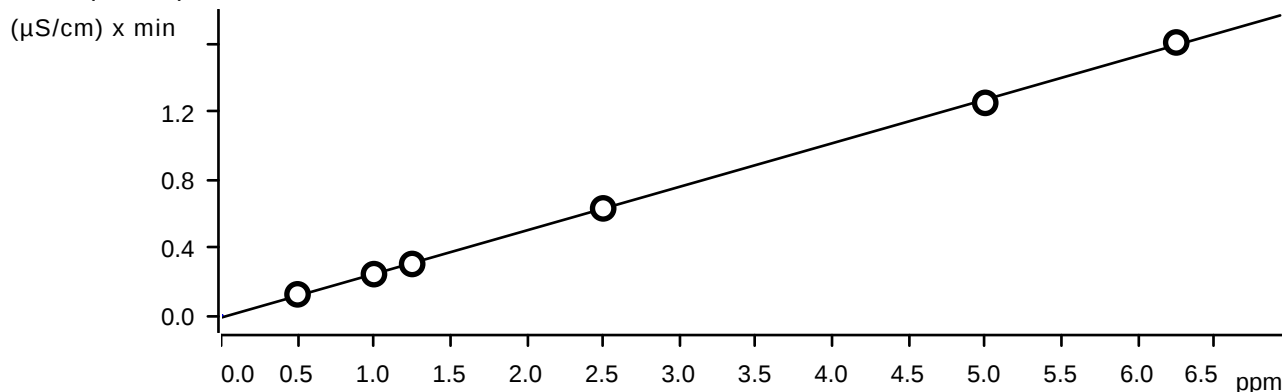


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

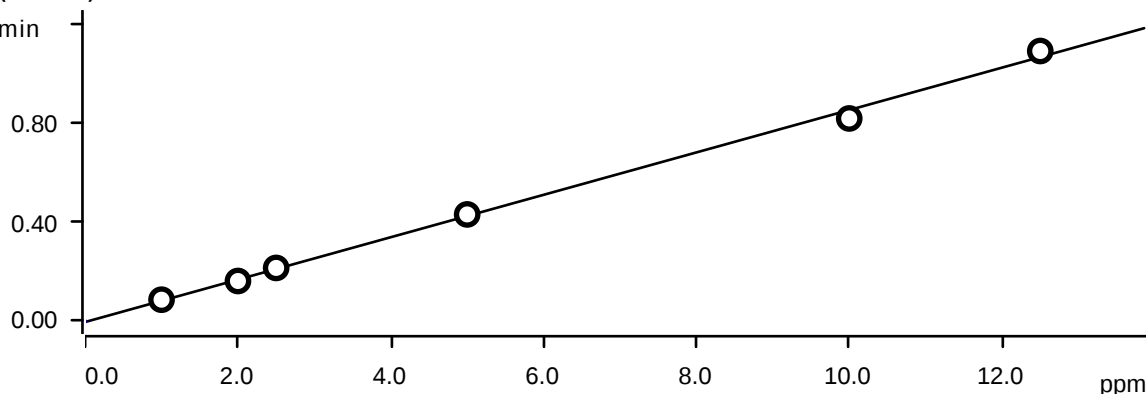
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

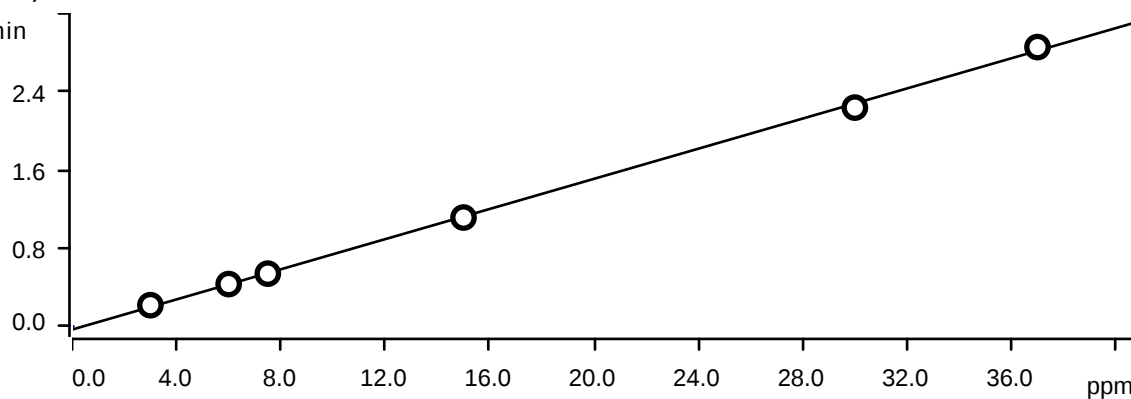 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used

Sample data


Ident LB136282BLS
Sample type Sample
Determination start 2025-06-26 09:28:13 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

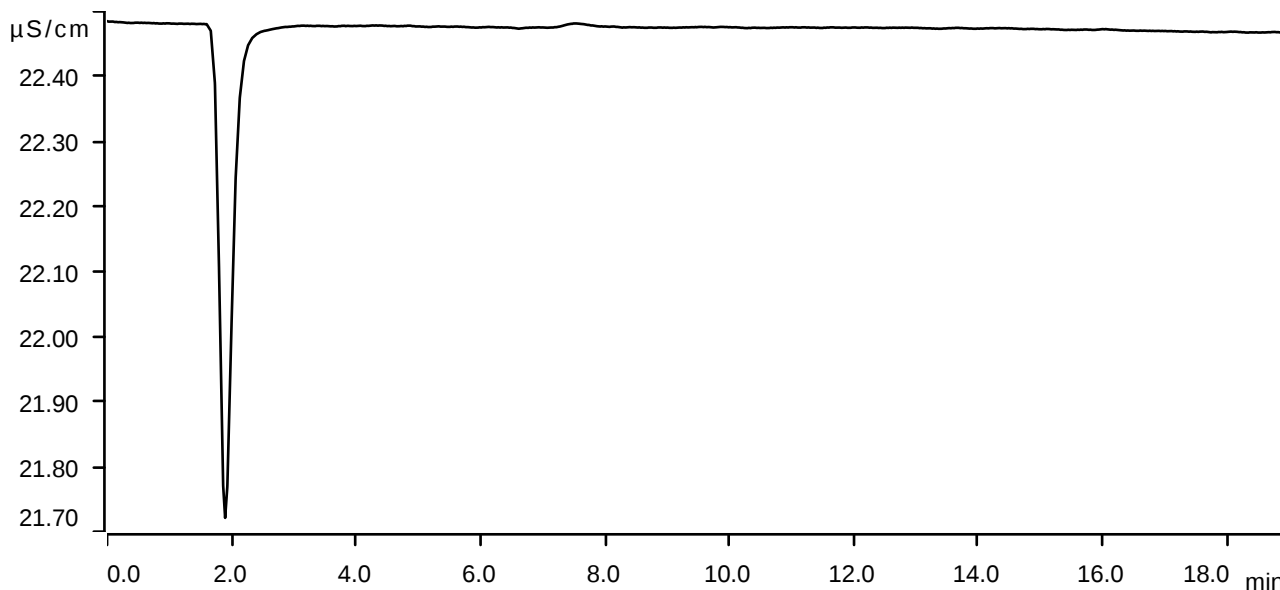Anions

Fluoride (Anions)

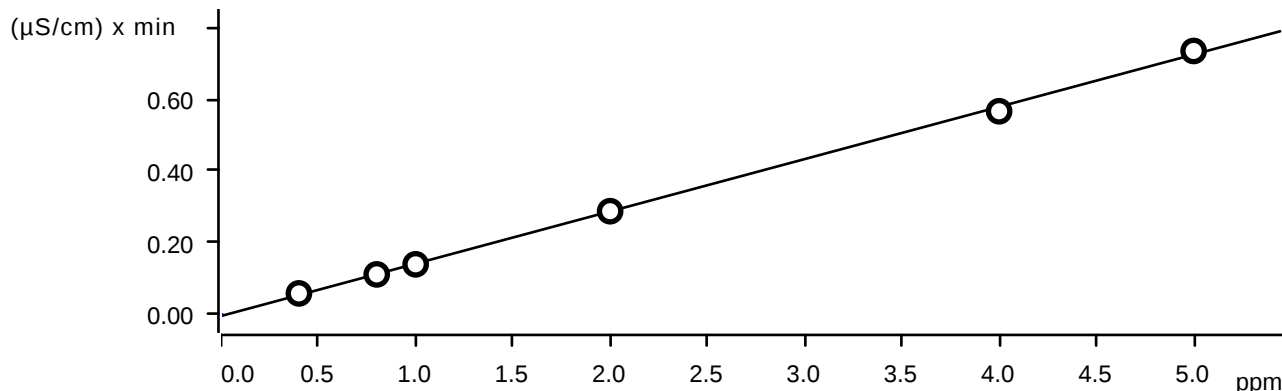


Function: $A = -4.55276E-3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

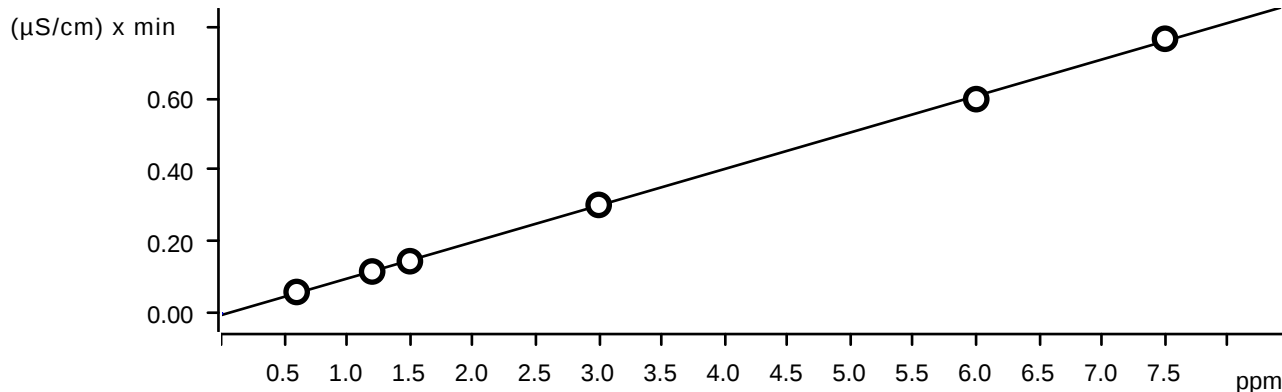

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

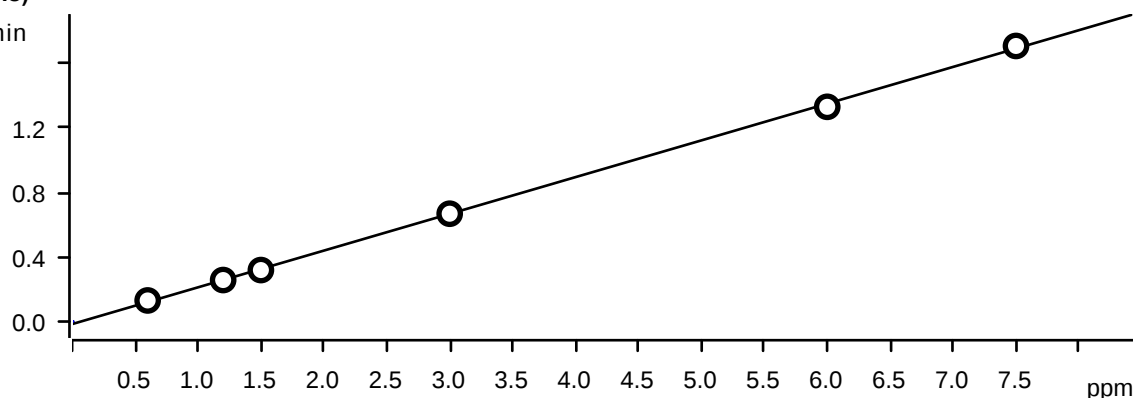
Function: $A = -0.0166933 + 0.0227623 \times Q$

Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

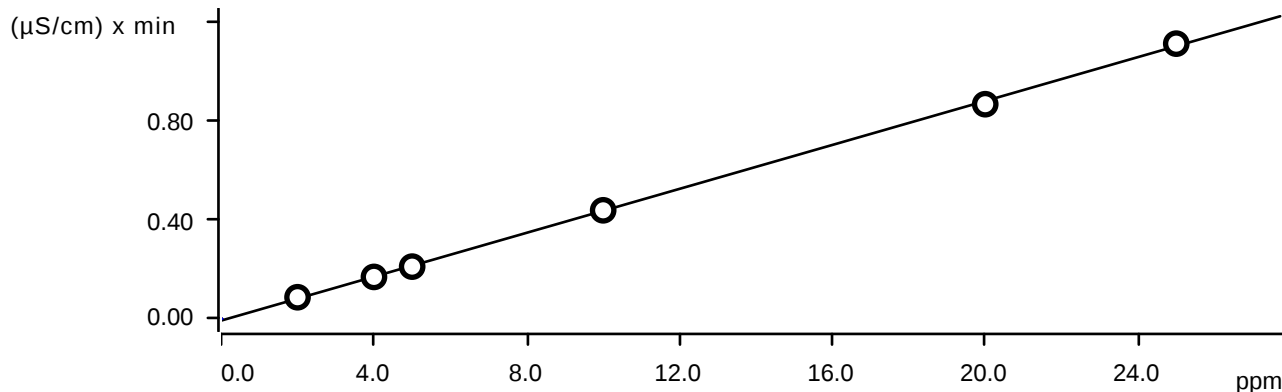


Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$

Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

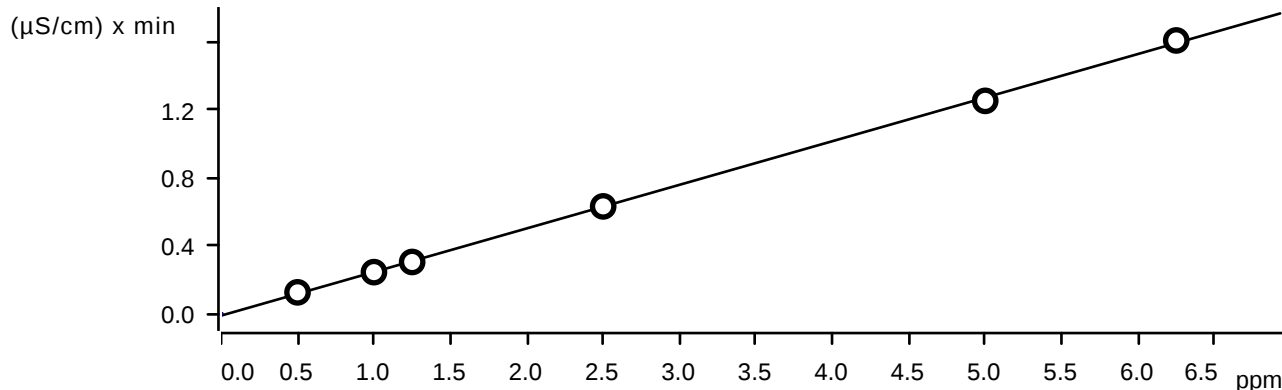


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

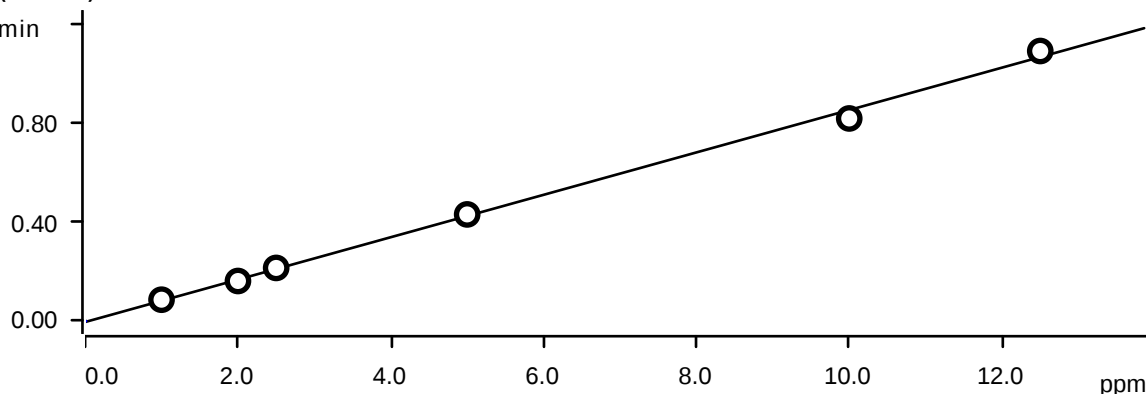
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

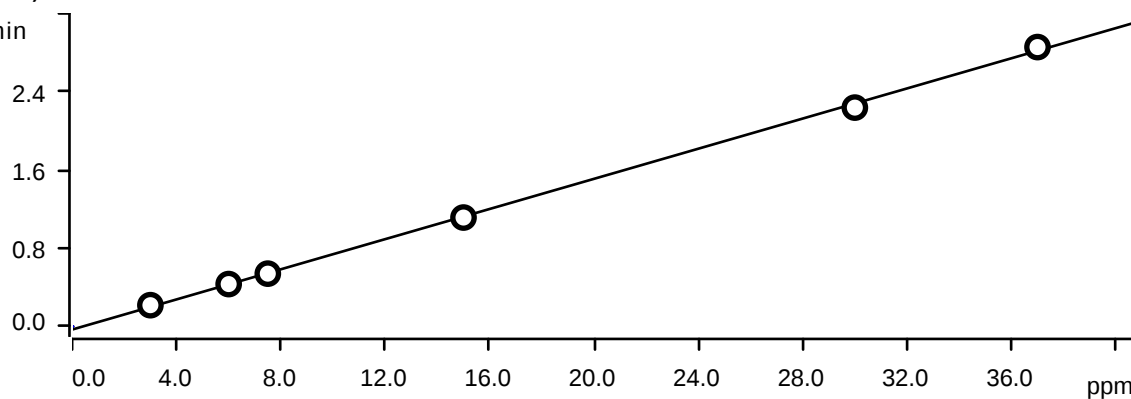 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident LB136282BSS
Sample type Check standard 1
Determination start 2025-06-26 09:49:44 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C


Anions

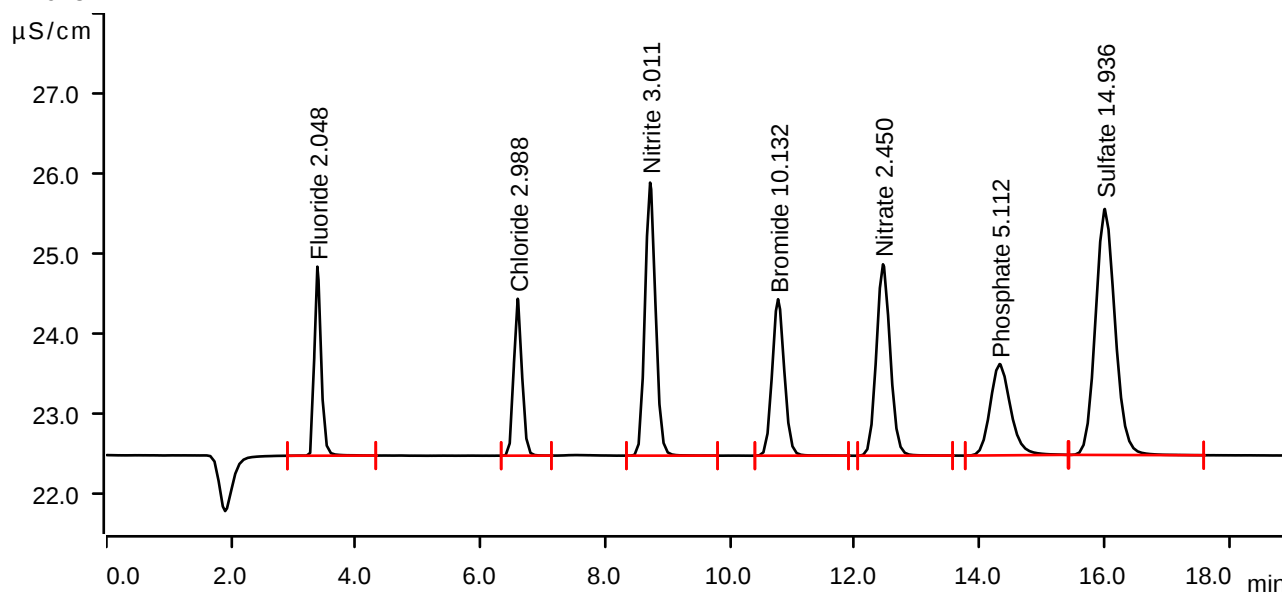

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.383	0.2941	2.361	2.048	Fluoride
2	6.595	0.2997	1.960	2.988	Chloride
3	8.718	0.6687	3.411	3.011	Nitrite
4	10.770	0.4409	1.955	10.132	Bromide
5	12.452	0.6157	2.391	2.450	Nitrate
6	14.322	0.4328	1.141	5.112	Phosphate
7	16.008	1.1191	3.073	14.936	Sulfate

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

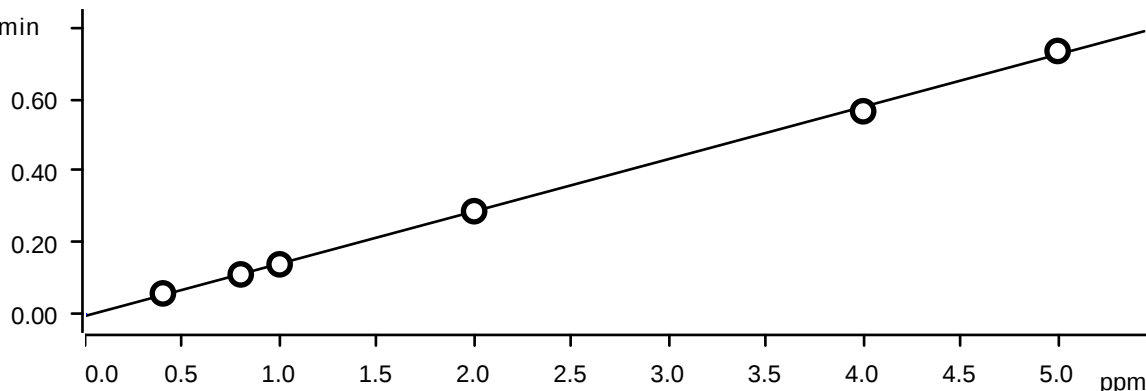

Function: $A = -4.55276E-3 + 0.0145788 \times Q$


Relative standard deviation: 2.633289 %

Correlation coefficient: 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

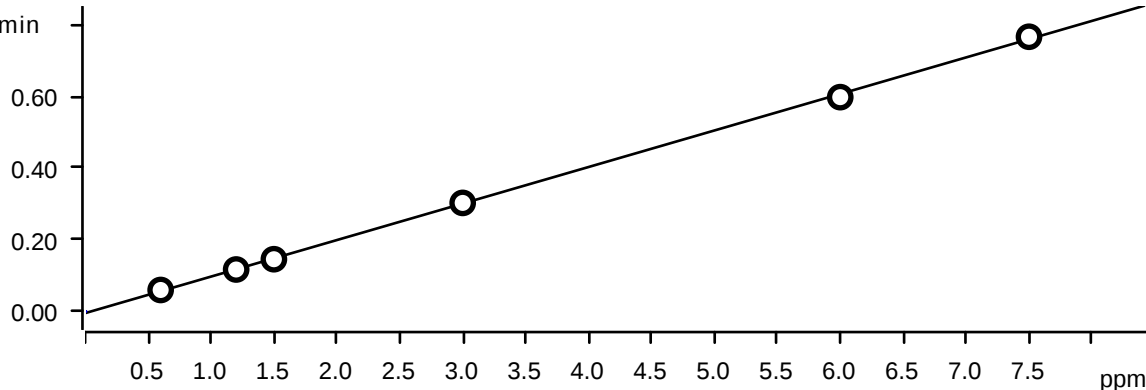

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

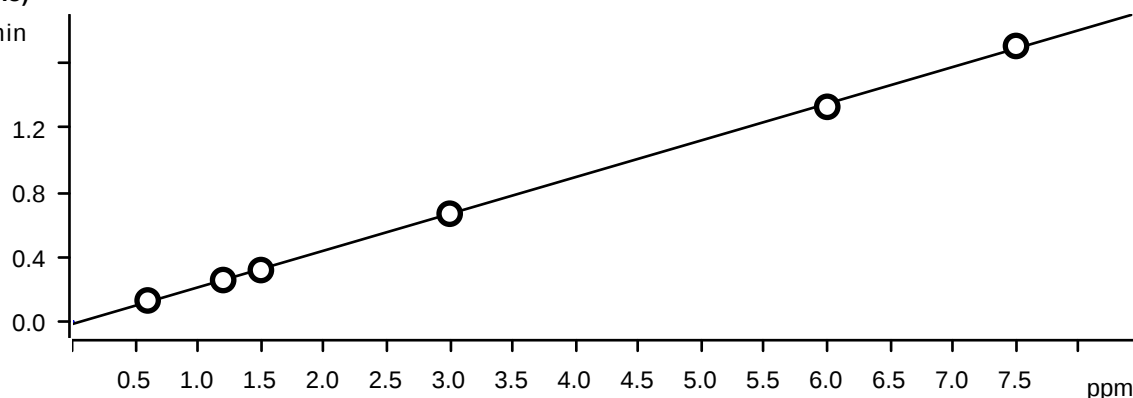
Function: $A = -0.0166933 + 0.0227623 \times Q$

Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

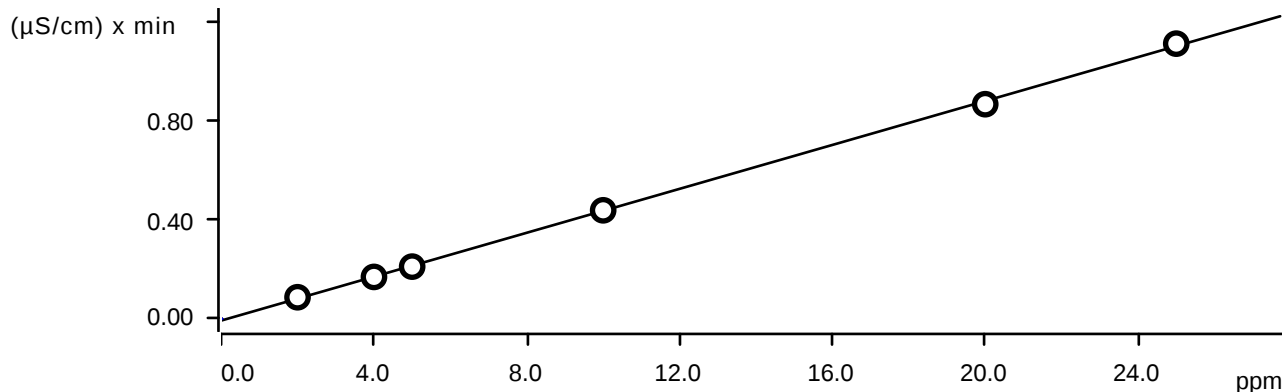


Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$

Relative standard deviation 1.851347 %

Correlation coefficient 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

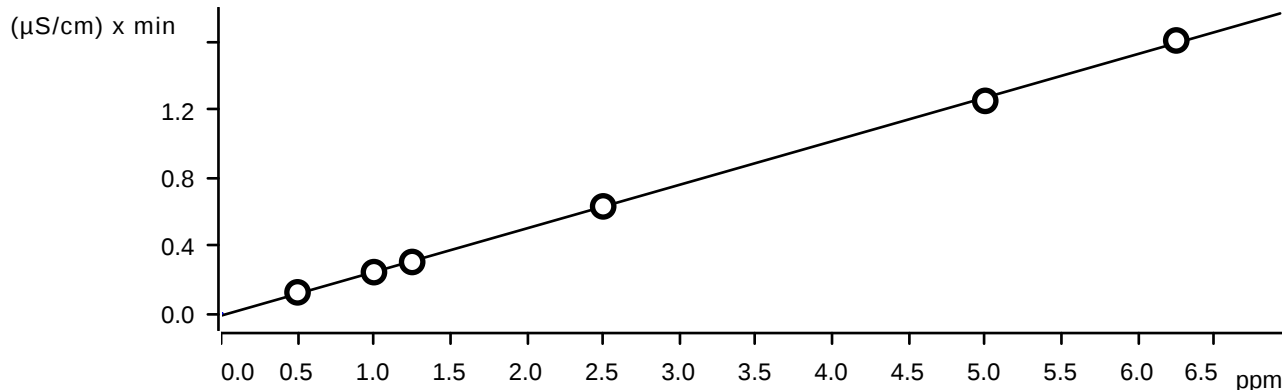


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

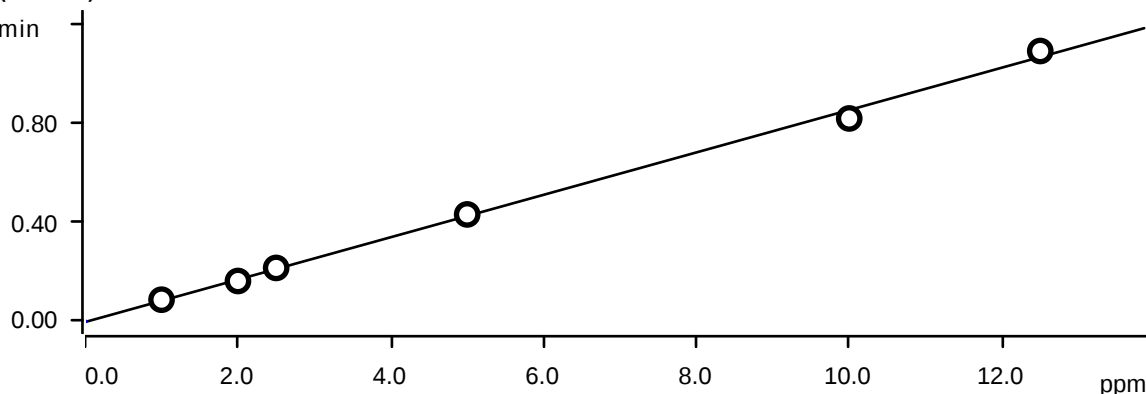
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

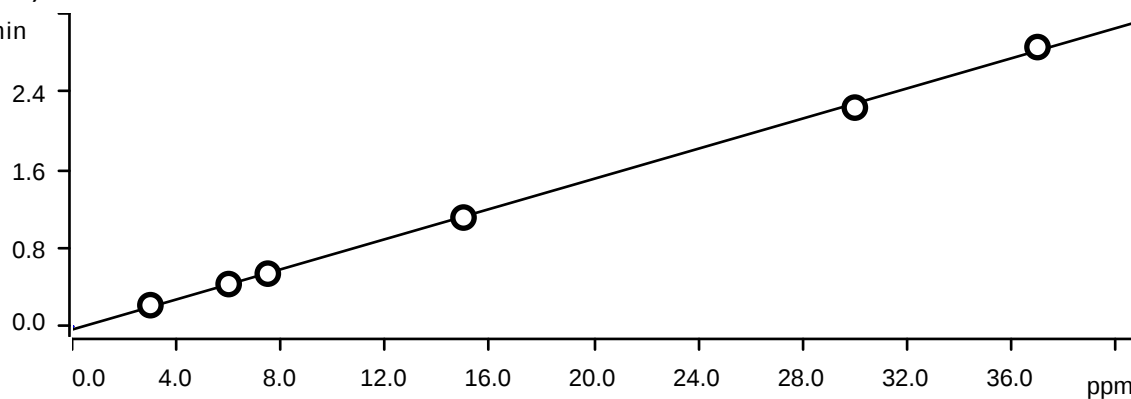 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident Q2425-01
Sample type Sample
Determination start 2025-06-26 10:27:26 UTC-4
Method IC1-062325
Operator

Anions


Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

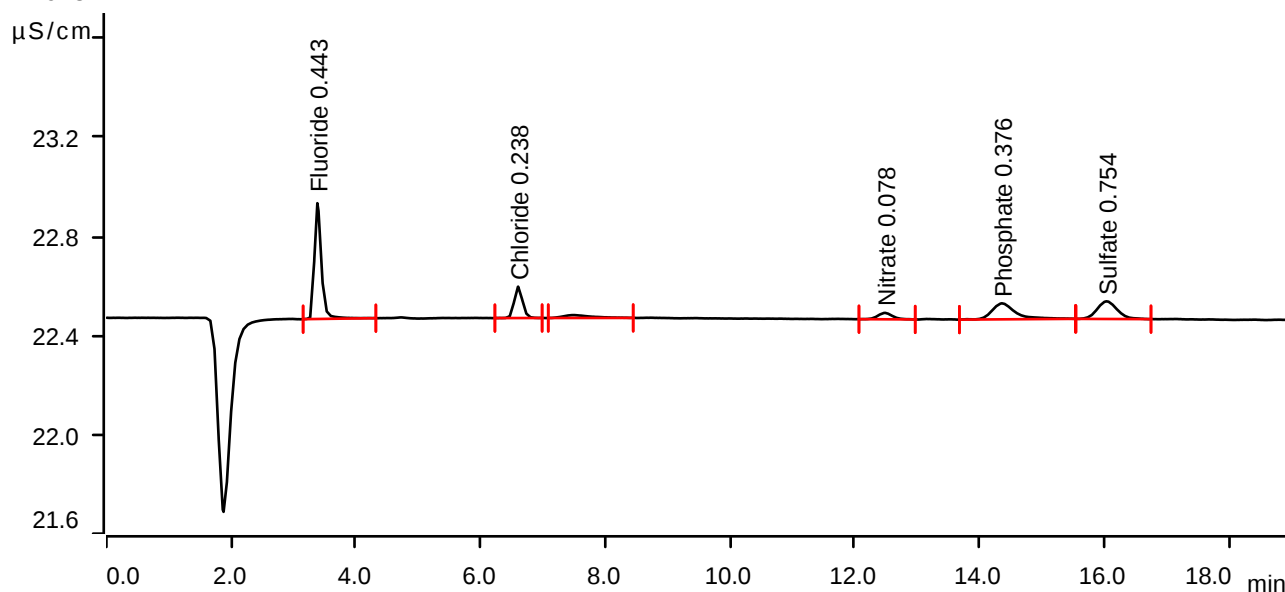

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.383	0.0600	0.467	0.443	Fluoride
2	6.603	0.0196	0.126	0.238	Chloride
3	7.508	0.0061	0.012	invalid	
4	12.488	0.0070	0.026	0.078	Nitrate
5	14.358	0.0285	0.065	0.376	Phosphate
6	16.033	0.0266	0.071	0.754	Sulfate

Fluoride (Anions)

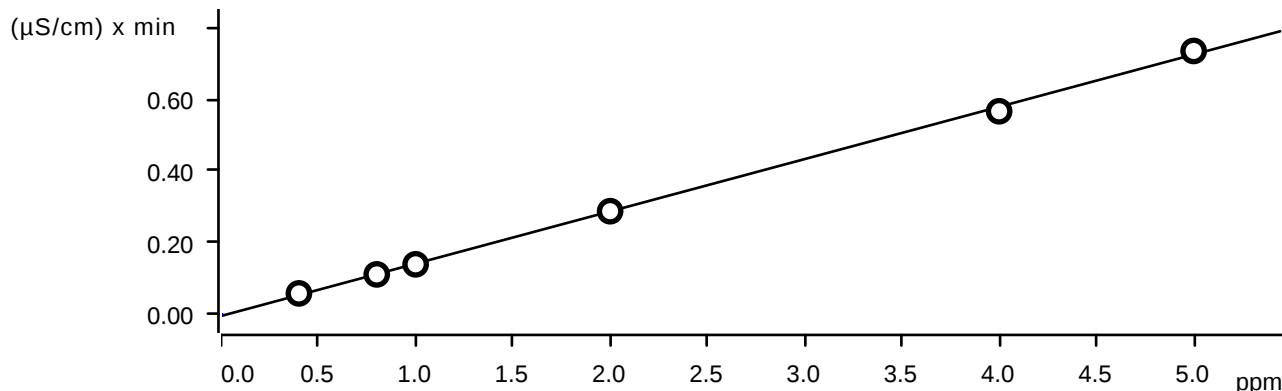


Function: $A = -4.55276E-3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

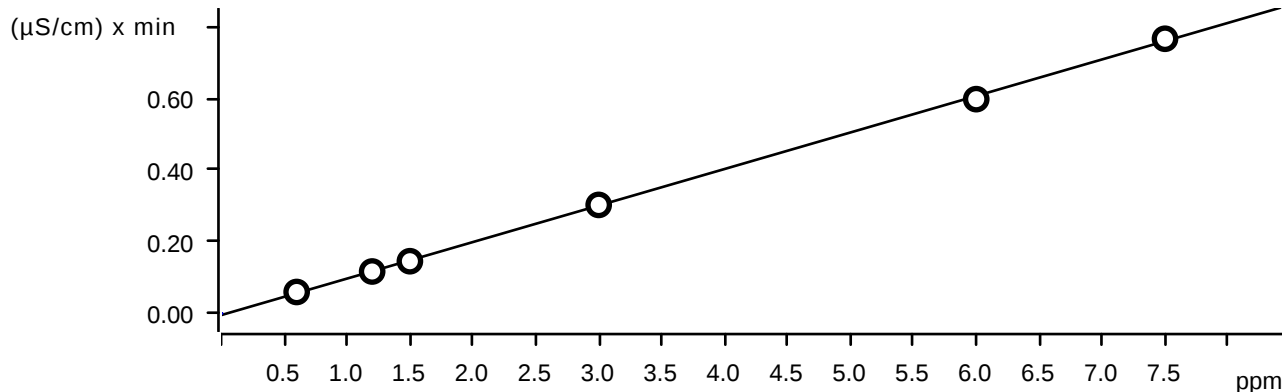

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

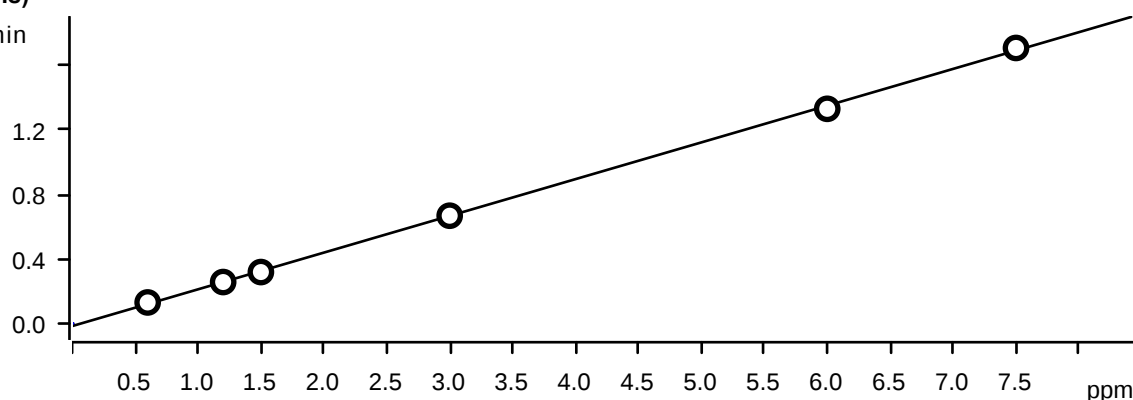
Function: $A = -0.0166933 + 0.0227623 \times Q$

Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

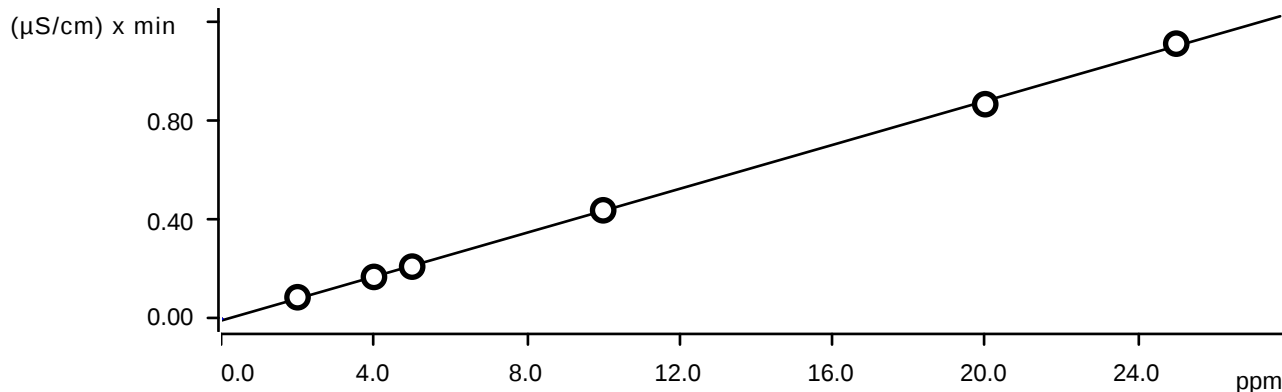


Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$

Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

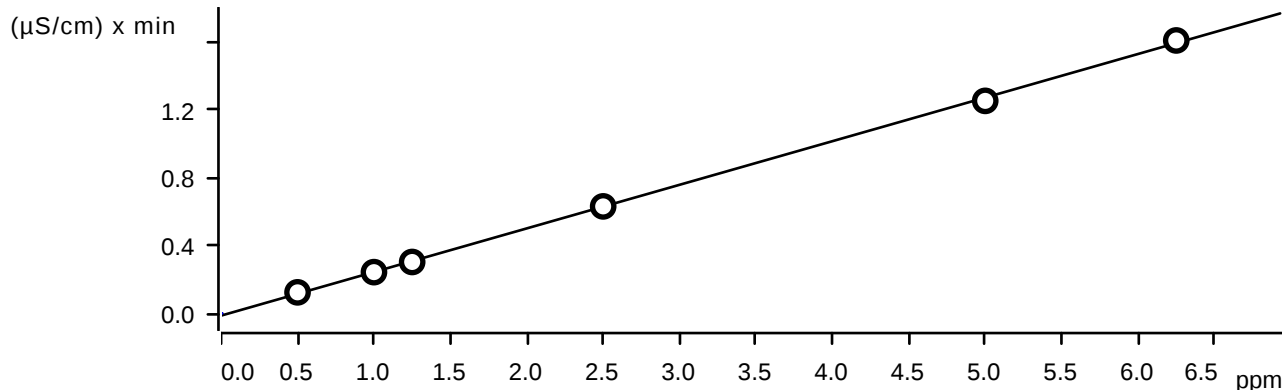


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

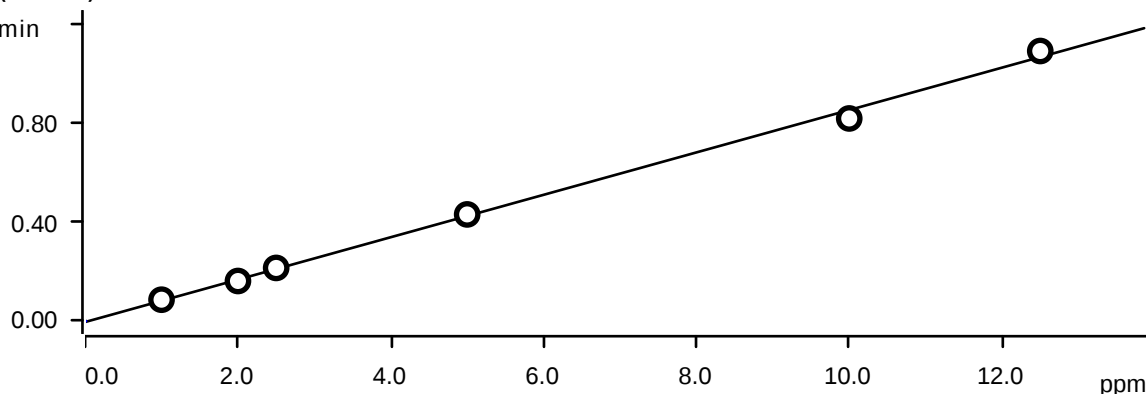
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

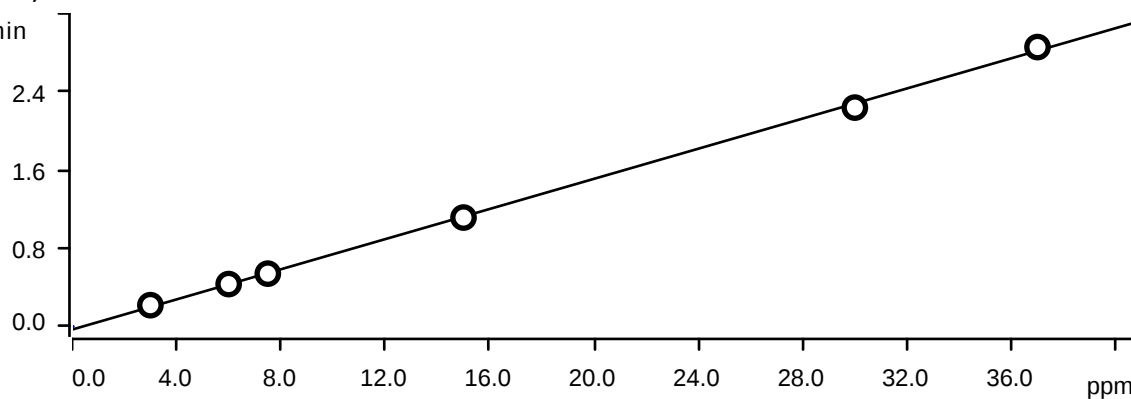 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident Q2425-01MS
Sample type Sample
Determination start 2025-06-26 10:49:04 UTC-4
Method IC1-062325
Operator


Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

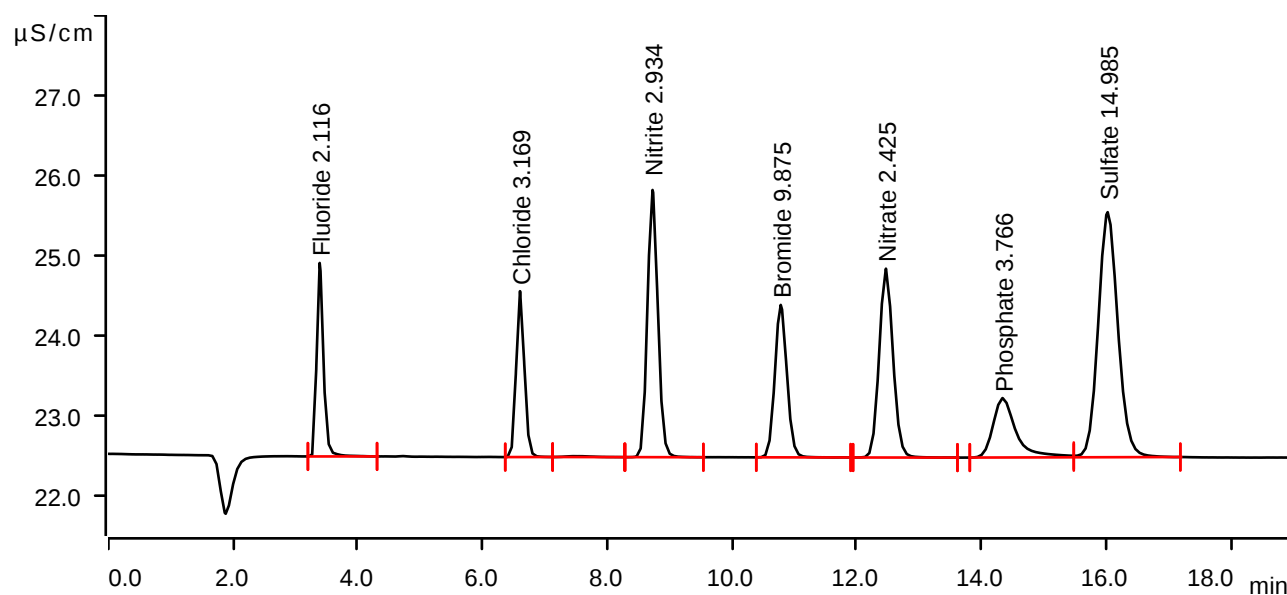


Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.388	0.3039	2.417	2.116	Fluoride
2	6.602	0.3180	2.072	3.169	Chloride
3	7.493	0.0052	0.011	invalid	
4	8.725	0.6511	3.339	2.934	Nitrite
5	10.780	0.4296	1.905	9.875	Bromide
6	12.465	0.6093	2.359	2.425	Nitrate
7	14.338	0.3179	0.742	3.766	Phosphate
8	16.022	1.1228	3.062	14.985	Sulfate

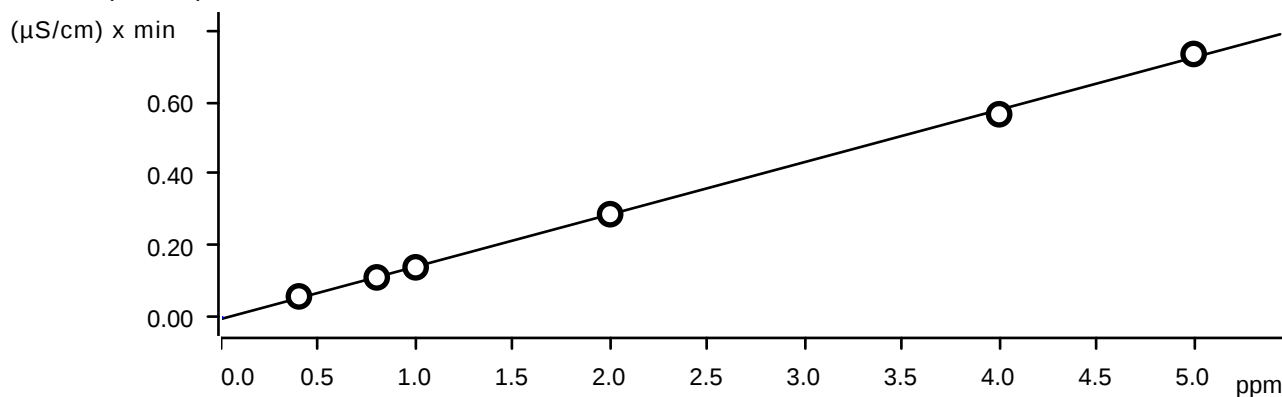Fluoride (Anions)Function: $A = -4.55276\text{E-}3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

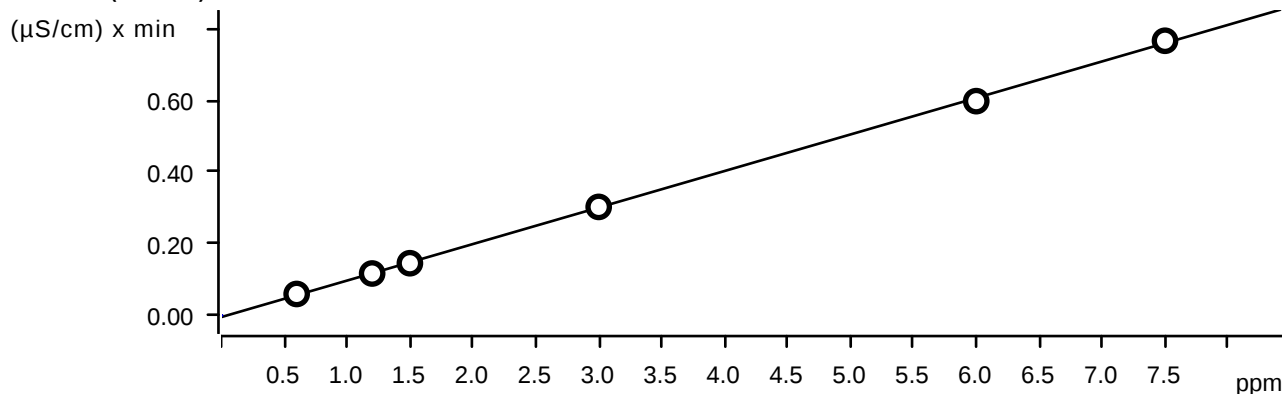Chloride (Anions)Function: $A = -4.66825\text{E-}3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

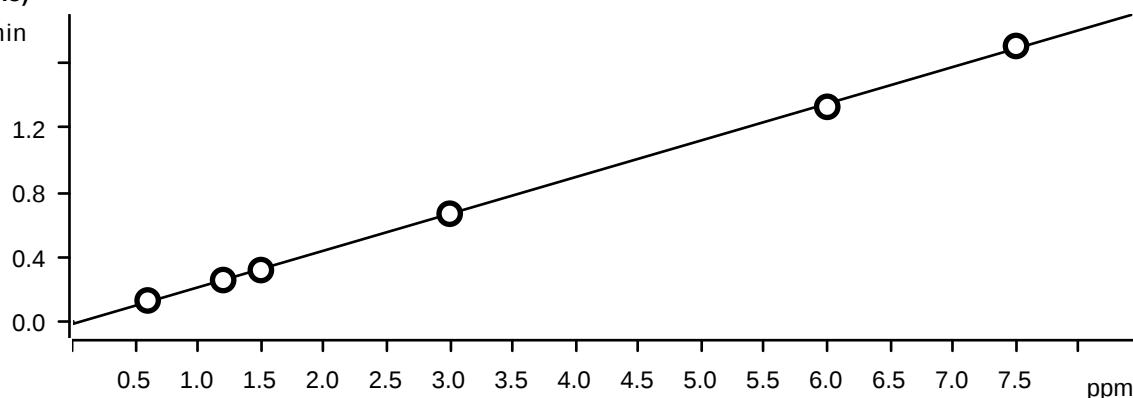Function: $A = -0.0166933 + 0.0227623 \times Q$


Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

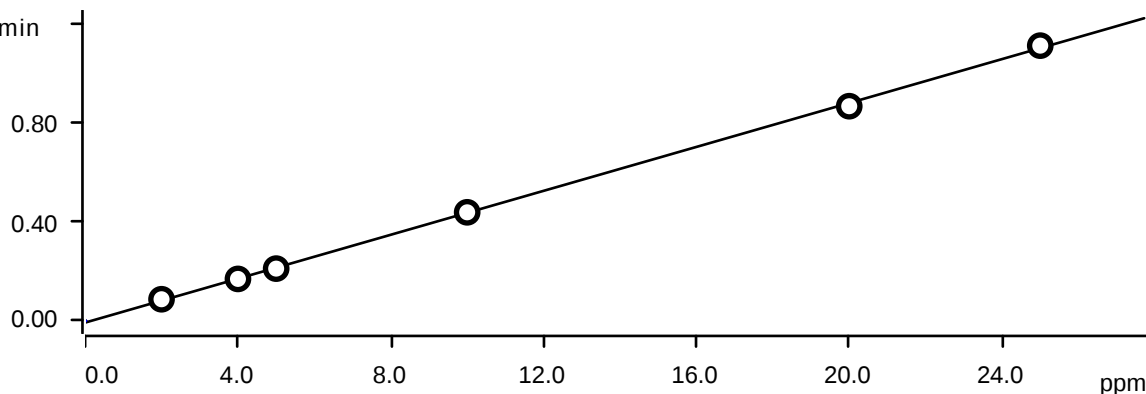

Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$


Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

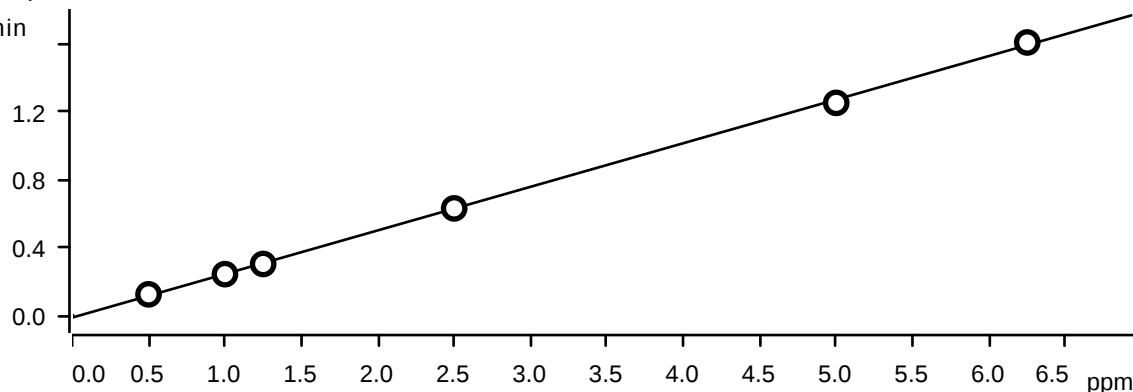


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

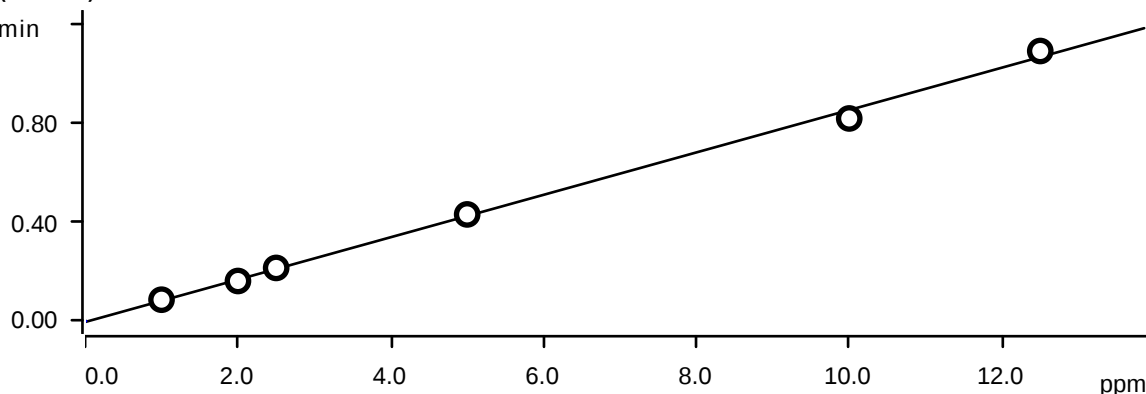
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

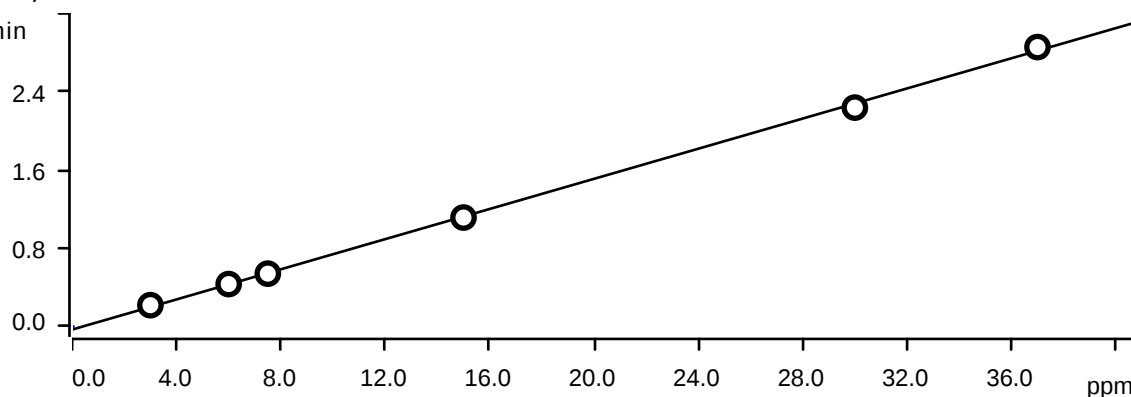 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident Q2425-01MSD
Sample type Sample
Determination start 2025-06-26 11:10:37 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C


Anions

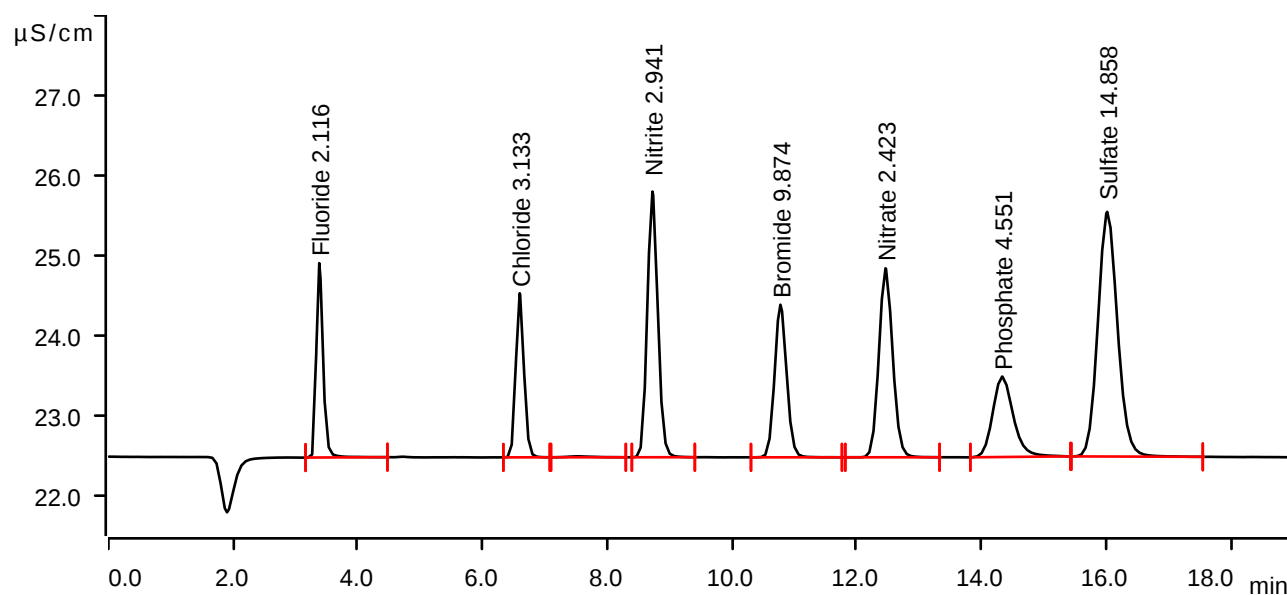

Peak number	Retention time min	Area ($\mu\text{S}/\text{cm}$) x min	Height $\mu\text{S}/\text{cm}$	Concentration ppm	Component name
1	3.382	0.3039	2.428	2.116	Fluoride
2	6.595	0.3144	2.050	3.133	Chloride
3	7.512	0.0053	0.012	invalid	
4	8.723	0.6529	3.320	2.941	Nitrite
5	10.775	0.4296	1.907	9.874	Bromide
6	12.460	0.6088	2.361	2.423	Nitrate
7	14.330	0.3849	1.005	4.551	Phosphate
8	16.015	1.1131	3.057	14.858	Sulfate

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

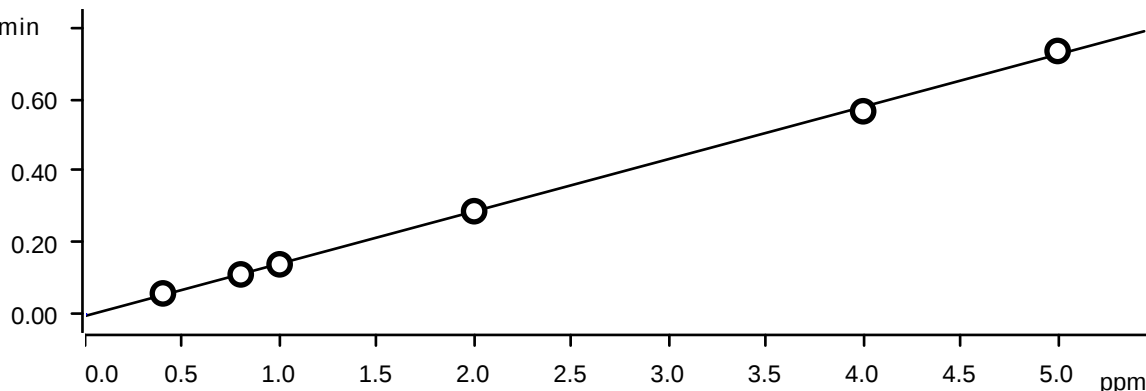

Function: $A = -4.55276E-3 + 0.0145788 \times Q$


Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

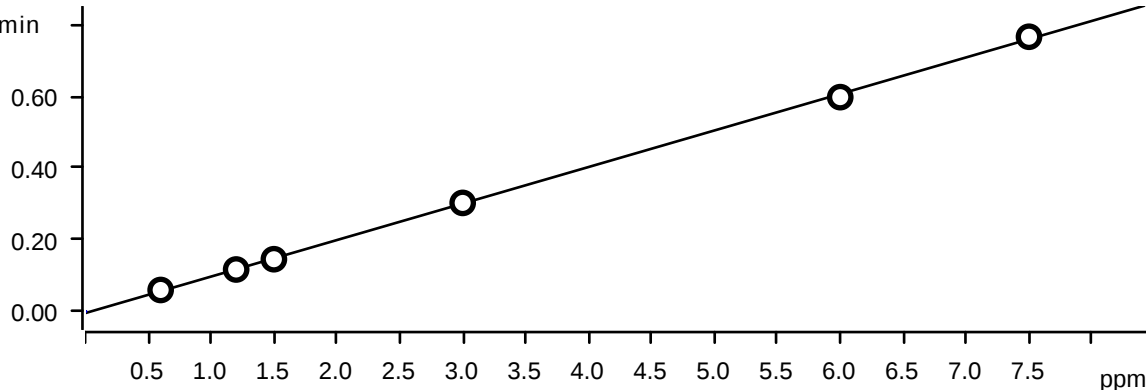

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

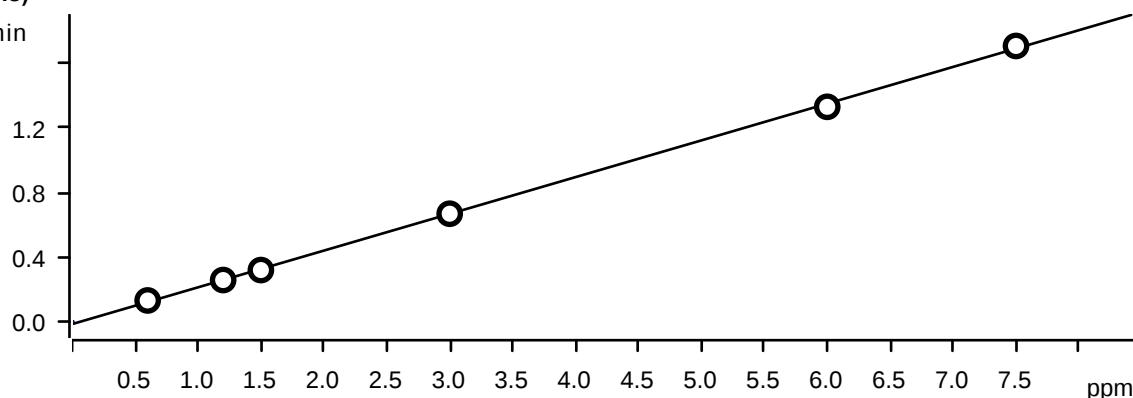
Function: $A = -0.0166933 + 0.0227623 \times Q$

Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

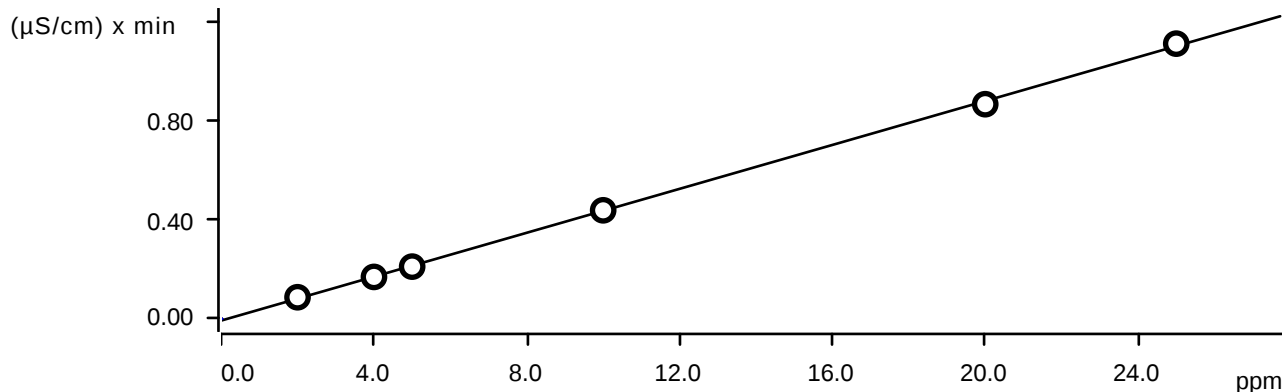


Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$

Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

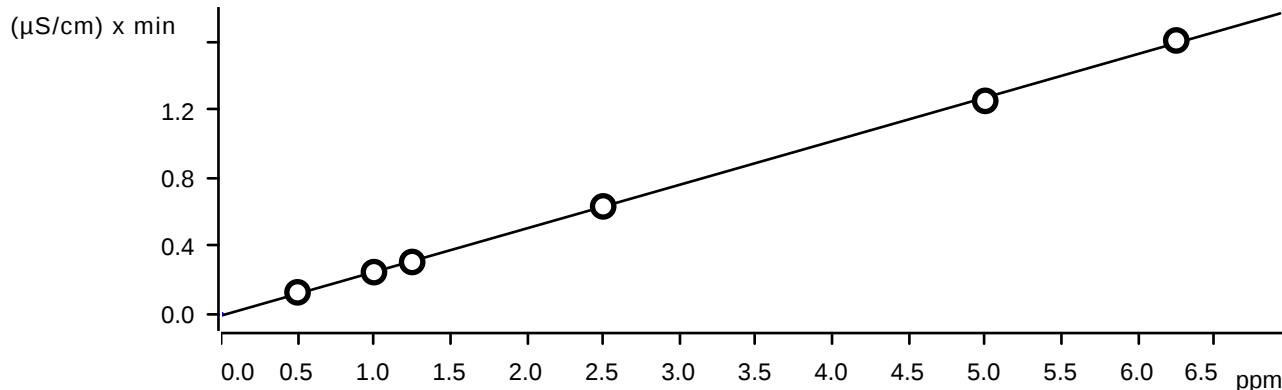


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

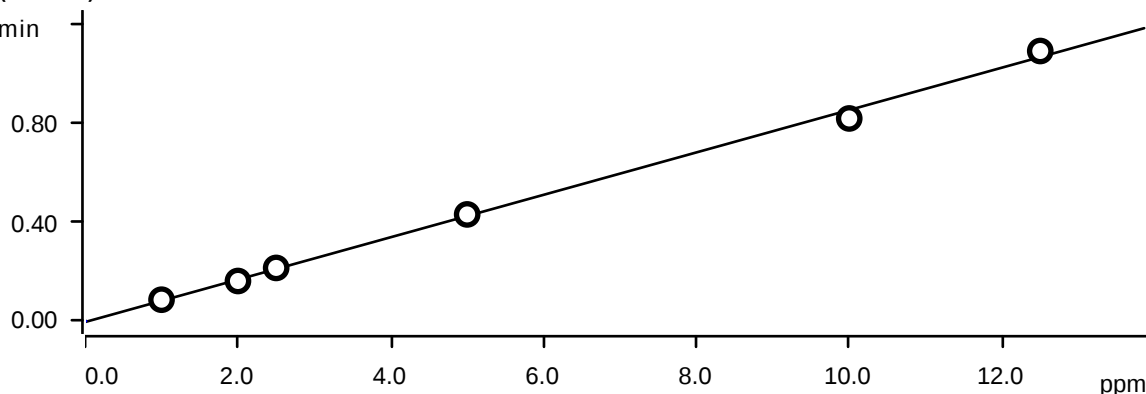
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

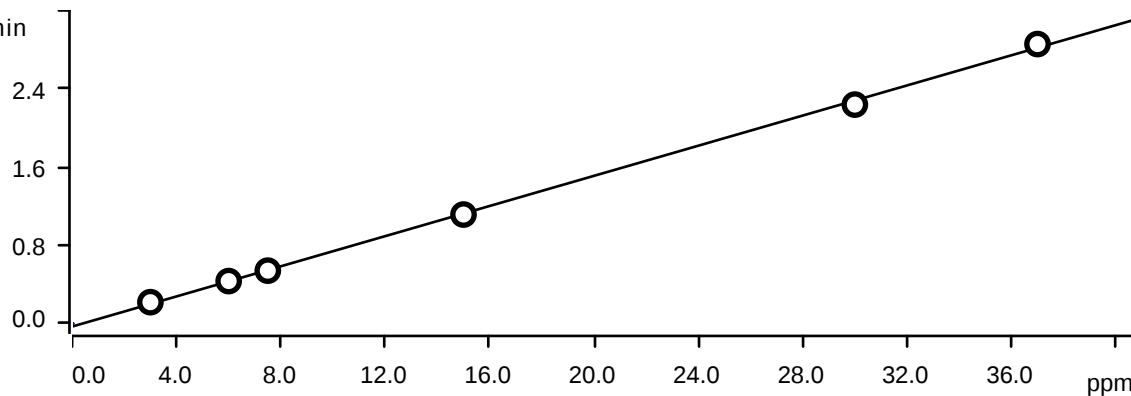 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident Q2425-02
Sample type Sample
Determination start 2025-06-26 11:32:11 UTC-4
Method IC1-062325
Operator

Anions


Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

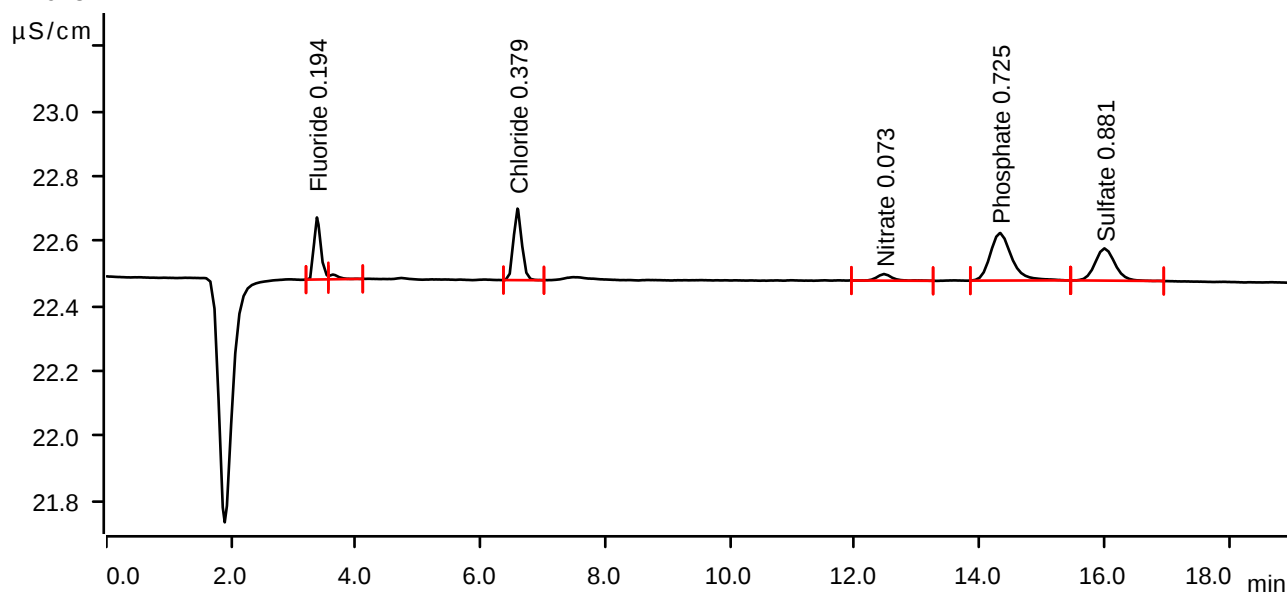

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.377	0.0238	0.191	0.194	Fluoride
2	3.635	0.0025	0.014	invalid	
3	6.592	0.0339	0.220	0.379	Chloride
4	12.468	0.0057	0.020	0.073	Nitrate
5	14.327	0.0583	0.146	0.725	Phosphate
6	16.003	0.0364	0.099	0.881	Sulfate

Fluoride (Anions)

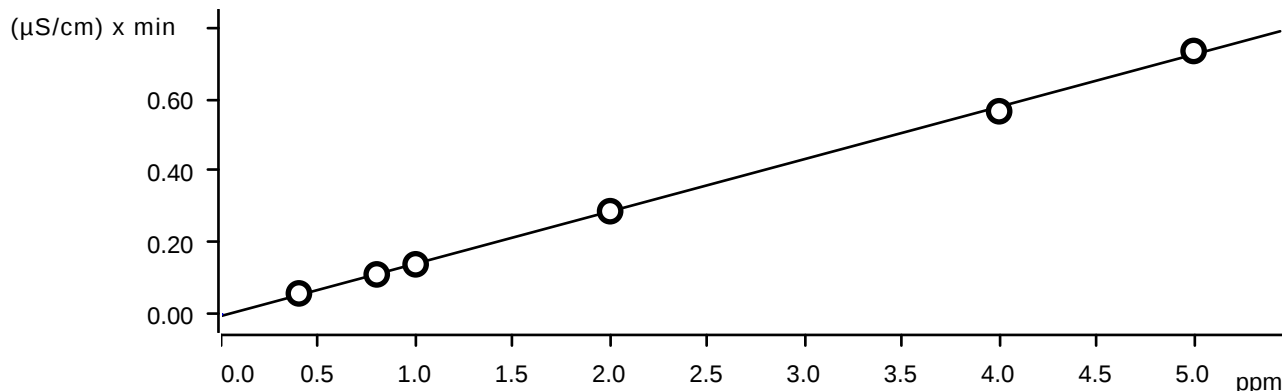


Function: $A = -4.55276E-3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

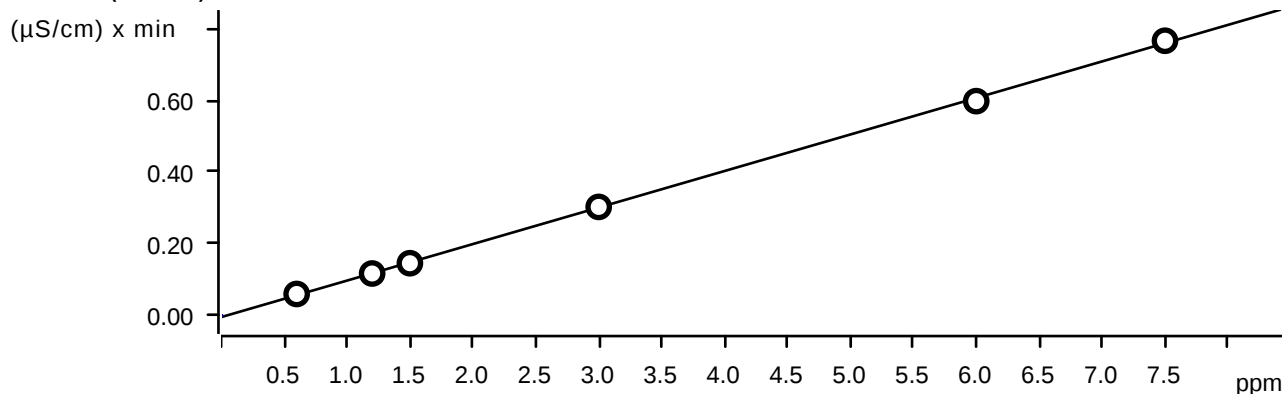

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

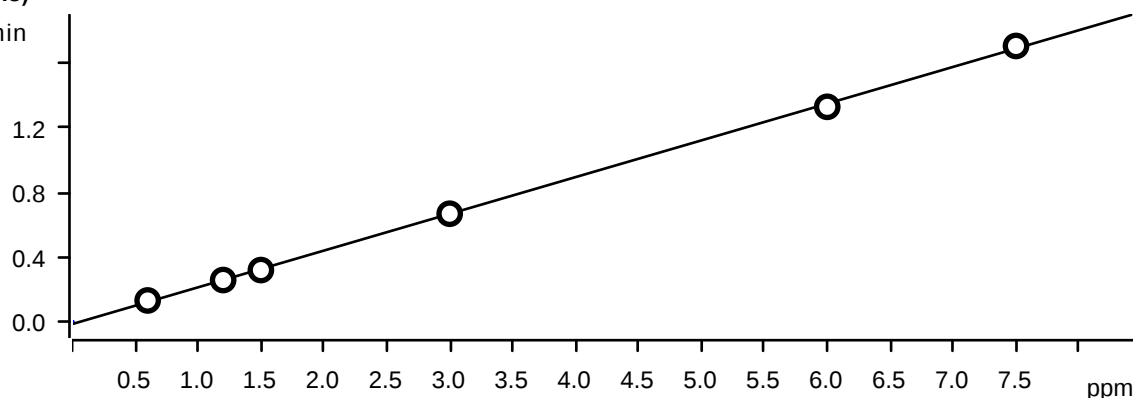Function: $A = -0.0166933 + 0.0227623 \times Q$


Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

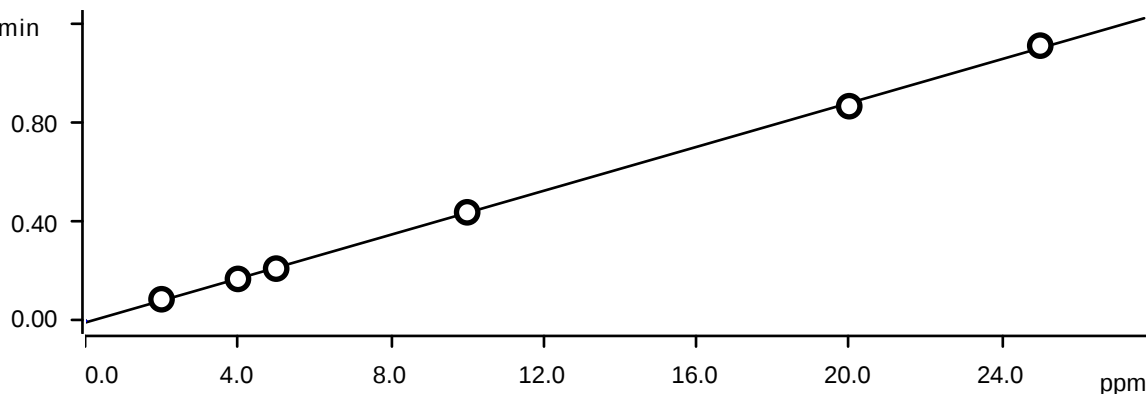

Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$


Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

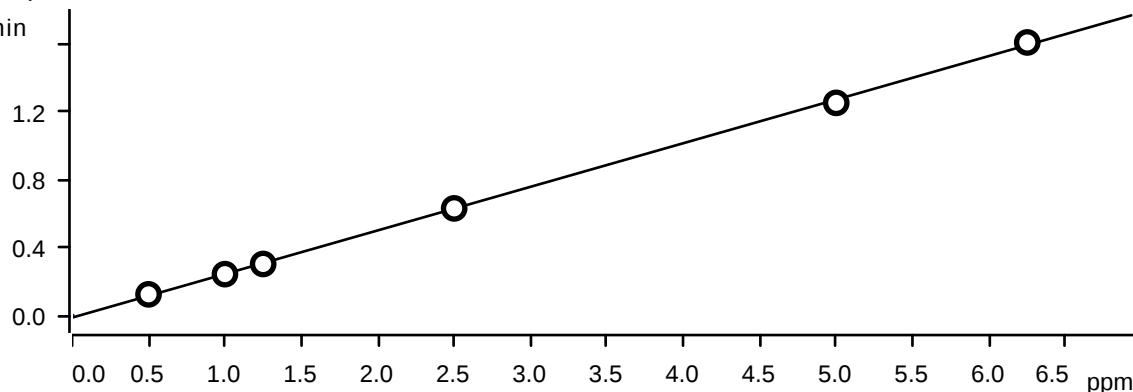


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

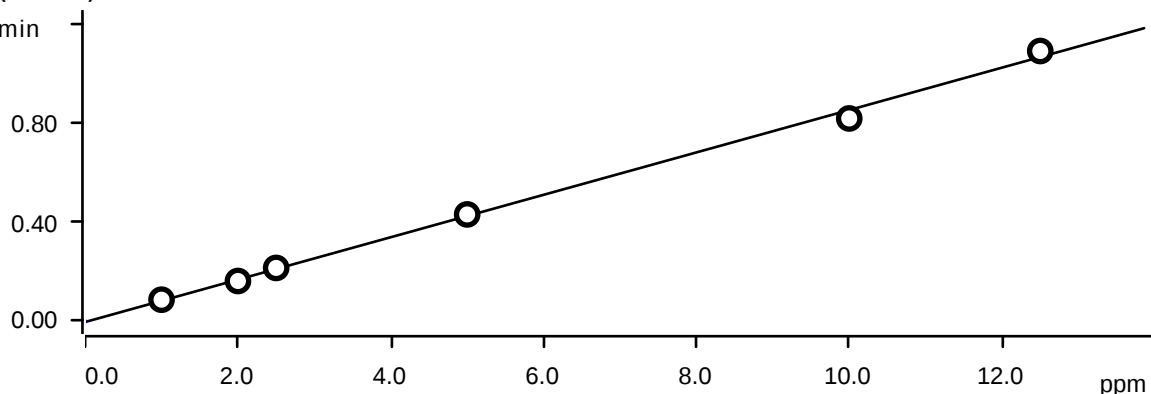
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

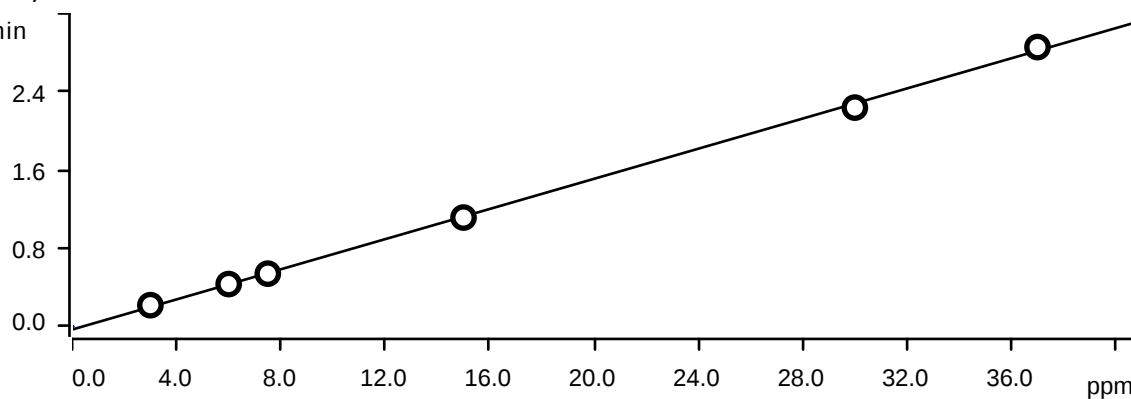 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident Q2425-03
Sample type Sample
Determination start 2025-06-26 11:53:45 UTC-4
Method IC1-062325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C


Anions

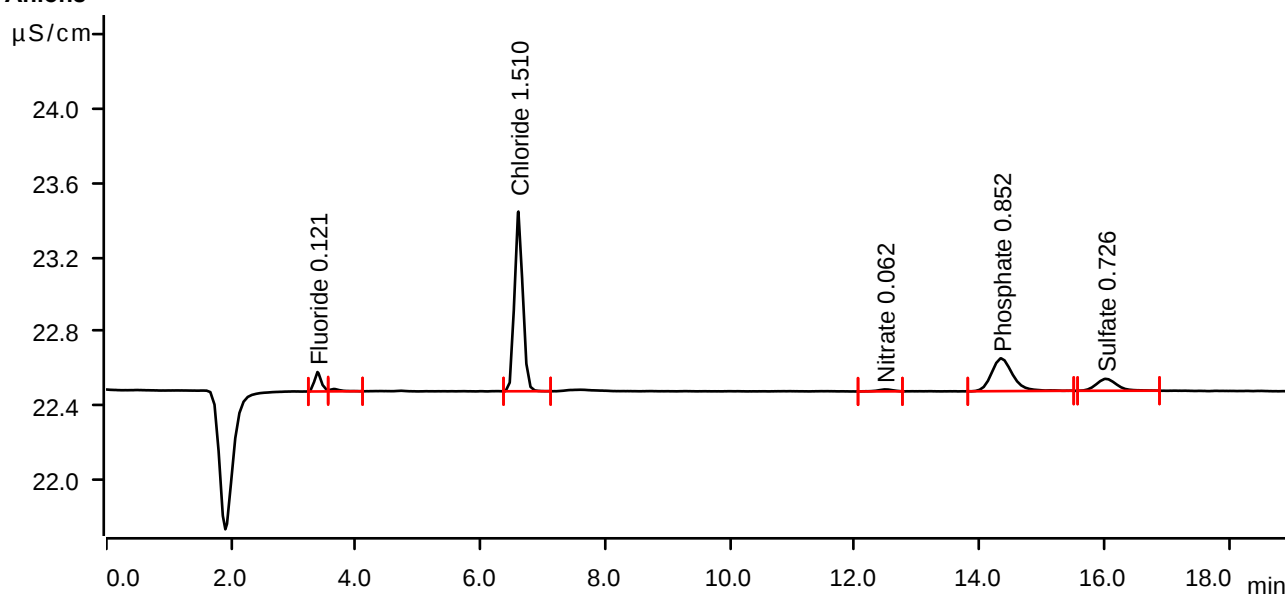

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.385	0.0131	0.105	0.121	Fluoride
2	3.645	0.0025	0.013	invalid	
3	6.607	0.1491	0.967	1.510	Chloride
4	12.477	0.0029	0.010	0.062	Nitrate
5	14.345	0.0691	0.177	0.852	Phosphate
6	16.020	0.0244	0.064	0.726	Sulfate

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

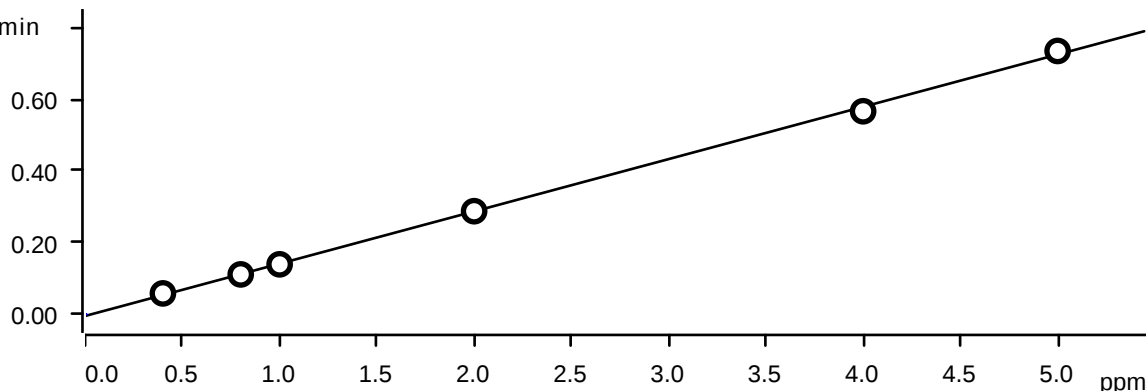

Function: $A = -4.55276E-3 + 0.0145788 \times Q$


Relative standard deviation: 2.633289 %

Correlation coefficient: 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

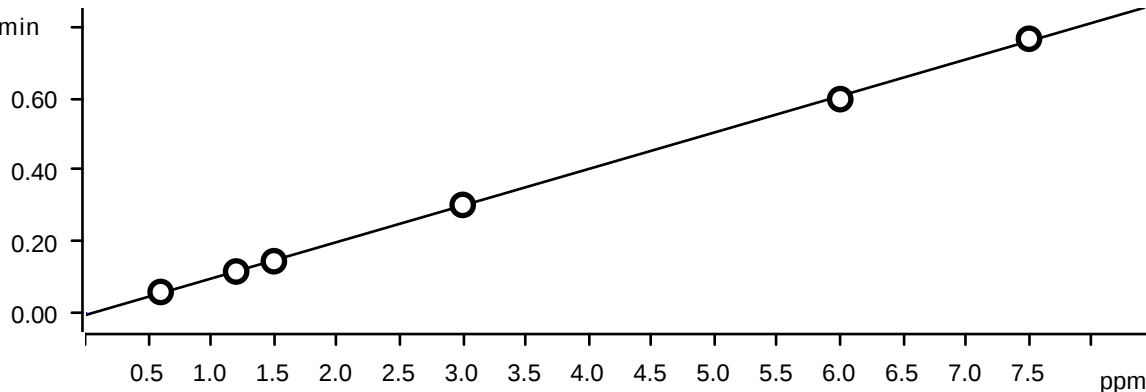


Function: $A = -4.66825E-3 + 0.0101843 \times Q$

Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

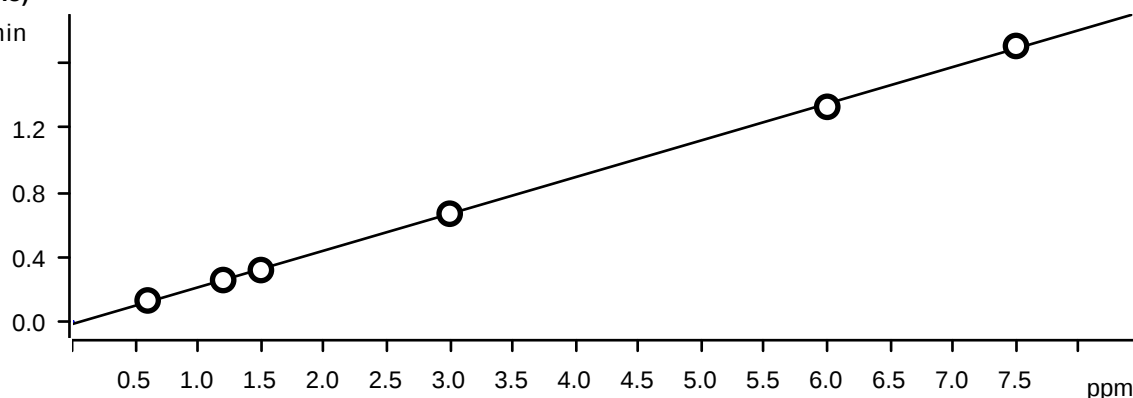Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0166933 + 0.0227623 \times Q$


Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

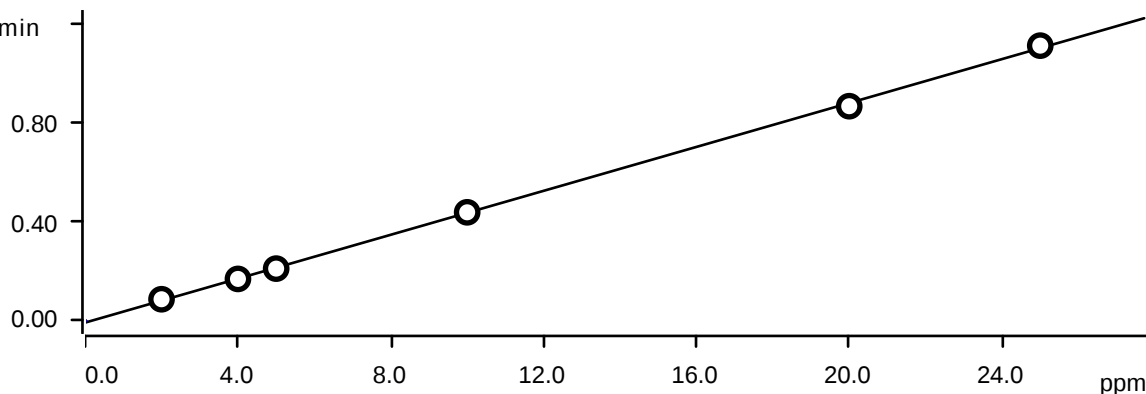

Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$


Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

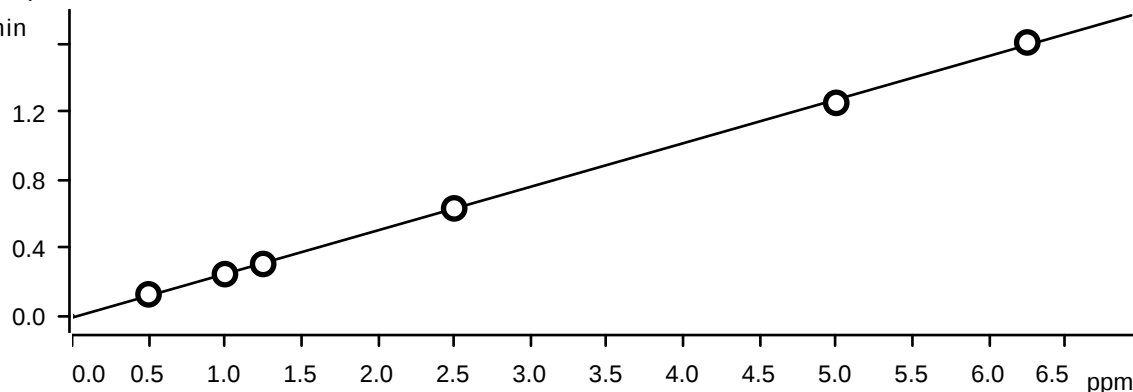


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

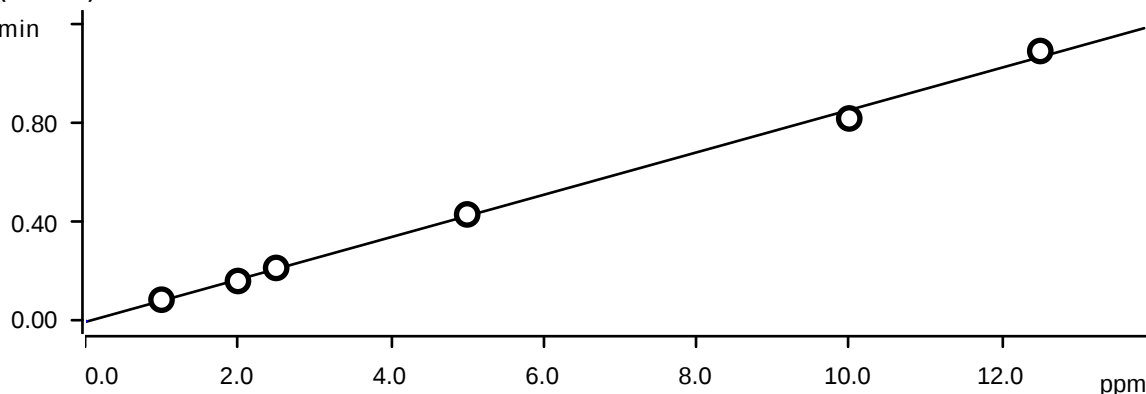
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

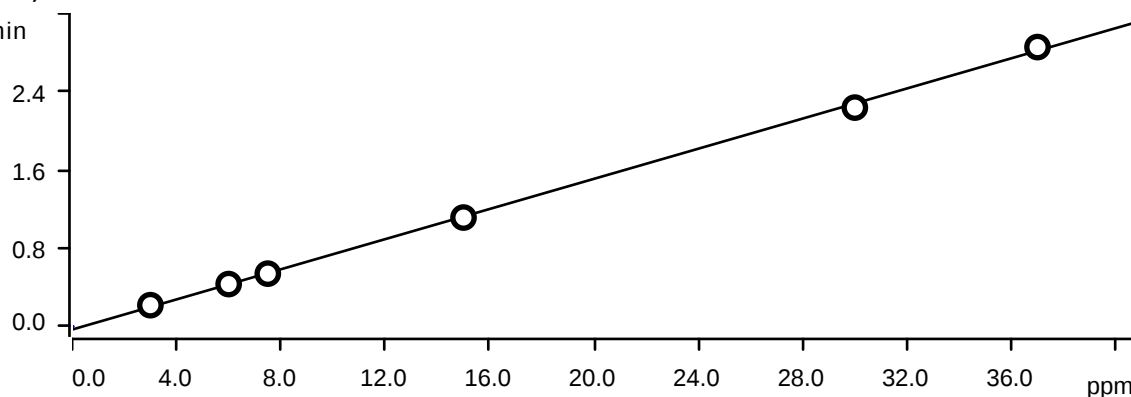 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-26 12:15:19 UTC-4
Method IC1-062325
Operator

Anions


Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

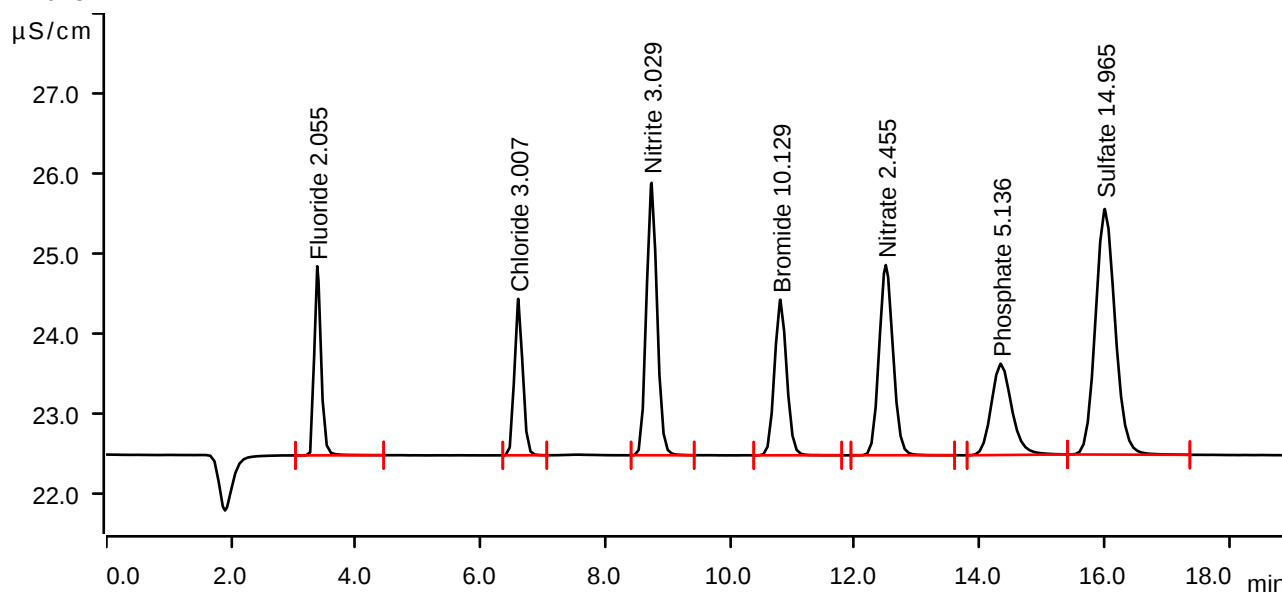

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.382	0.2951	2.362	2.055	Fluoride
2	6.605	0.3016	1.955	3.007	Chloride
3	8.742	0.6728	3.404	3.029	Nitrite
4	10.807	0.4408	1.944	10.129	Bromide
5	12.497	0.6171	2.377	2.455	Nitrate
6	14.340	0.4348	1.140	5.136	Phosphate
7	16.008	1.1213	3.068	14.965	Sulfate

Fluoride (Anions)

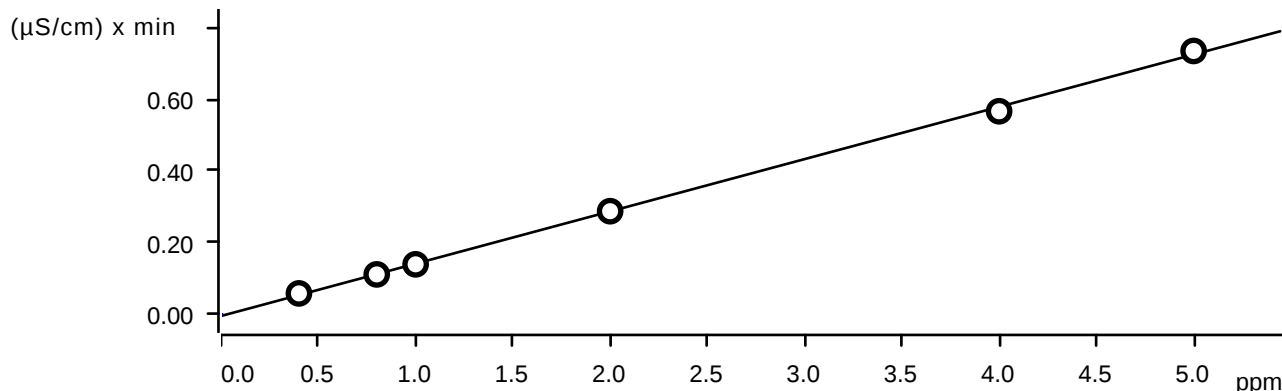


Function: $A = -4.55276E-3 + 0.0145788 \times Q$

Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

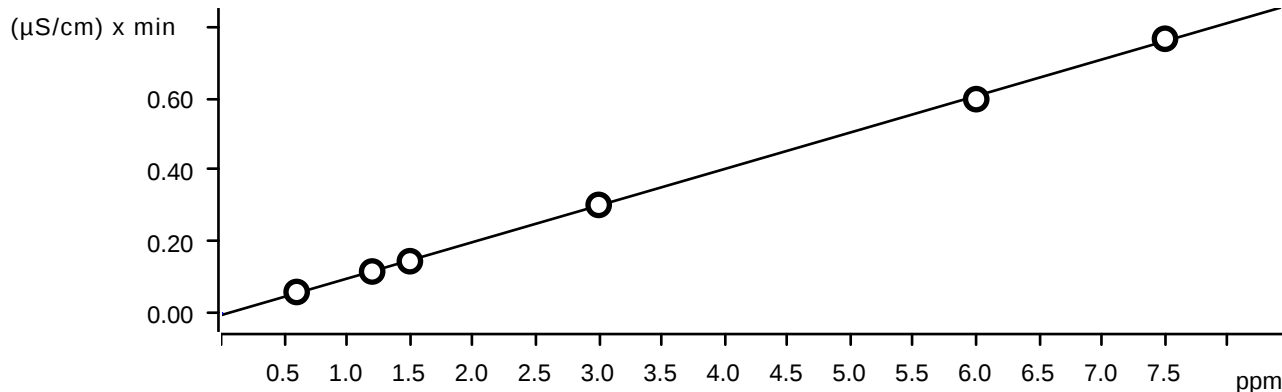


Function: $A = -4.66825E-3 + 0.0101843 \times Q$

Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

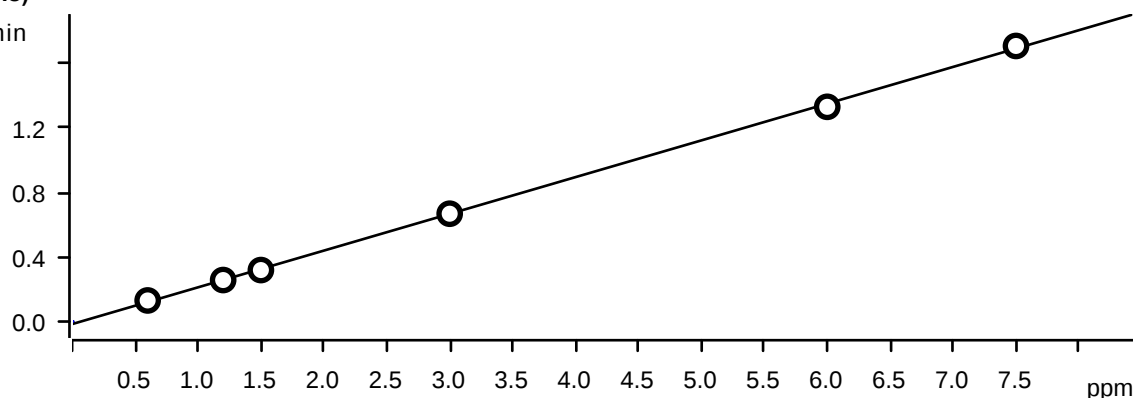Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0166933 + 0.0227623 \times Q$


Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

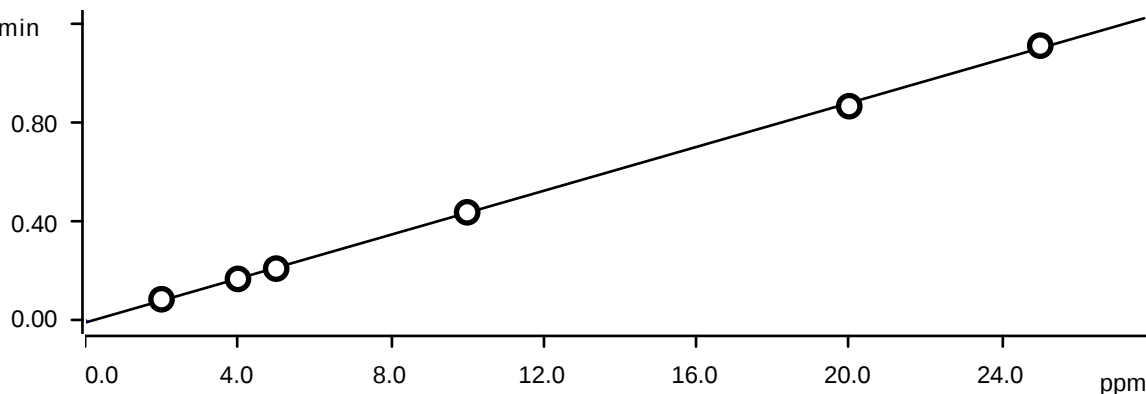

Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$


Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

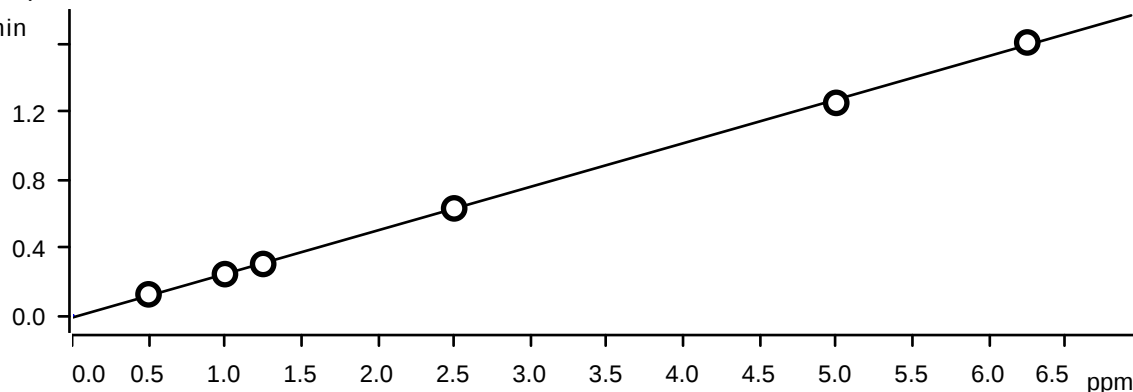


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

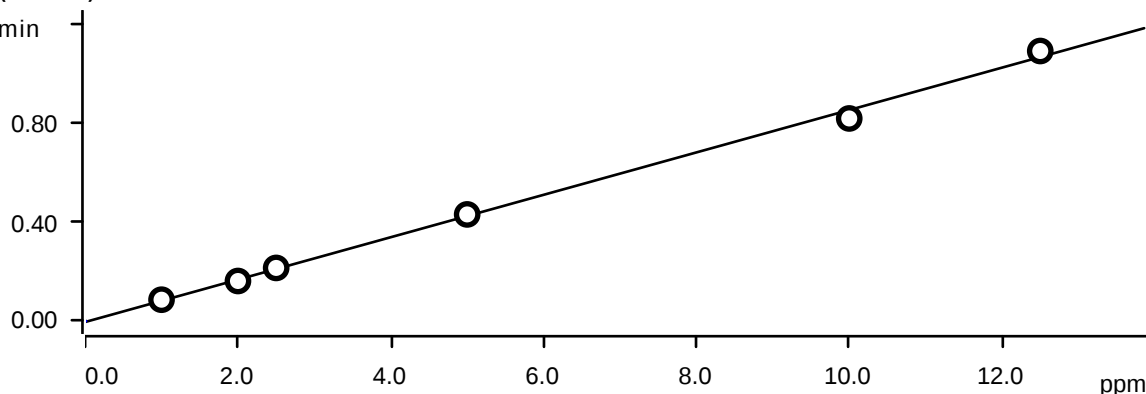
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

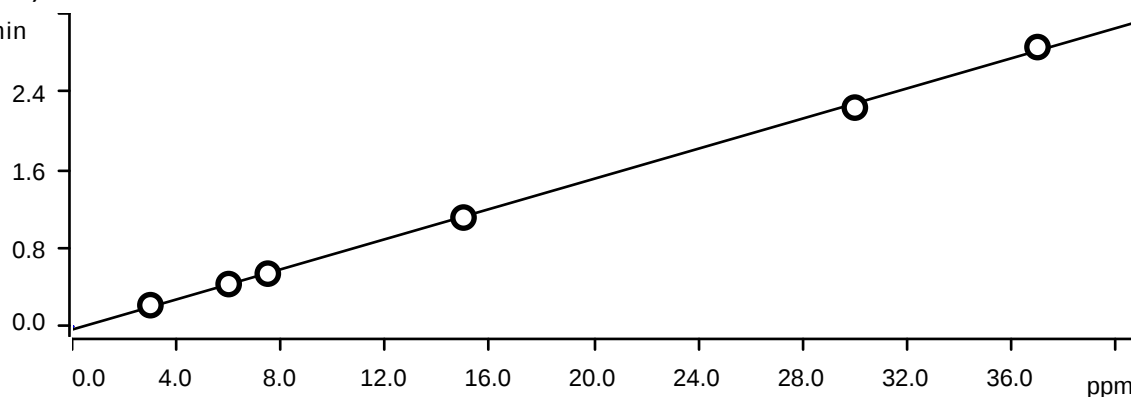 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-26 12:36:49 UTC-4
Method IC1-062325
Operator


Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

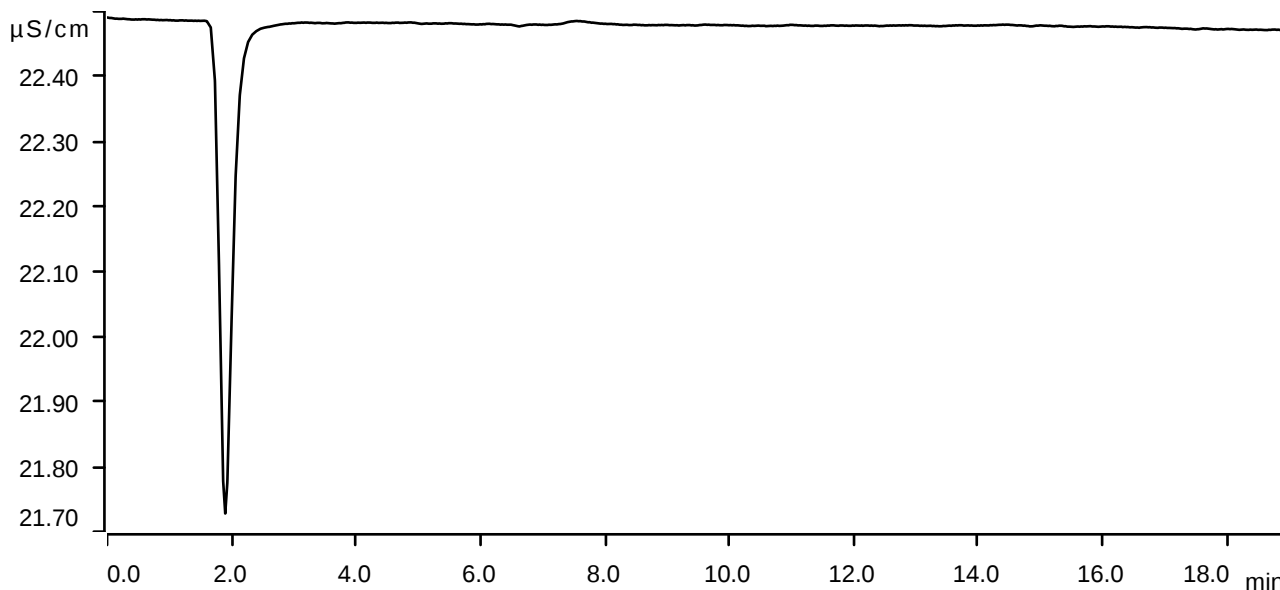Anions

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

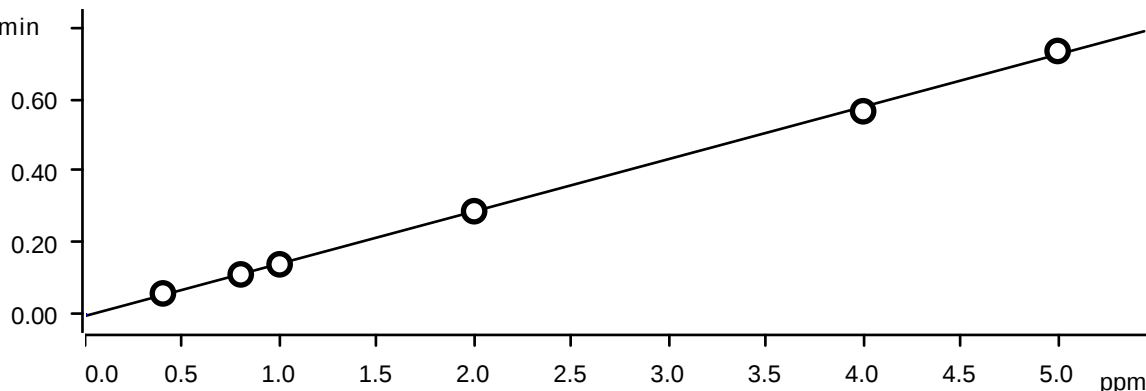

Function: $A = -4.55276E-3 + 0.0145788 \times Q$


Relative standard deviation 2.633289 %

Correlation coefficient 0.999633

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.288	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2025-06-23 17:25:53 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

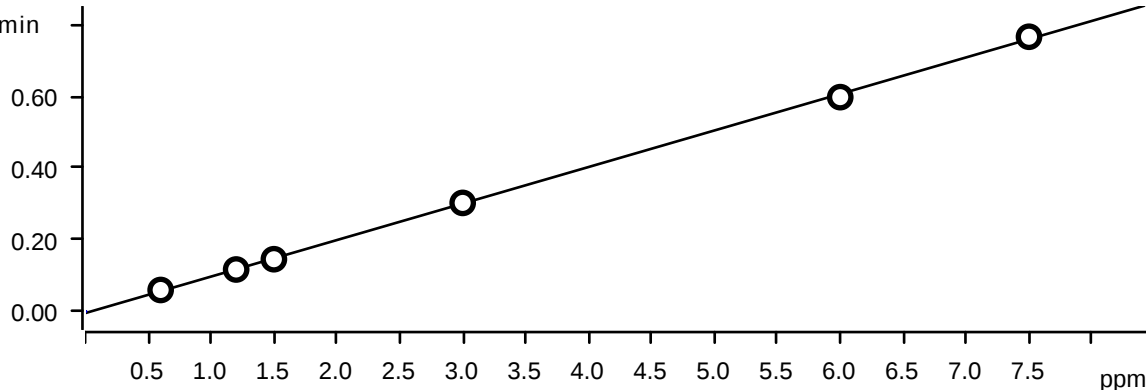

Function: $A = -4.66825E-3 + 0.0101843 \times Q$


Relative standard deviation 1.824872 %

Correlation coefficient 0.999824

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.303	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.597	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.766	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

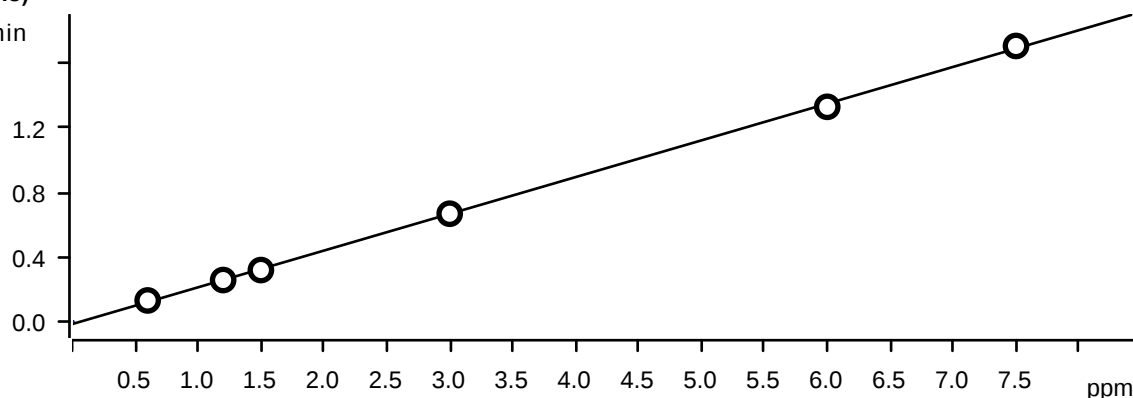Function: $A = -0.0166933 + 0.0227623 \times Q$


Relative standard deviation 1.905382 %

Correlation coefficient 0.999811

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.130	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.667	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.329	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.706	STD7	2025-06-23 17:25:53 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

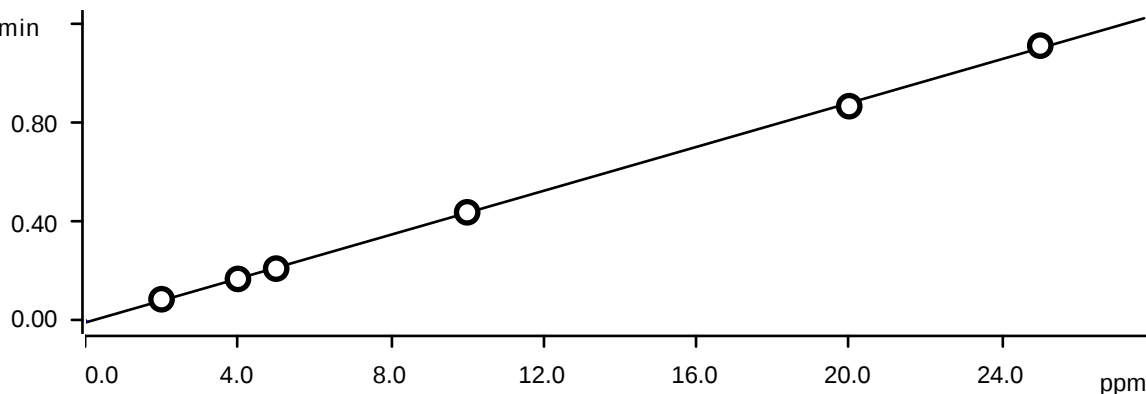

Function: $A = -7.05131E-3 + 4.42168E-3 \times Q$


Relative standard deviation: 1.851347 %

Correlation coefficient: 0.999819

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.087	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.437	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.864	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.108	STD7	2025-06-23 17:25:53 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

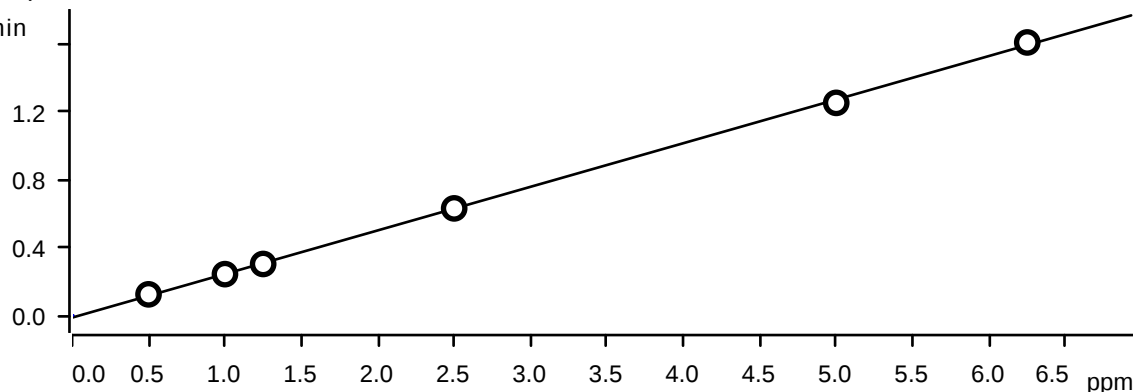


Function: $A = -0.0130270 + 0.0256654 \times Q$

Relative standard deviation: 1.929849 %

Correlation coefficient 0.999804

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.243	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.303	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.630	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.251	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.606	STD7	2025-06-23 17:25:53 UTC-4	used

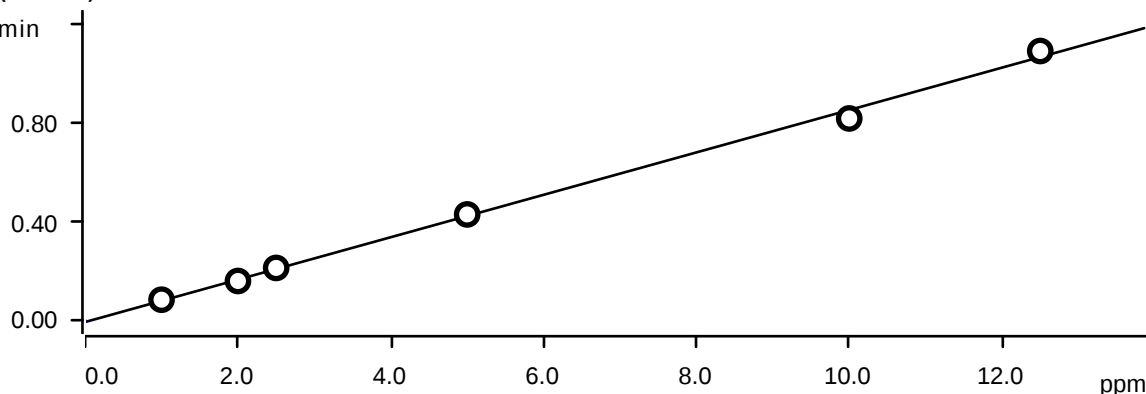
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.61656E-3 + 8.53718E-3 \times Q$

Relative standard deviation 4.618615 %

Correlation coefficient 0.998857

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.086	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.430	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.816	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-06-23 17:25:53 UTC-4	used

Sulfate (Anions)

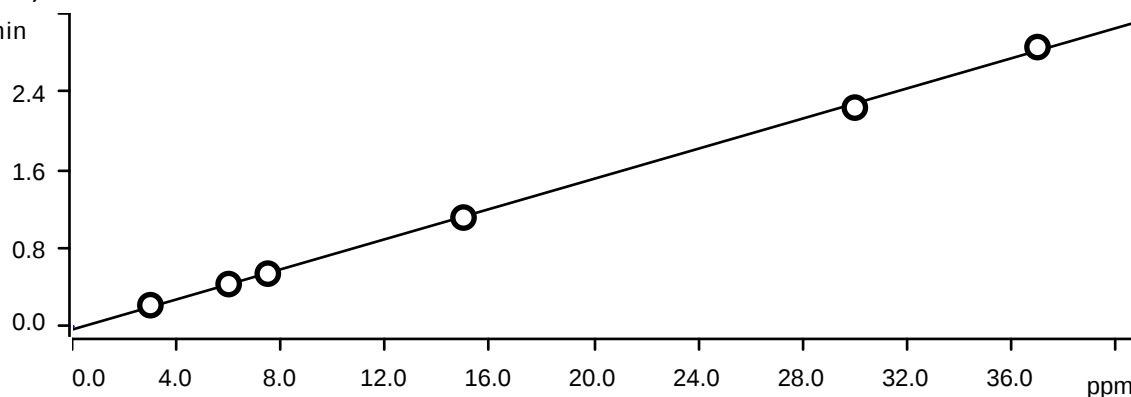 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0315238 + 7.70359E-3 \times Q$

Relative standard deviation 2.454303 %

Correlation coefficient 0.999685

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-06-23 15:17:36 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-06-23 15:38:59 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.434	STD3	2025-06-23 16:00:23 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.540	STD4	2025-06-23 16:21:47 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.114	STD5	2025-06-23 16:43:01 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.237	STD6	2025-06-23 17:04:27 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.856	STD7	2025-06-23 17:25:53 UTC-4	used