

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
 Data File : BF142929.D
 Acq On : 30 Jun 2025 22:15
 Operator : RC/JU
 Sample : Q2436-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-84

Quant Time: Jul 01 01:25:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	85331	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	316172	20.000	ng	-0.01
39) Acenaphthene-d10	9.916	164	159254	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	249233	20.000	ng	0.00
76) Chrysene-d12	14.045	240	161494	20.000	ng	-0.01
86) Perylene-d12	15.539	264	195795	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	450284	87.857	ng	0.00
7) Phenol-d6	6.504	99	527501	87.237	ng	0.00
23) Nitrobenzene-d5	7.434	82	320893	55.670	ng	-0.01
42) 2,4,6-Tribromophenol	10.704	330	133976	81.751	ng	-0.01
45) 2-Fluorobiphenyl	9.233	172	639464	52.749	ng	-0.01
79) Terphenyl-d14	12.986	244	495576	42.400	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063025\
Data File : BF142929.D
Acq On : 30 Jun 2025 22:15
Operator : RC/JU
Sample : Q2436-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-84

Quant Time: Jul 01 01:25:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration




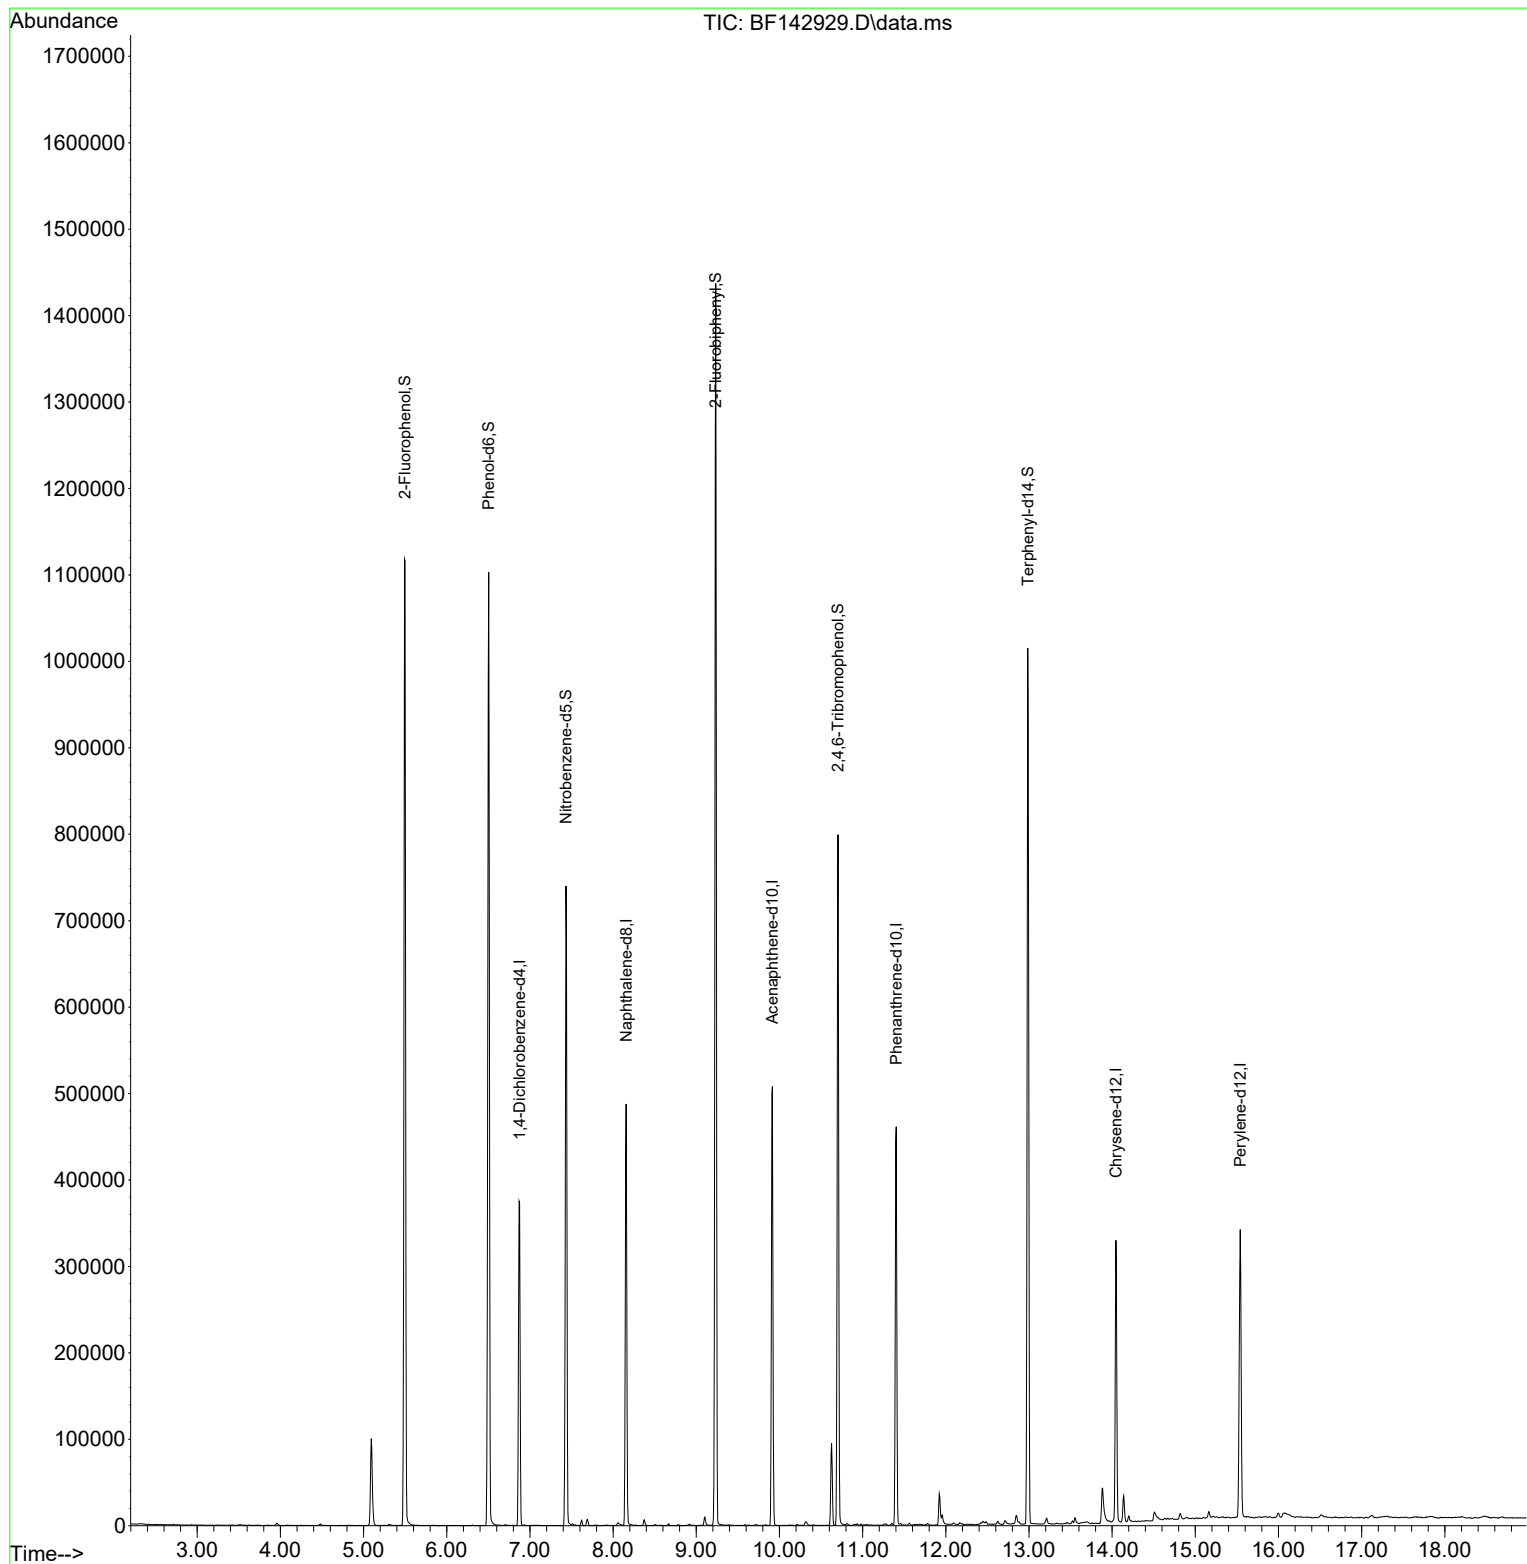




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 79
Delta R.T. -0.006 min
Lab File: BF142929.D
Acq: 30 Jun 2025 22:15




Instrument :
BNA_F
ClientSampleId :
TP-84


Tgt Ion:152 Resp: 85331
Ion Ratio Lower Upper
152 100
150 158.6 127.2 190.8
115 56.6 46.6 69.8

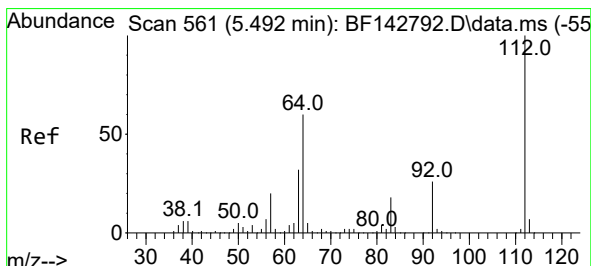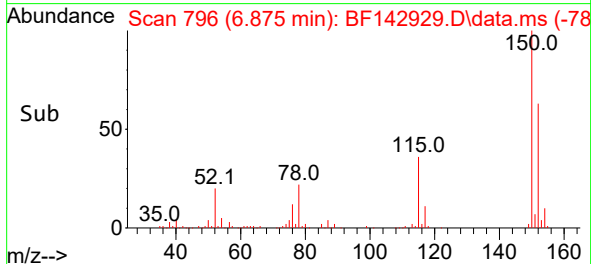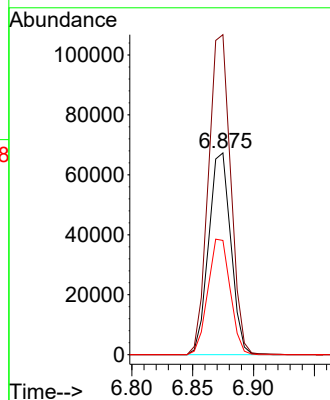

#5
2-Fluorophenol
Concen: 87.857 ng
RT: 5.498 min Scan# 562
Delta R.T. 0.006 min
Lab File: BF142929.D
Acq: 30 Jun 2025 22:15

Tgt Ion:112 Resp: 450284
Ion Ratio Lower Upper
112 100
64 56.7 48.2 72.2
63 30.2 25.7 38.5


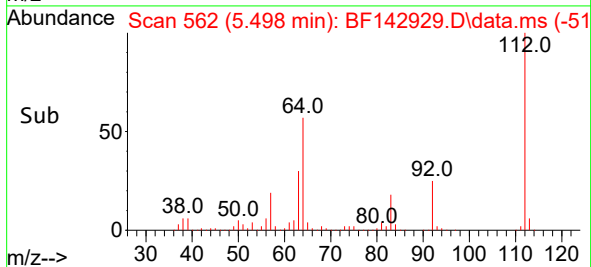
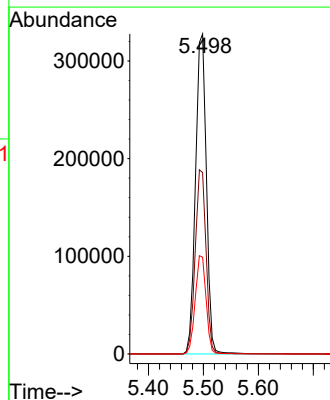
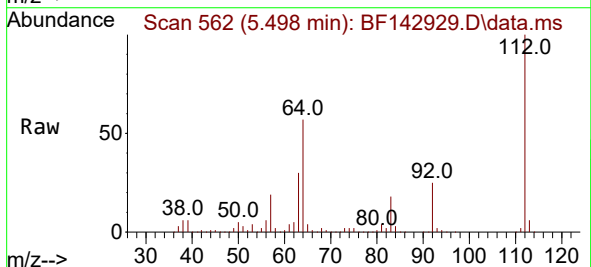


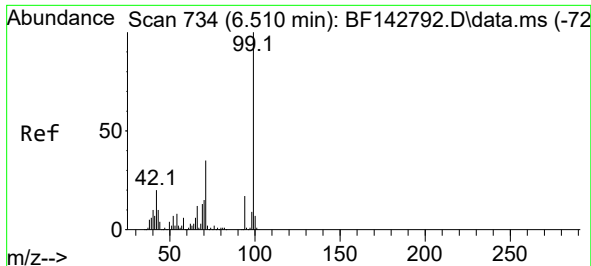

#7
Phenol-d6
Concen: 87.237 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF142929.D
Acq: 30 Jun 2025 22:15




Instrument :
BNA_F
ClientSampleId :
TP-84


Tgt Ion: 99 Resp: 527501
Ion Ratio Lower Upper
99 100
42 19.2 15.9 23.9
71 35.3 27.8 41.8

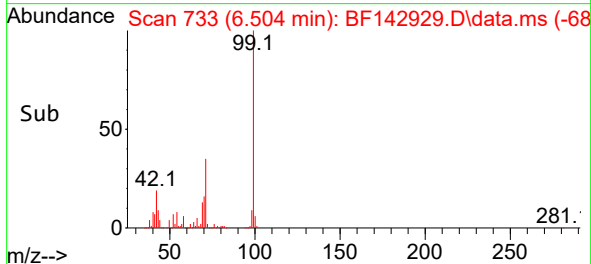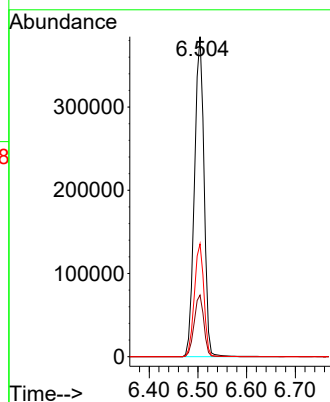

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1014
Delta R.T. -0.012 min
Lab File: BF142929.D
Acq: 30 Jun 2025 22:15

Tgt Ion: 136 Resp: 316172
Ion Ratio Lower Upper
136 100
137 10.7 8.4 12.6
54 7.5 6.3 9.5
68 4.3 3.7 5.5

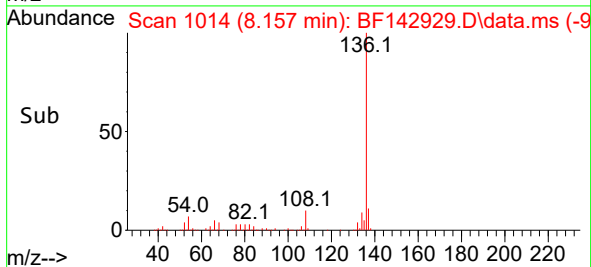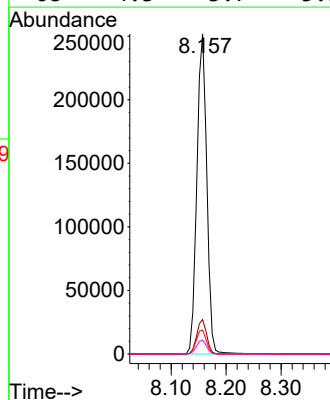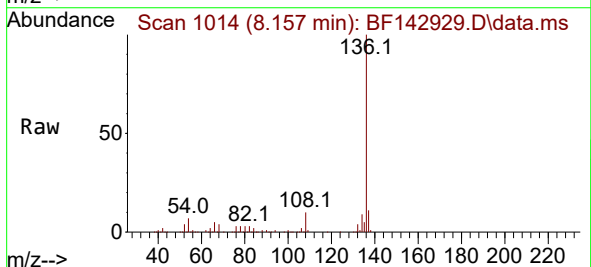

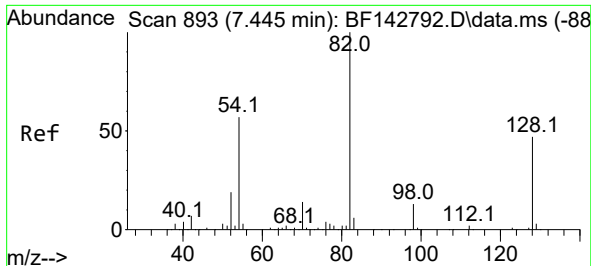

#23

Nitrobenzene-d5

Concen: 55.670 ng

RT: 7.434 min Scan# 89

Delta R.T. -0.011 min

Lab File: BF142929.D

Acq: 30 Jun 2025 22:15

Instrument :

BNA_F

ClientSampleId :

TP-84





Tgt Ion: 82 Resp: 320893

Ion Ratio Lower Upper

82 100

128 47.2 37.7 56.5

54 55.7 45.7 68.5

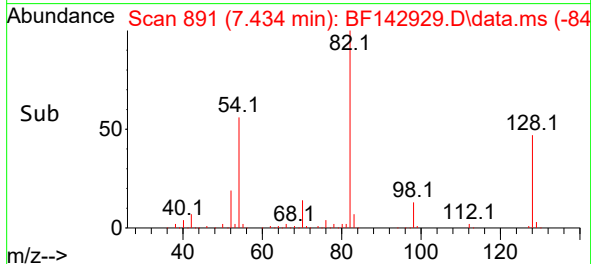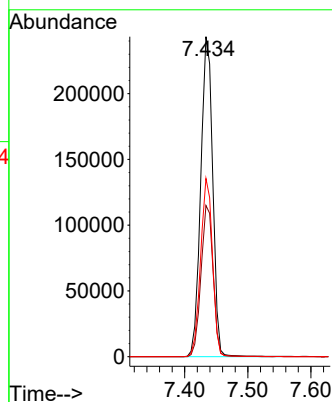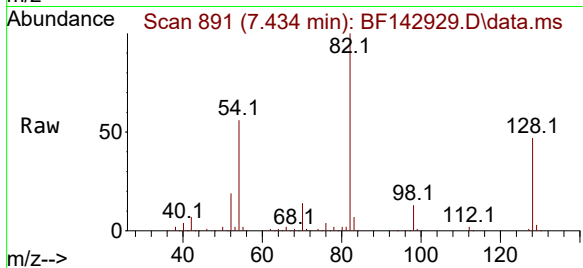

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.916 min Scan# 1313

Delta R.T. -0.006 min

Lab File: BF142929.D

Acq: 30 Jun 2025 22:15




Tgt Ion:164 Resp: 159254


Ion Ratio Lower Upper

164 100

162 99.9 81.8 122.8

160 43.6 36.0 54.0


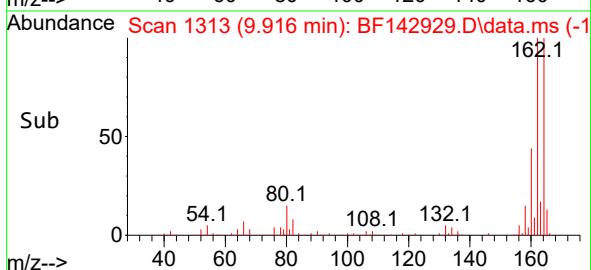
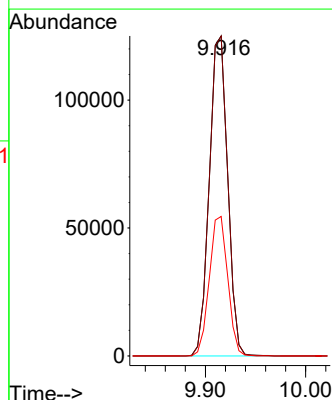
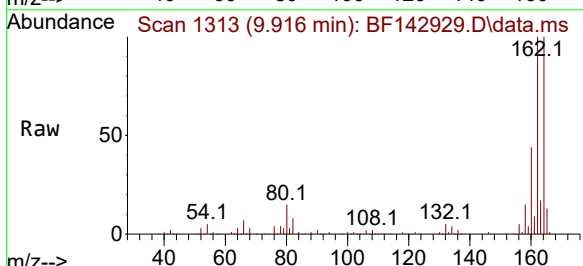


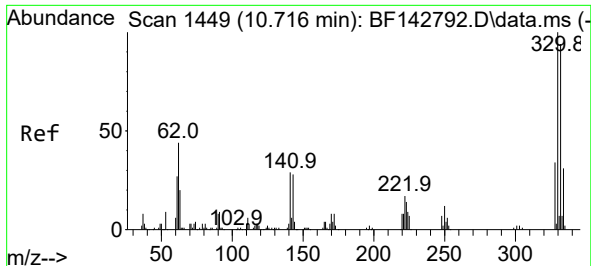

#42
 2,4,6-Tribromophenol
 Concen: 81.751 ng
 RT: 10.704 min Scan# 1447
 Delta R.T. -0.012 min
 Lab File: BF142929.D
 Acq: 30 Jun 2025 22:15




Instrument :
 BNA_F
 ClientSampleId :
 TP-84


Tgt Ion: 330 Resp: 133976
 Ion Ratio Lower Upper
 330 100
 332 97.9 75.0 112.6
 141 32.4 25.3 37.9

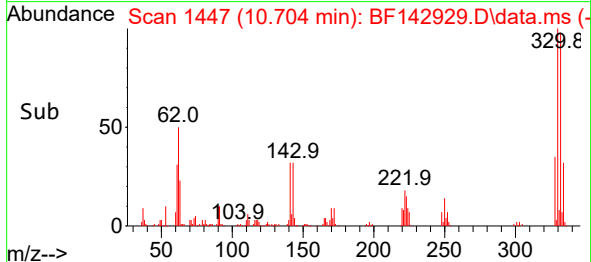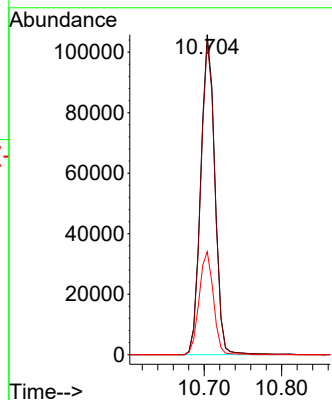

#45
 2-Fluorobiphenyl
 Concen: 52.749 ng
 RT: 9.233 min Scan# 1197
 Delta R.T. -0.012 min
 Lab File: BF142929.D
 Acq: 30 Jun 2025 22:15

Tgt Ion: 172 Resp: 639464
 Ion Ratio Lower Upper
 172 100
 171 34.9 28.2 42.4
 170 22.9 18.5 27.7


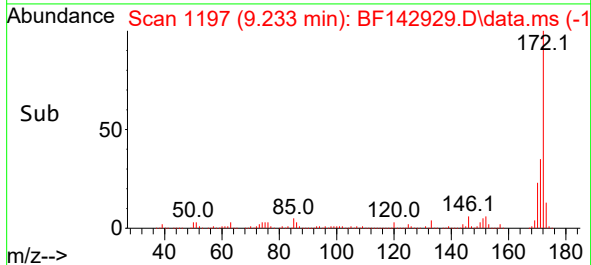
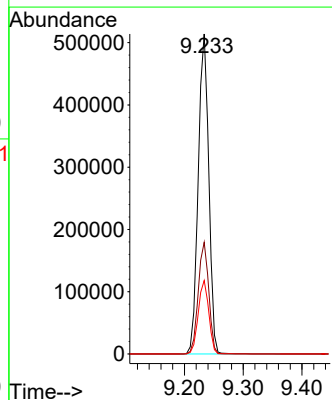
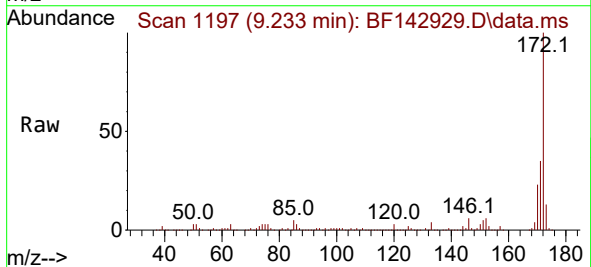


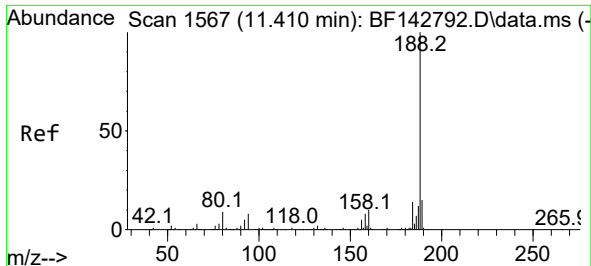

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF142929.D
Acq: 30 Jun 2025 22:15




Instrument :
BNA_F
ClientSampleId :
TP-84


Tgt Ion:188 Resp: 249233
Ion Ratio Lower Upper
188 100
94 7.7 6.7 10.1
80 7.7 6.9 10.3

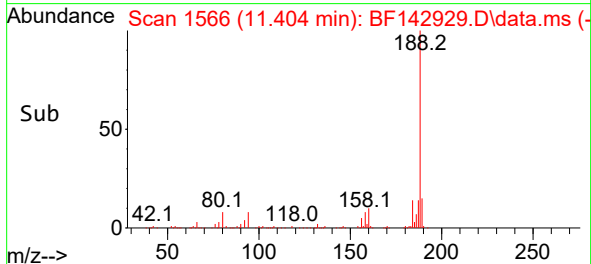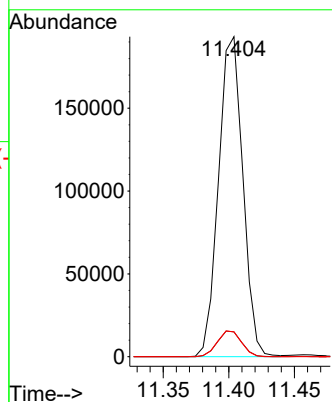

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2015
Delta R.T. -0.012 min
Lab File: BF142929.D
Acq: 30 Jun 2025 22:15

Tgt Ion:240 Resp: 161494
Ion Ratio Lower Upper
240 100
120 10.1 8.2 12.2
236 23.9 19.8 29.8


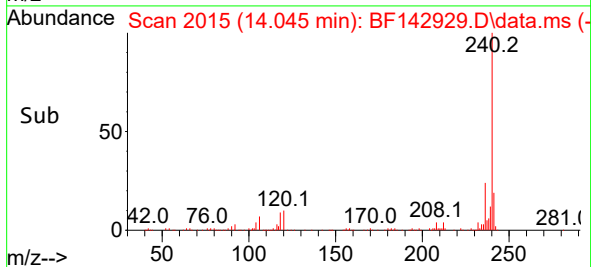
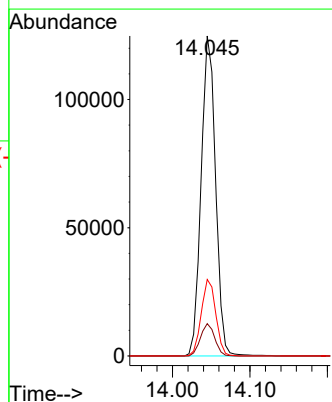
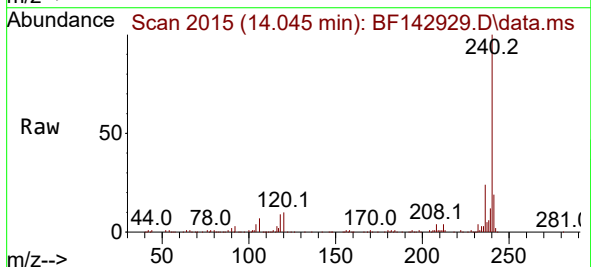


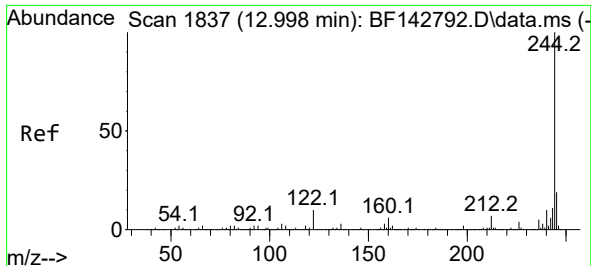

#79
 Terphenyl-d14
 Concen: 42.400 ng
 RT: 12.986 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BF142929.D
 Acq: 30 Jun 2025 22:15

Instrument :
 BNA_F
 ClientSampleId :
 TP-84

Tgt Ion:244 Resp: 495576
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.4 8.0
 122 10.5 8.2 12.2

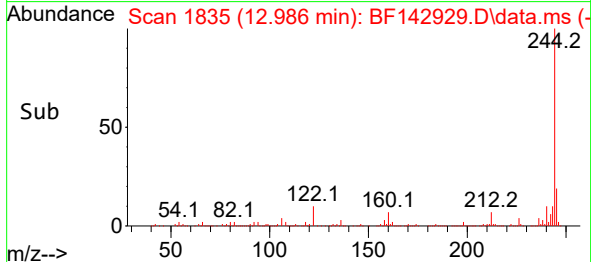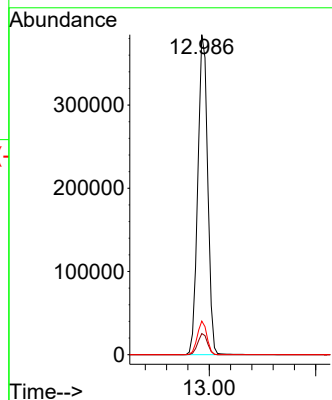

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.539 min Scan# 2269
 Delta R.T. -0.006 min
 Lab File: BF142929.D
 Acq: 30 Jun 2025 22:15

Tgt Ion:264 Resp: 195795
 Ion Ratio Lower Upper
 264 100
 260 22.5 18.1 27.1
 265 21.4 16.6 25.0

