


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070125\
Data File : BP025051.D
Acq On : 01 Jul 2025 11:15
Operator : RC/JU
Sample : DFTPP625
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP625

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP063025.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Jul 01 11:17:33 2025

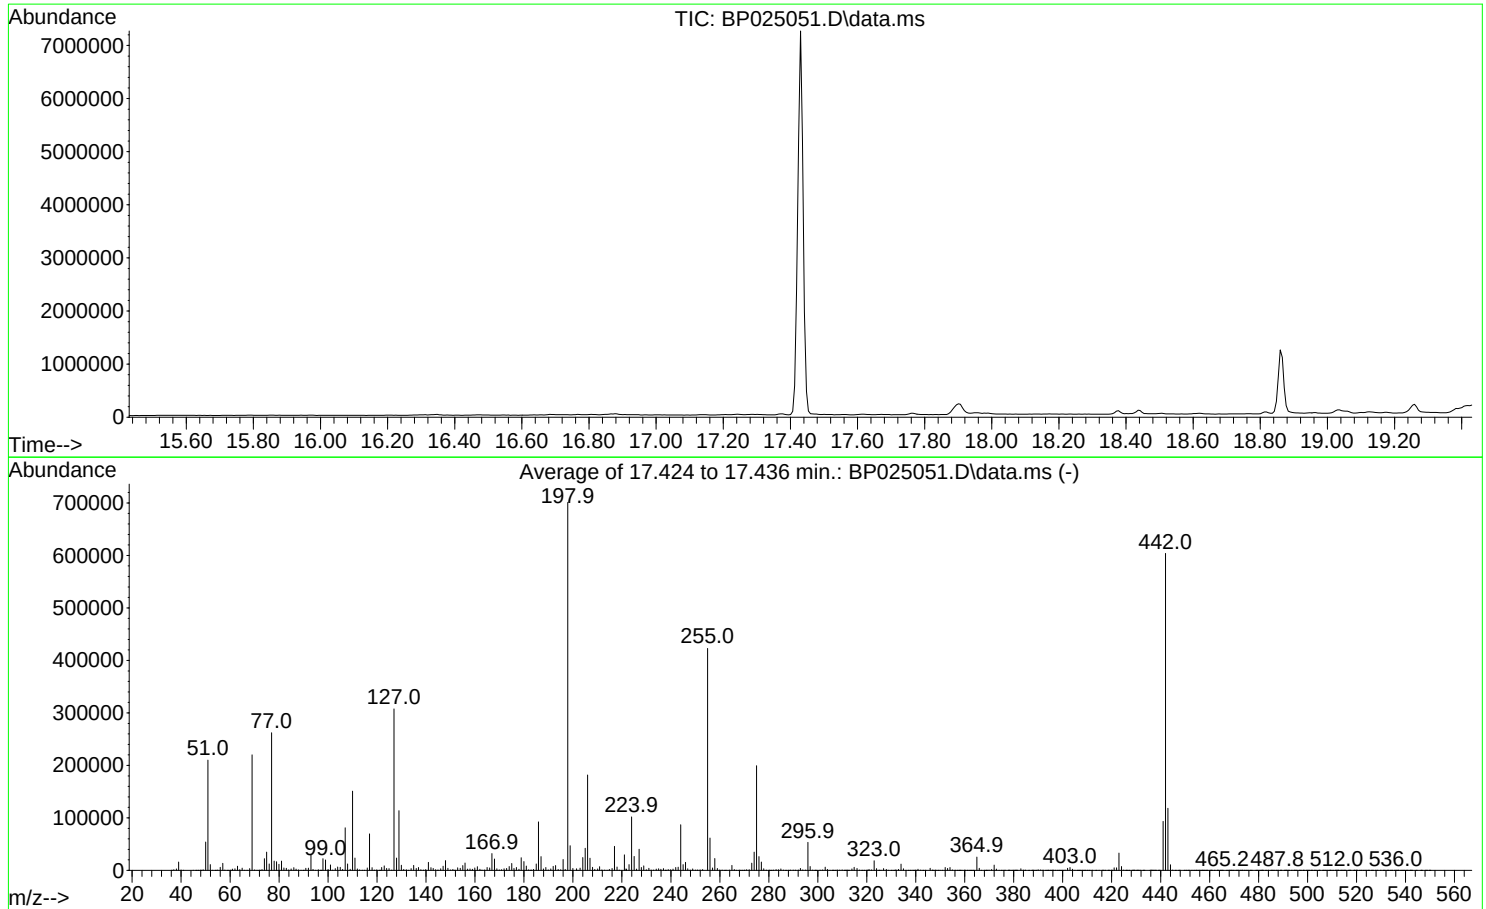

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	210113	PASS
68	69	0.00	2	1.5	3394	PASS
69	198	0.00	100	31.4	220111	PASS
70	69	0.00	2	0.4	818	PASS
127	198	10	80	43.9	307600	PASS
197	198	0.00	2	0.3	2003	PASS
198	198	100	100	100.0	700879	PASS
199	198	5	9	6.7	46824	PASS
275	198	10	60	28.5	199451	PASS
365	198	1	100	3.6	25234	PASS
441	198	0.01	100	13.3	93170	PASS
442	198	50	100	86.2	603814	PASS
443	442	15	24	19.6	118357	PASS