
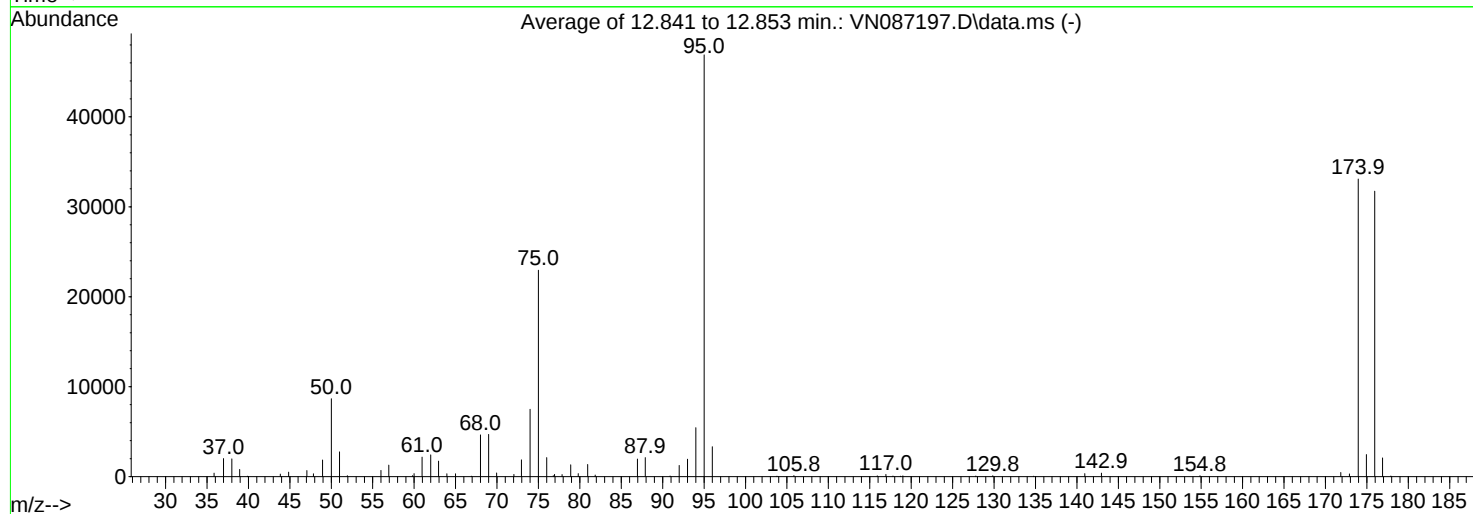


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062625\
Data File : VN087197.D
Acq On : 26 Jun 2025 16:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062625W.M
Title : SW846 8260
Last Update : Fri Jun 27 05:55:21 2025

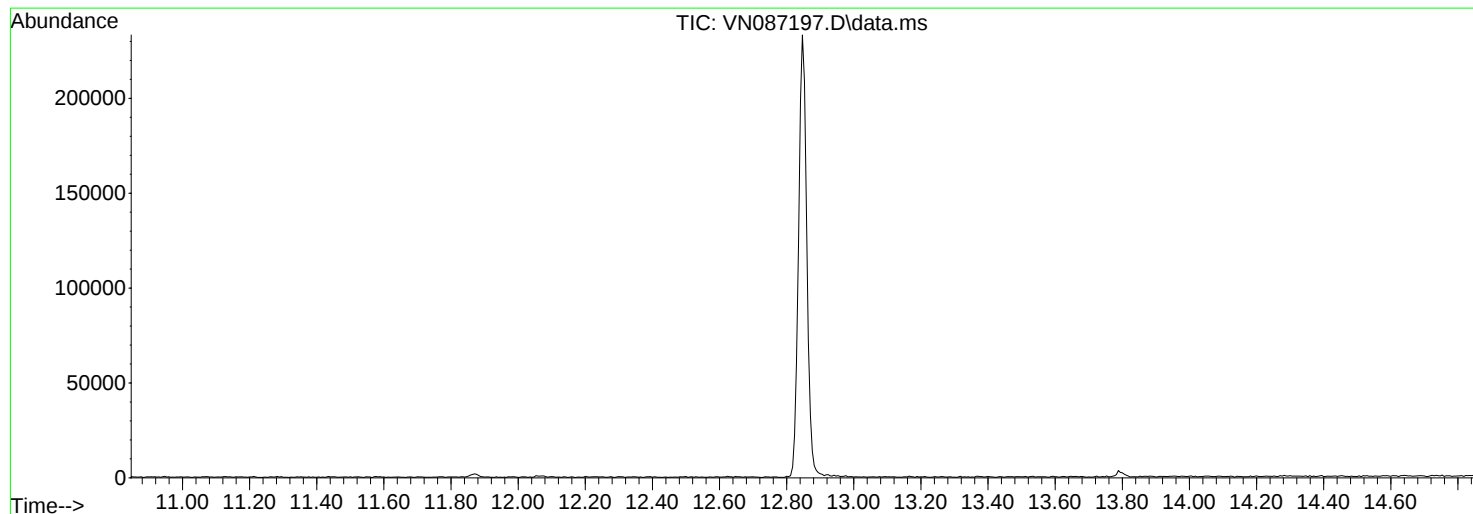

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	8671	PASS
75	95	30	60	49.0	22957	PASS
95	95	100	100	100.0	46896	PASS
96	95	5	9	7.1	3332	PASS
173	174	0.00	2	0.9	311	PASS
174	95	50	100	70.6	33091	PASS
175	174	5	9	7.4	2461	PASS
176	174	95	101	95.9	31733	PASS
177	176	5	9	6.6	2079	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	391	51.00	2754	66.90	58	77.85	231
37.00	2007	51.95	115	68.00	4643	78.90	131
38.00	1975	56.00	695	69.00	4689	79.80	33
38.95	799	56.95	1278	69.95	405	80.95	135
39.90	62	59.80	111	72.05	244	81.85	180
43.85	287	60.00	337	72.95	1862	86.95	1967
44.85	493	60.95	2167	74.00	7491	87.90	2127
47.05	683	62.00	2426	75.00	22957	90.90	66
47.85	327	62.95	1733	76.00	2118	92.00	1242
48.95	1845	63.95	313	76.80	115	93.00	1943
50.00	8671	65.00	326	76.95	250	94.00	5447

Average of 12.841 to 12.853 min.: VN087197.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	46896	134.80	54				
96.00	3332	140.95	335				
103.80	54	142.95	385				
105.85	129	154.85	115				
115.90	82	171.85	467				
116.95	249	172.90	311				
117.80	68	173.95	33091				
118.70	60	174.95	2461				
119.00	93	175.95	31733				
127.80	65	176.90	2079				
129.85	104	177.90	71				

Instrument :

MSVOA_N

ClientSampleId :

BFB