
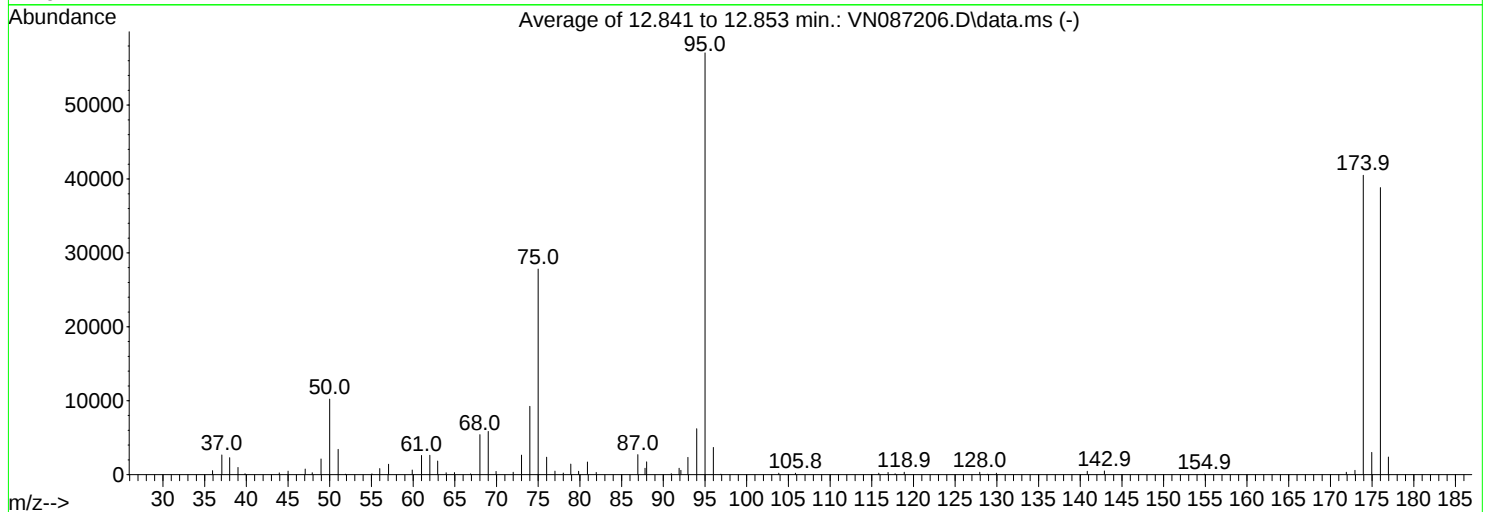


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062725\
Data File : VN087206.D
Acq On : 27 Jun 2025 08:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062625W.M
Title : SW846 8260
Last Update : Fri Jun 27 05:55:21 2025

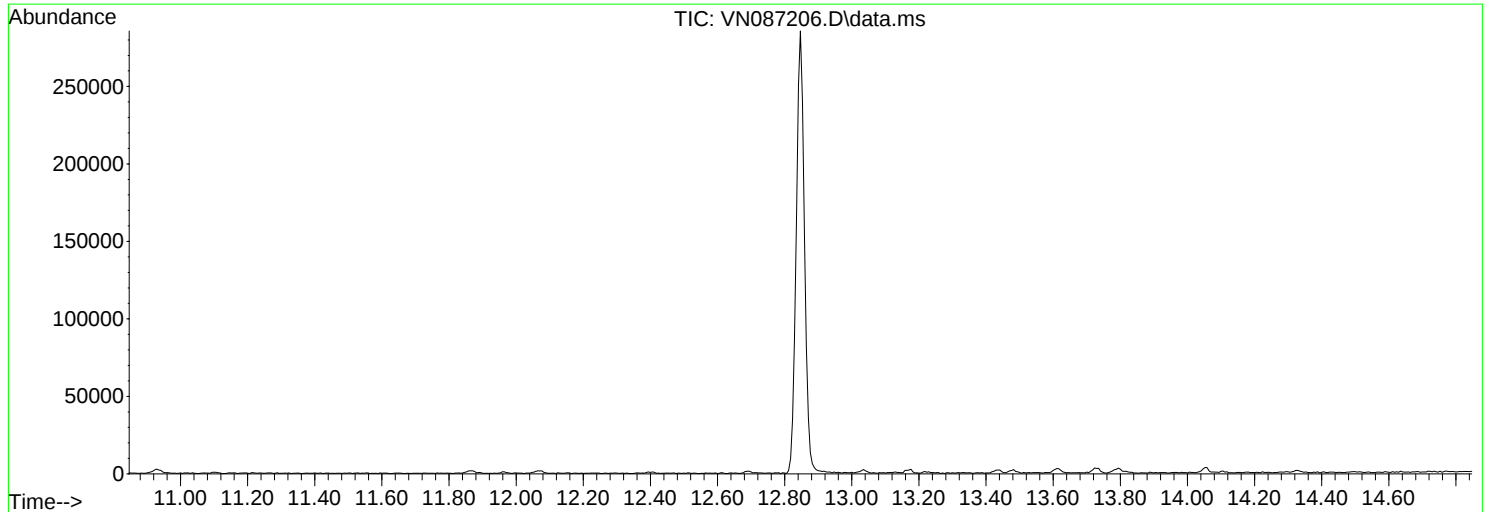

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	10223	PASS
75	95	30	60	48.8	27827	PASS
95	95	100	100	100.0	57064	PASS
96	95	5	9	6.5	3691	PASS
173	174	0.00	2	1.4	577	PASS
174	95	50	100	71.0	40493	PASS
175	174	5	9	7.4	3005	PASS
176	174	95	101	95.9	38845	PASS
177	176	5	9	6.1	2386	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	536	51.00	3413	66.90	113	78.90	142
37.05	2655	51.90	66	68.00	5422	79.85	46
38.00	2289	55.05	117	69.00	5854	80.90	170
39.00	982	56.00	814	69.95	432	81.95	29
39.85	133	57.05	1400	72.00	324	86.95	2706
43.95	228	59.90	632	73.00	2634	87.80	864
45.00	484	61.00	2590	74.00	9239	88.00	1724
47.05	752	62.00	2614	75.00	27827	90.95	132
47.90	270	62.95	1851	76.00	2353	91.90	862
48.95	2115	63.95	270	77.00	480	92.10	595
50.00	10223	64.95	293	78.00	218	92.95	2342

Average of 12.841 to 12.853 min.: VN087206.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	6208	128.90	57				
95.00	57064	129.95	186				
96.00	3691	140.85	447				
96.90	56	142.90	491				
103.85	188	154.90	58				
105.85	196	171.90	336				
115.85	196	172.95	577				
116.95	305	173.95	40493				
117.80	141	174.95	3005				
118.90	334	176.00	38845				
127.95	318	176.95	2386				

Instrument :

MSVOA_N

ClientSampleId :

BFB