


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037385.D
Acq On : 26 Jun 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 26 16:06:33 2025

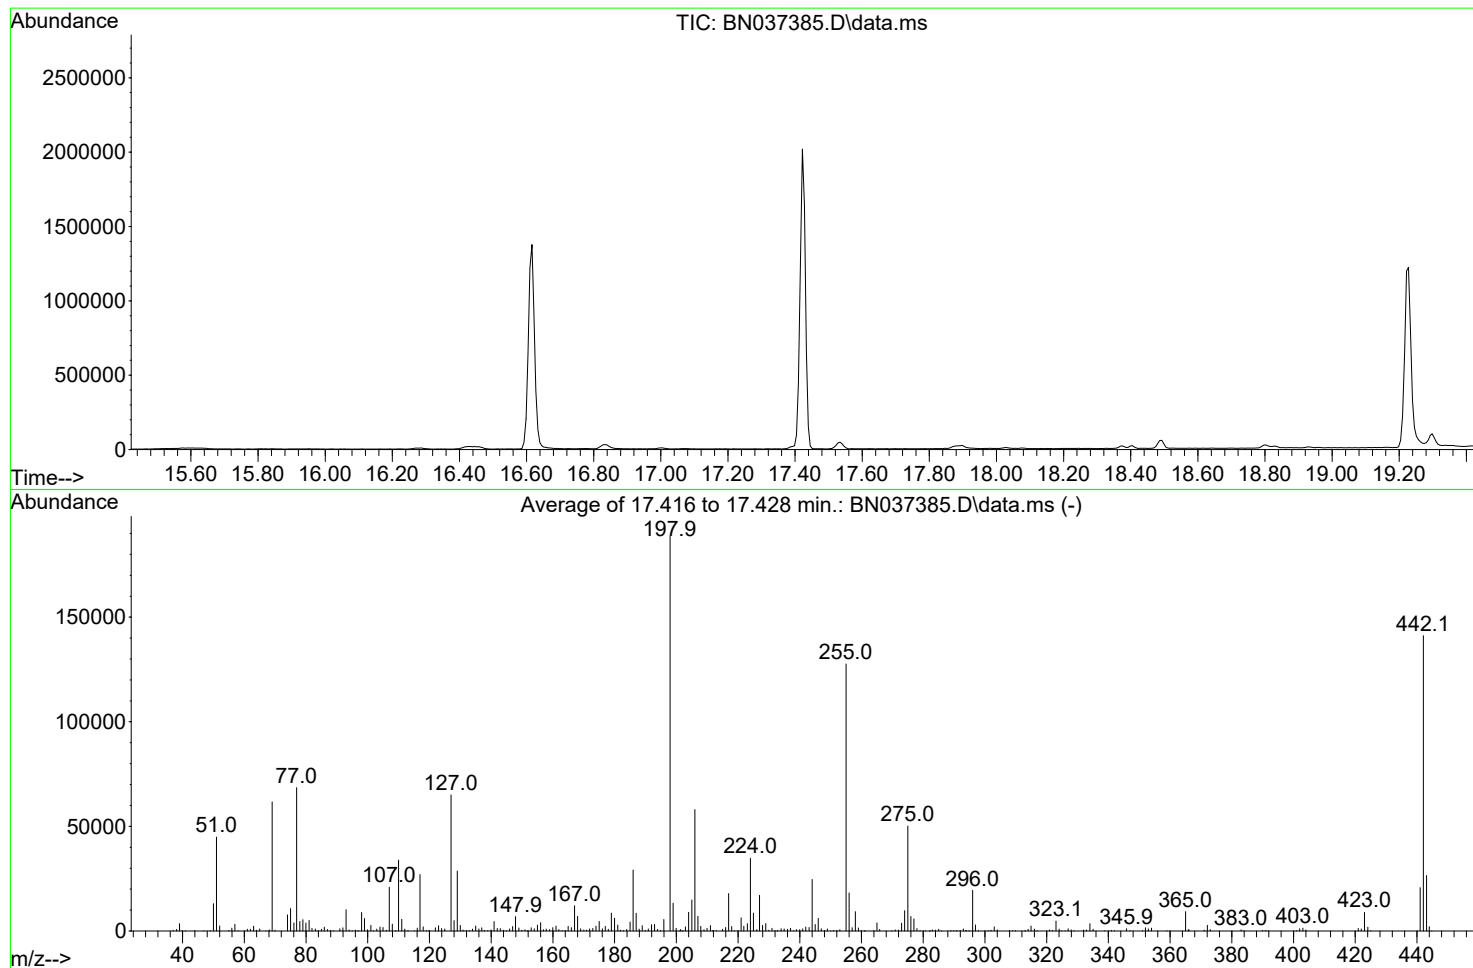

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	565	PASS
69	69	100	100	100.0	61709	PASS
70	69	0.00	2	0.6	395	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188693	PASS
199	198	5	9	7.1	13336	PASS
365	198	1	100	4.9	9289	PASS
441	443	0.01	150	78.0	20689	PASS
442	442	100	100	100.0	141205	PASS
443	442	15	24	18.8	26534	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/26/2025	BNA_N	<u>BN037385.D</u>
Compound Name	Response	Retention Time
DDT	575237	20.469
DDD	9375	20.028
DDE	1379	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10754	585991	1.84

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037385.D
Acq On : 26 Jun 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 26 17:27:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

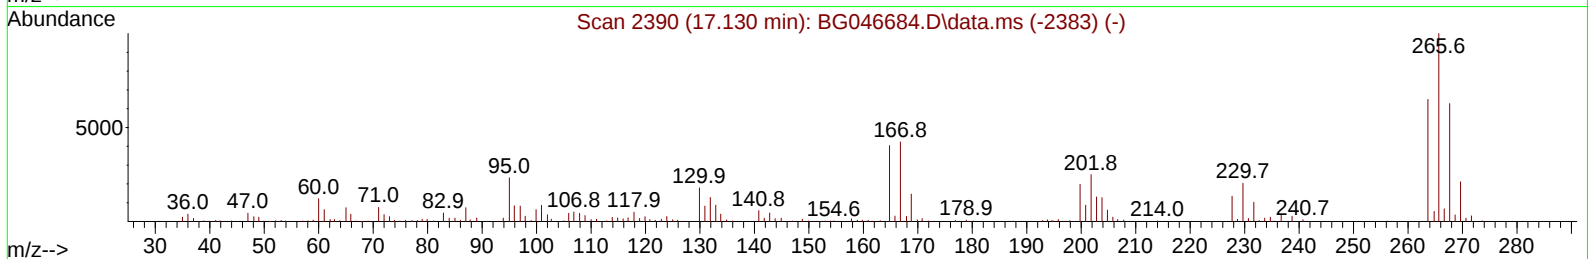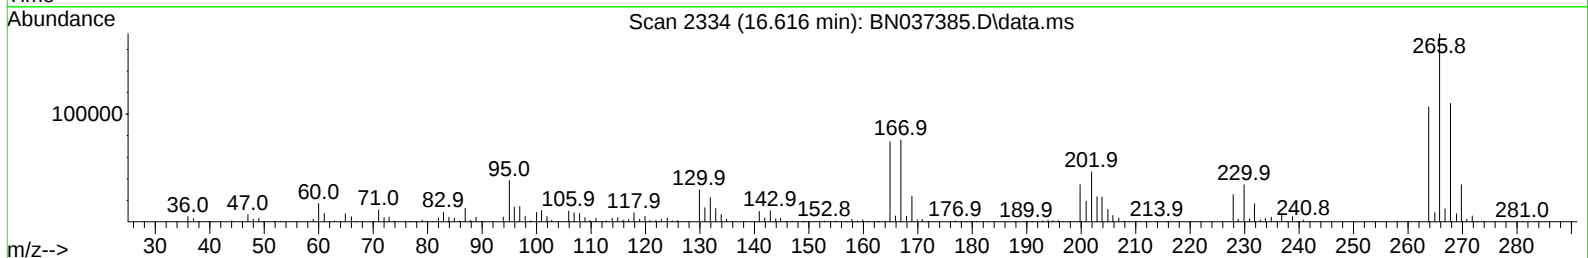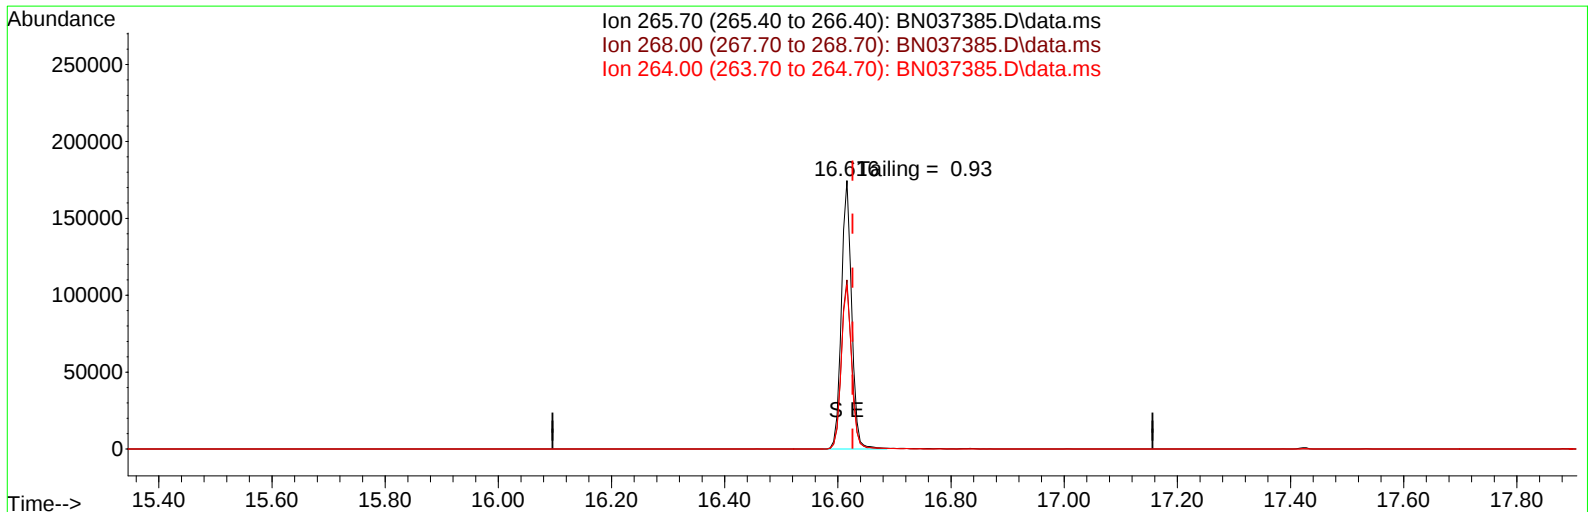

TIC: BN037385.D\data.ms

(70) Pentachlorophenol (C)

16.616min (-0.010) 22827.65 ng




response 218916

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.95
264.00	61.60	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037385.D
Acq On : 26 Jun 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 26 17:27:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

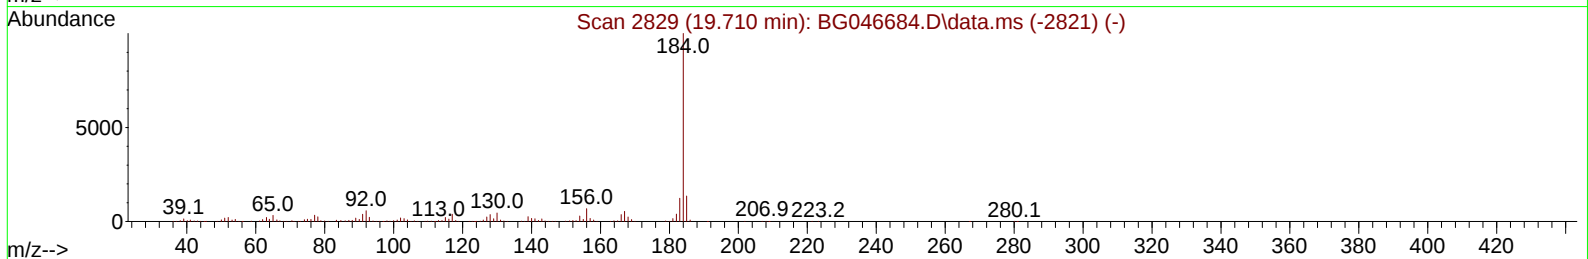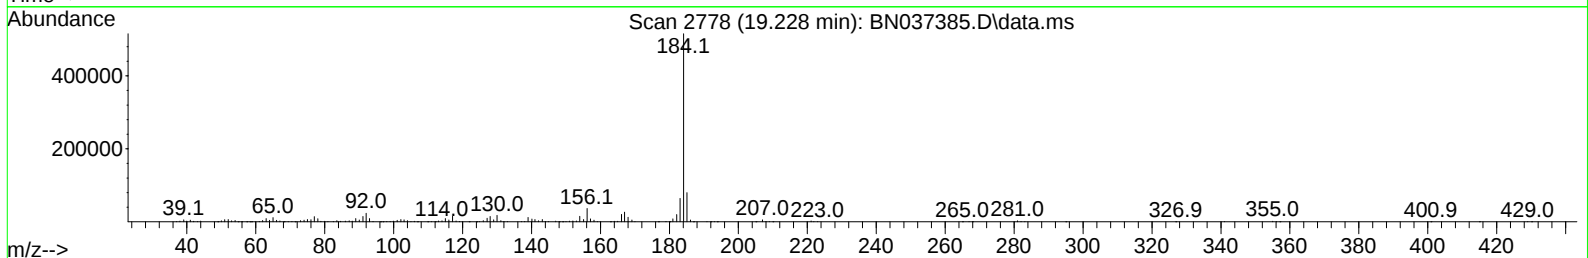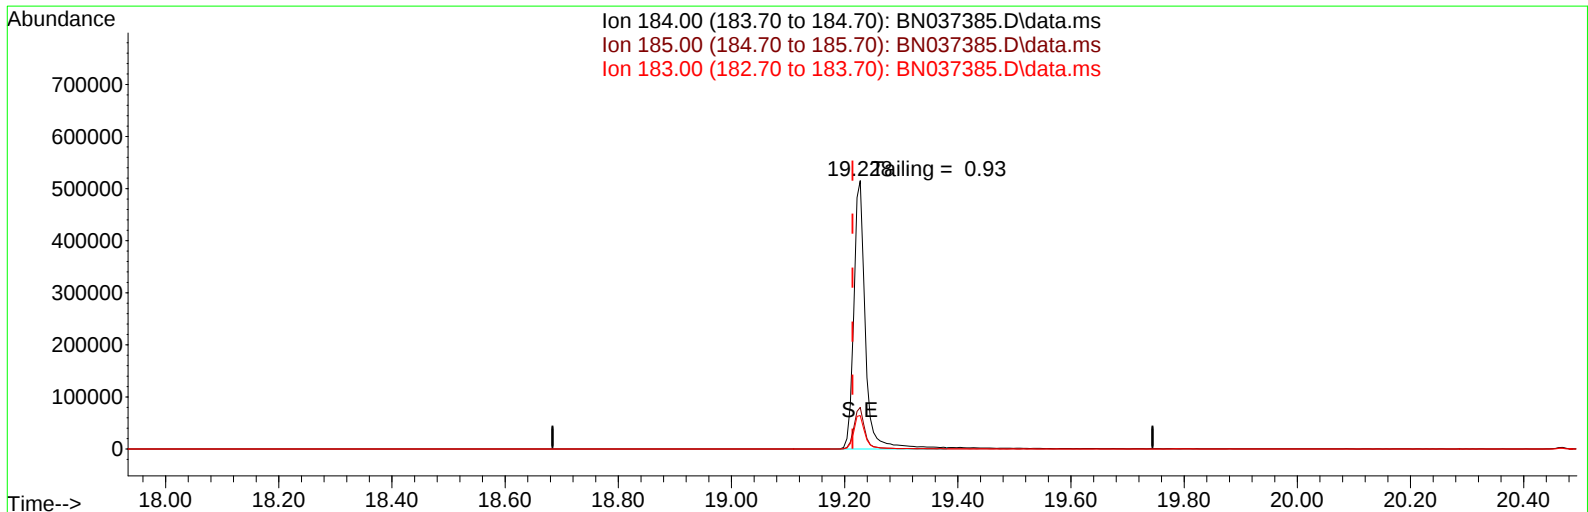

TIC: BN037385.D\data.ms

(77) Benzidine

19.228min (+ 0.014) 0.00 ng

response 733495

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.54
183.00	13.20	12.50
0.00	0.00	0.00