


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070225\
Data File : BN037424.D
Acq On : 02 Jul 2025 13:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 26 16:06:33 2025

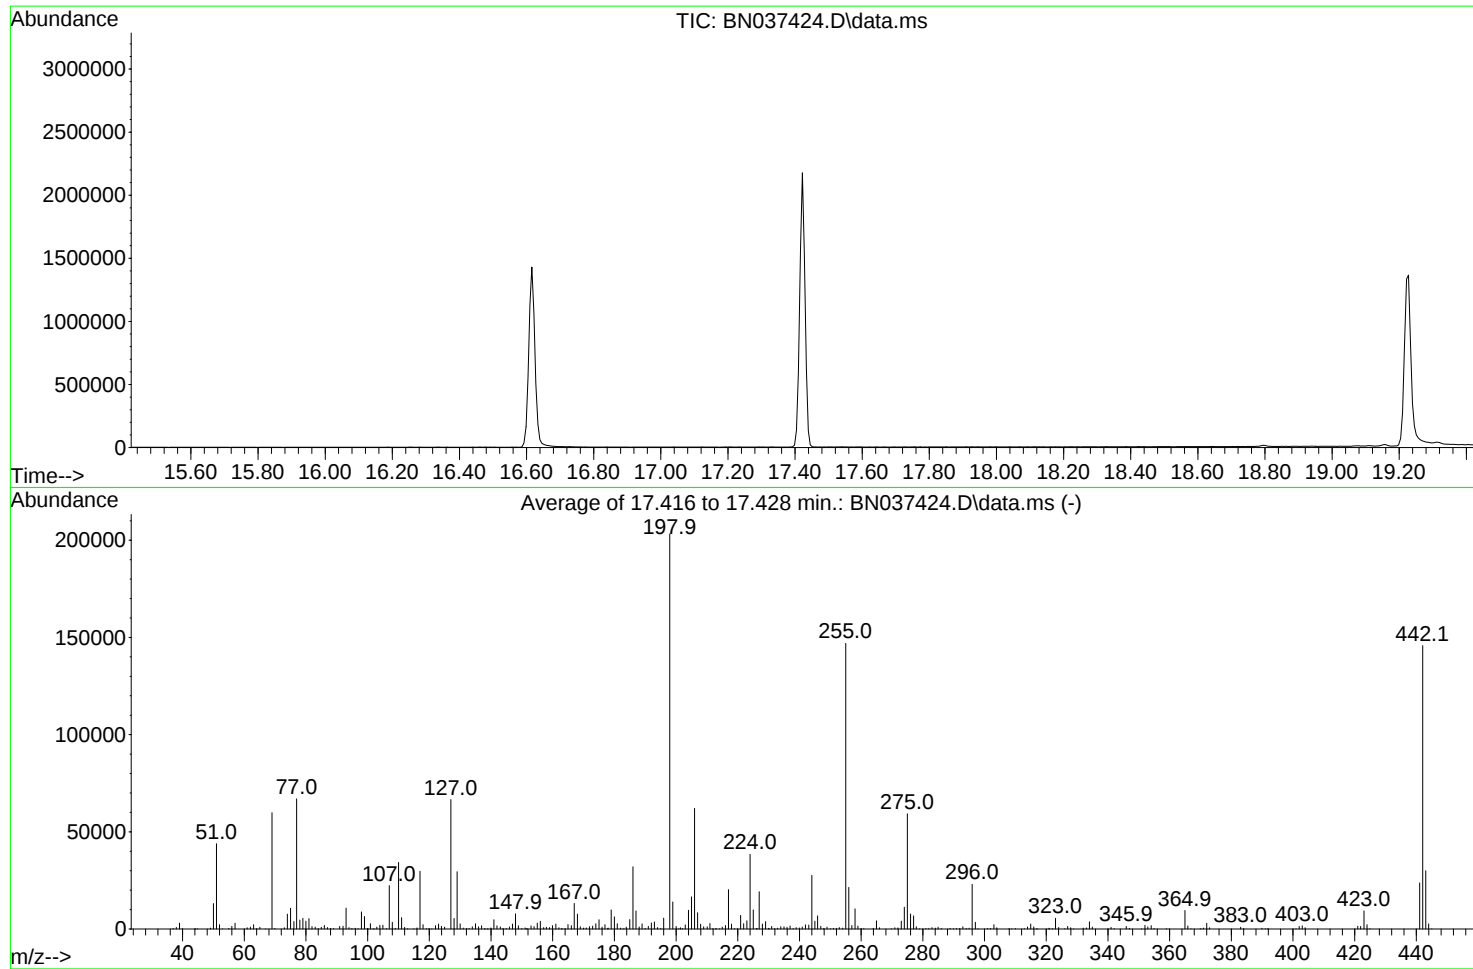




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	59808	PASS
70	69	0.00	2	0.6	333	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	203136	PASS
199	198	5	9	6.9	13930	PASS
365	198	1	100	4.7	9529	PASS
441	443	0.01	150	79.0	23674	PASS
442	442	100	100	100.0	145789	PASS
443	442	15	24	20.6	29979	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070225\
Data File : BN037424.D
Acq On : 02 Jul 2025 13:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 16:01:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

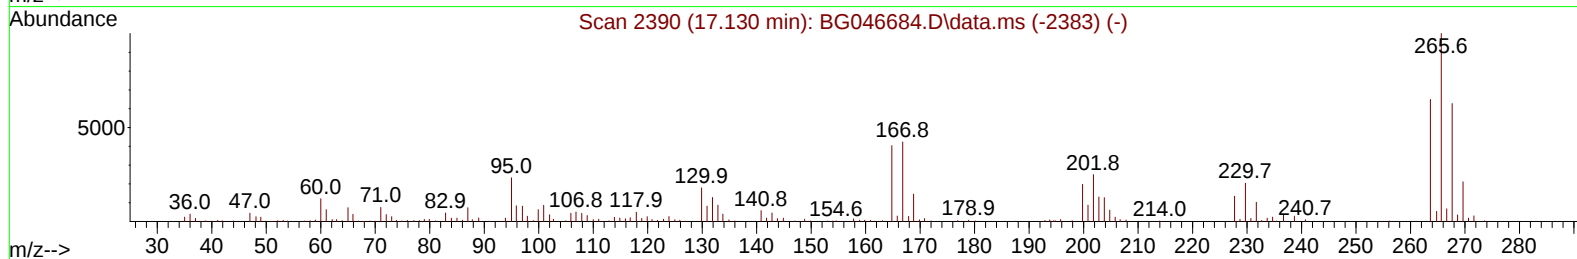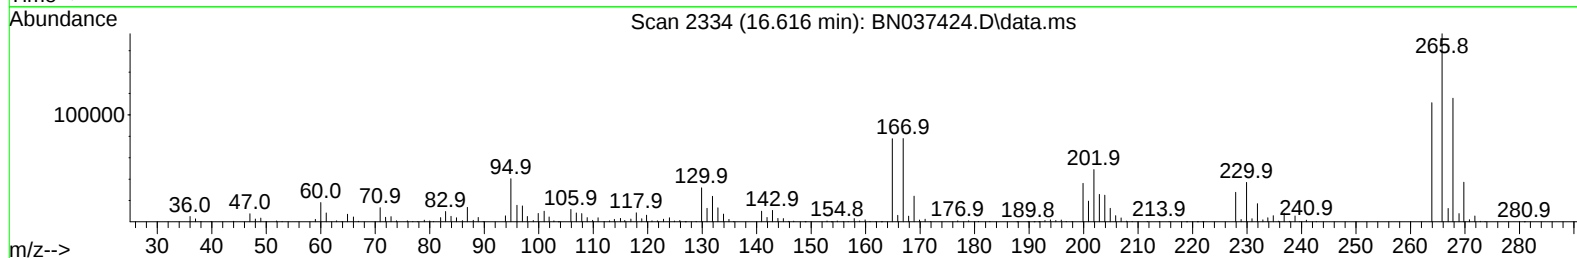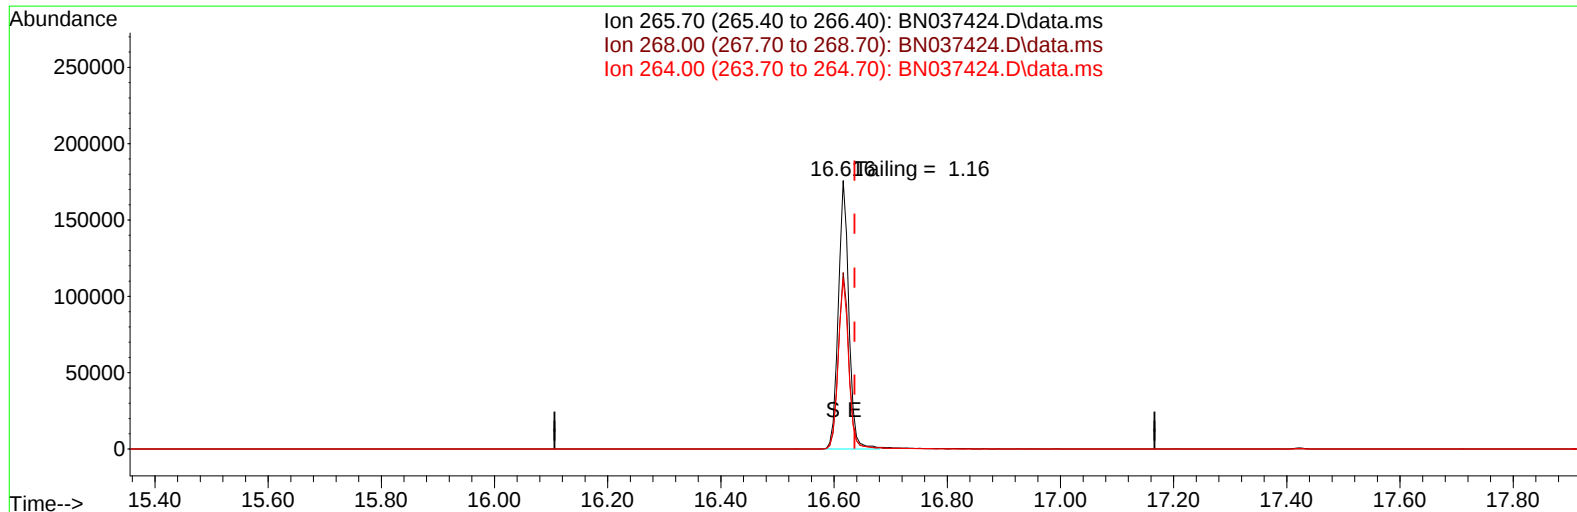

TIC: BN037424.D\data.ms

(70) Pentachlorophenol (C)

16.616min (-0.020) 20970.50 ng




response 228754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.73
264.00	61.60	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070225\
Data File : BN037424.D
Acq On : 02 Jul 2025 13:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 16:01:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

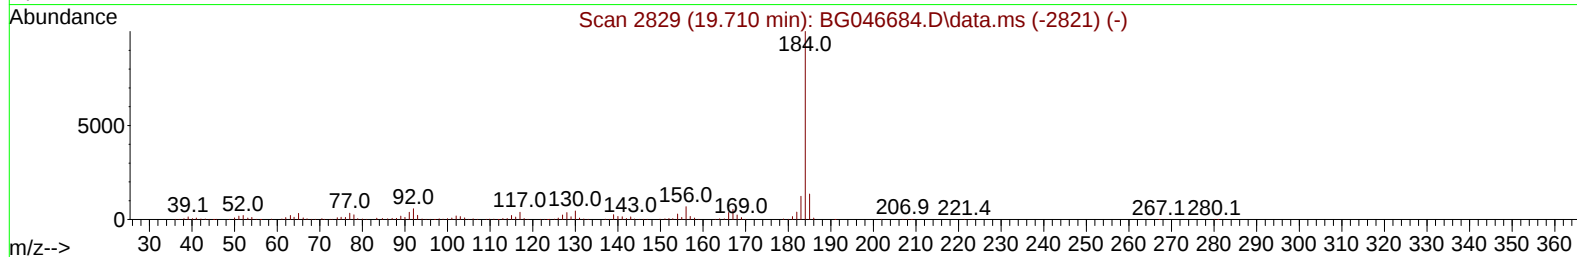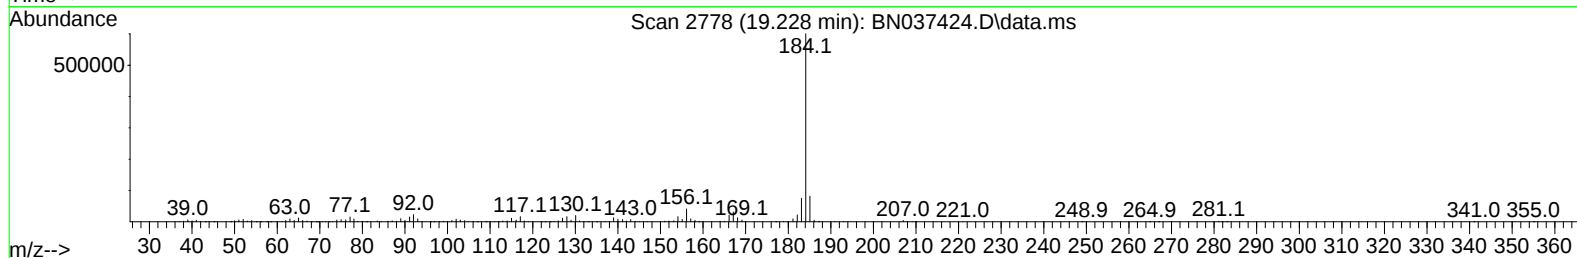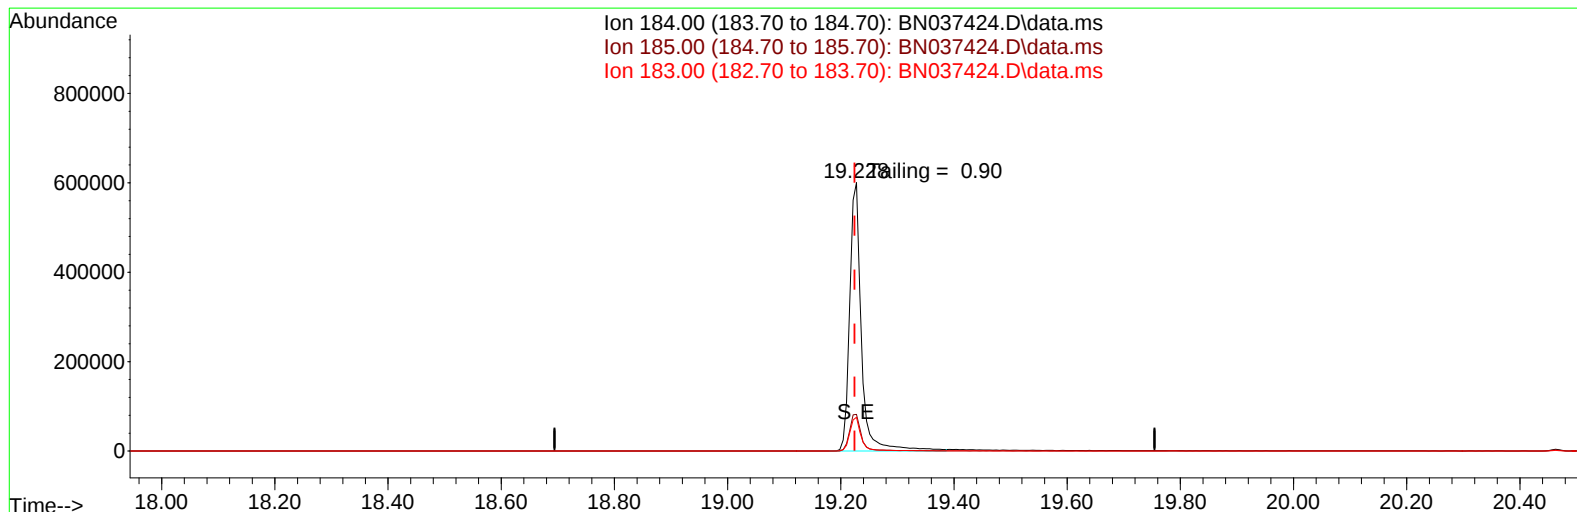

TIC: BN037424.D\data.ms

(77) Benzidine

19.228min (+ 0.004) 0.00 ng

response 863602

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	12.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/2/2025	BNA_N	<u>BN037424.D</u>
Compound Name	Response	Retention Time
DDT	689344	20.463
DDD	16883	20.022
DDE	2741	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19624	708968	2.77

Instrument :
BNA_N
ClientSampleId :
DFTPP