


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142940.D
Acq On : 01 Jul 2025 09:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

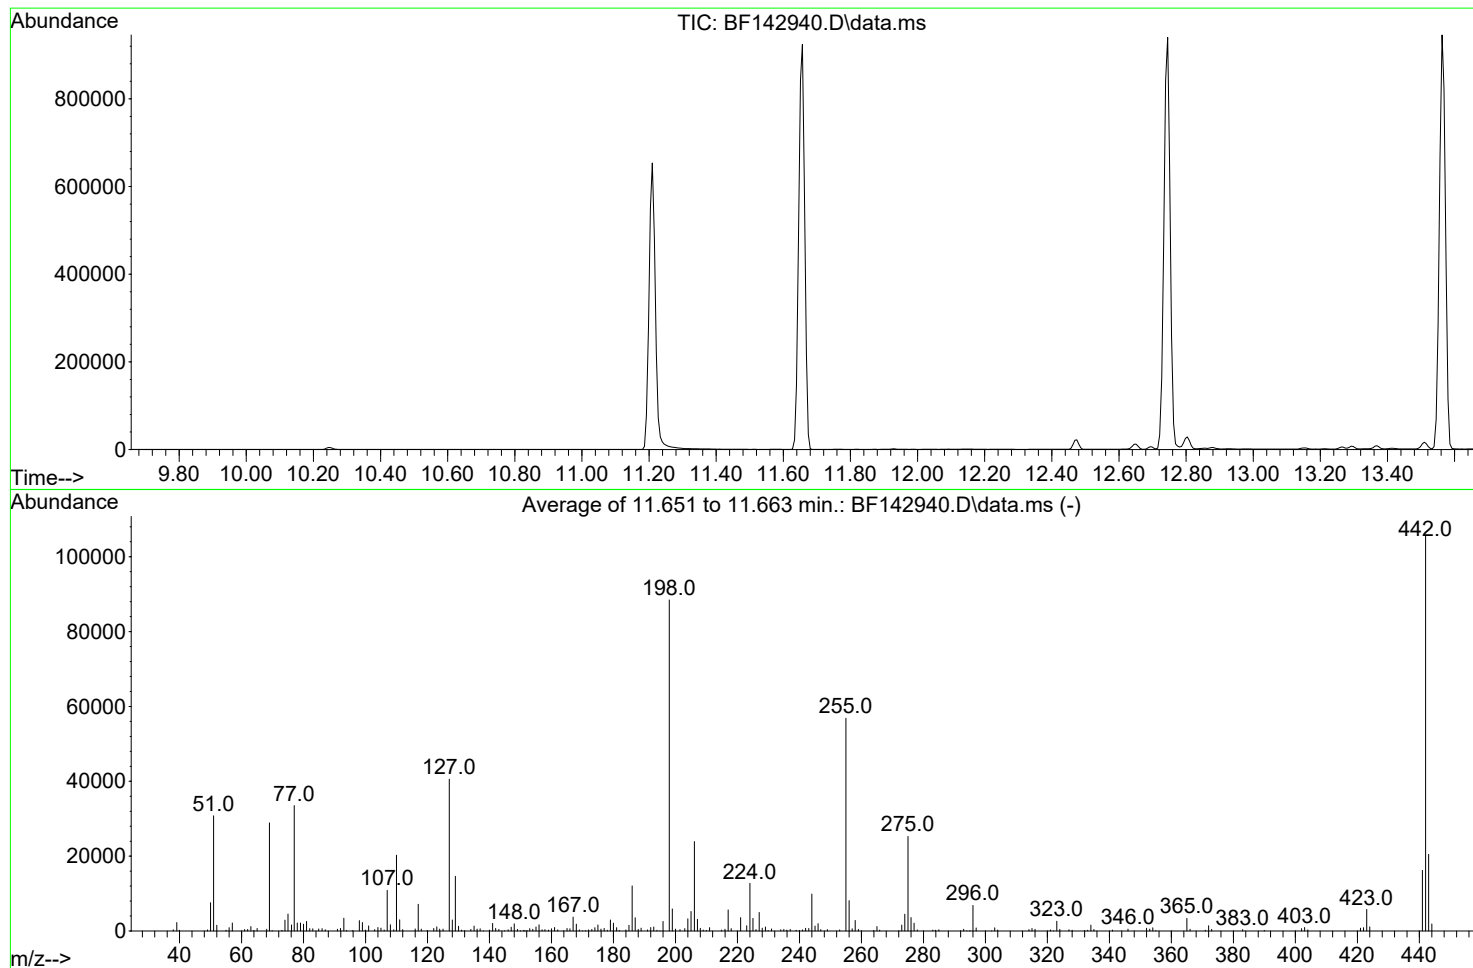

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1601

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	473	PASS
69	69	100	100	100.0	28920	PASS
70	69	0.00	2	0.5	142	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88464	PASS
199	198	5	9	6.7	5906	PASS
365	198	1	100	3.8	3402	PASS
441	443	0.01	150	79.1	16192	PASS
442	442	100	100	100.0	105496	PASS
443	442	15	24	19.4	20483	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/1/2025	BNA_F	<u>BF142940.D</u>
Compound Name	Response	Retention Time
DDT	242723	13.563
DDD	4666	13.292
DDE	432	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5098	247821	2.06

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142940.D
Acq On : 01 Jul 2025 09:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 11:49:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

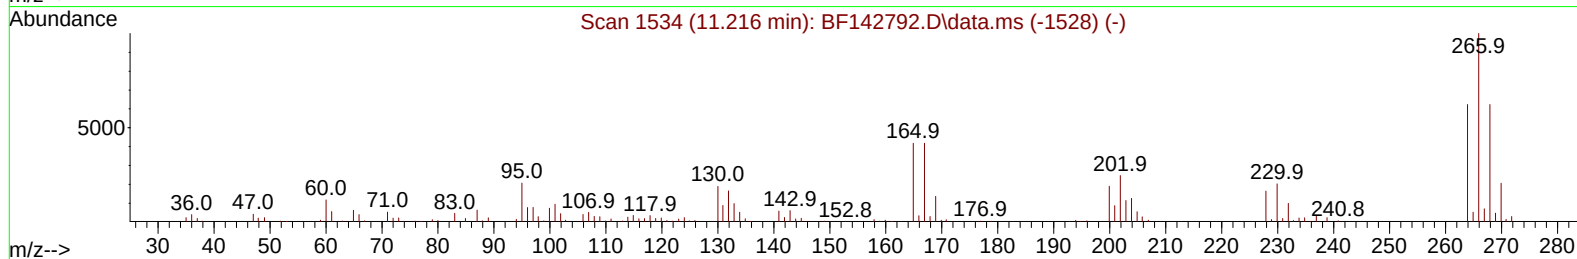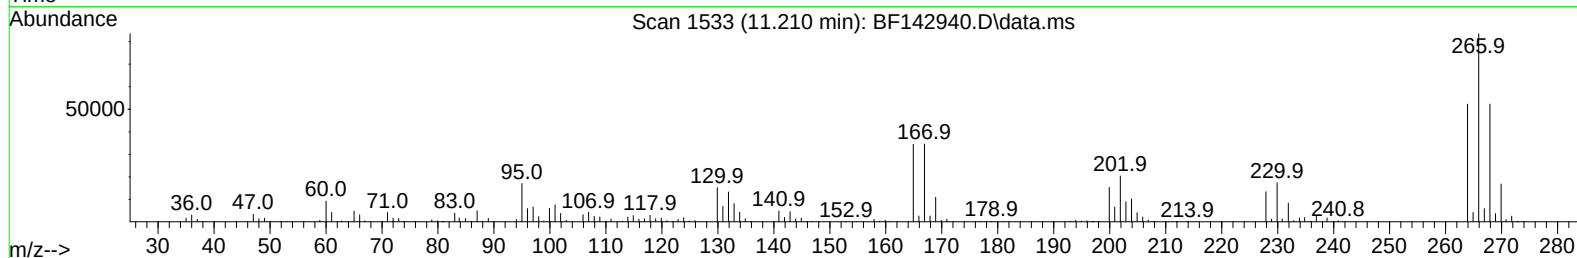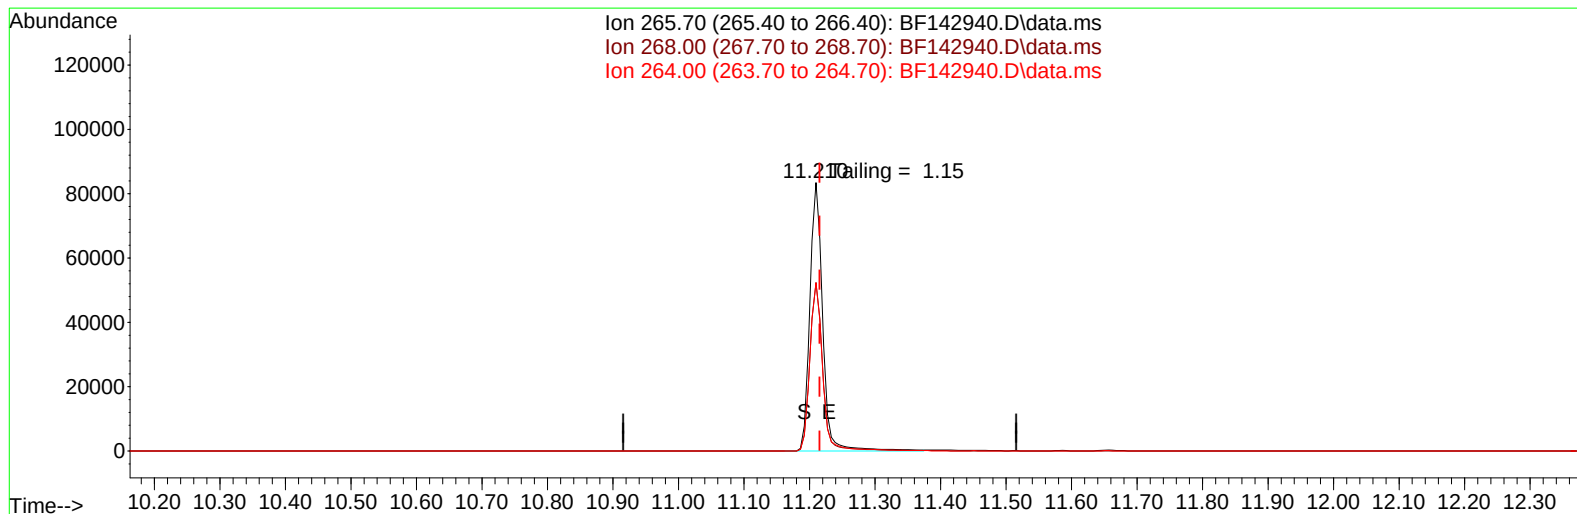

TIC: BF142940.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 34015.90 ng




response 113393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.73
264.00	62.40	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070125\
Data File : BF142940.D
Acq On : 01 Jul 2025 09:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 11:49:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

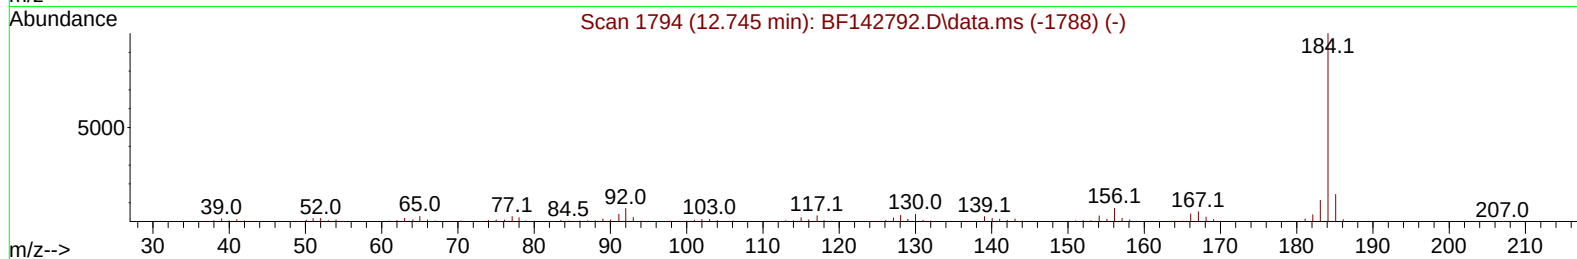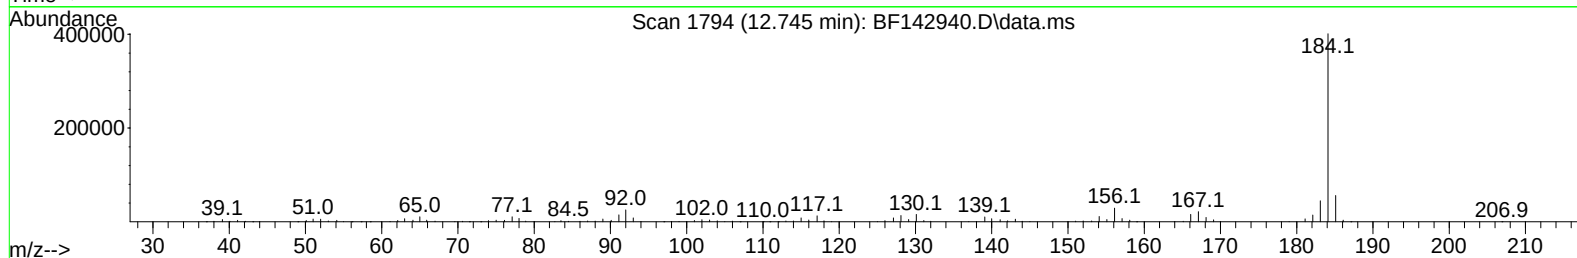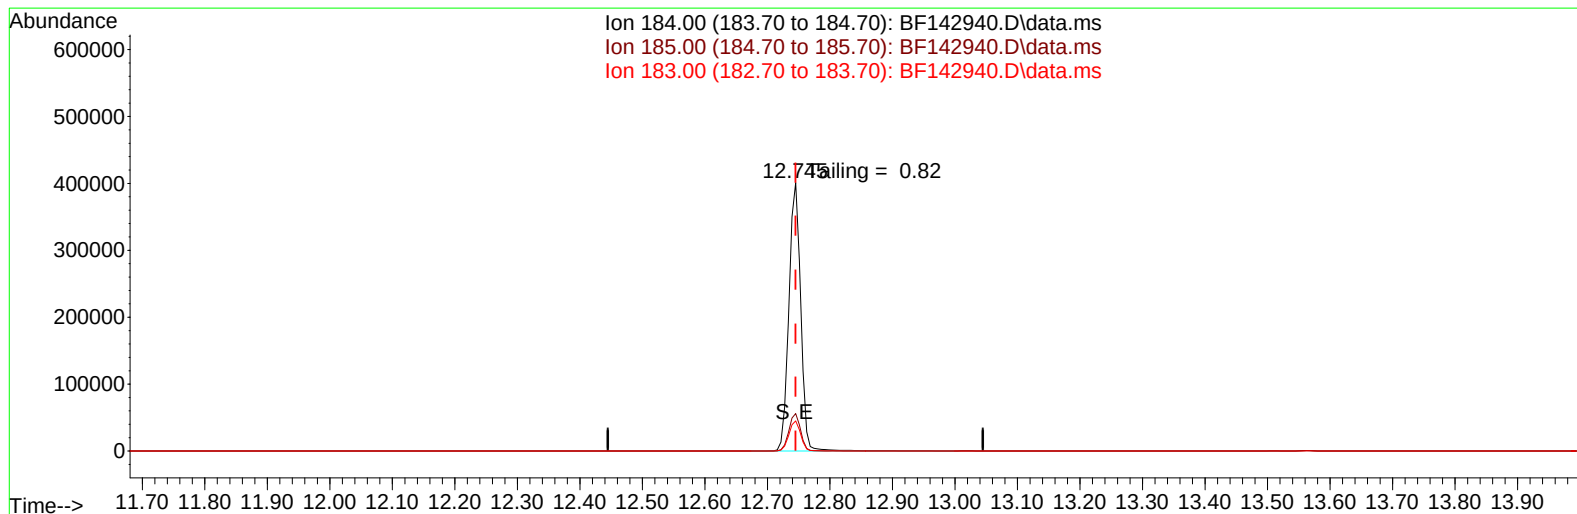

TIC: BF142940.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 528206

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.20	11.23
0.00	0.00	0.00