


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070225\
Data File : BF142963.D
Acq On : 02 Jul 2025 11:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

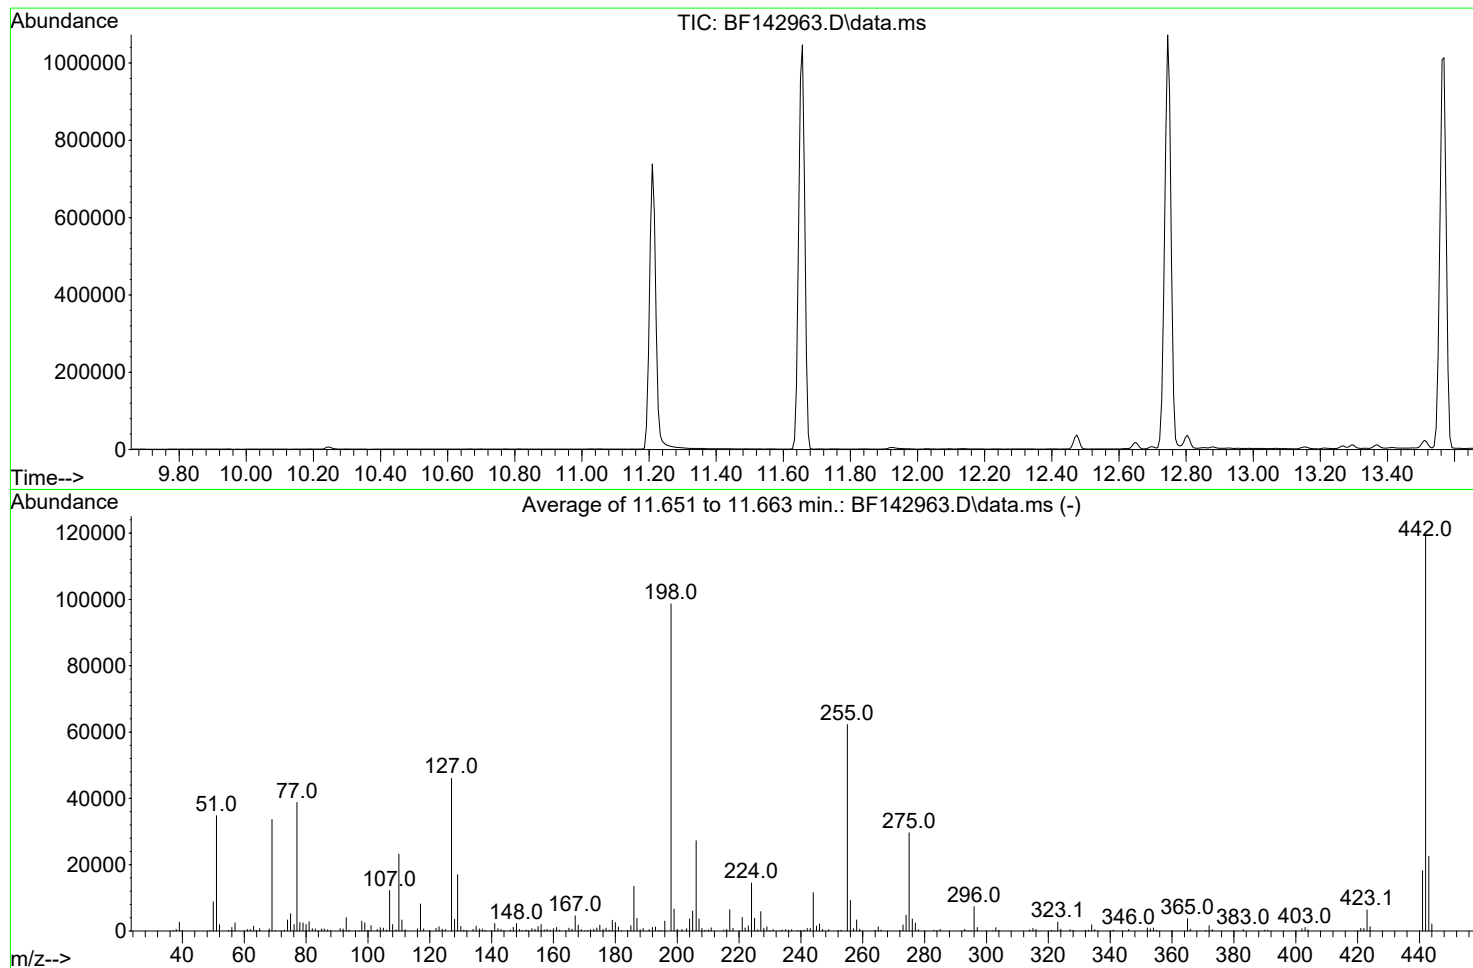

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	624	PASS
69	69	100	100	100.0	33651	PASS
70	69	0.00	2	0.4	133	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98616	PASS
199	198	5	9	6.7	6630	PASS
365	198	1	100	3.8	3728	PASS
441	443	0.01	150	81.0	18210	PASS
442	442	100	100	100.0	119077	PASS
443	442	15	24	18.9	22491	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/2/2025	BNA_F	<u>BF142963.D</u>
Compound Name	Response	Retention Time
DDT	275405	13.569
DDD	6210	13.292
DDE	759	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6969	282374	2.47

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070225\
Data File : BF142963.D
Acq On : 02 Jul 2025 11:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 12:34:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

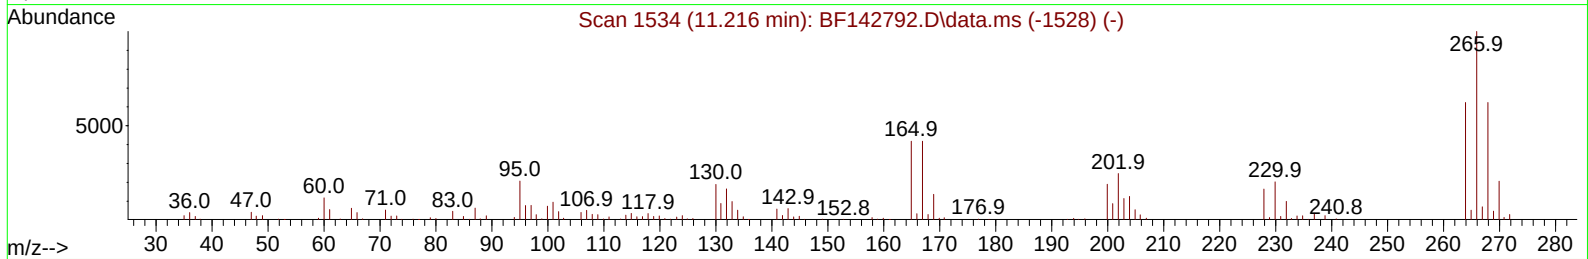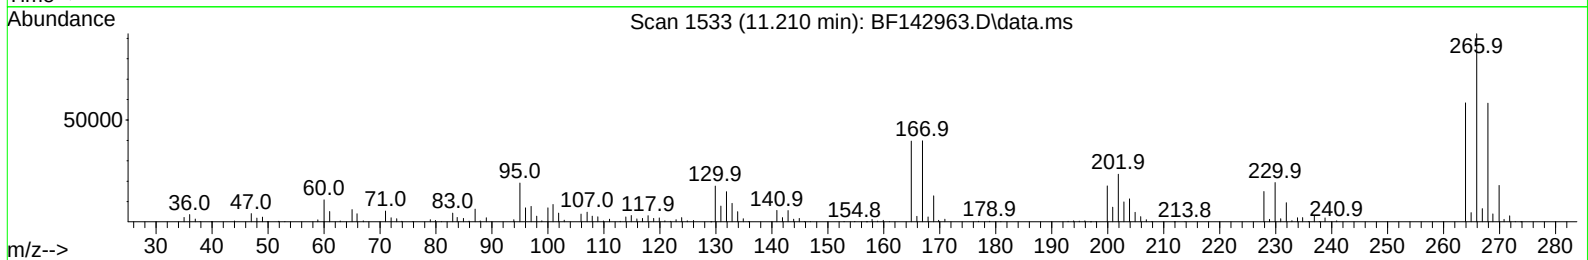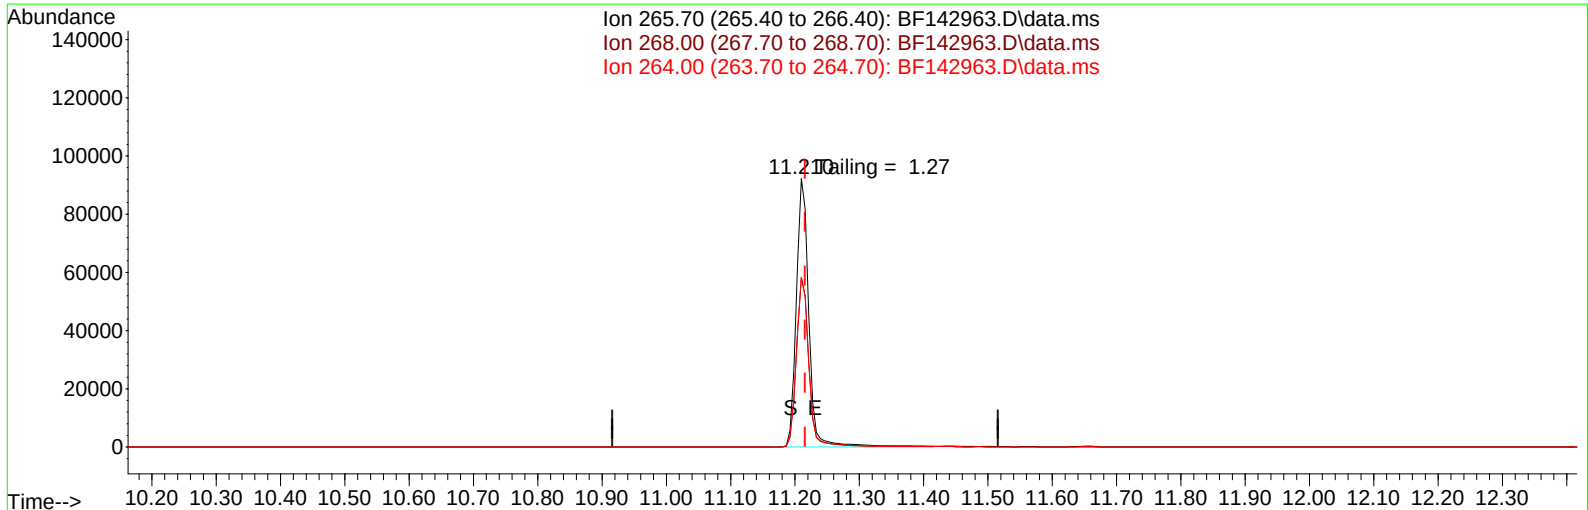

TIC: BF142963.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 40110.10 ng




response 126631

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.15
264.00	62.40	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070225\
Data File : BF142963.D
Acq On : 02 Jul 2025 11:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 12:34:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

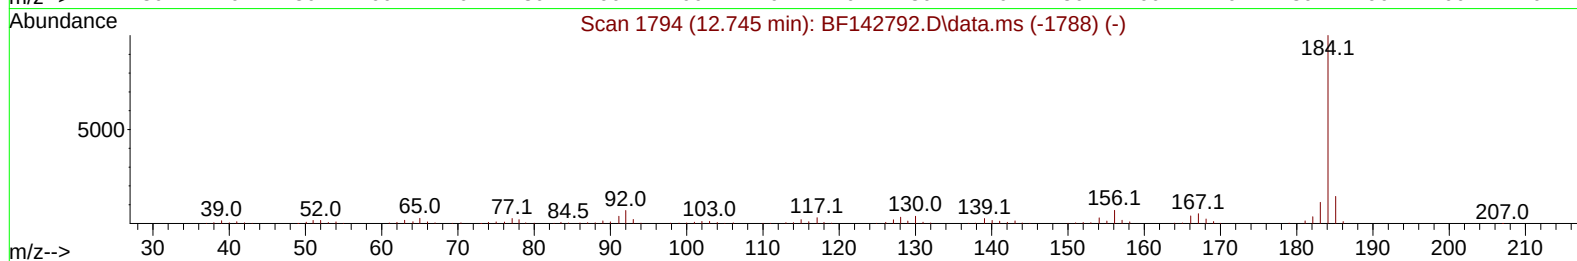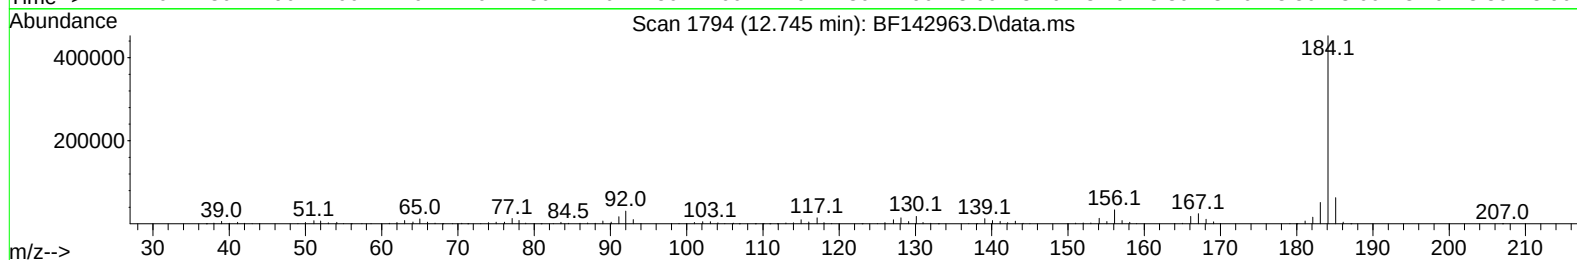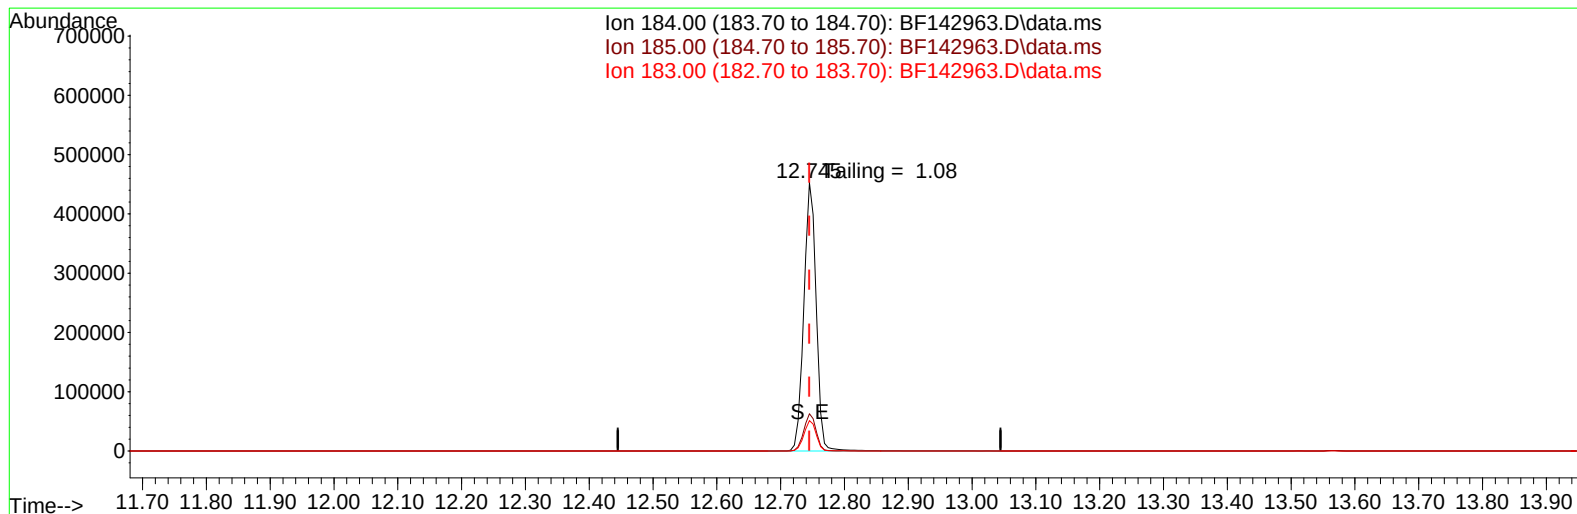

TIC: BF142963.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 612096

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.89
183.00	11.20	11.35
0.00	0.00	0.00