
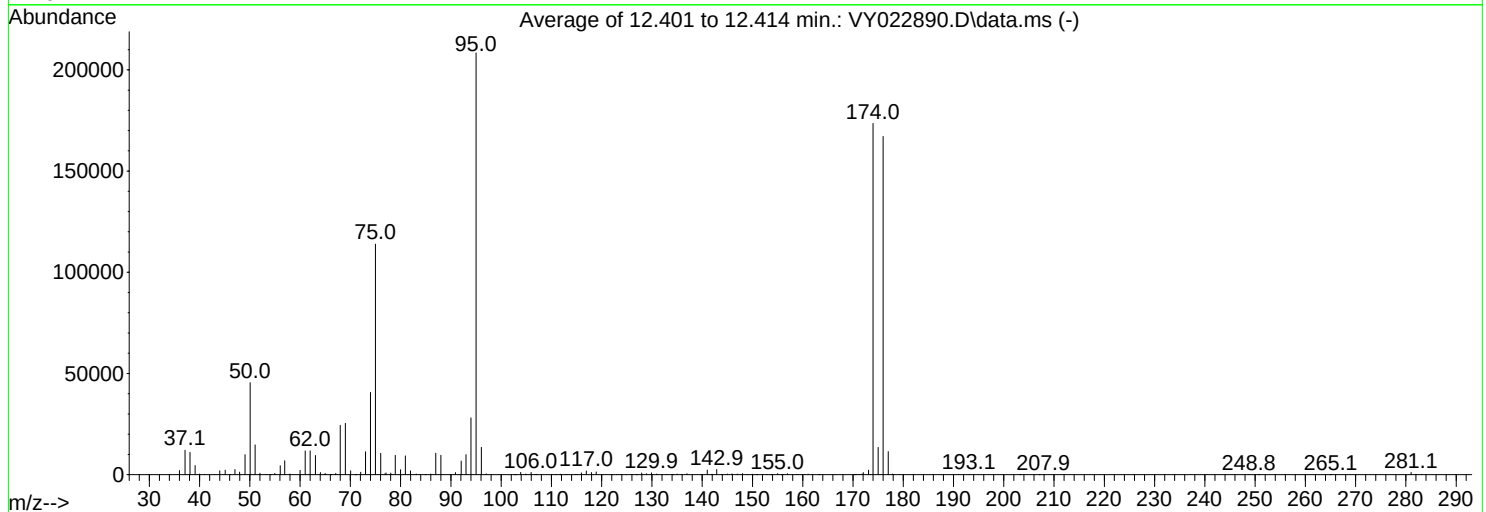


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070125\
Data File : VY022890.D
Acq On : 01 Jul 2025 08:47
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Title : SW846 8260
Last Update : Tue Jun 24 08:29:52 2025

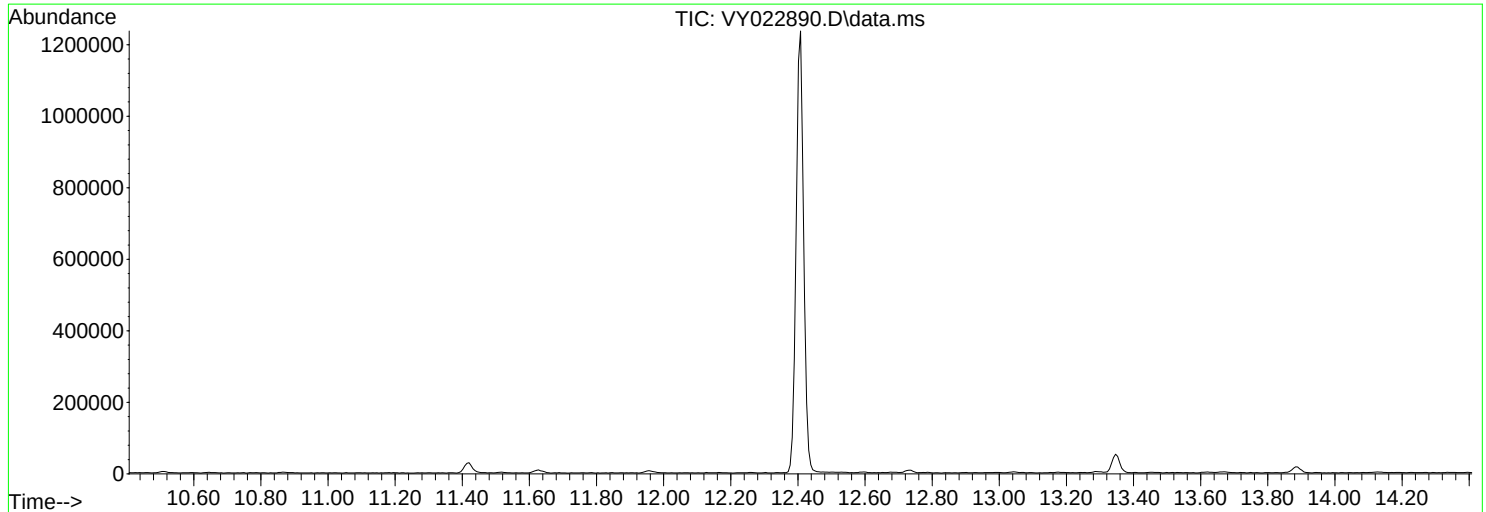

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	45461	PASS
75	95	30	60	54.7	113920	PASS
95	95	100	100	100.0	208405	PASS
96	95	5	9	6.5	13554	PASS
173	174	0.00	2	1.3	2202	PASS
174	95	50	100	83.3	173525	PASS
175	174	5	9	7.7	13418	PASS
176	174	95	101	96.3	167104	PASS
177	176	5	9	6.8	11381	PASS