

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061125\
 Data File : P0111586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2025 10:21
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 12:10:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 11 12:09:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.677	3.673	117.0E6	106.8E6	20.308	19.004
2) SA Decachlor...	8.713	8.662	108.8E6	36486352	20.730	20.525

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061125\
Data File : PO111586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2025 10:21
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 12:10:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 11 12:09:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

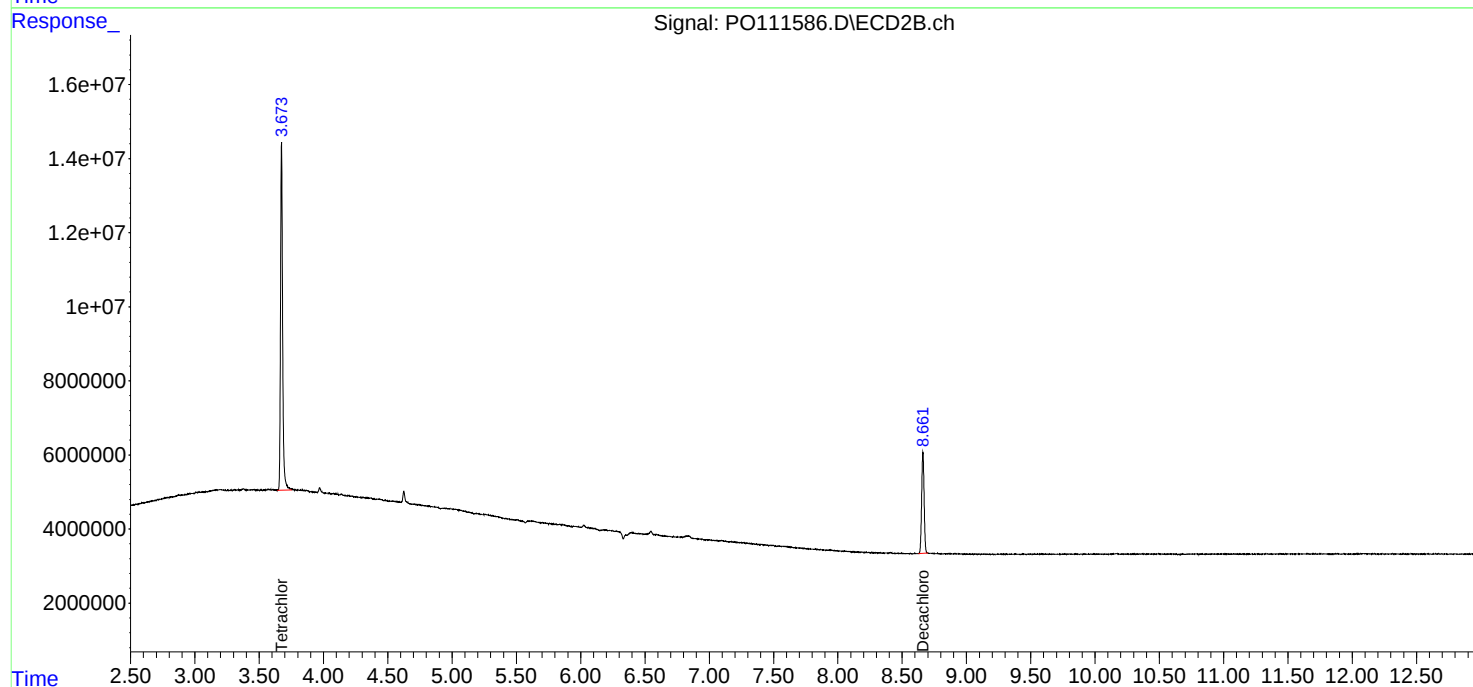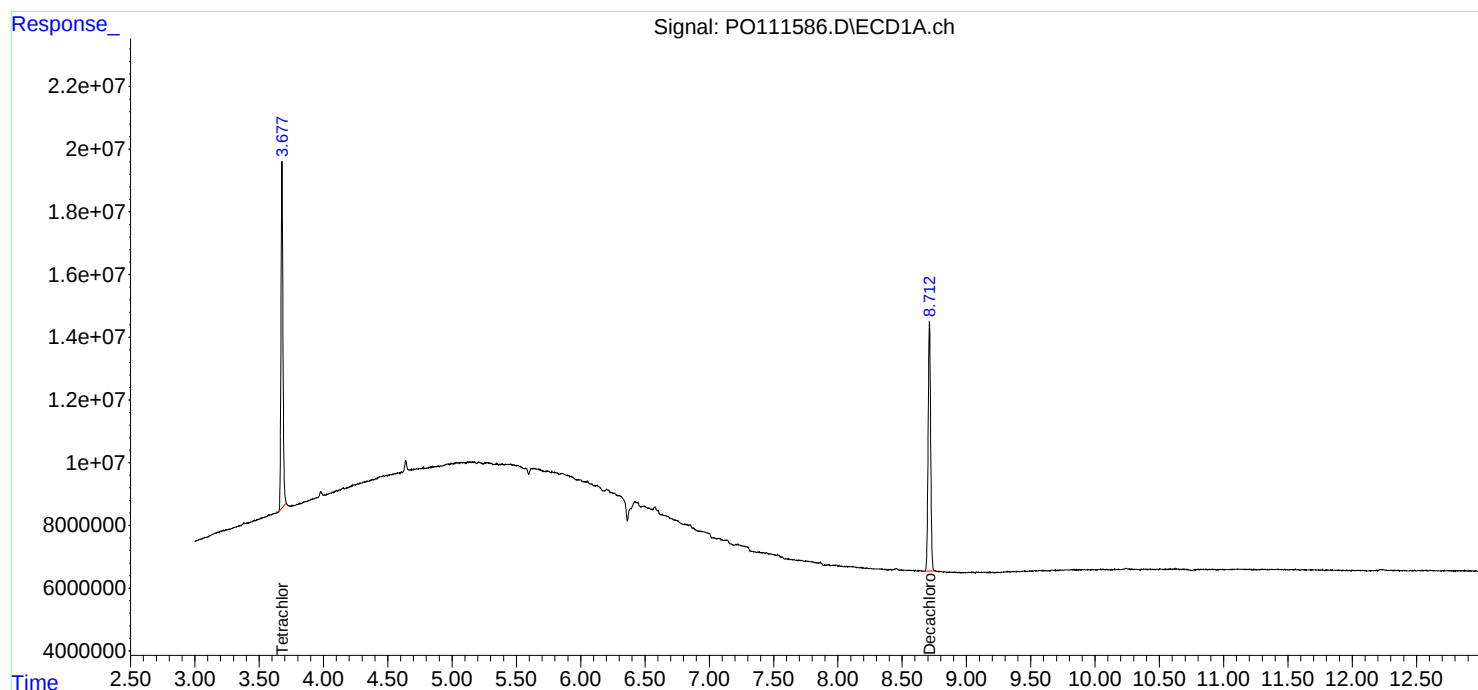


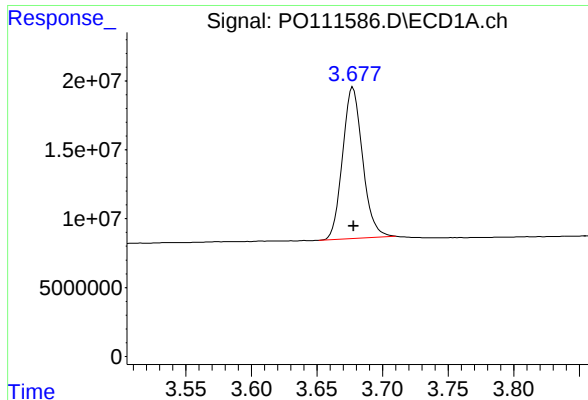

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 116962361
Conc: 20.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

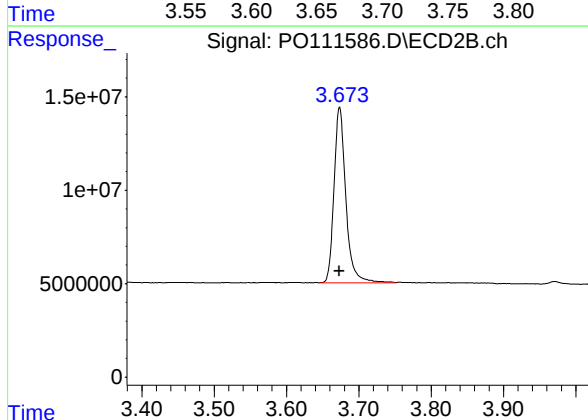


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 106750459
Conc: 19.00 ng/ml

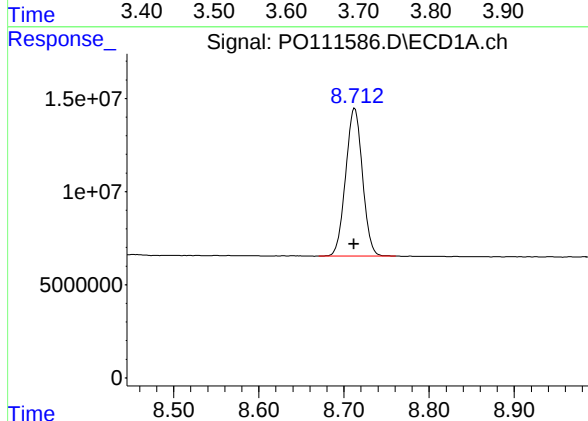

#2 Decachlorobiphenyl

R.T.: 8.713 min
Delta R.T.: 0.001 min
Response: 108816924
Conc: 20.73 ng/ml

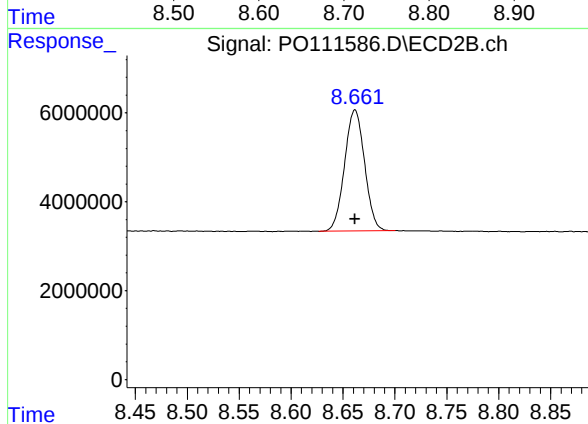

#2 Decachlorobiphenyl

R.T.: 8.662 min
Delta R.T.: 0.000 min
Response: 36486352
Conc: 20.52 ng/ml