


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061725\
Data File : VX046715.D
Acq On : 17 Jun 2025 08:46
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Title : SW846 8260
Last Update : Wed Jun 18 03:09:16 2025

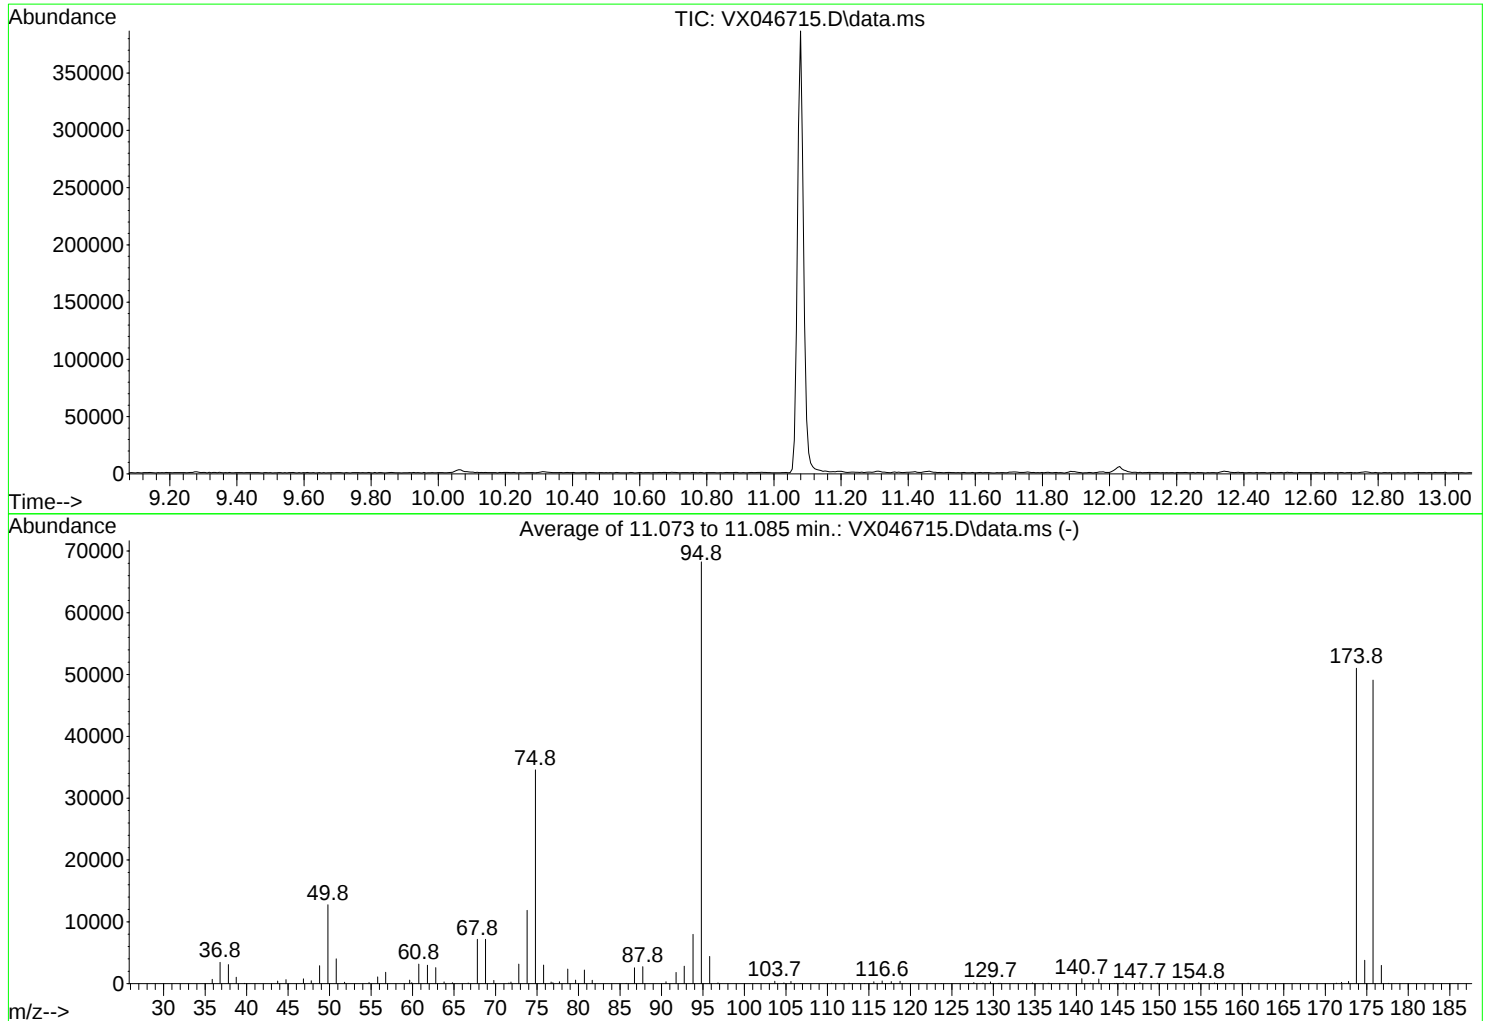

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	12764	PASS
75	95	30	60	50.7	34573	PASS
95	95	100	100	100.0	68235	PASS
96	95	5	9	6.5	4402	PASS
173	174	0.00	2	0.7	374	PASS
174	95	50	100	74.8	51016	PASS
175	174	5	9	7.4	3785	PASS
176	174	95	101	96.2	49101	PASS
177	176	5	9	6.0	2956	PASS