

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
 Data File : PP073459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 16:36
 Operator : YP\AJ
 Sample : Q2473-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PIT#3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2025
 Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:37:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 02 04:02:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.487	3.783	32535098	38072236	20.382m	21.467
2) SA Decachlor...	10.180	8.789	25526825	26038364	17.964	18.819

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP070225\
Data File : PP073459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 16:36
Operator : YP\AJ
Sample : Q2473-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PIT#3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:37:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 02 04:02:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

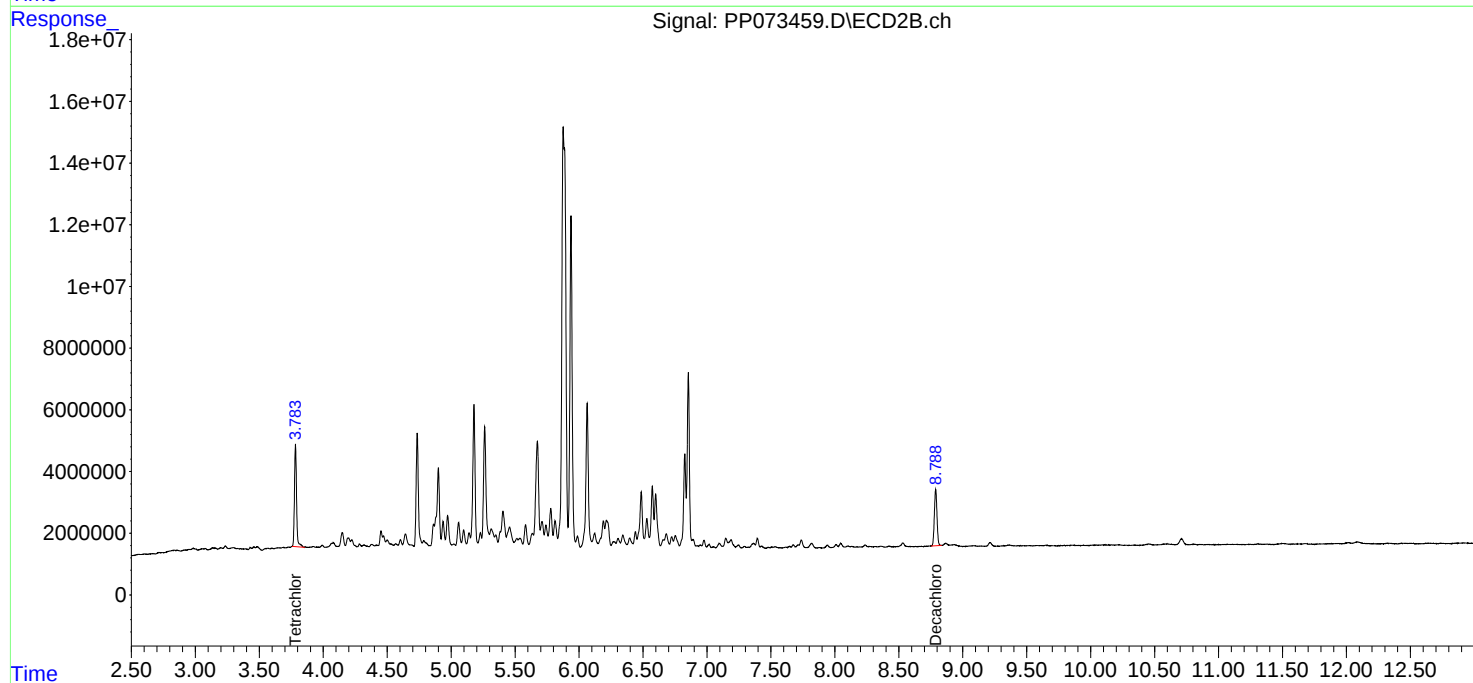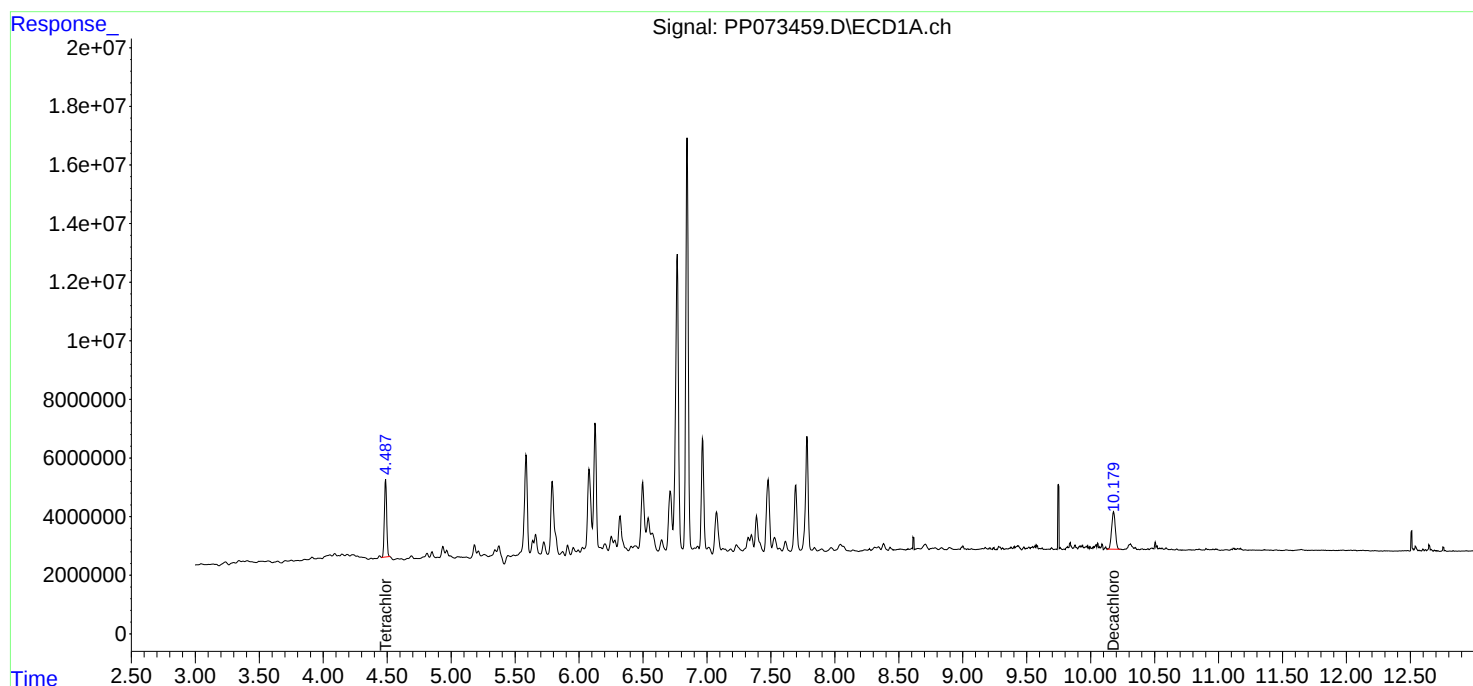

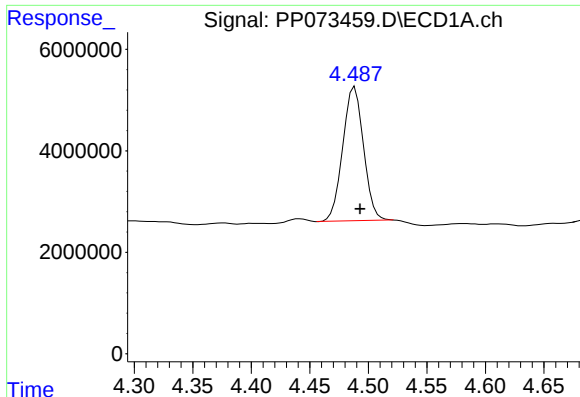


#1 Tetrachloro-m-xylene

R.T.: 4.487 min
Delta R.T.: -0.006 min
Response: 32535098
Conc: 20.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
PIT#3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

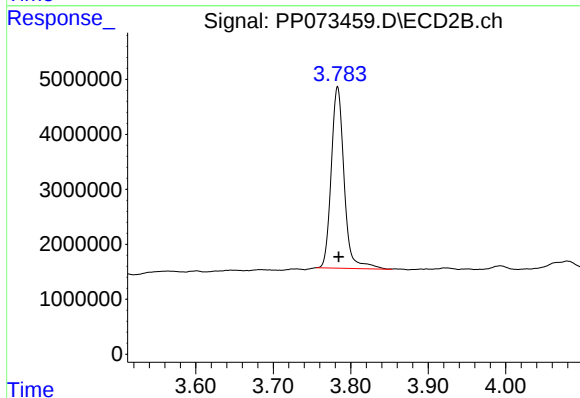


#1 Tetrachloro-m-xylene

R.T.: 3.783 min
Delta R.T.: -0.001 min
Response: 38072236
Conc: 21.47 ng/ml

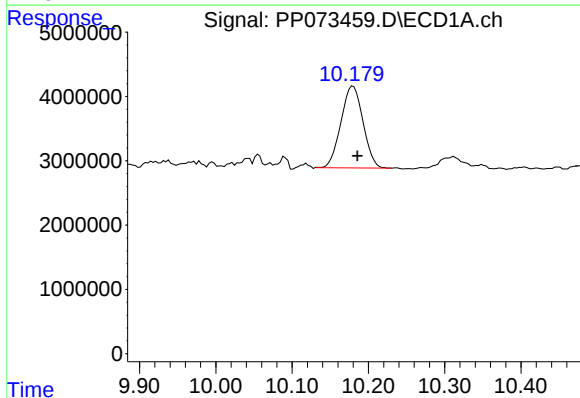

#2 Decachlorobiphenyl

R.T.: 10.180 min
Delta R.T.: -0.006 min
Response: 25526825
Conc: 17.96 ng/ml

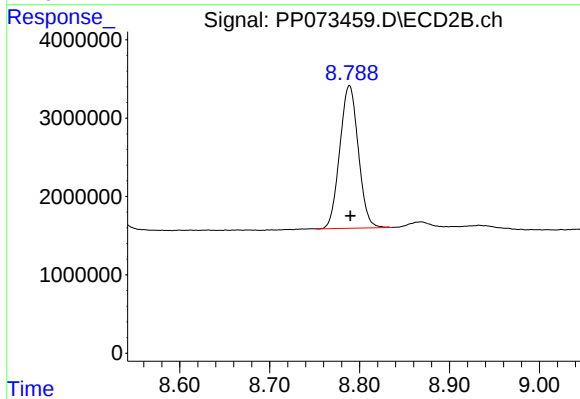

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.001 min
Response: 26038364
Conc: 18.82 ng/ml