


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070325\
Data File : BF142986.D
Acq On : 03 Jul 2025 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

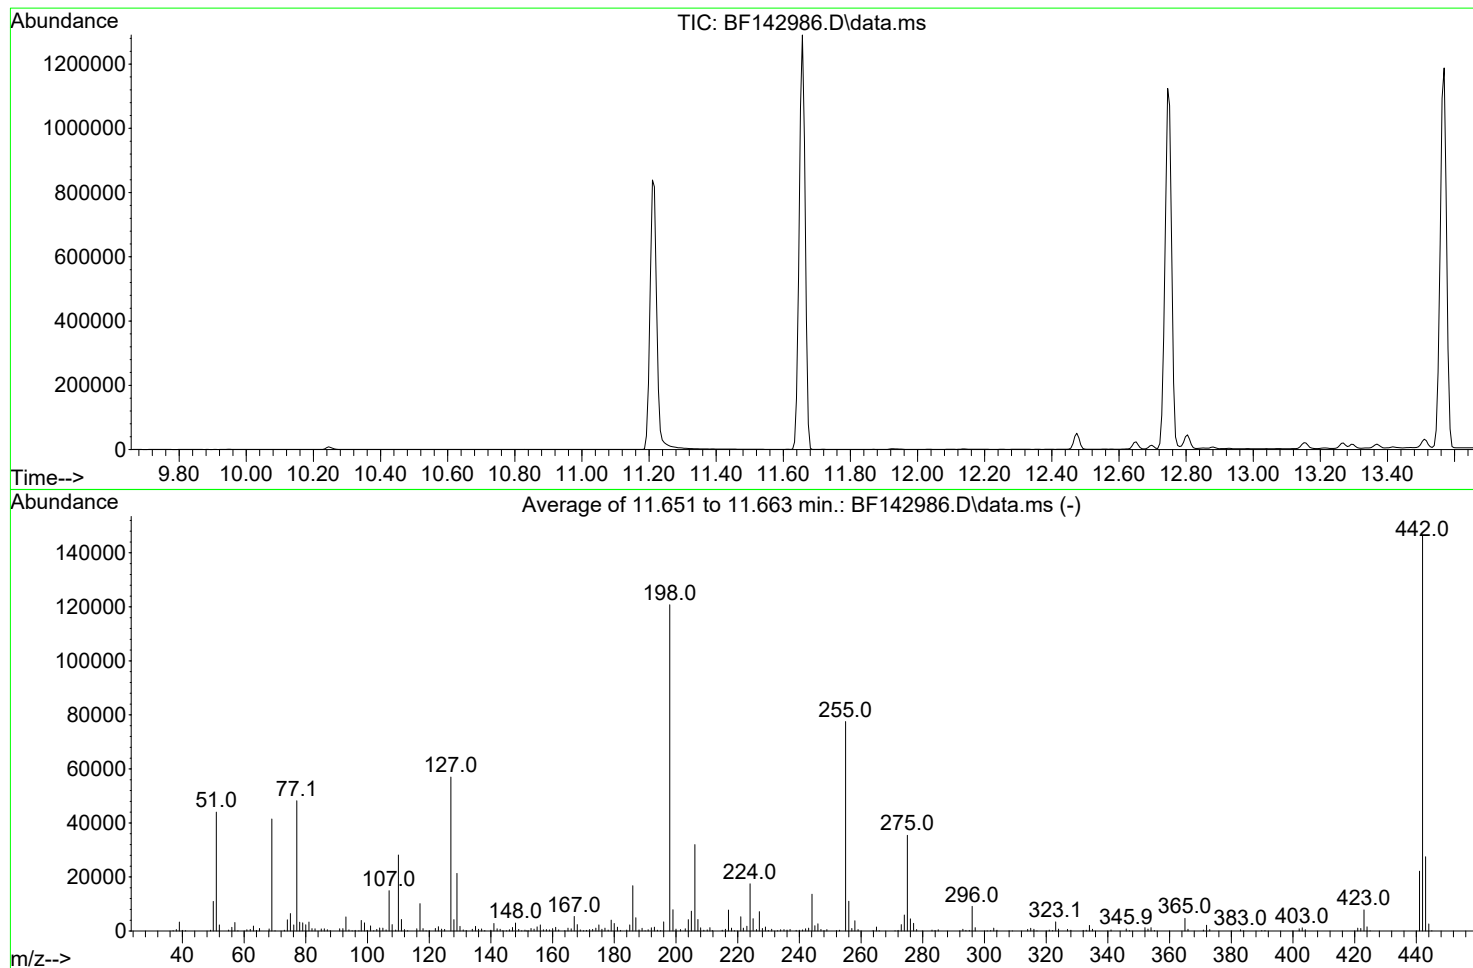

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1601

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	753	PASS
69	69	100	100	100.0	41448	PASS
70	69	0.00	2	0.3	128	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120760	PASS
199	198	5	9	6.5	7874	PASS
365	198	1	100	3.9	4686	PASS
441	443	0.01	150	80.6	22149	PASS
442	442	100	100	100.0	146165	PASS
443	442	15	24	18.8	27493	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
7/3/2025	BNA_F	<u>BF142940.D</u>
Compound Name	Response	Retention Time
DDT	315072	13.569
DDD	9738	13.269
DDE	534	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10272	325344	3.16

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070325\
Data File : BF142986.D
Acq On : 03 Jul 2025 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 03 11:16:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

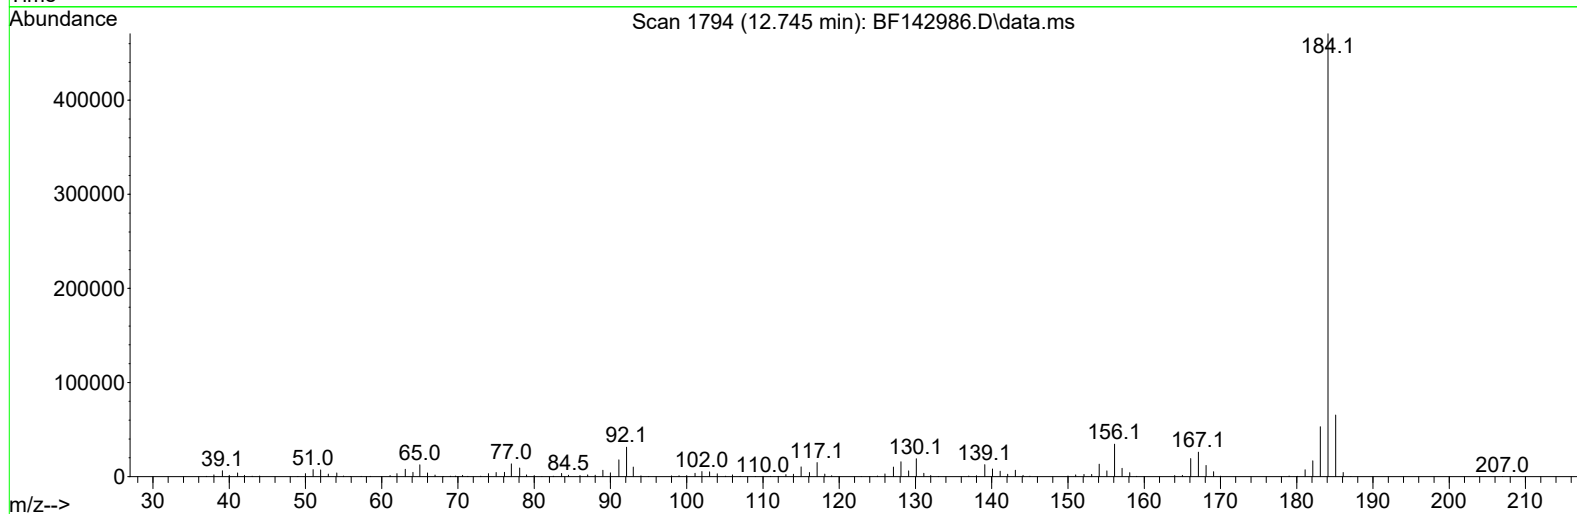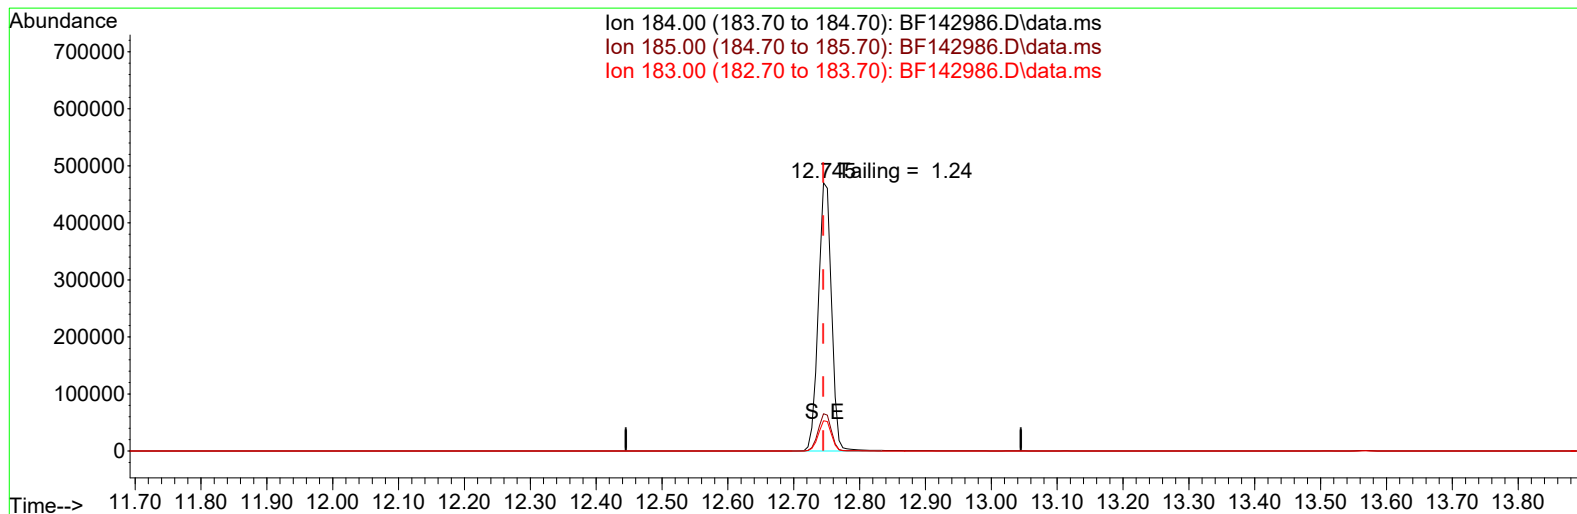

TIC: BF142986.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng



response 654353

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.91
183.00	11.20	11.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070325\
Data File : BF142986.D
Acq On : 03 Jul 2025 09:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 03 11:16:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

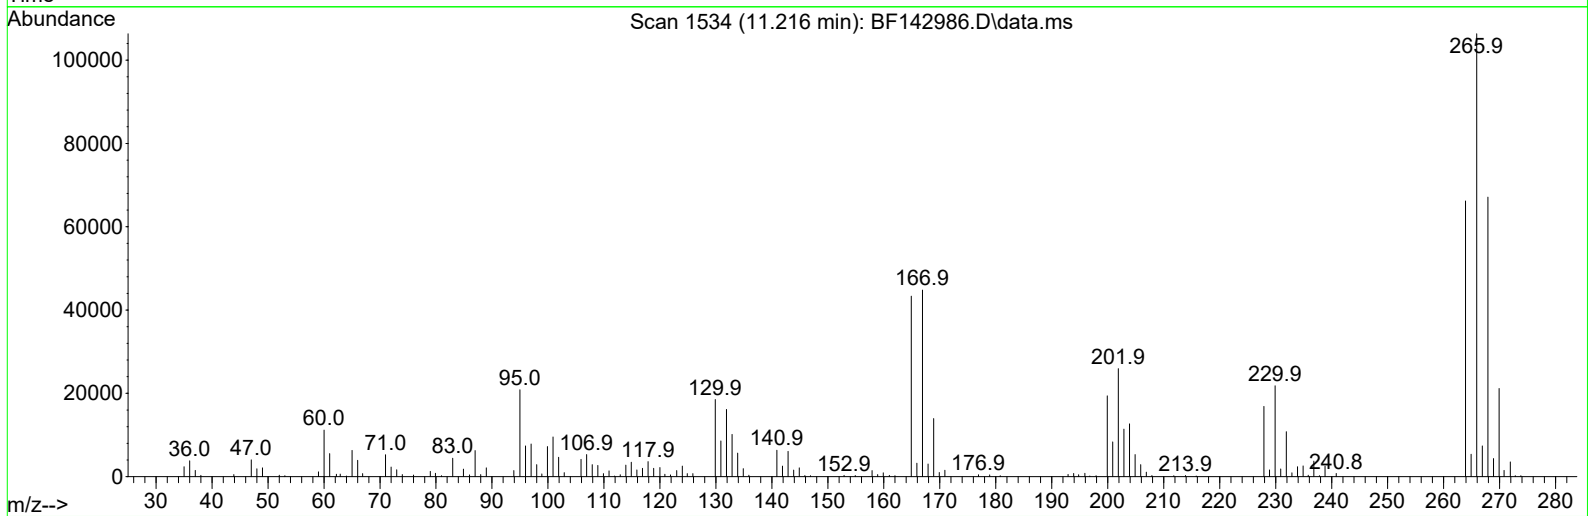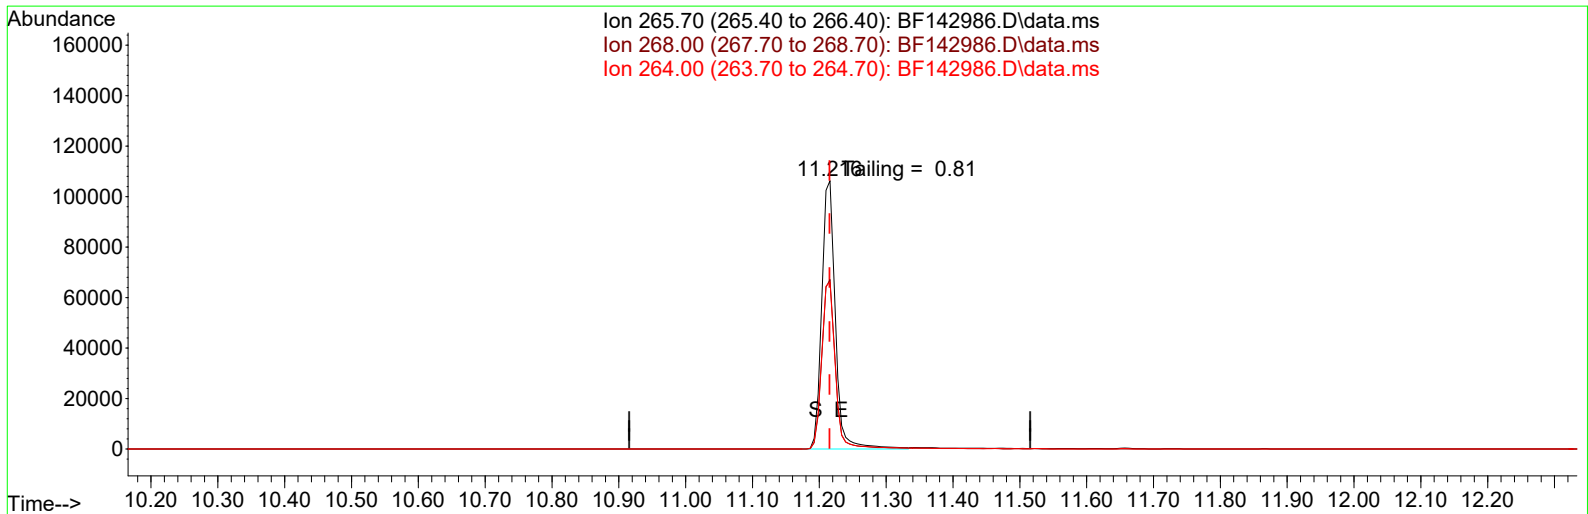

TIC: BF142986.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 44040.02 ng

response 150694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.11
264.00	62.40	62.24
0.00	0.00	0.00