
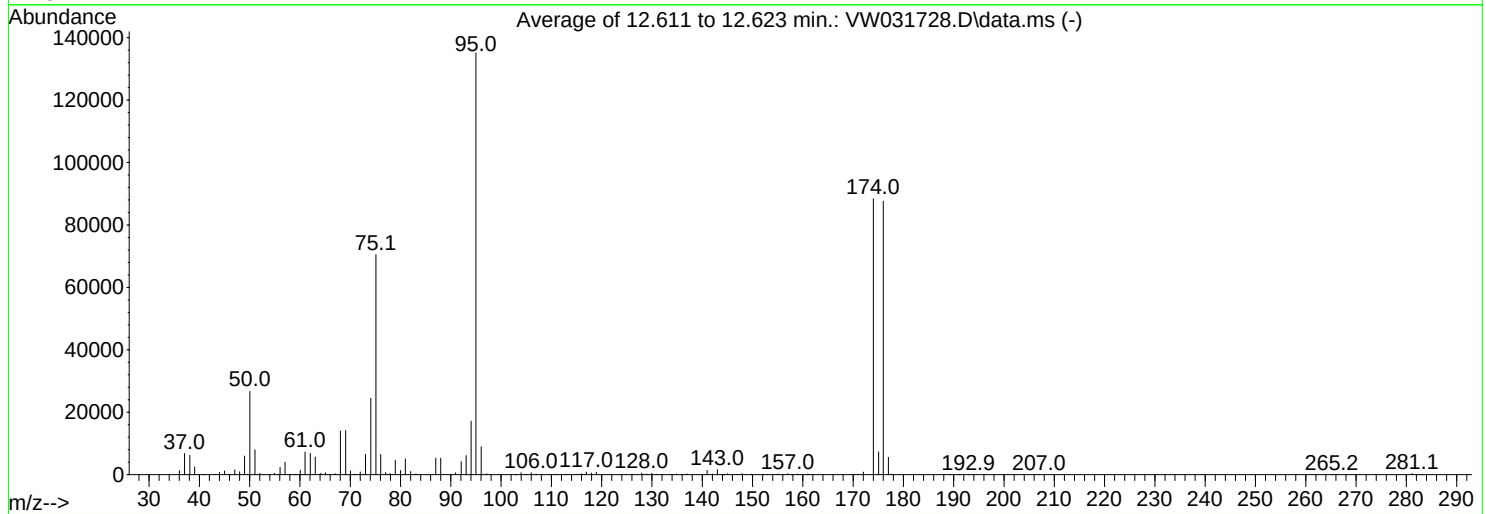


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW063025\  
Data File : VW031728.D  
Acq On : 30 Jun 2025 08:56  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\82W063025S.M  
Title : SW846 8260  
Last Update : Tue Jul 01 03:35:17 2025

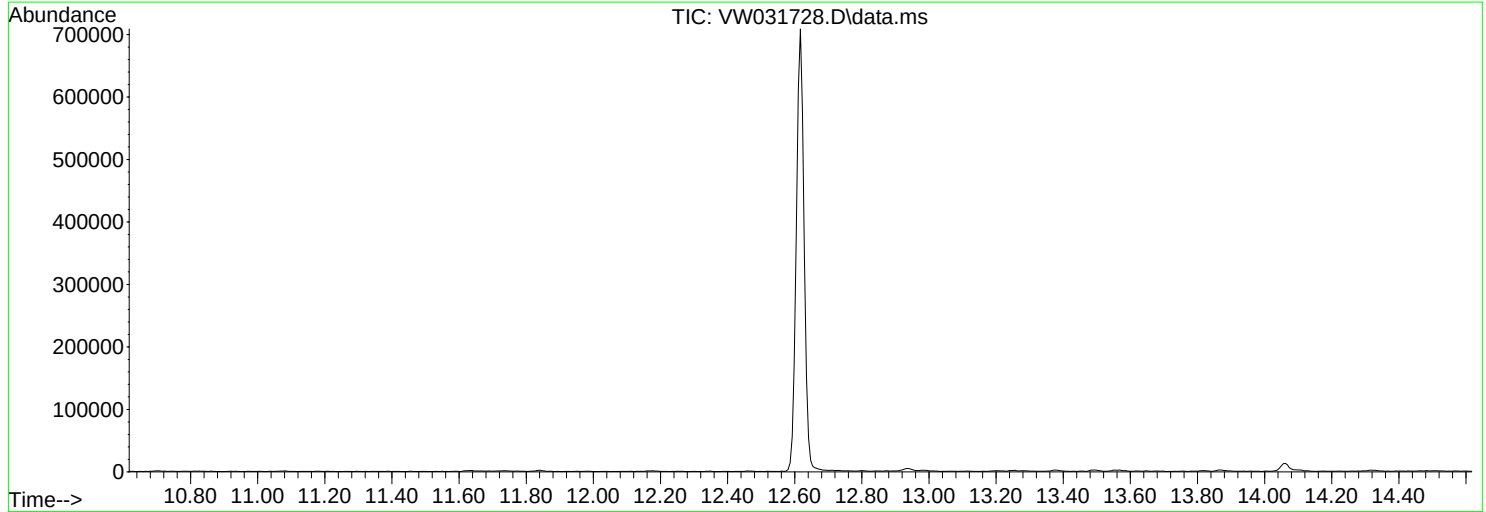

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.7         | 26685      | PASS                |
| 75             | 95              | 30              | 60              | 52.1         | 70472      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 135149     | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 8992       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 65.4         | 88384      | PASS                |
| 175            | 174             | 5               | 9               | 8.2          | 7275       | PASS                |
| 176            | 174             | 95              | 101             | 99.2         | 87643      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 5529       | PASS                |