


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071025\
Data File : VW031790.D
Acq On : 10 Jul 2025 08:16
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Title : SW846 8260
Last Update : Tue Jul 01 03:35:17 2025

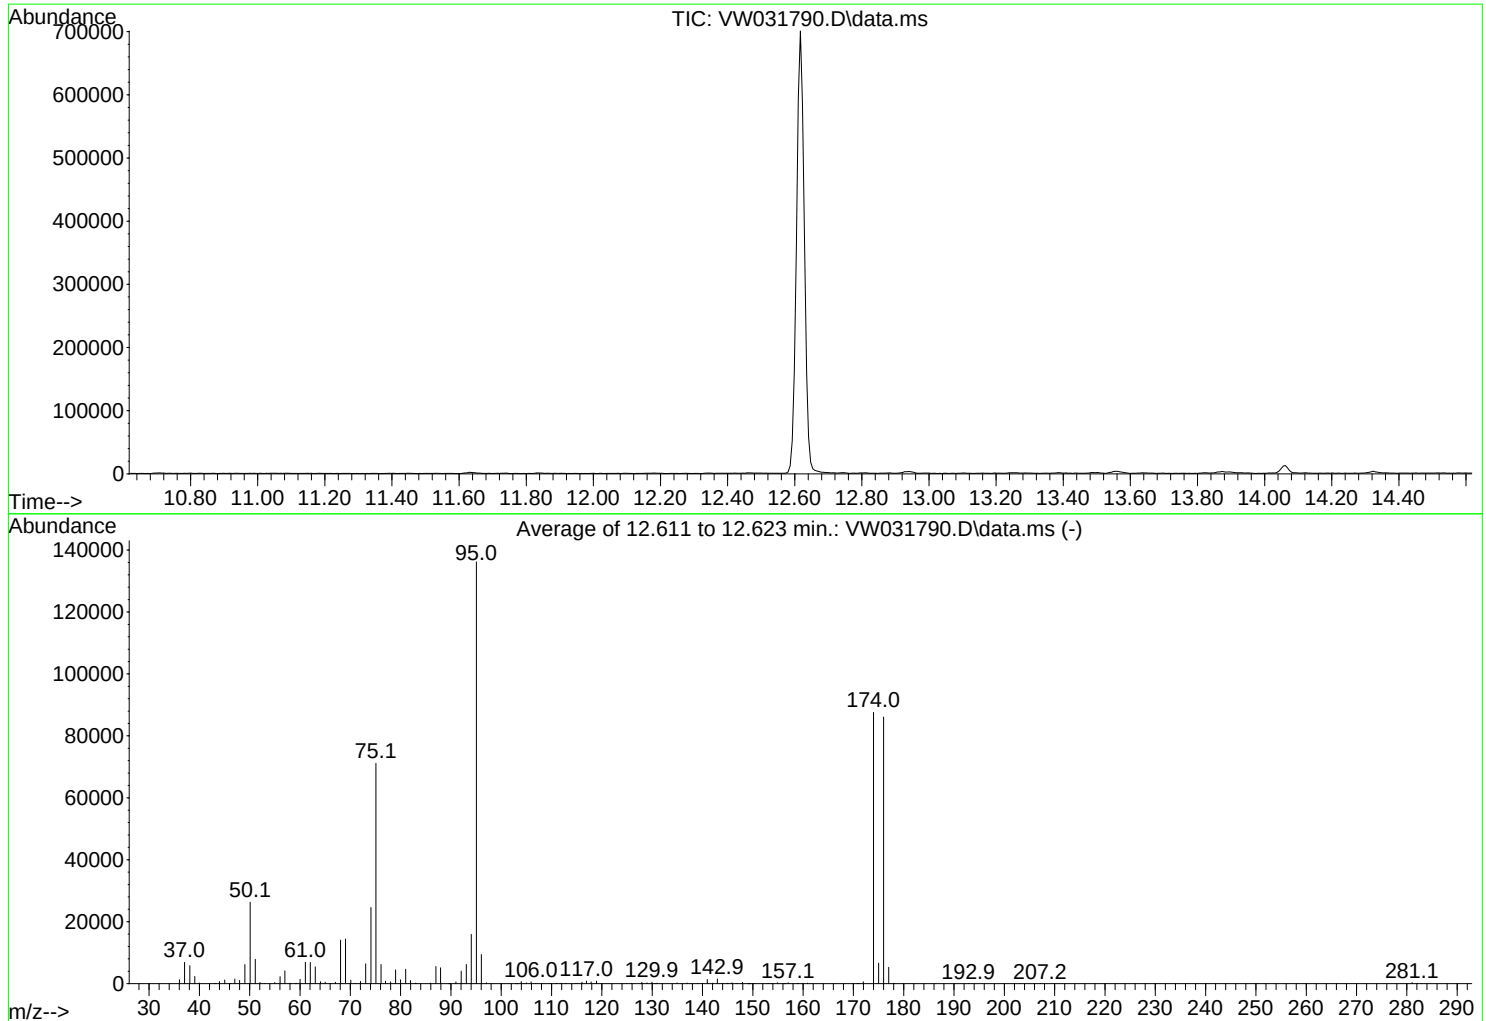

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	26320	PASS
75	95	30	60	52.2	71152	PASS
95	95	100	100	100.0	136197	PASS
96	95	5	9	6.9	9431	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	64.3	87584	PASS
175	174	5	9	7.6	6647	PASS
176	174	95	101	98.3	86056	PASS
177	176	5	9	6.1	5274	PASS