
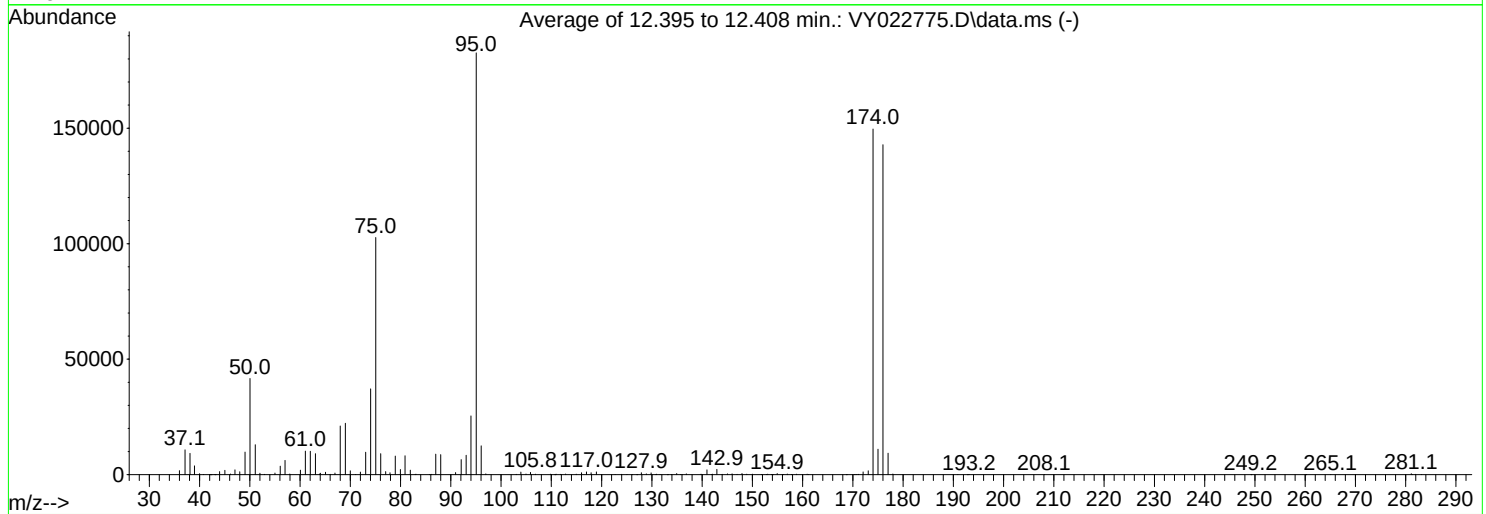


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062325\
Data File : VY022775.D
Acq On : 23 Jun 2025 10:17
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Title : SW846 8260
Last Update : Tue Jun 24 08:29:52 2025

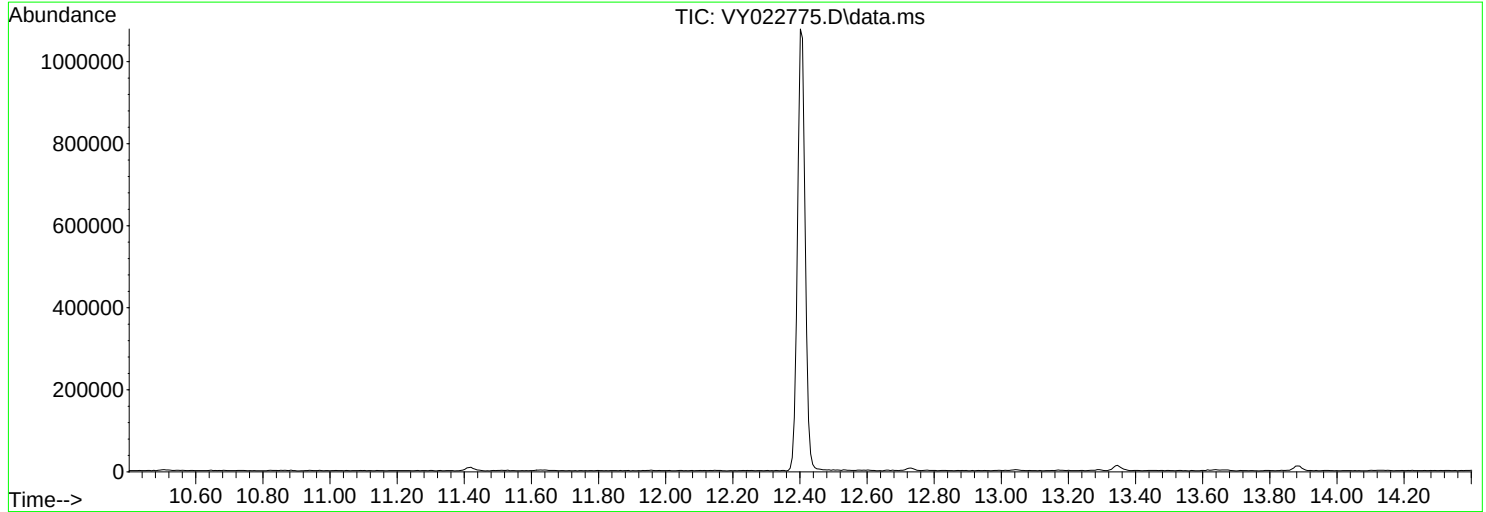

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.8	41667	PASS
75	95	30	60	56.2	102659	PASS
95	95	100	100	100.0	182635	PASS
96	95	5	9	6.8	12459	PASS
173	174	0.00	2	1.1	1700	PASS
174	95	50	100	81.9	149608	PASS
175	174	5	9	7.4	11034	PASS
176	174	95	101	95.5	142859	PASS
177	176	5	9	6.5	9270	PASS