

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071425\
 Data File : VX046962.D
 Acq On : 14 Jul 2025 10:54
 Operator : JC/MD
 Sample : VX0714MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0714MBL01

Quant Time: Jul 15 01:14:05 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 03 05:51:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	353449	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	590149	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	542379	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	279389	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	242617	51.959	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.920%
35) Dibromofluoromethane	5.397	113	199801	49.876	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.760%
50) Toluene-d8	8.653	98	689113	48.756	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.520%
62) 4-Bromofluorobenzene	11.079	95	278070	51.766	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071425\
Data File : VX046962.D
Acq On : 14 Jul 2025 10:54
Operator : JC/MD
Sample : VX0714MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0714MBL01

Quant Time: Jul 15 01:14:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 03 05:51:11 2025
Response via : Initial Calibration




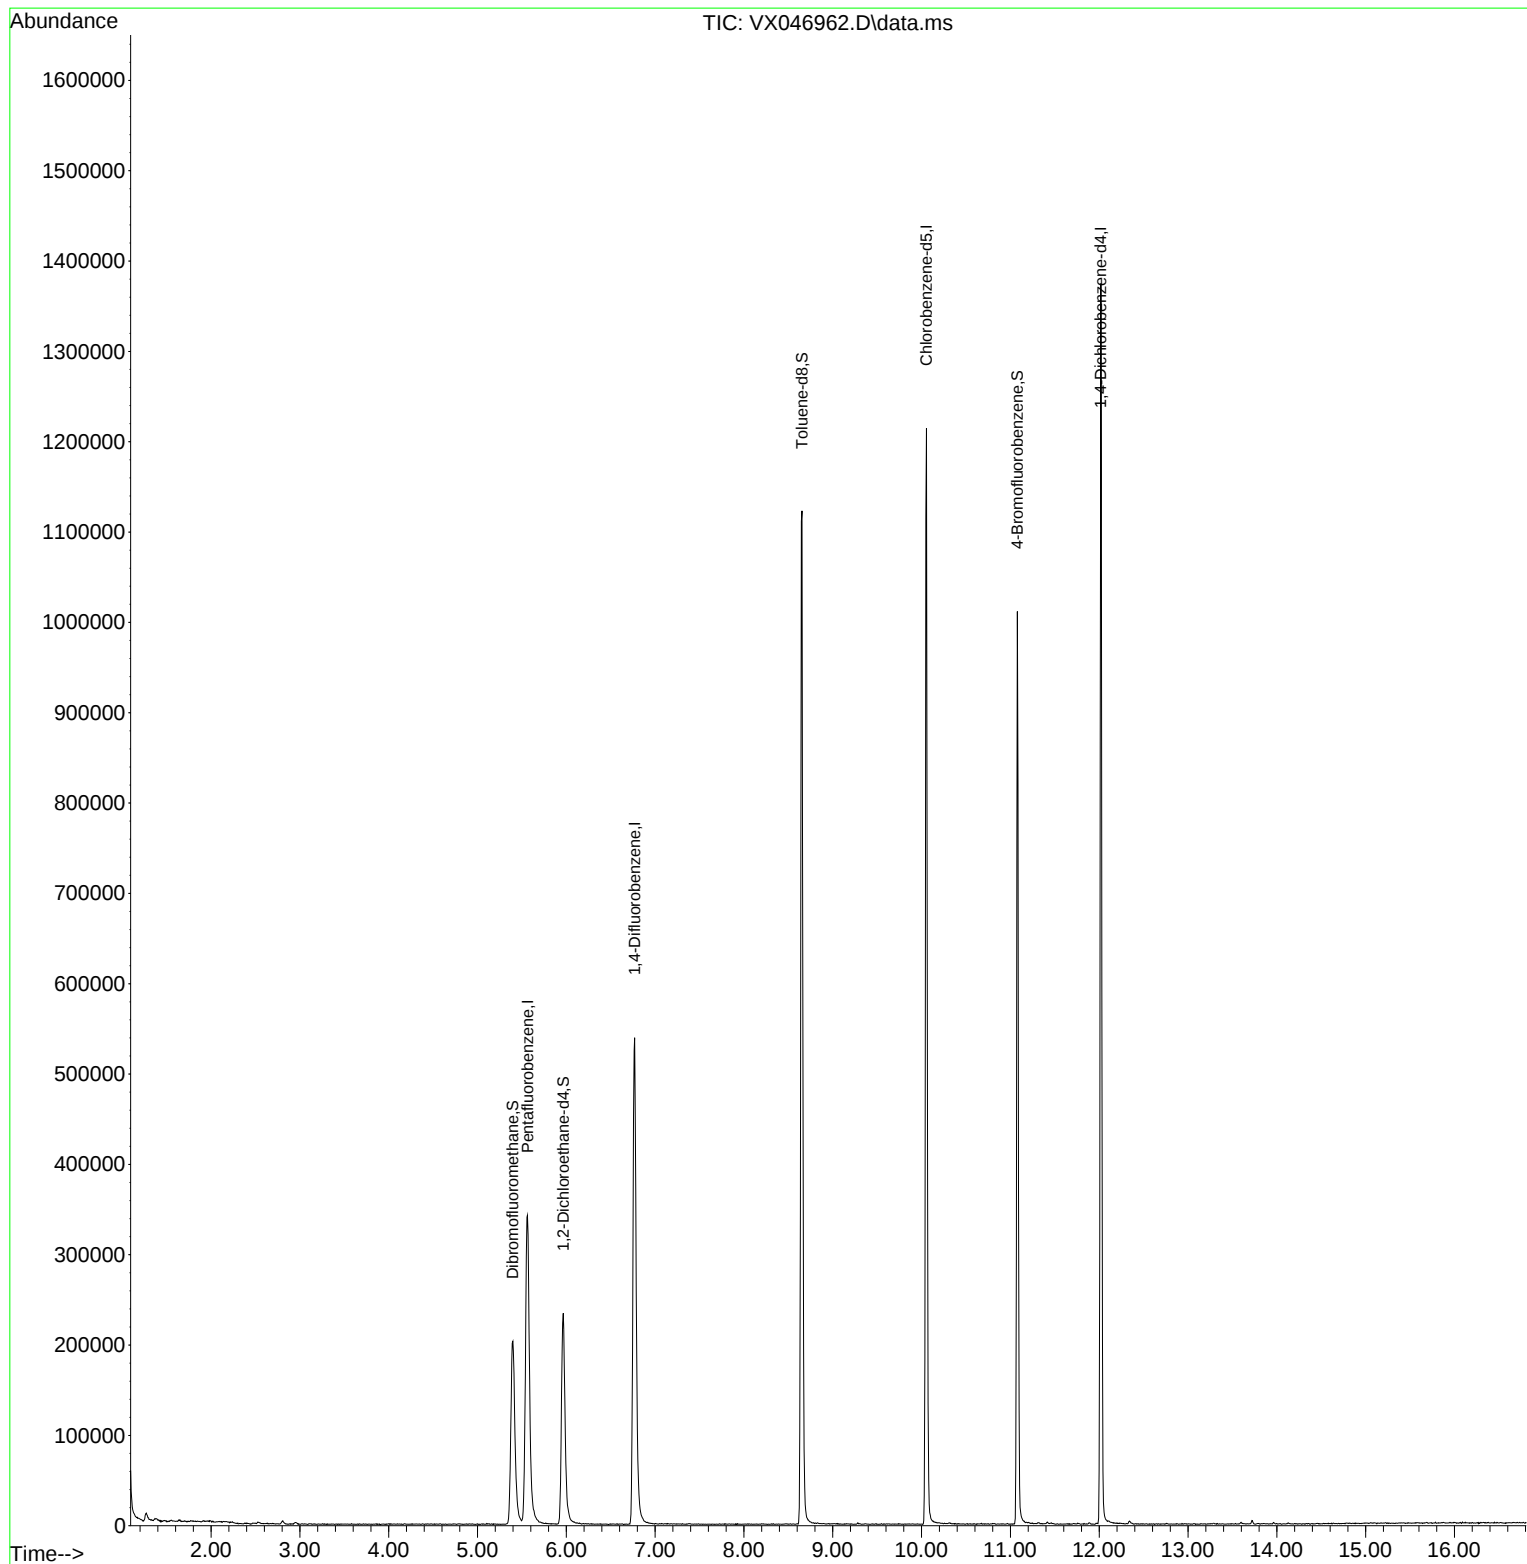


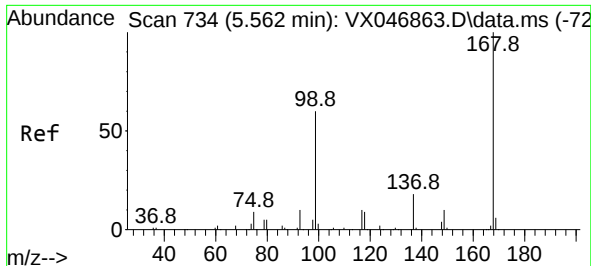

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54




Instrument :
MSVOA_X
ClientSampleId :
VX0714MBL01


Tgt Ion:168 Resp: 353449
Ion Ratio Lower Upper
168 100
99 60.5 48.8 73.2

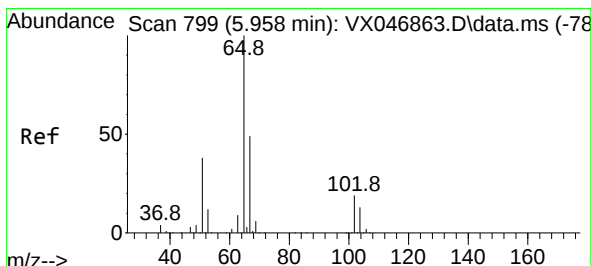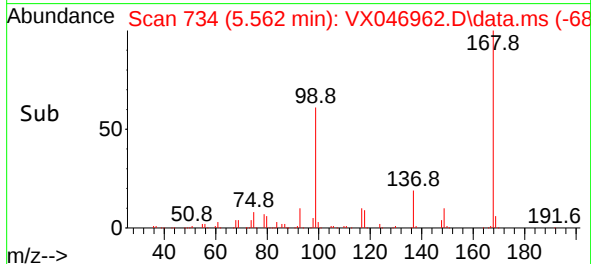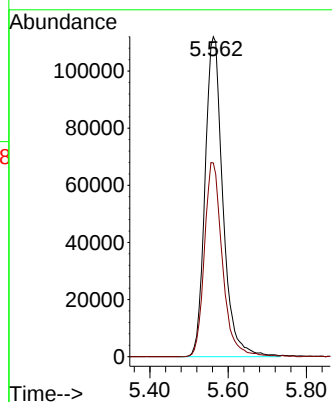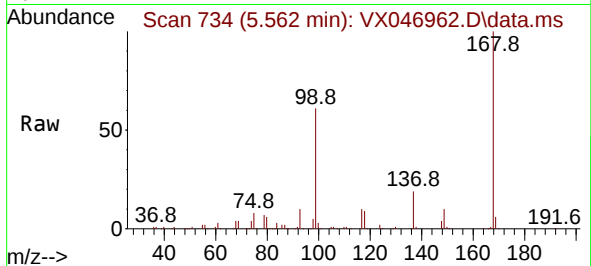

#33
1,2-Dichloroethane-d4
Concen: 51.959 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54

Tgt Ion: 65 Resp: 242617
Ion Ratio Lower Upper
65 100
67 52.6 0.0 105.2


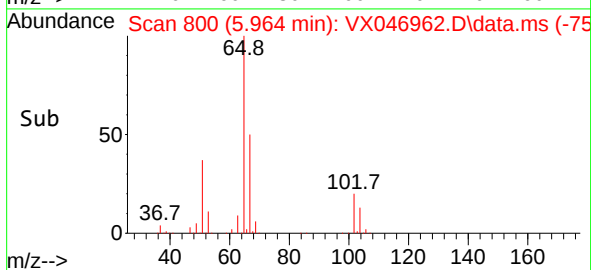
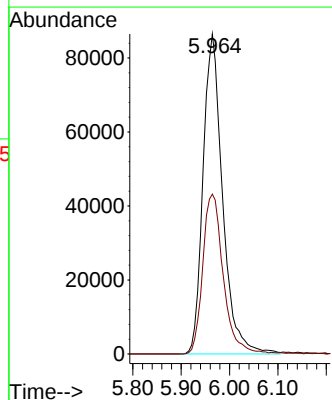
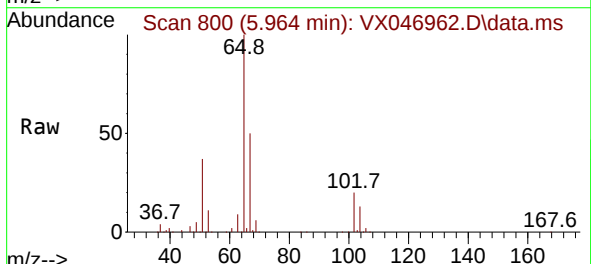


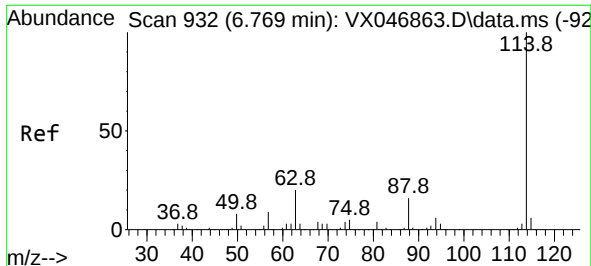

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54




Instrument :
MSVOA_X
ClientSampleId :
VX0714MBL01


Tgt Ion:114 Resp: 590149
Ion Ratio Lower Upper
114 100
63 21.2 0.0 40.4
88 16.3 0.0 31.0

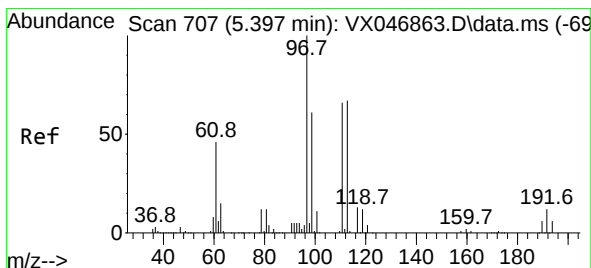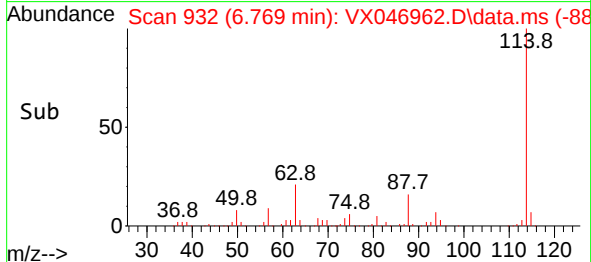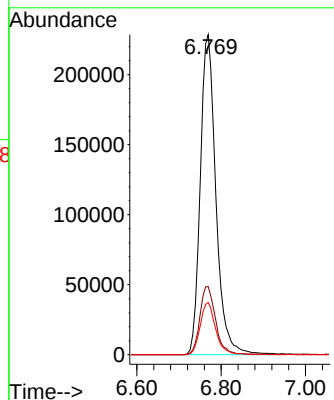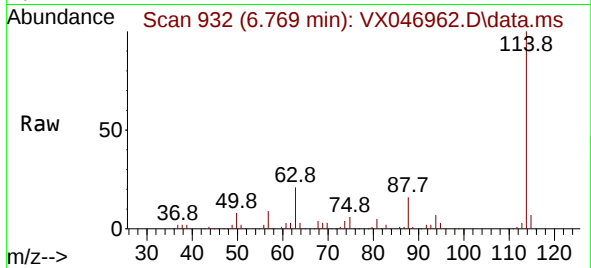

#35
Dibromofluoromethane
Concen: 49.876 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.000 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54

Tgt Ion:113 Resp: 199801
Ion Ratio Lower Upper
113 100
111 102.1 81.2 121.8
192 18.9 15.3 22.9


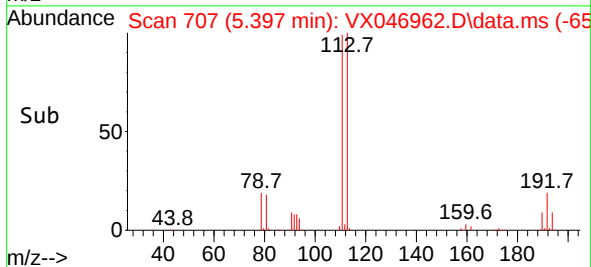
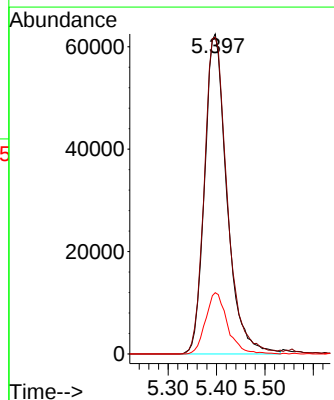
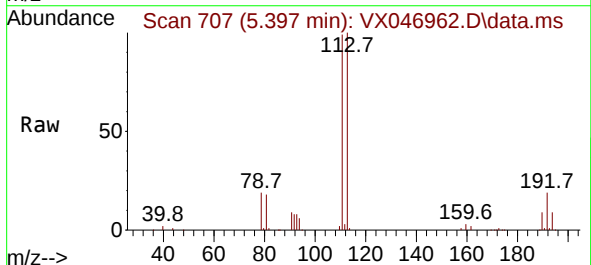


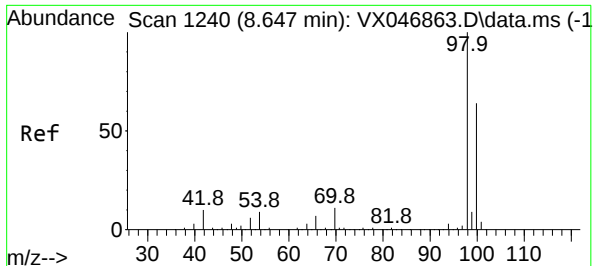

#50
Toluene-d8
Concen: 48.756 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54




Instrument :
MSVOA_X
ClientSampleId :
VX0714MBL01


Tgt Ion: 98 Resp: 689113
Ion Ratio Lower Upper
98 100
100 66.7 53.0 79.6

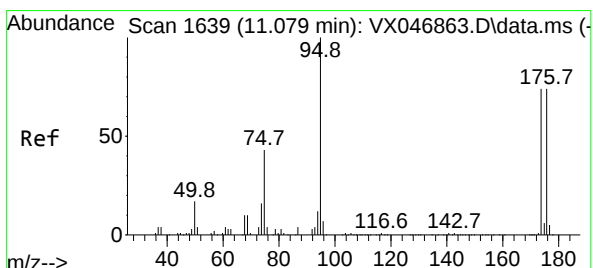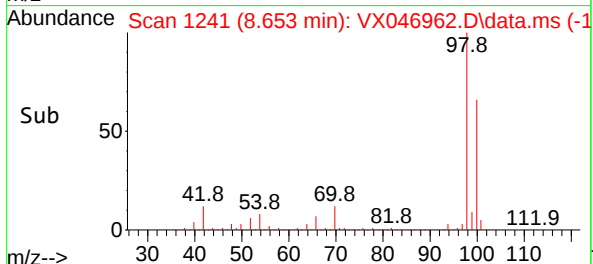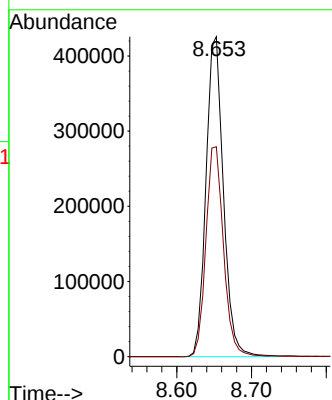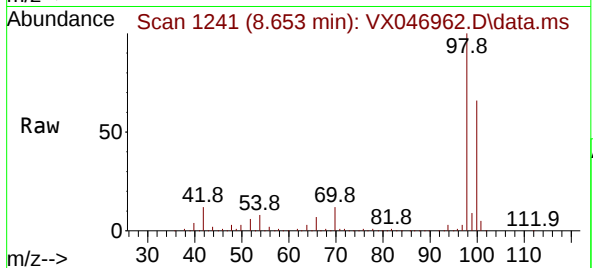

#62
4-Bromofluorobenzene
Concen: 51.766 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54

Tgt Ion: 95 Resp: 278070
Ion Ratio Lower Upper
95 100
174 73.9 0.0 152.0
176 70.9 0.0 145.2


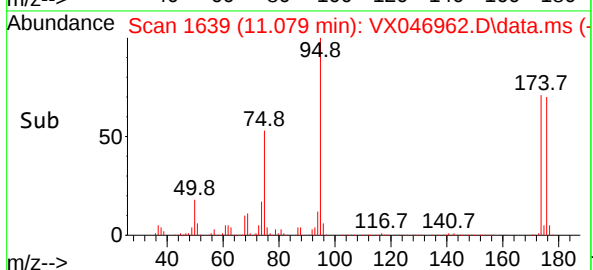
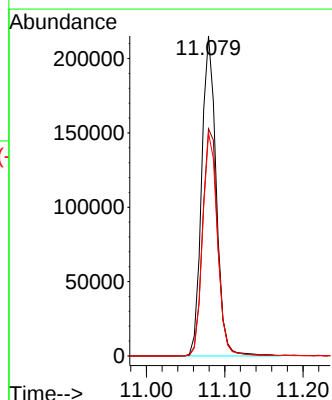
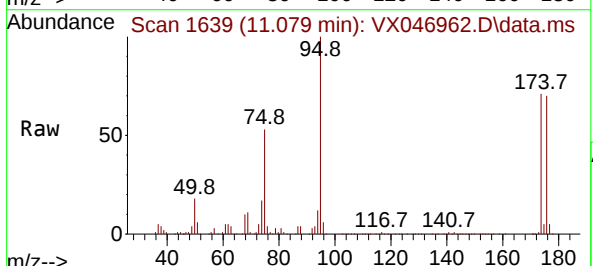


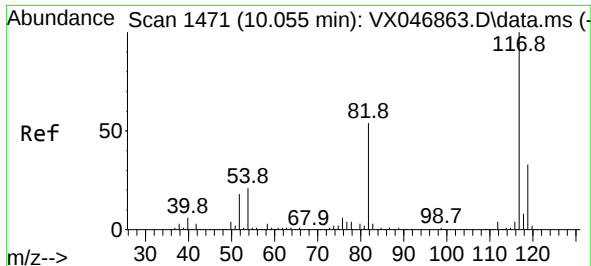

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54

Instrument :
MSVOA_X
ClientSampleId :
VX0714MBL01

Tgt Ion:117 Resp: 542379
Ion Ratio Lower Upper
117 100
82 56.3 43.3 64.9
119 32.6 26.4 39.6

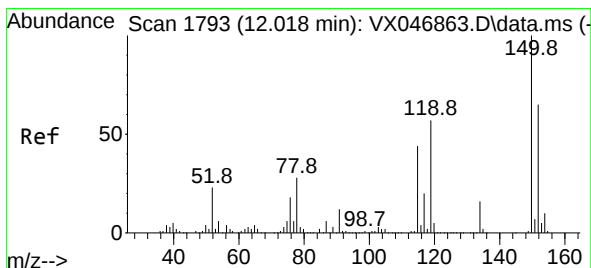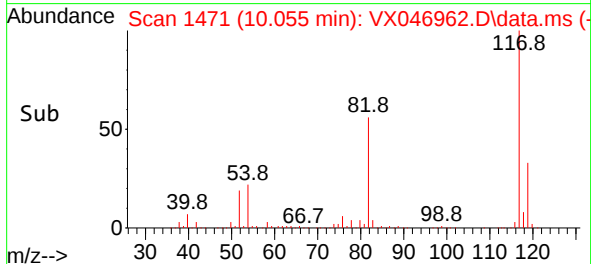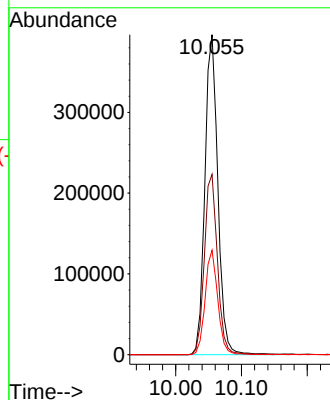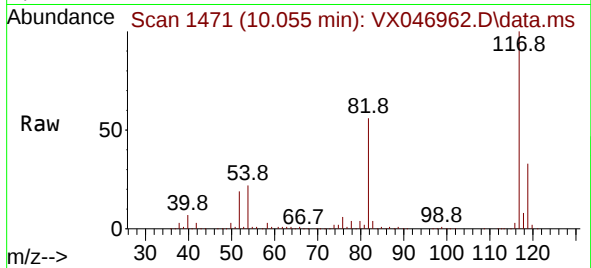

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046962.D
Acq: 14 Jul 2025 10:54

Tgt Ion:152 Resp: 279389
Ion Ratio Lower Upper
152 100
115 61.1 42.4 127.1
150 156.9 0.0 349.2

