

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070325\
 Data File : P0112011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2025 11:56
 Operator : YP/AJ
 Sample : Q2481-03 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CC0625-OXBL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/07/2025
 Supervised By :mohammad ahmed 07/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 05:45:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.672	3.675	4808355	8509322	0.835m	1.515m#
2) SA Decachlor...	8.701	8.653	3591643	1250192	0.684	0.703

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070325\
Data File : PO112011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2025 11:56
Operator : YP/AJ
Sample : Q2481-03 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CC0625-OXBL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2025
Supervised By :mohammad ahmed 07/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 05:45:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

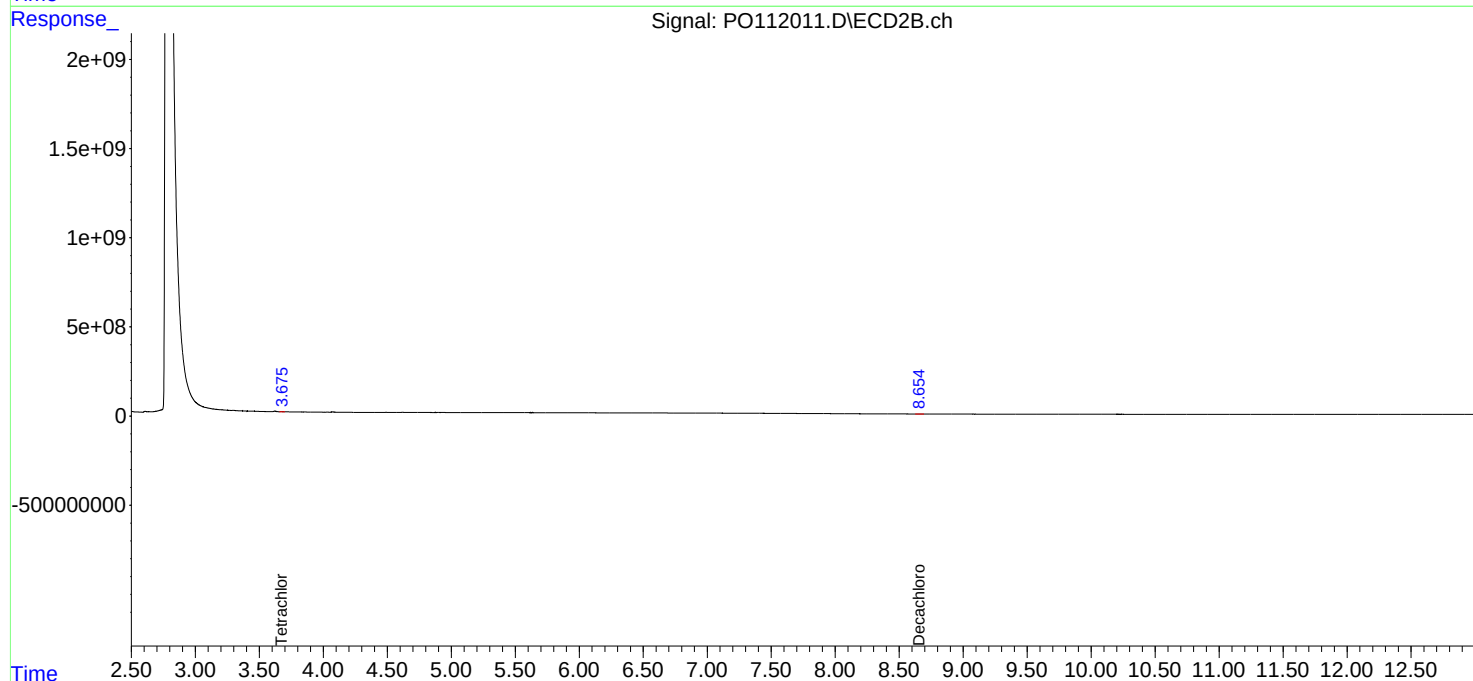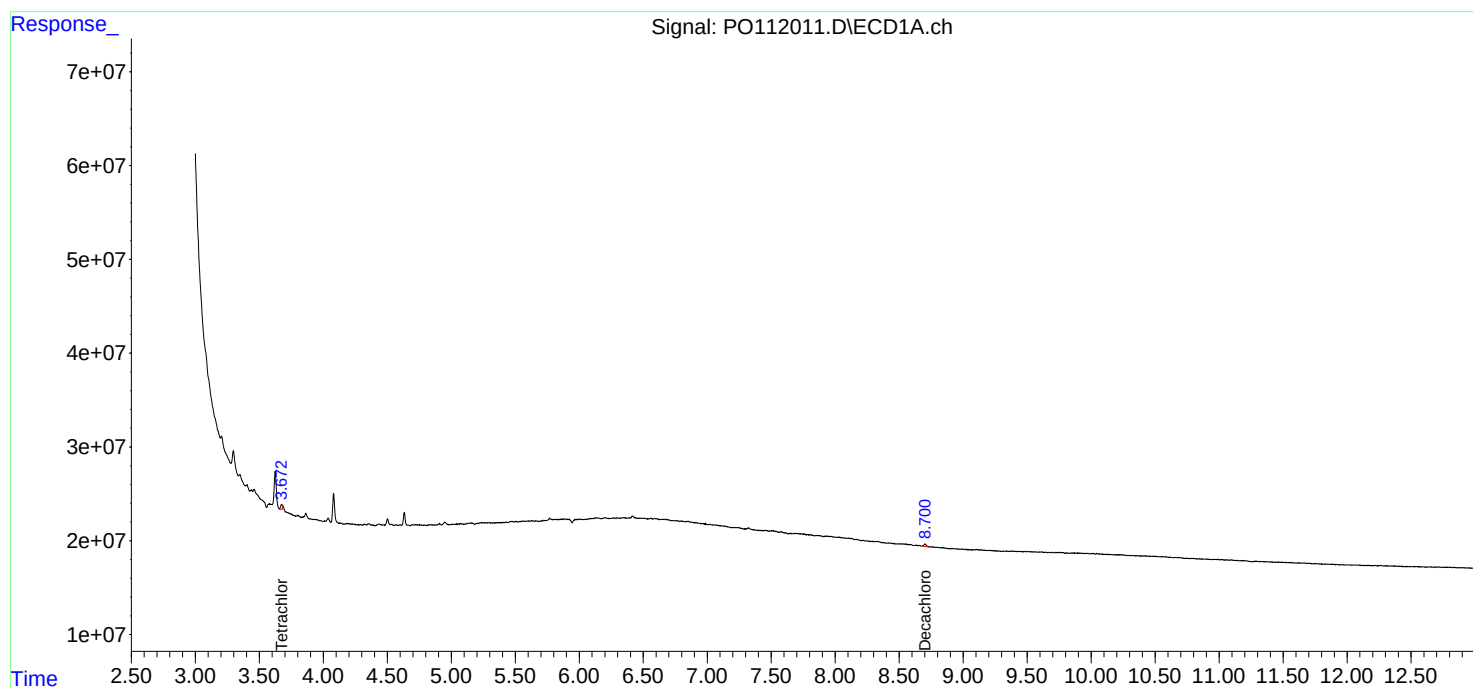

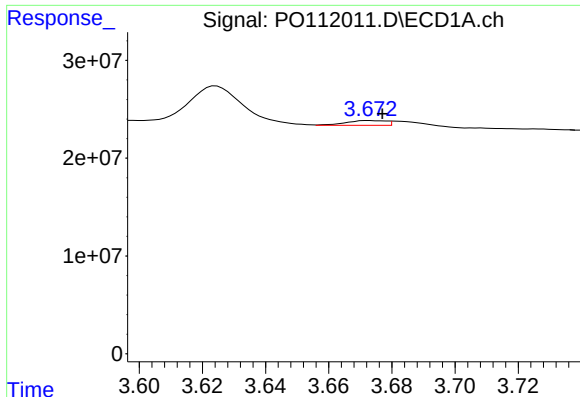


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.005 min
Response: 4808355
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC0625-OXBL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2025
Supervised By :mohammad ahmed 07/08/2025

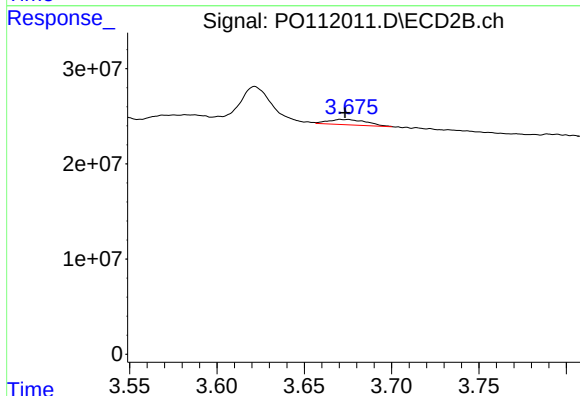


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: 0.002 min
Response: 8509322
Conc: 1.51 ng/ml m

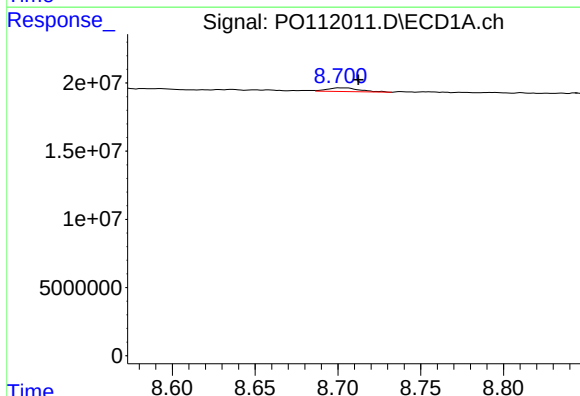

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.011 min
Response: 3591643
Conc: 0.68 ng/ml

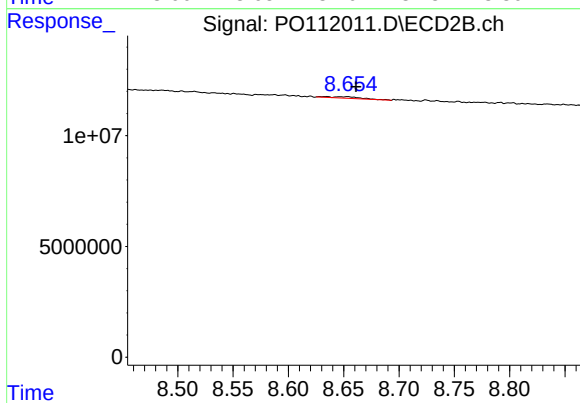

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: -0.008 min
Response: 1250192
Conc: 0.70 ng/ml