


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072125\
Data File : BP025194.D
Acq On : 21 Jul 2025 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 22 02:55:21 2025

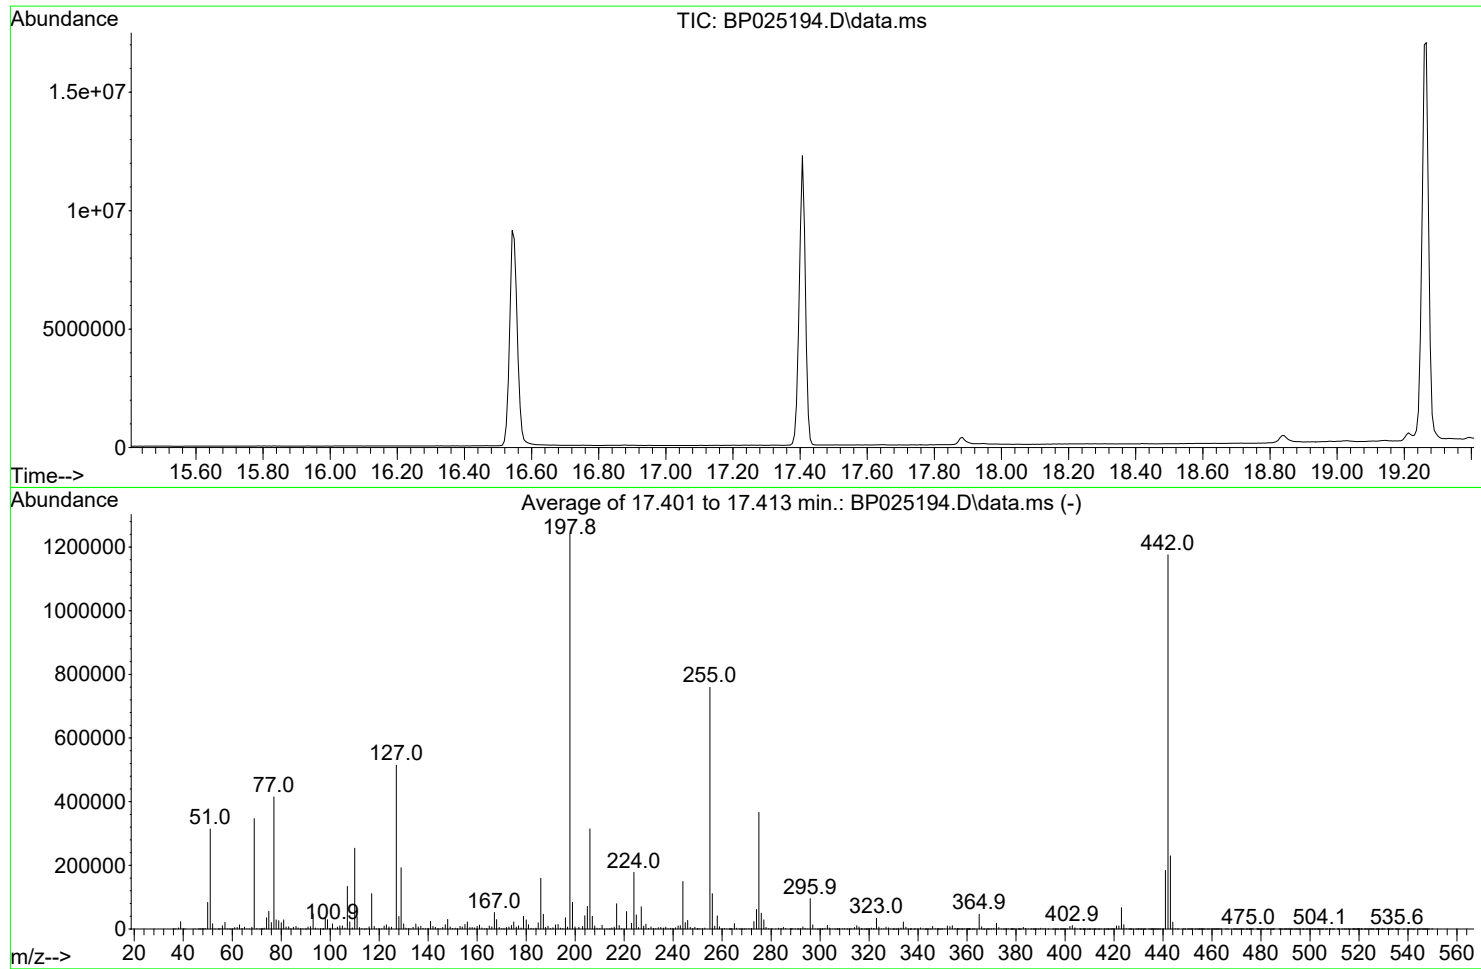

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5798	PASS
69	69	100	100	100.0	347092	PASS
70	69	0.00	2	0.5	1776	PASS
197	198	0.00	2	0.5	5935	PASS
198	198	100	100	100.0	1240464	PASS
199	198	5	9	6.8	84213	PASS
365	198	1	100	3.7	46101	PASS
441	443	0.01	150	80.1	183987	PASS
442	442	100	100	100.0	1176021	PASS
443	442	15	24	19.5	229824	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/21/2025	BNA_P	<u>BP025194.D</u>
Compound Name	Response	Retention Time
DDT	4575135	20.571
DDD	116048	20.101
DDE	9251	19.577
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
125299	4700434	2.67

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072125\
Data File : BP025194.D
Acq On : 21 Jul 2025 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 22 04:16:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

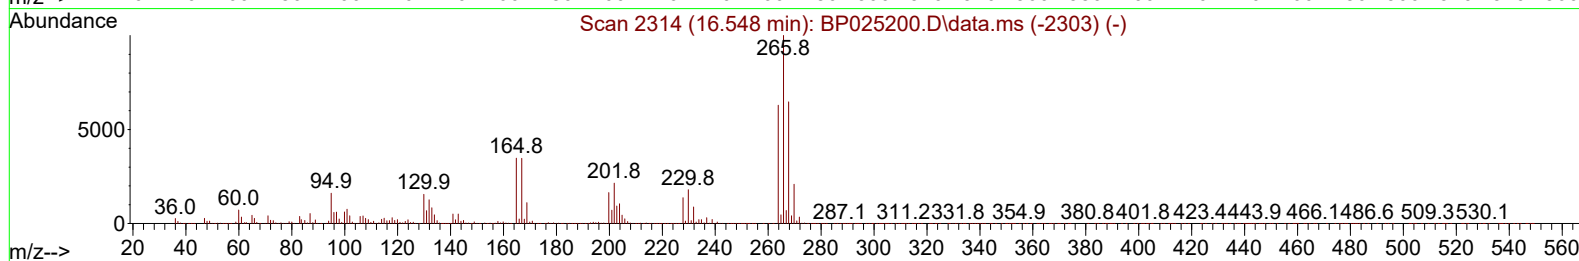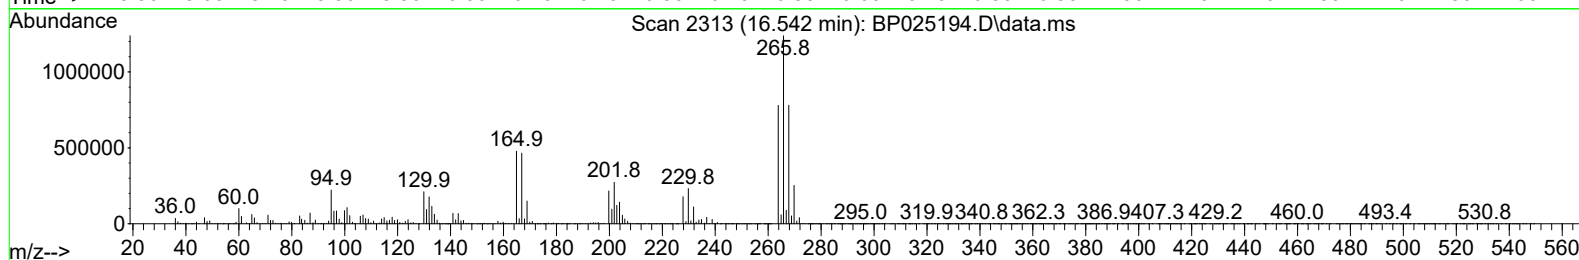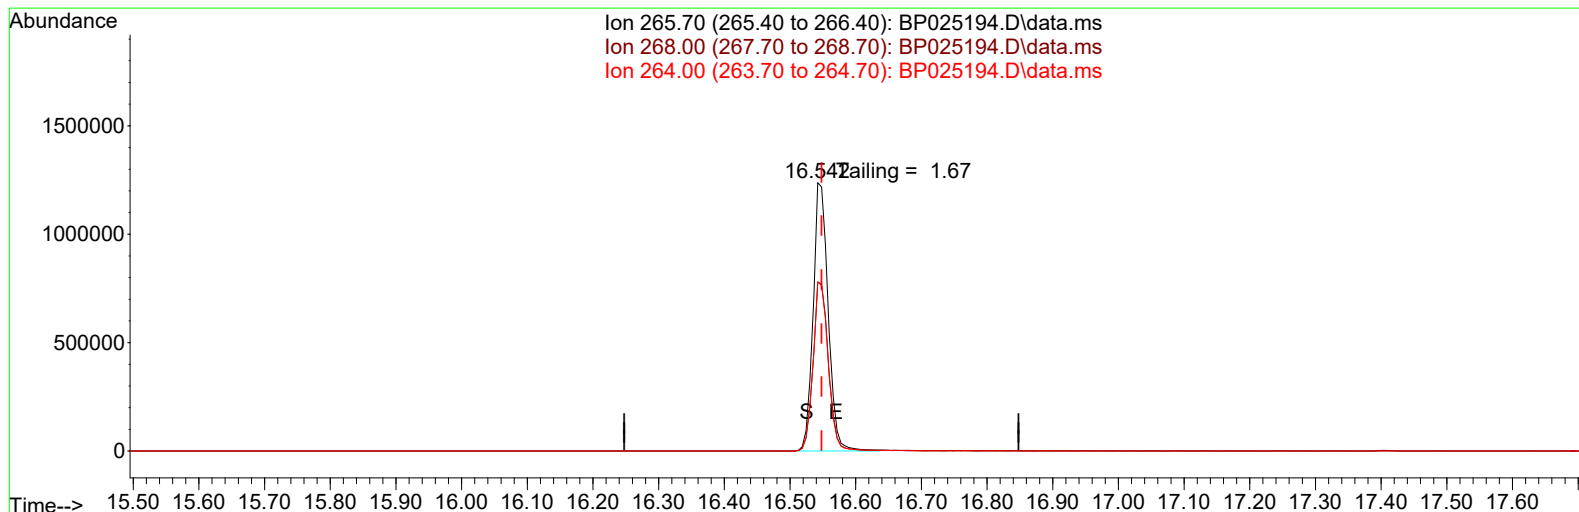

TIC: BP025194.D\data.ms

(70) Pentachlorophenol (C)

16.542min (-0.006) 139254.46 ng




response 1981776

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.05
264.00	62.90	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072125\
Data File : BP025194.D
Acq On : 21 Jul 2025 13:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 22 04:16:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

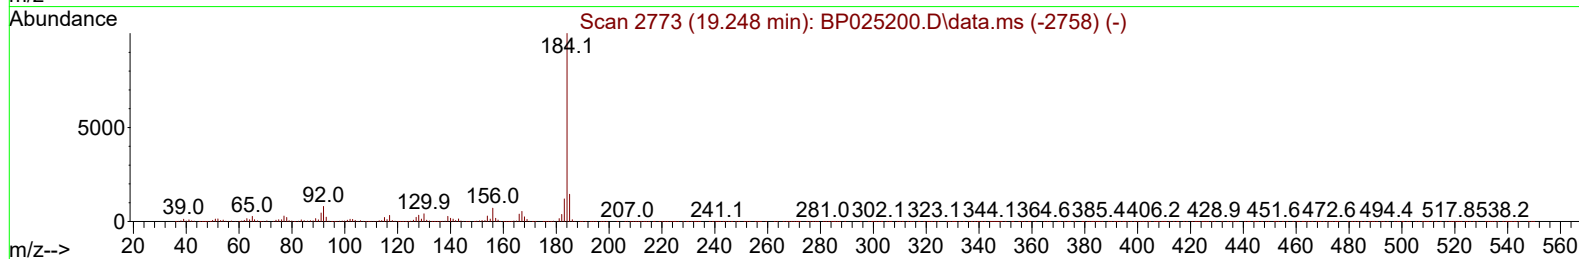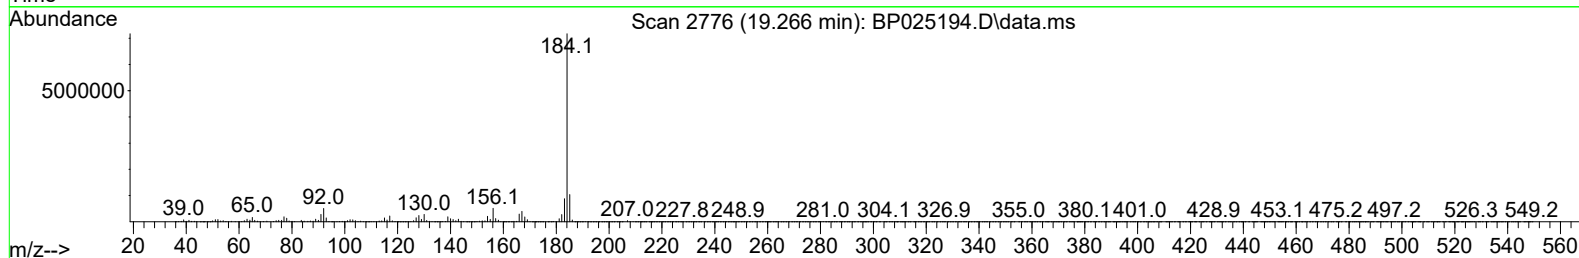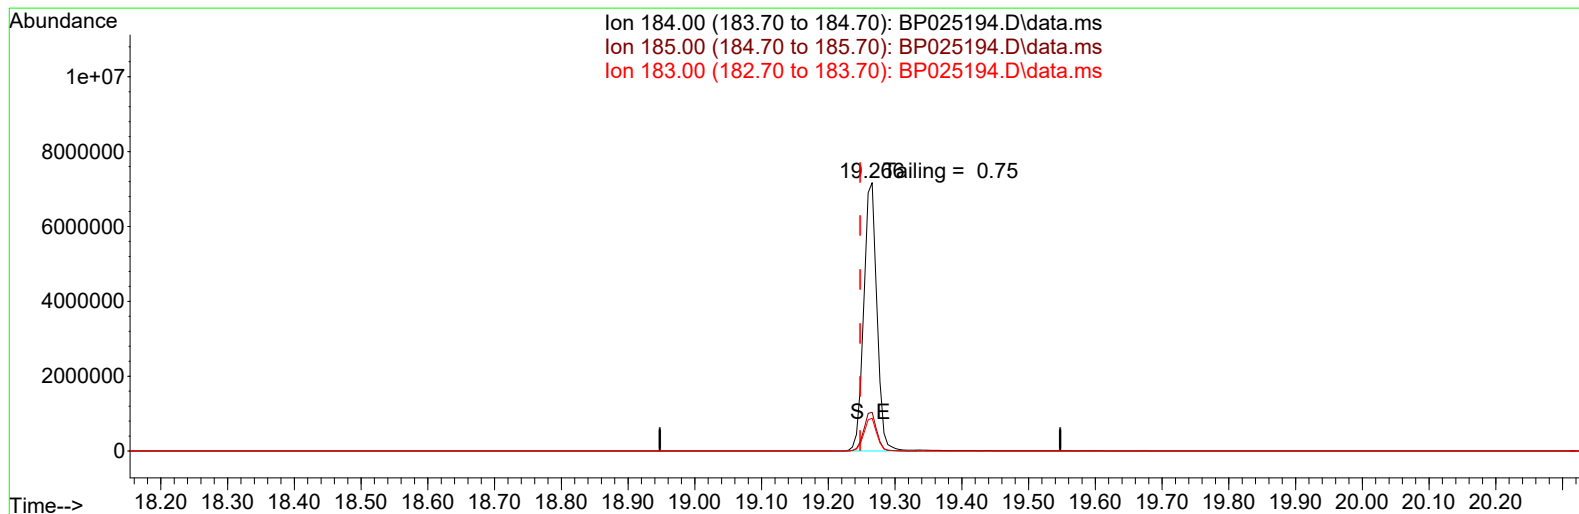

TIC: BP025194.D\data.ms

(77) Benzidine

19.266min (+ 0.018) 25003.16 ng

response 9830583

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.45
183.00	12.00	12.25
0.00	0.00	0.00