

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070325\
 Data File : PD089318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 20:31
 Operator : AR\AJ
 Sample : Q2484-02 (Sig #1); Q2484-01 (Sig #2)
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-57

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/03/2025
 Supervised By : mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:44:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 05:39:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.879	44281696	283.5E6	15.520	16.725m
28) SA Decachlor...	9.075	8.072	32881104	154.5E6	8.372	7.815

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070325\
Data File : PD089318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 20:31
Operator : AR\AJ
Sample : Q2484-02 (Sig #1); Q2484-01 (Sig #2)
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-57


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:44:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 05:39:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

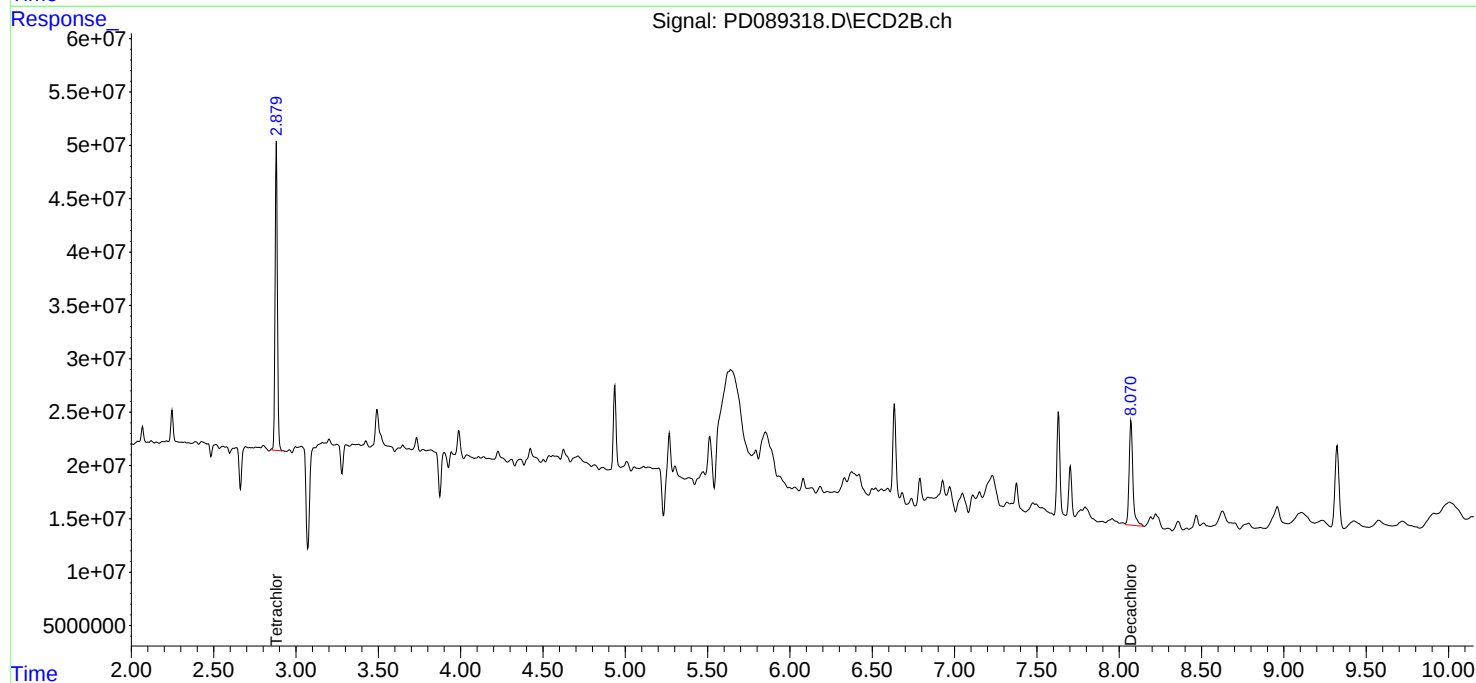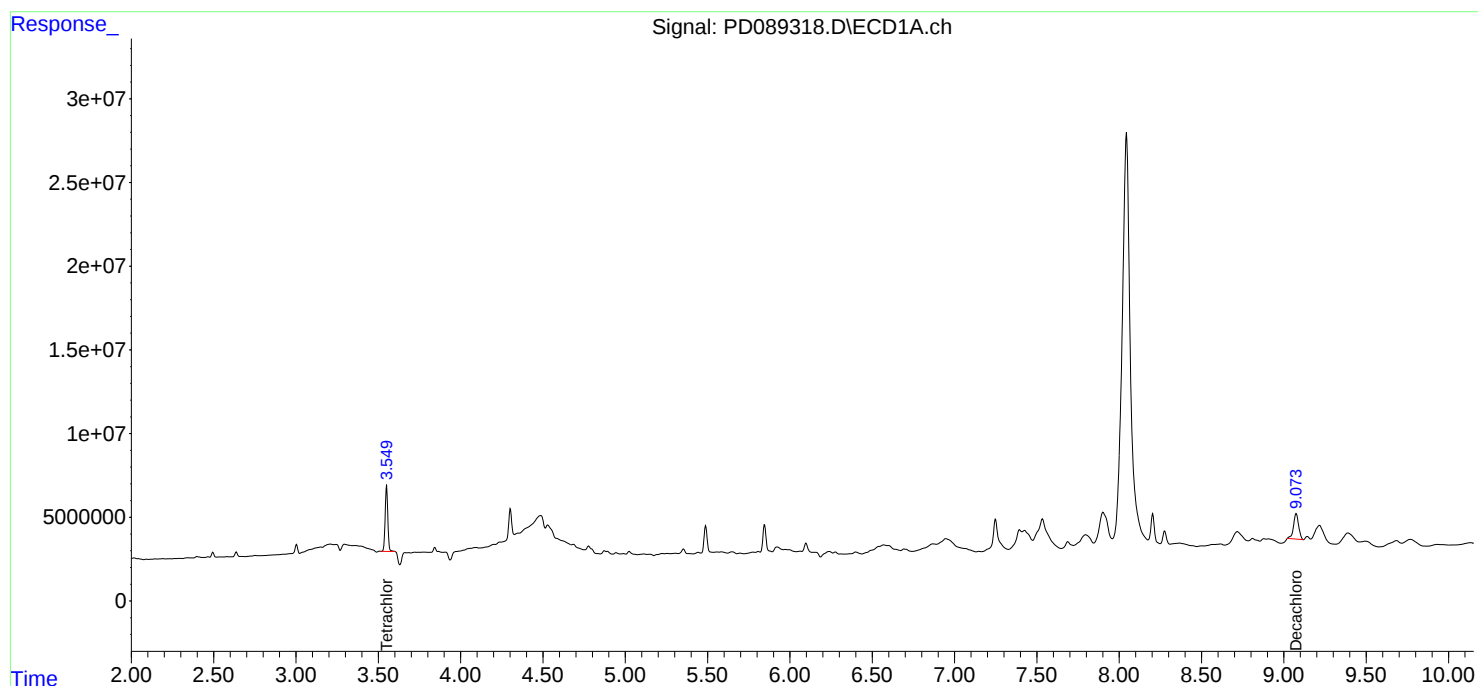

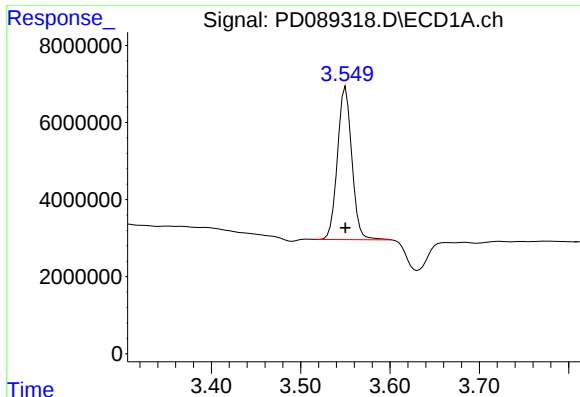


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 44281696
Conc: 15.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-57


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

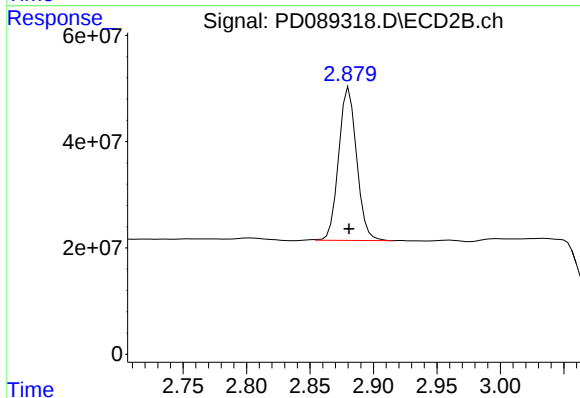


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: -0.001 min
Response: 283538981
Conc: 16.72 ng/ml m

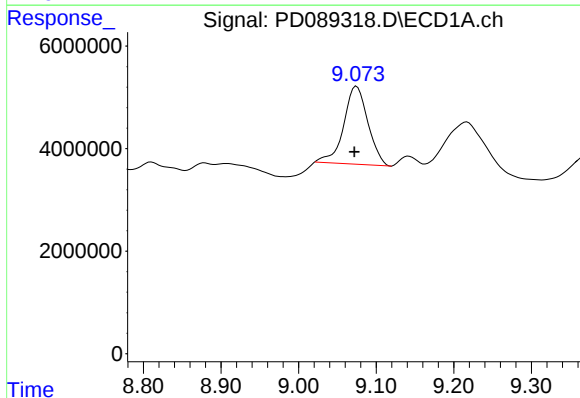

#28 Decachlorobiphenyl

R.T.: 9.075 min
Delta R.T.: 0.003 min
Response: 32881104
Conc: 8.37 ng/ml

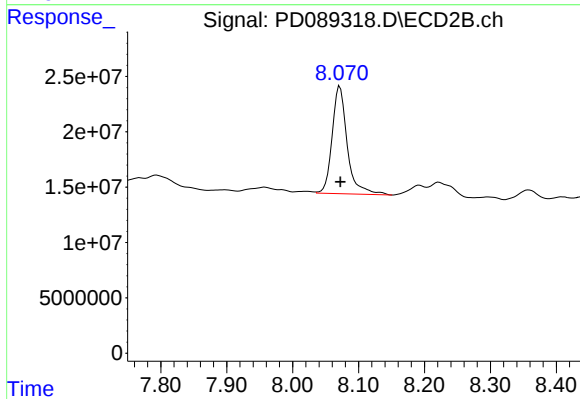

#28 Decachlorobiphenyl

R.T.: 8.072 min
Delta R.T.: 0.000 min
Response: 154502438
Conc: 7.82 ng/ml