

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
 Data File : BF143021.D
 Acq On : 07 Jul 2025 21:22
 Operator : RC/JU
 Sample : Q2484-03 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-64

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	485	490	501	rBB	6610	10122	2.87%	0.360%
2	5.493	557	561	573	rBV	79274	113866	32.26%	4.048%
3	6.510	729	734	744	rBV	71625	107363	30.41%	3.817%
4	6.875	791	796	805	rBV	205254	250366	70.92%	8.901%
5	7.434	887	891	905	rBV	47928	66204	18.75%	2.354%
6	8.157	1009	1014	1043	rVB	239786	302544	85.70%	10.756%
7	9.234	1192	1197	1207	rBV	110809	137768	39.03%	4.898%
8	9.916	1308	1313	1318	rBV	260951	318103	90.11%	11.309%
9	10.334	1378	1384	1389	rBV6	3248	7215	2.04%	0.256%
10	10.563	1419	1423	1427	rVB4	2568	4397	1.25%	0.156%
11	10.628	1427	1434	1439	rBV	23800	31164	8.83%	1.108%
12	10.710	1443	1448	1458	rVV	51774	71408	20.23%	2.539%
13	10.822	1462	1467	1473	rVB4	6079	10593	3.00%	0.377%
14	11.257	1537	1541	1544	rBV3	2471	4160	1.18%	0.148%
15	11.404	1561	1566	1576	rBV	257926	353015	100.00%	12.550%
16	11.739	1619	1623	1627	rVB4	3320	4559	1.29%	0.162%
17	11.933	1649	1656	1661	rBV5	8219	18359	5.20%	0.653%
18	12.022	1667	1671	1679	rVB5	7814	16600	4.70%	0.590%
19	12.098	1680	1684	1689	rBV6	4421	7022	1.99%	0.250%
20	12.145	1689	1692	1696	rBV5	3931	5452	1.54%	0.194%
21	12.386	1730	1733	1737	rBV6	5115	8184	2.32%	0.291%
22	12.457	1742	1745	1747	rBV	9456	11659	3.30%	0.414%
23	12.622	1769	1773	1778	rBV	42013	54961	15.57%	1.954%
24	12.857	1808	1813	1818	rBV	50358	78581	22.26%	2.794%
25	12.992	1831	1836	1843	rBV	130445	178243	50.49%	6.337%
26	14.057	2012	2017	2023	rBV	241209	351703	99.63%	12.503%
27	15.557	2268	2272	2279	rVB	178622	289281	81.95%	10.284%




Sum of corrected areas: 2812892

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
Data File : BF143021.D
Acq On : 07 Jul 2025 21:22
Operator : RC/JU
Sample : Q2484-03 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

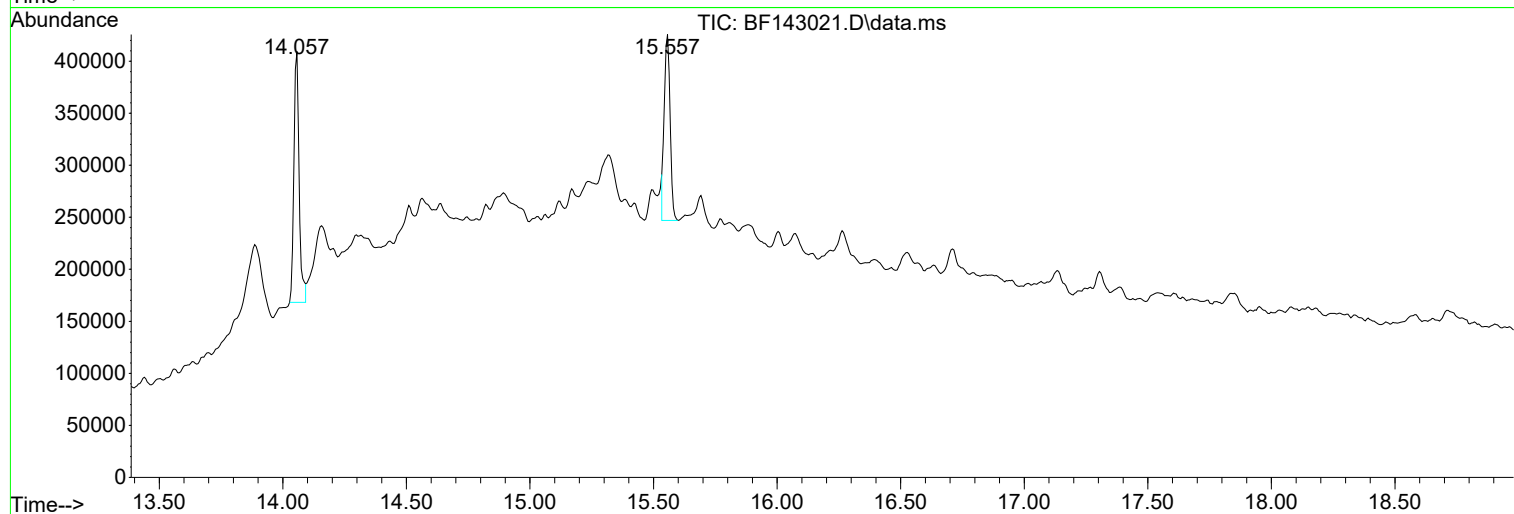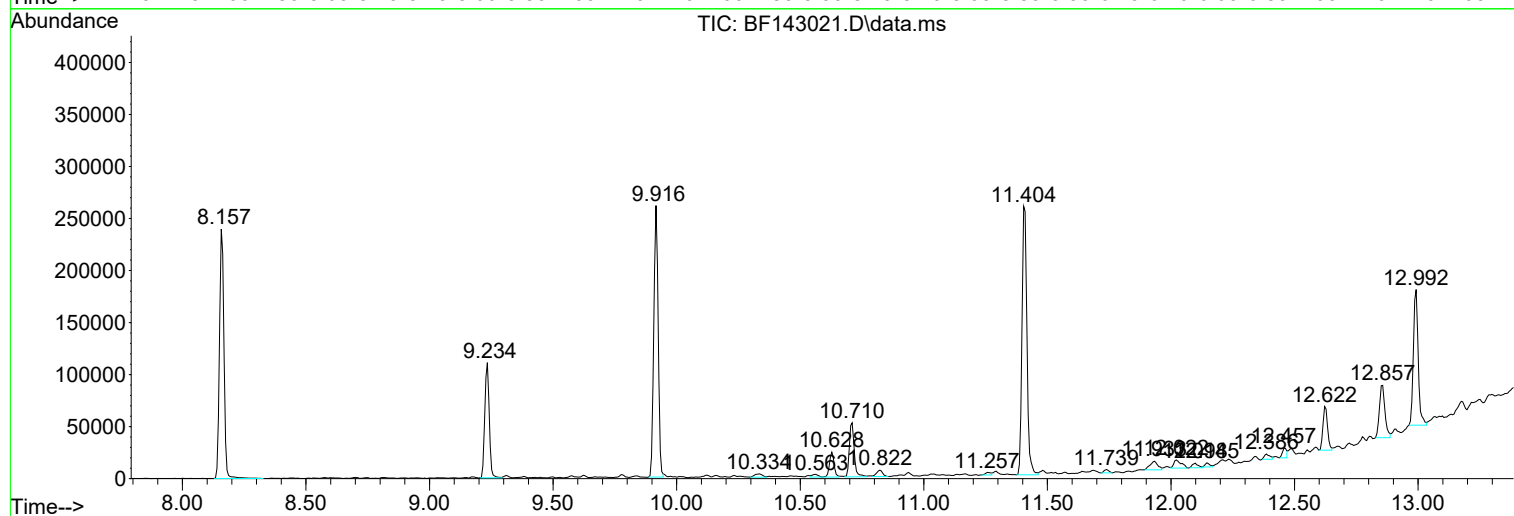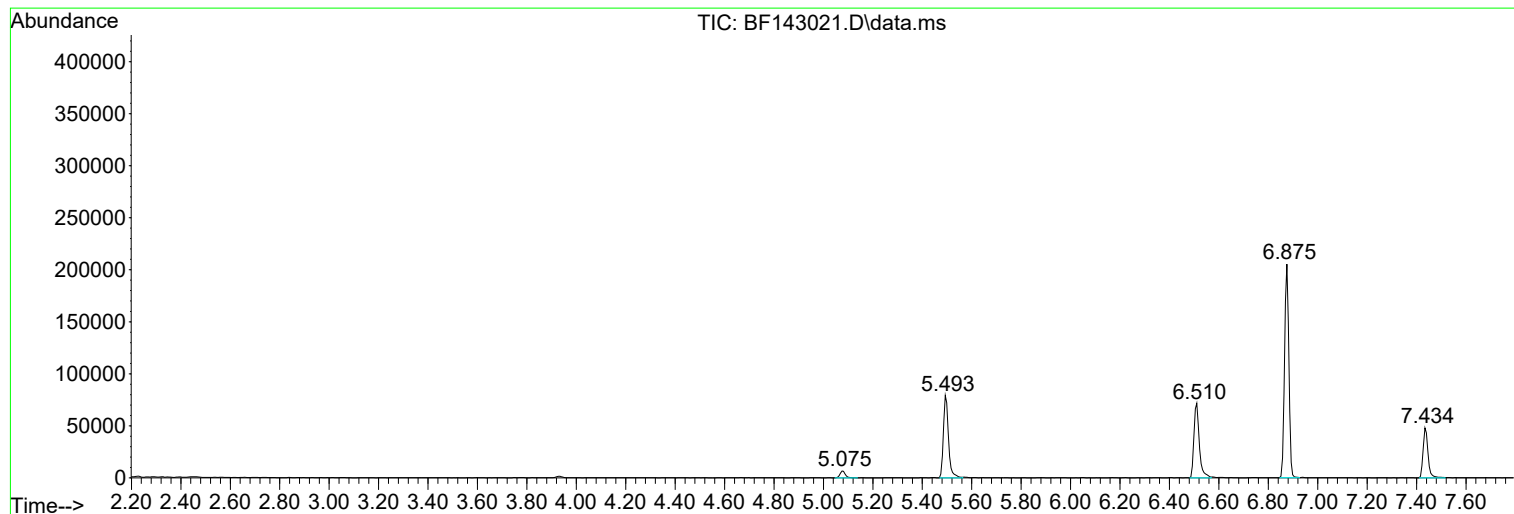

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
Data File : BF143021.D
Acq On : 07 Jul 2025 21:22
Operator : RC/JU
Sample : Q2484-03 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
Data File : BF143021.D
Acq On : 07 Jul 2025 21:22
Operator : RC/JU
Sample : Q2484-03 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------