


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070325\
Data File : VY022928.D
Acq On : 03 Jul 2025 08:03
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Title : SW846 8260
Last Update : Tue Jun 24 08:29:52 2025

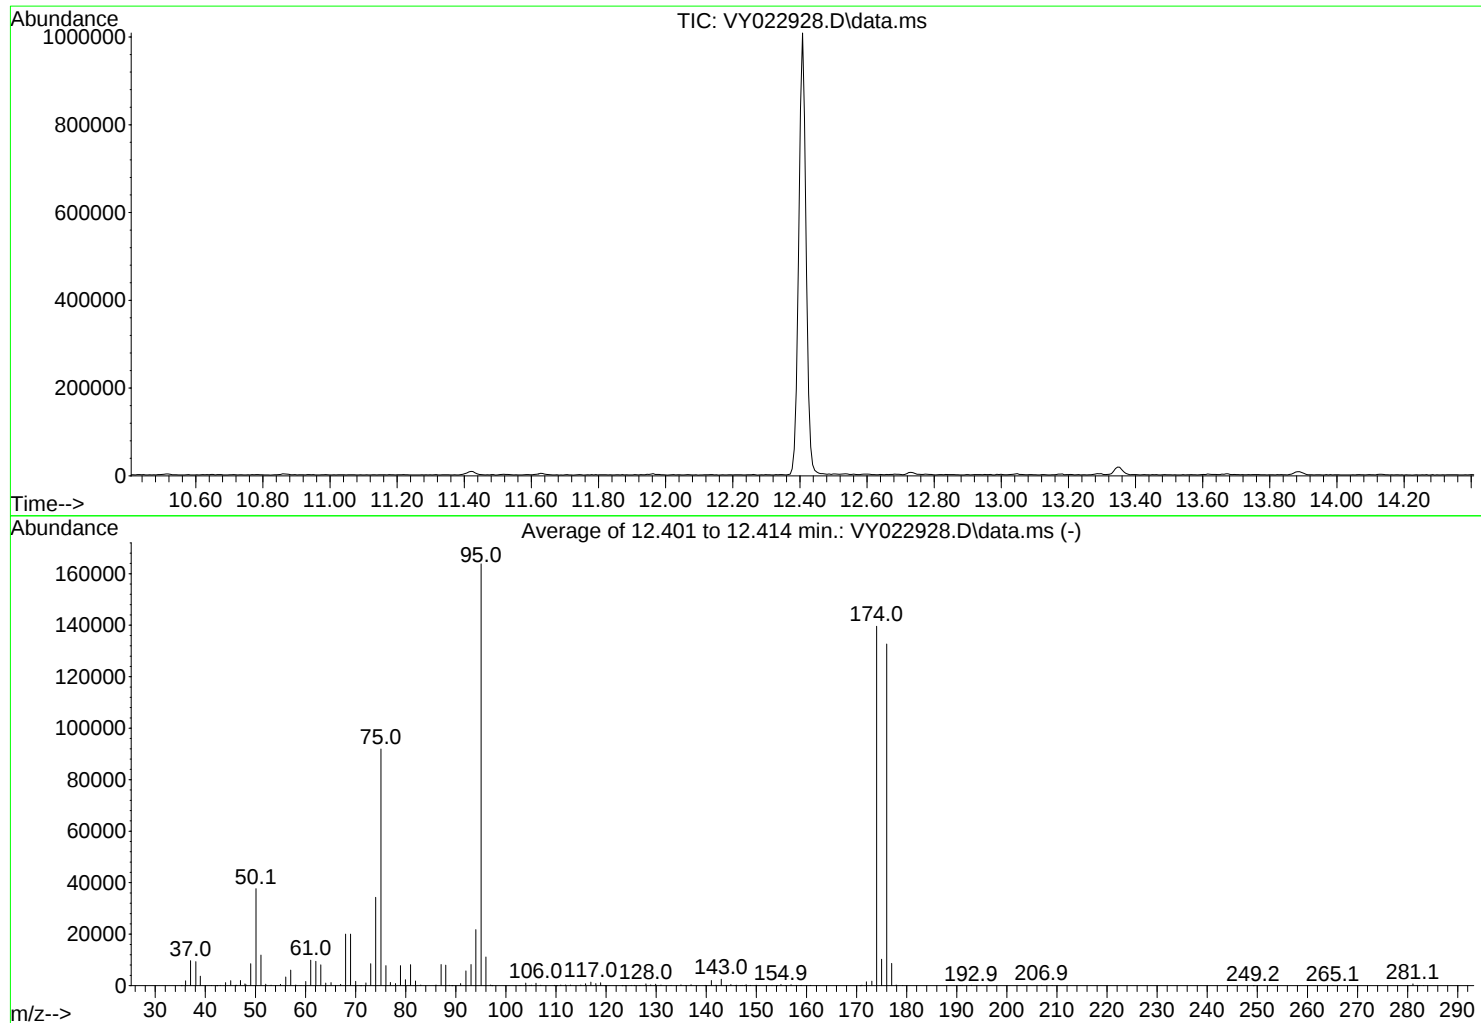

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	37680	PASS
75	95	30	60	56.1	91939	PASS
95	95	100	100	100.0	163840	PASS
96	95	5	9	6.8	11141	PASS
173	174	0.00	2	1.3	1759	PASS
174	95	50	100	85.2	139597	PASS
175	174	5	9	7.3	10242	PASS
176	174	95	101	95.1	132707	PASS
177	176	5	9	6.5	8654	PASS