
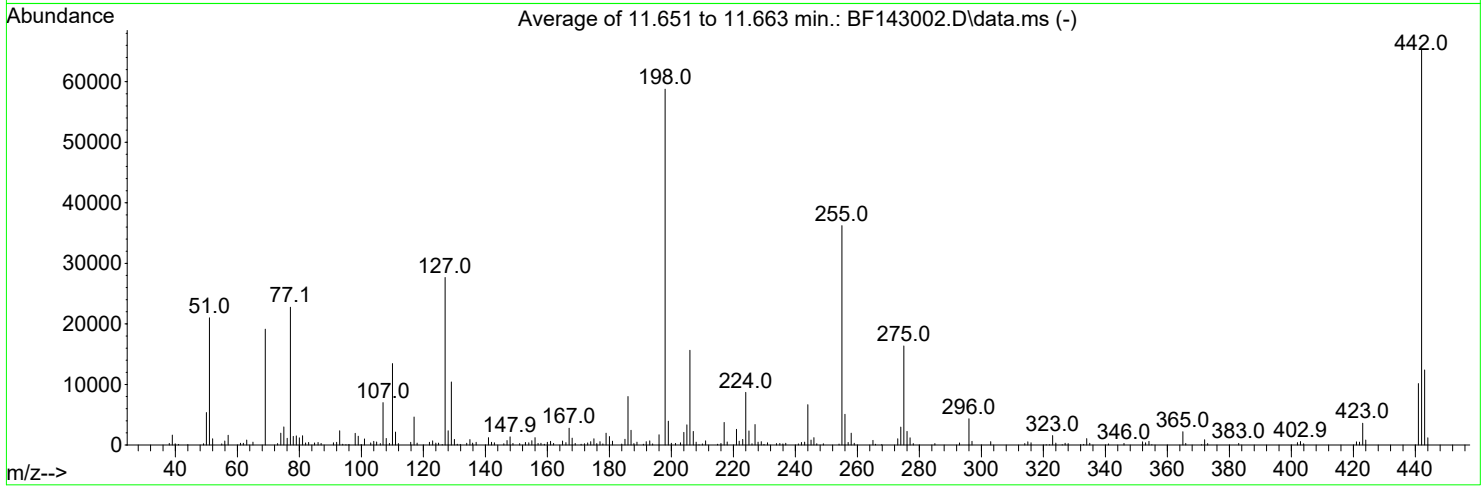


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
 Data File : BF143002.D
 Acq On : 07 Jul 2025 11:12
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 24 05:28:21 2025

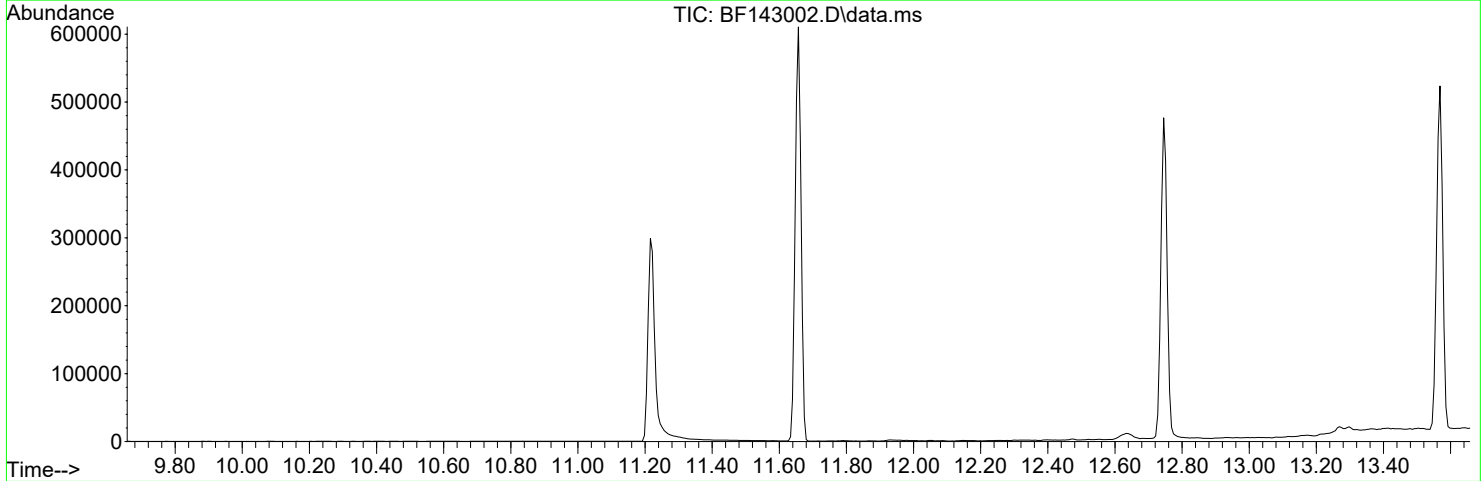

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	19140	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58773	PASS
199	198	5	9	6.7	3928	PASS
365	198	1	100	3.7	2188	PASS
441	443	0.01	150	81.7	10137	PASS
442	442	100	100	100.0	65205	PASS
443	442	15	24	19.0	12401	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/7/2025	BNA_F	<u>BF143002.D</u>
Compound Name	Response	Retention Time
DDT	129967	13.568
DDD	4973	13.268
DDE	479	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5452	135419	4.03

Instrument :
 BNA_F
ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
 Data File : BF143002.D
 Acq On : 07 Jul 2025 11:12
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Quant Time: Jul 07 13:07:55 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

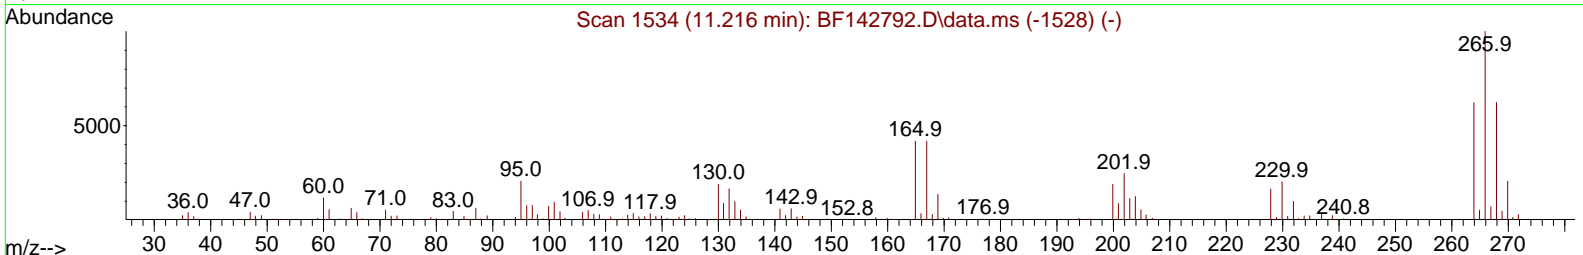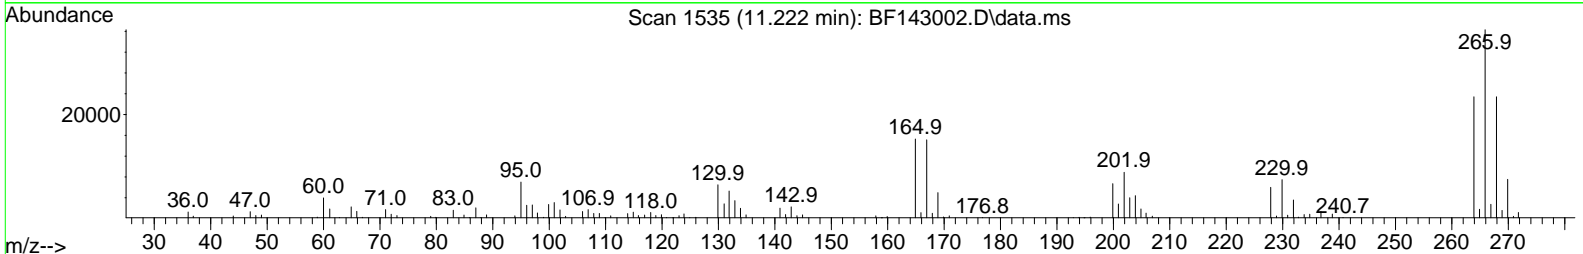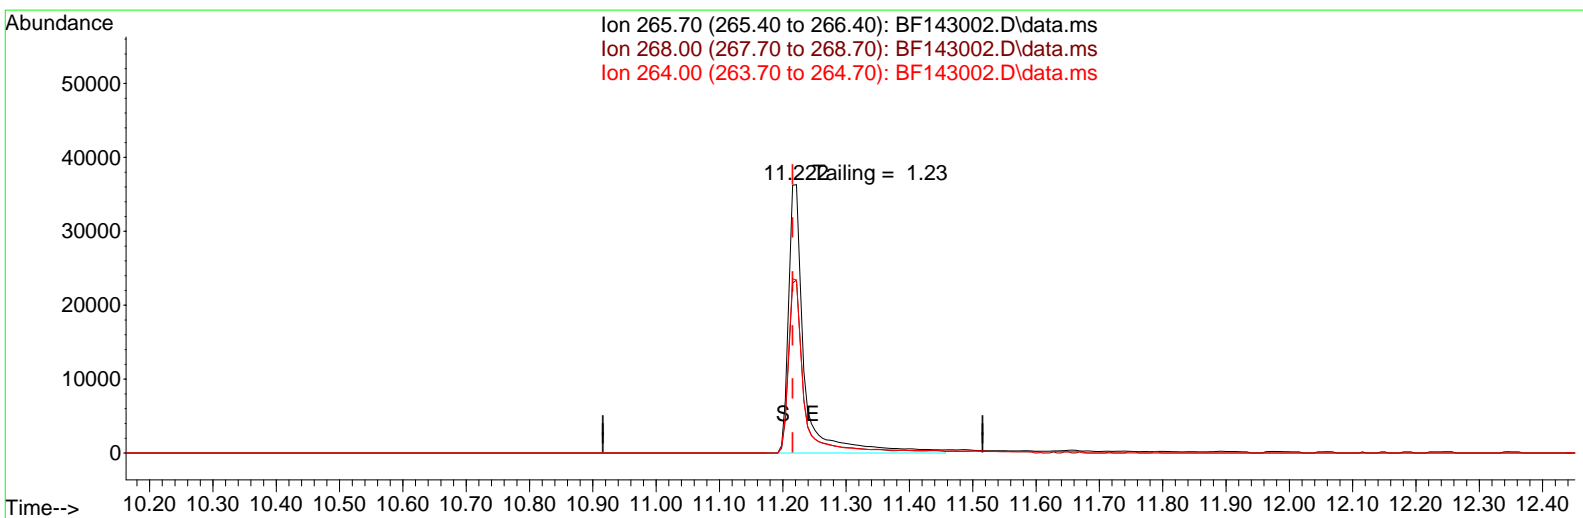

TIC: BF143002.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 41433.17 ng




response 63968

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.49
264.00	62.40	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070725\
 Data File : BF143002.D
 Acq On : 07 Jul 2025 11:12
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :
 DFTPP

Quant Time: Jul 07 13:07:55 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

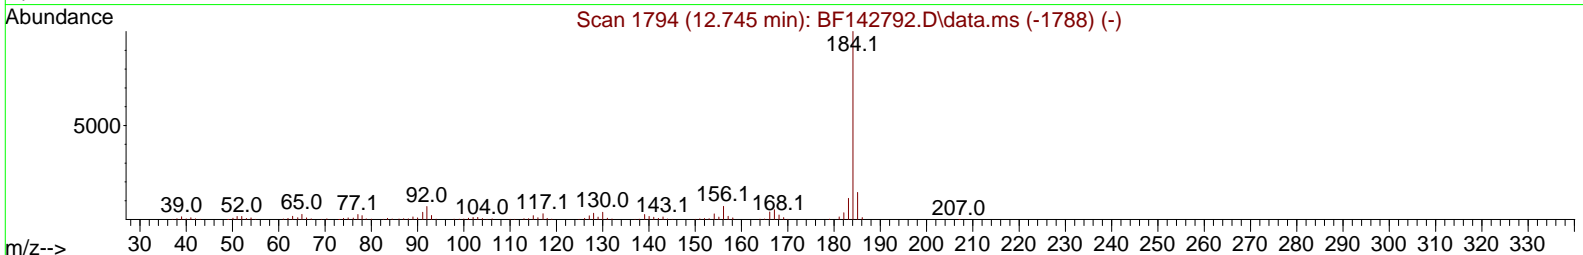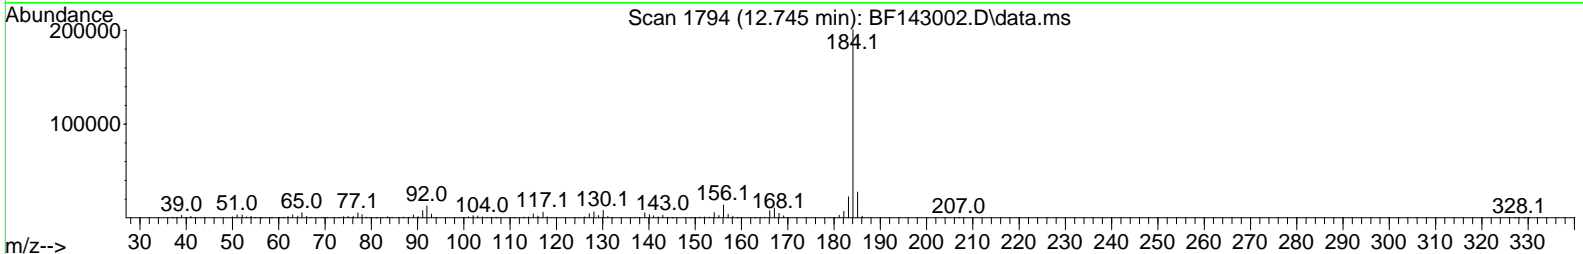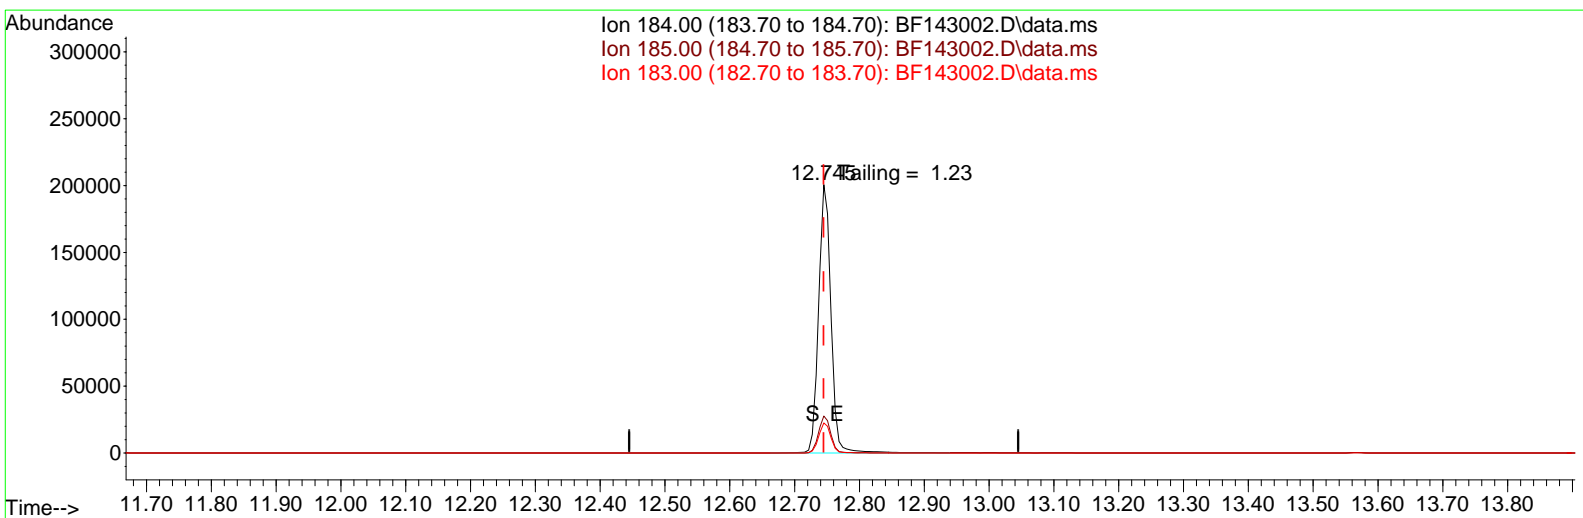

TIC: BF143002.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 267776

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.80
183.00	11.20	11.22
0.00	0.00	0.00