
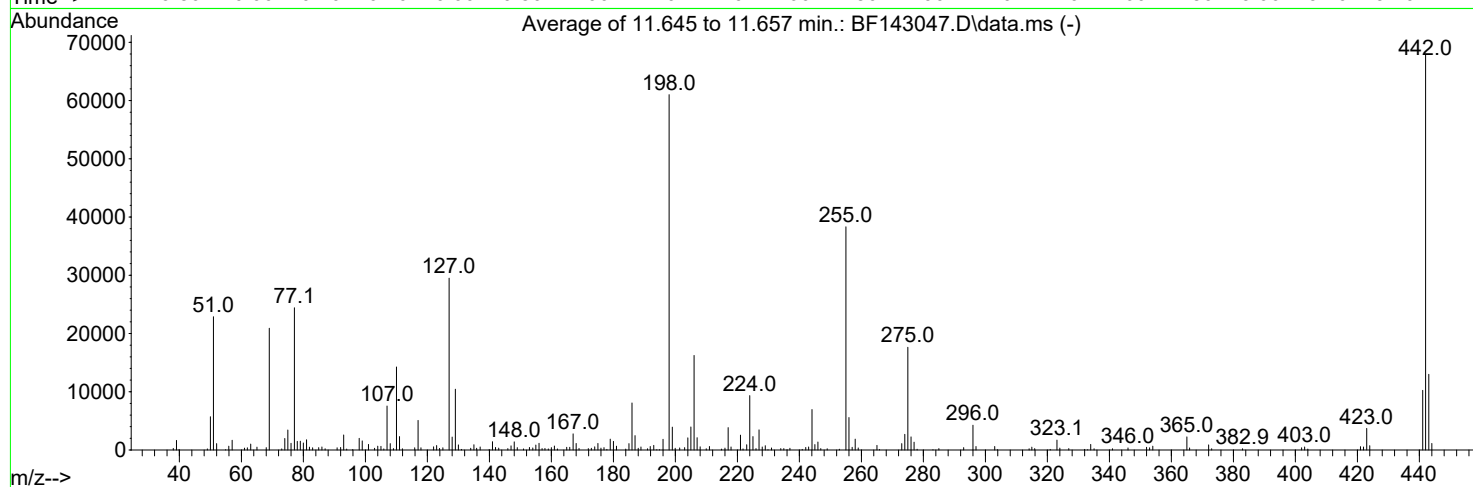


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
 Data File : BF143047.D
 Acq On : 09 Jul 2025 10:22
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 24 05:28:21 2025

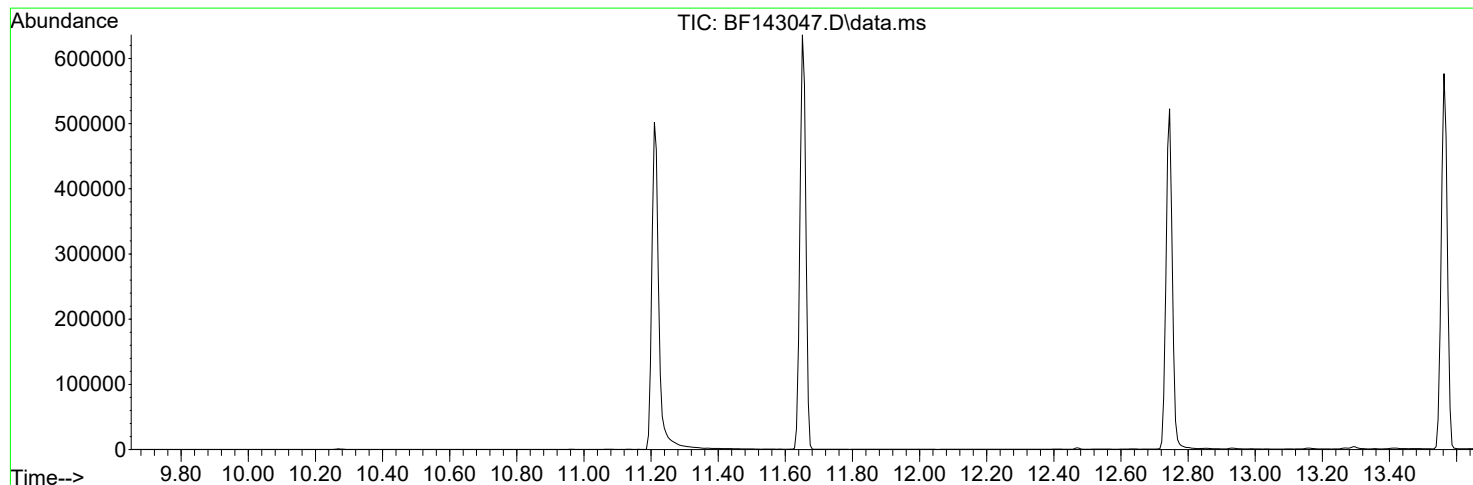

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	406	PASS
69	69	100	100	100.0	20917	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61016	PASS
199	198	5	9	6.5	3939	PASS
365	198	1	100	3.7	2249	PASS
441	443	0.01	150	78.8	10250	PASS
442	442	100	100	100.0	67792	PASS
443	442	15	24	19.2	13004	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/9/2025	BNA_F	<u>BF143047.D</u>
Compound Name	Response	Retention Time
DDT	150121	13.563
DDD	2906	13.292
DDE	645	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3551	153672	2.31

Instrument :
 BNA_F
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
 Data File : BF143047.D
 Acq On : 09 Jul 2025 10:22
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 09 11:29:10 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

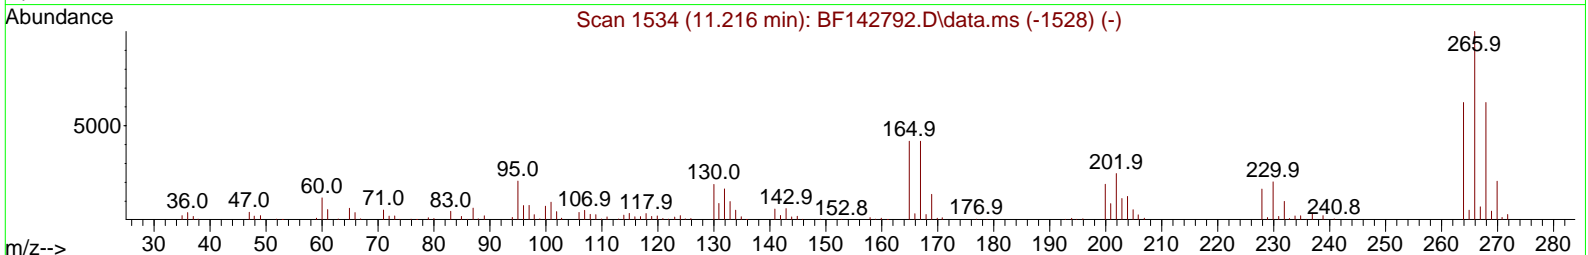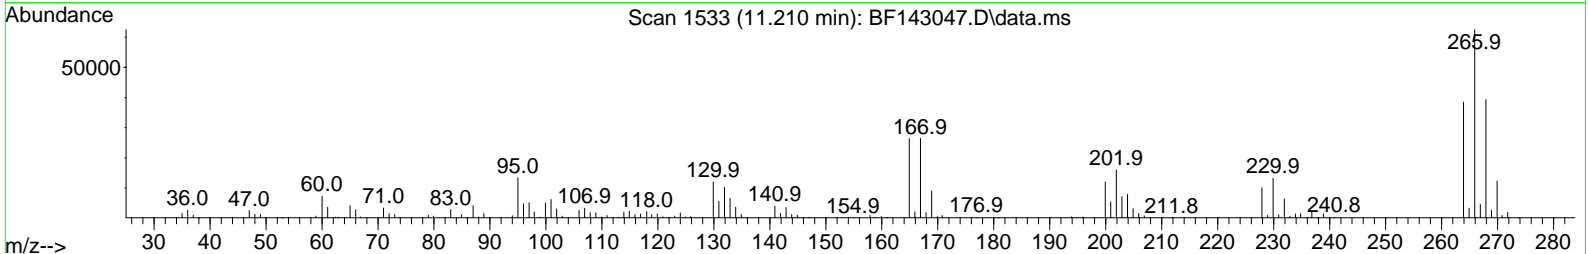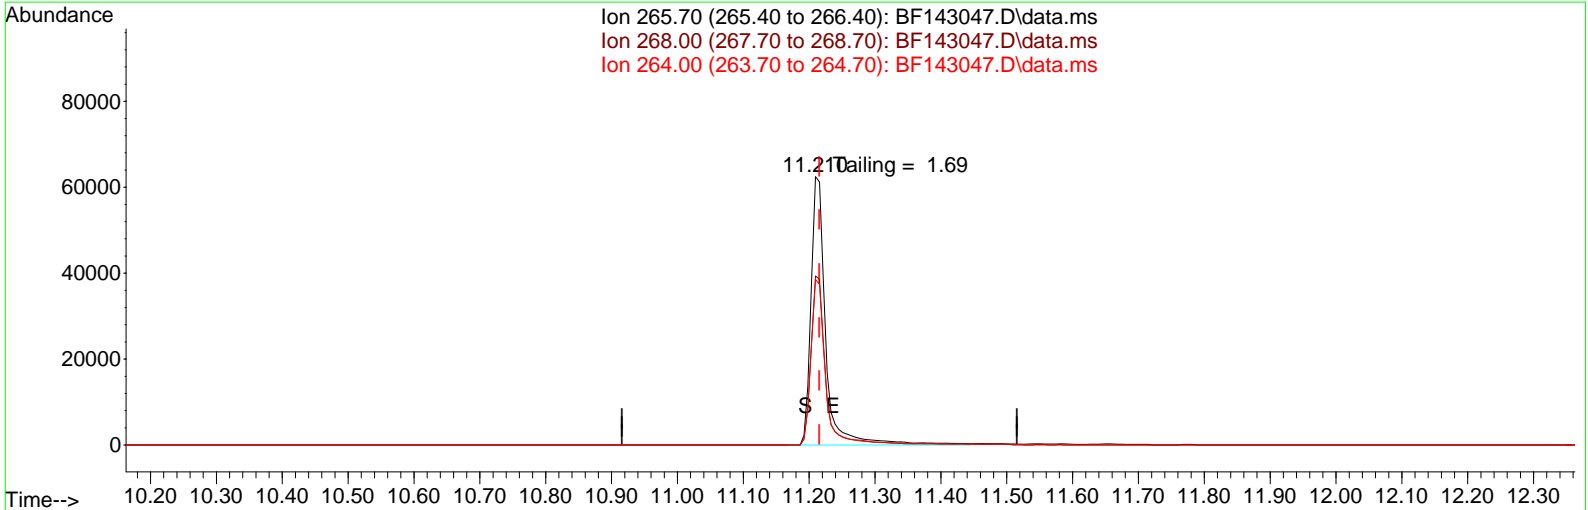

TIC: BF143047.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 48733.15 ng




response 96735

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.02
264.00	62.40	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
 Data File : BF143047.D
 Acq On : 09 Jul 2025 10:22
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 09 11:29:10 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 24 05:28:21 2025
 Response via : Initial Calibration

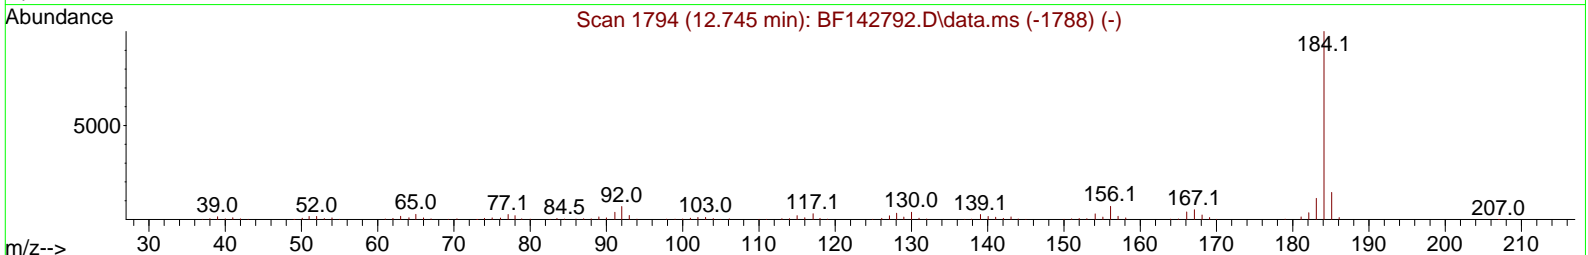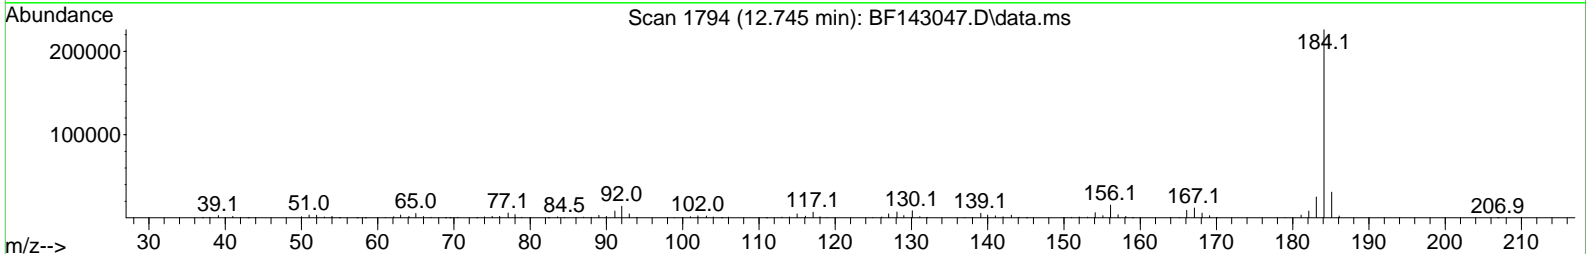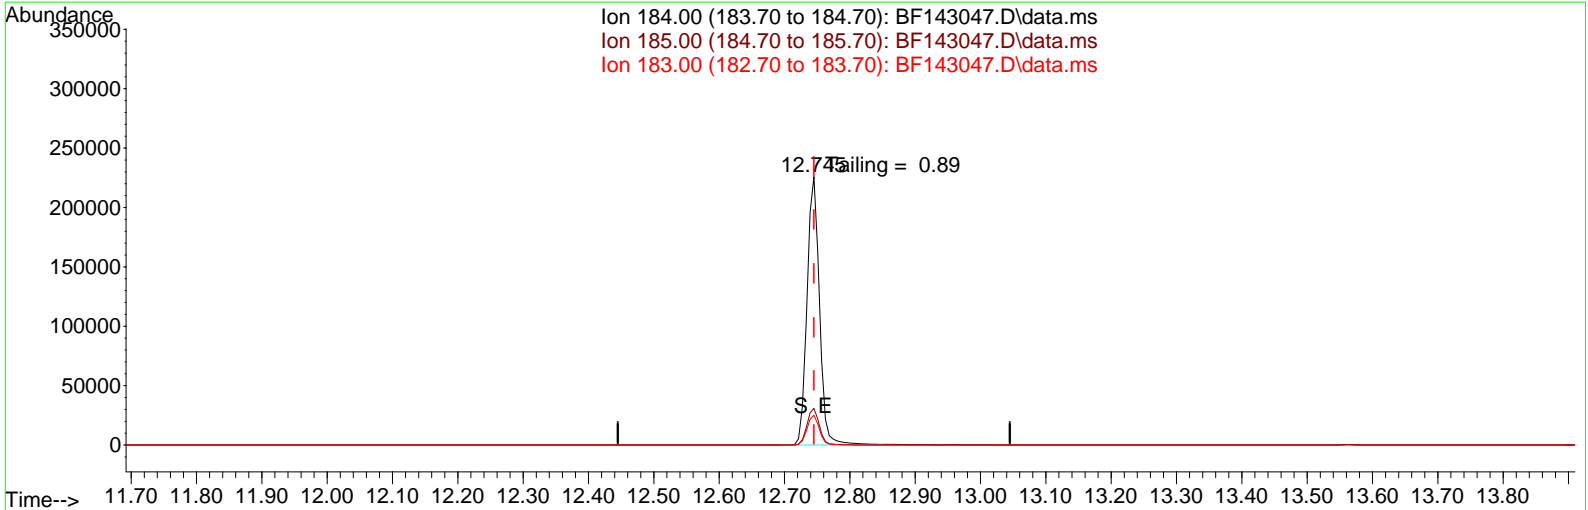

TIC: BF143047.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 301867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.67
183.00	11.20	11.11
0.00	0.00	0.00