
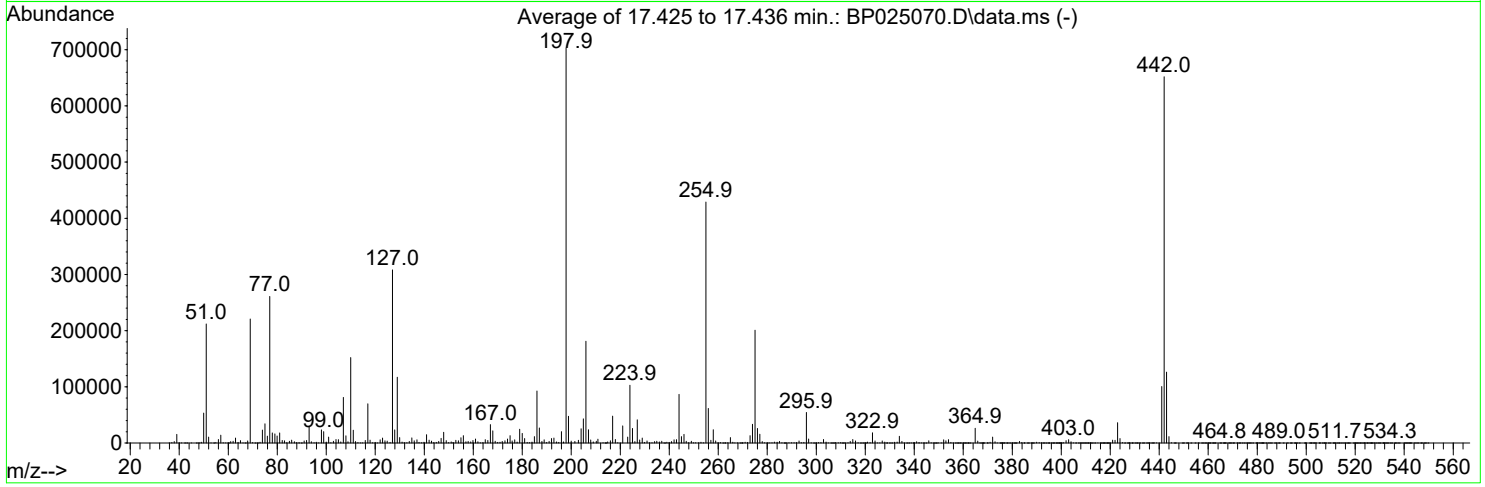


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070325\
 Data File : BP025070.D
 Acq On : 03 Jul 2025 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 03 16:05:44 2025

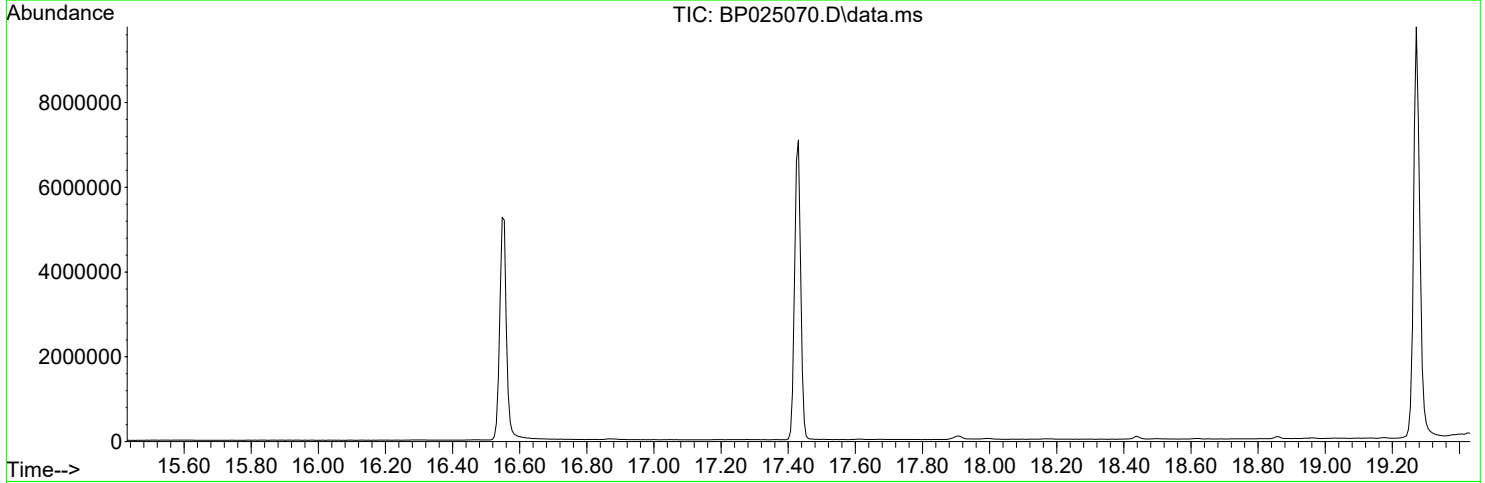

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	3747	PASS
69	69	100	100	100.0	220616	PASS
70	69	0.00	2	0.4	974	PASS
197	198	0.00	2	0.3	1975	PASS
198	198	100	100	100.0	702809	PASS
199	198	5	9	6.8	47648	PASS
365	198	1	100	3.7	26203	PASS
441	443	0.01	150	79.7	100672	PASS
442	442	100	100	100.0	651937	PASS
443	442	15	24	19.4	126320	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
7/3/2025	BNA_P	<u>BP025070.D</u>
Compound Name	Response	Retention Time
DDT	2078463	20.595
DDD	21773	20.183
DDE	1831	19.595
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23604	2102067	1.12

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070325\
 Data File : BP025070.D
 Acq On : 03 Jul 2025 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP

Quant Time: Jul 03 16:24:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 03 16:05:44 2025
 Response via : Initial Calibration

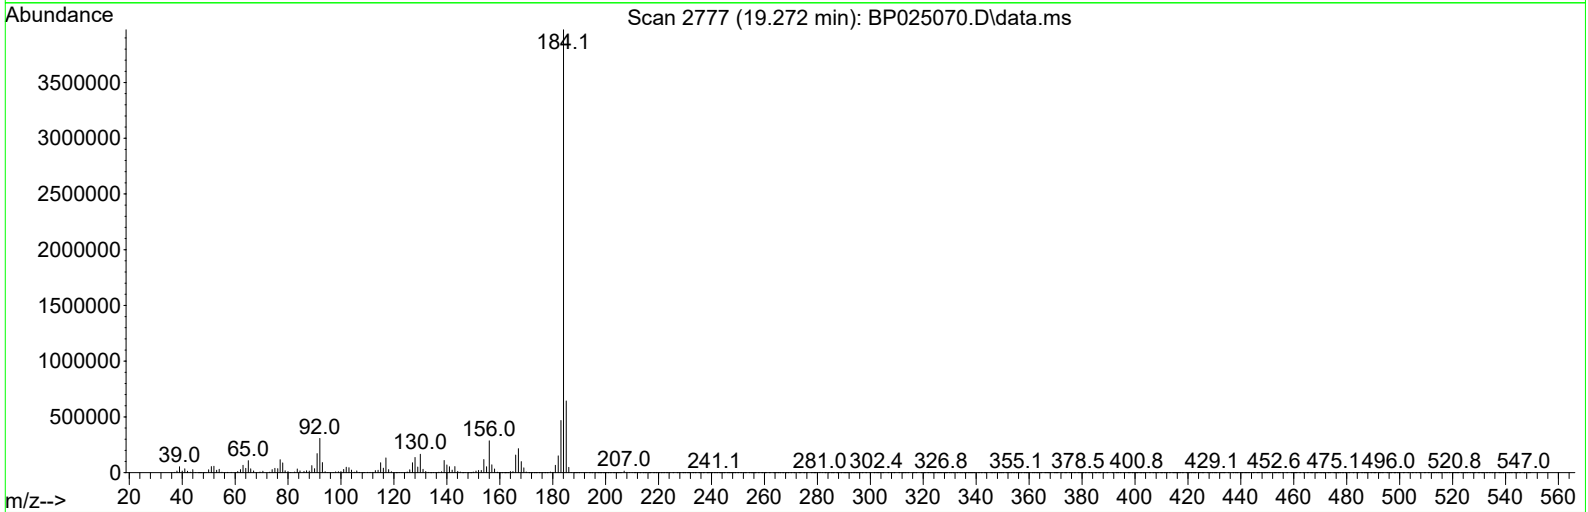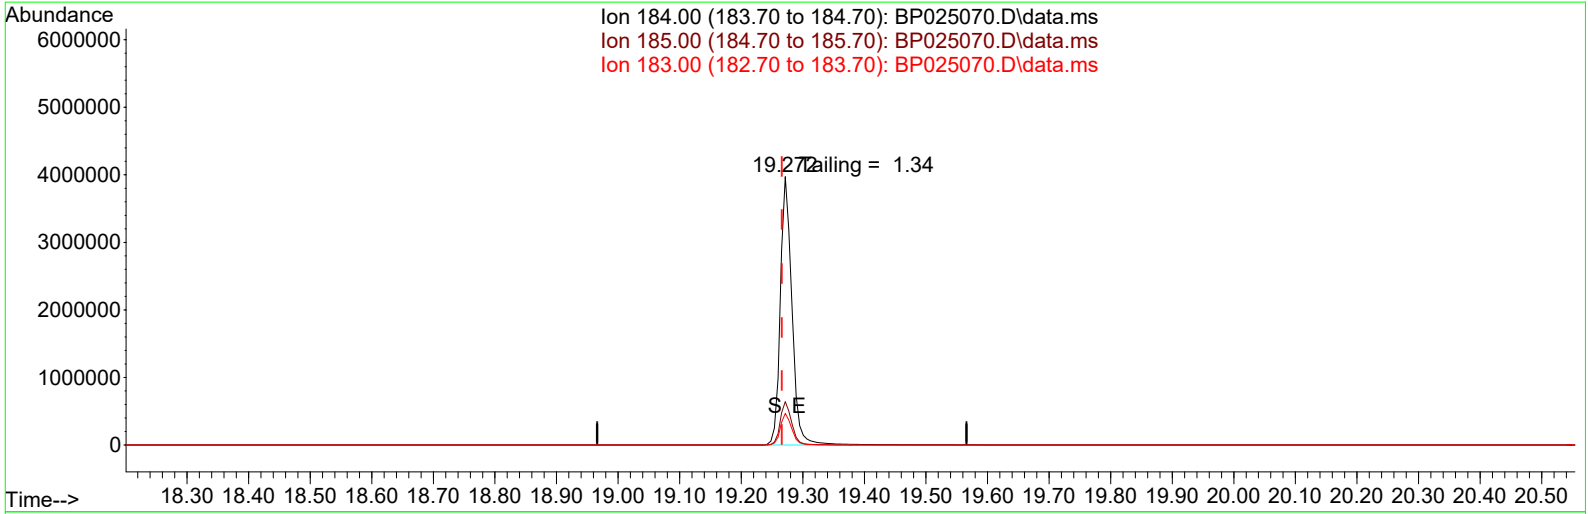

TIC: BP025070.D\data.ms

(77) Benzidine

19.272min (+ 0.006) 5891.13 ng



response 5273970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.19
183.00	11.80	11.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070325\
 Data File : BP025070.D
 Acq On : 03 Jul 2025 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP

Quant Time: Jul 03 16:24:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 03 16:05:44 2025
 Response via : Initial Calibration

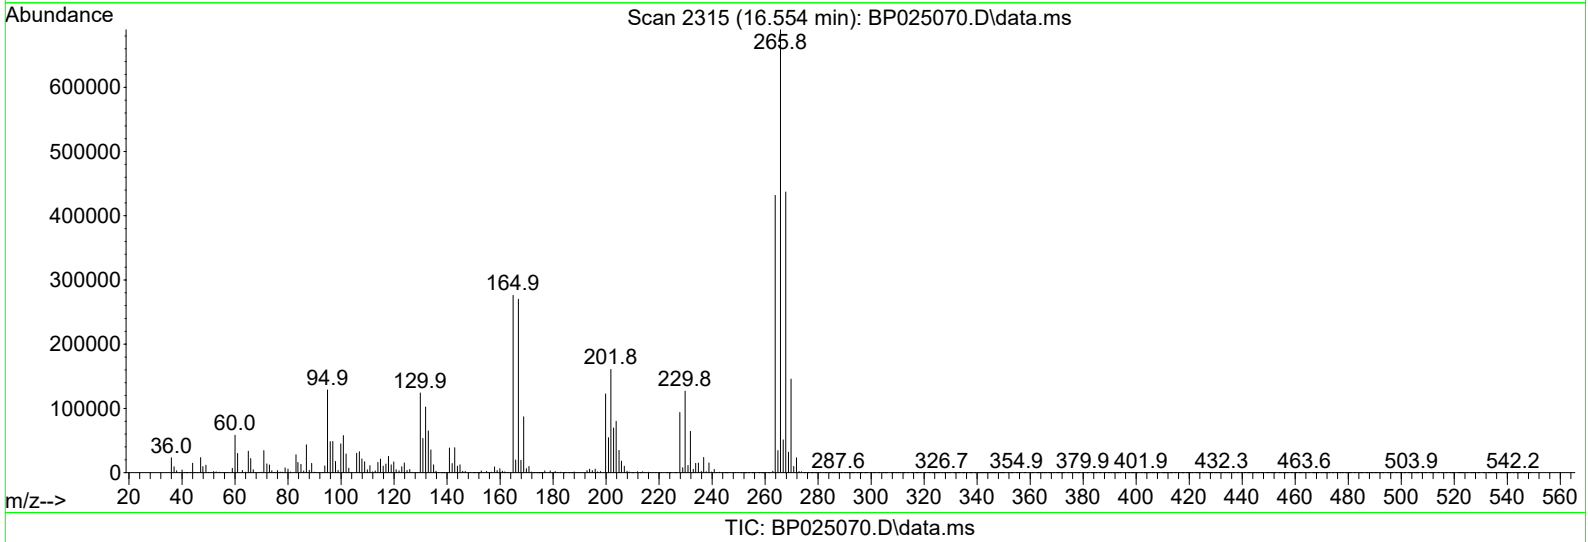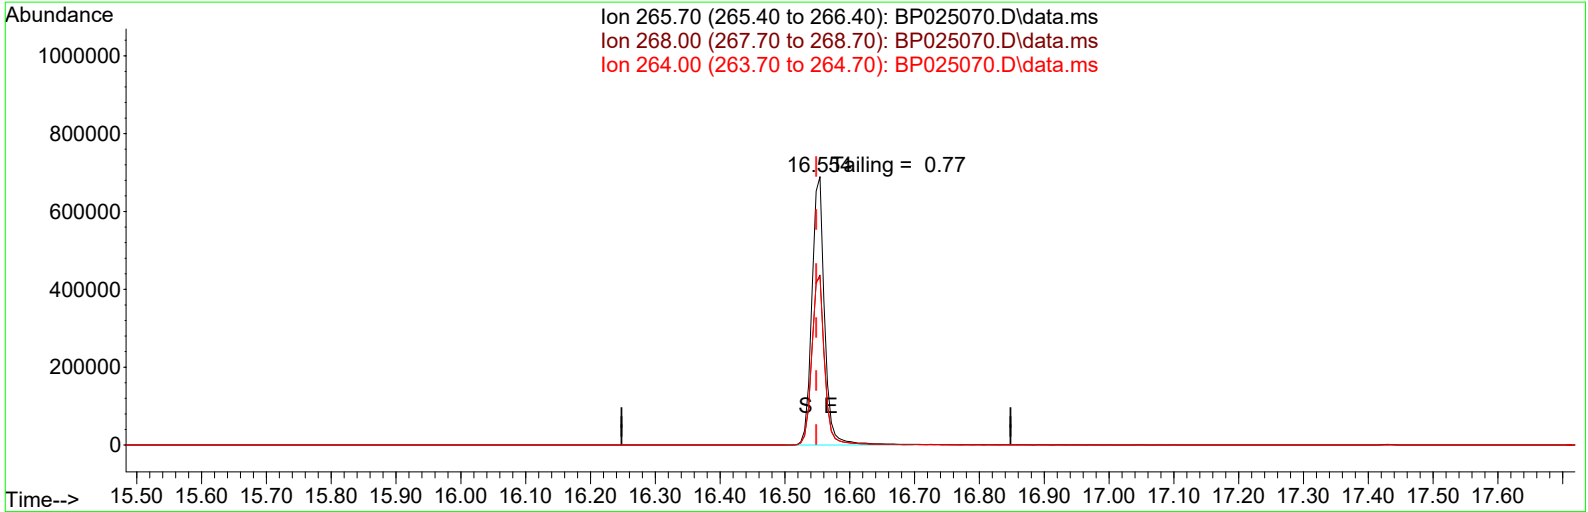

(70) Pentachlorophenol (C)

16.554min (+ 0.006) 170301.74 ng

response 942789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.35
264.00	62.70	62.60
0.00	0.00	0.00