
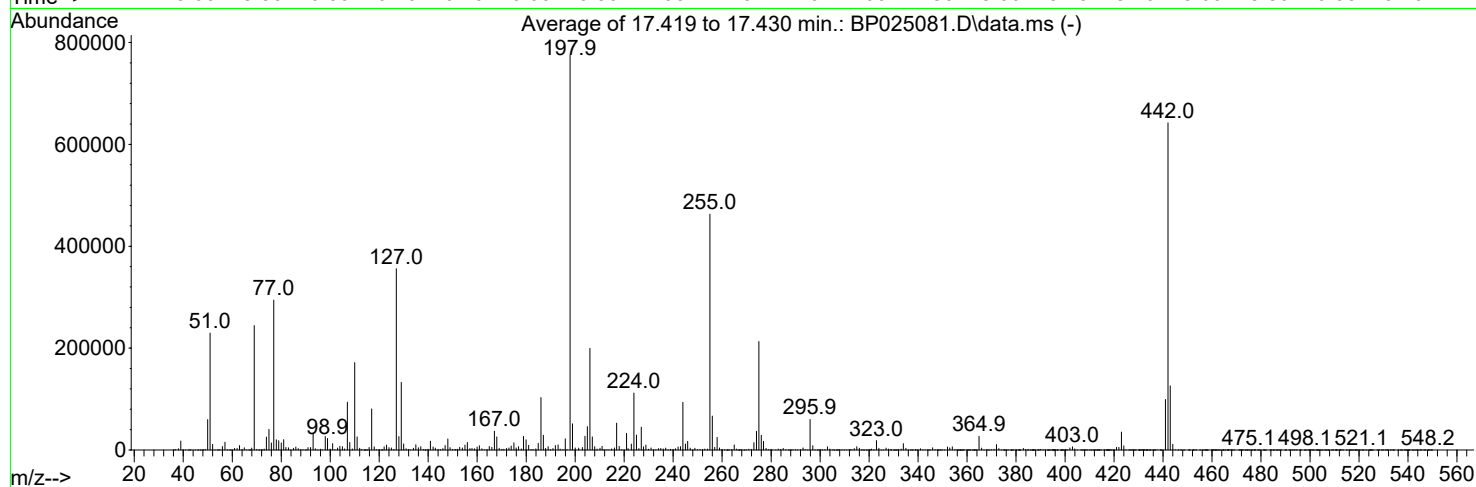


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071025\
 Data File : BP025081.D
 Acq On : 10 Jul 2025 13:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 03 16:05:44 2025

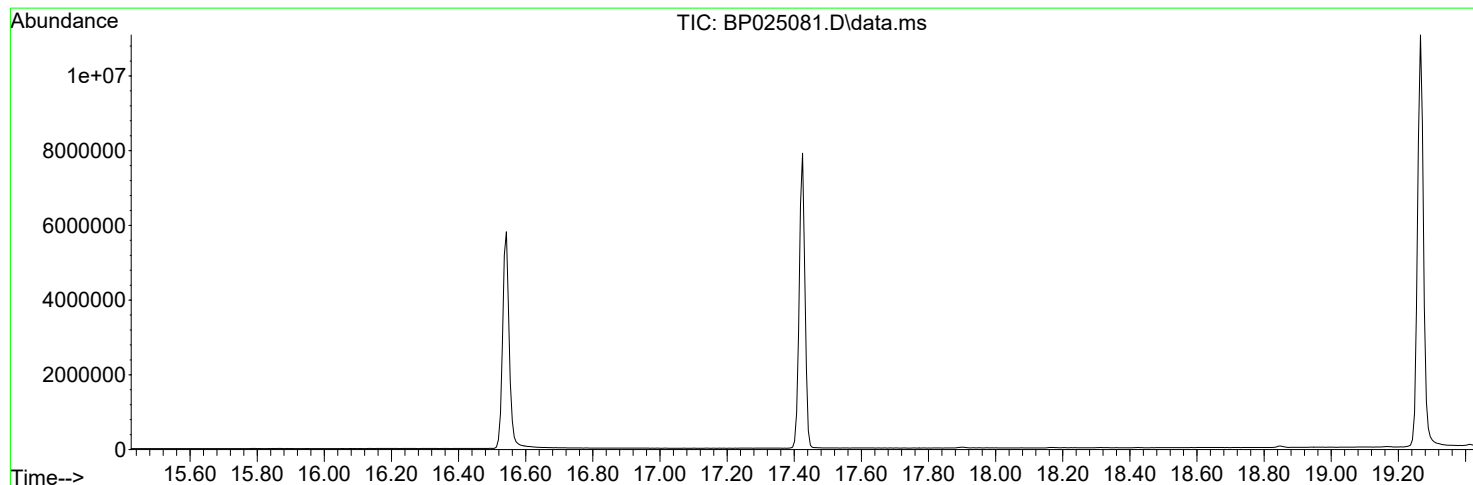

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	3778	PASS
69	69	100	100	100.0	244532	PASS
70	69	0.00	2	0.5	1252	PASS
197	198	0.00	2	0.1	745	PASS
198	198	100	100	100.0	775174	PASS
199	198	5	9	6.7	51677	PASS
365	198	1	100	3.5	27166	PASS
441	443	0.01	150	78.8	99320	PASS
442	442	100	100	100.0	642507	PASS
443	442	15	24	19.6	126088	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/10/2025	BNA_P	<u>BP025081.D</u>
Compound Name	Response	Retention Time
DDT	2296271	20.571
DDD	29620	20.113
DDE	2816	19.589
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32436	2328707	1.39

Instrument :
 BNA_P
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071025\
 Data File : BP025081.D
 Acq On : 10 Jul 2025 13:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 10 15:22:57 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 03 16:05:44 2025
 Response via : Initial Calibration

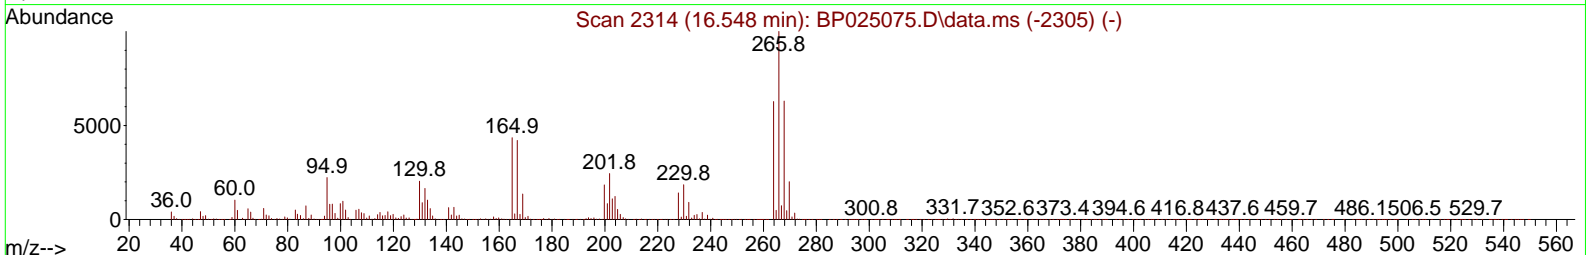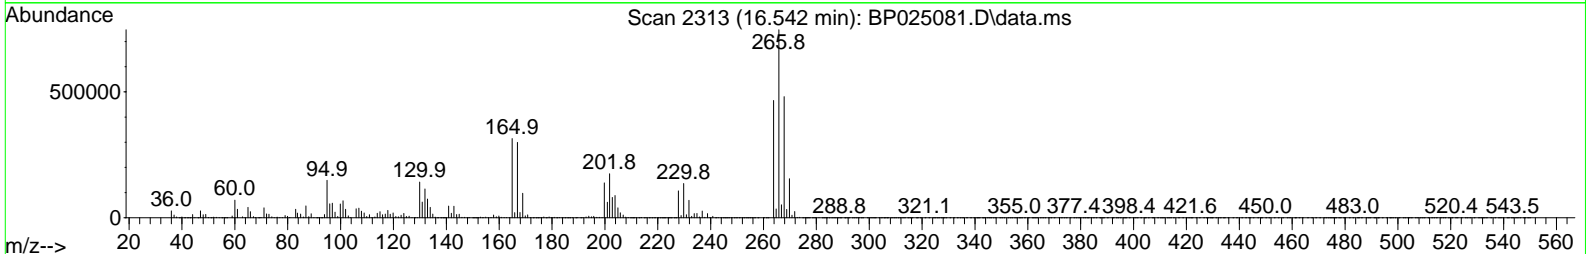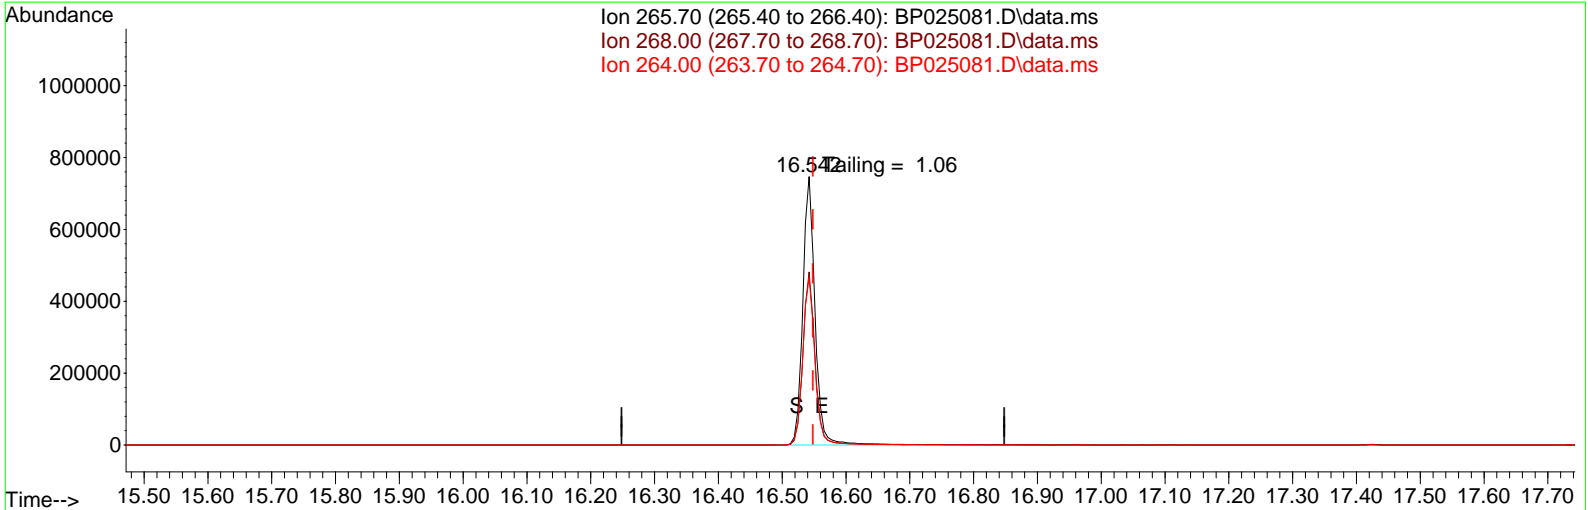

TIC: BP025081.D\data.ms

(70) Pentachlorophenol (C)

16.542min (-0.006) 1224837.14 ng




response 1004163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.46
264.00	62.70	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071025\
 Data File : BP025081.D
 Acq On : 10 Jul 2025 13:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 10 15:22:57 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 03 16:05:44 2025
 Response via : Initial Calibration

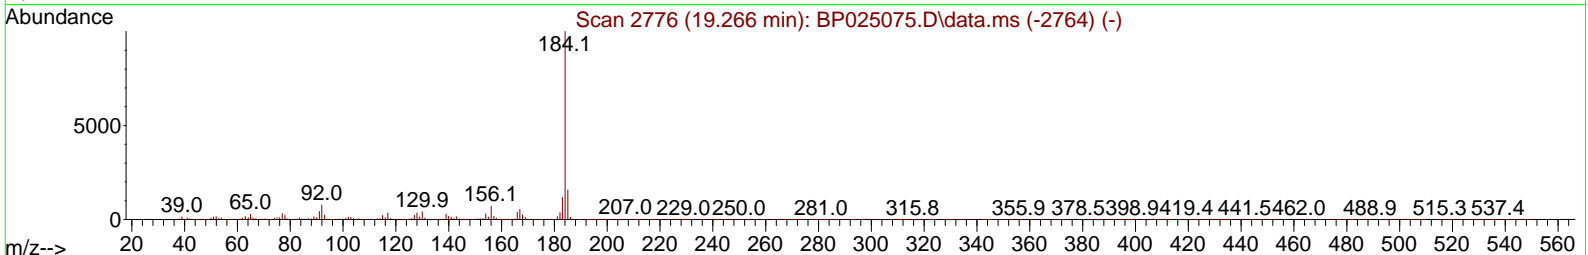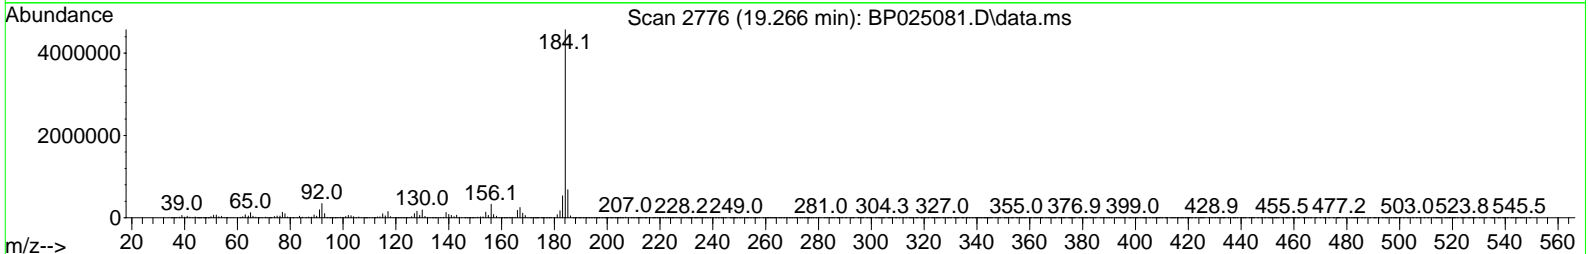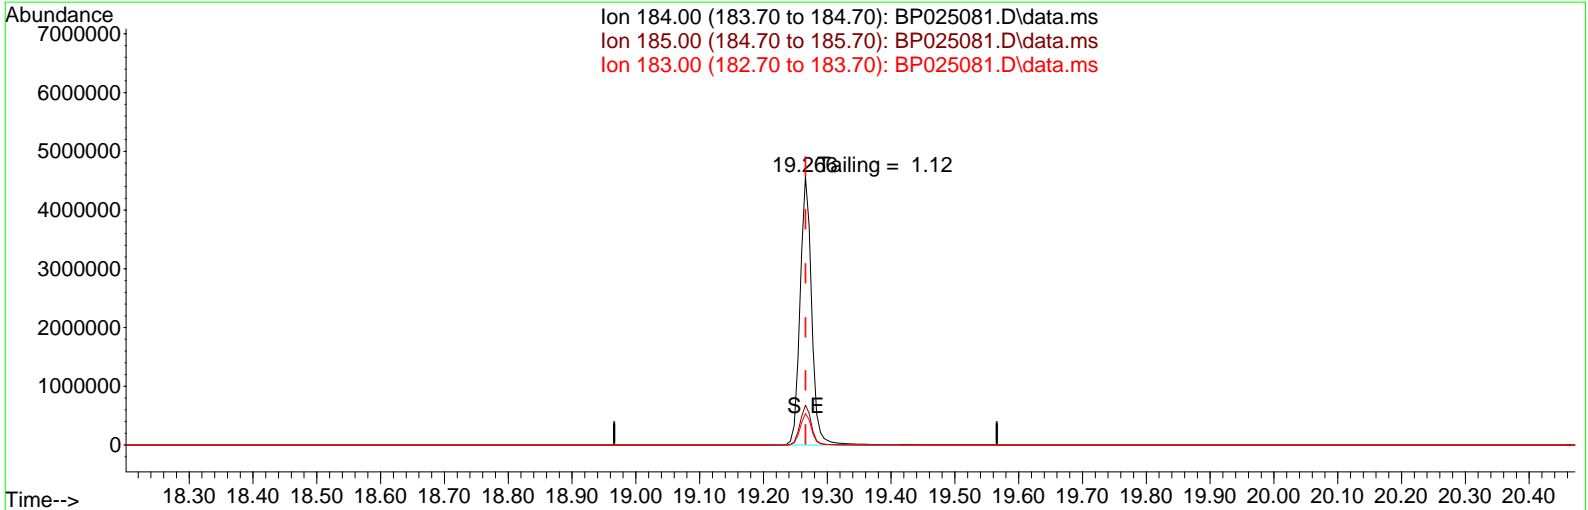

TIC: BP025081.D\data.ms

(77) Benzidine

19.266min (-0.000) 557908.95 ng

response 5813536

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.87
183.00	11.80	11.69
0.00	0.00	0.00