
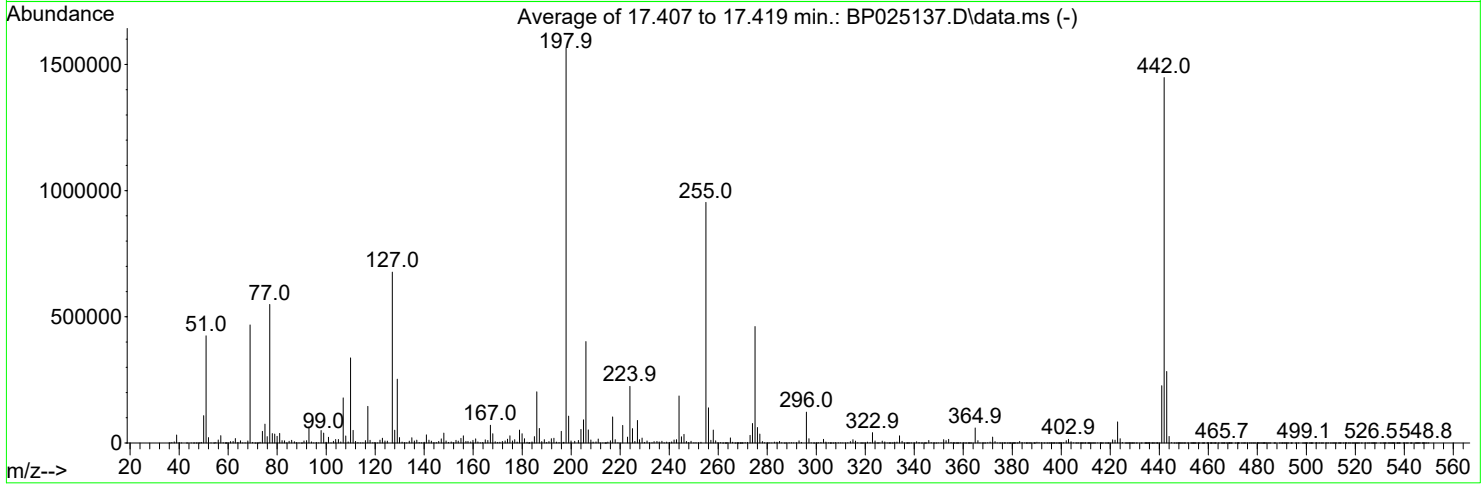


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071525\
 Data File : BP025137.D
 Acq On : 15 Jul 2025 08:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 03 16:05:44 2025

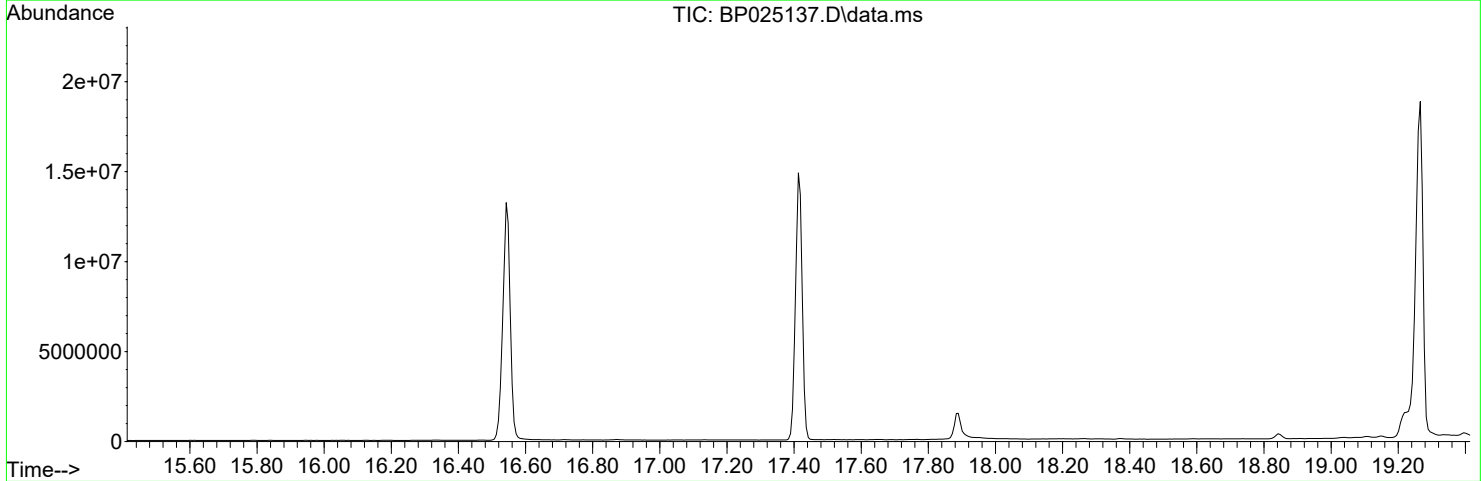

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	8083	PASS
69	69	100	100	100.0	467686	PASS
70	69	0.00	2	0.5	2432	PASS
197	198	0.00	2	0.2	3025	PASS
198	198	100	100	100.0	1564419	PASS
199	198	5	9	6.8	106484	PASS
365	198	1	100	3.8	59381	PASS
441	443	0.01	150	79.9	226731	PASS
442	442	100	100	100.0	1448320	PASS
443	442	15	24	19.6	283648	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/15/2025	BNA_P	<u>BP025137.D</u>
Compound Name	Response	Retention Time
DDT	5862215	20.571
DDD	105722	20.154
DDE	3773	19.577
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
109495	5971710	1.83

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071525\
 Data File : BP025137.D
 Acq On : 15 Jul 2025 08:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP

Quant Time: Jul 15 11:52:02 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 03 16:05:44 2025
 Response via : Initial Calibration

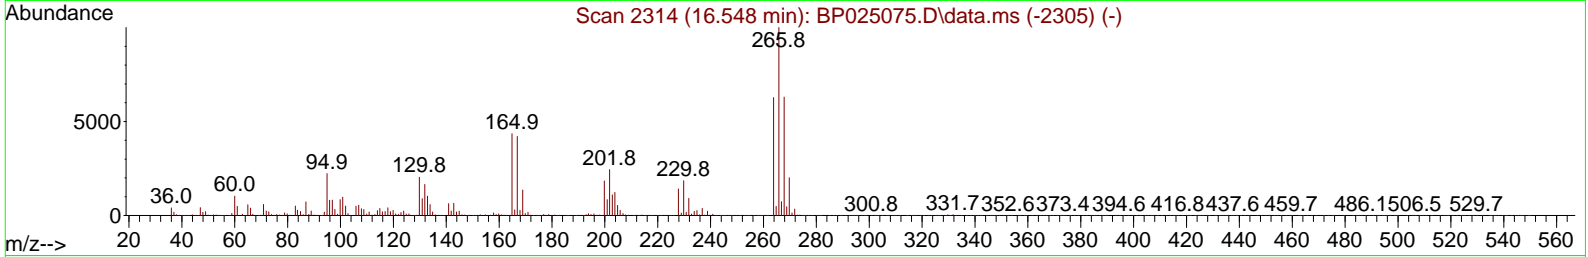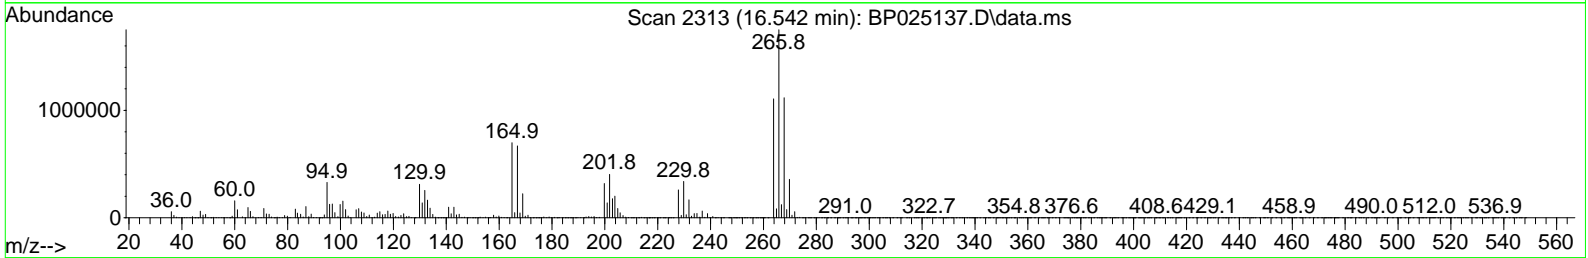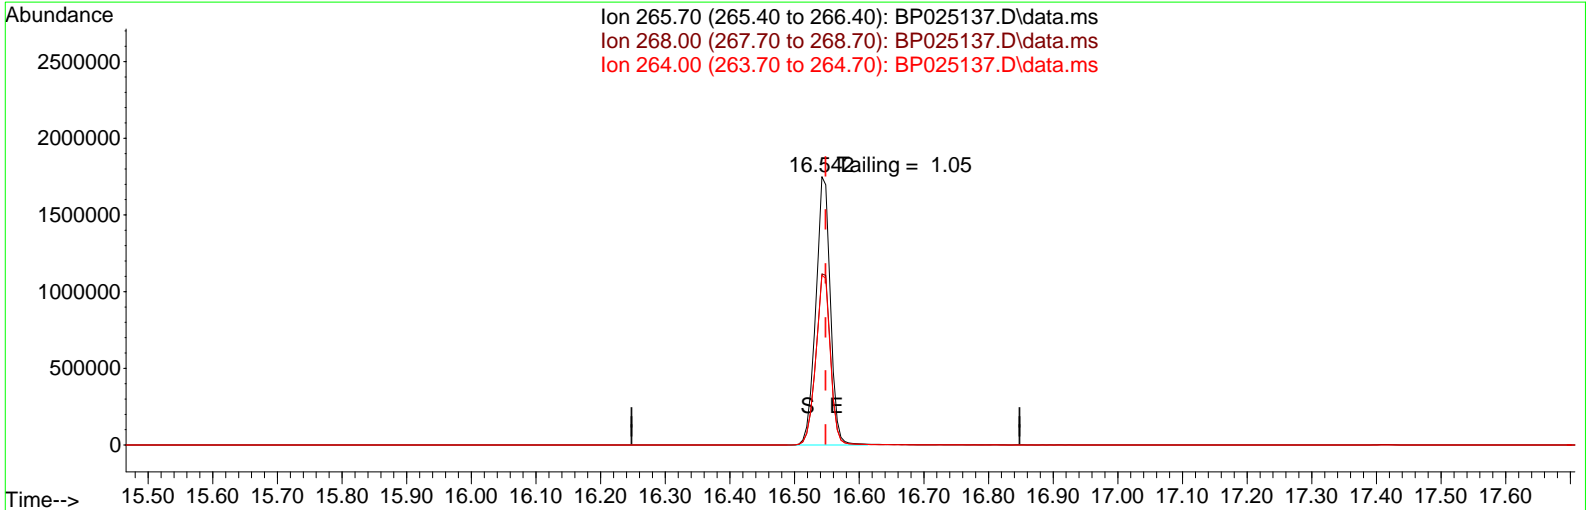

TIC: BP025137.D\data.ms

(70) Pentachlorophenol (C)

16.542min (-0.006) 102240.67 ng




response 2751382

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.81
264.00	62.70	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071525\
 Data File : BP025137.D
 Acq On : 15 Jul 2025 08:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 11:52:02 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 03 16:05:44 2025
 Response via : Initial Calibration

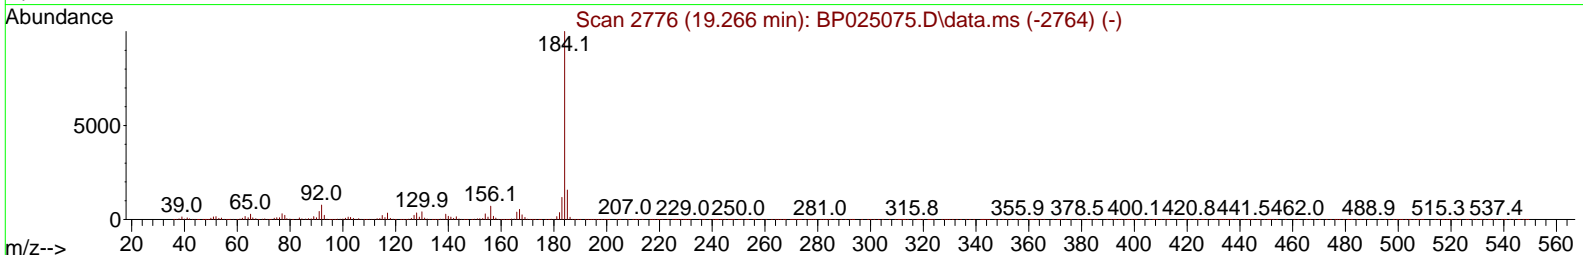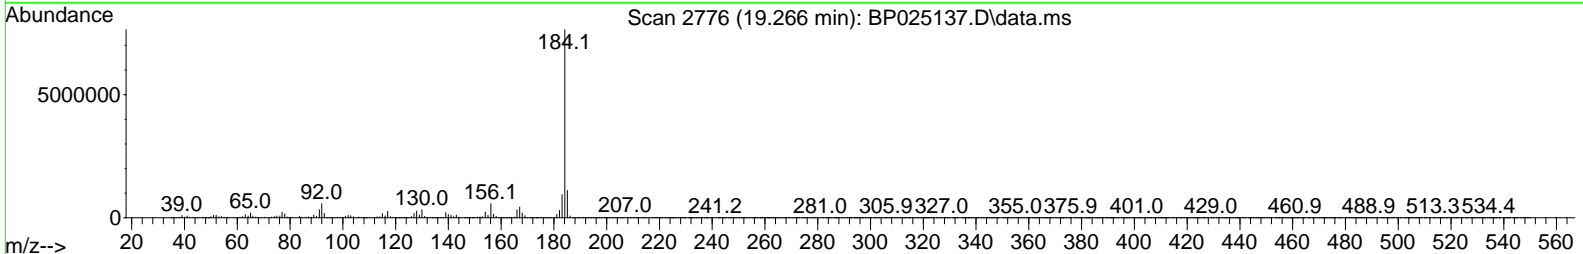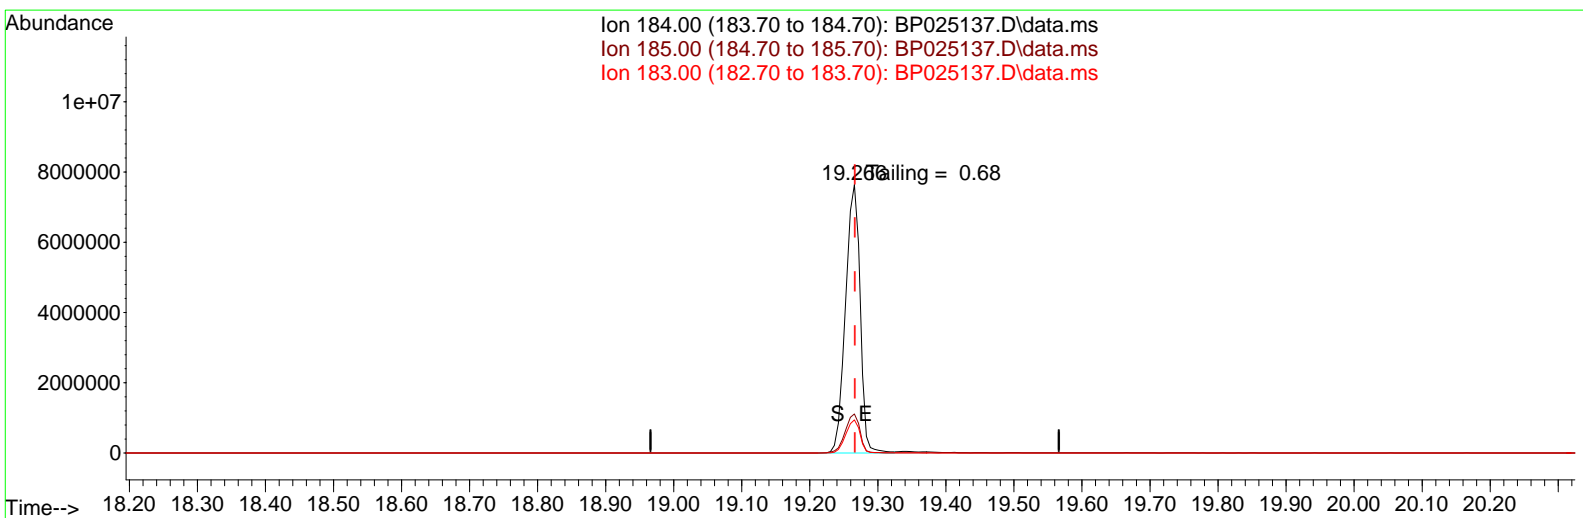

TIC: BP025137.D\data.ms

(77) Benzidine

19.266min (-0.000) 24087.44 ng

response 11322496

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.57
183.00	11.80	12.35
0.00	0.00	0.00