
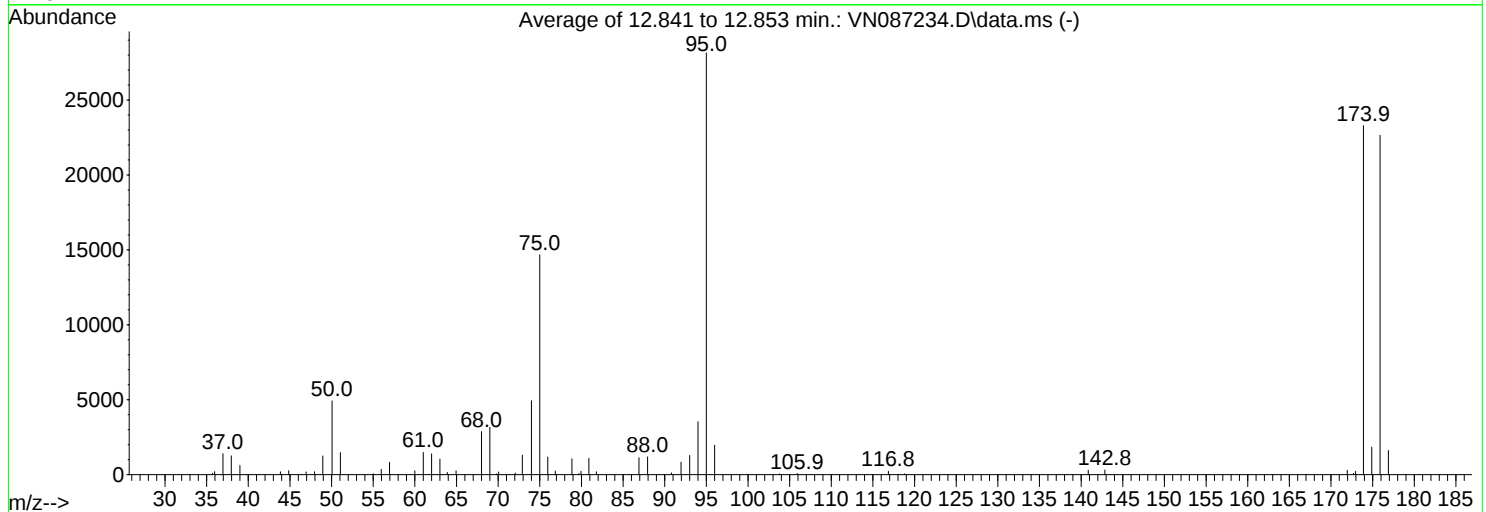


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN063025\
Data File : VN087234.D
Acq On : 30 Jun 2025 09:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Title : SW846 8260
Last Update : Tue Jul 01 03:15:00 2025

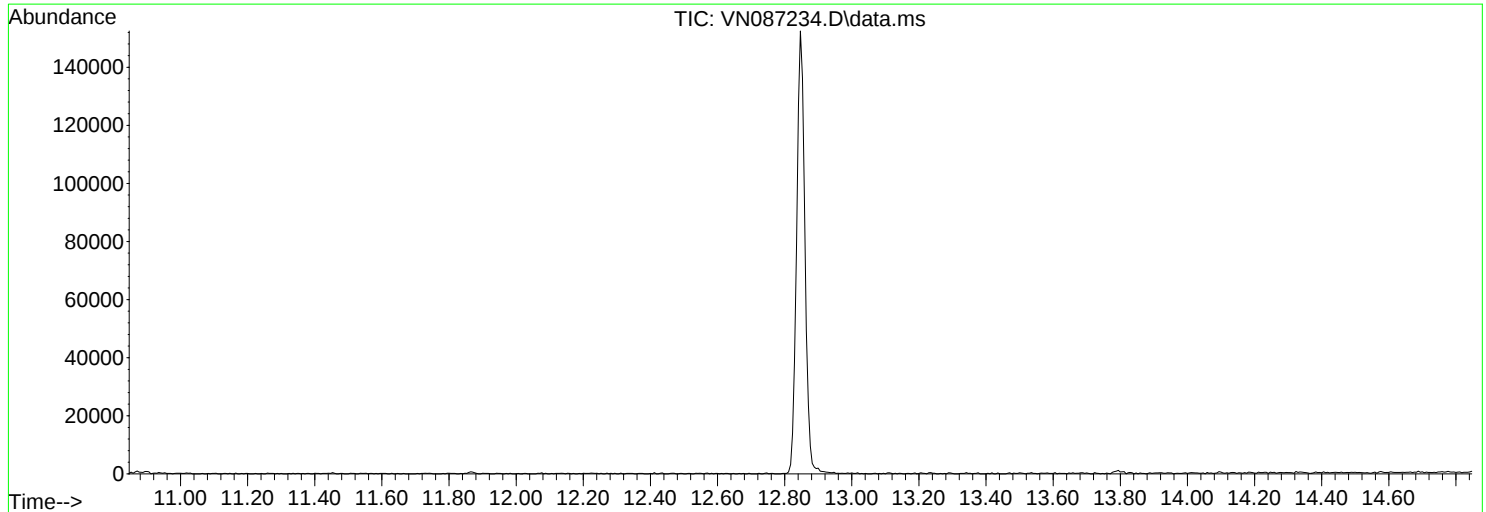

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4928	PASS
75	95	30	60	52.1	14668	PASS
95	95	100	100	100.0	28149	PASS
96	95	5	9	7.0	1968	PASS
173	174	0.00	2	0.9	221	PASS
174	95	50	100	82.7	23293	PASS
175	174	5	9	7.9	1836	PASS
176	174	95	101	97.2	22643	PASS
177	176	5	9	7.1	1613	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	100	51.05	1478	69.00	3162	79.95	221
35.95	206	55.00	64	69.80	54	80.90	109
36.95	1397	55.95	358	70.05	180	81.80	19
37.95	1257	56.95	818	72.05	112	86.90	112
39.00	611	60.00	254	72.90	1302	87.95	1181
43.85	189	61.00	1485	74.00	4937	90.80	123
44.85	271	62.00	1386	75.00	14668	91.95	830
46.95	177	63.00	1037	75.95	1173	93.00	1283
47.95	191	63.90	146	76.85	242	94.00	3536
48.95	1251	64.95	254	78.85	1062	95.00	28149
50.05	4928	68.00	2872	79.70	77	96.00	1968

Average of 12.841 to 12.853 min.: VN087234.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.80	55	175.90	22643				
105.90	70	176.90	1613				
116.85	229						
118.80	59						
140.85	303						
142.85	314						
171.95	288						
172.70	84						
172.95	221						
173.90	23293						
174.90	1836						

Instrument :

MSVOA_N

ClientSampleId :

BFB