
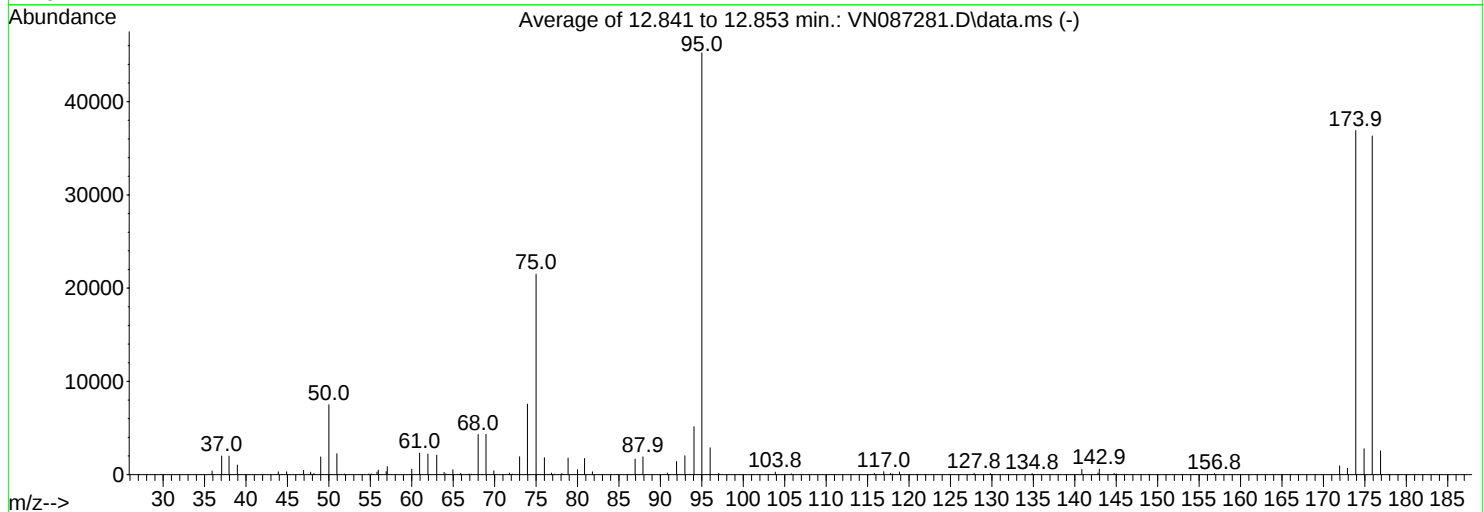


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN070725\
Data File : VN087281.D
Acq On : 07 Jul 2025 08:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N063025W.M
Title : SW846 8260
Last Update : Tue Jul 01 03:15:00 2025

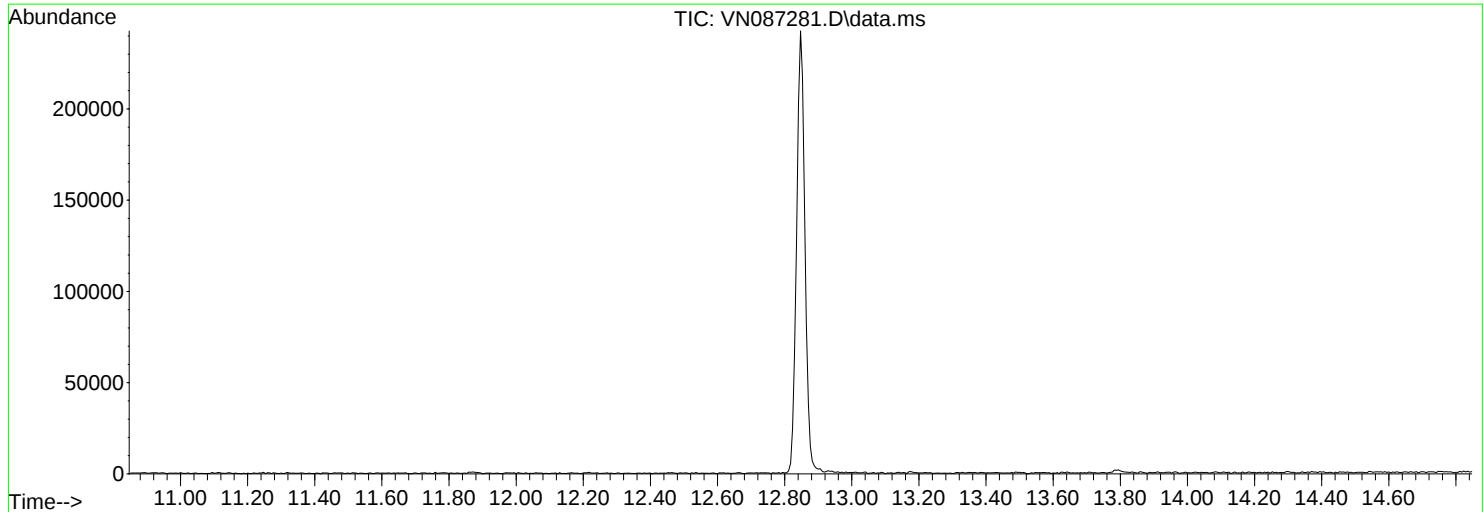

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	7493	PASS
75	95	30	60	47.5	21507	PASS
95	95	100	100	100.0	45235	PASS
96	95	5	9	6.4	2883	PASS
173	174	0.00	2	1.9	683	PASS
174	95	50	100	81.6	36891	PASS
175	174	5	9	7.6	2789	PASS
176	174	95	101	98.5	36323	PASS
177	176	5	9	7.1	2565	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	398	50.95	2250	63.00	2103	72.10	71
37.05	2003	51.90	66	63.90	248	73.00	192
37.95	1985	54.80	71	64.10	79	73.95	756
38.95	1025	55.10	92	64.95	541	75.00	2150
43.90	310	55.80	269	65.90	134	76.00	1817
44.90	307	55.95	474	66.90	65	76.85	167
46.95	463	56.90	327	67.20	56	77.20	56
47.80	276	57.05	856	68.00	4317	78.10	126
48.20	142	60.00	579	68.95	4331	78.85	1781
49.00	1899	60.95	2297	69.90	406	80.00	528
50.00	7493	61.95	2207	71.80	174	80.85	1734

Average of 12.841 to 12.853 min.: VN087281.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	305	105.80	87	142.95	586	177.90	60
86.95	1658	115.80	134	144.75	137		
87.90	1905	116.95	322	145.00	88		
90.85	179	117.75	137	146.00	54		
91.95	1417	118.00	89	156.85	120		
92.95	2025	118.85	293	171.95	953		
94.05	5150	127.85	151	172.90	683		
95.00	45235	129.80	119	173.90	36891		
96.00	2883	134.85	115	174.90	2789		
97.05	144	140.85	569	175.90	36323		
103.85	274	142.80	177	176.90	2565		

Instrument :

MSVOA_N

ClientSampleId :

BFB