
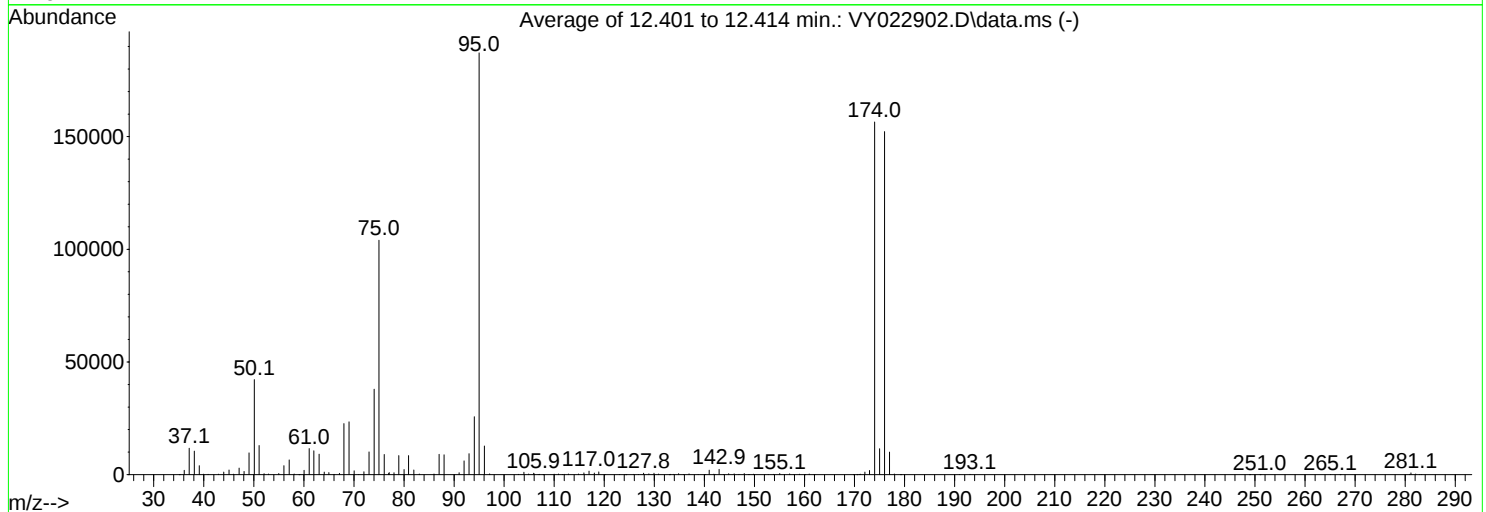


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070225\
Data File : VY022902.D
Acq On : 02 Jul 2025 08:51
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Title : SW846 8260
Last Update : Tue Jun 24 08:29:52 2025

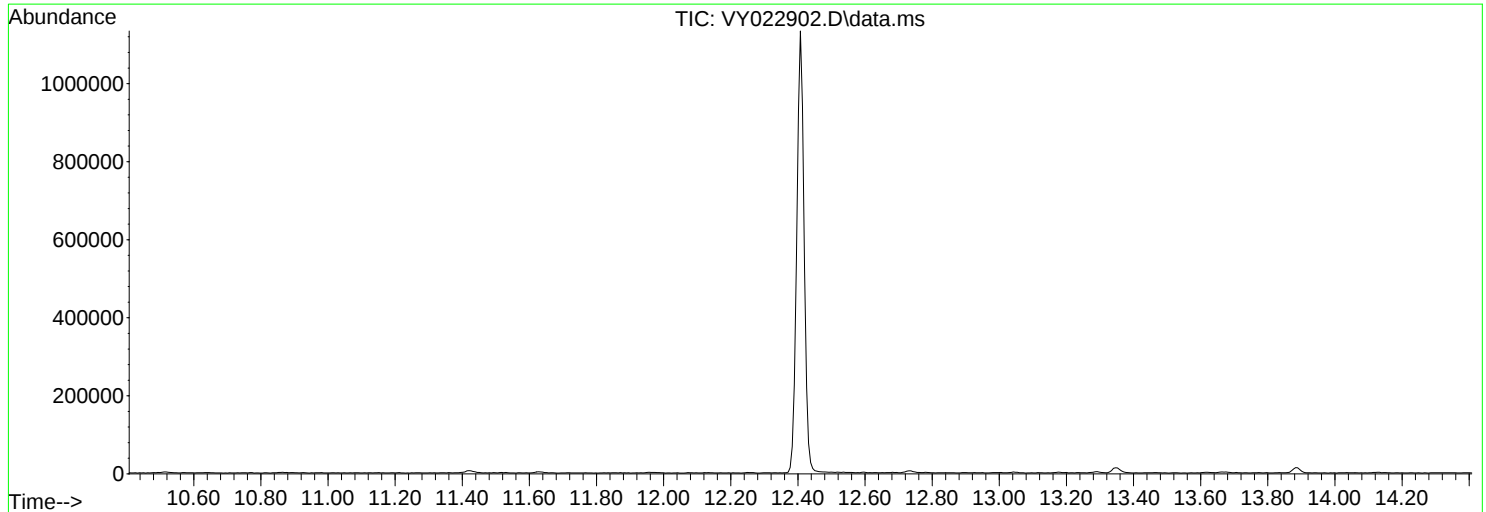

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	42181	PASS
75	95	30	60	55.6	103995	PASS
95	95	100	100	100.0	187179	PASS
96	95	5	9	6.8	12720	PASS
173	174	0.00	2	1.2	1816	PASS
174	95	50	100	83.6	156480	PASS
175	174	5	9	7.3	11484	PASS
176	174	95	101	97.3	152213	PASS
177	176	5	9	6.6	10021	PASS