

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070725\
 Data File : VY022956.D
 Acq On : 07 Jul 2025 13:38
 Operator : SY/MD
 Sample : Q2487-08
 Misc : 3.38g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 G1(10)

Quant Time: Jul 08 01:46:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 24 08:29:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	283210	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	516435	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	471025	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	158953	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	163131	51.609	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 103.220%	
35) Dibromofluoromethane	7.634	113	168212	53.559	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 107.120%	
50) Toluene-d8	10.103	98	621930	49.903	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 99.800%	
62) 4-Bromofluorobenzene	12.401	95	182265	45.494	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 90.980%	
Target Compounds						
					Qvalue	
16) Acetone	3.872	43	274566	459.574	ug/l	97
17) Carbon Disulfide	4.104	76	17293	1.867	ug/l	98
20) Methylene Chloride	4.610	84	29536	7.828	ug/l	98
25) 2-Butanone	6.896	43	93388	107.401	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070725\
Data File : VY022956.D
Acq On : 07 Jul 2025 13:38
Operator : SY/MD
Sample : Q2487-08
Misc : 3.38g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
G1(10)

Quant Time: Jul 08 01:46:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 24 08:29:52 2025
Response via : Initial Calibration




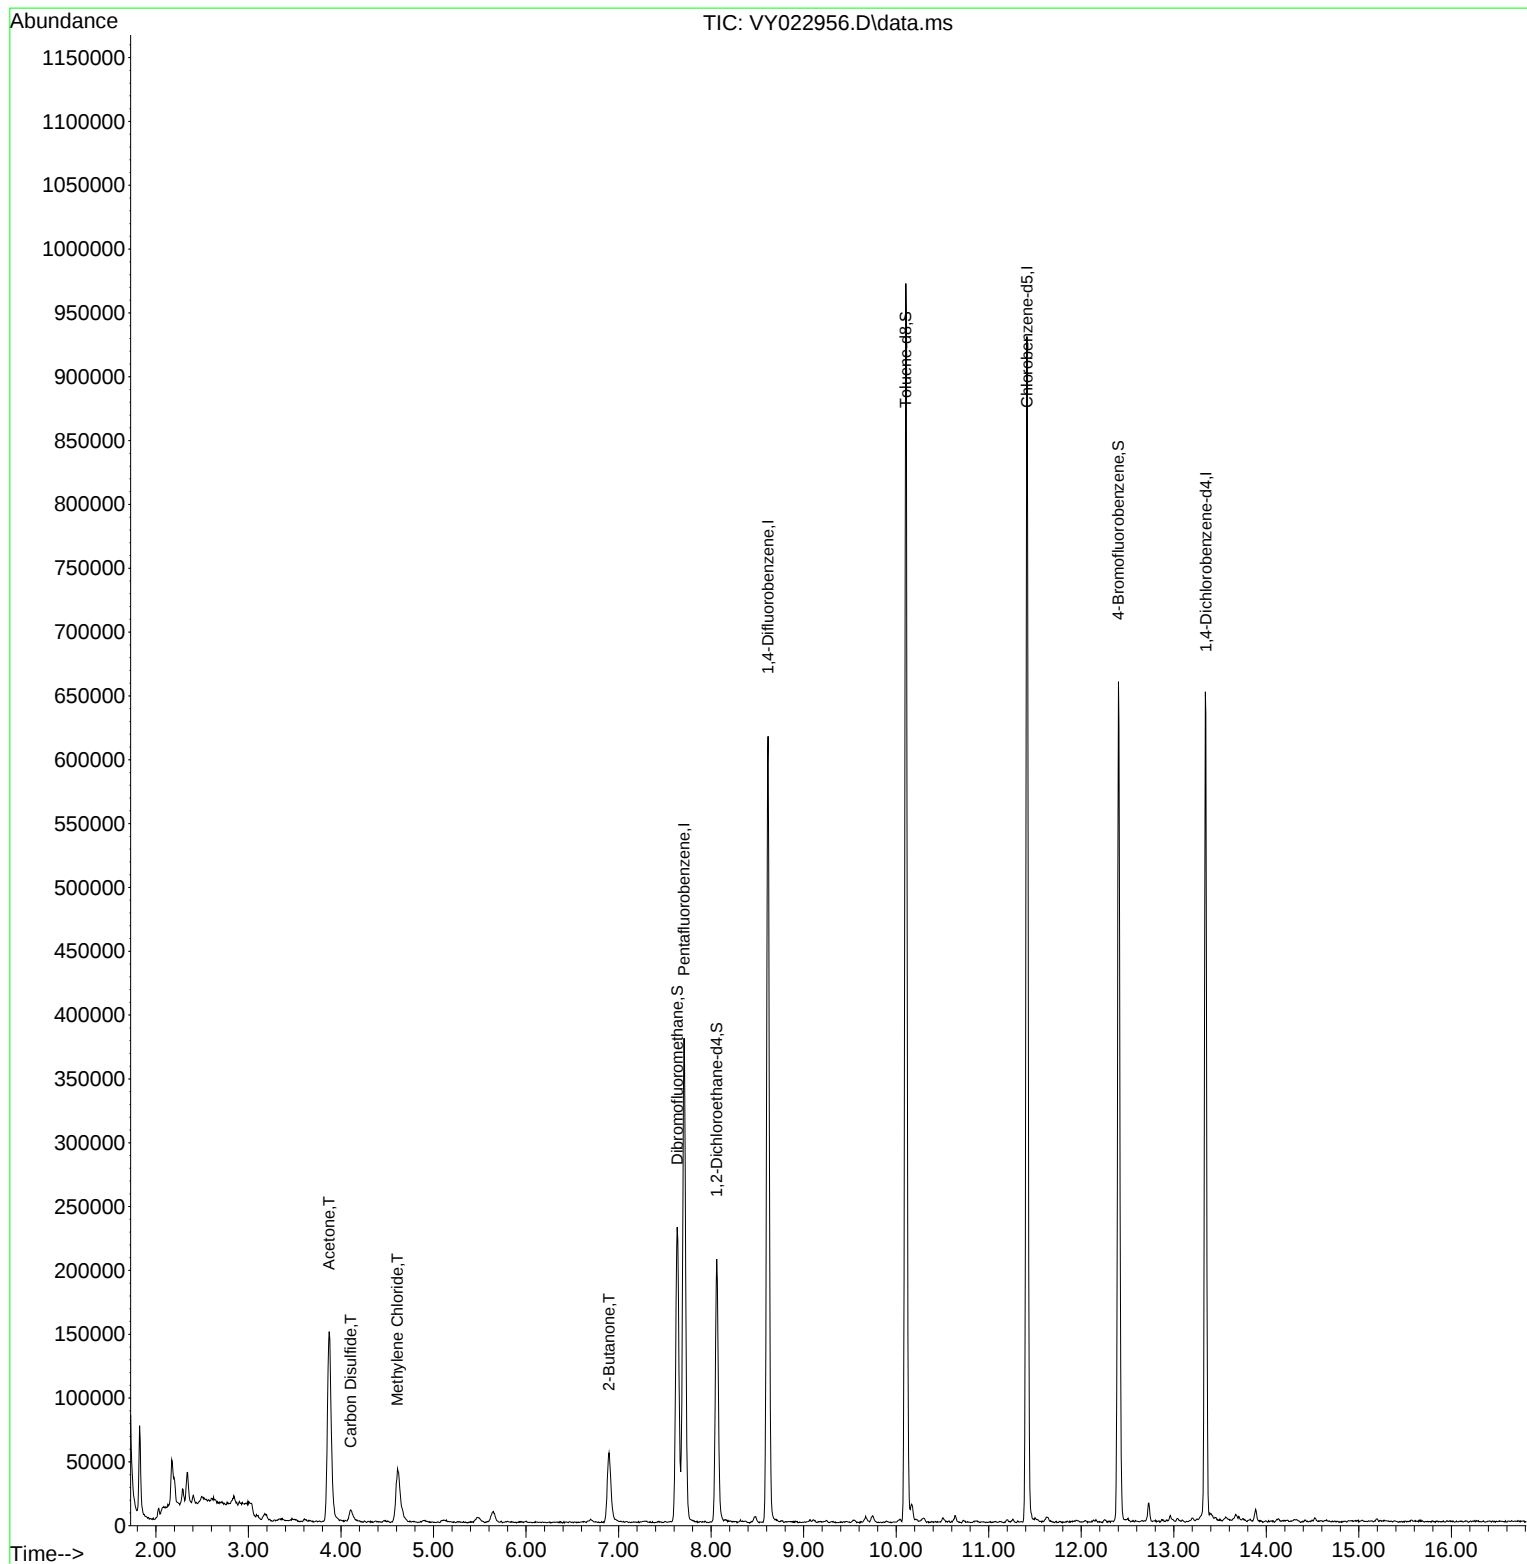


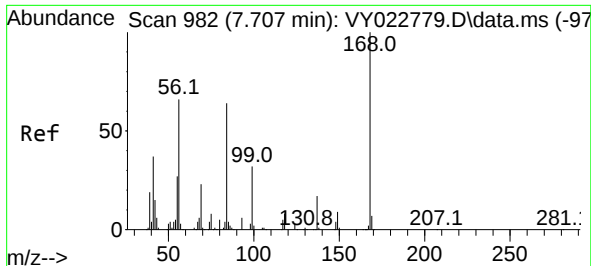

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38




Instrument :
MSVOA_Y
ClientSampleId :
G1(10)


Tgt Ion:168 Resp: 283210
Ion Ratio Lower Upper
168 100
99 56.4 44.3 66.5

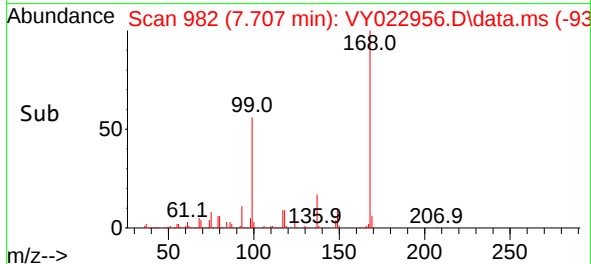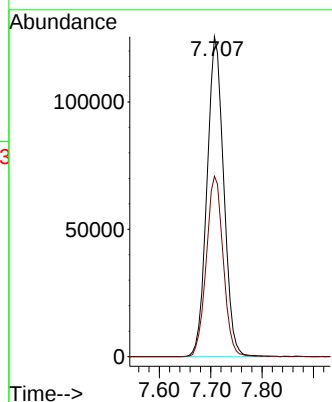

#16
Acetone
Concen: 459.574 ug/l
RT: 3.872 min Scan# 353
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38

Tgt Ion: 43 Resp: 274566
Ion Ratio Lower Upper
43 100
58 31.7 24.0 36.0


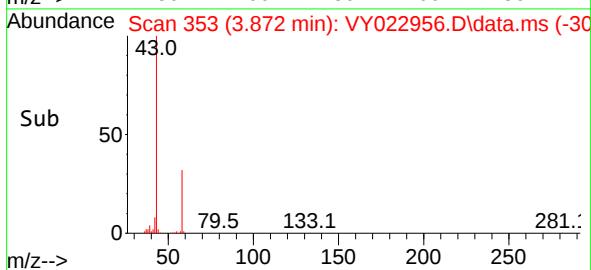
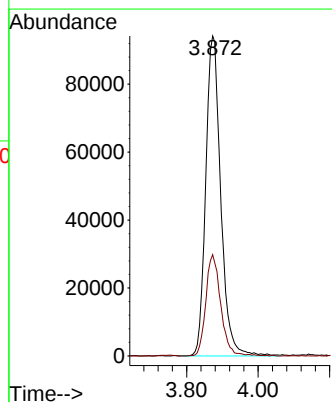
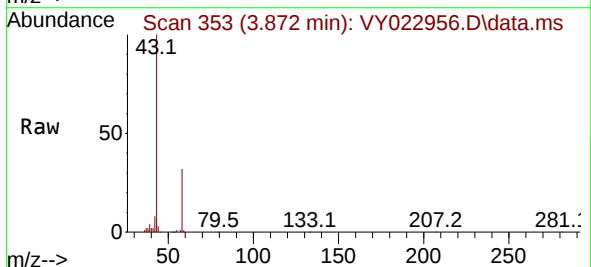


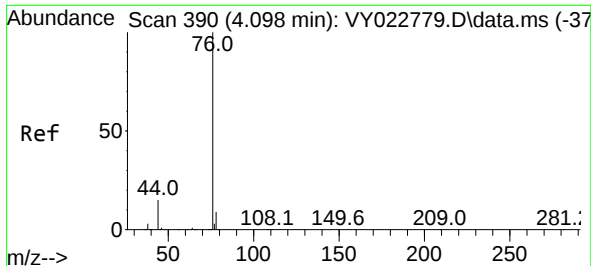

#17
Carbon Disulfide
Concen: 1.867 ug/l
RT: 4.104 min Scan# 391
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38




Instrument :
MSVOA_Y
ClientSampleId :
G1(10)


Tgt Ion: 76 Resp: 17293
Ion Ratio Lower Upper
76 100
78 8.6 7.4 11.2

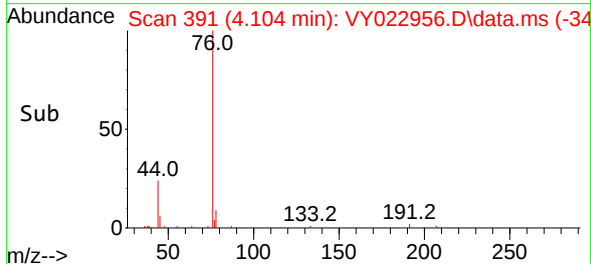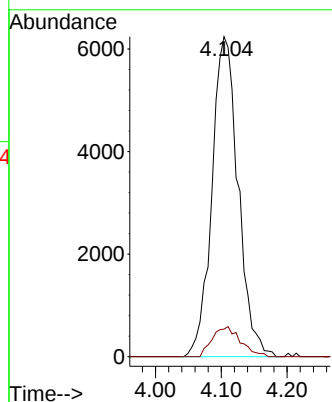

#20
Methylene Chloride
Concen: 7.828 ug/l
RT: 4.610 min Scan# 474
Delta R.T. -0.012 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38

Tgt Ion: 84 Resp: 29536
Ion Ratio Lower Upper
84 100
49 130.1 101.9 152.9
51 36.2 29.8 44.8
86 62.0 51.3 76.9


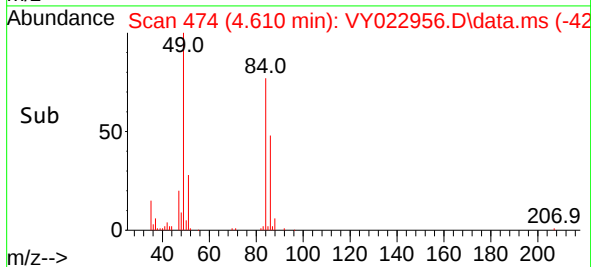
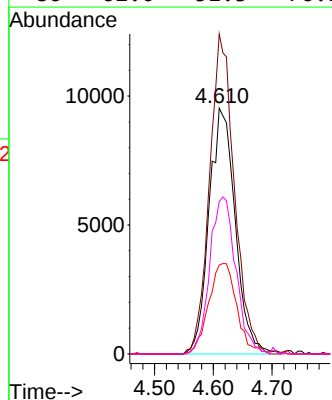
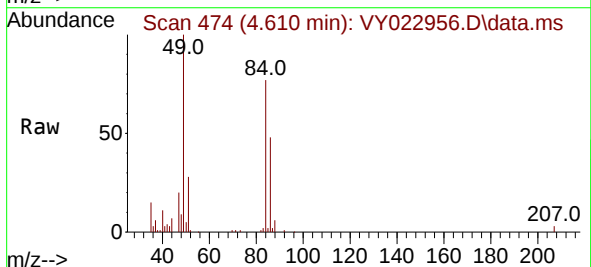


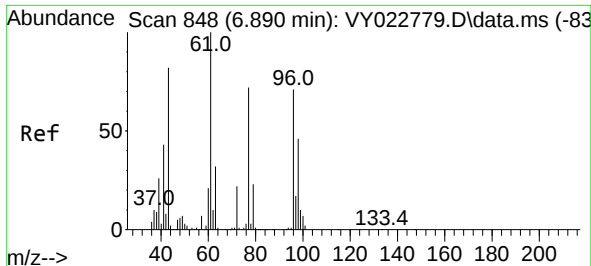

#25
2-Butanone
Concen: 107.401 ug/l
RT: 6.896 min Scan# 848
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38




Instrument :
MSVOA_Y
ClientSampleId :
G1(10)


Tgt Ion: 43 Resp: 93388
Ion Ratio Lower Upper
43 100
72 26.4 22.9 34.3

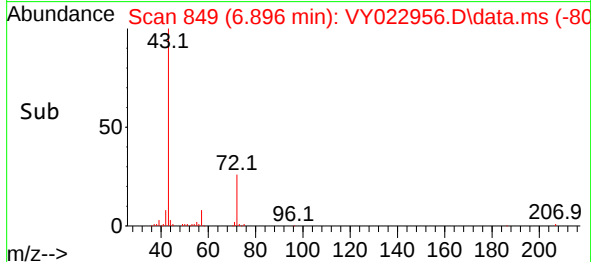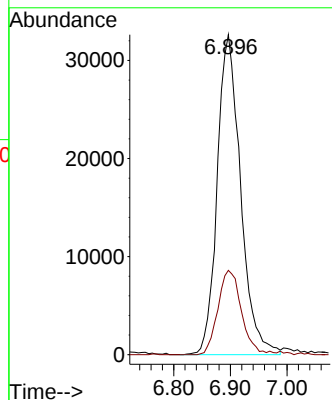

#33
1,2-Dichloroethane-d4
Concen: 51.609 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38

Tgt Ion: 65 Resp: 163131
Ion Ratio Lower Upper
65 100
67 51.7 0.0 103.4

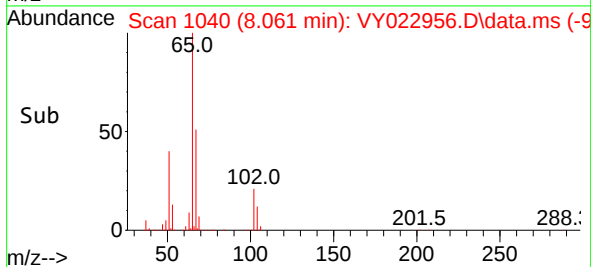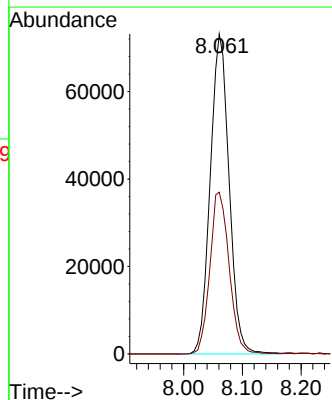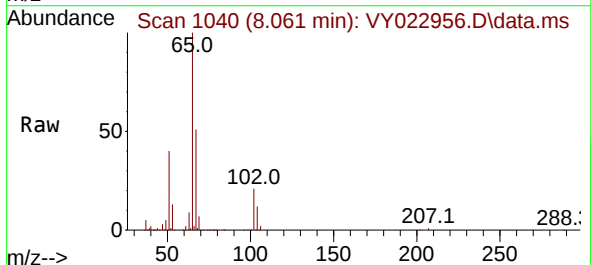

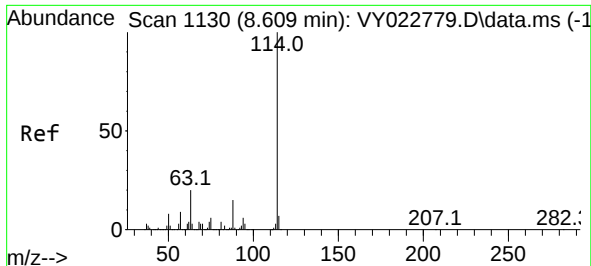

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.616 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY022956.D

Acq: 07 Jul 2025 13:38

Instrument :

MSVOA_Y

ClientSampleId :

G1(10)





Tgt Ion:114 Resp: 516435

Ion Ratio Lower Upper

114 100

63 19.6 0.0 40.8

88 14.6 0.0 27.8

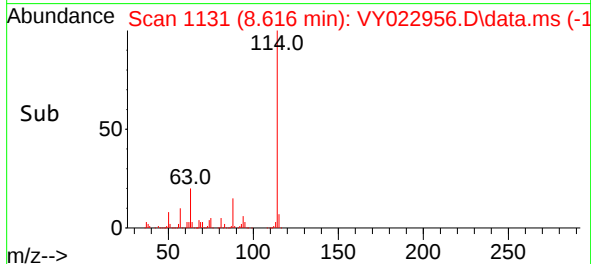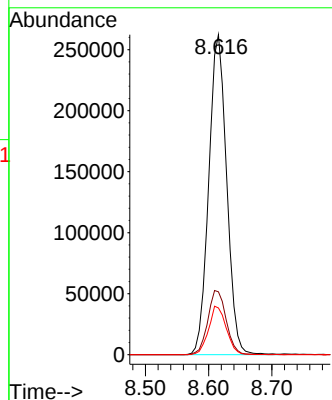

#35

Dibromofluoromethane

Concen: 53.559 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.006 min

Lab File: VY022956.D

Acq: 07 Jul 2025 13:38




Tgt Ion:113 Resp: 168212


Ion Ratio Lower Upper

113 100

111 102.8 81.1 121.7

192 19.1 14.2 21.2


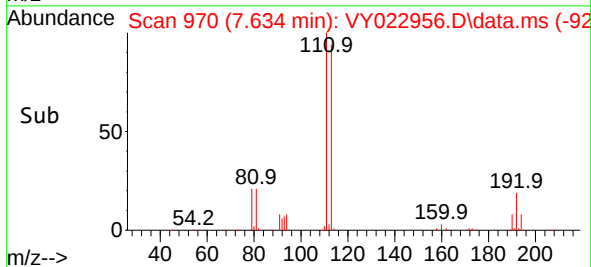
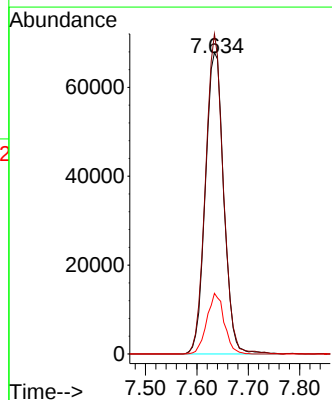
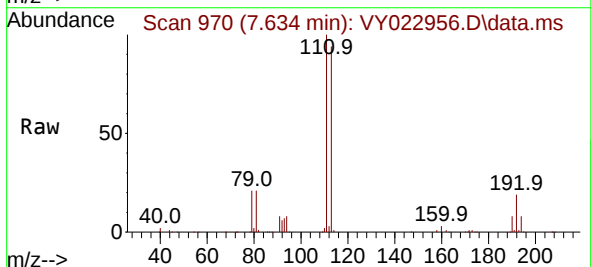


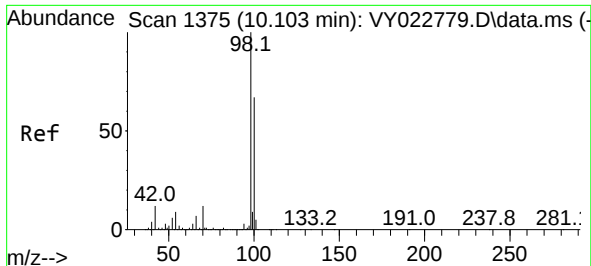

#50
Toluene-d8
Concen: 49.903 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38




Instrument :
MSVOA_Y
ClientSampleId :
G1(10)


Tgt Ion: 98 Resp: 621930
Ion Ratio Lower Upper
98 100
100 65.7 51.4 77.0

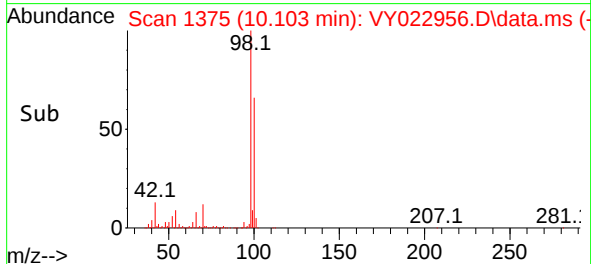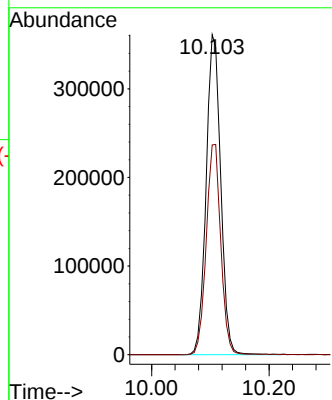

#62
4-Bromofluorobenzene
Concen: 45.494 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38

Tgt Ion: 95 Resp: 182265
Ion Ratio Lower Upper
95 100
174 83.5 0.0 170.0
176 79.5 0.0 166.2


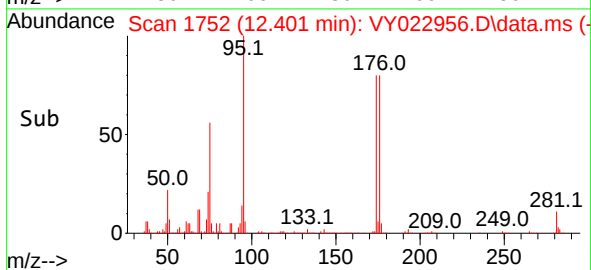
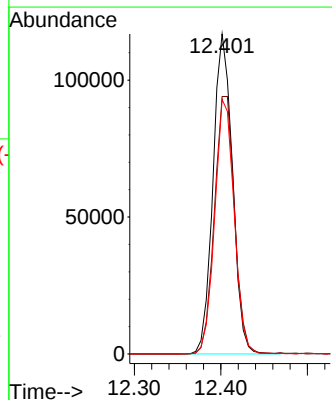
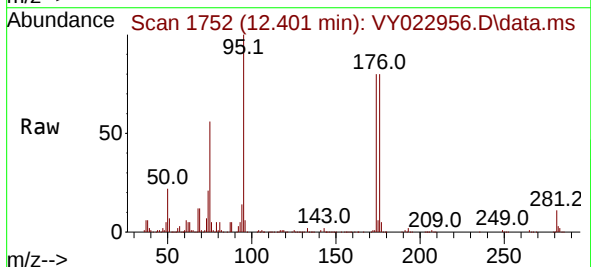


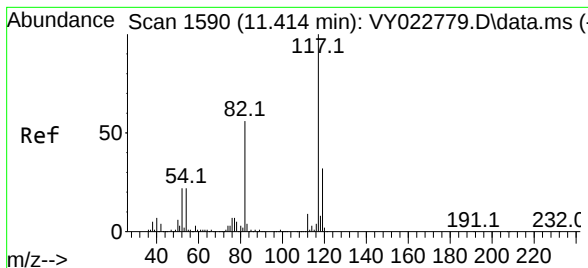

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38

Instrument :
MSVOA_Y
ClientSampleId :
G1(10)

Tgt Ion:117 Resp: 471025
Ion Ratio Lower Upper
117 100
82 57.5 44.6 66.8
119 30.9 25.4 38.0

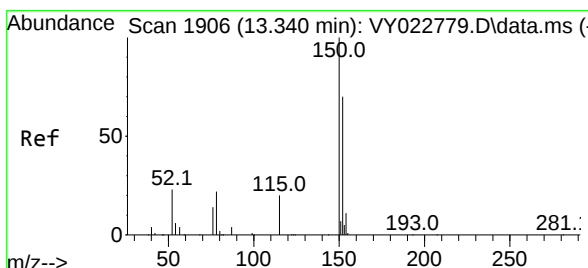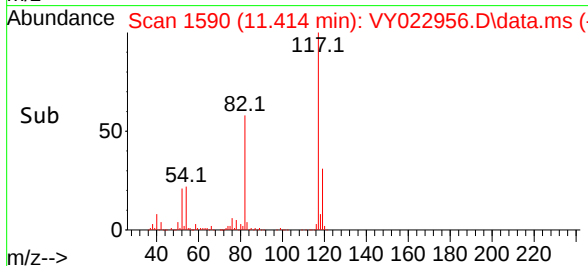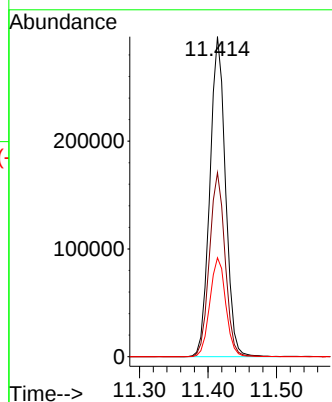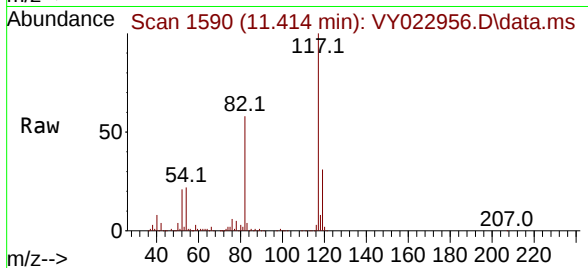

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY022956.D
Acq: 07 Jul 2025 13:38

Tgt Ion:152 Resp: 158953
Ion Ratio Lower Upper
152 100
115 58.7 28.9 86.7
150 158.6 0.0 349.6

