
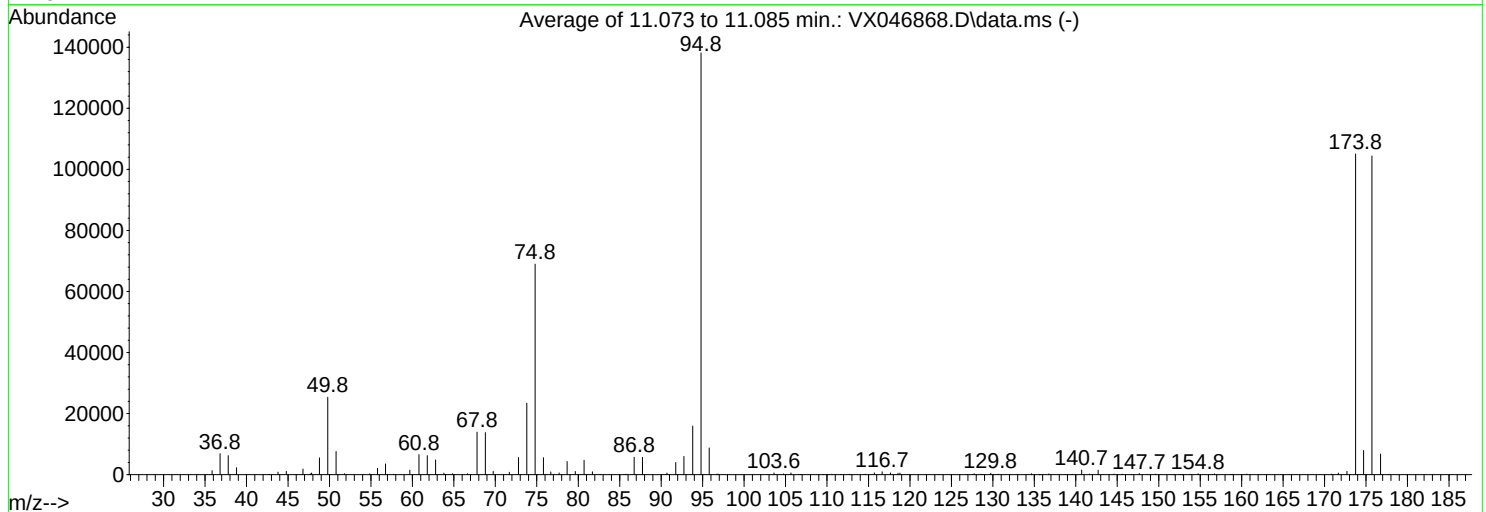


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX070325\  
Data File : VX046868.D  
Acq On : 03 Jul 2025 07:52  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X070225W.M  
Title : SW846 8260  
Last Update : Thu Jul 03 05:51:11 2025

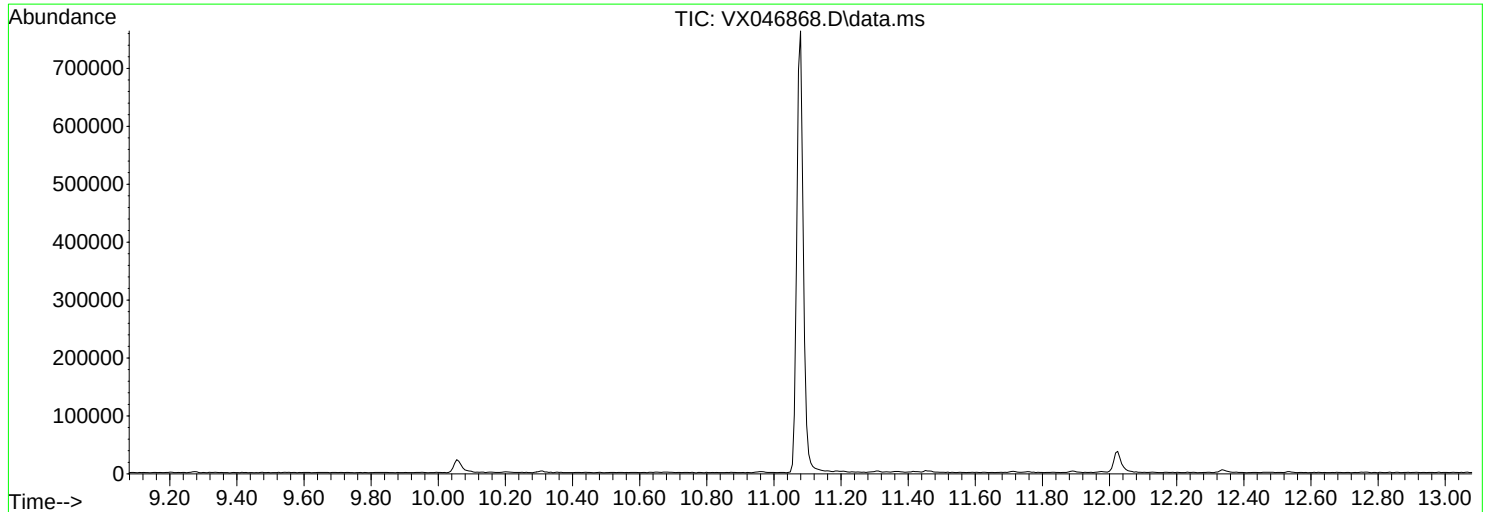

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.4         | 25355      | PASS                |
| 75             | 95              | 30              | 60              | 49.9         | 68992      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 138160     | PASS                |
| 96             | 95              | 5               | 9               | 6.3          | 8736       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.0          | 1090       | PASS                |
| 174            | 95              | 50              | 100             | 76.0         | 105016     | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 7936       | PASS                |
| 176            | 174             | 95              | 101             | 99.4         | 104379     | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 6758       | PASS                |