


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061925\
Data File : BF142787.D
Acq On : 19 Jun 2025 16:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 20 05:06:14 2025

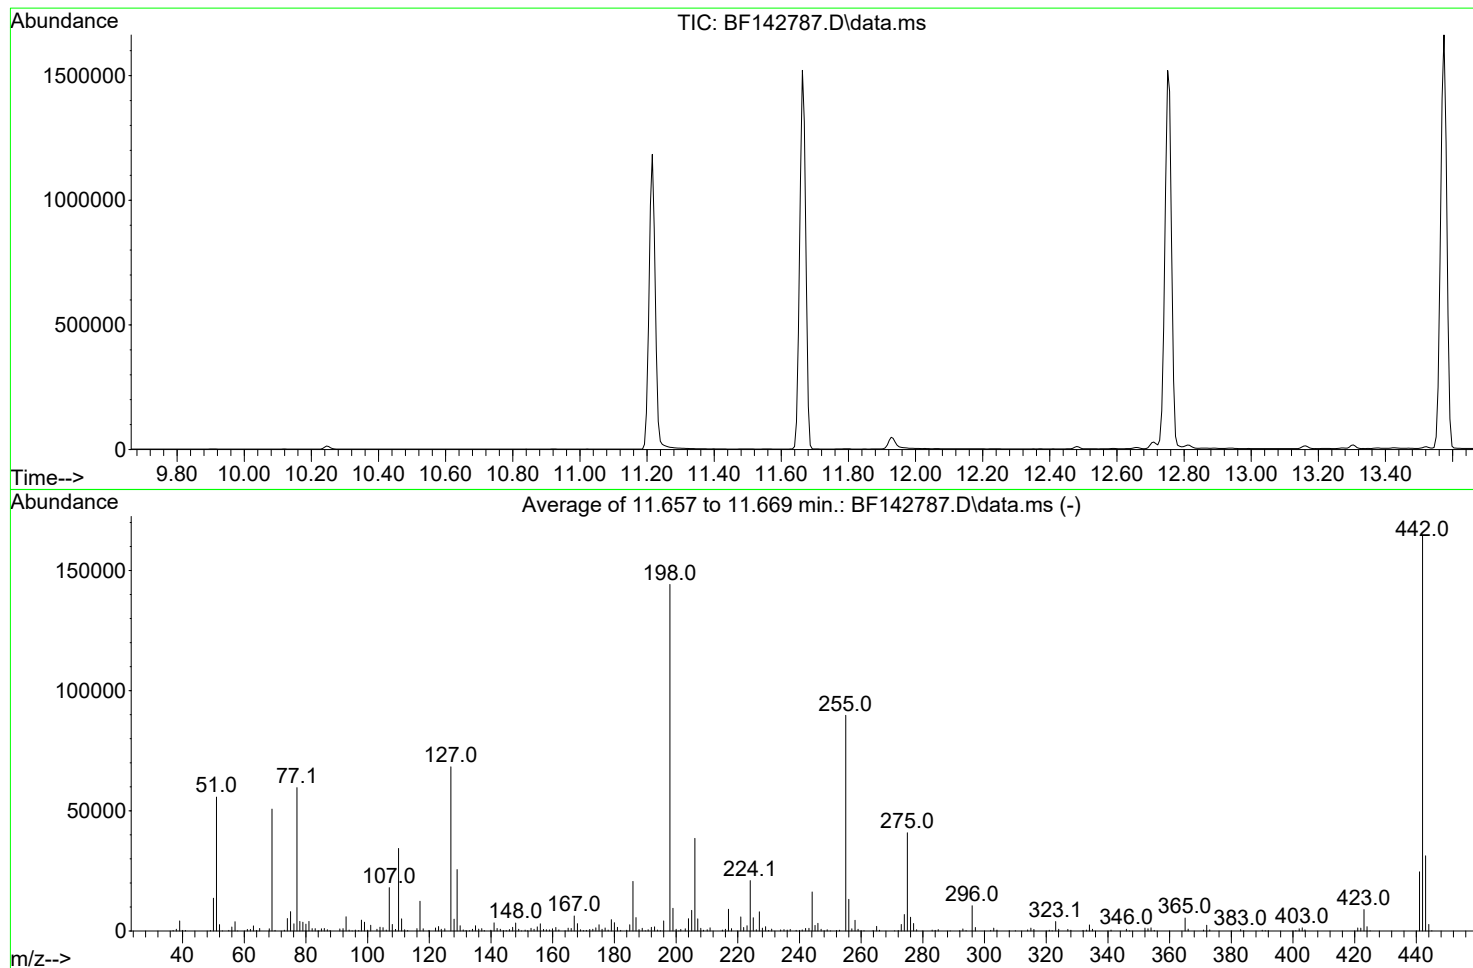

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	926	PASS
69	69	100	100	100.0	50712	PASS
70	69	0.00	2	0.5	243	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144192	PASS
199	198	5	9	6.6	9464	PASS
365	198	1	100	3.7	5372	PASS
441	443	0.01	150	78.8	24649	PASS
442	442	100	100	100.0	164283	PASS
443	442	15	24	19.1	31296	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/19/2025	BNA_F	<u>BF142787.D</u>
Compound Name	Response	Retention Time
DDT	429715	13.574
DDD	7712	13.304
DDE	717	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8429	438144	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061925\
Data File : BF142787.D
Acq On : 19 Jun 2025 16:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 20 05:38:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 20 05:06:14 2025
Response via : Initial Calibration

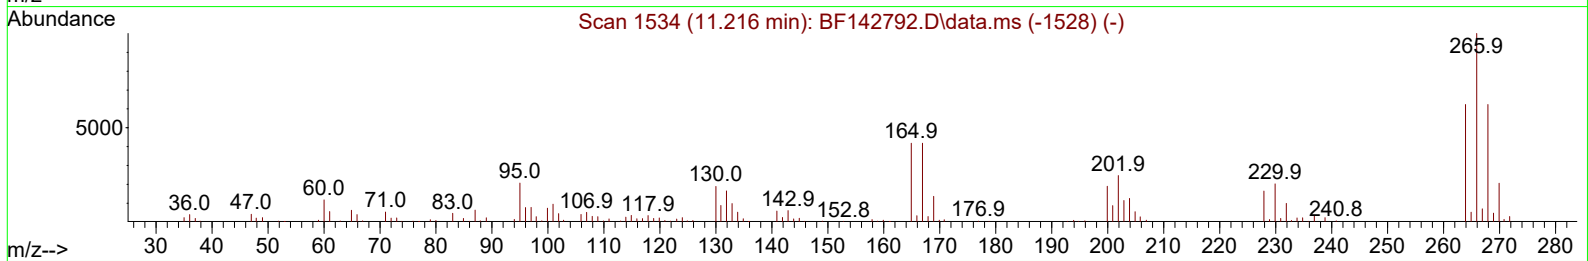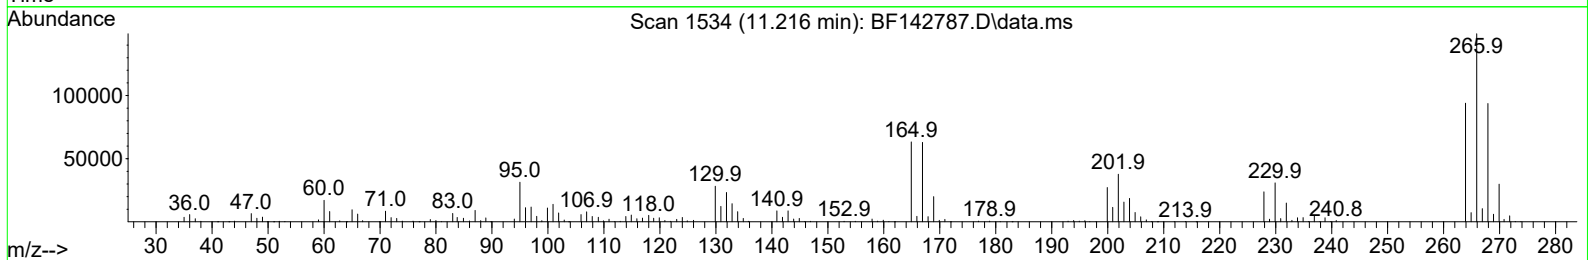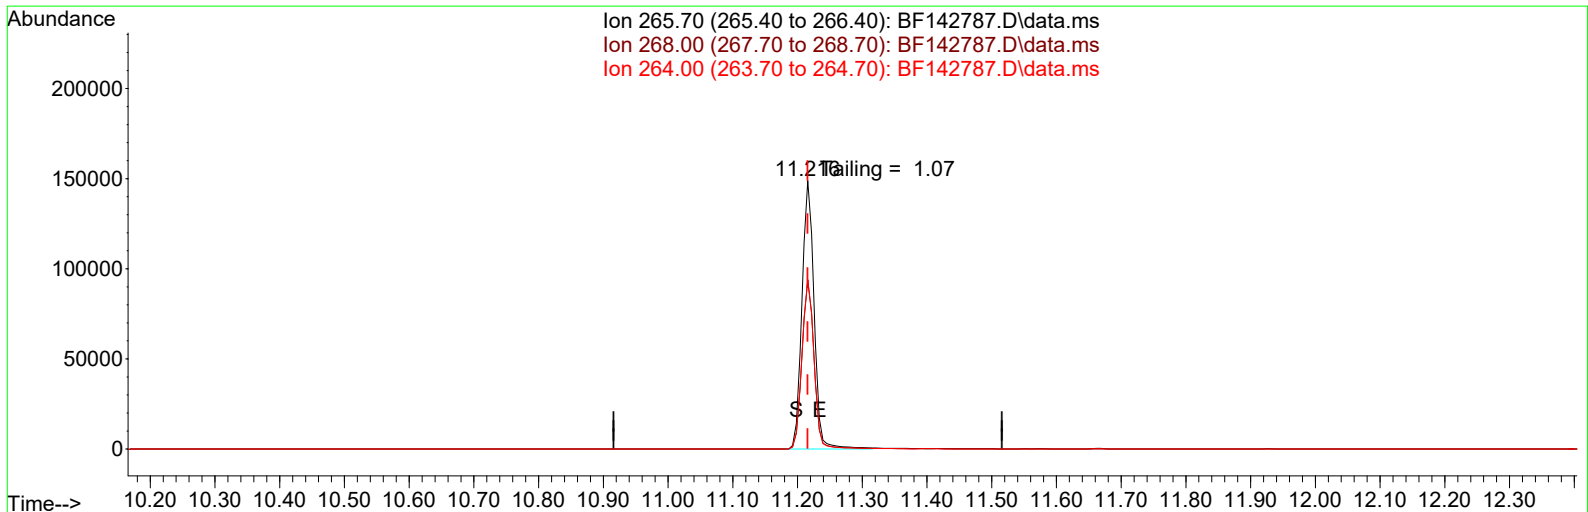

TIC: BF142787.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 37164.56 ng




response 195787

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.94
264.00	62.40	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061925\
Data File : BF142787.D
Acq On : 19 Jun 2025 16:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 20 05:38:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 20 05:06:14 2025
Response via : Initial Calibration

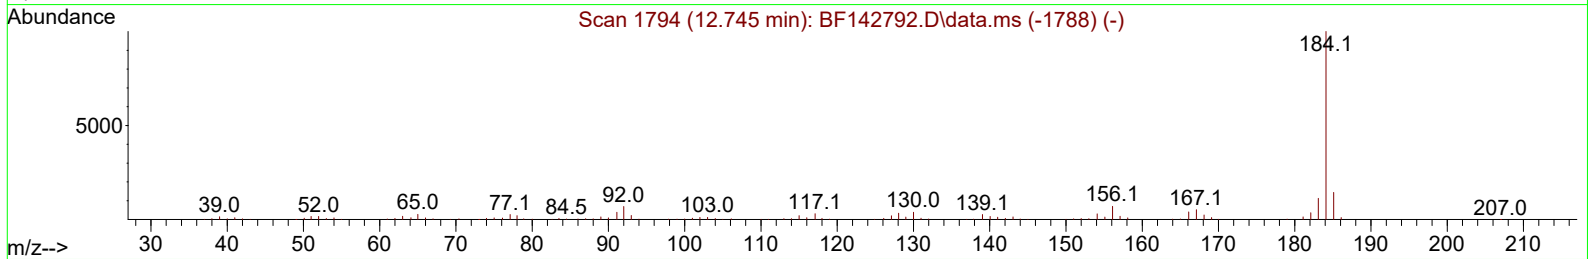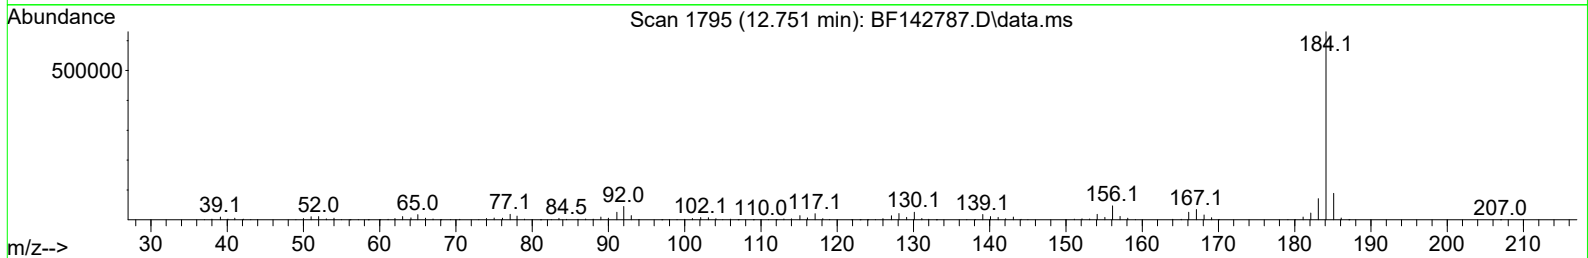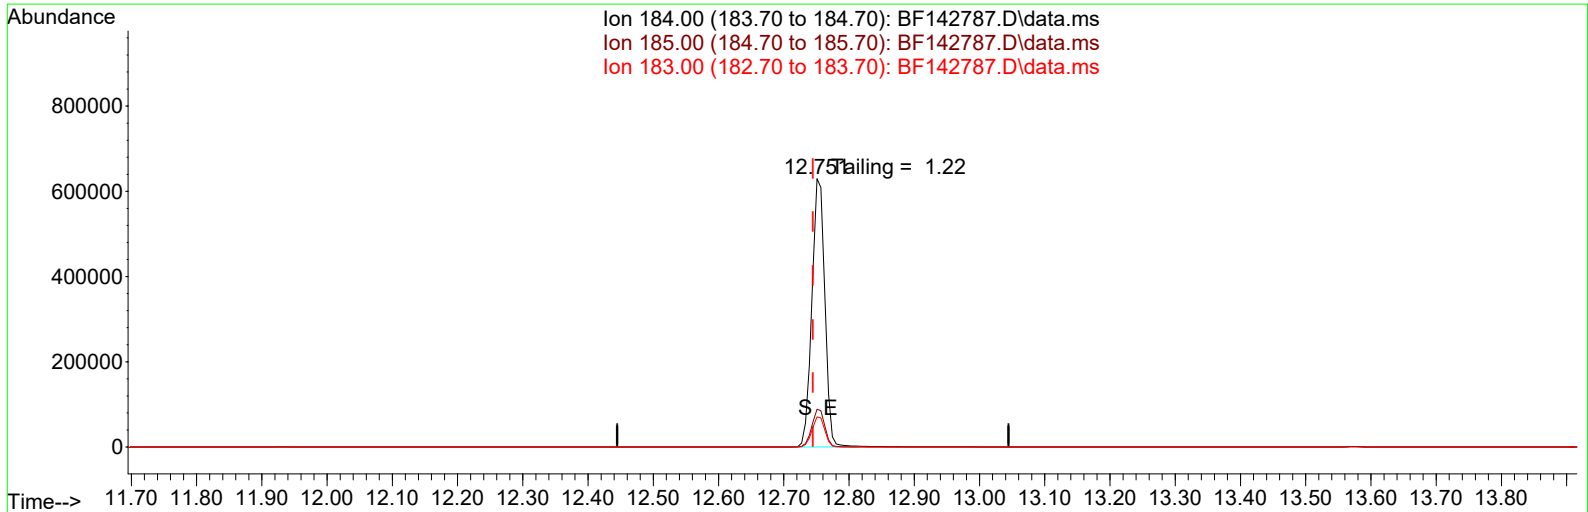

TIC: BF142787.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 874127

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.11
183.00	11.20	11.25
0.00	0.00	0.00