


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070825\
Data File : BF143024.D
Acq On : 08 Jul 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 24 05:28:21 2025

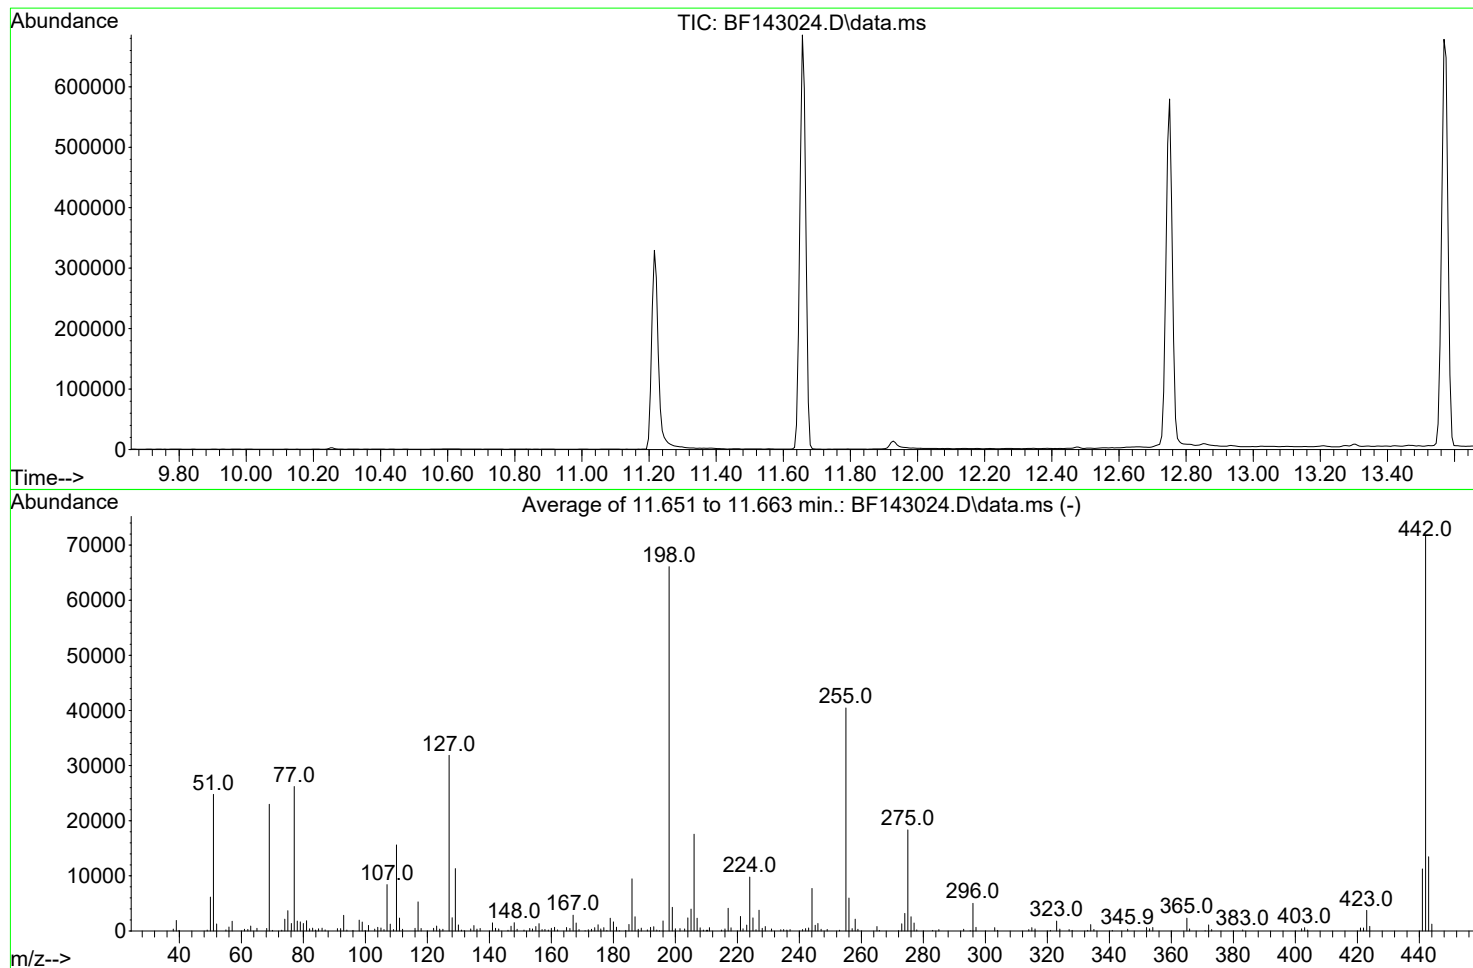

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	457	PASS
69	69	100	100	100.0	22973	PASS
70	69	0.00	2	0.5	123	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66072	PASS
199	198	5	9	6.5	4287	PASS
365	198	1	100	3.5	2336	PASS
441	443	0.01	150	83.6	11262	PASS
442	442	100	100	100.0	71613	PASS
443	442	15	24	18.8	13467	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/8/2025	BNA_F	<u>BF143024.D</u>
Compound Name	Response	Retention Time
DDT	179865	13.568
DDD	3904	13.298
DDE	604	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4508	184373	2.45

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070825\
Data File : BF143024.D
Acq On : 08 Jul 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 08 11:36:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

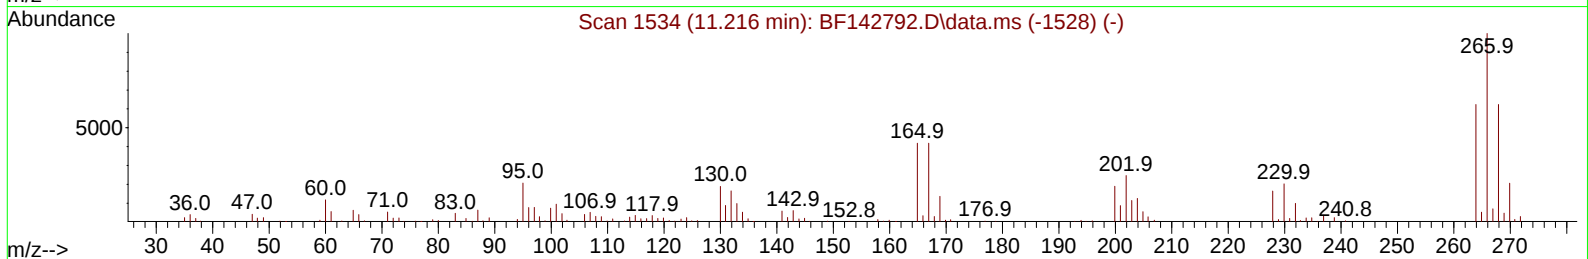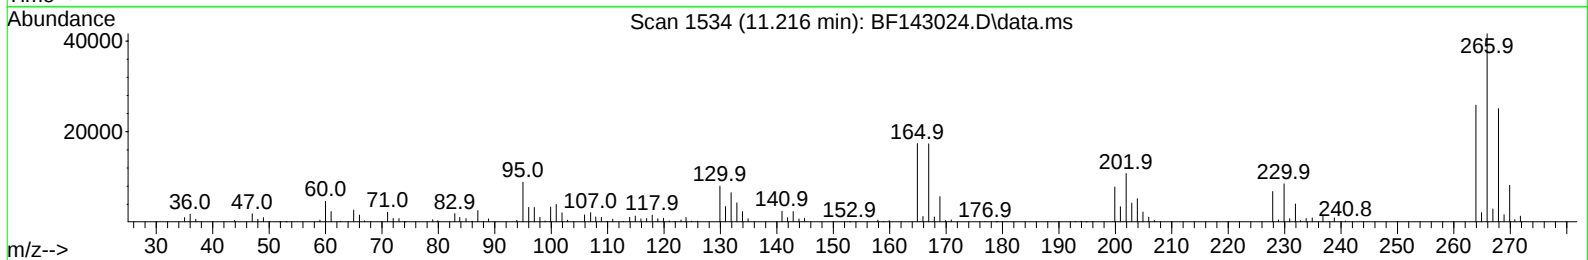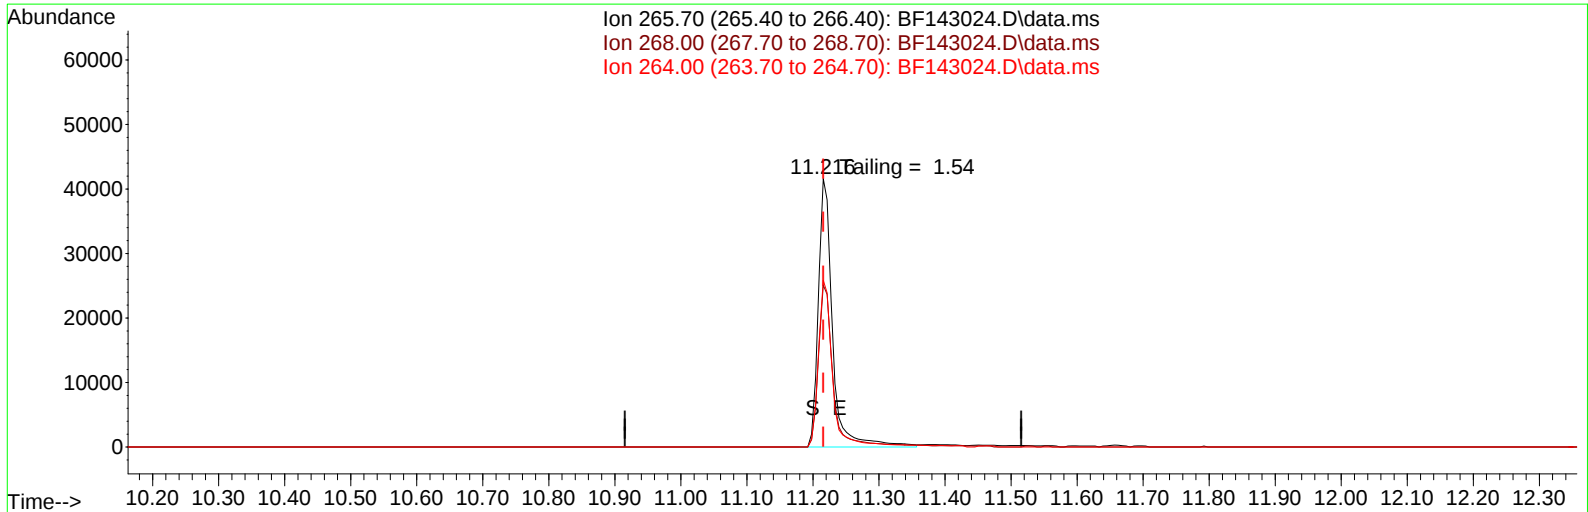

TIC: BF143024.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 28385.23 ng




response 62605

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	60.35
264.00	62.40	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070825\
Data File : BF143024.D
Acq On : 08 Jul 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 08 11:36:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

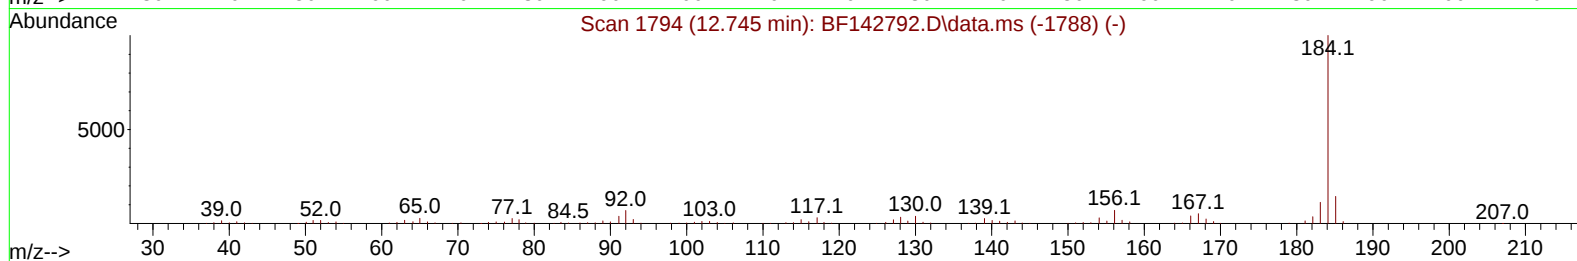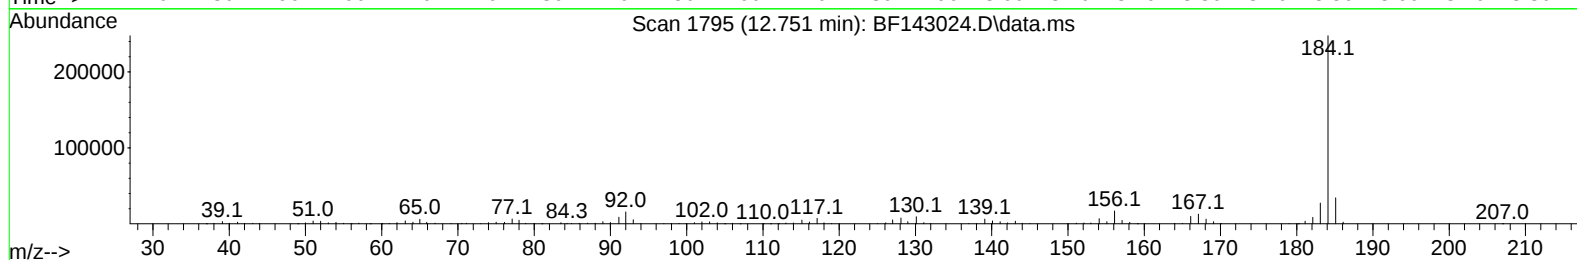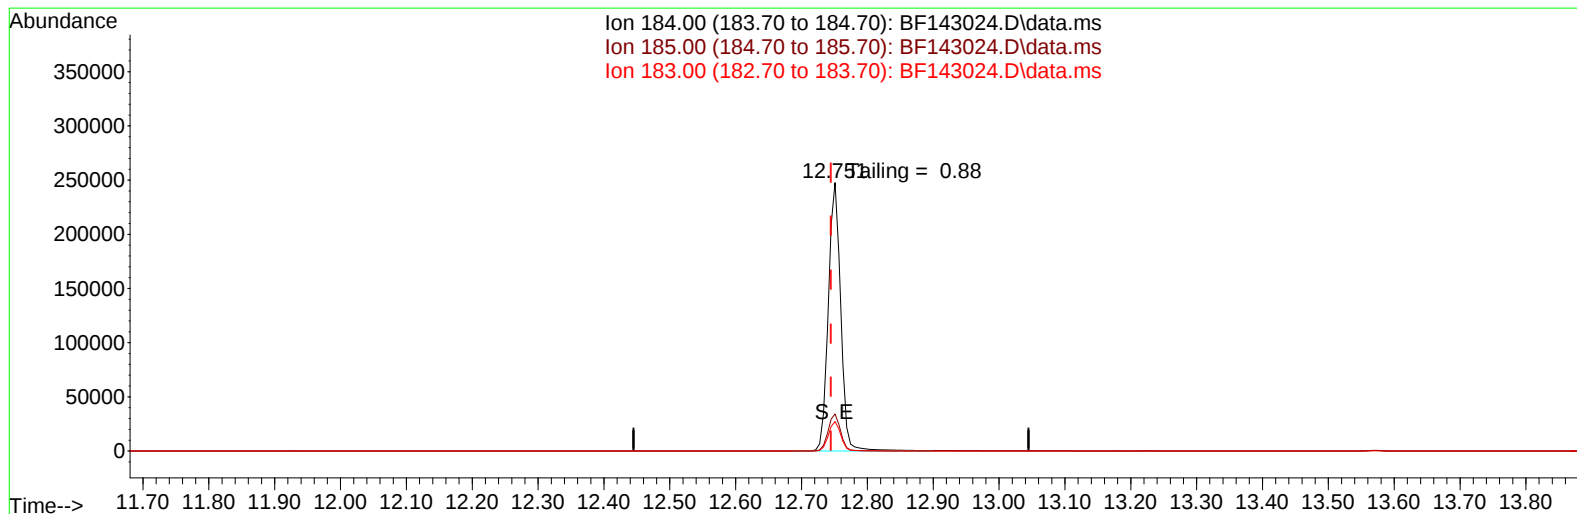

TIC: BF143024.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 0.00 ng

response 326123

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.81
183.00	11.20	11.00
0.00	0.00	0.00