
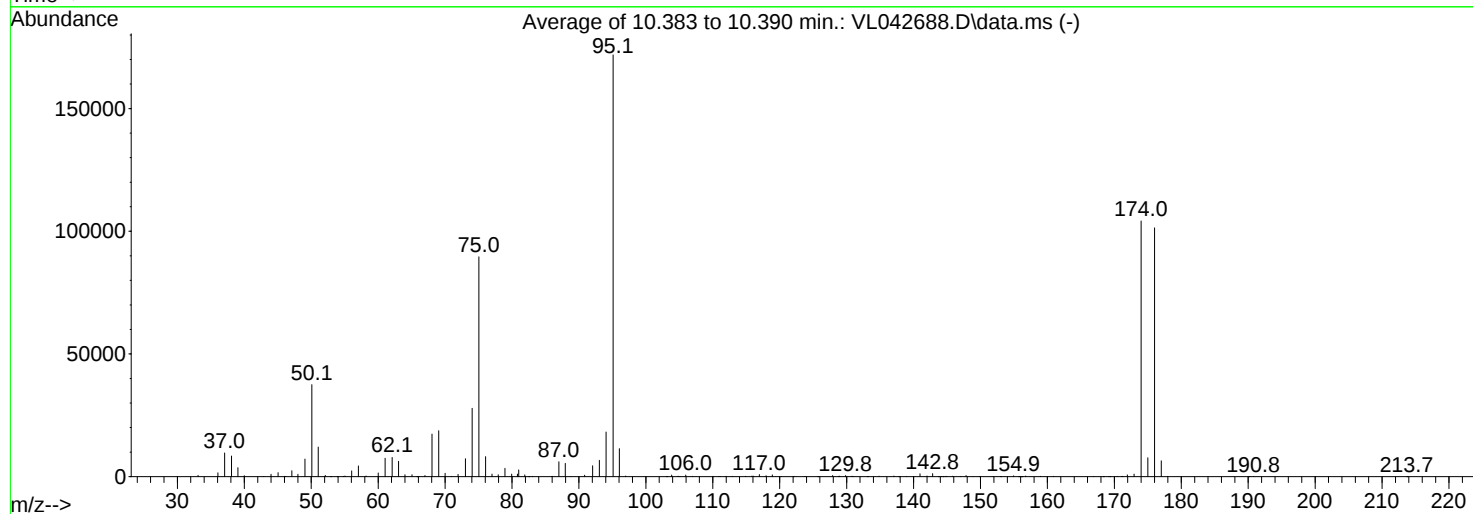


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070225\
Data File : VL042688.D
Acq On : 02 Jul 2025 07:41
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL070225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 03 01:50:16 2025

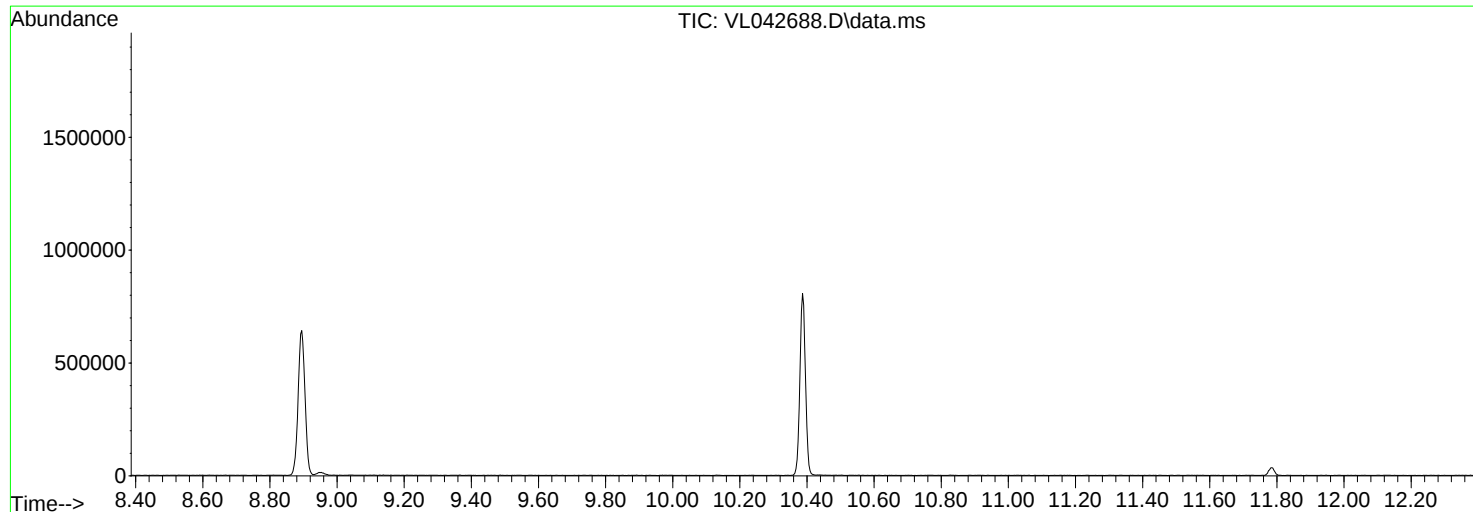

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3168

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	21.8	37520	PASS
75	95	30	66	52.1	89627	PASS
95	95	100	100	100.0	171904	PASS
96	95	5	9	6.6	11430	PASS
173	174	0.00	2	1.0	1048	PASS
174	95	50	120	60.6	104181	PASS
175	174	4	9	7.4	7723	PASS
176	174	93	101	97.3	101413	PASS
177	176	5	9	6.4	6441	PASS

Average of 10.383 to 10.390 min.: VL042688.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	545	47.10	2394	57.05	4387	68.05	1737
36.05	1593	48.00	1000	58.20	236	69.05	1874
37.05	9629	49.05	7197	60.00	1477	70.00	139
38.10	8434	50.10	37520	61.05	7520	70.95	6
39.05	3662	51.05	12063	62.10	7834	71.95	897
40.00	422	52.10	545	63.05	6255	73.05	7333
42.90	92	52.90	28	64.00	794	74.05	27877
44.00	1007	53.90	20	65.05	761	75.05	89627
45.05	1636	54.80	129	65.80	23	76.05	8161
46.00	109	55.05	251	66.10	109	77.00	1034
46.20	60	56.05	2352	67.00	432	77.95	811

Average of 10.383 to 10.390 min.: VL042688.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	3415	88.80	51	105.10	83	116.95	852
79.95	1040	90.85	567	105.95	682	117.95	394
80.80	1024	92.05	4447	106.95	140	118.90	719
81.00	2735	93.05	6669	110.05	104	120.20	40
81.90	750	94.05	18203	110.90	73	122.00	19
82.50	32	95.10	171904	111.10	52	123.80	133
83.05	152	96.05	11430	111.95	134	125.70	17
85.90	62	97.00	273	112.90	105	127.90	466
86.00	151	103.10	27	114.90	120	128.80	115
87.00	6093	103.85	635	115.85	285	128.95	196
87.95	5423	104.80	211	116.10	180	129.85	475

Average of 10.383 to 10.390 min.: VL042688.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.80	186	143.70	26	153.00	23	169.30	39
131.00	97	144.20	57	154.95	339	170.40	115
133.10	27	144.40	17	155.70	25	171.10	62
134.85	213	144.80	52	156.00	33	171.25	167
137.05	244	144.95	109	156.20	22	171.95	725
137.80	21	145.85	227	156.75	246	172.95	1048
138.95	61	147.00	41	158.95	146	174.00	104181
140.00	88	147.85	484	160.90	144	175.00	7723
140.95	1206	148.90	76	166.90	48	176.00	101413
142.00	286	149.80	94	168.35	39	177.00	6441
142.85	1272	151.90	58	169.10	78	177.95	167

Average of 10.383 to 10.390 min.: VL042688.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
190.10	25						
190.80	53						
213.70	18						

Instrument :

MSVOA_L

ClientSampleId :

BFB