


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050387.D
Acq On : 10 Jul 2025 13:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 08 18:32:25 2025

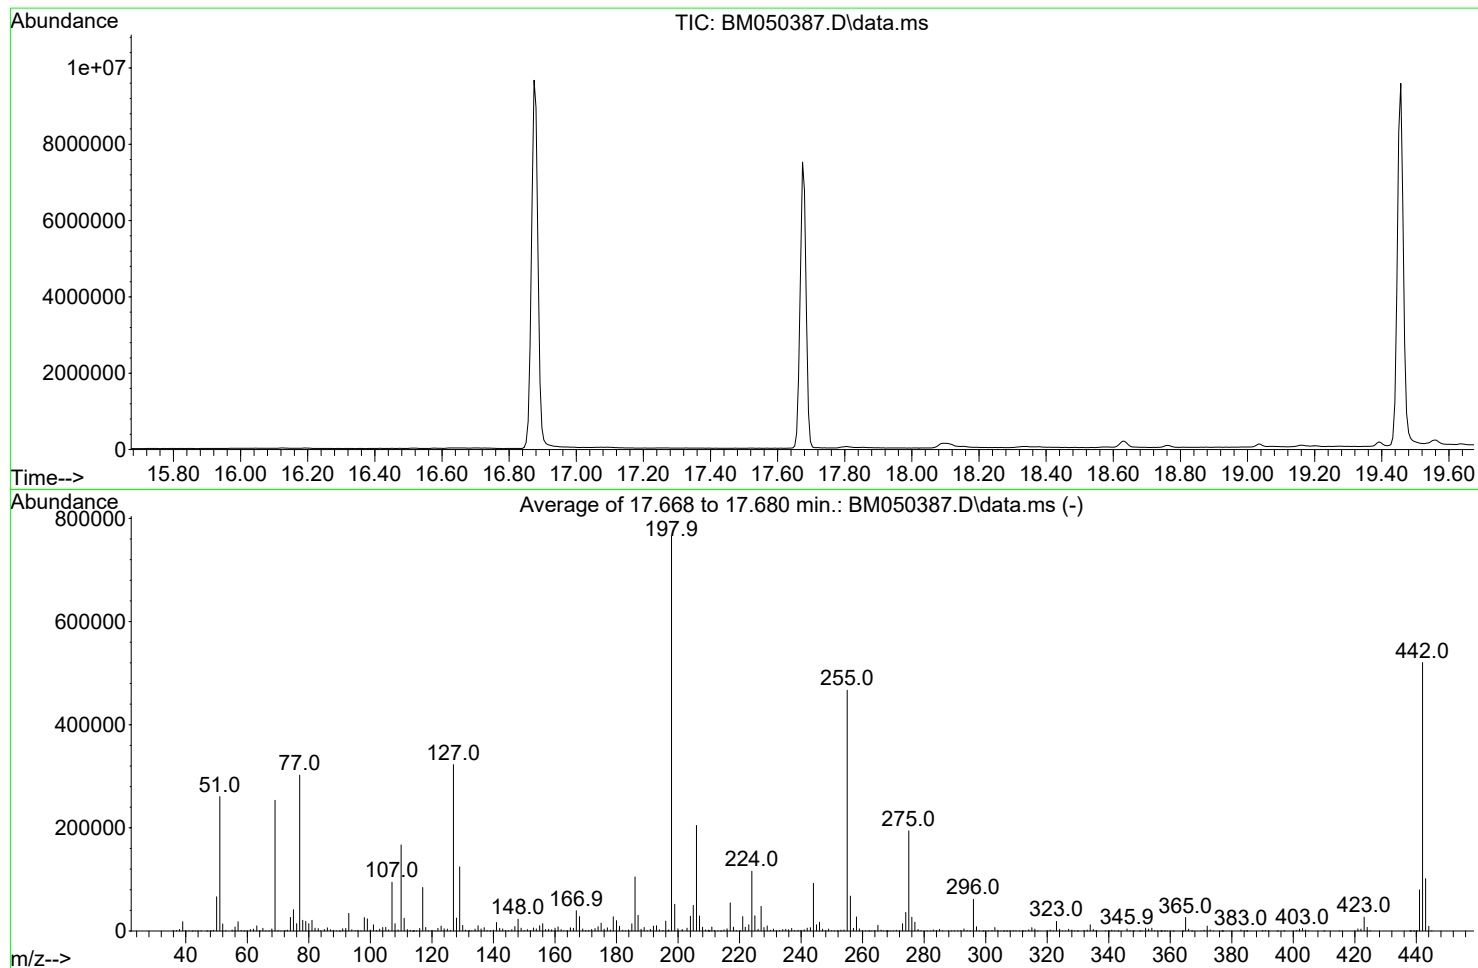

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	3907	PASS
69	69	100	100	100.0	253638	PASS
70	69	0.00	2	0.6	1422	PASS
197	198	0.00	2	0.3	2191	PASS
198	198	100	100	100.0	765568	PASS
199	198	5	9	6.8	51856	PASS
365	198	1	100	3.4	26267	PASS
441	443	0.01	150	78.8	79867	PASS
442	442	100	100	100.0	520619	PASS
443	442	15	24	19.5	101363	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/10/2025	BNA_M	<u>BM050387.D</u>
Compound Name	Response	Retention Time
DDT	2346830	20.692
DDD	18238	20.309
DDE	1010	19.756
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19248	2366078	0.81

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050387.D
Acq On : 10 Jul 2025 13:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 10 14:36:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

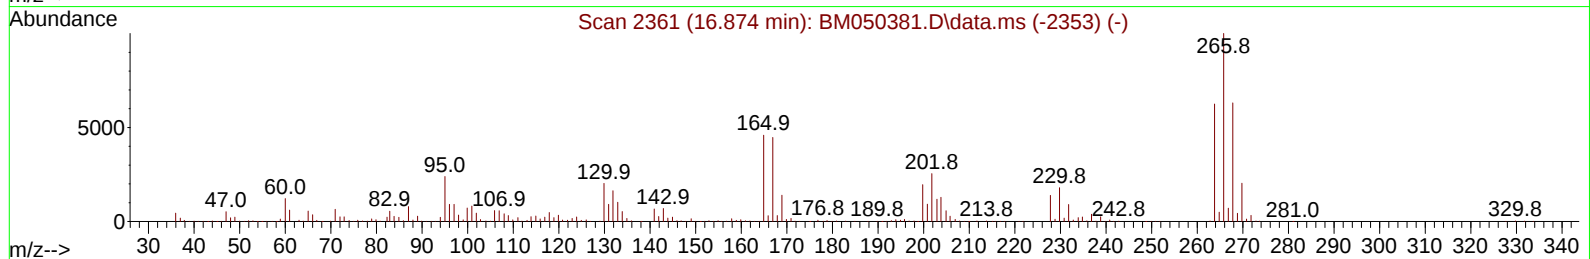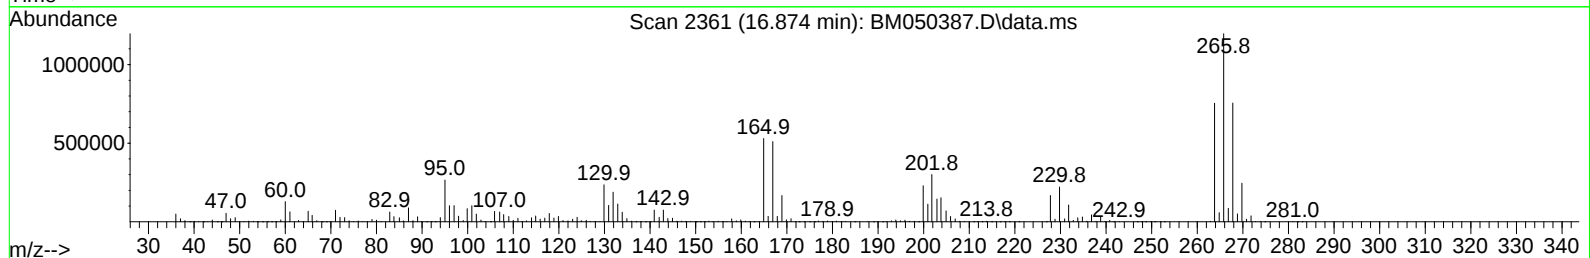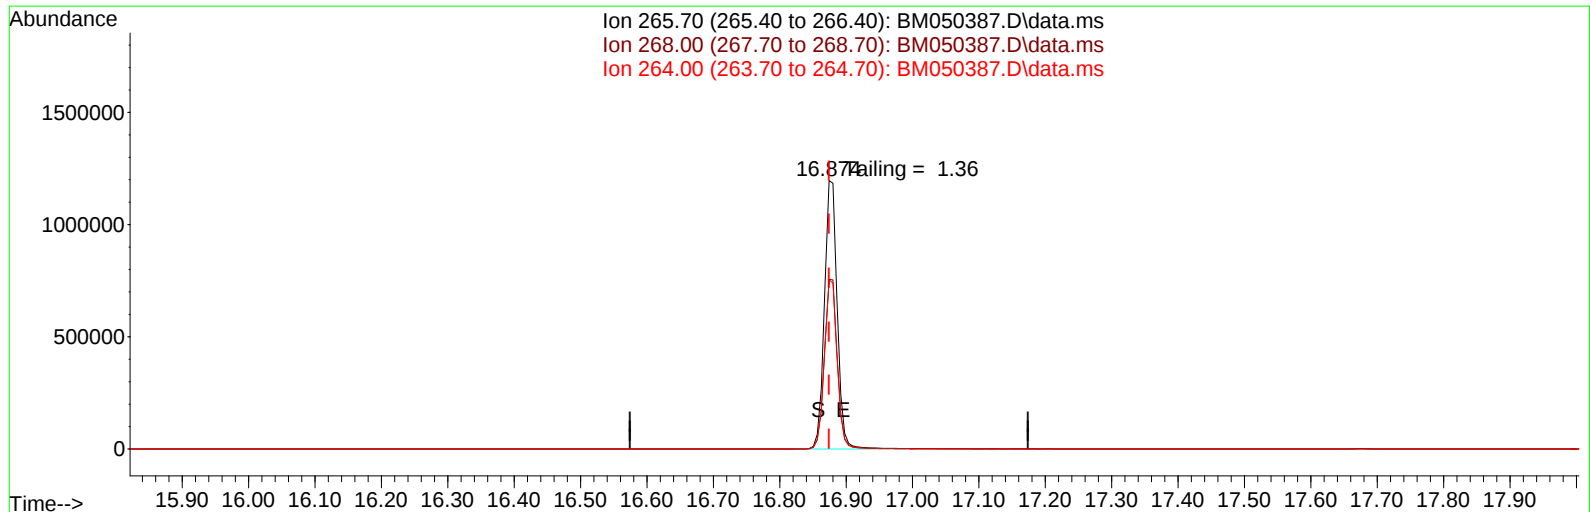

TIC: BM050387.D\data.ms

(70) Pentachlorophenol (C)

16.874min (+ 0.000) 1991582.93 ng




response 1613299

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.20
264.00	62.40	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071025\
Data File : BM050387.D
Acq On : 10 Jul 2025 13:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 10 14:36:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

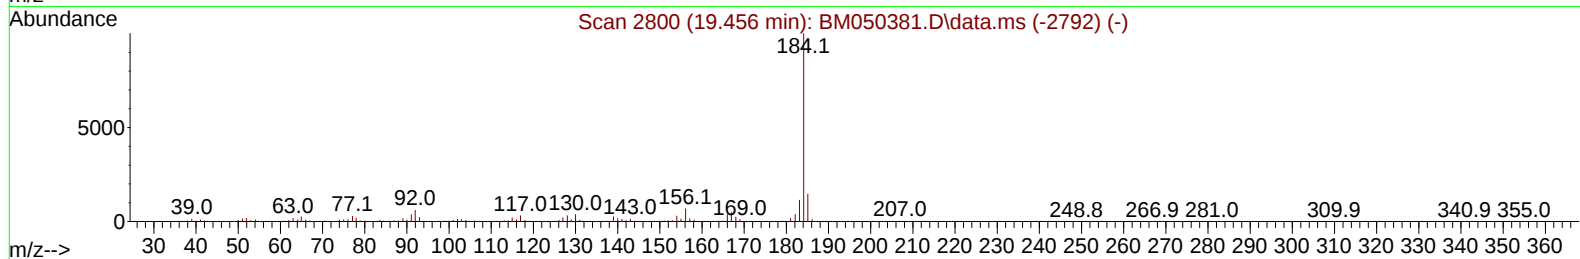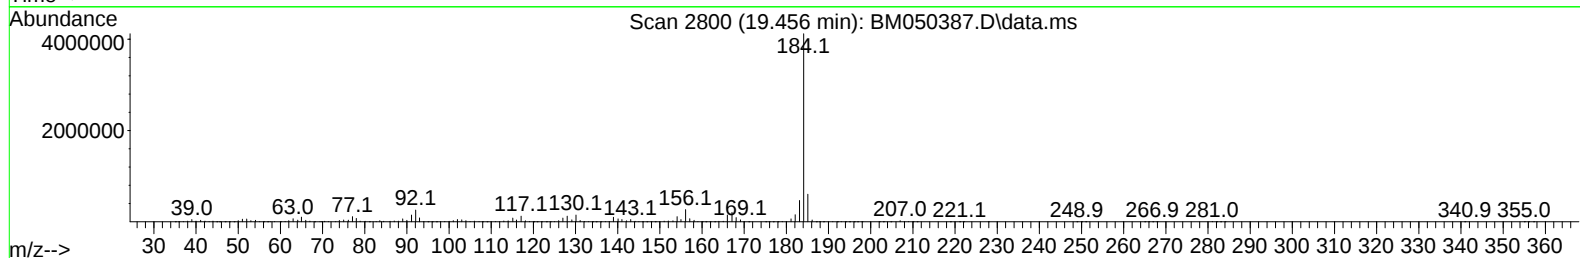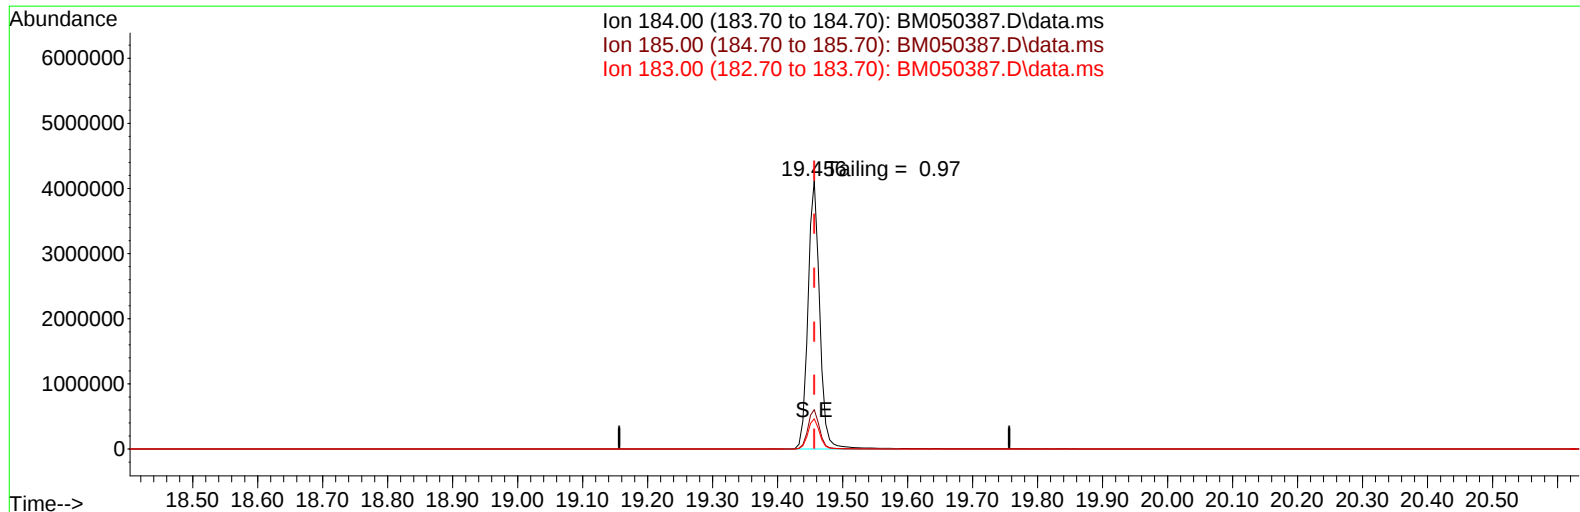

TIC: BM050387.D\data.ms

(77) Benzidine

19.456min (+ 0.000) 4529.57 ng

response 5211463

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.67
183.00	11.30	11.30
0.00	0.00	0.00