


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025154.D
Acq On : 16 Jul 2025 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 03 16:05:44 2025

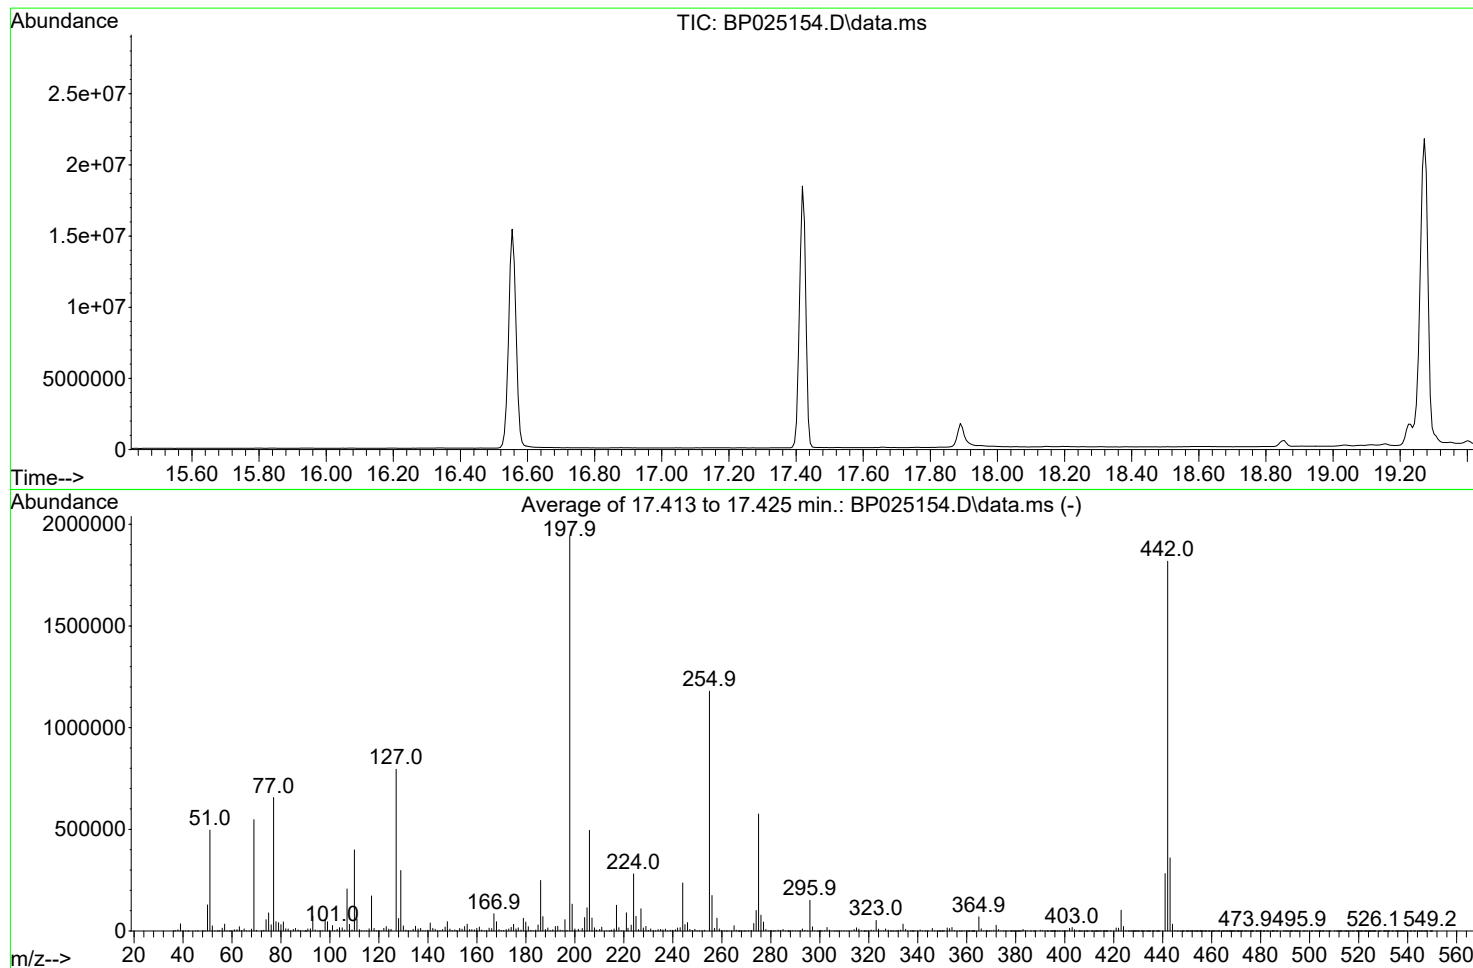

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2451

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	9499	PASS
69	69	100	100	100.0	547610	PASS
70	69	0.00	2	0.6	3175	PASS
197	198	0.00	2	0.2	3324	PASS
198	198	100	100	100.0	1941472	PASS
199	198	5	9	6.8	132421	PASS
365	198	1	100	3.6	69917	PASS
441	443	0.01	150	78.5	282261	PASS
442	442	100	100	100.0	1818101	PASS
443	442	15	24	19.8	359579	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/16/2025	BNA_P	<u>BP025154.D</u>
Compound Name	Response	Retention Time
DDT	7110729	20.578
DDD	166967	20.107
DDE	9571	19.583
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
176538	7287267	2.42

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025154.D
Acq On : 16 Jul 2025 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 16 14:37:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

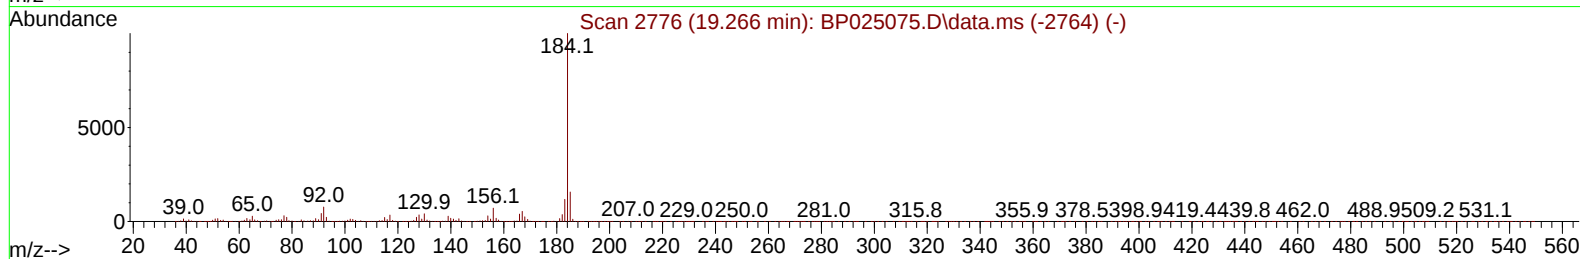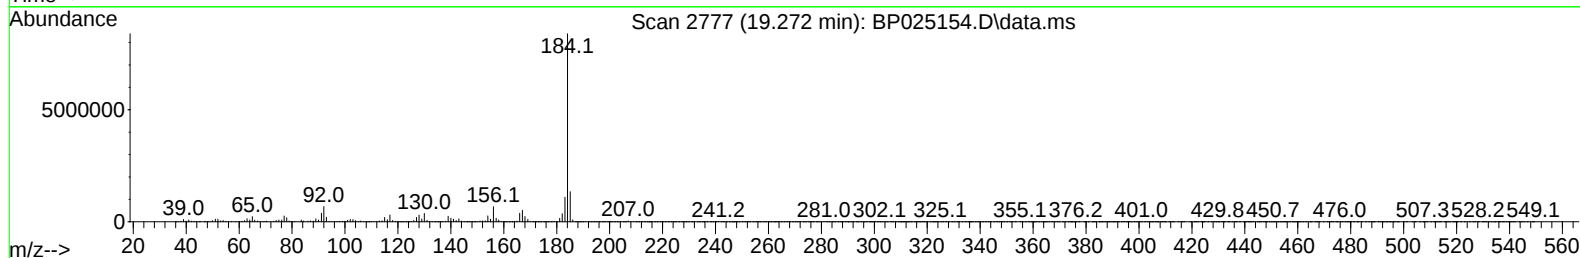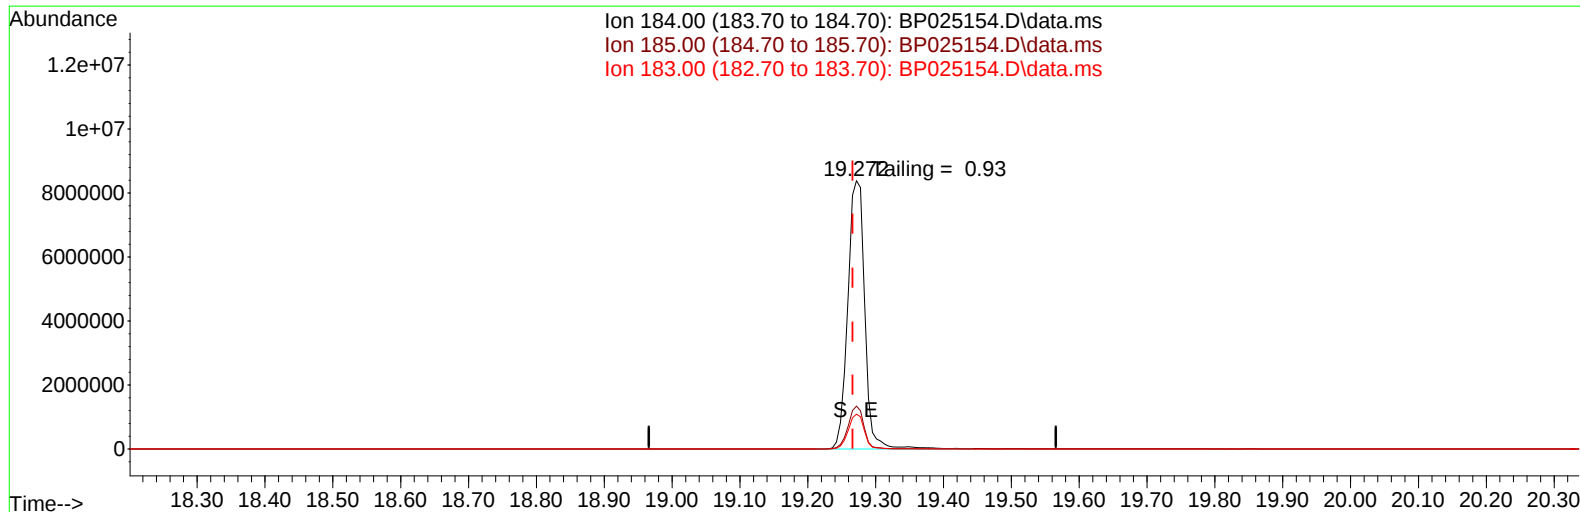

TIC: BP025154.D\data.ms

(77) Benzidine

19.272min (+ 0.006) 56461.29 ng




response 14377417

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.02
183.00	11.80	13.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025154.D
Acq On : 16 Jul 2025 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 16 14:37:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

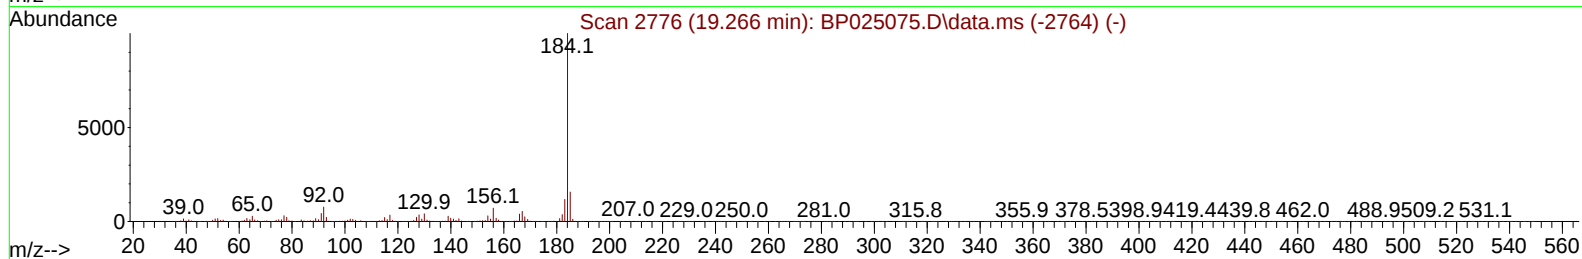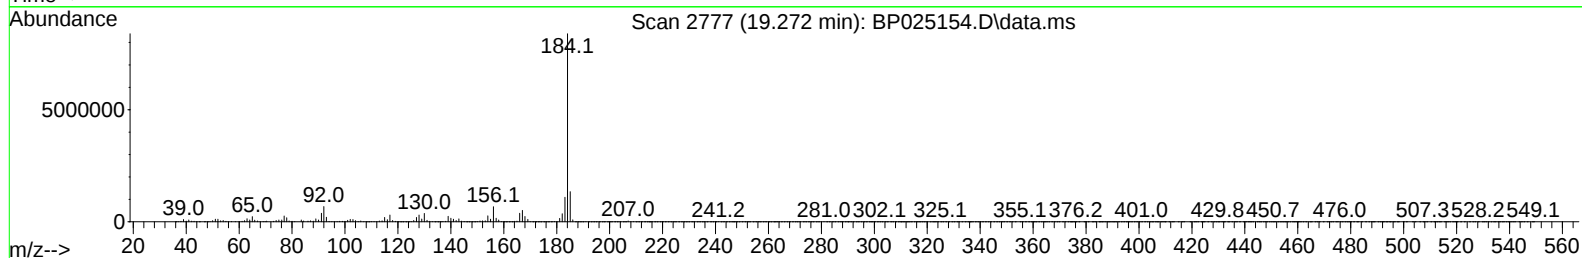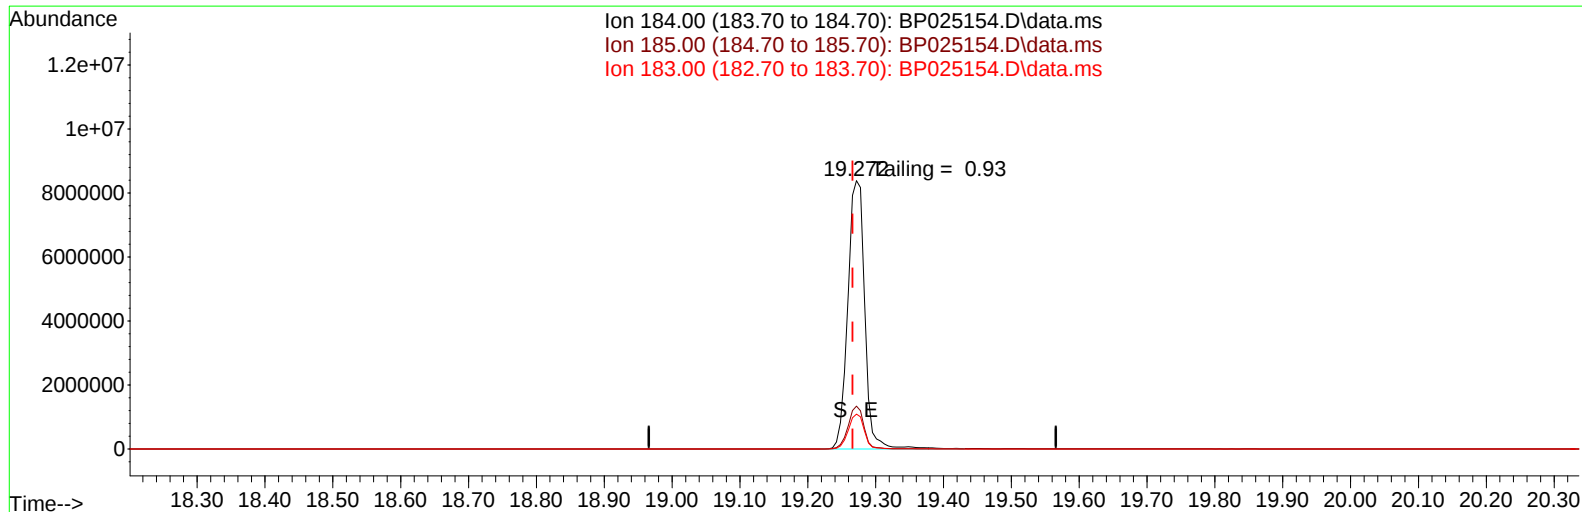

TIC: BP025154.D\data.ms

(77) Benzidine

19.272min (+ 0.006) 56461.29 ng

response 14377417

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.02
183.00	11.80	13.02
0.00	0.00	0.00