


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071125\
Data File : BP025097.D
Acq On : 11 Jul 2025 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 03 16:05:44 2025

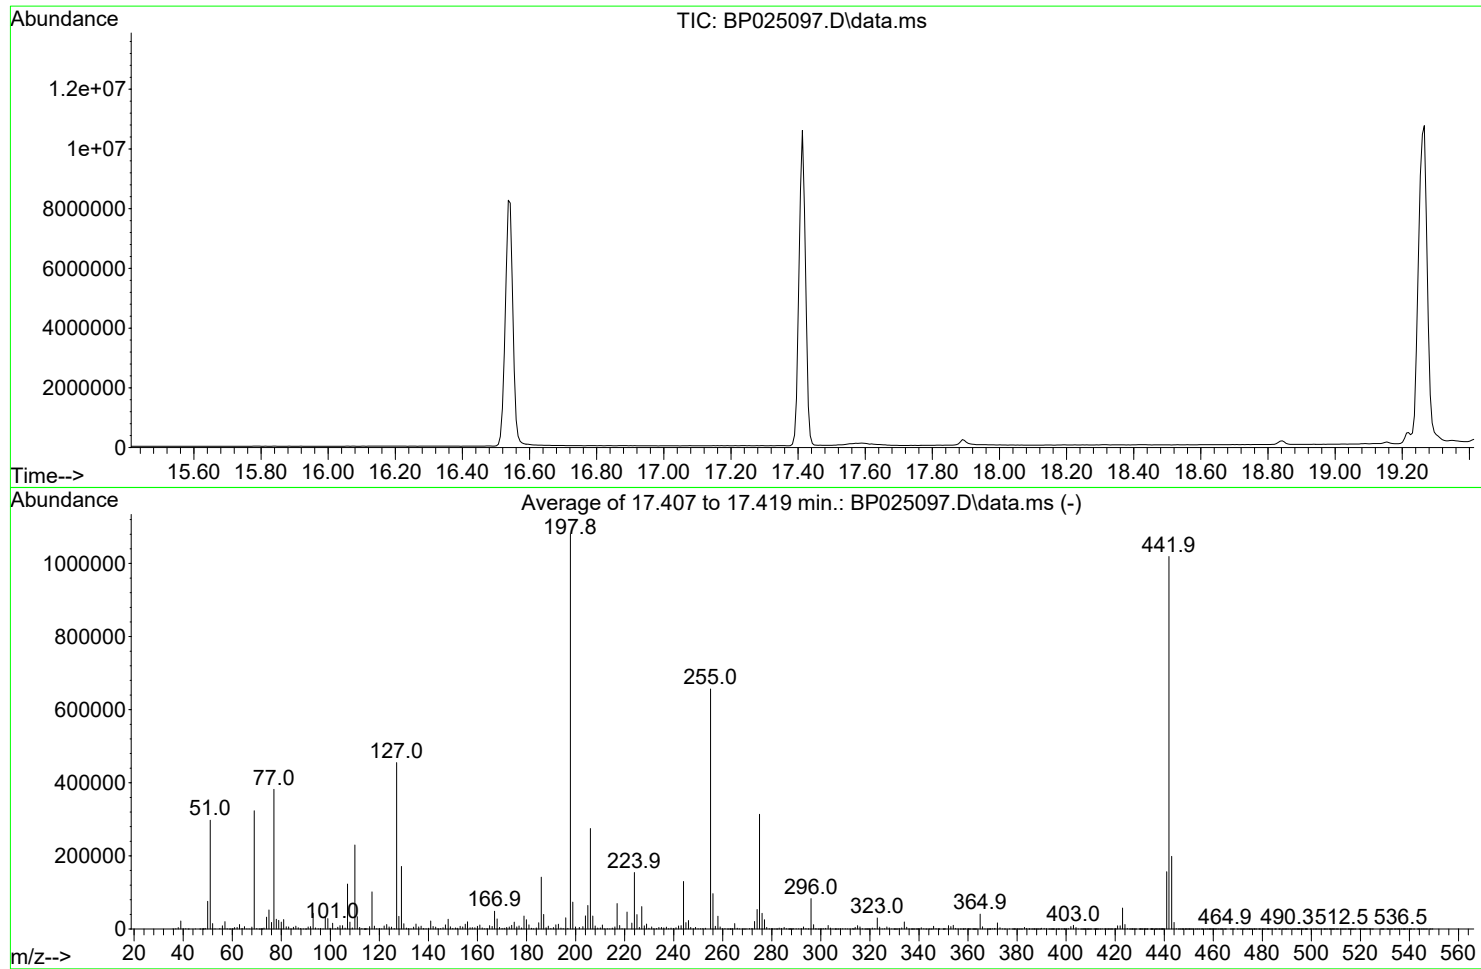

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2451

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5389	PASS
69	69	100	100	100.0	323529	PASS
70	69	0.00	2	0.5	1547	PASS
197	198	0.00	2	0.2	1806	PASS
198	198	100	100	100.0	1080103	PASS
199	198	5	9	6.8	73351	PASS
365	198	1	100	3.8	40848	PASS
441	443	0.01	150	78.8	156747	PASS
442	442	100	100	100.0	1018980	PASS
443	442	15	24	19.5	198827	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/11/2025	BNA_P	<u>BP025097.D</u>
Compound Name	Response	Retention Time
DDT	4034163	20.577
DDD	94451	20.107
DDE	2988	19.583
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
97439	4131602	2.36

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071125\
Data File : BP025097.D
Acq On : 11 Jul 2025 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 11 11:31:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

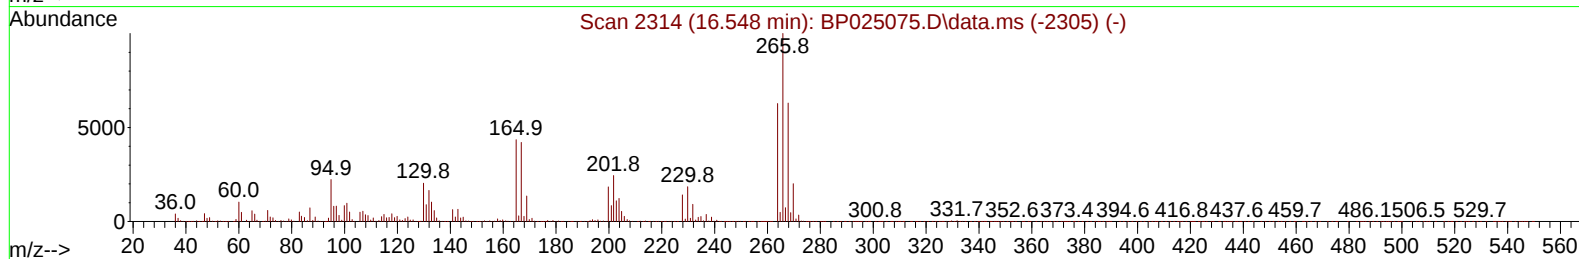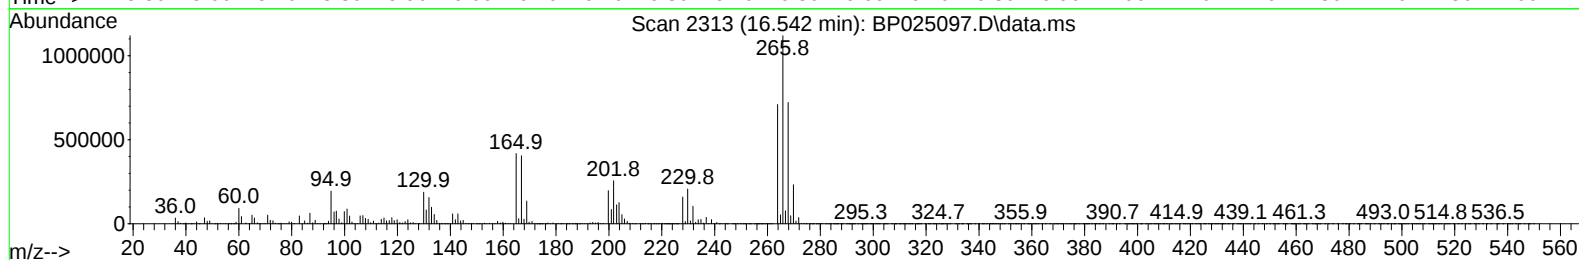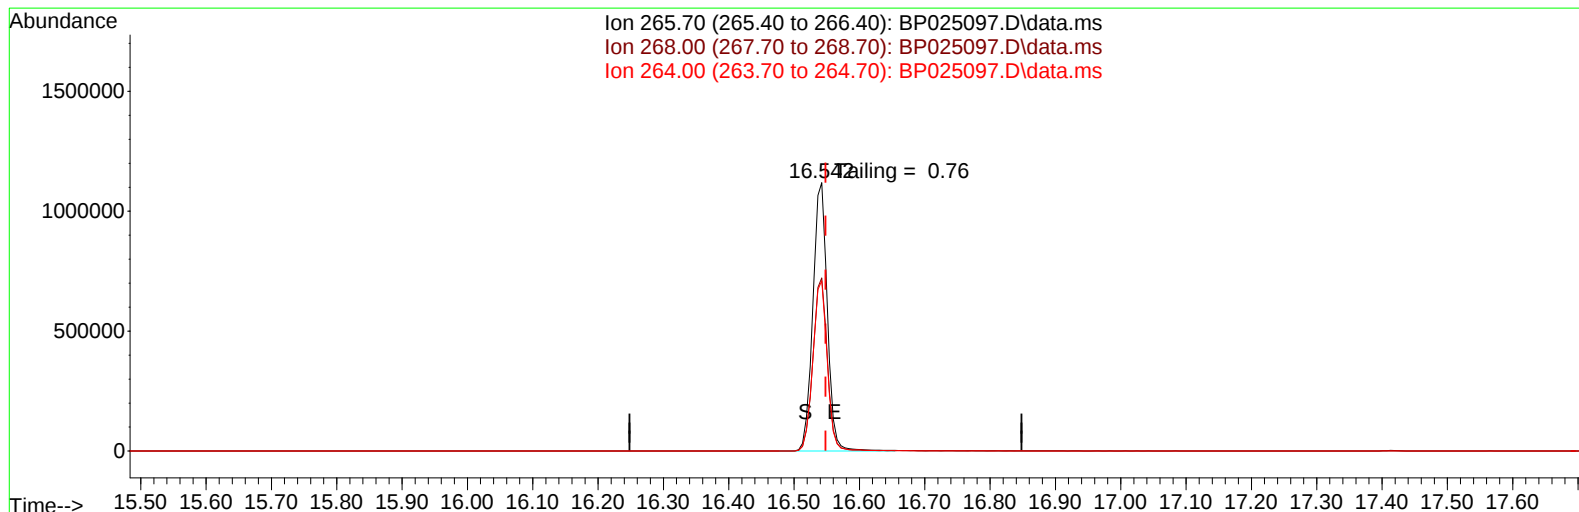

TIC: BP025097.D\data.ms

(70) Pentachlorophenol (C)

16.542min (-0.006) 760889.98 ng




response 1729929

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.54
264.00	62.70	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071125\
Data File : BP025097.D
Acq On : 11 Jul 2025 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 11 11:31:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

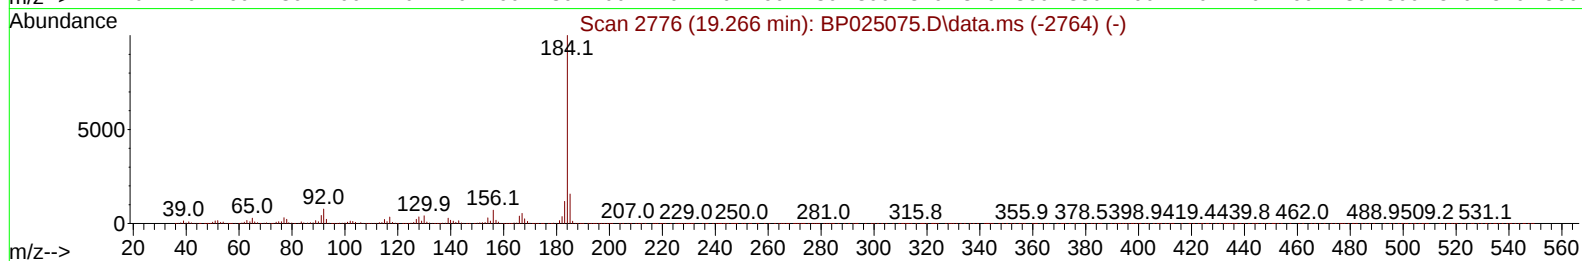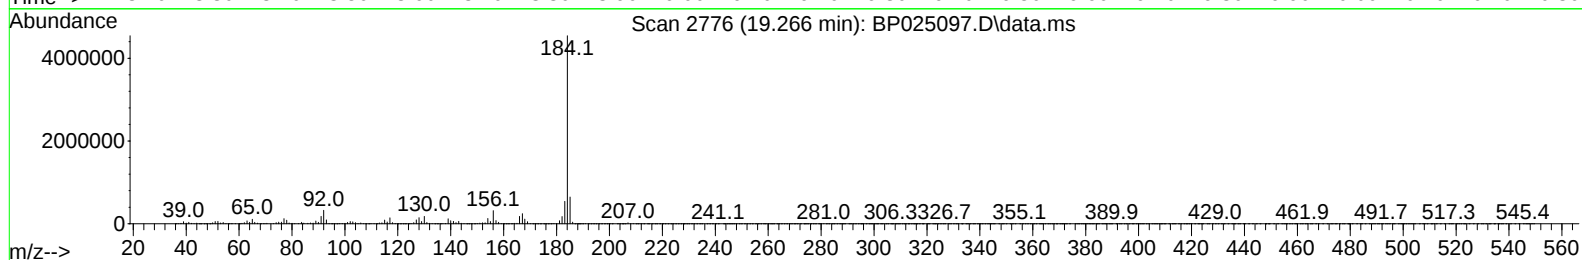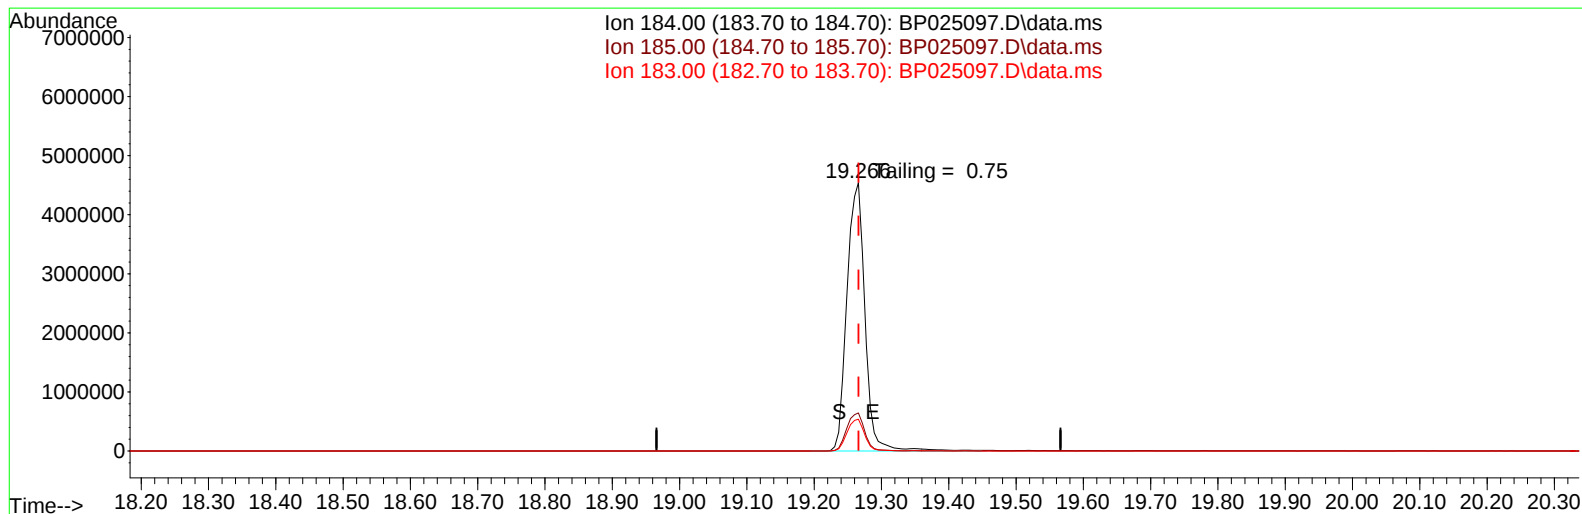

TIC: BP025097.D\data.ms

(77) Benzidine

19.266min (-0.000) 535019.97 ng

response 8334194

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.22
183.00	11.80	11.88
0.00	0.00	0.00