



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Cover Page

Order ID : Q2552

Project ID : NJ Drinking Water PT

Client : Alliance Technical Group, LLC - Newark

Lab Sample Number

Q2552-01
Q2552-02
Q2552-03
Q2552-04
Q2552-05
Q2552-06
Q2552-07
Q2552-08
Q2552-09
Q2552-10
Q2552-11

Client Sample Number

WS0725-PT-TURB-WS
WS0725-PT-TURB-WS
WS0725-PT-MIN-WS
WS0725-PT-TM-WS
WS0725-PT-HG-WS
WS0725-PT-SIO2-WS
WS0725-PT-RVOA-WS
WS0725-PT-UNROVA-WS
WS0725-PT-THM-WS
WS0725-PT-ADD-WS
WS0725-PT-EDBCP-WS

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 7/24/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

CASE NARRATIVE

Alliance Technical Group, LLC - Newark

Project Name: NJ Drinking Water PT

Project # N/A

Order ID # Q2552

Test Name: VOCMS Group1

A. Number of Samples and Date of Receipt:

1 Water sample was received on 07/09/2025.

B. Parameters

According to the Chain of Custody document, the following analyses were requested:
VOCMS Group1. This data package contains results for VOCMS Group1.

C. Analytical Techniques:

The analysis performed on instrument MSVOA_U were done using GC column DB-624UI 20m 0.18mm 1.0 um. Cat#121-1324UI. The analysis of VOCMS Group1 was based on method 524.2.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Surrogate recoveries were met for all analysis.

The Internal Standards Areas were met for all analysis.

The Retention Times were met for all analysis.

The RPD for {VU0717WBSD01} with File ID: VU063522.D met criteria except for Acetone[21%] due to difference in results of BS and BSD.

The Blank Spike met requirements for all compounds.

The Blank Spike Duplicate met requirements for all compounds.

The Blank analysis did not indicate the presence of lab contamination.

The %RSD is greater than 20% in the Initial Calibration method (524U071625DW.M) Iodomethane this compound is passing on Linear Regression and Nitrobenzene ,1,2-Dibromo-3-Chloropropane these compounds are passing on Quadratic Regression

The Continuous Calibration File ID VU063519.D met the requirements except for Acetone is failing high but no positive hit in associate sample therefore no corrective action taken.

The Continuous Calibration File ID VU063532.D met the requirements except for 2-Butanone and Acetone are failing high but no positive hit in associate sample therefore no corrective action taken.



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

The Tuning criteria met requirements.

Sample WS0725-PT-RVOA-WS was diluted due to high concentration.

E. Additional Comments:

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

F. Manual Integration Comments:

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as "12 B".
E	Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY

ORDER ID: Q2552

MATRIX: Water

METHOD: 524.2

		NA	NO	YES
1.	Chromatograms Labeled/Compounds Identified. (Field samples and Method Blanks)			✓
2.	GC/MS Tuning Specifications BFB Meet Criteria (NOTE THAT THERE ARE DIFFERENT CRITERIA FOR NY ASP CLP, CLP AND NJ)			✓
3.	GC/MS Tuning Frequency - Performed every 24 hours for 600 series and 12 hours for 8000 Series.			✓
4.	GC/MS Calibration - Initial Calibration performed before sample analysis and continuing calibration performed within 24 hours of sample analysis for 600 series and 12 hours for 8000 series.			✓
5.	GC/MS Calibration Requirements. The %RSD is greater than 20% in the Initial Calibration method (524U071625DW.M) Iodomethane this compound is passing on Linear Regression and Nitrobenzene ,1,2- Dibromo-3-Chloropropane these compounds are passing on Quadratic Regression The Continuous Calibration File ID VU063519.D met the requirements except for Acetone is failing high but no positive hit in associate sample therefore no corrective action taken. The Continuous Calibration File ID VU063532.D met the requirements except for 2- Butanone and Acetone are failing high but no positive hit in associate sample therefore no corrective action taken.			✓
6.	Blank Contamination - If yes, list compounds and concentrations in each blank:			✓
7.	Surrogate Recoveries Meet Criteria If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			✓
8.	Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria If not met, list those compounds and their recoveries which fall outside the acceptable range. The RPD for {VU0717WBSD01} with File ID: VU063522.D met criteria except for Acetone[21%] due to difference in results of BS and BSD.			✓
9.	Internal Standard Area/Retention Time Shift Meet Criteria			✓
	Comments:			
10.	Analysis Holding Time Met If not met, list number of days exceeded for each sample:			✓

ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)

NA NO YES

ADDITIONAL COMMENTS:

Sample WS0725-PT-RVOA-WS was diluted due to high concentration.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

QA REVIEW

Date

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2552

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

LAB CHRONICLE

OrderID:	Q2552	OrderDate:	7/9/2025 3:45:00 PM
Client:	Alliance Technical Group, LLC - Newark	Project:	NJ Drinking Water PT
Contact:	Mohammad Ahmed	Location:	QA Office, VOA Lab

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2552-07	WS0725-PT-RVOA-WS	Water	VOCMS Group1	524.2	07/07/25		07/17/25	07/09/25
Q2552-07DL	WS0725-PT-RVOA-WS DL	Water	VOCMS Group1	524.2	07/07/25		07/18/25	07/09/25

Hit Summary Sheet
SW-846

SDG No.: Q2552
Client: Alliance Technical Group, LLC - Newark

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Client ID:	WS0725-PT-RVOA-WS							
Q2552-07	WS0725-PT-RVOA Water	Vinyl Chloride		22.8	E	0.12	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,1-Dichloroethene		8.60		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Methylene Chloride		13.3		0.44	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	trans-1,2-Dichloroethene		18.5	E	0.14	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Carbon Tetrachloride		2.30		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	cis-1,2-Dichloroethene		5.10		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,1,1-Trichloroethane		17.9	E	0.12	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Benzene		15.0	E	0.11	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,2-Dichloroethane		13.2		0.14	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Trichloroethene		11.9		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,2-Dichloropropane		14.4		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Toluene		2.30		0.11	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,1,2-Trichloroethane		14.3		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Tetrachloroethene		13.1		0.14	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Chlorobenzene		17.8	E	0.11	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Ethyl Benzene		16.4	E	0.41	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	Total Xylenes		26.6		1.09	1.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	m/p-Xylenes		13.4		0.73	1.00	ug/L
Q2552-07	WS0725-PT-RVOA Water	o-Xylene		13.2		0.36	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,4-Dichlorobenzene		6.10		0.13	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,2-Dichlorobenzene		5.60		0.14	0.50	ug/L
Q2552-07	WS0725-PT-RVOA Water	1,2,4-Trichlorobenzene		16.9	E	0.21	0.50	ug/L
Total Voc :					262			
Total Concentration:					262			
Client ID:	WS0725-PT-RVOA-WSDL							
Q2552-07DL	WS0725-PT-RVOA Water	Vinyl Chloride		24.9	D	0.60	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	1,1-Dichloroethene		9.30	D	0.65	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	Methylene Chloride		18.0	D	2.20	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	trans-1,2-Dichloroethene		21.0	D	0.70	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	Carbon Tetrachloride		2.40	JD	0.65	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	cis-1,2-Dichloroethene		6.10	D	0.65	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	1,1,1-Trichloroethane		19.1	D	0.60	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	Benzene		16.1	D	0.55	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	1,2-Dichloroethane		15.1	D	0.70	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	Trichloroethene		12.3	D	0.65	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA Water	1,2-Dichloropropane		16.7	D	0.65	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

**Hit Summary Sheet
SW-846**

SDG No.: Q2552
Client: Alliance Technical Group, LLC - Newark

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Q2552-07DL	WS0725-PT-RVOA	Water	Toluene	2.40	JD	0.55	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	1,1,2-Trichloroethane	16.7	D	0.65	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	Tetrachloroethene	14.1	D	0.70	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	Chlorobenzene	19.4	D	0.55	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	Ethyl Benzene	17.3	D	2.10	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	Total Xylenes	27.2	D	5.50	7.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	m/p-Xylenes	13.6	D	3.70	5.00	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	o-Xylene	13.6	D	1.80	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	1,4-Dichlorobenzene	6.40	D	0.65	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	1,2-Dichlorobenzene	6.10	D	0.70	2.50	ug/L
Q2552-07DL	WS0725-PT-RVOA	Water	1,2,4-Trichlorobenzene	16.8	D	1.10	2.50	ug/L
Total Voc :				287				
Total Concentration:				287				



QC

SUMMARY

Surrogate Summary

SDG No.: Q2552

Client: Alliance Technical Group, LLC - Newark

Analytical Method: SW524.2

Lab Sample ID	Client ID	Parameter	Spike	Result	Recovery (%)	Qual	Limits (%)	
							Low	High
Q2552-07	WS0725-PT-RVOA-WS	1,2-Dichlorobenzene-d4	1	1.01	101		70	130
		4-Bromofluorobenzene	1	1.00	100		70	130
Q2552-07DL	WS0725-PT-RVOA-WSDL	1,2-Dichlorobenzene-d4	1	1.02	102		70	130
		4-Bromofluorobenzene	1	1.03	103		70	130
VU0717WBL01	VU0717WBL01	1,2-Dichlorobenzene-d4	1	0.94	94		70	130
		4-Bromofluorobenzene	1	1.07	107		70	130
VU0717WBS01	VU0717WBS01	1,2-Dichlorobenzene-d4	1	0.94	94		70	130
		4-Bromofluorobenzene	1	1.00	100		70	130
VU0717WBSD01	VU0717WBSD01	1,2-Dichlorobenzene-d4	1	1.10	110		70	130
		4-Bromofluorobenzene	1	1.03	103		70	130
VU0718WBL01	VU0718WBL01	1,2-Dichlorobenzene-d4	1	0.72	72		70	130
		4-Bromofluorobenzene	1	0.79	79		70	130
VU0718WBS02	VU0718WBS02	1,2-Dichlorobenzene-d4	1	1.05	105		70	130
		4-Bromofluorobenzene	1	1.03	103		70	130

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	Q2552	Analytical Method:	SW524.2
Client:	Alliance Technical Group, LLC - New	Datafile :	VU063521.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VU0717WBS01	Dichlorodifluoromethane	2	1.90	ug/L	95			70	130	
	Chloromethane	2	2.20	ug/L	110			70	130	
	Vinyl Chloride	2	2.00	ug/L	100			70	130	
	Bromomethane	2	2.30	ug/L	115			70	130	
	Chloroethane	2	2.00	ug/L	100			70	130	
	Tetrahydrofuran	4	4.70	ug/L	117			70	130	
	Trichlorofluoromethane	2	2.10	ug/L	105			70	130	
	1,1,2-Trichloro-1,2,2-trifluoroethane	2	2.00	ug/L	100			70	130	
	tert-Butyl Alcohol	20	20.3	ug/L	102			70	130	
	Diethyl Ether	2	2.10	ug/L	105			70	130	
	1,1-Dichloroethene	2	2.10	ug/L	105			70	130	
	Acrylonitrile	4	4.00	ug/L	100			70	130	
	Acetone	10	12.8	ug/L	128			70	130	
	Carbon disulfide	2	1.80	ug/L	90			70	130	
	Methyl tert-butyl Ether	2	2.10	ug/L	105			70	130	
	Methyl acrylate	2	1.90	ug/L	95			70	130	
	Methylene Chloride	2	2.30	ug/L	115			70	130	
	trans-1,2-Dichloroethene	2	2.00	ug/L	100			70	130	
	1,1-Dichloroethane	2	2.10	ug/L	105			70	130	
	Cyclohexane	2	2.10	ug/L	105			70	130	
	2-Butanone	10	11.2	ug/L	112			70	130	
	Carbon Tetrachloride	2	1.90	ug/L	95			70	130	
	2,2-Dichloropropane	2	2.00	ug/L	100			70	130	
	cis-1,2-Dichloroethene	2	2.10	ug/L	105			70	130	
	Bromochloromethane	2	2.10	ug/L	105			70	130	
	Chloroform	2	2.10	ug/L	105			70	130	
	1,1,1-Trichloroethane	2	2.00	ug/L	100			70	130	
	Methylcyclohexane	2	1.80	ug/L	90			70	130	
	1,1-Dichloropropene	2	2.10	ug/L	105			70	130	
	Propionitrile	10	10.4	ug/L	104			70	130	
	Benzene	2	2.20	ug/L	110			70	130	
	1,2-Dichloroethane	2	2.20	ug/L	110			70	130	
	Trichloroethene	2	1.80	ug/L	90			70	130	
	1,2-Dichloropropane	2	1.90	ug/L	95			70	130	
	1-Chlorobutane	2	2.10	ug/L	105			70	130	
	Dibromomethane	2	1.80	ug/L	90			70	130	
	Bromodichloromethane	2	1.80	ug/L	90			70	130	
	4-Methyl-2-Pentanone	10	9.70	ug/L	97			70	130	
	Toluene	2	1.90	ug/L	95			70	130	
	t-1,3-Dichloropropene	2	1.60	ug/L	80			70	130	
	cis-1,3-Dichloropropene	2	1.70	ug/L	85			70	130	
	1,1,2-Trichloroethane	2	2.00	ug/L	100			70	130	
	1,3-Dichloropropene	2	2.00	ug/L	100			70	130	
	2-Hexanone	10	10.2	ug/L	102			70	130	
	Dibromochloromethane	2	1.80	ug/L	90			70	130	
	1,2-Dibromoethane	2	1.90	ug/L	95			70	130	
	Tetrachloroethene	2	1.90	ug/L	95			70	130	
	Chlorobenzene	2	1.90	ug/L	95			70	130	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	Q2552	Analytical Method:	SW524.2
Client:	Alliance Technical Group, LLC - New	Datafile :	VU063521.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VU0717WBS01	1,1,1,2-Tetrachloroethane	2	1.70	ug/L	85			70	130	
	Hexachloroethane	2	1.60	ug/L	80			70	130	
	Ethyl Benzene	2	1.90	ug/L	95			70	130	
	m/p-Xylenes	4	3.80	ug/L	95			70	130	
	o-Xylene	2	2.00	ug/L	100			70	130	
	Styrene	2	1.90	ug/L	95			70	130	
	Bromoform	2	1.60	ug/L	80			70	130	
	Isopropylbenzene	2	2.00	ug/L	100			70	130	
	1,1,2,2-Tetrachloroethane	2	1.90	ug/L	95			70	130	
	1,2,3-Trichloropropane	2	1.90	ug/L	95			70	130	
	Bromobenzene	2	1.90	ug/L	95			70	130	
	N-propylbenzene	2	2.00	ug/L	100			70	130	
	2-Chlorotoluene	2	2.00	ug/L	100			70	130	
	1,3,5-Trimethylbenzene	2	1.90	ug/L	95			70	130	
	4-Chlorotoluene	2	2.00	ug/L	100			70	130	
	tert-Butylbenzene	2	1.90	ug/L	95			70	130	
	1,2,4-Trimethylbenzene	2	1.90	ug/L	95			70	130	
	Sec-butylbenzene	2	2.00	ug/L	100			70	130	
	p-Isopropyltoluene	2	2.00	ug/L	100			70	130	
	1,3-Dichlorobenzene	2	1.90	ug/L	95			70	130	
	1,4-Dichlorobenzene	2	1.90	ug/L	95			70	130	
	n-Butylbenzene	2	2.00	ug/L	100			70	130	
	1,2-Dichlorobenzene	2	1.90	ug/L	95			70	130	
	1,2-Dibromo-3-Chloropropane	2	1.70	ug/L	85			70	130	
	1,2,4-Trichlorobenzene	2	1.90	ug/L	95			70	130	
	Hexachlorobutadiene	2	1.90	ug/L	95			70	130	
	Naphthalene	2	1.80	ug/L	90			70	130	
	1,2,3-Trichlorobenzene	2	1.80	ug/L	90			70	130	
	Nitrobenzene	10	11.7	ug/L	117			70	130	
	Iodomethane	2	1.80	ug/L	90			70	130	
	Allyl Chloride	2	2.00	ug/L	100			70	130	
	t-1,4-Dichloro-2-butene	4	3.40	ug/L	85			70	130	
	Methacrylonitrile	2	1.90	ug/L	95			70	130	
	Ethyl methacrylate	2	1.90	ug/L	95			70	130	
	Isopropyl Ether	2	2.10	ug/L	105			70	130	
	Methyl methacrylate	4	3.50	ug/L	88			70	130	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	Q2552	Analytical Method:	SW524.2
Client:	Alliance Technical Group, LLC - New	Datafile :	VU063522.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VU0717WBSD01	Dichlorodifluoromethane	2	2.00	ug/L	100	5		70	130	20
	Chloromethane	2	2.20	ug/L	110	0		70	130	20
	Vinyl Chloride	2	2.10	ug/L	105	5		70	130	20
	Bromomethane	2	2.30	ug/L	115	0		70	130	20
	Chloroethane	2	2.10	ug/L	105	5		70	130	20
	Tetrahydrofuran	4	4.10	ug/L	103	13		70	130	20
	Trichlorofluoromethane	2	2.10	ug/L	105	0		70	130	20
	1,1,2-Trichloro-1,2,2-trifluoroethane	2	2.20	ug/L	110	10		70	130	20
	tert-Butyl Alcohol	20	21.0	ug/L	105	3		70	130	20
	Diethyl Ether	2	2.20	ug/L	110	5		70	130	20
	1,1-Dichloroethene	2	2.10	ug/L	105	0		70	130	20
	Acrylonitrile	4	4.20	ug/L	105	5		70	130	20
	Acetone	10	10.4	ug/L	104	21	*	70	130	20
	Carbon disulfide	2	1.90	ug/L	95	5		70	130	20
	Methyl tert-butyl Ether	2	2.20	ug/L	110	5		70	130	20
	Methyl acrylate	2	2.00	ug/L	100	5		70	130	20
	Methylene Chloride	2	2.30	ug/L	115	0		70	130	20
	trans-1,2-Dichloroethene	2	2.10	ug/L	105	5		70	130	20
	1,1-Dichloroethane	2	2.20	ug/L	110	5		70	130	20
	Cyclohexane	2	2.20	ug/L	110	5		70	130	20
	2-Butanone	10	10.5	ug/L	105	6		70	130	20
	Carbon Tetrachloride	2	2.00	ug/L	100	5		70	130	20
	2,2-Dichloropropane	2	2.00	ug/L	100	0		70	130	20
	cis-1,2-Dichloroethene	2	2.10	ug/L	105	0		70	130	20
	Bromochloromethane	2	2.10	ug/L	105	0		70	130	20
	Chloroform	2	2.20	ug/L	110	5		70	130	20
	1,1,1-Trichloroethane	2	2.10	ug/L	105	5		70	130	20
	Methylcyclohexane	2	1.90	ug/L	95	5		70	130	20
	1,1-Dichloropropene	2	2.20	ug/L	110	5		70	130	20
	Propionitrile	10	11.4	ug/L	114	9		70	130	20
	Benzene	2	1.80	ug/L	90	20		70	130	20
	1,2-Dichloroethane	2	1.80	ug/L	90	20		70	130	20
	Trichloroethene	2	1.90	ug/L	95	5		70	130	20
	1,2-Dichloropropane	2	2.00	ug/L	100	5		70	130	20
	1-Chlorobutane	2	2.00	ug/L	100	5		70	130	20
	Dibromomethane	2	2.00	ug/L	100	11		70	130	20
	Bromodichloromethane	2	1.80	ug/L	90	0		70	130	20
	4-Methyl-2-Pentanone	10	10.1	ug/L	101	4		70	130	20
	Toluene	2	2.00	ug/L	100	5		70	130	20
	t-1,3-Dichloropropene	2	1.70	ug/L	85	6		70	130	20
	cis-1,3-Dichloropropene	2	1.80	ug/L	90	6		70	130	20
	1,1,2-Trichloroethane	2	2.10	ug/L	105	5		70	130	20
	1,3-Dichloropropene	2	2.10	ug/L	105	5		70	130	20
	2-Hexanone	10	10.3	ug/L	103	1		70	130	20
	Dibromochloromethane	2	1.80	ug/L	90	0		70	130	20
	1,2-Dibromoethane	2	2.00	ug/L	100	5		70	130	20
	Tetrachloroethene	2	2.00	ug/L	100	5		70	130	20
	Chlorobenzene	2	2.00	ug/L	100	5		70	130	20

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	Q2552	Analytical Method:	SW524.2
Client:	Alliance Technical Group, LLC - New	Datafile :	VU063522.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VU0717WBSD01	1,1,1,2-Tetrachloroethane	2	1.80	ug/L	90	6		70	130	20
	Hexachloroethane	2	1.70	ug/L	85	6		70	130	20
	Ethyl Benzene	2	2.00	ug/L	100	5		70	130	20
	m/p-Xylenes	4	4.00	ug/L	100	5		70	130	20
	o-Xylene	2	2.00	ug/L	100	0		70	130	20
	Styrene	2	2.00	ug/L	100	5		70	130	20
	Bromoform	2	1.60	ug/L	80	0		70	130	20
	Isopropylbenzene	2	2.10	ug/L	105	5		70	130	20
	1,1,2,2-Tetrachloroethane	2	2.00	ug/L	100	5		70	130	20
	1,2,3-Trichloropropane	2	1.70	ug/L	85	11		70	130	20
	Bromobenzene	2	2.00	ug/L	100	5		70	130	20
	N-propylbenzene	2	2.00	ug/L	100	0		70	130	20
	2-Chlorotoluene	2	2.00	ug/L	100	0		70	130	20
	1,3,5-Trimethylbenzene	2	2.00	ug/L	100	5		70	130	20
	4-Chlorotoluene	2	2.00	ug/L	100	0		70	130	20
	tert-Butylbenzene	2	2.00	ug/L	100	5		70	130	20
	1,2,4-Trimethylbenzene	2	2.00	ug/L	100	5		70	130	20
	Sec-butylbenzene	2	2.00	ug/L	100	0		70	130	20
	p-Isopropyltoluene	2	2.00	ug/L	100	0		70	130	20
	1,3-Dichlorobenzene	2	2.00	ug/L	100	5		70	130	20
	1,4-Dichlorobenzene	2	2.00	ug/L	100	5		70	130	20
	n-Butylbenzene	2	2.10	ug/L	105	5		70	130	20
	1,2-Dichlorobenzene	2	2.00	ug/L	100	5		70	130	20
	1,2-Dibromo-3-Chloropropane	2	2.00	ug/L	100	16		70	130	20
	1,2,4-Trichlorobenzene	2	2.00	ug/L	100	5		70	130	20
	Hexachlorobutadiene	2	2.00	ug/L	100	5		70	130	20
	Naphthalene	2	2.10	ug/L	105	15		70	130	20
	1,2,3-Trichlorobenzene	2	2.00	ug/L	100	11		70	130	20
	Nitrobenzene	10	10.3	ug/L	103	13		70	130	20
	Iodomethane	2	1.90	ug/L	95	5		70	130	20
	Allyl Chloride	2	2.10	ug/L	105	5		70	130	20
	t-1,4-Dichloro-2-butene	4	3.60	ug/L	90	6		70	130	20
	Methacrylonitrile	2	2.00	ug/L	100	5		70	130	20
	Ethyl methacrylate	2	2.00	ug/L	100	5		70	130	20
	Isopropyl Ether	2	2.20	ug/L	110	5		70	130	20
	Methyl methacrylate	4	3.70	ug/L	93	6		70	130	20

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	Q2552	Analytical Method:	SW524.2
Client:	Alliance Technical Group, LLC - New	Datafile :	VU063535.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VU0718WBS02	Dichlorodifluoromethane	2	1.90	ug/L	95			70	130	
	Chloromethane	2	2.10	ug/L	105			70	130	
	Vinyl Chloride	2	2.10	ug/L	105			70	130	
	Bromomethane	2	2.30	ug/L	115			70	130	
	Chloroethane	2	2.20	ug/L	110			70	130	
	Tetrahydrofuran	4	4.80	ug/L	120			70	130	
	Trichlorofluoromethane	2	2.20	ug/L	110			70	130	
	1,1,2-Trichloro-1,2,2-trifluoroethane	2	2.20	ug/L	110			70	130	
	tert-Butyl Alcohol	20	20.7	ug/L	104			70	130	
	Diethyl Ether	2	2.30	ug/L	115			70	130	
	1,1-Dichloroethene	2	2.20	ug/L	110			70	130	
	Acrylonitrile	4	4.00	ug/L	100			70	130	
	Acetone	10	10.2	ug/L	102			70	130	
	Carbon disulfide	2	1.80	ug/L	90			70	130	
	Methyl tert-butyl Ether	2	2.20	ug/L	110			70	130	
	Methyl acrylate	2	2.10	ug/L	105			70	130	
	Methylene Chloride	2	2.20	ug/L	110			70	130	
	trans-1,2-Dichloroethene	2	2.10	ug/L	105			70	130	
	1,1-Dichloroethane	2	2.20	ug/L	110			70	130	
	Cyclohexane	2	2.20	ug/L	110			70	130	
	2-Butanone	10	11.0	ug/L	110			70	130	
	Carbon Tetrachloride	2	2.00	ug/L	100			70	130	
	2,2-Dichloropropane	2	2.00	ug/L	100			70	130	
	cis-1,2-Dichloroethene	2	2.20	ug/L	110			70	130	
	Bromochloromethane	2	2.20	ug/L	110			70	130	
	Chloroform	2	2.30	ug/L	115			70	130	
	1,1,1-Trichloroethane	2	2.10	ug/L	105			70	130	
	Methylcyclohexane	2	1.80	ug/L	90			70	130	
	1,1-Dichloropropene	2	2.20	ug/L	110			70	130	
	Propionitrile	10	11.1	ug/L	111			70	130	
	Benzene	2	1.80	ug/L	90			70	130	
	1,2-Dichloroethane	2	1.80	ug/L	90			70	130	
	Trichloroethene	2	1.90	ug/L	95			70	130	
	1,2-Dichloropropane	2	1.90	ug/L	95			70	130	
	1-Chlorobutane	2	2.00	ug/L	100			70	130	
	Dibromomethane	2	2.00	ug/L	100			70	130	
	Bromodichloromethane	2	1.80	ug/L	90			70	130	
	4-Methyl-2-Pentanone	10	10.5	ug/L	105			70	130	
	Toluene	2	2.00	ug/L	100			70	130	
	t-1,3-Dichloropropene	2	1.50	ug/L	75			70	130	
	cis-1,3-Dichloropropene	2	1.60	ug/L	80			70	130	
	1,1,2-Trichloroethane	2	2.10	ug/L	105			70	130	
	1,3-Dichloropropene	2	2.10	ug/L	105			70	130	
	2-Hexanone	10	10.0	ug/L	100			70	130	
	Dibromochloromethane	2	1.60	ug/L	80			70	130	
	1,2-Dibromoethane	2	1.90	ug/L	95			70	130	
	Tetrachloroethene	2	1.90	ug/L	95			70	130	
	Chlorobenzene	2	2.00	ug/L	100			70	130	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	Q2552	Analytical Method:	SW524.2
Client:	Alliance Technical Group, LLC - New	Datafile :	VU063535.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VU0718WBS02	1,1,1,2-Tetrachloroethane	2	1.70	ug/L	85			70	130	
	Hexachloroethane	2	1.50	ug/L	75			70	130	
	Ethyl Benzene	2	1.90	ug/L	95			70	130	
	m/p-Xylenes	4	3.90	ug/L	98			70	130	
	o-Xylene	2	2.00	ug/L	100			70	130	
	Styrene	2	2.00	ug/L	100			70	130	
	Bromoform	2	1.40	ug/L	70			70	130	
	Isopropylbenzene	2	2.00	ug/L	100			70	130	
	1,1,2,2-Tetrachloroethane	2	2.00	ug/L	100			70	130	
	1,2,3-Trichloropropane	2	2.00	ug/L	100			70	130	
	Bromobenzene	2	1.90	ug/L	95			70	130	
	N-propylbenzene	2	2.00	ug/L	100			70	130	
	2-Chlorotoluene	2	1.90	ug/L	95			70	130	
	1,3,5-Trimethylbenzene	2	1.90	ug/L	95			70	130	
	4-Chlorotoluene	2	2.00	ug/L	100			70	130	
	tert-Butylbenzene	2	2.00	ug/L	100			70	130	
	1,2,4-Trimethylbenzene	2	2.00	ug/L	100			70	130	
	Sec-butylbenzene	2	2.00	ug/L	100			70	130	
	p-Isopropyltoluene	2	2.00	ug/L	100			70	130	
	1,3-Dichlorobenzene	2	2.00	ug/L	100			70	130	
	1,4-Dichlorobenzene	2	2.00	ug/L	100			70	130	
	n-Butylbenzene	2	2.00	ug/L	100			70	130	
	1,2-Dichlorobenzene	2	2.00	ug/L	100			70	130	
	1,2-Dibromo-3-Chloropropane	2	1.90	ug/L	95			70	130	
	1,2,4-Trichlorobenzene	2	1.90	ug/L	95			70	130	
	Hexachlorobutadiene	2	1.90	ug/L	95			70	130	
	Naphthalene	2	2.00	ug/L	100			70	130	
	1,2,3-Trichlorobenzene	2	2.00	ug/L	100			70	130	
	Nitrobenzene	10	8.60	ug/L	86			70	130	
	Iodomethane	2	1.90	ug/L	95			70	130	
	Allyl Chloride	2	2.00	ug/L	100			70	130	
	t-1,4-Dichloro-2-butene	4	4.60	ug/L	115			70	130	
	Methacrylonitrile	2	2.00	ug/L	100			70	130	
	Ethyl methacrylate	2	2.00	ug/L	100			70	130	
	Isopropyl Ether	2	2.30	ug/L	115			70	130	
	Methyl methacrylate	4	3.70	ug/L	93			70	130	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE METHOD BLANK SUMMARY

Client ID

VU0717WBL01

Lab Name: Alliance

Contract: ALLI03

Lab Code: ACE

SDG NO.: Q2552

Lab File ID: VU063520.D

Lab Sample ID: VU0717WBL01

Date Analyzed: 07/17/2025

Time Analyzed: 11:31

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA_U

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VU0717WBS01	VU0717WBS01	VU063521.D	07/17/2025
VU0717WBSD01	VU0717WBSD01	VU063522.D	07/17/2025
WS0725-PT-RVOA-WS	Q2552-07	VU063529.D	07/17/2025

COMMENTS:



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE METHOD BLANK SUMMARY

Client ID

VU0718WBL01

Lab Name: Alliance

Contract: ALLI03

Lab Code: ACE

SDG NO.: Q2552

Lab File ID: VU063533.D

Lab Sample ID: VU0718WBL01

Date Analyzed: 07/18/2025

Time Analyzed: 10:49

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA_U

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VU0718WBS02	VU0718WBS02	VU063535.D	07/18/2025
WS0725-PT-RVOA-WSDL	Q2552-07DL	VU063541.D	07/18/2025

COMMENTS:



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance
 Lab Code: ACE
 Lab File ID: VU063510.D
 Instrument ID: MSVOA_U
 GC Column: DB-624UI ID: 0.18 (mm)

Contract: ALLI03
 SDG NO.: Q2552
 BFB Injection Date: 07/16/2025
 BFB Injection Time: 08:13
 Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	19
75	30.0 - 60.0% of mass 95	53.3
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.6
173	Less than 2.0% of mass 174	0.8 (1) 1
174	50.0 - 100.0% of mass 95	79
175	5.0 - 9.0% of mass 174	6.1 (7.7) 1
176	95.0 - 101.0% of mass 174	77.5 (98.1) 1
177	5.0 - 9.0% of mass 176	4.9 (6.3) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDICC0.5	VSTDICC0.5	VU063511.D	07/16/2025	09:24
VSTDICC001	VSTDICC001	VU063512.D	07/16/2025	09:54
VSTDICC002	VSTDICC002	VU063513.D	07/16/2025	10:27
VSTDICC005	VSTDICC005	VU063514.D	07/16/2025	11:00
VSTDICCC010	VSTDICCC010	VU063515.D	07/16/2025	11:37
VSTDICC015	VSTDICC015	VU063516.D	07/16/2025	12:11



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance
 Lab Code: ACE
 Lab File ID: VU063518.D
 Instrument ID: MSVOA_U
 GC Column: DB-624UI ID: 0.18 (mm)

Contract: ALLI03
 SDG NO.: Q2552
 BFB Injection Date: 07/17/2025
 BFB Injection Time: 08:10
 Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	18.2
75	30.0 - 60.0% of mass 95	52.6
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.5
173	Less than 2.0% of mass 174	0.8 (1.1) 1
174	50.0 - 100.0% of mass 95	73.7
175	5.0 - 9.0% of mass 174	5.5 (7.5) 1
176	95.0 - 101.0% of mass 174	70.5 (95.7) 1
177	5.0 - 9.0% of mass 176	4.7 (6.6) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC010	VSTDCCC010	VU063519.D	07/17/2025	09:25
VU0717WBL01	VU0717WBL01	VU063520.D	07/17/2025	11:31
VU0717WBS01	VU0717WBS01	VU063521.D	07/17/2025	12:43
VU0717WBSD01	VU0717WBSD01	VU063522.D	07/17/2025	13:13
WS0725-PT-RVOA-WS	Q2552-07	VU063529.D	07/17/2025	17:20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: Alliance
 Lab Code: ACE
 Lab File ID: VU063531.D
 Instrument ID: MSVOA_U
 GC Column: DB-624UI ID: 0.18 (mm)

Contract: ALLI03
 SDG NO.: Q2552
 BFB Injection Date: 07/18/2025
 BFB Injection Time: 08:07
 Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	19.3
75	30.0 - 60.0% of mass 95	53.6
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	7
173	Less than 2.0% of mass 174	0.7 (1) 1
174	50.0 - 100.0% of mass 95	71.8
175	5.0 - 9.0% of mass 174	5.3 (7.4) 1
176	95.0 - 101.0% of mass 174	69.8 (97.1) 1
177	5.0 - 9.0% of mass 176	4.4 (6.4) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

CLIENT ID	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC010	VSTDCCC010	VU063532.D	07/18/2025	09:11
VU0718WBL01	VU0718WBL01	VU063533.D	07/18/2025	10:49
VU0718WBS02	VU0718WBS02	VU063535.D	07/18/2025	11:50
WS0725-PT-RVOA-WSDL	Q2552-07DL	VU063541.D	07/18/2025	17:25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: ALLI03
Lab Code: ACE SDG NO.: Q2552
Lab File ID: VU063519.D Date Analyzed: 07/17/2025
Instrument ID: MSVOA_U Time Analyzed: 09:25
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	27500	6.10	0	0.00	0	0.00
	35750	6.6	0		0	
	19250	5.6	0		0	
EPA SAMPLE NO.						
WS0725-PT-RVOA-WS	21368	6.10	0	0.00	0	0.00
VU0717WBL01	22965	6.10	0	0.00	0	0.00
VU0717WBS01	21864	6.10	0	0.00	0	0.00
VU0717WBSD01	21661	6.10	0	0.00	0	0.00

IS1 = Fluorobenzene

IS2 =

IS3 =

AREA UPPER LIMIT = +30% of internal standard area

AREA LOWER LIMIT = -30% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: ALLI03
Lab Code: ACE SDG NO.: Q2552
Lab File ID: VU063519.D Date Analyzed: 07/17/2025
Instrument ID: MSVOA_U Time Analyzed: 09:25
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS4 AREA #	RT #				
12 HOUR STD	0	0				
	0					
	0					
EPA SAMPLE NO.						
WS0725-PT-RVOA-WS	0	0.00				
VU0717WBL01	0	0.00				
VU0717WBS01	0	0.00				
VU0717WBSD01	0	0.00				

IS4 =

AREA UPPER LIMIT = +30% of internal standard area

AREA LOWER LIMIT = -30% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: ALLI03
Lab Code: ACE SDG NO.: Q2552
Lab File ID: VU063532.D Date Analyzed: 07/18/2025
Instrument ID: MSVOA_U Time Analyzed: 09:11
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	22137	6.10	0	0.00	0	0.00
UPPER LIMIT	28778.1	6.597	0		0	
LOWER LIMIT	15495.9	5.597	0		0	
EPA SAMPLE NO.						
WS0725-PT-RVOA-WSDL	16405	6.10	0	0.00	0	0.00
VU0718WBL01	25256	6.10	0	0.00	0	0.00
VU0718WBS02	20233	6.10	0	0.00	0	0.00

IS1 = Fluorobenzene

IS2 =

IS3 =

AREA UPPER LIMIT = +30% of internal standard area

AREA LOWER LIMIT = -30% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: Alliance Contract: ALLI03
Lab Code: ACE SDG NO.: Q2552
Lab File ID: VU063532.D Date Analyzed: 07/18/2025
Instrument ID: MSVOA_U Time Analyzed: 09:11
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS4 AREA #	RT #				
12 HOUR STD	0	0				
UPPER LIMIT	0					
LOWER LIMIT	0					
EPA SAMPLE NO.						
WS0725-PT-RVOA-WSDL	0	0.00				
VU0718WBL01	0	0.00				
VU0718WBS02	0	0.00				

IS4 =

AREA UPPER LIMIT = +30% of internal standard area

AREA LOWER LIMIT = -30% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



SAMPLE

DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25	
Project:	NJ Drinking Water PT			Date Received:	07/09/25	
Client Sample ID:	WS0725-PT-RVOA-WS			SDG No.:	Q2552	
Lab Sample ID:	Q2552-07			Matrix:	Water	
Analytical Method:	E524.2			% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063529.D	1	07/17/25 17:20	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	0.12	U	0.12	0.50	ug/L
74-87-3	Chloromethane	0.13	U	0.13	0.50	ug/L
75-01-4	Vinyl Chloride	22.8	E	0.12	0.50	ug/L
74-83-9	Bromomethane	0.15	U	0.15	0.50	ug/L
75-00-3	Chloroethane	0.14	U	0.14	0.50	ug/L
109-99-9	Tetrahydrofuran	0.42	U	0.42	1.00	ug/L
75-69-4	Trichlorofluoromethane	0.20	U	0.20	0.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	0.11	U	0.11	0.50	ug/L
75-65-0	tert-Butyl Alcohol	3.60	U	3.60	10.0	ug/L
60-29-7	Diethyl Ether	0.13	U	0.13	0.50	ug/L
75-35-4	1,1-Dichloroethene	8.60		0.13	0.50	ug/L
107-13-1	Acrylonitrile	0.44	U	0.44	1.00	ug/L
67-64-1	Acetone	0.97	U	0.97	2.50	ug/L
75-15-0	Carbon Disulfide	0.12	U	0.12	0.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	0.11	U	0.11	0.50	ug/L
96-33-3	Methyl acrylate	0.33	U	0.33	0.50	ug/L
75-09-2	Methylene Chloride	13.3		0.44	0.50	ug/L
156-60-5	trans-1,2-Dichloroethene	18.5	E	0.14	0.50	ug/L
75-34-3	1,1-Dichloroethane	0.13	U	0.13	0.50	ug/L
110-82-7	Cyclohexane	0.14	U	0.14	0.50	ug/L
78-93-3	2-Butanone	0.72	U	0.72	2.50	ug/L
56-23-5	Carbon Tetrachloride	2.30		0.13	0.50	ug/L
594-20-7	2,2-Dichloropropane	0.12	U	0.12	0.50	ug/L
156-59-2	cis-1,2-Dichloroethene	5.10		0.13	0.50	ug/L
74-97-5	Bromoform	0.17	U	0.17	0.50	ug/L
67-66-3	Chloroform	0.17	U	0.17	0.50	ug/L
71-55-6	1,1,1-Trichloroethane	17.9	E	0.12	0.50	ug/L
108-87-2	Methylcyclohexane	0.090	U	0.090	0.50	ug/L
563-58-6	1,1-Dichloropropene	0.11	U	0.11	0.50	ug/L
107-12-0	Propionitrile	1.20	U	1.20	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25
Project:	NJ Drinking Water PT			Date Received:	07/09/25
Client Sample ID:	WS0725-PT-RVOA-WS			SDG No.:	Q2552
Lab Sample ID:	Q2552-07			Matrix:	Water
Analytical Method:	E524.2			% Solid:	0
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063529.D	1	07/17/25 17:20	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	15.0	E	0.11	0.50	ug/L
107-06-2	1,2-Dichloroethane	13.2		0.14	0.50	ug/L
79-01-6	Trichloroethene	11.9		0.13	0.50	ug/L
78-87-5	1,2-Dichloropropane	14.4		0.13	0.50	ug/L
109-69-3	1-Chlorobutane	0.12	U	0.12	0.50	ug/L
74-95-3	Dibromomethane	0.15	U	0.15	0.50	ug/L
75-27-4	Bromodichloromethane	0.13	U	0.13	0.50	ug/L
108-10-1	4-Methyl-2-Pentanone	0.63	U	0.63	2.50	ug/L
108-88-3	Toluene	2.30		0.11	0.50	ug/L
10061-02-6	t-1,3-Dichloropropene	0.11	U	0.11	0.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	0.11	U	0.11	0.50	ug/L
79-00-5	1,1,2-Trichloroethane	14.3		0.13	0.50	ug/L
142-28-9	1,3-Dichloropropane	0.12	U	0.12	0.50	ug/L
591-78-6	2-Hexanone	0.65	U	0.65	2.50	ug/L
124-48-1	Dibromochloromethane	0.20	U	0.20	0.50	ug/L
106-93-4	1,2-Dibromoethane	0.13	U	0.13	0.50	ug/L
127-18-4	Tetrachloroethene	13.1		0.14	0.50	ug/L
108-90-7	Chlorobenzene	17.8	E	0.11	0.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	0.13	U	0.13	0.50	ug/L
67-72-1	Hexachloroethane	0.12	U	0.12	0.50	ug/L
100-41-4	Ethyl Benzene	16.4	E	0.41	0.50	ug/L
179601-23-1	m/p-Xylenes	13.4		0.73	1.00	ug/L
1330-20-7	Total Xylenes	26.6		1.09	1.50	ug/L
95-47-6	o-Xylene	13.2		0.36	0.50	ug/L
100-42-5	Styrene	0.38	U	0.38	0.50	ug/L
75-25-2	Bromoform	0.31	U	0.31	0.50	ug/L
98-82-8	Isopropylbenzene	0.38	U	0.38	0.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	0.13	U	0.13	0.50	ug/L
96-18-4	1,2,3-Trichloropropane	0.19	U	0.19	0.50	ug/L
108-86-1	Bromobenzene	0.13	U	0.13	0.50	ug/L
103-65-1	n-propylbenzene	0.42	U	0.42	0.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25
Project:	NJ Drinking Water PT			Date Received:	07/09/25
Client Sample ID:	WS0725-PT-RVOA-WS			SDG No.:	Q2552
Lab Sample ID:	Q2552-07			Matrix:	Water
Analytical Method:	E524.2			% Solid:	0
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063529.D	1	07/17/25 17:20	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	0.27	U	0.27	0.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	0.37	U	0.37	0.50	ug/L
106-43-4	4-Chlorotoluene	0.27	U	0.27	0.50	ug/L
98-06-6	tert-Butylbenzene	0.37	U	0.37	0.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	0.40	U	0.40	0.50	ug/L
135-98-8	sec-Butylbenzene	0.36	U	0.36	0.50	ug/L
99-87-6	p-Isopropyltoluene	0.42	U	0.42	0.50	ug/L
541-73-1	1,3-Dichlorobenzene	0.13	U	0.13	0.50	ug/L
106-46-7	1,4-Dichlorobenzene	6.10		0.13	0.50	ug/L
104-51-8	n-Butylbenzene	0.43	U	0.43	0.50	ug/L
95-50-1	1,2-Dichlorobenzene	5.60		0.14	0.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	0.24	U	0.24	0.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	16.9	E	0.21	0.50	ug/L
87-68-3	Hexachlorobutadiene	0.14	U	0.14	0.50	ug/L
91-20-3	Naphthalene	0.33	U	0.33	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	0.31	U	0.31	0.50	ug/L
98-95-3	Nitrobenzene	1.80	U	1.80	5.00	ug/L
363-72-4	Pentachloroethane	0.16	U	0.16	0.50	ug/L
74-88-4	Iodomethane	0.090	U	0.090	1.00	ug/L
107-05-1	Allyl Chloride	0.13	U	0.13	0.50	ug/L
126-98-7	Methacrylonitrile	0.24	U	0.24	0.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	0.21	U	0.21	1.00	ug/L
97-63-2	Ethyl methacrylate	0.12	U	0.12	0.50	ug/L
108-20-3	Isopropyl Ether	0.14	U	0.14	0.50	ug/L
80-62-6	Methyl methacrylate	0.24	U	0.24	1.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	1.00		70 - 130	101%	SPK: 1
460-00-4	4-Bromofluorobenzene	1.00		70 - 130	100%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	21400		6.097		



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25
Project:	NJ Drinking Water PT			Date Received:	07/09/25
Client Sample ID:	WS0725-PT-RVOA-WS			SDG No.:	Q2552
Lab Sample ID:	Q2552-07			Matrix:	Water
Analytical Method:	E524.2			% Solid:	0
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000 uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063529.D	1	07/17/25 17:20	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063529.D
 Acq On : 17 Jul 2025 17:20
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

Quant Time: Jul 18 05:57:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 18 05:14:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	21368m	1.000	ug/l	0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	8119	1.004	ug/l	0.00
Spiked Amount 1.000			Recovery	=	100.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	7549	1.009	ug/l	0.00
Spiked Amount 1.000			Recovery	=	101.000%	
Target Compounds						
				Qvalue		
4) Vinyl Chloride	1.599	62	169988	22.788	ug/l	99
9) 1,1-Dichloroethene	2.567	96	47673	8.594	ug/l	96
15) Methylene Chloride	3.030	84	87096	13.335	ug/l	98
16) trans-1,2-Dichloroethene	3.335	96	116242	18.450	ug/l	99
22) cis-1,2-Dichloroethene	4.647	96	34837	5.096	ug/l	90
28) 1,1,1-Trichloroethane	5.293	97	180945	17.891	ug/l	98
30) Carbon Tetrachloride	5.496	117	18569	2.281	ug/l	93
35) Benzene	5.750	78	377988	15.016	ug/l	99
36) 1,2-Dichloroethane	5.779	62	103598	13.245	ug/l	99
37) Trichloroethene	6.525	130	76177	11.861	ug/l	97
38) 1,2-Dichloropropane	6.779	63	85102	14.445	ug/l	99
49) Toluene	7.959	92	31066	2.260	ug/l	97
52) 1,1,2-Trichloroethane	8.393	97	58960	14.349	ug/l	99
58) Tetrachloroethene	8.541	164	77148	13.124	ug/l	98
59) Chlorobenzene	9.438	112	280950	17.797	ug/l	100
63) Ethyl Benzene	9.560	91	445992	16.418	ug/l	99
64) m/p-Xylenes	9.685	106	141952	13.444	ug/l	98
65) o-Xylene	10.090	106	133669	13.175	ug/l	97
83) 1,4-Dichlorobenzene	11.830	146	77219	6.091	ug/l	99
85) 1,2-Dichlorobenzene	12.206	146	66816	5.615	ug/l	99
87) 1,2,4-Trichlorobenzene	13.833	180	125271	16.930	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063529.D
 Acq On : 17 Jul 2025 17:20
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1


Quant Time: Jul 18 05:57:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 18 05:14:02 2025
 Response via : Initial Calibration

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

**Manual Integrations
APPROVED**


Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

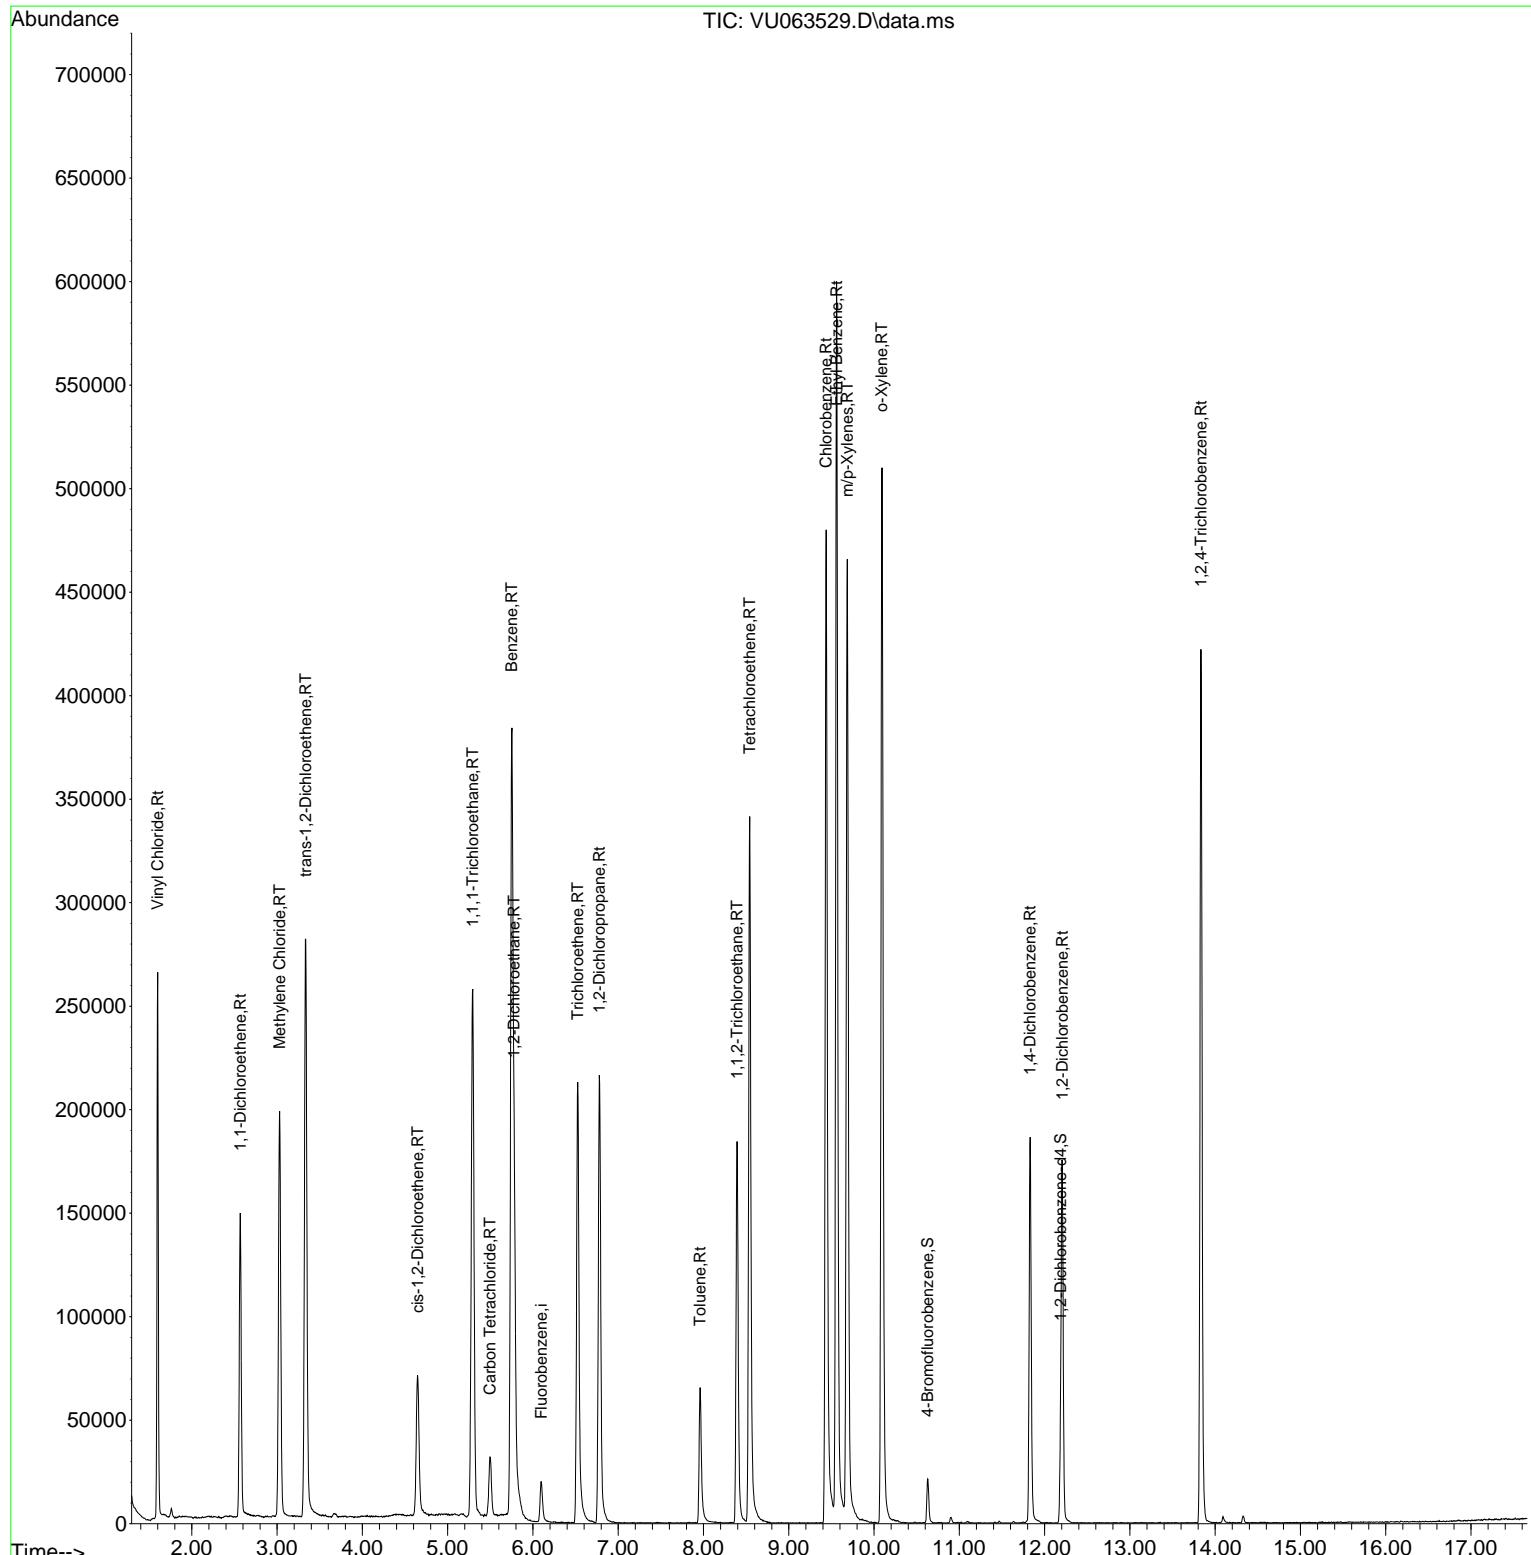



#1
Fluorobenzene
Concen: 1.000 ug/l m
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20




Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WS




Tgt Ion: 96 Resp: 21368
Ion Ratio Lower Upper
96 100
70 19.1 15.0 22.4
95 7.6 7.4 11.0
97 0.0 0.0 0.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

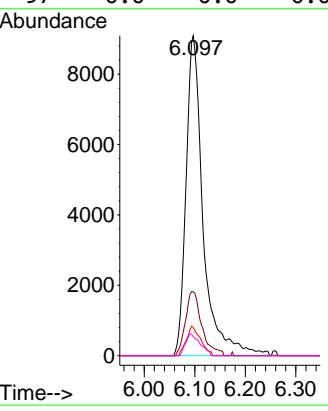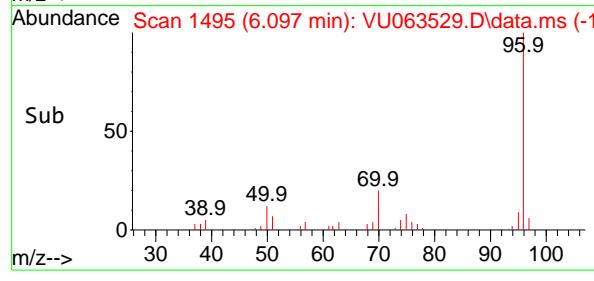


#4
Vinyl Chloride
Concen: 22.788 ug/l
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20




Tgt Ion: 62 Resp: 169988
Ion Ratio Lower Upper
62 100
64 32.5 25.7 38.5

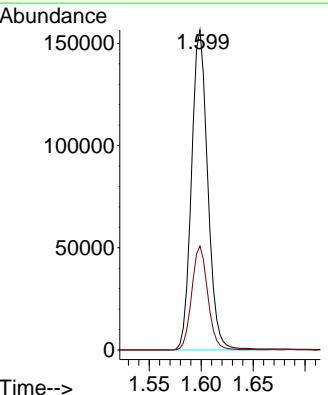



#9
1,1-Dichloroethene
Concen: 8.594 ug/l
RT: 2.567 min Scan# 397
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20



Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WS




Tgt Ion: 96 Resp: 4767
Ion Ratio Lower Upper
96 100
61 174.7 0.0 504.3
98 63.6 0.0 126.8

Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025









#15
Methylene Chloride
Concen: 13.335 ug/l
RT: 3.030 min Scan# 541
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

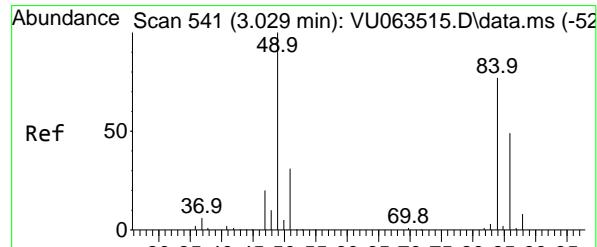

Tgt Ion: 84 Resp: 87096
Ion Ratio Lower Upper
84 100
49 132.8 103.8 155.8
51 41.5 0.0 80.4
86 65.2 51.1 76.7

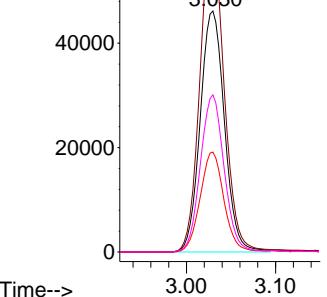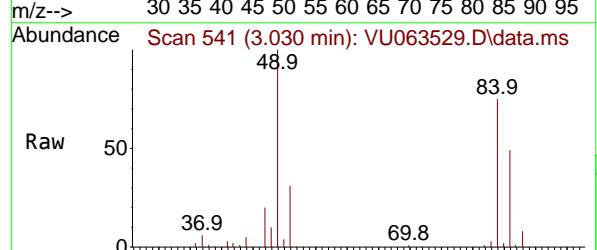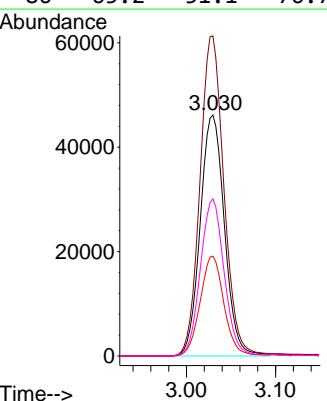




#16

trans-1,2-Dichloroethene
Concen: 18.450 ug/l
RT: 3.335 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WS


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#22
cis-1,2-Dichloroethene
Concen: 5.096 ug/l
RT: 4.647 min Scan# 1044
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Tgt Ion: 96 Resp: 34837
Ion Ratio Lower Upper
96 100
61 137.5 0.0 384.7
98 62.8 32.1 96.3





#28

1,1,1-Trichloroethane

Concen: 17.891 ug/l

RT: 5.293 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063529.D

Acq: 17 Jul 2025 17:20


Instrument :

MSVOA_U

ClientSampleId :


WS0725-PT-RVOA-WS


**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


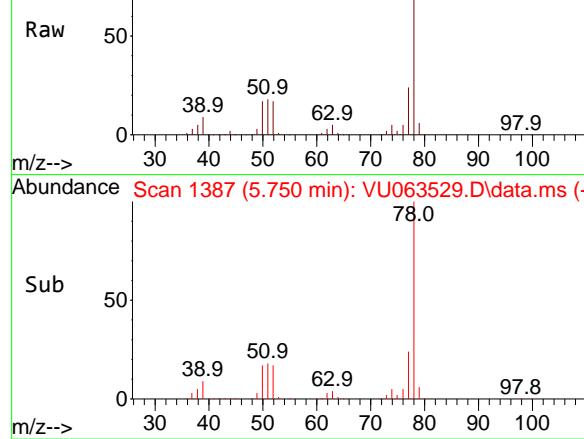
#30
Carbon Tetrachloride
Concen: 2.281 ug/l
RT: 5.496 min Scan# 1308
Delta R.T. -0.006 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Tgt Ion:117 Resp: 18569
Ion Ratio Lower Upper
117 100
119 91.0 79.2 118.8
121 30.0 25.5 38.3

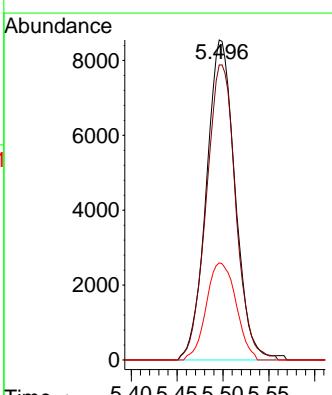




Abundance Scan 1387 (5.750 min): VU063529.D\data.ms



Abundance Scan 1387 (5.750 min): VU063529.D\data.ms (-1)

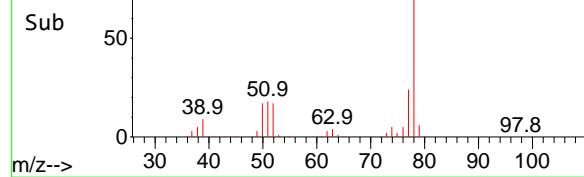

#35

Benzene

Concen: 15.016 ug/l

RT: 5.750 min Scan# 1

Delta R.T. -0.006 min


Lab File: VU063529.D

Acq: 17 Jul 2025 17:20


Instrument : MSVOA_U
 ClientSampleId : WS0725-PT-RVOA-WS

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

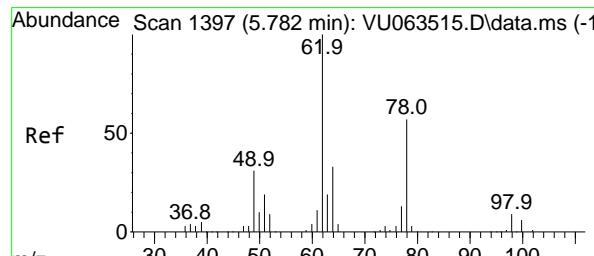

Abundance Scan 1396 (5.779 min): VU063529.D\data.ms

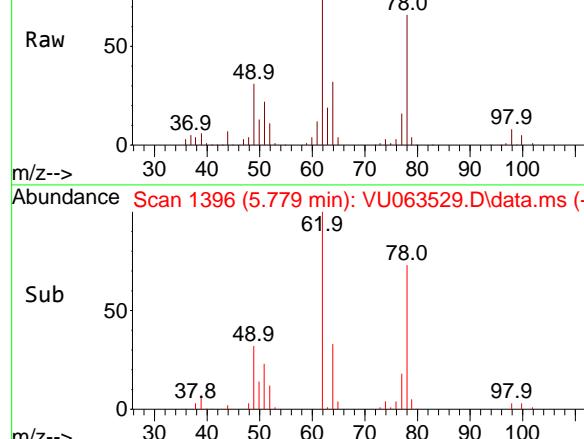

Abundance Scan 1396 (5.779 min): VU063529.D\data.ms (-1)

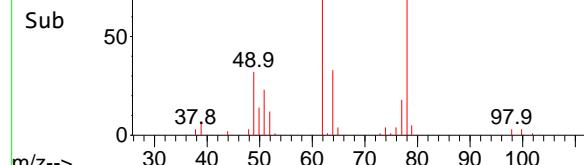

#36

1,2-Dichloroethane

Concen: 13.245 ug/l

RT: 5.779 min Scan# 1396

Delta R.T. -0.003 min

Lab File: VU063529.D



Acq: 17 Jul 2025 17:20


Tgt Ion: 62 Resp: 103598

Ion Ratio Lower Upper

62 100


98 7.7 6.4 9.6

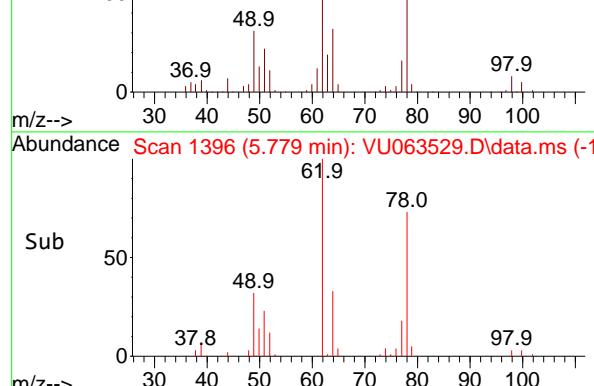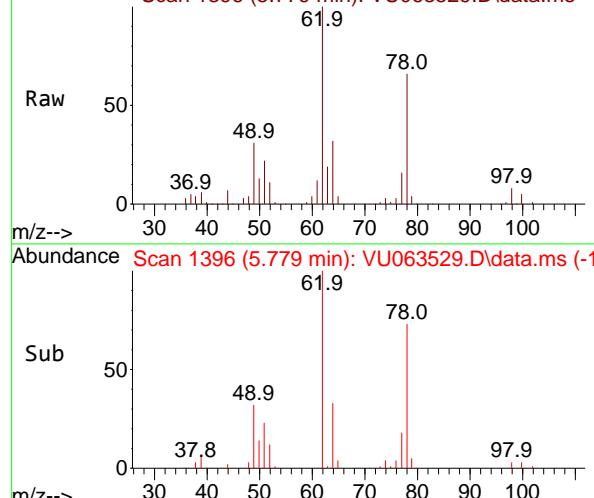



#37
Trichloroethene
Concen: 11.861 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20




Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WS




Tgt Ion:130 Resp: 7617
Ion Ratio Lower Upper
130 100
95 103.0 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


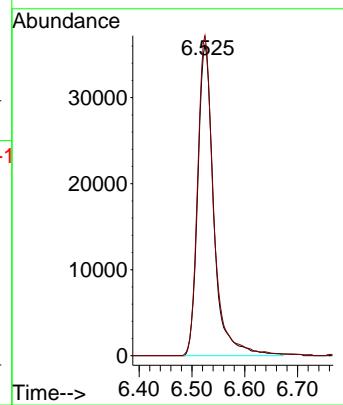



#38
1,2-Dichloropropane
Concen: 14.445 ug/l
RT: 6.779 min Scan# 1707
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20



Tgt Ion: 63 Resp: 85102
Ion Ratio Lower Upper
63 100
65 30.1 24.6 36.8

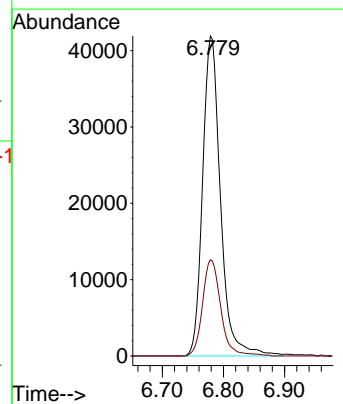







#49
Toluene
Concen: 2.260 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WS


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

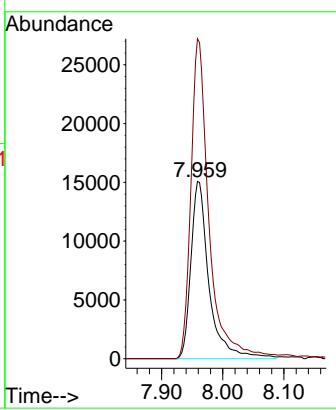

#52
1,1,2-Trichloroethane
Concen: 14.349 ug/l
RT: 8.393 min Scan# 2209
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Tgt Ion: 97 Resp: 58960
Ion Ratio Lower Upper
97 100
83 88.3 70.2 105.2
85 58.1 45.2 67.8
99 62.2 50.1 75.1

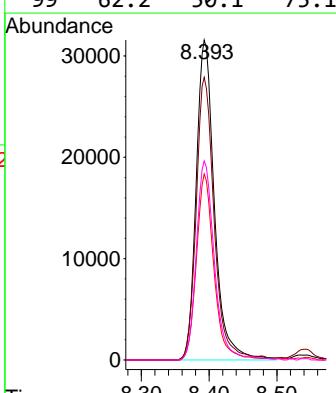


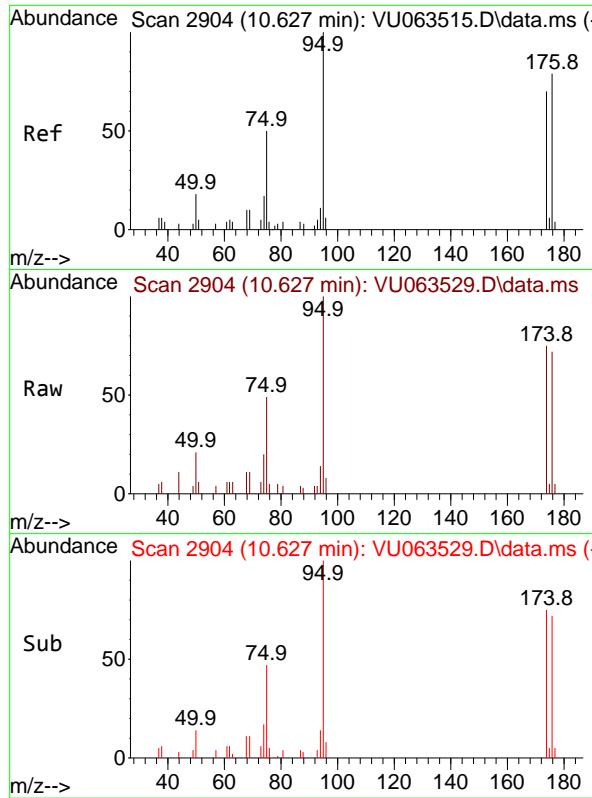


#57
4-Bromofluorobenzene
Concen: 1.004 ug/l
RT: 10.627 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

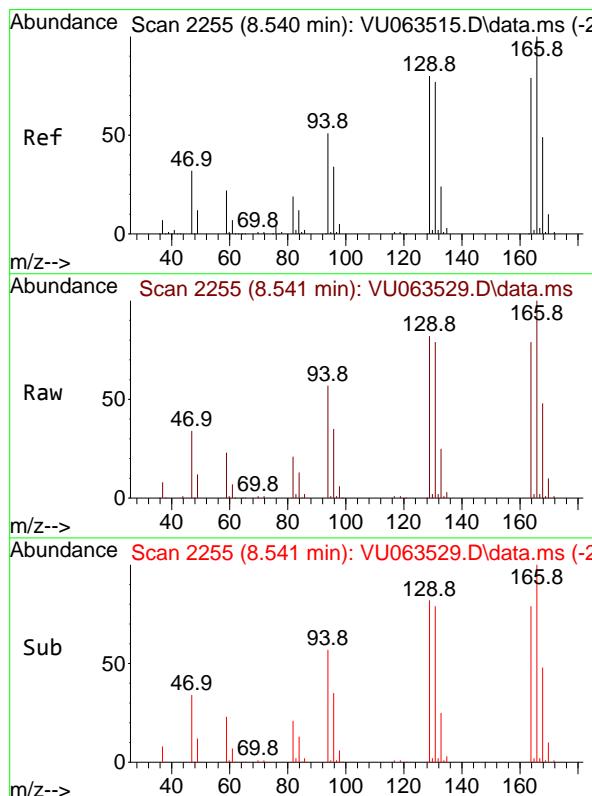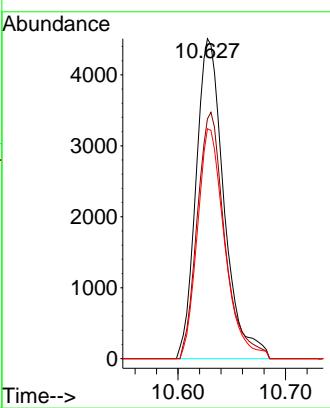

#58
Tetrachloroethene
Concen: 13.124 ug/l
RT: 8.541 min Scan# 2255
Delta R.T. 0.000 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Tgt	Ion:164	Resp:	77148
Ion	Ratio	Lower	Upper
164	100		
166	126.7	100.7	151.1
129	104.0	80.6	120.8
131	99.5	77.3	115.9

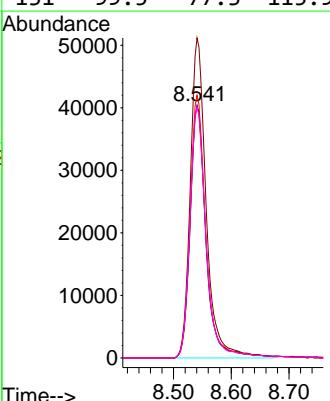



#59

Chlorobenzene

Concen: 17.797 ug/l

RT: 9.438 min Scan# 2

Delta R.T. -0.003 min




Lab File: VU063529.D

Acq: 17 Jul 2025 17:20

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

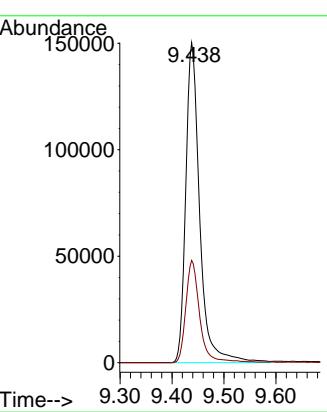

#63
Ethyl Benzene
Concen: 16.418 ug/l
RT: 9.560 min Scan# 2572
Delta R.T. -0.003 min
Lab File: VU063529.D
Acq: 17 Jul 2025 17:20

Tgt Ion: 91 Resp: 445992
Ion Ratio Lower Upper
91 100
106 31.1 25.4 38.0

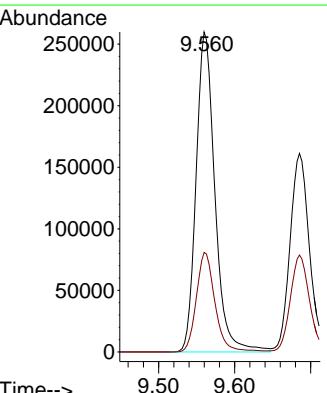



#64

m/p-Xylenes

Concen: 13.444 ug/l

RT: 9.685 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063529.D




Acq: 17 Jul 2025 17:20

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS

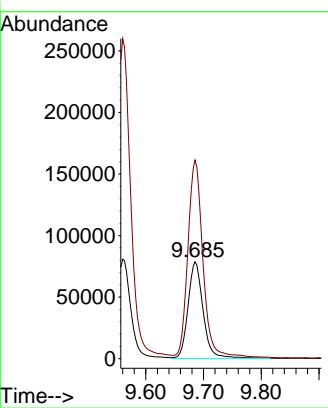**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#65

o-Xylene



Concen: 13.175 ug/l




RT: 10.090 min Scan# 2737

Delta R.T. -0.003 min

Lab File: VU063529.D

Acq: 17 Jul 2025 17:20

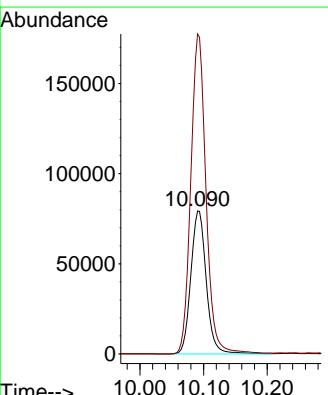Tgt Ion:106 Resp: 133669
Ion Ratio Lower Upper
106 100
91 220.7 108.1 324.4



#68

1,2-Dichlorobenzene-d4

Concen: 1.009 ug/l

RT: 12.187 min Scan# 3

Instrument :

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063529.D

Acq: 17 Jul 2025 17:20





ClientSampleId :

WS0725-PT-RVOA-WS

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#83

1,4-Dichlorobenzene

Concen: 6.091 ug/l


RT: 11.830 min Scan# 3278




Delta R.T. 0.000 min

Lab File: VU063529.D

Acq: 17 Jul 2025 17:20

Tgt	Ion:146	Resp:	77219
Ion	Ratio	Lower	Upper
146	100		
111	40.9	32.0	48.0
148	62.3	50.2	75.2

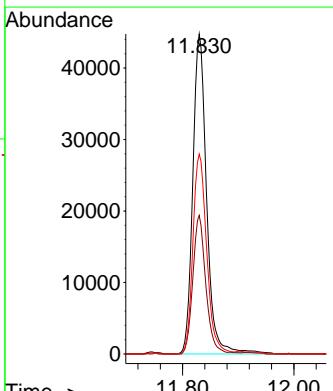

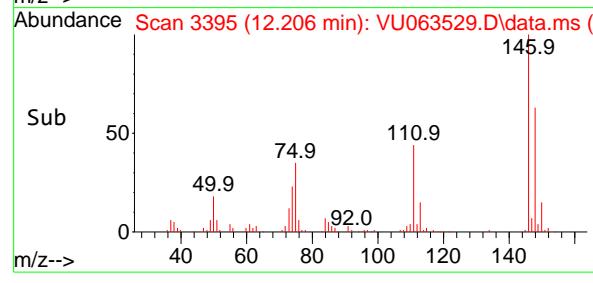

#85

1,2-Dichlorobenzene

Concen: 5.615 ug/l

RT: 12.206 min Scan# 3395

Delta R.T. 0.000 min





Lab File: VU063529.D

Acq: 17 Jul 2025 17:20

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

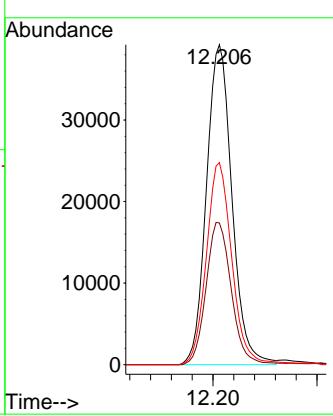

#87

1,2,4-Trichlorobenzene

Concen: 16.930 ug/l


RT: 13.833 min Scan# 3901

Delta R.T. 0.000 min

Lab File: VU063529.D

Acq: 17 Jul 2025 17:20

Tgt Ion:180 Resp: 125271
Ion Ratio Lower Upper
180 100
182 95.2 76.2 114.4
145 32.7 26.2 39.2





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25	
Project:	NJ Drinking Water PT			Date Received:	07/09/25	
Client Sample ID:	WS0725-PT-RVOA-WSDL			SDG No.:	Q2552	
Lab Sample ID:	Q2552-07DL			Matrix:	Water	
Analytical Method:	E524.2			% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063541.D	5	07/18/25 17:25	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	0.60	UD	0.60	2.50	ug/L
74-87-3	Chloromethane	0.65	UD	0.65	2.50	ug/L
75-01-4	Vinyl Chloride	24.9	D	0.60	2.50	ug/L
74-83-9	Bromomethane	0.75	UD	0.75	2.50	ug/L
75-00-3	Chloroethane	0.70	UD	0.70	2.50	ug/L
109-99-9	Tetrahydrofuran	2.10	UD	2.10	5.00	ug/L
75-69-4	Trichlorofluoromethane	1.00	UD	1.00	2.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	0.55	UD	0.55	2.50	ug/L
75-65-0	tert-Butyl Alcohol	18.0	UD	18.0	50.0	ug/L
60-29-7	Diethyl Ether	0.65	UD	0.65	2.50	ug/L
75-35-4	1,1-Dichloroethene	9.30	D	0.65	2.50	ug/L
107-13-1	Acrylonitrile	2.20	UD	2.20	5.00	ug/L
67-64-1	Acetone	4.90	UD	4.90	12.5	ug/L
75-15-0	Carbon Disulfide	0.60	UD	0.60	2.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	0.55	UD	0.55	2.50	ug/L
96-33-3	Methyl acrylate	1.70	UD	1.70	2.50	ug/L
75-09-2	Methylene Chloride	18.0	D	2.20	2.50	ug/L
156-60-5	trans-1,2-Dichloroethene	21.0	D	0.70	2.50	ug/L
75-34-3	1,1-Dichloroethane	0.65	UD	0.65	2.50	ug/L
110-82-7	Cyclohexane	0.70	UD	0.70	2.50	ug/L
78-93-3	2-Butanone	3.60	UD	3.60	12.5	ug/L
56-23-5	Carbon Tetrachloride	2.40	JD	0.65	2.50	ug/L
594-20-7	2,2-Dichloropropane	0.60	UD	0.60	2.50	ug/L
156-59-2	cis-1,2-Dichloroethene	6.10	D	0.65	2.50	ug/L
74-97-5	Bromoform	0.85	UD	0.85	2.50	ug/L
67-66-3	Chloroform	0.85	UD	0.85	2.50	ug/L
71-55-6	1,1,1-Trichloroethane	19.1	D	0.60	2.50	ug/L
108-87-2	Methylcyclohexane	0.46	UD	0.46	2.50	ug/L
563-58-6	1,1-Dichloropropene	0.55	UD	0.55	2.50	ug/L
107-12-0	Propionitrile	5.80	UD	5.80	12.5	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25
Project:	NJ Drinking Water PT			Date Received:	07/09/25
Client Sample ID:	WS0725-PT-RVOA-WSDL			SDG No.:	Q2552
Lab Sample ID:	Q2552-07DL			Matrix:	Water
Analytical Method:	E524.2			% Solid:	0
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000 uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063541.D	5	07/18/25 17:25	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	16.1	D	0.55	2.50	ug/L
107-06-2	1,2-Dichloroethane	15.1	D	0.70	2.50	ug/L
79-01-6	Trichloroethene	12.3	D	0.65	2.50	ug/L
78-87-5	1,2-Dichloropropane	16.7	D	0.65	2.50	ug/L
109-69-3	1-Chlorobutane	0.60	UD	0.60	2.50	ug/L
74-95-3	Dibromomethane	0.75	UD	0.75	2.50	ug/L
75-27-4	Bromodichloromethane	0.65	UD	0.65	2.50	ug/L
108-10-1	4-Methyl-2-Pentanone	3.20	UD	3.20	12.5	ug/L
108-88-3	Toluene	2.40	JD	0.55	2.50	ug/L
10061-02-6	t-1,3-Dichloropropene	0.55	UD	0.55	2.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	0.55	UD	0.55	2.50	ug/L
79-00-5	1,1,2-Trichloroethane	16.7	D	0.65	2.50	ug/L
142-28-9	1,3-Dichloropropane	0.60	UD	0.60	2.50	ug/L
591-78-6	2-Hexanone	3.30	UD	3.30	12.5	ug/L
124-48-1	Dibromochloromethane	1.00	UD	1.00	2.50	ug/L
106-93-4	1,2-Dibromoethane	0.65	UD	0.65	2.50	ug/L
127-18-4	Tetrachloroethene	14.1	D	0.70	2.50	ug/L
108-90-7	Chlorobenzene	19.4	D	0.55	2.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	0.65	UD	0.65	2.50	ug/L
67-72-1	Hexachloroethane	0.60	UD	0.60	2.50	ug/L
100-41-4	Ethyl Benzene	17.3	D	2.10	2.50	ug/L
179601-23-1	m/p-Xylenes	13.6	D	3.70	5.00	ug/L
1330-20-7	Total Xylenes	27.2	D	5.50	7.50	ug/L
95-47-6	o-Xylene	13.6	D	1.80	2.50	ug/L
100-42-5	Styrene	1.90	UD	1.90	2.50	ug/L
75-25-2	Bromoform	1.60	UD	1.60	2.50	ug/L
98-82-8	Isopropylbenzene	1.90	UD	1.90	2.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	0.65	UD	0.65	2.50	ug/L
96-18-4	1,2,3-Trichloropropane	0.95	UD	0.95	2.50	ug/L
108-86-1	Bromobenzene	0.65	UD	0.65	2.50	ug/L
103-65-1	n-propylbenzene	2.10	UD	2.10	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25
Project:	NJ Drinking Water PT			Date Received:	07/09/25
Client Sample ID:	WS0725-PT-RVOA-WSDL			SDG No.:	Q2552
Lab Sample ID:	Q2552-07DL			Matrix:	Water
Analytical Method:	E524.2			% Solid:	0
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000 uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063541.D	5	07/18/25 17:25	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	1.40	UD	1.40	2.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	1.90	UD	1.90	2.50	ug/L
106-43-4	4-Chlorotoluene	1.40	UD	1.40	2.50	ug/L
98-06-6	tert-Butylbenzene	1.90	UD	1.90	2.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	2.00	UD	2.00	2.50	ug/L
135-98-8	sec-Butylbenzene	1.80	UD	1.80	2.50	ug/L
99-87-6	p-Isopropyltoluene	2.10	UD	2.10	2.50	ug/L
541-73-1	1,3-Dichlorobenzene	0.65	UD	0.65	2.50	ug/L
106-46-7	1,4-Dichlorobenzene	6.40	D	0.65	2.50	ug/L
104-51-8	n-Butylbenzene	2.20	UD	2.20	2.50	ug/L
95-50-1	1,2-Dichlorobenzene	6.10	D	0.70	2.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	1.20	UD	1.20	2.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	16.8	D	1.10	2.50	ug/L
87-68-3	Hexachlorobutadiene	0.70	UD	0.70	2.50	ug/L
91-20-3	Naphthalene	1.70	UD	1.70	5.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	1.60	UD	1.60	2.50	ug/L
98-95-3	Nitrobenzene	8.80	UD	8.80	25.0	ug/L
363-72-4	Pentachloroethane	0.80	UD	0.80	2.50	ug/L
74-88-4	Iodomethane	0.47	UD	0.47	5.00	ug/L
107-05-1	Allyl Chloride	0.65	UD	0.65	2.50	ug/L
126-98-7	Methacrylonitrile	1.20	UD	1.20	2.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	1.10	UD	1.10	5.00	ug/L
97-63-2	Ethyl methacrylate	0.60	UD	0.60	2.50	ug/L
108-20-3	Isopropyl Ether	0.70	UD	0.70	2.50	ug/L
80-62-6	Methyl methacrylate	1.20	UD	1.20	5.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	1.00		70 - 130	102%	SPK: 1
460-00-4	4-Bromofluorobenzene	1.00		70 - 130	103%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	16400		6.097		



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	07/07/25
Project:	NJ Drinking Water PT			Date Received:	07/09/25
Client Sample ID:	WS0725-PT-RVOA-WSDL			SDG No.:	Q2552
Lab Sample ID:	Q2552-07DL			Matrix:	Water
Analytical Method:	E524.2			% Solid:	0
Sample Wt/Vol:	25	Units:	mL	Final Vol:	25000 uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063541.D	5	07/18/25 17:25	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063541.D
 Acq On : 18 Jul 2025 17:25
 Operator : MD/SY
 Sample : Q2552-07DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WSDL

Quant Time: Jul 18 23:52:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	16405	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	6421	1.034	ug/l	0.00
Spiked Amount 1.000			Recovery	=	103.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	5884	1.024	ug/l	0.00
Spiked Amount 1.000			Recovery	=	102.000%	
Target Compounds						
				Qvalue		
4) Vinyl Chloride	1.599	62	28569	4.989	ug/l	99
9) 1,1-Dichloroethene	2.570	96	7910	1.857	ug/l	93
15) Methylene Chloride	3.030	84	18061	3.602	ug/l	99
16) trans-1,2-Dichloroethene	3.335	96	20327	4.202	ug/l	98
22) cis-1,2-Dichloroethene	4.650	96	6421	1.223	ug/l	87
28) 1,1,1-Trichloroethane	5.293	97	29732	3.829	ug/l	99
30) Carbon Tetrachloride	5.496	117	3051	0.488	ug/l	98
35) Benzene	5.753	78	62135	3.215	ug/l	98
36) 1,2-Dichloroethane	5.782	62	18106	3.015	ug/l	96
37) Trichloroethene	6.528	130	12102	2.454	ug/l	90
38) 1,2-Dichloropropane	6.782	63	15126	3.344	ug/l	99
49) Toluene	7.962	92	5105	0.484	ug/l	97
52) 1,1,2-Trichloroethane	8.396	97	10566	3.349	ug/l	97
58) Tetrachloroethene	8.541	164	12701	2.814	ug/l	97
59) Chlorobenzene	9.438	112	46978	3.876	ug/l	99
63) Ethyl Benzene	9.563	91	72286	3.466	ug/l	97
64) m/p-Xylenes	9.685	106	22061	2.721	ug/l	100
65) o-Xylene	10.094	106	21152	2.715	ug/l	94
83) 1,4-Dichlorobenzene	11.833	146	12497	1.284	ug/l	96
85) 1,2-Dichlorobenzene	12.206	146	11072	1.212	ug/l	99
87) 1,2,4-Trichlorobenzene	13.836	180	19064	3.356	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063541.D
 Acq On : 18 Jul 2025 17:25
 Operator : MD/SY
 Sample : Q2552-07DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WSDL

Quant Time: Jul 18 23:52:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration


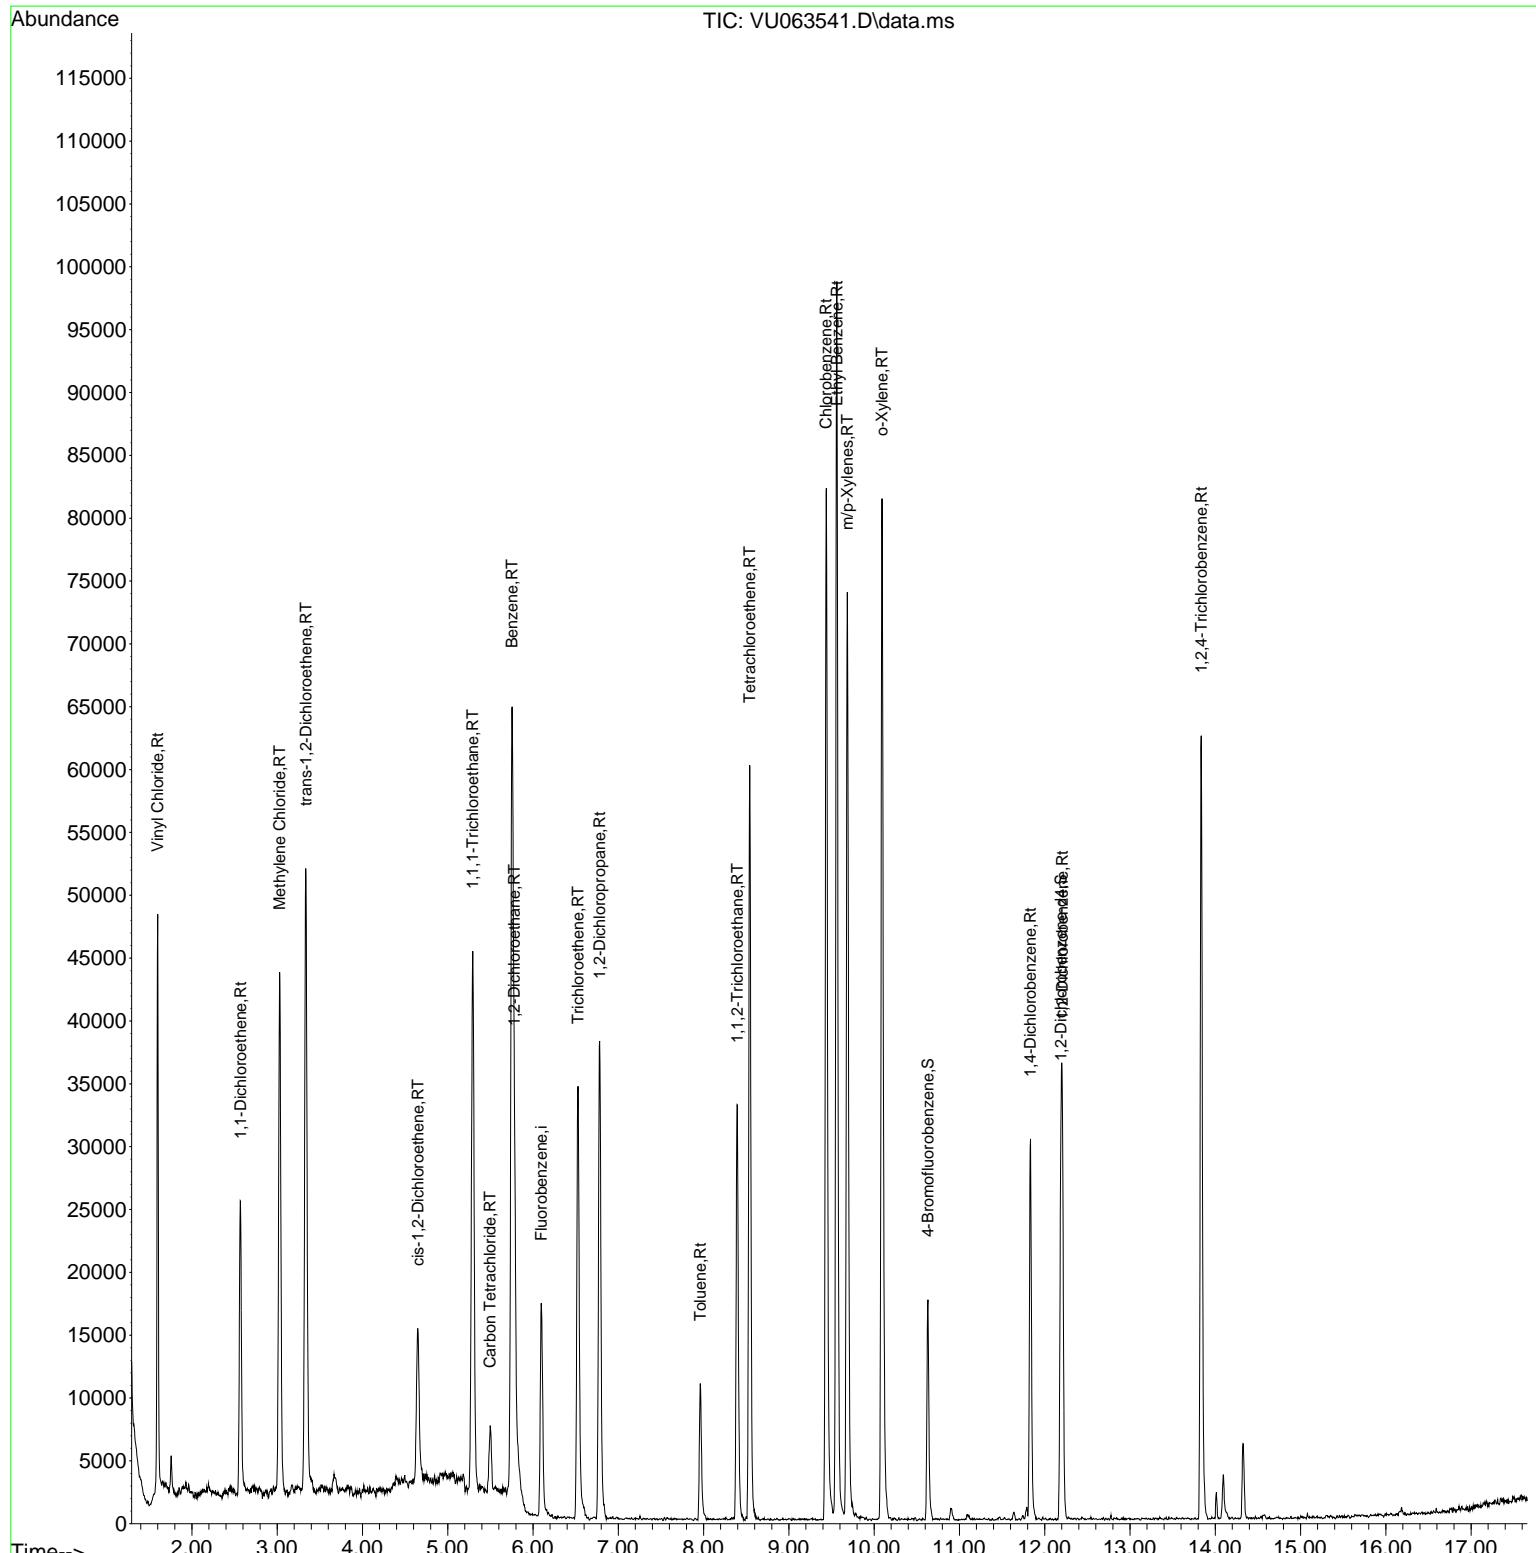


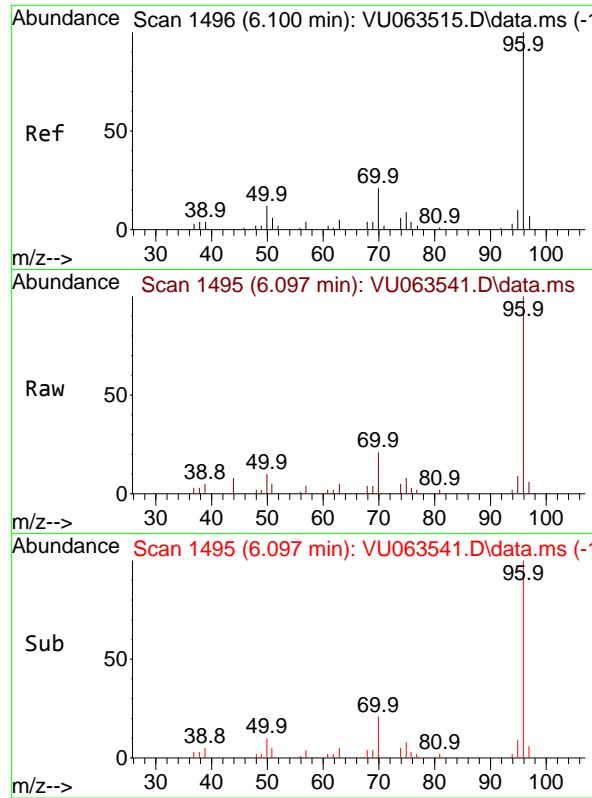

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25


Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WSDL


Tgt Ion: 96 Resp: 16405
Ion Ratio Lower Upper
96 100
70 19.2 15.0 22.4
95 8.7 7.4 11.0
97 5.5 0.0 0.0#

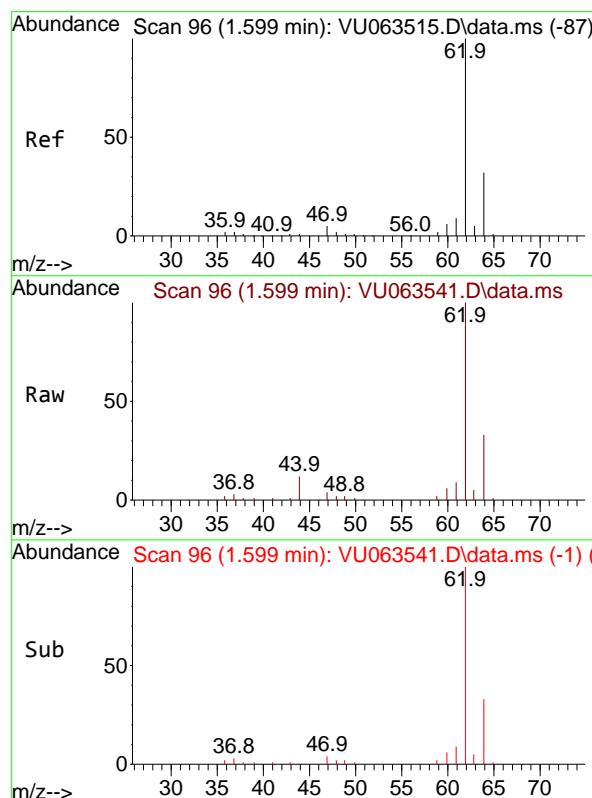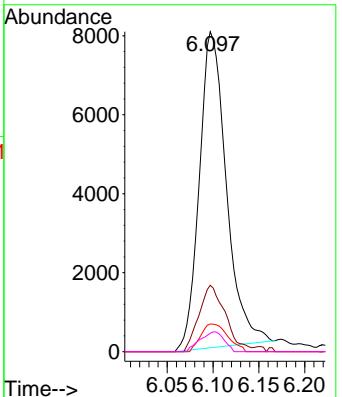


#4
Vinyl Chloride
Concen: 4.989 ug/l
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25

Tgt Ion: 62 Resp: 28569
Ion Ratio Lower Upper
62 100
64 32.6 25.7 38.5


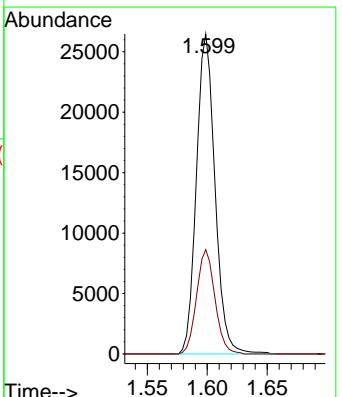





#9
1,1-Dichloroethene
Concen: 1.857 ug/l
RT: 2.570 min Scan# 3
Instrument : MSVOA_U
Delta R.T. 0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25






Tgt Ion: 96 Resp: 7910
Ion Ratio Lower Upper
96 100
61 178.5 0.0 504.3
98 66.9 0.0 126.8






#15
Methylene Chloride
Concen: 3.602 ug/l
RT: 3.030 min Scan# 541
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25

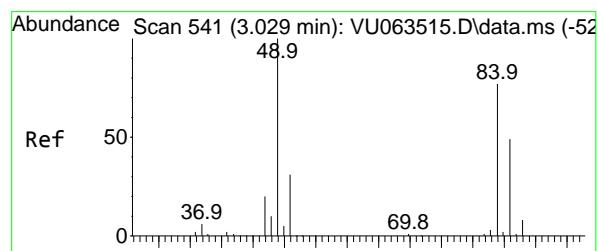

Tgt Ion: 84 Resp: 18061
Ion Ratio Lower Upper
84 100
49 132.4 103.8 155.8
51 40.2 0.0 80.4
86 64.4 51.1 76.7


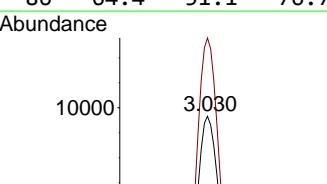
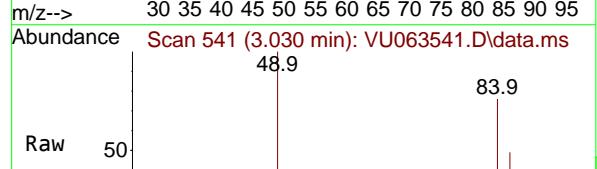
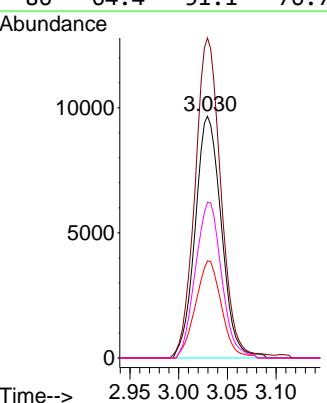


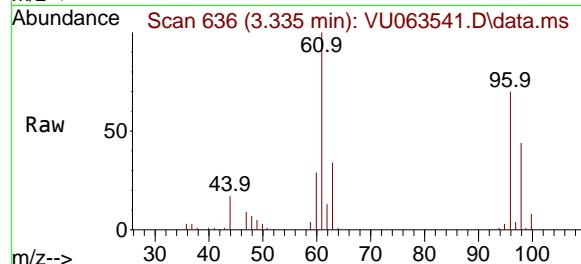

#16
trans-1,2-Dichloroethene
Concen: 4.202 ug/l
RT: 3.335 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25


Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WSDL







Tgt Ion: 96 Resp: 20327
Ion Ratio Lower Upper
96 100
61 143.8 117.2 175.8
98 63.1 51.4 77.2

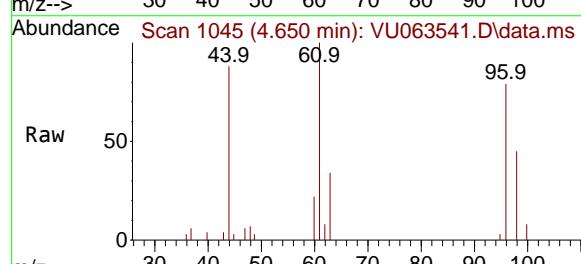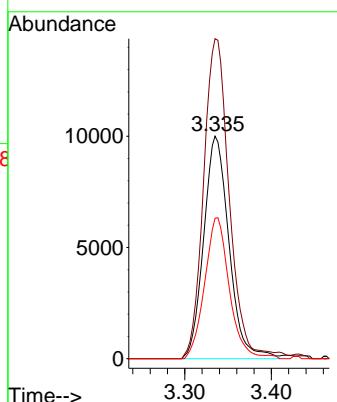

#22
cis-1,2-Dichloroethene
Concen: 1.223 ug/l
RT: 4.650 min Scan# 1045
Delta R.T. 0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25

Tgt Ion: 96 Resp: 6421
Ion Ratio Lower Upper
96 100
61 132.5 0.0 384.7
98 60.0 32.1 96.3

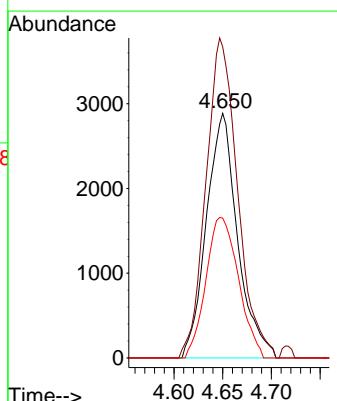




#28

1,1,1-Trichloroethane
Concen: 3.829 ug/l
RT: 5.293 min Scan# 1

Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WSDL
Acq: 18 Jul 2025 17:25


Tgt Ion: 97 Resp: 29732
Ion Ratio Lower Upper
97 100
99 63.2 31.8 95.3
61 47.8 23.3 69.9

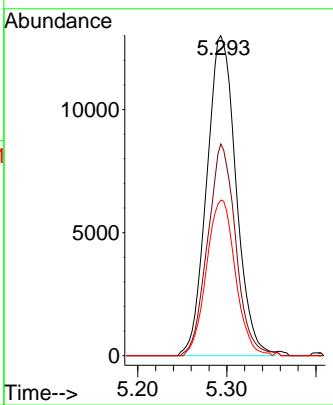


#30

Carbon Tetrachloride
Concen: 0.488 ug/l
RT: 5.496 min Scan# 1308
Delta R.T. -0.006 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25


Tgt Ion:117 Resp: 3051
Ion Ratio Lower Upper
117 100
119 99.1 79.2 118.8
121 28.5 25.5 38.3








#35
Benzene
Concen: 3.215 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25


Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WSDL





Tgt Ion: 78 Resp: 62135
Ion Ratio Lower Upper
78 100
77 23.5 19.4 29.2

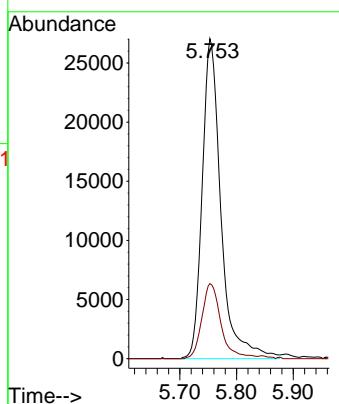


#36
1,2-Dichloroethane
Concen: 3.015 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25




Tgt Ion: 62 Resp: 18106
Ion Ratio Lower Upper
62 100
98 6.7 6.4 9.6

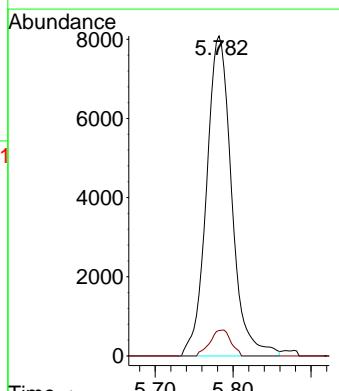





#37
Trichloroethene
Concen: 2.454 ug/l
RT: 6.528 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25


Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WSDL





Tgt Ion:130 Resp: 12102
Ion Ratio Lower Upper
130 100
95 110.2 80.3 120.5




#38
1,2-Dichloropropane
Concen: 3.344 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25

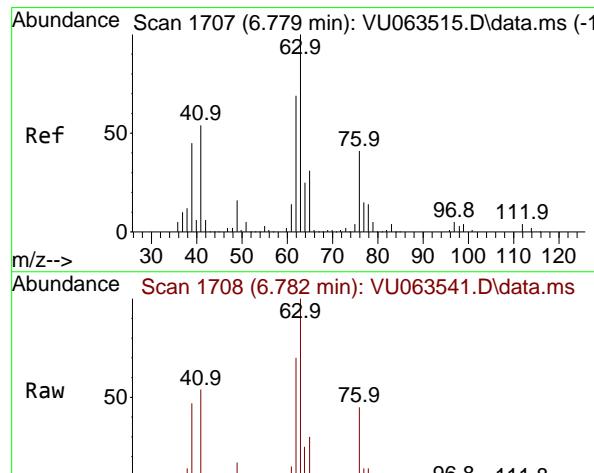


Tgt Ion: 63 Resp: 15126
Ion Ratio Lower Upper
63 100
65 30.1 24.6 36.8


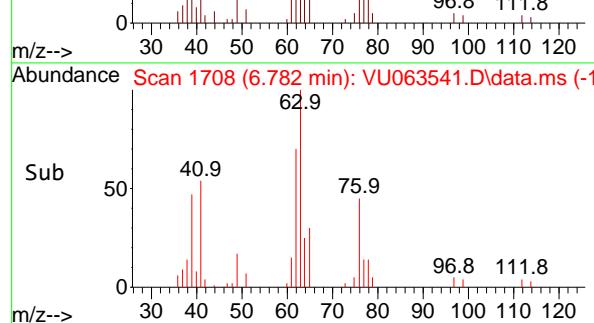
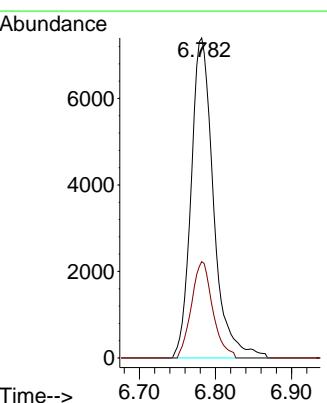





#49
Toluene
Concen: 0.484 ug/l
RT: 7.962 min Scan# 2
Instrument : MSVOA_U
Delta R.T. 0.003 min
Lab File: VU063541.D
ClientSampleId : WS0725-PT-RVOA-WSDL
Acq: 18 Jul 2025 17:25





Tgt Ion: 92 Resp: 5105
Ion Ratio Lower Upper
92 100
91 180.1 140.4 210.6

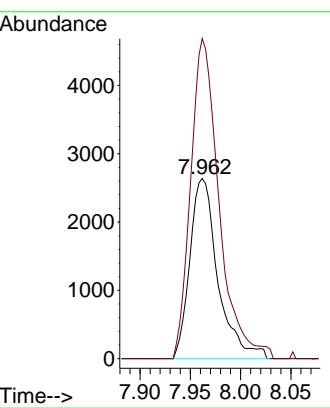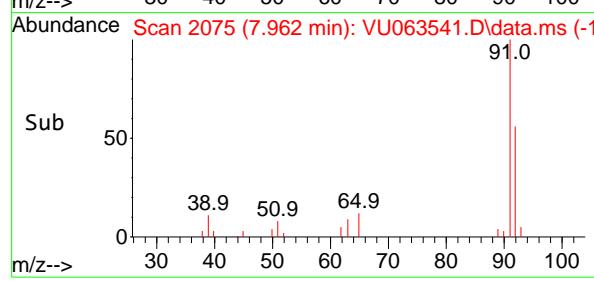


#52
1,1,2-Trichloroethane
Concen: 3.349 ug/l
RT: 8.396 min Scan# 2210
Delta R.T. 0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25



Tgt Ion: 97 Resp: 10566
Ion Ratio Lower Upper
97 100
83 82.0 70.2 105.2
85 57.9 45.2 67.8
99 61.9 50.1 75.1

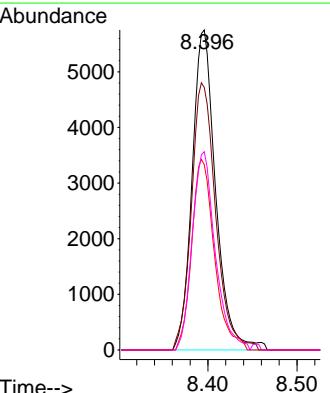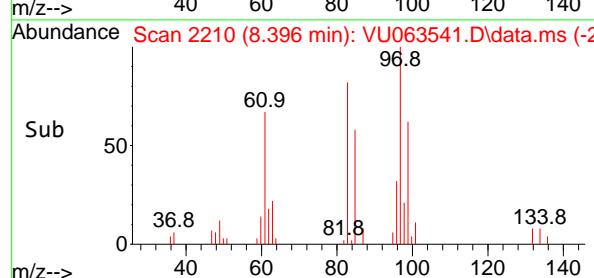

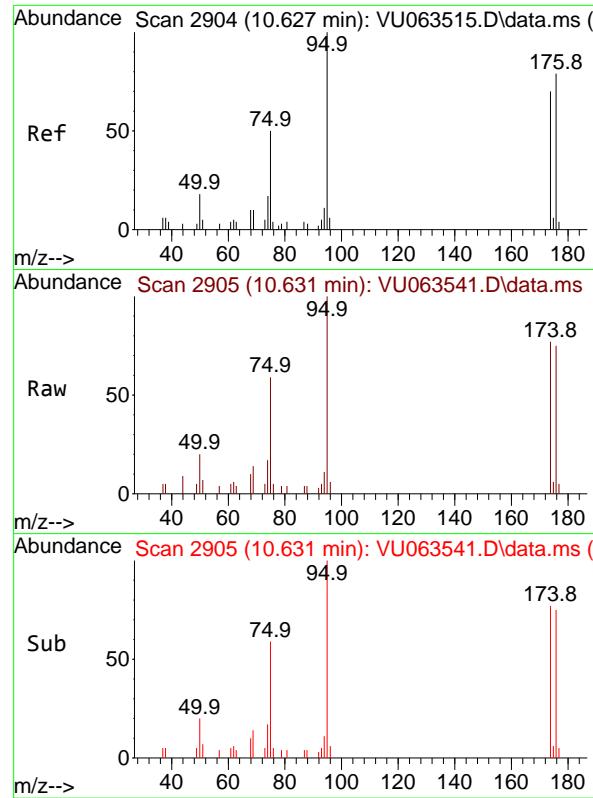

#57

4-Bromofluorobenzene

Concen: 1.034 ug/l

RT: 10.631 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063541.D

Acq: 18 Jul 2025 17:25

Instrument:

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WSDL



Tgt Ion: 95 Resp: 6421

Ion Ratio Lower Upper

95 100

174 77.6 59.8 89.8

176 72.3 61.8 92.8

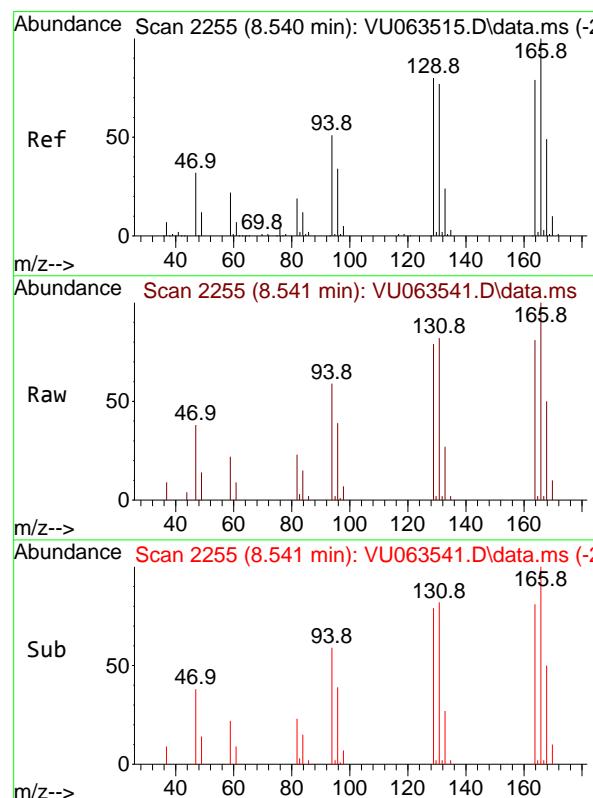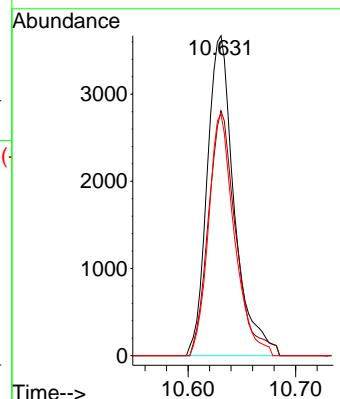

#58

Tetrachloroethene

Concen: 2.814 ug/l

RT: 8.541 min Scan# 2255

Delta R.T. 0.000 min

Lab File: VU063541.D

Acq: 18 Jul 2025 17:25

Tgt Ion: 164 Resp: 12701


Ion Ratio Lower Upper


164 100

166 123.7 100.7 151.1

129 98.0 80.6 120.8



131 101.7 77.3 115.9

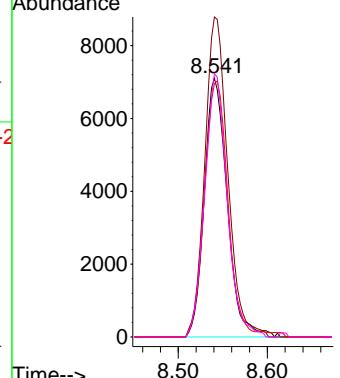

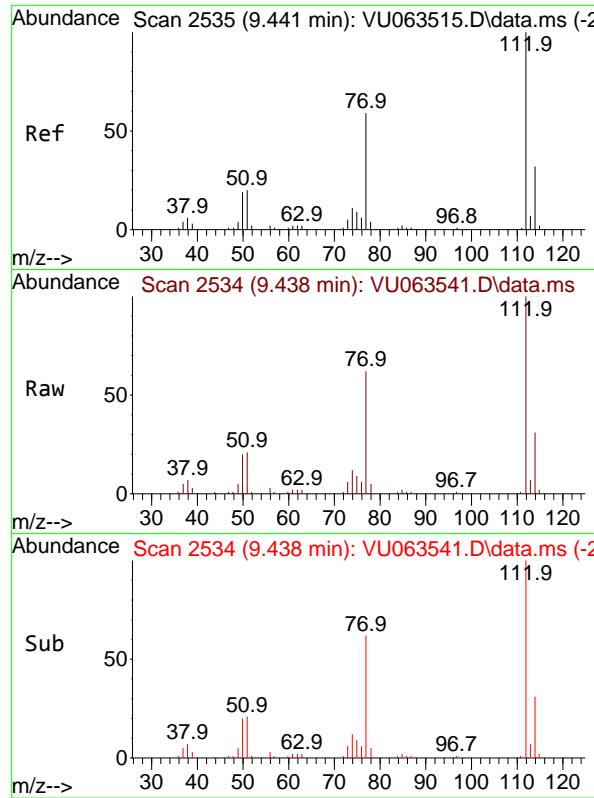


#59
Chlorobenzene
Concen: 3.876 ug/l
RT: 9.438 min Scan# 2
Instrument : MSVOA_U
Delta R.T. -0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25 ClientSampleId : WS0725-PT-RVOA-WSDL


Tgt Ion:112 Resp: 46978
Ion Ratio Lower Upper
112 100
114 31.1 25.4 38.2

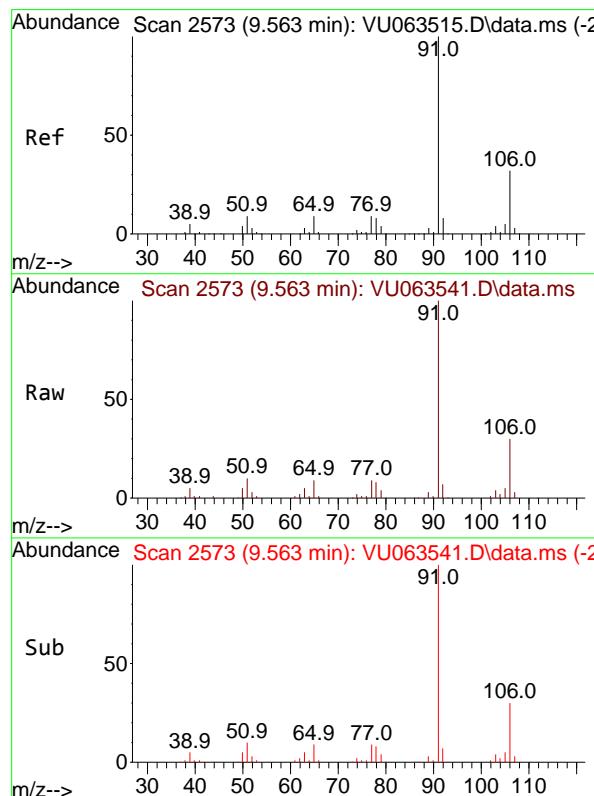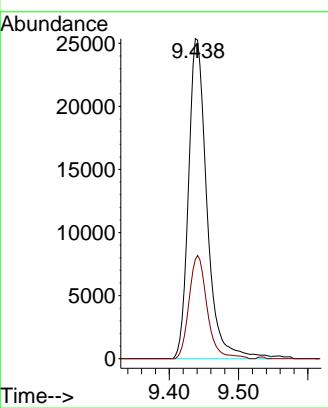

#63
Ethyl Benzene
Concen: 3.466 ug/l
RT: 9.563 min Scan# 2573
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25



Tgt Ion: 91 Resp: 72286
Ion Ratio Lower Upper
91 100
106 30.0 25.4 38.0

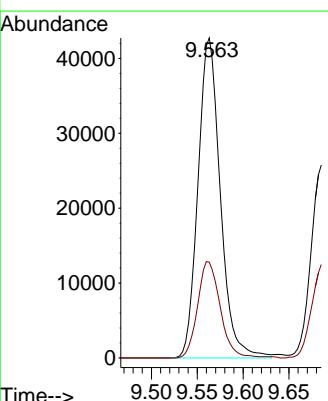

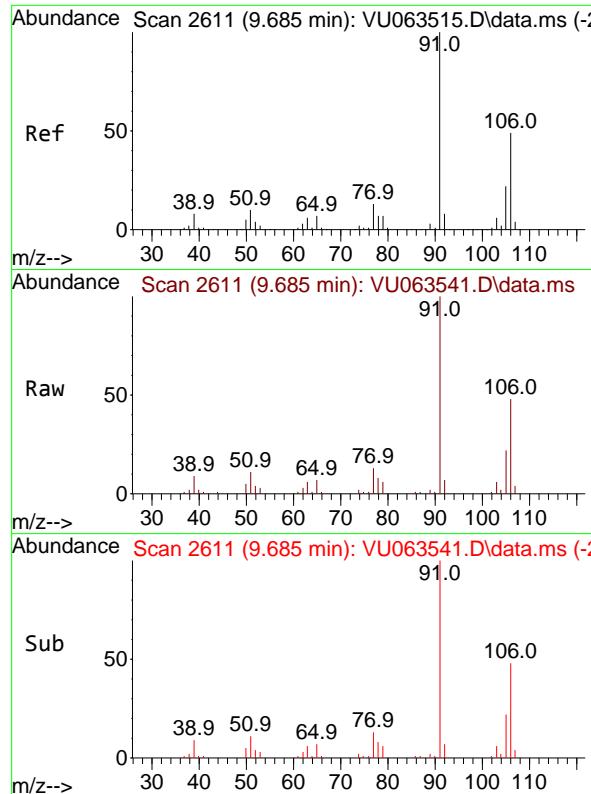


#64
m/p-Xylenes
Concen: 2.721 ug/l
RT: 9.685 min Scan# 2
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25
ClientSampleId : WS0725-PT-RVOA-WSDL


Tgt Ion:106 Resp: 22061
Ion Ratio Lower Upper
106 100
91 204.8 163.6 245.4

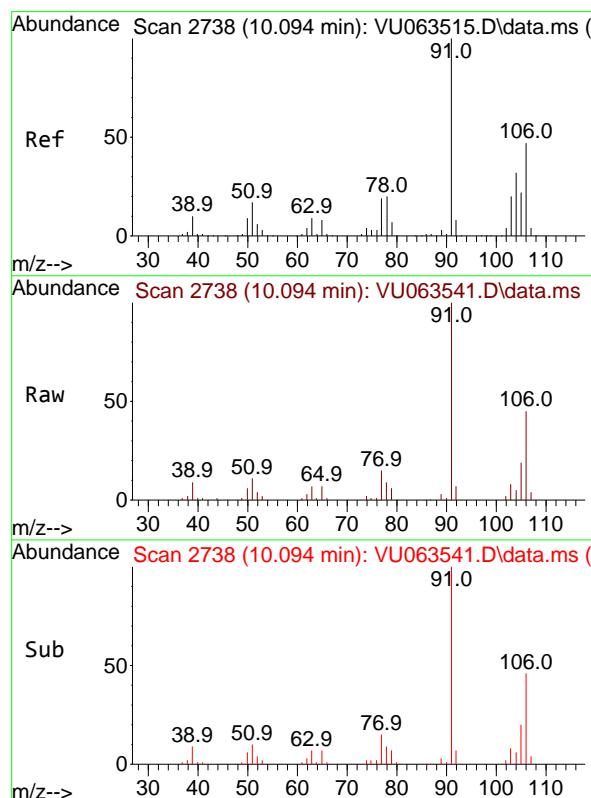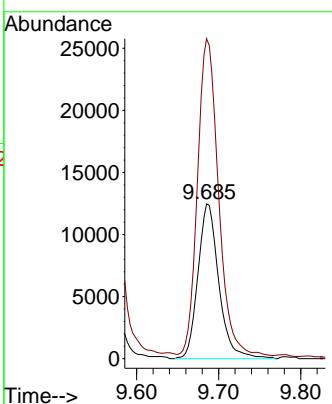

#65
o-Xylene
Concen: 2.715 ug/l
RT: 10.094 min Scan# 2738
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25

Tgt Ion:106 Resp: 21152
Ion Ratio Lower Upper
106 100
91 225.3 108.1 324.4

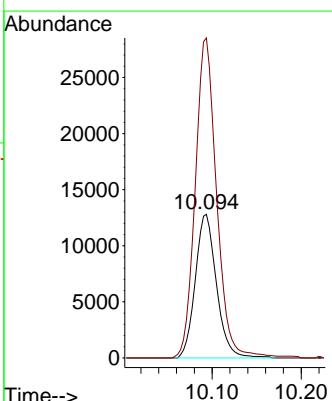

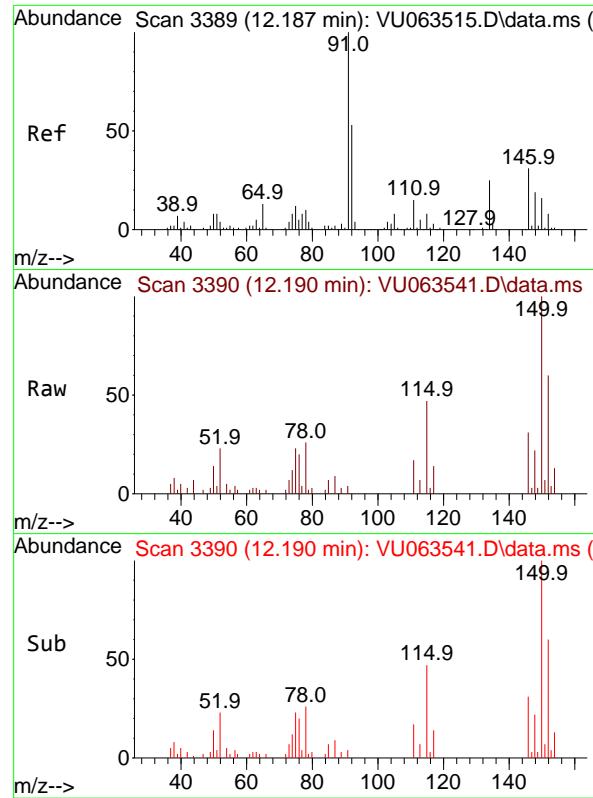

#68

1,2-Dichlorobenzene-d4

Concen: 1.024 ug/l

RT: 12.190 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063541.D

Acq: 18 Jul 2025 17:25

Instrument:

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WSDL


Tgt Ion:152 Resp: 5884

Ion Ratio Lower Upper

152 100

115 74.1 0.0 262.2

150 184.5 0.0 651.2

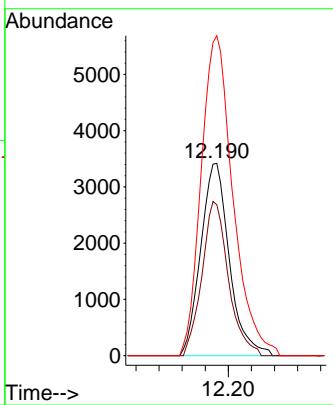

#83

1,4-Dichlorobenzene

Concen: 1.284 ug/l

RT: 11.833 min Scan# 3279

Delta R.T. 0.003 min

Lab File: VU063541.D

Acq: 18 Jul 2025 17:25



Tgt Ion:146 Resp: 12497


Ion Ratio Lower Upper

146 100

111 43.2 32.0 48.0


148 65.2 50.2 75.2

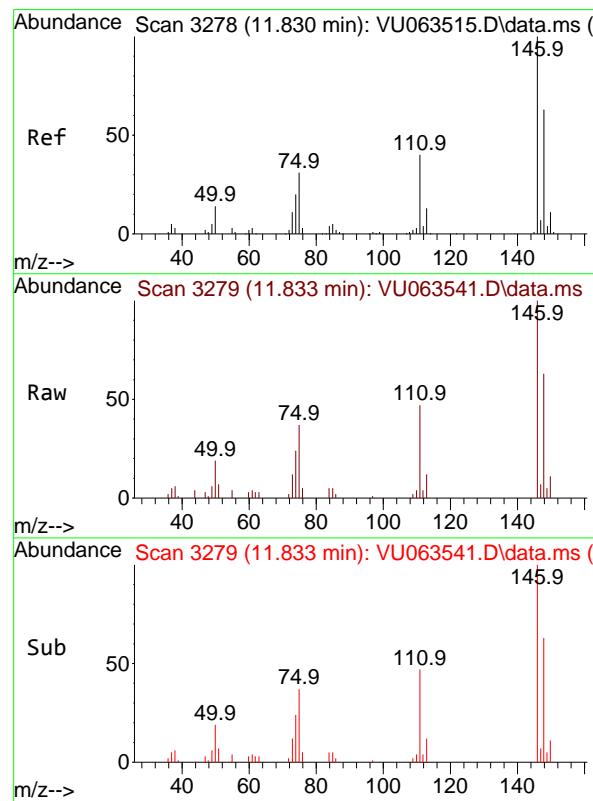

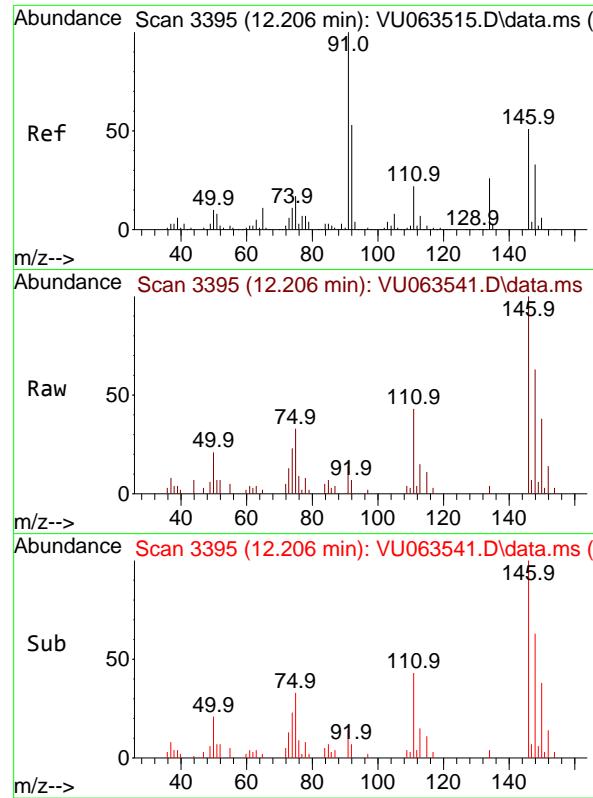


#85
1,2-Dichlorobenzene
Concen: 1.212 ug/l
RT: 12.206 min Scan# 3
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25
ClientSampleId : WS0725-PT-RVOA-WSDL

Tgt Ion:146 Resp: 11072
Ion Ratio Lower Upper
146 100
111 44.6 21.7 65.1
148 63.7 31.8 95.3




Time-->

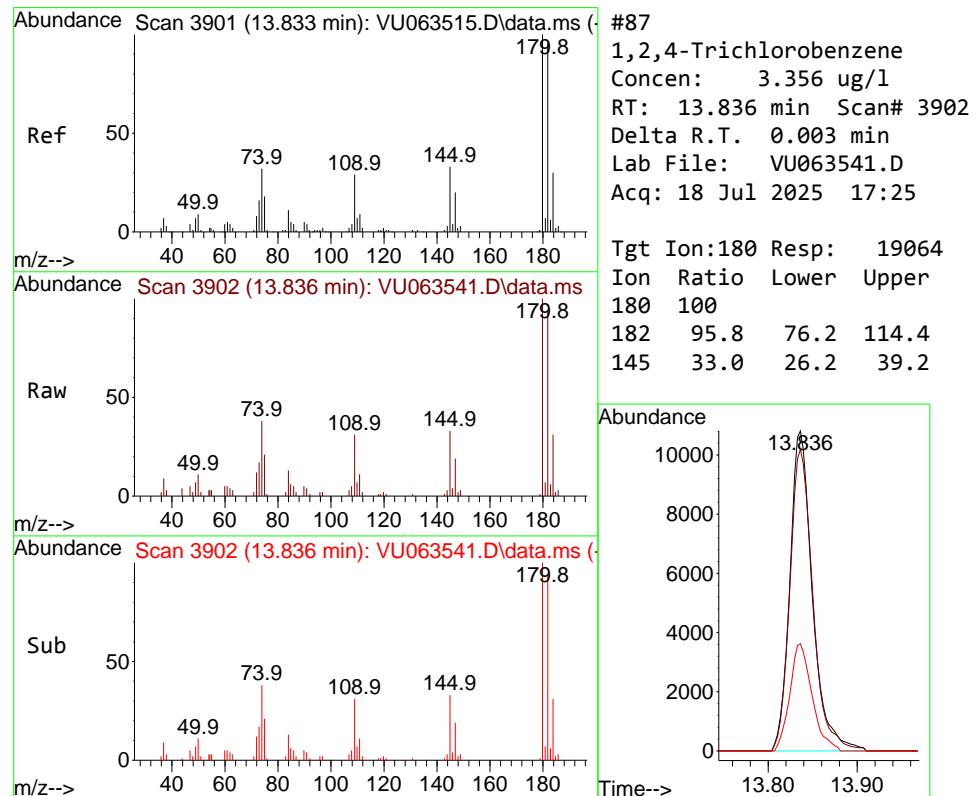

#87
1,2,4-Trichlorobenzene
Concen: 3.356 ug/l
RT: 13.836 min Scan# 3902
Delta R.T. 0.003 min
Lab File: VU063541.D
Acq: 18 Jul 2025 17:25

Tgt Ion:180 Resp: 19064
Ion Ratio Lower Upper
180 100
182 95.8 76.2 114.4
145 33.0 26.2 39.2

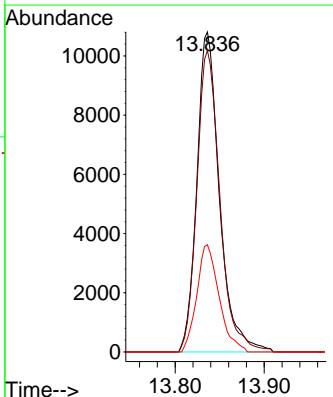

Time-->



CALIBRATION

SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date(s):	07/16/2025
Heated Purge:	(Y/N) N	Calibration Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

LAB FILE ID:	RRF0.5 = VU063511.D	RRF001 = VU063512.D	RRF002 = VU063513.D					
COMPOUND	RRF0.5	RRF001	RRF002	RRF005	RRF010	RRF015	RRF	% RSD
Dichlorodifluoromethane	0.297	0.288	0.281	0.290	0.296	0.317	0.295	4.1
Chloromethane	0.269	0.291	0.261	0.270	0.268	0.285	0.274	4.1
Vinyl Chloride	0.338	0.353	0.333	0.340	0.355	0.376	0.349	4.5
Bromomethane	0.275	0.289	0.267	0.252	0.244	0.254	0.263	6.4
Chloroethane	0.208	0.212	0.199	0.207	0.214	0.226	0.211	4.3
Tetrahydrofuran	0.079	0.054	0.054	0.050	0.052	0.055	0.057	18.6
Trichlorofluoromethane	0.493	0.508	0.471	0.494	0.509	0.532	0.501	4.1
1,1,2-Trichloro-1,2,2-trifluoroethane	0.248	0.267	0.252	0.261	0.266	0.278	0.262	4.1
tert-Butyl Alcohol		0.025	0.022	0.023	0.024	0.025	0.024	5.8
Diethyl Ether	0.172	0.202	0.194	0.199	0.206	0.213	0.198	7.2
1,1-Dichloroethene	0.260	0.262	0.241	0.256	0.265	0.274	0.260	4.3
Acrylonitrile	0.067	0.069	0.064	0.062	0.063	0.063	0.065	4.3
Acetone	0.055	0.049	0.053	0.045	0.050	0.061	0.052	10.7
Carbon Disulfide	0.817	0.848	0.786	0.819	0.861	0.900	0.839	4.8
Methyl tert-Butyl Ether	0.635	0.700	0.646	0.666	0.693	0.727	0.678	5.2
Methyl acrylate	0.162	0.161	0.140	0.152	0.168	0.174	0.160	7.7
Methylene Chloride	0.327	0.328	0.287	0.290	0.293	0.308	0.306	6.1
trans-1,2-Dichloroethene	0.287	0.312	0.278	0.284	0.298	0.310	0.295	4.7
1,1-Dichloroethane	0.530	0.569	0.520	0.539	0.549	0.572	0.546	3.8
Cyclohexane	0.451	0.495	0.435	0.449	0.462	0.484	0.463	4.9
2-Butanone	0.080	0.081	0.079	0.074	0.080	0.090	0.081	6.4
Carbon Tetrachloride	0.333	0.383	0.362	0.381	0.392	0.435	0.381	8.8
2,2-Dichloropropane	0.482	0.487	0.447	0.433	0.454	0.489	0.465	5.1
cis-1,2-Dichloroethene	0.310	0.347	0.298	0.309	0.320	0.335	0.320	5.6
Bromochloromethane	0.128	0.131	0.127	0.132	0.138	0.145	0.134	5.1
Chloroform	0.551	0.584	0.537	0.543	0.547	0.583	0.558	3.7
1,1,1-Trichloroethane	0.457	0.477	0.449	0.471	0.482	0.505	0.473	4.2
Methylcyclohexane	0.442	0.440	0.402	0.406	0.490	0.519	0.450	10.3
1,1-Dichloropropene	0.413	0.455	0.432	0.430	0.434	0.468	0.438	4.5
Propionitrile	0.025	0.026	0.024	0.025	0.023	0.024	0.025	3.8

* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date(s):	07/16/2025 07/16/2025
Heated Purge:	(Y/N) N	Calibration Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

LAB FILE ID:	RRF0.5 = VU063511.D	RRF001 = VU063512.D	RRF002 = VU063513.D					
COMPOUND	RRF0.5	RRF001	RRF002	RRF005	RRF010	RRF015	RRF	% RSD
Benzene	1.218	1.011	1.165	1.205	1.202	1.269	1.178	7.5
1,2-Dichloroethane	0.360	0.332	0.363	0.371	0.376	0.394	0.366	5.7
Trichloroethene	0.314	0.283	0.269	0.271	0.323	0.345	0.301	10.3
1,2-Dichloropropane	0.235	0.261	0.251	0.258	0.315	0.334	0.276	14.4
1-Chlorobutane	0.575	0.575	0.553	0.583	0.591	0.621	0.583	3.9
Dibromomethane	0.132	0.134	0.131	0.138	0.154	0.168	0.143	10.4
Bromodichloromethane	0.304	0.304	0.300	0.310	0.328	0.388	0.322	10.4
4-Methyl-2-Pentanone	0.136	0.147	0.136	0.146	0.152	0.166	0.147	7.8
Toluene	0.582	0.650	0.596	0.642	0.671	0.718	0.643	7.8
t-1,3-Dichloropropene	0.213	0.231	0.223	0.250	0.285	0.313	0.253	15.5
cis-1,3-Dichloropropene	0.284	0.311	0.292	0.334	0.362	0.452	0.339	18.4
1,1,2-Trichloroethane	0.173	0.197	0.180	0.191	0.202	0.211	0.192	7.4
1,3-Dichloropropane	0.310	0.327	0.318	0.330	0.344	0.364	0.332	5.8
2-Hexanone	0.090	0.097	0.087	0.096	0.103	0.114	0.098	10
Dibromochloromethane	0.165	0.184	0.185	0.206	0.232	0.248	0.203	15.5
1,2-Dibromoethane	0.164	0.169	0.161	0.171	0.179	0.189	0.172	5.9
Tetrachloroethene	0.254	0.279	0.266	0.270	0.285	0.295	0.275	5.4
Chlorobenzene	0.680	0.735	0.686	0.732	0.771	0.828	0.739	7.5
1,1,1,2-Tetrachloroethane	0.211	0.236	0.218	0.233	0.254	0.273	0.238	9.6
Hexachloroethane	0.134	0.146	0.143	0.170	0.192	0.213	0.166	18.7
Ethyl Benzene	1.195	1.261	1.191	1.259	1.314	1.408	1.271	6.4
m/p-Xylenes	0.459	0.470	0.464	0.488	0.519	0.564	0.494	8.2
o-Xylene	0.428	0.462	0.432	0.473	0.504	0.550	0.475	9.8
Styrene	0.649	0.715	0.690	0.764	0.823	0.900	0.757	12.2
Bromoform	0.096	0.085	0.092	0.105	0.118	0.131	0.104	16.8
Isopropylbenzene	1.016	1.118	1.057	1.148	1.230	1.318	1.148	9.7
1,1,2,2-Tetrachloroethane	0.222	0.229	0.217	0.230	0.243	0.264	0.234	7.3
1,2,3-Trichloropropane	0.171	0.198	0.182	0.177	0.208	0.204	0.190	8
Bromobenzene	0.284	0.283	0.265	0.293	0.309	0.343	0.296	9.1
n-propylbenzene	0.303	0.327	0.323	0.344	0.375	0.402	0.346	10.6

* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date(s):	07/16/2025
Heated Purge:	(Y/N) N	Calibration Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

LAB FILE ID:	RRF0.5 = VU063511.D	RRF001 = VU063512.D	RRF002 = VU063513.D					
COMPOUND	RRF0.5	RRF001	RRF002	RRF005	RRF010	RRF015	RRF	% RSD
2-Chlorotoluene	0.278	0.298	0.285	0.301	0.322	0.349	0.305	8.6
1,3,5-Trimethylbenzene	0.966	1.036	1.013	1.102	1.182	1.280	1.097	10.7
4-Chlorotoluene	0.269	0.300	0.296	0.311	0.330	0.355	0.310	9.5
tert-Butylbenzene	0.954	0.987	0.975	1.042	1.123	1.207	1.048	9.4
1,2,4-Trimethylbenzene	0.953	1.029	1.004	1.096	1.178	1.268	1.088	10.8
sec-Butylbenzene	1.226	1.376	1.304	1.417	1.516	1.641	1.413	10.5
p-Isopropyltoluene	1.023	1.104	1.091	1.202	1.275	1.384	1.180	11.3
1,3-Dichlorobenzene	0.539	0.571	0.543	0.594	0.629	0.681	0.593	9.2
1,4-Dichlorobenzene	0.512	0.572	0.539	0.590	0.635	0.711	0.593	12.1
n-Butylbenzene	0.933	1.004	0.985	1.113	1.211	1.319	1.094	13.6
1,2-Dichlorobenzene	0.504	0.538	0.502	0.552	0.597	0.649	0.557	10.2
1,2-Dibromo-3-Chloropropane	0.024	0.027	0.031	0.034	0.040	0.044	0.033	23.1
1,2,4-Trichlorobenzene	0.304	0.313	0.310	0.341	0.385	0.425	0.346	14.1
Hexachlorobutadiene	0.179	0.185	0.180	0.195	0.211	0.231	0.197	10.5
Naphthalene		0.533	0.520	0.587	0.679	0.785	0.621	17.9
1,2,3-Trichlorobenzene	0.269	0.294	0.283	0.321	0.352	0.400	0.320	15.3
Nitrobenzene	0.002	0.004	0.003	0.004	0.005	0.006	0.004	34.4
1,2-Dichlorobenzene-d4	0.318	0.364	0.326	0.342	0.359	0.392	0.350	7.7
4-Bromofluorobenzene	0.373	0.410	0.361	0.361	0.369	0.398	0.379	5.4
Iodomethane		0.238	0.241	0.306	0.369	0.413	0.314	24.7
Allyl Chloride	0.346	0.373	0.389	0.359	0.382	0.401	0.375	5.4
t-1,4-Dichloro-2-butene	0.052	0.060	0.050	0.051	0.063	0.056	0.055	9.3
Methacrylonitrile	0.139	0.105	0.107	0.096	0.101	0.106	0.109	13.9
Ethyl methacrylate	0.206	0.200	0.218	0.226	0.252	0.271	0.229	11.9
Isopropyl Ether	0.796	0.855	0.789	0.810	0.831	0.867	0.825	3.9
Methyl methacrylate	0.107	0.107	0.108	0.117	0.127	0.154	0.120	15.3

* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA_U\Method\

Method File : 524U071625DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Last Update : Thu Jul 17 03:49:40 2025

Response Via : Initial Calibration

Calibration Files

0.5 =VU063511.D 1 =VU063512.D 2 =VU063513.D 5 =VU063514.D 10 =VU063515.D 15 =VU063516.D

	Compound	0.5	1	2	5	10	15	Avg	%RSD
<hr/>									
1) i	Fluorobenzene				-----ISTD-----				
2) T	Dichlorodifluo...	0.297	0.288	0.281	0.290	0.296	0.317	0.295	4.12
3) t	Chloromethane	0.269	0.291	0.261	0.270	0.268	0.285	0.274	4.08
4) Rt	Vinyl Chloride	0.338	0.353	0.333	0.340	0.355	0.376	0.349	4.46
5) T	Bromomethane	0.275	0.289	0.267	0.252	0.244	0.254	0.263	6.39
6) T	Chloroethane	0.208	0.212	0.199	0.207	0.214	0.226	0.211	4.25
7) T	Trichlorofluor...	0.493	0.508	0.471	0.494	0.509	0.532	0.501	4.10
8)	1,1,2-Trichlor...	0.248	0.267	0.252	0.261	0.266	0.278	0.262	4.11
9) Rt	1,1-Dichloroet...	0.260	0.262	0.241	0.256	0.265	0.274	0.260	4.27
10) t	Iodomethane		0.238	0.241	0.306	0.369	0.413	0.314	24.71
11) t	Allyl Chloride	0.346	0.373	0.389	0.359	0.382	0.401	0.375	5.38
12) t	Acrylonitrile	0.067	0.069	0.064	0.062	0.063	0.063	0.065	4.27
13) T	Acetone	0.055	0.049	0.053	0.045	0.050	0.061	0.052	10.71
14) T	Carbon Disulfide	0.817	0.848	0.786	0.819	0.861	0.900	0.839	4.77
15) RT	Methylene Chlo...	0.327	0.328	0.287	0.290	0.293	0.308	0.306	6.09
16) RT	trans-1,2-Dich...	0.287	0.312	0.278	0.284	0.298	0.310	0.295	4.69
17) t	1,1-Dichloroet...	0.530	0.569	0.520	0.539	0.549	0.572	0.546	3.82
18) T	2-Butanone	0.080	0.081	0.079	0.074	0.080	0.090	0.081	6.36
19)	Cyclohexane	0.451	0.495	0.435	0.449	0.462	0.484	0.463	4.90
20)	Methylcyclohexane	0.442	0.440	0.402	0.406	0.490	0.519	0.450	10.30
21) T	2,2-Dichloropr...	0.482	0.487	0.447	0.433	0.454	0.489	0.465	5.09
22) RT	cis-1,2-Dichlo...	0.310	0.347	0.298	0.309	0.320	0.335	0.320	5.63
23) t	Diethyl Ether	0.172	0.202	0.194	0.199	0.206	0.213	0.198	7.18
24) t	tert-Butyl Alc...		0.025	0.022	0.023	0.024	0.025	0.024	5.81
25) t	Methyl tert-Bu...	0.635	0.700	0.646	0.666	0.693	0.727	0.678	5.16
26) t	Bromochloromet...	0.128	0.131	0.127	0.132	0.137	0.145	0.134	5.06
27) t	Chloroform	0.551	0.584	0.537	0.543	0.547	0.583	0.558	3.73
28) RT	1,1,1-Trichlor...	0.457	0.477	0.449	0.471	0.482	0.505	0.473	4.20
29) T	1,1-Dichloropr...	0.413	0.455	0.432	0.430	0.434	0.468	0.438	4.51
30) RT	Carbon Tetrach...	0.333	0.383	0.362	0.381	0.392	0.435	0.381	8.80
31) t	Isopropyl Ether	0.796	0.855	0.789	0.810	0.831	0.867	0.825	3.86
32)	Ethyl-t-butyl ...	0.739	0.800	0.735	0.725	0.769	0.811	0.763	4.73
33)	Tert-Amyl meth...	0.683	0.601	0.655	0.652	0.666	0.719	0.663	5.88
34) t	Propionitrile	0.025	0.026	0.024	0.025	0.023	0.024	0.025	3.80
35) RT	Benzene	1.218	1.011	1.165	1.205	1.202	1.269	1.178	7.52
36) RT	1,2-Dichloroet...	0.360	0.332	0.363	0.371	0.376	0.394	0.366	5.67
37) RT	Trichloroethene	0.314	0.283	0.269	0.271	0.323	0.345	0.301	10.31
38) Rt	1,2-Dichloropr...	0.235	0.261	0.251	0.258	0.315	0.334	0.276	14.35
39) t	Methacrylonitrile	0.139	0.105	0.107	0.096	0.101	0.106	0.109	13.89
40) t	Methyl acrylate	0.162	0.161	0.140	0.152	0.168	0.174	0.159	7.70
41) t	Tetrahydrofuran	0.079	0.054	0.054	0.050	0.052	0.055	0.057	18.63
42) t	1-Chlorobutane	0.575	0.575	0.553	0.583	0.591	0.621	0.583	3.91
43) T	Dibromomethane	0.132	0.134	0.131	0.138	0.154	0.168	0.143	10.38
44) T	Bromodichlorom...	0.304	0.304	0.300	0.310	0.328	0.388	0.322	10.45
45) T	4-Methyl-2-Pen...	0.136	0.147	0.136	0.146	0.152	0.166	0.147	7.83
46) t	t-1,4-Dichloro...	0.052	0.060	0.050	0.051	0.063	0.056	0.055	9.32
47) t	Methyl methacr...	0.107	0.107	0.108	0.117	0.127	0.154	0.120	15.28
48) t	Ethyl methacry...	0.206	0.200	0.218	0.226	0.252	0.271	0.229	11.94
49) Rt	Toluene	0.582	0.650	0.596	0.642	0.671	0.718	0.643	7.75
50) T	t-1,3-Dichloro...	0.213	0.231	0.223	0.250	0.285	0.313	0.253	15.47
51) T	cis-1,3-Dichlo...	0.284	0.311	0.292	0.334	0.362	0.452	0.339	18.37
52) RT	1,1,2-Trichlor...	0.173	0.197	0.180	0.191	0.202	0.211	0.192	7.42
53) t	1,3-Dichloropr...	0.310	0.327	0.318	0.330	0.344	0.364	0.332	5.82
54) t	2-Hexanone	0.090	0.097	0.087	0.096	0.103	0.114	0.098	9.98
55) t	Dibromochlorom...	0.165	0.184	0.185	0.206	0.232	0.248	0.203	15.53
56) T	1,2-Dibromoethane	0.164	0.169	0.161	0.171	0.179	0.189	0.172	5.92
57) S	4-Bromofluorob...	0.373	0.410	0.361	0.361	0.369	0.398	0.379	5.40

Method Path : Z:\voasrv\HPCHEM1\MSVOA_U\Method\


Method File : 524U071625DW.M

58)	RT	Tetrachloroethene	0.254	0.279	0.266	0.270	0.285	0.295	0.275	5.39
59)	Rt	Chlorobenzene	0.680	0.735	0.686	0.732	0.771	0.828	0.739	7.52
60)	T	1,1,1,2-Tetrac...	0.211	0.236	0.218	0.233	0.254	0.273	0.238	9.63
61)	t	Pentachloroethane	0.148	0.150	0.148	0.169	0.186	0.207	0.168	14.57
62)	t	Hexachloroethane	0.134	0.146	0.143	0.170	0.192	0.213	0.166	18.74
63)	Rt	Ethyl Benzene	1.195	1.261	1.191	1.259	1.314	1.408	1.271	6.40
64)	RT	m/p-Xylenes	0.459	0.470	0.464	0.488	0.519	0.564	0.494	8.22
65)	RT	o-Xylene	0.428	0.462	0.432	0.473	0.504	0.550	0.475	9.75
66)	RT	Styrene	0.649	0.715	0.690	0.764	0.823	0.900	0.757	12.22
67)	t	Bromoform	0.096	0.085	0.092	0.105	0.118	0.131	0.104	16.81
68)	S	1,2-Dichlorobe...	0.318	0.364	0.326	0.342	0.359	0.392	0.350	7.68
69)	T	Isopropylbenzene	1.016	1.118	1.057	1.148	1.230	1.318	1.148	9.72
70)	T	1,1,2,2-Tetrac...	0.222	0.229	0.217	0.230	0.243	0.264	0.234	7.34
71)	T	1,2,3-Trichlor...	0.171	0.198	0.182	0.177	0.208	0.204	0.190	8.02
72)	t	Bromobenzene	0.284	0.283	0.265	0.293	0.309	0.343	0.296	9.11
73)	t	n-propylbenzene	0.303	0.327	0.323	0.344	0.375	0.402	0.346	10.58
74)	t	2-Chlorotoluene	0.278	0.298	0.285	0.301	0.322	0.349	0.305	8.59
75)	t	1,3,5-Trimethyl...	0.966	1.036	1.013	1.102	1.182	1.280	1.097	10.69
76)	t	4-Chlorotoluene	0.269	0.300	0.296	0.311	0.330	0.355	0.310	9.49
77)	t	tert-Butylbenzene	0.954	0.987	0.975	1.042	1.123	1.207	1.048	9.44
78)	t	1,2,4-Trimethyl...	0.953	1.029	1.004	1.096	1.178	1.268	1.088	10.83
79)	t	sec-Butylbenzene	1.226	1.376	1.304	1.417	1.516	1.641	1.413	10.53
80)		Nitrobenzene	0.002	0.004	0.003	0.004	0.005	0.006	0.004	34.42
81)	t	p-Isopropyltol...	1.023	1.104	1.091	1.202	1.275	1.384	1.180	11.33
82)	t	1,3-Dichlorobe...	0.539	0.571	0.543	0.594	0.629	0.681	0.593	9.16
83)	Rt	1,4-Dichlorobe...	0.512	0.572	0.539	0.590	0.635	0.711	0.593	12.06
84)	t	n-Butylbenzene	0.933	1.004	0.985	1.113	1.210	1.319	1.094	13.57
85)	Rt	1,2-Dichlorobe...	0.504	0.538	0.502	0.552	0.597	0.649	0.557	10.23
86)	t	1,2-Dibromo-3....	0.024	0.027	0.031	0.034	0.040	0.044	0.033	23.11
87)	Rt	1,2,4-Trichlor...	0.304	0.313	0.310	0.341	0.385	0.425	0.346	14.06
88)	t	Hexachlorobuta...	0.179	0.185	0.180	0.195	0.211	0.231	0.197	10.50
89)	t	Naphthalene	0.533	0.520	0.587	0.679	0.785	0.621		17.89
90)	t	1,2,3-Trichlor...	0.269	0.294	0.283	0.321	0.352	0.400	0.320	15.31

(#) = Out of Range

1, 2-Dibromo-3-Chloropropane


Response Ratio

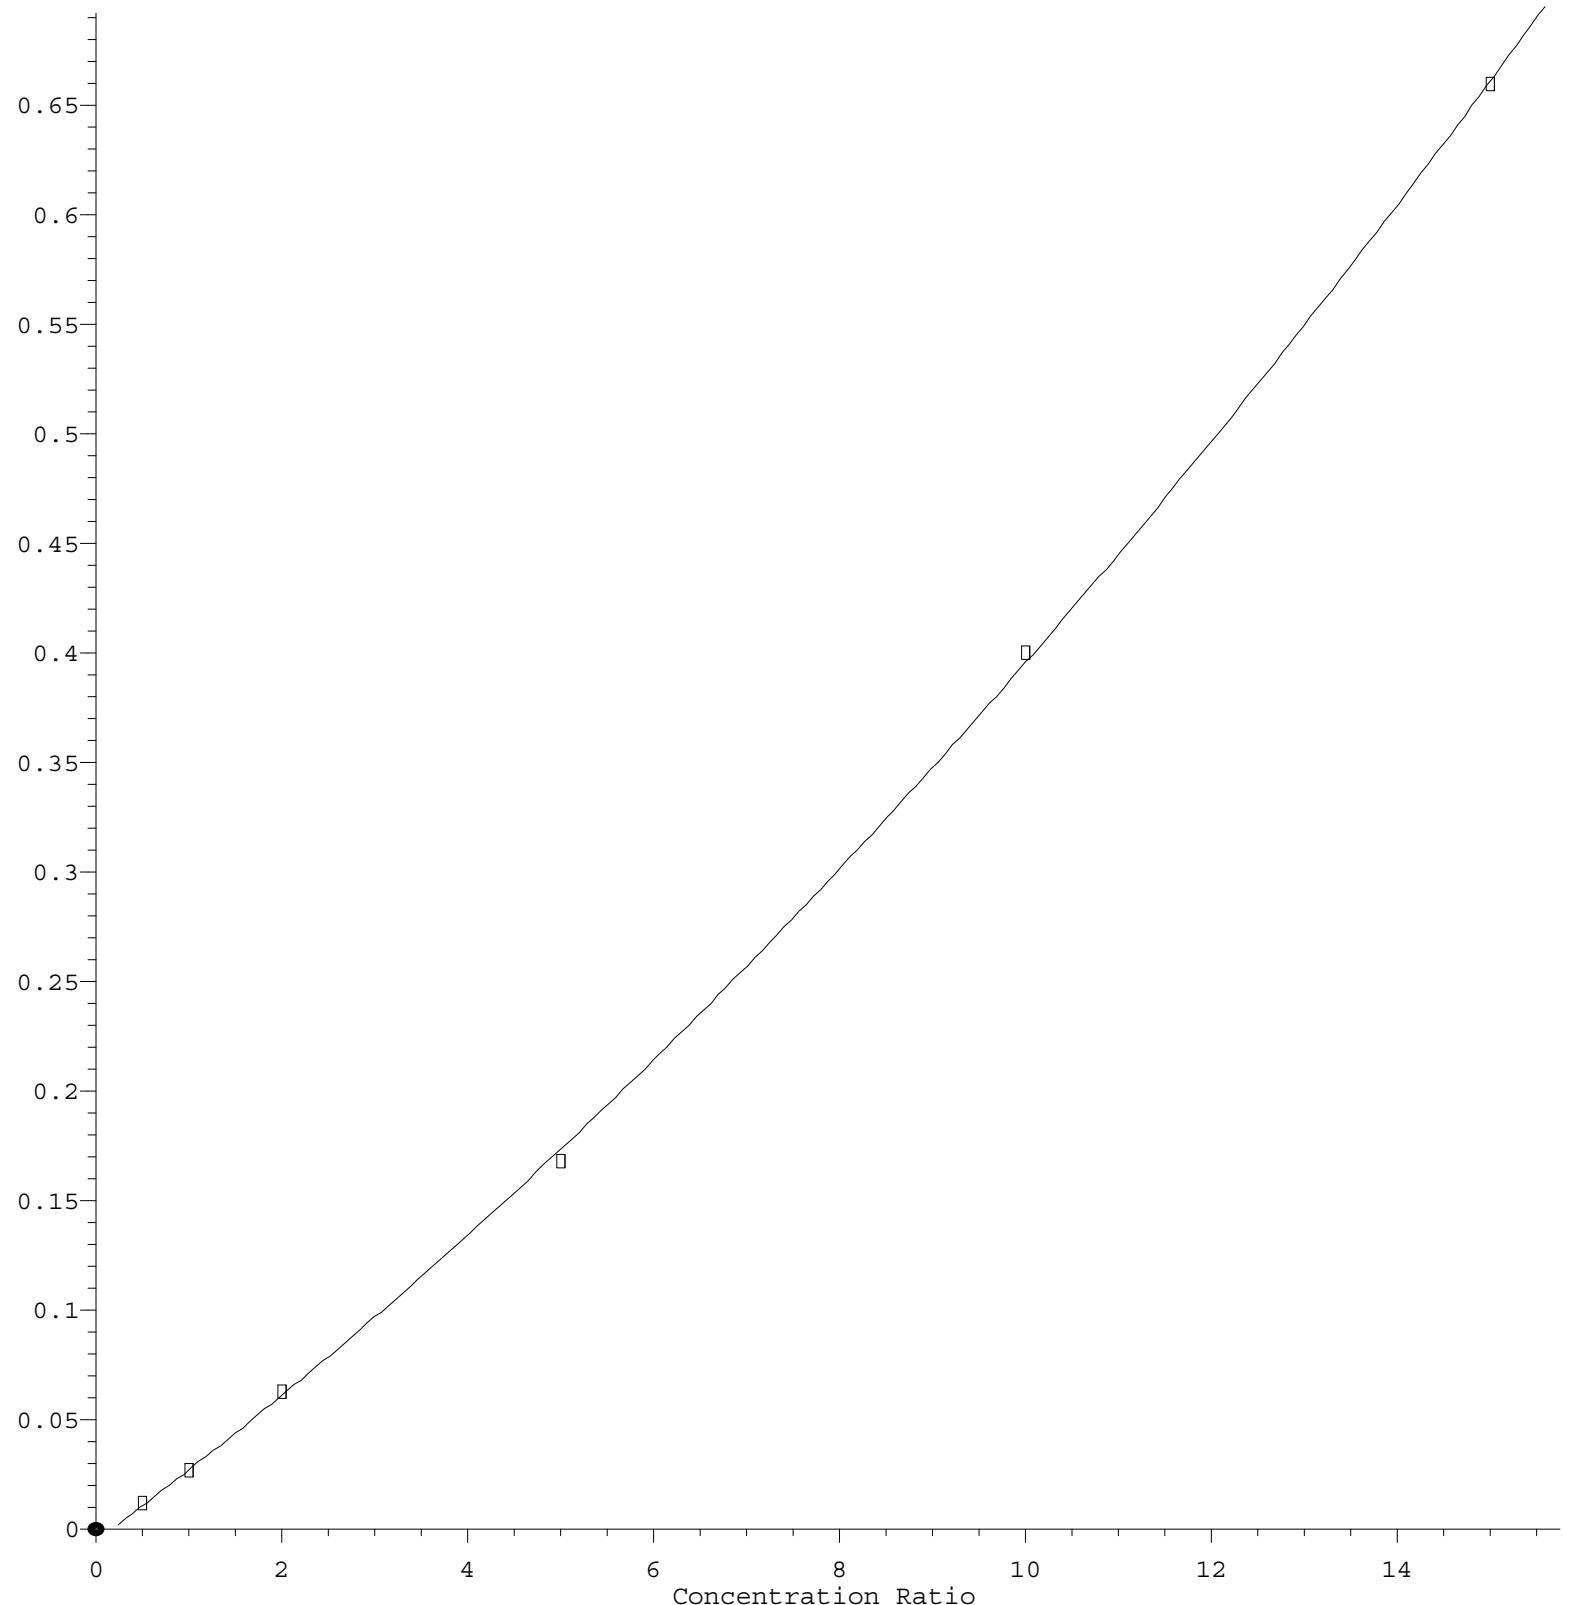

R = 8.705e-004 A*A + 3.135e-002 A - 5.068e-003
Coef of Det (r^2) = 0.999831 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U071625DW.M
Calibration Table Last Updated: Thu Jul 17 03:49:40 2025


Nitrobenzene

Response Ratio

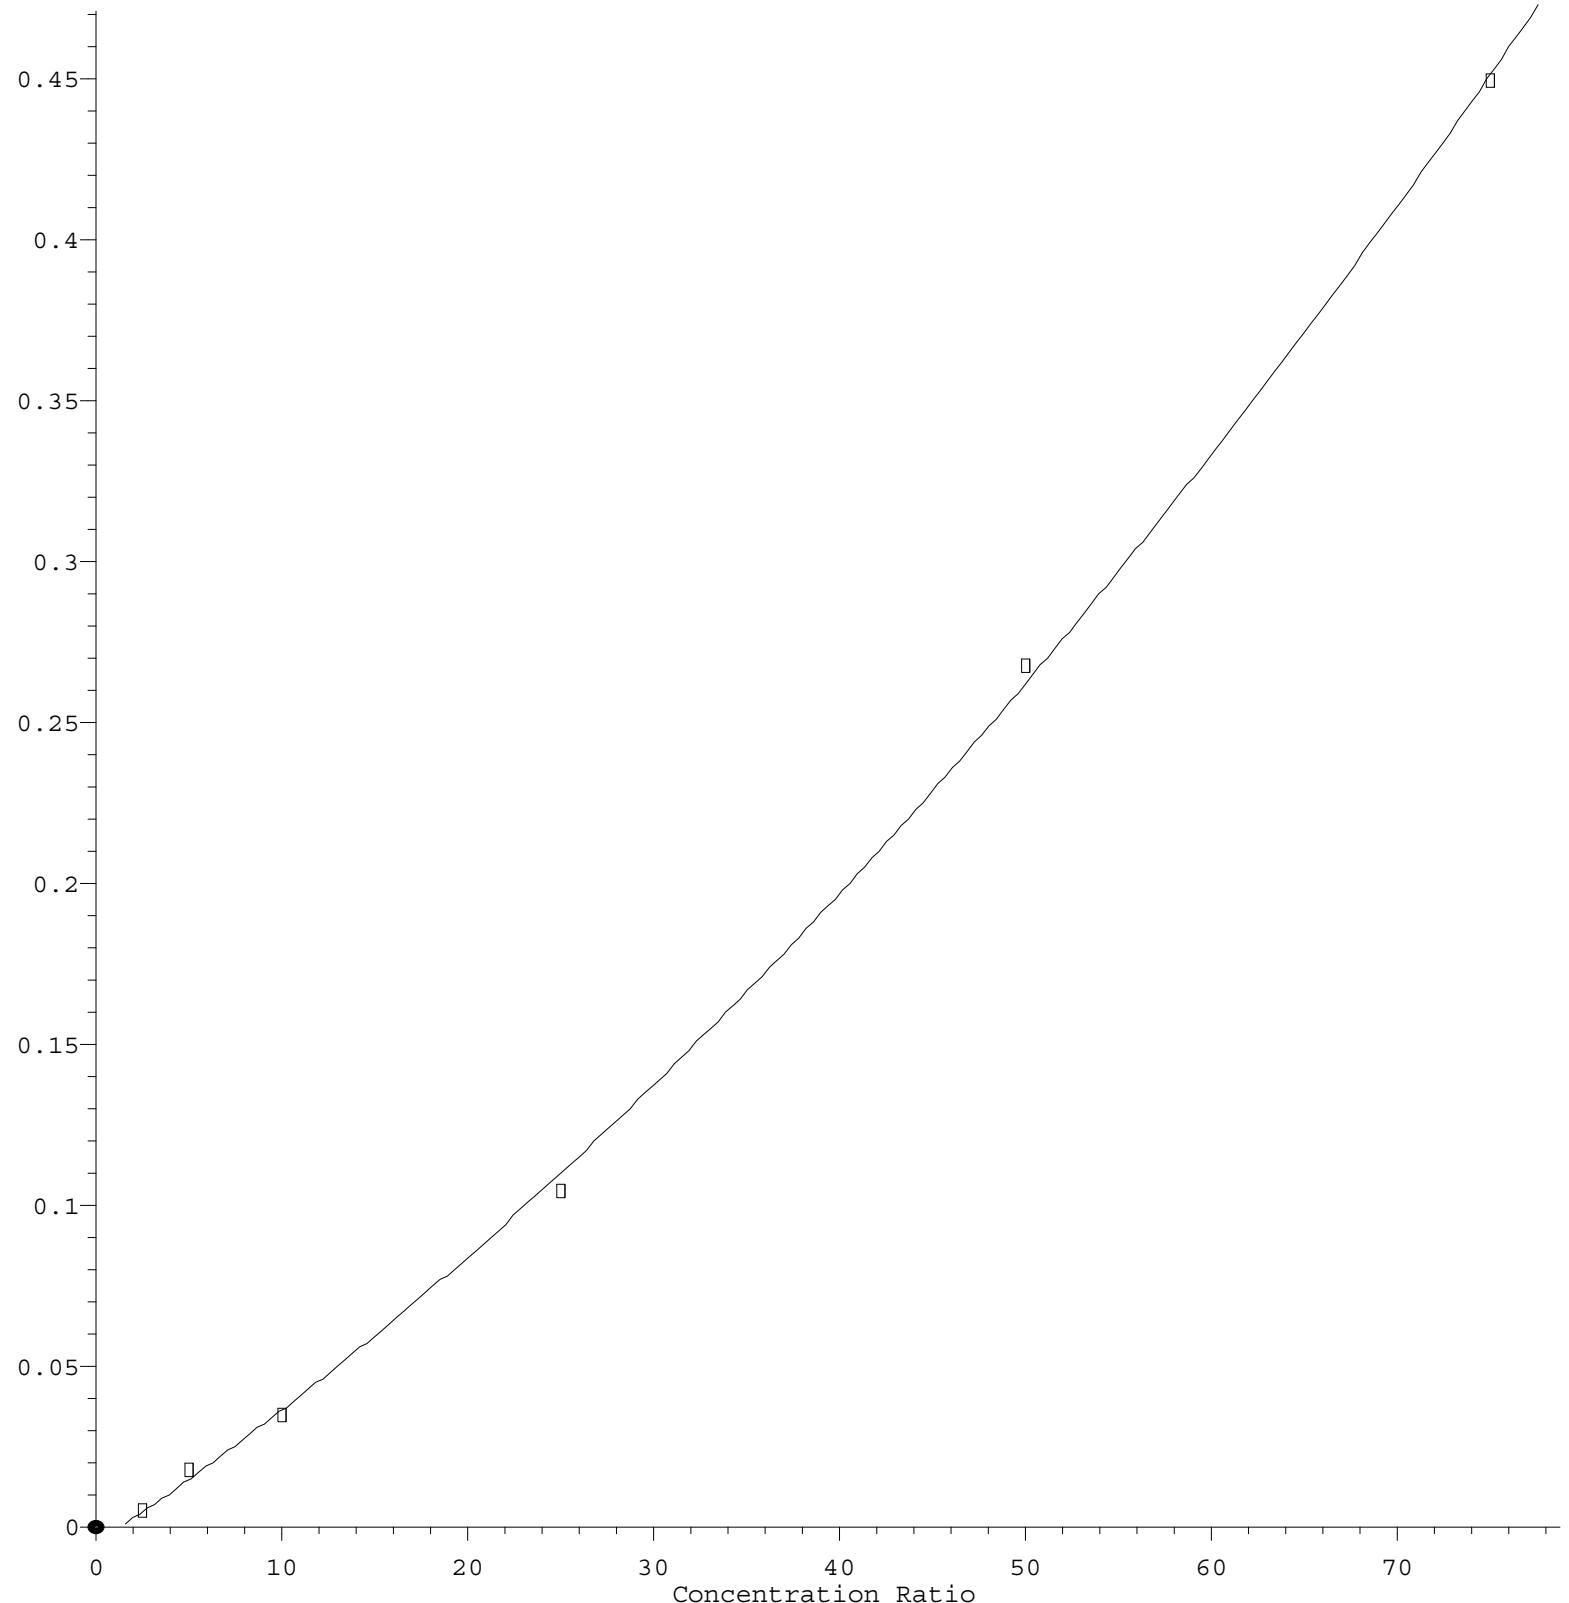

R = 2.957e-005 A*A + 3.869e-003 A - 5.219e-003
Coef of Det (r^2) = 0.999519 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U071625DW.M
Calibration Table Last Updated: Thu Jul 17 03:49:40 2025

Iodomethane

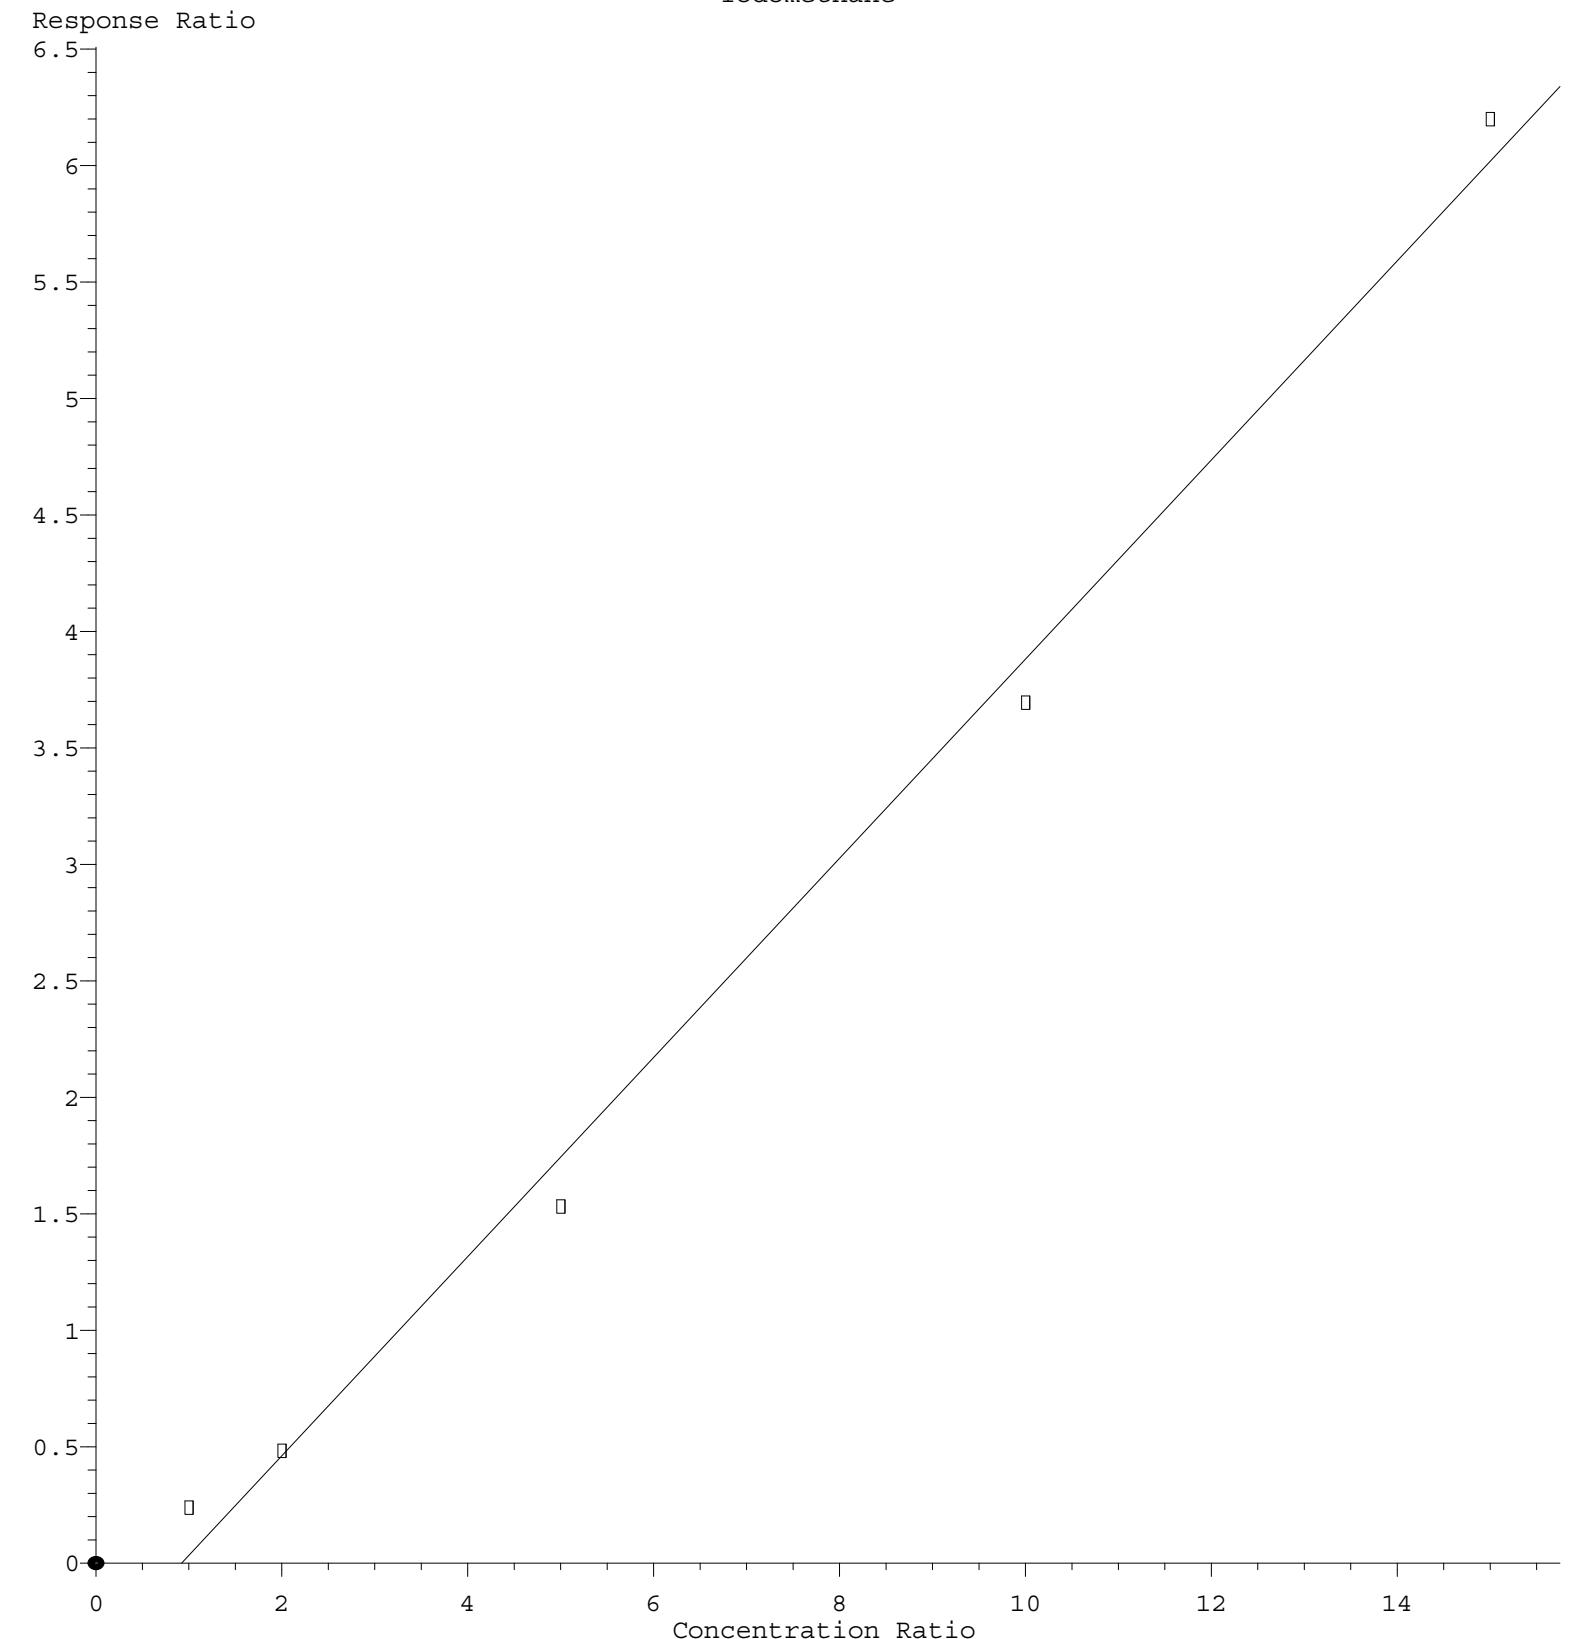

Response = 4.273e-001 * Amt - 3.914e-001
Coef of Det (r^2) = 0.993851 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U071625DW.M
Calibration Table Last Updated: Thu Jul 17 03:49:40 2025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063511.D
 Acq On : 16 Jul 2025 09:24
 Operator : MD/SY
 Sample : VSTDICC0.5
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC0.5

Quant Time: Jul 17 03:21:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.100	96	25423	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	9489	0.986	ug/l	0.00
Spiked Amount 1.000			Recovery	=	99.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	8092	0.909	ug/l	0.00
Spiked Amount 1.000			Recovery	=	91.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	3779	0.504	ug/l	95
3) Chloromethane	1.518	50	3425	0.492	ug/l	97
4) Vinyl Chloride	1.599	62	4301	0.485	ug/l	98
5) Bromomethane	1.850	94	3492	0.522	ug/l	92
6) Chloroethane	1.927	64	2643	0.493	ug/l	94
7) Trichlorofluoromethane	2.129	101	6269	0.492	ug/l	97
8) 1,1,2-Trichloro-1,2,2-...	2.570	101	3157	0.474	ug/l	97
9) 1,1-Dichloroethene	2.570	96	3303	0.500	ug/l	91
11) Allyl Chloride	2.911	41	4399	0.461	ug/l	97
12) Acrylonitrile	3.309	53	1715m	1.038	ug/l	
13) Acetone	2.618	43	3474	2.627	ug/l	98
14) Carbon Disulfide	2.782	76	10386	0.487	ug/l	99
15) Methylene Chloride	3.030	84	4161	0.535	ug/l	97
16) trans-1,2-Dichloroethene	3.338	96	3653	0.487	ug/l	92
17) 1,1-Dichloroethane	3.853	63	6739	0.485	ug/l	99
18) 2-Butanone	4.711	43	5053	2.467	ug/l	99
19) Cyclohexane	5.364	56	5734	0.487	ug/l	94
20) Methylcyclohexane	6.740	83	5613	0.491	ug/l	97
21) 2,2-Dichloropropane	4.644	77	6127	0.518	ug/l	97
22) cis-1,2-Dichloroethene	4.647	96	3941	0.484	ug/l	95
23) Diethyl Ether	2.370	59	2188	0.435	ug/l	# 82
25) Methyl tert-Butyl Ether	3.361	73	8075	0.469	ug/l	# 91
26) Bromochloromethane	4.956	128	1623	0.478	ug/l	93
27) Chloroform	5.075	83	7007	0.494	ug/l	98
28) 1,1,1-Trichloroethane	5.296	97	5809	0.483	ug/l	99
29) 1,1-Dichloropropene	5.505	75	5244	0.470	ug/l	# 91
30) Carbon Tetrachloride	5.505	117	4239	0.438	ug/l	95
31) Isopropyl Ether	3.994	45	10123	0.483	ug/l	100
32) Ethyl-t-butyl ether	4.502	59	9396	0.484	ug/l	97
33) Tert-Amyl methyl ether	5.943	73	8680	0.515	ug/l	97
34) Propionitrile	4.779	54	1601m	2.565	ug/l	
35) Benzene	5.759	78	15477	0.517	ug/l	96
36) 1,2-Dichloroethane	5.782	62	4577	0.492	ug/l	99
37) Trichloroethene	6.528	130	3989	0.522	ug/l	95
38) 1,2-Dichloropropane	6.782	63	2987	0.426	ug/l	91
39) Methacrylonitrile	4.981	41	1767m	0.645	ug/l	
40) Methyl acrylate	4.846	55	2059	0.508	ug/l	# 88
41) Tetrahydrofuran	5.062	42	2008	1.376	ug/l	# 77
42) 1-Chlorobutane	5.441	56	7303	0.493	ug/l	93
43) Dibromomethane	6.907	93	1679	0.462	ug/l	94
44) Bromodichloromethane	7.097	83	3861	0.471	ug/l	95
45) 4-Methyl-2-Pentanone	7.801	43	8613	2.301	ug/l	98
46) t-1,4-Dichloro-2-butene	10.827	75	1314m	0.990	ug/l	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063511.D
 Acq On : 16 Jul 2025 09:24
 Operator : MD/SY
 Sample : VSTDICC0.5
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC0.5

Quant Time: Jul 17 03:21:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
47) Methyl methacrylate	6.968	69	2712	0.889	ug/l	89
48) Ethyl methacrylate	8.341	69	2622	0.451	ug/l	82
49) Toluene	7.965	92	7397	0.452	ug/l	100
50) t-1,3-Dichloropropene	8.209	75	2708	0.421	ug/l	94
51) cis-1,3-Dichloropropene	7.602	75	3613	0.419	ug/l	93
52) 1,1,2-Trichloroethane	8.396	97	2194	0.449	ug/l	94
53) 1,3-Dichloropropane	8.570	76	3944	0.467	ug/l	96
54) 2-Hexanone	8.698	43	5691	2.289	ug/l	98
55) Dibromochloromethane	8.804	129	2097	0.406	ug/l	97
56) 1,2-Dibromoethane	8.920	107	2089	0.477	ug/l	92
58) Tetrachloroethene	8.544	164	3225	0.461	ug/l	95
59) Chlorobenzene	9.441	112	8639	0.460	ug/l	99
60) 1,1,1,2-Tetrachloroethane	9.528	131	2686	0.445	ug/l	99
61) Pentachloroethane	11.418	117	1880	0.441	ug/l	98
62) Hexachloroethane	12.467	117	1703	0.403	ug/l	99
63) Ethyl Benzene	9.566	91	15188	0.470	ug/l	95
64) m/p-Xylenes	9.689	106	11672	0.929	ug/l	91
65) o-Xylene	10.094	106	5435	0.450	ug/l	100
66) Styrene	10.113	104	8244	0.429	ug/l	100
67) Bromoform	10.283	173	1214	0.458	ug/l #	90
69) Isopropylbenzene	10.476	105	12913	0.442	ug/l	94
70) 1,1,2,2-Tetrachloroethane	10.775	83	2820	0.474	ug/l #	87
71) 1,2,3-Trichloropropene	10.817	75	2178m	0.449	ug/l	
72) Bromobenzene	10.778	156	3609	0.479	ug/l	93
73) n-propylbenzene	10.901	120	3852	0.438	ug/l	93
74) 2-Chlorotoluene	10.981	126	3528	0.454	ug/l	96
75) 1,3,5-Trimethylbenzene	11.081	105	12281	0.441	ug/l	99
76) 4-Chlorotoluene	11.097	126	3423	0.434	ug/l	99
77) tert-Butylbenzene	11.412	119	12124	0.455	ug/l	98
78) 1,2,4-Trimethylbenzene	11.463	105	12110	0.438	ug/l	99
79) sec-Butylbenzene	11.637	105	15578	0.434	ug/l	98
80) Nitrobenzene	13.229	77	131	2.628	ug/l #	44
81) p-Isopropyltoluene	11.785	119	13001	0.433	ug/l	97
82) 1,3-Dichlorobenzene	11.743	146	6856	0.455	ug/l	97
83) 1,4-Dichlorobenzene	11.836	146	6510	0.432	ug/l	95
84) n-Butylbenzene	12.206	91	11864	0.427	ug/l	96
85) 1,2-Dichlorobenzene	12.206	146	6401	0.452	ug/l	97
86) 1,2-Dibromo-3-Chloropr...	12.991	75	302	0.533	ug/l	88
87) 1,2,4-Trichlorobenzene	13.843	180	3867	0.439	ug/l	98
88) Hexachlorobutadiene	14.013	225	2280	0.456	ug/l	92
90) 1,2,3-Trichlorobenzene	14.331	180	3421	0.420	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063511.D
Acq On : 16 Jul 2025 09:24
Operator : MD/SY
Sample : VSTDICC0.5
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC0.5

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

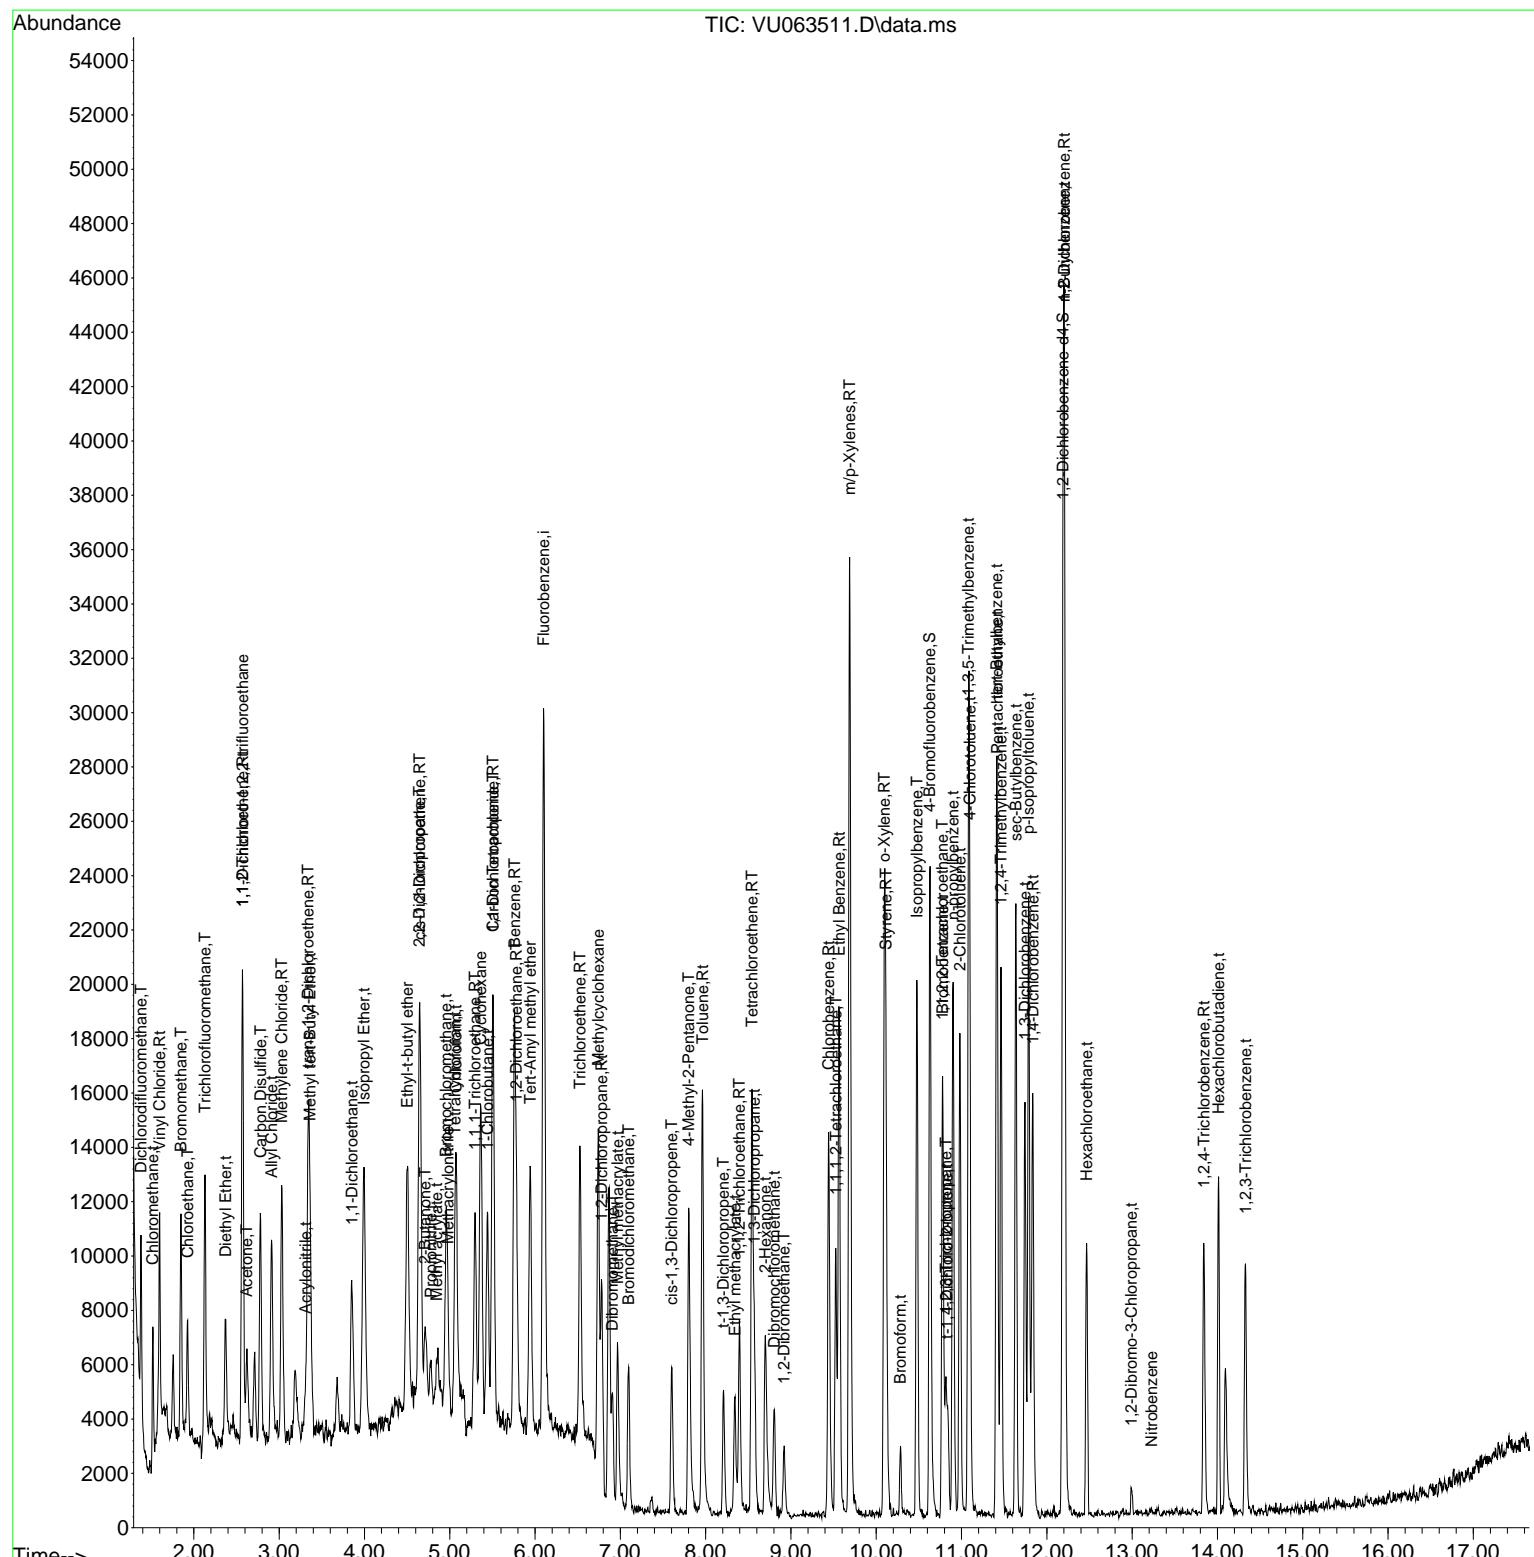

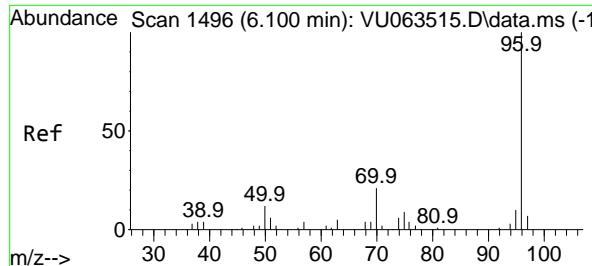

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5






Tgt Ion: 96 Resp: 25421

Ion Ratio Lower Upper


Ion	Ratio	Lower	Upper
96	100		
70	20.1	15.0	22.4
95	9.4	7.4	11.0
97	6.7	0.0	0.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

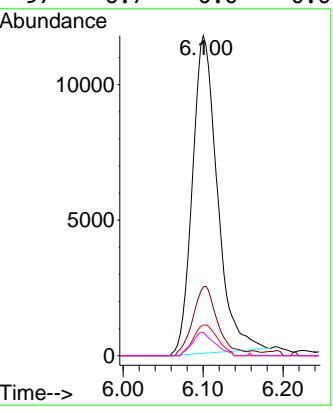
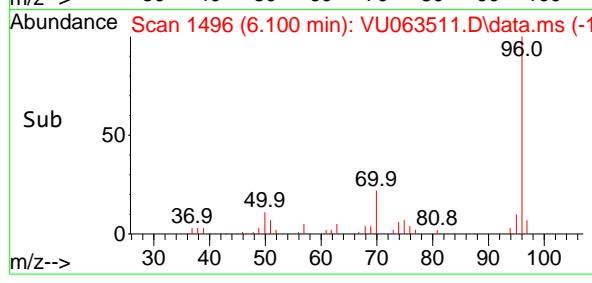





#2
Dichlorodifluoromethane
Concen: 0.504 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24



Tgt Ion: 85 Resp: 3779

Ion	Ratio	Lower	Upper
85	100		
87	34.5	16.0	47.9





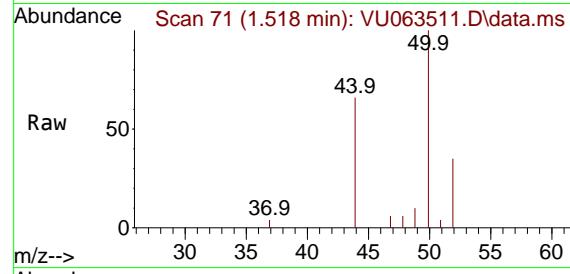



#3
Chloromethane
Concen: 0.492 ug/l
RT: 1.518 min Scan# 7
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument :
MSVOA_U
ClientSampleId :
VSTDICCO.5


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#4
Vinyl Chloride
Concen: 0.485 ug/l
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Tgt Ion: 62 Resp: 4301
Ion Ratio Lower Upper
62 100
64 33.1 25.7 38.5

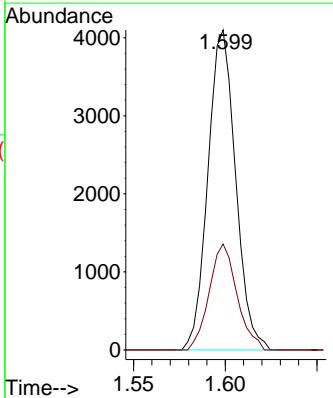

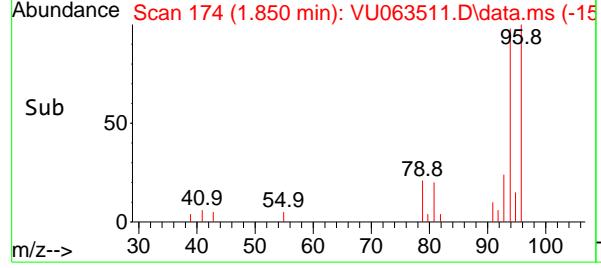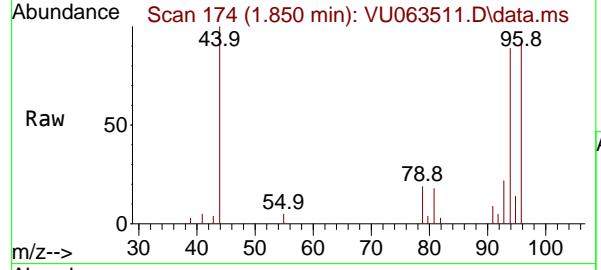

#5

Bromomethane

Concen: 0.522 ug/l

RT: 1.850 min Scan# 1

Delta R.T. 0.010 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24




Instrument:

MSVOA_U

ClientSampleId :

VSTDICCO.5

**Manual Integrations
APPROVED**

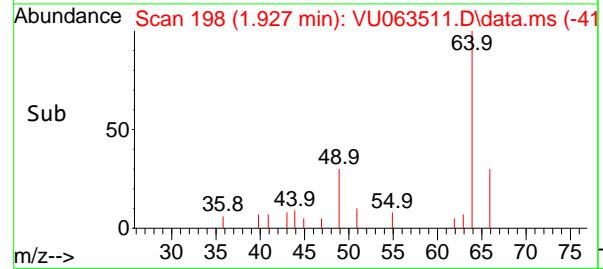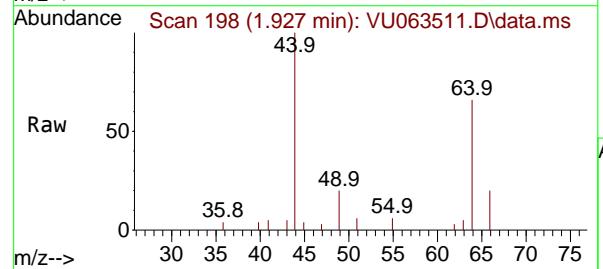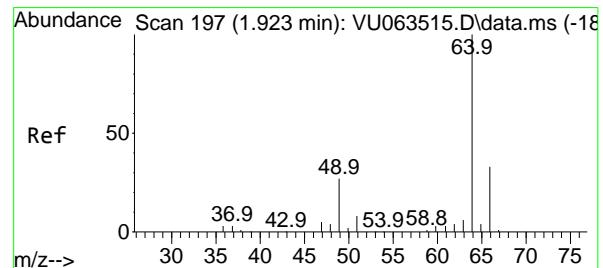 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#6

Chloroethane

Concen: 0.493 ug/l

RT: 1.927 min Scan# 198

Delta R.T. 0.003 min

Lab File: VU063511.D


Acq: 16 Jul 2025 09:24


Tgt Ion: 64 Resp: 2643

Ion Ratio Lower Upper

64 100


66 29.5 26.2 39.4

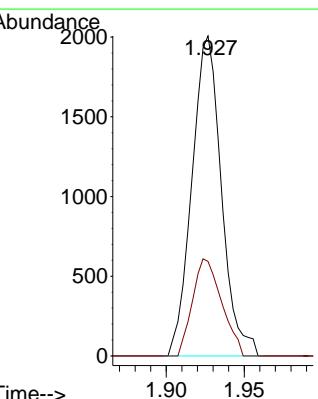



#7
Trichlorofluoromethane
Concen: 0.492 ug/l
RT: 2.129 min Scan# 2
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
ClientSampleId : VSTDICC0.5




Tgt Ion:101 Resp: 6269
Ion Ratio Lower Upper
101 100
103 63.2 52.2 78.4

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

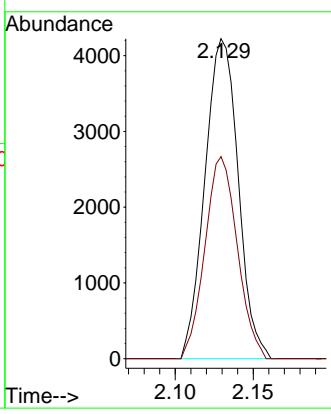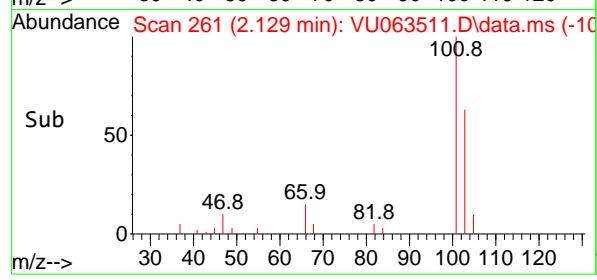


#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.474 ug/l
RT: 2.570 min Scan# 398
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Tgt Ion:101 Resp: 3157
Ion Ratio Lower Upper
101 100
85 42.5 37.8 56.6
151 73.3 59.2 88.8

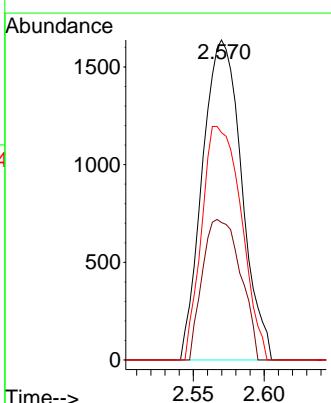



#9
1,1-Dichloroethene
Concen: 0.500 ug/l
RT: 2.570 min Scan# 3
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
ClientSampleId : VSTDICC0.5

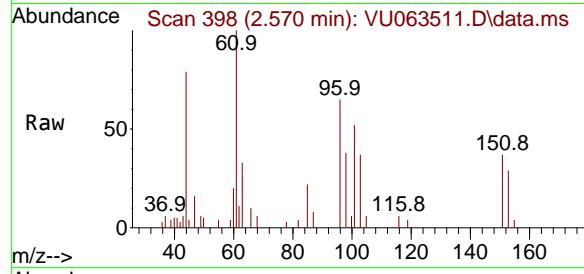


Tgt Ion: 96 Resp: 3301
Ion Ratio Lower Upper
96 100
61 154.0 0.0 504.3
98 58.8 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

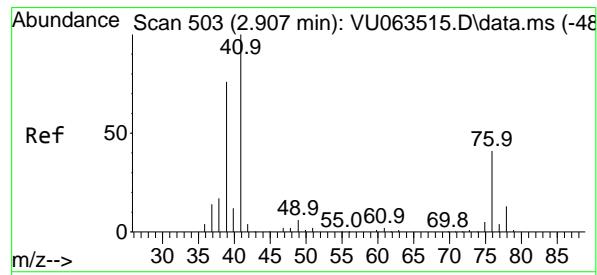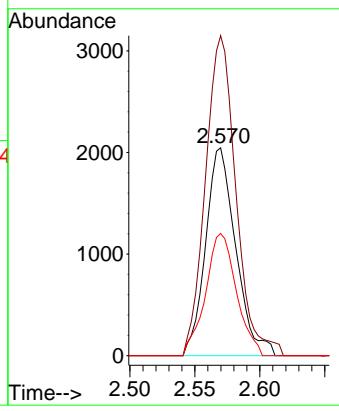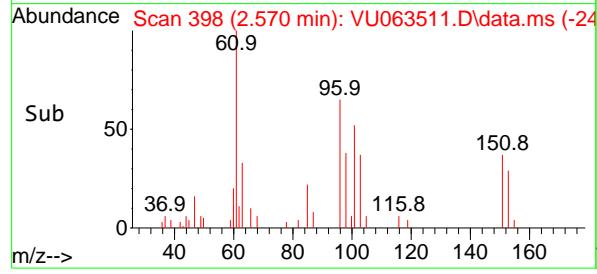


#11
Allyl Chloride
Concen: 0.461 ug/l
RT: 2.911 min Scan# 504
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

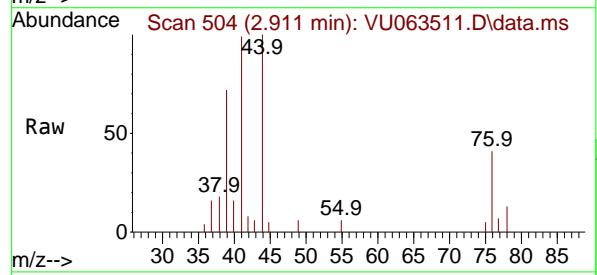

Tgt Ion: 41 Resp: 4399
Ion Ratio Lower Upper
41 100
39 79.3 61.5 92.3

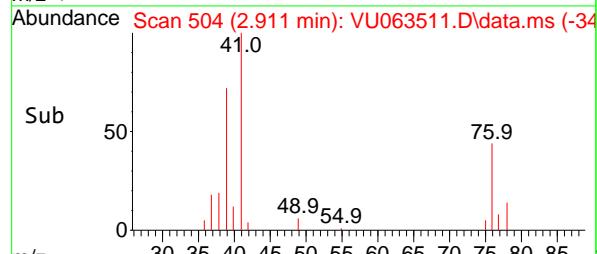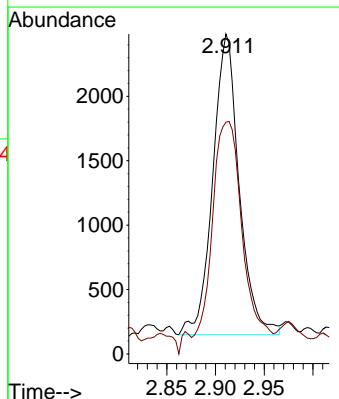




#12

Acrylonitrile
 Concen: 1.038 ug/l m
 RT: 3.309 min Scan# 61
 Delta R.T. 0.003 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
 ClientSampleId : VSTDICC0.5



Tgt Ion: 53 Resp: 171
 Ion Ratio Lower Upper
 53 100
 52 75.6 64.3 96.5
 51 42.2 27.8 41.8




Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

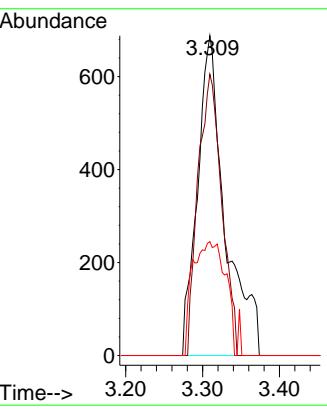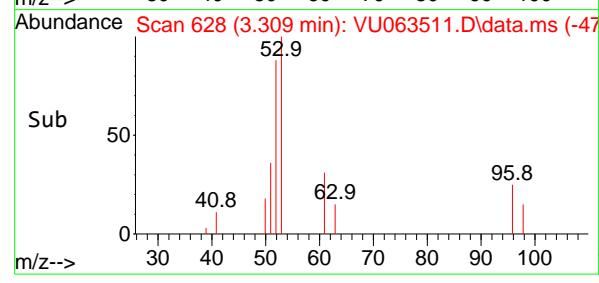

#13
 Acetone
 Concen: 2.627 ug/l
 RT: 2.618 min Scan# 413
 Delta R.T. 0.000 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24

Tgt Ion: 43 Resp: 3474
 Ion Ratio Lower Upper
 43 100
 58 30.7 25.4 38.0



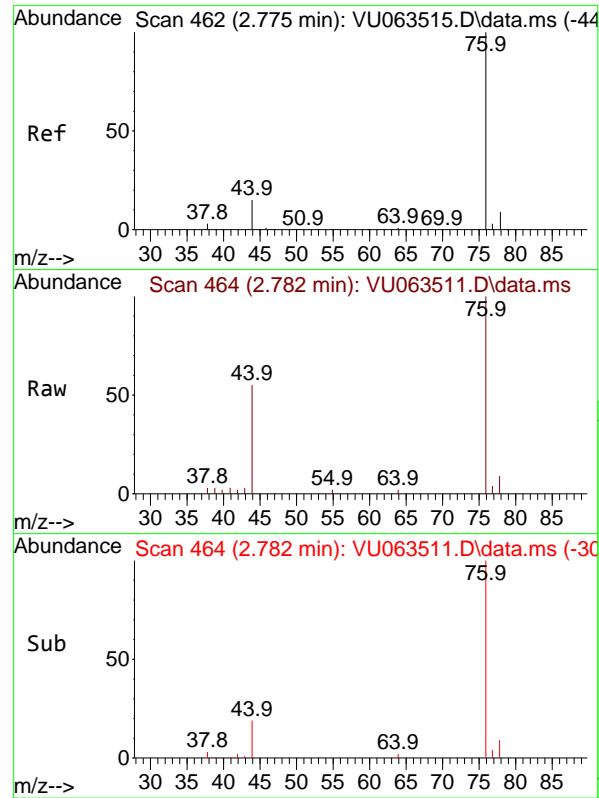

#14

Carbon Disulfide

Concen: 0.487 ug/l

RT: 2.782 min Scan# 4

Delta R.T. 0.007 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument:



MSVOA_U

ClientSampleId :

VSTDICCO.5

Tgt Ion: 76 Resp: 10380
 Ion Ratio Lower Upper
 76 100
 78 9.3 7.0 10.6

**Manual Integrations
APPROVED**

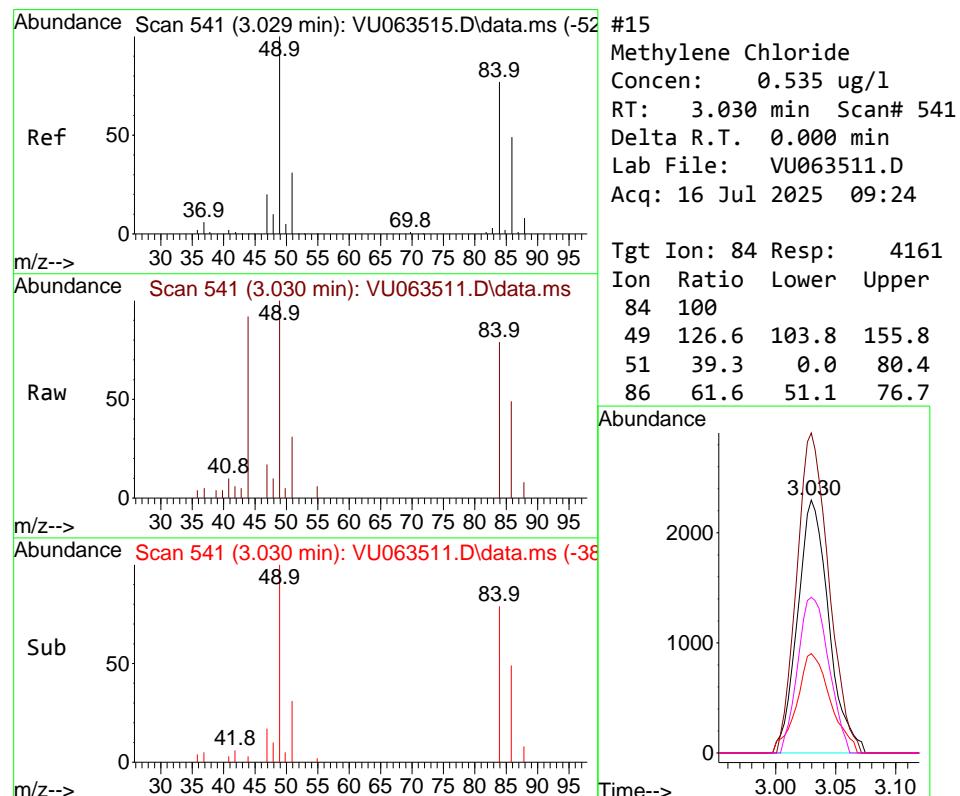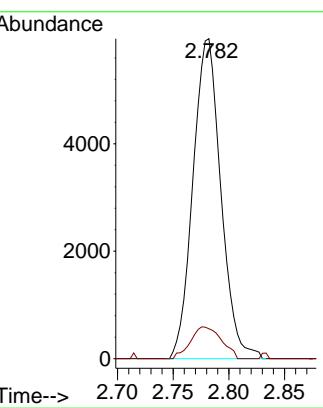 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#15

Methylene Chloride

Concen: 0.535 ug/l


RT: 3.030 min Scan# 541







Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Tgt Ion: 84 Resp: 4161
 Ion Ratio Lower Upper
 84 100
 49 126.6 103.8 155.8
 51 39.3 0.0 80.4
 86 61.6 51.1 76.7

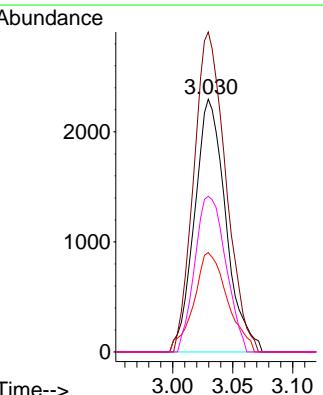

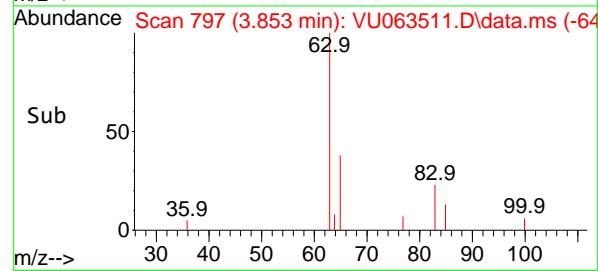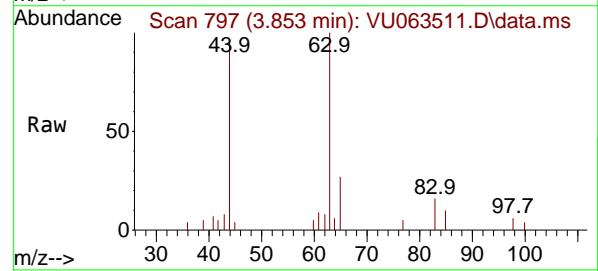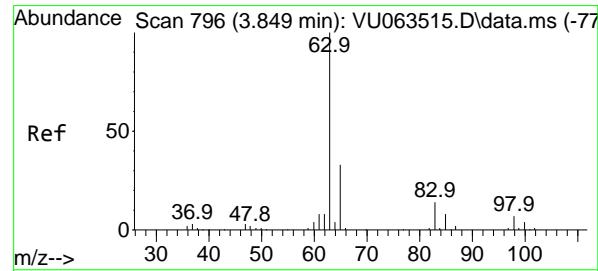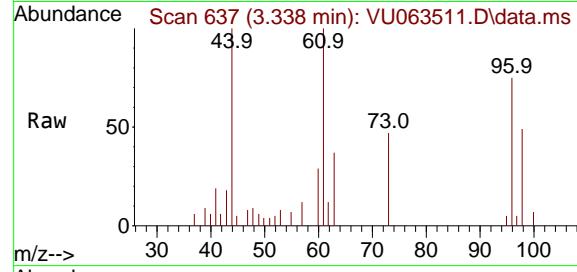

#16

trans-1,2-Dichloroethene

Concen: 0.487 ug/l

RT: 3.338 min Scan# 6

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument:

MSVOA_U


ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**


Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025



#17
1,1-Dichloroethane
Concen: 0.485 ug/l
RT: 3.853 min Scan# 797
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24


Tgt Ion: 63 Resp: 6739
Ion Ratio Lower Upper
63 100
98 6.2 3.4 10.2
100 4.2 2.1 6.2

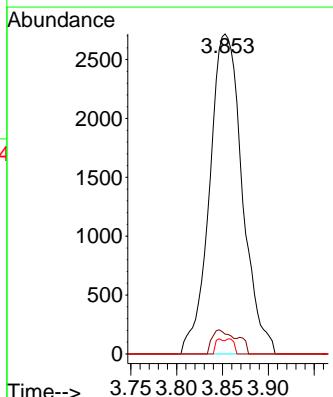



#18
2-Butanone
Concen: 2.467 ug/l
RT: 4.711 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
ClientSampleId : VSTDICC0.5

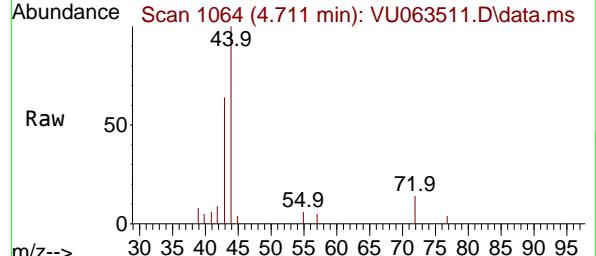


Tgt Ion: 43 Resp: 5051
Ion Ratio Lower Upper
43 100
57 8.4 0.0 16.4

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#19
Cyclohexane
Concen: 0.487 ug/l
RT: 5.364 min Scan# 1267
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24



Tgt Ion: 56 Resp: 5734
Ion Ratio Lower Upper
56 100
69 38.3 26.6 39.8
84 84.7 71.0 106.4

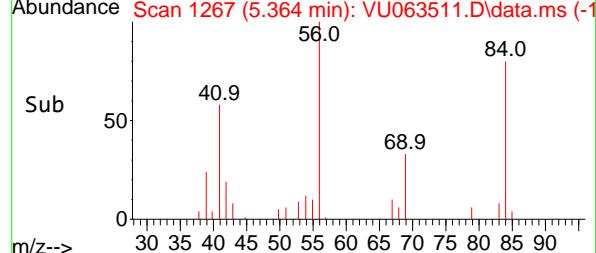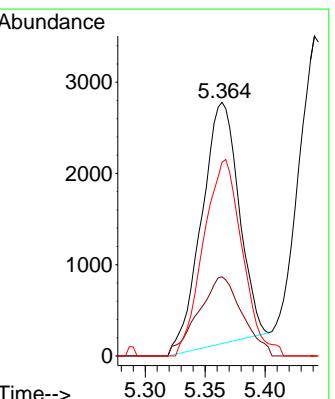



#20

Methylcyclohexane



Concen: 0.491 ug/l

RT: 6.740 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


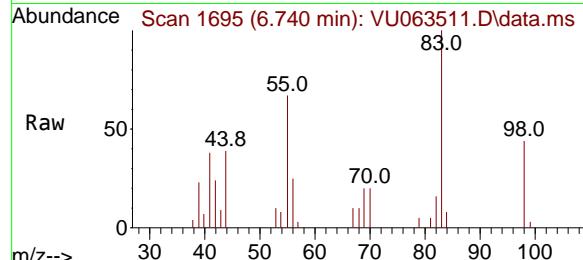


Tgt Ion: 83 Resp: 561
Ion Ratio Lower Upper


83	100
55	78.2
98	43.3
	60.6
	35.8
	90.8
	53.8

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025





#21
2,2-Dichloropropane
Concen: 0.518 ug/l
RT: 4.644 min Scan# 1043
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24



Tgt Ion: 77 Resp: 6127
Ion Ratio Lower Upper


77	100
97	20.9
	17.8
	26.8





#22
cis-1,2-Dichloroethene
Concen: 0.484 ug/l
RT: 4.647 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5




Tgt Ion: 96 Resp: 394:
Ion Ratio Lower Upper
96 100
61 147.0 0.0 384.7
98 60.6 32.1 96.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


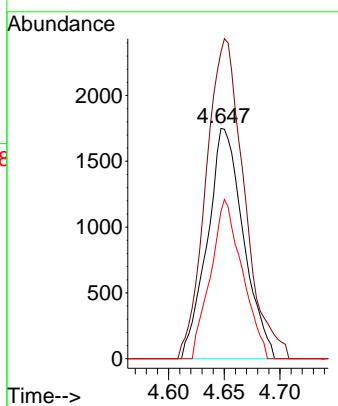



#23
Diethyl Ether
Concen: 0.435 ug/l
RT: 2.370 min Scan# 336
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24



Tgt Ion: 59 Resp: 2188
Ion Ratio Lower Upper
59 100
45 86.5 55.1 82.7#
74 84.3 58.2 87.4

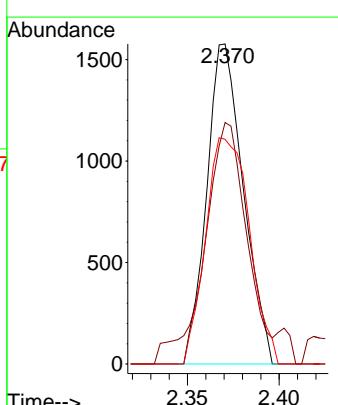



#25

Methyl tert-Butyl Ether

Concen: 0.469 ug/l

RT: 3.361 min Scan# 6





Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U

ClientSampleId : VSTDICCO.5

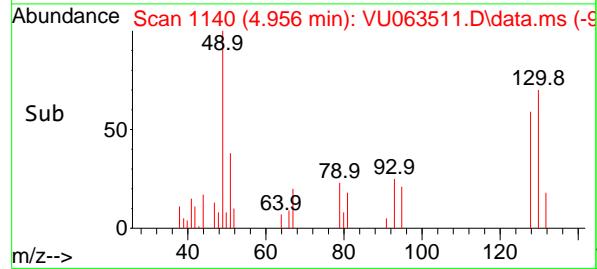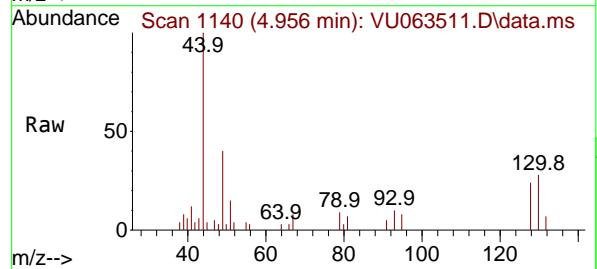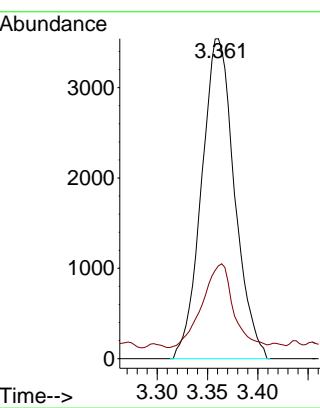**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#26

Bromochloromethane

Concen: 0.478 ug/l


RT: 4.956 min Scan# 1140


Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion:	Ion	Ratio	Lower	Upper
128	100			
49	179.4	0.0	340.8	
130	133.5	100.5	150.7	

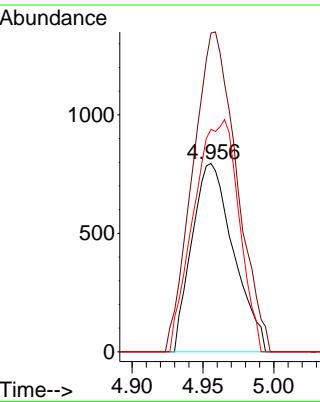



#27
 Chloroform
 Concen: 0.494 ug/l
 RT: 5.075 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
 ClientSampleId : VSTDICC0.5

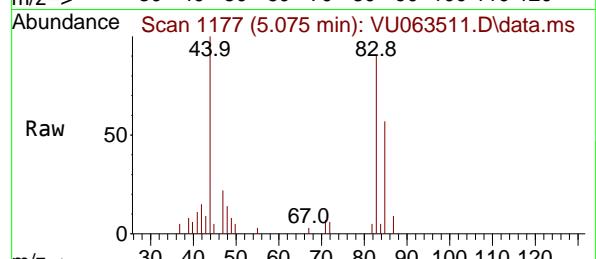


Tgt Ion: 83 Resp: 700
 Ion Ratio Lower Upper
 83 100
 85 63.7 0.0 130.0

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

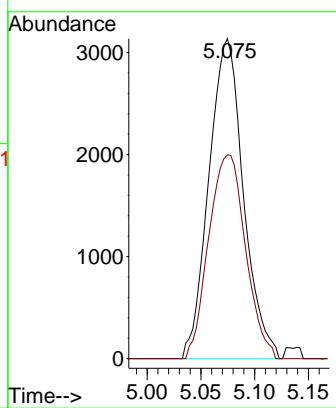


#28
 1,1,1-Trichloroethane
 Concen: 0.483 ug/l
 RT: 5.296 min Scan# 1246
 Delta R.T. 0.000 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24



Tgt Ion: 97 Resp: 5809
 Ion Ratio Lower Upper
 97 100
 99 62.5 31.8 95.3
 61 46.1 23.3 69.9

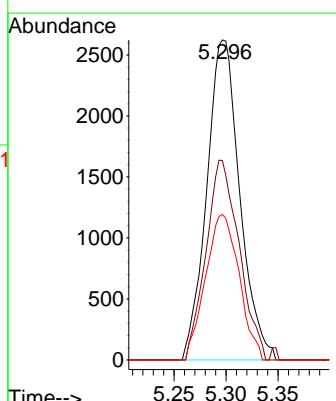


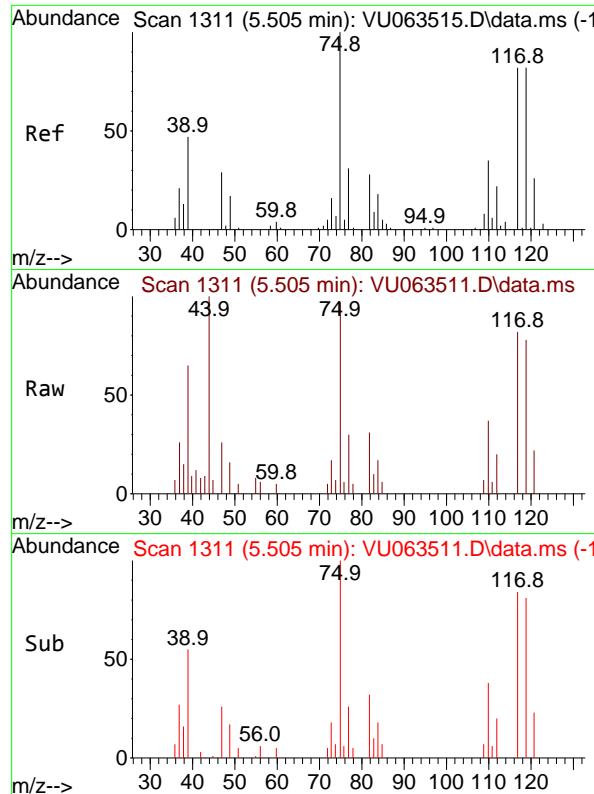


#29
 1,1-Dichloropropene
 Concen: 0.470 ug/l
 RT: 5.505 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
 ClientSampleId : VSTDICCO.5


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

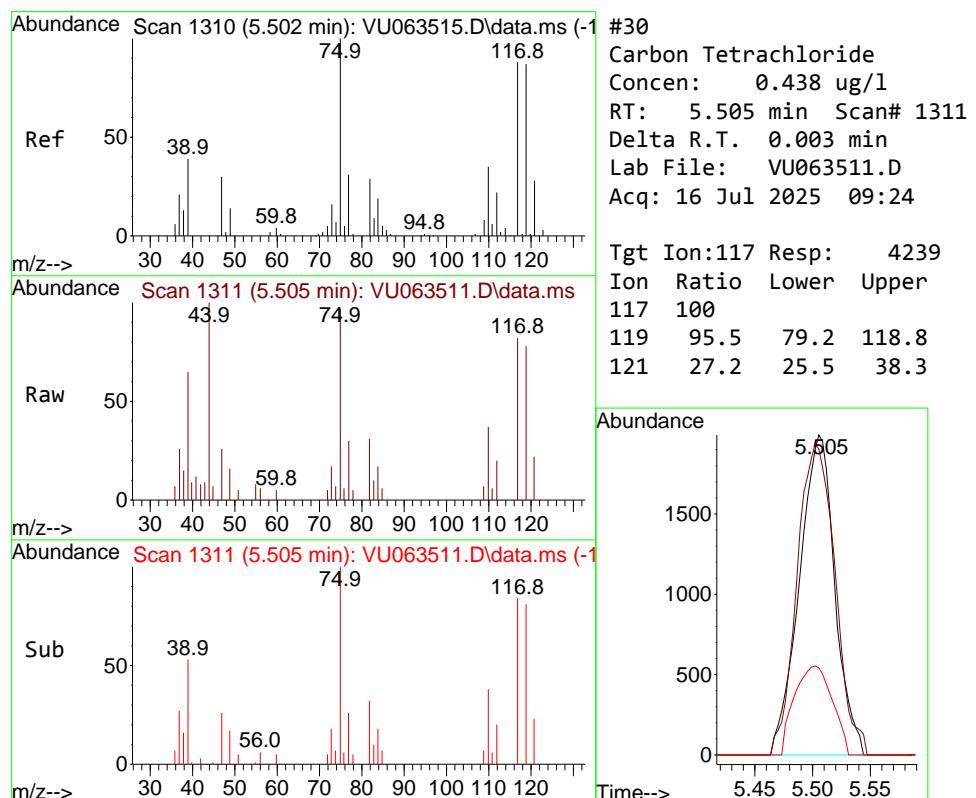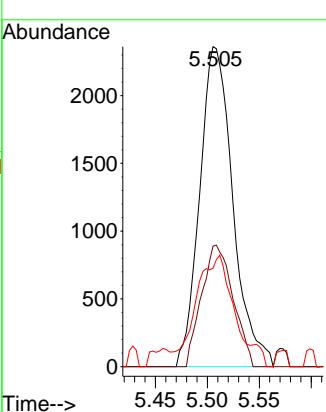

#30
 Carbon Tetrachloride
 Concen: 0.438 ug/l
 RT: 5.505 min Scan# 1311
 Delta R.T. 0.003 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24

Tgt Ion:117 Resp: 4239
 Ion Ratio Lower Upper
 117 100
 119 95.5 79.2 118.8
 121 27.2 25.5 38.3

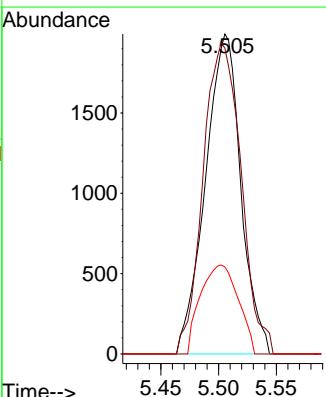



#31

Isopropyl Ether

Concen: 0.483 ug/l

RT: 3.994 min Scan# 8

Instrument :

Delta R.T. 0.003 min

MSVOA_U

Lab File: VU063511.D

ClientSampleId :

Acq: 16 Jul 2025 09:24

VSTDICCO.5

Tgt Ion: 45 Resp: 1012

Ion Ratio Lower Upper





45 100

43 51.1 25.7 77.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

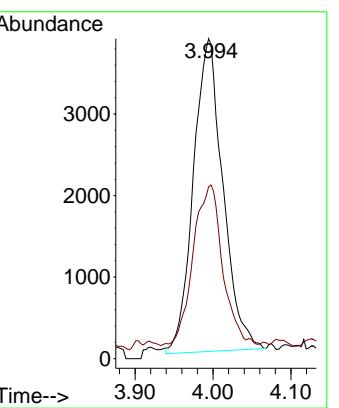

#32

Ethyl-t-butyl ether

Concen: 0.484 ug/l

RT: 4.502 min Scan# 999

Delta R.T. 0.000 min

Lab File: VU063511.D


Acq: 16 Jul 2025 09:24




Tgt Ion: 59 Resp: 9396

Ion Ratio Lower Upper

59 100

87 38.8 32.6 49.0

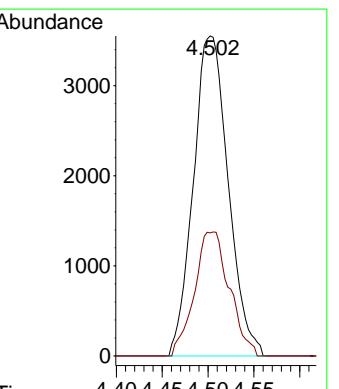



#33





Tert-Amyl methyl ether
Concen: 0.515 ug/l
RT: 5.943 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
ClientSampleId : VSTDICC0.5

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


Tgt Ion: 73 Resp: 8680
Ion Ratio Lower Upper
73 100
87 22.5 19.4 29.2
71 12.2 8.9 13.3

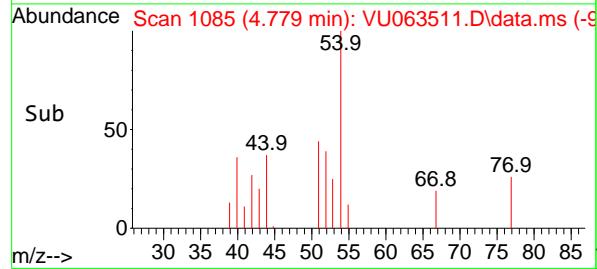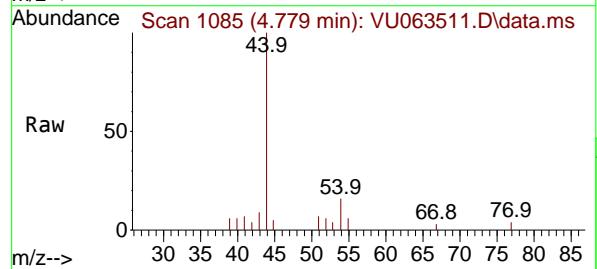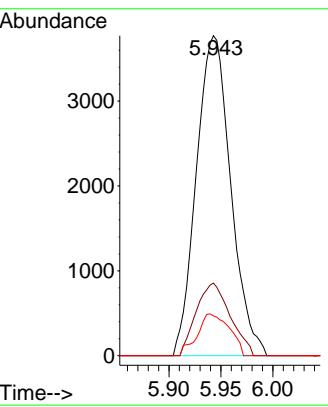


#34


Propionitrile
Concen: 2.565 ug/l m
RT: 4.779 min Scan# 1085
Delta R.T. 0.007 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Tgt Ion: 54 Resp: 1601
Ion Ratio Lower Upper
54 100
52 20.9 17.0 25.4
55 13.1 13.6 20.4#
40 10.9 6.4 9.6#

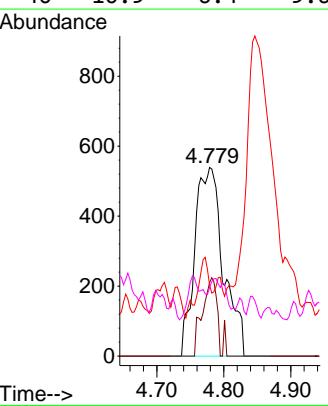






#35
Benzene
Concen: 0.517 ug/l
RT: 5.759 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Tgt Ion: 78 Resp: 1547
Ion Ratio Lower Upper
78 100
77 26.4 19.4 29.2

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

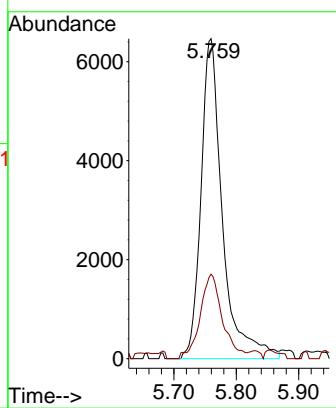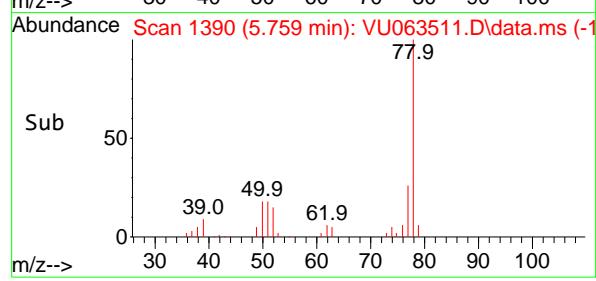


#36
1,2-Dichloroethane
Concen: 0.492 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Tgt Ion: 62 Resp: 4577
Ion Ratio Lower Upper
62 100
98 8.5 6.4 9.6

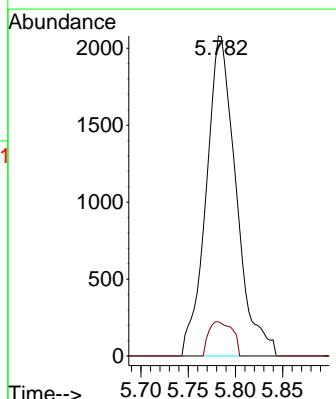



#37
Trichloroethene
Concen: 0.522 ug/l
RT: 6.528 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5




Tgt Ion:130 Resp: 3989
Ion Ratio Lower Upper
130 100
95 95.9 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


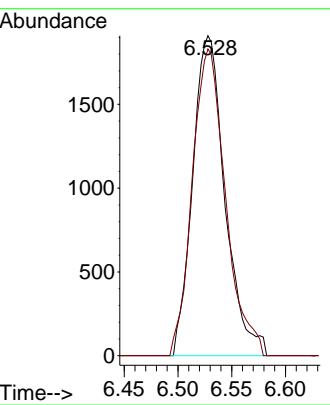



#38
1,2-Dichloropropane
Concen: 0.426 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

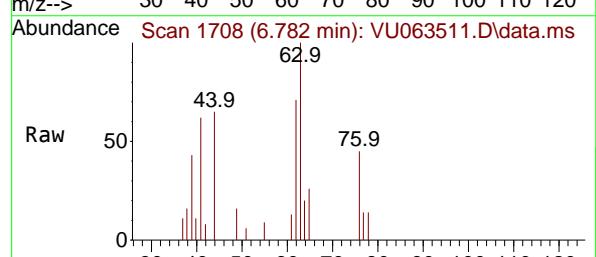

Tgt Ion: 63 Resp: 2987
Ion Ratio Lower Upper
63 100
65 25.9 24.6 36.8

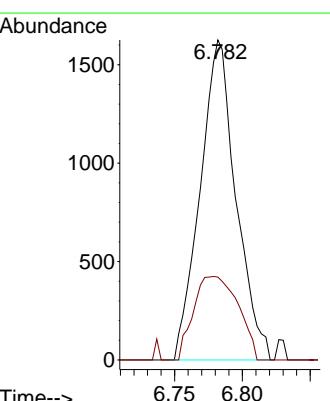



#39

Methacrylonitrile

Concen: 0.645 ug/l m

RT: 4.981 min Scan# 1

Delta R.T. 0.010 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument:

MSVOA_U




ClientSampleId :

VSTDICCO.5

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

 Tgt Ion: 41 Resp: 1761
 Ion Ratio Lower Upper

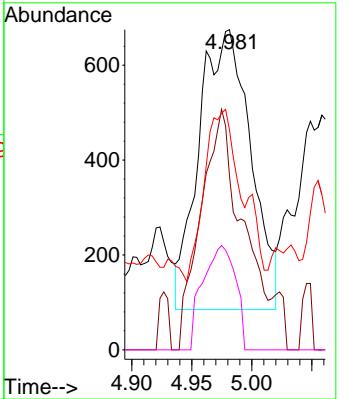 41 100
 67 69.3 62.7 94.1#
 39 38.3 43.1 64.7#
 52 23.6 27.4 41.0#


#40

Methyl acrylate

Concen: 0.508 ug/l

RT: 4.846 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Tgt Ion: 55 Resp: 2059


Ion Ratio Lower Upper


55 100

85 11.8 12.8 19.2#

58 0.0 7.0 10.4#

42 6.9 7.0 10.4#

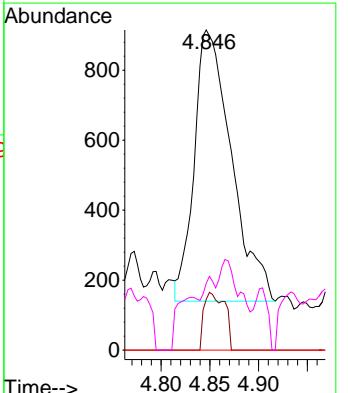



#41

Tetrahydrofuran

Concen: 1.376 ug/l

RT: 5.062 min Scan# 1


Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U

ClientSampleId : VSTDICCO.5



Tgt Ion: 42 Resp: 2003

Ion Ratio Lower Upper

42 100







72 29.3 39.2 58.8


71 33.5 34.8 52.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025
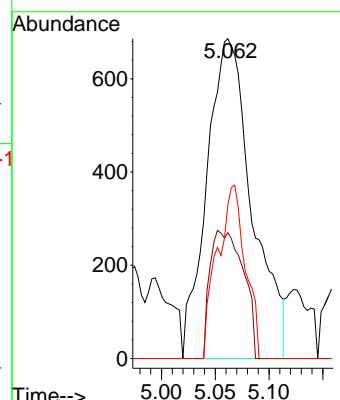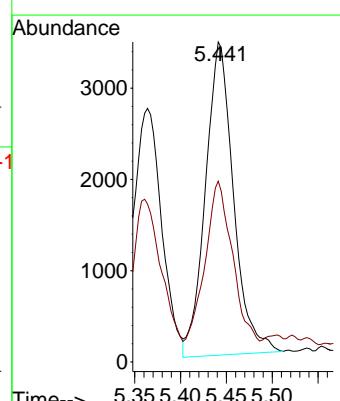
#42
1-Chlorobutane
Concen: 0.493 ug/l
RT: 5.441 min Scan# 1291
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24Tgt Ion: 56 Resp: 7303
Ion Ratio Lower Upper
56 100
41 48.2 26.7 80.0



#43
Dibromomethane
Concen: 0.462 ug/l
RT: 6.907 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24




Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5




Tgt Ion: 93 Resp: 1679
Ion Ratio Lower Upper
93 100
95 77.2 67.9 101.9
174 89.3 74.6 111.8

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


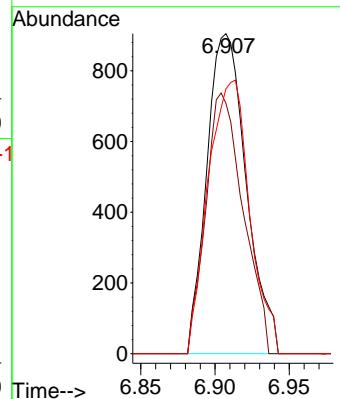



#44
Bromodichloromethane
Concen: 0.471 ug/l
RT: 7.097 min Scan# 1806
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24



Tgt Ion: 83 Resp: 3861
Ion Ratio Lower Upper
83 100
85 61.2 52.7 79.1
127 10.1 8.1 12.1

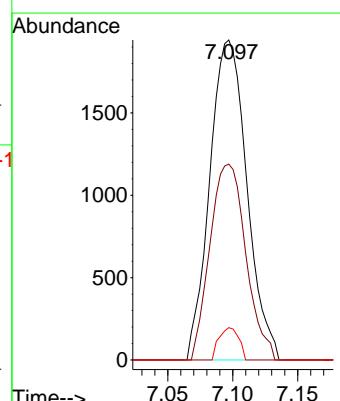



#45

4-Methyl-2-Pentanone

Concen: 2.301 ug/l

RT: 7.801 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#46

t-1,4-Dichloro-2-butene

Concen: 0.990 ug/l

RT: 10.827 min Scan# 2966

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Tgt Ion: 75 Resp: 1314


Ion Ratio Lower Upper




75 100

53 50.0 48.4 72.6

89 20.9 30.6 45.8#

88 21.0 25.3 37.9#

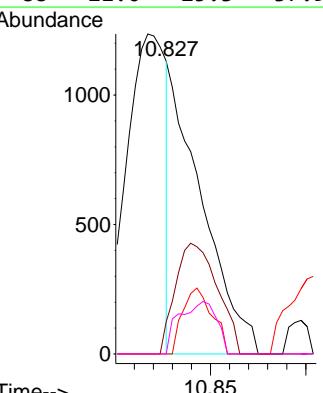



#47

Methyl methacrylate

Concen: 0.889 ug/l

RT: 6.968 min Scan# 1

Delta R.T. 0.007 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025





 Tgt Ion: 69 Resp: 271
 Ion Ratio Lower Upper

 69 100
 41 123.9 0.0 224.0

39 78.5 55.3 82.9

100 30.8 29.0 43.6

Abundance

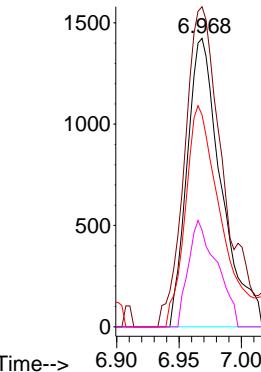

#48

Ethyl methacrylate

Concen: 0.451 ug/l

RT: 8.341 min Scan# 2193

Delta R.T. 0.007 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion: 69 Resp: 2622


Ion Ratio Lower Upper

69 100

41 75.1 30.8 92.4



Abundance

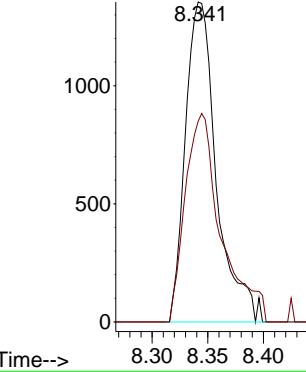



#49
Toluene
Concen: 0.452 ug/l
RT: 7.965 min Scan# 2150
Delta R.T. 0.007 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24



Instrument: MSVOA_U
ClientSampleId: VSTDICC0.5

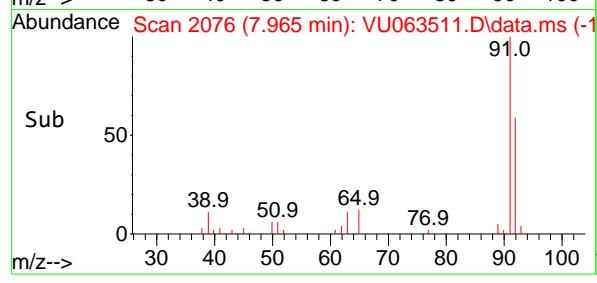


Tgt Ion: 92 Resp: 7391
Ion Ratio Lower Upper
92 100
91 175.6 140.4 210.6

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#50
t-1,3-Dichloropropene
Concen: 0.421 ug/l
RT: 8.209 min Scan# 2152
Delta R.T. 0.007 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24





Tgt Ion: 75 Resp: 2708
Ion Ratio Lower Upper
75 100
77 34.3 24.9 37.3

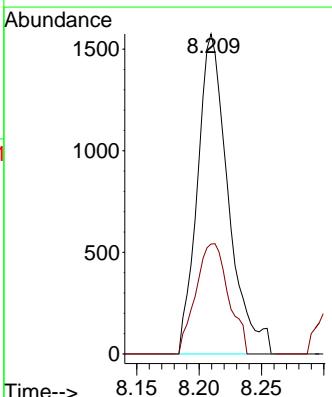



#51
cis-1,3-Dichloropropene
 Concen: 0.419 ug/l
 RT: 7.602 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24



Instrument : MSVOA_U
 ClientSampleId : VSTDICCO.5




Tgt Ion: 75 Resp: 361
 Ion Ratio Lower Upper
 75 100
 77 34.8 25.1 37.7
 39 52.3 37.8 56.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025





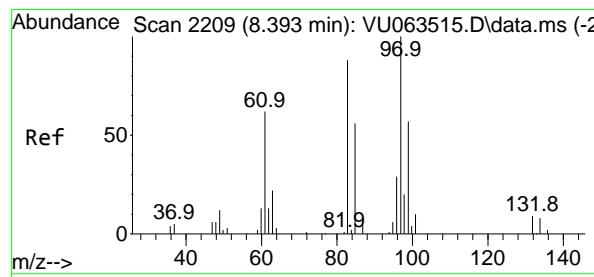
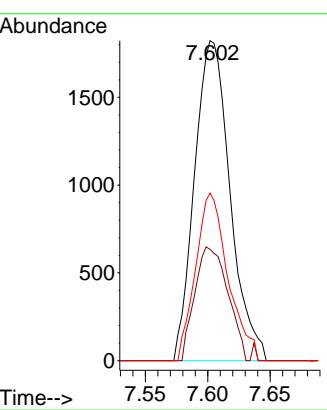


#52
 1,1,2-Trichloroethane
 Concen: 0.449 ug/l
 RT: 8.396 min Scan# 2210
 Delta R.T. 0.003 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24



Tgt Ion: 97 Resp: 2194
 Ion Ratio Lower Upper
 97 100
 83 91.2 70.2 105.2
 85 59.1 45.2 67.8
 99 70.4 50.1 75.1

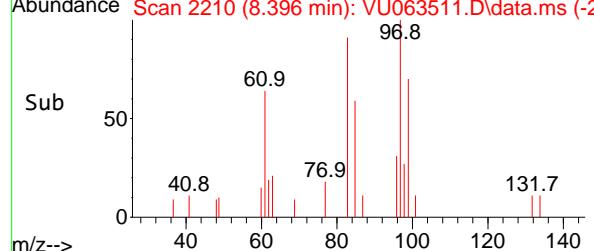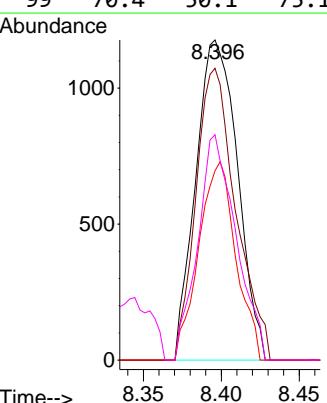



#53

1,3-Dichloropropane

Concen: 0.467 ug/l

RT: 8.570 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC0.5

Tgt Ion: 76 Resp: 394

Ion Ratio Lower Upper


76 100

78 30.2 26.0 39.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

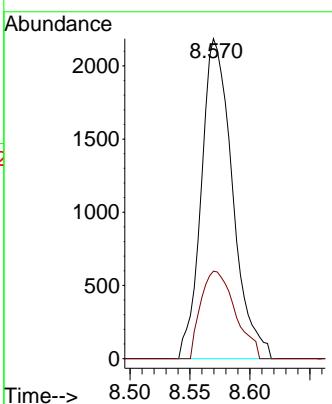

#54

2-Hexanone

Concen: 2.289 ug/l

RT: 8.698 min Scan# 2304

Delta R.T. 0.010 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion: 43 Resp: 5691







Ion Ratio Lower Upper

43 100

58 54.1 34.8 74.8

57 17.3 0.0 39.5

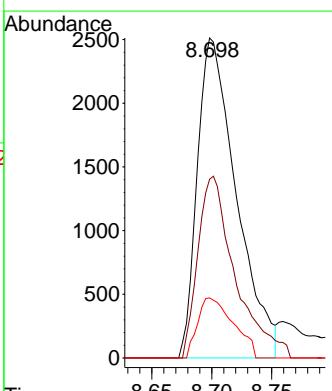

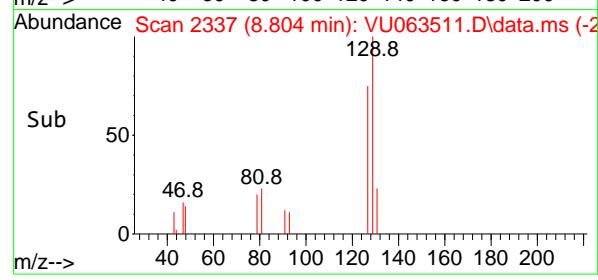

#55

Dibromochloromethane

Concen: 0.406 ug/l

RT: 8.804 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument :


MSVOA_U

ClientSampleId :

VSTDICC0.5

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

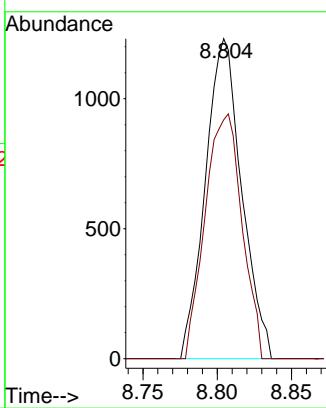

#56

1,2-Dibromoethane

Concen: 0.477 ug/l

RT: 8.920 min Scan# 2373

Delta R.T. 0.003 min

Lab File: VU063511.D


Acq: 16 Jul 2025 09:24




Tgt Ion:107 Resp: 2089

Ion Ratio Lower Upper

107 100

109 85.6 0.0 186.4

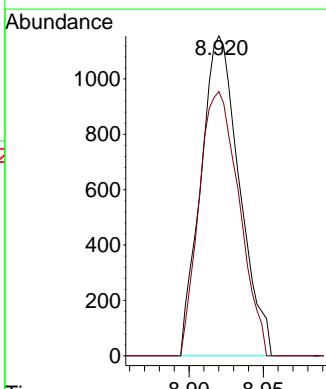



#57

4-Bromofluorobenzene

Concen: 0.986 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**

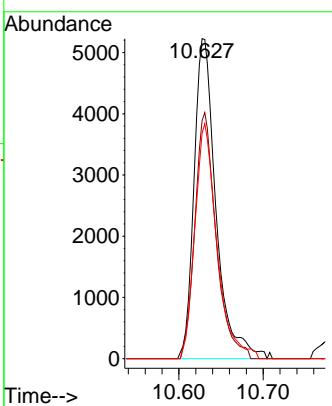 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#58

Tetrachloroethene


Concen: 0.461 ug/l


RT: 8.544 min Scan# 2256

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


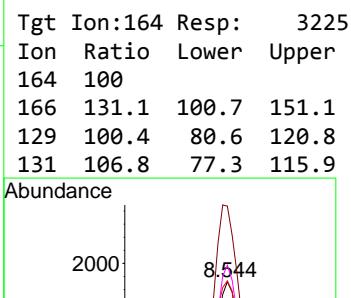


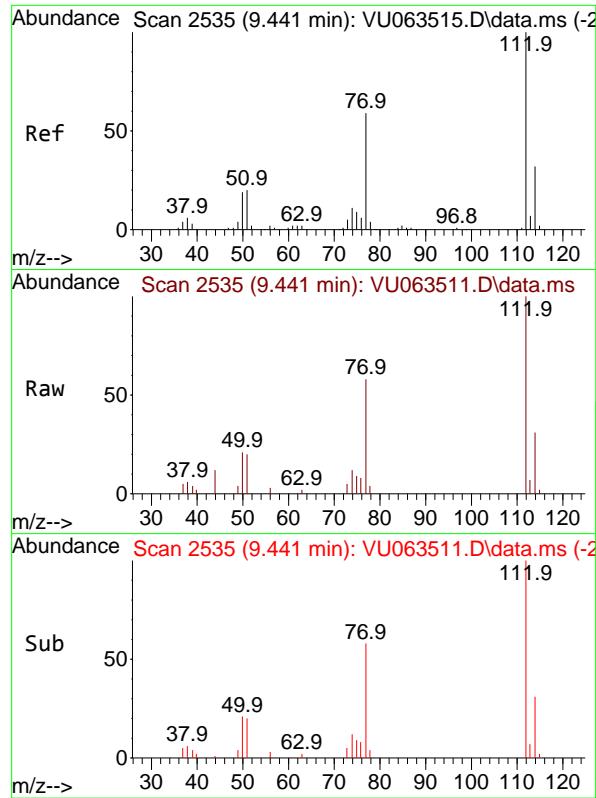

#59
Chlorobenzene
Concen: 0.460 ug/l
RT: 9.441 min Scan# 2
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24
ClientSampleId : VSTDICC0.5


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

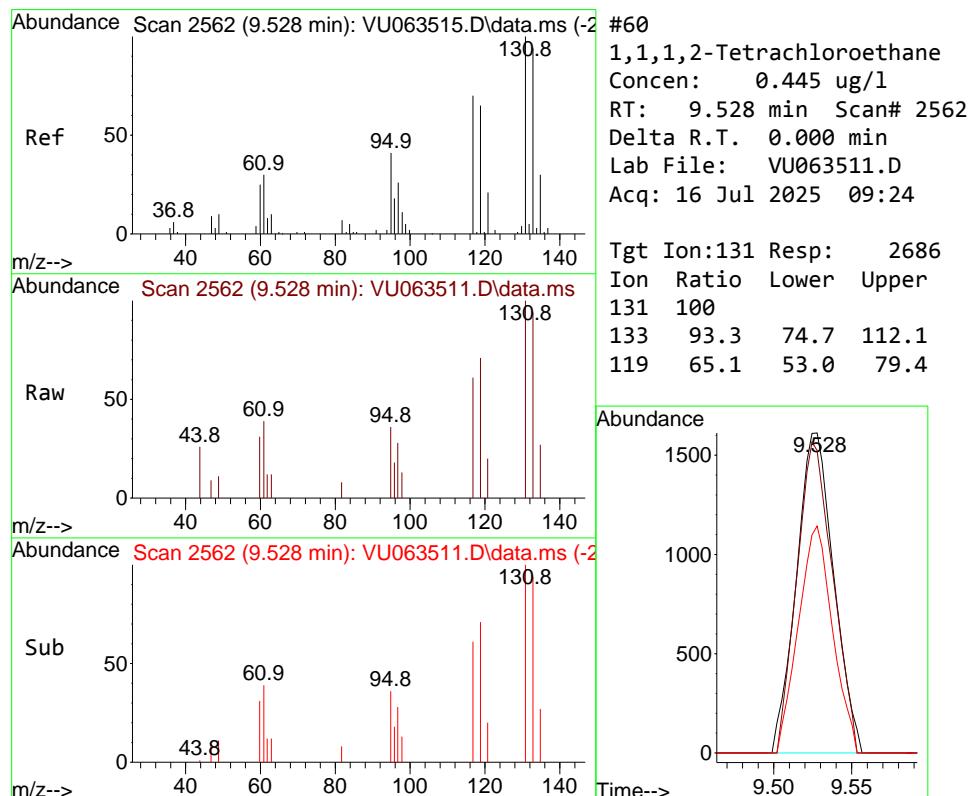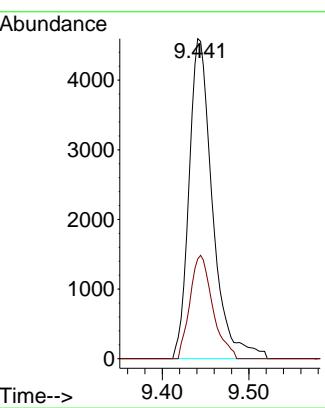

#60
1,1,1,2-Tetrachloroethane
Concen: 0.445 ug/l
RT: 9.528 min Scan# 2562
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Tgt Ion:131 Resp: 2686
Ion Ratio Lower Upper
131 100
133 93.3 74.7 112.1
119 65.1 53.0 79.4

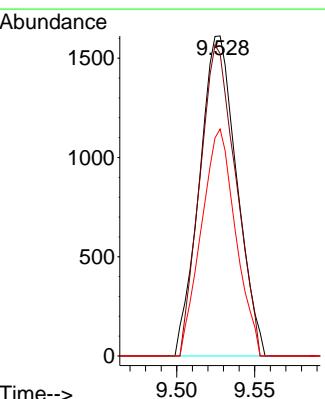

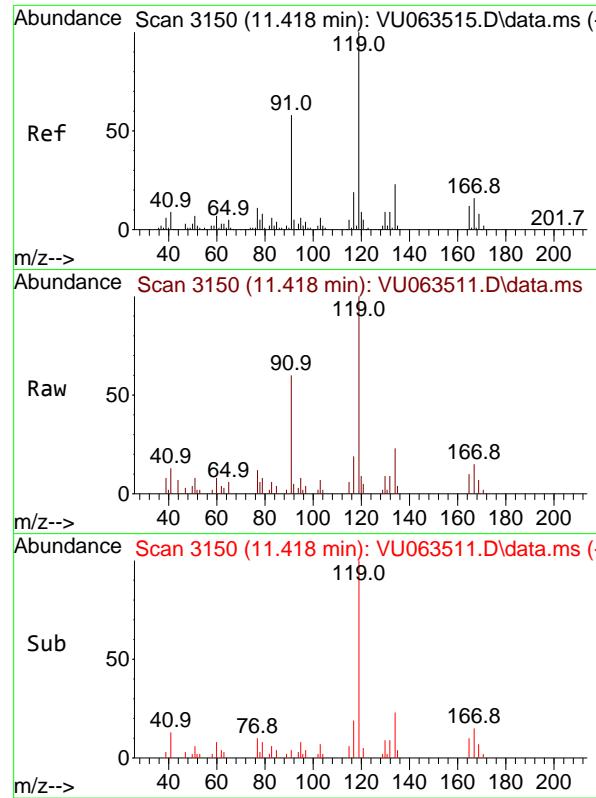

#61

Pentachloroethane

Concen: 0.441 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument :

MSVOA_U



ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

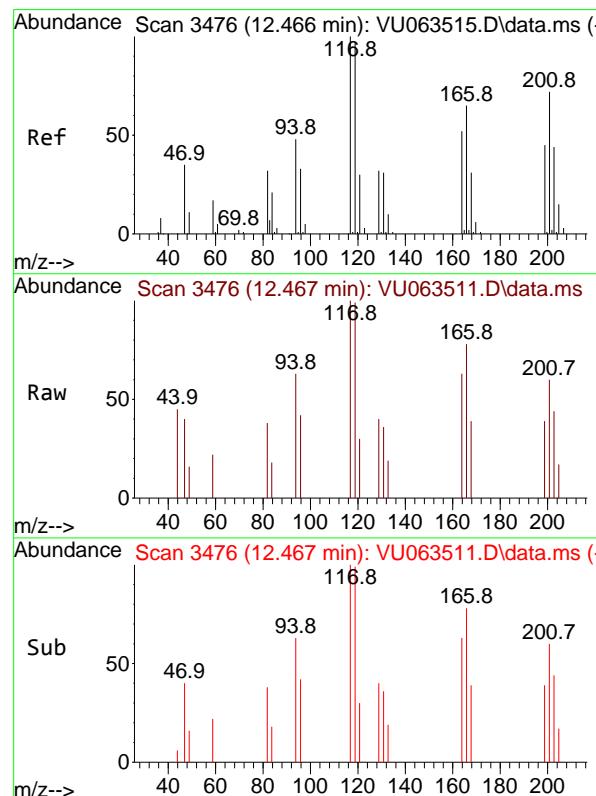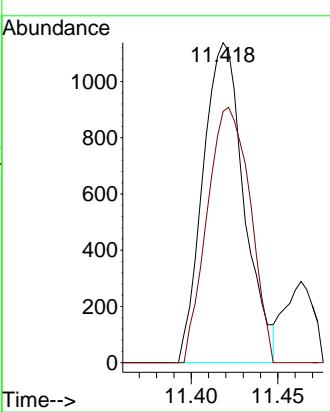

#62

Hexachloroethane

Concen: 0.403 ug/l

RT: 12.467 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063511.D


Acq: 16 Jul 2025 09:24


Tgt Ion:117 Resp: 1703

Ion Ratio Lower Upper

117 100

201 70.8 57.4 86.0

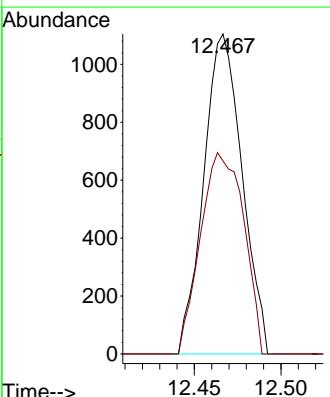



#63

Ethyl Benzene

Concen: 0.470 ug/l

RT: 9.566 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument:

MSVOA_U

ClientSampleId :



VSTDICC0.5



Tgt Ion: 91 Resp: 15182
 Ion Ratio Lower Upper
 91 100
 106 28.7 25.4 38.0



Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025





#64
 m/p-Xylenes
 Concen: 0.929 ug/l
 RT: 9.689 min Scan# 2612
 Delta R.T. 0.003 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24

Tgt Ion:106 Resp: 11672
 Ion Ratio Lower Upper
 106 100
 91 190.8 163.6 245.4

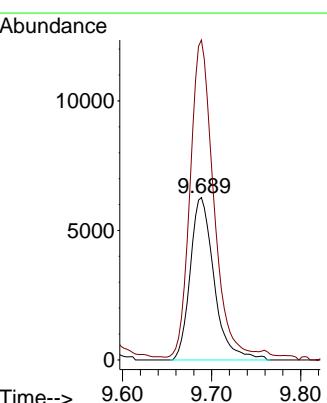

Abundance Scan 2612 (9.689 min): VU063511.D\data.ms (-2)

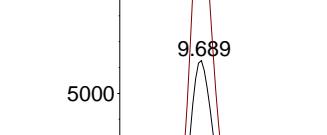


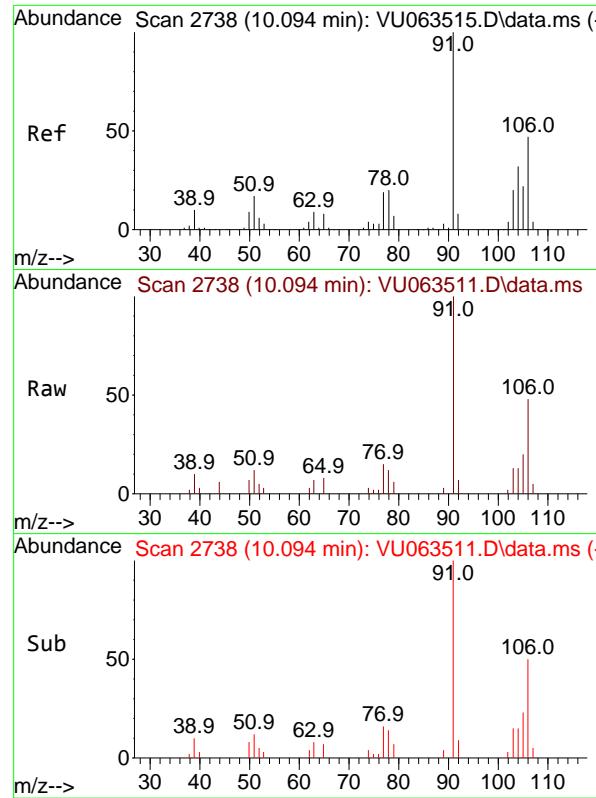


#65
o-Xylene
Concen: 0.450 ug/l
RT: 10.094 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

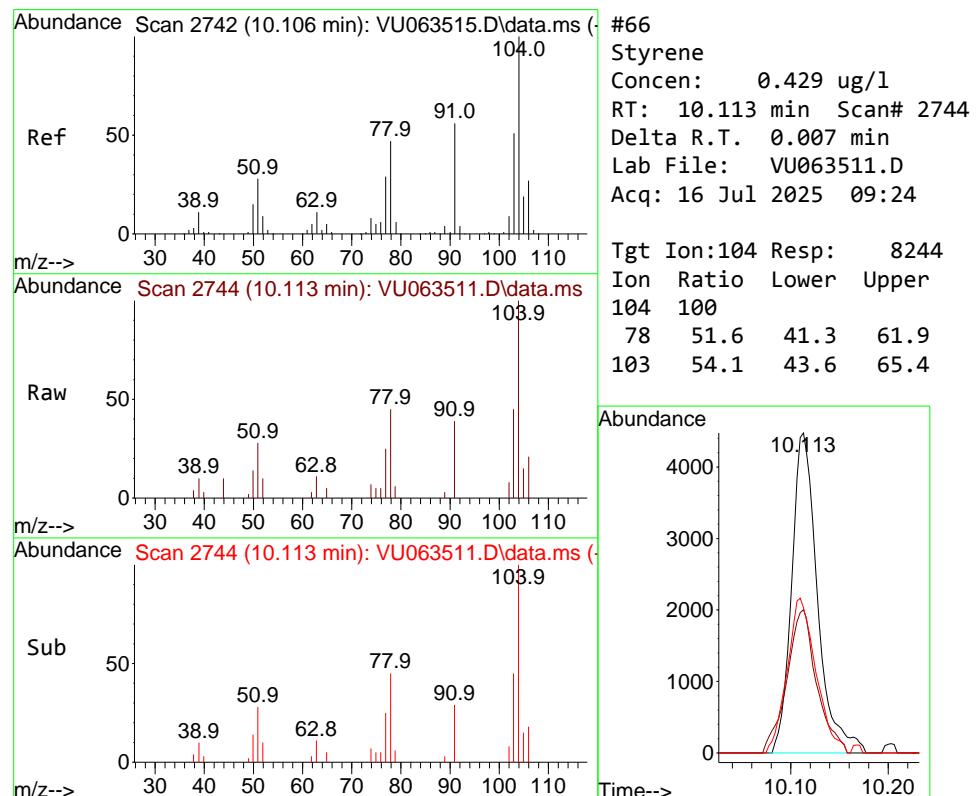

#66
Styrene
Concen: 0.429 ug/l
RT: 10.113 min Scan# 2744
Delta R.T. 0.007 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Tgt Ion:104 Resp: 8244
Ion Ratio Lower Upper
104 100
78 51.6 41.3 61.9
103 54.1 43.6 65.4



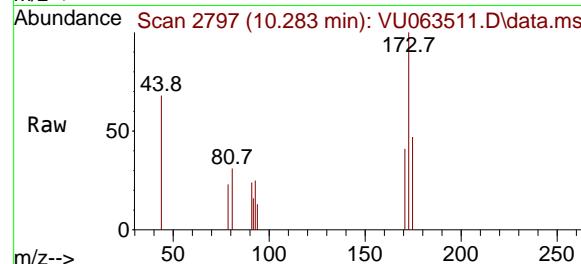

#67

Bromoform

Concen: 0.458 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument:

MSVOA_U





ClientSampleId :

VSTDICCO.5

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

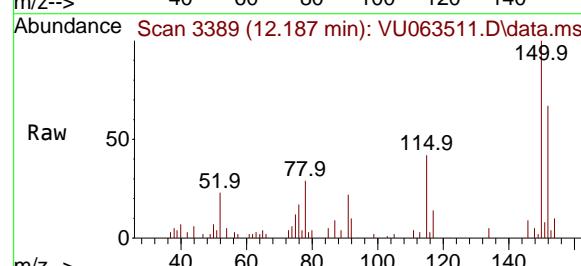

#68

1,2-Dichlorobenzene-d4

Concen: 0.909 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Tgt	Ion:152	Resp:	8092
Ion	Ratio	Lower	Upper
152	100		
115	69.1	0.0	262.2
150	163.6	0.0	651.2





#69

Isopropylbenzene

Concen: 0.442 ug/l

RT: 10.476 min Scan# 2

Instrument :

Delta R.T. 0.000 min

MSVOA_U

Lab File: VU063511.D

ClientSampleId :




Acq: 16 Jul 2025 09:24

VSTDICC0.5

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 0.474 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion: 83 Resp: 2820




Ion Ratio Lower Upper

83 100

131 5.4 8.4 12.6#

85 54.9 51.9 77.9

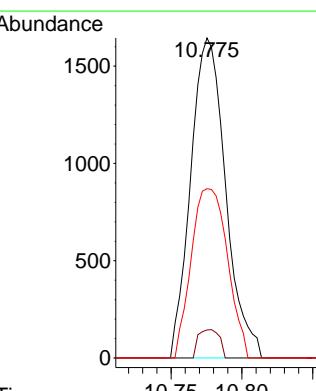



#71

1,2,3-Trichloropropane

Concen: 0.449 ug/l m

RT: 10.817 min Scan# 2173

Delta R.T. 0.000 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

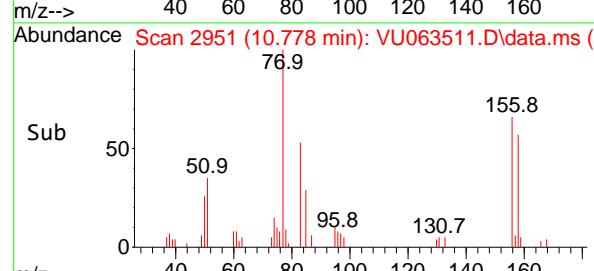

#72

Bromobenzene

Concen: 0.479 ug/l

RT: 10.778 min Scan# 2951

Delta R.T. 0.003 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion:156 Resp: 3609




Ion Ratio Lower Upper

156 100

77 152.5 0.0 315.2

158 84.9 0.0 195.4

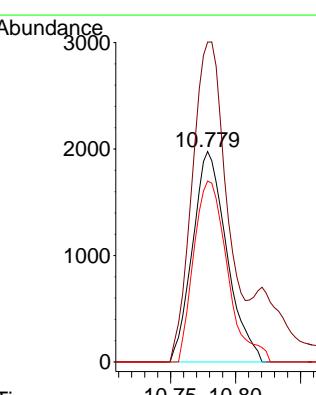



#73

n-propylbenzene

Concen: 0.438 ug/l

RT: 10.901 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063511.D




Acq: 16 Jul 2025 09:24

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC0.5

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#74

2-Chlorotoluene

Concen: 0.454 ug/l

RT: 10.981 min Scan# 3014

Delta R.T. 0.003 min

Lab File: VU063511.D


Acq: 16 Jul 2025 09:24




Tgt Ion:126 Resp: 3528

Ion Ratio Lower Upper

126 100

91 295.8 0.0 606.0

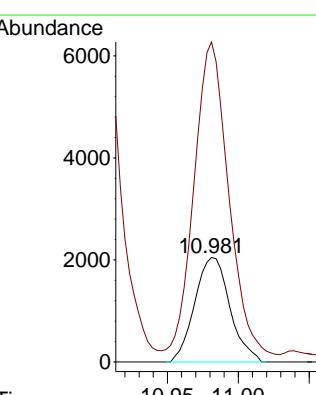






#75
1,3,5-Trimethylbenzene
Concen: 0.441 ug/l
RT: 11.081 min Scan# 3045
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#76
4-Chlorotoluene
Concen: 0.434 ug/l
RT: 11.097 min Scan# 3050
Delta R.T. 0.007 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Tgt Ion:126 Resp: 3423
Ion Ratio Lower Upper
126 100
91 339.4 0.0 682.2





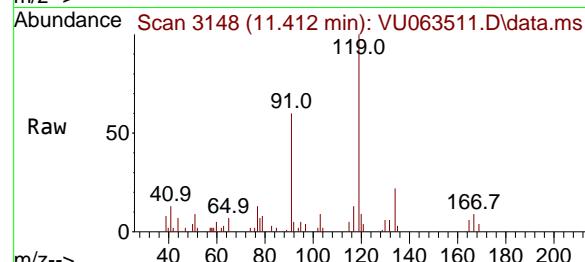



#77
tert-Butylbenzene
Concen: 0.455 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. 0.000 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

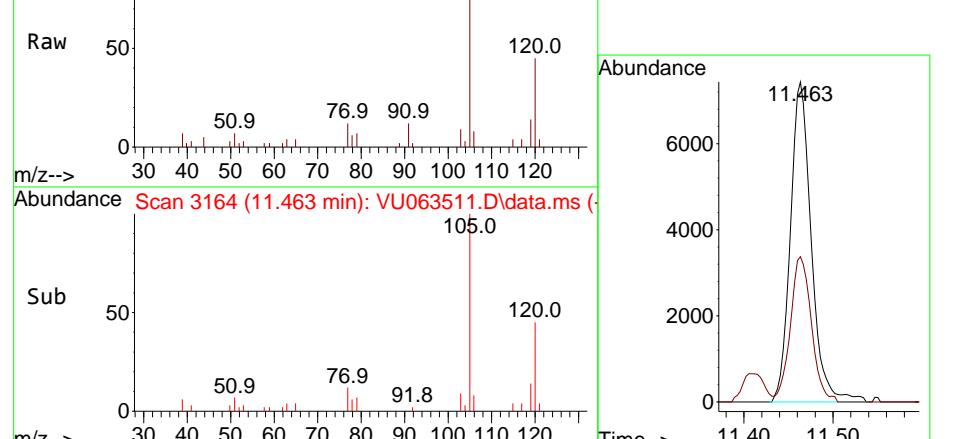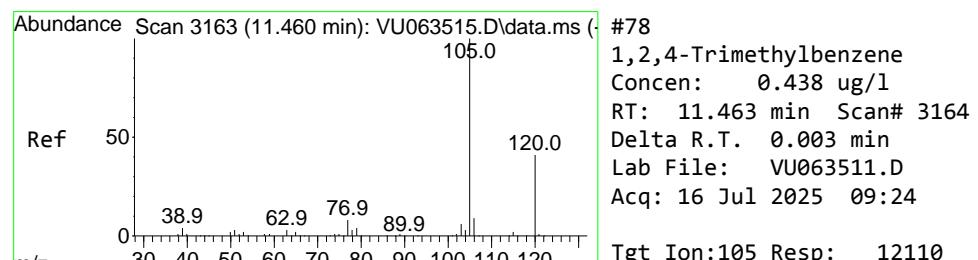


#78
1,2,4-Trimethylbenzene
Concen: 0.438 ug/l
RT: 11.463 min Scan# 3164
Delta R.T. 0.003 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Tgt Ion:105 Resp: 12110
Ion Ratio Lower Upper
105 100
120 45.6 22.7 68.0

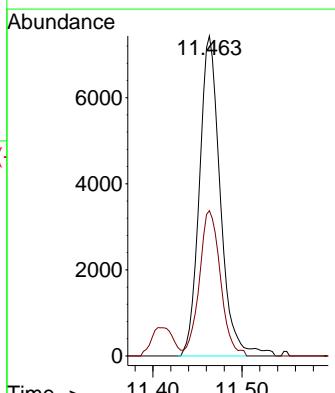




Abundance Scan 3218 (11.637 min): VU063511.D\data.ms (-)

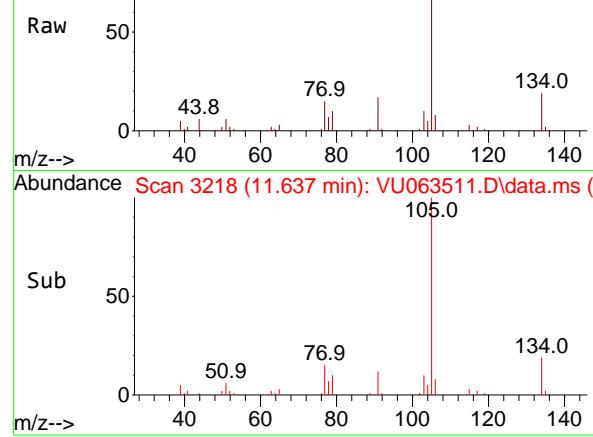

Abundance Scan 3218 (11.637 min): VU063511.D\data.ms (-)

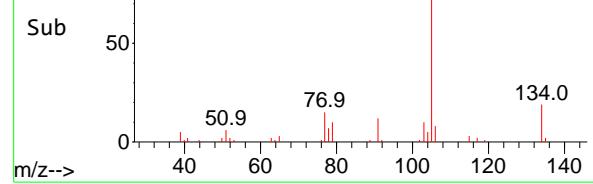

#79

sec-Butylbenzene

Concen: 0.434 ug/l

RT: 11.637 min Scan# 3

Instrument:

Delta R.T. 0.003 min

MSVOA_U

Lab File: VU063511.D

ClientSampleId :

Acq: 16 Jul 2025 09:24

VSTDICC0.5

Tgt Ion:105 Resp: 1557

Ion Ratio Lower Upper


105 100

134 19.3 16.2 24.4


Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025



Abundance Scan 3713 (13.229 min): VU063511.D\data.ms (-)

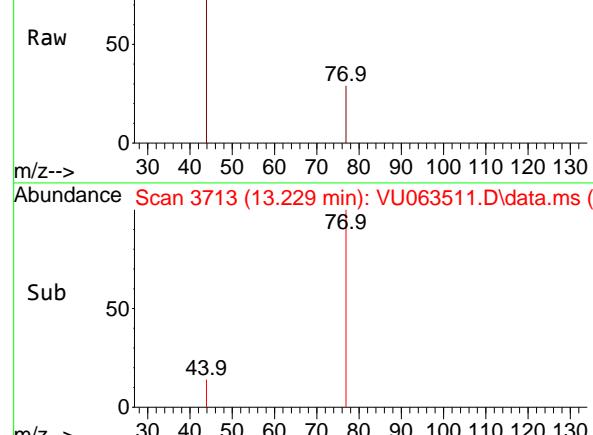

Abundance Scan 3713 (13.229 min): VU063511.D\data.ms (-)

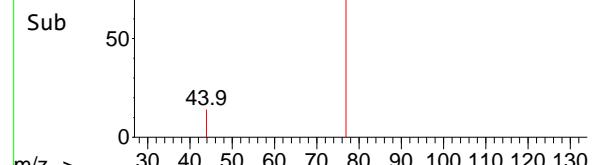

#80

Nitrobenzene

Concen: 2.628 ug/l

RT: 13.229 min Scan# 3713

Delta R.T. 0.026 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion: 77 Resp: 131



Ion Ratio Lower Upper

77 100

123 0.0 16.9 59.7#

65 0.0 16.5 20.9#



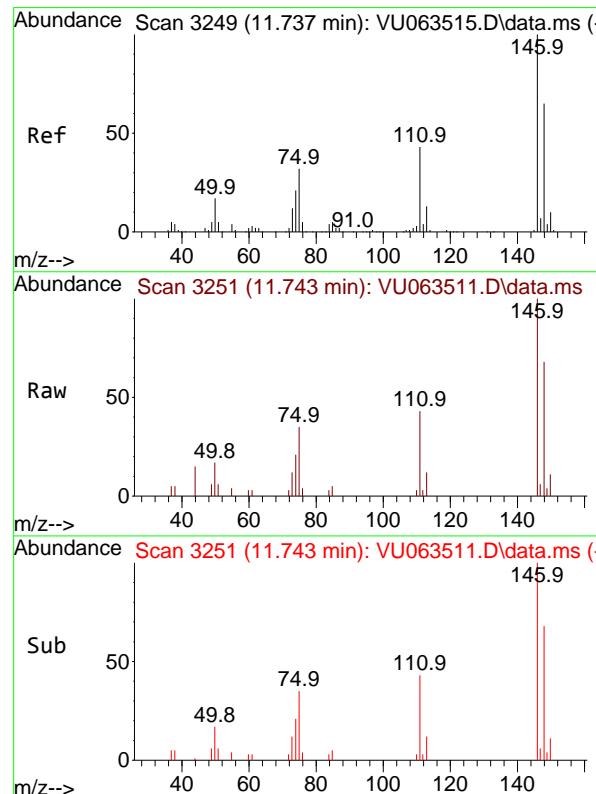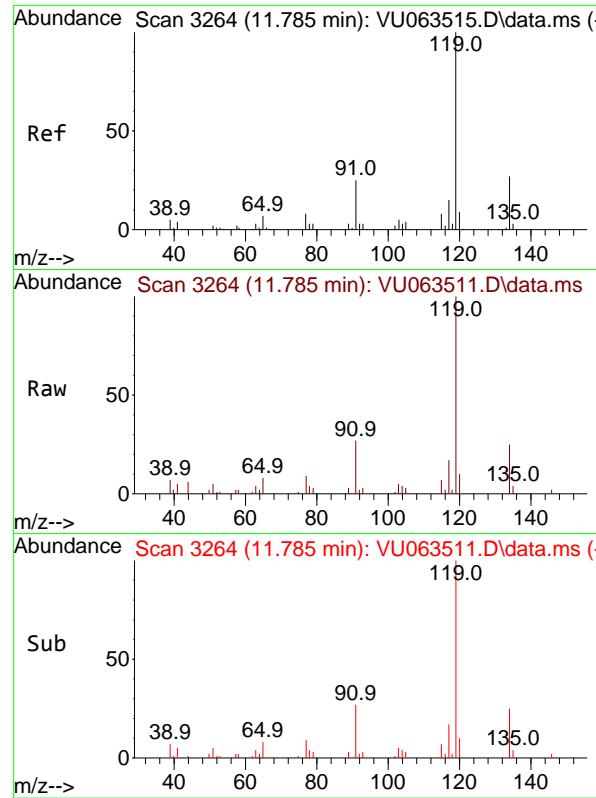

#81

p-Isopropyltoluene

Concen: 0.433 ug/l

RT: 11.785 min Scan# 3

Instrument : MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063511.D ClientSampleId :

Acq: 16 Jul 2025 09:24 VSTDICCO.5

Tgt Ion:119 Resp: 1300

Ion Ratio Lower Upper

119 100


134 26.0 21.1 31.7

91 27.6 19.8 29.8

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#82

1,3-Dichlorobenzene

Concen: 0.455 ug/l

RT: 11.743 min Scan# 3251

Delta R.T. 0.007 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24


Tgt Ion:146 Resp: 6856




Ion Ratio Lower Upper

146 100

111 40.7 33.8 50.6

148 66.7 51.5 77.3

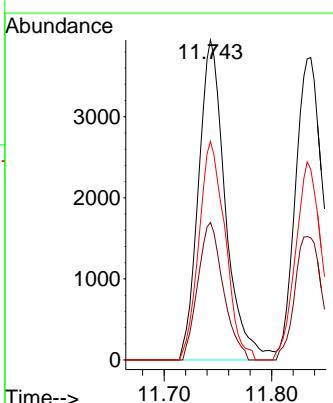

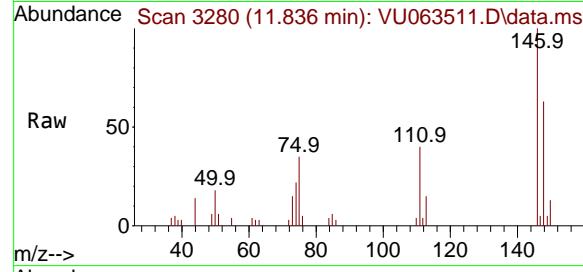

#83

1,4-Dichlorobenzene

Concen: 0.432 ug/l

RT: 11.836 min Scan# 3

Instrument : MSVOA_U

Delta R.T. 0.007 min

Lab File: VU063511.D




Acq: 16 Jul 2025 09:24

VSTDICCO.5

Tgt	Ion:146	Resp:	6510
Ion	Ratio	Lower	Upper
146	100		
111	42.7	32.0	48.0
148	67.1	50.2	75.2

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#84

n-Butylbenzene

Concen: 0.427 ug/l


RT: 12.206 min Scan# 3395




Delta R.T. 0.006 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Tgt	Ion: 91	Resp:	11864
Ion	Ratio	Lower	Upper
91	100		
92	49.0	41.5	62.3
134	23.6	20.6	30.8

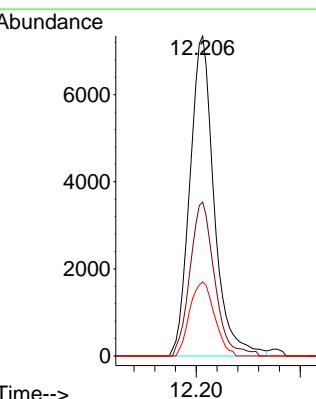

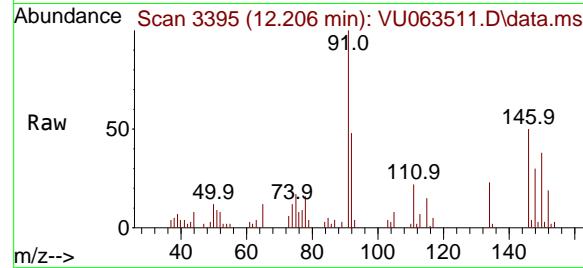

#85

1,2-Dichlorobenzene

Concen: 0.452 ug/l

RT: 12.206 min Scan# 3

Instrument: MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063511.D




Acq: 16 Jul 2025 09:24

VSTDICC0.5

Tgt	Ion:146	Resp:	640
Ion	Ratio	Lower	Upper
146	100		
111	46.3	21.7	65.1
148	61.8	31.8	95.3

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 0.533 ug/l


RT: 12.991 min Scan# 3639


Delta R.T. 0.004 min

Lab File: VU063511.D

Acq: 16 Jul 2025 09:24

Tgt	Ion: 75	Resp:	302
Ion	Ratio	Lower	Upper
75	100		
155	65.9	65.8	98.6
157	108.6	81.4	122.2

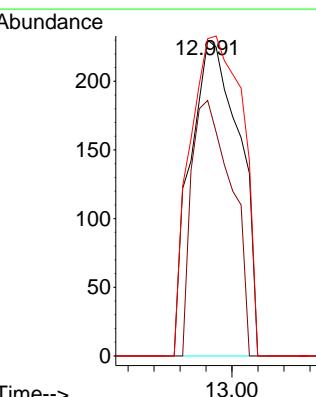


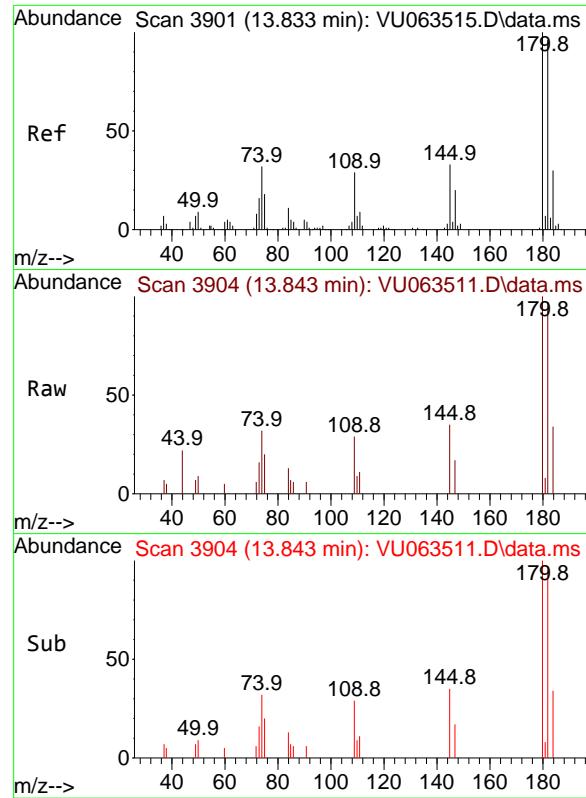


#87
 1,2,4-Trichlorobenzene
 Concen: 0.439 ug/l
 RT: 13.843 min Scan# 3904
 Delta R.T. 0.010 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
 ClientSampleId : VSTDICCO.5


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

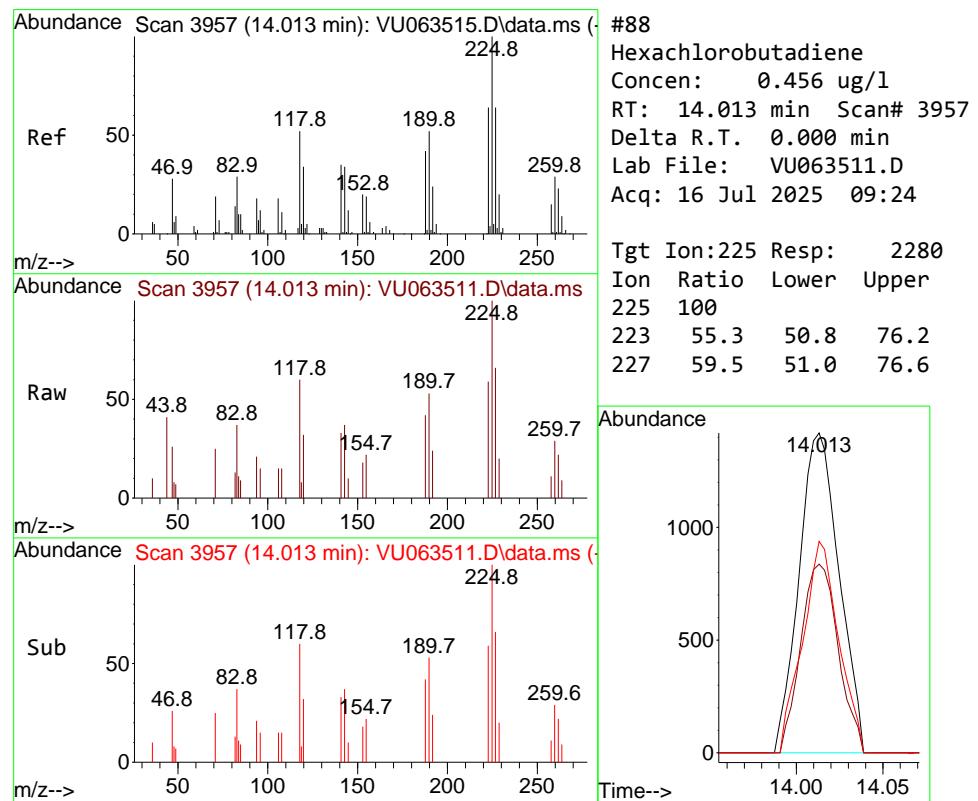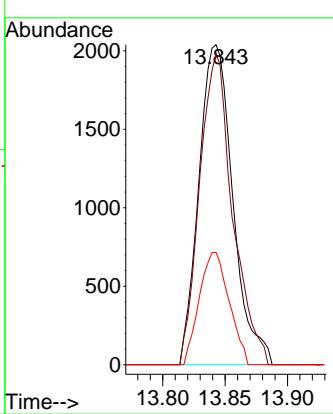

#88
 Hexachlorobutadiene
 Concen: 0.456 ug/l
 RT: 14.013 min Scan# 3957
 Delta R.T. 0.000 min
 Lab File: VU063511.D
 Acq: 16 Jul 2025 09:24

Tgt Ion:225 Resp: 2280
 Ion Ratio Lower Upper
 225 100
 223 55.3 50.8 76.2
 227 59.5 51.0 76.6

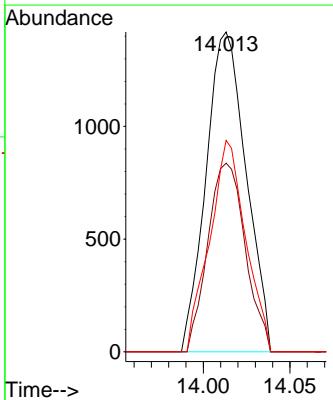

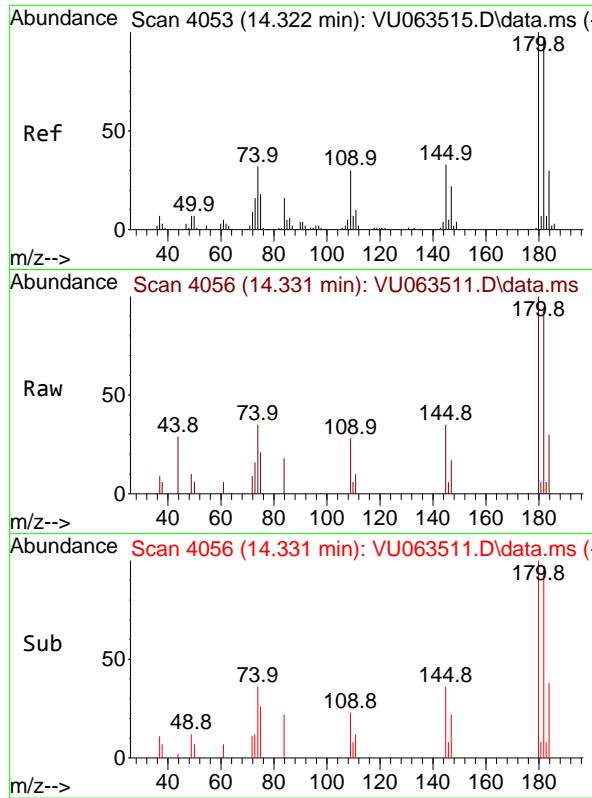


#90
1,2,3-Trichlorobenzene
Concen: 0.420 ug/l
RT: 14.331 min Scan# 4056
Delta R.T. 0.010 min
Lab File: VU063511.D
Acq: 16 Jul 2025 09:24

Instrument : MSVOA_U
ClientSampleId : VSTDICCO.5

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

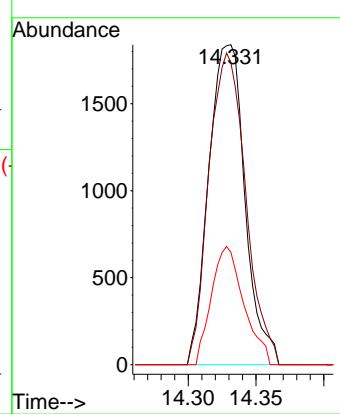

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063512.D
 Acq On : 16 Jul 2025 09:54
 Operator : MD/SY
 Sample : VSTDICC001
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC001

Quant Time: Jul 17 03:22:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	22455	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	9200	1.082	ug/l	0.00
Spiked Amount 1.000			Recovery	=	108.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	8165	1.038	ug/l	0.00
Spiked Amount 1.000			Recovery	=	104.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	6462	0.976	ug/l	96
3) Chloromethane	1.518	50	6530	1.061	ug/l	98
4) Vinyl Chloride	1.599	62	7920	1.010	ug/l	100
5) Bromomethane	1.846	94	6488	1.098	ug/l	95
6) Chloroethane	1.927	64	4751	1.004	ug/l	98
7) Trichlorofluoromethane	2.129	101	11403	1.013	ug/l	99
8) 1,1,2-Trichloro-1,2,2-...	2.570	101	5996	1.019	ug/l	99
9) 1,1-Dichloroethene	2.567	96	5877	1.008	ug/l	95
10) Iodomethane	2.708	142	5353	1.474	ug/l	98
11) Allyl Chloride	2.911	41	8367	0.993	ug/l	94
12) Acrylonitrile	3.306	53	3107	2.130	ug/l	95
13) Acetone	2.618	43	5459	4.673	ug/l	99
14) Carbon Disulfide	2.779	76	19044	1.011	ug/l	98
15) Methylene Chloride	3.030	84	7367	1.073	ug/l	91
16) trans-1,2-Dichloroethene	3.335	96	6995	1.056	ug/l	86
17) 1,1-Dichloroethane	3.849	63	12773	1.041	ug/l	99
18) 2-Butanone	4.714	43	9101	5.031	ug/l	99
19) Cyclohexane	5.354	56	11111	1.069	ug/l	99
20) Methylcyclohexane	6.743	83	9890	0.979	ug/l	98
21) 2,2-Dichloropropane	4.644	77	10936	1.047	ug/l	97
22) cis-1,2-Dichloroethene	4.644	96	7782	1.083	ug/l	96
23) Diethyl Ether	2.370	59	4538	1.022	ug/l	# 89
24) tert-Butyl Alcohol	3.190	59	5615	10.471	ug/l	95
25) Methyl tert-Butyl Ether	3.361	73	15721	1.033	ug/l	96
26) Bromochloromethane	4.959	128	2951	0.984	ug/l	95
27) Chloroform	5.071	83	13121	1.048	ug/l	96
28) 1,1,1-Trichloroethane	5.293	97	10709	1.008	ug/l	98
29) 1,1-Dichloropropene	5.502	75	10221	1.038	ug/l	99
30) Carbon Tetrachloride	5.496	117	8599	1.005	ug/l	99
31) Isopropyl Ether	3.994	45	19202	1.037	ug/l	98
32) Ethyl-t-butyl ether	4.502	59	17970	1.048	ug/l	97
33) Tert-Amyl methyl ether	5.943	73	13496	0.907	ug/l	98
34) Propionitrile	4.779	54	2874	5.214	ug/l	# 97
35) Benzene	5.756	78	22692	0.858	ug/l	99
36) 1,2-Dichloroethane	5.782	62	7451	0.906	ug/l	# 85
37) Trichloroethene	6.528	130	6347	0.940	ug/l	99
38) 1,2-Dichloropropane	6.782	63	5862	0.947	ug/l	98
39) Methacrylonitrile	4.972	41	2368	0.979	ug/l	89
40) Methyl acrylate	4.843	55	3610	1.008	ug/l	# 85
41) Tetrahydrofuran	5.065	42	2432	1.887	ug/l	93
42) 1-Chlorobutane	5.435	56	12913	0.987	ug/l	99
43) Dibromomethane	6.910	93	3011	0.939	ug/l	94
44) Bromodichloromethane	7.097	83	6824	0.943	ug/l	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063512.D
 Acq On : 16 Jul 2025 09:54
 Operator : MD/SY
 Sample : VSTDICC001
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTDICC001

Quant Time: Jul 17 03:22:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	16478	4.985	ug/1	96
46) t-1,4-Dichloro-2-butene	10.823	75	2681m	2.286	ug/1	
47) Methyl methacrylate	6.968	69	4791	1.779	ug/1	97
48) Ethyl methacrylate	8.338	69	4500	0.875	ug/1	84
49) Toluene	7.962	92	14592	1.010	ug/1	100
50) t-1,3-Dichloropropene	8.209	75	5194	0.915	ug/1	97
51) cis-1,3-Dichloropropene	7.602	75	6989	0.918	ug/1	99
52) 1,1,2-Trichloroethane	8.396	97	4414	1.022	ug/1	94
53) 1,3-Dichloropropane	8.569	76	7339	0.985	ug/1	100
54) 2-Hexanone	8.695	43	10847	4.940	ug/1	93
55) Dibromochloromethane	8.804	129	4122	0.903	ug/1	97
56) 1,2-Dibromoethane	8.920	107	3787	0.980	ug/1	99
58) Tetrachloroethene	8.541	164	6276	1.016	ug/1	97
59) Chlorobenzene	9.441	112	16495	0.994	ug/1	96
60) 1,1,1,2-Tetrachloroethane	9.524	131	5306	0.995	ug/1	98
61) Pentachloroethane	11.418	117	3370	0.894	ug/1	98
62) Hexachloroethane	12.466	117	3268	0.875	ug/1	97
63) Ethyl Benzene	9.563	91	28308	0.992	ug/1	98
64) m/p-Xylenes	9.688	106	21130	1.904	ug/1	97
65) o-Xylene	10.094	106	10385	0.974	ug/1	97
66) Styrene	10.110	104	16060	0.945	ug/1	98
67) Bromoform	10.286	173	1899	0.810	ug/1 #	94
69) Isopropylbenzene	10.476	105	25098	0.974	ug/1	99
70) 1,1,2,2-Tetrachloroethane	10.778	83	5141	0.978	ug/1 #	98
71) 1,2,3-Trichloropropane	10.817	75	4435m	1.034	ug/1	
72) Bromobenzene	10.778	156	6362	0.956	ug/1	96
73) n-propylbenzene	10.901	120	7341	0.946	ug/1	96
74) 2-Chlorotoluene	10.978	126	6695	0.976	ug/1	95
75) 1,3,5-Trimethylbenzene	11.081	105	23269	0.945	ug/1	99
76) 4-Chlorotoluene	11.094	126	6734	0.967	ug/1	99
77) tert-Butylbenzene	11.412	119	22171	0.942	ug/1	95
78) 1,2,4-Trimethylbenzene	11.463	105	23102	0.946	ug/1	100
79) sec-Butylbenzene	11.637	105	30908	0.974	ug/1	98
80) Nitrobenzene	13.232	77	400m	5.705	ug/1	
81) p-Isopropyltoluene	11.785	119	24799	0.936	ug/1	99
82) 1,3-Dichlorobenzene	11.743	146	12830	0.964	ug/1	98
83) 1,4-Dichlorobenzene	11.833	146	12848	0.964	ug/1	97
84) n-Butylbenzene	12.203	91	22541	0.917	ug/1	98
85) 1,2-Dichlorobenzene	12.206	146	12071	0.965	ug/1	98
86) 1,2-Dibromo-3-Chloropr...	12.991	75	603	0.991	ug/1	92
87) 1,2,4-Trichlorobenzene	13.839	180	7020	0.903	ug/1	98
88) Hexachlorobutadiene	14.013	225	4144	0.938	ug/1	98
89) Naphthalene	14.087	128	11965	0.859	ug/1	97
90) 1,2,3-Trichlorobenzene	14.325	180	6612	0.920	ug/1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063512.D
Acq On : 16 Jul 2025 09:54
Operator : MD/SY
Sample : VSTDIICC001
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1


Quant Time: Jul 17 03:22:19 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:16:16 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC001

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

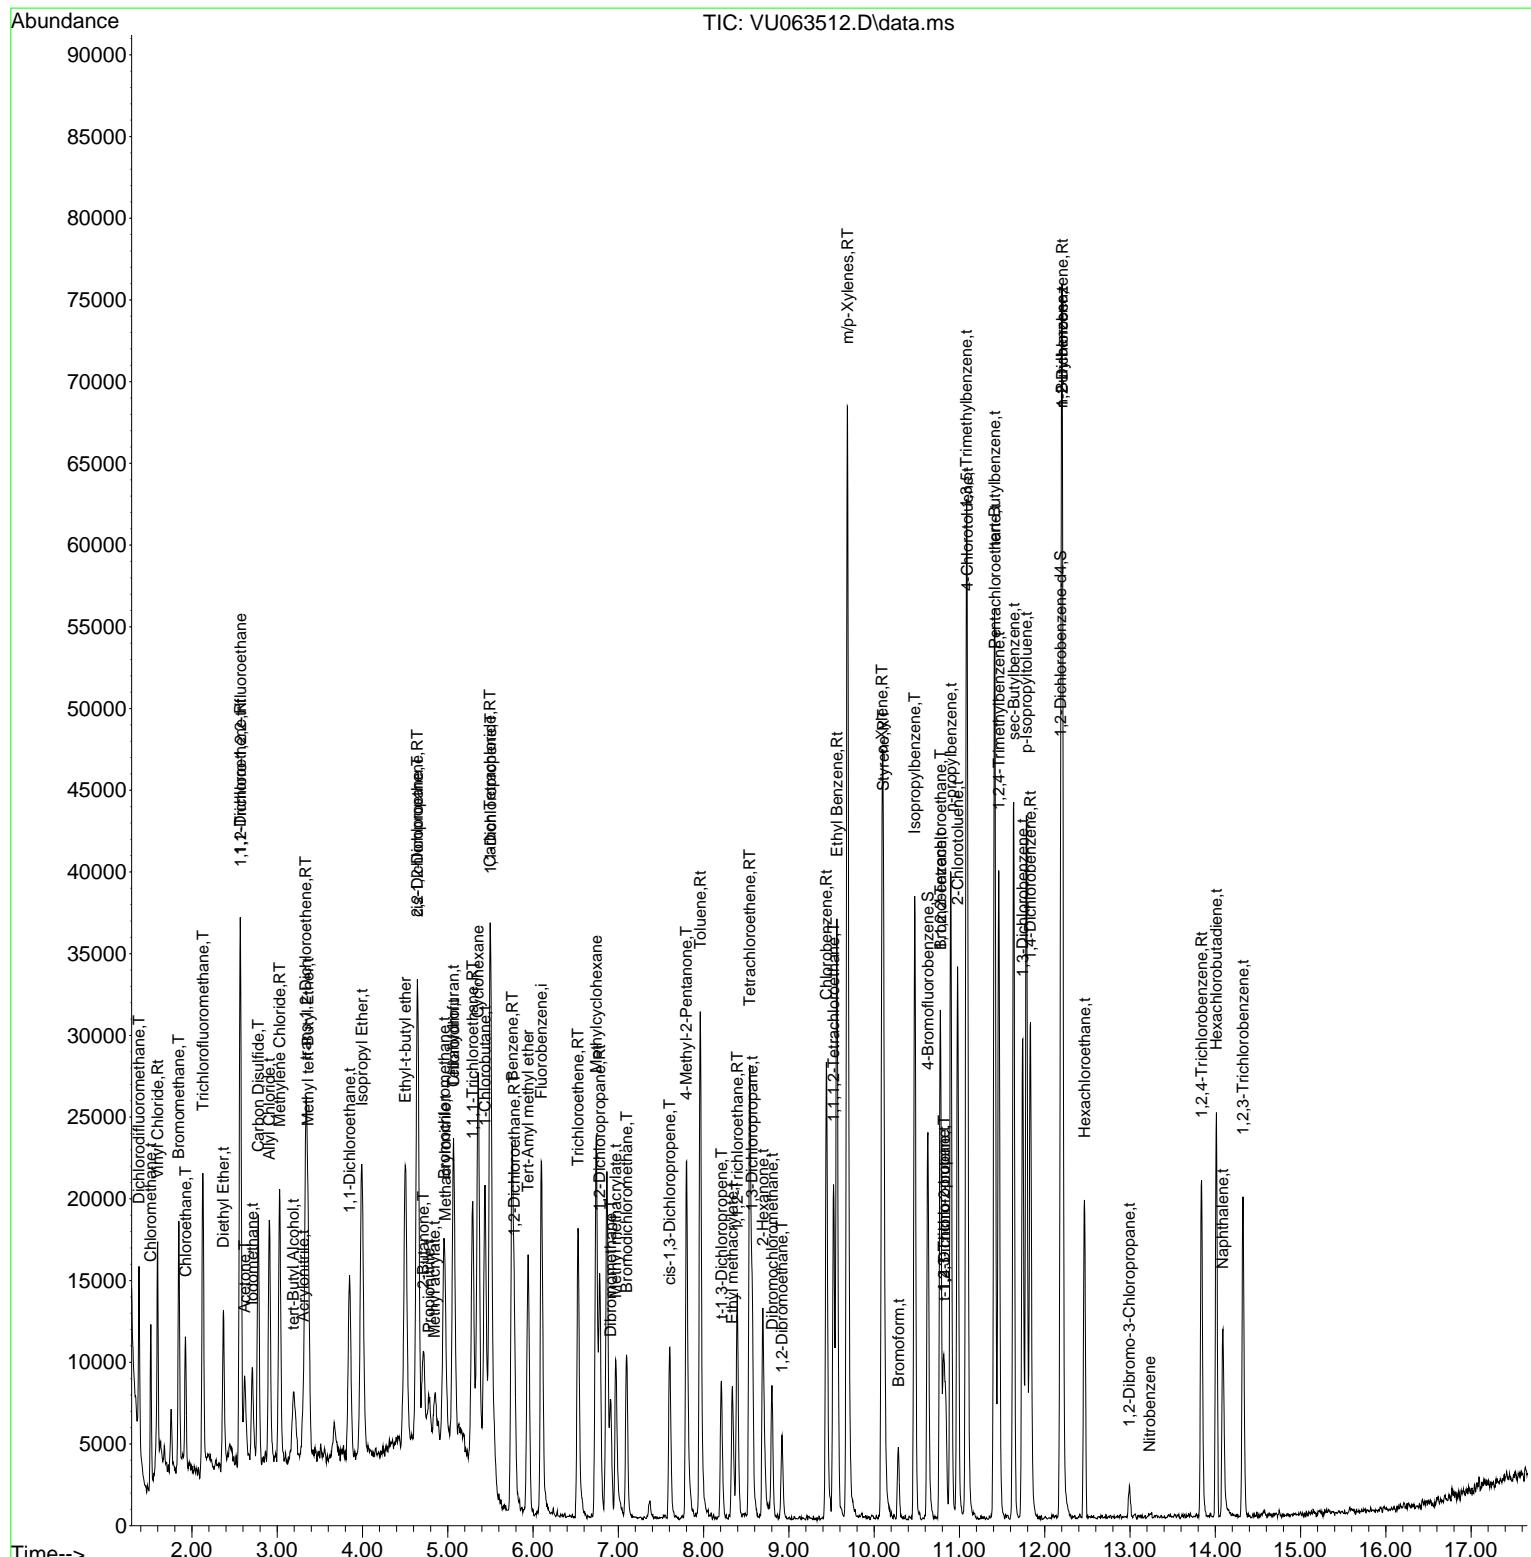

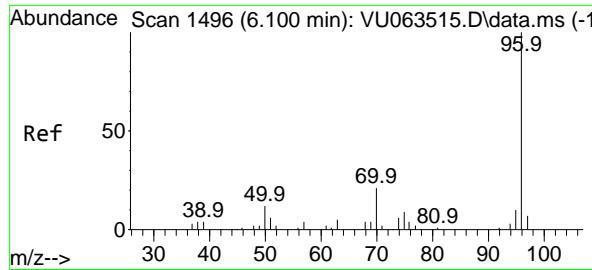

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
ClientSampleId : VSTDICC001






Tgt Ion: 96 Resp: 22451

Ion Ratio Lower Upper


Ion	Lower	Upper
96	100	
70	20.0	15.0
95	8.0	7.4
97	6.2	0.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

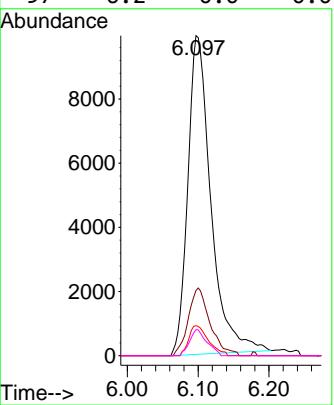
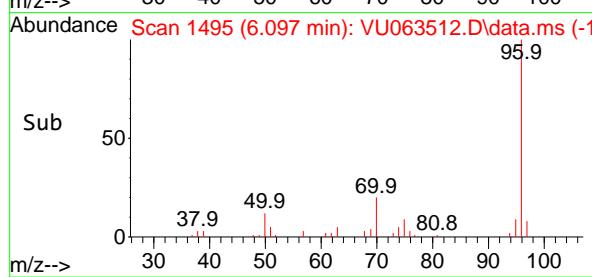





#2
Dichlorodifluoromethane
Concen: 0.976 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54



Tgt Ion: 85 Resp: 6462

Ion	Lower	Upper
85	100	
87	29.9	16.0

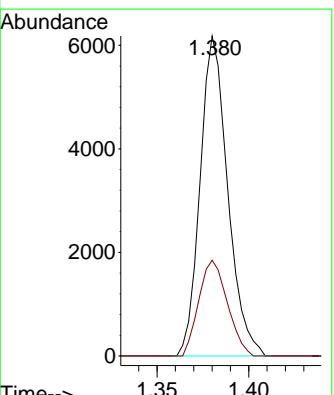







#3
Chloromethane
Concen: 1.061 ug/l
RT: 1.518 min Scan# 7
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
ClientSampleId : VSTDICC001


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

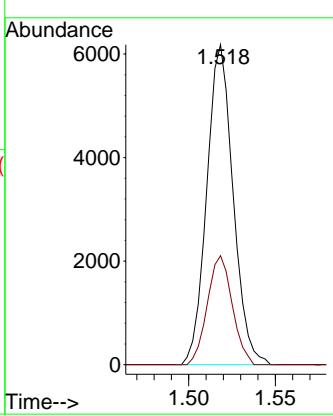

#4
Vinyl Chloride
Concen: 1.010 ug/l
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Tgt Ion: 62 Resp: 7920
Ion Ratio Lower Upper
62 100
64 32.3 25.7 38.5

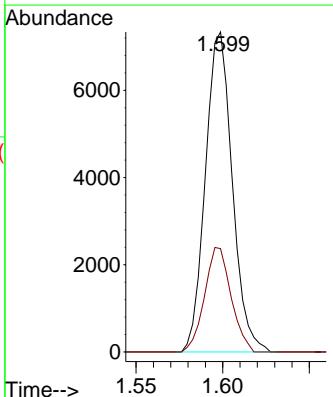


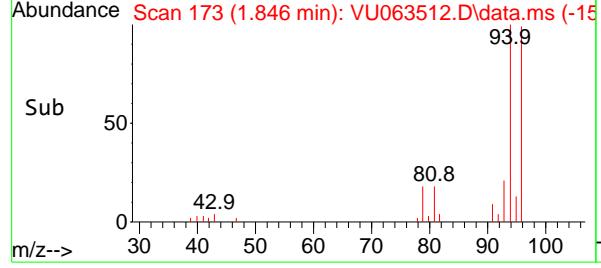
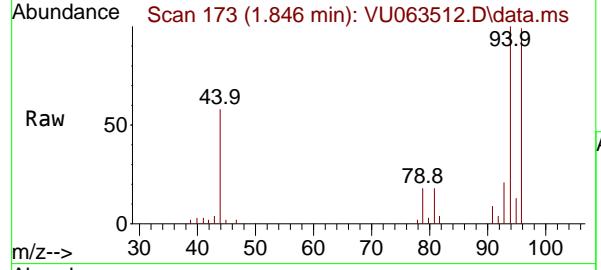



#5
 Bromomethane
 Concen: 1.098 ug/l
 RT: 1.846 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
 ClientSampleId : VSTDICC001


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

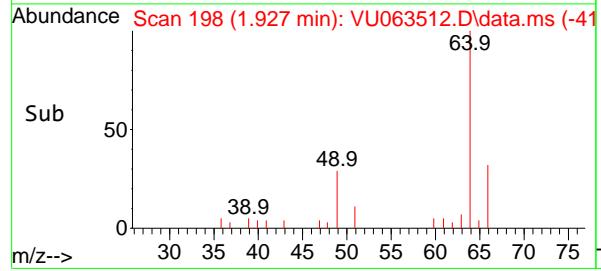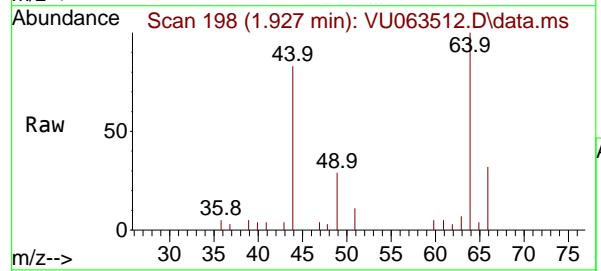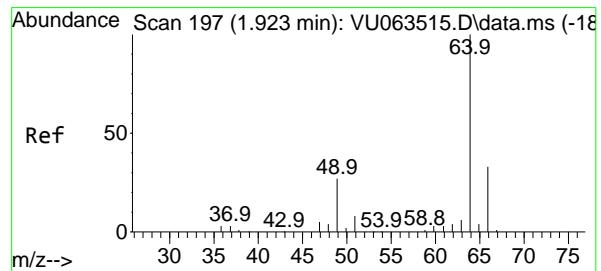

#6
 Chloroethane
 Concen: 1.004 ug/l
 RT: 1.927 min Scan# 198
 Delta R.T. 0.003 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54


Tgt Ion: 64 Resp: 4751
 Ion Ratio Lower Upper
 64 100
 66 31.5 26.2 39.4

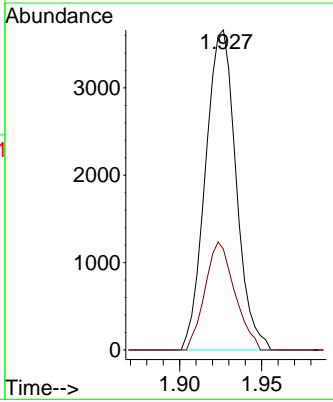



#7
Trichlorofluoromethane
Concen: 1.013 ug/l
RT: 2.129 min Scan# 2
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
ClientSampleId : VSTDICC001




Tgt Ion:101 Resp: 11400
Ion Ratio Lower Upper
101 100
103 65.9 52.2 78.4

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

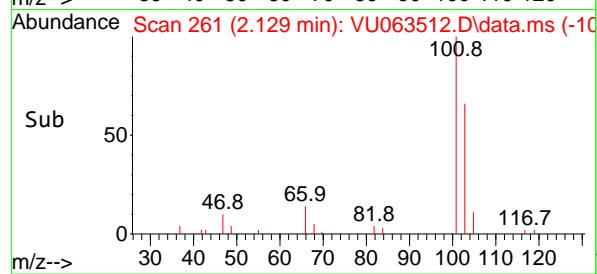


#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 1.019 ug/l
RT: 2.570 min Scan# 398
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Tgt Ion:101 Resp: 5996
Ion Ratio Lower Upper
101 100
85 47.3 37.8 56.6
151 75.6 59.2 88.8

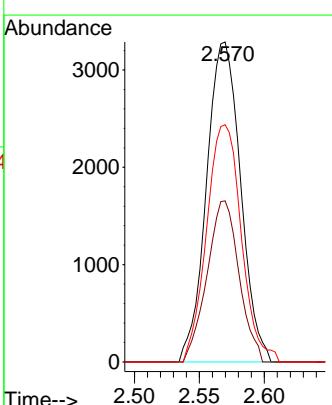



#9
1,1-Dichloroethene
Concen: 1.008 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
ClientSampleId : VSTDICC001

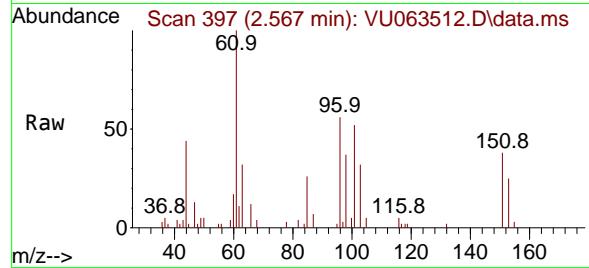


Tgt Ion: 96 Resp: 587
Ion Ratio Lower Upper
96 100
61 177.4 0.0 504.3
98 64.8 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#10
Iodomethane
Concen: 1.474 ug/l
RT: 2.708 min Scan# 441
Delta R.T. -0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Tgt Ion:142 Resp: 5353
Ion Ratio Lower Upper
142 100
127 46.2 37.9 56.9

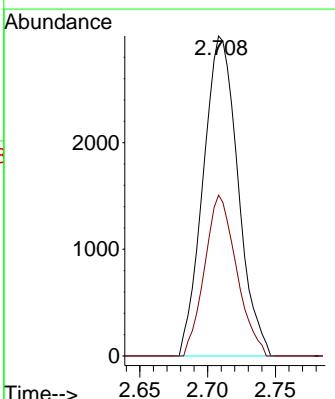



#11
Allyl Chloride
 Concen: 0.993 ug/l
 RT: 2.911 min Scan# 5
 Delta R.T. 0.003 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
 ClientSampleId : VSTDICC001

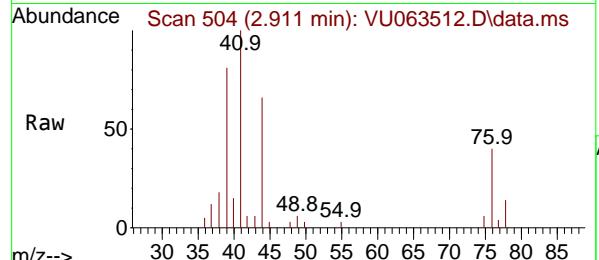


Tgt Ion: 41 Resp: 836
 Ion Ratio Lower Upper
 41 100
 39 82.2 61.5 92.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

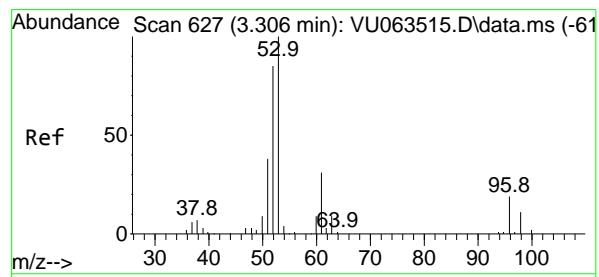
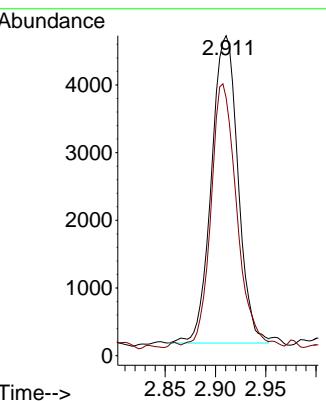
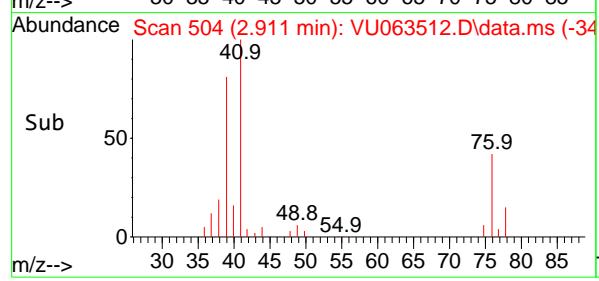


#12
Acrylonitrile
 Concen: 2.130 ug/l
 RT: 3.306 min Scan# 627
 Delta R.T. 0.000 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54



Tgt Ion: 53 Resp: 3107
 Ion Ratio Lower Upper
 53 100
 52 73.7 64.3 96.5
 51 35.1 27.8 41.8

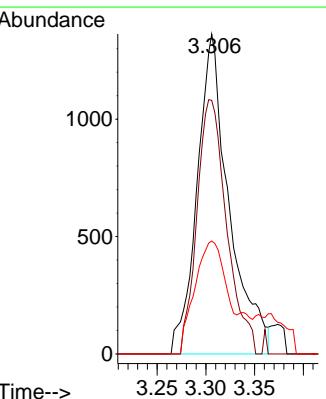

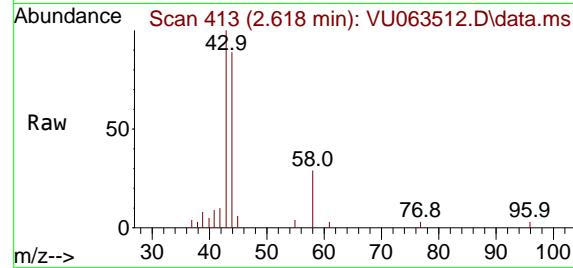

#13

Acetone

Concen: 4.673 ug/l

RT: 2.618 min Scan# 4

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

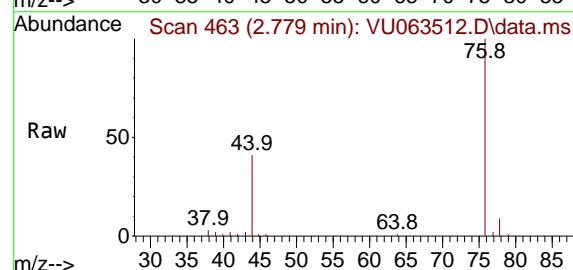 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#14

Carbon Disulfide

Concen: 1.011 ug/l

RT: 2.779 min Scan# 463

Delta R.T. 0.003 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54




Tgt Ion: 76 Resp: 19044

Ion Ratio Lower Upper

76 100

78 9.4 7.0 10.6

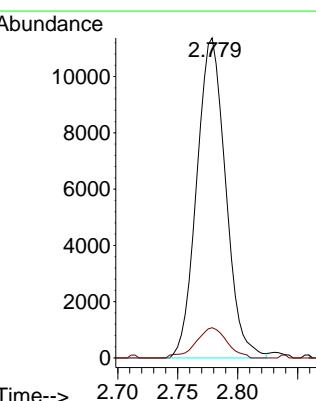

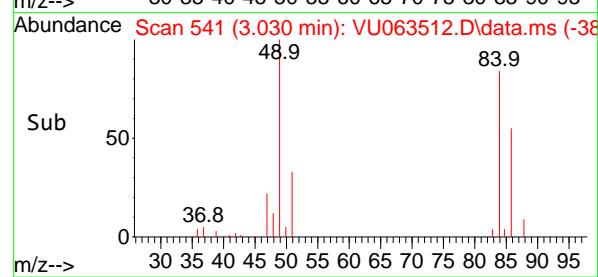

#15

Methylene Chloride

Concen: 1.073 ug/l

RT: 3.030 min Scan# 541

Delta R.T. 0.000 min

Lab File: VU063512.D




Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

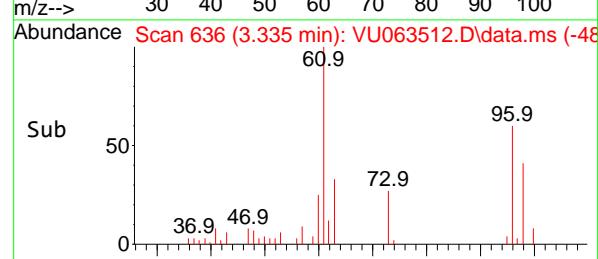 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#16

trans-1,2-Dichloroethene

Concen: 1.056 ug/l

RT: 3.335 min Scan# 636

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt Ion: 96 Resp: 6995

Ion Ratio Lower Upper

96 100


61 167.9 117.2 175.8

98 68.9 51.4 77.2


Time--> 2.95 3.00 3.05 3.10




Time--> 3.25 3.30 3.35 3.40

Abundance



Abundance

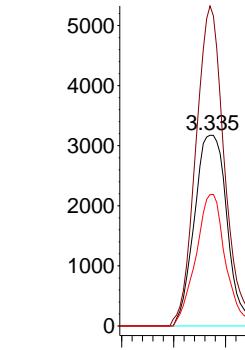



#17

1,1-Dichloroethane

Concen: 1.041 ug/l

RT: 3.849 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#18

2-Butanone

Concen: 5.031 ug/l

RT: 4.714 min Scan# 1065

Delta R.T. 0.003 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54


Tgt Ion: 43 Resp: 9101

Ion Ratio Lower Upper

43 100

57 7.7 0.0 16.4

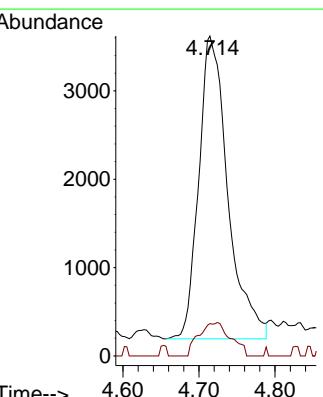


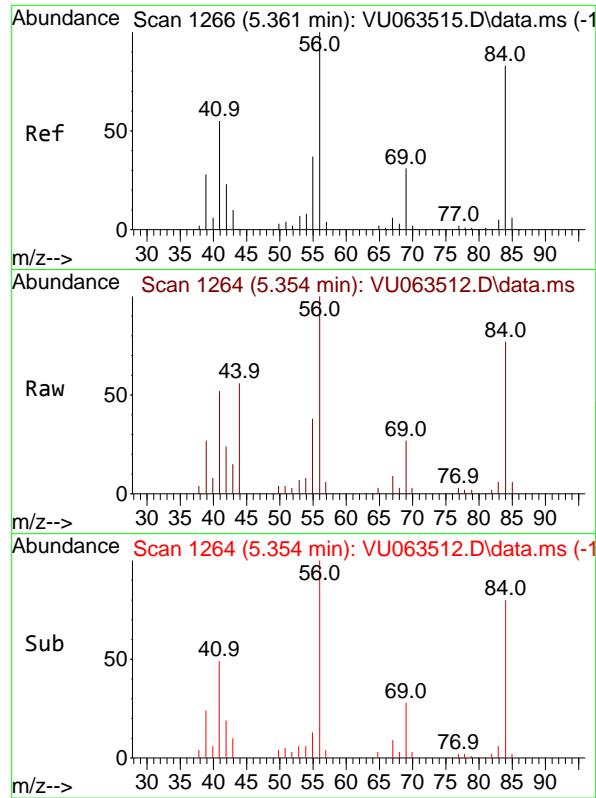


#19
Cyclohexane
Concen: 1.069 ug/l
RT: 5.354 min Scan# 1
Delta R.T. -0.006 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
ClientSampleId : VSTDICC001


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

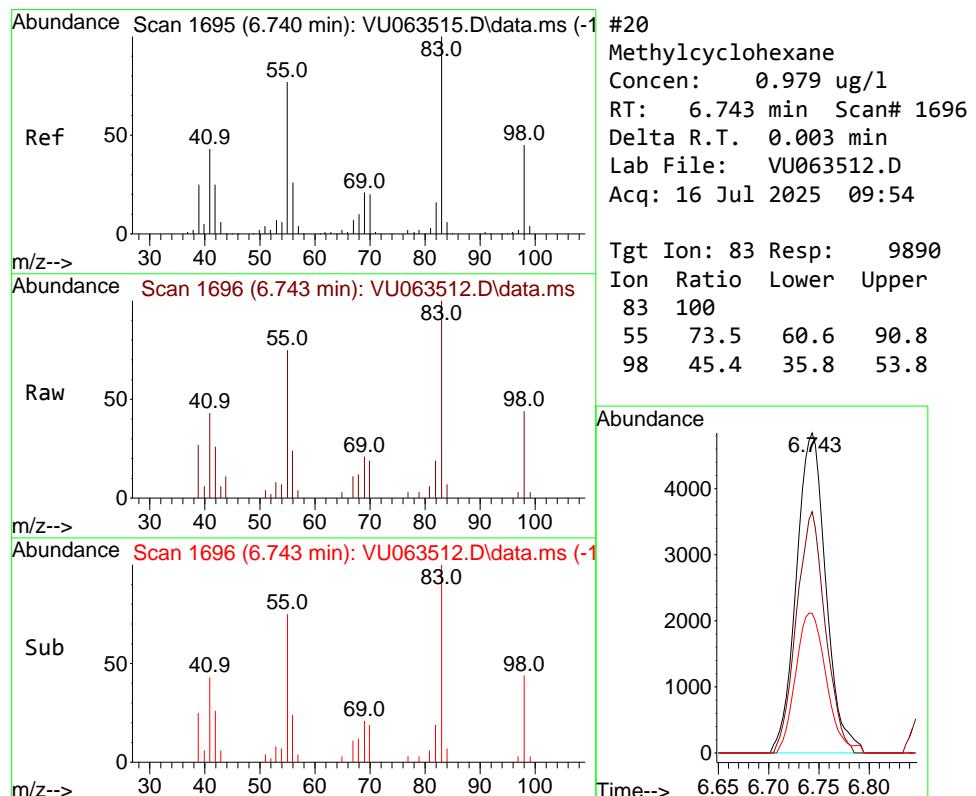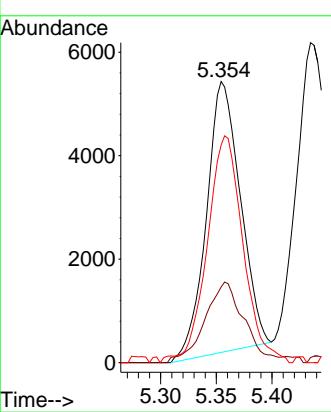

#20
Methylcyclohexane
Concen: 0.979 ug/l
RT: 6.743 min Scan# 1696
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54


Tgt Ion: 83 Resp: 9890
Ion Ratio Lower Upper
83 100
55 73.5 60.6 90.8
98 45.4 35.8 53.8

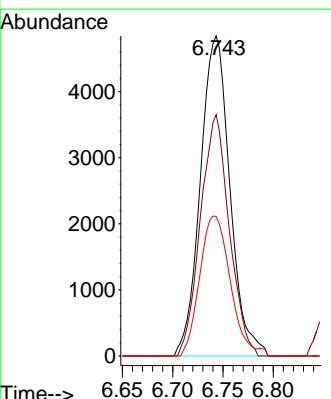



#21
2,2-Dichloropropane
Concen: 1.047 ug/l
RT: 4.644 min Scan# 1043
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
ClientSampleId : VSTDICC001



Tgt Ion: 77 Resp: 10930
Ion Ratio Lower Upper
77 100
97 20.7 17.8 26.8



Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

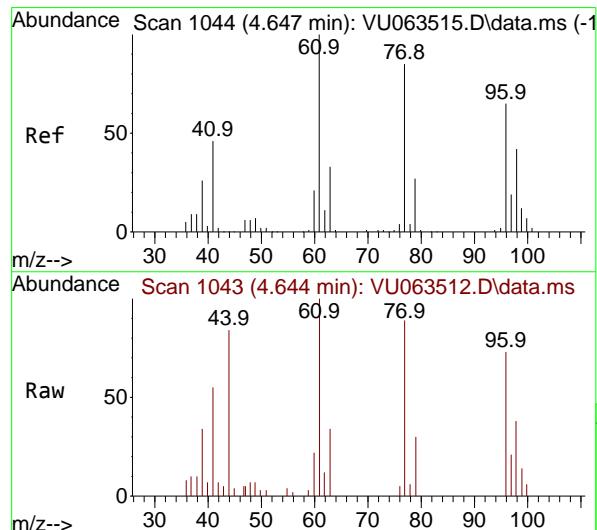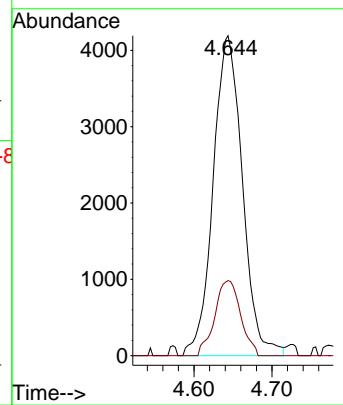

#22
cis-1,2-Dichloroethene
Concen: 1.083 ug/l
RT: 4.644 min Scan# 1043
Delta R.T. -0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Tgt Ion: 96 Resp: 7782
Ion Ratio Lower Upper
96 100
61 147.2 0.0 384.7
98 62.3 32.1 96.3

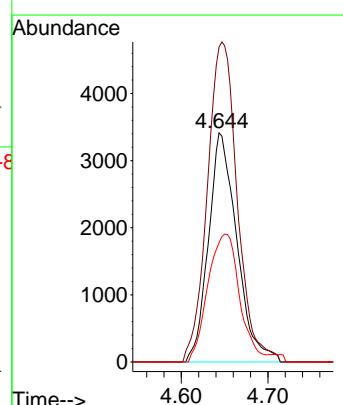

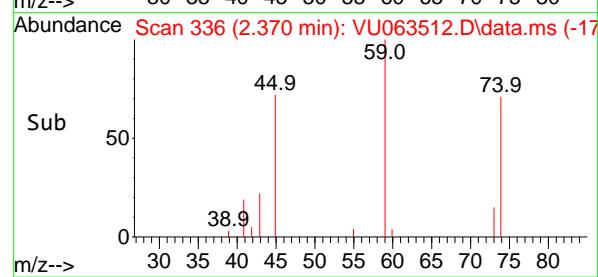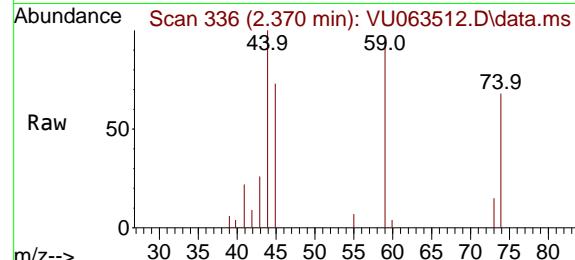

#23

Diethyl Ether

Concen: 1.022 ug/l

RT: 2.370 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

Tgt Ion: 59 Resp: 4538

Ion Ratio Lower Upper

59 100

45 84.9 55.1 82.7


74 70.6 58.2 87.4

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#24

tert-Butyl Alcohol

Concen: 10.471 ug/l

RT: 3.190 min Scan# 591

Delta R.T. 0.000 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54


Tgt Ion: 59 Resp: 5615

Ion Ratio Lower Upper

59 100

57 8.7 8.6 12.8

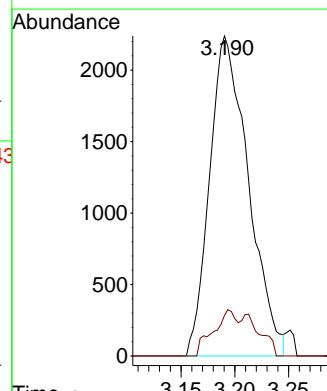

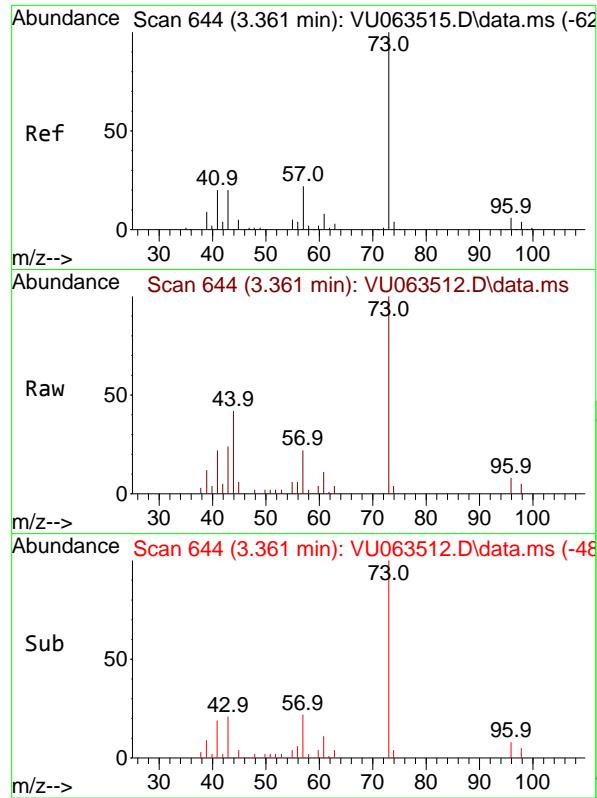

#25



Methyl tert-Butyl Ether
Concen: 1.033 ug/l
RT: 3.361 min Scan# 6

Instrument : MSVOA_U
ClientSampleId : VSTDICC001
Acq: 16 Jul 2025 09:54

Tgt Ion: 73 Resp: 1572
Ion Ratio Lower Upper
73 100
43 21.8 16.2 24.2

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

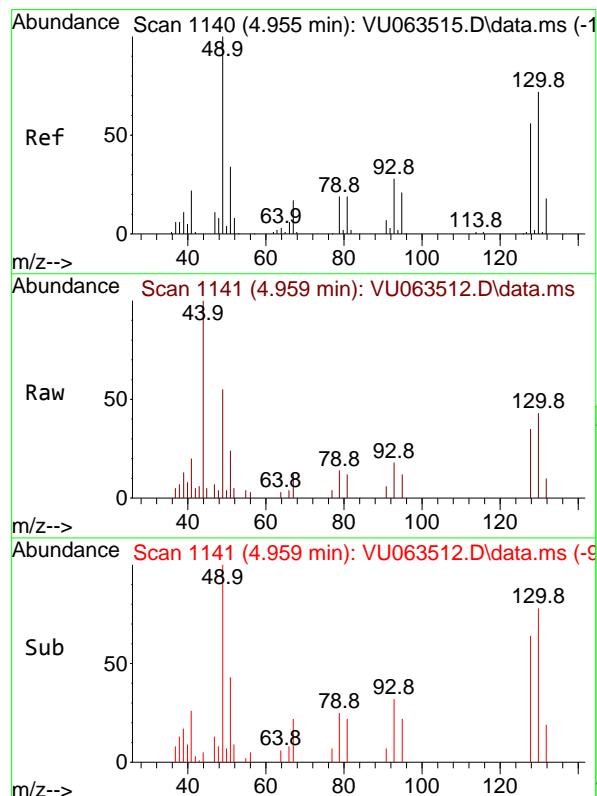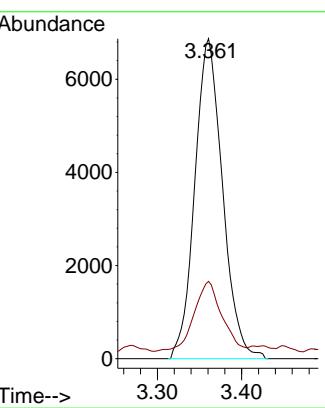


#26

Bromochloromethane
Concen: 0.984 ug/l
RT: 4.959 min Scan# 1141
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54


Tgt Ion:128 Resp: 2951
Ion Ratio Lower Upper
128 100
49 175.9 0.0 340.8
130 133.8 100.5 150.7

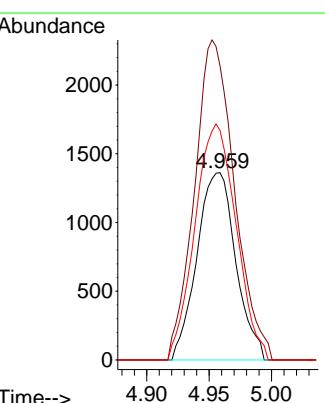



#27
 Chloroform
 Concen: 1.048 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
 ClientSampleId : VSTDICC001

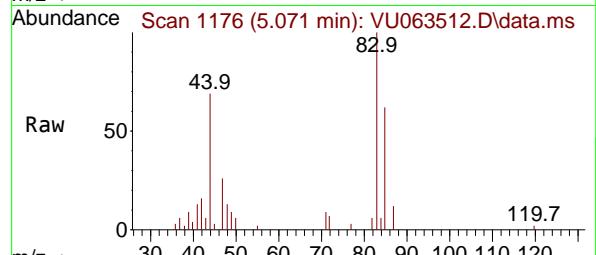


Tgt Ion: 83 Resp: 1312
 Ion Ratio Lower Upper
 83 100
 85 61.7 0.0 130.0

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

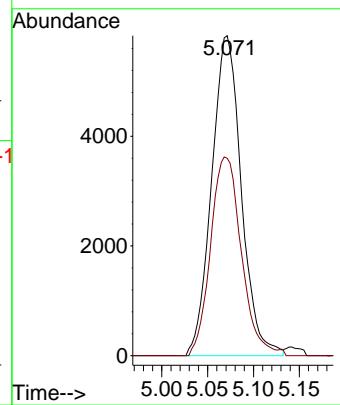


#28
 1,1,1-Trichloroethane
 Concen: 1.008 ug/l
 RT: 5.293 min Scan# 1245
 Delta R.T. -0.003 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54

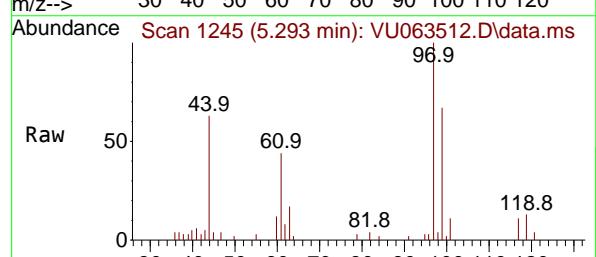

Tgt Ion: 97 Resp: 10709
 Ion Ratio Lower Upper
 97 100
 99 65.0 31.8 95.3
 61 47.7 23.3 69.9

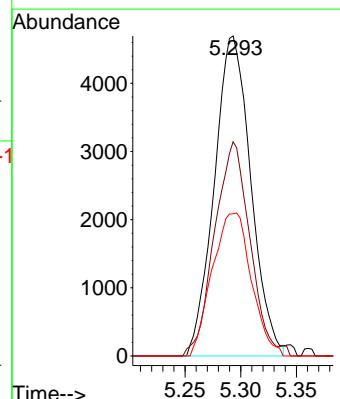

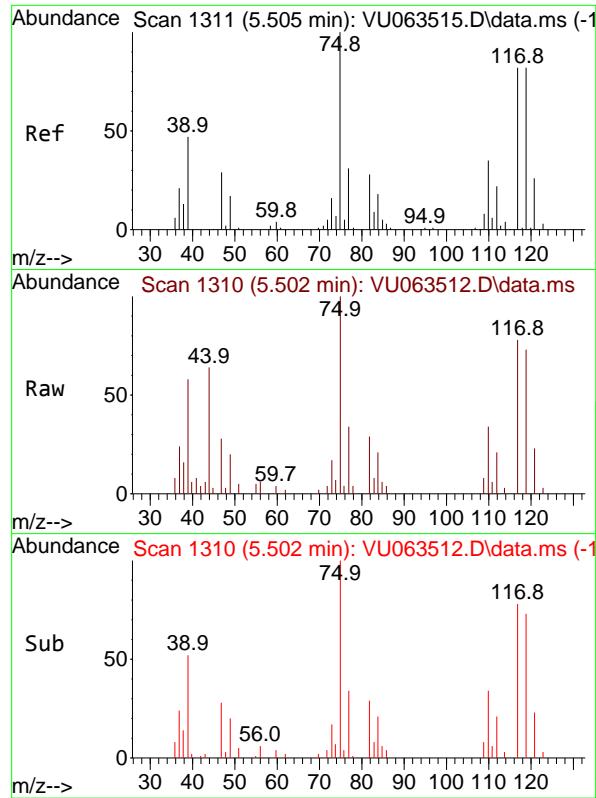

#29

1,1-Dichloropropene


Concen: 1.038 ug/l

RT: 5.502 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54


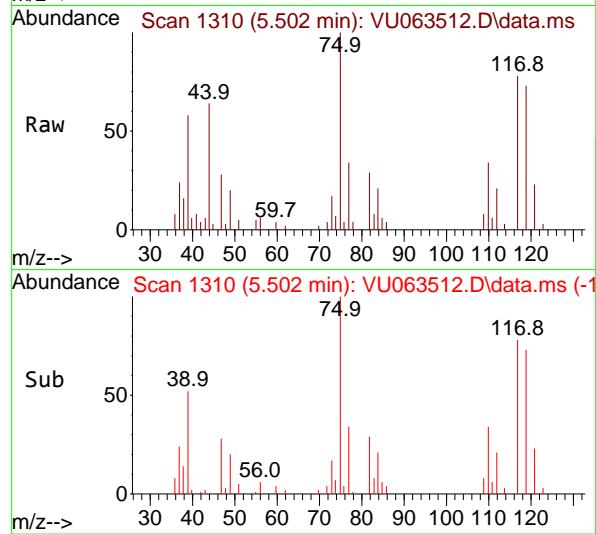


Tgt Ion: 75 Resp: 1022

Ion Ratio	Lower	Upper
75	100	
110	34.3	17.8
77	30.5	24.6

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

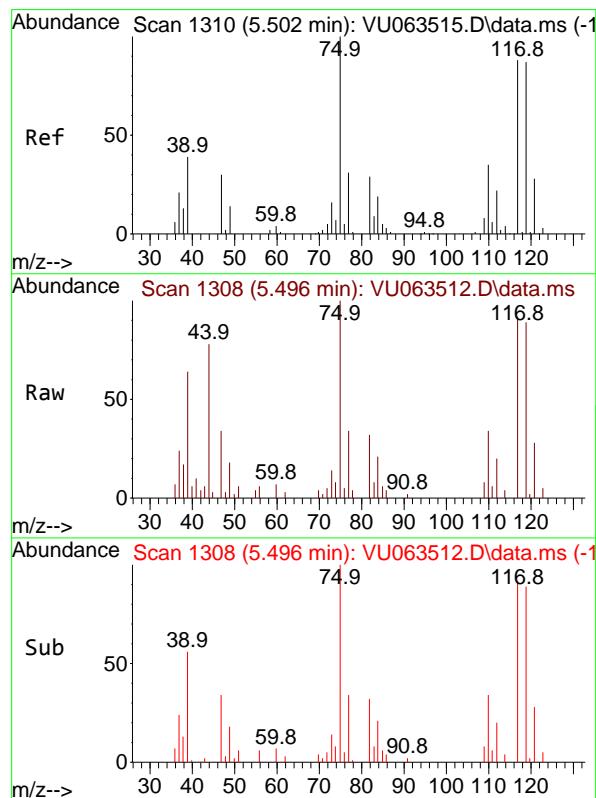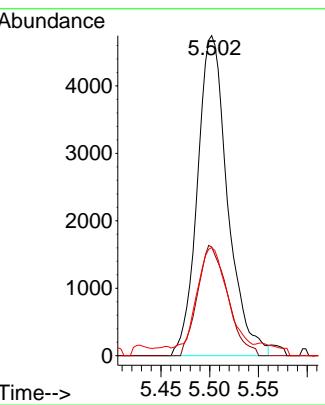

#30

Carbon Tetrachloride

Concen: 1.005 ug/l

RT: 5.496 min Scan# 1308


Delta R.T. -0.006 min




Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt Ion:117 Resp: 8599

Ion Ratio	Lower	Upper
117	100	
119	99.4	79.2
121	30.1	25.5

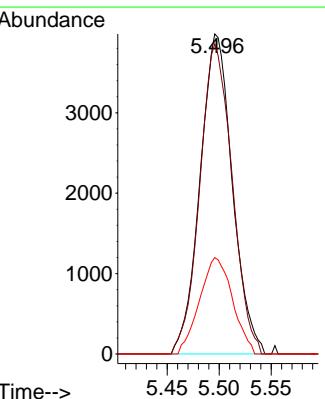

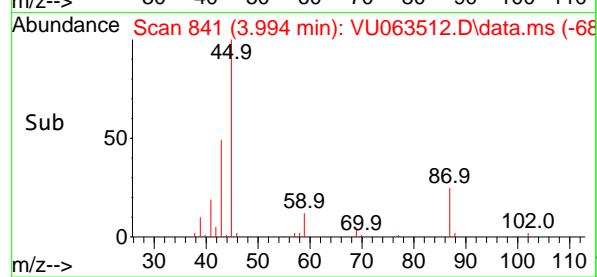

#31

Isopropyl Ether

Concen: 1.037 ug/l

RT: 3.994 min Scan# 8

Instrument :

Delta R.T. 0.003 min

MSVOA_U

Lab File: VU063512.D

ClientSampleId :

Acq: 16 Jul 2025 09:54

VSTDICC001

Tgt Ion: 45 Resp: 1920

Ion Ratio Lower Upper




45 100

43 52.6 25.7 77.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

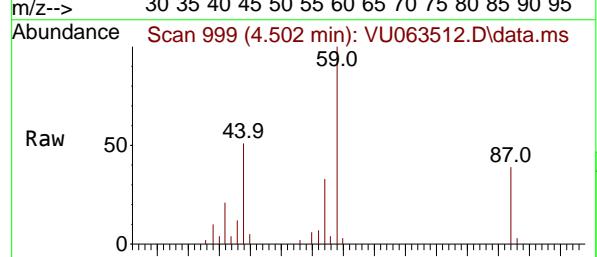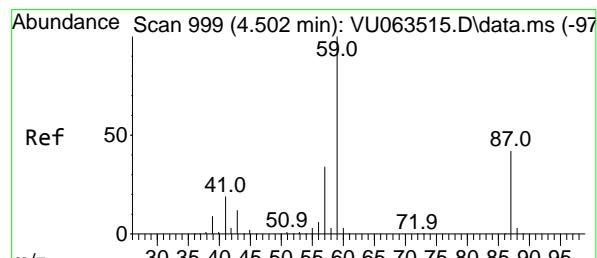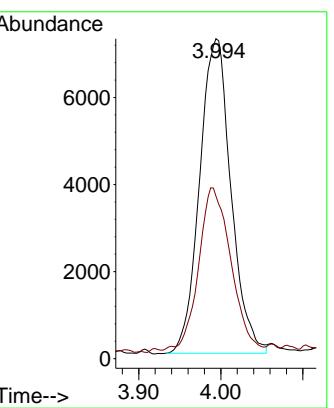

#32

Ethyl-t-butyl ether

Concen: 1.048 ug/l

RT: 4.502 min Scan# 999

Delta R.T. 0.000 min

Lab File: VU063512.D



Acq: 16 Jul 2025 09:54




Tgt Ion: 59 Resp: 17970

Ion Ratio Lower Upper

59 100

87 42.8 32.6 49.0

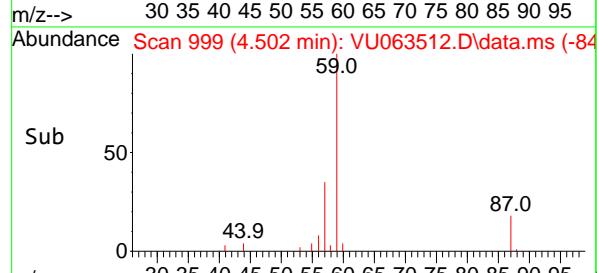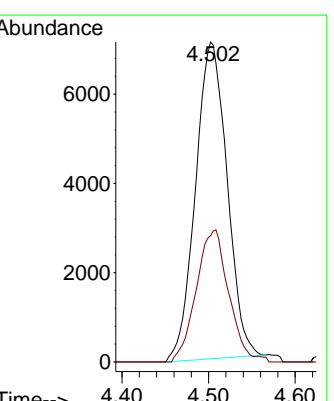

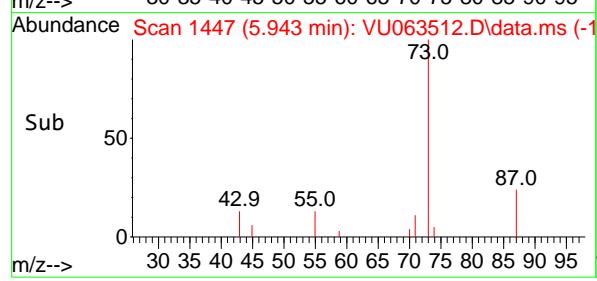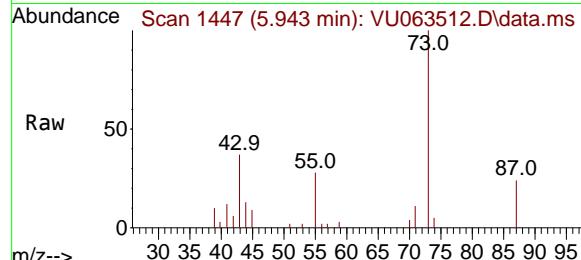

#33

Tert-Amyl methyl ether

Concen: 0.907 ug/l

RT: 5.943 min Scan# 13490

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54





Instrument:

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

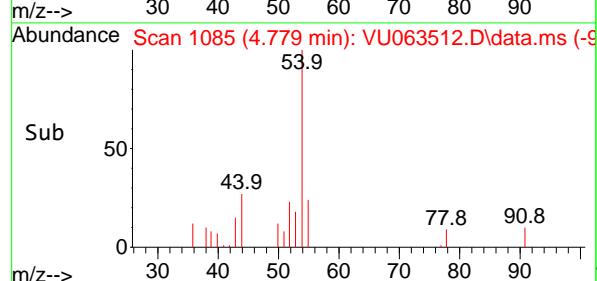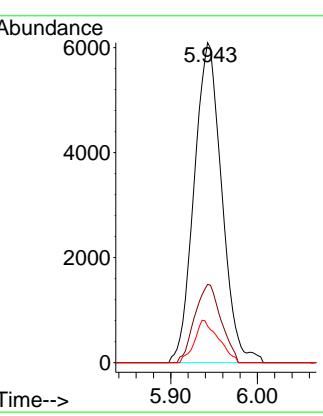 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#34

Propionitrile

Concen: 5.214 ug/l


RT: 4.779 min Scan# 1085


Delta R.T. 0.006 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54


Tgt	Ion	Resp:	2874
Ion	Ratio	Lower	Upper
54	100		
52	20.1	17.0	25.4
55	16.6	13.6	20.4
40	4.1	6.4	9.6#

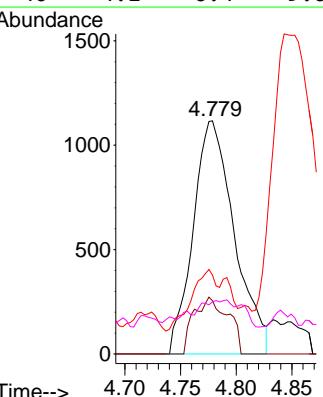



#35
Benzene
Concen: 0.858 ug/l
RT: 5.756 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
ClientSampleId : VSTDICC001




Tgt Ion: 78 Resp: 2269:
Ion Ratio Lower Upper
78 100
77 25.0 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

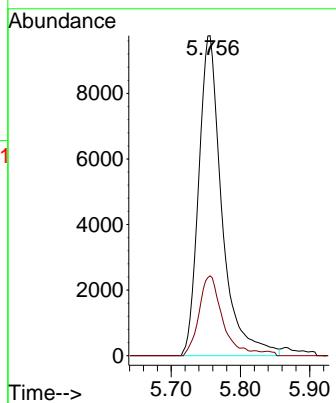


#36
1,2-Dichloroethane
Concen: 0.906 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Tgt Ion: 62 Resp: 7451
Ion Ratio Lower Upper
62 100
98 2.7 6.4 9.6#

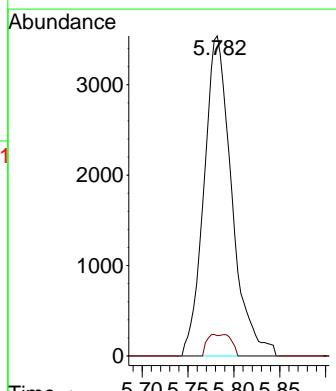



#37
Trichloroethene
Concen: 0.940 ug/l
RT: 6.528 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
ClientSampleId : VSTDICC001




Tgt Ion:130 Resp: 6341
Ion Ratio Lower Upper
130 100
95 100.9 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


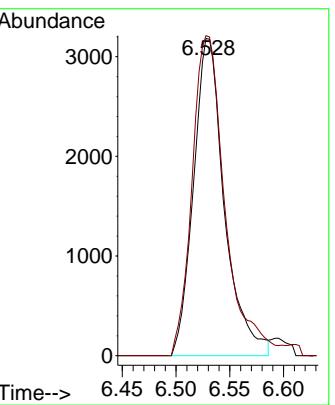
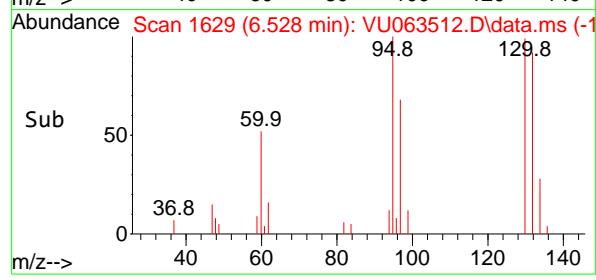


#38
1,2-Dichloropropane
Concen: 0.947 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54



Tgt Ion: 63 Resp: 5862
Ion Ratio Lower Upper
63 100
65 32.0 24.6 36.8

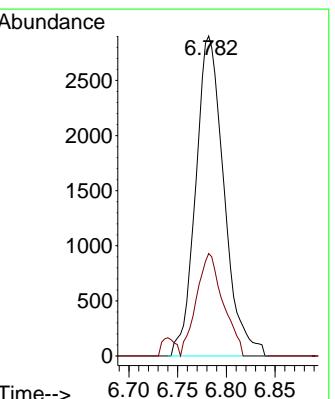

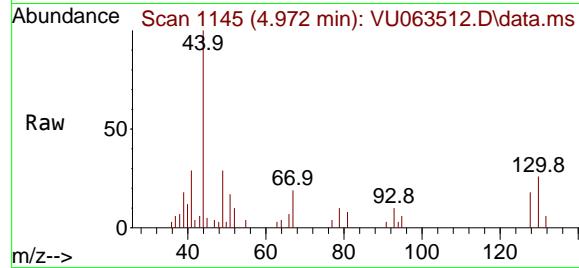

#39

Methacrylonitrile

Concen: 0.979 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

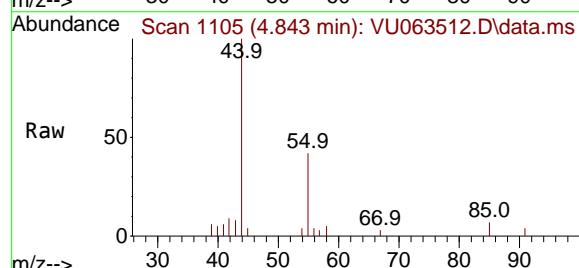 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#40

Methyl acrylate

Concen: 1.008 ug/l

RT: 4.843 min Scan# 1105

Delta R.T. -0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt Ion: 55 Resp: 3610



Ion Ratio Lower Upper


55 100

85 8.5 12.8 19.2#

58 9.1 7.0 10.4

42 16.8 7.0 10.4#

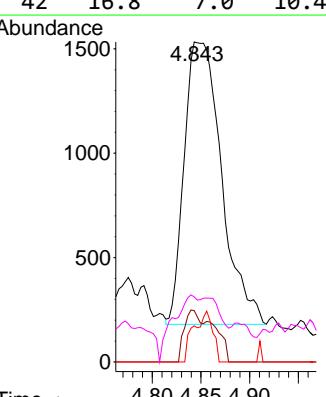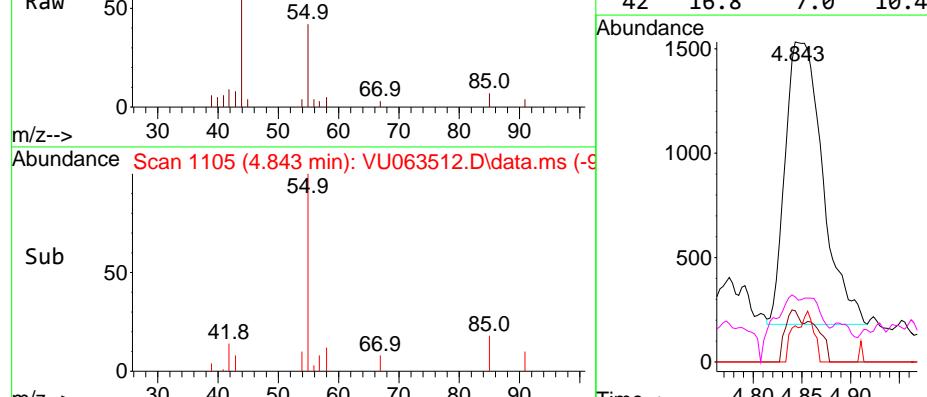



#41

Tetrahydrofuran

Concen: 1.887 ug/l

RT: 5.065 min Scan# 1

Delta R.T. 0.006 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001



Tgt Ion: 42 Resp: 243.0

Ion Ratio Lower Upper

42 100







72 45.0 39.2 58.8


71 49.1 34.8 52.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025
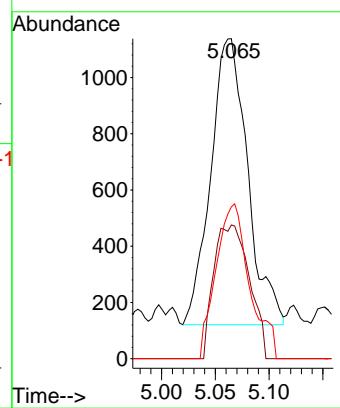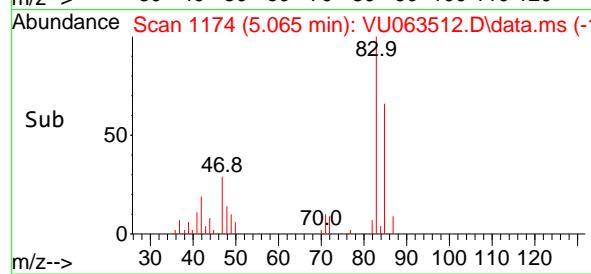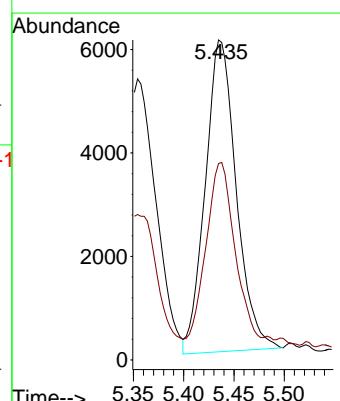
#42
1-Chlorobutane
Concen: 0.987 ug/l
RT: 5.435 min Scan# 1289
Delta R.T. -0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54



#43
Dibromomethane
Concen: 0.939 ug/l
RT: 6.910 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54




Instrument : MSVOA_U
ClientSampleId : VSTDICC001




Tgt Ion: 93 Resp: 301
Ion Ratio Lower Upper
93 100
95 81.8 67.9 101.9
174 86.0 74.6 111.8

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

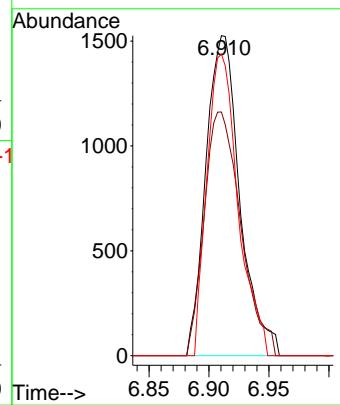


#44
Bromodichloromethane
Concen: 0.943 ug/l
RT: 7.097 min Scan# 1806
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54



Tgt Ion: 83 Resp: 6824
Ion Ratio Lower Upper
83 100
85 70.4 52.7 79.1
127 9.6 8.1 12.1


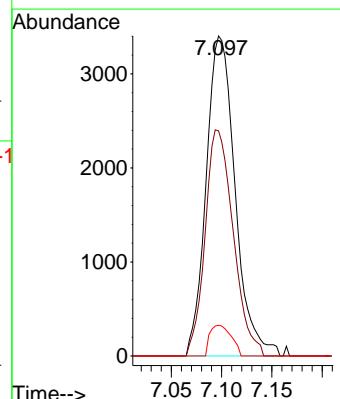


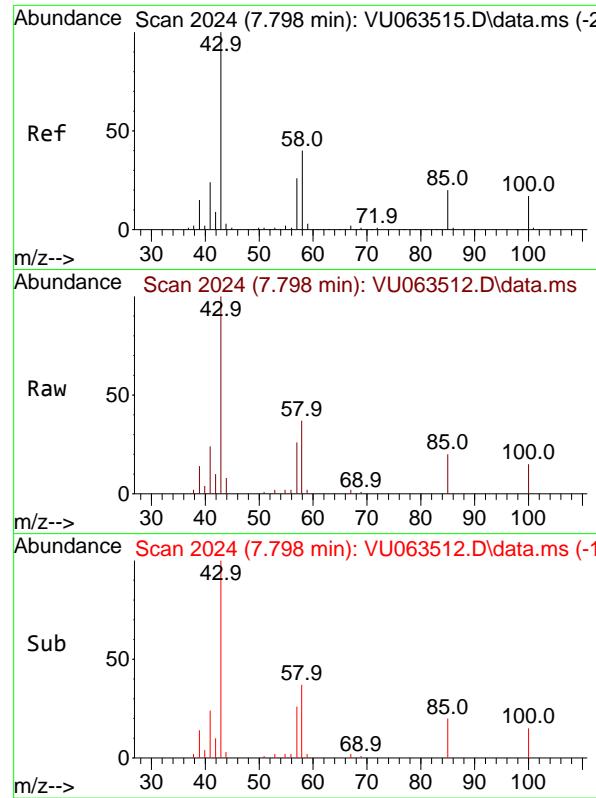

#45
 4-Methyl-2-Pentanone
 Concen: 4.985 ug/l
 RT: 7.798 min Scan# 2
Instrument :
 Delta R.T. 0.000 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54
ClientSampleId :
 VSTDICC001


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

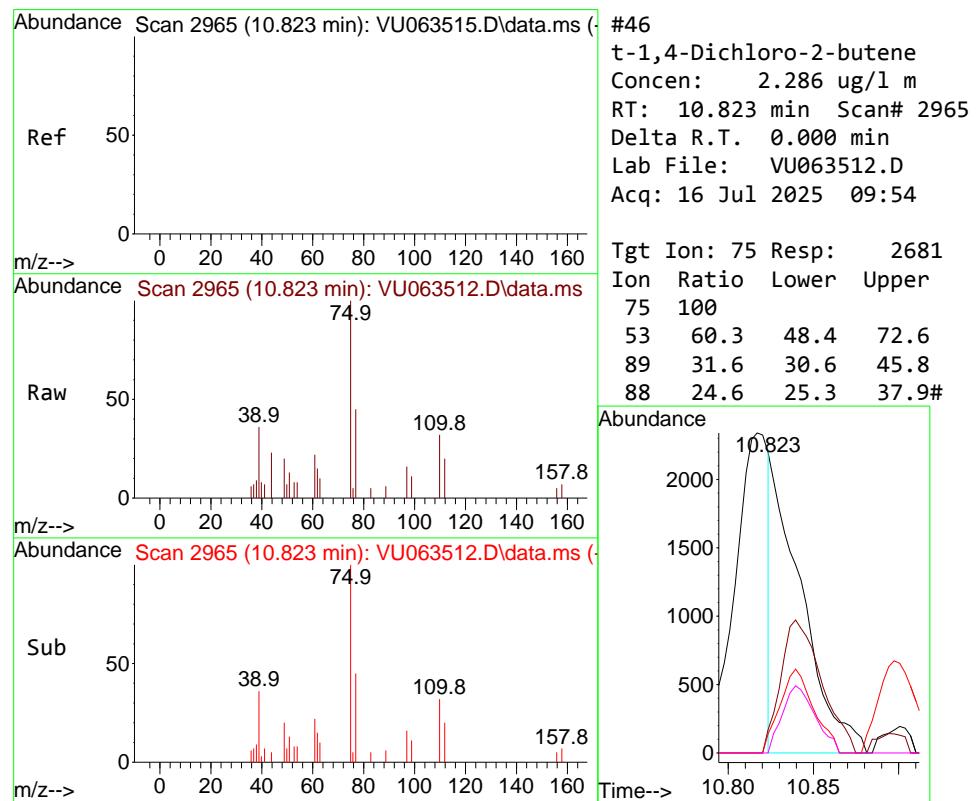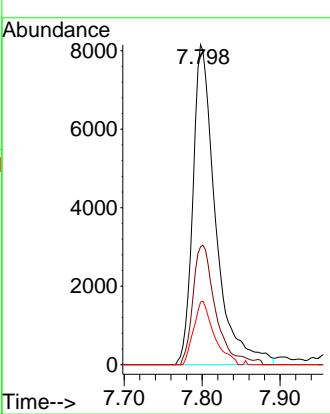

#46
 t-1,4-Dichloro-2-butene
 Concen: 2.286 ug/l m
 RT: 10.823 min Scan# 2965
 Delta R.T. 0.000 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54

Tgt Ion: 75 Resp: 2681
 Ion Ratio Lower Upper
 75 100
 53 60.3 48.4 72.6
 89 31.6 30.6 45.8
 88 24.6 25.3 37.9#

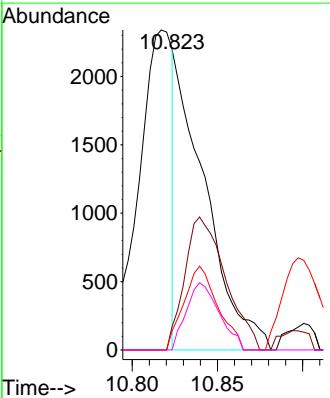



#47

Methyl methacrylate






Concen: 1.779 ug/l

RT: 6.968 min Scan# 1

Delta R.T. 0.006 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54







Instrument : MSVOA_U

ClientSampleId : VSTDICC001

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

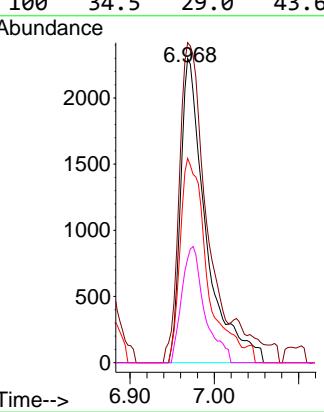

#48

Ethyl methacrylate

Concen: 0.875 ug/l

RT: 8.338 min Scan# 2192

Delta R.T. 0.003 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54


Tgt Ion: 69 Resp: 4500

Ion Ratio Lower Upper

69 100



41 73.9 30.8 92.4

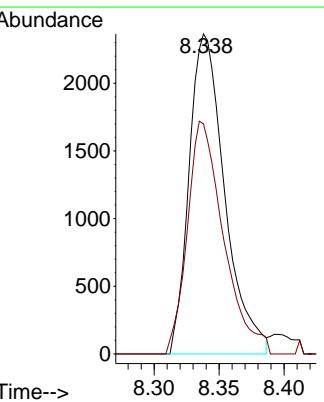



#49
Toluene
Concen: 1.010 ug/l
RT: 7.962 min Scan# 2
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54



Instrument : MSVOA_U
ClientSampleId : VSTDICC001

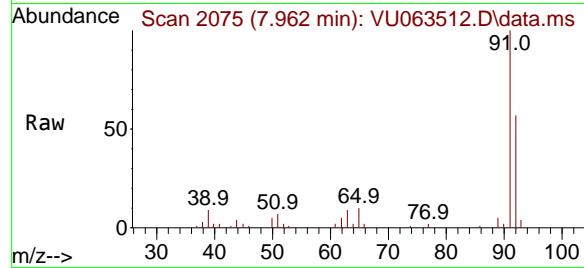


Tgt Ion: 92 Resp: 14592
Ion Ratio Lower Upper
92 100
91 175.8 140.4 210.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

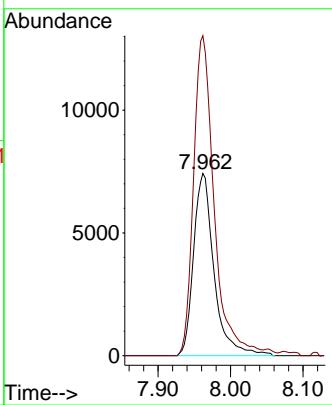


#50
t-1,3-Dichloropropene
Concen: 0.915 ug/l
RT: 8.209 min Scan# 2152
Delta R.T. 0.006 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54





Tgt Ion: 75 Resp: 5194
Ion Ratio Lower Upper
75 100
77 32.8 24.9 37.3

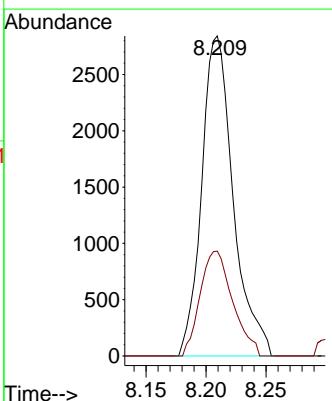



#51
cis-1,3-Dichloropropene
 Concen: 0.918 ug/l
 RT: 7.602 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54



Instrument : MSVOA_U
 ClientSampleId : VSTDICC001

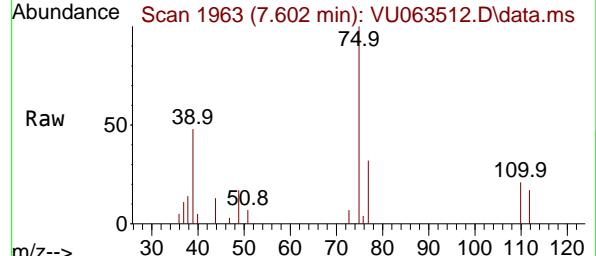


Tgt Ion: 75 Resp: 6989
 Ion Ratio Lower Upper
 75 100
 77 32.2 25.1 37.7
 39 47.8 37.8 56.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025



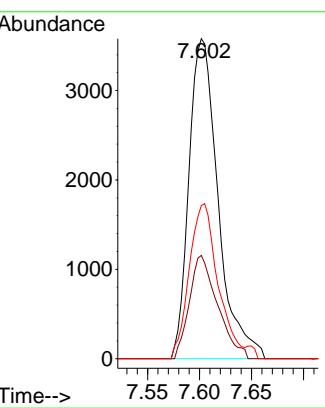


#52
 1,1,2-Trichloroethane
 Concen: 1.022 ug/l
 RT: 8.396 min Scan# 2210
 Delta R.T. 0.003 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54



Tgt Ion: 97 Resp: 4414
 Ion Ratio Lower Upper
 97 100
 83 85.5 70.2 105.2
 85 59.8 45.2 67.8
 99 72.0 50.1 75.1

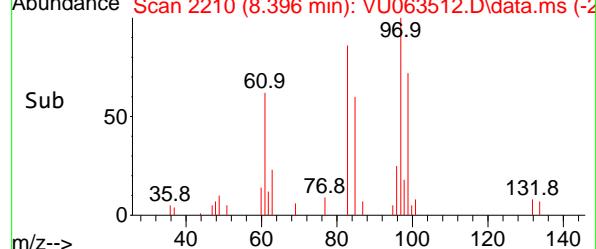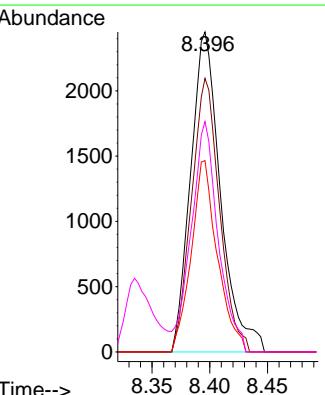



#53

1,3-Dichloropropane

Concen: 0.985 ug/l

RT: 8.569 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

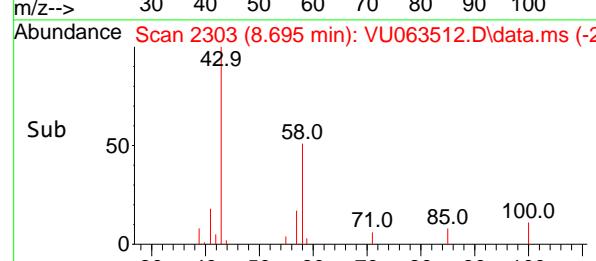 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#54

2-Hexanone

Concen: 4.940 ug/l

RT: 8.695 min Scan# 2303

Delta R.T. 0.006 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54


Tgt Ion: 43 Resp: 10847







Ion Ratio Lower Upper

43 100

58 49.3 34.8 74.8

57 17.1 0.0 39.5

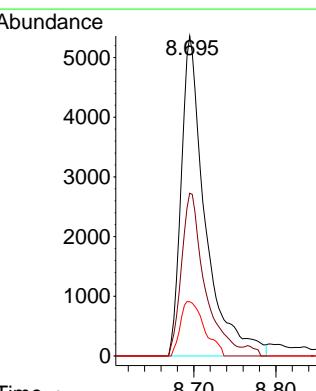

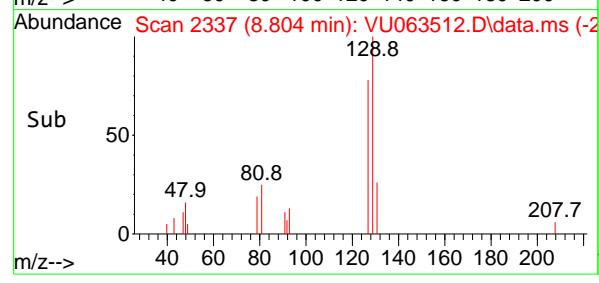

#55

Dibromochloromethane

Concen: 0.903 ug/l

RT: 8.804 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument :

MSVOA_U


ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#56

1,2-Dibromoethane

Concen: 0.980 ug/l

RT: 8.920 min Scan# 2373

Delta R.T. 0.003 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54




Tgt Ion:107 Resp: 3787

Ion Ratio Lower Upper

107 100

109 91.8 0.0 186.4

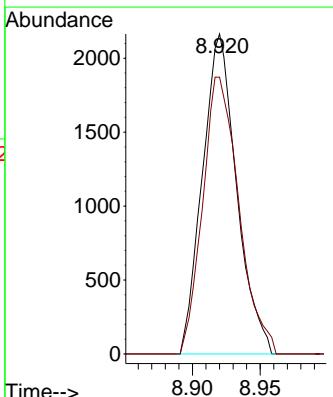



#57

4-Bromofluorobenzene

Concen: 1.082 ug/l

RT: 10.631 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

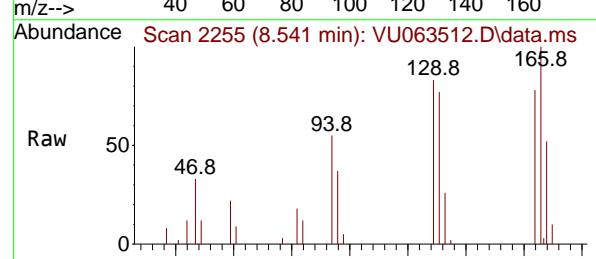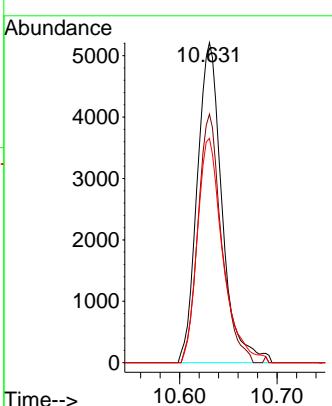 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#58

Tetrachloroethene

Concen: 1.016 ug/l


RT: 8.541 min Scan# 2255




Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt	Ion:164	Resp:	6276
Ion	Ratio	Lower	Upper
164	100		
166	128.5	100.7	151.1
129	106.3	80.6	120.8
131	99.0	77.3	115.9

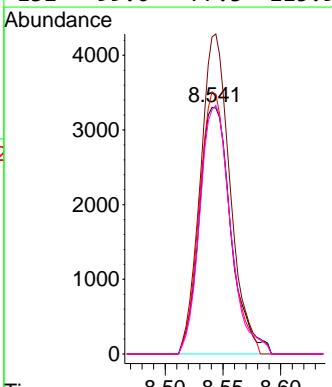

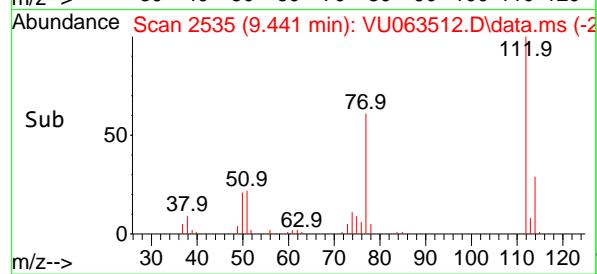

#59

Chlorobenzene

Concen: 0.994 ug/l

RT: 9.441 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

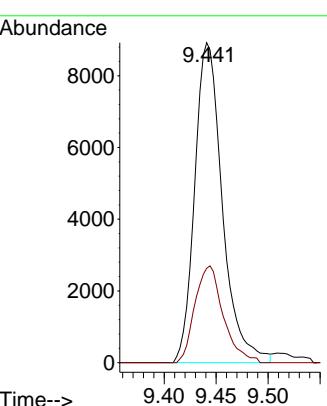 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#60

1,1,1,2-Tetrachloroethane


Concen: 0.995 ug/l




RT: 9.524 min Scan# 2561

Delta R.T. -0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

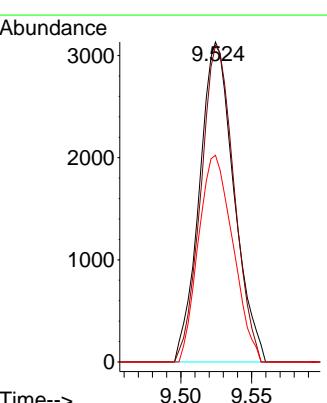 Tgt Ion:131 Resp: 5306
 Ion Ratio Lower Upper
 131 100
 133 94.8 74.7 112.1
 119 64.5 53.0 79.4




#61

Pentachloroethane

Concen: 0.894 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument :

MSVOA_U




ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#62

Hexachloroethane

Concen: 0.875 ug/l

RT: 12.466 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54


Tgt Ion:117 Resp: 3268

Ion Ratio Lower Upper

117 100

201 74.5 57.4 86.0

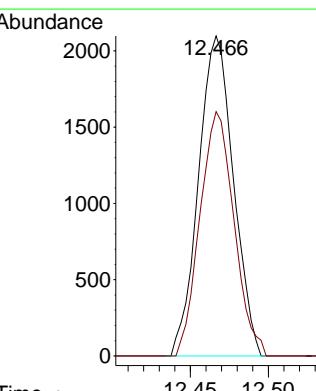



#63

Ethyl Benzene

Concen: 0.992 ug/l

RT: 9.563 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument :

MSVOA_U

ClientSampleId :




VSTDICC001



Tgt Ion: 91 Resp: 2830
 Ion Ratio Lower Upper
 91 100
 106 30.7 25.4 38.0



Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

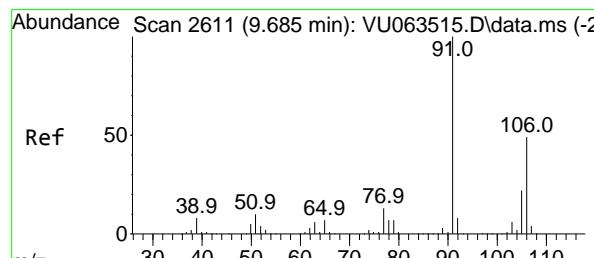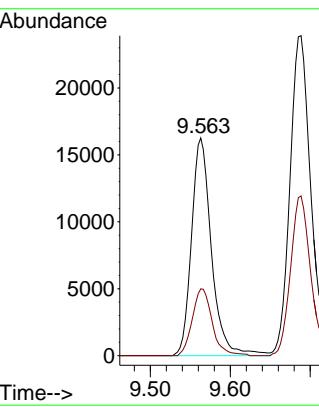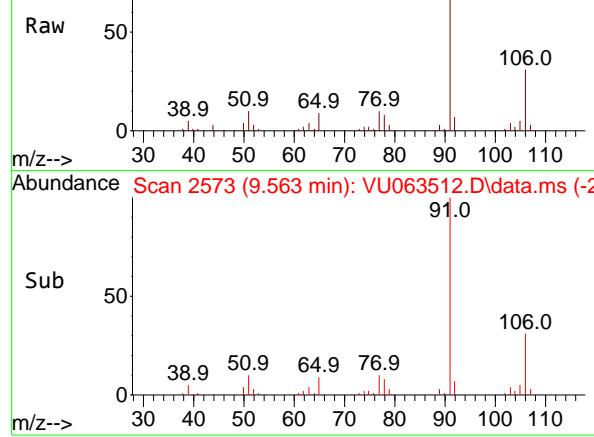

#64
 m/p-Xylenes
 Concen: 1.904 ug/l
 RT: 9.688 min Scan# 2612
 Delta R.T. 0.003 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54

Tgt Ion:106 Resp: 21130
 Ion Ratio Lower Upper
 106 100
 91 209.8 163.6 245.4

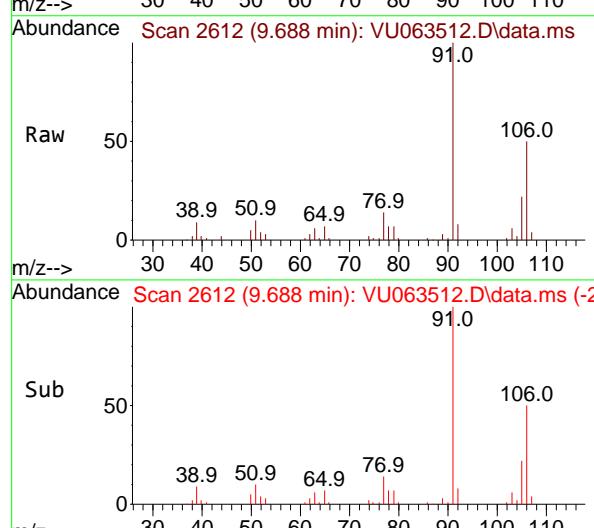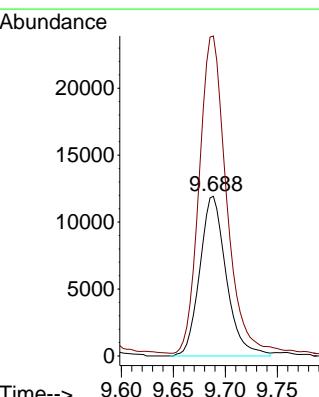


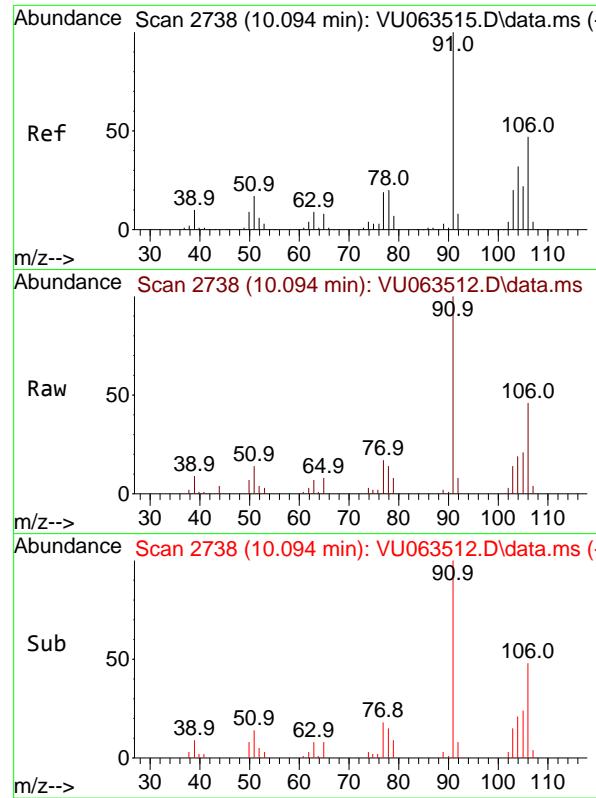


#65
o-Xylene
Concen: 0.974 ug/l
RT: 10.094 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
ClientSampleId : VSTDICC001


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

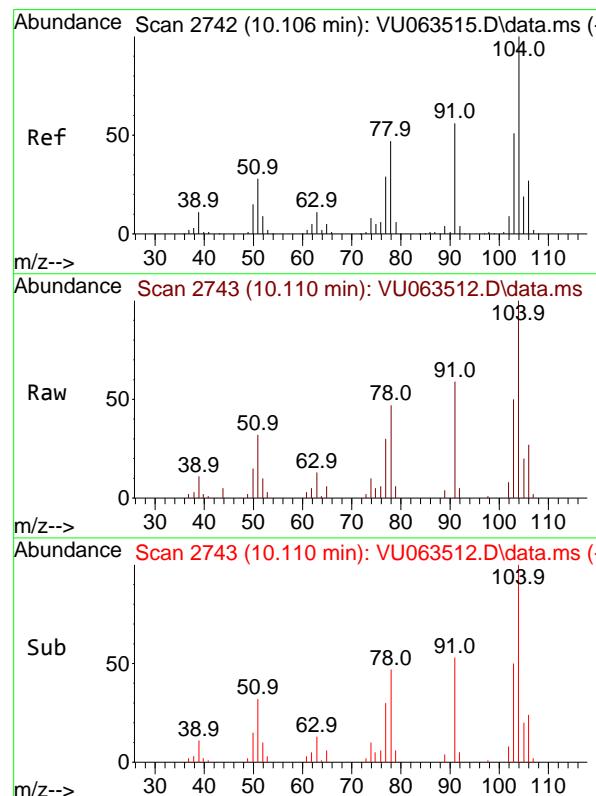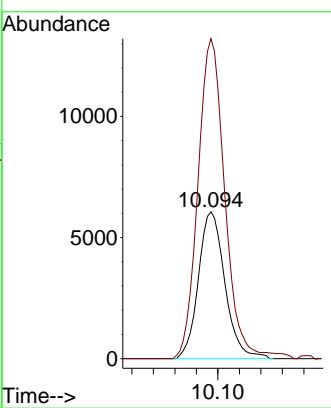

#66
Styrene
Concen: 0.945 ug/l
RT: 10.110 min Scan# 2743
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Tgt Ion:104 Resp: 16060
Ion Ratio Lower Upper
104 100
78 53.8 41.3 61.9
103 55.0 43.6 65.4

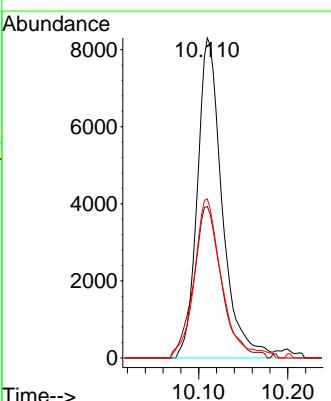



#67

Bromoform

Concen: 0.810 ug/l

RT: 10.286 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

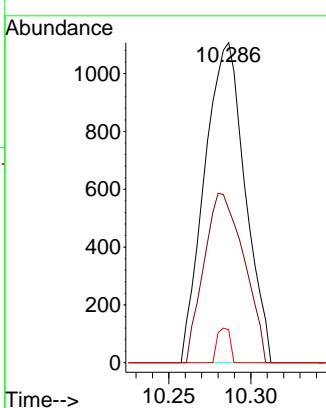 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.038 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt	Ion:152	Resp:	8165
Ion	Ratio	Lower	Upper
152	100		
115	75.3	0.0	262.2
150	170.7	0.0	651.2

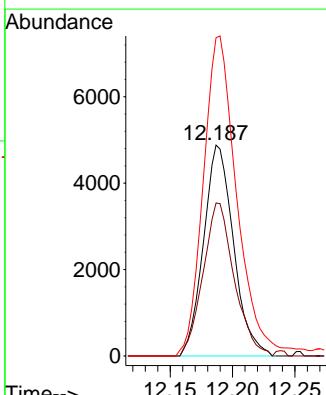

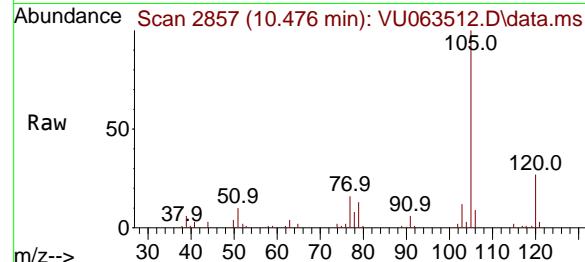

#69

Isopropylbenzene

Concen: 0.974 ug/l

RT: 10.476 min Scan# 2

Instrument :

Delta R.T. 0.000 min

MSVOA_U

Lab File: VU063512.D

ClientSampleId :

Acq: 16 Jul 2025 09:54

VSTDICC001

Tgt Ion:105 Resp: 2509:

Ion Ratio Lower Upper




105 100

120 27.1 13.2 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

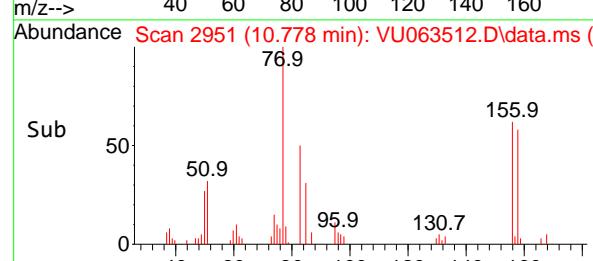

#70

1,1,2,2-Tetrachloroethane

Concen: 0.978 ug/l

RT: 10.778 min Scan# 2951

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54


Tgt Ion: 83 Resp: 5141




Ion Ratio Lower Upper

83 100

131 7.8 8.4 12.6#

85 64.3 51.9 77.9

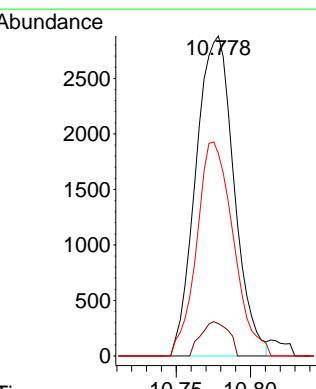



#71

1,2,3-Trichloropropane

Concen: 1.034 ug/l m

RT: 10.817 min Scan# 2963

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#72

Bromobenzene

Concen: 0.956 ug/l

RT: 10.778 min Scan# 2951

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54


Tgt Ion:156 Resp: 6362




Ion Ratio Lower Upper

156 100

77 166.4 0.0 315.2

158 97.5 0.0 195.4

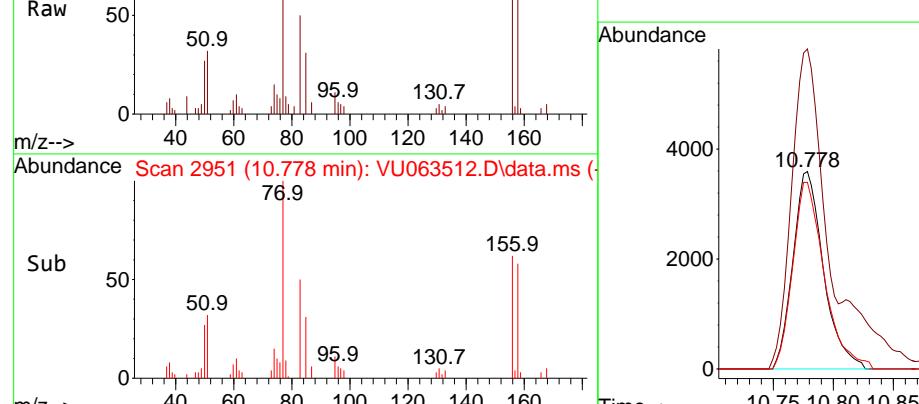



#73

n-propylbenzene

Concen: 0.946 ug/l

RT: 10.901 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063512.D




Acq: 16 Jul 2025 09:54

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#74

2-Chlorotoluene

Concen: 0.976 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063512.D


Acq: 16 Jul 2025 09:54




Tgt Ion:126 Resp: 6695

Ion Ratio Lower Upper

126 100

91 293.8 0.0 606.0

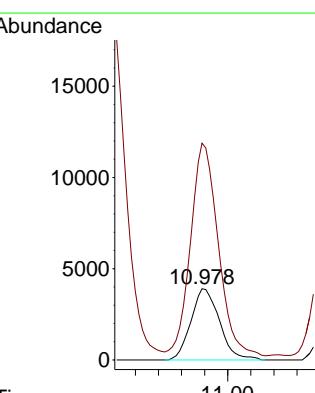



#75

1,3,5-Trimethylbenzene

Concen: 0.945 ug/l

RT: 11.081 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

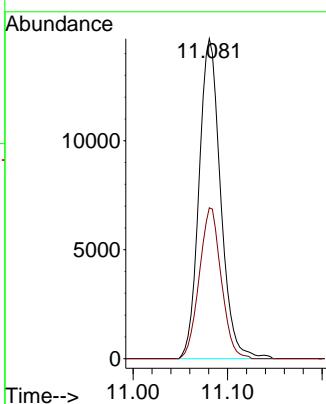 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#76

4-Chlorotoluene


Concen: 0.967 ug/l




RT: 11.094 min Scan# 3049

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

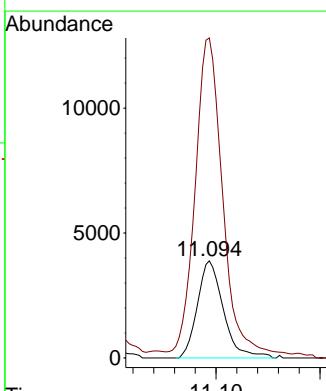 Tgt Ion:126 Resp: 6734
 Ion Ratio Lower Upper
 126 100
 91 339.5 0.0 682.2

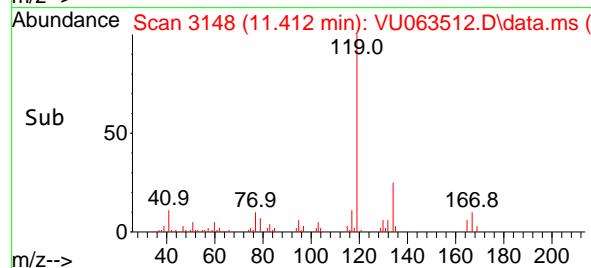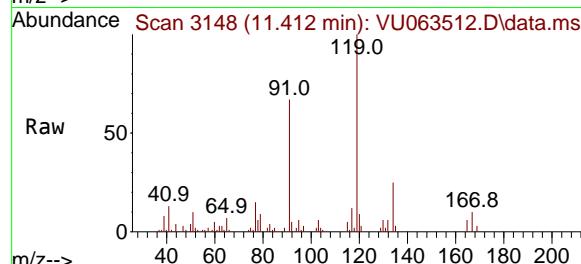


#77

tert-Butylbenzene

Concen: 0.942 ug/l

RT: 11.412 min Scan# 3148

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

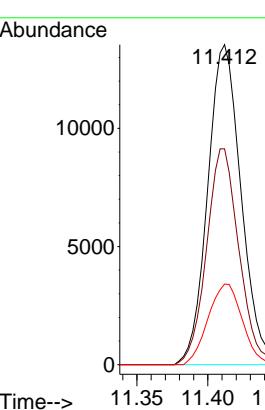

#78

1,2,4-Trimethylbenzene

Concen: 0.946 ug/l


RT: 11.463 min Scan# 3164




Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt	Ion:105	Resp:	23102
Ion	Ratio	Lower	Upper
105	100		
120	45.5	22.7	68.0

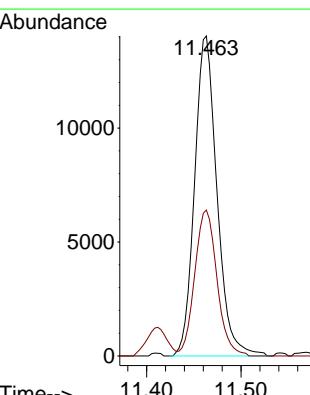







#79
sec-Butylbenzene
Concen: 0.974 ug/l
RT: 11.637 min Scan# 30903
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
ClientSampleId : VSTDICC001


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

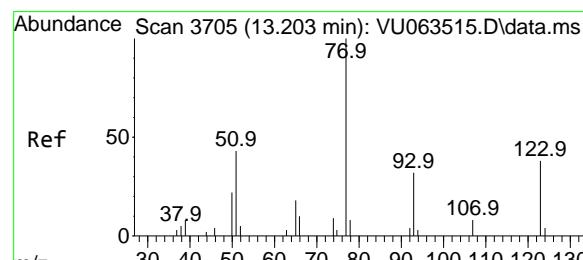

#80
Nitrobenzene
Concen: 5.705 ug/l m
RT: 13.232 min Scan# 3714
Delta R.T. 0.029 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Tgt Ion: 77 Resp: 400
Ion Ratio Lower Upper
77 100
123 5.0 16.9 59.7#
65 0.0 16.5 20.9#





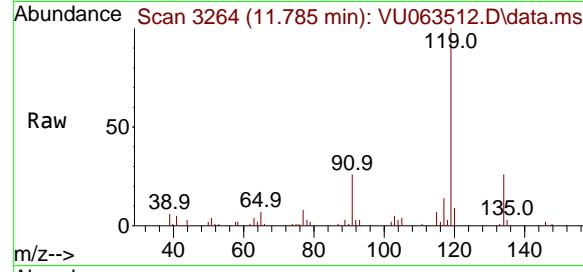



#81
 p-Isopropyltoluene
 Concen: 0.936 ug/l
 RT: 11.785 min Scan# 3
 Delta R.T. 0.000 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54

Instrument : MSVOA_U
 ClientSampleId : VSTDICC001


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

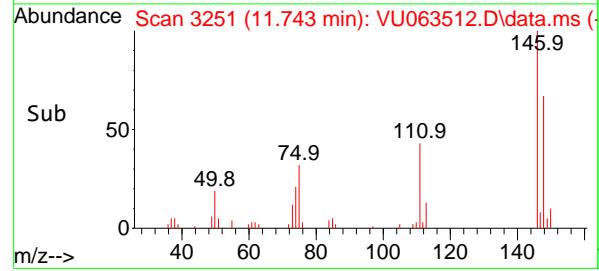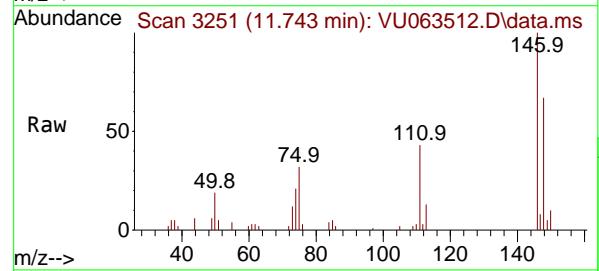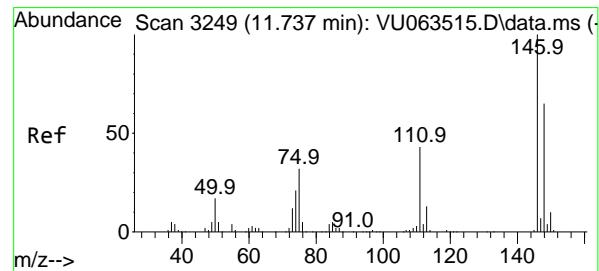

#82
 1,3-Dichlorobenzene
 Concen: 0.964 ug/l
 RT: 11.743 min Scan# 3251
 Delta R.T. 0.006 min
 Lab File: VU063512.D
 Acq: 16 Jul 2025 09:54

Tgt Ion:146 Resp: 12830
 Ion Ratio Lower Upper
 146 100
 111 43.7 33.8 50.6
 148 65.6 51.5 77.3

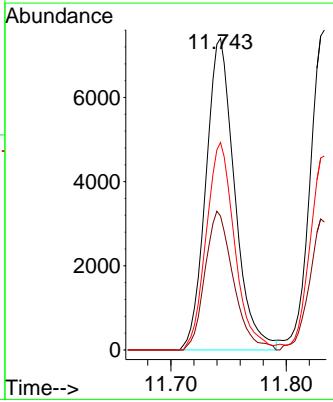



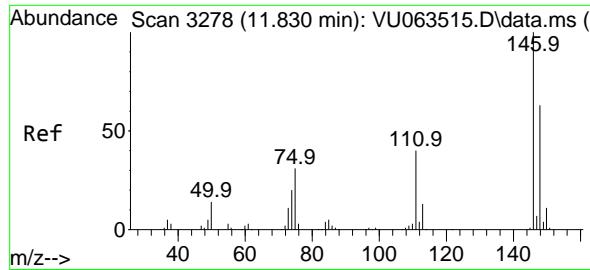


#83
1,4-Dichlorobenzene
Concen: 0.964 ug/l
RT: 11.833 min Scan# 31
Instrument :
Delta R.T. 0.003 min MSVOA_U
Lab File: VU063512.D ClientSampleId :
Acq: 16 Jul 2025 09:54 VSTDICC001

Instrument :
SVOA_U
ClientSampleId :
STDICC001




**Manual Integrations
APPROVED**




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

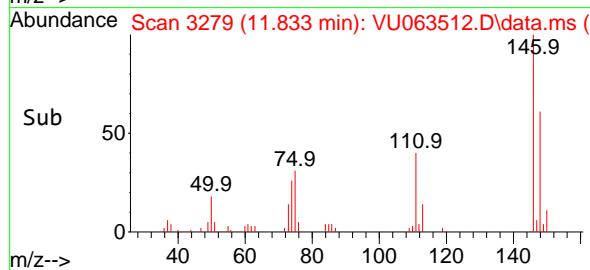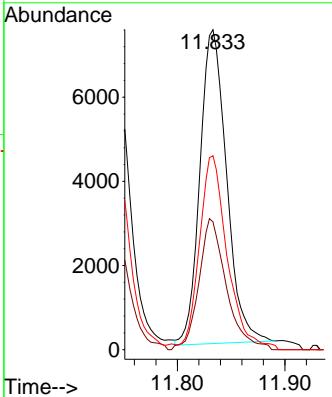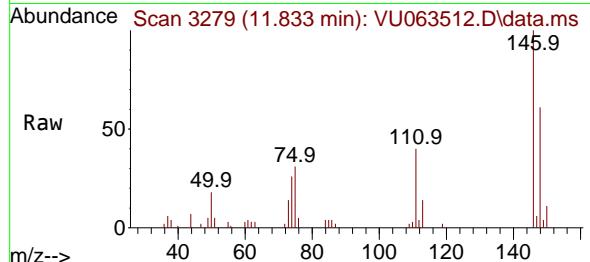

Time--> 11.80 11.90
#84
n-Butylbenzene
Concen: 0.917 ug/l
RT: 12.203 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VU063512.D
Acq: 16 Jul 2025 09:54

Tgt	Ion:	91	Resp:	22541
Ion	Ratio		Lower	Upper
91	100			
92	52.3	41.5	62.3	
134	23.4	20.6	30.8	

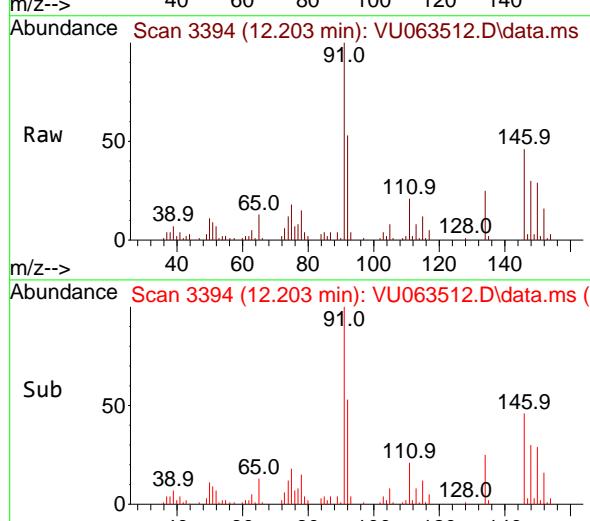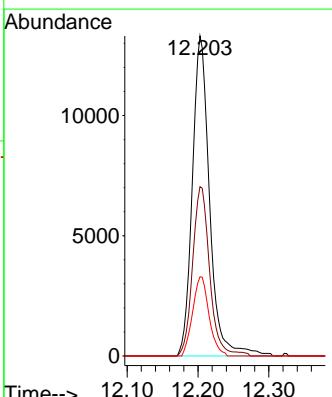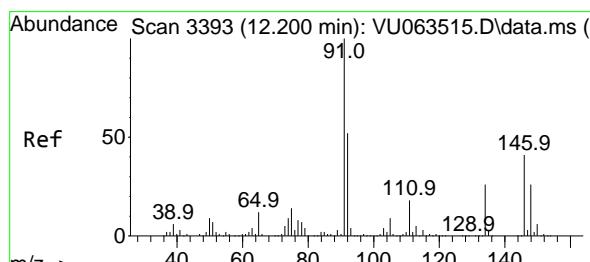



#85

1,2-Dichlorobenzene

Concen: 0.965 ug/l

RT: 12.206 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC001

Tgt Ion:146 Resp: 1207:

Ion Ratio Lower Upper

146 100




111 44.3 21.7 65.1

148 64.8 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 0.991 ug/l

RT: 12.991 min Scan# 3639

Delta R.T. 0.004 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54


Tgt Ion: 75 Resp: 603




Ion Ratio Lower Upper

75 100

155 84.2 65.8 98.6

157 114.8 81.4 122.2

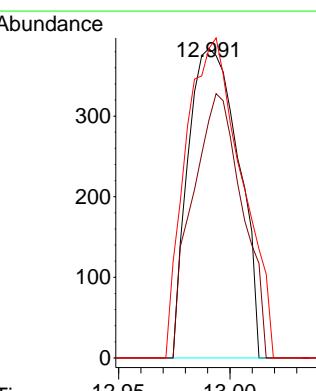

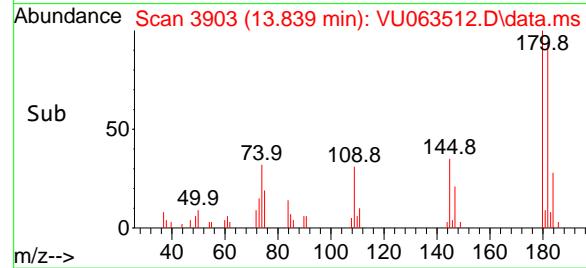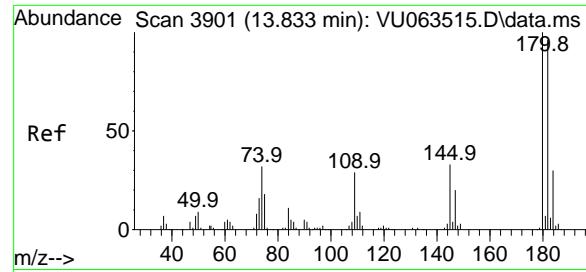

#87

1,2,4-Trichlorobenzene

Concen: 0.903 ug/l

RT: 13.839 min Scan# 3

Delta R.T. 0.006 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Instrument:

MSVOA_U





ClientSampleId :

VSTDICC001

Tgt	Ion:180	Resp:	7020
Ion	Ratio	Lower	Upper
180	100		
182	97.5	76.2	114.4
145	32.6	26.2	39.2

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

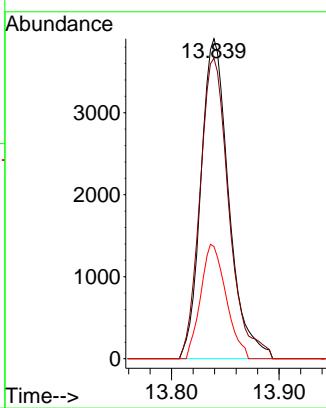

#88

Hexachlorobutadiene

Concen: 0.938 ug/l


RT: 14.013 min Scan# 3957




Delta R.T. 0.000 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt	Ion:225	Resp:	4144
Ion	Ratio	Lower	Upper
225	100		
223	61.8	50.8	76.2
227	65.3	51.0	76.6

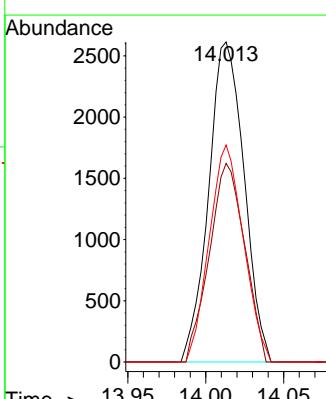

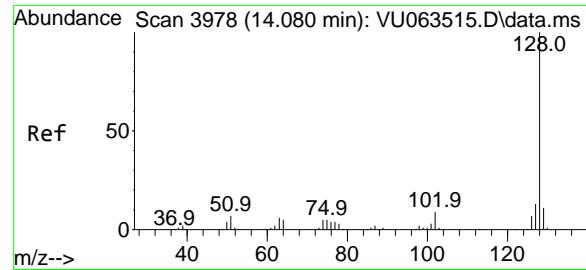

#89

Naphthalene

Concen: 0.859 ug/l

RT: 14.087 min Scan# 3

Instrument : MSVOA_U





Delta R.T. 0.007 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

ClientSampleId : VSTDICC001

**Manual Integrations
APPROVED**

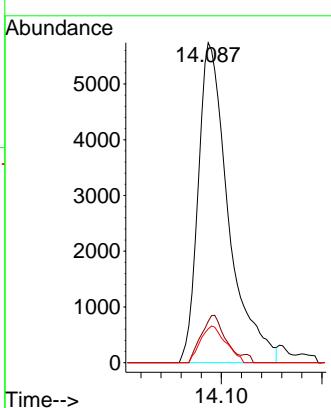 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#90

1,2,3-Trichlorobenzene

Concen: 0.920 ug/l


RT: 14.325 min Scan# 4054

Delta R.T. 0.003 min

Lab File: VU063512.D

Acq: 16 Jul 2025 09:54

Tgt	Ion:180	Resp:	6612
Ion	Ratio	Lower	Upper
180	100		
182	97.4	78.0	117.0
145	33.1	27.3	40.9

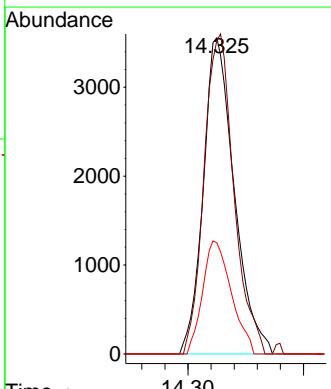

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063513.D
 Acq On : 16 Jul 2025 10:27
 Operator : MD/SY
 Sample : VSTDICC002
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC002

Quant Time: Jul 17 03:23:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	24713	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	8919	0.953	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	8064	0.932	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	13901	1.908	ug/l	99
3) Chloromethane	1.515	50	12922	1.908	ug/l	96
4) Vinyl Chloride	1.596	62	16476	1.910	ug/l	95
5) Bromomethane	1.846	94	13182	2.026	ug/l	99
6) Chloroethane	1.924	64	9817	1.885	ug/l	99
7) Trichlorofluoromethane	2.126	101	23274	1.879	ug/l	99
8) 1,1,2-Trichloro-1,2,2-...	2.567	101	12436	1.921	ug/l	99
9) 1,1-Dichloroethene	2.567	96	11909	1.856	ug/l	98
10) Iodomethane	2.708	142	11910	2.044	ug/l	99
11) Allyl Chloride	2.908	41	19248	2.077	ug/l	94
12) Acrylonitrile	3.306	53	6375m	3.971	ug/l	
13) Acetone	2.618	43	12988	10.102	ug/l	99
14) Carbon Disulfide	2.776	76	38838	1.874	ug/l	97
15) Methylene Chloride	3.030	84	14190	1.878	ug/l	97
16) trans-1,2-Dichloroethene	3.335	96	13749	1.887	ug/l	99
17) 1,1-Dichloroethane	3.846	63	25721	1.904	ug/l	99
18) 2-Butanone	4.715	43	19497	9.792	ug/l	98
19) Cyclohexane	5.358	56	21512	1.881	ug/l	98
20) Methylcyclohexane	6.743	83	19848	1.786	ug/l	97
21) 2,2-Dichloropropane	4.644	77	22099	1.922	ug/l	98
22) cis-1,2-Dichloroethene	4.647	96	14739	1.864	ug/l	98
23) Diethyl Ether	2.367	59	9590	1.962	ug/l	97
24) tert-Butyl Alcohol	3.190	59	11035	18.698	ug/l	# 93
25) Methyl tert-Butyl Ether	3.361	73	31927	1.906	ug/l	98
26) Bromochloromethane	4.956	128	6299	1.908	ug/l	95
27) Chloroform	5.071	83	26561	1.927	ug/l	99
28) 1,1,1-Trichloroethane	5.293	97	22170	1.895	ug/l	99
29) 1,1-Dichloropropene	5.502	75	21342	1.970	ug/l	95
30) Carbon Tetrachloride	5.499	117	17885	1.900	ug/l	93
31) Isopropyl Ether	3.988	45	39017	1.914	ug/l	99
32) Ethyl-t-butyl ether	4.502	59	36341	1.926	ug/l	100
33) Tert-Amyl methyl ether	5.943	73	32364	1.977	ug/l	99
34) Propionitrile	4.772	54	5922	9.762	ug/l	98
35) Benzene	5.753	78	57563	1.977	ug/l	100
36) 1,2-Dichloroethane	5.782	62	17934	1.982	ug/l	100
37) Trichloroethene	6.528	130	13293	1.790	ug/l	97
38) 1,2-Dichloropropane	6.782	63	12386	1.818	ug/l	97
39) Methacrylonitrile	4.968	41	5277	1.982	ug/l	93
40) Methyl acrylate	4.846	55	6918	1.755	ug/l	96
41) Tetrahydrofuran	5.065	42	5330	3.757	ug/l	96
42) 1-Chlorobutane	5.438	56	27320	1.896	ug/l	100
43) Dibromomethane	6.907	93	6494	1.840	ug/l	94
44) Bromodichloromethane	7.097	83	14822	1.862	ug/l	# 94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063513.D
 Acq On : 16 Jul 2025 10:27
 Operator : MD/SY
 Sample : VSTDICC002
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC002

Quant Time: Jul 17 03:23:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	33590	9.233	ug/l	100
46) t-1,4-Dichloro-2-butene	10.824	75	4957m	3.841	ug/l	
47) Methyl methacrylate	6.968	69	10710	3.613	ug/l	96
48) Ethyl methacrylate	8.335	69	10760	1.902	ug/l	97
49) Toluene	7.959	92	29457	1.853	ug/l	97
50) t-1,3-Dichloropropene	8.206	75	11035	1.767	ug/l	99
51) cis-1,3-Dichloropropene	7.602	75	14409	1.719	ug/l	99
52) 1,1,2-Trichloroethane	8.393	97	8889	1.871	ug/l	98
53) 1,3-Dichloropropane	8.570	76	15693	1.913	ug/l	99
54) 2-Hexanone	8.692	43	21569	8.926	ug/l	98
55) Dibromochloromethane	8.801	129	9158	1.824	ug/l	99
56) 1,2-Dibromoethane	8.920	107	7956	1.871	ug/l	99
58) Tetrachloroethene	8.541	164	13165	1.936	ug/l	95
59) Chlorobenzene	9.441	112	33922	1.858	ug/l	99
60) 1,1,1,2-Tetrachloroethane	9.525	131	10771	1.835	ug/l	98
61) Pentachloroethane	11.418	117	7292	1.758	ug/l	93
62) Hexachloroethane	12.467	117	7073	1.722	ug/l	93
63) Ethyl Benzene	9.563	91	58862	1.874	ug/l	100
64) m/p-Xylenes	9.685	106	45864	3.756	ug/l	97
65) o-Xylene	10.094	106	21340	1.819	ug/l	98
66) Styrene	10.110	104	34112	1.824	ug/l	96
67) Bromoform	10.283	173	4536	1.759	ug/l	# 92
69) Isopropylbenzene	10.476	105	52260	1.842	ug/l	99
70) 1,1,2,2-Tetrachloroethane	10.775	83	10710	1.852	ug/l	97
71) 1,2,3-Trichloropropane	10.817	75	8980m	1.903	ug/l	
72) Bromobenzene	10.775	156	13109	1.791	ug/l	79
73) n-propylbenzene	10.901	120	15950	1.868	ug/l	98
74) 2-Chlorotoluene	10.978	126	14070	1.864	ug/l	98
75) 1,3,5-Trimethylbenzene	11.081	105	50061	1.847	ug/l	98
76) 4-Chlorotoluene	11.094	126	14644	1.911	ug/l	91
77) tert-Butylbenzene	11.412	119	48176	1.860	ug/l	99
78) 1,2,4-Trimethylbenzene	11.460	105	49637	1.846	ug/l	99
79) sec-Butylbenzene	11.634	105	64443	1.845	ug/l	98
80) Nitrobenzene	13.219	77	861	9.644	ug/l	# 78
81) p-Isopropyltoluene	11.785	119	53922	1.850	ug/l	99
82) 1,3-Dichlorobenzene	11.740	146	26844	1.833	ug/l	99
83) 1,4-Dichlorobenzene	11.833	146	26650	1.818	ug/l	98
84) n-Butylbenzene	12.203	91	48694	1.801	ug/l	99
85) 1,2-Dichlorobenzene	12.206	146	24834	1.805	ug/l	99
86) 1,2-Dibromo-3-Chloropr...	12.994	75	1550	2.046	ug/l	91
87) 1,2,4-Trichlorobenzene	13.836	180	15327	1.791	ug/l	97
88) Hexachlorobutadiene	14.013	225	8872	1.826	ug/l	98
89) Naphthalene	14.087	128	25691	1.675	ug/l	98
90) 1,2,3-Trichlorobenzene	14.325	180	13999	1.770	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063513.D
 Acq On : 16 Jul 2025 10:27
 Operator : MD/SY
 Sample : VSTDICC002
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1


Quant Time: Jul 17 03:23:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Instrument :
 MSVOA_U
ClientSampleId :
 VSTDICC002

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

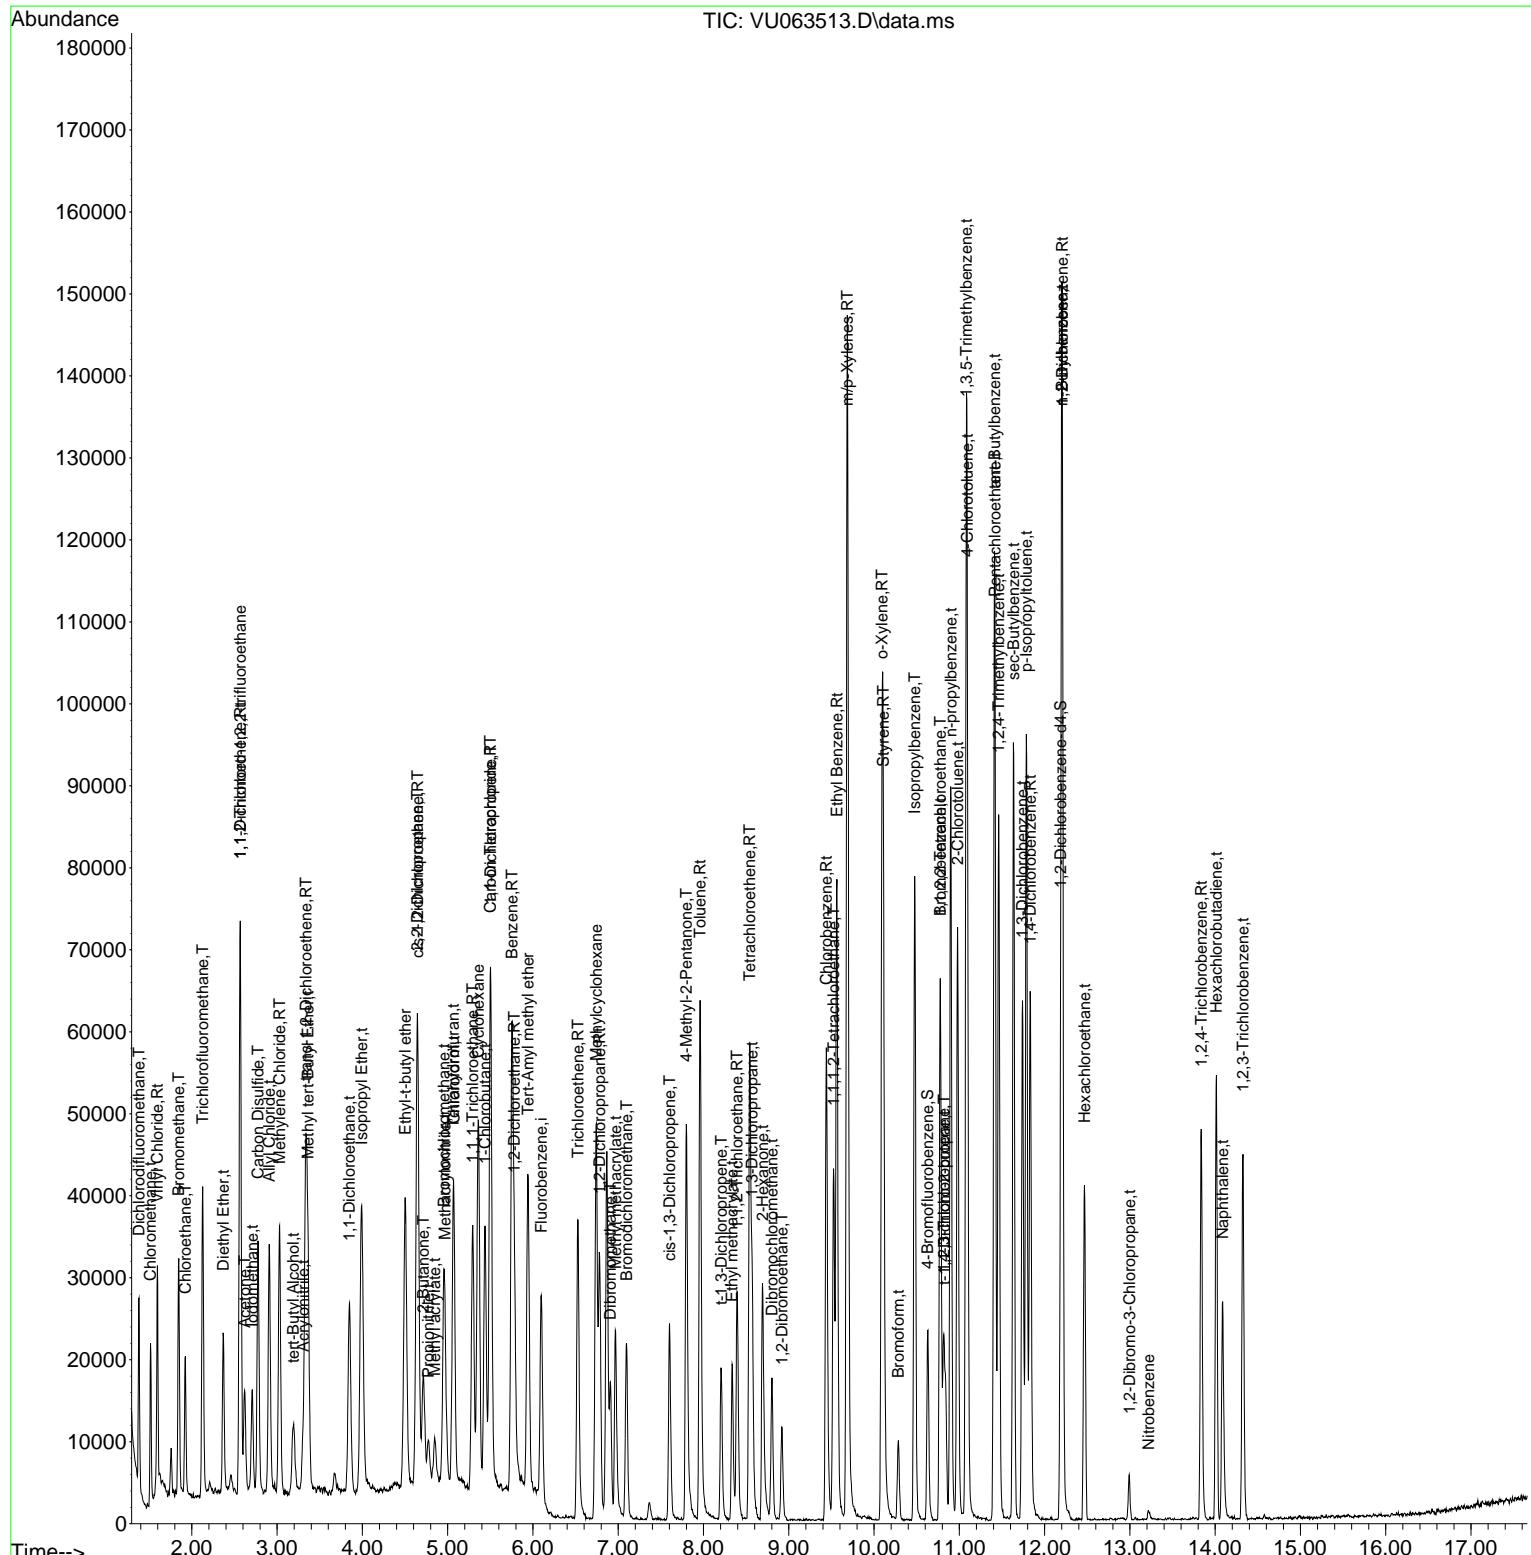


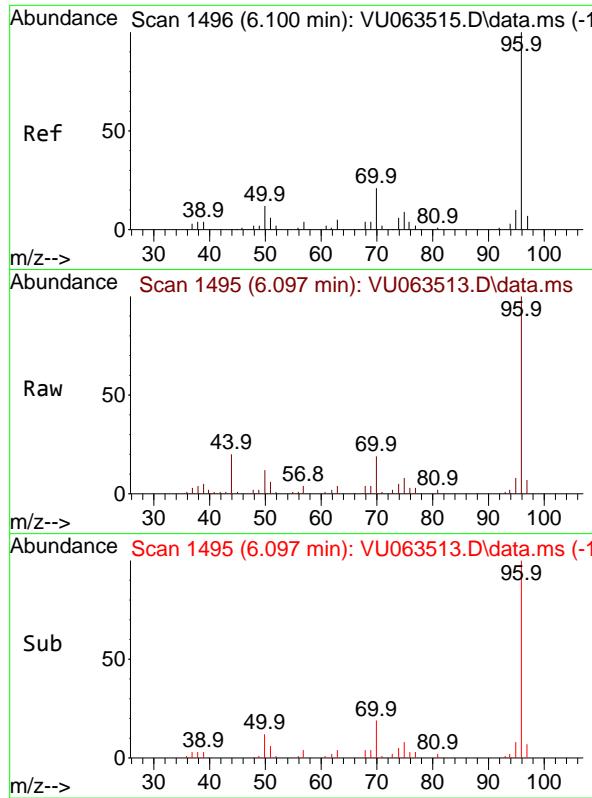


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U
ClientSampleId : VSTDICC002


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

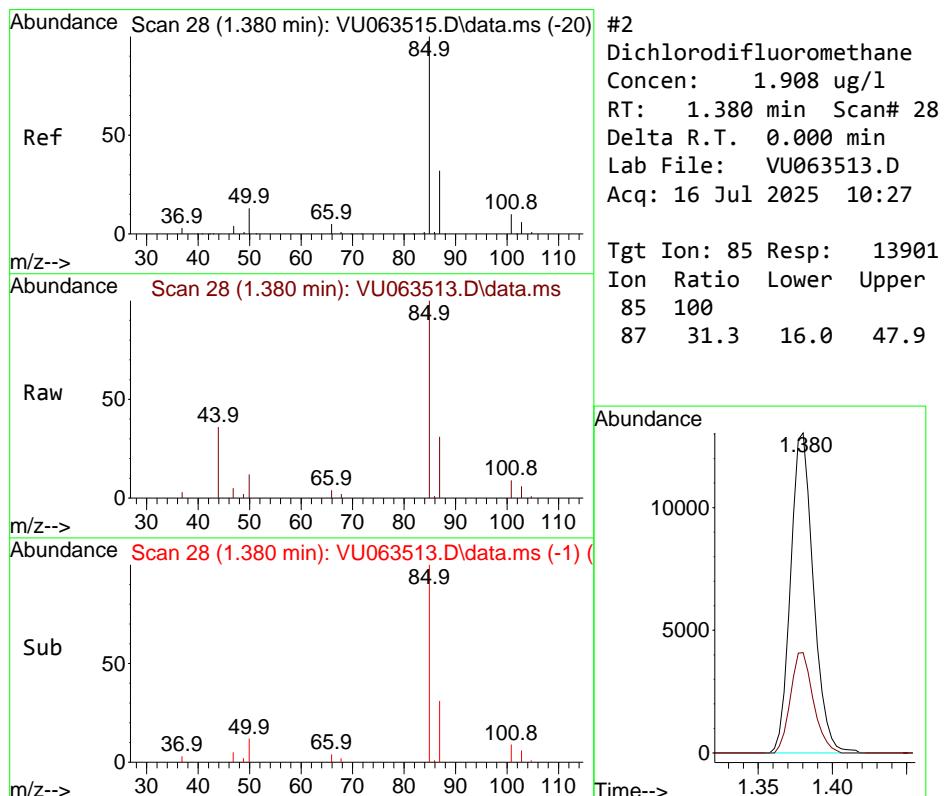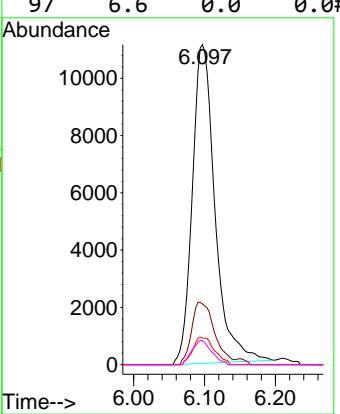



#2
Dichlorodifluoromethane
Concen: 1.908 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion: 85 Resp: 13901
Ion Ratio Lower Upper
85 100
87 31.3 16.0 47.9

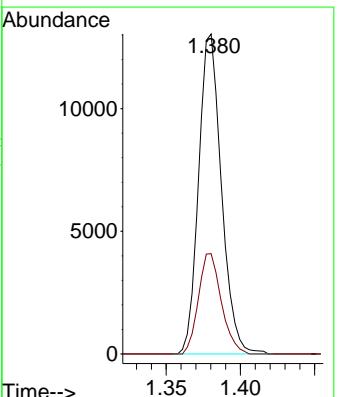




Abundance Scan 70 (1.515 min): VU063513.D\data.ms

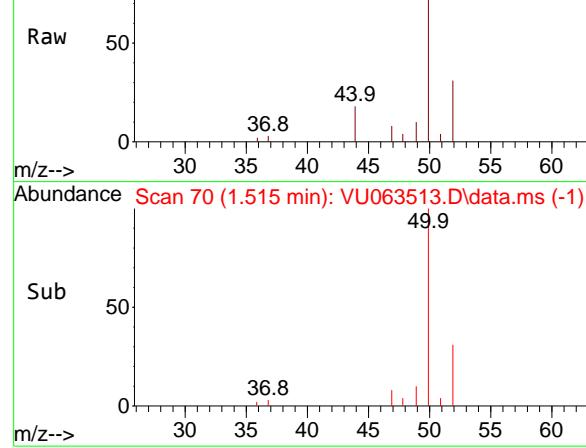

Abundance Scan 95 (1.596 min): VU063513.D\data.ms

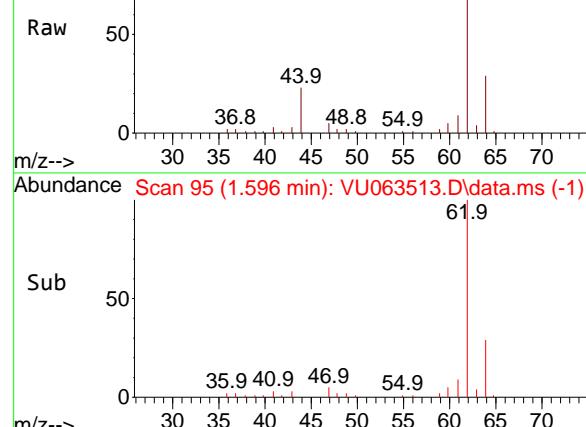

#3

Chloromethane

Concen: 1.908 ug/l

RT: 1.515 min Scan# 7

Delta R.T. -0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

Tgt Ion: 50 Resp: 1292

Ion Ratio Lower Upper

50 100


52 30.8 26.3 39.5

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

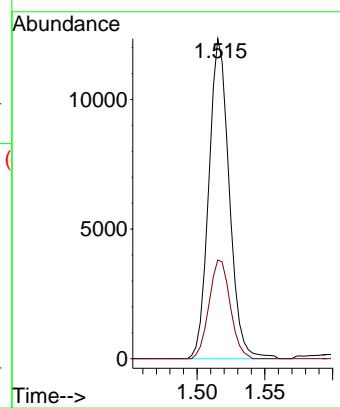

#4

Vinyl Chloride

Concen: 1.910 ug/l

RT: 1.596 min Scan# 95

Delta R.T. -0.003 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27




Tgt Ion: 62 Resp: 16476

Ion Ratio Lower Upper

62 100

64 29.4 25.7 38.5

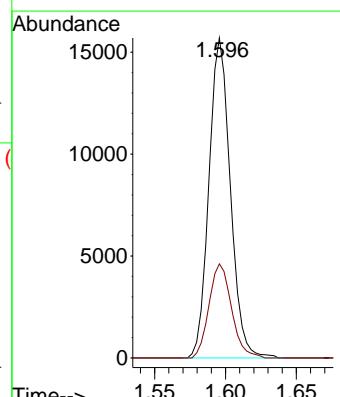



#5

Bromomethane

Concen: 2.026 ug/l

RT: 1.846 min Scan# 1

Delta R.T. 0.007 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

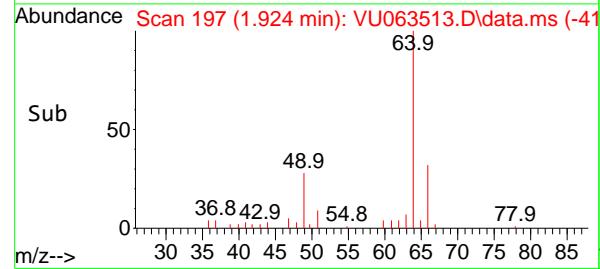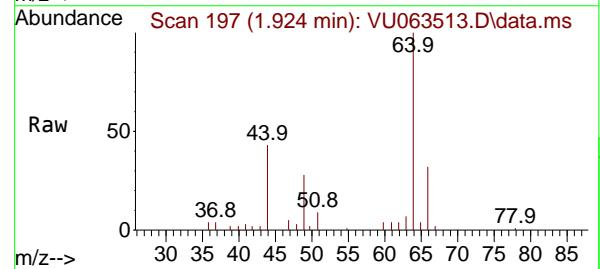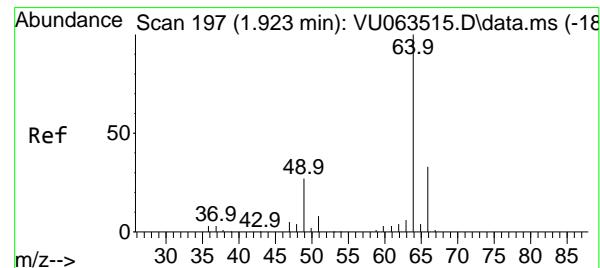 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#6

Chloroethane

Concen: 1.885 ug/l

RT: 1.924 min Scan# 197

Delta R.T. 0.000 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27




Tgt Ion: 64 Resp: 9817

Ion Ratio Lower Upper

64 100

66 32.2 26.2 39.4

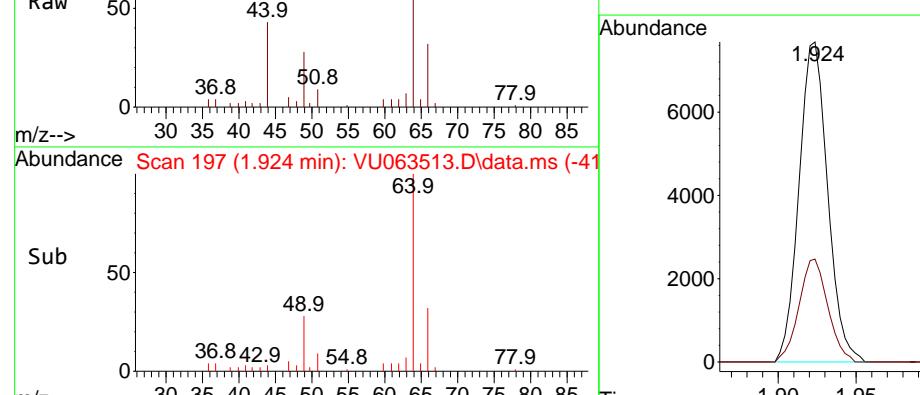

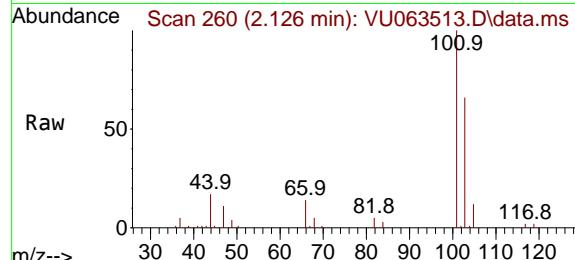



#7
Trichlorofluoromethane
Concen: 1.879 ug/l
RT: 2.126 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27


Instrument : MSVOA_U
ClientSampleId : VSTDICC002

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 1.921 ug/l
RT: 2.567 min Scan# 397
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27




Tgt Ion:101 Resp: 12436
Ion Ratio Lower Upper
101 100
85 48.4 37.8 56.6
151 74.0 59.2 88.8





#9
1,1-Dichloroethene
Concen: 1.856 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27




Instrument : MSVOA_U
ClientSampleId : VSTDICC002

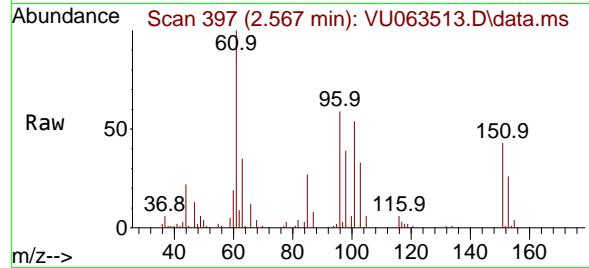


Tgt Ion: 96 Resp: 11909
Ion Ratio Lower Upper
96 100
61 169.6 0.0 504.3
98 65.5 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

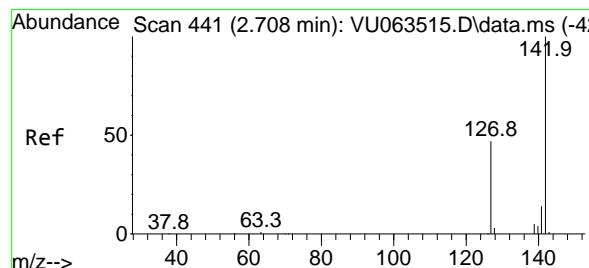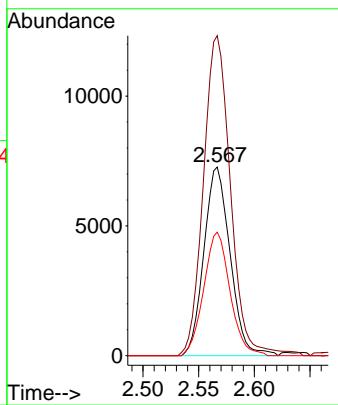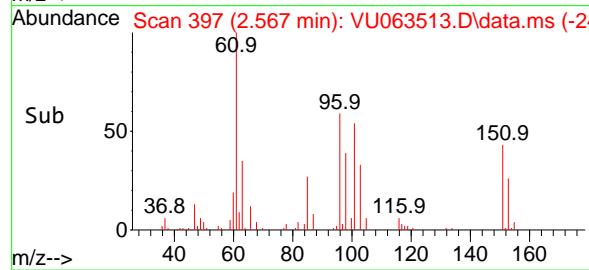


#10
Iodomethane
Concen: 2.044 ug/l
RT: 2.708 min Scan# 441
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

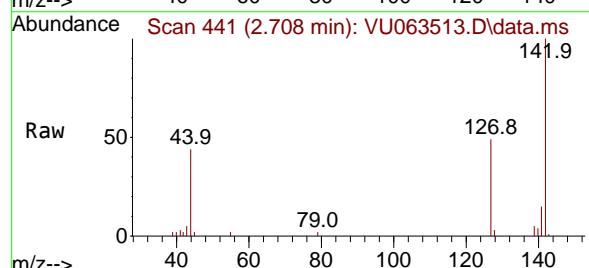


Tgt Ion:142 Resp: 11910
Ion Ratio Lower Upper
142 100
127 48.3 37.9 56.9

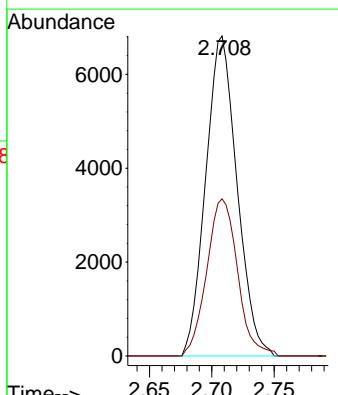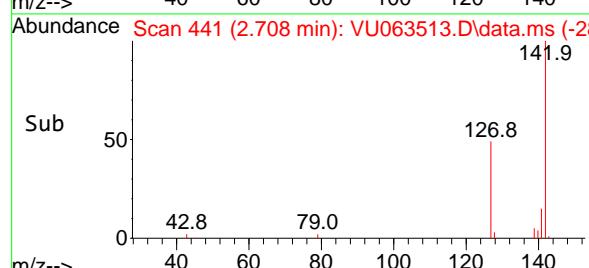



#11
Allyl Chloride
 Concen: 2.077 ug/l
 RT: 2.908 min Scan# 5
 Delta R.T. 0.000 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27




Instrument : MSVOA_U
 ClientSampleId : VSTDICC002

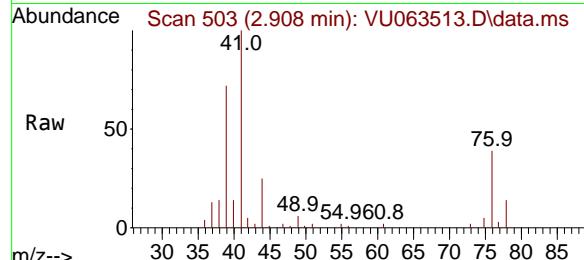


Tgt Ion: 41 Resp: 1924:
 Ion Ratio Lower Upper
 41 100
 39 71.6 61.5 92.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

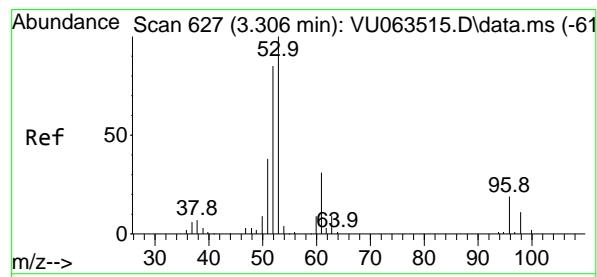

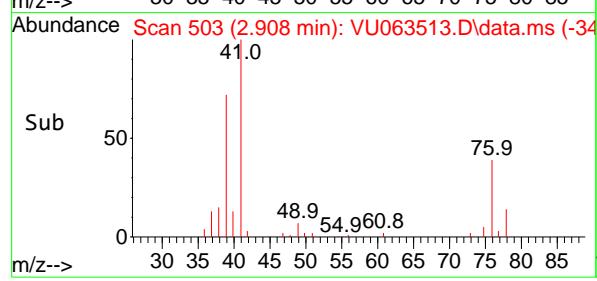


#12
Acrylonitrile
 Concen: 3.971 ug/l m
 RT: 3.306 min Scan# 627
 Delta R.T. 0.000 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27

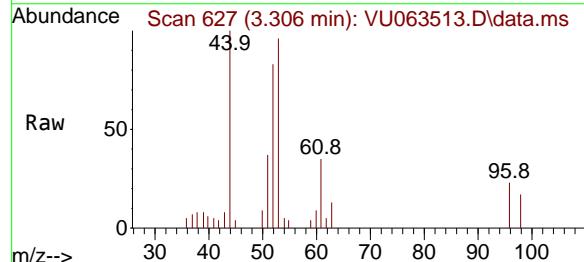

Tgt Ion: 53 Resp: 6375
 Ion Ratio Lower Upper
 53 100
 52 74.6 64.3 96.5
 51 44.0 27.8 41.8#

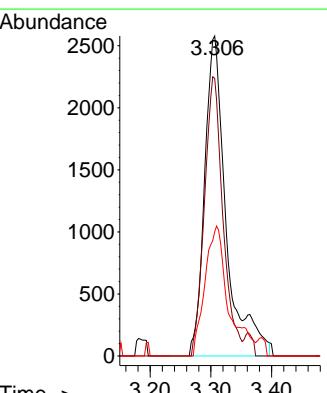



#13

Acetone

Concen: 10.102 ug/l

RT: 2.618 min Scan# 413

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#14

Carbon Disulfide

Concen: 1.874 ug/l

RT: 2.776 min Scan# 462

Delta R.T. 0.000 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27




Tgt Ion: 76 Resp: 38838

Ion Ratio Lower Upper

76 100

78 10.0 7.0 10.6



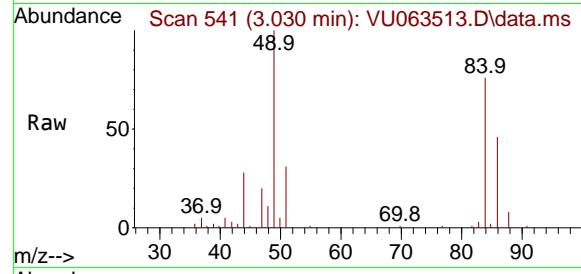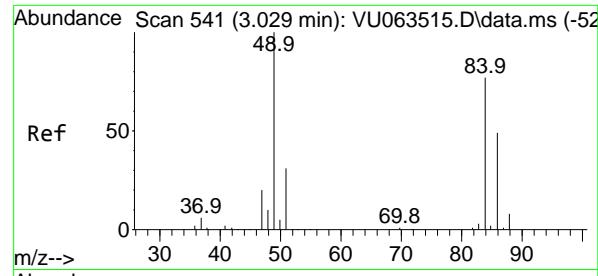

#15

Methylene Chloride

Concen: 1.878 ug/l

RT: 3.030 min Scan# 5

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

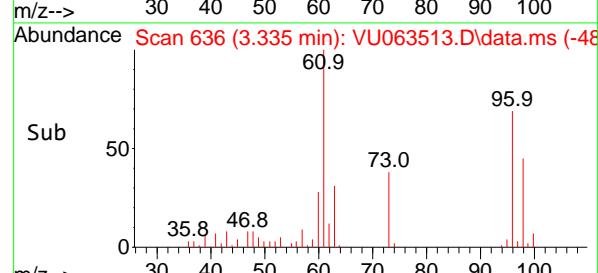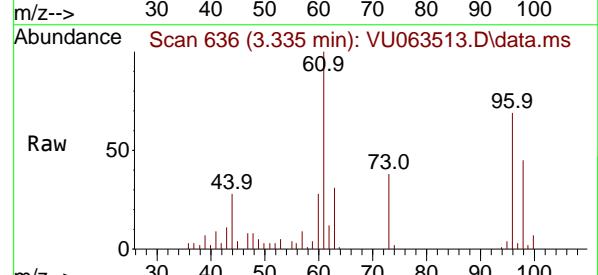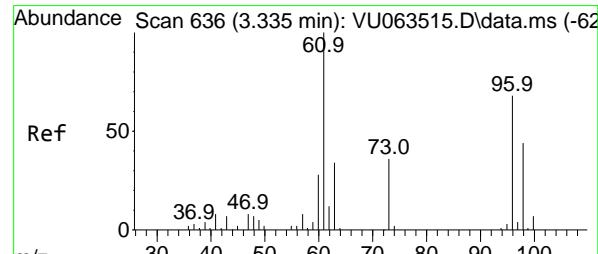

#16

trans-1,2-Dichloroethene

Concen: 1.887 ug/l

RT: 3.335 min Scan# 636

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27



Tgt Ion: 96 Resp: 13749




Ion Ratio Lower Upper

96 100

61 145.4 117.2 175.8

98 65.5 51.4 77.2

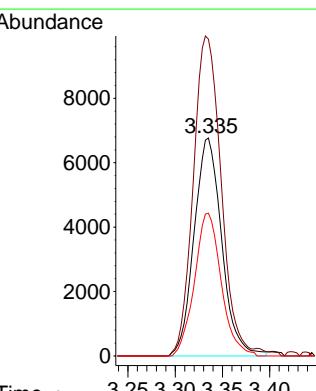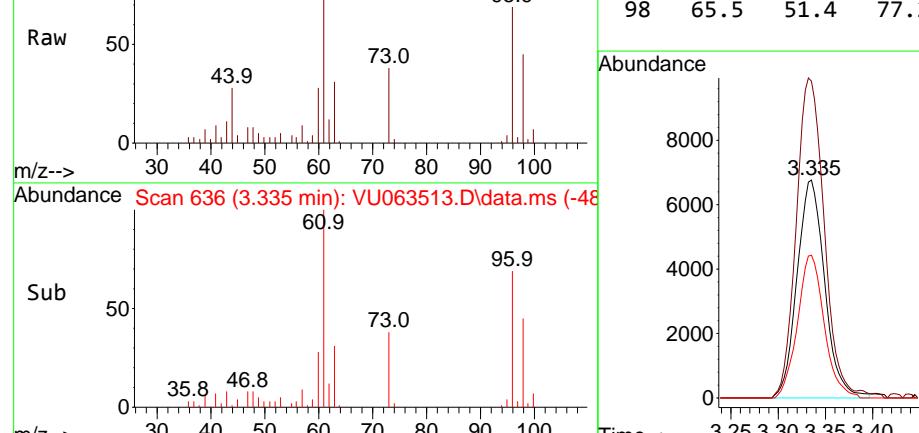



#17

1,1-Dichloroethane

Concen: 1.904 ug/l

RT: 3.846 min Scan# 7

Delta R.T. -0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#18

2-Butanone

Concen: 9.792 ug/l

RT: 4.715 min Scan# 1065

Delta R.T. 0.003 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27


Tgt Ion: 43 Resp: 19497

Ion Ratio Lower Upper

43 100


57 8.9 0.0 16.4

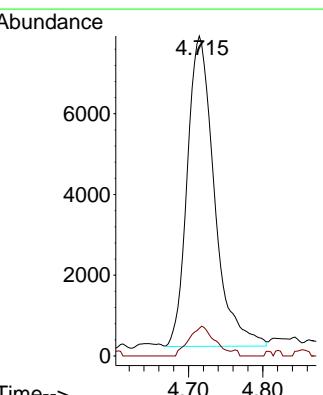



#19
Cyclohexane
Concen: 1.881 ug/l
RT: 5.358 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27




Instrument : MSVOA_U
ClientSampleId : VSTDICC002




Tgt Ion: 56 Resp: 2151:
Ion Ratio Lower Upper
56 100
69 32.7 26.6 39.8
84 86.3 71.0 106.4

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


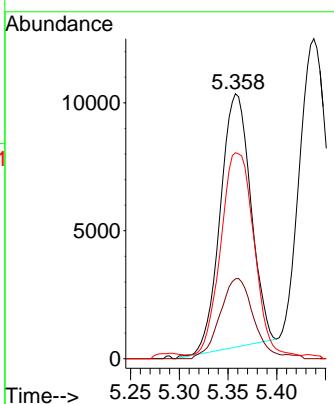
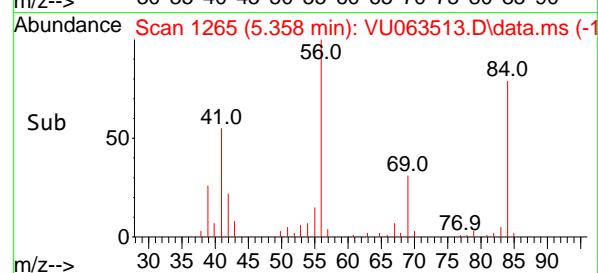


#20
Methylcyclohexane
Concen: 1.786 ug/l
RT: 6.743 min Scan# 1696
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27



Tgt Ion: 83 Resp: 19848
Ion Ratio Lower Upper
83 100
55 74.1 60.6 90.8
98 47.9 35.8 53.8

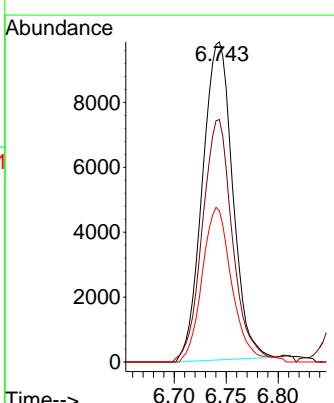

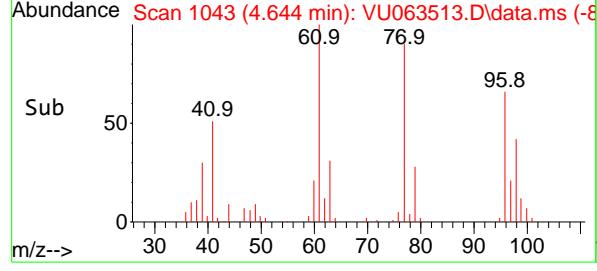

#21

2,2-Dichloropropane

Concen: 1.922 ug/l

RT: 4.644 min Scan# 1043

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27





Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

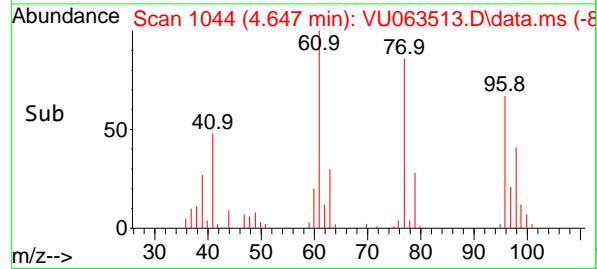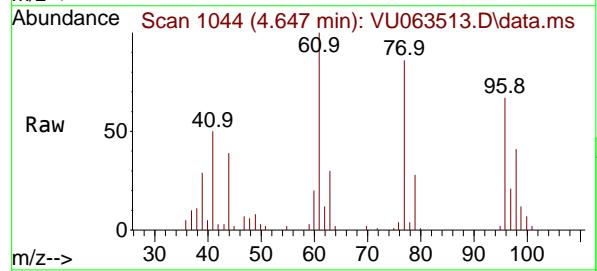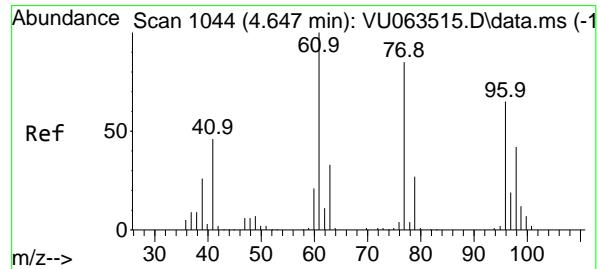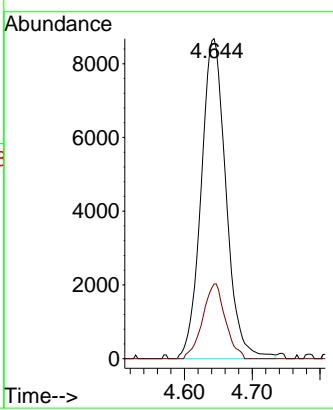 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#22

cis-1,2-Dichloroethene

Concen: 1.864 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion: 96 Resp: 14739




Ion Ratio Lower Upper

96 100

61 152.6 0.0 384.7

98 62.1 32.1 96.3

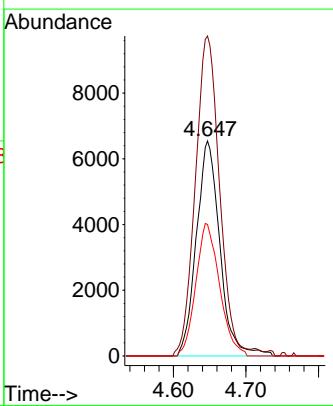

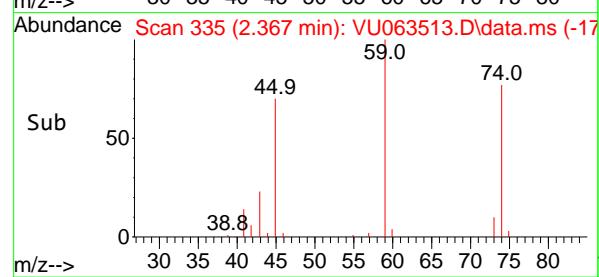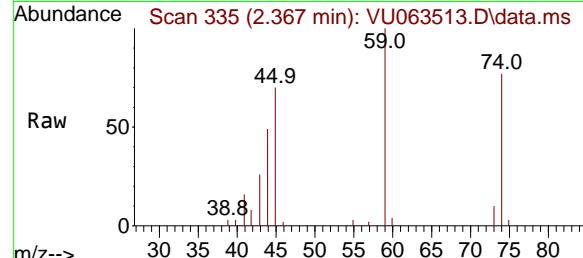

#23

Diethyl Ether

Concen: 1.962 ug/l

RT: 2.367 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27





Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

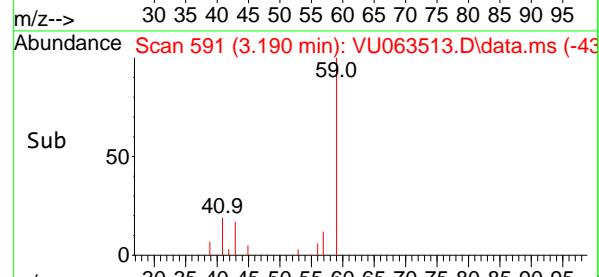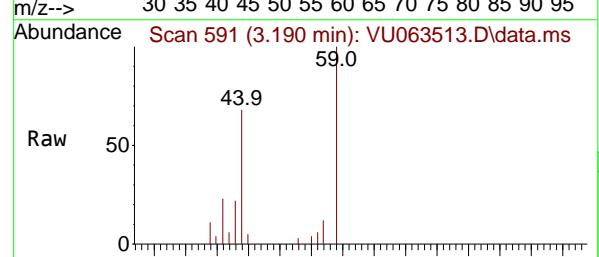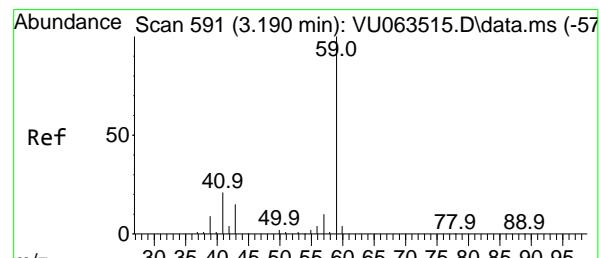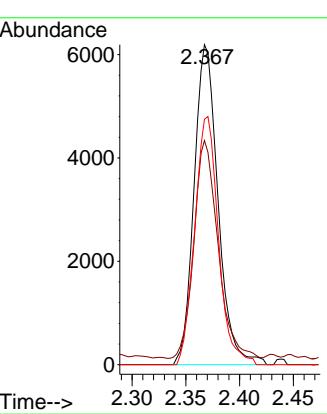 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#24

tert-Butyl Alcohol


Concen: 18.698 ug/l


RT: 3.190 min Scan# 591

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

 Tgt Ion: 59 Resp: 11035
 Ion Ratio Lower Upper
 59 100
 57 13.4 8.6 12.8#

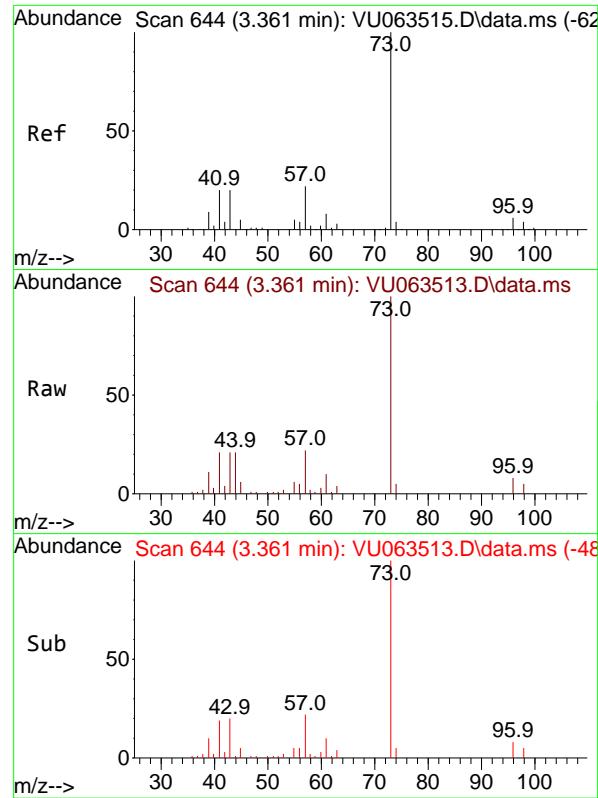


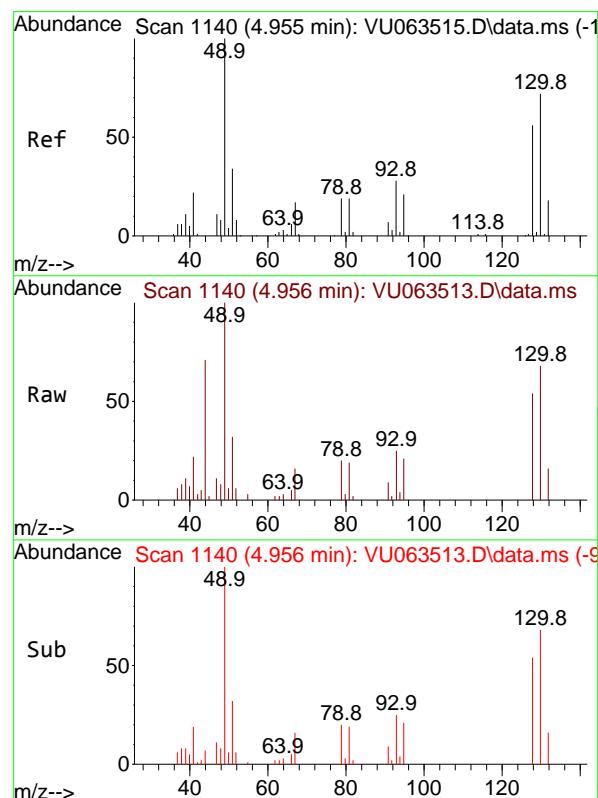
#25

Methyl tert-Butyl Ether
Concen: 1.906 ug/l
RT: 3.361 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U
ClientSampleId : VSTDICC002

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#26

Bromochloromethane
Concen: 1.908 ug/l
RT: 4.956 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27


Tgt Ion:128 Resp: 6299
Ion Ratio Lower Upper
128 100
49 179.5 0.0 340.8
130 128.5 100.5 150.7

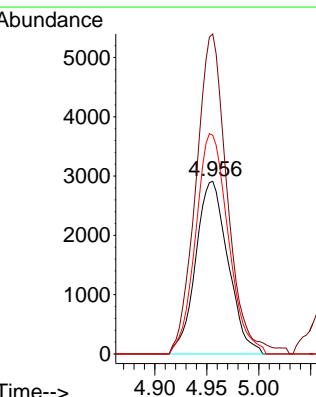



#27
 Chloroform
 Concen: 1.927 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27




Instrument : MSVOA_U
 ClientSampleId : VSTDICC002

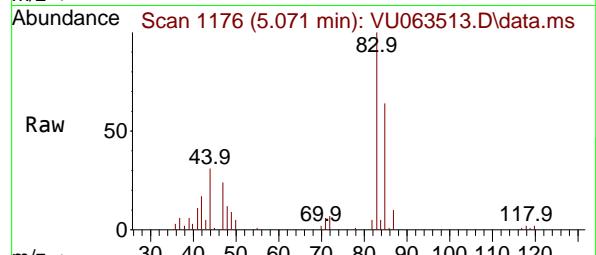


Tgt Ion: 83 Resp: 2656
 Ion Ratio Lower Upper
 83 100
 85 63.9 0.0 130.0

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

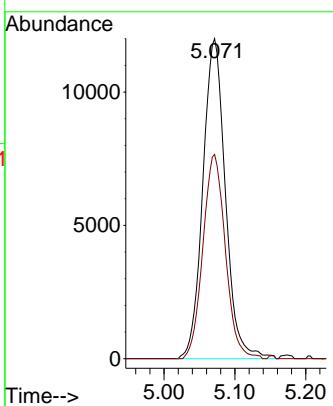


#28
 1,1,1-Trichloroethane
 Concen: 1.895 ug/l
 RT: 5.293 min Scan# 1245
 Delta R.T. -0.003 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27

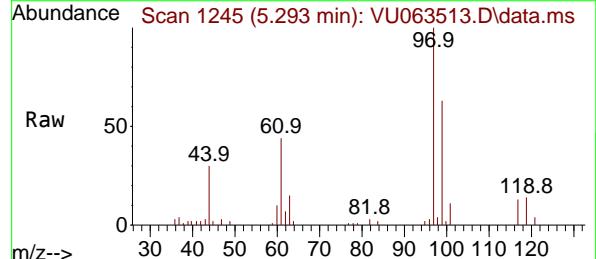

Tgt Ion: 97 Resp: 22170
 Ion Ratio Lower Upper
 97 100
 99 64.2 31.8 95.3
 61 47.0 23.3 69.9

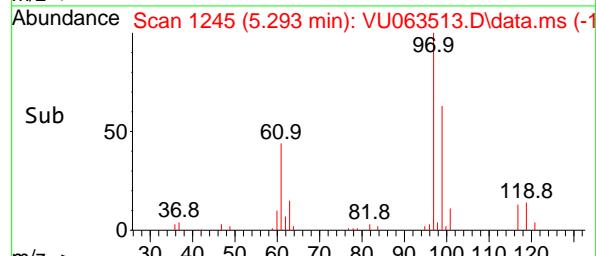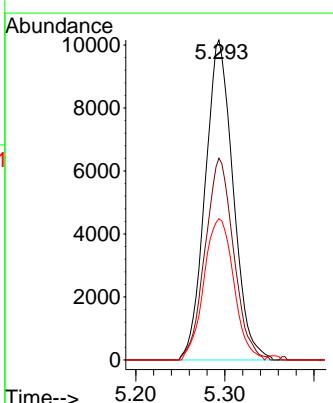

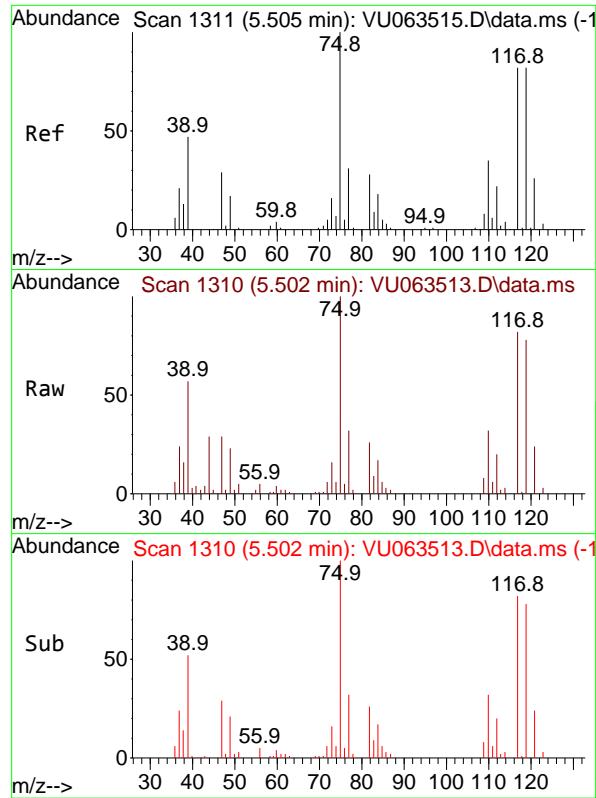

#29

1,1-Dichloropropene

Concen: 1.970 ug/l

RT: 5.502 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U



ClientSampleId :

VSTDICC002

Tgt	Ion	Ion Ratio	Resp:	2134:
			Lower	Upper
75	100			
110	31.6		17.8	53.4
77	29.0		24.6	37.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

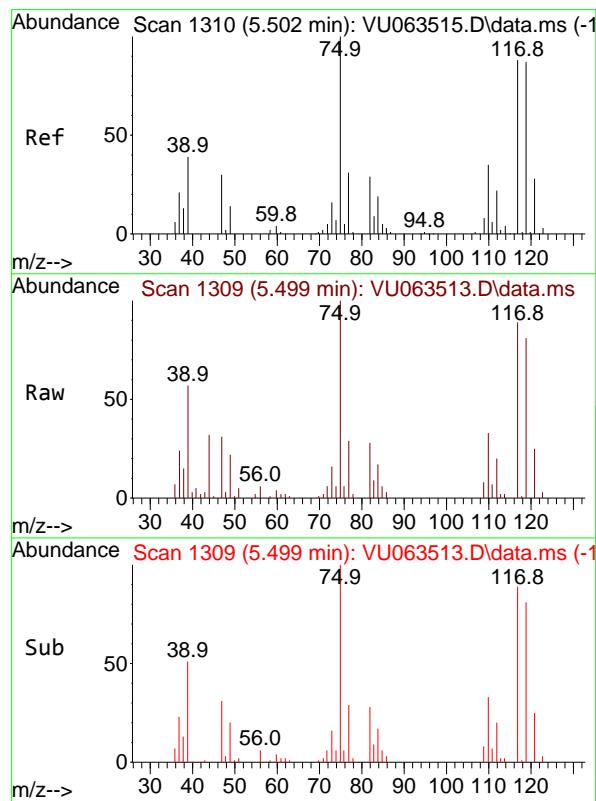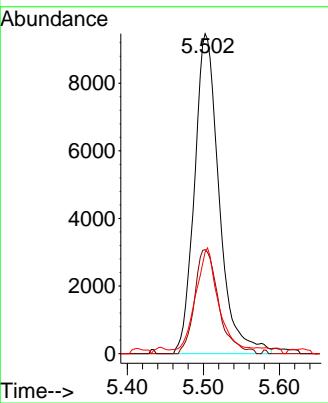

#30

Carbon Tetrachloride

Concen: 1.900 ug/l


RT: 5.499 min Scan# 1309


Delta R.T. -0.003 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27

Tgt	Ion:117	Resp:	17885
117	100		
119	91.2		79.2 118.8
121	28.7		25.5 38.3


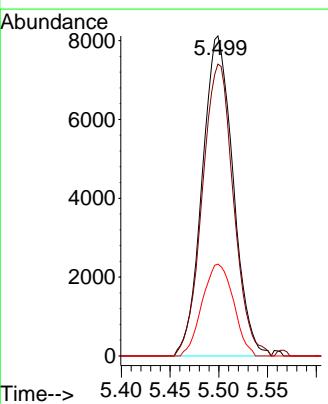





Abundance Scan 839 (3.988 min): VU063513.D\data.ms

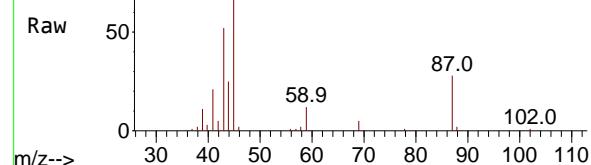


Abundance Scan 839 (3.988 min): VU063513.D\data.ms (-68)

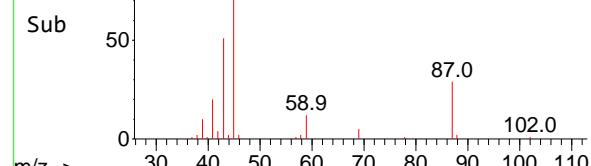

Abundance Scan 999 (4.502 min): VU063513.D\data.ms

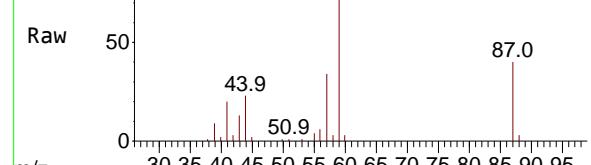

Abundance Scan 999 (4.502 min): VU063513.D\data.ms (-84)

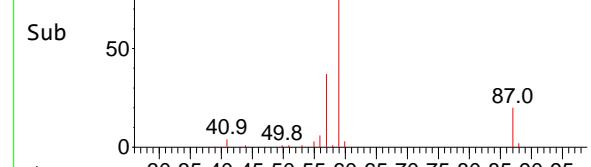

#31

Isopropyl Ether

Concen: 1.914 ug/l

RT: 3.988 min Scan# 8

Delta R.T. -0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002


**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

Abundance

3.988



#32

Ethyl-t-butyl ether

Concen: 1.926 ug/l

RT: 4.502 min Scan# 999

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt Ion: 59 Resp: 36341


Ion Ratio Lower Upper


59 100

87 40.5 32.6 49.0

Abundance

4.502



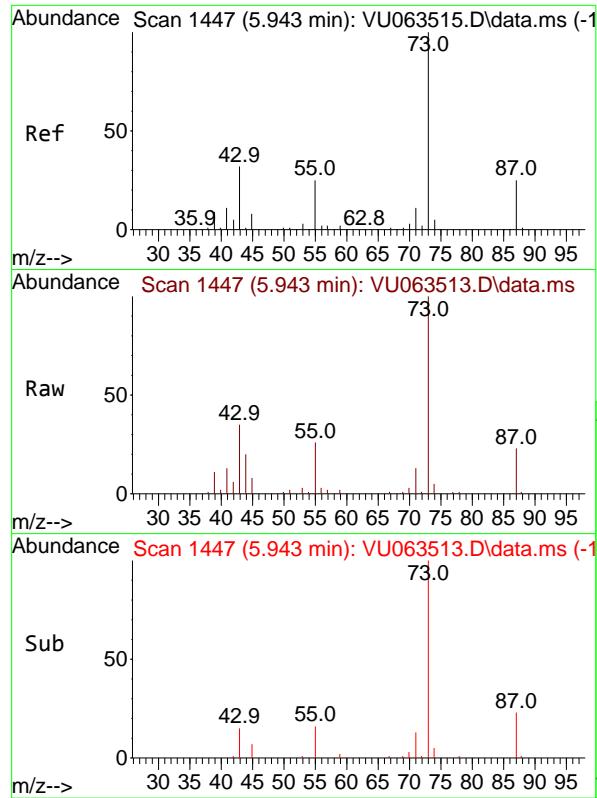


#33

Tert-Amyl methyl ether
Concen: 1.977 ug/l
RT: 5.943 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument: MSVOA_U
ClientSampleId: VSTDICC002

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

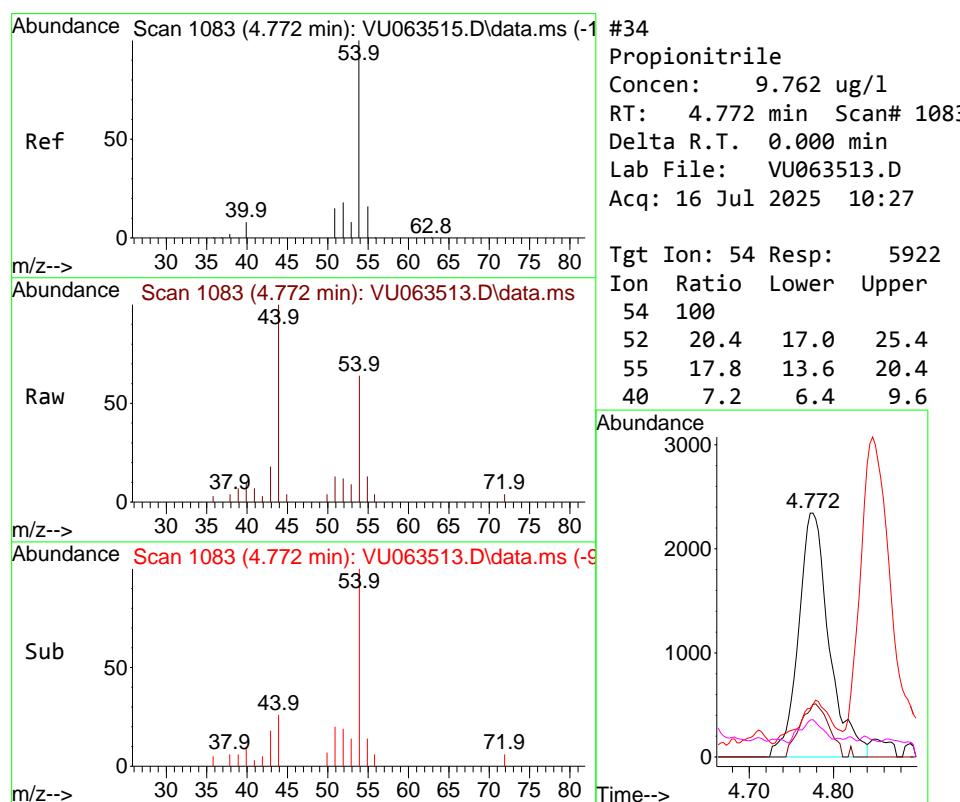


#34


Propionitrile
Concen: 9.762 ug/l
RT: 4.772 min Scan# 1083
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion: 54 Resp: 5922
Ion Ratio Lower Upper
54 100
52 20.4 17.0 25.4
55 17.8 13.6 20.4
40 7.2 6.4 9.6








#35
Benzene
Concen: 1.977 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27




Tgt Ion: 78 Resp: 5756
Ion Ratio Lower Upper
78 100
77 24.1 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

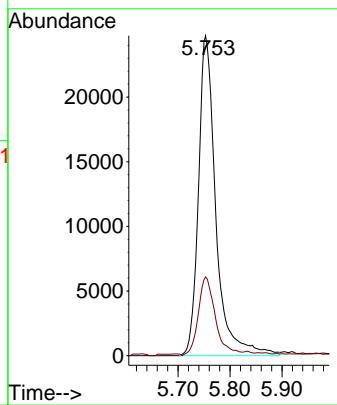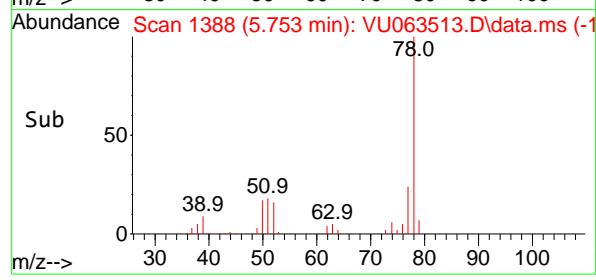


#36
1,2-Dichloroethane
Concen: 1.982 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27




Tgt Ion: 62 Resp: 17934
Ion Ratio Lower Upper
62 100
98 8.0 6.4 9.6

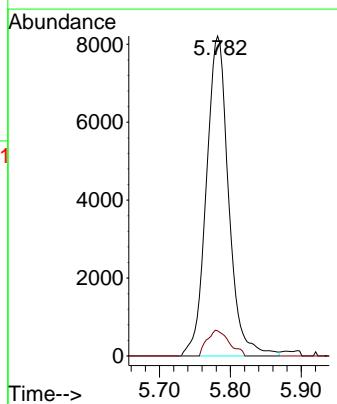



#37
Trichloroethene
Concen: 1.790 ug/l
RT: 6.528 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27



Instrument : MSVOA_U
ClientSampleId : VSTDICC002




Tgt Ion:130 Resp: 13291
Ion Ratio Lower Upper
130 100
95 97.1 80.3 120.5

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



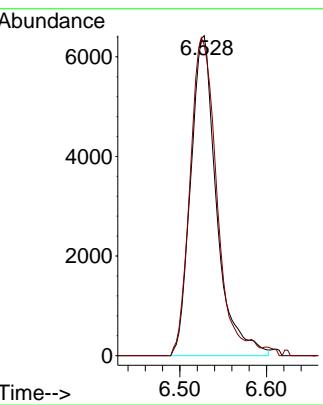


#38
1,2-Dichloropropane
Concen: 1.818 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27



Tgt Ion: 63 Resp: 12386
Ion Ratio Lower Upper
63 100
65 29.1 24.6 36.8

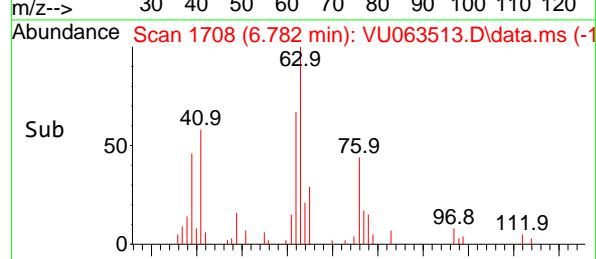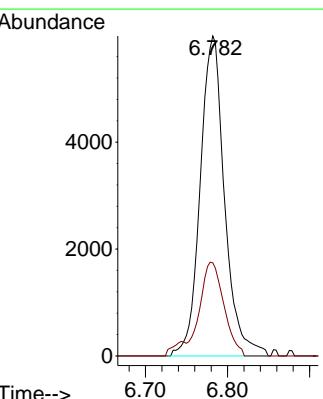

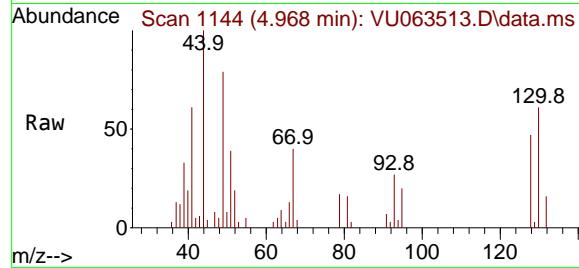

#39

Methacrylonitrile

Concen: 1.982 ug/l

RT: 4.968 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

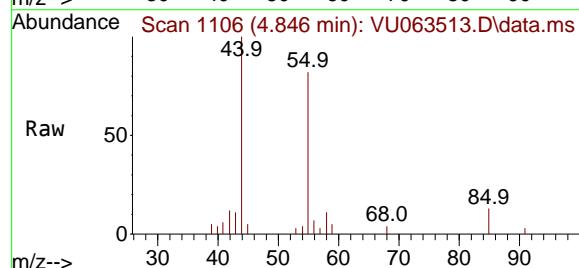 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#40

Methyl acrylate

Concen: 1.755 ug/l

RT: 4.846 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt Ion: 55 Resp: 6918


Ion Ratio Lower Upper




55 100

85 17.8 12.8 19.2

58 9.5 7.0 10.4

42 10.4 7.0 10.4

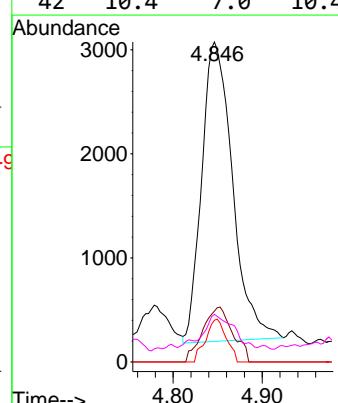

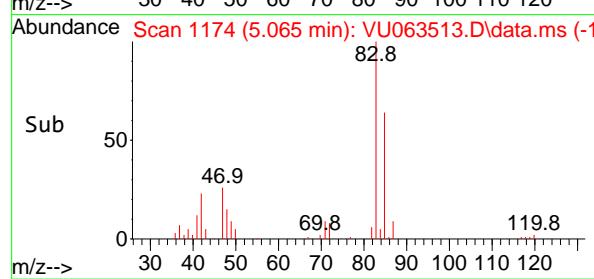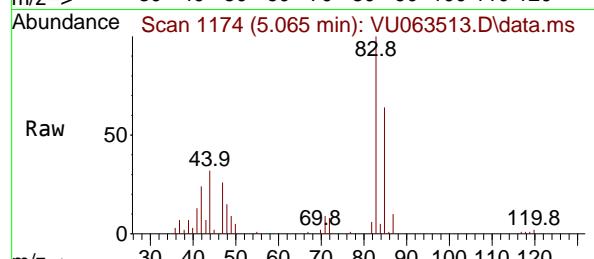

#41

Tetrahydrofuran

Concen: 3.757 ug/l

RT: 5.065 min Scan# 1

Delta R.T. 0.007 min





Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U

ClientSampleId : VSTDICC002

**Manual Integrations
APPROVED**

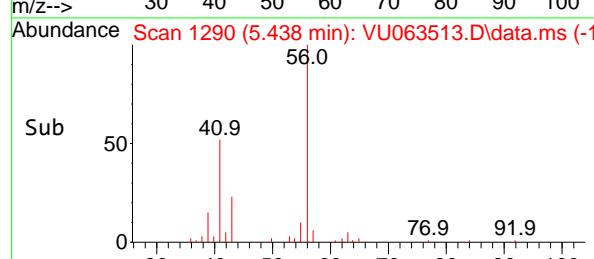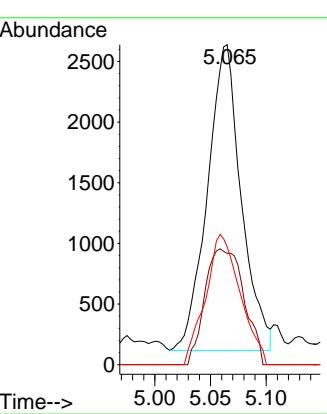 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#42

1-Chlorobutane


Concen: 1.896 ug/l


RT: 5.438 min Scan# 1290

Delta R.T. 0.000 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27

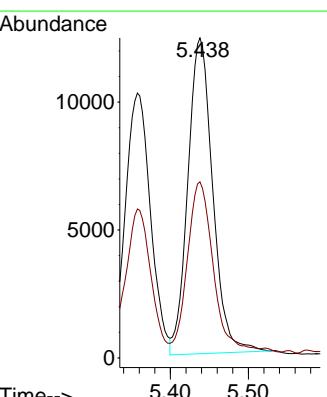 Tgt Ion: 56 Resp: 27320
 Ion Ratio Lower Upper
 56 100
 41 53.4 26.7 80.0




#43
Dibromomethane
Concen: 1.840 ug/l
RT: 6.907 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27




Instrument : MSVOA_U
ClientSampleId : VSTDICC002




Tgt Ion: 93 Resp: 6494
Ion Ratio Lower Upper
93 100
95 81.0 67.9 101.9
174 85.7 74.6 111.8

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


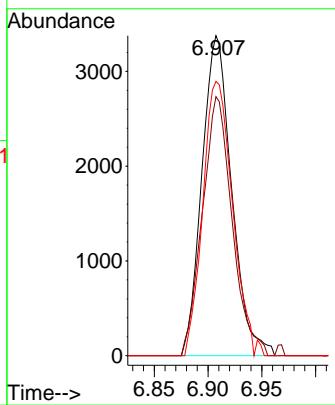
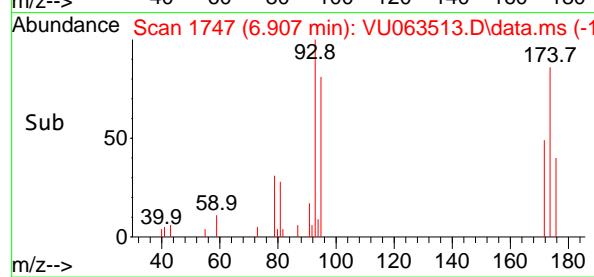


#44
Bromodichloromethane
Concen: 1.862 ug/l
RT: 7.097 min Scan# 1806
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27



Tgt Ion: 83 Resp: 14822
Ion Ratio Lower Upper
83 100
85 61.4 52.7 79.1
127 7.2 8.1 12.1#

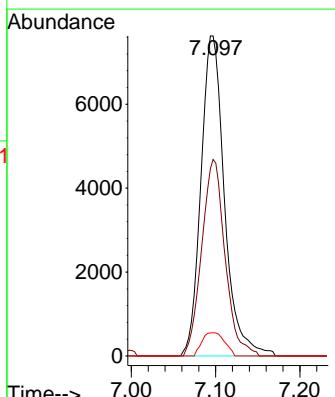



#45

4-Methyl-2-Pentanone

Concen: 9.233 ug/l

RT: 7.798 min Scan# 2

Instrument :

MSVOA_U

Delta R.T. 0.000 min




Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#46

t-1,4-Dichloro-2-butene

Concen: 3.841 ug/l

RT: 10.824 min Scan# 2965

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt Ion: 75 Resp: 4957


Ion Ratio Lower Upper


75 100

53 63.2 48.4 72.6

89 35.9 30.6 45.8

88 28.0 25.3 37.9

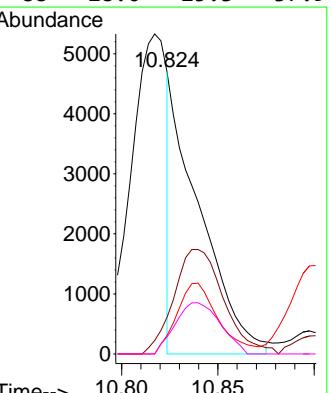








```
#47  
Methyl methacrylate  
Concen: 3.613 ug/l  
RT: 6.968 min Scan# 1  
Delta R.T. 0.007 min  
Lab File: VU063513.D  
Acq: 16 Jul 2025 10:27
```





Instrument :
MSVOA_U
ClientSampleId :
VSTDICC002


Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

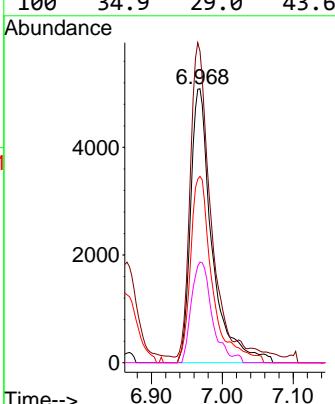



#48
Ethyl methacrylate
Concen: 1.902 ug/l
RT: 8.335 min Scan# 2191
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

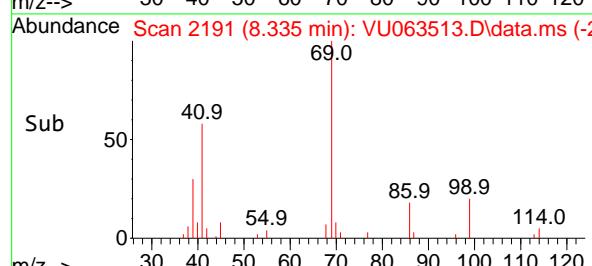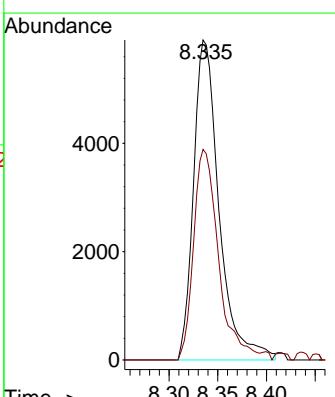



#49
Toluene
Concen: 1.853 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27



Instrument : MSVOA_U
ClientSampleId : VSTDICC002

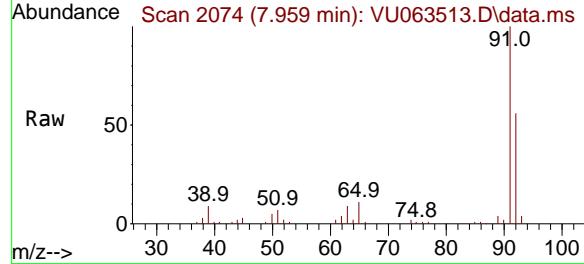


Tgt Ion: 92 Resp: 2945
Ion Ratio Lower Upper
92 100
91 179.2 140.4 210.6

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#50
t-1,3-Dichloropropene
Concen: 1.767 ug/l
RT: 8.206 min Scan# 2151
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27





Tgt Ion: 75 Resp: 11035
Ion Ratio Lower Upper
75 100
77 31.7 24.9 37.3





#51
cis-1,3-Dichloropropene
 Concen: 1.719 ug/l
 RT: 7.602 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27



Instrument : MSVOA_U
 ClientSampleId : VSTDICC002

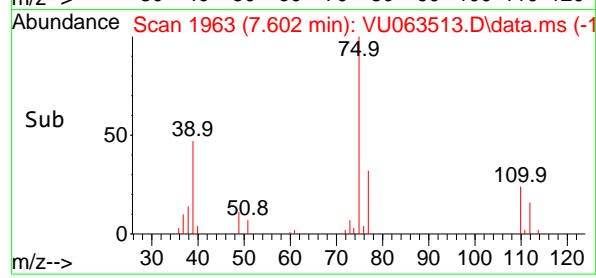


Tgt Ion: 75 Resp: 14409
 Ion Ratio Lower Upper
 75 100
 77 32.1 25.1 37.7
 39 47.3 37.8 56.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025









#52
 1,1,2-Trichloroethane
 Concen: 1.871 ug/l
 RT: 8.393 min Scan# 2209
 Delta R.T. 0.000 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27



Tgt Ion: 97 Resp: 8889
 Ion Ratio Lower Upper
 97 100
 83 87.2 70.2 105.2
 85 52.3 45.2 67.8
 99 62.2 50.1 75.1

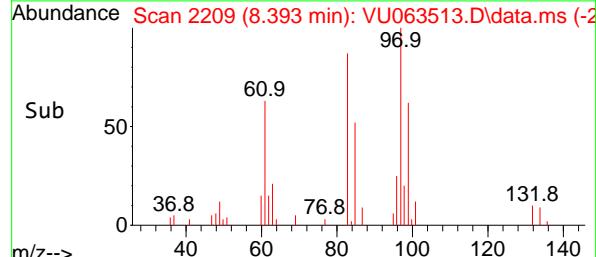

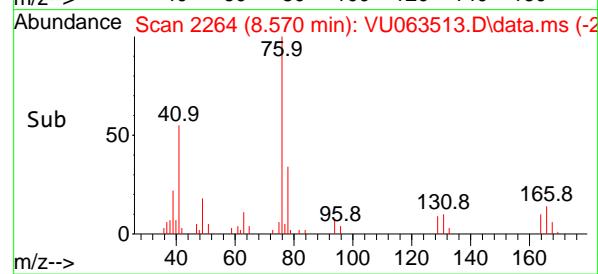

#53

1,3-Dichloropropane

Concen: 1.913 ug/l

RT: 8.570 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC002

Tgt Ion: 76 Resp: 1569

Ion Ratio Lower Upper


76 100

78 33.0 26.0 39.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

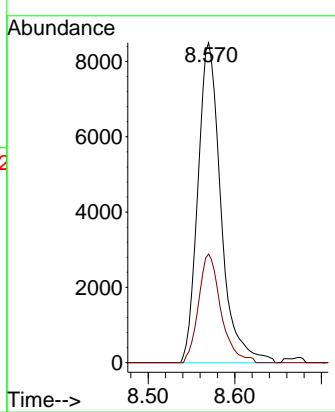

#54

2-Hexanone

Concen: 8.926 ug/l

RT: 8.692 min Scan# 2302

Delta R.T. 0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion: 43 Resp: 21569




Ion Ratio Lower Upper

43 100

58 56.1 34.8 74.8

57 20.2 0.0 39.5

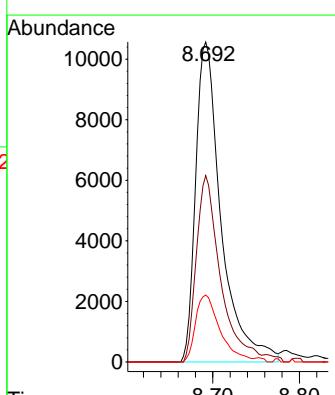



#55

Dibromochloromethane

Concen: 1.824 ug/l

RT: 8.801 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#56

1,2-Dibromoethane

Concen: 1.871 ug/l

RT: 8.920 min Scan# 2373

Delta R.T. 0.003 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27




Tgt Ion:107 Resp: 7956

Ion Ratio Lower Upper

107 100

109 93.9 0.0 186.4

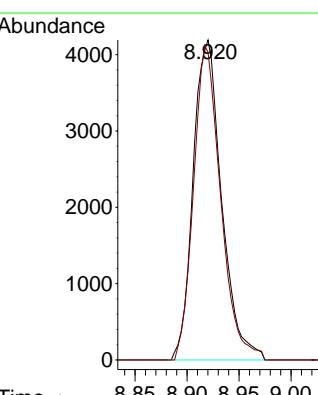



#57

4-Bromofluorobenzene

Concen: 0.953 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument :

MSVOA_U





ClientSampleId :

VSTDICC002

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#58

Tetrachloroethene

Concen: 1.936 ug/l


RT: 8.541 min Scan# 2255




Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt	Ion:164	Resp:	13165
Ion	Ratio	Lower	Upper
164	100		
166	120.2	100.7	151.1
129	98.1	80.6	120.8
131	89.2	77.3	115.9

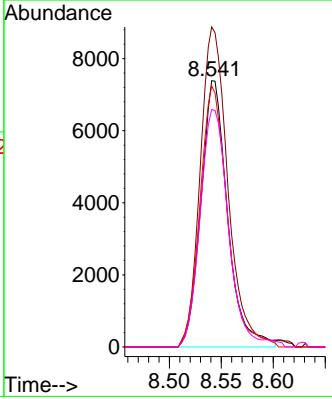

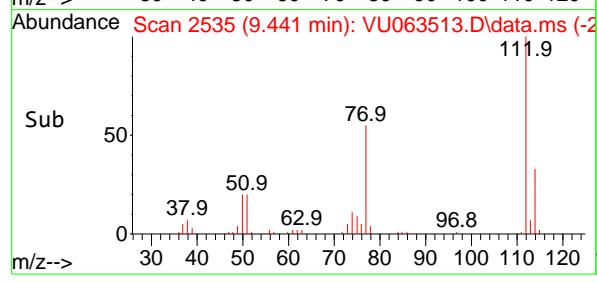

#59

Chlorobenzene

Concen: 1.858 ug/l

RT: 9.441 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063513.D




Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#60

1,1,1,2-Tetrachloroethane

Concen: 1.835 ug/l



RT: 9.525 min Scan# 2561




Delta R.T. -0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt Ion:131 Resp: 10771
Ion Ratio Lower Upper
131 100
133 94.5 74.7 112.1
119 63.8 53.0 79.4

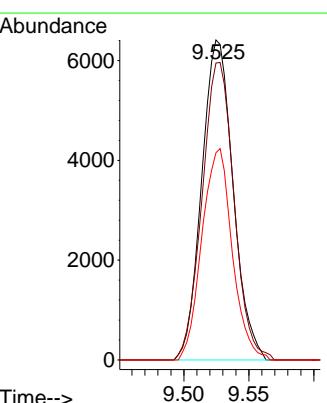



#61

Pentachloroethane

Concen: 1.758 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument :

MSVOA_U





ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

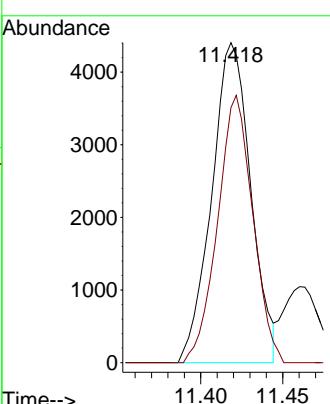

#62

Hexachloroethane

Concen: 1.722 ug/l


RT: 12.467 min Scan# 3476


Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt Ion:117 Resp: 7073
 Ion Ratio Lower Upper
 117 100
 201 66.1 57.4 86.0

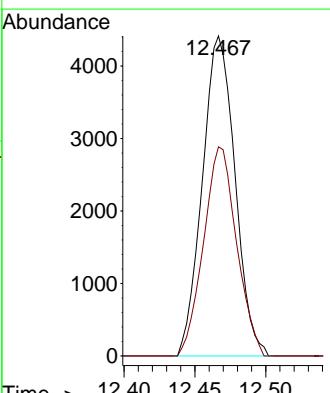



#63

Ethyl Benzene

Concen: 1.874 ug/l

RT: 9.563 min Scan# 2

Instrument:

MSVOA_U


Delta R.T. 0.000 min

Lab File: VU063513.D

ClientSampleId :

Acq: 16 Jul 2025 10:27



VSTDICC002

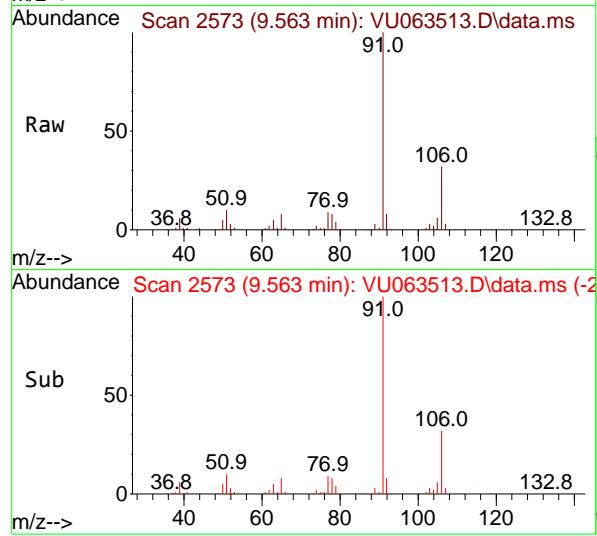

Tgt Ion: 91 Resp: 58862
 Ion Ratio Lower Upper
 91 100
 106 31.8 25.4 38.0


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

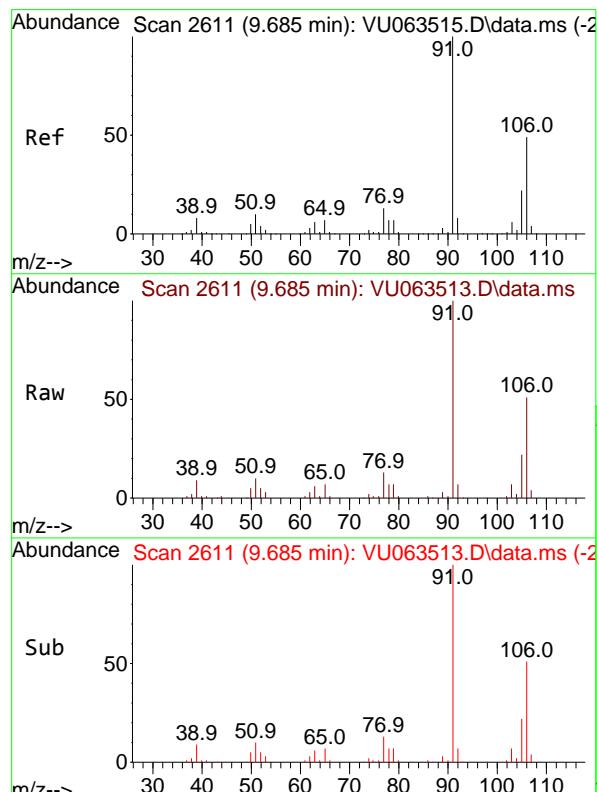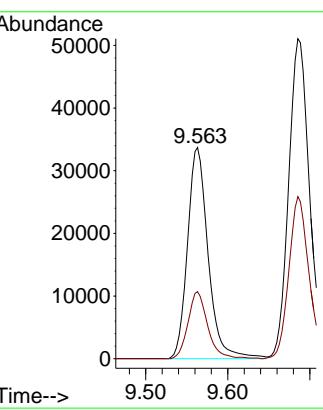

#64
 m/p-Xylenes
 Concen: 3.756 ug/l
 RT: 9.685 min Scan# 2611
 Delta R.T. 0.000 min
 Lab File: VU063513.D
 Acq: 16 Jul 2025 10:27

Tgt Ion:106 Resp: 45864
 Ion Ratio Lower Upper
 106 100
 91 200.6 163.6 245.4

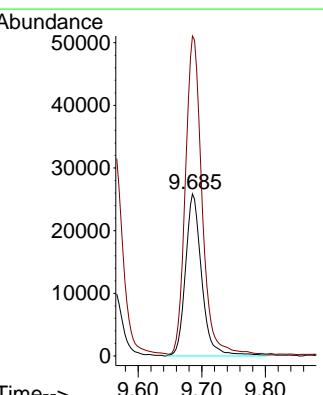


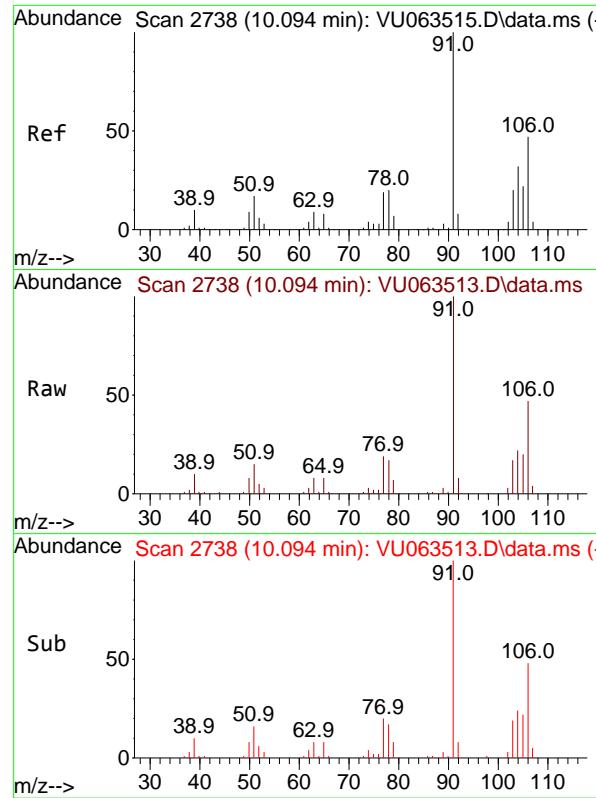


#65
o-Xylene
Concen: 1.819 ug/l
RT: 10.094 min Scan# 21340
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U
ClientSampleId : VSTDICC002


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

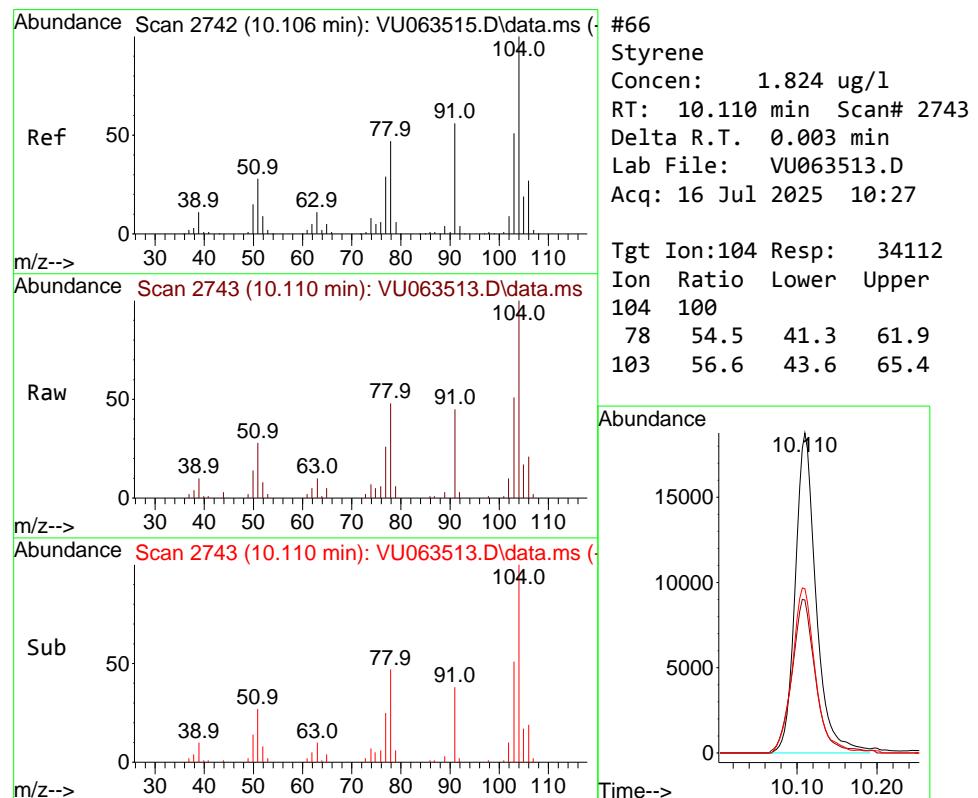

#66
Styrene
Concen: 1.824 ug/l
RT: 10.110 min Scan# 2743
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion:104 Resp: 34112
Ion Ratio Lower Upper
104 100
78 54.5 41.3 61.9
103 56.6 43.6 65.4

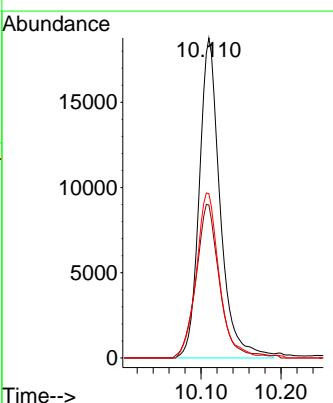

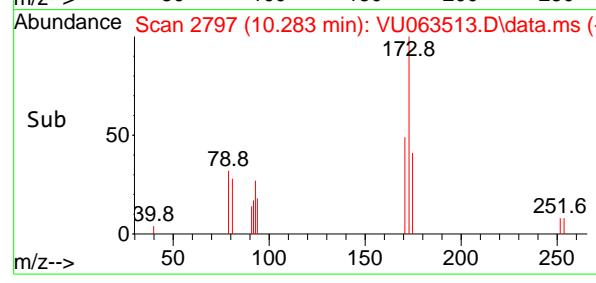

#67

Bromoform

Concen: 1.759 ug/l

RT: 10.283 min Scan# 2

Instrument:

Delta R.T. 0.000 min

MSVOA_U

Lab File: VU063513.D

ClientSampleId :





Acq: 16 Jul 2025 10:27

VSTDICC002

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

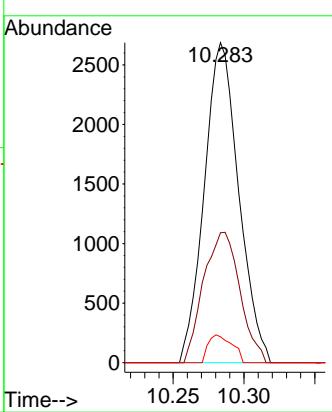

#68

1,2-Dichlorobenzene-d4

Concen: 0.932 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Tgt	Ion:152	Resp:	8064
Ion	Ratio	Lower	Upper
152	100		
115	81.3	0.0	262.2
150	189.8	0.0	651.2

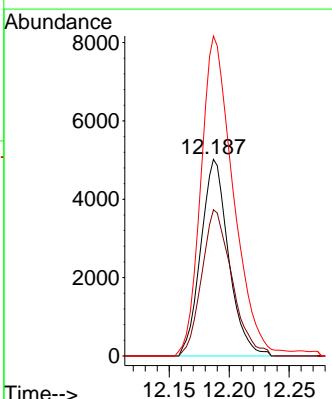

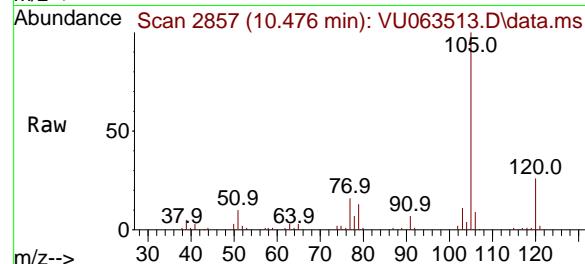

#69

Isopropylbenzene

Concen: 1.842 ug/l

RT: 10.476 min Scan# 2

Instrument :

Delta R.T. 0.000 min

MSVOA_U

Lab File: VU063513.D

ClientSampleId :

Acq: 16 Jul 2025 10:27

VSTDICC002

Tgt Ion:105 Resp: 52260

Ion Ratio Lower Upper




105 100

120 26.0 13.2 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 1.852 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion: 83 Resp: 10710




Ion Ratio Lower Upper

83 100

131 9.2 8.4 12.6

85 62.4 51.9 77.9

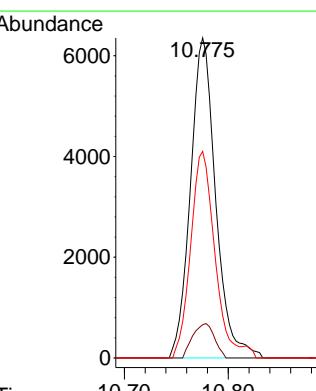



#71

1,2,3-Trichloropropane

Concen: 1.903 ug/l m

RT: 10.817 min Scan# 2963

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#72

Bromobenzene

Concen: 1.791 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion:156 Resp: 13109




Ion Ratio Lower Upper

156 100

77 200.0 0.0 315.2

158 100.1 0.0 195.4

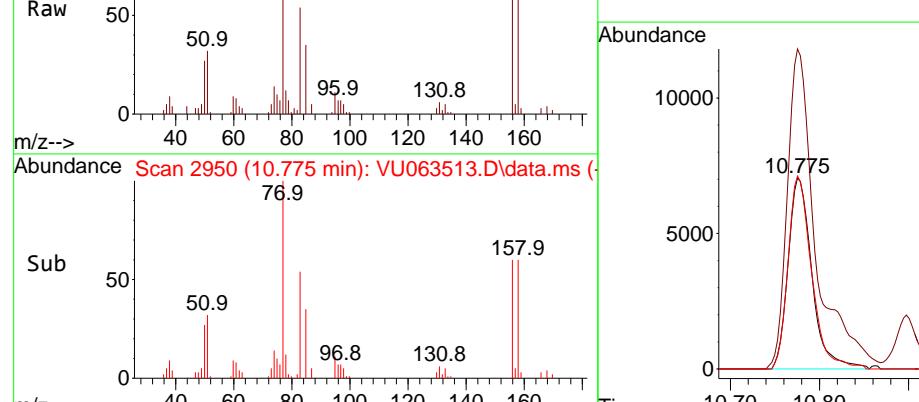



#73

n-propylbenzene

Concen: 1.868 ug/l

RT: 10.901 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#74

2-Chlorotoluene

Concen: 1.864 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063513.D


Acq: 16 Jul 2025 10:27




Tgt Ion:126 Resp: 14070

Ion Ratio Lower Upper

126 100

91 299.8 0.0 606.0

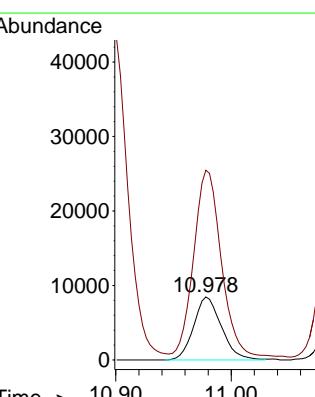






#75
1,3,5-Trimethylbenzene
Concen: 1.847 ug/l
RT: 11.081 min Scan# 3045
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U
ClientSampleId : VSTDICC002


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#76
4-Chlorotoluene
Concen: 1.911 ug/l
RT: 11.094 min Scan# 3049
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion:126 Resp: 14644
Ion Ratio Lower Upper
126 100
91 322.3 0.0 682.2




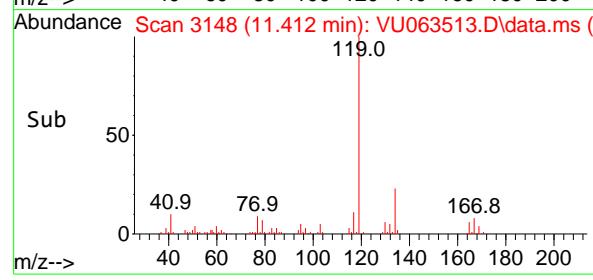




#77
tert-Butylbenzene
Concen: 1.860 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U
ClientSampleId : VSTDICC002


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025





#78
1,2,4-Trimethylbenzene
Concen: 1.846 ug/l
RT: 11.460 min Scan# 3163
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion:105 Resp: 49637
Ion Ratio Lower Upper
105 100
120 45.0 22.7 68.0

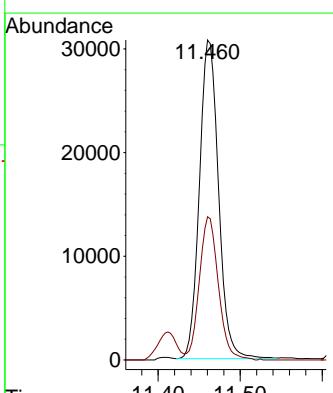





Abundance Scan 3217 (11.634 min): VU063513.D\data.ms (-)

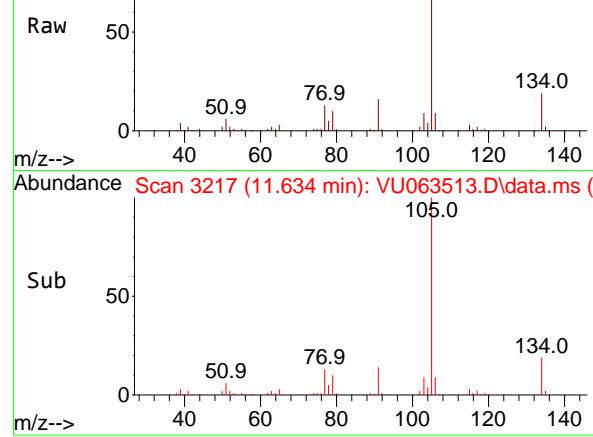

Abundance Scan 3705 (13.203 min): VU063515.D\data.ms (-)

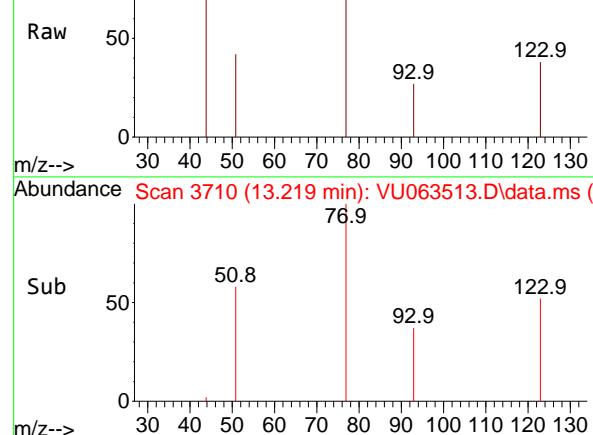

Abundance Scan 3710 (13.219 min): VU063513.D\data.ms (-)

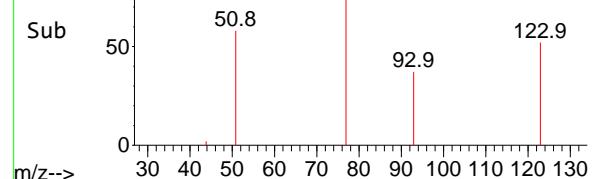

#79

sec-Butylbenzene

Concen: 1.845 ug/l

RT: 11.634 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

Tgt Ion:105 Resp: 6444

Ion Ratio Lower Upper


105 100

134 19.4 16.2 24.4

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

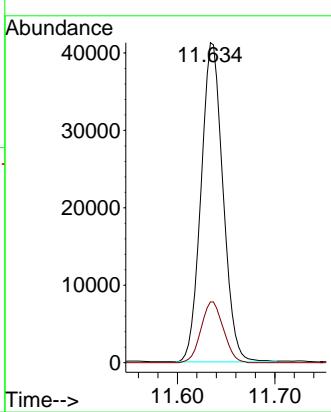

#80

Nitrobenzene

Concen: 9.644 ug/l

RT: 13.219 min Scan# 3710

Delta R.T. 0.016 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion: 77 Resp: 861




Ion Ratio Lower Upper

77 100

123 31.0 16.9 59.7

65 0.0 16.5 20.9#



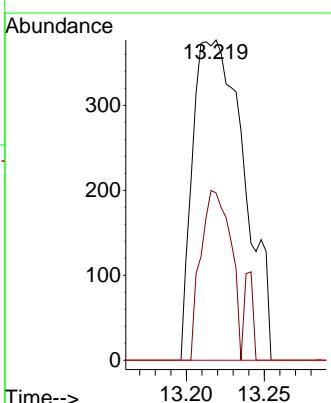


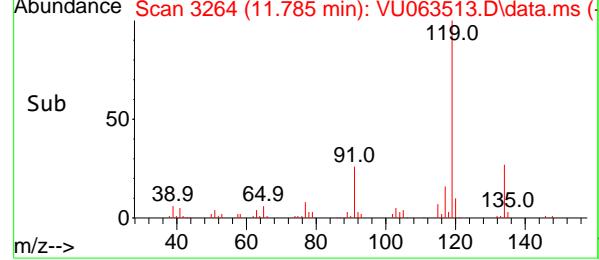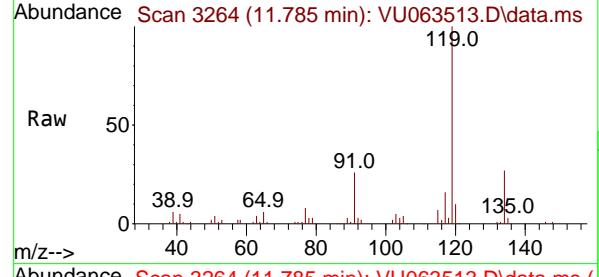

#81
p-Isopropyltoluene
Concen: 1.850 ug/l
RT: 11.785 min Scan# 3
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27
ClientSampleId : VSTDICC002


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

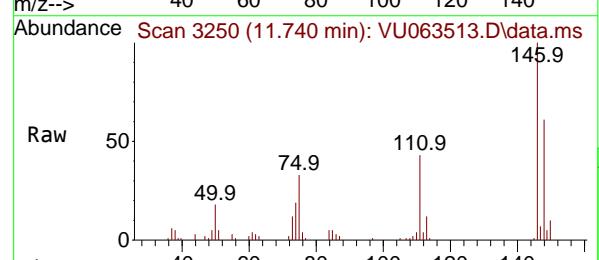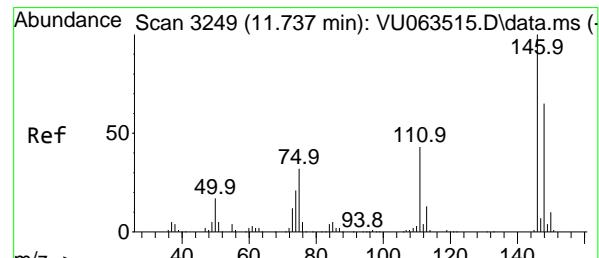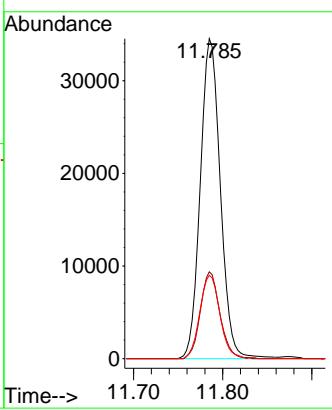

#82
1,3-Dichlorobenzene
Concen: 1.833 ug/l
RT: 11.740 min Scan# 3250
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion:146 Resp: 26844
Ion Ratio Lower Upper
146 100
111 43.2 33.8 50.6
148 63.5 51.5 77.3

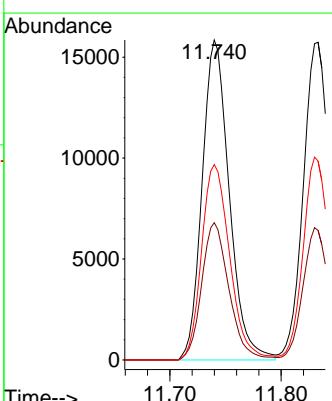


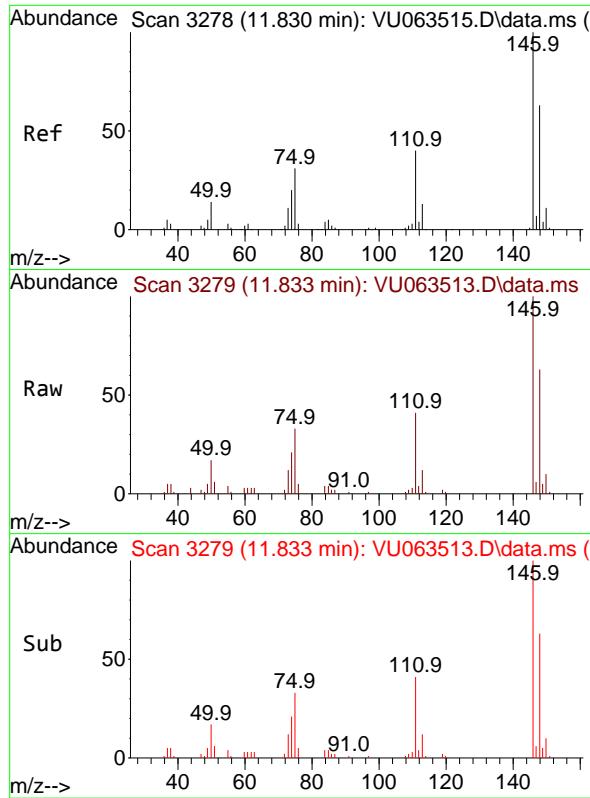


#83
1,4-Dichlorobenzene
Concen: 1.818 ug/l
RT: 11.833 min Scan# 31
Instrument : MSVOA_U
Delta R.T. 0.003 min
Lab File: VU063513.D ClientSampleId :
Acq: 16 Jul 2025 10:27 VSTDICC002

Instrument : SVOA_U
ClientSampleId : STDICC002

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

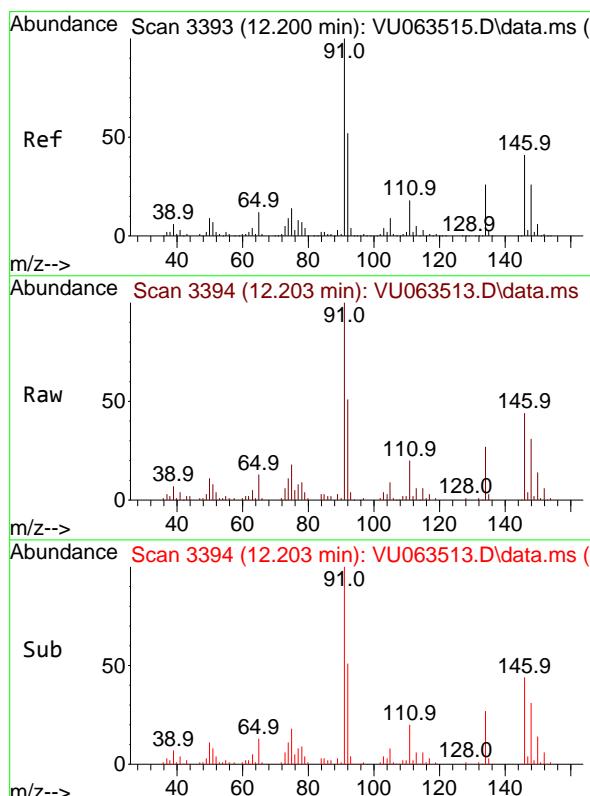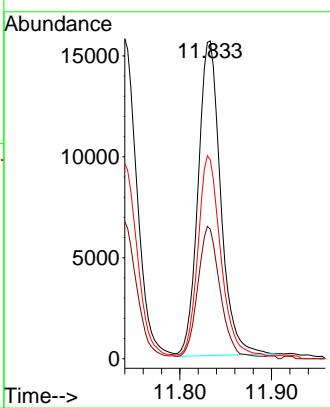





#84
n-Butylbenzene
Concen: 1.801 ug/l
RT: 12.203 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

```

Tgt Ion: 91 Resp: 48694
Ion Ratio Lower Upper
 91 100
 92 52.6 41.5 62.3
134 25.2 20.6 30.8

```

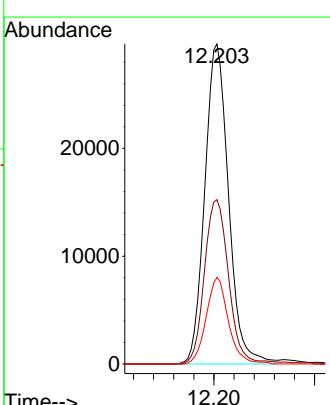

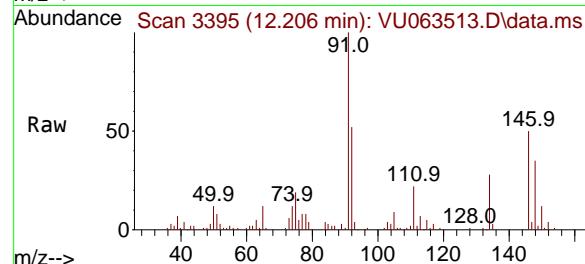

#85

1,2-Dichlorobenzene

Concen: 1.805 ug/l

RT: 12.206 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC002

Tgt Ion:146 Resp: 24834

Ion Ratio Lower Upper

146 100




111 43.8 21.7 65.1

148 64.9 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 2.046 ug/l

RT: 12.994 min Scan# 3640

Delta R.T. 0.007 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion: 75 Resp: 1550


Ion Ratio Lower Upper

75 100

155 69.8 65.8 98.6

157 97.1 81.4 122.2

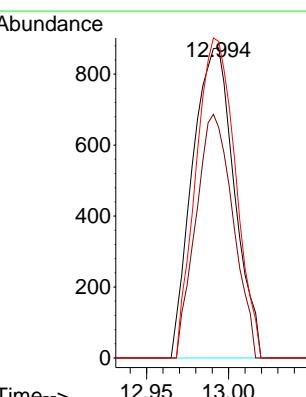


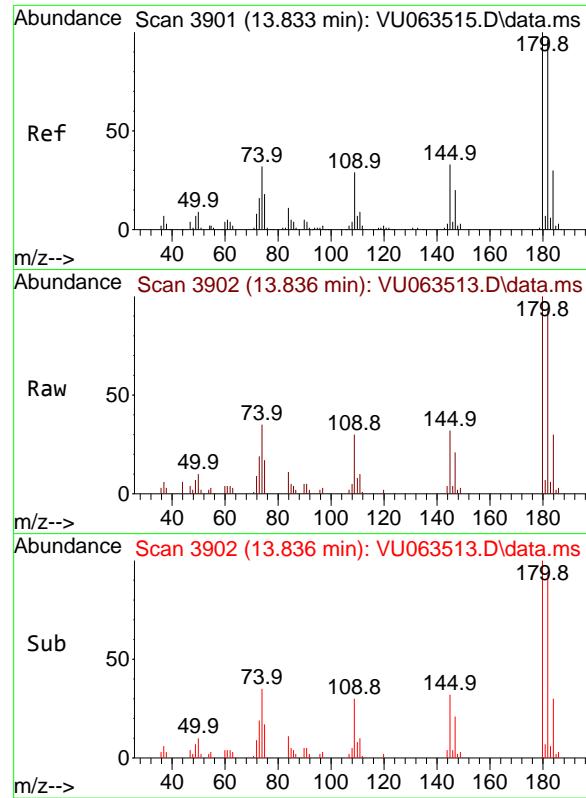


#87
1,2,4-Trichlorobenzene
Concen: 1.791 ug/l
RT: 13.836 min Scan# 3902
Delta R.T. 0.003 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Instrument : MSVOA_U
ClientSampleId : VSTDICC002


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

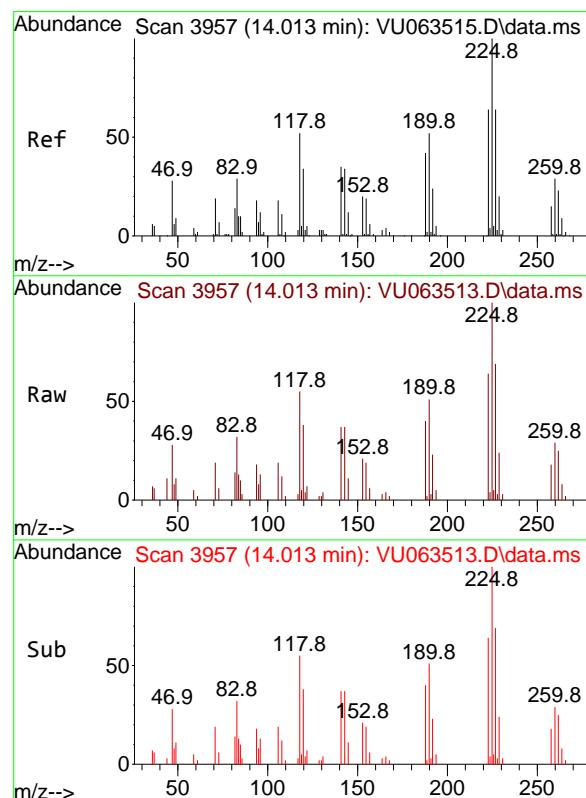

#88
Hexachlorobutadiene
Concen: 1.826 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063513.D
Acq: 16 Jul 2025 10:27

Tgt Ion:225 Resp: 8872
Ion Ratio Lower Upper
225 100
223 62.3 50.8 76.2
227 66.2 51.0 76.6



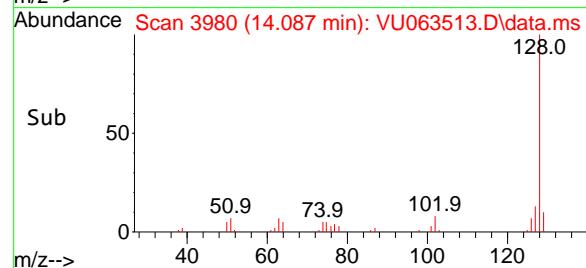

#89

Naphthalene

Concen: 1.675 ug/l

RT: 14.087 min Scan# 3

Delta R.T. 0.007 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC002

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#90

1,2,3-Trichlorobenzene

Concen: 1.770 ug/l

RT: 14.325 min Scan# 4054

Delta R.T. 0.003 min

Lab File: VU063513.D

Acq: 16 Jul 2025 10:27


Tgt Ion:180 Resp: 13999

Ion Ratio Lower Upper

180 100

182 98.2 78.0 117.0

145 33.8 27.3 40.9

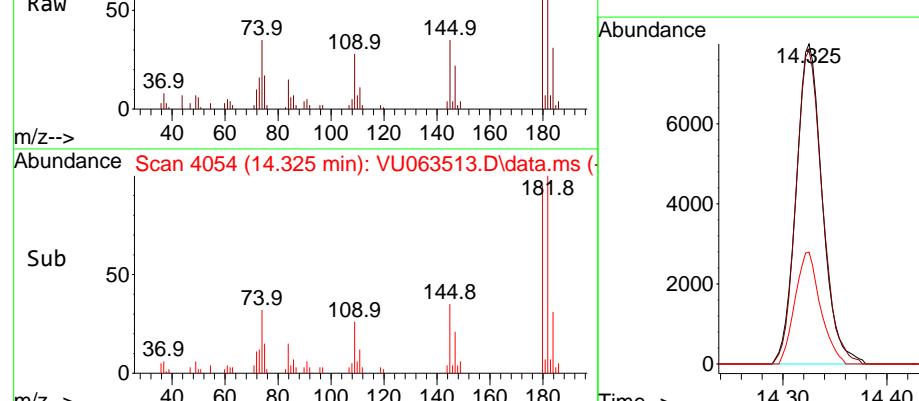

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063514.D
 Acq On : 16 Jul 2025 11:00
 Operator : MD/SY
 Sample : VSTDICC005
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC005

Quant Time: Jul 17 03:24:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	26058	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	9401	0.953	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	8923	0.978	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	37785	4.918	ug/l	100
3) Chloromethane	1.518	50	35181	4.926	ug/l	99
4) Vinyl Chloride	1.599	62	44244	4.864	ug/l	99
5) Bromomethane	1.846	94	32799	4.782	ug/l	100
6) Chloroethane	1.923	64	26955	4.908	ug/l	99
7) Trichlorofluoromethane	2.129	101	64344	4.927	ug/l	99
8) 1,1,2-Trichloro-1,2,2-...	2.566	101	34008	4.983	ug/l	99
9) 1,1-Dichloroethene	2.566	96	33329	4.927	ug/l	98
10) Iodomethane	2.708	142	39902	4.500	ug/l	99
11) Allyl Chloride	2.907	41	46826	4.791	ug/l	97
12) Acrylonitrile	3.306	53	16229	9.586	ug/l	99
13) Acetone	2.618	43	29387	21.677	ug/l	98
14) Carbon Disulfide	2.779	76	106742	4.885	ug/l	99
15) Methylene Chloride	3.029	84	37774	4.742	ug/l	99
16) trans-1,2-Dichloroethene	3.335	96	37017	4.818	ug/l	96
17) 1,1-Dichloroethane	3.849	63	70167	4.927	ug/l	98
18) 2-Butanone	4.714	43	48390	23.049	ug/l	100
19) Cyclohexane	5.361	56	58522	4.854	ug/l	100
20) Methylcyclohexane	6.740	83	52941	4.517	ug/l	98
21) 2,2-Dichloropropane	4.644	77	56419	4.653	ug/l	99
22) cis-1,2-Dichloroethene	4.650	96	40321	4.836	ug/l	99
23) Diethyl Ether	2.370	59	25929	5.030	ug/l	99
24) tert-Butyl Alcohol	3.190	59	29561	47.503	ug/l	99
25) Methyl tert-Butyl Ether	3.361	73	86741	4.911	ug/l	98
26) Bromochloromethane	4.955	128	17243	4.953	ug/l	95
27) Chloroform	5.071	83	70739	4.868	ug/l	100
28) 1,1,1-Trichloroethane	5.293	97	61347	4.974	ug/l	99
29) 1,1-Dichloropropene	5.505	75	55976	4.899	ug/l	99
30) Carbon Tetrachloride	5.499	117	49682	5.005	ug/l	100
31) Isopropyl Ether	3.994	45	105534	4.909	ug/l	99
32) Ethyl-t-butyl ether	4.502	59	94505	4.751	ug/l	99
33) Tert-Amyl methyl ether	5.943	73	84936	4.920	ug/l	99
34) Propionitrile	4.775	54	16304	25.489	ug/l	96
35) Benzene	5.753	78	156970	5.113	ug/l	96
36) 1,2-Dichloroethane	5.782	62	48312	5.065	ug/l	100
37) Trichloroethene	6.525	130	35295	4.506	ug/l	94
38) 1,2-Dichloropropane	6.782	63	33611	4.678	ug/l	98
39) Methacrylonitrile	4.972	41	12545	4.468	ug/l	96
40) Methyl acrylate	4.846	55	19739	4.749	ug/l	98
41) Tetrahydrofuran	5.058	42	13119	8.771	ug/l	99
42) 1-Chlorobutane	5.438	56	75929	4.999	ug/l	93
43) Dibromomethane	6.907	93	17942	4.821	ug/l	95
44) Bromodichloromethane	7.094	83	40349	4.807	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063514.D
 Acq On : 16 Jul 2025 11:00
 Operator : MD/SY
 Sample : VSTDICC005
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC005

Quant Time: Jul 17 03:24:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	95213	24.821	ug/1	99
46) t-1,4-Dichloro-2-butene	10.823	75	13369m	9.823	ug/1	
47) Methyl methacrylate	6.965	69	30554	9.775	ug/1	97
48) Ethyl methacrylate	8.335	69	29487	4.943	ug/1	95
49) Toluene	7.959	92	83681	4.993	ug/1	100
50) t-1,3-Dichloropropene	8.206	75	32573	4.946	ug/1	98
51) cis-1,3-Dichloropropene	7.602	75	43517	4.923	ug/1	99
52) 1,1,2-Trichloroethane	8.393	97	24935	4.976	ug/1	98
53) 1,3-Dichloropropane	8.569	76	42938	4.964	ug/1	98
54) 2-Hexanone	8.688	43	62636	24.583	ug/1	99
55) Dibromochloromethane	8.801	129	26834	5.067	ug/1	98
56) 1,2-Dibromoethane	8.917	107	22293	4.971	ug/1	100
58) Tetrachloroethene	8.544	164	35190	4.909	ug/1	98
59) Chlorobenzene	9.441	112	95389	4.955	ug/1	99
60) 1,1,1,2-Tetrachloroethane	9.524	131	30337	4.901	ug/1	98
61) Pentachloroethane	11.418	117	21959	5.020	ug/1	96
62) Hexachloroethane	12.466	117	22137	5.110	ug/1	97
63) Ethyl Benzene	9.563	91	163996	4.951	ug/1	99
64) m/p-Xylenes	9.685	106	127196	9.878	ug/1	98
65) o-Xylene	10.090	106	61641	4.982	ug/1	98
66) Styrene	10.106	104	99507	5.046	ug/1	98
67) Bromoform	10.283	173	13680	5.030	ug/1	99
69) Isopropylbenzene	10.476	105	149628	5.002	ug/1	100
70) 1,1,2,2-Tetrachloroethane	10.775	83	29913	4.906	ug/1	99
71) 1,2,3-Trichloropropane	10.817	75	23113m	4.645	ug/1	
72) Bromobenzene	10.775	156	38144	4.941	ug/1	99
73) n-propylbenzene	10.897	120	44825	4.978	ug/1	96
74) 2-Chlorotoluene	10.978	126	39249	4.932	ug/1	94
75) 1,3,5-Trimethylbenzene	11.081	105	143599	5.025	ug/1	100
76) 4-Chlorotoluene	11.090	126	40518	5.014	ug/1	100
77) tert-Butylbenzene	11.412	119	135731	4.970	ug/1	99
78) 1,2,4-Trimethylbenzene	11.460	105	142811	5.038	ug/1	99
79) sec-Butylbenzene	11.634	105	184683	5.015	ug/1	100
80) Nitrobenzene	13.206	77	2721	23.955	ug/1 #	90
81) p-Isopropyltoluene	11.785	119	156566	5.093	ug/1	99
82) 1,3-Dichlorobenzene	11.740	146	77340	5.007	ug/1	98
83) 1,4-Dichlorobenzene	11.830	146	76910	4.975	ug/1	99
84) n-Butylbenzene	12.200	91	145033	5.087	ug/1	100
85) 1,2-Dichlorobenzene	12.206	146	71942	4.958	ug/1	99
86) 1,2-Dibromo-3-Chloropr...	12.987	75	4378	4.863	ug/1	95
87) 1,2,4-Trichlorobenzene	13.833	180	44492	4.931	ug/1	99
88) Hexachlorobutadiene	14.013	225	25355	4.948	ug/1	99
89) Naphthalene	14.081	128	76448	4.728	ug/1	100
90) 1,2,3-Trichlorobenzene	14.322	180	41834	5.017	ug/1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063514.D
Acq On : 16 Jul 2025 11:00
Operator : MD/SY
Sample : VSTDIICC005
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1


Quant Time: Jul 17 03:24:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:16:16 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC005

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

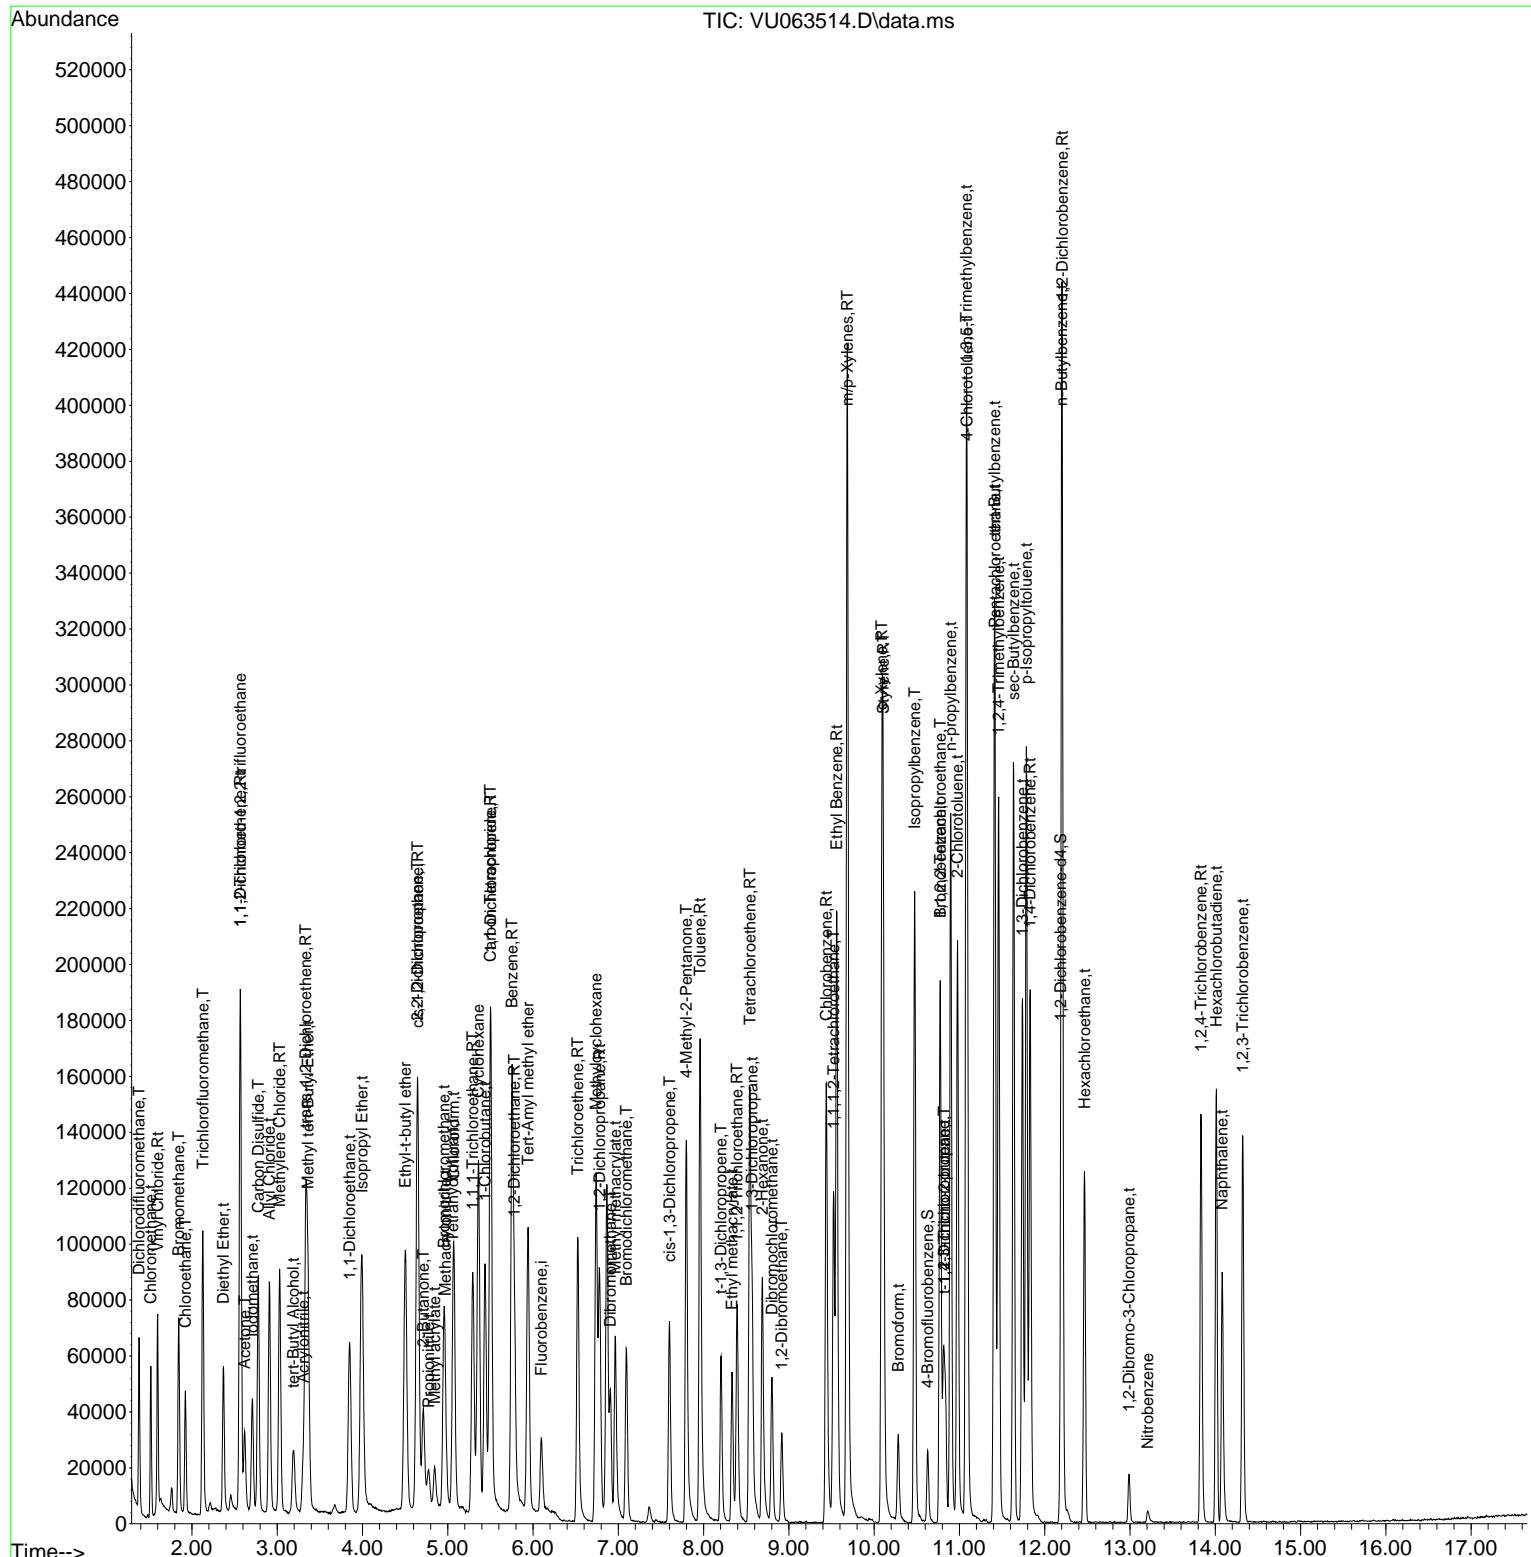

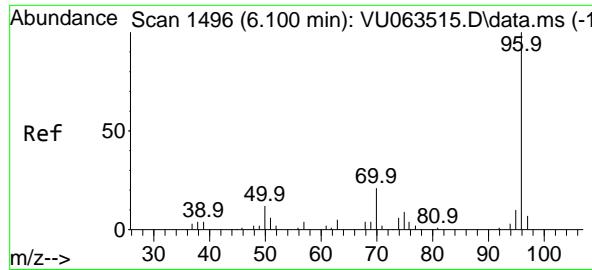

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U
ClientSampleId : VSTDICC005






Tgt Ion: 96 Resp: 26053

Ion Ratio Lower Upper


Ion	Ratio	Lower	Upper
96	100		
70	18.6	15.0	22.4
95	9.1	7.4	11.0
97	6.7	0.0	0.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

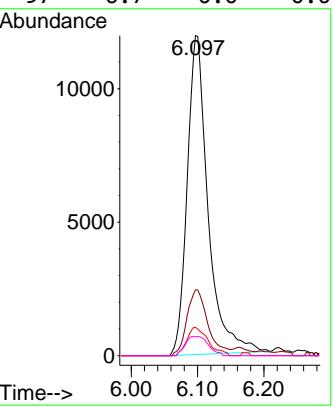
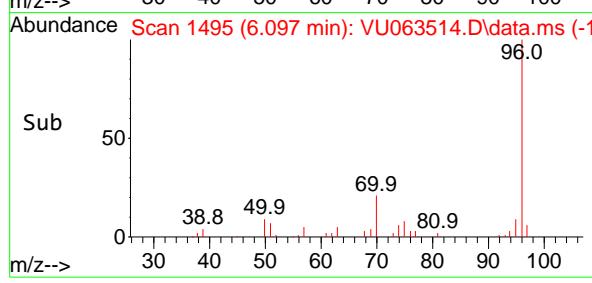





#2
Dichlorodifluoromethane
Concen: 4.918 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00



Tgt Ion: 85 Resp: 37785

Ion	Ratio	Lower	Upper
85	100		
87	31.7	16.0	47.9

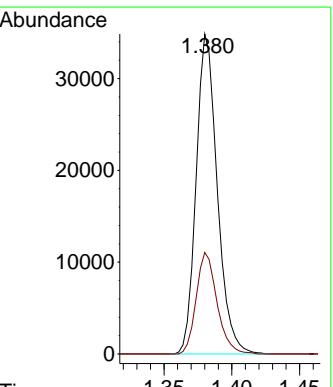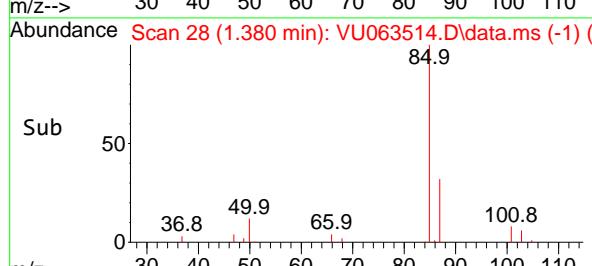



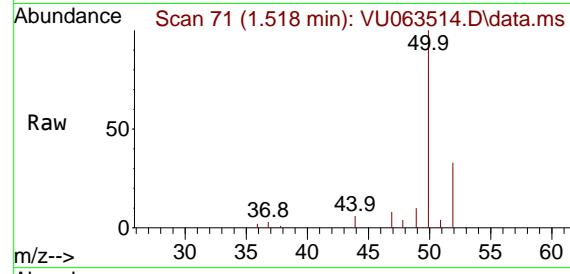



#3
Chloromethane
Concen: 4.926 ug/l
RT: 1.518 min Scan# 7
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U
ClientSampleId : VSTDICC005


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

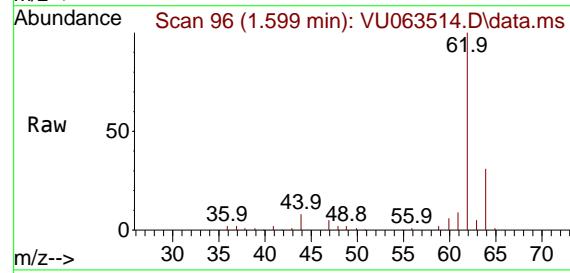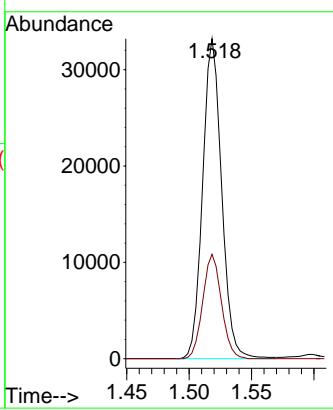

#4
Vinyl Chloride
Concen: 4.864 ug/l
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Tgt Ion: 62 Resp: 44244
Ion Ratio Lower Upper
62 100
64 31.5 25.7 38.5



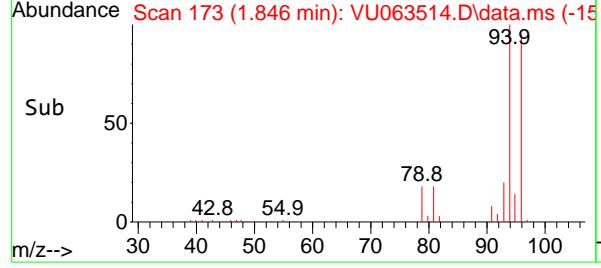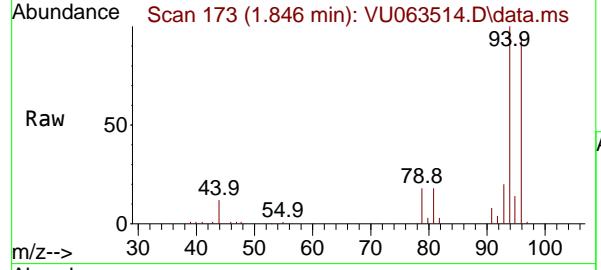

#5

Bromomethane

Concen: 4.782 ug/l

RT: 1.846 min Scan# 1

Delta R.T. 0.006 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

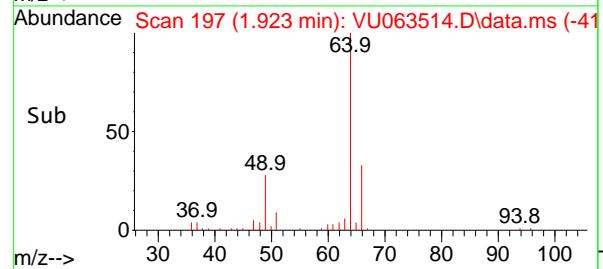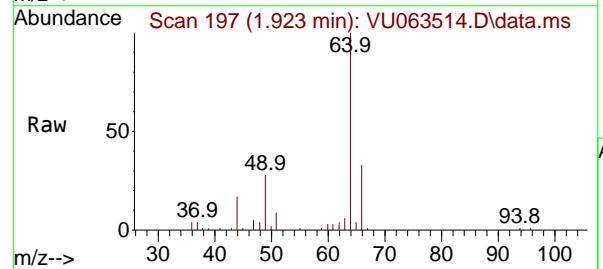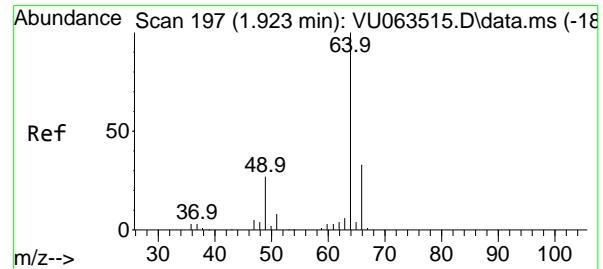 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#6

Chloroethane


Concen: 4.908 ug/l




RT: 1.923 min Scan# 197

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

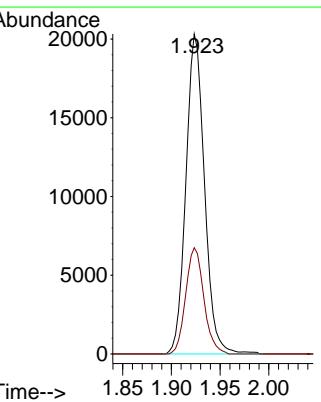 Tgt Ion: 64 Resp: 26955
 Ion Ratio Lower Upper
 64 100
 66 33.2 26.2 39.4




#7

Trichlorofluoromethane

Concen: 4.927 ug/l

RT: 2.129 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#8

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 4.983 ug/l

RT: 2.566 min Scan# 397

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00





Tgt Ion:101 Resp: 34008


Ion Ratio Lower Upper

101 100

85 46.3 37.8 56.6


151 73.2 59.2 88.8

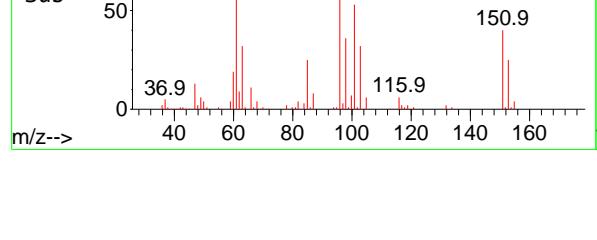



#9
1,1-Dichloroethene
Concen: 4.927 ug/l
RT: 2.566 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00




Instrument : MSVOA_U
ClientSampleId : VSTDICC005

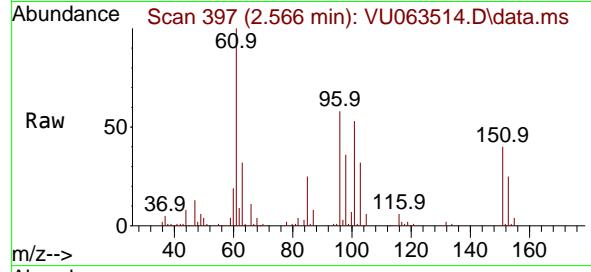


Tgt Ion: 96 Resp: 33329
Ion Ratio Lower Upper
96 100
61 172.1 0.0 504.3
98 62.5 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

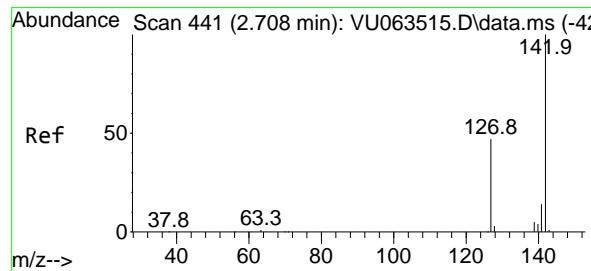
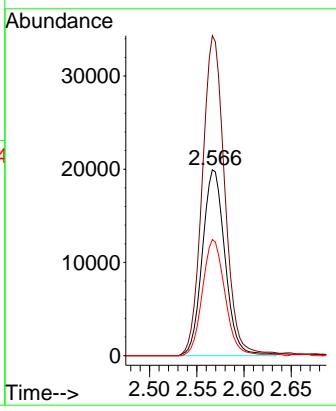
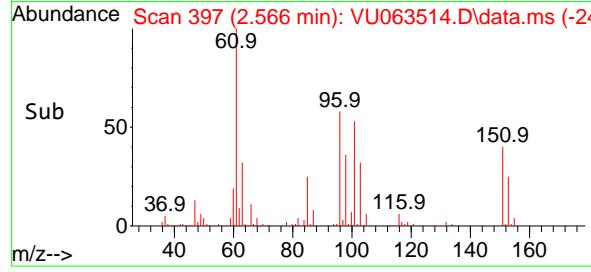


#10
Iodomethane
Concen: 4.500 ug/l
RT: 2.708 min Scan# 441
Delta R.T. -0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

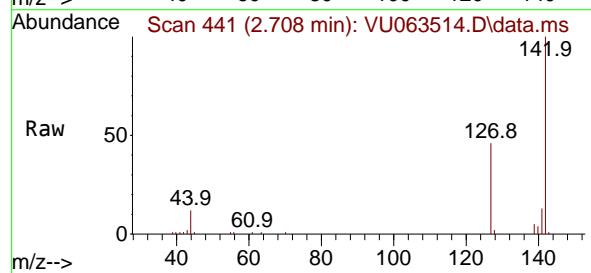

Tgt Ion:142 Resp: 39902
Ion Ratio Lower Upper
142 100
127 47.8 37.9 56.9

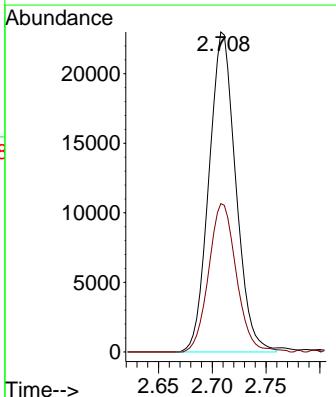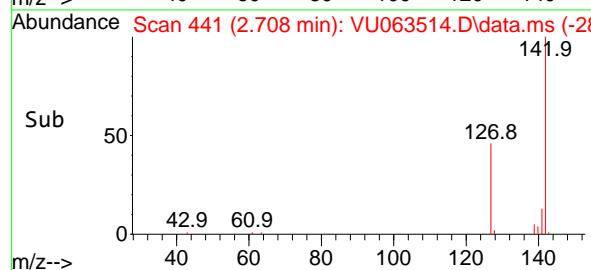

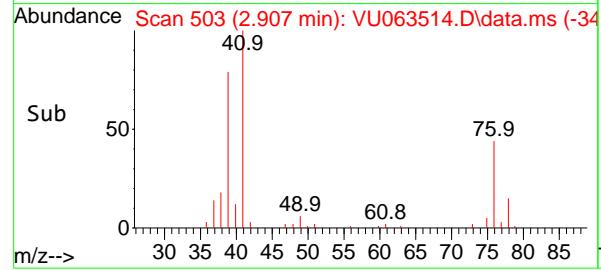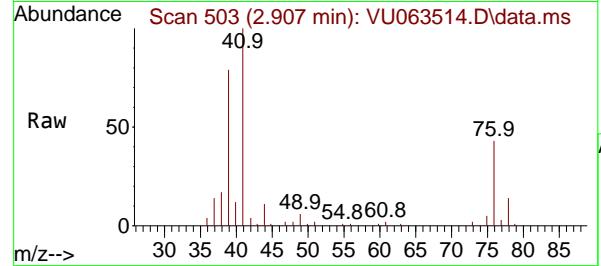

#11

Allyl Chloride

Concen: 4.791 ug/l

RT: 2.907 min Scan# 503

Delta R.T. 0.000 min




Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U

ClientSampleId : VSTDICC005

**Manual Integrations
APPROVED**

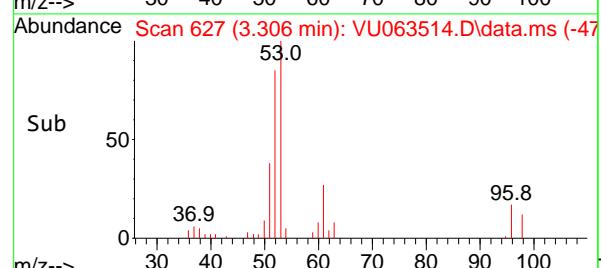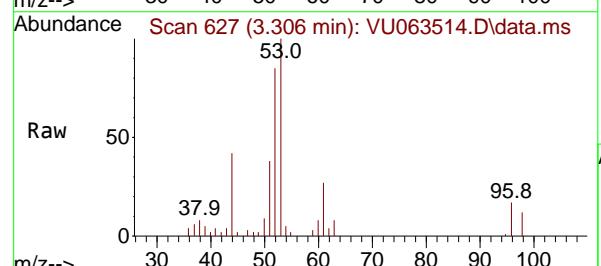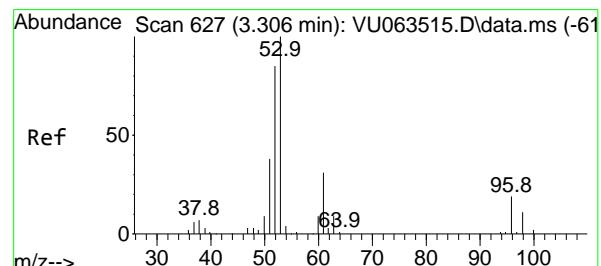 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#12

Acrylonitrile

Concen: 9.586 ug/l

RT: 3.306 min Scan# 627

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt Ion: 53 Resp: 16229


Ion Ratio Lower Upper


53 100

52 79.2 64.3 96.5



51 34.4 27.8 41.8

Abundance

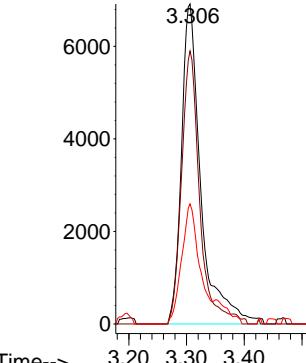




Abundance Scan 413 (2.618 min): VU063514.D\data.ms

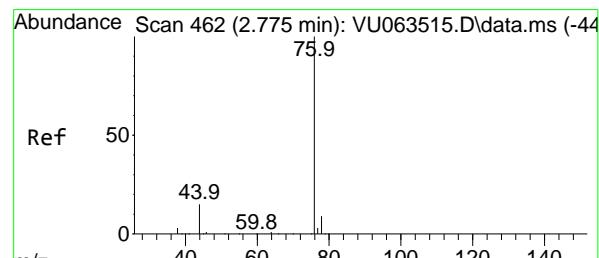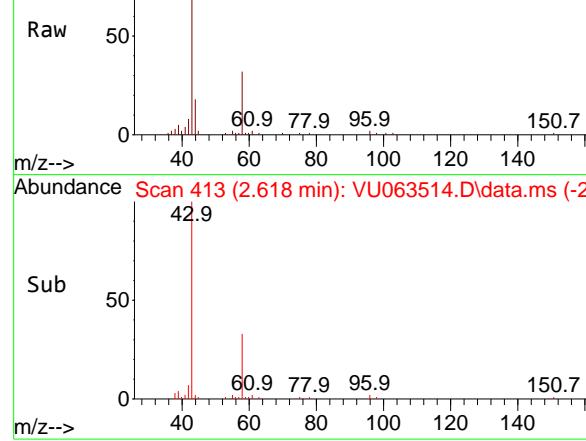

Abundance Scan 463 (2.779 min): VU063514.D\data.ms

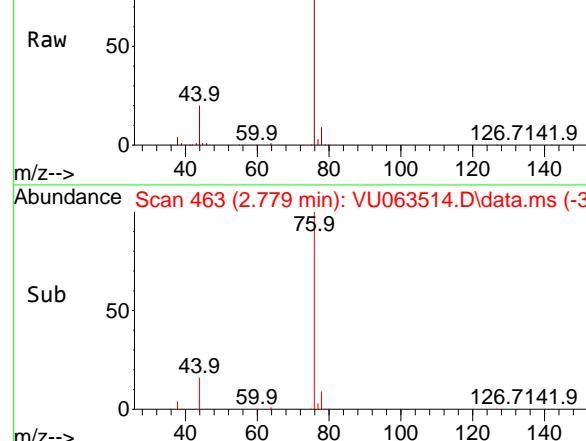

#13

Acetone

Concen: 21.677 ug/l

RT: 2.618 min Scan# 413


Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U

ClientSampleId : VSTDICC005

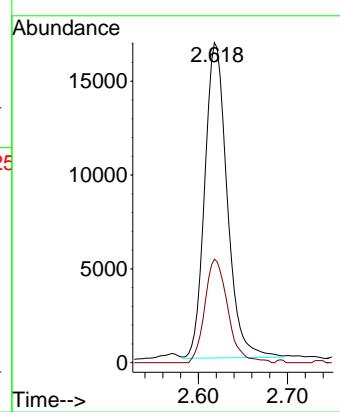**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#14

Carbon Disulfide


Concen: 4.885 ug/l




RT: 2.779 min Scan# 463

Delta R.T. 0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

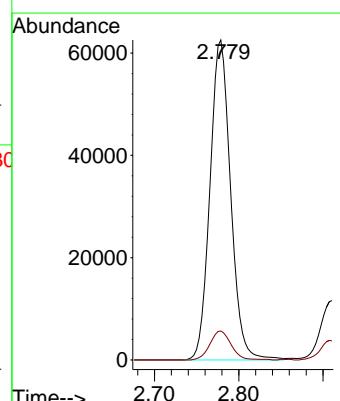Tgt Ion: 76 Resp: 106742
Ion Ratio Lower Upper
76 100
78 9.0 7.0 10.6

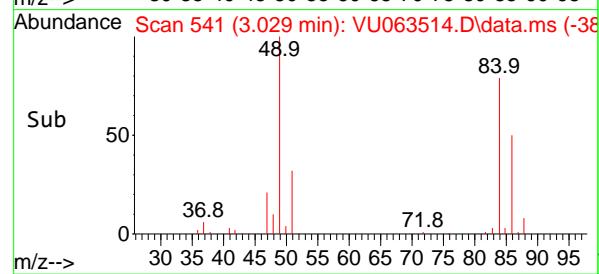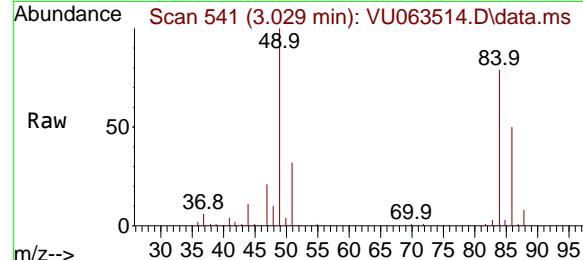

#15

Methylene Chloride

Concen: 4.742 ug/l

RT: 3.029 min Scan# 5

Delta R.T. 0.000 min

Lab File: VU063514.D




Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

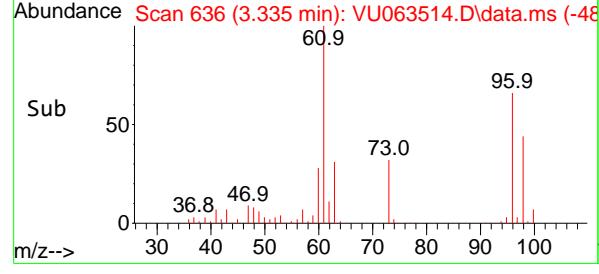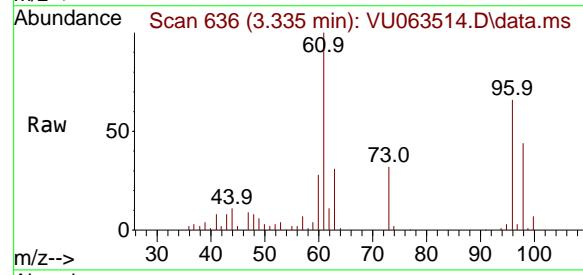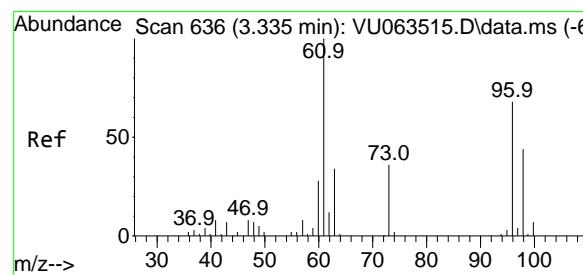 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#16

trans-1,2-Dichloroethene

Concen: 4.818 ug/l

RT: 3.335 min Scan# 636

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion: 96 Resp: 37017




Ion Ratio Lower Upper

96 100

61 152.1 117.2 175.8

98 67.3 51.4 77.2

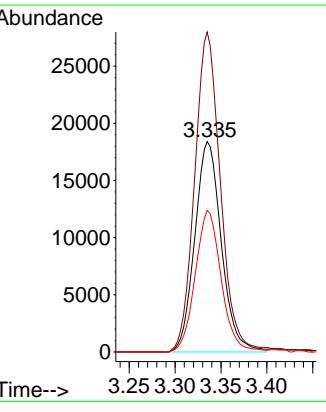



#17

1,1-Dichloroethane

Concen: 4.927 ug/l

RT: 3.849 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#18

2-Butanone

Concen: 23.049 ug/l

RT: 4.714 min Scan# 1065

Delta R.T. 0.003 min

Lab File: VU063514.D


Acq: 16 Jul 2025 11:00


Tgt Ion: 43 Resp: 48390

Ion Ratio Lower Upper

43 100

57 8.3 0.0 16.4

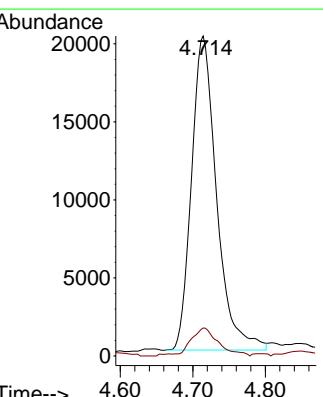



#19

Cyclohexane

Concen: 4.854 ug/l

RT: 5.361 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063514.D


Acq: 16 Jul 2025 11:00

Instrument:

MSVOA_U

ClientSampleId :



VSTDICC005

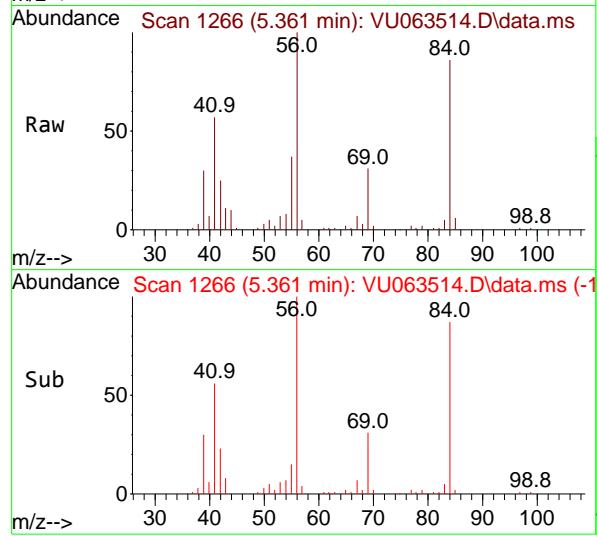

Tgt	Ion:	56	Ion	Ratio	Resp:	5852
		100				
		69	32.7	26.6	39.8	
		84	88.7	71.0	106.4	


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

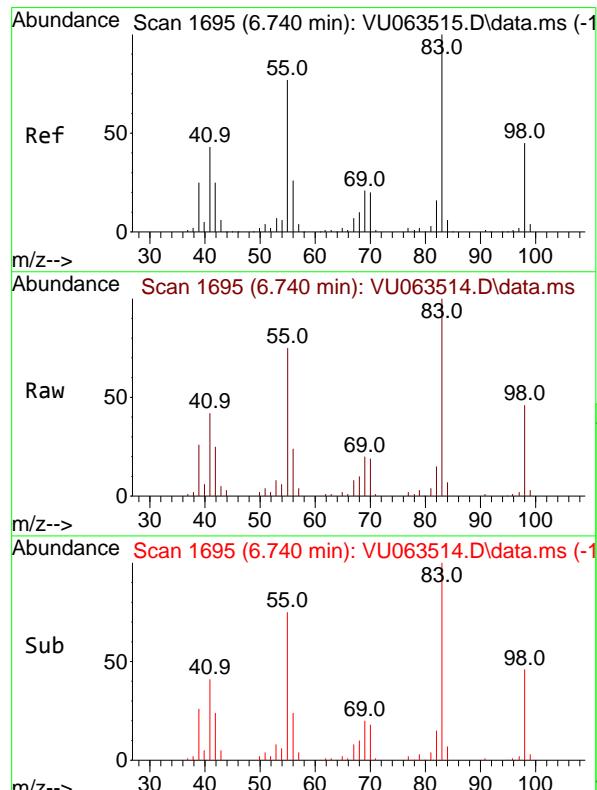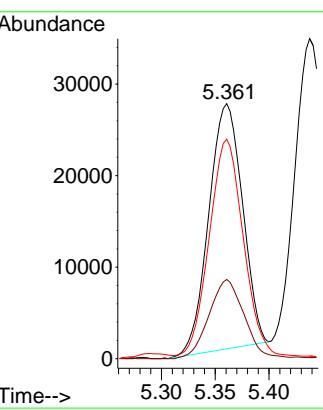

#20
Methylcyclohexane
Concen: 4.517 ug/l
RT: 6.740 min Scan# 1695
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Tgt	Ion:	83	Ion	Ratio	Resp:	52941
		100				
		55	74.8	60.6	90.8	
		98	46.5	35.8	53.8	

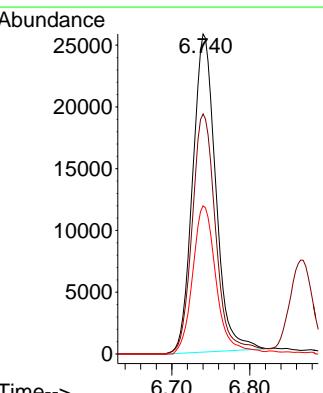

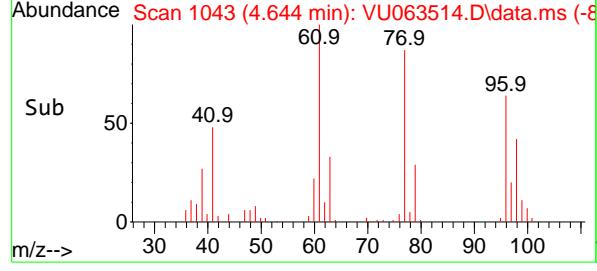

#21

2,2-Dichloropropane

Concen: 4.653 ug/l

RT: 4.644 min Scan# 1043

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

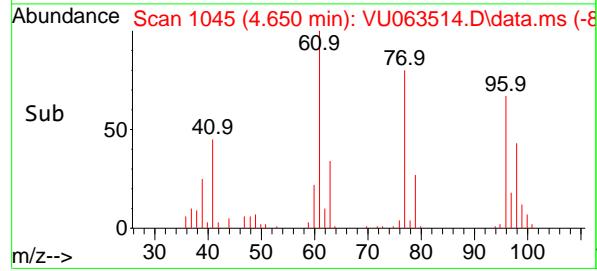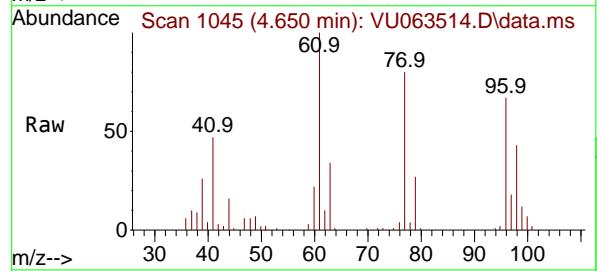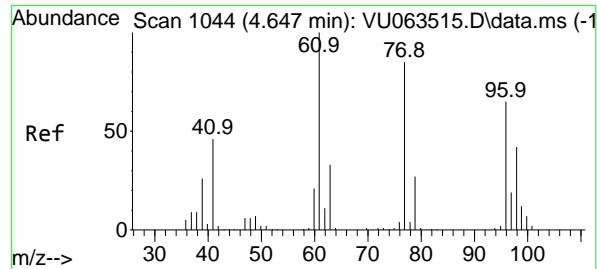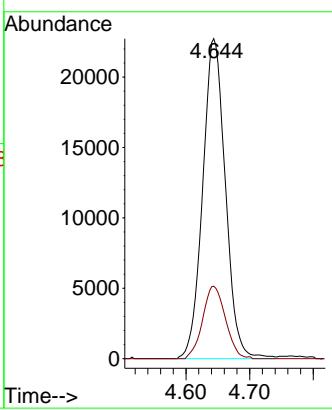 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#22

cis-1,2-Dichloroethene

Concen: 4.836 ug/l


RT: 4.650 min Scan# 1045







Delta R.T. 0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt	Ion	Resp:	
Ion	Ratio	Lower	Upper
96	100		
61	155.3	0.0	384.7
98	65.0	32.1	96.3

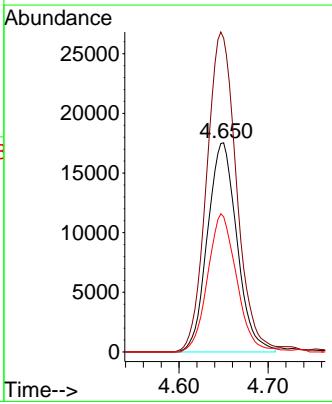

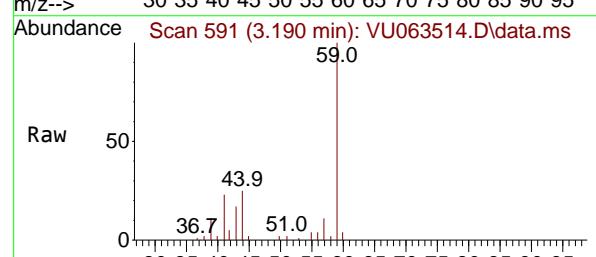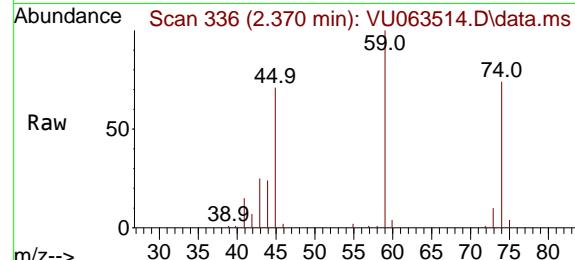

#23

Diethyl Ether

Concen: 5.030 ug/l

RT: 2.370 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument :

MSVOA_U


ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

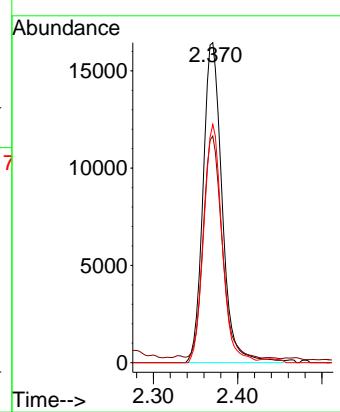

#24

tert-Butyl Alcohol

Concen: 47.503 ug/l


RT: 3.190 min Scan# 591


Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt Ion: 59 Resp: 29561
 Ion Ratio Lower Upper
 59 100
 57 11.0 8.6 12.8

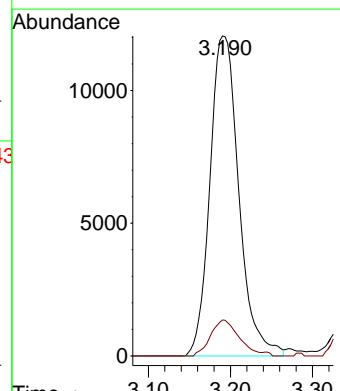

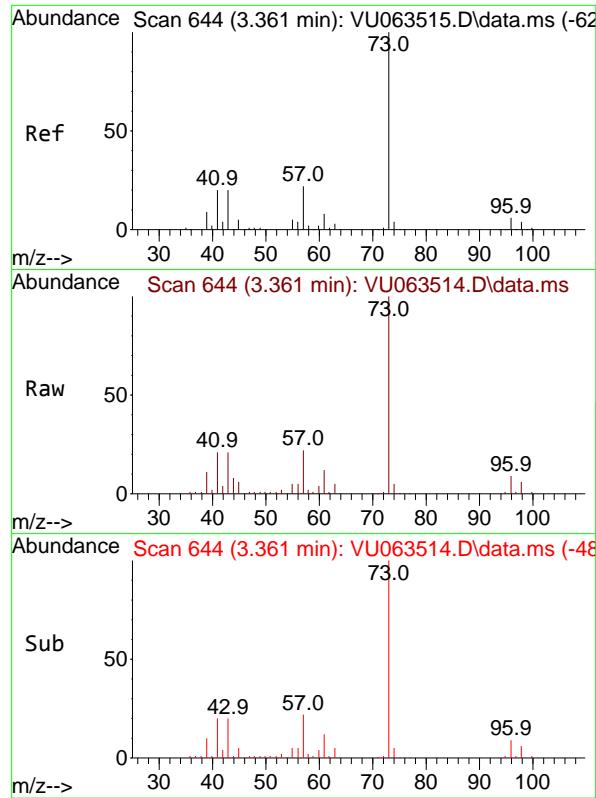



#25

Methyl tert-Butyl Ether
Concen: 4.911 ug/l
RT: 3.361 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U
ClientSampleId : VSTDICC005

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

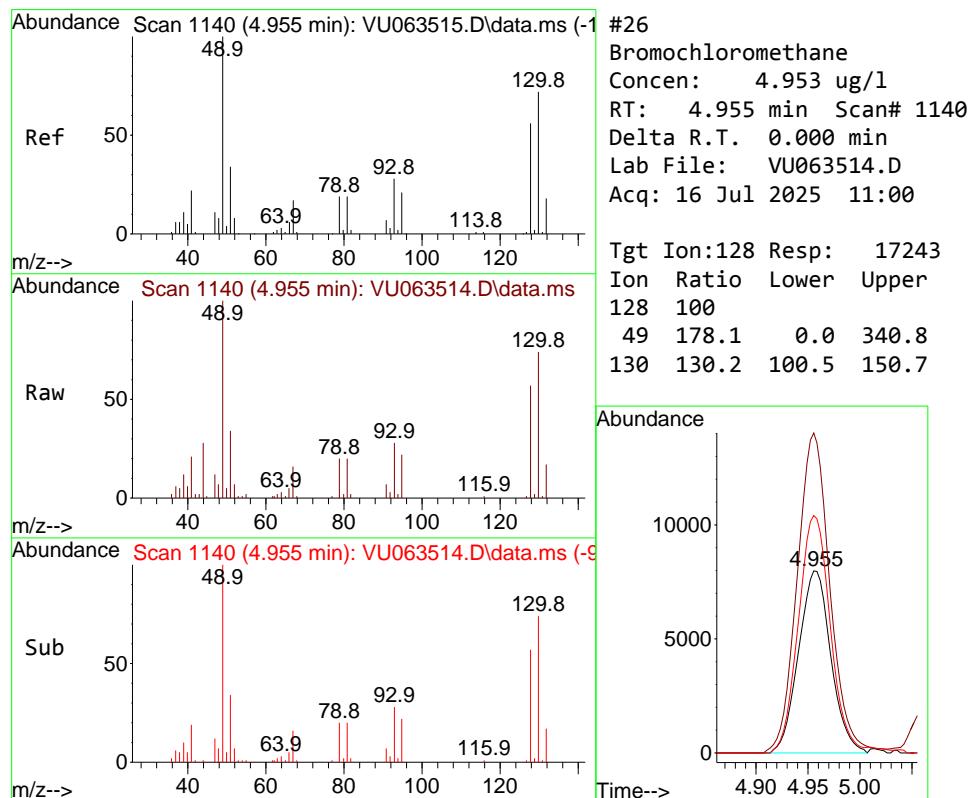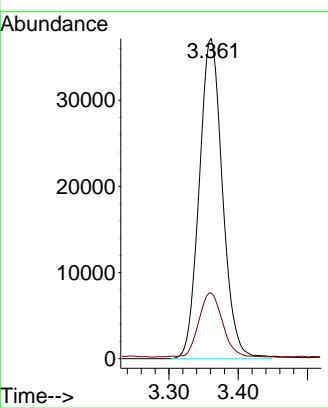


#26

Bromochloromethane
Concen: 4.953 ug/l
RT: 4.955 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00


Tgt Ion:128 Resp: 17243
Ion Ratio Lower Upper
128 100
49 178.1 0.0 340.8
130 130.2 100.5 150.7

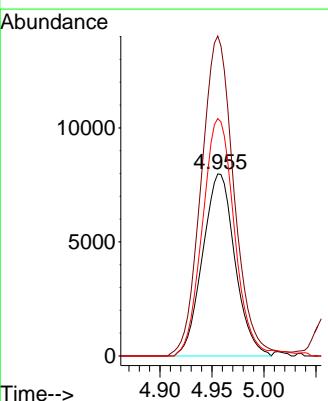



#27
 Chloroform
 Concen: 4.868 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063514.D
 Acq: 16 Jul 2025 11:00




Instrument : MSVOA_U
 ClientSampleId : VSTDICC005




Tgt Ion: 83 Resp: 70739
 Ion Ratio Lower Upper
 83 100
 85 64.9 0.0 130.0

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

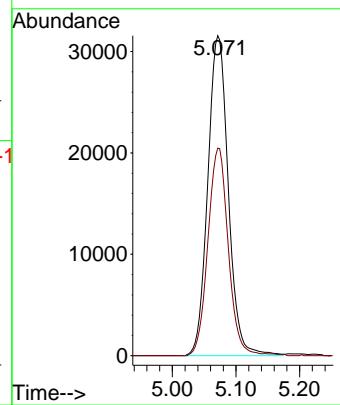


#28
 1,1,1-Trichloroethane
 Concen: 4.974 ug/l
 RT: 5.293 min Scan# 1245
 Delta R.T. -0.003 min
 Lab File: VU063514.D
 Acq: 16 Jul 2025 11:00

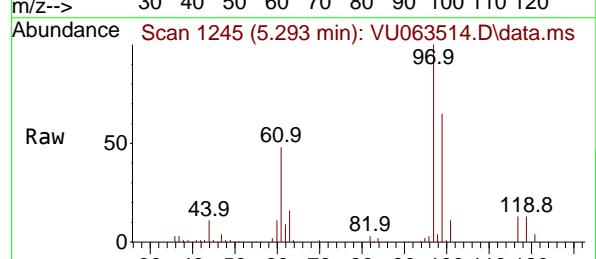

Tgt Ion: 97 Resp: 61347
 Ion Ratio Lower Upper
 97 100
 99 63.9 31.8 95.3
 61 48.0 23.3 69.9

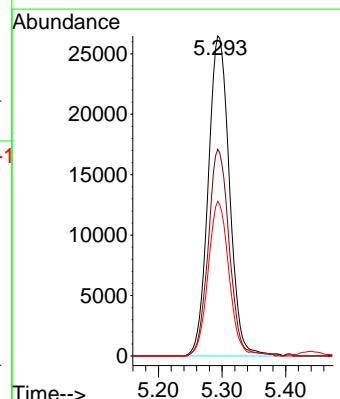

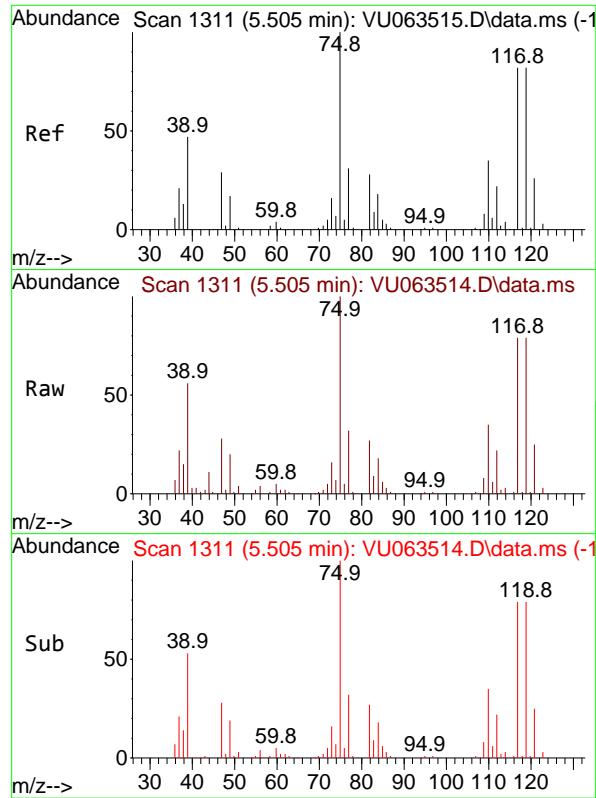

#29

1,1-Dichloropropene

Concen: 4.899 ug/l

RT: 5.505 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument:

MSVOA_U



ClientSampleId :

VSTDICC005

Tgt	Ion:	75	Ion	Ratio	55970
		100			
110		35.1	17.8		53.4
77		31.0	24.6		37.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

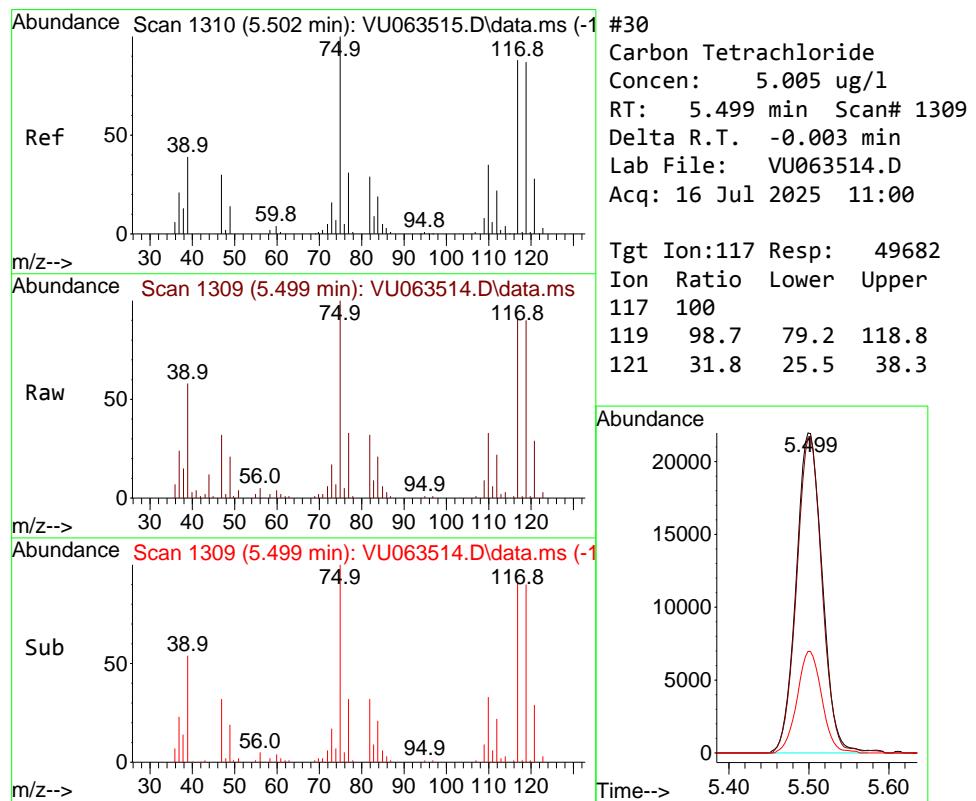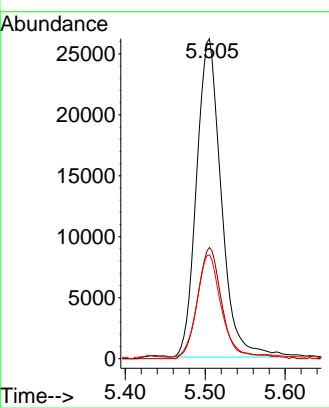

#30

Carbon Tetrachloride

Concen: 5.005 ug/l


RT: 5.499 min Scan# 1309


Delta R.T. -0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt	Ion:	117	Ion	Ratio	49682
		100			
119		98.7	79.2		118.8
121		31.8	25.5		38.3

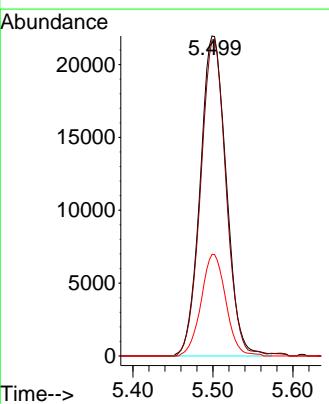



Ref 50
0

44.9 59.0 87.0 102.0

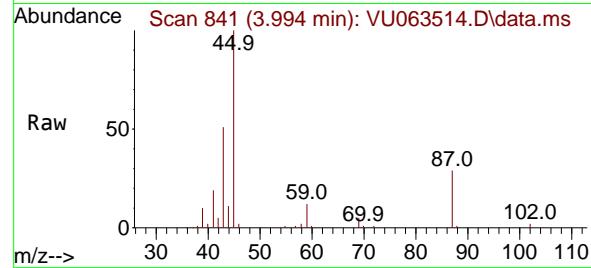

Raw 50
0

44.9 59.0 87.0 102.0

Abundance Scan 841 (3.994 min): VU063514.D\data.ms (-68)

Sub 50
0

44.9 59.0 87.0 102.0

m/z-->

Time-->

#31

Isopropyl Ether

Concen: 4.909 ug/l

RT: 3.994 min Scan# 8

Instrument:

Delta R.T. 0.003 min

MSVOA_U

Lab File: VU063514.D


ClientSampleId :

Acq: 16 Jul 2025 11:00

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




Ref 50
0

59.0 41.0 87.0 71.9

50.9

m/z-->

Time-->

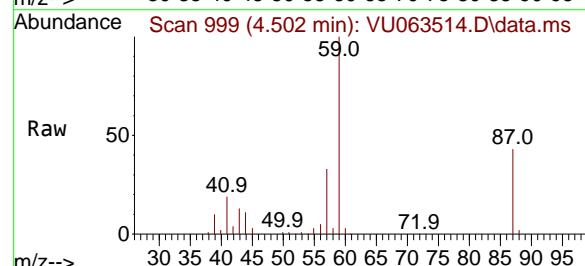


Raw 50
0

59.0 40.9 87.0 71.9

49.9

m/z-->

Time-->



Sub 50
0

59.0 40.9 87.0 71.9

50.9

m/z-->

Time-->

#32

Ethyl-t-butyl ether

Concen: 4.751 ug/l

RT: 4.502 min Scan# 999

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion: 59 Resp: 94505

Ion Ratio Lower Upper

59 100




87 41.5 32.6 49.0

Abundance Scan 999 (4.502 min): VU063514.D\data.ms (-84)

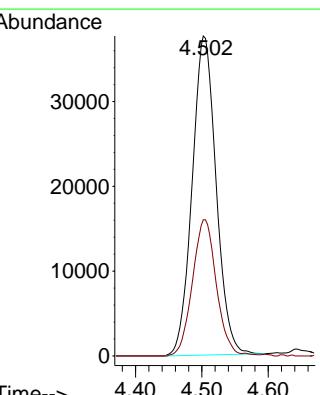

30000
20000
10000
0

4.502

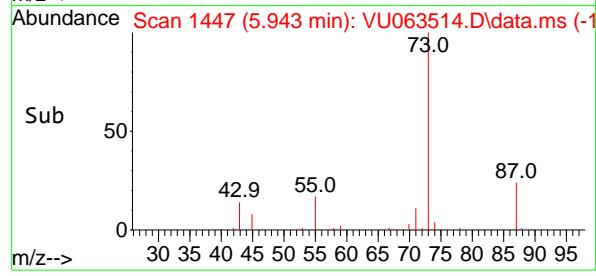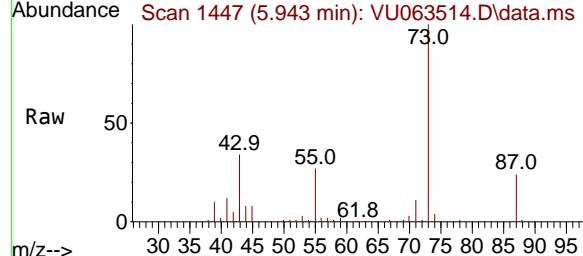

#33

Tert-Amyl methyl ether

Concen: 4.920 ug/l

RT: 5.943 min Scan# 1447

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

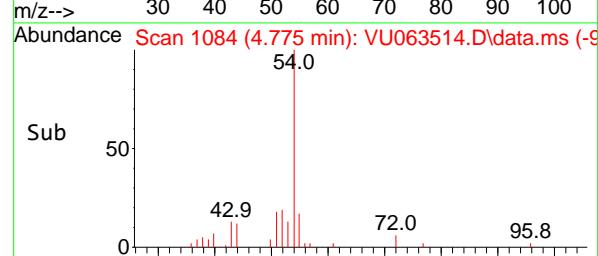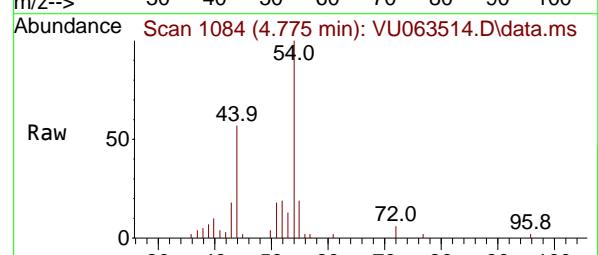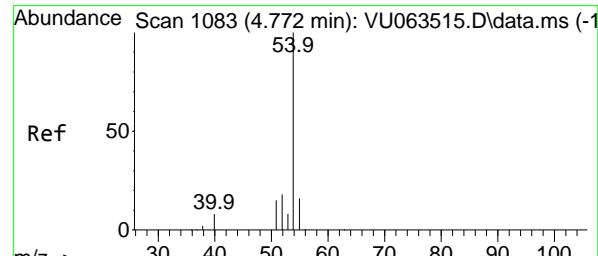 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#34

Propionitrile

Concen: 25.489 ug/l

RT: 4.775 min Scan# 1084

Delta R.T. 0.003 min


Lab File: VU063514.D


Acq: 16 Jul 2025 11:00

Tgt Ion: 54 Resp: 16304

Ion Ratio Lower Upper


	54	100
52	20.2	17.0
55	13.8	13.6
40	6.6	6.4

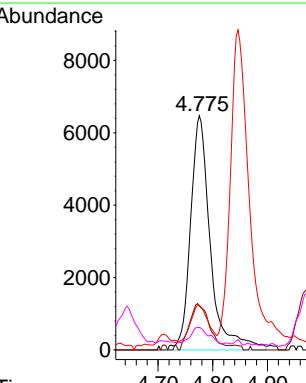



#35
Benzene
Concen: 5.113 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00




Instrument : MSVOA_U
ClientSampleId : VSTDICC005




Tgt Ion: 78 Resp: 156970
Ion Ratio Lower Upper
78 100
77 22.5 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#36
1,2-Dichloroethane
Concen: 5.065 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00




Tgt Ion: 62 Resp: 48312
Ion Ratio Lower Upper
62 100
98 8.2 6.4 9.6

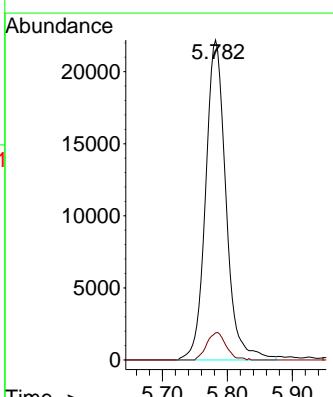



#37
Trichloroethene
Concen: 4.506 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00




Instrument : MSVOA_U
ClientSampleId : VSTDICC005




Tgt Ion:130 Resp: 35295
Ion Ratio Lower Upper
130 100
95 106.3 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


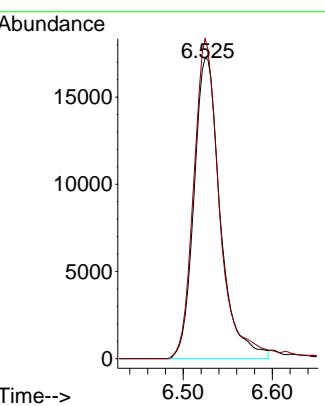



#38
1,2-Dichloropropane
Concen: 4.678 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00



Tgt Ion: 63 Resp: 33611
Ion Ratio Lower Upper
63 100
65 29.9 24.6 36.8

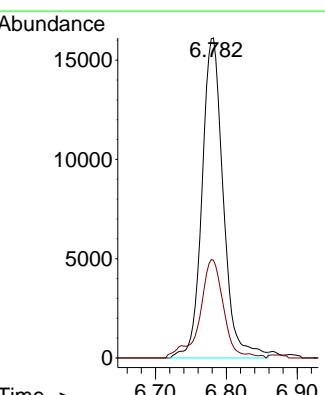



#39

Methacrylonitrile

Concen: 4.468 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument:

MSVOA_U





ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

 Tgt Ion: 41 Resp: 12541
 Ion Ratio Lower Upper

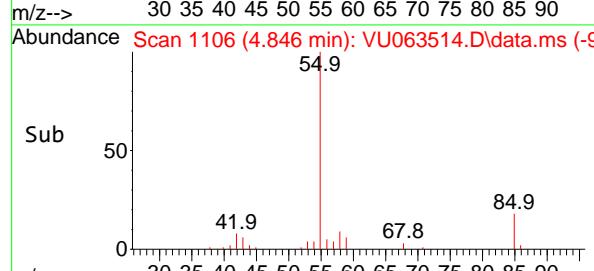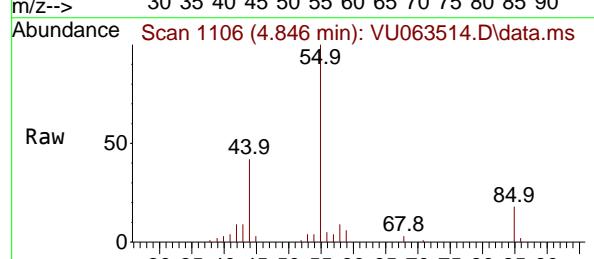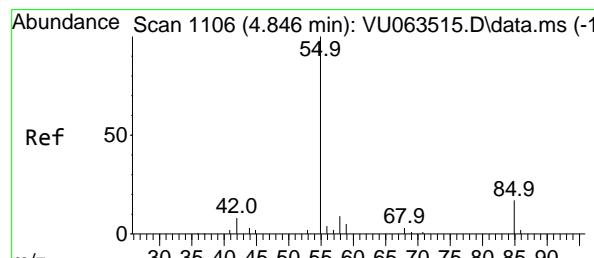 41 100
 67 82.1 62.7 94.1
 39 57.1 43.1 64.7
 52 34.9 27.4 41.0


#40

Methyl acrylate

Concen: 4.749 ug/l


RT: 4.846 min Scan# 1106


Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt Ion: 55 Resp: 19739

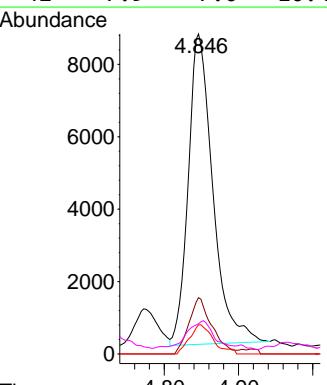 Ion Ratio Lower Upper
 55 100
 85 16.8 12.8 19.2
 58 9.0 7.0 10.4
 42 7.9 7.0 10.4




#41

Tetrahydrofuran



Concen: 8.771 ug/l

RT: 5.058 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063514.D



Acq: 16 Jul 2025 11:00

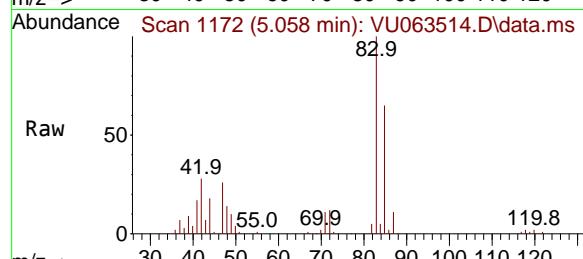



Tgt	Ion:	42	Ion Ratio	100	Resp:	13119
		72		49.2	Lower	39.2
		71		42.8	Upper	58.8

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#42
1-Chlorobutane
Concen: 4.999 ug/l
RT: 5.438 min Scan# 1290
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

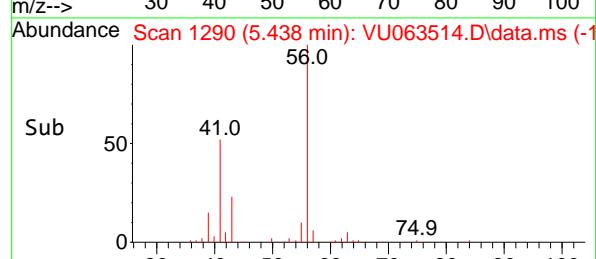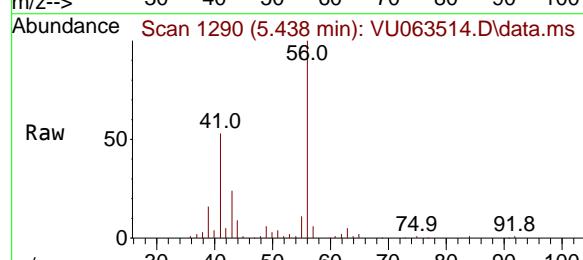


Tgt	Ion:	56	Ion Ratio	100	Resp:	75929
		41		48.2	Lower	26.7

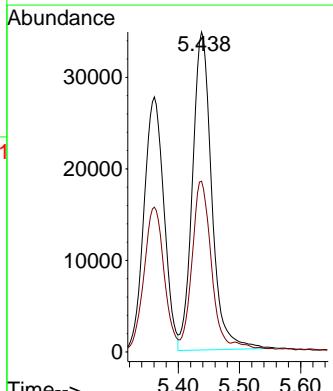



#43
Dibromomethane
Concen: 4.821 ug/l
RT: 6.907 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00




Instrument : MSVOA_U
ClientSampleId : VSTDICC005




Tgt Ion: 93 Resp: 1794
Ion Ratio Lower Upper
93 100
95 83.0 67.9 101.9
174 85.0 74.6 111.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

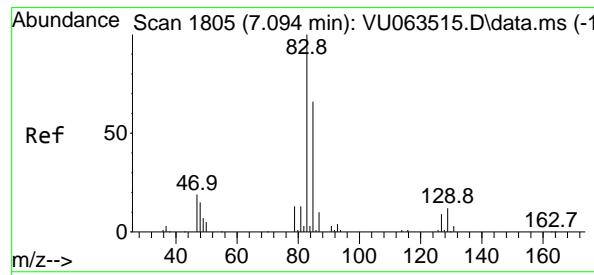
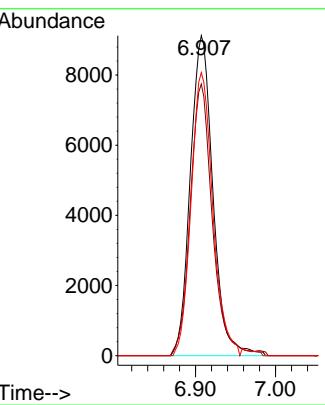
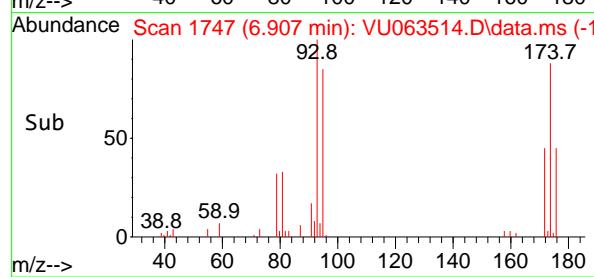


#44
Bromodichloromethane
Concen: 4.807 ug/l
RT: 7.094 min Scan# 1805
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00



Tgt Ion: 83 Resp: 40349
Ion Ratio Lower Upper
83 100
85 67.3 52.7 79.1
127 8.6 8.1 12.1

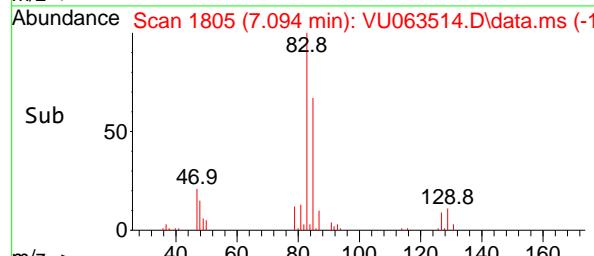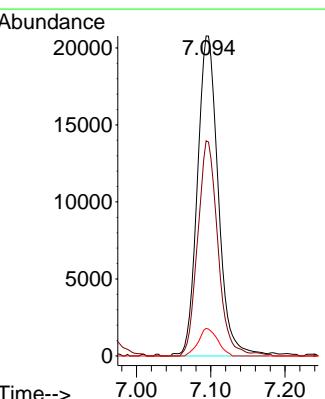



#45

4-Methyl-2-Pentanone

Concen: 24.821 ug/l

RT: 7.798 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#46

t-1,4-Dichloro-2-butene

Concen: 9.823 ug/l

RT: 10.823 min Scan# 2965

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt Ion: 75 Resp: 13369


Ion Ratio Lower Upper


75 100

53 61.7 48.4 72.6

89 37.5 30.6 45.8

88 30.4 25.3 37.9

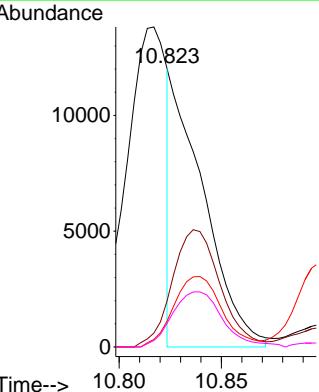

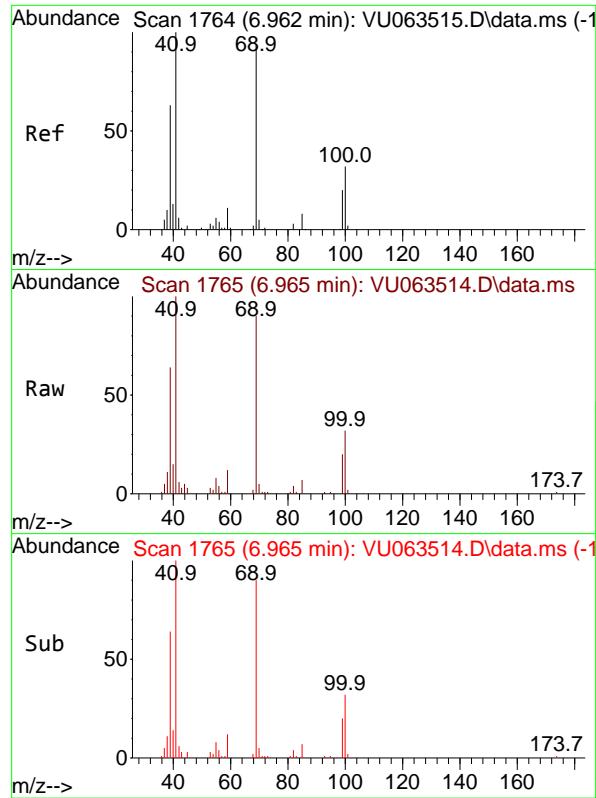

#47

Methyl methacrylate

Concen: 9.775 ug/l

RT: 6.965 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument :

MSVOA_U



ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

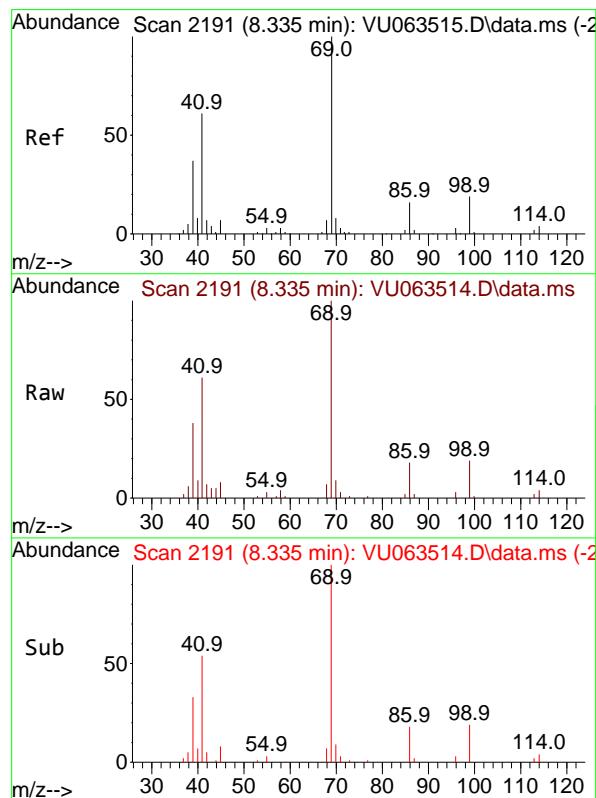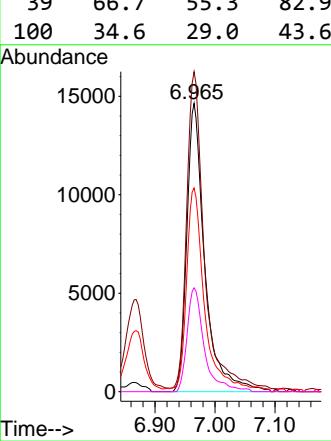

#48

Ethyl methacrylate

Concen: 4.943 ug/l

RT: 8.335 min Scan# 2191


Delta R.T. 0.000 min


Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt Ion: 69 Resp: 29487



Ion	Ratio	Lower	Upper
69	100		
41	65.3	30.8	92.4

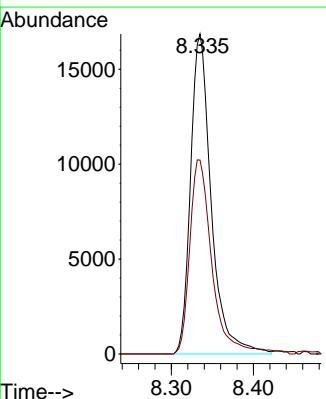



#49
Toluene
Concen: 4.993 ug/l
RT: 7.959 min Scan# 2150
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00



Instrument: MSVOA_U
ClientSampleId: VSTDICC005




Tgt Ion: 92 Resp: 8368
Ion Ratio Lower Upper
92 100
91 175.3 140.4 210.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

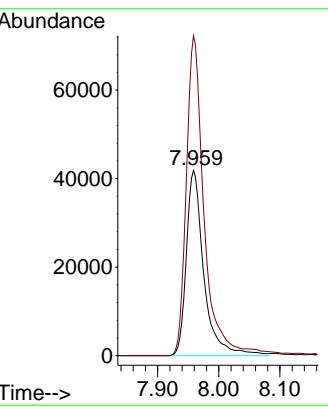


#50
t-1,3-Dichloropropene
Concen: 4.946 ug/l
RT: 8.206 min Scan# 2151
Delta R.T. 0.003 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00





Tgt Ion: 75 Resp: 32573
Ion Ratio Lower Upper
75 100
77 32.5 24.9 37.3

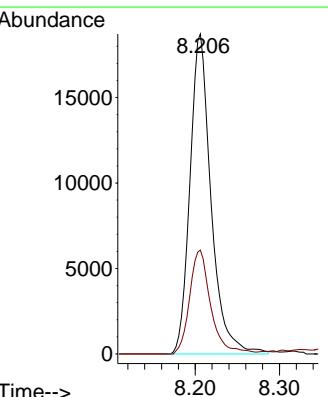



#51
cis-1,3-Dichloropropene
 Concen: 4.923 ug/l
 RT: 7.602 min Scan# 1
 Delta R.T. 0.003 min
 Lab File: VU063514.D
 Acq: 16 Jul 2025 11:00



Instrument : MSVOA_U
 ClientSampleId : VSTDICC005




Tgt Ion: 75 Resp: 4351
 Ion Ratio Lower Upper
 75 100
 77 31.3 25.1 37.7
 39 46.0 37.8 56.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025



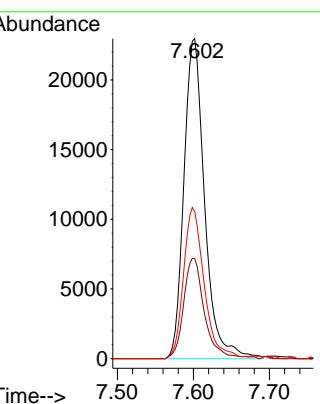


#52
 1,1,2-Trichloroethane
 Concen: 4.976 ug/l
 RT: 8.393 min Scan# 2209
 Delta R.T. 0.000 min
 Lab File: VU063514.D
 Acq: 16 Jul 2025 11:00



Tgt Ion: 97 Resp: 24935
 Ion Ratio Lower Upper
 97 100
 83 85.9 70.2 105.2
 85 54.1 45.2 67.8
 99 63.2 50.1 75.1

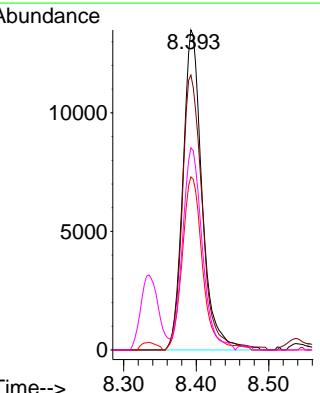

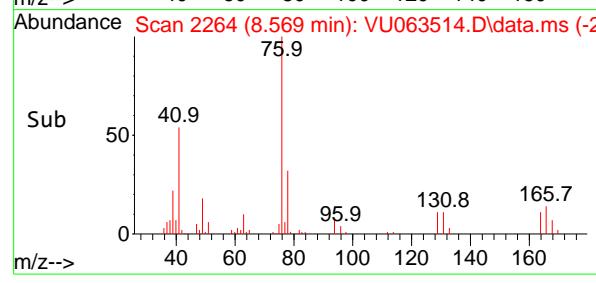

#53

1,3-Dichloropropane

Concen: 4.964 ug/l

RT: 8.569 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

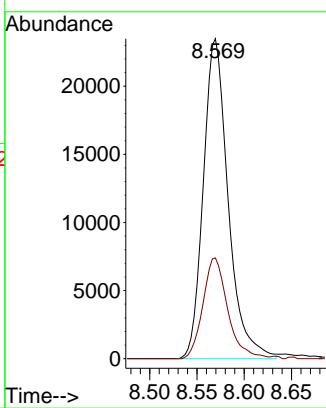 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#54

2-Hexanone


Concen: 24.583 ug/l




RT: 8.688 min Scan# 2301

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

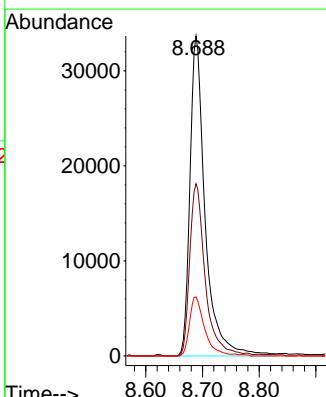 Tgt Ion: 43 Resp: 62636
 Ion Ratio Lower Upper
 43 100
 58 54.7 34.8 74.8
 57 18.2 0.0 39.5

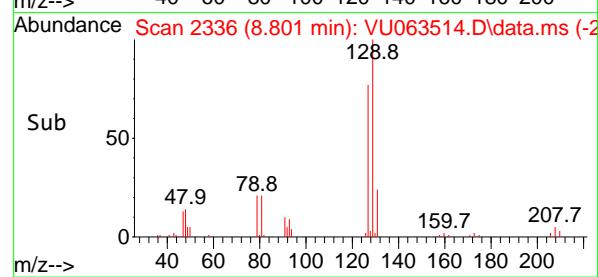


#55

Dibromochloromethane

Concen: 5.067 ug/l

RT: 8.801 min Scan# 2336

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

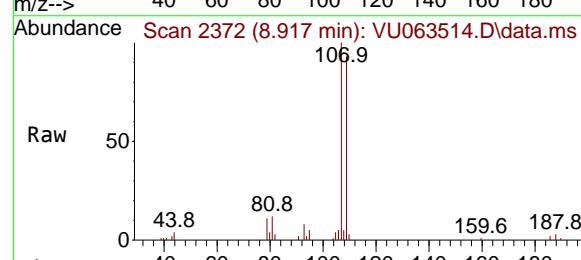

#56

1,2-Dibromoethane

Concen: 4.971 ug/l

RT: 8.917 min Scan# 2372

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt Ion:107 Resp: 22293

Ion Ratio Lower Upper


107 100




109 93.3 0.0 186.4

Abundance

Time-->

8.75 8.80 8.85

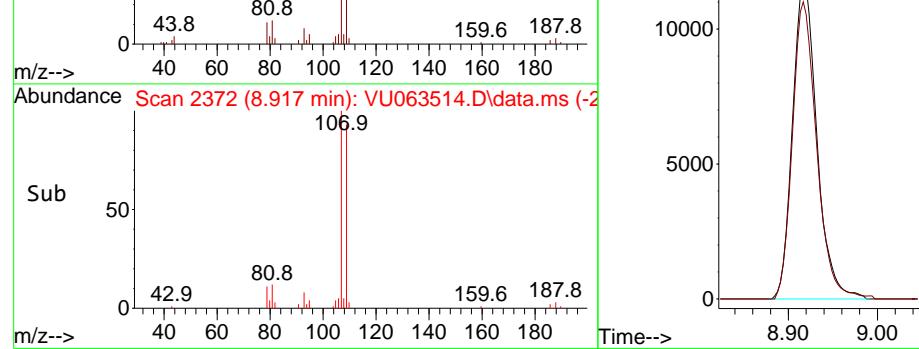



#57

4-Bromofluorobenzene

Concen: 0.953 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC005

Manual Integrations
APPROVED

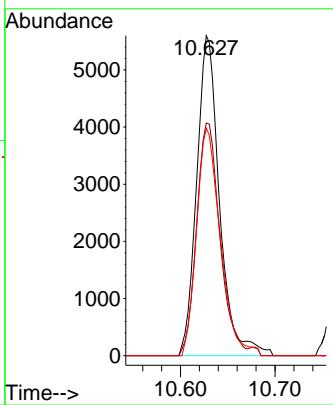 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#58

Tetrachloroethene

Concen: 4.909 ug/l


RT: 8.544 min Scan# 2256




Delta R.T. 0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Tgt	Ion:164	Resp:	35190
Ion	Ratio	Lower	Upper
164	100		
166	128.5	100.7	151.1
129	103.5	80.6	120.8
131	98.9	77.3	115.9

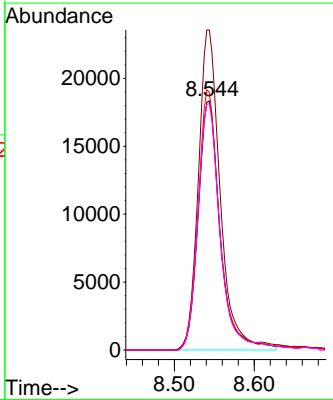



#59

Chlorobenzene

Concen: 4.955 ug/l

RT: 9.441 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

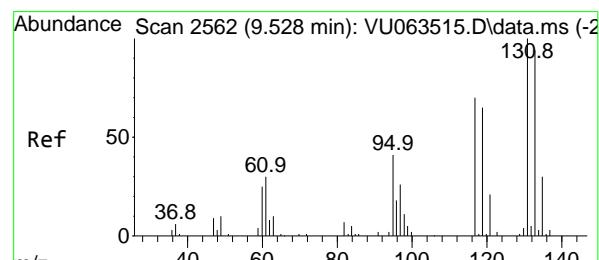 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#60

1,1,1,2-Tetrachloroethane

Concen: 4.901 ug/l

RT: 9.524 min Scan# 2561

Delta R.T. -0.003 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion:131 Resp: 30337




Ion Ratio Lower Upper

131 100

133 96.2 74.7 112.1

119 66.6 53.0 79.4

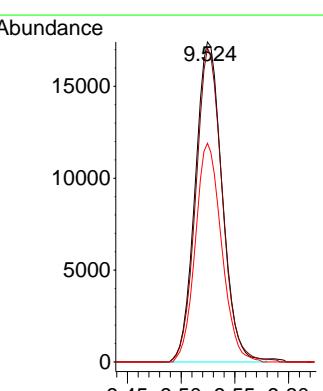

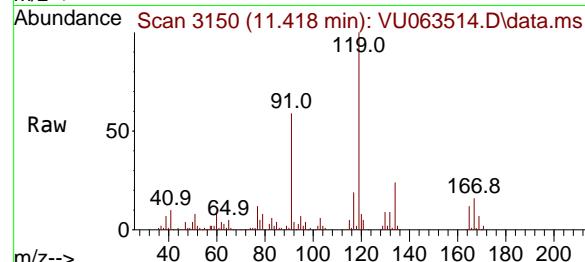

#61

Pentachloroethane

Concen: 5.020 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument :

MSVOA_U




ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**


Reviewed By :Mahesh Dadoda 07/17/2025







Supervised By :Semsettin Yesilyurt 07/17/2025

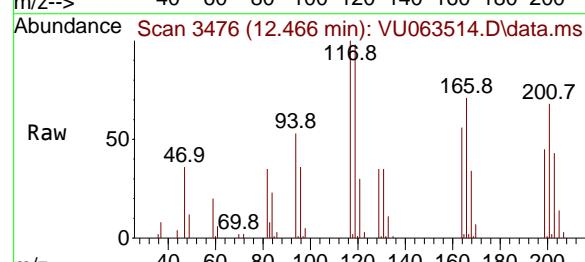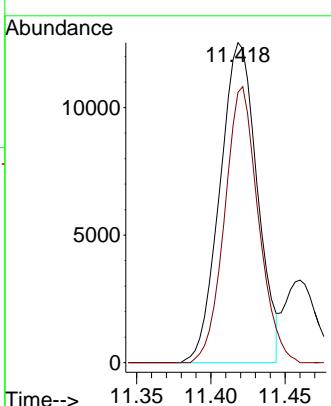

#62
Hexachloroethane
Concen: 5.110 ug/l
RT: 12.466 min Scan# 3476
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Tgt Ion:117 Resp: 22137
Ion Ratio Lower Upper
117 100
201 69.3 57.4 86.0

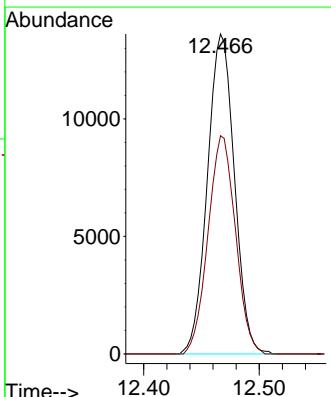



#63

Ethyl Benzene

Concen: 4.951 ug/l

RT: 9.563 min Scan# 2

Instrument:

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063514.D

ClientSampleId :

Acq: 16 Jul 2025 11:00

VSTDICC005

Tgt Ion: 91 Resp: 163990

Ion Ratio Lower Upper

91 100


106 31.1 25.4 38.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

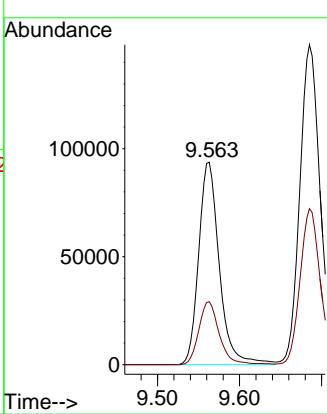

#64

m/p-Xylenes

Concen: 9.878 ug/l

RT: 9.685 min Scan# 2611

Delta R.T. 0.000 min

Lab File: VU063514.D


Acq: 16 Jul 2025 11:00


Tgt Ion: 106 Resp: 127196

Ion Ratio Lower Upper

106 100

91 207.3 163.6 245.4

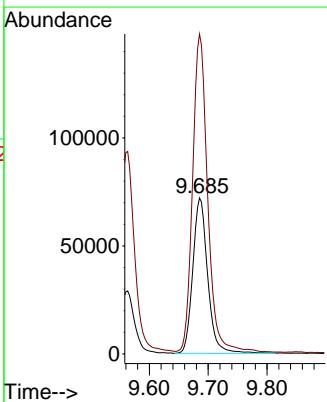


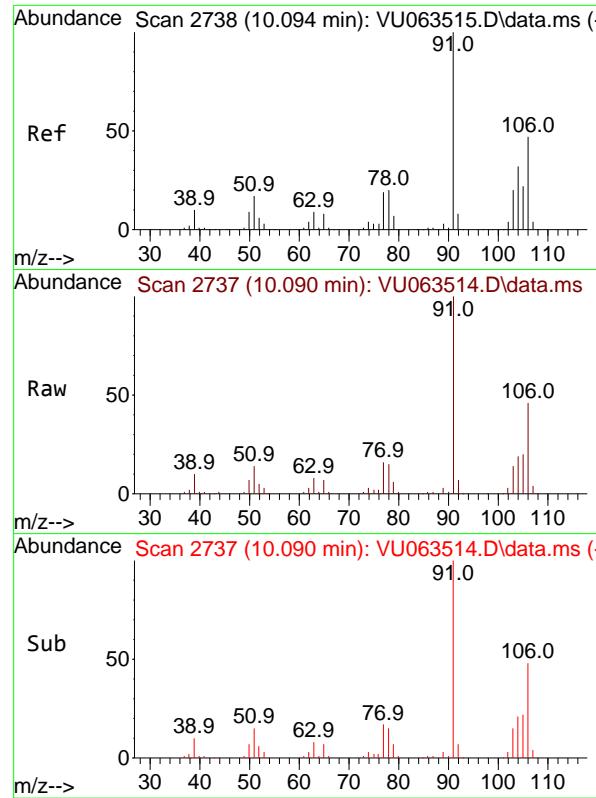


#65
o-Xylene
Concen: 4.982 ug/l
RT: 10.090 min Scan# 2
Delta R.T. -0.003 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U
ClientSampleId : VSTDICC005


Manual Integrations
APPROVED







Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

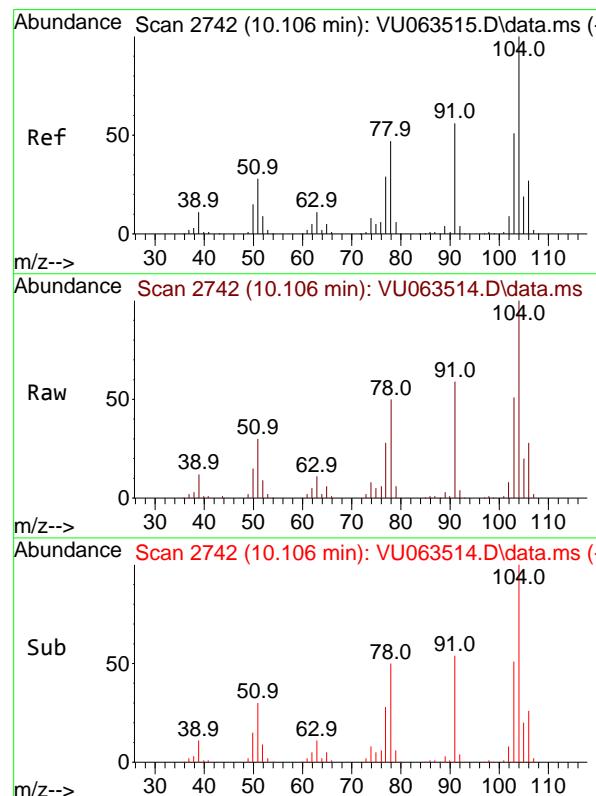

#66
Styrene
Concen: 5.046 ug/l
RT: 10.106 min Scan# 2742
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Tgt Ion:104 Resp: 99507
Ion Ratio Lower Upper
104 100
78 53.2 41.3 61.9
103 55.4 43.6 65.4





#67

Bromoform

Concen: 5.030 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Instrument :

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

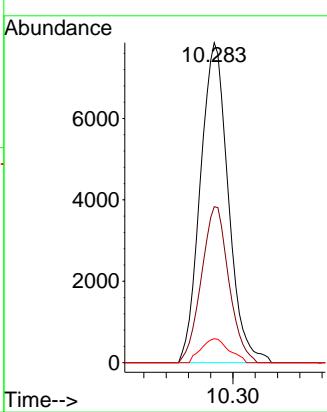 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#68

1,2-Dichlorobenzene-d4

Concen: 0.978 ug/l

RT: 12.187 min Scan# 3389

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion:152 Resp: 8923




Ion Ratio Lower Upper

152 100

115 100.6 0.0 262.2

150 234.6 0.0 651.2



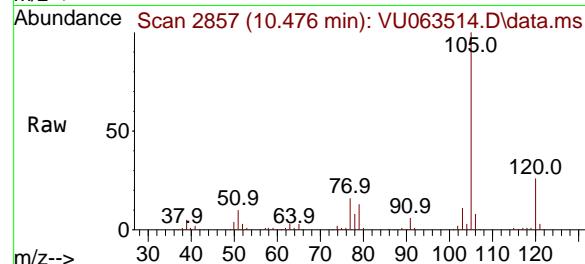

#69

Isopropylbenzene

Concen: 5.002 ug/l

RT: 10.476 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument :

MSVOA_U




ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 4.906 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion: 83 Resp: 29913

Ion Ratio Lower Upper




83 100

131 10.0 8.4 12.6

85 64.1 51.9 77.9

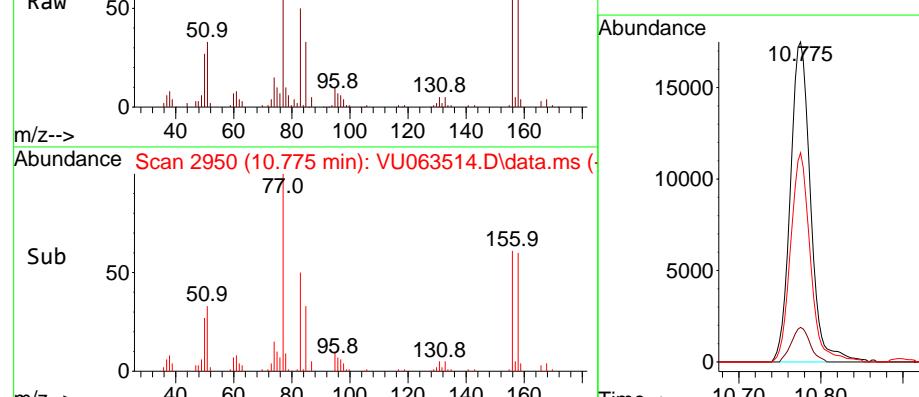

10.775



#71

1,2,3-Trichloropropane

Concen: 4.645 ug/l m

RT: 10.817 min Scan# 2963

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#72

Bromobenzene

Concen: 4.941 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion:156 Resp: 38144


Ion Ratio Lower Upper

156 100



77 156.6 0.0 315.2

158 95.5 0.0 195.4

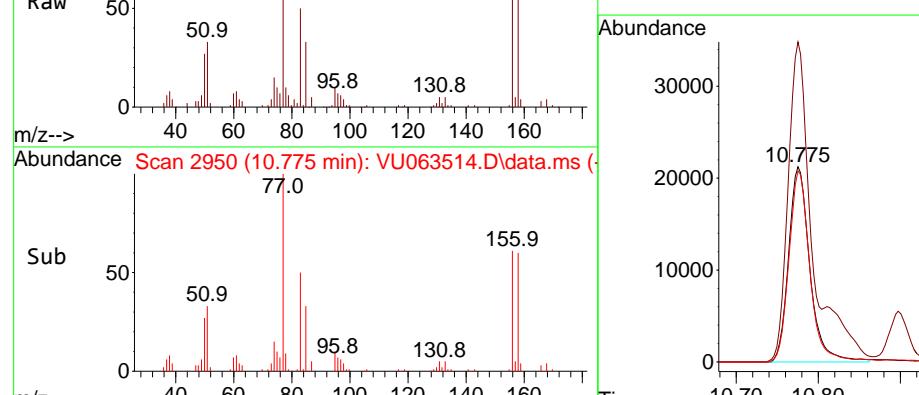




Abundance Scan 2988 (10.897 min): VU063514.D\data.ms (-)

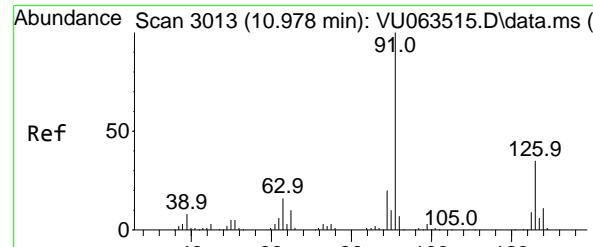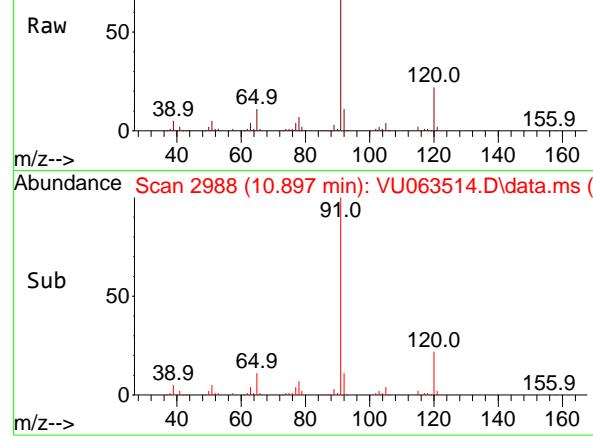

Abundance Scan 3013 (10.978 min): VU063514.D\data.ms (-)

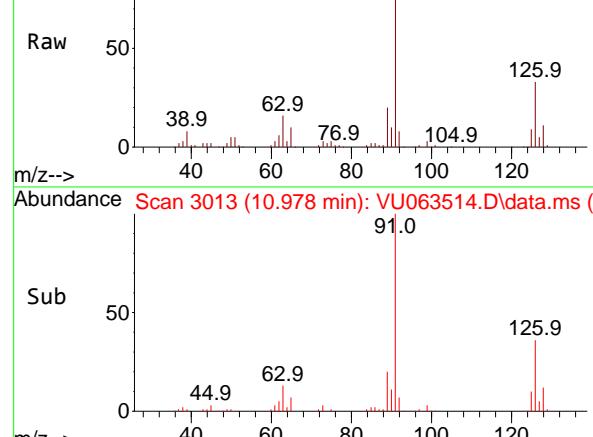

Abundance Scan 3013 (10.978 min): VU063514.D\data.ms (-)

#73

n-propylbenzene

Concen: 4.978 ug/l

RT: 10.897 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC005

Tgt Ion:120 Resp: 4482

Ion Ratio Lower Upper


120 100

91 438.5 343.1 514.7

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#74

2-Chlorotoluene

Concen: 4.932 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063514.D


Acq: 16 Jul 2025 11:00


Tgt Ion:126 Resp: 39249

Ion Ratio Lower Upper

126 100


91 292.1 0.0 606.0

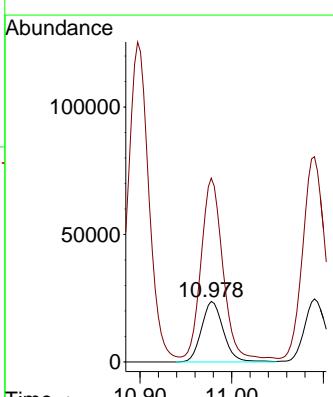

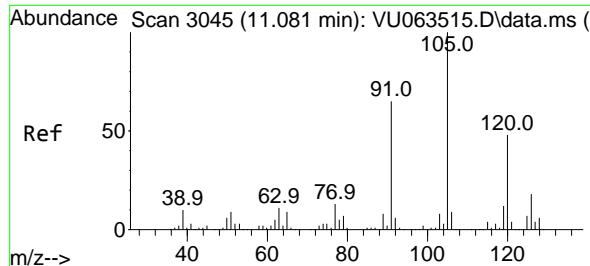

#75
1,3,5-Trimethylbenzene
Concen: 5.025 ug/l
RT: 11.081 min Scan#
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00




Instrument :
MSVOA_U
ClientSampleId :
VSTDICC005

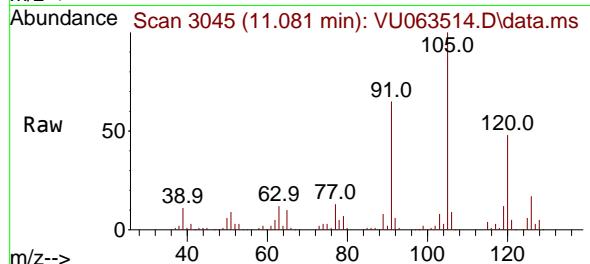


Tgt	Ion:105	Resp:	14359
Ion	Ratio	Lower	Upper
105	100		
120	47.5	37.8	56.8

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

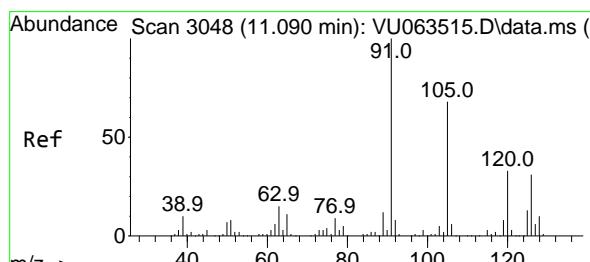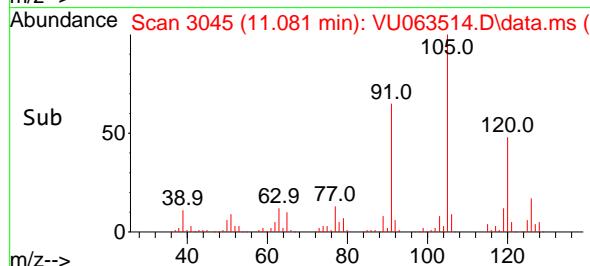



#76
4-Chlorotoluene
Concen: 5.014 ug/l
RT: 11.090 min Scan# 3048
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00



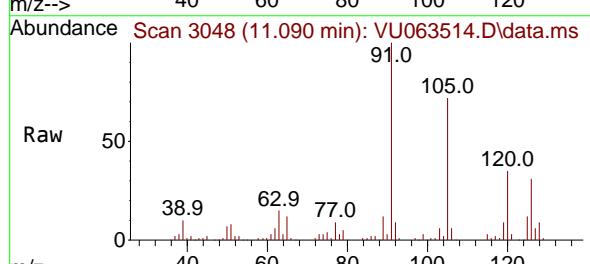


```

Tgt Ion:126 Resp: 40518
Ion Ratio Lower Upper
126 100
 91 341.9    0.0 682.2

```

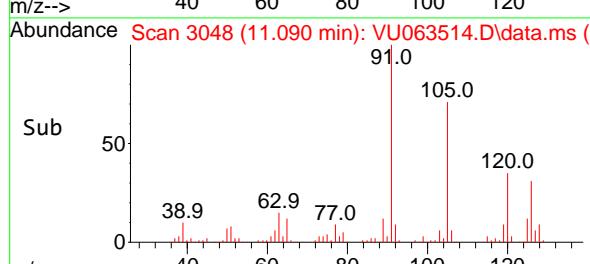



#77

tert-Butylbenzene

Concen: 4.970 ug/l

RT: 11.412 min Scan# 3148

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00





Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

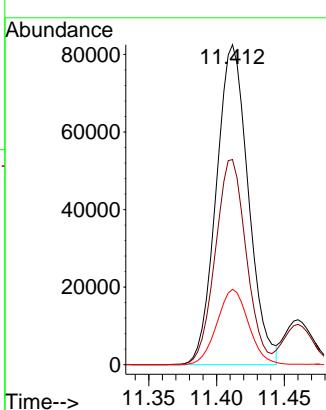 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#78

1,2,4-Trimethylbenzene


Concen: 5.038 ug/l




RT: 11.460 min Scan# 3163

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

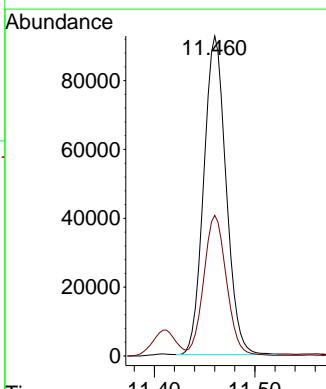 Tgt Ion:105 Resp: 142811
 Ion Ratio Lower Upper
 105 100
 120 44.8 22.7 68.0




#79

sec-Butylbenzene

Concen: 5.015 ug/l

RT: 11.634 min Scan# 3217

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#80

Nitrobenzene

Concen: 23.955 ug/l

RT: 13.206 min Scan# 3706

Delta R.T. 0.003 min

Lab File: VU063514.D



Acq: 16 Jul 2025 11:00

Tgt Ion: 77 Resp: 2721

Ion Ratio Lower Upper

77	100
123	39.0
65	6.5

#

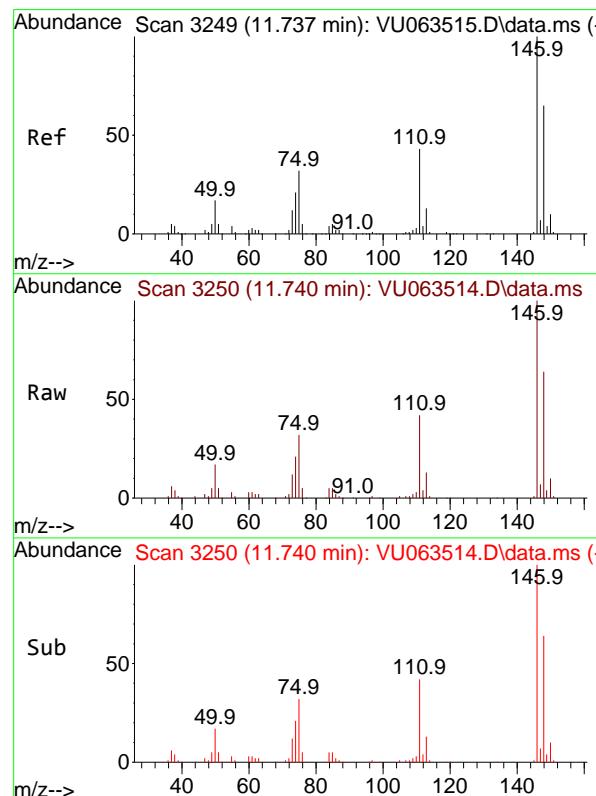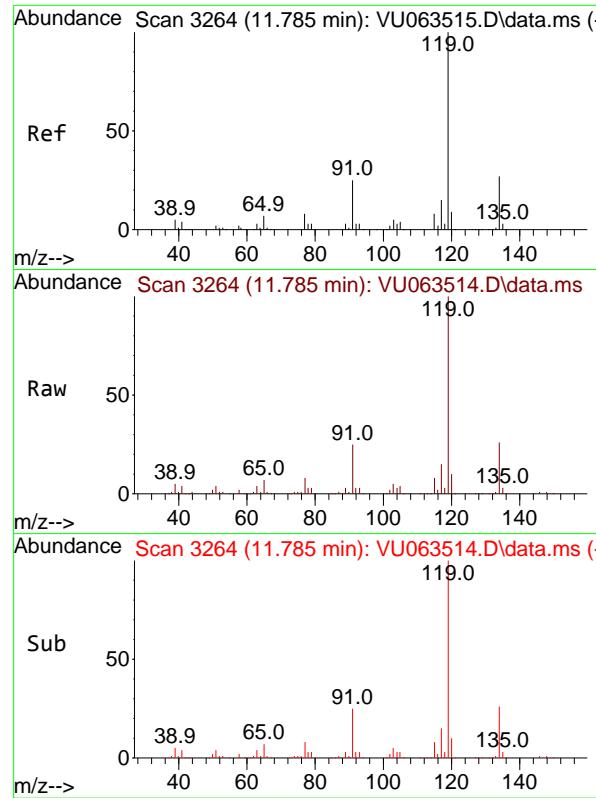


#81
p-Isopropyltoluene
Concen: 5.093 ug/l
RT: 11.785 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U
ClientSampleId : VSTDICC005

Tgt Ion:119 Resp: 156560
Ion Ratio Lower Upper
119 100
134 25.3 21.1 31.7
91 24.6 19.8 29.8


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

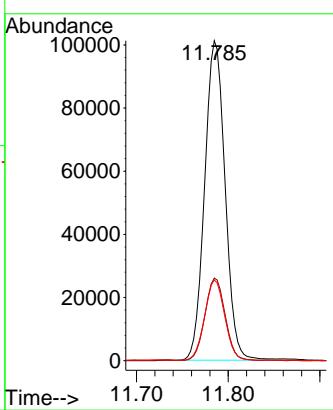

#82
1,3-Dichlorobenzene
Concen: 5.007 ug/l
RT: 11.740 min Scan# 3250
Delta R.T. 0.003 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Tgt Ion:146 Resp: 77340
Ion Ratio Lower Upper
146 100
111 41.4 33.8 50.6
148 62.7 51.5 77.3

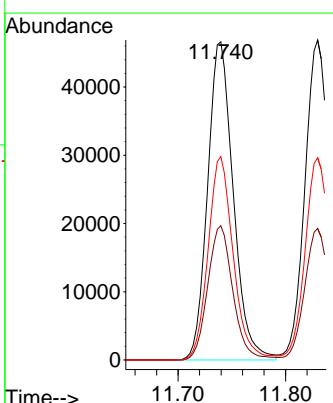



#83

1,4-Dichlorobenzene

Concen: 4.975 ug/l

RT: 11.830 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument :

MSVOA_U


ClientSampleId :

VSTDICC005

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

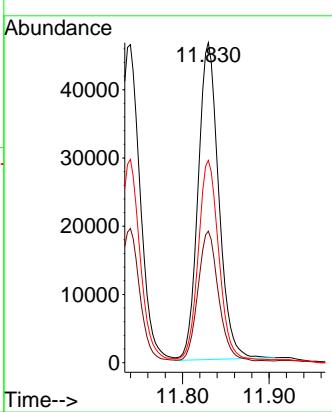

#84

n-Butylbenzene

Concen: 5.087 ug/l

RT: 12.200 min Scan# 3393

Delta R.T. -0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion: 91 Resp: 145033




Ion Ratio Lower Upper

91 100

92 52.0 41.5 62.3

134 25.4 20.6 30.8

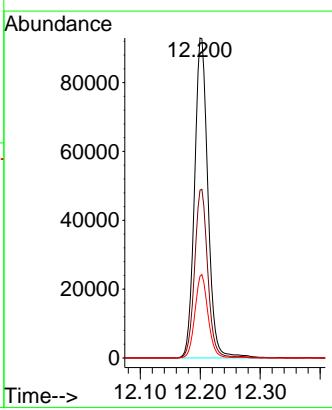



#85

1,2-Dichlorobenzene

Concen: 4.958 ug/l

RT: 12.206 min Scan# 3

Instrument : MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

ClientSampleId : VSTDICC005

Tgt Ion:146 Resp: 7194:

Ion Ratio Lower Upper

146 100




111 44.5 21.7 65.1

148 63.3 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 4.863 ug/l

RT: 12.987 min Scan# 3638

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00


Tgt Ion: 75 Resp: 4378


Ion Ratio Lower Upper

75 100

155 82.6 65.8 98.6

157 111.0 81.4 122.2

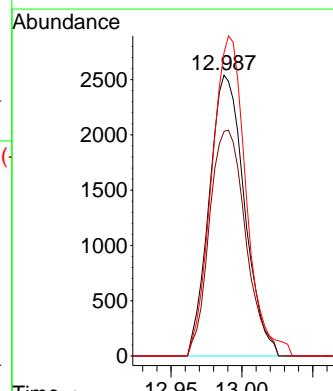


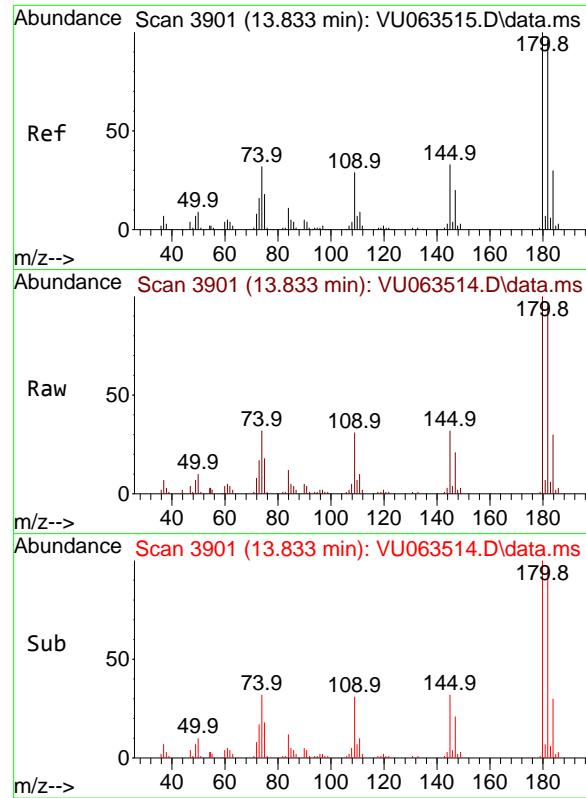


#87
1,2,4-Trichlorobenzene
Concen: 4.931 ug/l
RT: 13.833 min Scan# 3901
Delta R.T. -0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Instrument : MSVOA_U
ClientSampleId : VSTDICC005


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

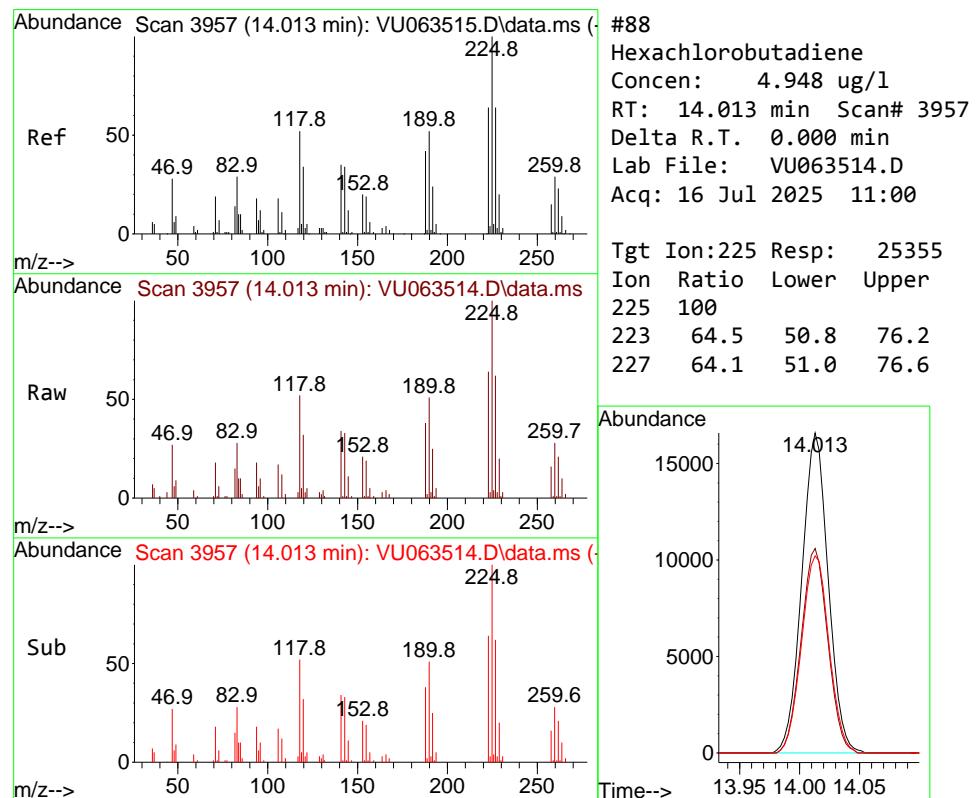

#88
Hexachlorobutadiene
Concen: 4.948 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063514.D
Acq: 16 Jul 2025 11:00

Tgt Ion:225 Resp: 25355
Ion Ratio Lower Upper
225 100
223 64.5 50.8 76.2
227 64.1 51.0 76.6

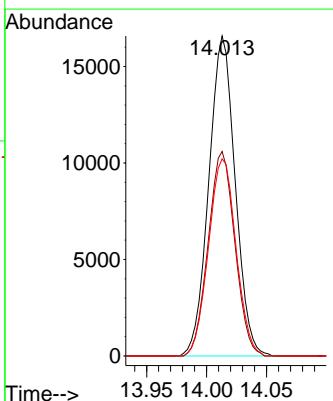

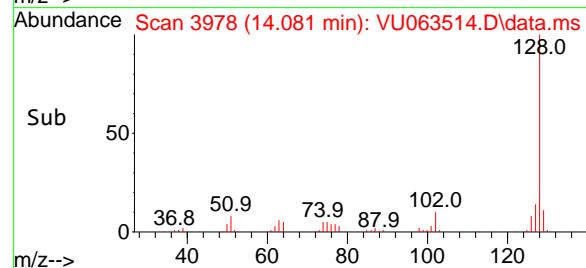

#89

Naphthalene

Concen: 4.728 ug/l

RT: 14.081 min Scan# 3

Delta R.T. 0.001 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00

Instrument:

MSVOA_U




ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#90

1,2,3-Trichlorobenzene

Concen: 5.017 ug/l

RT: 14.322 min Scan# 4053

Delta R.T. 0.000 min

Lab File: VU063514.D

Acq: 16 Jul 2025 11:00



Tgt Ion:180 Resp: 41834

Ion Ratio Lower Upper

180 100

182 95.9 78.0 117.0

145 33.9 27.3 40.9

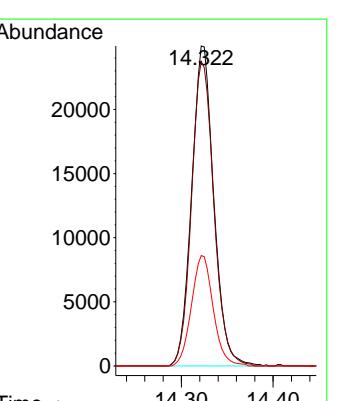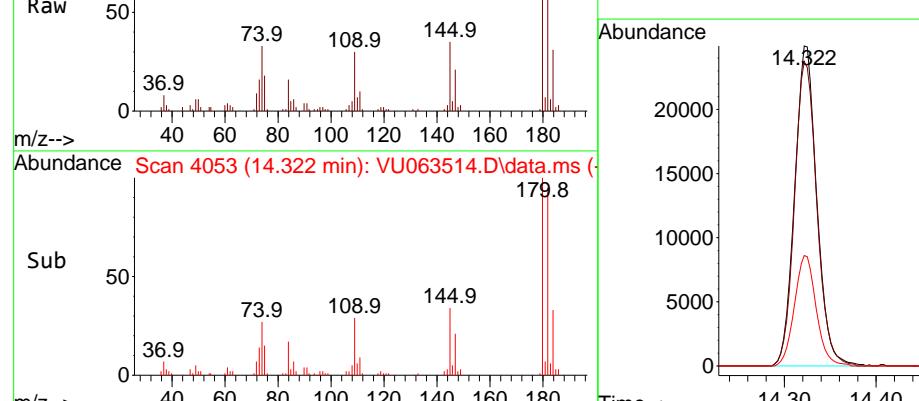

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063515.D
 Acq On : 16 Jul 2025 11:37
 Operator : MD/SY
 Sample : VSTDICCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTDICCC010

Quant Time: Jul 17 03:25:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.100	96	25507	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	9419	0.975	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	9149	1.024	ug/l	0.00
Spiked Amount 1.000			Recovery	=	102.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	75576	10.049	ug/l	100
3) Chloromethane	1.518	50	68401	9.784	ug/l	100
4) Vinyl Chloride	1.599	62	90489	10.162	ug/l	100
5) Bromomethane	1.840	94	62116	9.251	ug/l	100
6) Chloroethane	1.923	64	54599	10.156	ug/l	100
7) Trichlorofluoromethane	2.126	101	129904	10.161	ug/l	100
8) 1,1,2-Trichloro-1,2,2-...	2.566	101	67855	10.156	ug/l	100
9) 1,1-Dichloroethene	2.566	96	67577	10.205	ug/l	100
10) Iodomethane	2.708	142	94216	9.560	ug/l	100
11) Allyl Chloride	2.907	41	97312	10.172	ug/l	100
12) Acrylonitrile	3.306	53	32316	19.501	ug/l	100
13) Acetone	2.618	43	63754	48.044	ug/l	100
14) Carbon Disulfide	2.775	76	219662	10.270	ug/l	100
15) Methylene Chloride	3.029	84	74766	9.590	ug/l	100
16) trans-1,2-Dichloroethene	3.335	96	76110	10.120	ug/l	100
17) 1,1-Dichloroethane	3.849	63	139986	10.042	ug/l	100
18) 2-Butanone	4.711	43	101743	49.509	ug/l	100
19) Cyclohexane	5.361	56	117794	9.980	ug/l	100
20) Methylcyclohexane	6.740	83	124959	10.893	ug/l	100
21) 2,2-Dichloropropane	4.644	77	115814	9.757	ug/l	100
22) cis-1,2-Dichloroethene	4.647	96	81707	10.012	ug/l	100
23) Diethyl Ether	2.367	59	52619	10.428	ug/l	100
24) tert-Butyl Alcohol	3.190	59	60952	100.062	ug/l	100
25) Methyl tert-Butyl Ether	3.361	73	176642	10.218	ug/l	100
26) Bromochloromethane	4.955	128	35072	10.293	ug/l	100
27) Chloroform	5.071	83	139474	9.805	ug/l	100
28) 1,1,1-Trichloroethane	5.296	97	122824	10.174	ug/l	100
29) 1,1-Dichloropropene	5.505	75	110654	9.894	ug/l	100
30) Carbon Tetrachloride	5.502	117	99861	10.277	ug/l	100
31) Isopropyl Ether	3.991	45	212065	10.078	ug/l	100
32) Ethyl-t-butyl ether	4.502	59	196224	10.077	ug/l	100
33) Tert-Amyl methyl ether	5.943	73	169757	10.045	ug/l	100
34) Propionitrile	4.772	54	29396	46.949	ug/l	100
35) Benzene	5.756	78	306660	10.205	ug/l	100
36) 1,2-Dichloroethane	5.782	62	95989	10.281	ug/l	100
37) Trichloroethene	6.525	130	82269	10.731	ug/l	100
38) 1,2-Dichloropropane	6.779	63	80452	11.439	ug/l	100
39) Methacrylonitrile	4.972	41	25859	9.408	ug/l	100
40) Methyl acrylate	4.846	55	42948	10.557	ug/l	100
41) Tetrahydrofuran	5.058	42	26672	18.218	ug/l	100
42) 1-Chlorobutane	5.438	56	150746	10.139	ug/l	100
43) Dibromomethane	6.907	93	39219	10.765	ug/l	100
44) Bromodichloromethane	7.094	83	83585	10.173	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063515.D
 Acq On : 16 Jul 2025 11:37
 Operator : MD/SY
 Sample : VSTDICCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICCC010

Quant Time: Jul 17 03:25:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	194373	51.766	ug/l	100
46) t-1,4-Dichloro-2-butene	10.820	75	32073m	24.076	ug/l	
47) Methyl methacrylate	6.962	69	64875	21.203	ug/l	100
48) Ethyl methacrylate	8.335	69	64347	11.020	ug/l	100
49) Toluene	7.959	92	171146	10.432	ug/l	100
50) t-1,3-Dichloropropene	8.203	75	72787	11.292	ug/l	100
51) cis-1,3-Dichloropropene	7.598	75	92302	10.668	ug/l	100
52) 1,1,2-Trichloroethane	8.393	97	51547	10.510	ug/l	100
53) 1,3-Dichloropropane	8.569	76	87683	10.355	ug/l	100
54) 2-Hexanone	8.688	43	131332	52.658	ug/l	100
55) Dibromochloromethane	8.801	129	59098	11.401	ug/l	100
56) 1,2-Dibromoethane	8.917	107	45601	10.388	ug/l	100
58) Tetrachloroethene	8.540	164	72806	10.376	ug/l	100
59) Chlorobenzene	9.441	112	196780	10.443	ug/l	100
60) 1,1,1,2-Tetrachloroethane	9.528	131	64850	10.702	ug/l	100
61) Pentachloroethane	11.418	117	47516	11.097	ug/l	100
62) Hexachloroethane	12.466	117	49020	11.561	ug/l	100
63) Ethyl Benzene	9.563	91	335269	10.340	ug/l	100
64) m/p-Xylenes	9.685	106	264769	21.007	ug/l	100
65) o-Xylene	10.094	106	128634	10.621	ug/l	100
66) Styrene	10.106	104	209876	10.873	ug/l	100
67) Bromoform	10.283	173	30149	11.325	ug/l	100
69) Isopropylbenzene	10.476	105	313810	10.718	ug/l	100
70) 1,1,2,2-Tetrachloroethane	10.775	83	61909	10.373	ug/l	100
71) 1,2,3-Trichloropropane	10.817	75	53057m	10.893	ug/l	
72) Bromobenzene	10.775	156	78897	10.441	ug/l	100
73) n-propylbenzene	10.897	120	95656	10.853	ug/l	100
74) 2-Chlorotoluene	10.978	126	82104	10.540	ug/l	100
75) 1,3,5-Trimethylbenzene	11.081	105	301469	10.778	ug/l	100
76) 4-Chlorotoluene	11.090	126	84140	10.636	ug/l	100
77) tert-Butylbenzene	11.412	119	286405	10.714	ug/l	100
78) 1,2,4-Trimethylbenzene	11.460	105	300364	10.824	ug/l	100
79) sec-Butylbenzene	11.634	105	386577	10.724	ug/l	100
80) Nitrobenzene	13.203	77	6826	50.800	ug/l	100
81) p-Isopropyltoluene	11.785	119	325219	10.808	ug/l	100
82) 1,3-Dichlorobenzene	11.737	146	160312	10.603	ug/l	100
83) 1,4-Dichlorobenzene	11.830	146	161963	10.702	ug/l	100
84) n-Butylbenzene	12.200	91	308761	11.063	ug/l	100
85) 1,2-Dichlorobenzene	12.206	146	152208	10.716	ug/l	100
86) 1,2-Dibromo-3-Chloropr...	12.987	75	10205	10.093	ug/l	100
87) 1,2,4-Trichlorobenzene	13.833	180	98105	11.107	ug/l	100
88) Hexachlorobutadiene	14.013	225	53764	10.718	ug/l	100
89) Naphthalene	14.080	128	173115	10.937	ug/l	100
90) 1,2,3-Trichlorobenzene	14.322	180	89908	11.015	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063515.D
Acq On : 16 Jul 2025 11:37
Operator : MD/SY
Sample : VSTDICCC010
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1


Quant Time: Jul 17 03:25:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:16:16 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VSTDICCC010

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

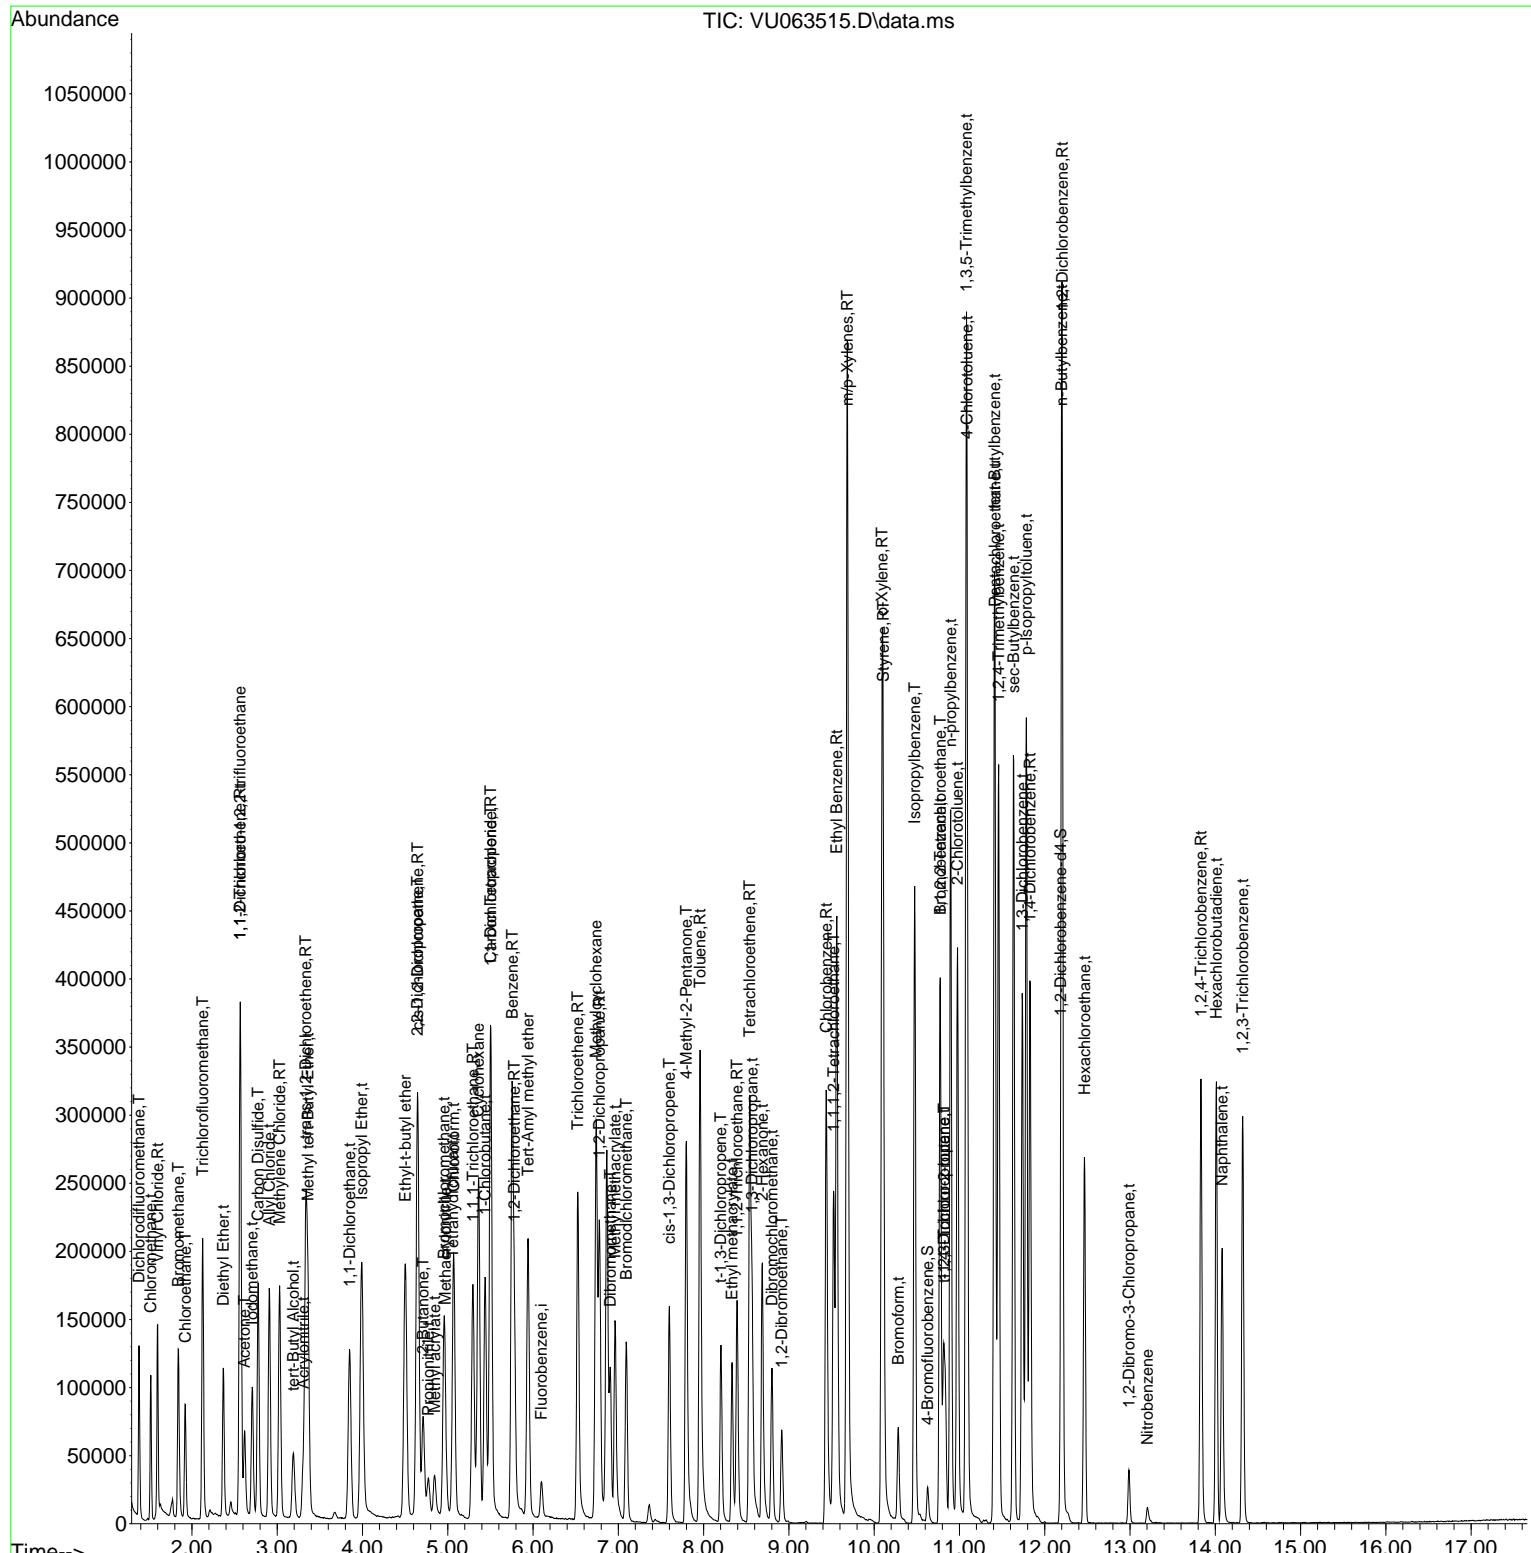





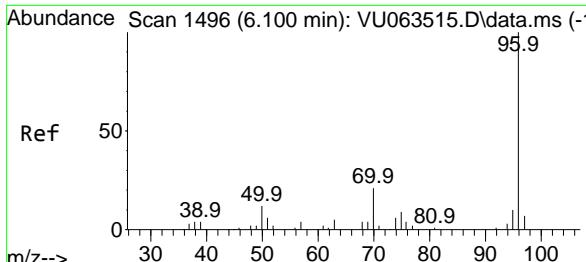


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37





Instrument :
SVOA_U
ClientSampleId :
STDICCC010


Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

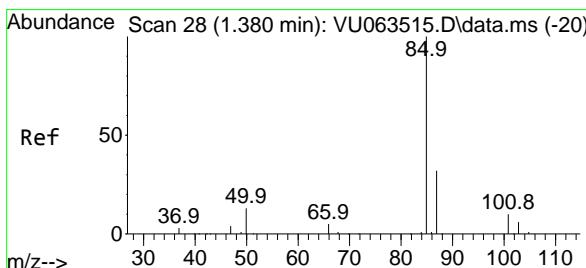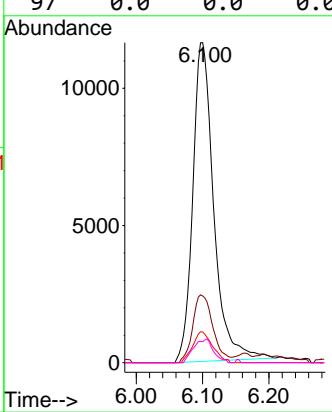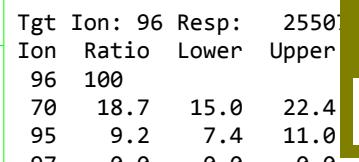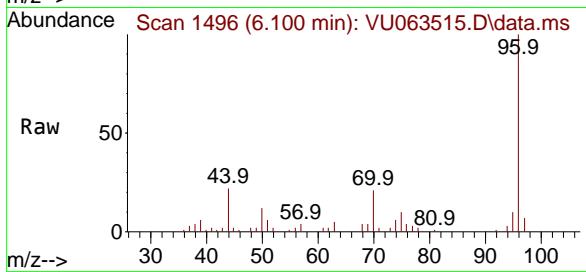

```
#2  
Dichlorodifluoromethane  
Concen: 10.049 ug/l  
RT: 1.380 min Scan# 28  
Delta R.T. 0.000 min  
Lab File: VU063515.D  
Acq: 16 Jul 2025 11:37
```

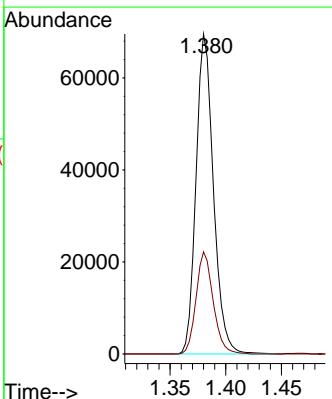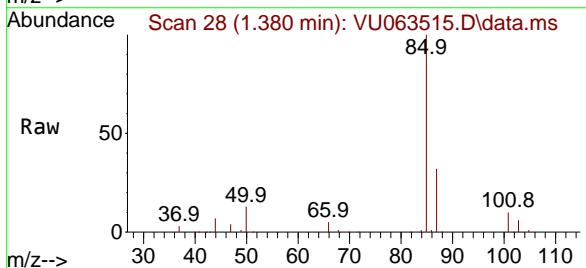




Ref Scan 71 (1.518 min): VU063515.D\data.ms

Abundance Scan 71 (1.518 min): VU063515.D\data.ms


m/z-->

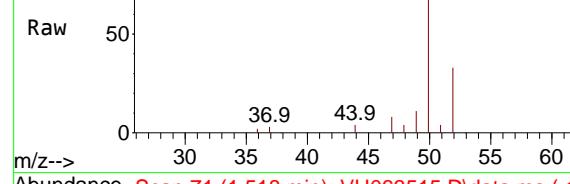

Abundance Scan 71 (1.518 min): VU063515.D\data.ms (-1)

Sub Scan 71 (1.518 min): VU063515.D\data.ms (-1)

m/z-->

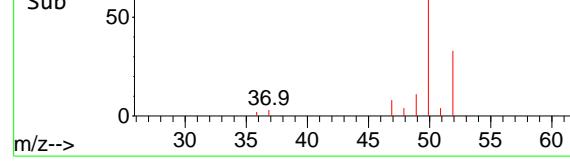


Abundance Scan 96 (1.599 min): VU063515.D\data.ms (-87)

Ref Scan 96 (1.599 min): VU063515.D\data.ms

Abundance Scan 96 (1.599 min): VU063515.D\data.ms


m/z-->

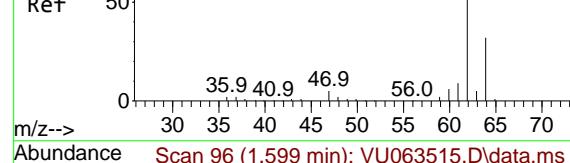

Abundance Scan 96 (1.599 min): VU063515.D\data.ms (-1)

Sub Scan 96 (1.599 min): VU063515.D\data.ms (-1)

m/z-->

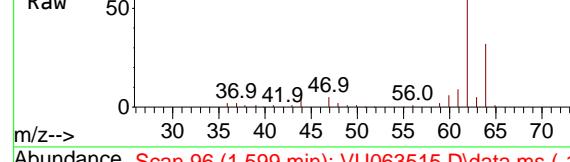

#3

Chloromethane

Concen: 9.784 ug/l

RT: 1.518 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

Tgt Ion: 50 Resp: 6840

Ion Ratio Lower Upper

50 100


52 32.9 26.3 39.5

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

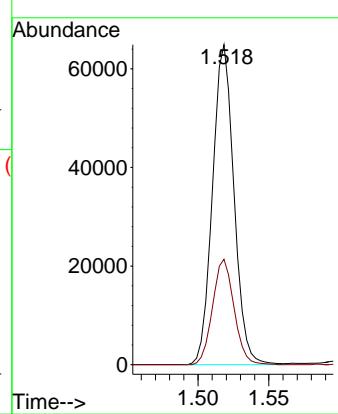

#4

Vinyl Chloride

Concen: 10.162 ug/l

RT: 1.599 min Scan# 96

Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37


Tgt Ion: 62 Resp: 90489

Ion Ratio Lower Upper

62 100


64 32.1 25.7 38.5

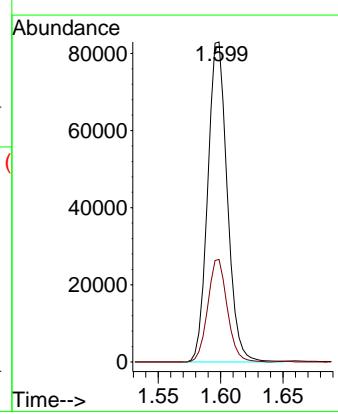



#5
Bromomethane
Concen: 9.251 ug/l
RT: 1.840 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37



Instrument : MSVOA_U
ClientSampleId : VSTDICCC010




Tgt Ion: 94 Resp: 62110
Ion Ratio Lower Upper
94 100
96 94.7 75.8 113.6

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#6
Chloroethane
Concen: 10.156 ug/l
RT: 1.923 min Scan# 197
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Tgt Ion: 64 Resp: 54599
Ion Ratio Lower Upper
64 100
66 32.8 26.2 39.4

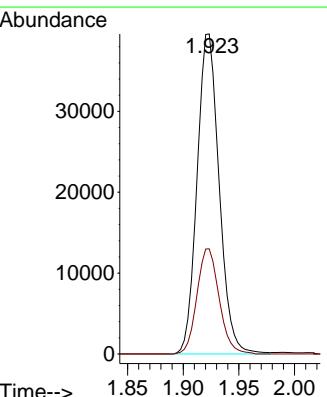



#7
Trichlorofluoromethane
Concen: 10.161 ug/l
RT: 2.126 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

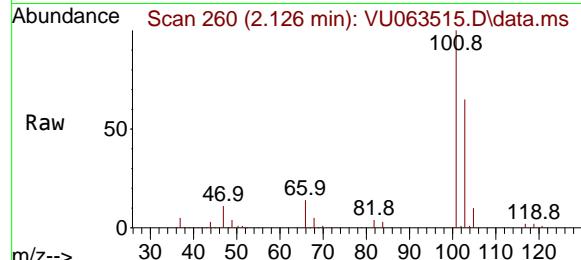

Tgt Ion:101 Resp: 12990
Ion Ratio Lower Upper
101 100
103 65.3 52.2 78.4



Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

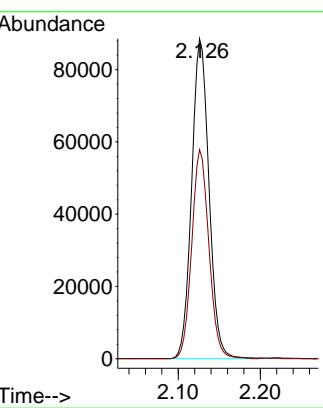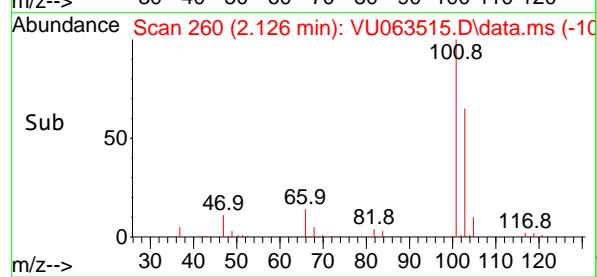

#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 10.156 ug/l
RT: 2.566 min Scan# 397
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37


Tgt Ion:101 Resp: 67855
Ion Ratio Lower Upper
101 100
85 47.2 37.8 56.6
151 74.0 59.2 88.8

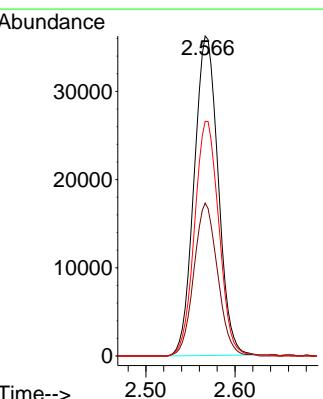



#9
1,1-Dichloroethene
Concen: 10.205 ug/l
RT: 2.566 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

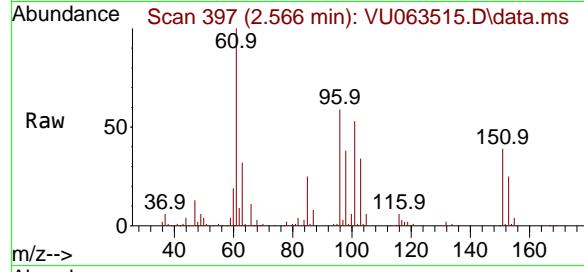


Tgt Ion: 96 Resp: 6757
Ion Ratio Lower Upper
96 100
61 168.1 0.0 504.3
98 63.4 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

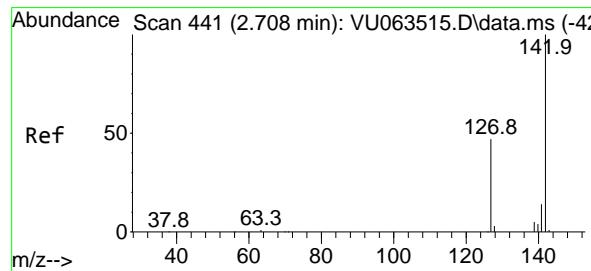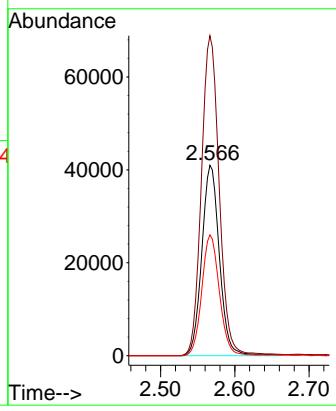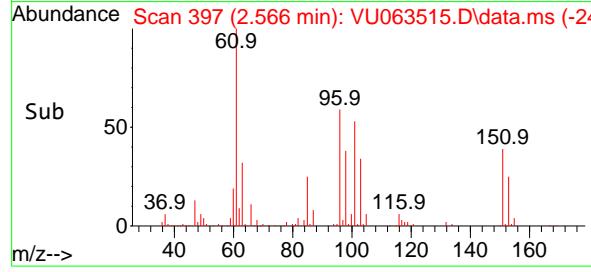


#10
Iodomethane
Concen: 9.560 ug/l
RT: 2.708 min Scan# 441
Delta R.T. -0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

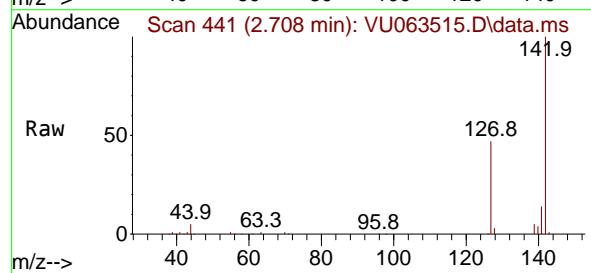


Tgt Ion:142 Resp: 94216
Ion Ratio Lower Upper
142 100
127 47.4 37.9 56.9

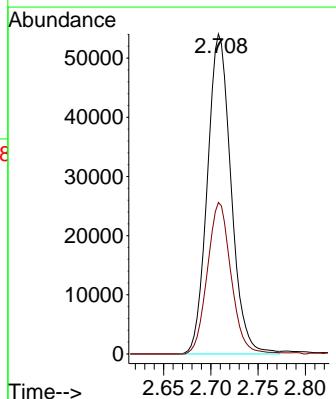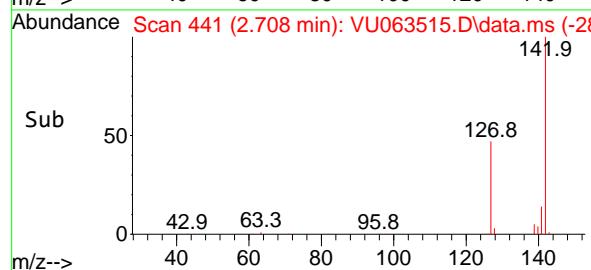



#11
Allyl Chloride
Concen: 10.172 ug/l
RT: 2.907 min Scan# 5
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

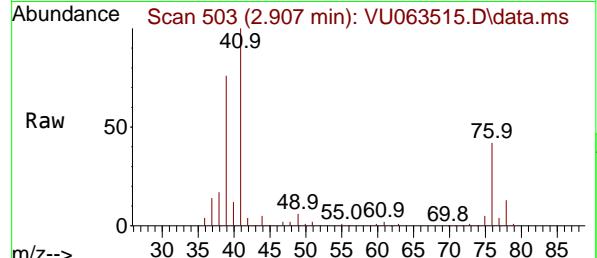


Tgt Ion: 41 Resp: 9731
Ion Ratio Lower Upper
41 100
39 76.9 61.5 92.3

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

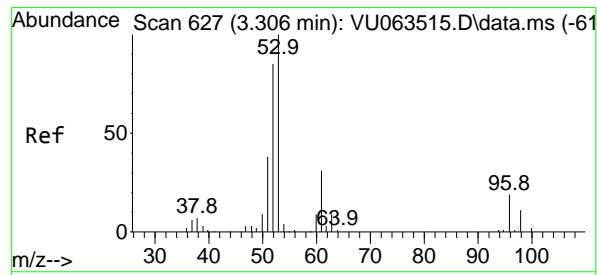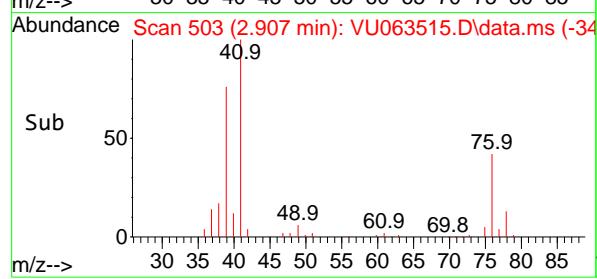


#12
Acrylonitrile
Concen: 19.501 ug/l
RT: 3.306 min Scan# 627
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Tgt Ion: 53 Resp: 32316
Ion Ratio Lower Upper
53 100
52 80.4 64.3 96.5
51 34.8 27.8 41.8






Abundance Scan 413 (2.618 min): VU063515.D\data.ms

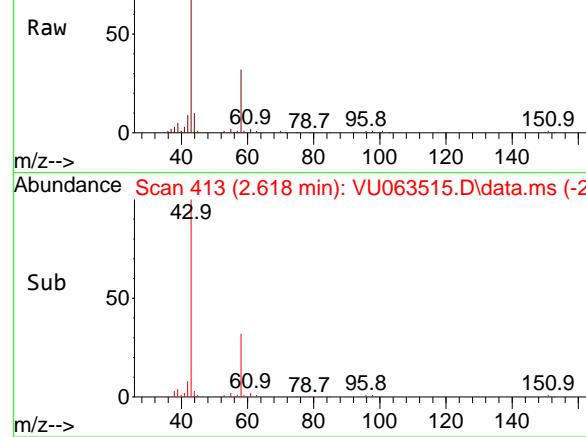

Abundance Scan 413 (2.618 min): VU063515.D\data.ms (-25)

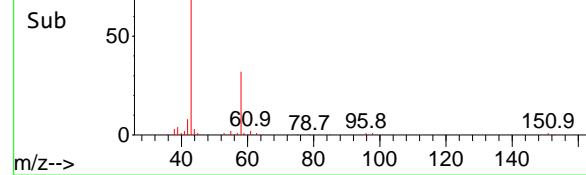

#13

Acetone

Concen: 48.044 ug/l

RT: 2.618 min Scan# 413

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37



Instrument :

MSVOA_U


ClientSampleId :

VSTDICCC010


**Manual Integrations
APPROVED**

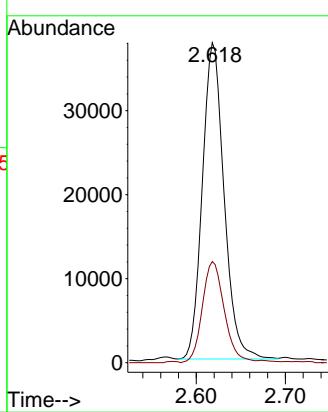 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


Abundance Scan 462 (2.775 min): VU063515.D\data.ms

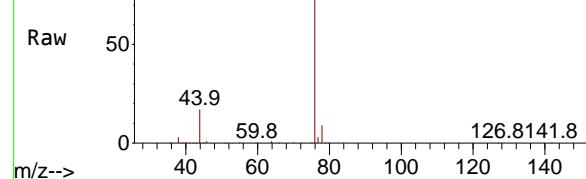

Abundance Scan 462 (2.775 min): VU063515.D\data.ms (-30)

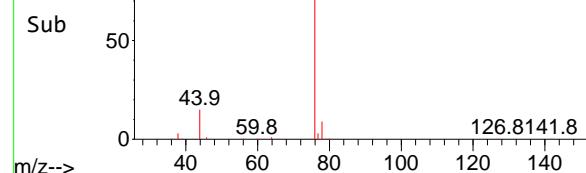

#14

Carbon Disulfide

Concen: 10.270 ug/l

RT: 2.775 min Scan# 462

Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37







Tgt Ion: 76 Resp: 219662

Ion Ratio Lower Upper

76 100

78 8.8 7.0 10.6

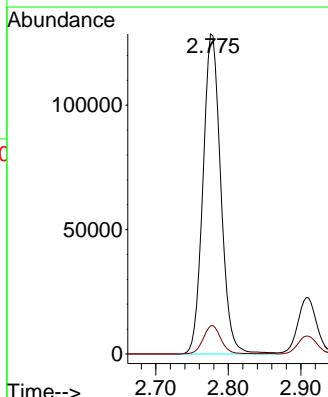

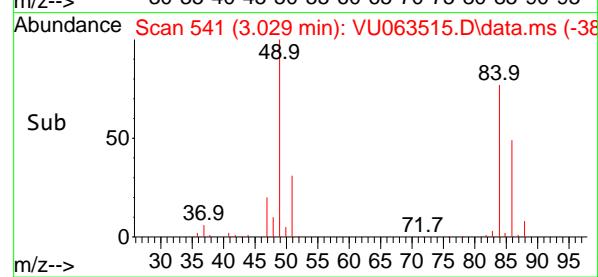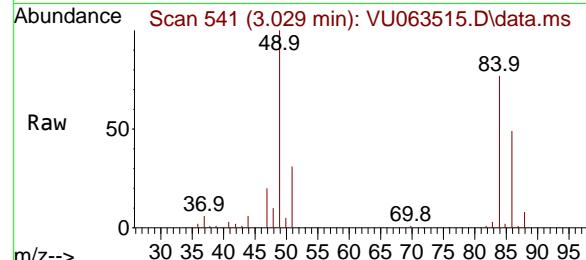

#15

Methylene Chloride

Concen: 9.590 ug/l

RT: 3.029 min Scan# 541

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U

ClientSampleId : VSTDICCC010

Tgt Ion: 84 Resp: 74760

Ion Ratio Lower Upper

84 100

49 129.8 103.8 155.8

51 40.2 0.0 80.4


86 63.9 51.1 76.7

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

Abundance

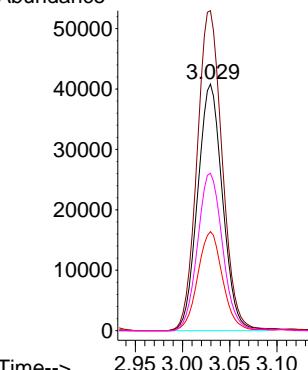

#16

trans-1,2-Dichloroethene

Concen: 10.120 ug/l

RT: 3.335 min Scan# 636

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Tgt Ion: 96 Resp: 76110


Ion Ratio Lower Upper




96 100

61 146.5 117.2 175.8

98 64.3 51.4 77.2

Abundance

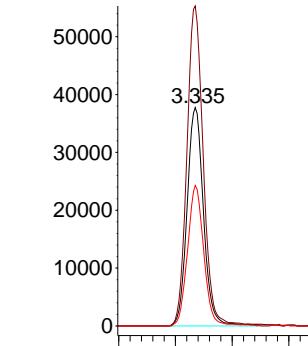



#17

1,1-Dichloroethane

Concen: 10.042 ug/l

RT: 3.849 min Scan# 796

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument :

MSVOA_U




ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#18

2-Butanone

Concen: 49.509 ug/l

RT: 4.711 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37




Tgt Ion: 43 Resp: 101743

Ion Ratio Lower Upper

43 100

57 8.2 0.0 16.4

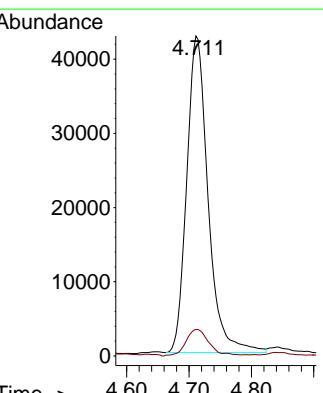



#19

Cyclohexane

Concen: 9.980 ug/l

RT: 5.361 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U




ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#20

Methylcyclohexane

Concen: 10.893 ug/l

RT: 6.740 min Scan# 1695

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion: 83 Resp: 124959




Ion Ratio Lower Upper

83 100

55 75.7 60.6 90.8

98 44.8 35.8 53.8

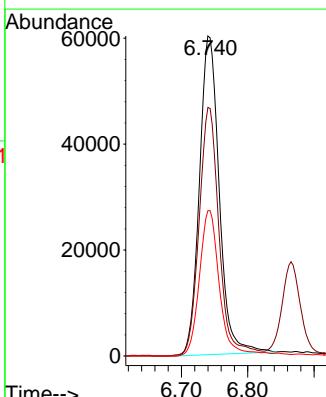

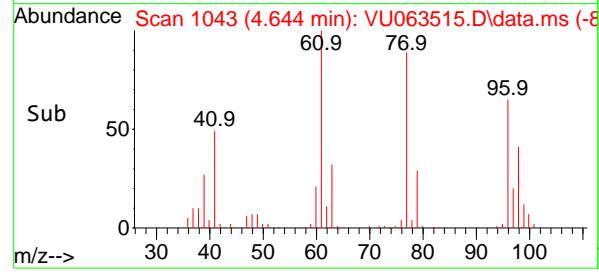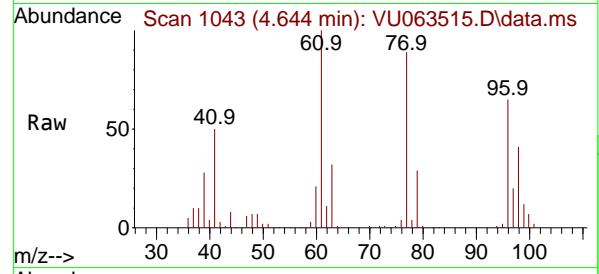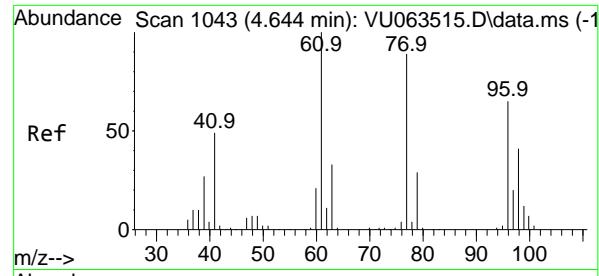

#21

2,2-Dichloropropane

Concen: 9.757 ug/l

RT: 4.644 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#22

cis-1,2-Dichloroethene

Concen: 10.012 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion: 96 Resp: 81707




Ion Ratio Lower Upper

96 100

61 153.9 0.0 384.7

98 64.2 32.1 96.3

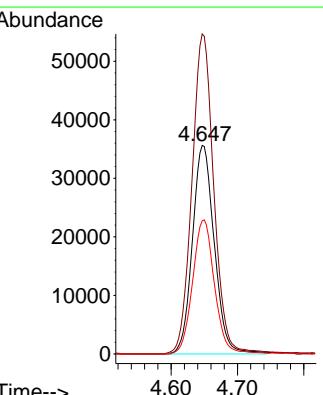

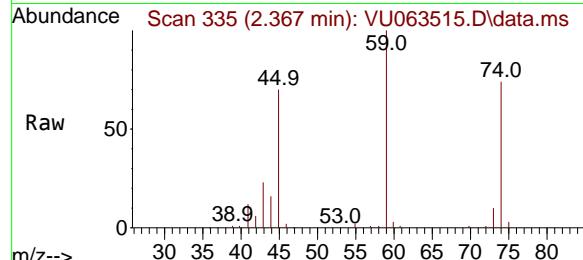

#23

Diethyl Ether

Concen: 10.428 ug/l

RT: 2.367 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

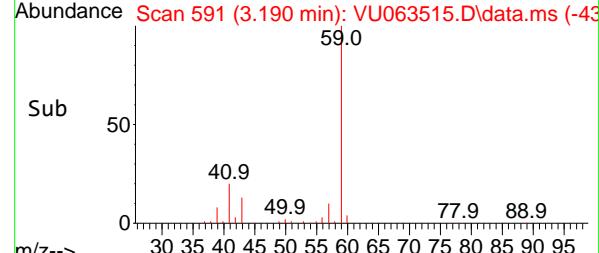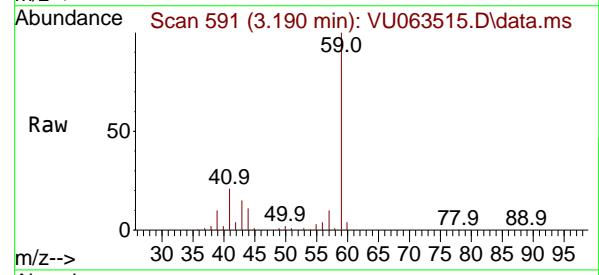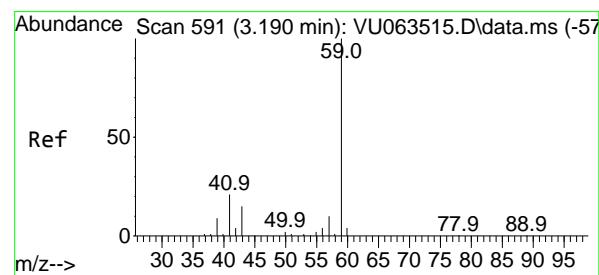 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#24

tert-Butyl Alcohol

Concen: 100.062 ug/l

RT: 3.190 min Scan# 591

Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37



Tgt Ion: 59 Resp: 60952

Ion Ratio Lower Upper

59 100

57 10.7 8.6 12.8

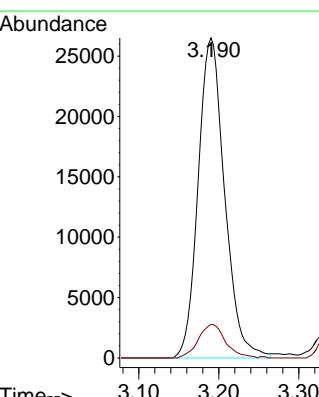

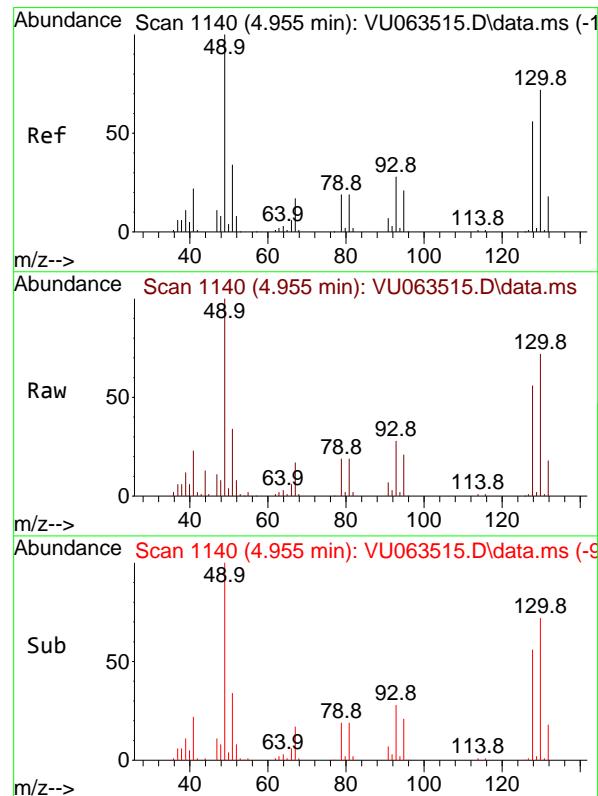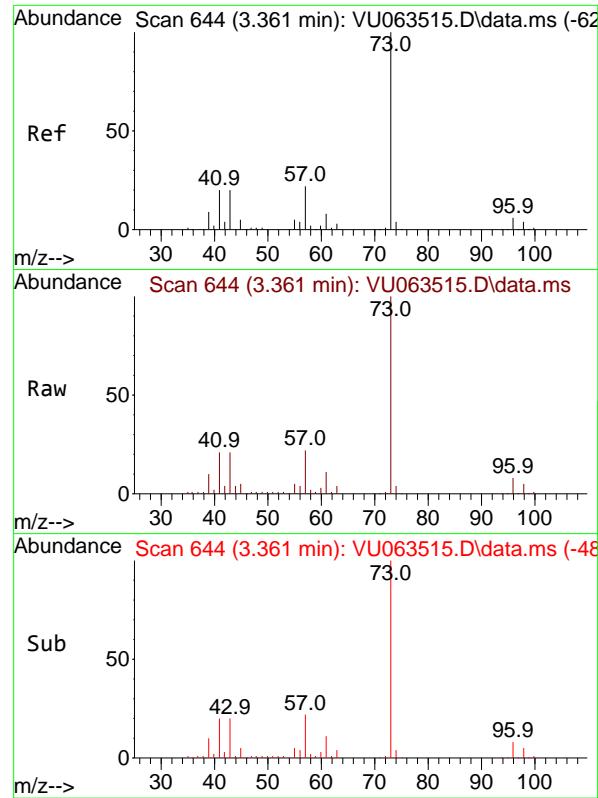

#25


Methyl tert-Butyl Ether
Concen: 10.218 ug/l
RT: 3.361 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

Tgt Ion: 73 Resp: 17664
Ion Ratio Lower Upper
73 100
43 20.2 16.2 24.2

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

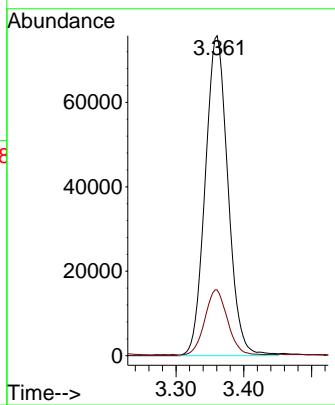


#26

Bromochloromethane
Concen: 10.293 ug/l
RT: 4.955 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:128 Resp: 35072
Ion Ratio Lower Upper
128 100
49 170.4 0.0 340.8
130 125.6 100.5 150.7

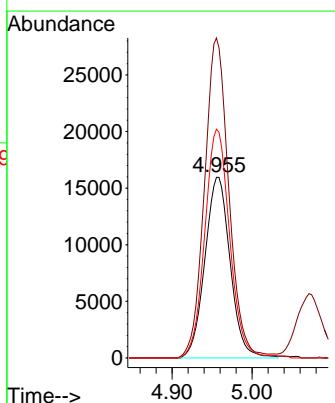


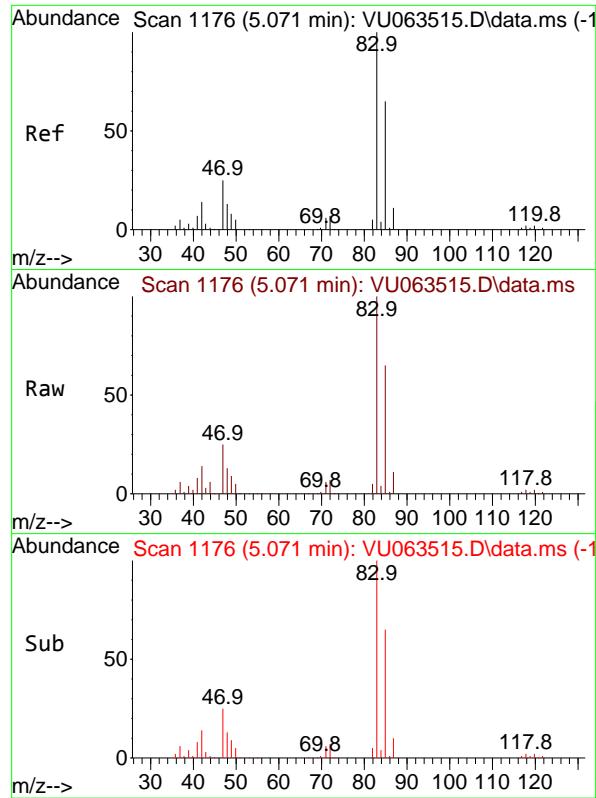


#27
 Chloroform
 Concen: 9.805 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063515.D
 Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
 ClientSampleId : VSTDICCC010


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

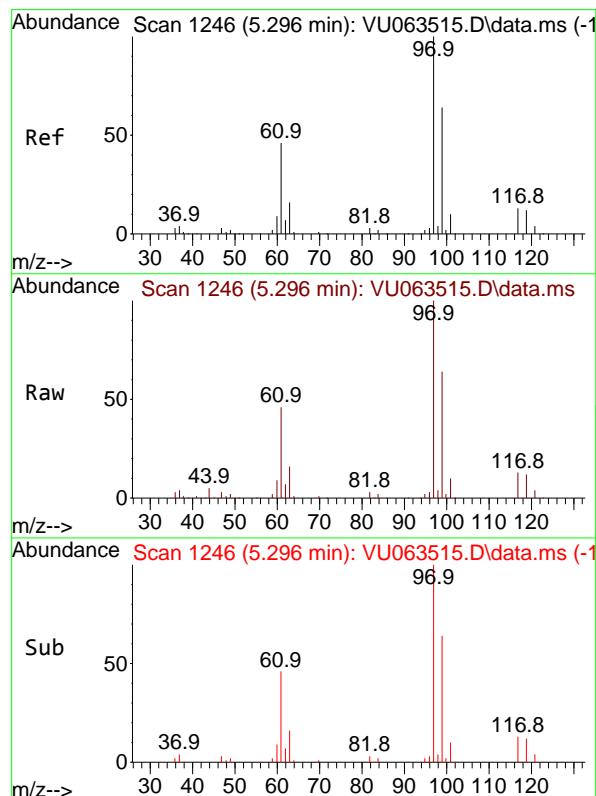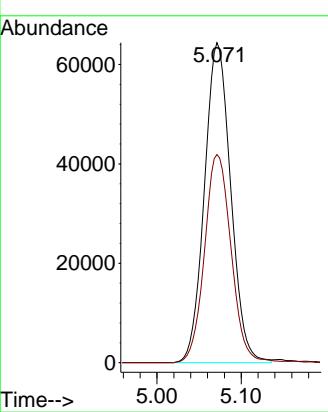

#28
 1,1,1-Trichloroethane
 Concen: 10.174 ug/l
 RT: 5.296 min Scan# 1246
 Delta R.T. 0.000 min
 Lab File: VU063515.D
 Acq: 16 Jul 2025 11:37

Tgt Ion: 97 Resp: 122824
 Ion Ratio Lower Upper
 97 100
 99 63.5 31.8 95.3
 61 46.6 23.3 69.9




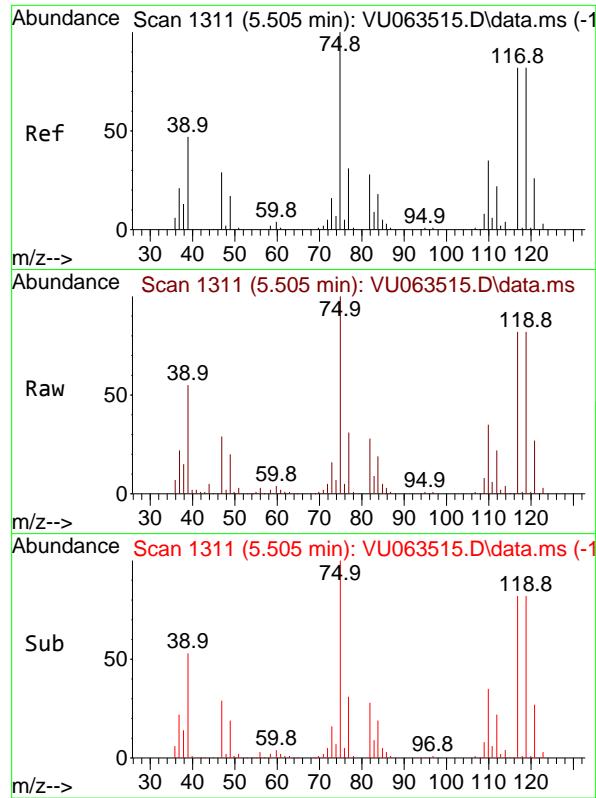


#29
1,1-Dichloropropene
Concen: 9.894 ug/l
RT: 5.505 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010


Manual Integrations
APPROVED







Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

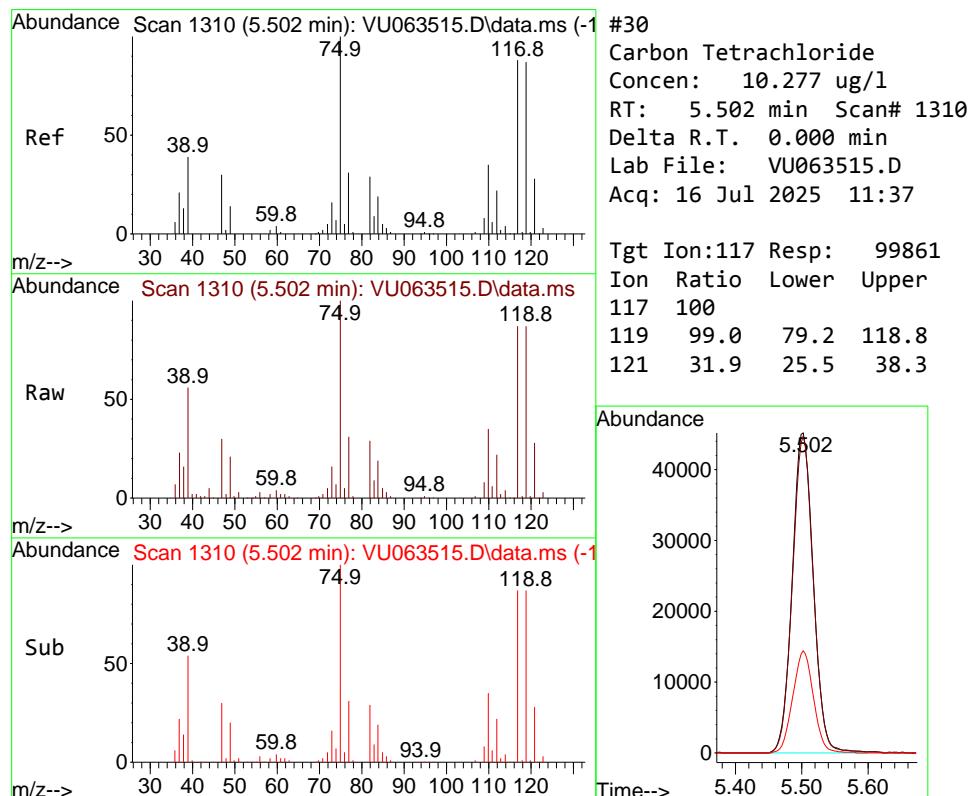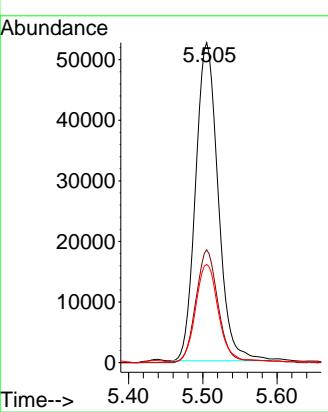

#30
Carbon Tetrachloride
Concen: 10.277 ug/l
RT: 5.502 min Scan# 1310
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:117 Resp: 99861
Ion Ratio Lower Upper
117 100
119 99.0 79.2 118.8
121 31.9 25.5 38.3





#31

Isopropyl Ether

Concen: 10.078 ug/l

RT: 3.991 min Scan# 81

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#32

Ethyl-t-butyl ether


Concen: 10.077 ug/l


RT: 4.502 min Scan# 999

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

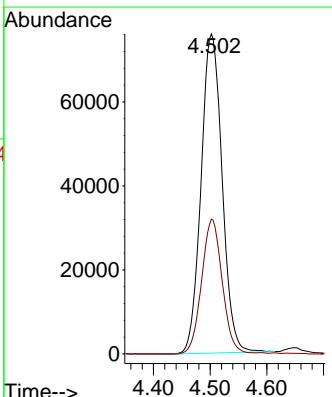 Tgt Ion: 59 Resp: 196224
 Ion Ratio Lower Upper
 59 100
 87 40.8 32.6 49.0

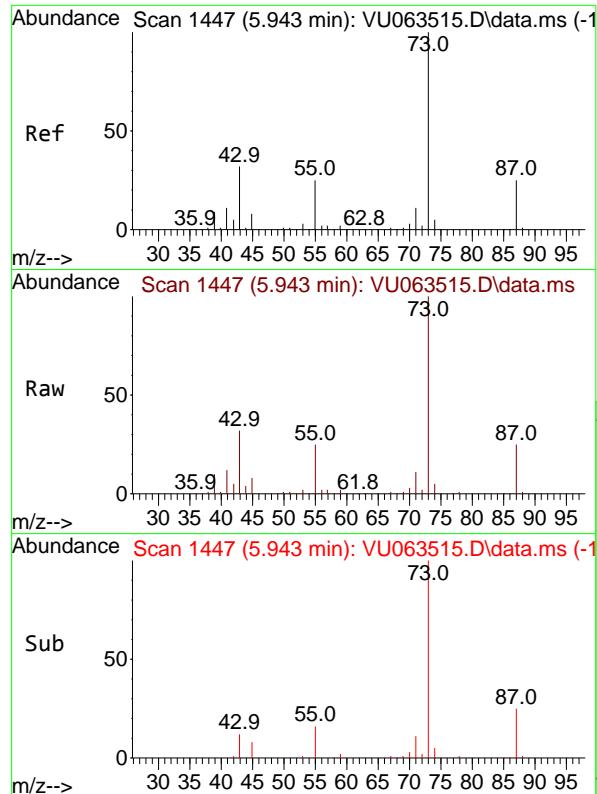


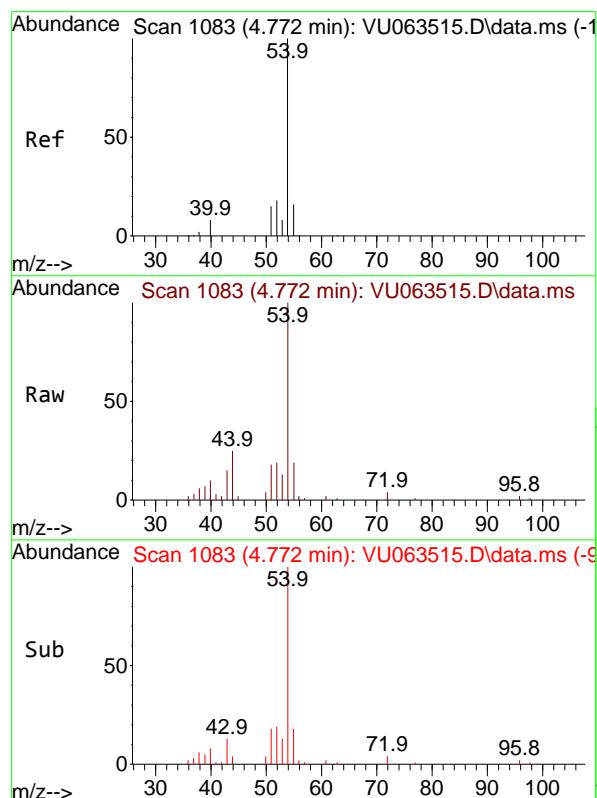

#33

Tert-Amyl methyl ether
Concen: 10.045 ug/l
RT: 5.943 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#34


Propionitrile
Concen: 46.949 ug/l
RT: 4.772 min Scan# 1083
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion: 54 Resp: 29396
Ion Ratio Lower Upper
54 100
52 21.2 17.0 25.4
55 17.0 13.6 20.4
40 8.0 6.4 9.6

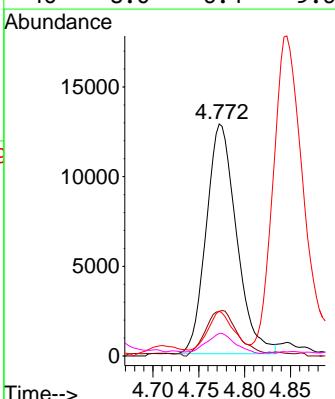






#35
Benzene
Concen: 10.205 ug/l
RT: 5.756 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Tgt Ion: 78 Resp: 306660
Ion Ratio Lower Upper
78 100
77 24.3 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#36
1,2-Dichloroethane
Concen: 10.281 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

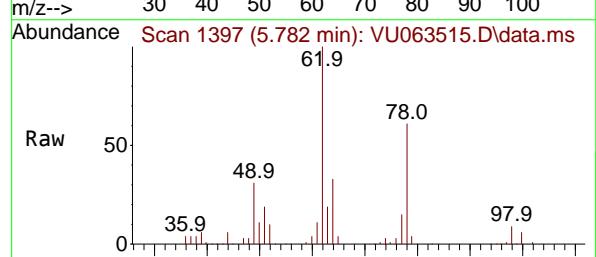


Tgt Ion: 62 Resp: 95989
Ion Ratio Lower Upper
62 100
98 8.0 6.4 9.6



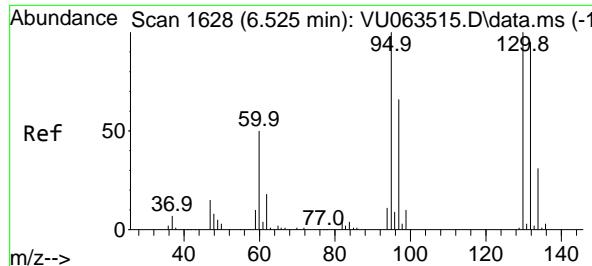

#37
Trichloroethene
Concen: 10.731 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

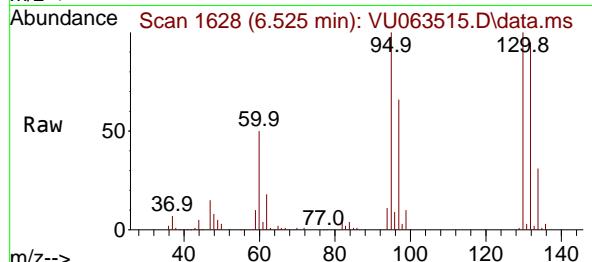


Tgt Ion:130 Resp: 82269
Ion Ratio Lower Upper
130 100
95 100.4 80.3 120.5

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

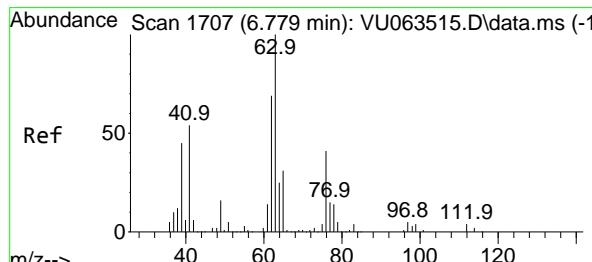

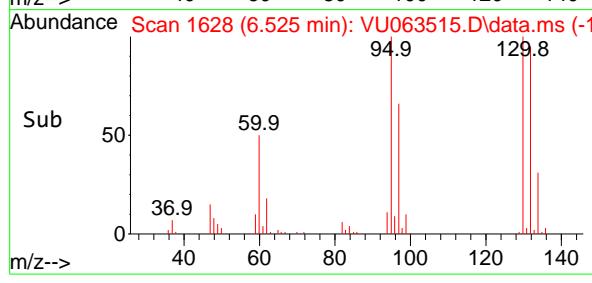


#38
1,2-Dichloropropane
Concen: 11.439 ug/l
RT: 6.779 min Scan# 1707
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

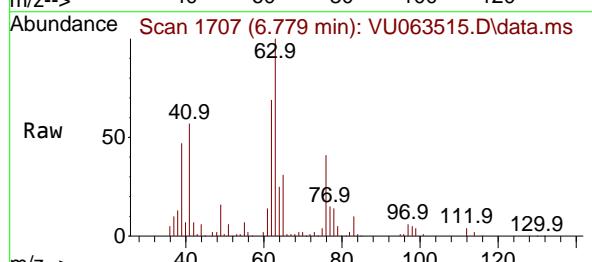

Tgt Ion: 63 Resp: 80452
Ion Ratio Lower Upper
63 100
65 30.7 24.6 36.8

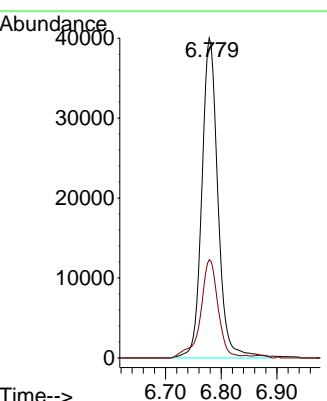

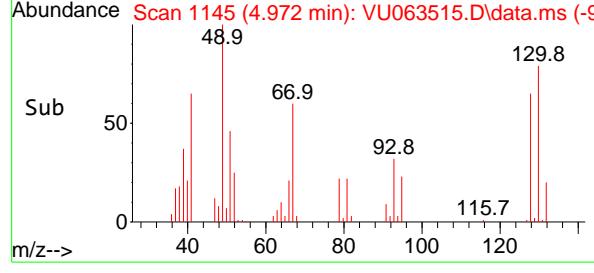

#39

Methacrylonitrile

Concen: 9.408 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

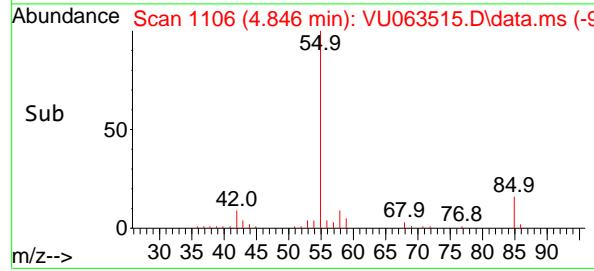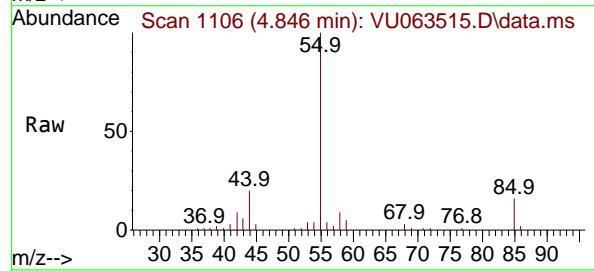 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#40

Methyl acrylate

Concen: 10.557 ug/l

RT: 4.846 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Tgt Ion: 55 Resp: 42948

Ion Ratio Lower Upper


55 100


85 16.0 12.8 19.2

58 8.7 7.0 10.4

42 8.7 7.0 10.4

Abundance

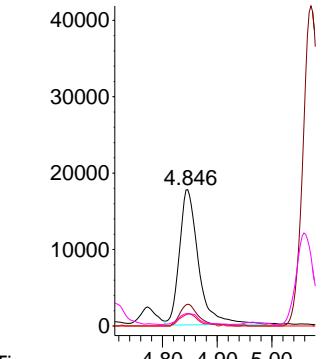


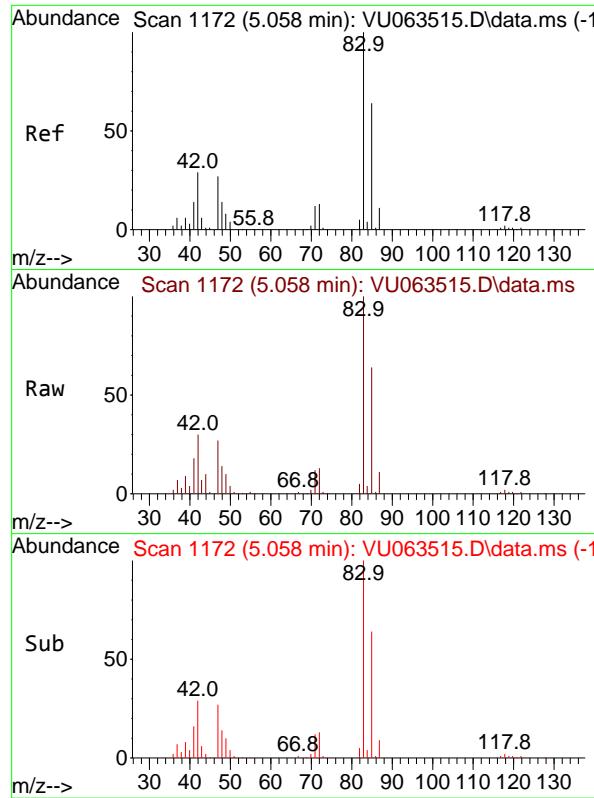


#41
Tetrahydrofuran
Concen: 18.218 ug/l
RT: 5.058 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

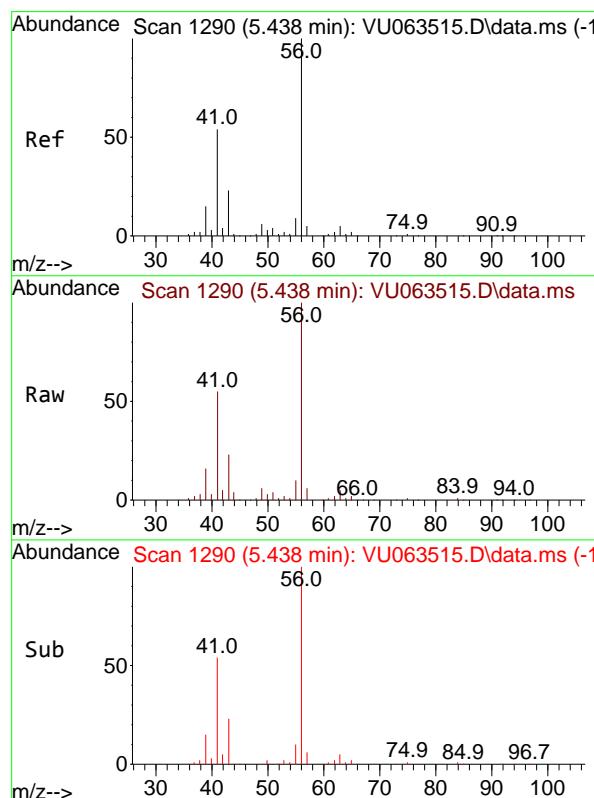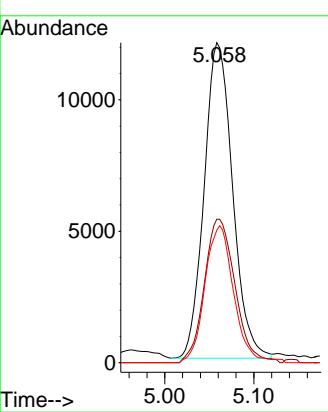

#42
1-Chlorobutane
Concen: 10.139 ug/l
RT: 5.438 min Scan# 1290
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37


Tgt Ion: 56 Resp: 150746
Ion Ratio Lower Upper
56 100
41 53.3 26.7 80.0





#43
Dibromomethane
Concen: 10.765 ug/l
RT: 6.907 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37




Instrument : MSVOA_U
ClientSampleId : VSTDICCC010




Tgt Ion: 93 Resp: 39219
Ion Ratio Lower Upper
93 100
95 84.9 67.9 101.9
174 93.2 74.6 111.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

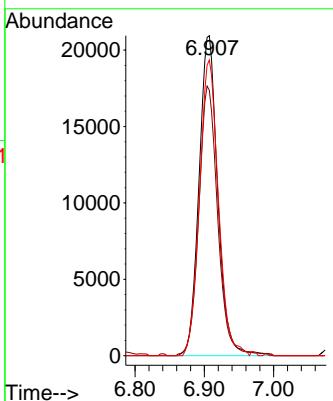


#44
Bromodichloromethane
Concen: 10.173 ug/l
RT: 7.094 min Scan# 1805
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37



Tgt Ion: 83 Resp: 83585
Ion Ratio Lower Upper
83 100
85 65.9 52.7 79.1
127 10.1 8.1 12.1

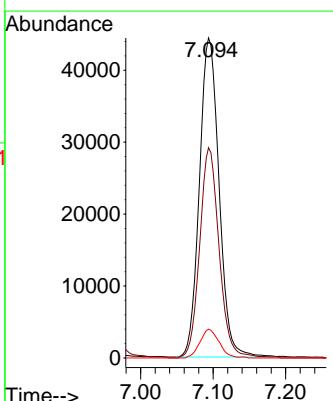

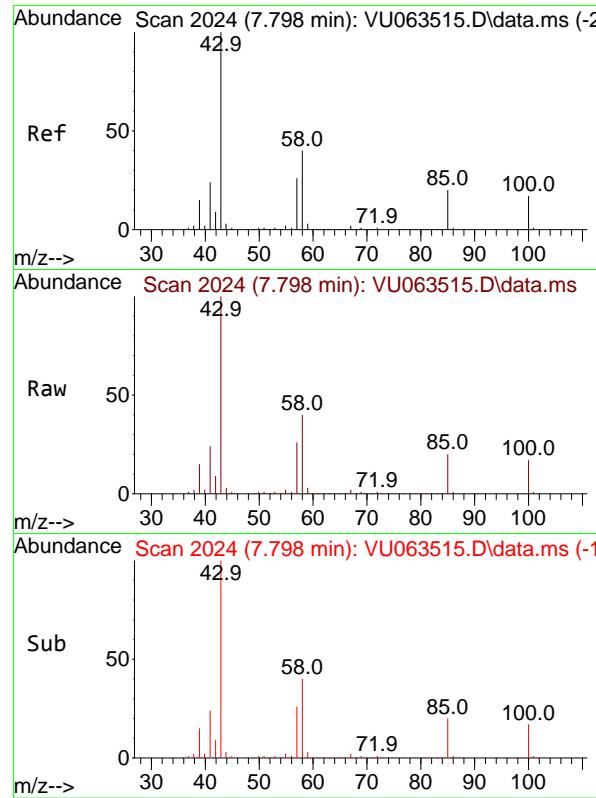


#45
 4-Methyl-2-Pentanone
 Concen: 51.766 ug/l
 RT: 7.798 min Scan# 2
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

ClientSampleId : VSTDICCC010


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

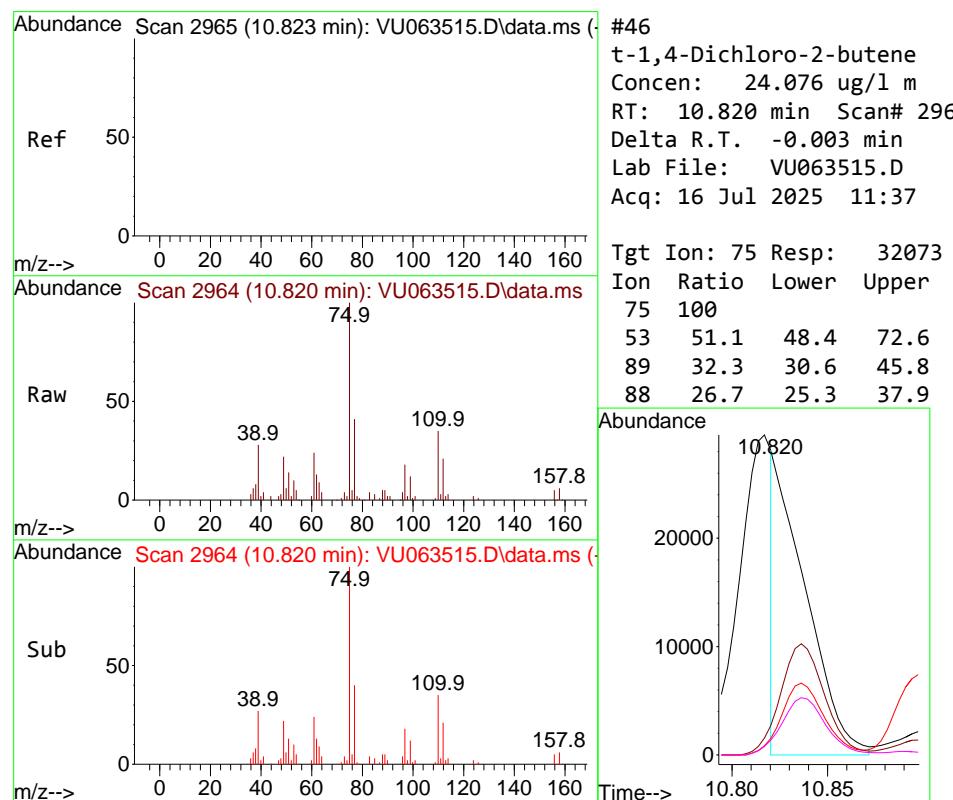

#46
 t-1,4-Dichloro-2-butene
 Concen: 24.076 ug/l m
 RT: 10.820 min Scan# 2964
 Delta R.T. -0.003 min
 Lab File: VU063515.D
 Acq: 16 Jul 2025 11:37

Tgt Ion: 75 Resp: 32073
 Ion Ratio Lower Upper
 75 100
 53 51.1 48.4 72.6
 89 32.3 30.6 45.8
 88 26.7 25.3 37.9

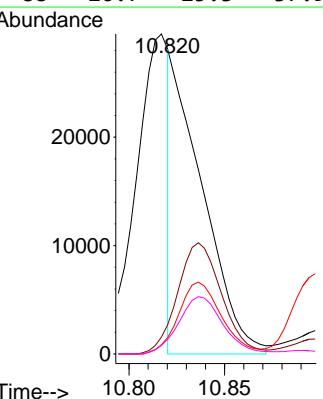



#47

Methyl methacrylate
Concen: 21.203 ug/l
RT: 6.962 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37





Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

Tgt Ion: 69 Resp: 64871

Ion	Ratio	Lower	Upper
69	100		
41	112.0	0.0	224.0
39	69.1	55.3	82.9
100	36.3	29.0	43.6

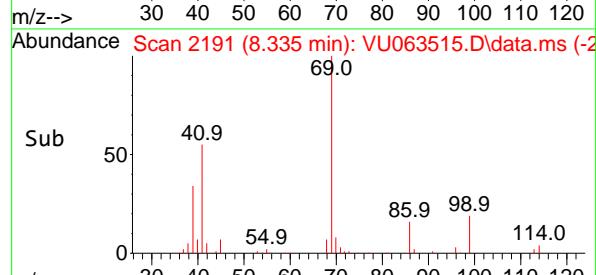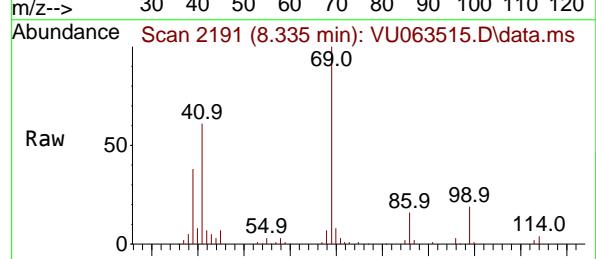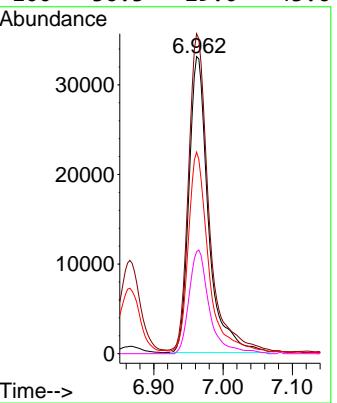



#48

Ethyl methacrylate
Concen: 11.020 ug/l
RT: 8.335 min Scan# 2191
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion: 69 Resp: 64347



Ion	Ratio	Lower	Upper
69	100		
41	61.6	30.8	92.4

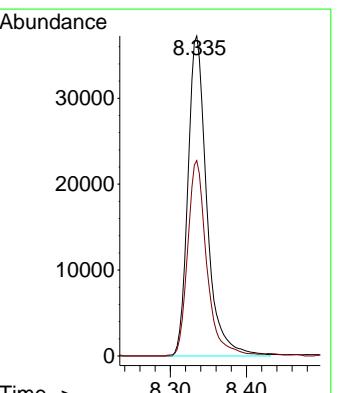



#49
Toluene
Concen: 10.432 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37



Instrument: MSVOA_U
ClientSampleId: VSTDICCC010




Tgt Ion: 92 Resp: 171140
Ion Ratio Lower Upper
92 100
91 175.5 140.4 210.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

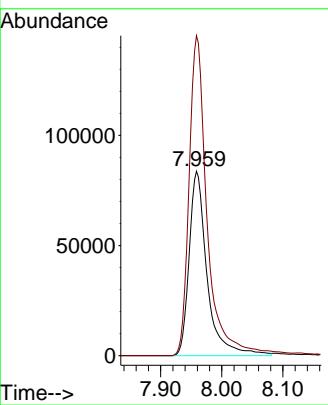


#50
t-1,3-Dichloropropene
Concen: 11.292 ug/l
RT: 8.203 min Scan# 2150
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37





Tgt Ion: 75 Resp: 72787
Ion Ratio Lower Upper
75 100
77 31.1 24.9 37.3

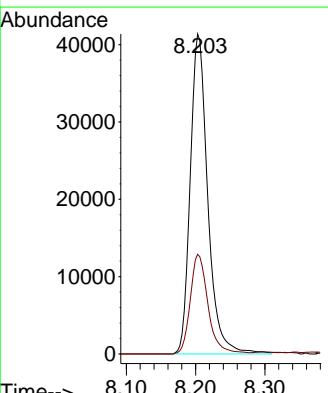



#51
cis-1,3-Dichloropropene
 Concen: 10.668 ug/l
 RT: 7.598 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063515.D
 Acq: 16 Jul 2025 11:37



Instrument : MSVOA_U
 ClientSampleId : VSTDICCC010

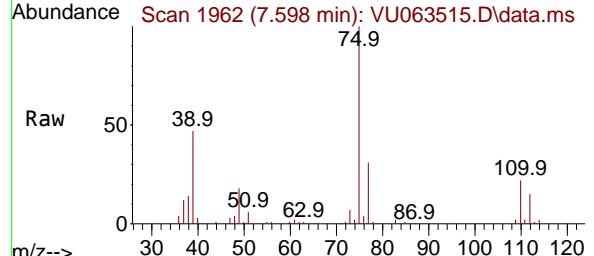


Tgt Ion: 75 Resp: 9230
 Ion Ratio Lower Upper
 75 100
 77 31.4 25.1 37.7
 39 47.2 37.8 56.6

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


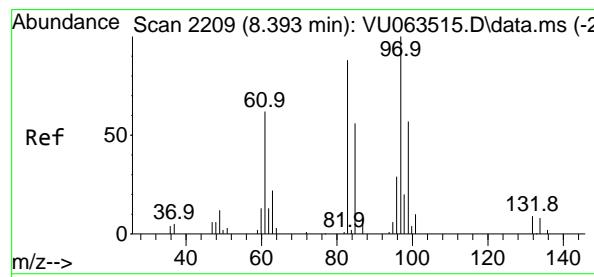



#52
 1,1,2-Trichloroethane
 Concen: 10.510 ug/l
 RT: 8.393 min Scan# 2209
 Delta R.T. 0.000 min
 Lab File: VU063515.D
 Acq: 16 Jul 2025 11:37



Tgt Ion: 97 Resp: 51547
 Ion Ratio Lower Upper
 97 100
 83 87.7 70.2 105.2
 85 56.5 45.2 67.8
 99 62.6 50.1 75.1

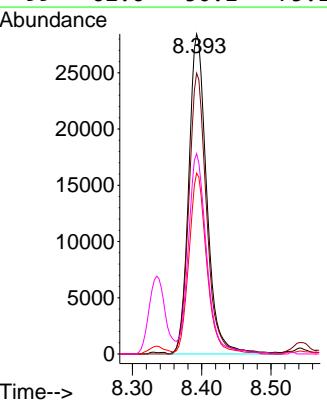

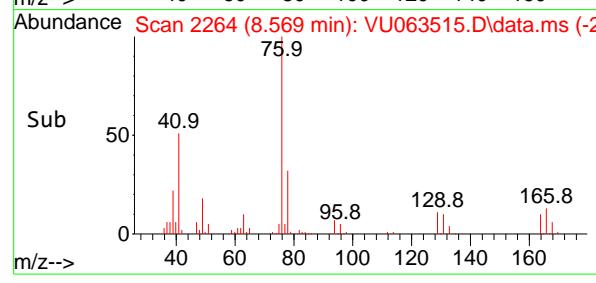

#53

1,3-Dichloropropane

Concen: 10.355 ug/l

RT: 8.569 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#54

2-Hexanone

Concen: 52.658 ug/l

RT: 8.688 min Scan# 2301

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion: 43 Resp: 131332




Ion Ratio Lower Upper

43 100

58 54.8 34.8 74.8

57 19.5 0.0 39.5

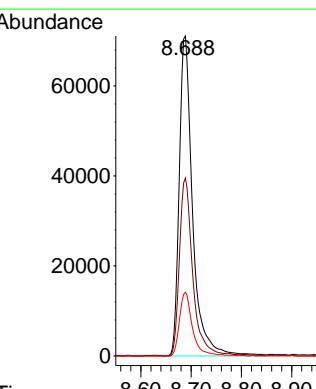






#55

Dibromochloromethane
Concen: 11.401 ug/l
RT: 8.801 min Scan# 2336
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025







#56

1,2-Dibromoethane
Concen: 10.388 ug/l
RT: 8.917 min Scan# 2372
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:107 Resp: 45601
Ion Ratio Lower Upper
107 100
109 93.2 0.0 186.4

Abundance

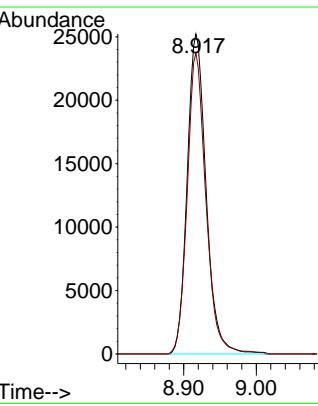



#57

4-Bromofluorobenzene

Concen: 0.975 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37





Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

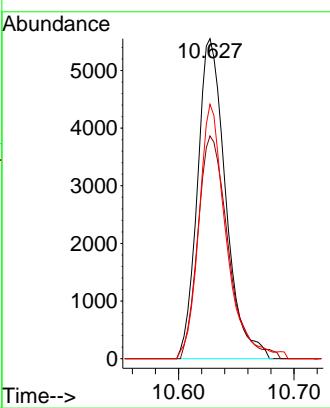 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#58

Tetrachloroethene

Concen: 10.376 ug/l


RT: 8.540 min Scan# 2255


Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Tgt	Ion:	164	Resp:	72806
Ion	Ratio	Lower	Upper	
164	100			
166	125.9	100.7	151.1	
129	100.7	80.6	120.8	
131	96.6	77.3	115.9	

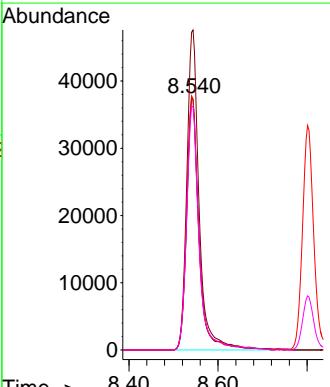


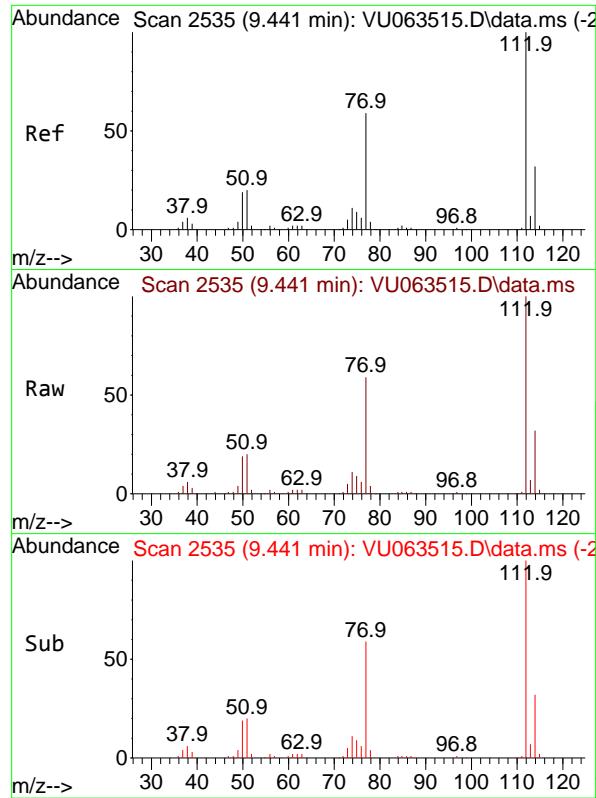


#59
Chlorobenzene
Concen: 10.443 ug/l
RT: 9.441 min Scan# 2
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

ClientSampleId : VSTDICCC010


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

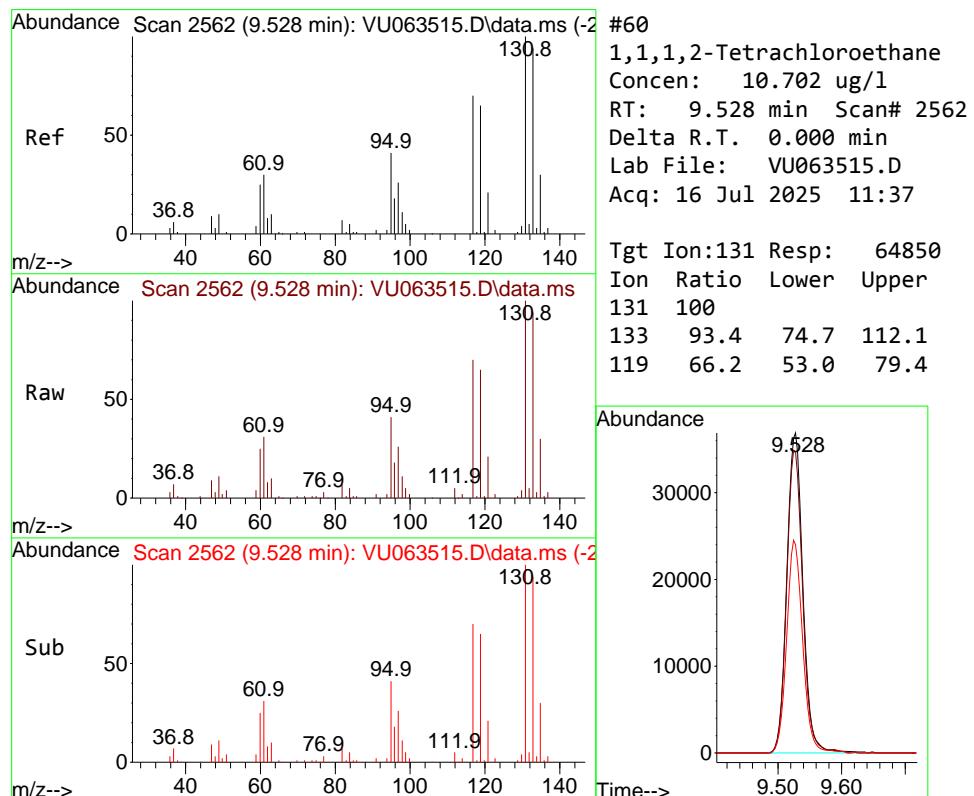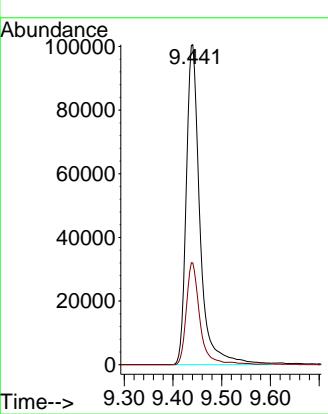

#60
1,1,1,2-Tetrachloroethane
Concen: 10.702 ug/l
RT: 9.528 min Scan# 2562
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:131 Resp: 64850
Ion Ratio Lower Upper
131 100
133 93.4 74.7 112.1
119 66.2 53.0 79.4





#61

Pentachloroethane

Concen: 11.097 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument :

MSVOA_U





ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

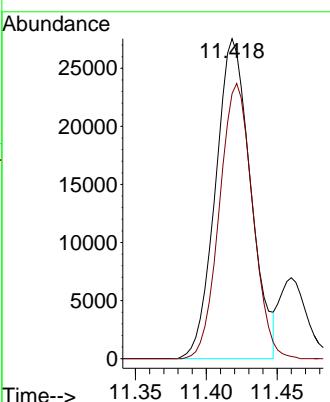

#62

Hexachloroethane


Concen: 11.561 ug/l




RT: 12.466 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

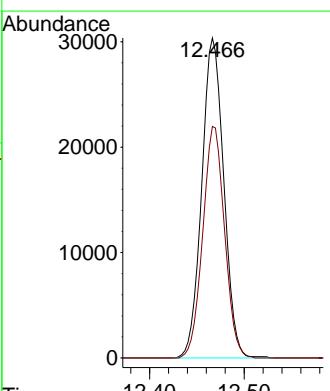Tgt Ion:117 Resp: 49020
Ion Ratio Lower Upper
117 100
201 71.7 57.4 86.0




#63

Ethyl Benzene

Concen: 10.340 ug/l

RT: 9.563 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




Instrument:

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#64

m/p-Xylenes

Concen: 21.007 ug/l

RT: 9.685 min Scan# 2611

Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37


Tgt Ion:106 Resp: 264769

Ion Ratio Lower Upper

106 100

91 204.5 163.6 245.4




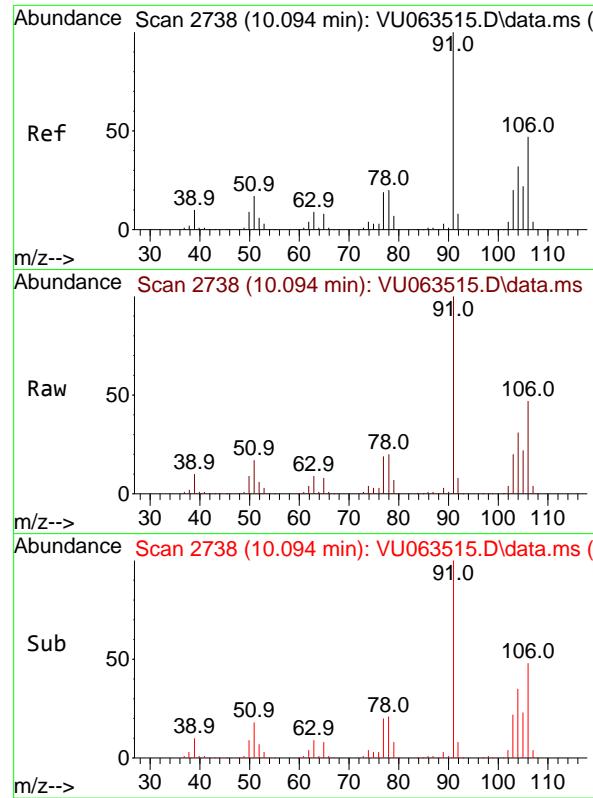


#65
o-Xylene
Concen: 10.621 ug/l
RT: 10.094 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument :
MSVOA_U
ClientSampleId :
VSTDICCC010


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

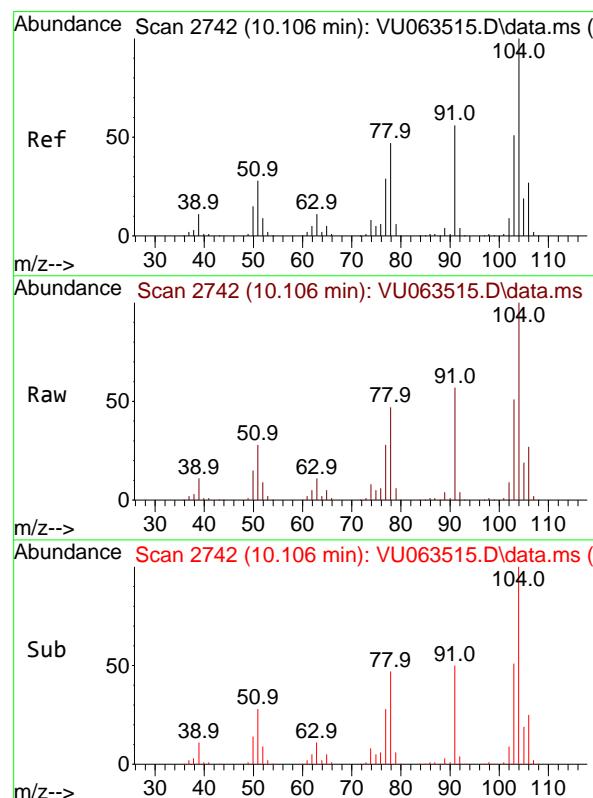

#66
Styrene
Concen: 10.873 ug/l
RT: 10.106 min Scan# 2742
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:104 Resp: 209876
Ion Ratio Lower Upper
104 100
78 51.6 41.3 61.9
103 54.5 43.6 65.4

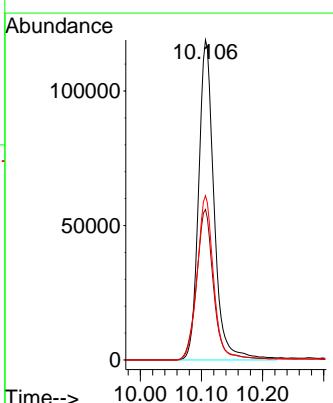



#67

Bromoform

Concen: 11.325 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37





Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

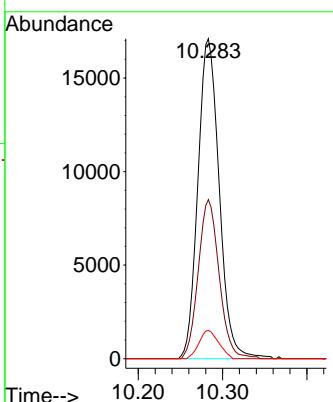 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.024 ug/l

RT: 12.187 min Scan# 3389

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Tgt

Ion:

152

100

Ion:

115

131.1

Ion:

150

325.6

Lower

0.0

262.2


0.0




651.2

Upper

Resp:

9149





#69

Isopropylbenzene

Concen: 10.718 ug/l

RT: 10.476 min Scan# 2

Instrument :

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 10.373 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37



Tgt Ion: 83 Resp: 61909




Ion Ratio Lower Upper

83 100

131 10.5 8.4 12.6

85 64.9 51.9 77.9

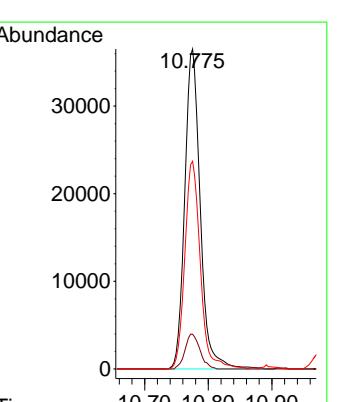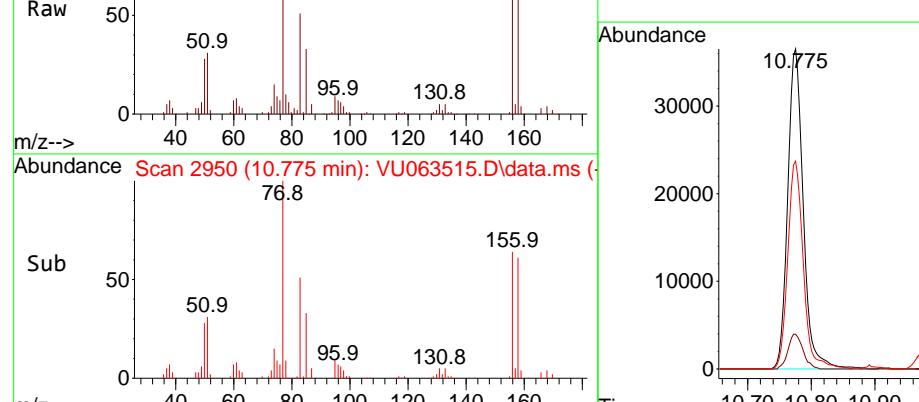



#71

1,2,3-Trichloropropane

Concen: 10.893 ug/l m

RT: 10.817 min Scan# 2963

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37




Instrument:

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#72

Bromobenzene

Concen: 10.441 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion:156 Resp: 78897


Ion Ratio Lower Upper

156 100

77 157.6 0.0 315.2

158 97.7 0.0 195.4

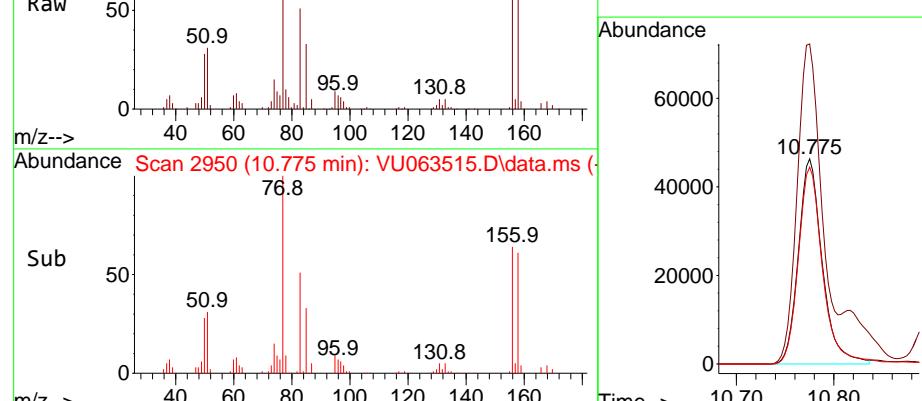


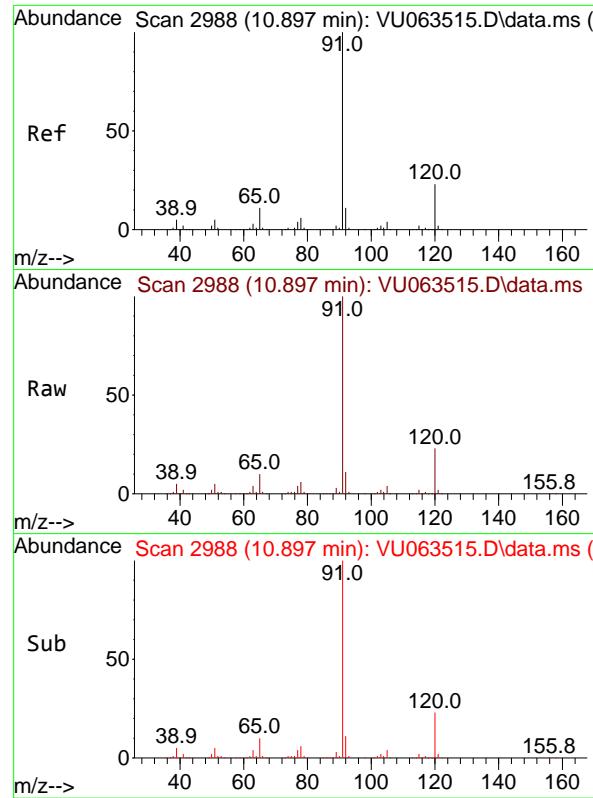


#73
n-propylbenzene
Concen: 10.853 ug/l
RT: 10.897 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

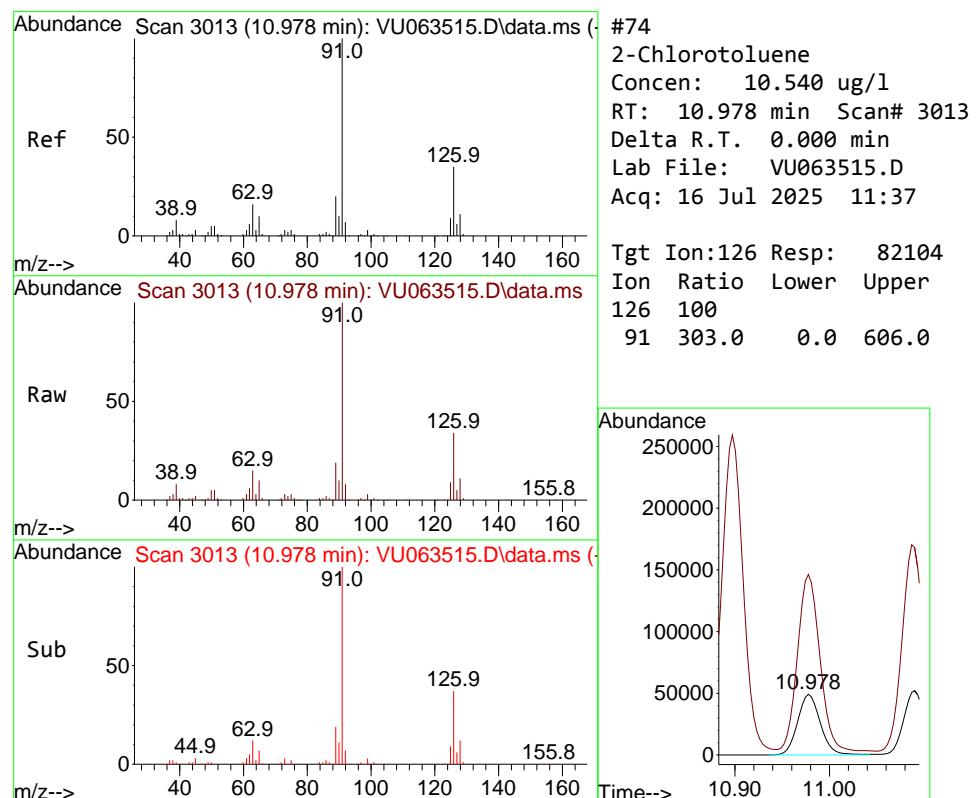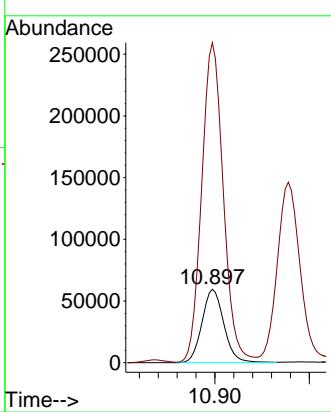

#74
2-Chlorotoluene
Concen: 10.540 ug/l
RT: 10.978 min Scan# 3013
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:126 Resp: 82104
Ion Ratio Lower Upper
126 100
91 303.0 0.0 606.0

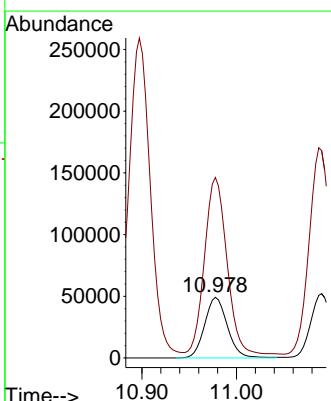

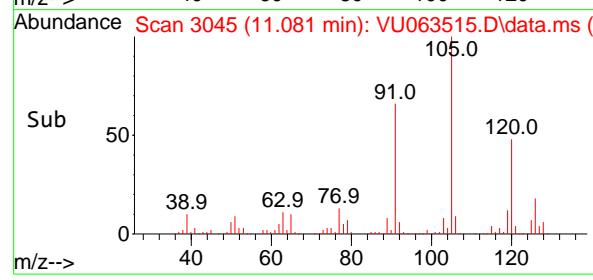

#75

1,3,5-Trimethylbenzene

Concen: 10.778 ug/l

RT: 11.081 min Scan# 3045

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37





Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#76

4-Chlorotoluene


Concen: 10.636 ug/l




RT: 11.090 min Scan# 3048

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

 Tgt Ion:126 Resp: 84140
 Ion Ratio Lower Upper
 126 100
 91 341.1 0.0 682.2




#77

tert-Butylbenzene

Concen: 10.714 ug/l

RT: 11.412 min Scan# 3148

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37





Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

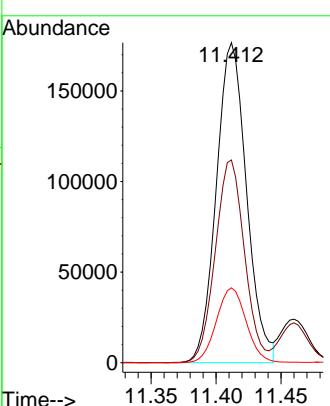 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#78

1,2,4-Trimethylbenzene

Concen: 10.824 ug/l

RT: 11.460 min Scan# 3163

Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37


Tgt Ion:105 Resp: 300364

Ion Ratio Lower Upper



105 100

120 45.3 22.7 68.0

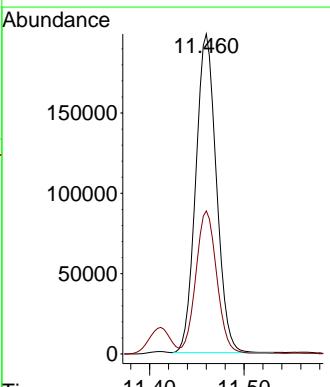




Abundance Scan 3217 (11.634 min): VU063515.D\data.ms (-)

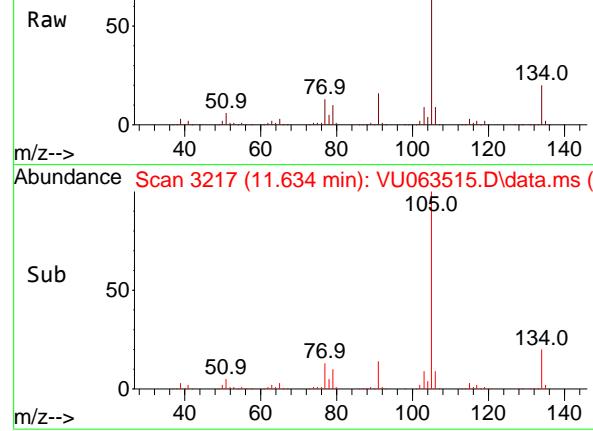

Abundance Scan 3705 (13.203 min): VU063515.D\data.ms (-)

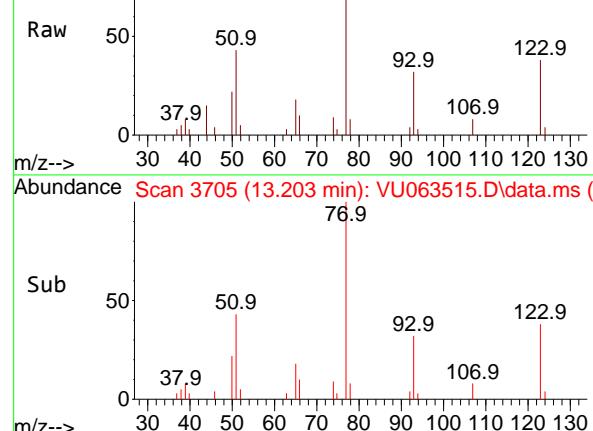

Abundance Scan 3705 (13.203 min): VU063515.D\data.ms (-)

#79

sec-Butylbenzene

Concen: 10.724 ug/l

RT: 11.634 min Scan# 3

Instrument : MSVOA_U


Delta R.T. 0.000 min

Lab File: VU063515.D


Acq: 16 Jul 2025 11:37

ClientSampleId :


VSTDICCC010



Abundance Scan 3264 (11.785 min): VU063515.D\data.ms (-)

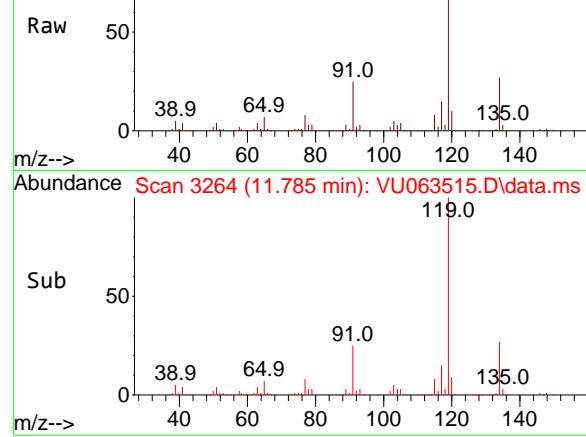

Abundance Scan 3264 (11.785 min): VU063515.D\data.ms (-)

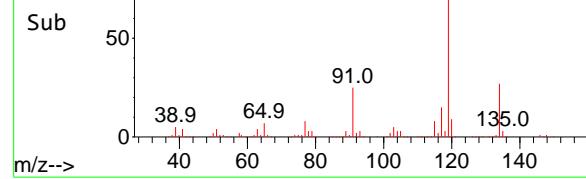

#81

p-Isopropyltoluene

Concen: 10.808 ug/l

RT: 11.785 min Scan# 3264

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument :

MSVOA_U


ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025

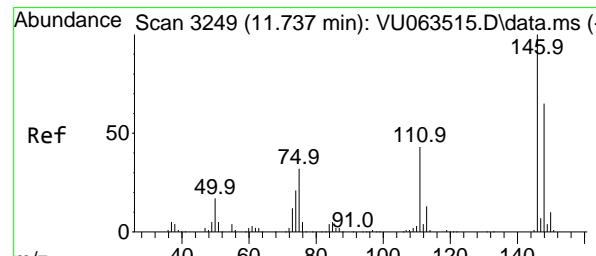

Abundance Scan 3249 (11.737 min): VU063515.D\data.ms (-)



Abundance Scan 3249 (11.737 min): VU063515.D\data.ms (-)

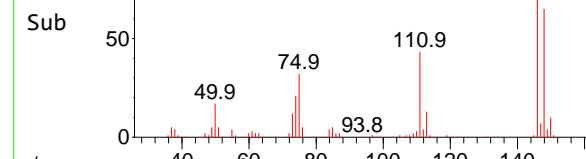

#82

1,3-Dichlorobenzene

Concen: 10.603 ug/l

RT: 11.737 min Scan# 3249

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion:146 Resp: 160312


Ion Ratio Lower Upper

Tgt Ion	Ion Ratio	Lower	Upper
146	100		
111	42.2	33.8	50.6
148	64.4	51.5	77.3

Abundance Scan 3249 (11.737 min): VU063515.D\data.ms (-)

Abundance

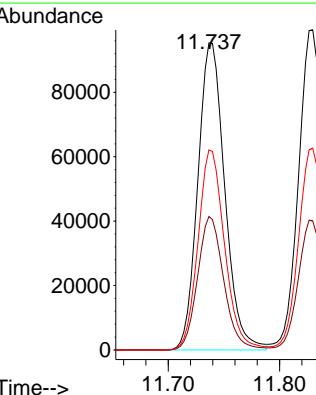


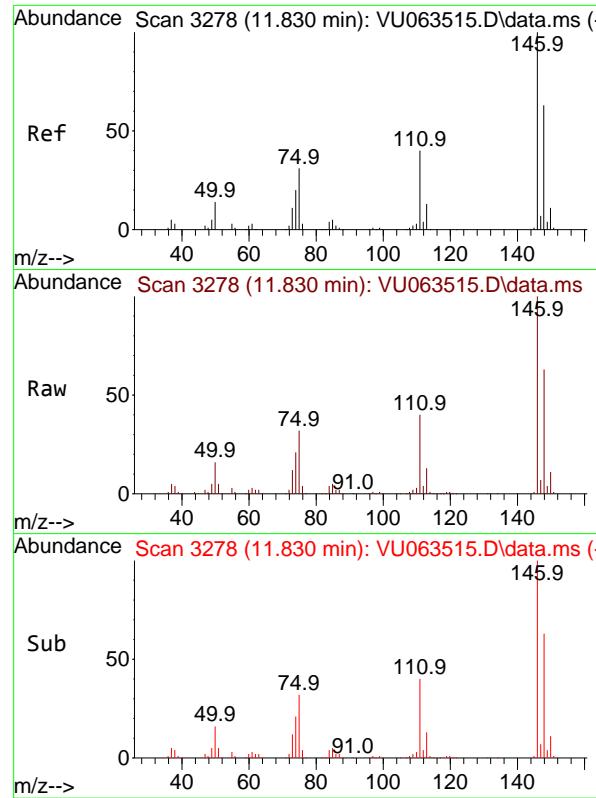


#83
1,4-Dichlorobenzene
Concen: 10.702 ug/l
RT: 11.830 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

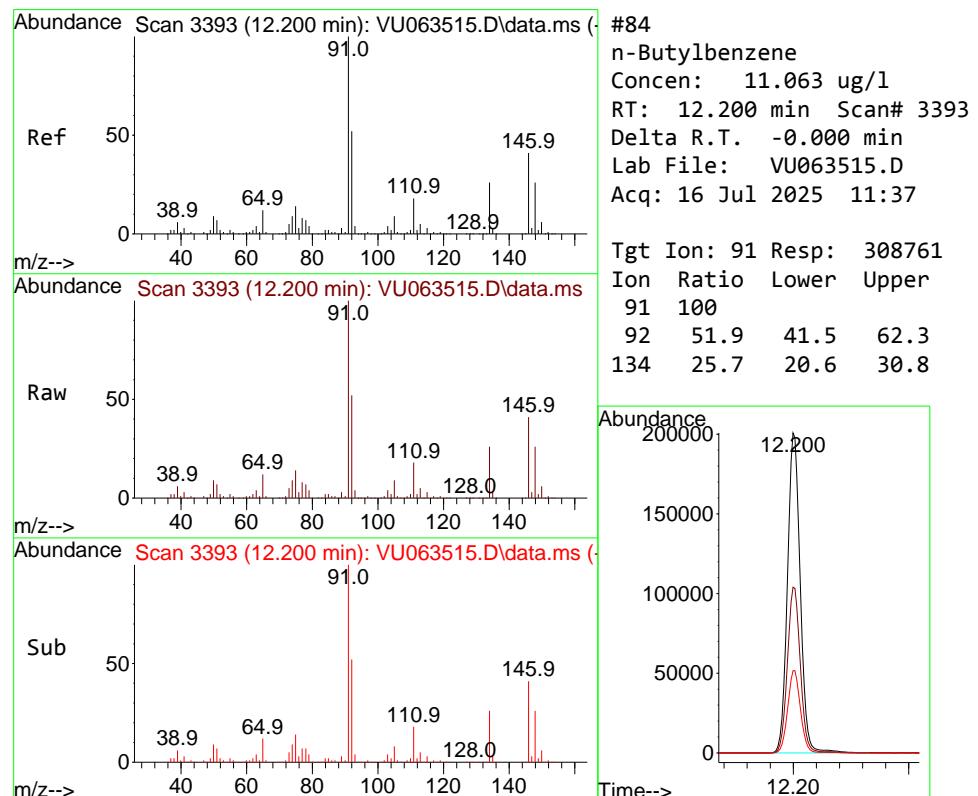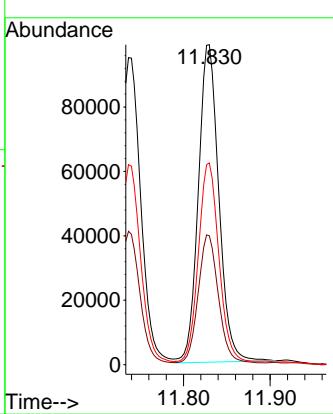

#84
n-Butylbenzene
Concen: 11.063 ug/l
RT: 12.200 min Scan# 3393
Delta R.T. -0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion: 91 Resp: 308761
Ion Ratio Lower Upper
91 100
92 51.9 41.5 62.3
134 25.7 20.6 30.8

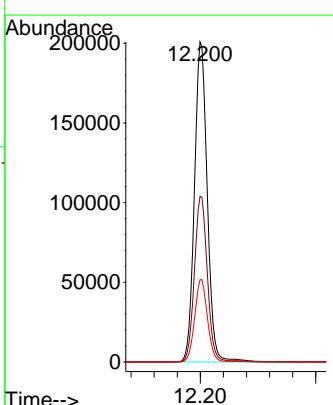

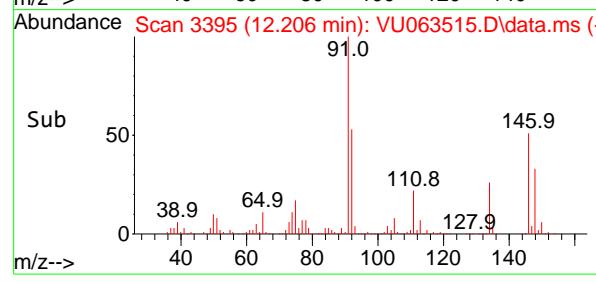

#85

1,2-Dichlorobenzene

Concen: 10.716 ug/l

RT: 12.206 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument :

MSVOA_U

ClientSampleId :

VSTDICCC010

Tgt Ion:146 Resp: 152203

Ion Ratio Lower Upper

146 100




111 43.4 21.7 65.1

148 63.5 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 10.093 ug/l

RT: 12.987 min Scan# 3638

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion: 75 Resp: 10205


Ion Ratio Lower Upper

75 100

155 82.2 65.8 98.6

157 101.8 81.4 122.2




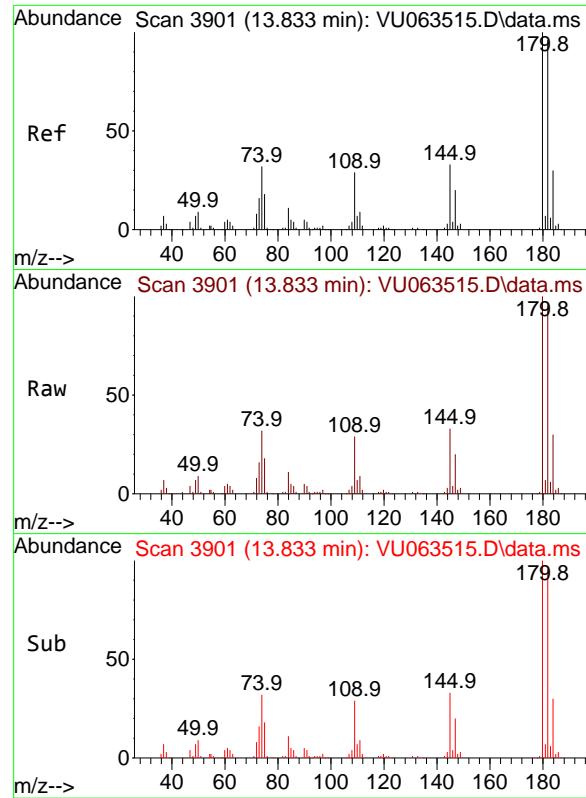


#87
1,2,4-Trichlorobenzene
Concen: 11.107 ug/l
RT: 13.833 min Scan# 3901
Delta R.T. -0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Instrument : MSVOA_U
ClientSampleId : VSTDICCC010


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

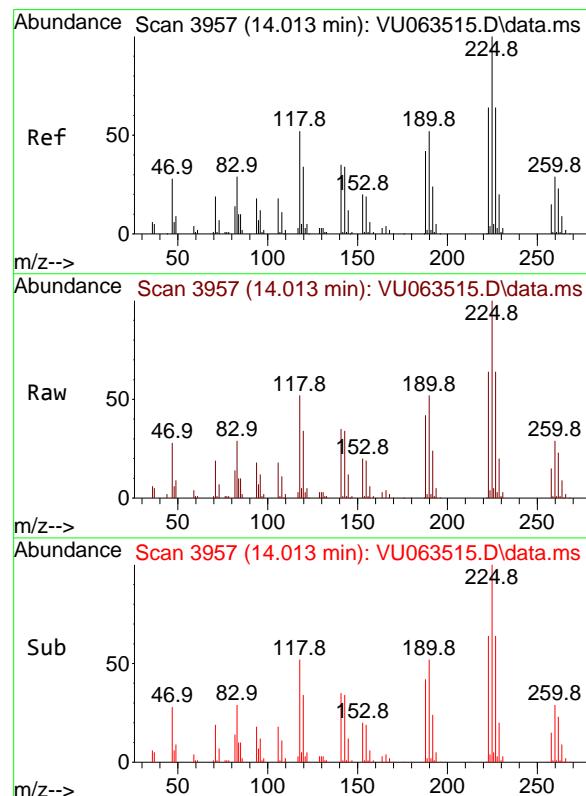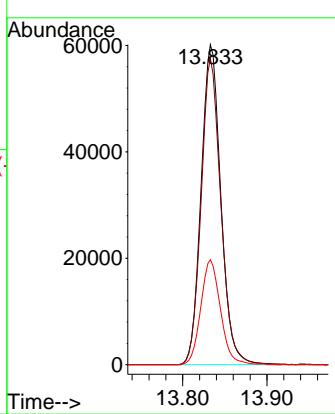

#88
Hexachlorobutadiene
Concen: 10.718 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063515.D
Acq: 16 Jul 2025 11:37

Tgt Ion:225 Resp: 53764
Ion Ratio Lower Upper
225 100
223 63.5 50.8 76.2
227 63.8 51.0 76.6

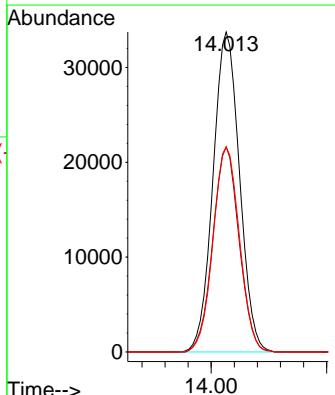

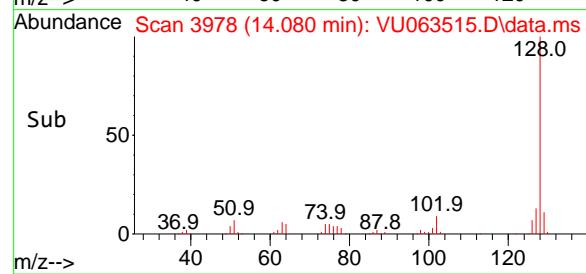

#89

Naphthalene

Concen: 10.937 ug/l

RT: 14.080 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37

Instrument:

MSVOA_U





ClientSampleId :

VSTDICCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

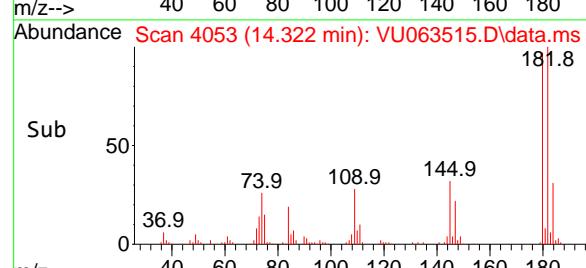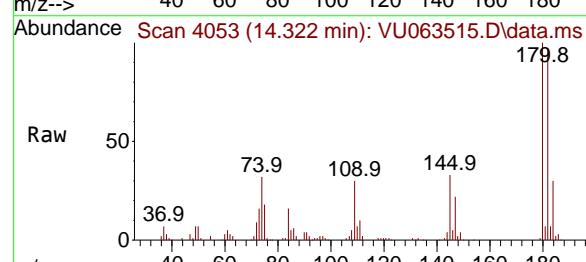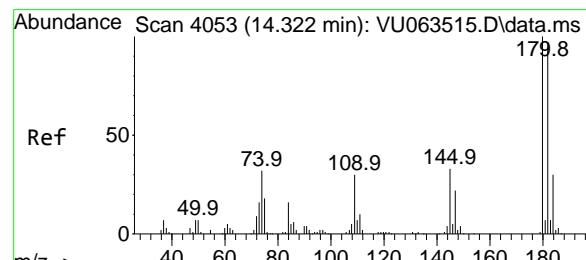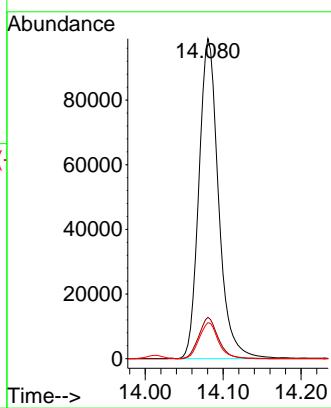

#90

1,2,3-Trichlorobenzene

Concen: 11.015 ug/l

RT: 14.322 min Scan# 4053

Delta R.T. 0.000 min

Lab File: VU063515.D

Acq: 16 Jul 2025 11:37


Tgt Ion:180 Resp: 89908

Ion Ratio Lower Upper

180 100

182 97.5 78.0 117.0

145 34.1 27.3 40.9

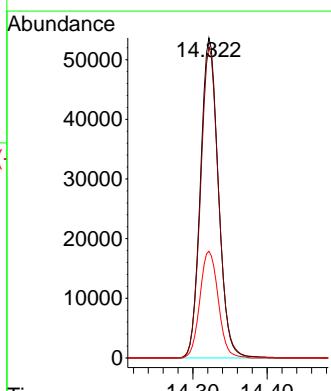

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063516.D
 Acq On : 16 Jul 2025 12:11
 Operator : MD/SY
 Sample : VSTDICC015
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC015

Quant Time: Jul 17 03:26:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.100	96	24893	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	9905	1.051	ug/l	0.00
Spiked Amount 1.000			Recovery	=	105.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	9748	1.118	ug/l	0.00
Spiked Amount 1.000			Recovery	=	112.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	118195	16.103	ug/l	100
3) Chloromethane	1.519	50	106285	15.578	ug/l	100
4) Vinyl Chloride	1.596	62	140324	16.148	ug/l	99
5) Bromomethane	1.837	94	94776	14.463	ug/l	99
6) Chloroethane	1.920	64	84236	16.055	ug/l	99
7) Trichlorofluoromethane	2.126	101	198726	15.928	ug/l	98
8) 1,1,2-Trichloro-1,2,2-...	2.567	101	103637	15.895	ug/l	99
9) 1,1-Dichloroethene	2.567	96	102475	15.857	ug/l	98
10) Iodomethane	2.708	142	154304	15.423	ug/l	99
11) Allyl Chloride	2.908	41	149875	16.053	ug/l	99
12) Acrylonitrile	3.303	53	46936	29.022	ug/l	96
13) Acetone	2.618	43	114282	88.245	ug/l	99
14) Carbon Disulfide	2.776	76	336090	16.100	ug/l	99
15) Methylene Chloride	3.030	84	115170	15.136	ug/l	99
16) trans-1,2-Dichloroethene	3.335	96	115592	15.749	ug/l	99
17) 1,1-Dichloroethane	3.850	63	213678	15.707	ug/l	99
18) 2-Butanone	4.708	43	167820	83.678	ug/l	100
19) Cyclohexane	5.364	56	180806	15.697	ug/l	98
20) Methylcyclohexane	6.743	83	193667	17.299	ug/l	99
21) 2,2-Dichloropropane	4.644	77	182585	15.761	ug/l	99
22) cis-1,2-Dichloroethene	4.650	96	125136	15.711	ug/l	99
23) Diethyl Ether	2.367	59	79700	16.184	ug/l	98
24) tert-Butyl Alcohol	3.187	59	95177	160.102	ug/l	99
25) Methyl tert-Butyl Ether	3.358	73	271458	16.090	ug/l	100
26) Bromochloromethane	4.956	128	54202	16.299	ug/l	99
27) Chloroform	5.071	83	217821	15.691	ug/l	99
28) 1,1,1-Trichloroethane	5.296	97	188574	16.005	ug/l	99
29) 1,1-Dichloropropene	5.505	75	174673	16.004	ug/l	98
30) Carbon Tetrachloride	5.502	117	162285	17.113	ug/l	96
31) Isopropyl Ether	3.991	45	323879	15.772	ug/l	98
32) Ethyl-t-butyl ether	4.502	59	302903	15.939	ug/l	98
33) Tert-Amyl methyl ether	5.940	73	268560	16.283	ug/l	99
34) Propionitrile	4.772	54	45659	74.722	ug/l	97
35) Benzene	5.756	78	473682	16.153	ug/l	99
36) 1,2-Dichloroethane	5.782	62	147295	16.165	ug/l	99
37) Trichloroethene	6.525	130	128676	17.198	ug/l	98
38) 1,2-Dichloropropane	6.779	63	124831	18.188	ug/l	100
39) Methacrylonitrile	4.972	41	39512	14.730	ug/l	99
40) Methyl acrylate	4.843	55	65123	16.402	ug/l	99
41) Tetrahydrofuran	5.059	42	40858	28.595	ug/l	100
42) 1-Chlorobutane	5.438	56	232046	15.991	ug/l	99
43) Dibromomethane	6.904	93	62716	17.639	ug/l	99
44) Bromodichloromethane	7.094	83	144794	18.058	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063516.D
 Acq On : 16 Jul 2025 12:11
 Operator : MD/SY
 Sample : VSTDICC015
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC015

Quant Time: Jul 17 03:26:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.795	43	310822	84.821	ug/l	100
46) t-1,4-Dichloro-2-butene	10.824	75	41713m	32.085	ug/l	
47) Methyl methacrylate	6.962	69	114716	38.417	ug/l	98
48) Ethyl methacrylate	8.335	69	101021	17.728	ug/l	99
49) Toluene	7.959	92	268202	16.751	ug/l	99
50) t-1,3-Dichloropropene	8.203	75	116990	18.597	ug/l	97
51) cis-1,3-Dichloropropene	7.595	75	168909	20.004	ug/l	100
52) 1,1,2-Trichloroethane	8.393	97	78885	16.480	ug/l	99
53) 1,3-Dichloropropane	8.566	76	135862	16.441	ug/l	100
54) 2-Hexanone	8.689	43	213057	87.533	ug/l	99
55) Dibromochloromethane	8.801	129	92530	18.292	ug/l	98
56) 1,2-Dibromoethane	8.917	107	70483	16.452	ug/l	98
58) Tetrachloroethene	8.541	164	110328	16.111	ug/l	98
59) Chlorobenzene	9.441	112	309351	16.822	ug/l	100
60) 1,1,1,2-Tetrachloroethane	9.525	131	101862	17.225	ug/l	98
61) Pentachloroethane	11.418	117	77252	18.487	ug/l	99
62) Hexachloroethane	12.467	117	79431	19.195	ug/l	99
63) Ethyl Benzene	9.563	91	525757	16.614	ug/l	99
64) m/p-Xylenes	9.685	106	421278	34.249	ug/l	100
65) o-Xylene	10.091	106	205249	17.365	ug/l	98
66) Styrene	10.107	104	336001	17.837	ug/l	100
67) Bromoform	10.283	173	48978	18.852	ug/l	99
69) Isopropylbenzene	10.476	105	492082	17.221	ug/l	99
70) 1,1,2,2-Tetrachloroethane	10.775	83	98628	16.933	ug/l	100
71) 1,2,3-Trichloropropane	10.817	75	76288m	16.049	ug/l	
72) Bromobenzene	10.775	156	128042	17.363	ug/l	97
73) n-propylbenzene	10.898	120	149954	17.433	ug/l	100
74) 2-Chlorotoluene	10.978	126	130274	17.136	ug/l	98
75) 1,3,5-Trimethylbenzene	11.081	105	478010	17.511	ug/l	99
76) 4-Chlorotoluene	11.090	126	132384	17.147	ug/l	98
77) tert-Butylbenzene	11.412	119	450846	17.282	ug/l	100
78) 1,2,4-Trimethylbenzene	11.460	105	473538	17.485	ug/l	99
79) sec-Butylbenzene	11.634	105	612652	17.415	ug/l	99
80) Nitrobenzene	13.203	77	11188	74.783	ug/l	94
81) p-Isopropyltoluene	11.785	119	516607	17.591	ug/l	99
82) 1,3-Dichlorobenzene	11.737	146	254102	17.221	ug/l	99
83) 1,4-Dichlorobenzene	11.830	146	265531	17.978	ug/l	98
84) n-Butylbenzene	12.200	91	492464	18.081	ug/l	100
85) 1,2-Dichlorobenzene	12.203	146	242217	17.474	ug/l	100
86) 1,2-Dibromo-3-Chloropr...	12.988	75	16421	14.975	ug/l	98
87) 1,2,4-Trichlorobenzene	13.833	180	158574	18.396	ug/l	99
88) Hexachlorobutadiene	14.013	225	86303	17.630	ug/l	99
89) Naphthalene	14.077	128	292967	18.966	ug/l	100
90) 1,2,3-Trichlorobenzene	14.322	180	149249	18.735	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063516.D
Acq On : 16 Jul 2025 12:11
Operator : MD/SY
Sample : VSTDIICC015
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1


Quant Time: Jul 17 03:26:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:16:16 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VSTDICC015

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

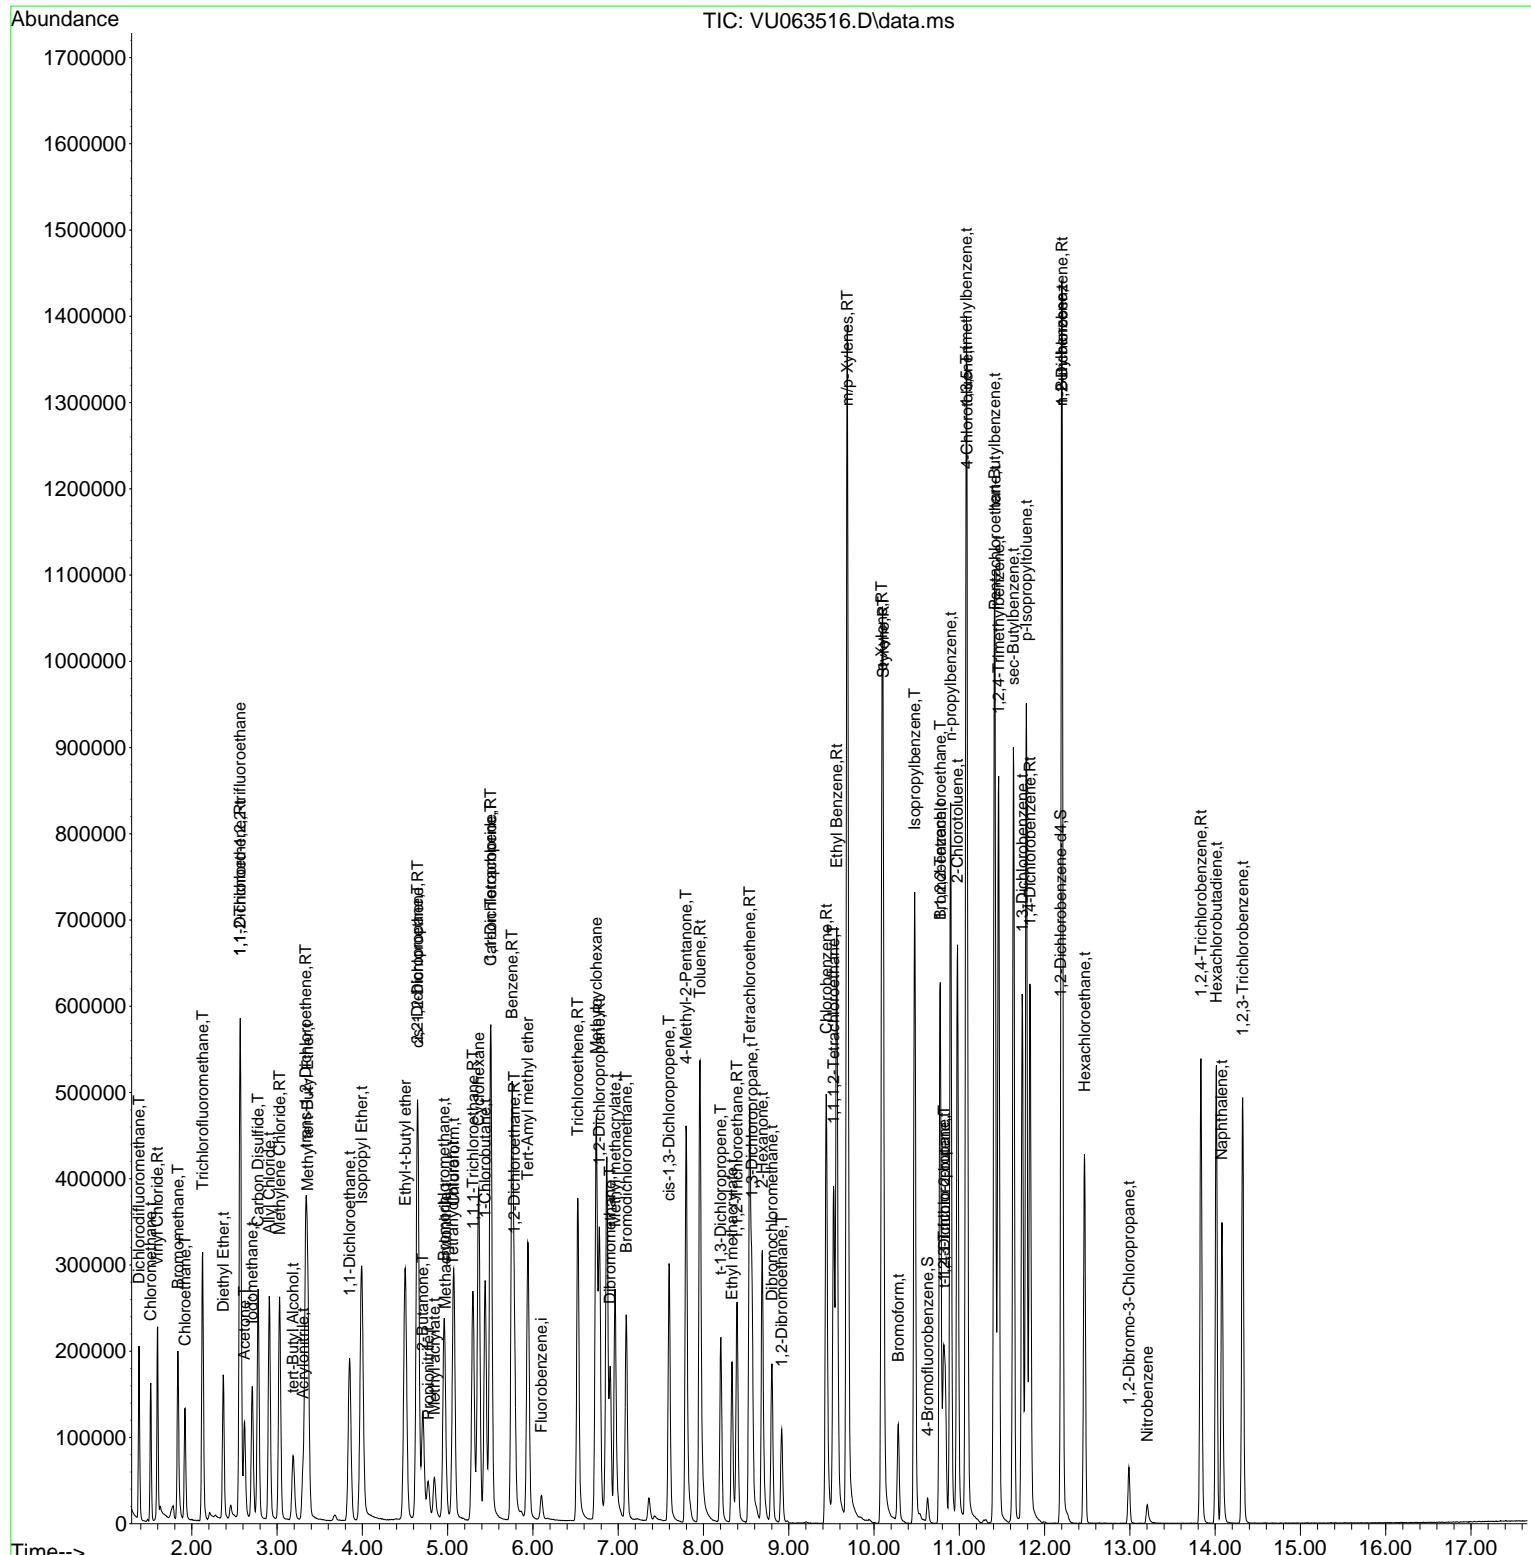

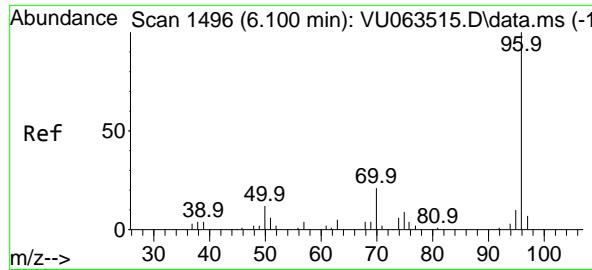

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Instrument : MSVOA_U
ClientSampleId : VSTDICC015

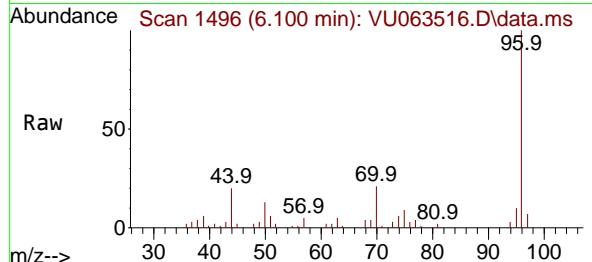


Tgt Ion: 96 Resp: 24891
Ion Ratio Lower Upper
96 100
70 19.2 15.0 22.4
95 0.0 7.4 11.0
97 0.0 0.0 0.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

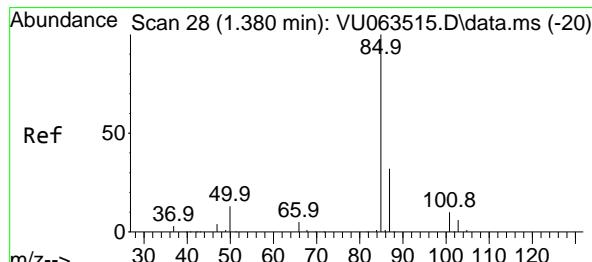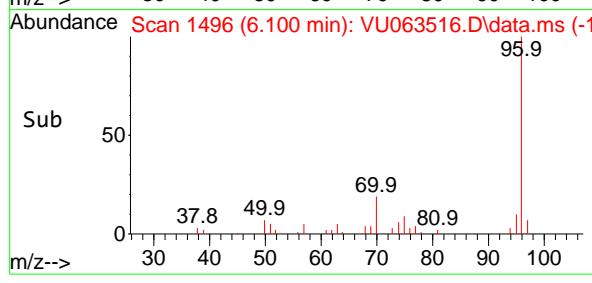


#2
Dichlorodifluoromethane
Concen: 16.103 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

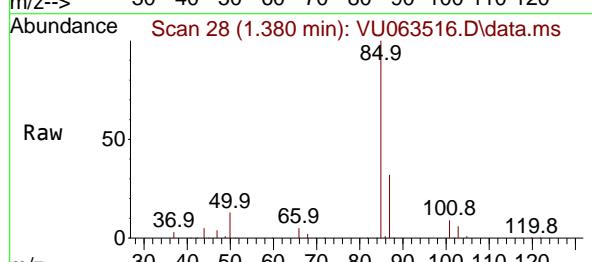


Tgt Ion: 85 Resp: 118195
Ion Ratio Lower Upper
85 100
87 32.0 16.0 47.9

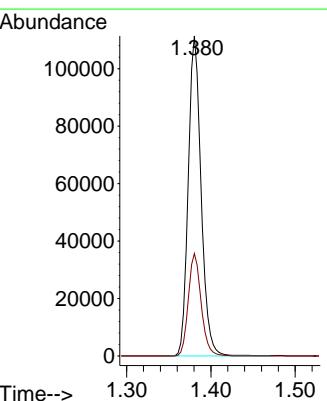
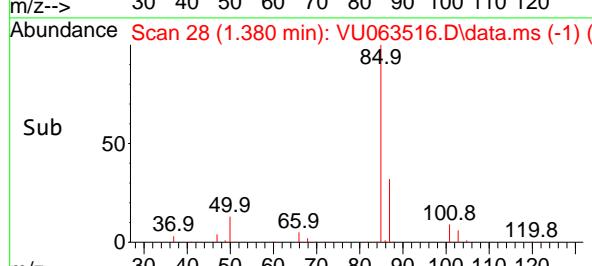





Ref Scan 71 (1.519 min): VU063516.D\data.ms

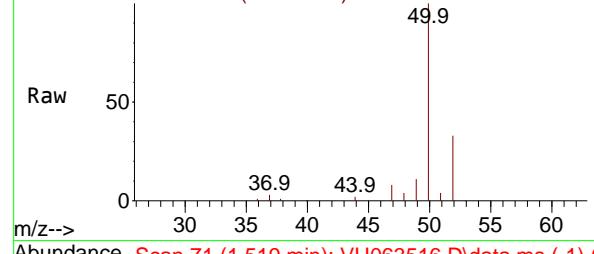


Raw Scan 71 (1.519 min): VU063516.D\data.ms

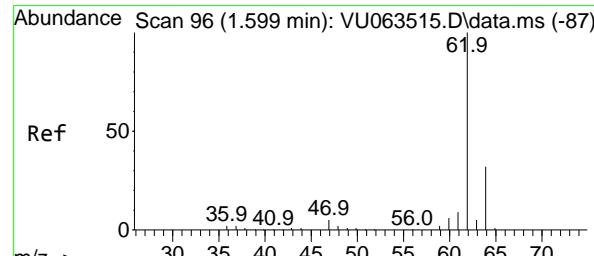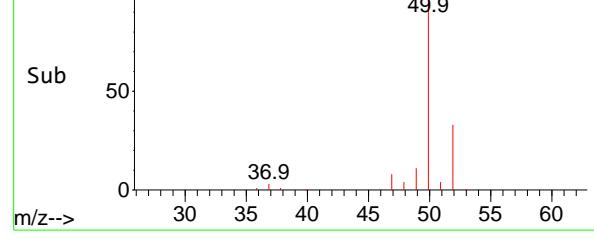

Ref Scan 95 (1.596 min): VU063516.D\data.ms

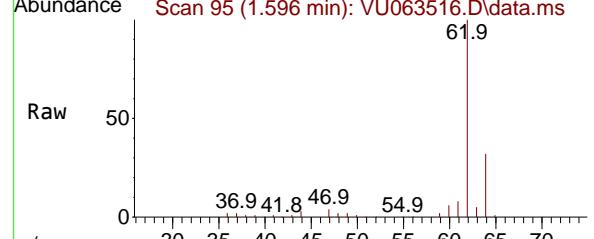

Raw Scan 95 (1.596 min): VU063516.D\data.ms (-1)

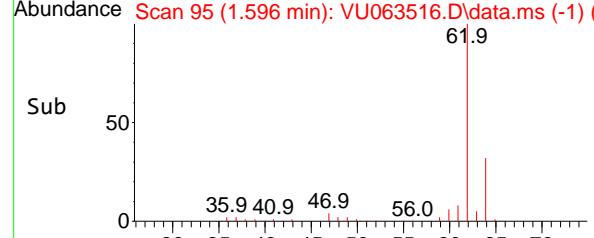

#3

Chloromethane

Concen: 15.578 ug/l

RT: 1.519 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

Tgt Ion: 50 Resp: 10628

Ion Ratio Lower Upper


50 100

52 33.1 26.3 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

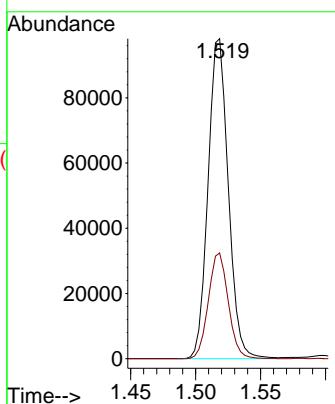


#4
Vinyl Chloride
Concen: 16.148 ug/l
RT: 1.596 min Scan# 95
Delta R.T. -0.003 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Tgt Ion: 62 Resp: 140324

Ion Ratio Lower Upper

62 100

64 32.5 25.7 38.5

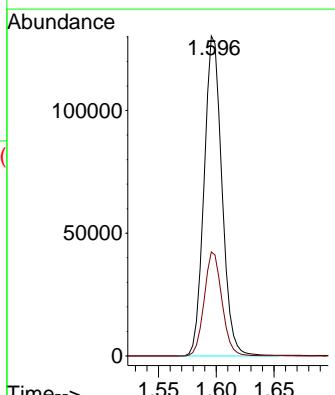



#5

Bromomethane

Concen: 14.463 ug/l

RT: 1.837 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

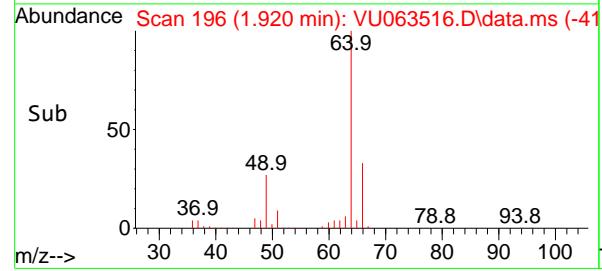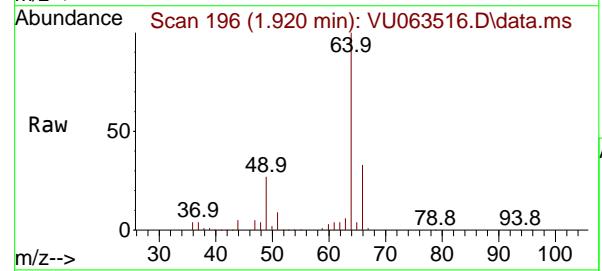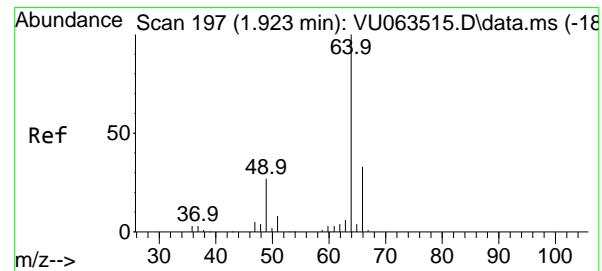 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#6

Chloroethane


Concen: 16.055 ug/l


RT: 1.920 min Scan# 196

Delta R.T. -0.003 min



Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

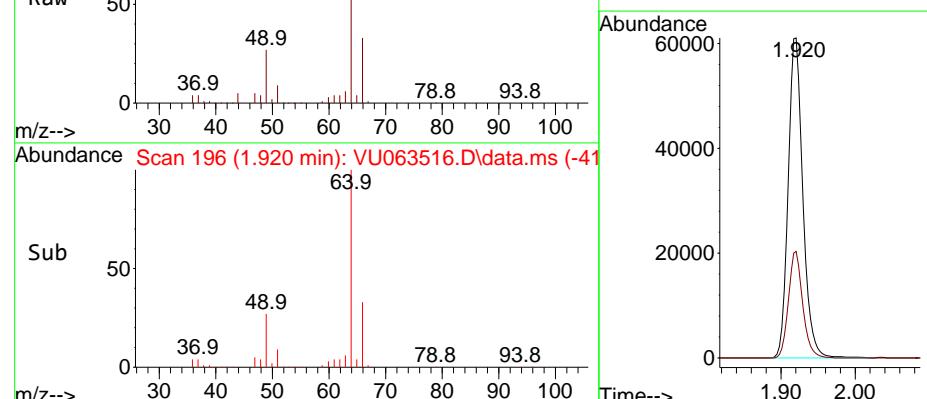 Tgt Ion: 64 Resp: 84236
 Ion Ratio Lower Upper
 64 100
 66 33.3 26.2 39.4




Ref Scan 260 (2.126 min): VU063516.D\data.ms

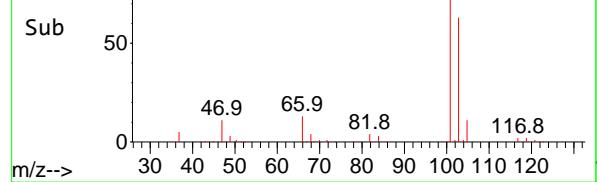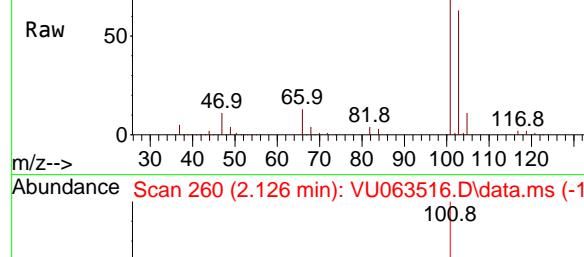



#7

Trichlorofluoromethane
Concen: 15.928 ug/l
RT: 2.126 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11



Instrument : MSVOA_U
ClientSampleId : VSTDICC015

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

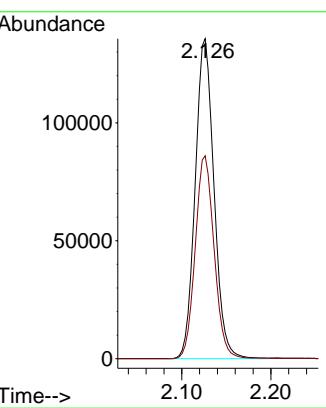


Ref Scan 397 (2.567 min): VU063516.D\data.ms

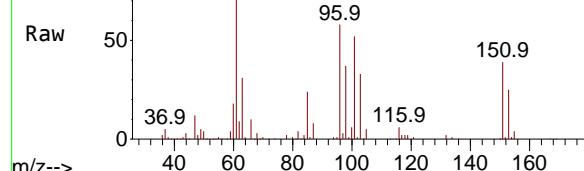


#8

1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 15.895 ug/l
RT: 2.567 min Scan# 397
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11


Tgt Ion:101 Resp: 103637
Ion Ratio Lower Upper
101 100
85 47.1 37.8 56.6
151 75.9 59.2 88.8

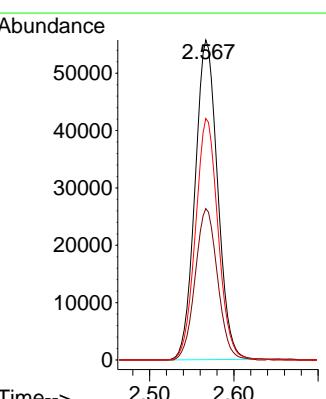



#9
1,1-Dichloroethene
Concen: 15.857 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Instrument : MSVOA_U
ClientSampleId : VSTDICC015




Tgt Ion: 96 Resp: 102475
Ion Ratio Lower Upper
96 100
61 172.3 0.0 504.3
98 63.7 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

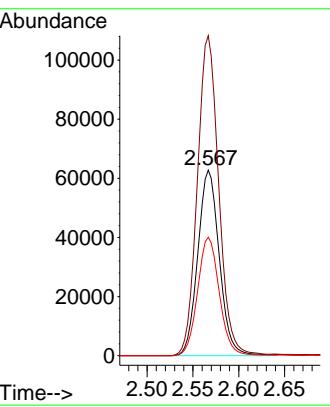


#10
Iodomethane
Concen: 15.423 ug/l
RT: 2.708 min Scan# 441
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Tgt Ion:142 Resp: 154304
Ion Ratio Lower Upper
142 100
127 48.2 37.9 56.9

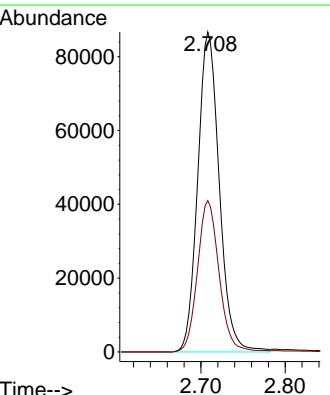



#11
Allyl Chloride
 Concen: 16.053 ug/l
 RT: 2.908 min Scan# 5
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11



Instrument : MSVOA_U
 ClientSampleId : VSTDICC015

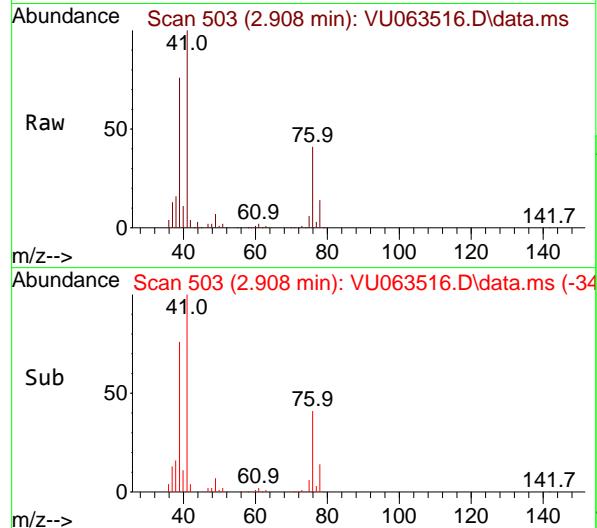


Tgt Ion: 41 Resp: 14987
 Ion Ratio Lower Upper
 41 100
 39 76.2 61.5 92.3

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

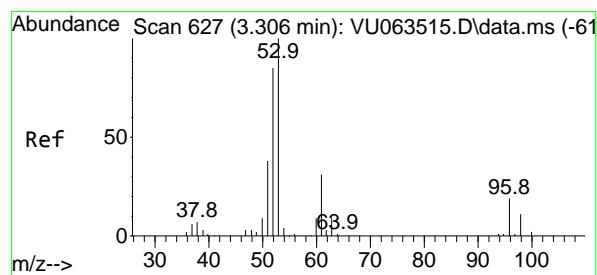


#12
Acrylonitrile
 Concen: 29.022 ug/l
 RT: 3.303 min Scan# 626
 Delta R.T. -0.003 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11


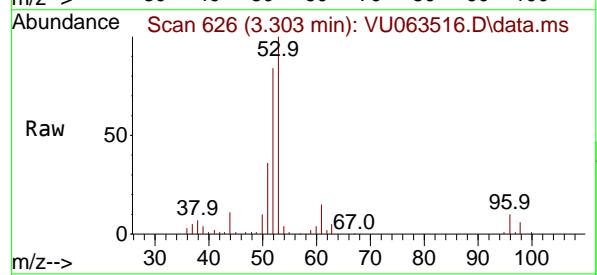


Tgt Ion: 53 Resp: 46936
 Ion Ratio Lower Upper
 53 100
 52 84.6 64.3 96.5
 51 36.8 27.8 41.8

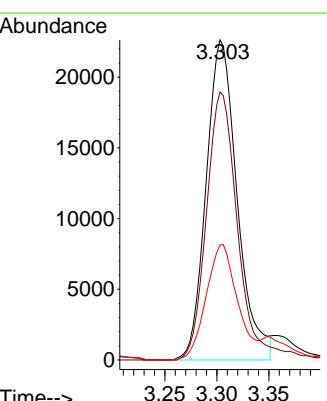




Abundance Scan 413 (2.618 min): VU063516.D\data.ms

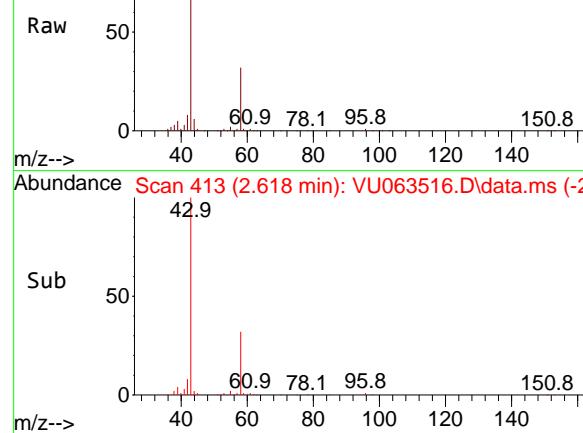

Abundance Scan 462 (2.776 min): VU063516.D\data.ms

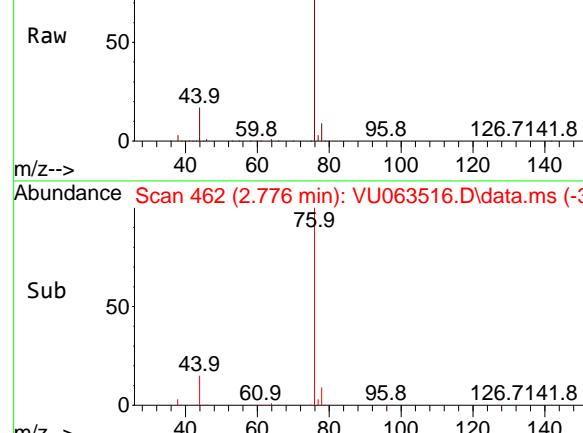

#13

Acetone

Concen: 88.245 ug/l

RT: 2.618 min Scan# 413

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

Tgt Ion: 43 Resp: 114283

Ion Ratio Lower Upper


43 100

58 32.3 25.4 38.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

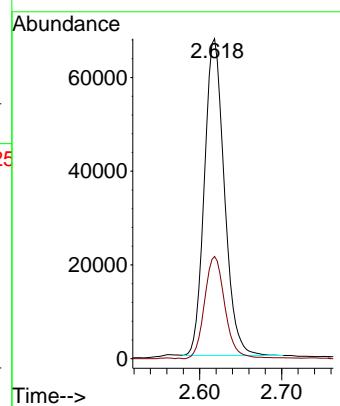

#14

Carbon Disulfide

Concen: 16.100 ug/l

RT: 2.776 min Scan# 462

Delta R.T. 0.000 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11







Tgt Ion: 76 Resp: 336090

Ion Ratio Lower Upper

76 100

78 9.1 7.0 10.6

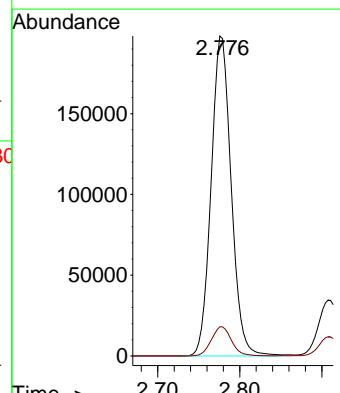



#15

Methylene Chloride

Concen: 15.136 ug/l

RT: 3.030 min Scan# 5

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument:

MSVOA_U


ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

 Tgt Ion: 84 Resp: 115170
 Ion Ratio Lower Upper

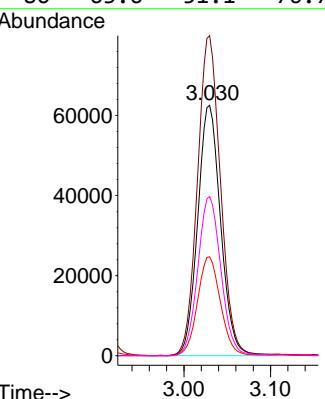 84 100
 49 127.8 103.8 155.8
 51 39.5 0.0 80.4
 86 63.6 51.1 76.7


#16

trans-1,2-Dichloroethene

Concen: 15.749 ug/l


RT: 3.335 min Scan# 636




Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Tgt Ion: 96 Resp: 115592

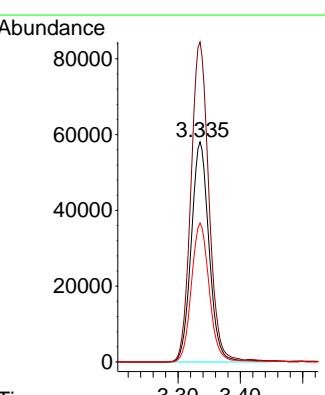 Ion Ratio Lower Upper
 96 100
 61 145.4 117.2 175.8
 98 63.1 51.4 77.2




#17

1,1-Dichloroethane

Concen: 15.707 ug/l

RT: 3.850 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#18

2-Butanone

Concen: 83.678 ug/l

RT: 4.708 min Scan# 1063

Delta R.T. -0.003 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11


Tgt Ion: 43 Resp: 167820

Ion Ratio Lower Upper

43 100

57 8.2 0.0 16.4

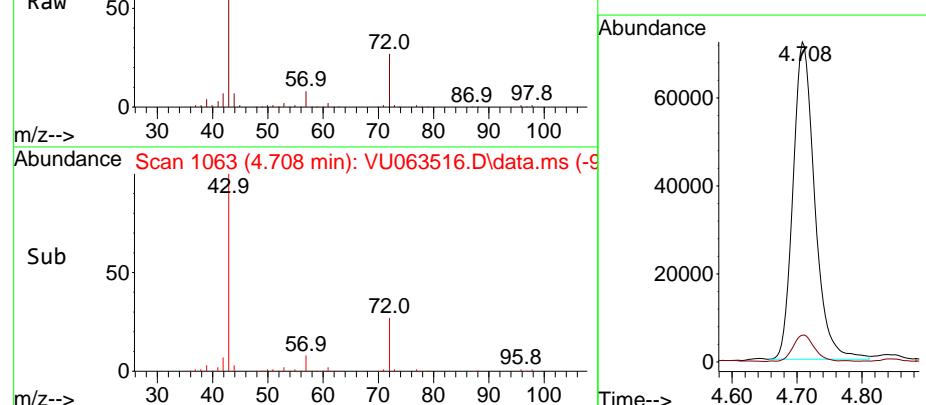

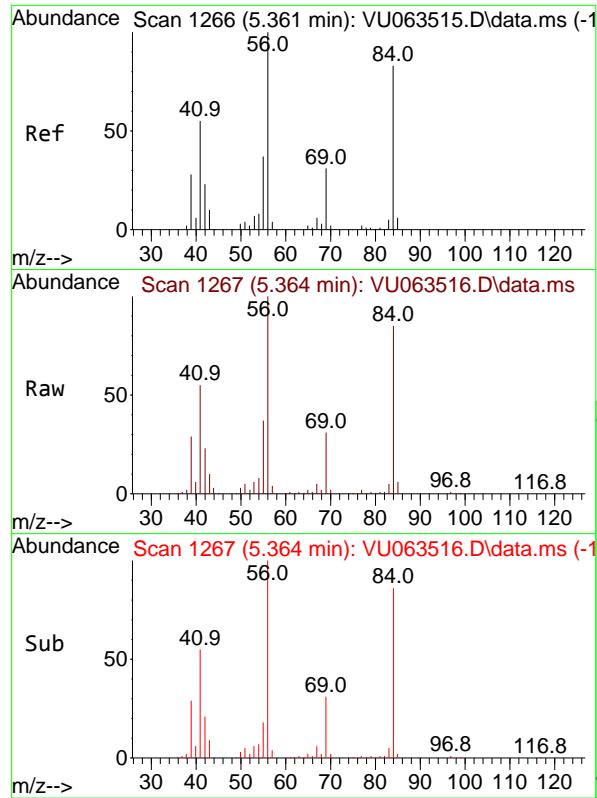

#19

Cyclohexane

Concen: 15.697 ug/l

RT: 5.364 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11



Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

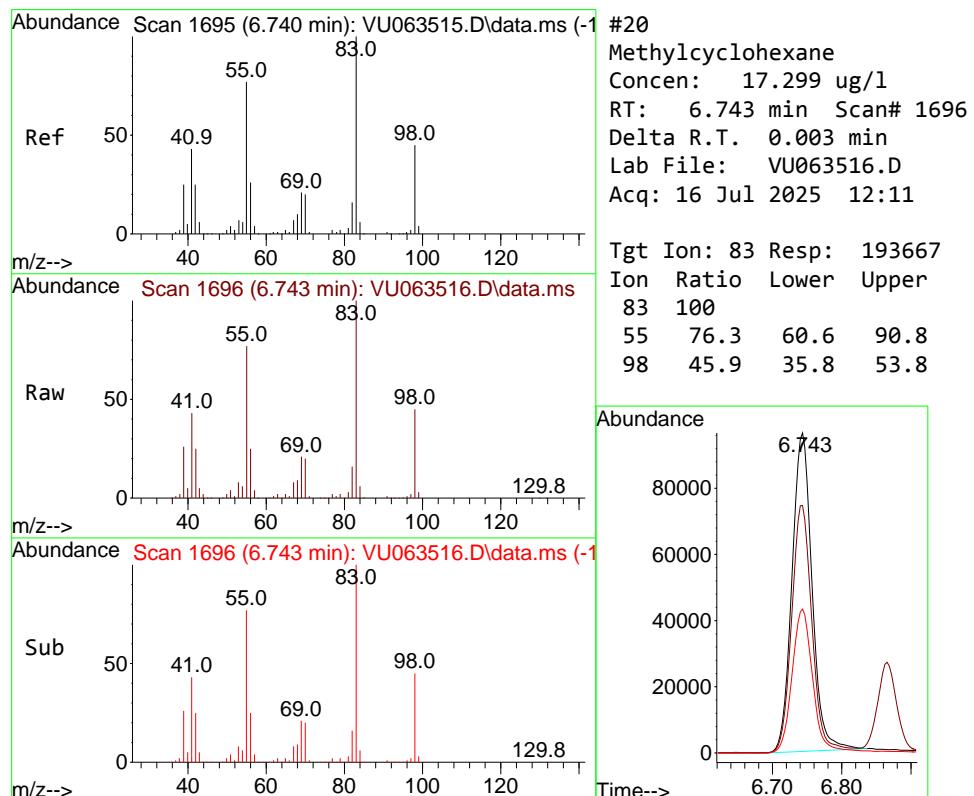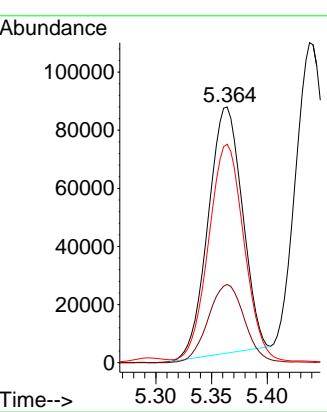 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#20

Methylcyclohexane


Concen: 17.299 ug/l


RT: 6.743 min Scan# 1696

Delta R.T. 0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

 Tgt Ion: 83 Resp: 193667
 Ion Ratio Lower Upper
 83 100
 55 76.3 60.6 90.8
 98 45.9 35.8 53.8




#21

2,2-Dichloropropane



Concen: 15.761 ug/l

RT: 4.644 min Scan# 1043

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

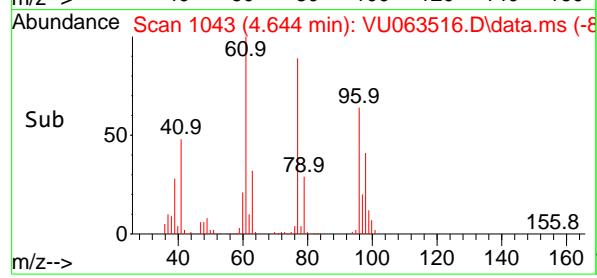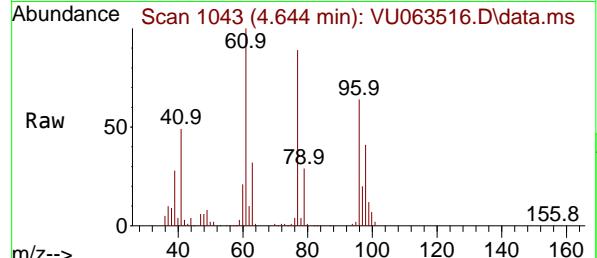




Tgt Ion: 77 Resp: 18258

Ion Ratio Lower Upper

77	100
97	22.0


17.8	26.8
------	------




**Manual Integrations
APPROVED**

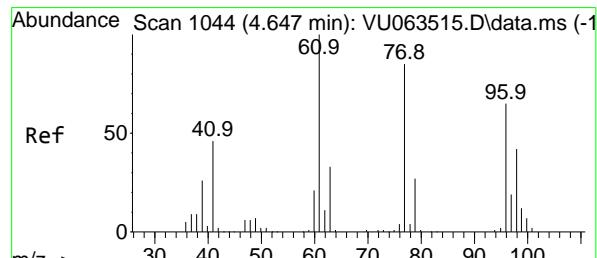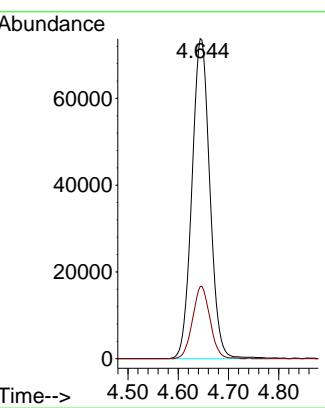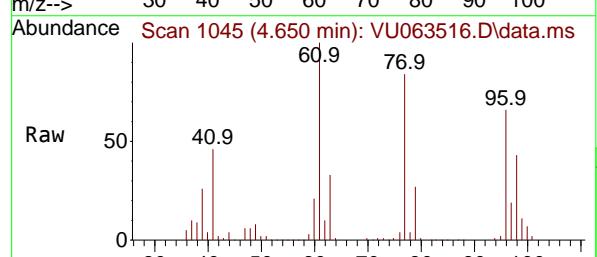 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

 #22
 cis-1,2-Dichloroethene
 Concen: 15.711 ug/l
 RT: 4.650 min Scan# 1045
 Delta R.T. 0.003 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

 Tgt Ion: 96 Resp: 125136
 Ion Ratio Lower Upper

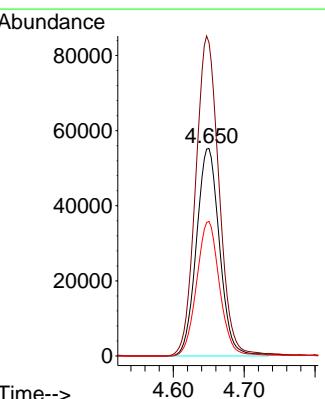96	100
61	156.1
98	64.6

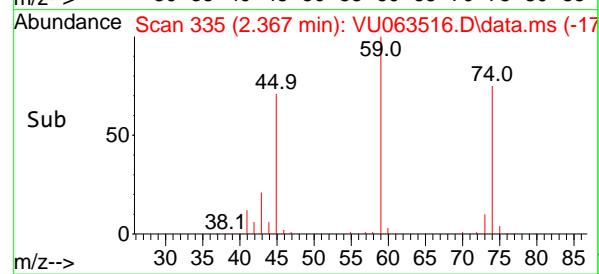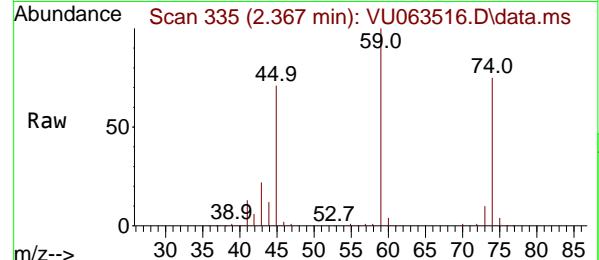0.0	384.7
32.1	96.3





#23

Diethyl Ether

Concen: 16.184 ug/l

RT: 2.367 min Scan# 3

Instrument: MSVOA_U

Delta R.T. 0.000 min




Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

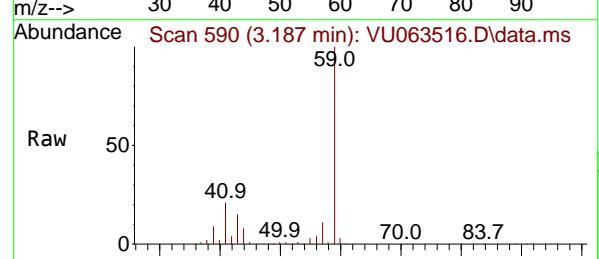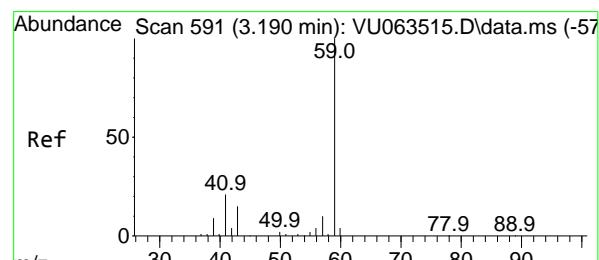

#24

tert-Butyl Alcohol

Concen: 160.102 ug/l

RT: 3.187 min Scan# 590

Delta R.T. -0.003 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11



Tgt Ion: 59 Resp: 95177

Ion Ratio Lower Upper

59 100

57 11.0 8.6 12.8

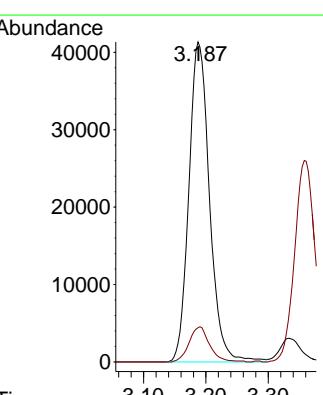

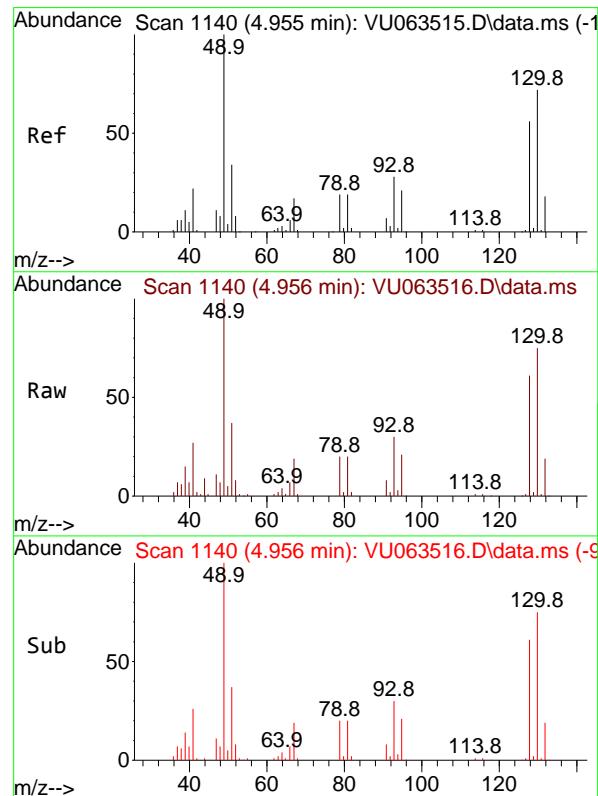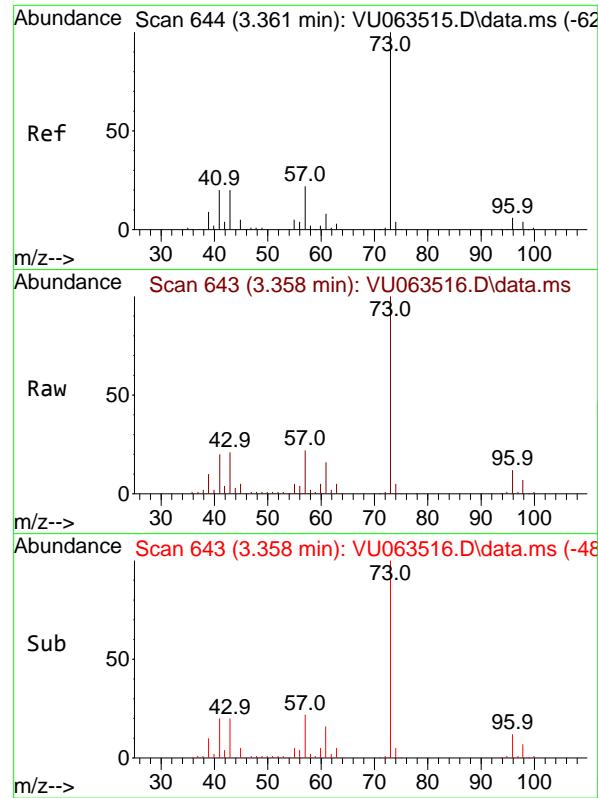


#25

Methyl tert-Butyl Ether
Concen: 16.090 ug/l
RT: 3.358 min Scan# 6
Delta R.T. -0.003 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
ClientSampleId : VSTDICC015

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#26

Bromochloromethane
Concen: 16.299 ug/l
RT: 4.956 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Tgt Ion:128 Resp: 54202
Ion Ratio Lower Upper
128 100
49 170.9 0.0 340.8
130 127.0 100.5 150.7

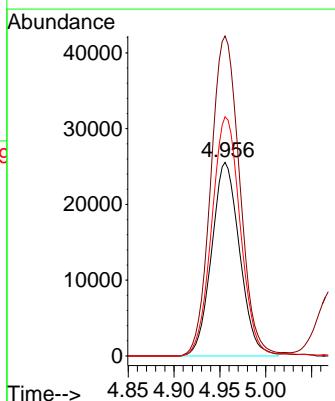


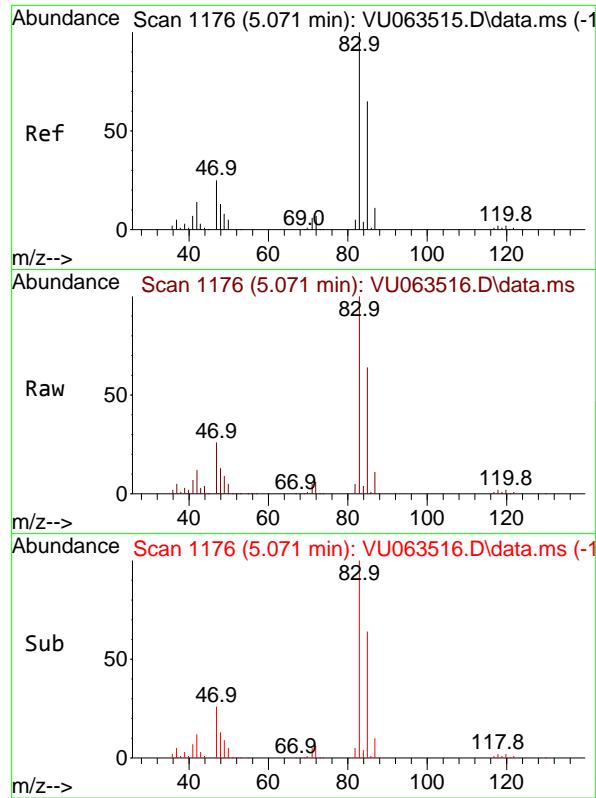


#27
 Chloroform
 Concen: 15.691 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
 ClientSampleId : VSTDICC015


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

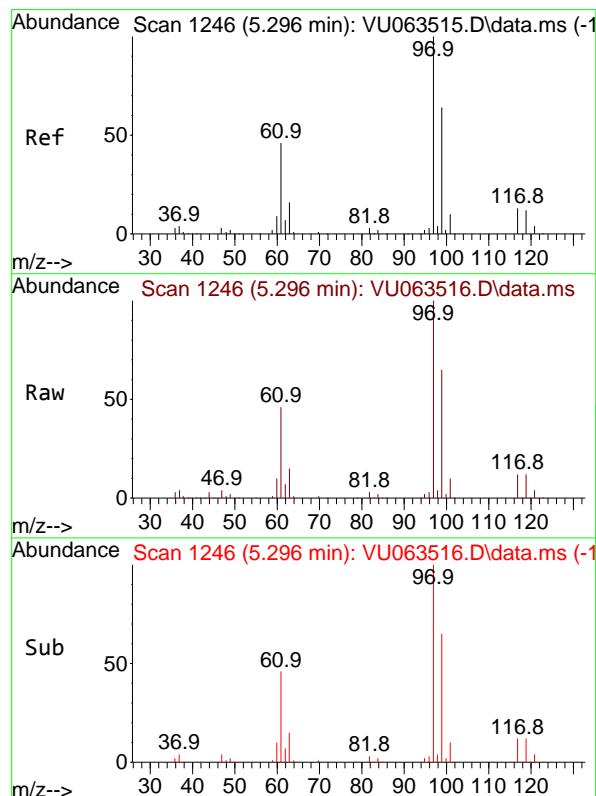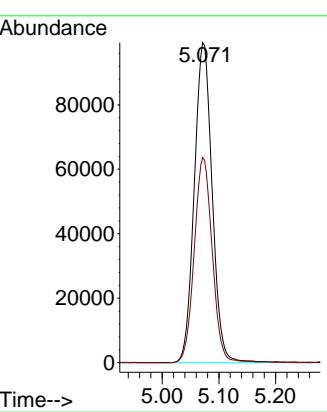

#28
 1,1,1-Trichloroethane
 Concen: 16.005 ug/l
 RT: 5.296 min Scan# 1246
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

Tgt Ion: 97 Resp: 188574
 Ion Ratio Lower Upper
 97 100
 99 64.7 31.8 95.3
 61 46.7 23.3 69.9

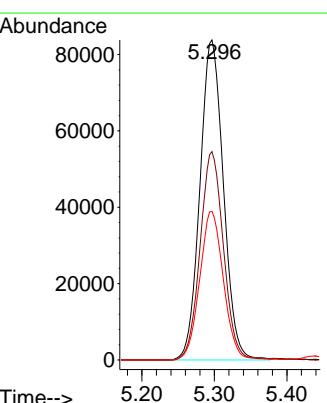


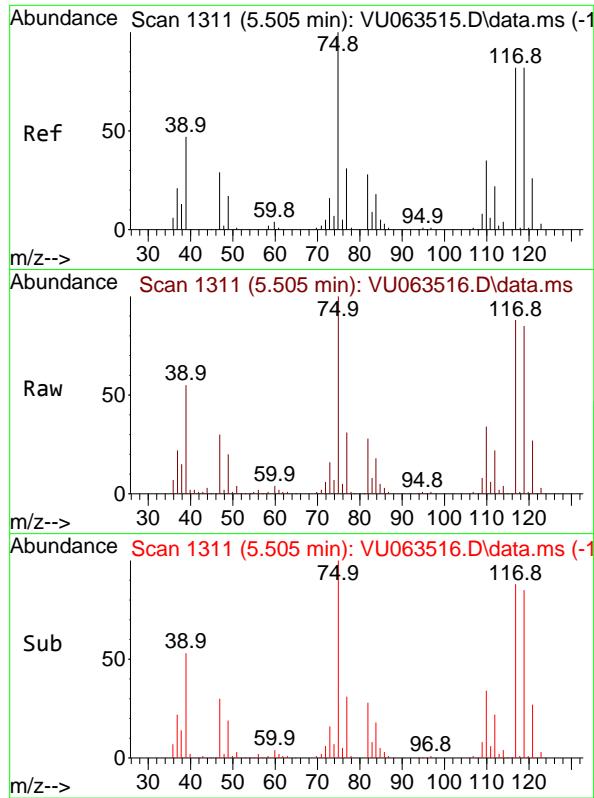


#29
1,1-Dichloropropene
Concen: 16.004 ug/l
RT: 5.505 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
ClientSampleId : VSTDICC015


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

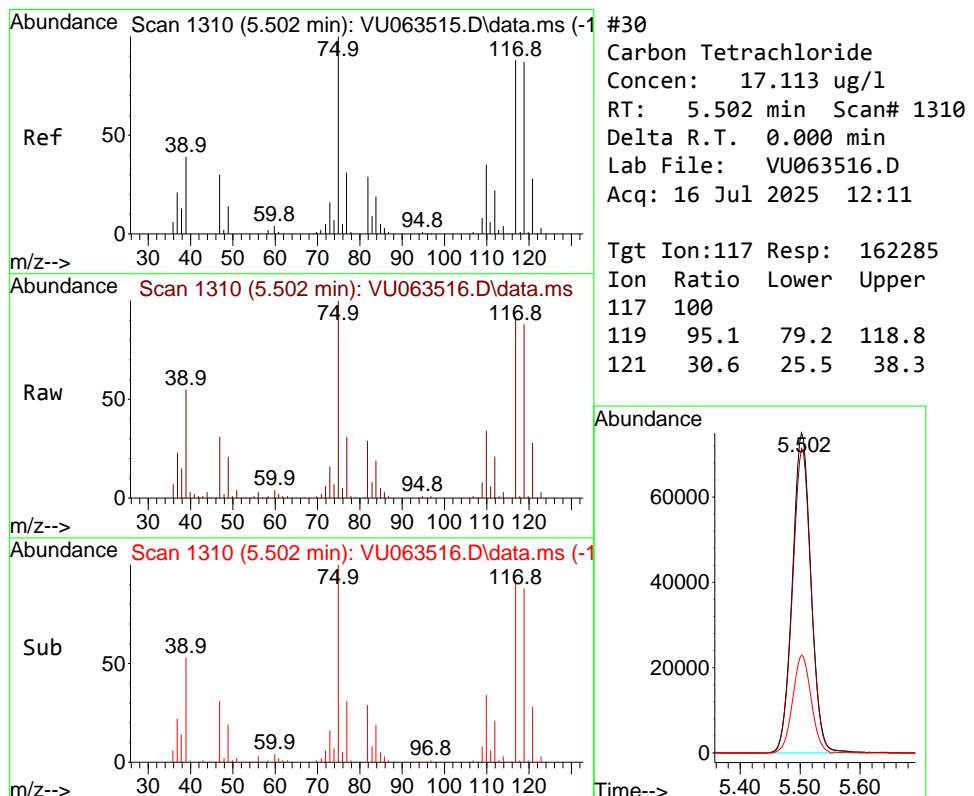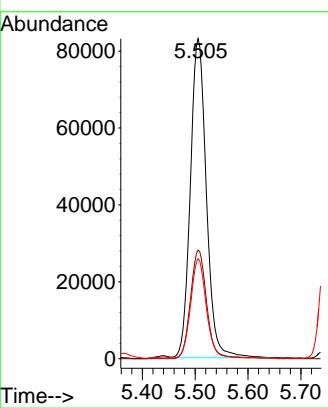

#30
Carbon Tetrachloride
Concen: 17.113 ug/l
RT: 5.502 min Scan# 1310
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Tgt Ion:117 Resp: 162285
Ion Ratio Lower Upper
117 100
119 95.1 79.2 118.8
121 30.6 25.5 38.3





#31

Isopropyl Ether

Concen: 15.772 ug/l

RT: 3.991 min Scan# 8

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#32

Ethyl-t-butyl ether

Concen: 15.939 ug/l

RT: 4.502 min Scan# 999

Delta R.T. 0.000 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11


Tgt Ion: 59 Resp: 302903

Ion Ratio Lower Upper

59 100

87 41.8 32.6 49.0

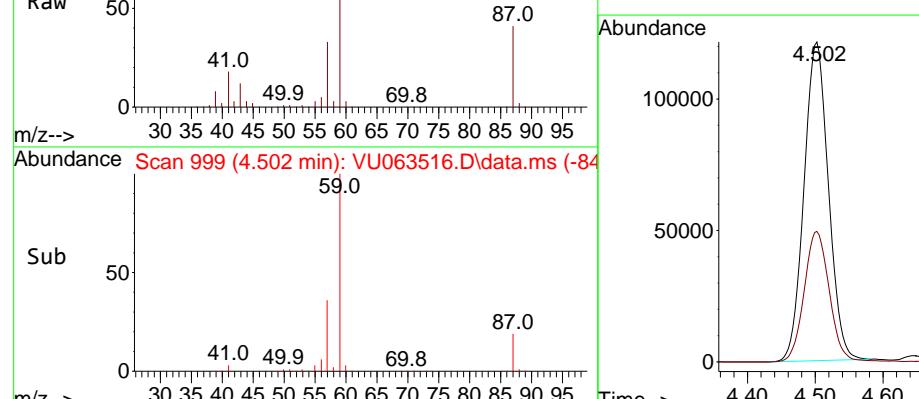

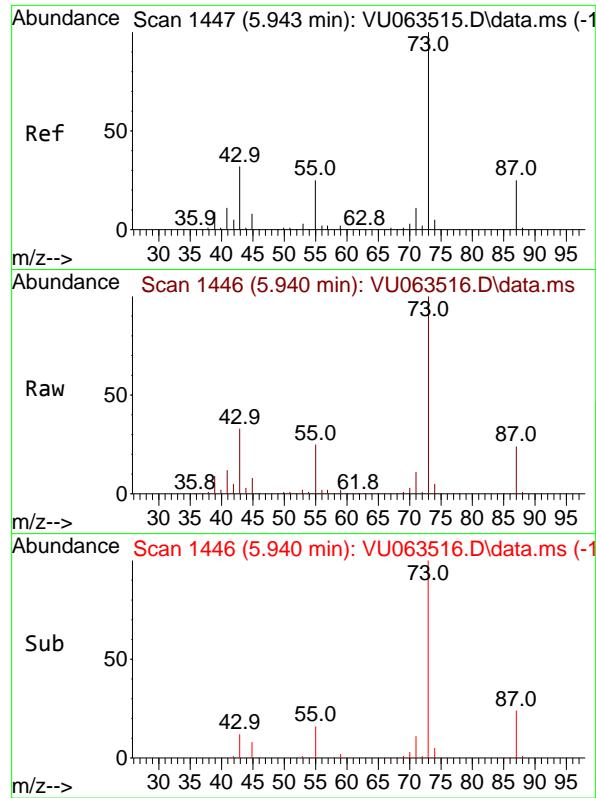



#33

Tert-Amyl methyl ether
Concen: 16.283 ug/l
RT: 5.940 min Scan# 1447
Delta R.T. -0.003 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
ClientSampleId : VSTDICC015

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

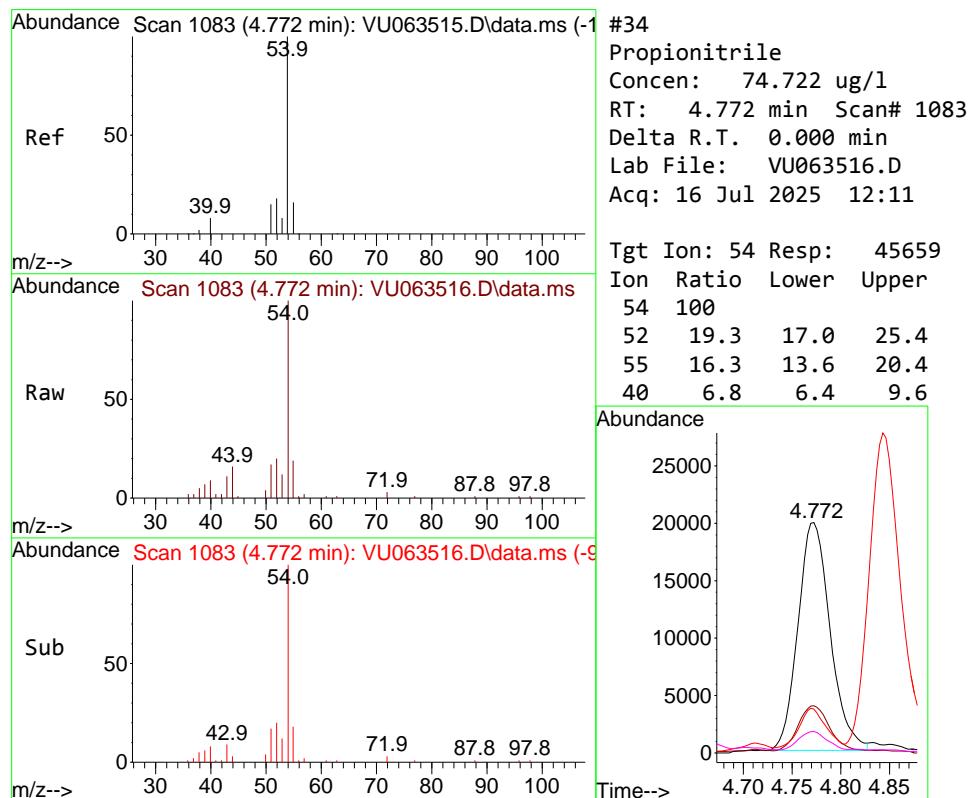


#34

Propionitrile
Concen: 74.722 ug/l
RT: 4.772 min Scan# 1083
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11


Tgt Ion: 54 Resp: 45659
Ion Ratio Lower Upper
54 100
52 19.3 17.0 25.4
55 16.3 13.6 20.4
40 6.8 6.4 9.6





#35
Benzene
Concen: 16.153 ug/l
RT: 5.756 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Instrument : MSVOA_U
ClientSampleId : VSTDICC015




Tgt Ion: 78 Resp: 47368
Ion Ratio Lower Upper
78 100
77 23.8 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

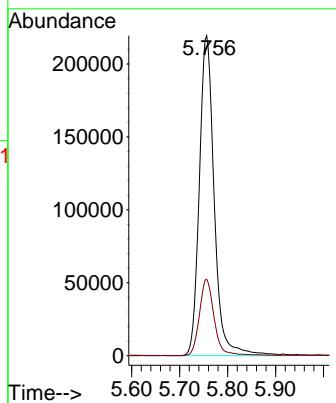


#36
1,2-Dichloroethane
Concen: 16.165 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11





Tgt Ion: 62 Resp: 147295
Ion Ratio Lower Upper
62 100
98 8.3 6.4 9.6

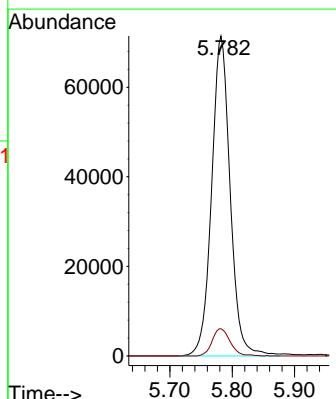





#37
Trichloroethene
Concen: 17.198 ug/l
RT: 6.525 min Scan# 1
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063516.D
ClientSampleId : VSTDICC015
Acq: 16 Jul 2025 12:11

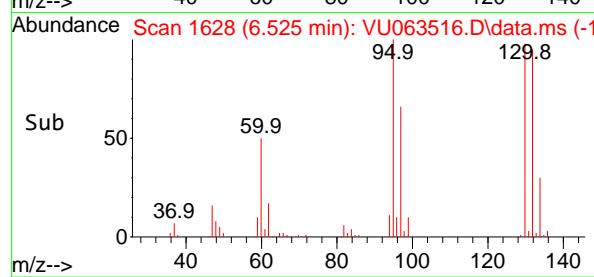


Tgt Ion:130 Resp: 128670
Ion Ratio Lower Upper
130 100
95 102.3 80.3 120.5

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025






#38
1,2-Dichloropropane
Concen: 18.188 ug/l
RT: 6.779 min Scan# 1707
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11



Tgt Ion: 63 Resp: 124831
Ion Ratio Lower Upper
63 100
65 30.6 24.6 36.8





#39

Methacrylonitrile

Concen: 14.730 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#40

Methyl acrylate

Concen: 16.402 ug/l

RT: 4.843 min Scan# 1105

Delta R.T. -0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Tgt Ion: 55 Resp: 65123



Ion Ratio Lower Upper


55 100

85 16.8 12.8 19.2

58 8.7 7.0 10.4

42 8.8 7.0 10.4

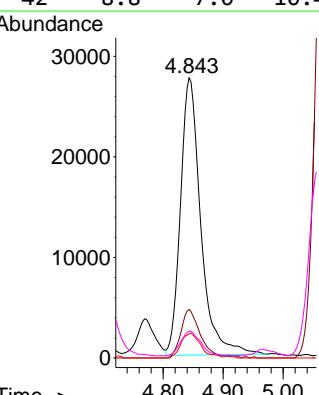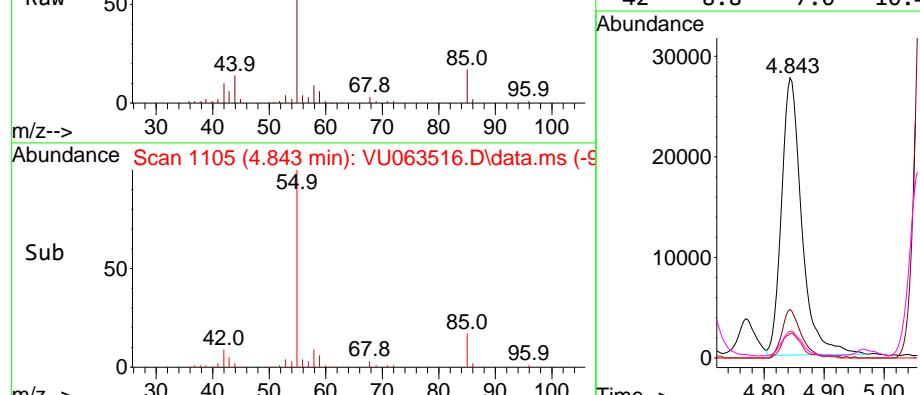

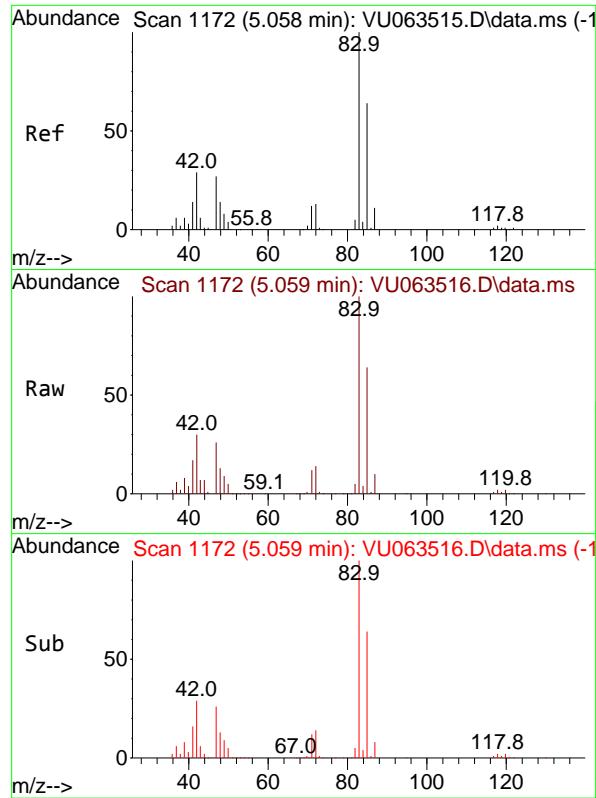

#41

Tetrahydrofuran

Concen: 28.595 ug/l


RT: 5.059 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11



Instrument : MSVOA_U
 ClientSampleId : VSTDICC015

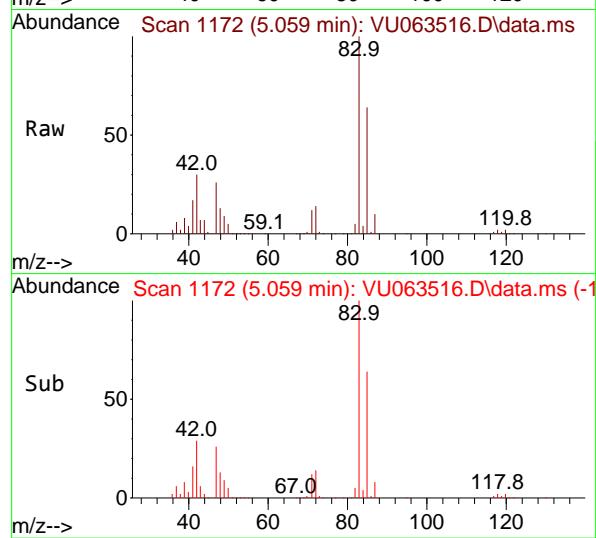

Tgt Ion: 42 Resp: 40853
 Ion Ratio Lower Upper
 42 100
 72 49.0 39.2 58.8
 71 43.0 34.8 52.2


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

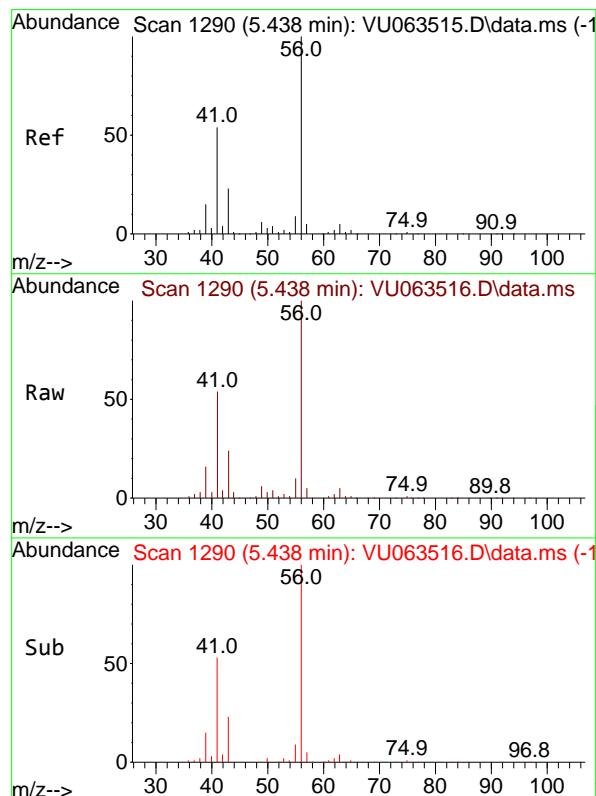

#42
 1-Chlorobutane
 Concen: 15.991 ug/l
 RT: 5.438 min Scan# 1290
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11


Tgt Ion: 56 Resp: 232046
 Ion Ratio Lower Upper
 56 100
 41 54.1 26.7 80.0





#43
Dibromomethane
Concen: 17.639 ug/l
RT: 6.904 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Instrument : MSVOA_U
ClientSampleId : VSTDICC015




Tgt Ion: 93 Resp: 62710
Ion Ratio Lower Upper
93 100
95 84.7 67.9 101.9
174 92.1 74.6 111.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

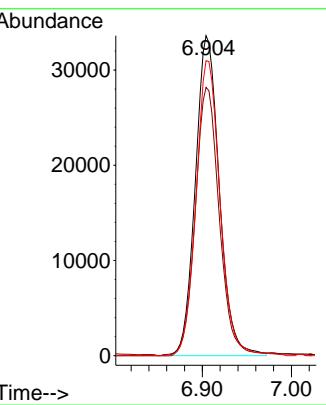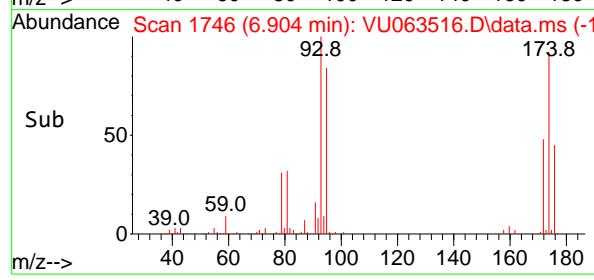


#44
Bromodichloromethane
Concen: 18.058 ug/l
RT: 7.094 min Scan# 1805
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11



Tgt Ion: 83 Resp: 144794
Ion Ratio Lower Upper
83 100
85 63.1 52.7 79.1
127 9.0 8.1 12.1

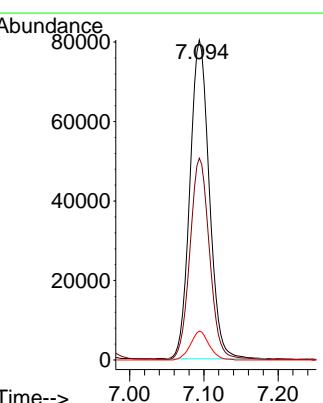


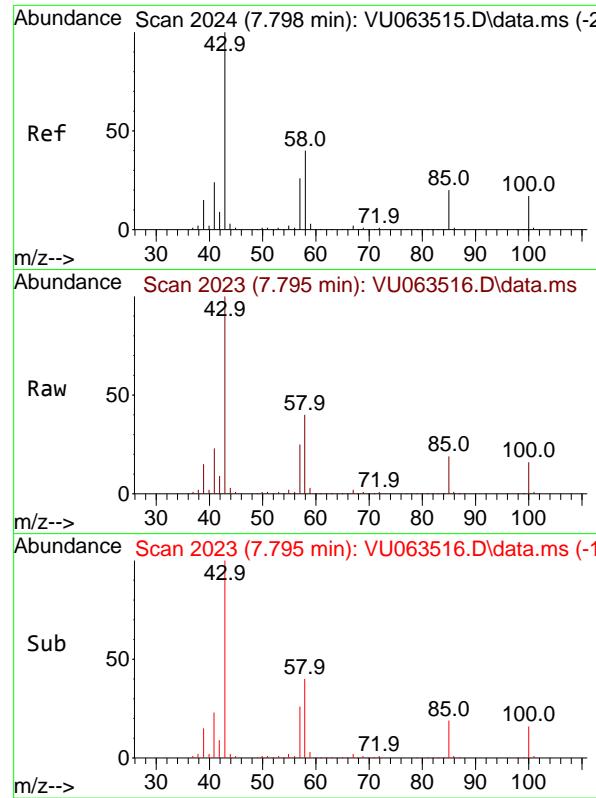

#45
 4-Methyl-2-Pentanone
 Concen: 84.821 ug/l
 RT: 7.795 min Scan# 2
Instrument :
 Delta R.T. -0.003 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11
ClientSampleId :
 VSTDICC015


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

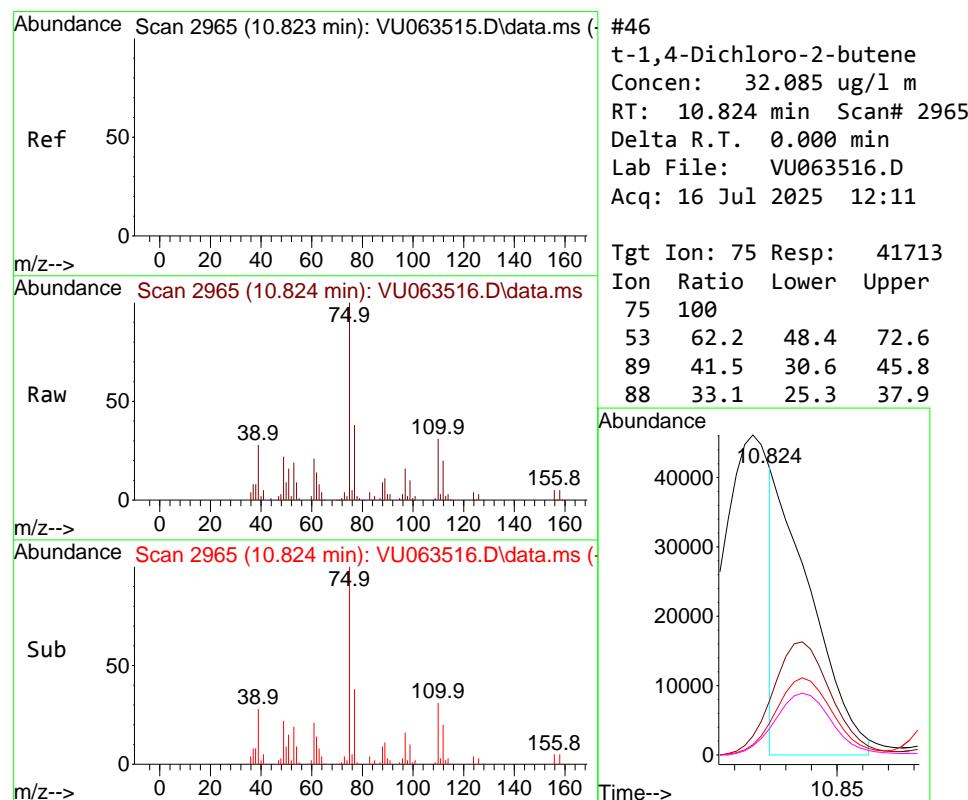

#46
 t-1,4-Dichloro-2-butene
 Concen: 32.085 ug/l m
 RT: 10.824 min Scan# 2965
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

Tgt Ion: 75 Resp: 41713
 Ion Ratio Lower Upper
 75 100
 53 62.2 48.4 72.6
 89 41.5 30.6 45.8
 88 33.1 25.3 37.9

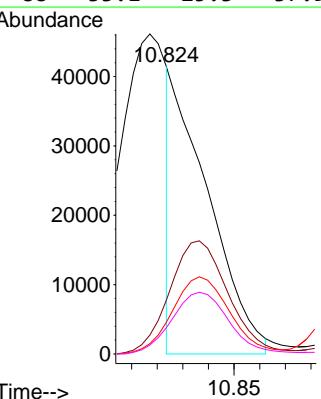

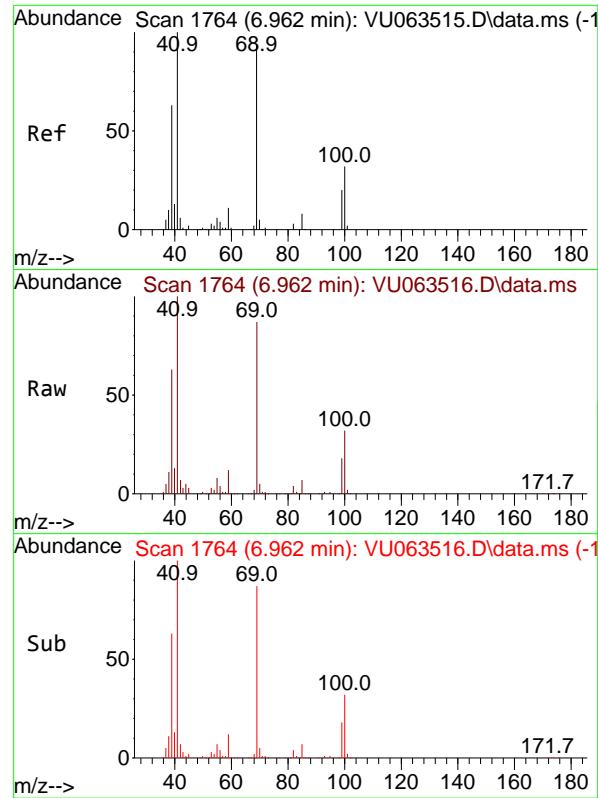

#47

Methyl methacrylate

Concen: 38.417 ug/l

RT: 6.962 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument:

MSVOA_U



ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

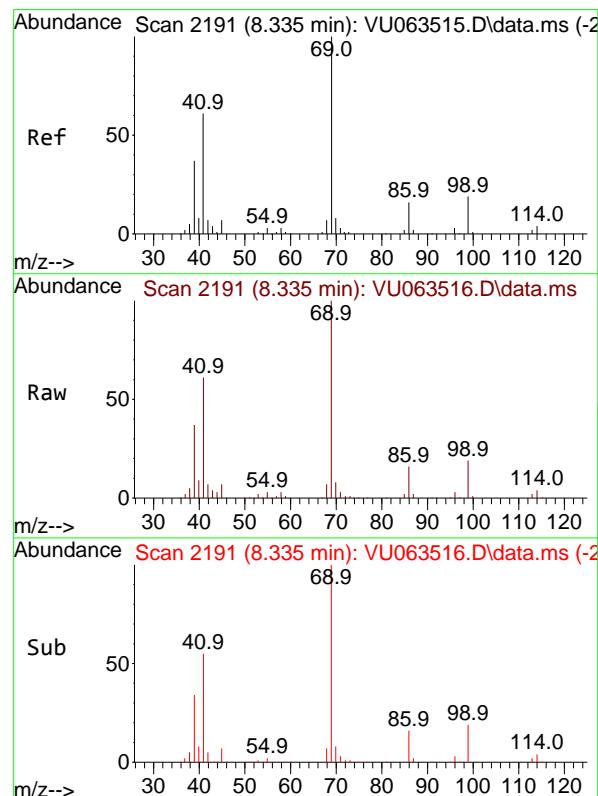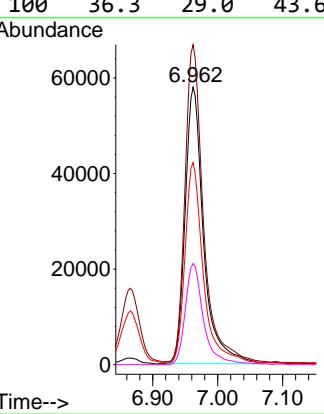

#48

Ethyl methacrylate

Concen: 17.728 ug/l

RT: 8.335 min Scan# 2191


Delta R.T. 0.000 min


Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Tgt Ion: 69 Resp: 101021


Ion	Ratio	Lower	Upper
69	100		
41	62.2	30.8	92.4

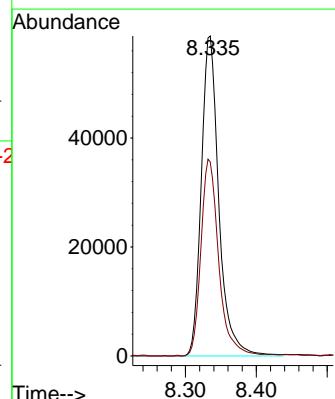



#49
Toluene
Concen: 16.751 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11




Instrument: MSVOA_U
ClientSampleId: VSTDICC015




Tgt Ion: 92 Resp: 26820
Ion Ratio Lower Upper
92 100
91 173.9 140.4 210.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

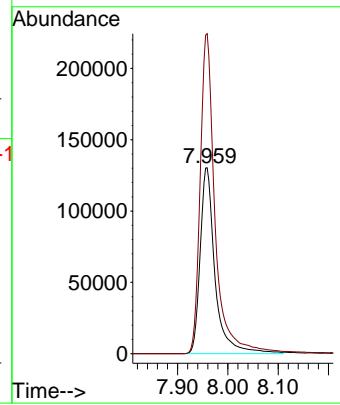


#50
t-1,3-Dichloropropene
Concen: 18.597 ug/l
RT: 8.203 min Scan# 2150
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11



Tgt Ion: 75 Resp: 116990
Ion Ratio Lower Upper
75 100
77 33.0 24.9 37.3

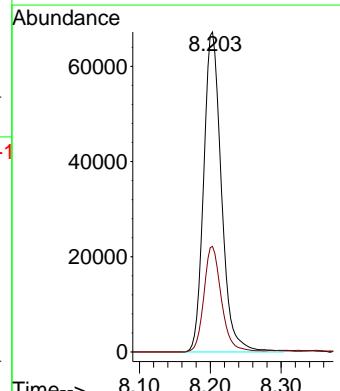


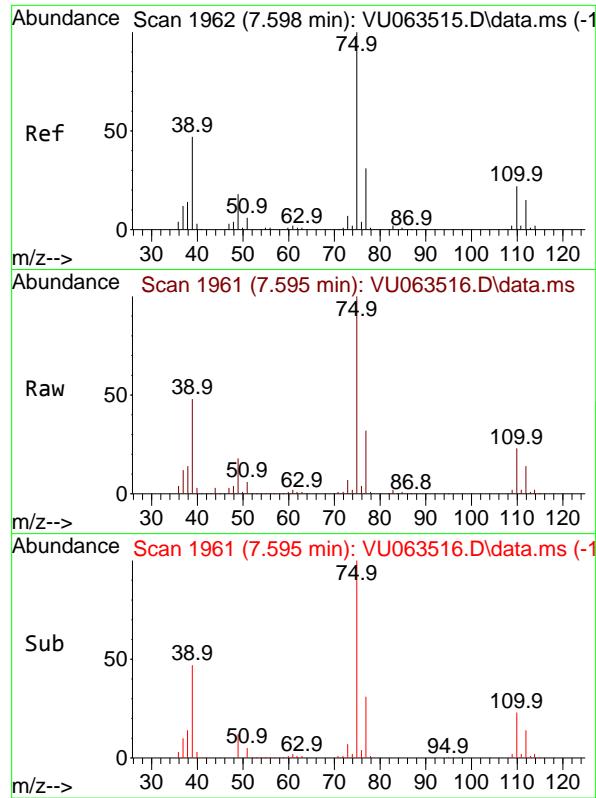


#51
cis-1,3-Dichloropropene
Concen: 20.004 ug/l
RT: 7.595 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
ClientSampleId : VSTDICC015

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

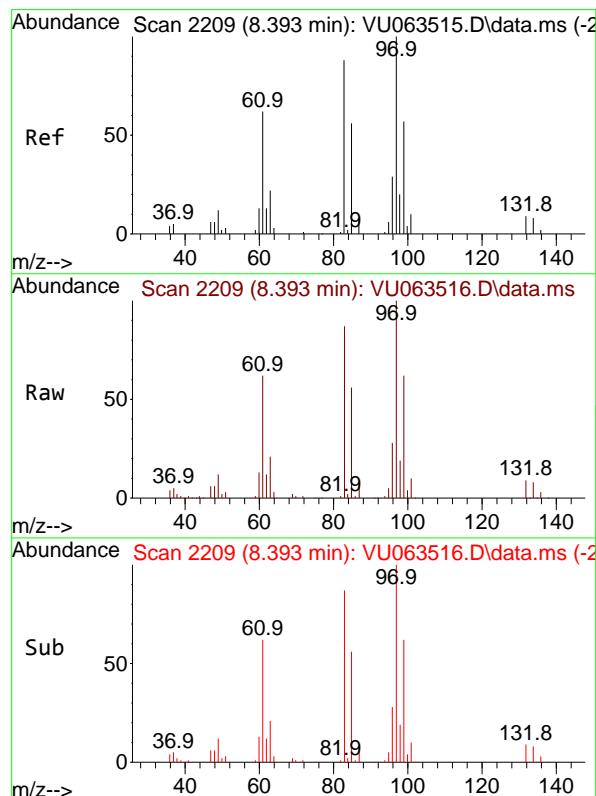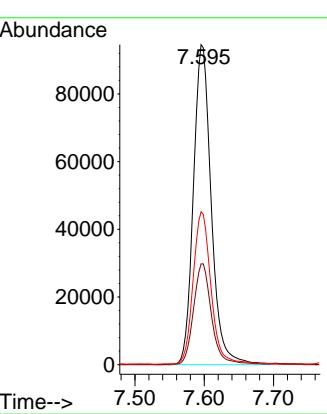


#52
1,1,2-Trichloroethane
Concen: 16.480 ug/l
RT: 8.393 min Scan# 2209
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11


Tgt Ion: 97 Resp: 78885
Ion Ratio Lower Upper

	97	100
83	86.9	70.2
85	55.9	45.2
99	61.5	50.1


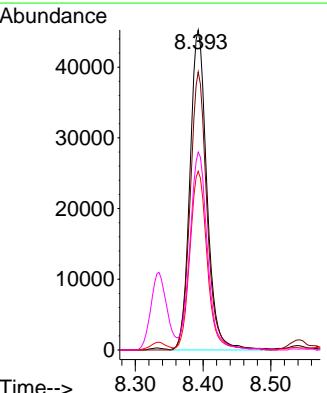





Abundance Scan 2263 (8.566 min): VU063516.D\data.ms

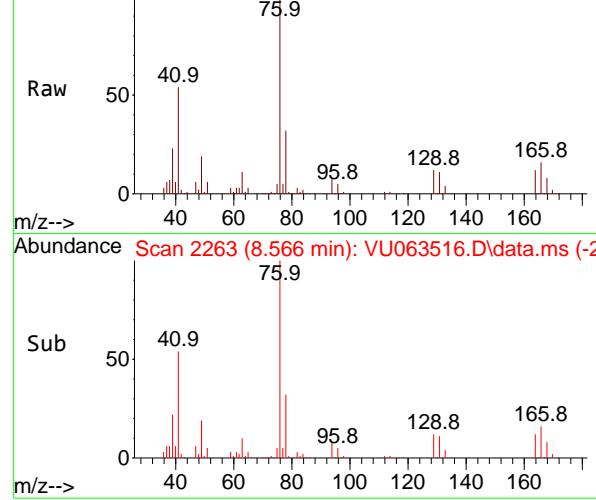


Abundance Scan 2263 (8.566 min): VU063516.D\data.ms (-2)

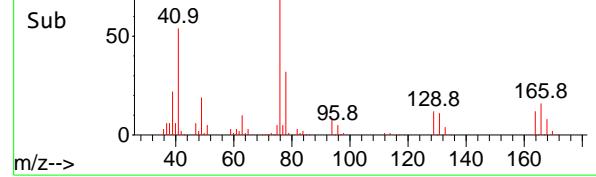

Abundance Scan 2301 (8.689 min): VU063516.D\data.ms

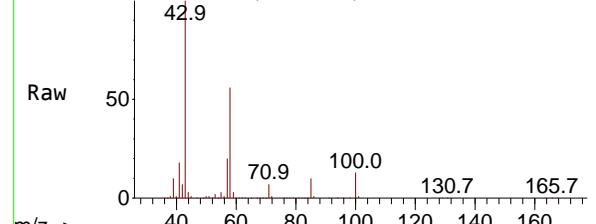

Abundance Scan 2301 (8.689 min): VU063516.D\data.ms (-2)

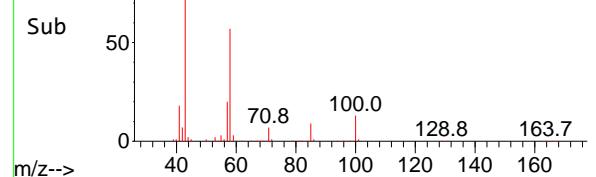

#53

1,3-Dichloropropane

Concen: 16.441 ug/l

RT: 8.566 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#54

2-Hexanone

Concen: 87.533 ug/l

RT: 8.689 min Scan# 2301

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Tgt Ion: 43 Resp: 213057







Ion Ratio Lower Upper

43 100

58 55.4 34.8 74.8

57 19.5 0.0 39.5

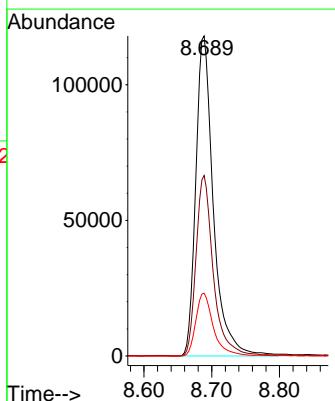

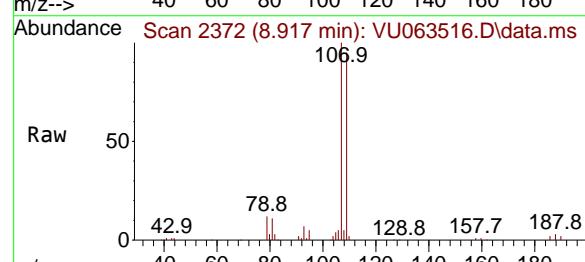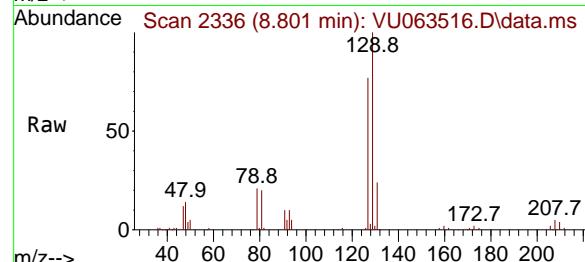

#55

Dibromochloromethane

Concen: 18.292 ug/l

RT: 8.801 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument :

MSVOA_U


ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#56

1,2-Dibromoethane

Concen: 16.452 ug/l

RT: 8.917 min Scan# 2372

Delta R.T. 0.000 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11




Tgt Ion:107 Resp: 70483

Ion Ratio Lower Upper

107 100

109 94.8 0.0 186.4

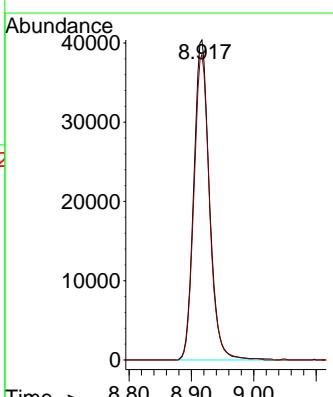



#57

4-Bromofluorobenzene

Concen: 1.051 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

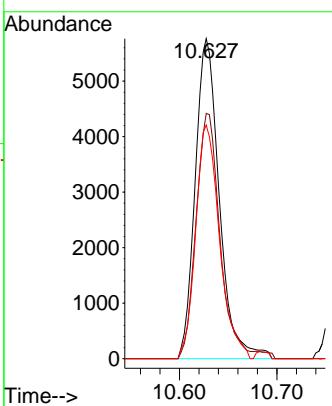 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#58

Tetrachloroethene

Concen: 16.111 ug/l


RT: 8.541 min Scan# 2255


Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Tgt	Ion:164	Resp:	110328
Ion	Ratio	Lower	Upper
164	100		
166	128.3	100.7	151.1
129	101.8	80.6	120.8
131	98.6	77.3	115.9

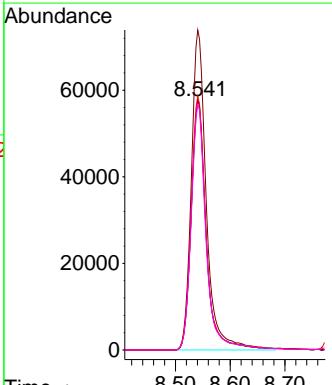

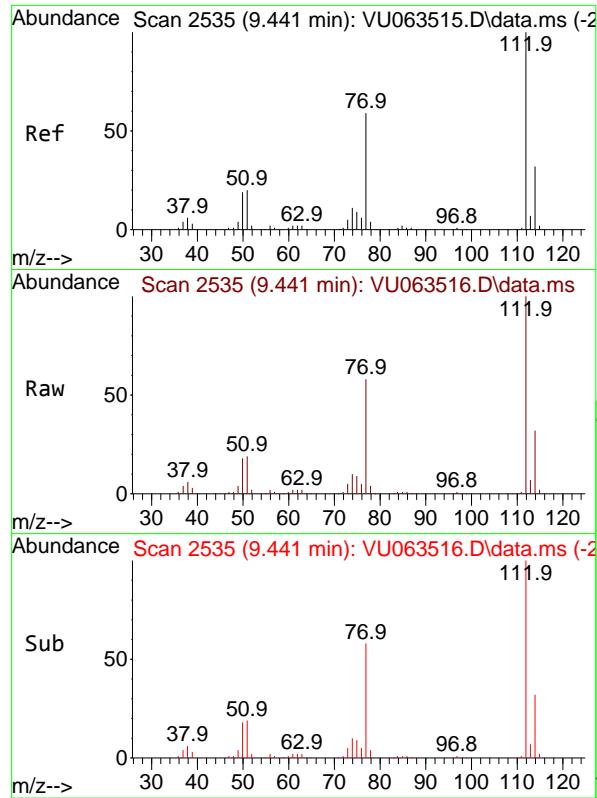

#59

Chlorobenzene

Concen: 16.822 ug/l

RT: 9.441 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D



Acq: 16 Jul 2025 12:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

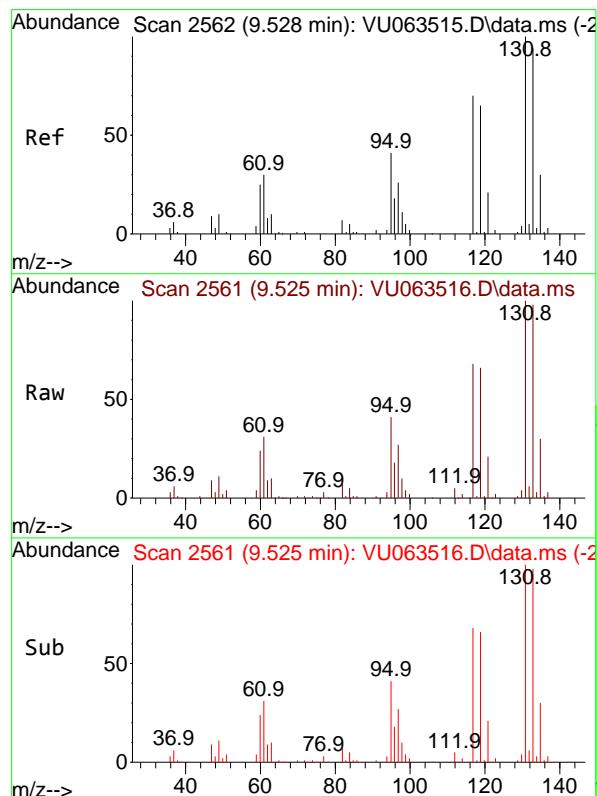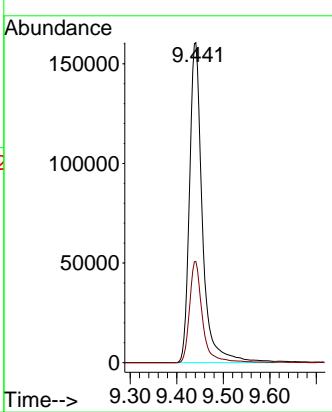Manual Integrations
APPROVED
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#60

1,1,1,2-Tetrachloroethane

Concen: 17.225 ug/l

RT: 9.525 min Scan# 2561

Delta R.T. -0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Tgt Ion:131 Resp: 101862


Ion Ratio Lower Upper

131 100

133 96.4 74.7 112.1

119 65.3 53.0 79.4

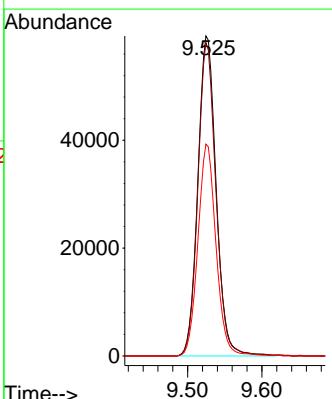


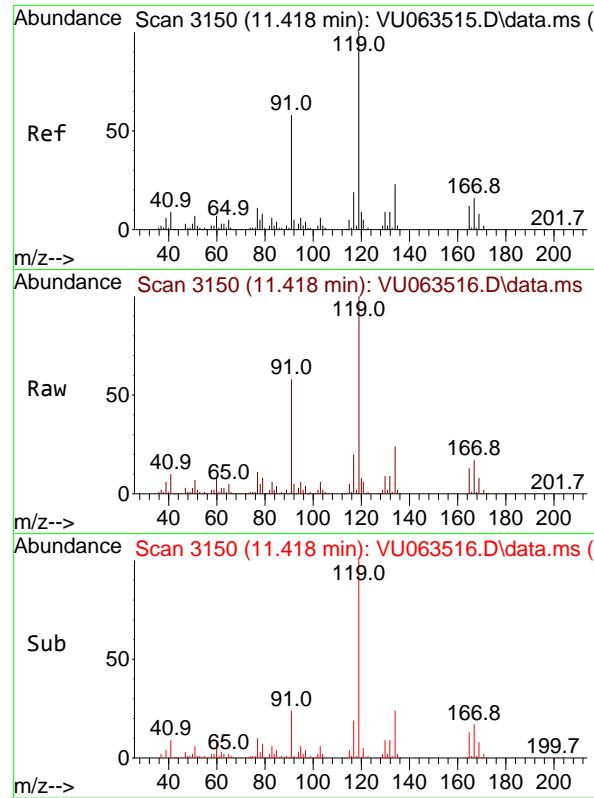


#61
 Pentachloroethane
 Concen: 18.487 ug/l
 RT: 11.418 min Scan# 3150
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
 ClientSampleId : VSTDICC015


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

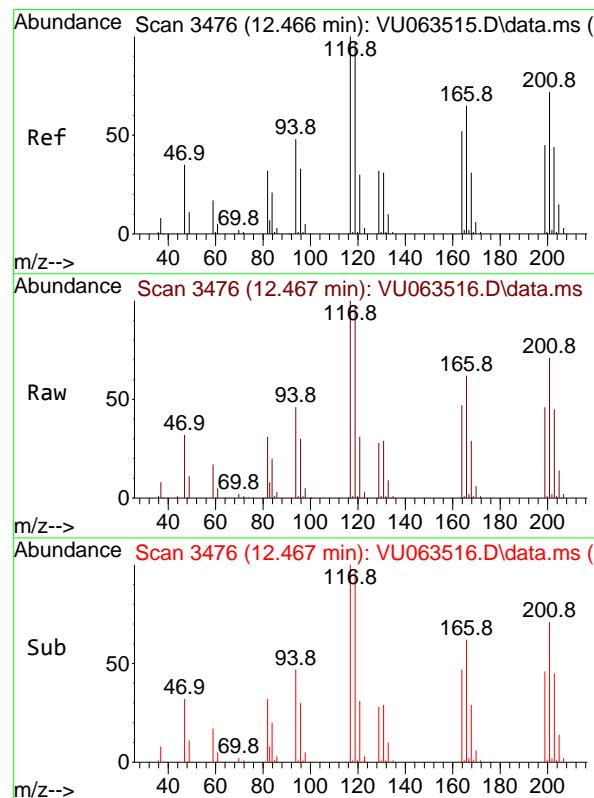



#62
 Hexachloroethane
 Concen: 19.195 ug/l
 RT: 12.467 min Scan# 3476
 Delta R.T. 0.000 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

Tgt Ion:117 Resp: 79431
 Ion Ratio Lower Upper
 117 100
 201 72.3 57.4 86.0

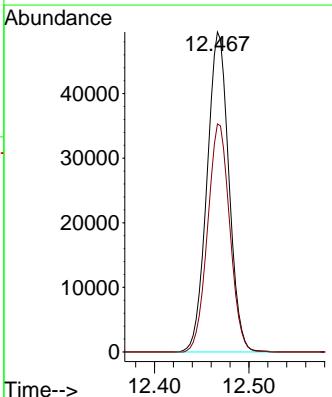


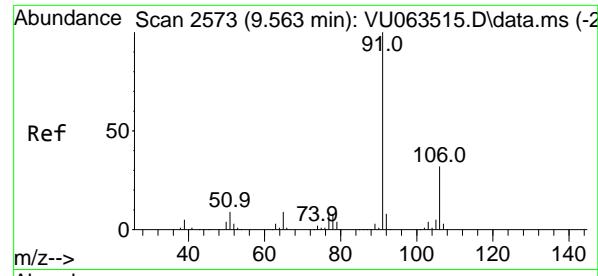

Abundance Scan 2573 (9.563 min): VU063516.D\data.ms

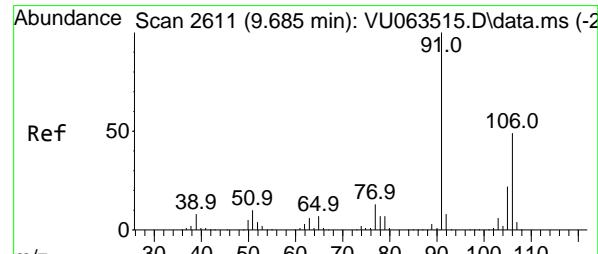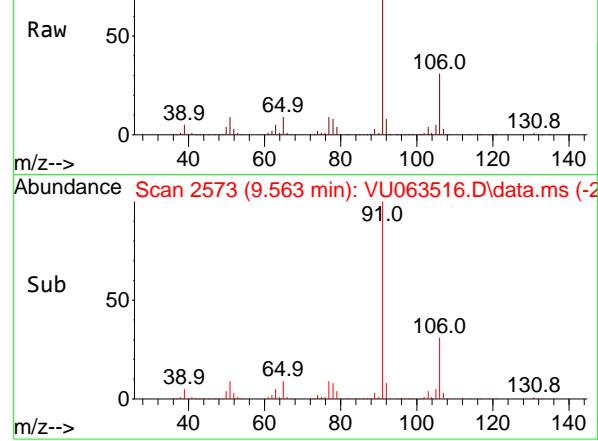

Abundance Scan 2611 (9.685 min): VU063516.D\data.ms

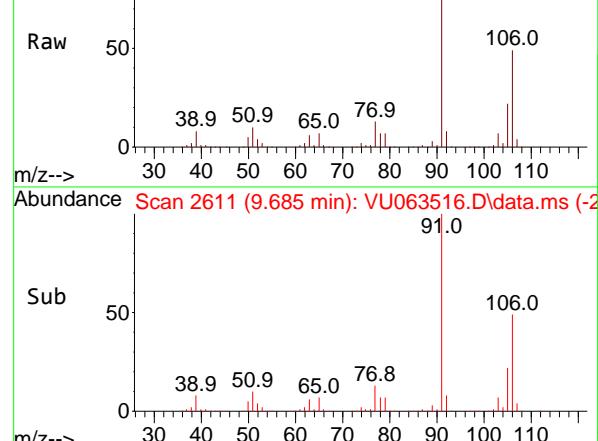

Abundance Scan 2611 (9.685 min): VU063516.D\data.ms (-2)

#63

Ethyl Benzene

Concen: 16.614 ug/l

RT: 9.563 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#64

m/p-Xylenes

Concen: 34.249 ug/l

RT: 9.685 min Scan# 2611

Delta R.T. 0.000 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11


Tgt Ion:106 Resp: 421278

Ion Ratio Lower Upper

106 100

91 204.6 163.6 245.4



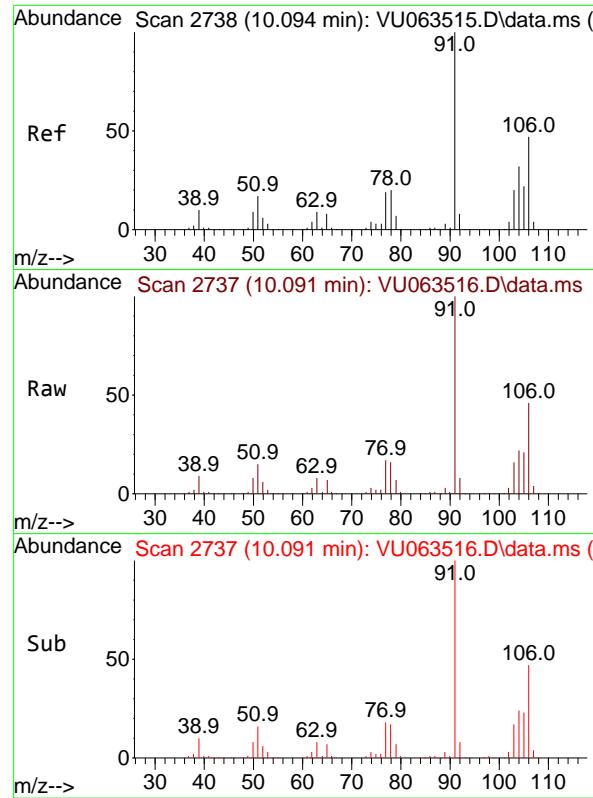



#65
o-Xylene
Concen: 17.365 ug/l
RT: 10.091 min Scan# 2
Instrument : MSVOA_U
Delta R.T. -0.003 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

ClientSampleId : VSTDICC015

Tgt Ion:106 Resp: 205249
Ion Ratio Lower Upper
106 100
91 213.5 108.1 324.4


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

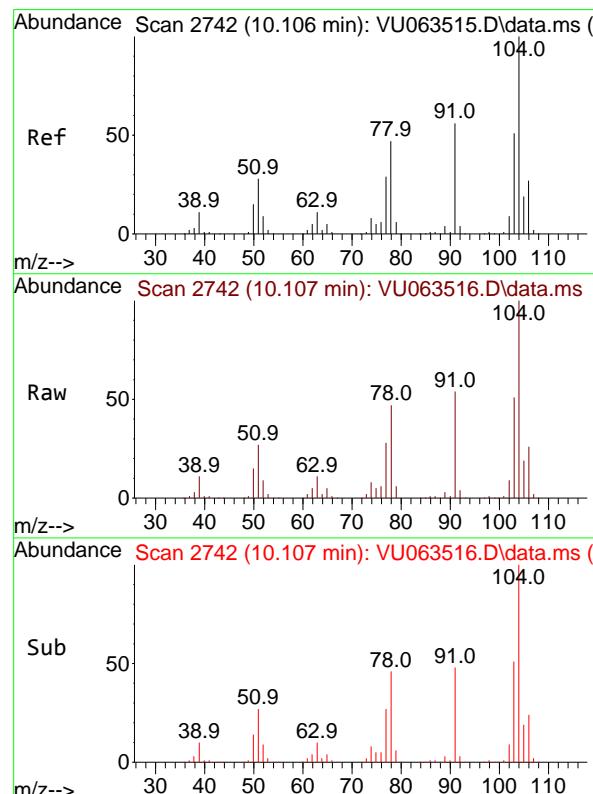

#66
Styrene
Concen: 17.837 ug/l
RT: 10.107 min Scan# 2742
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Tgt Ion:104 Resp: 336001
Ion Ratio Lower Upper
104 100
78 51.5 41.3 61.9
103 54.8 43.6 65.4

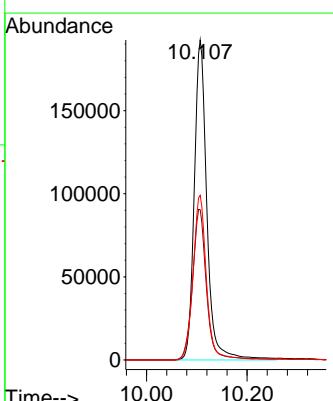



#67

Bromoform

Concen: 18.852 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

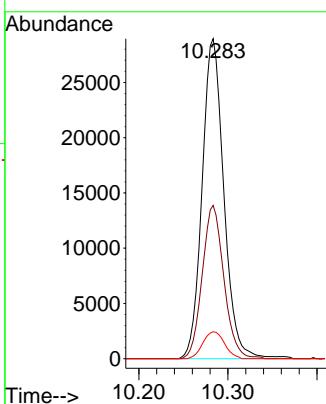 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.118 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
152	100		9748		
115	162.9	0.0		262.2	
150	405.8	0.0		651.2	

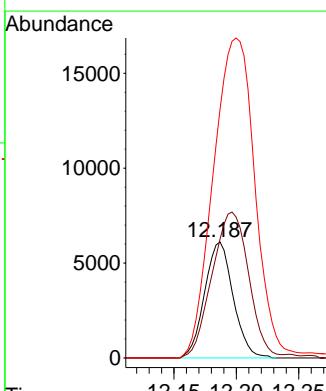



#69

Isopropylbenzene

Concen: 17.221 ug/l

RT: 10.476 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument :

MSVOA_U




ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 16.933 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Tgt Ion: 83 Resp: 98628




Ion Ratio Lower Upper

83 100

131 10.3 8.4 12.6

85 64.7 51.9 77.9

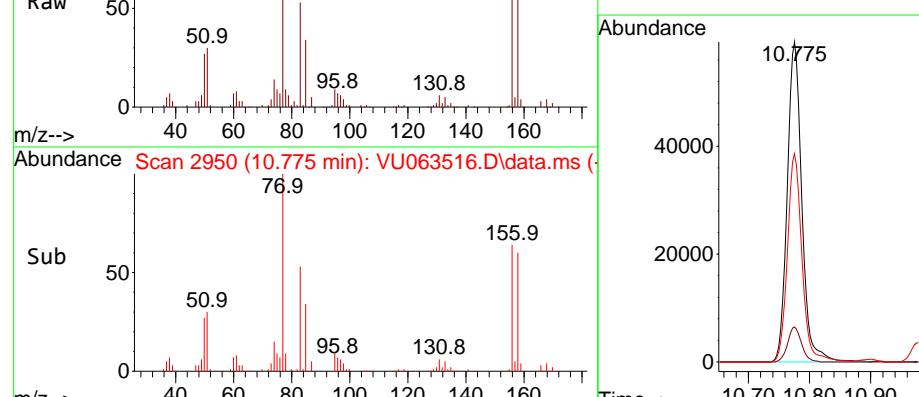



#71

1,2,3-Trichloropropane

Concen: 16.049 ug/l m

RT: 10.817 min Scan# 2963

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#72

Bromobenzene

Concen: 17.363 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Tgt Ion:156 Resp: 128042




Ion Ratio Lower Upper

156 100

77 152.6 0.0 315.2

158 97.1 0.0 195.4

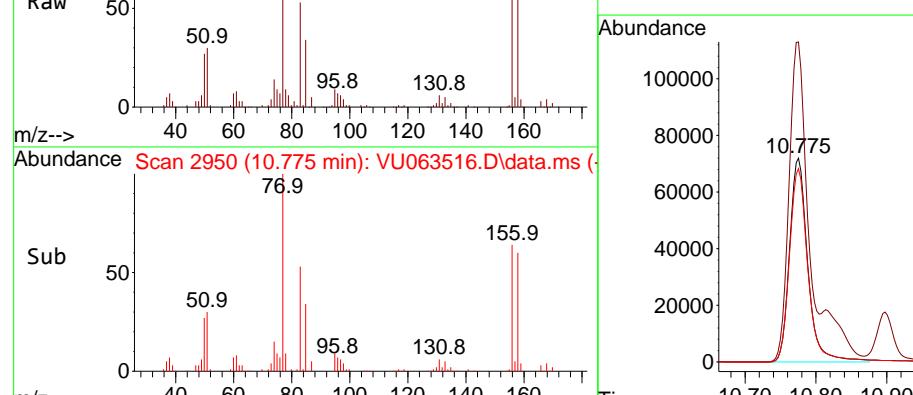

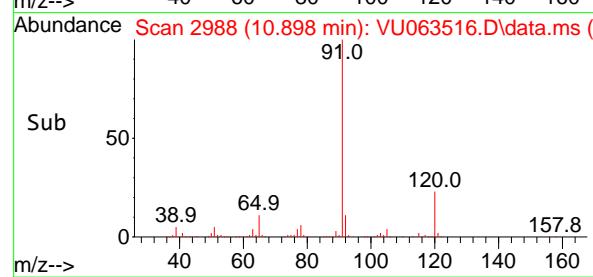

#73

n-propylbenzene

Concen: 17.433 ug/l

RT: 10.898 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11





Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

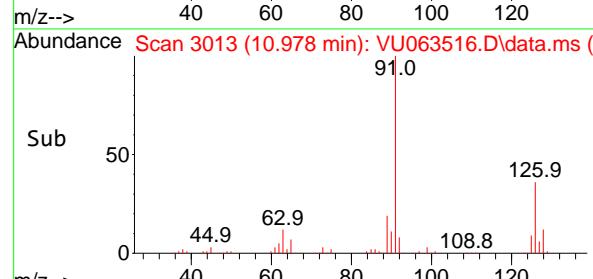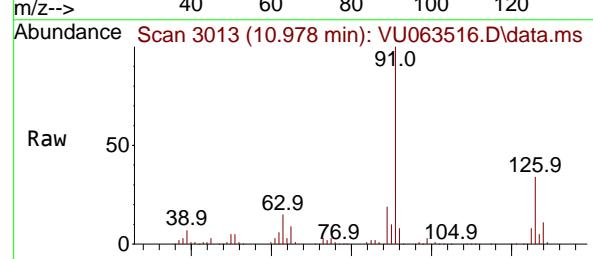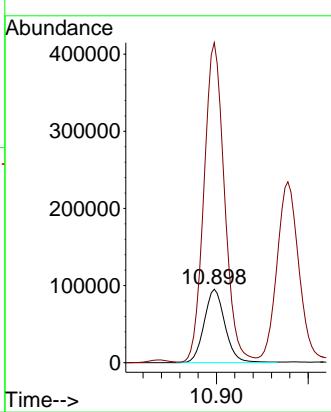 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#74

2-Chlorotoluene

Concen: 17.136 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11




Tgt Ion:126 Resp: 130274

Ion Ratio Lower Upper

126 100

91 299.6 0.0 606.0

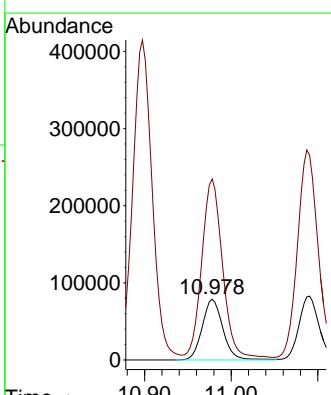







#75
1,3,5-Trimethylbenzene
Concen: 17.511 ug/l
RT: 11.081 min Scan# 3045
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
ClientSampleId : VSTDICC015


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#76
4-Chlorotoluene
Concen: 17.147 ug/l
RT: 11.090 min Scan# 3048
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Tgt Ion:126 Resp: 132384
Ion Ratio Lower Upper
126 100
91 337.8 0.0 682.2

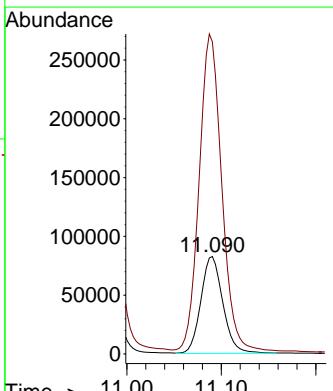



#77

tert-Butylbenzene

Concen: 17.282 ug/l

RT: 11.412 min Scan# 3148

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#78

1,2,4-Trimethylbenzene

Concen: 17.485 ug/l

RT: 11.460 min Scan# 3163

Delta R.T. 0.000 min

Lab File: VU063516.D


Acq: 16 Jul 2025 12:11


Tgt Ion:105 Resp: 473538

Ion Ratio Lower Upper


105 100

120 44.9 22.7 68.0

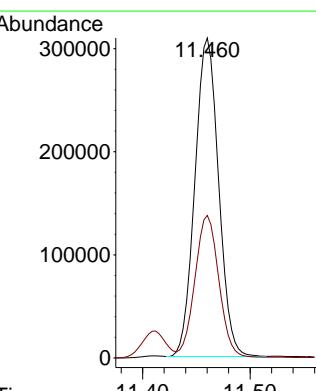




Abundance Scan 3217 (11.634 min): VU063516.D\data.ms (-)

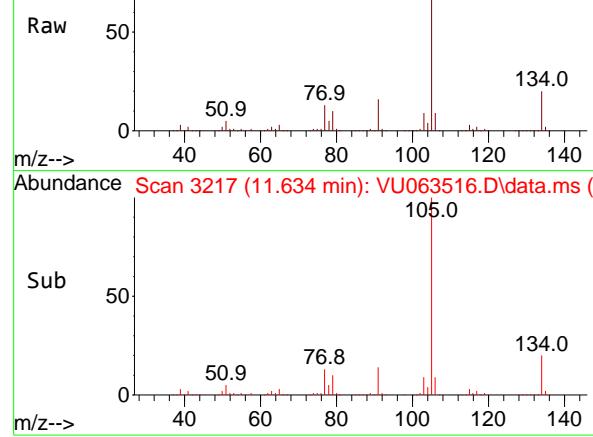

Abundance Scan 3217 (11.634 min): VU063516.D\data.ms (-)

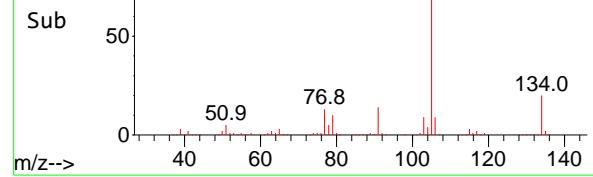

#79

sec-Butylbenzene

Concen: 17.415 ug/l

RT: 11.634 min Scan# 3217

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument:

MSVOA_U


ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025

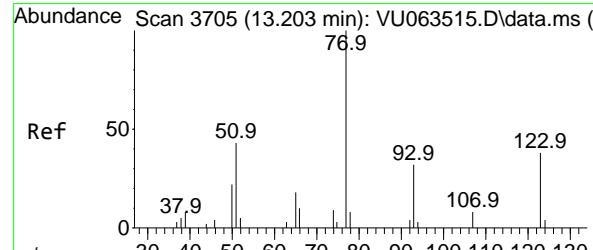

Abundance Scan 3705 (13.203 min): VU063516.D\data.ms (-)



Abundance Scan 3705 (13.203 min): VU063516.D\data.ms (-)

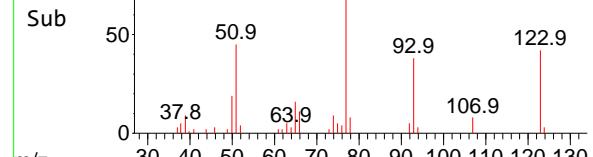

#80

Nitrobenzene

Concen: 74.783 ug/l

RT: 13.203 min Scan# 3705

Delta R.T. -0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Tgt Ion: 77 Resp: 11188

Ion Ratio Lower Upper

77 100

123 42.7 16.9 59.7

65 19.5 16.5 20.9

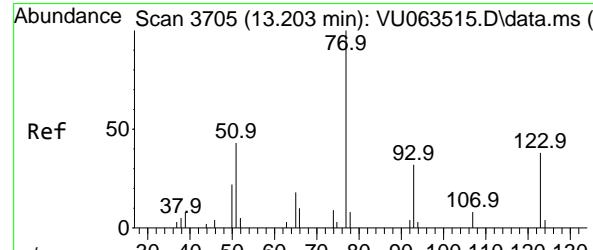

Abundance Scan 3705 (13.203 min): VU063516.D\data.ms (-)





Abundance Scan 3705 (13.203 min): VU063516.D\data.ms (-)



Abundance

Scan 3705 (13.203 min): VU063516.D\data.ms (-)

Time-->



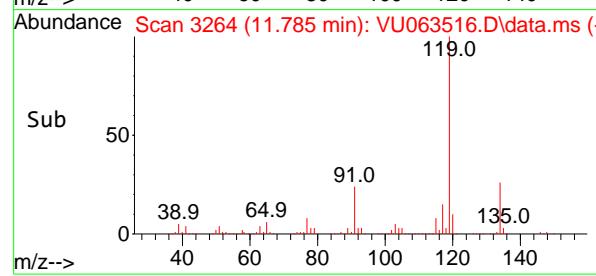



#81
p-Isopropyltoluene
Concen: 17.591 ug/l
RT: 11.785 min Scan# 3264
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Instrument : MSVOA_U
ClientSampleId : VSTDICC015


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

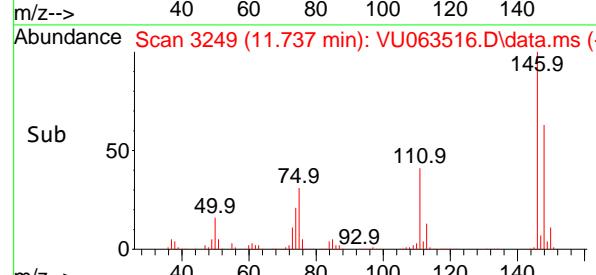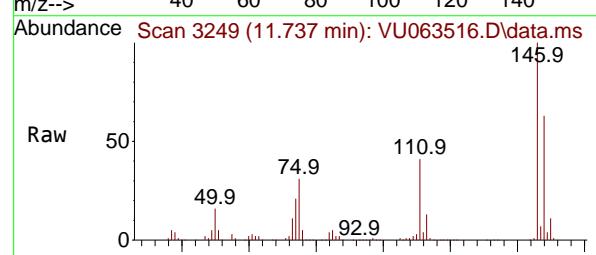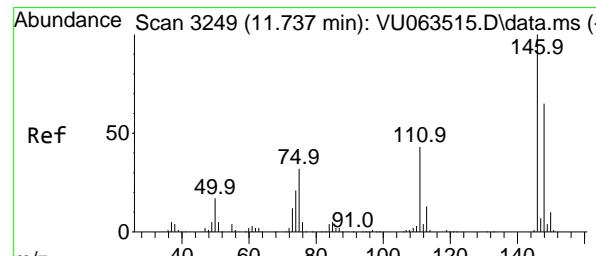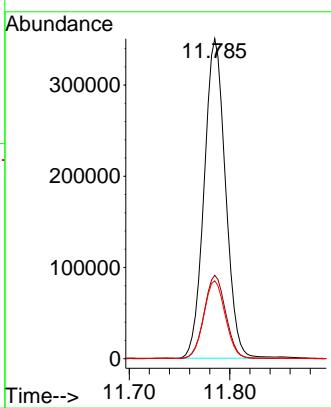

#82
1,3-Dichlorobenzene
Concen: 17.221 ug/l
RT: 11.737 min Scan# 3249
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Tgt Ion:146 Resp: 254102
Ion Ratio Lower Upper
146 100
111 41.5 33.8 50.6
148 63.8 51.5 77.3

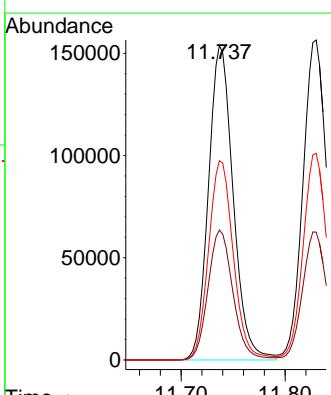

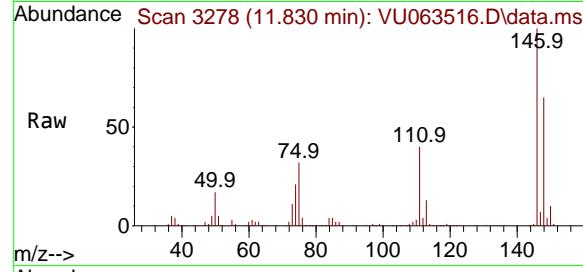

#83

1,4-Dichlorobenzene

Concen: 17.978 ug/l

RT: 11.830 min Scan# 3278

Instrument: MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063516.D





Acq: 16 Jul 2025 12:11

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

Tgt	Ion	Ion Ratio	Resp:	265533
			Lower	Upper
	146	100		
	111	40.6	32.0	48.0
	148	64.3	50.2	75.2

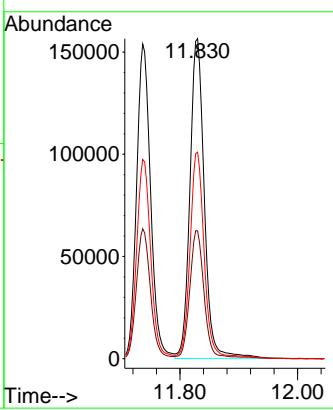

#84

n-Butylbenzene

Concen: 18.081 ug/l


RT: 12.200 min Scan# 3393




Delta R.T. -0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Tgt	Ion	Ion Ratio	Resp:	492464
			Lower	Upper
	91	100		
	92	52.2	41.5	62.3
	134	25.9	20.6	30.8





#85

1,2-Dichlorobenzene

Concen: 17.474 ug/l

RT: 12.203 min Scan# 3

Delta R.T. -0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11




Instrument:



MSVOA_U


ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**

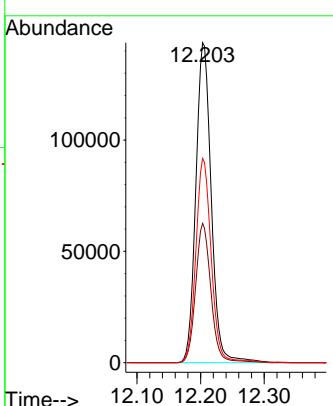 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

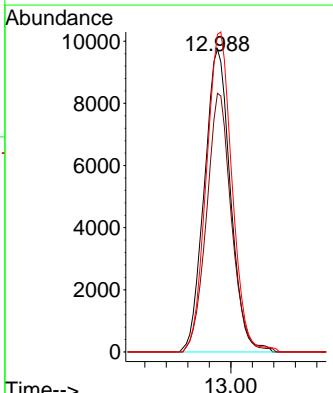 #86
 1,2-Dibromo-3-Chloropropane
 Concen: 14.975 ug/l
 RT: 12.988 min Scan# 3638
 Delta R.T. 0.001 min
 Lab File: VU063516.D
 Acq: 16 Jul 2025 12:11

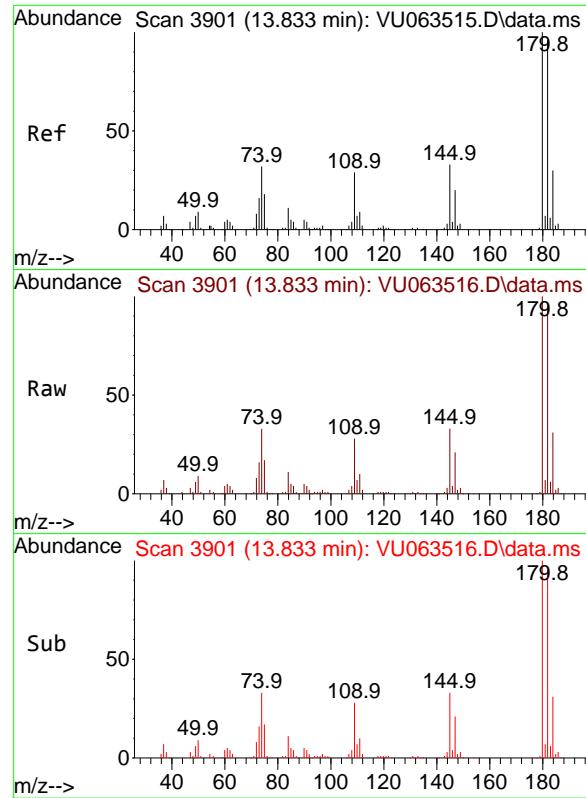 Tgt Ion: 75 Resp: 16421
 Ion Ratio Lower Upper
 75 100
 155 81.4 65.8 98.6
 157 104.0 81.4 122.2




#87

1,2,4-Trichlorobenzene

Concen: 18.396 ug/l

RT: 13.833 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument :

MSVOA_U

ClientSampleId :

VSTDICC015

Tgt Ion:180 Resp: 15857

Ion Ratio Lower Upper

180 100



182 96.5 76.2 114.4

145 32.5 26.2 39.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

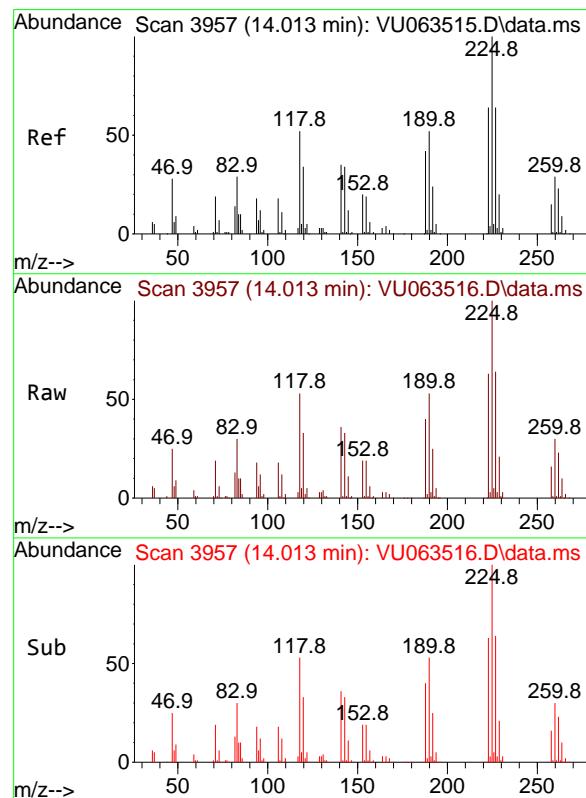

#88

Hexachlorobutadiene

Concen: 17.630 ug/l

RT: 14.013 min Scan# 3957

Delta R.T. 0.000 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11


Tgt Ion:225 Resp: 86303







Ion Ratio Lower Upper

225 100

223 63.1 50.8 76.2

227 63.4 51.0 76.6

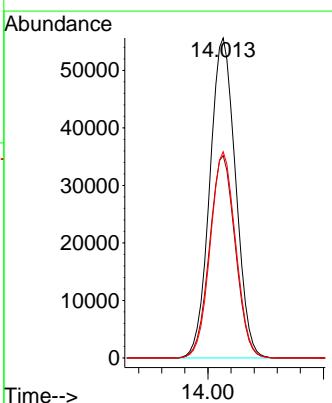

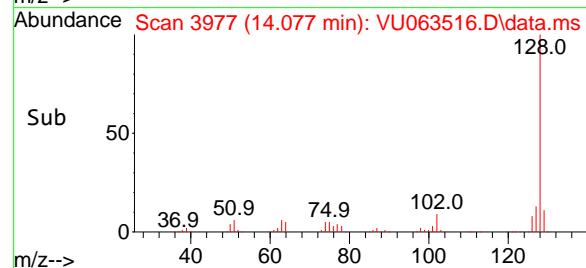

#89

Naphthalene

Concen: 18.966 ug/l

RT: 14.077 min Scan# 3

Delta R.T. -0.003 min

Lab File: VU063516.D

Acq: 16 Jul 2025 12:11

Instrument:

MSVOA_U


ClientSampleId :

VSTDICC015

**Manual Integrations
APPROVED**


Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

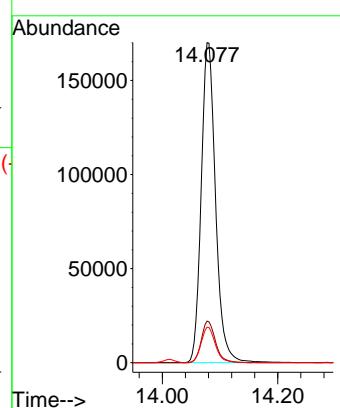

#90
1,2,3-Trichlorobenzene
Concen: 18.735 ug/l
RT: 14.322 min Scan# 4053
Delta R.T. 0.000 min
Lab File: VU063516.D
Acq: 16 Jul 2025 12:11

Tgt Ion:180 Resp: 149249
Ion Ratio Lower Upper
180 100
182 96.1 78.0 117.0
145 33.6 27.3 40.9

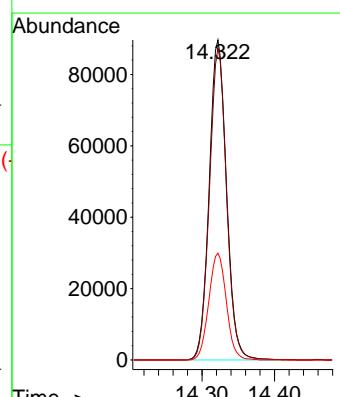

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063517.D
 Acq On : 16 Jul 2025 14:19
 Operator : MD/SY
 Sample : VSTDICV010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Quant Time: Jul 17 03:27:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.100	96	22543	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	10918	1.279	ug/l	0.00
Spiked Amount 1.000			Recovery	=	128.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	9055	1.147	ug/l	0.00
Spiked Amount 1.000			Recovery	=	115.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	47518	7.149	ug/l	98
3) Chloromethane	1.518	50	59639	9.652	ug/l	99
4) Vinyl Chloride	1.599	62	75020	9.533	ug/l	99
5) Bromomethane	1.846	94	57124	9.626	ug/l	97
6) Chloroethane	1.924	64	48669	10.243	ug/l	100
7) Trichlorofluoromethane	2.129	101	117095	10.364	ug/l	99
8) 1,1,2-Trichloro-1,2,2-...	2.567	101	67543	11.439	ug/l	98
9) 1,1-Dichloroethene	2.567	96	68402	11.688	ug/l	95
10) Iodomethane	2.708	142	78640	9.080	ug/l	98
11) Allyl Chloride	2.907	41	104721	12.385	ug/l	99
12) Acrylonitrile	3.306	53	78654	53.704	ug/l	97
13) Acetone	2.618	43	76920	65.587	ug/l	100
14) Carbon Disulfide	2.776	76	197248	10.434	ug/l	99
15) Methylene Chloride	3.026	84	76711	11.133	ug/l	98
16) trans-1,2-Dichloroethene	3.332	96	71158	10.705	ug/l	98
17) 1,1-Dichloroethane	3.846	63	140320	11.390	ug/l	100
18) 2-Butanone	4.714	43	107346	59.104	ug/l	99
19) Cyclohexane	5.357	56	120201	11.523	ug/l	100
20) Methylcyclohexane	6.743	83	103883	10.246	ug/l	98
21) 2,2-Dichloropropane	4.644	77	118031	11.251	ug/l	100
22) cis-1,2-Dichloroethene	4.647	96	84773	11.753	ug/l	97
23) Diethyl Ether	2.370	59	48588	10.895	ug/l	99
24) tert-Butyl Alcohol	3.194	59	29533	54.858	ug/l	99
25) Methyl tert-Butyl Ether	3.361	73	182299	11.931	ug/l	99
26) Bromochloromethane	4.956	128	32227	10.701	ug/l	95
27) Chloroform	5.068	83	141992	11.295	ug/l	100
28) 1,1,1-Trichloroethane	5.293	97	124774	11.694	ug/l	100
29) 1,1-Dichloropropene	5.499	75	104813	10.604	ug/l	97
30) Carbon Tetrachloride	5.496	117	102031	11.881	ug/l	96
31) Isopropyl Ether	3.994	45	217473	11.694	ug/l	# 1
34) Propionitrile	4.775	54	61045	110.315	ug/l	96
35) Benzene	5.753	78	251880	9.485	ug/l	99
36) 1,2-Dichloroethane	5.782	62	75983	9.208	ug/l	99
37) Trichloroethene	6.525	130	66834	9.864	ug/l	95
38) 1,2-Dichloropropane	6.782	63	63102	10.152	ug/l	98
39) Methacrylonitrile	4.972	41	25678	10.571	ug/l	98
40) Methyl acrylate	4.846	55	39416	10.962	ug/l	# 95
41) Tetrahydrofuran	5.062	42	67337	52.040	ug/l	97
42) 1-Chlorobutane	5.435	56	151540	11.532	ug/l	99
43) Dibromomethane	6.907	93	35899	11.149	ug/l	97
44) Bromodichloromethane	7.094	83	84311	11.611	ug/l	97
45) 4-Methyl-2-Pentanone	7.795	43	190879	57.520	ug/l	100
46) t-1,4-Dichloro-2-butene	10.827	75	12861m	10.924	ug/l	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063517.D
 Acq On : 16 Jul 2025 14:19
 Operator : MD/SY
 Sample : VSTDICV010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Quant Time: Jul 17 03:27:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
47) Methyl methacrylate	6.965	69	30655	11.336	ug/l	92
48) Ethyl methacrylate	8.332	69	62257	12.064	ug/l	100
49) Toluene	7.959	92	167696	11.565	ug/l	97
50) t-1,3-Dichloropropene	8.203	75	69274	12.160	ug/l	99
51) cis-1,3-Dichloropropene	7.599	75	87222	11.406	ug/l	99
52) 1,1,2-Trichloroethane	8.393	97	47565	10.973	ug/l	98
53) 1,3-Dichloropropane	8.566	76	81190	10.849	ug/l	99
54) 2-Hexanone	8.685	43	130609	59.254	ug/l	99
55) Dibromochloromethane	8.801	129	56885	12.417	ug/l	99
56) 1,2-Dibromoethane	8.917	107	42078	10.846	ug/l	98
58) Tetrachloroethene	8.541	164	70149	11.312	ug/l	98
59) Chlorobenzene	9.438	112	192479	11.557	ug/l	99
60) 1,1,1,2-Tetrachloroethane	9.524	131	58716	10.964	ug/l	98
61) Pentachloroethane	11.418	117	46643	12.325	ug/l	98
62) Hexachloroethane	12.466	117	46374	12.375	ug/l	100
63) Ethyl Benzene	9.560	91	327850	11.440	ug/l	100
64) m/p-Xylenes	9.685	106	261516	23.477	ug/l	98
65) o-Xylene	10.090	106	128236	11.980	ug/l	99
66) Styrene	10.106	104	207563	12.168	ug/l	99
67) Bromoform	10.283	173	28453	12.093	ug/l	100
69) Isopropylbenzene	10.476	105	336555	13.006	ug/l	100
70) 1,1,2,2-Tetrachloroethane	10.775	83	56769	10.762	ug/l	99
71) 1,2,3-Trichloropropane	10.814	75	39518m	9.180	ug/l	
72) Bromobenzene	10.775	156	77499	11.605	ug/l	99
73) n-propylbenzene	10.897	120	92519	11.877	ug/l	100
74) 2-Chlorotoluene	10.978	126	81148	11.787	ug/l	97
75) 1,3,5-Trimethylbenzene	11.081	105	296624	11.999	ug/l	98
76) 4-Chlorotoluene	11.090	126	83551	11.950	ug/l	96
77) tert-Butylbenzene	11.412	119	282930	11.976	ug/l	100
78) 1,2,4-Trimethylbenzene	11.460	105	296010	12.070	ug/l	99
79) sec-Butylbenzene	11.634	105	381524	11.975	ug/l	99
80) Nitrobenzene	13.216	77	1132m	13.031	ug/l	
81) p-Isopropyltoluene	11.785	119	326583	12.280	ug/l	99
82) 1,3-Dichlorobenzene	11.737	146	159160	11.911	ug/l	99
83) 1,4-Dichlorobenzene	11.830	146	155981	11.662	ug/l	97
84) n-Butylbenzene	12.200	91	300975	12.202	ug/l	98
85) 1,2-Dichlorobenzene	12.206	146	150510	11.990	ug/l	99
86) 1,2-Dibromo-3-Chloropr...	12.987	75	9053	10.124	ug/l	99
87) 1,2,4-Trichlorobenzene	13.833	180	98543	12.623	ug/l	100
88) Hexachlorobutadiene	14.013	225	51315	11.575	ug/l	98
89) Naphthalene	14.081	128	165643	11.841	ug/l	99
90) 1,2,3-Trichlorobenzene	14.322	180	85042	11.788	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
Data File : VU063517.D
Acq On : 16 Jul 2025 14:19
Operator : MD/SY
Sample : VSTDICV010
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1


Quant Time: Jul 17 03:27:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:16:16 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

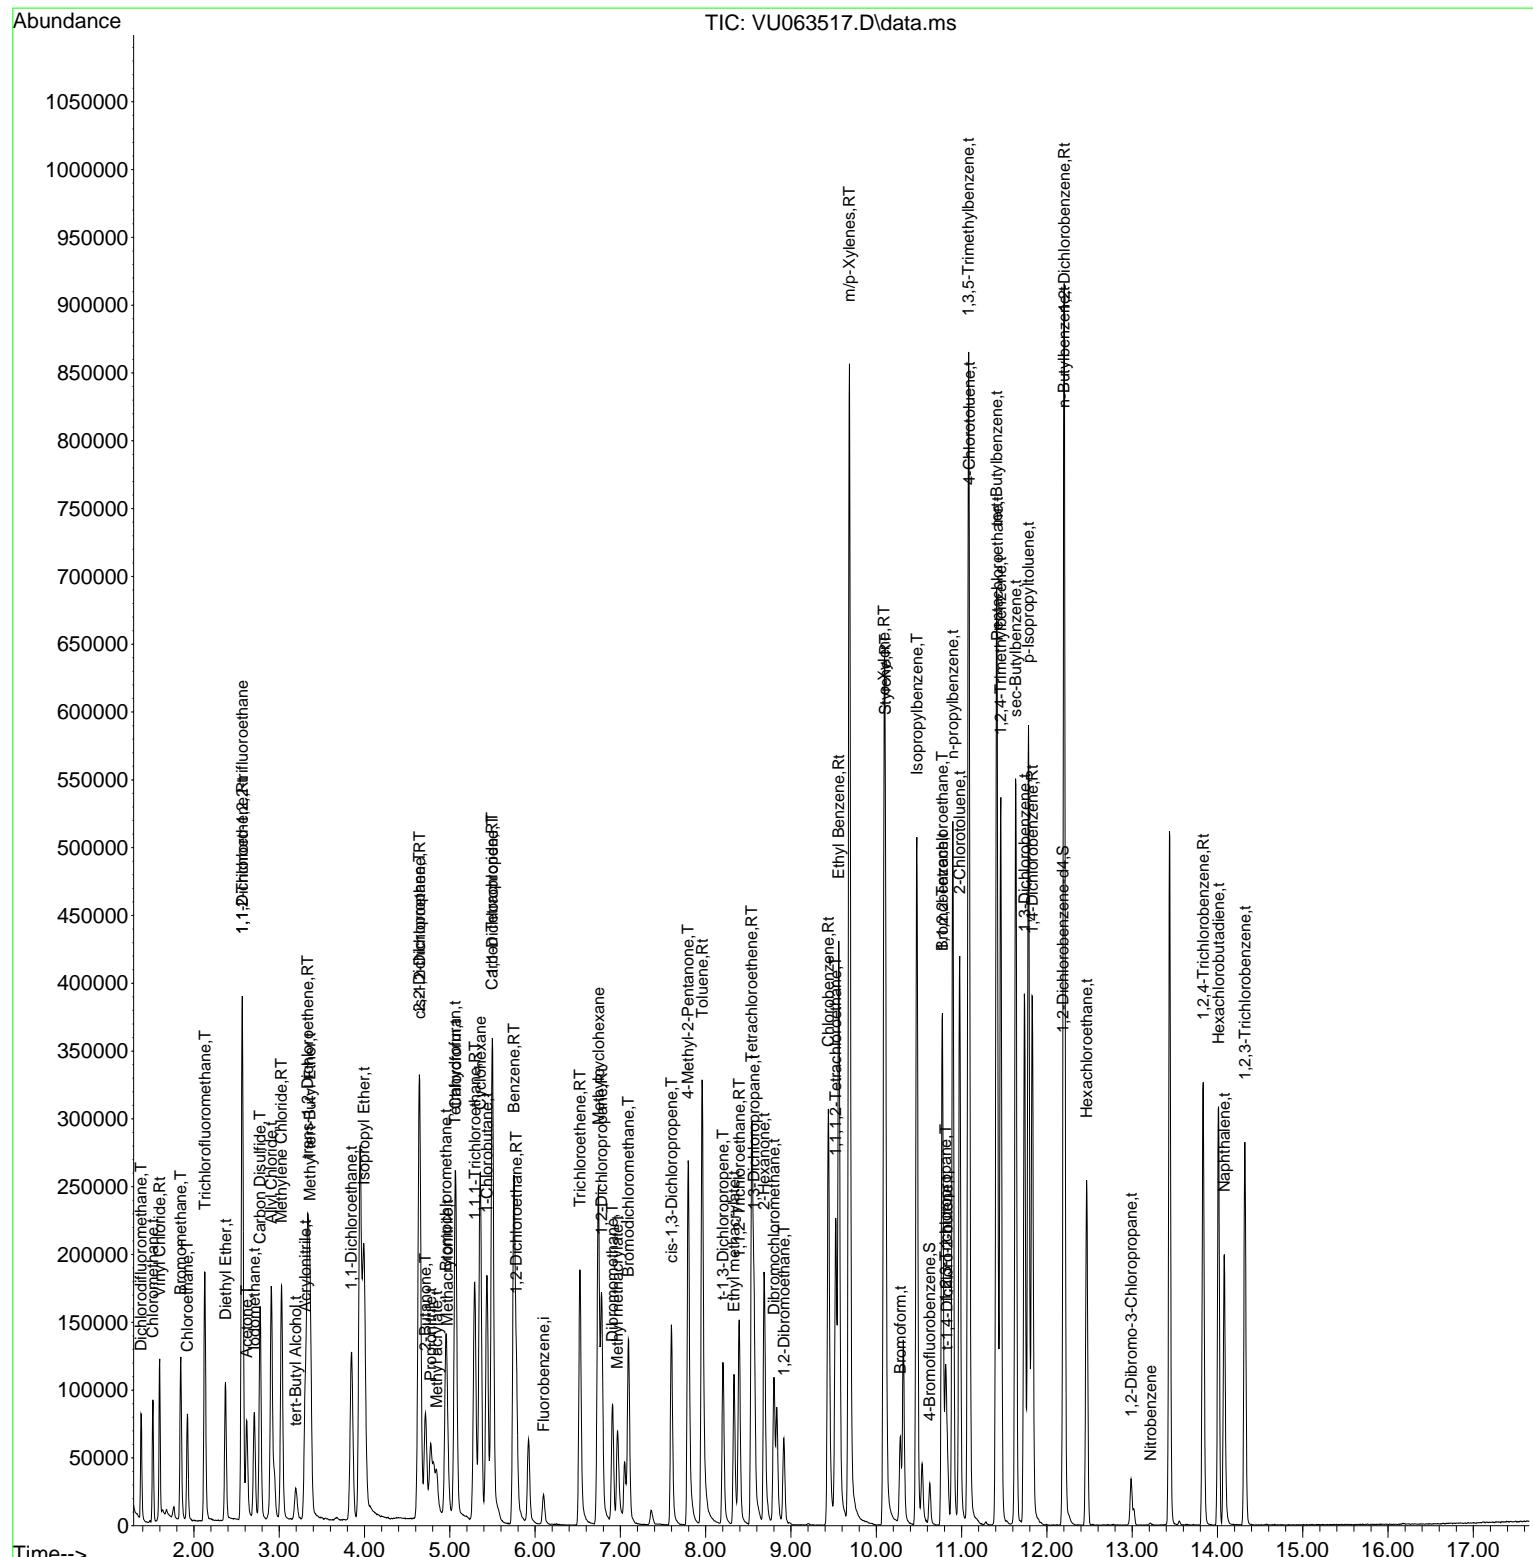



#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Instrument : MSVOA_U
ClientSampleId : ICVVU071625




Tgt Ion: 96 Resp: 2254
Ion Ratio Lower Upper
96 100
70 19.0 15.0 22.4
95 8.3 7.4 11.0
97 0.0 0.0 0.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025


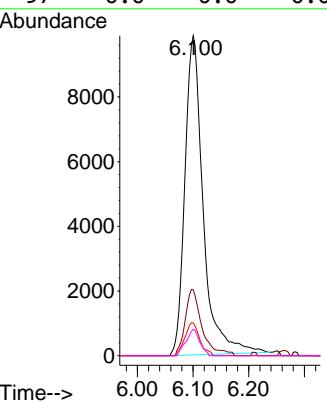



#2
Dichlorodifluoromethane
Concen: 7.149 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19



Tgt Ion: 85 Resp: 47518
Ion Ratio Lower Upper
85 100
87 32.8 16.0 47.9



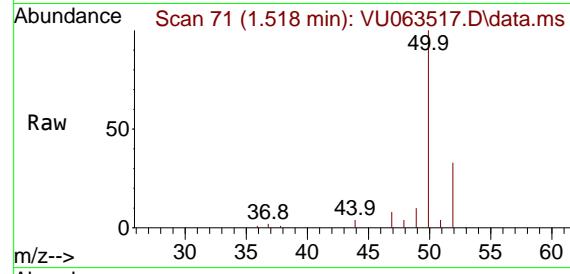

#3

Chloromethane

Concen: 9.652 ug/l

RT: 1.518 min Scan# 71

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

Tgt Ion: 50 Resp: 59639

Ion Ratio Lower Upper





50 100

52 32.6 26.3 39.5

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

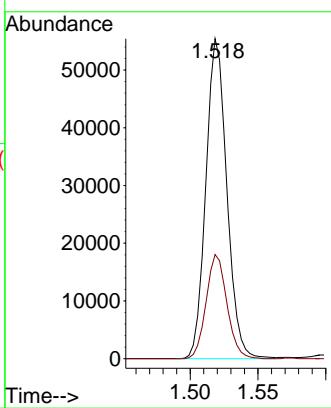

#4

Vinyl Chloride

Concen: 9.533 ug/l

RT: 1.599 min Scan# 96

Delta R.T. 0.000 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19




Tgt Ion: 62 Resp: 75020

Ion Ratio Lower Upper

62 100

64 32.4 25.7 38.5

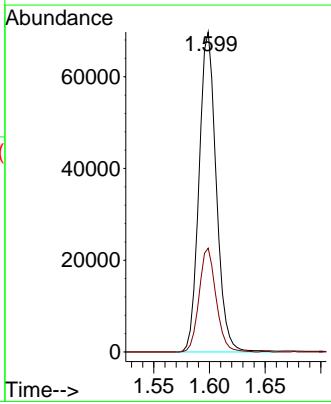



#5

Bromomethane

Concen: 9.626 ug/l

RT: 1.846 min Scan# 1

Delta R.T. 0.007 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19





Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

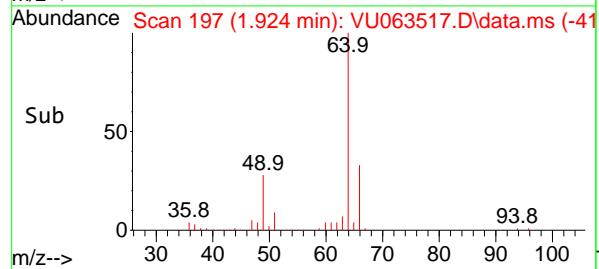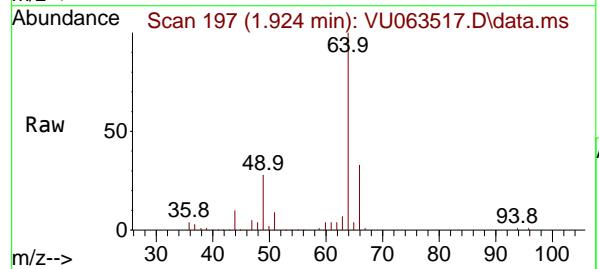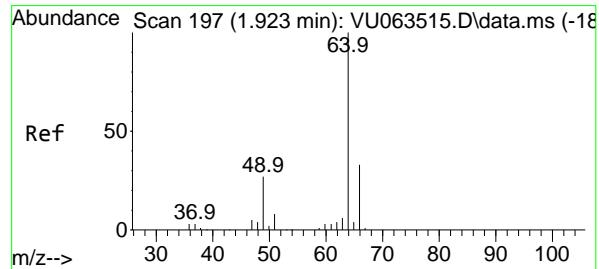 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#6

Chloroethane


Concen: 10.243 ug/l




RT: 1.924 min Scan# 197

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

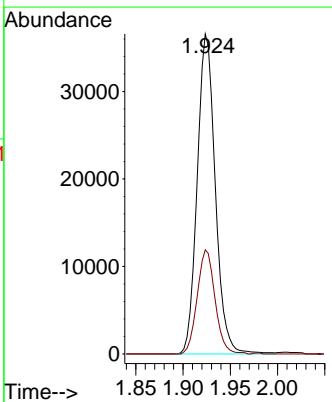 Tgt Ion: 64 Resp: 48669
 Ion Ratio Lower Upper
 64 100
 66 32.5 26.2 39.4

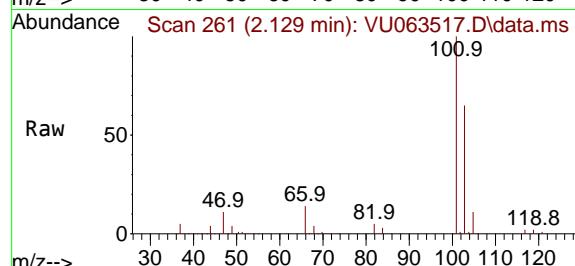



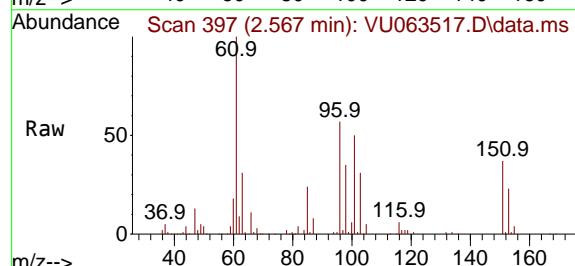


#7

Trichlorofluoromethane
Concen: 10.364 ug/l
RT: 2.129 min Scan# 2
Delta R.T. 0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#8

1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 11.439 ug/l
RT: 2.567 min Scan# 397
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19


Tgt Ion:101 Resp: 67543
Ion Ratio Lower Upper
101 100
85 48.3 37.8 56.6
151 75.8 59.2 88.8





#9
1,1-Dichloroethene
Concen: 11.688 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Instrument : MSVOA_U
ClientSampleId : ICVVU071625




Tgt Ion: 96 Resp: 6840
Ion Ratio Lower Upper
96 100
61 176.2 0.0 504.3
98 62.3 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025









#10
Iodomethane
Concen: 9.080 ug/l
RT: 2.708 min Scan# 441
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19



Tgt Ion:142 Resp: 78640
Ion Ratio Lower Upper
142 100
127 48.4 37.9 56.9

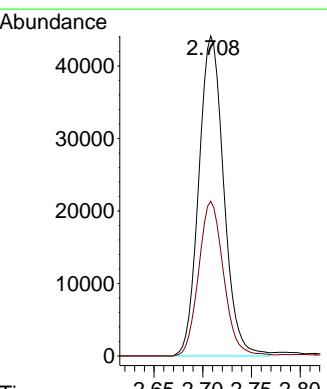

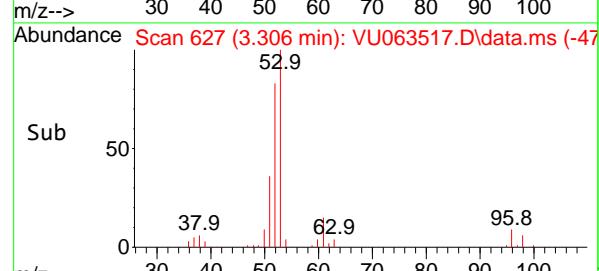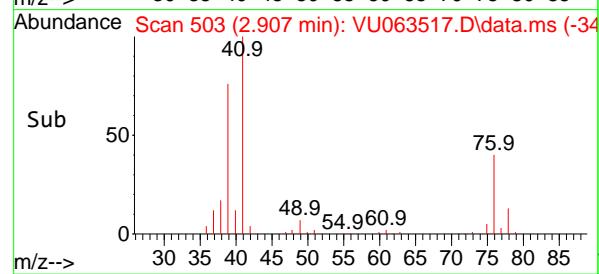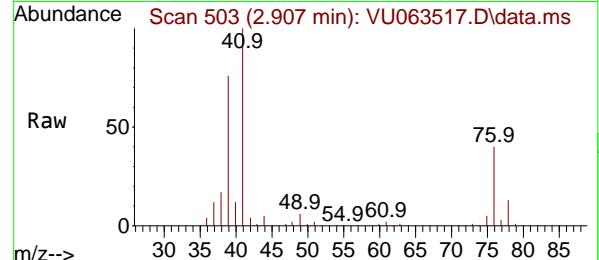

#11

Allyl Chloride

Concen: 12.385 ug/l

RT: 2.907 min Scan# 5

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

Tgt Ion: 41 Resp: 10472

Ion Ratio Lower Upper

41 100


39 75.9 61.5 92.3

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

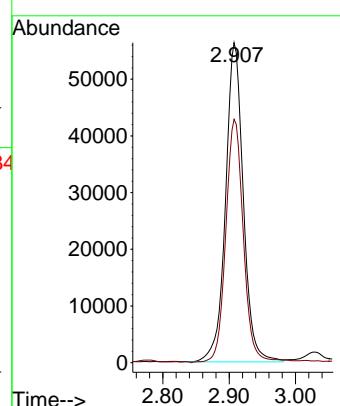

#12

Acrylonitrile

Concen: 53.704 ug/l

RT: 3.306 min Scan# 627

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion: 53 Resp: 78654






Ion Ratio Lower Upper

53 100

52 81.9 64.3 96.5

51 38.3 27.8 41.8

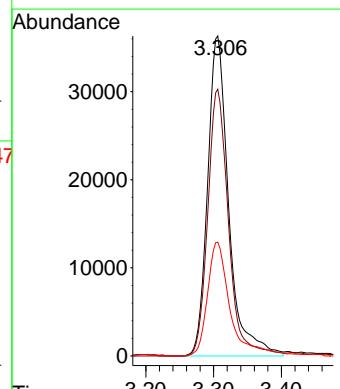

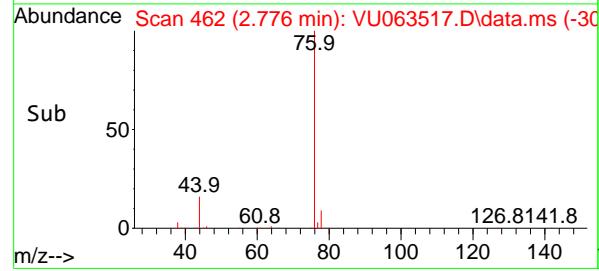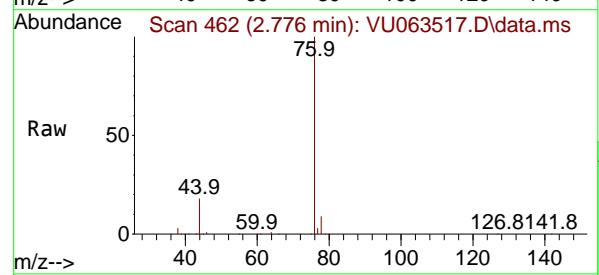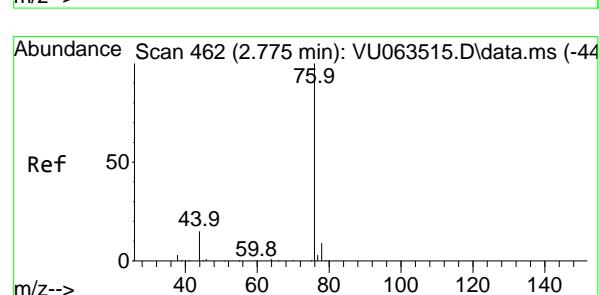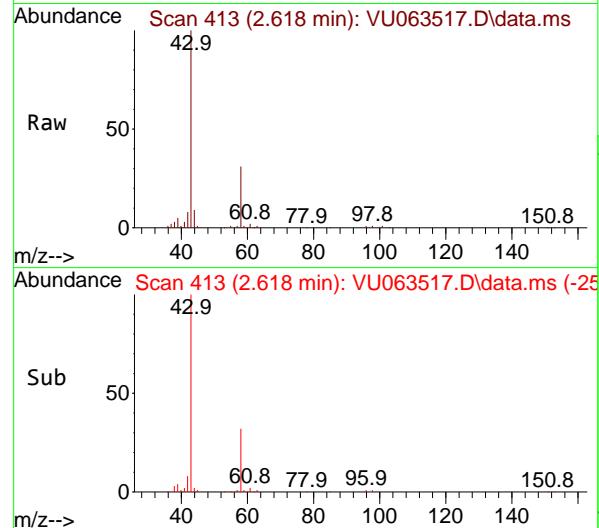

#13

Acetone
Concen: 65.587 ug/l

RT: 2.618 min Scan# 4

Delta R.T. 0.000 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

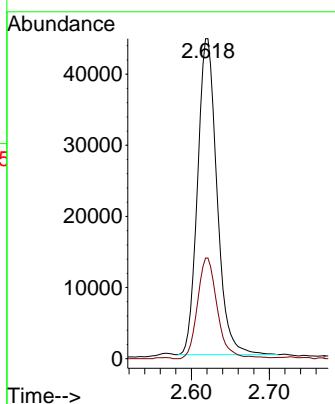**Manual Integrations
APPROVED**Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#14

Carbon Disulfide

Concen: 10.434 ug/l

RT: 2.776 min Scan# 462

Delta R.T. 0.000 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19







Tgt Ion: 76 Resp: 197248

Ion Ratio Lower Upper

76 100

78 9.2 7.0 10.6



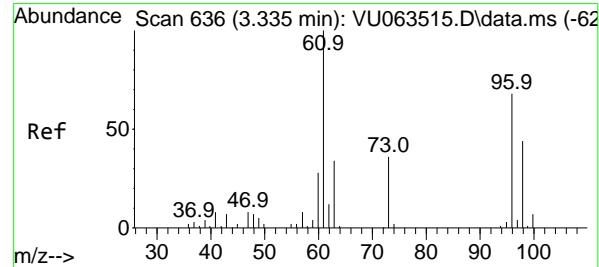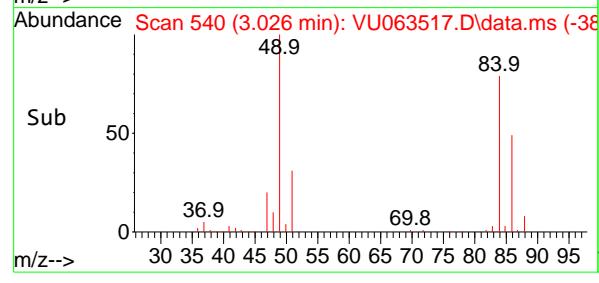

#15

Methylene Chloride

Concen: 11.133 ug/l

RT: 3.026 min Scan# 541

Delta R.T. -0.003 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

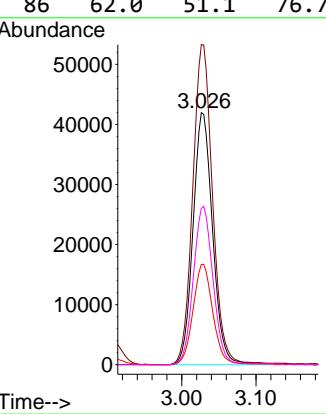**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#16

trans-1,2-Dichloroethene

Concen: 10.705 ug/l

RT: 3.332 min Scan# 635


Delta R.T. -0.003 min


Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt Ion: 96 Resp: 71158

Ion	Ratio	Lower	Upper
96	100		
61	148.2	117.2	175.8
98	61.6	51.4	77.2

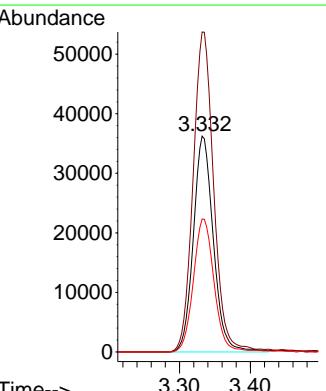


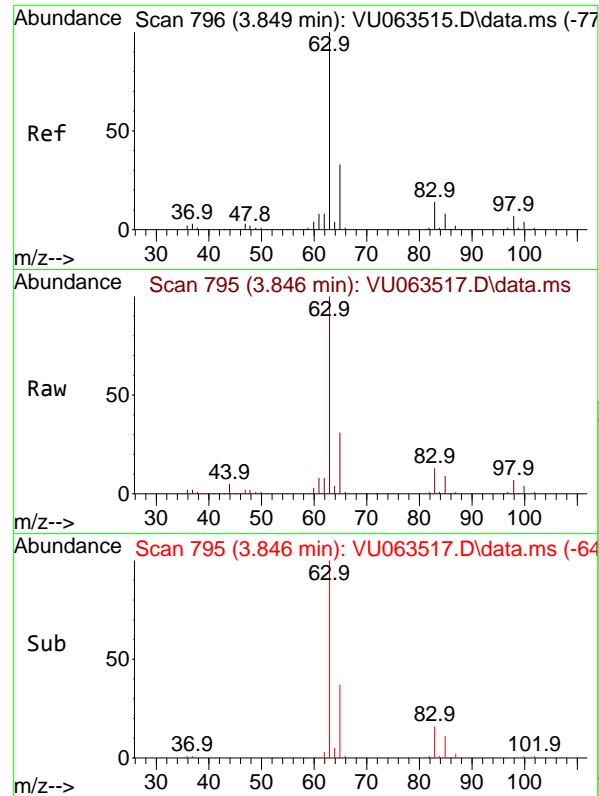


#17
1,1-Dichloroethane
Concen: 11.390 ug/l
RT: 3.846 min Scan# 7
Delta R.T. -0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

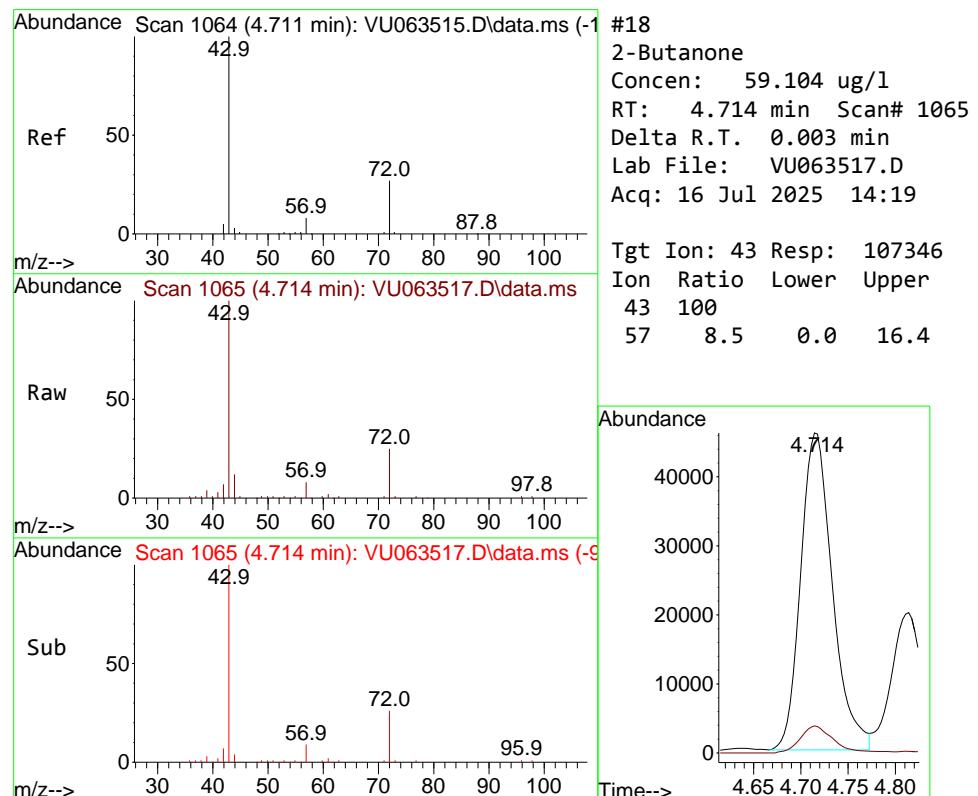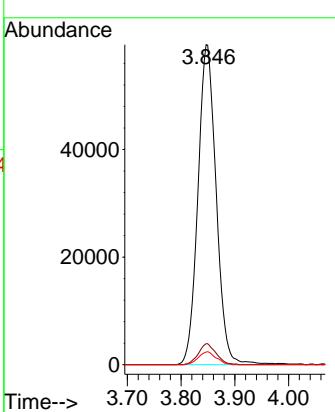

#18
2-Butanone
Concen: 59.104 ug/l
RT: 4.714 min Scan# 1065
Delta R.T. 0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Tgt Ion: 43 Resp: 107346
Ion Ratio Lower Upper
43 100
57 8.5 0.0 16.4

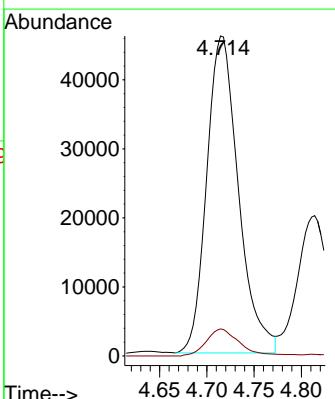



#19

Cyclohexane

Concen: 11.523 ug/l

RT: 5.357 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

Abundance Scan 1265 (5.357 min): VU063517.D\data.ms

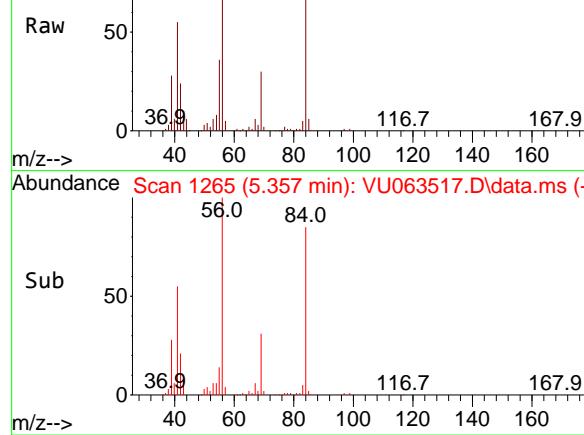






Tgt Ion: 56 Resp: 12020







Ion Ratio Lower Upper

56 100

69 33.2 26.6 39.8

84 88.4 71.0 106.4

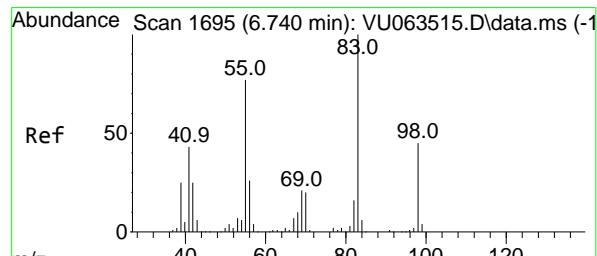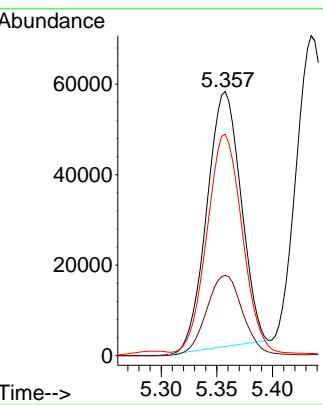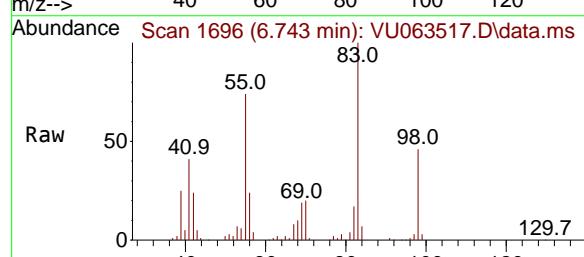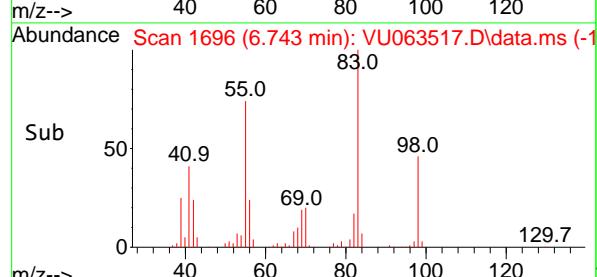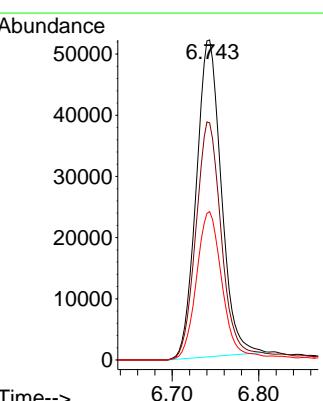**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025#20
Methylcyclohexane
Concen: 10.246 ug/l
RT: 6.743 min Scan# 1696
Delta R.T. 0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19Tgt Ion: 83 Resp: 103883
Ion Ratio Lower Upper
83 100
55 75.1 60.6 90.8
98 48.3 35.8 53.8

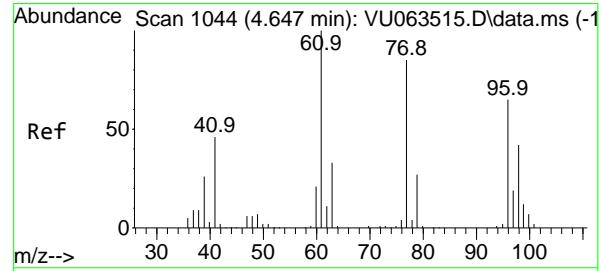

#21

2,2-Dichloropropane

Concen: 11.251 ug/l

RT: 4.644 min Scan# 11803

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#22

cis-1,2-Dichloroethene

Concen: 11.753 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion: 96 Resp: 84773




Ion Ratio Lower Upper

96 100

61 158.2 0.0 384.7

98 65.6 32.1 96.3



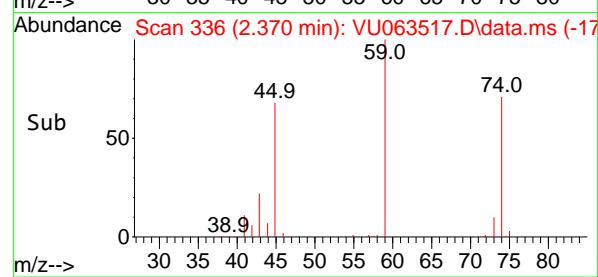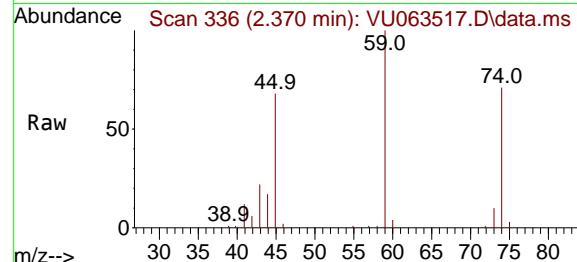

#23

Diethyl Ether

Concen: 10.895 ug/l

RT: 2.370 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U





ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

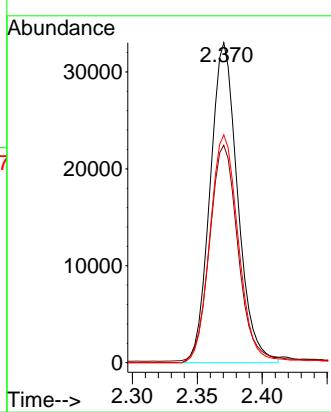

#24

tert-Butyl Alcohol

Concen: 54.858 ug/l


RT: 3.194 min Scan# 592



Delta R.T. 0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt Ion:	59	Resp:	29533
Ion Ratio	100	Lower	Upper
59	100		
57	11.1	8.6	12.8

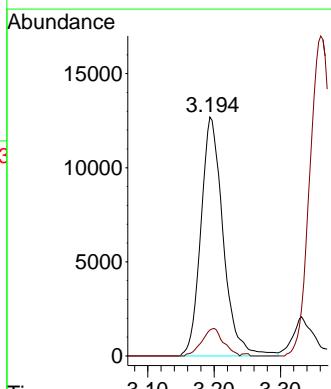

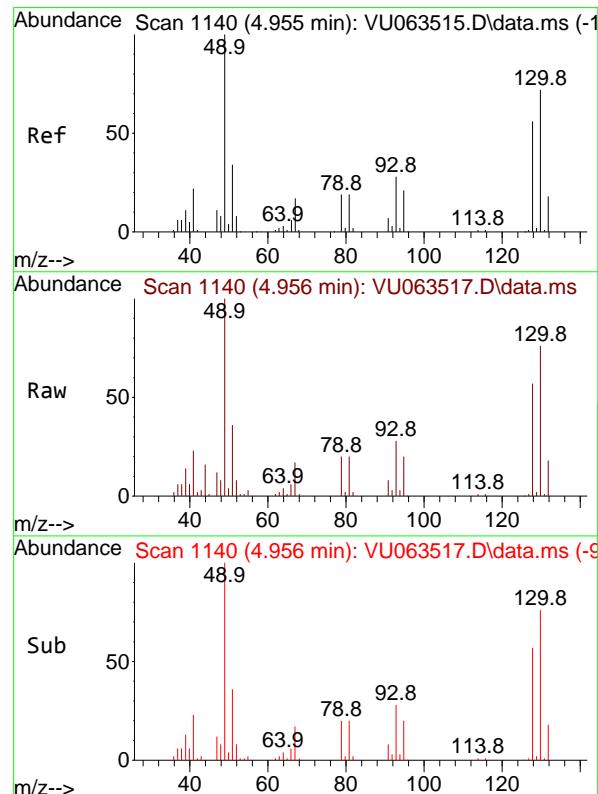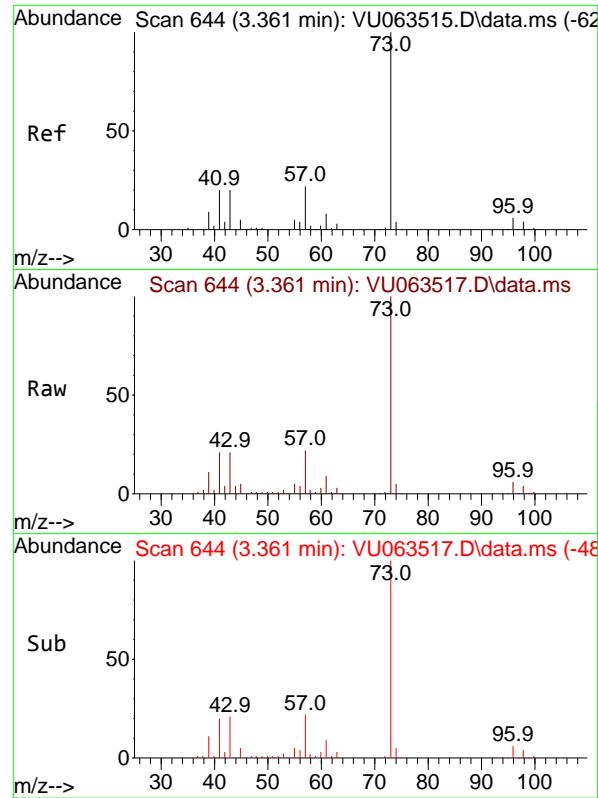


#25

Methyl tert-Butyl Ether
Concen: 11.931 ug/l
RT: 3.361 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025




#26

Bromochloromethane
Concen: 10.701 ug/l
RT: 4.956 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Tgt Ion:128 Resp: 32227
Ion Ratio Lower Upper
128 100
49 178.8 0.0 340.8
130 128.9 100.5 150.7

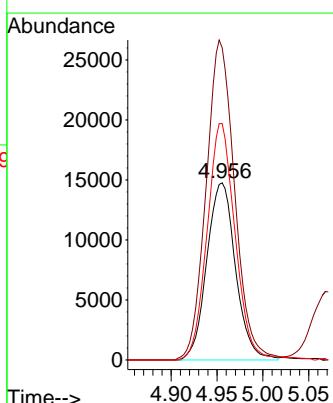


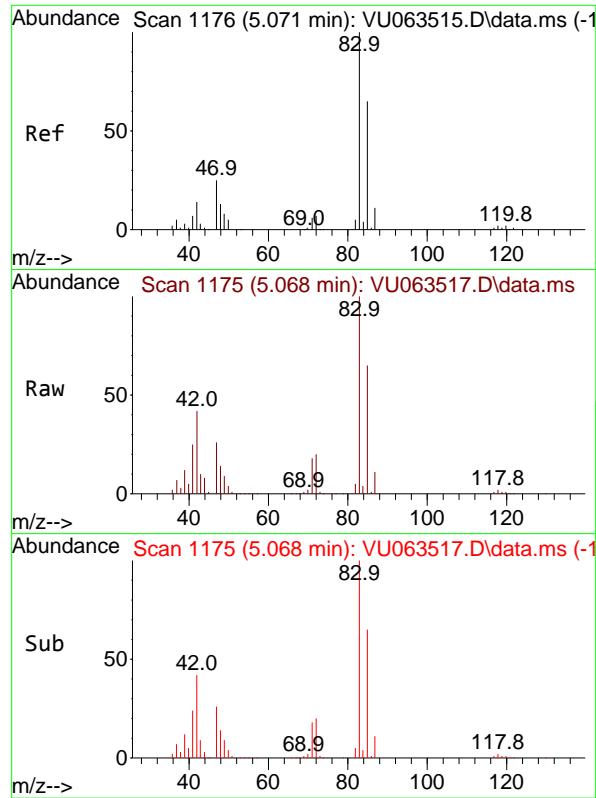


#27
Chloroform
Concen: 11.295 ug/l
RT: 5.068 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

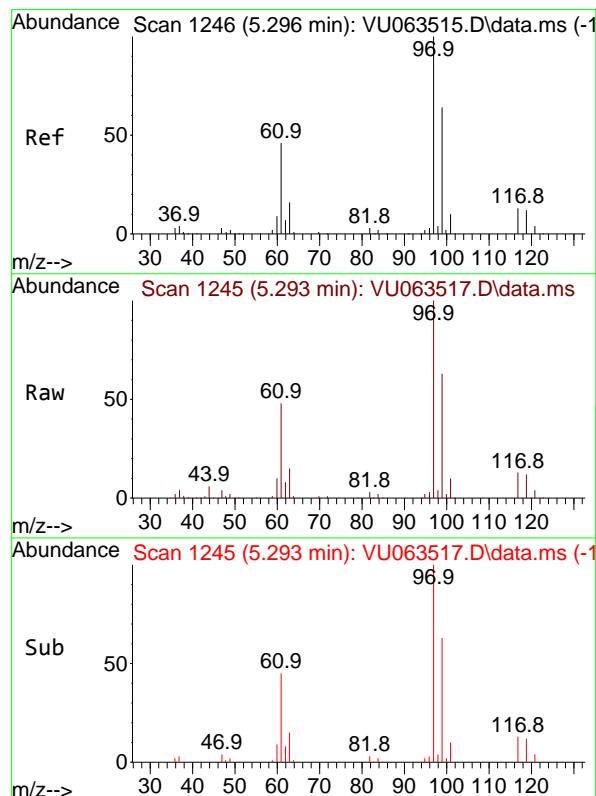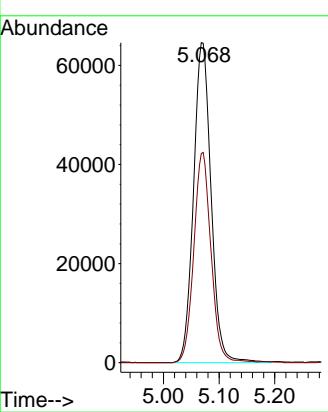

#28
1,1,1-Trichloroethane
Concen: 11.694 ug/l
RT: 5.293 min Scan# 1245
Delta R.T. -0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Tgt Ion: 97 Resp: 124774
Ion Ratio Lower Upper
97 100
99 63.6 31.8 95.3
61 46.7 23.3 69.9



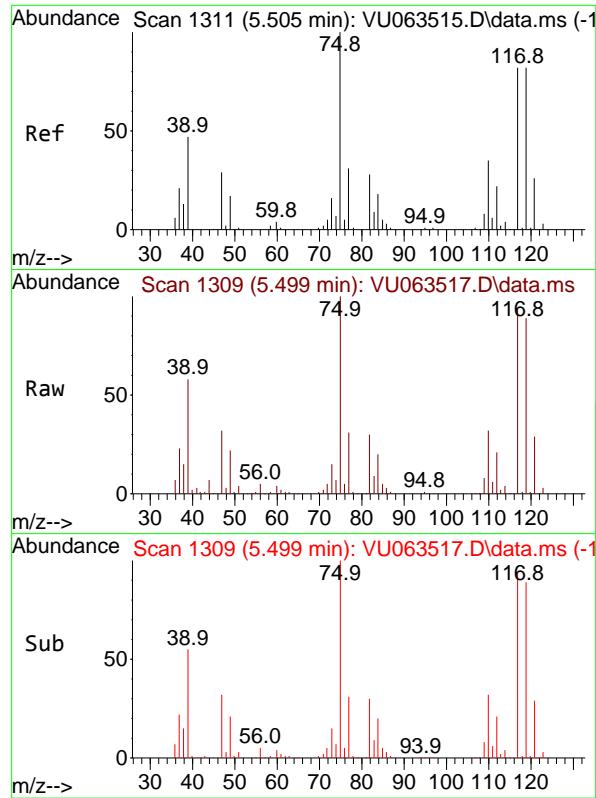

#29

1,1-Dichloropropene

Concen: 10.604 ug/l

RT: 5.499 min Scan# 1

Delta R.T. -0.006 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U



ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

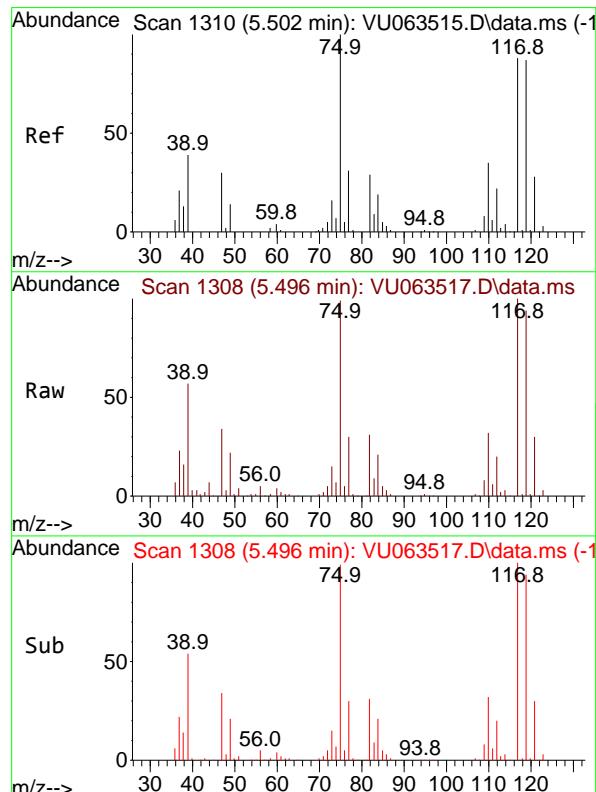

#30

Carbon Tetrachloride

Concen: 11.881 ug/l


RT: 5.496 min Scan# 1308


Delta R.T. -0.006 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt	Ion:117	Resp:	102031
Ion	Ratio	Lower	Upper
117	100		
119	94.1	79.2	118.8
121	30.2	25.5	38.3





#31

Isopropyl Ether

Concen: 11.694 ug/l

RT: 3.994 min Scan# 81

Delta R.T. 0.003 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625



Tgt Ion: 45 Resp: 21747

Ion Ratio Lower Upper







45 100


43 280.0 25.7 77.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025


Supervised By :Semsettin Yesilyurt 07/17/2025
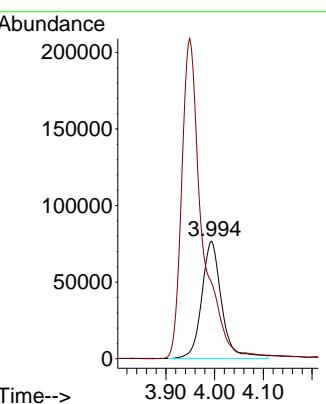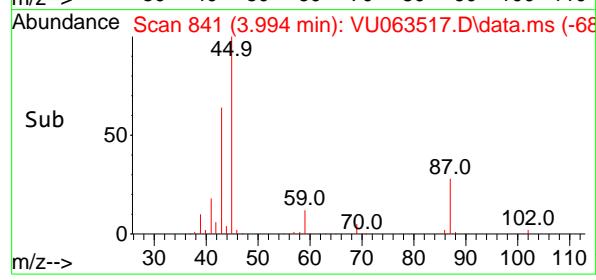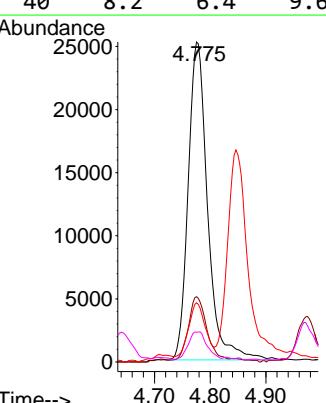
#34
Propionitrile
Concen: 110.315 ug/l
RT: 4.775 min Scan# 1084
Delta R.T. 0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19Tgt Ion: 54 Resp: 61045
Ion Ratio Lower Upper
54 100
52 18.3 17.0 25.4
55 15.3 13.6 20.4
40 8.2 6.4 9.6



#35
Benzene
Concen: 9.485 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Instrument : MSVOA_U
ClientSampleId : ICVVU071625




Tgt Ion: 78 Resp: 251880
Ion Ratio Lower Upper
78 100
77 23.7 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

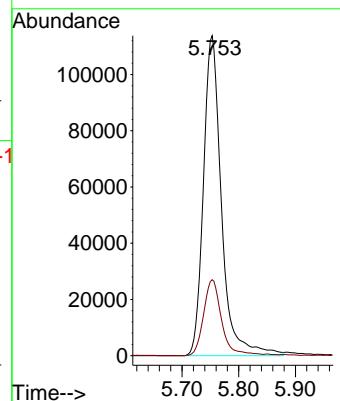


#36
1,2-Dichloroethane
Concen: 9.208 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Tgt Ion: 62 Resp: 75983
Ion Ratio Lower Upper
62 100
98 8.4 6.4 9.6

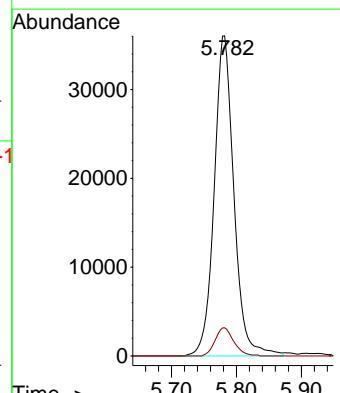



#37
Trichloroethene
Concen: 9.864 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19



Instrument : MSVOA_U
ClientSampleId : ICVVU071625




Tgt Ion:130 Resp: 66834
Ion Ratio Lower Upper
130 100
95 105.0 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025






#38
1,2-Dichloropropane
Concen: 10.152 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19



Tgt Ion: 63 Resp: 63102
Ion Ratio Lower Upper
63 100
65 32.0 24.6 36.8

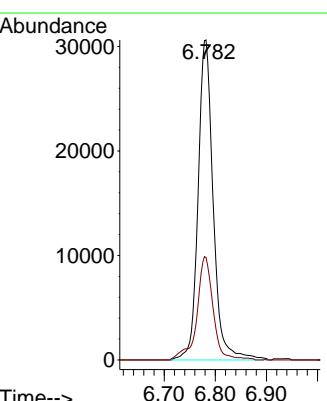



#39

Methacrylonitrile

Concen: 10.571 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025

Tgt Ion: 41 Resp: 2567

Ion Ratio Lower Upper




41 100

67 80.4 62.7 94.1

39 55.5 43.1 64.7

52 35.8 27.4 41.0

Abundance

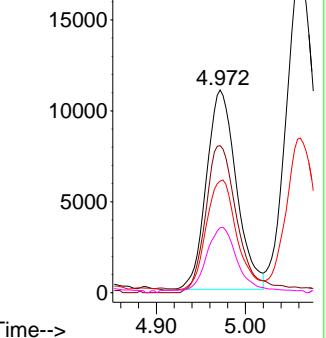

#40

Methyl acrylate

Concen: 10.962 ug/l

RT: 4.846 min Scan# 1106

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt Ion: 55 Resp: 39416

Ion Ratio Lower Upper



55 100


85 17.9 12.8 19.2

58 9.1 7.0 10.4

42 5.7 7.0 10.4#

Abundance

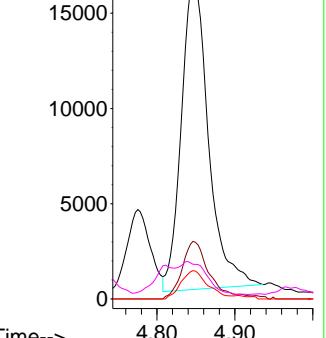



#41

Tetrahydrofuran

Concen: 52.040 ug/l

RT: 5.062 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U

ClientSampleId :



ICVVU071625

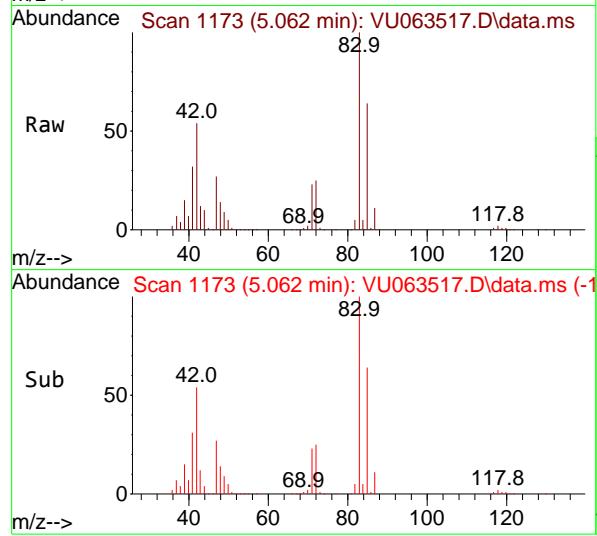

Tgt	Ion:	42	Ion Ratio	100	Resp:	6733
		72	45.7	39.2		58.8
		71	42.9	34.8		52.2


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

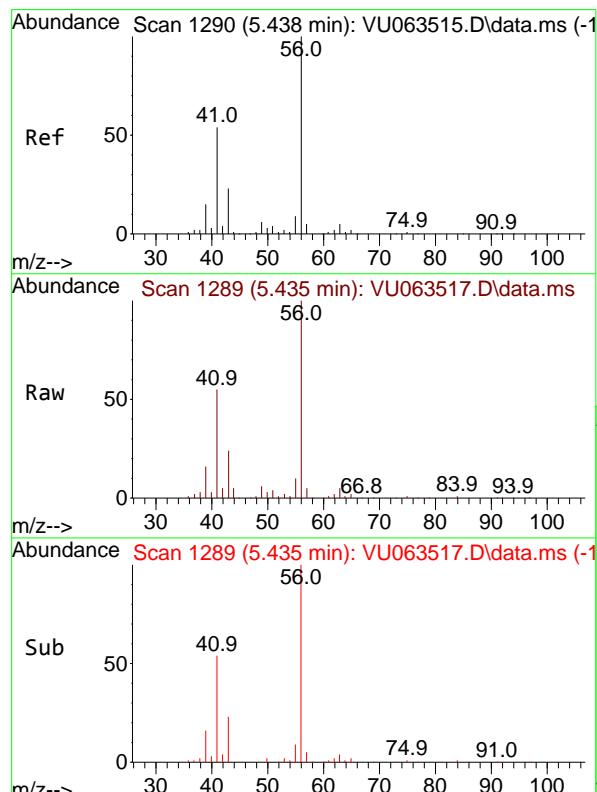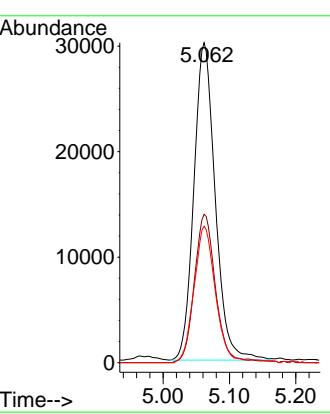

#42
1-Chlorobutane
Concen: 11.532 ug/l
RT: 5.435 min Scan# 1289
Delta R.T. -0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19


Tgt	Ion:	56	Ion Ratio	100	Resp:	151540
		41	53.7	26.7		80.0

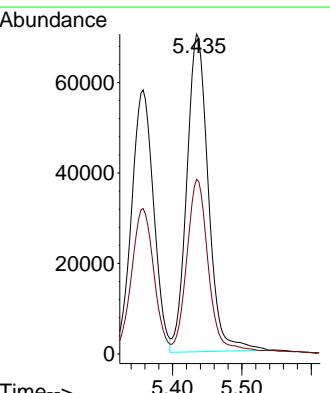



#43
Dibromomethane
Concen: 11.149 ug/l
RT: 6.907 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Instrument : MSVOA_U
ClientSampleId : ICVVU071625




Tgt Ion: 93 Resp: 35895
Ion Ratio Lower Upper
93 100
95 83.7 67.9 101.9
174 88.0 74.6 111.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

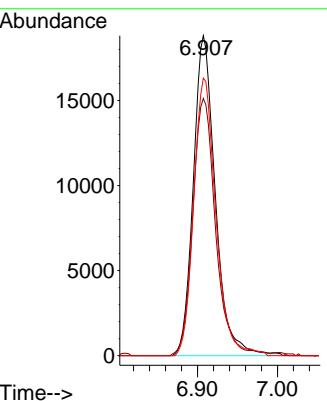



#44
Bromodichloromethane
Concen: 11.611 ug/l
RT: 7.094 min Scan# 1805
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19



Tgt Ion: 83 Resp: 84311
Ion Ratio Lower Upper
83 100
85 63.9 52.7 79.1
127 8.3 8.1 12.1

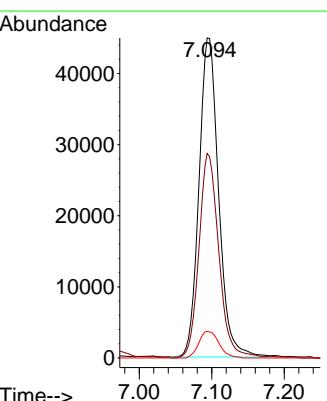

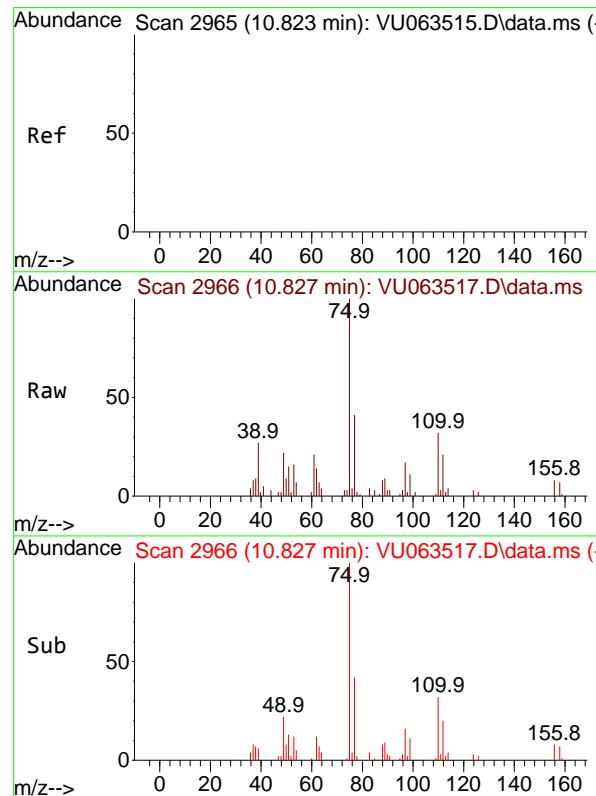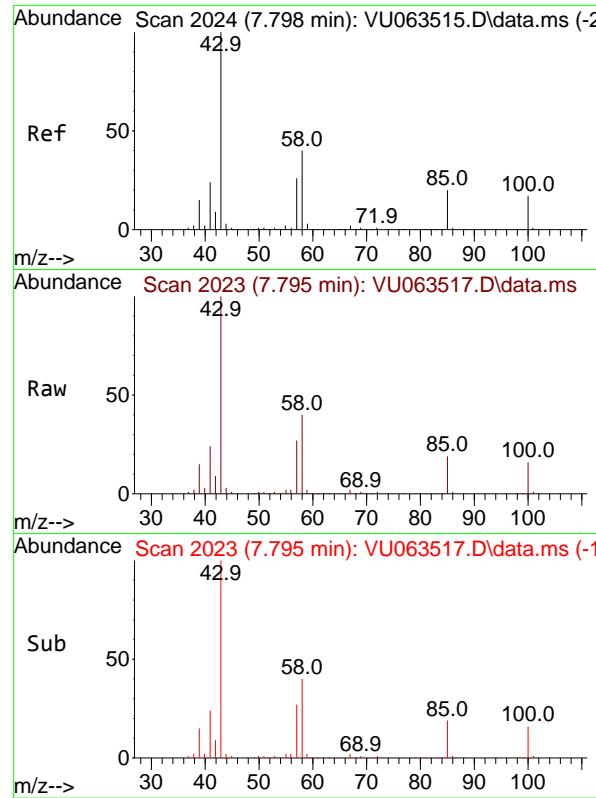

#45

4-Methyl-2-Pentanone

Concen: 57.520 ug/l

RT: 7.795 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

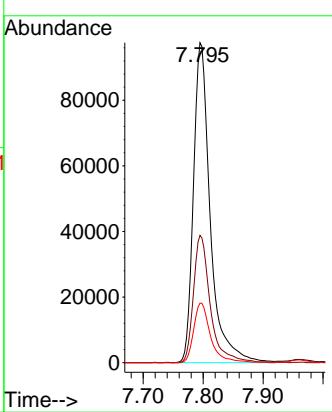 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#46

t-1,4-Dichloro-2-butene

Concen: 10.924 ug/l

RT: 10.827 min Scan# 2966


Delta R.T. 0.003 min


Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt Ion: 75 Resp: 12861

Ion	Ratio	Lower	Upper
75	100		
53	53.4	48.4	72.6
89	32.0	30.6	45.8
88	28.6	25.3	37.9

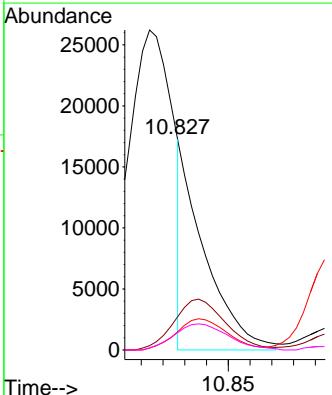



#47

Methyl methacrylate


Concen: 11.336 ug/l

RT: 6.965 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19



Tgt Ion: 69 Resp: 30651


Ion Ratio Lower Upper

69 100

41 100.5 0.0 224.0



39 64.1 55.3 82.9

100 36.1 29.0 43.6


**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

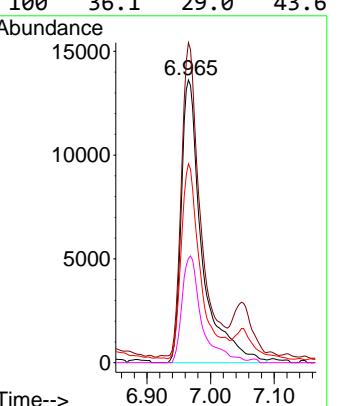

#48

Ethyl methacrylate


Concen: 12.064 ug/l

RT: 8.332 min Scan# 2190

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19






Tgt Ion: 69 Resp: 62257

Ion Ratio Lower Upper

69 100


41 61.9 30.8 92.4

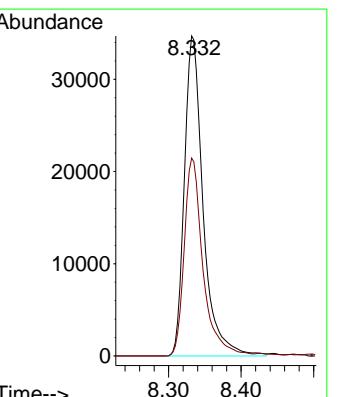



#49
Toluene
Concen: 11.565 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Instrument : MSVOA_U
ClientSampleId : ICVVU071625




Tgt Ion: 92 Resp: 167690
Ion Ratio Lower Upper
92 100
91 171.2 140.4 210.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

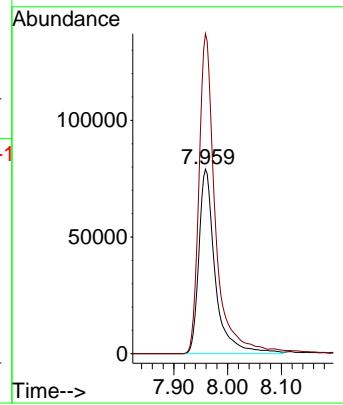


#50
t-1,3-Dichloropropene
Concen: 12.160 ug/l
RT: 8.203 min Scan# 2150
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19





Tgt Ion: 75 Resp: 69274
Ion Ratio Lower Upper
75 100
77 30.5 24.9 37.3

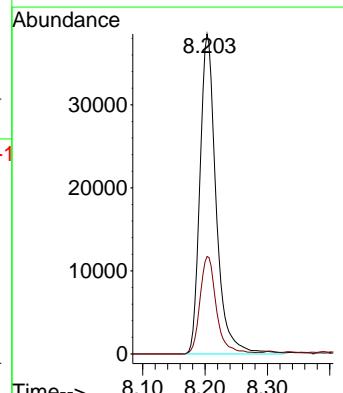



#51
cis-1,3-Dichloropropene
Concen: 11.406 ug/l
RT: 7.599 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19



Instrument : MSVOA_U
ClientSampleId : ICVVU071625

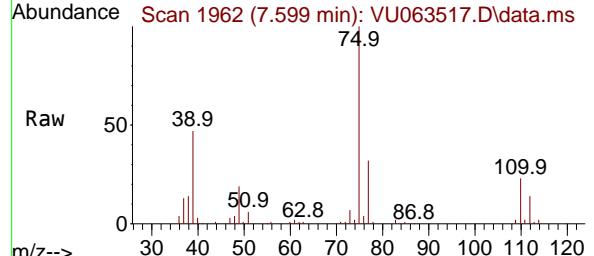


Tgt Ion: 75 Resp: 8722
Ion Ratio Lower Upper
75 100
77 32.4 25.1 37.7
39 47.1 37.8 56.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

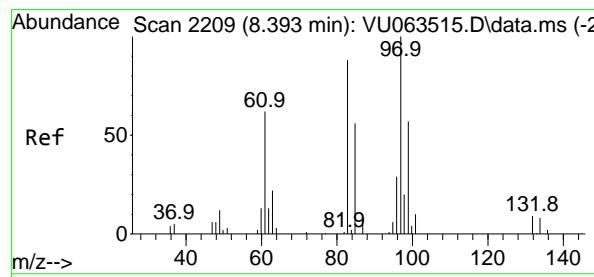


#52
1,1,2-Trichloroethane
Concen: 10.973 ug/l
RT: 8.393 min Scan# 2209
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19




Tgt Ion: 97 Resp: 47565
Ion Ratio Lower Upper
97 100
83 88.5 70.2 105.2
85 56.0 45.2 67.8
99 59.9 50.1 75.1

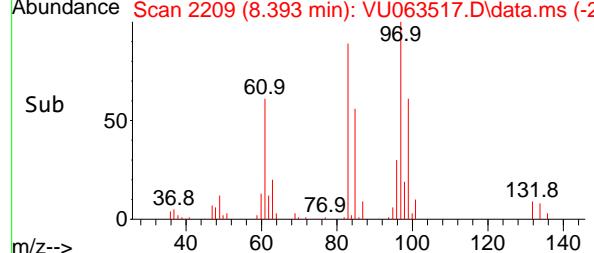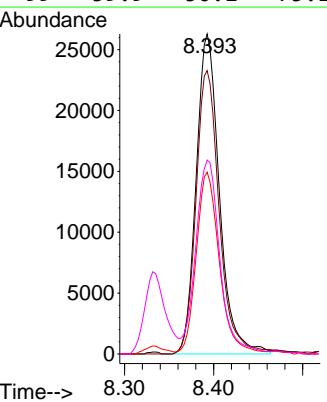





Abundance Scan 2263 (8.566 min): VU063517.D\data.ms

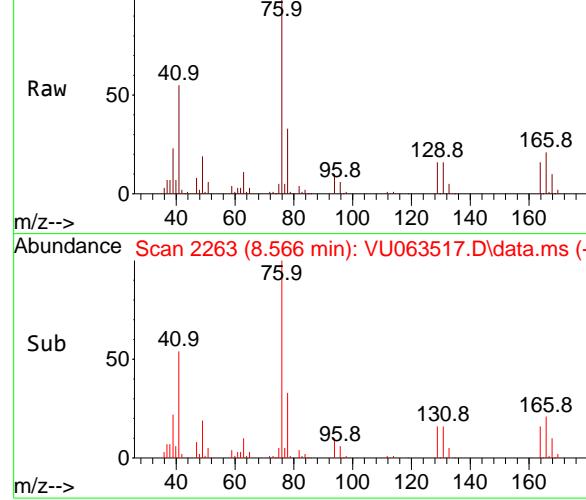


Abundance Scan 2263 (8.566 min): VU063517.D\data.ms (-2)

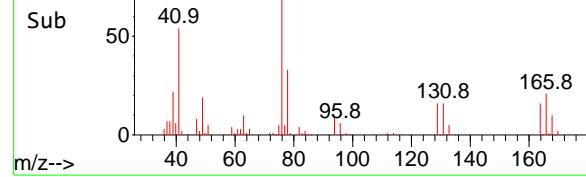


Abundance Scan 2301 (8.688 min): VU063515.D\data.ms (-2)

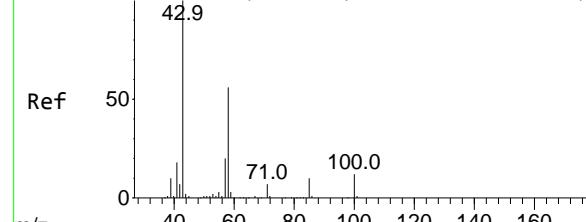

Abundance Scan 2300 (8.685 min): VU063517.D\data.ms

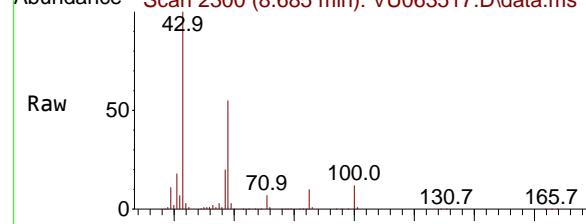

Abundance Scan 2300 (8.685 min): VU063517.D\data.ms (-2)

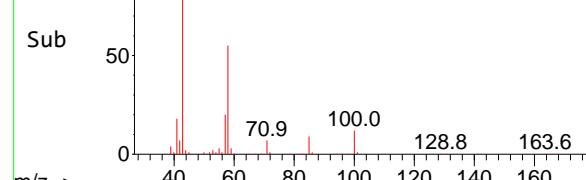

#53

1,3-Dichloropropane

Concen: 10.849 ug/l

RT: 8.566 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

Tgt Ion: 76 Resp: 81190

Ion Ratio Lower Upper


76 100

78 32.0 26.0 39.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

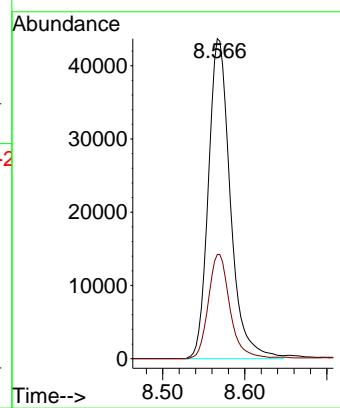

#54

2-Hexanone

Concen: 59.254 ug/l

RT: 8.685 min Scan# 2300

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion: 43 Resp: 130609







Ion Ratio Lower Upper

43 100

58 55.3 34.8 74.8

57 19.7 0.0 39.5

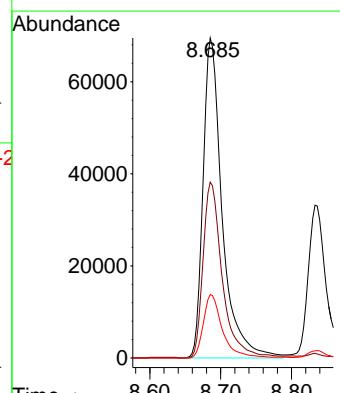



#55

Dibromochloromethane

Concen: 12.417 ug/l

RT: 8.801 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U


ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

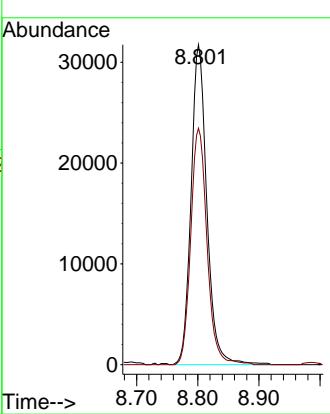

#56

1,2-Dibromoethane

Concen: 10.846 ug/l

RT: 8.917 min Scan# 2372

Delta R.T. 0.000 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19




Tgt Ion:107 Resp: 42078

Ion Ratio Lower Upper

107 100

109 95.2 0.0 186.4

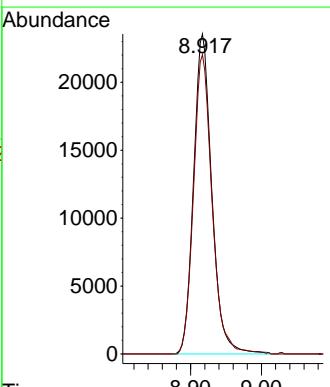



#57

4-Bromofluorobenzene

Concen: 1.279 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19





Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#58

Tetrachloroethene

Concen: 11.312 ug/l


RT: 8.541 min Scan# 2255




Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt	Ion:164	Resp:	70149
Ion	Ratio	Lower	Upper
164	100		
166	128.1	100.7	151.1
129	102.0	80.6	120.8
131	100.0	77.3	115.9

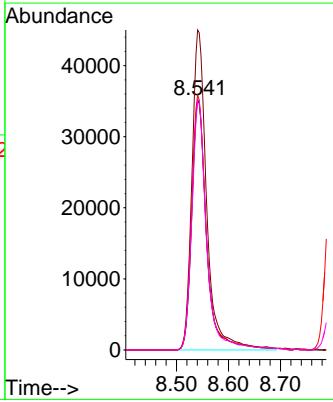

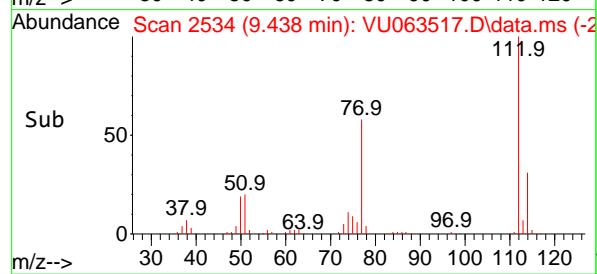

#59

Chlorobenzene

Concen: 11.557 ug/l

RT: 9.438 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063517.D




Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

#60

1,1,1,2-Tetrachloroethane

Concen: 10.964 ug/l

RT: 9.524 min Scan# 2561

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19




Tgt Ion:131 Resp: 58716




Ion Ratio Lower Upper

131 100

133 95.9 74.7 112.1

119 66.7 53.0 79.4

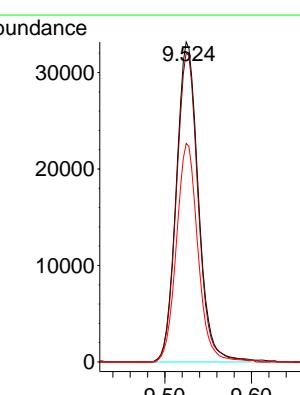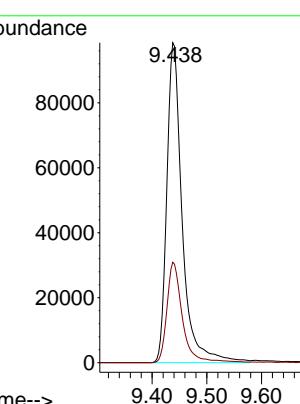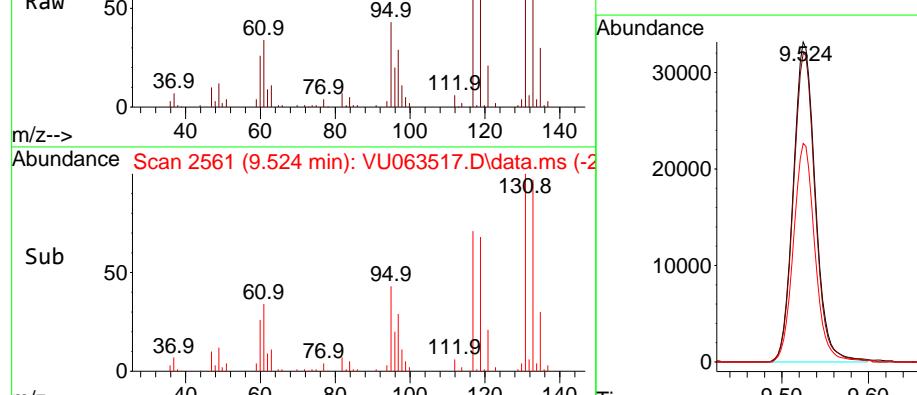



#61

Pentachloroethane

Concen: 12.325 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U




ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#62

Hexachloroethane


Concen: 12.375 ug/l







RT: 12.466 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

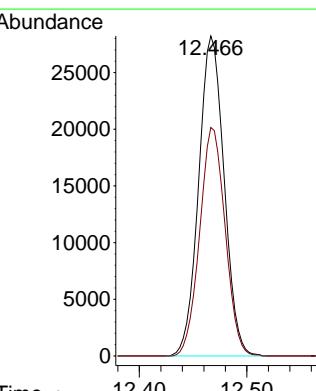Tgt Ion:117 Resp: 46374
Ion Ratio Lower Upper
117 100
201 71.5 57.4 86.0



#63

Ethyl Benzene

Concen: 11.440 ug/l

RT: 9.560 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

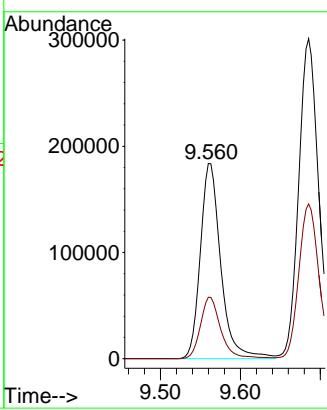 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#64

m/p-Xylenes


Concen: 23.477 ug/l


RT: 9.685 min Scan# 2611

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

 Tgt Ion:106 Resp: 261516
 Ion Ratio Lower Upper
 106 100
 91 208.1 163.6 245.4

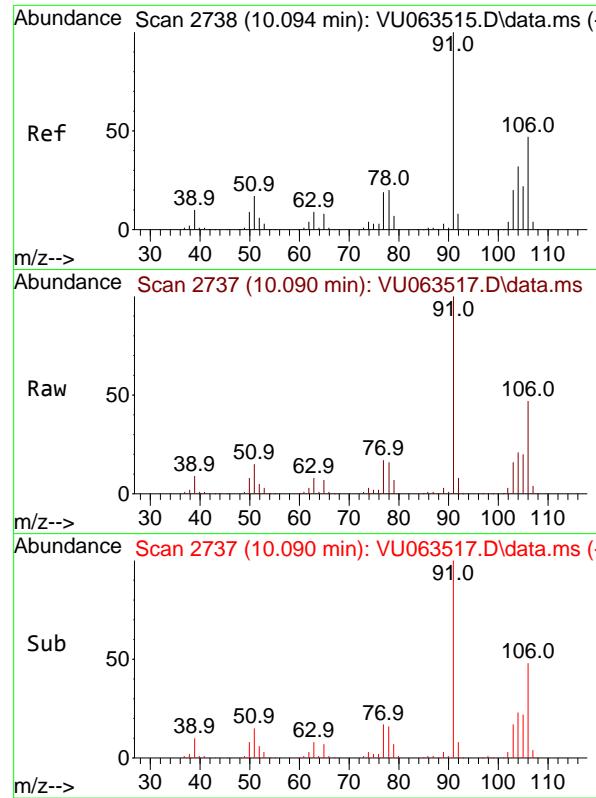
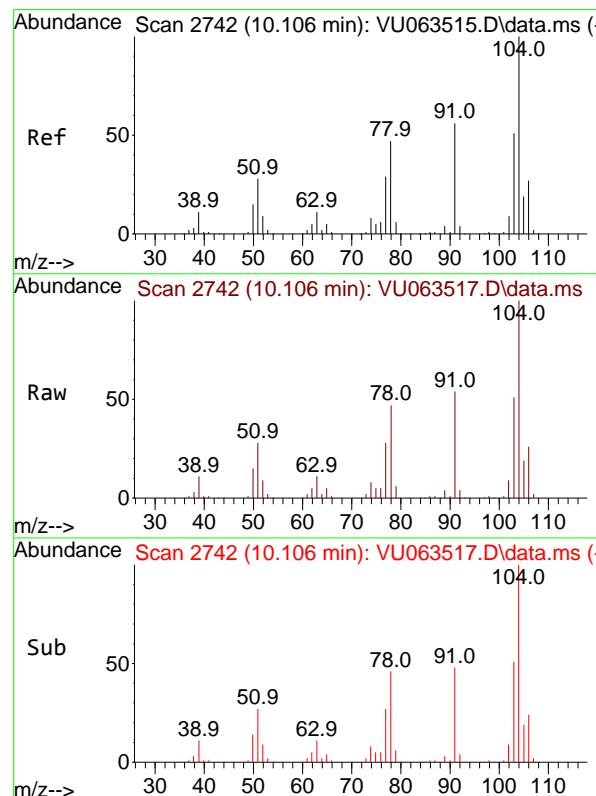
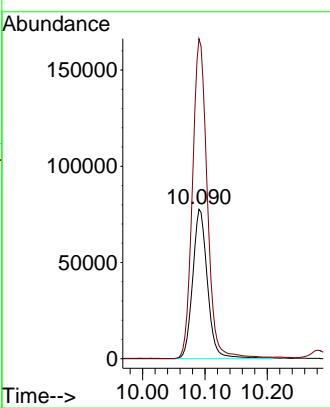


#65
o-Xylene
Concen: 11.980 ug/l
RT: 10.090 min Scan# 2
Delta R.T. -0.003 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#66
Styrene
Concen: 12.168 ug/l
RT: 10.106 min Scan# 2742
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Tgt Ion:104 Resp: 207563
Ion Ratio Lower Upper
104 100
78 51.6 41.3 61.9
103 55.3 43.6 65.4

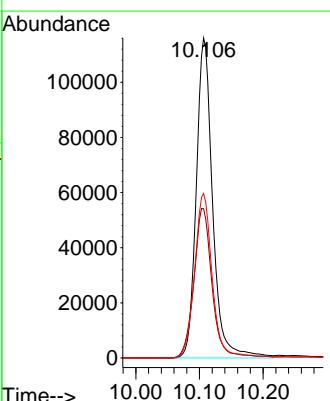

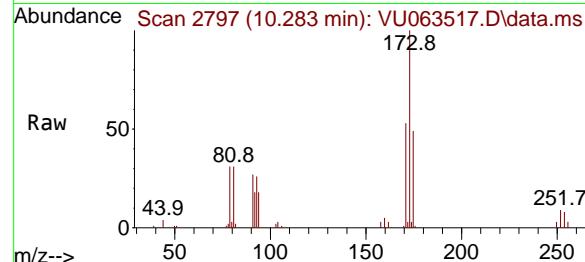

#67

Bromoform

Concen: 12.093 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19





Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

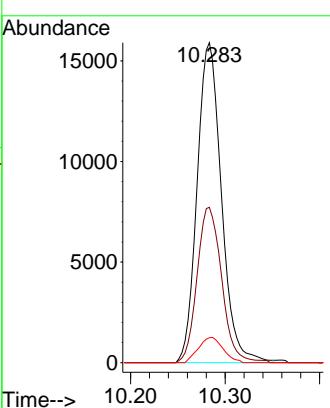 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.147 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt	Ion:152	Resp:	9055
Ion	Ratio	Lower	Upper
152	100		
115	133.8	0.0	262.2
150	316.7	0.0	651.2

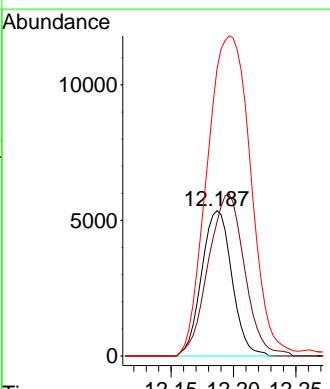

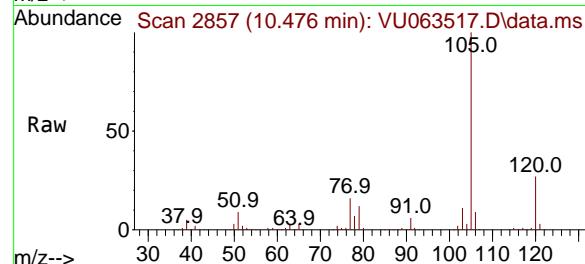

#69

Isopropylbenzene

Concen: 13.006 ug/l

RT: 10.476 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U




ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 10.762 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion: 83 Resp: 56769




Ion Ratio Lower Upper

83 100

131 10.5 8.4 12.6

85 64.2 51.9 77.9

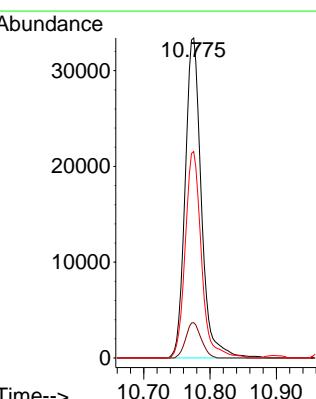



#71

1,2,3-Trichloropropane

Concen: 9.180 ug/l m

RT: 10.814 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19




Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#72

Bromobenzene

Concen: 11.605 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion:156 Resp: 77499




Ion Ratio Lower Upper

156 100

77 156.1 0.0 315.2

158 96.6 0.0 195.4

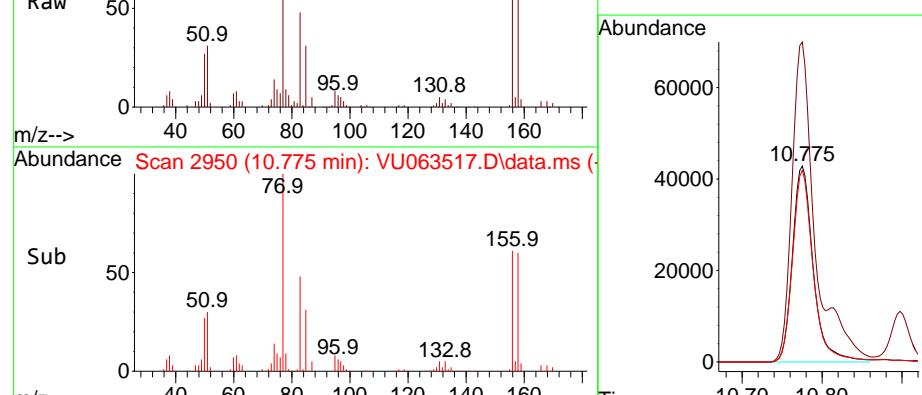



#73

n-propylbenzene

Concen: 11.877 ug/l

RT: 10.897 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19





Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

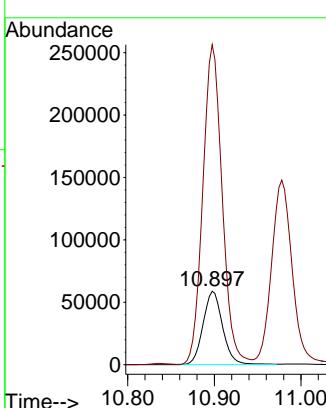 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#74

2-Chlorotoluene

Concen: 11.787 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063517.D


Acq: 16 Jul 2025 14:19




Tgt Ion:126 Resp: 81148

Ion Ratio Lower Upper

126 100

91 298.0 0.0 606.0

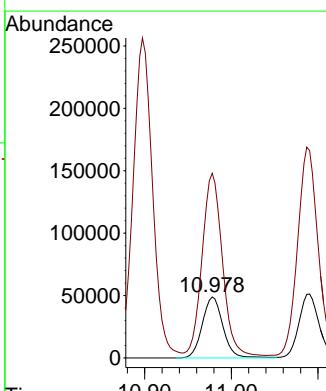



#75

1,3,5-Trimethylbenzene

Concen: 11.999 ug/l

RT: 11.081 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19





Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

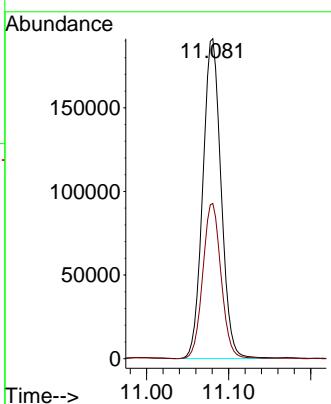 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#76

4-Chlorotoluene


Concen: 11.950 ug/l




RT: 11.090 min Scan# 3048

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

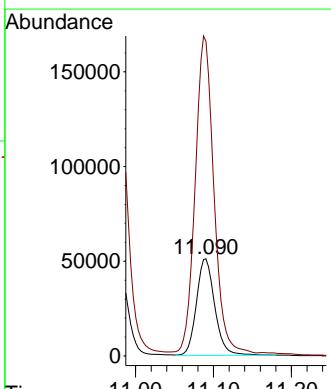 Tgt Ion:126 Resp: 83551
 Ion Ratio Lower Upper
 126 100
 91 332.4 0.0 682.2


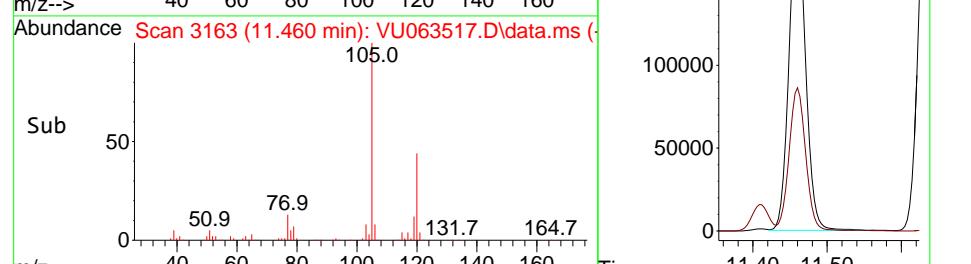
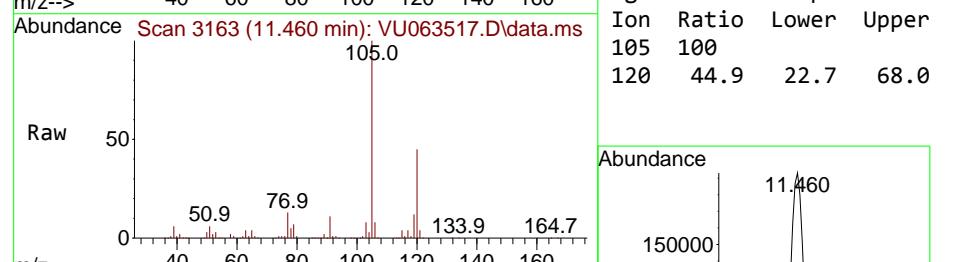
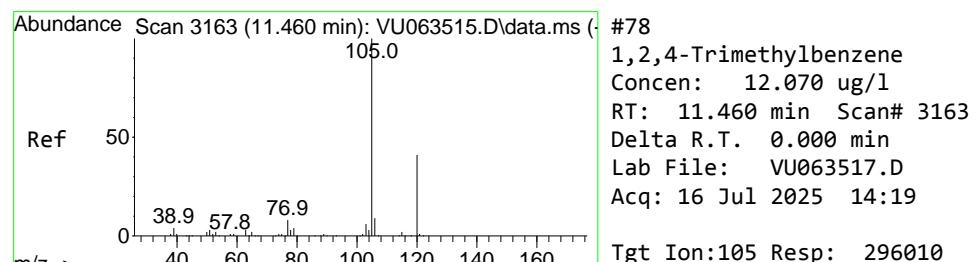
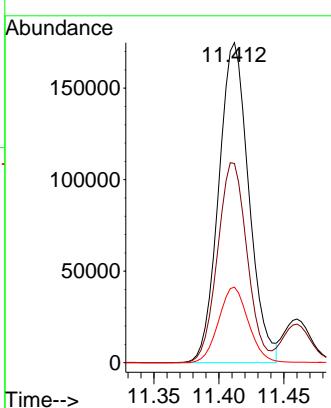


#77
tert-Butylbenzene
Concen: 11.976 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025



#78
1,2,4-Trimethylbenzene
Concen: 12.070 ug/l
RT: 11.460 min Scan# 3163
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Tgt Ion:105 Resp: 296010
Ion Ratio Lower Upper
105 100
120 44.9 22.7 68.0

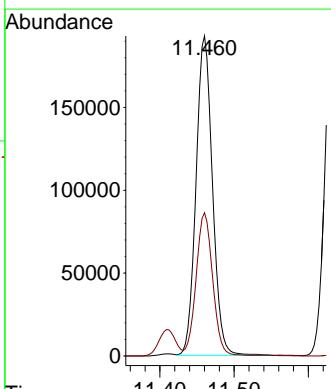

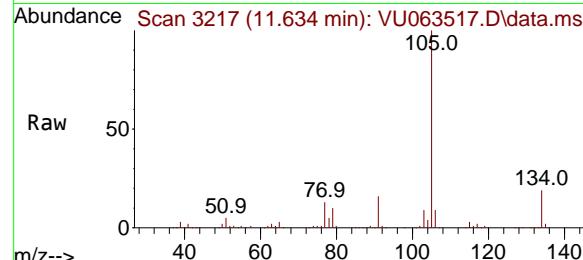

#79

sec-Butylbenzene

Concen: 11.975 ug/l

RT: 11.634 min Scan# 3

Instrument:

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063517.D

ClientSampleId :





Acq: 16 Jul 2025 14:19

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#80

Nitrobenzene

Concen: 13.031 ug/l m


RT: 13.216 min Scan# 3709




Delta R.T. 0.013 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
77	100		1132		
123	40.5	16.9		59.7	
65	0.0	16.5		20.9	#



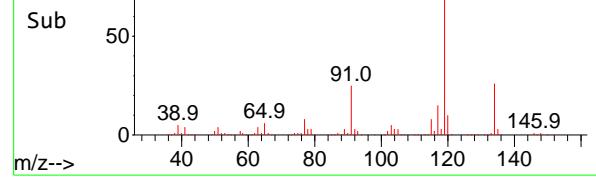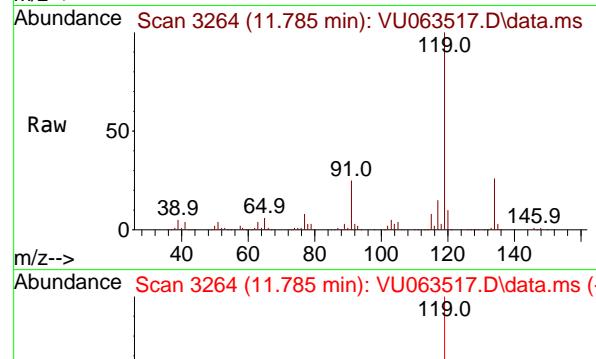

#81

p-Isopropyltoluene

Concen: 12.280 ug/l

RT: 11.785 min Scan# 32658

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument:

MSVOA_U





ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025

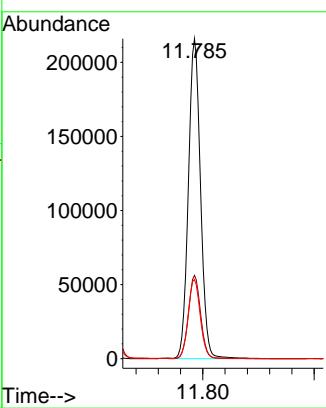

#82

1,3-Dichlorobenzene

Concen: 11.911 ug/l


RT: 11.737 min Scan# 3249




Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Tgt	Ion:146	Resp:	159160
Ion	Ratio	Lower	Upper
146	100		
111	41.8	33.8	50.6
148	63.6	51.5	77.3

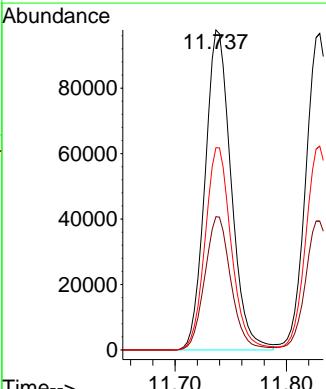



#83

1,4-Dichlorobenzene

Concen: 11.662 ug/l

RT: 11.830 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19




Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#84

n-Butylbenzene

Concen: 12.202 ug/l

RT: 12.200 min Scan# 3393

Delta R.T. -0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion: 91 Resp: 300975




Ion Ratio Lower Upper

91 100

92 53.2 41.5 62.3

134 26.3 20.6 30.8

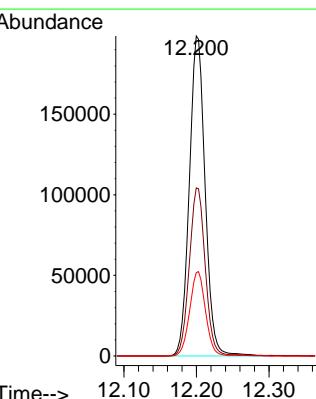

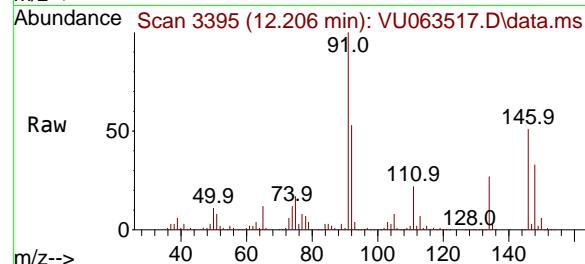

#85

1,2-Dichlorobenzene

Concen: 11.990 ug/l

RT: 12.206 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19

Instrument :

MSVOA_U

ClientSampleId :

ICVVU071625

Tgt Ion:146 Resp: 150510

Ion Ratio Lower Upper

146 100




111 42.3 21.7 65.1

148 64.3 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/17/2025

Supervised By :Semsettin Yesilyurt 07/17/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 10.124 ug/l

RT: 12.987 min Scan# 3638

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19



Tgt Ion: 75 Resp: 9053


Ion Ratio Lower Upper

75 100

155 80.4 65.8 98.6

157 101.9 81.4 122.2

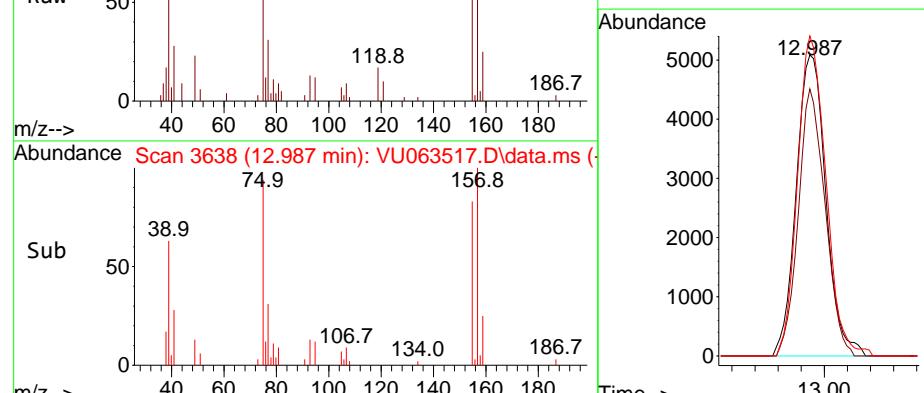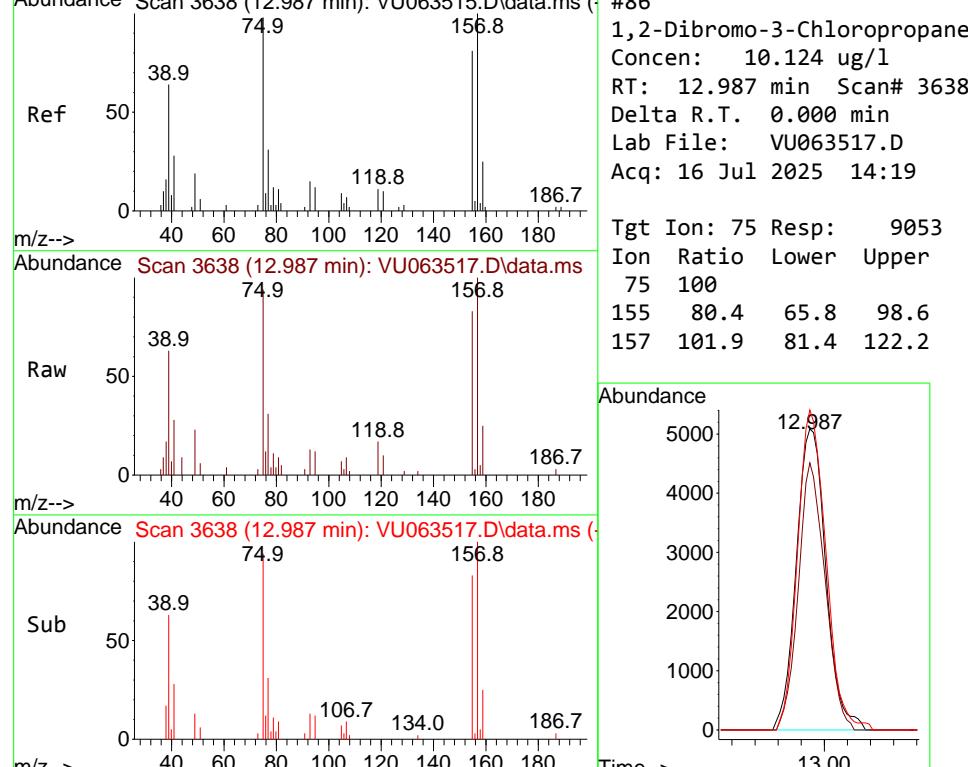


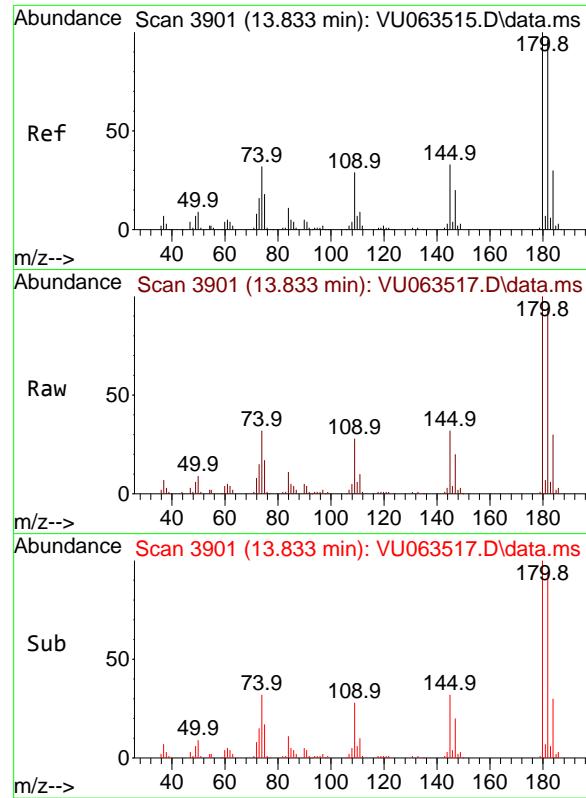


#87
1,2,4-Trichlorobenzene
Concen: 12.623 ug/l
RT: 13.833 min Scan# 3901
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Instrument : MSVOA_U
ClientSampleId : ICVVU071625


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/17/2025
Supervised By :Semsettin Yesilyurt 07/17/2025

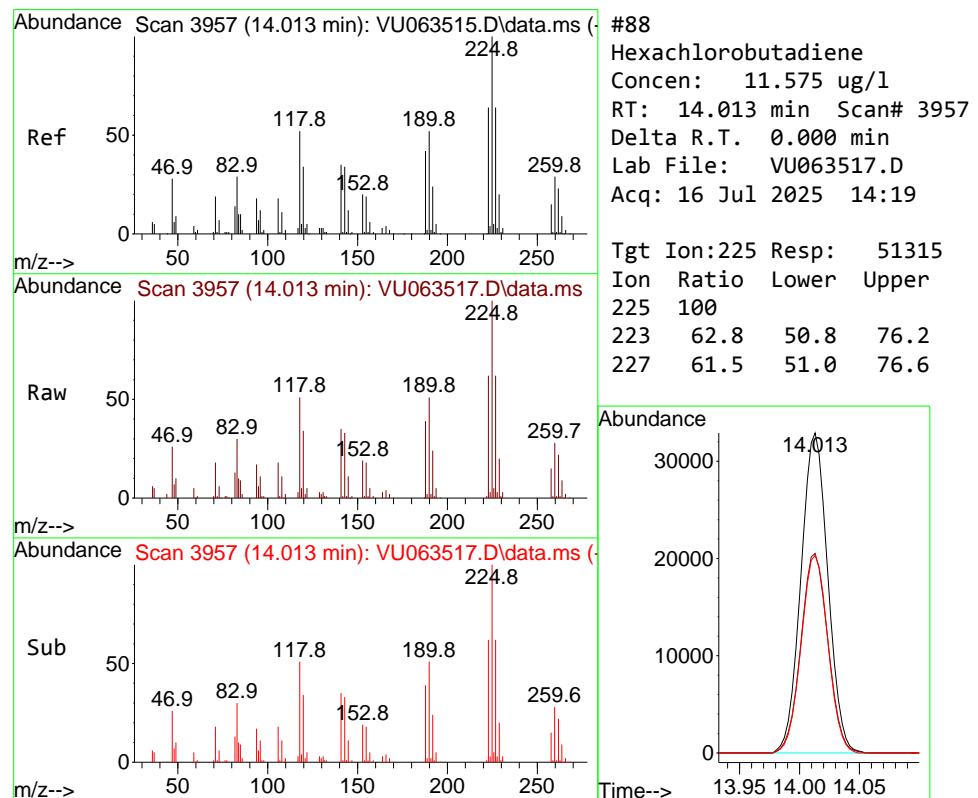

#88
Hexachlorobutadiene
Concen: 11.575 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063517.D
Acq: 16 Jul 2025 14:19

Tgt Ion:225 Resp: 51315
Ion Ratio Lower Upper
225 100
223 62.8 50.8 76.2
227 61.5 51.0 76.6

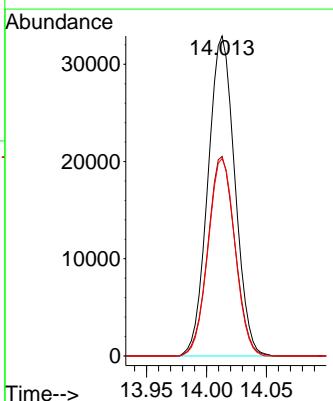



#89

Naphthalene

Concen: 11.841 ug/l

RT: 14.081 min Scan# 3

Delta R.T. 0.001 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19





Instrument:

MSVOA_U

ClientSampleId :

ICVVU071625

**Manual Integrations
APPROVED**

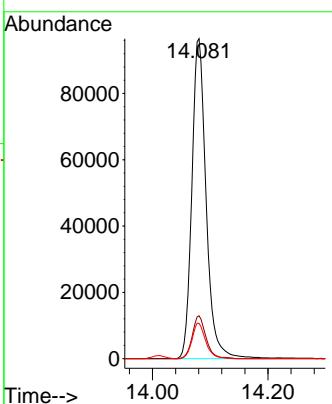 Reviewed By :Mahesh Dadoda 07/17/2025
 Supervised By :Semsettin Yesilyurt 07/17/2025


#90

1,2,3-Trichlorobenzene

Concen: 11.788 ug/l

RT: 14.322 min Scan# 4053

Delta R.T. 0.000 min

Lab File: VU063517.D

Acq: 16 Jul 2025 14:19


Tgt Ion:180 Resp: 85042

Ion Ratio Lower Upper

180 100

182 95.2 78.0 117.0

145 33.3 27.3 40.9

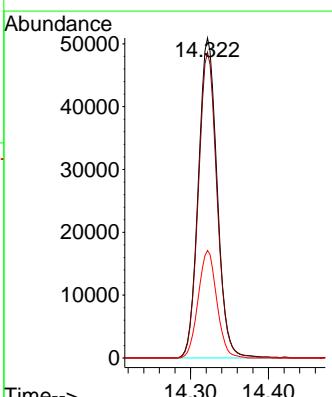

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063517.D
 Acq On : 16 Jul 2025 14:19
 Operator : MD/SY
 Sample : VSTDICV010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Quant Time: Jul 17 03:27:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 i	Fluorobenzene	1.000	1.000	0.0	88	0.00
2 T	Dichlorodifluoromethane	0.295	0.211	28.5	63	0.00
3 t	Chloromethane	0.274	0.265	3.3	87	0.00
4 Rt	Vinyl Chloride	0.349	0.333	4.6	83	0.00
5 T	Bromomethane	0.263	0.253	3.8	92	0.00
6 T	Chloroethane	0.211	0.216	-2.4	89	0.00
7 T	Trichlorofluoromethane	0.501	0.519	-3.6	90	0.00
8	1,1,2-Trichloro-1,2,2-trifl	0.262	0.300	-14.5	100	0.00
9 Rt	1,1-Dichloroethene	0.260	0.303	-16.5	101	0.00
10 t	Iodomethane	0.314	0.349	-11.1	83	0.00
11 t	Allyl Chloride	0.375	0.465	-24.0	108	0.00
12 t	Acrylonitrile	0.065	0.174	-167.7#	243#	0.00
13 T	Acetone	0.052	0.068	-30.8#	121	0.00
14 T	Carbon Disulfide	0.839	0.875	-4.3	90	0.00
15 RT	Methylene Chloride	0.306	0.340	-11.1	103	0.00
16 RT	trans-1,2-Dichloroethene	0.295	0.316	-7.1	93	0.00
17 t	1,1-Dichloroethane	0.546	0.622	-13.9	100	0.00
18 T	2-Butanone	0.081	0.095	-17.3	106	0.00
19	Cyclohexane	0.463	0.533	-15.1	102	0.00
20	Methylcyclohexane	0.450	0.461	-2.4	83	0.00
21 T	2,2-Dichloropropane	0.465	0.524	-12.7	102	0.00
22 RT	cis-1,2-Dichloroethene	0.320	0.376	-17.5	104	0.00
23 t	Diethyl Ether	0.198	0.216	-9.1	92	0.00
24 t	tert-Butyl Alcohol	0.024	0.013	45.8#	48	0.00
25 t	Methyl tert-Butyl Ether	0.678	0.809	-19.3	103	0.00
26 t	Bromochloromethane	0.134	0.143	-6.7	92	0.00
27 t	Chloroform	0.558	0.630	-12.9	102	0.00
28 RT	1,1,1-Trichloroethane	0.473	0.553	-16.9	102	0.00
29 T	1,1-Dichloropropene	0.438	0.465	-6.2	95	0.00
30 RT	Carbon Tetrachloride	0.381	0.453	-18.9	102	0.00
31 t	Isopropyl Ether	0.825	0.965	-17.0	103	0.00
32	Ethyl-t-butyl ether	0.763	0.000	100.0#	0#	-4.50#
33	Tert-Amyl methyl ether	0.663	0.000	100.0#	0#	-5.94#
34 t	Propionitrile	0.025	0.054	-116.0#	208#	0.00
35 RT	Benzene	1.178	1.117	5.2	82	0.00
36 RT	1,2-Dichloroethane	0.366	0.337	7.9	79	0.00
37 RT	Trichloroethene	0.301	0.296	1.7	81	0.00
38 Rt	1,2-Dichloropropane	0.276	0.280	-1.4	78	0.00
39 t	Methacrylonitrile	0.109	0.114	-4.6	99	0.00
40 t	Methyl acrylate	0.159	0.175	-10.1	92	0.00
41 t	Tetrahydrofuran	0.057	0.149	-161.4#	252#	0.00
42 t	1-Chlorobutane	0.583	0.672	-15.3	101	0.00
43 T	Dibromomethane	0.143	0.159	-11.2	92	0.00
44 T	Bromodichloromethane	0.322	0.374	-16.1	101	0.00
45 T	4-Methyl-2-Pentanone	0.147	0.169	-15.0	98	0.00
46 t	t-1,4-Dichloro-2-butene	0.055	0.029	47.3#	40	0.00
47 t	Methyl methacrylate	0.120	0.068	43.3#	47	0.00
48 t	Ethyl methacrylate	0.229	0.276	-20.5	97	0.00
49 Rt	Toluene	0.643	0.744	-15.7	98	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063517.D
 Acq On : 16 Jul 2025 14:19
 Operator : MD/SY
 Sample : VSTDICV010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Quant Time: Jul 17 03:27:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
50 T	t-1,3-Dichloropropene	0.253	0.307	-21.3	95	0.00
51 T	cis-1,3-Dichloropropene	0.339	0.387	-14.2	94	0.00
52 RT	1,1,2-Trichloroethane	0.192	0.211	-9.9	92	0.00
53 t	1,3-Dichloropropane	0.332	0.360	-8.4	93	0.00
54 t	2-Hexanone	0.098	0.116	-18.4	99	0.00
55 t	Dibromochloromethane	0.203	0.252	-24.1	96	0.00
56 T	1,2-Dibromoethane	0.172	0.187	-8.7	92	0.00
57 S	4-Bromofluorobenzene	0.379	0.484	-27.7	116	0.00
58 RT	Tetrachloroethene	0.275	0.311	-13.1	96	0.00
59 Rt	Chlorobenzene	0.739	0.854	-15.6	98	0.00
60 T	1,1,1,2-Tetrachloroethane	0.238	0.260	-9.2	91	0.00
61 t	Pentachloroethane	0.168	0.207	-23.2	98	0.00
62 t	Hexachloroethane	0.166	0.206	-24.1	95	0.00
63 Rt	Ethyl Benzene	1.271	1.454	-14.4	98	0.00
64 RT	m/p-Xylenes	0.494	0.580	-17.4	99	0.00
65 RT	o-Xylene	0.475	0.569	-19.8	100	0.00
66 RT	Styrene	0.757	0.921	-21.7	99	0.00
67 t	Bromoform	0.104	0.126	-21.2	94	0.00
68 S	1,2-Dichlorobenzene-d4	0.350	0.402	-14.9	99	0.00
69 T	Isopropylbenzene	1.148	1.493	-30.1#	107	0.00
70 T	1,1,2,2-Tetrachloroethane	0.234	0.252	-7.7	92	0.00
71 T	1,2,3-Trichloropropane	0.190	0.175	7.9	74	0.00
72 t	Bromobenzene	0.296	0.344	-16.2	98	0.00
73 t	n-propylbenzene	0.346	0.410	-18.5	97	0.00
74 t	2-Chlorotoluene	0.305	0.360	-18.0	99	0.00
75 t	1,3,5-Trimethylbenzene	1.097	1.316	-20.0	98	0.00
76 t	4-Chlorotoluene	0.310	0.371	-19.7	99	0.00
77 t	tert-Butylbenzene	1.048	1.255	-19.8	99	0.00
78 t	1,2,4-Trimethylbenzene	1.088	1.313	-20.7	99	0.00
79 t	sec-Butylbenzene	1.413	1.692	-19.7	99	0.00
80	Nitrobenzene	0.004	0.001	75.0#	17#	0.01
81 t	p-Isopropyltoluene	1.180	1.449	-22.8	100	0.00
82 t	1,3-Dichlorobenzene	0.593	0.706	-19.1	99	0.00
83 Rt	1,4-Dichlorobenzene	0.593	0.692	-16.7	96	0.00
84 t	n-Butylbenzene	1.094	1.335	-22.0	97	0.00
85 Rt	1,2-Dichlorobenzene	0.557	0.668	-19.9	99	0.00
86 t	1,2-Dibromo-3-Chloropropane	0.033	0.040	-21.2	89	0.00
87 Rt	1,2,4-Trichlorobenzene	0.346	0.437	-26.3	100	0.00
88 t	Hexachlorobutadiene	0.197	0.228	-15.7	95	0.00
89 t	Naphthalene	0.621	0.735	-18.4	96	0.00
90 t	1,2,3-Trichlorobenzene	0.320	0.377	-17.8	95	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063517.D
 Acq On : 16 Jul 2025 14:19
 Operator : MD/SY
 Sample : VSTDICV010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Quant Time: Jul 17 03:27:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 i	Fluorobenzene	1.000	1.000	0.0	88	0.00
2 T	Dichlorodifluoromethane	10.000	7.149	28.5	63	0.00
3 t	Chloromethane	10.000	9.652	3.5	87	0.00
4 Rt	Vinyl Chloride	10.000	9.533	4.7	83	0.00
5 T	Bromomethane	10.000	9.626	3.7	92	0.00
6 T	Chloroethane	10.000	10.243	-2.4	89	0.00
7 T	Trichlorofluoromethane	10.000	10.364	-3.6	90	0.00
8	1,1,2-Trichloro-1,2,2-trifl	10.000	11.439	-14.4	100	0.00
9 Rt	1,1-Dichloroethene	10.000	11.688	-16.9	101	0.00
10 t	Iodomethane	10.000	9.080	9.2	83	0.00
11 t	Allyl Chloride	10.000	12.385	-23.8	108	0.00
12 t	Acrylonitrile	20.000	53.704	-168.5#	243	0.00
13 T	Acetone	50.000	65.587	-31.2#	121	0.00
14 T	Carbon Disulfide	10.000	10.434	-4.3	90	0.00
15 RT	Methylene Chloride	10.000	11.133	-11.3	103	0.00
16 RT	trans-1,2-Dichloroethene	10.000	10.705	-7.1	93	0.00
17 t	1,1-Dichloroethane	10.000	11.390	-13.9	100	0.00
18 T	2-Butanone	50.000	59.104	-18.2	106	0.00
19	Cyclohexane	10.000	11.523	-15.2	102	0.00
20	Methylcyclohexane	10.000	10.246	-2.5	83	0.00
21 T	2,2-Dichloropropane	10.000	11.251	-12.5	102	0.00
22 RT	cis-1,2-Dichloroethene	10.000	11.753	-17.5	104	0.00
23 t	Diethyl Ether	10.000	10.895	-8.9	92	0.00
24 t	tert-Butyl Alcohol	100.000	54.858	45.1#	48	0.00
25 t	Methyl tert-Butyl Ether	10.000	11.931	-19.3	103	0.00
26 t	Bromochloromethane	10.000	10.701	-7.0	92	0.00
27 t	Chloroform	10.000	11.295	-13.0	102	0.00
28 RT	1,1,1-Trichloroethane	10.000	11.694	-16.9	102	0.00
29 T	1,1-Dichloropropene	10.000	10.604	-6.0	95	0.00
30 RT	Carbon Tetrachloride	10.000	11.881	-18.8	102	0.00
31 t	Isopropyl Ether	10.000	11.694	-16.9	103	0.00
32	Ethyl-t-butyl ether	10.000	0.000	100.0#	0	-4.50#
33	Tert-Amyl methyl ether	10.000	0.000	100.0#	0	-5.94#
34 t	Propionitrile	50.000	110.315	-120.6#	208	0.00
35 RT	Benzene	10.000	9.485	5.2	82	0.00
36 RT	1,2-Dichloroethane	10.000	9.208	7.9	79	0.00
37 RT	Trichloroethene	10.000	9.864	1.4	81	0.00
38 Rt	1,2-Dichloropropane	10.000	10.152	-1.5	78	0.00
39 t	Methacrylonitrile	10.000	10.571	-5.7	99	0.00
40 t	Methyl acrylate	10.000	10.962	-9.6	92	0.00
41 t	Tetrahydrofuran	20.000	52.040	-160.2#	252	0.00
42 t	1-Chlorobutane	10.000	11.532	-15.3	101	0.00
43 T	Dibromomethane	10.000	11.149	-11.5	92	0.00
44 T	Bromodichloromethane	10.000	11.611	-16.1	101	0.00
45 T	4-Methyl-2-Pentanone	50.000	57.520	-15.0	98	0.00
46 t	t-1,4-Dichloro-2-butene	20.000	10.924	45.4#	40	0.00
47 t	Methyl methacrylate	20.000	11.336	43.3#	47	0.00
48 t	Ethyl methacrylate	10.000	12.064	-20.6	97	0.00
49 Rt	Toluene	10.000	11.565	-15.6	98	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063517.D
 Acq On : 16 Jul 2025 14:19
 Operator : MD/SY
 Sample : VSTDICV010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ICVVU071625

Quant Time: Jul 17 03:27:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:16:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
50 T	t-1,3-Dichloropropene	10.000	12.160	-21.6	95	0.00
51 T	cis-1,3-Dichloropropene	10.000	11.406	-14.1	94	0.00
52 RT	1,1,2-Trichloroethane	10.000	10.973	-9.7	92	0.00
53 t	1,3-Dichloropropane	10.000	10.849	-8.5	93	0.00
54 t	2-Hexanone	50.000	59.254	-18.5	99	0.00
55 t	Dibromochloromethane	10.000	12.417	-24.2	96	0.00
56 T	1,2-Dibromoethane	10.000	10.846	-8.5	92	0.00
57 S	4-Bromofluorobenzene	1.000	1.279	-27.9	116	0.00
58 RT	Tetrachloroethene	10.000	11.312	-13.1	96	0.00
59 Rt	Chlorobenzene	10.000	11.557	-15.6	98	0.00
60 T	1,1,1,2-Tetrachloroethane	10.000	10.964	-9.6	91	0.00
61 t	Pentachloroethane	10.000	12.325	-23.2	98	0.00
62 t	Hexachloroethane	10.000	12.375	-23.8	95	0.00
63 Rt	Ethyl Benzene	10.000	11.440	-14.4	98	0.00
64 RT	m/p-Xylenes	20.000	23.477	-17.4	99	0.00
65 RT	o-Xylene	10.000	11.980	-19.8	100	0.00
66 RT	Styrene	10.000	12.168	-21.7	99	0.00
67 t	Bromoform	10.000	12.093	-20.9	94	0.00
68 S	1,2-Dichlorobenzene-d4	1.000	1.147	-14.7	99	0.00
69 T	Isopropylbenzene	10.000	13.006	-30.1#	107	0.00
70 T	1,1,2,2-Tetrachloroethane	10.000	10.762	-7.6	92	0.00
71 T	1,2,3-Trichloropropane	10.000	9.180	8.2	74	0.00
72 t	Bromobenzene	10.000	11.605	-16.1	98	0.00
73 t	n-propylbenzene	10.000	11.877	-18.8	97	0.00
74 t	2-Chlorotoluene	10.000	11.787	-17.9	99	0.00
75 t	1,3,5-Trimethylbenzene	10.000	11.999	-20.0	98	0.00
76 t	4-Chlorotoluene	10.000	11.950	-19.5	99	0.00
77 t	tert-Butylbenzene	10.000	11.976	-19.8	99	0.00
78 t	1,2,4-Trimethylbenzene	10.000	12.070	-20.7	99	0.00
79 t	sec-Butylbenzene	10.000	11.975	-19.7	99	0.00
80	Nitrobenzene	50.000	13.031	73.9#	17	0.01
81 t	p-Isopropyltoluene	10.000	12.280	-22.8	100	0.00
82 t	1,3-Dichlorobenzene	10.000	11.911	-19.1	99	0.00
83 Rt	1,4-Dichlorobenzene	10.000	11.662	-16.6	96	0.00
84 t	n-Butylbenzene	10.000	12.202	-22.0	97	0.00
85 Rt	1,2-Dichlorobenzene	10.000	11.990	-19.9	99	0.00
86 t	1,2-Dibromo-3-Chloropropane	10.000	10.124	-1.2	89	0.00
87 Rt	1,2,4-Trichlorobenzene	10.000	12.623	-26.2	100	0.00
88 t	Hexachlorobutadiene	10.000	11.575	-15.7	95	0.00
89 t	Naphthalene	10.000	11.841	-18.4	96	0.00
90 t	1,2,3-Trichlorobenzene	10.000	11.788	-17.9	95	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date/Time:	07/17/2025 09:25
Lab File ID:	VU063519.D	Init. Calib. Date(s):	07/16/2025 07/16/2025
Heated Purge: (Y/N)	N	Init. Calib. Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

COMPOUND	RRF	RRF010	MIN RRF	%D	MAX%D
Dichlorodifluoromethane	0.295	0.284		-3.73	30
Chloromethane	0.274	0.271		-1.1	30
Vinyl Chloride	0.349	0.339		-2.87	30
Bromomethane	0.263	0.242		-7.99	30
Chloroethane	0.211	0.206		-2.37	30
Tetrahydrofuran	0.057	0.051		-10.53	30
Trichlorofluoromethane	0.501	0.484		-3.39	30
1,1,2-Trichloro-1,2,2-trifluoroethane	0.262	0.259		-1.14	30
tert-Butyl Alcohol	0.024	0.023		-4.17	30
Diethyl Ether	0.198	0.199		0.5	30
1,1-Dichloroethene	0.260	0.255		-1.92	30
Acrylonitrile	0.065	0.063		-3.08	30
Acetone	0.052	0.080		53.85	30
Carbon Disulfide	0.839	0.805		-4.05	30
Methyl tert-Butyl Ether	0.678	0.681		0.44	30
Methyl acrylate	0.160	0.149		-6.88	30
Methylene Chloride	0.306	0.286		-6.54	30
trans-1,2-Dichloroethene	0.295	0.282		-4.41	30
1,1-Dichloroethane	0.546	0.536		-1.83	30
Cyclohexane	0.463	0.437		-5.62	30
2-Butanone	0.081	0.100		23.46	30
Carbon Tetrachloride	0.381	0.388		1.84	30
2,2-Dichloropropane	0.465	0.456		-1.93	30
cis-1,2-Dichloroethene	0.320	0.312		-2.5	30
Bromochloromethane	0.134	0.135		0.75	30
Chloroform	0.558	0.543		-2.69	30
1,1,1-Trichloroethane	0.473	0.466		-1.48	30
Methylcyclohexane	0.450	0.467		3.78	30
1,1-Dichloropropene	0.438	0.425		-2.97	30
Propionitrile	0.025	0.023		-8	30
Benzene	1.178	1.188		0.85	30
1,2-Dichloroethane	0.366	0.368		0.55	30
Trichloroethene	0.301	0.318		5.65	30
1,2-Dichloropropane	0.276	0.308		11.59	30
1-Chlorobutane	0.583	0.580		-0.51	30
Dibromomethane	0.143	0.144		0.7	30
Bromodichloromethane	0.322	0.324		0.62	30
4-Methyl-2-Pentanone	0.147	0.154		4.76	30

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date/Time:	07/17/2025 09:25
Lab File ID:	VU063519.D	Init. Calib. Date(s):	07/16/2025 07/16/2025
Heated Purge: (Y/N)	N	Init. Calib. Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

COMPOUND	RRF	RRF010	MIN RRF	%D	MAX%D
Toluene	0.643	0.653		1.55	30
t-1,3-Dichloropropene	0.253	0.278		9.88	30
cis-1,3-Dichloropropene	0.339	0.359		5.9	30
1,1,2-Trichloroethane	0.192	0.199		3.65	30
1,3-Dichloropropane	0.332	0.333		0.3	30
2-Hexanone	0.098	0.118		20.41	30
Dibromochloromethane	0.203	0.229		12.81	30
1,2-Dibromoethane	0.172	0.178		3.49	30
Tetrachloroethene	0.275	0.267		-2.91	30
Chlorobenzene	0.739	0.758		2.57	30
1,1,1,2-Tetrachloroethane	0.238	0.246		3.36	30
Hexachloroethane	0.166	0.183		10.24	30
Ethyl Benzene	1.271	1.290		1.5	30
m/p-Xylenes	0.494	0.510		3.24	30
o-Xylene	0.475	0.499		5.05	30
Styrene	0.757	0.817		7.93	30
Bromoform	0.104	0.116		11.54	30
Isopropylbenzene	1.148	1.207		5.14	30
1,1,2,2-Tetrachloroethane	0.234	0.245		4.7	30
1,2,3-Trichloropropane	0.190	0.195		2.63	30
Bromobenzene	0.296	0.311		5.07	30
n-propylbenzene	0.346	0.365		5.49	30
2-Chlorotoluene	0.305	0.319		4.59	30
1,3,5-Trimethylbenzene	1.097	1.162		5.93	30
4-Chlorotoluene	0.310	0.333		7.42	30
tert-Butylbenzene	1.048	1.102		5.15	30
1,2,4-Trimethylbenzene	1.088	1.163		6.89	30
sec-Butylbenzene	1.413	1.483		4.95	30
p-Isopropyltoluene	1.180	1.264		7.12	30
1,3-Dichlorobenzene	0.593	0.622		4.89	30
1,4-Dichlorobenzene	0.593	0.625		5.4	30
n-Butylbenzene	1.094	1.206		10.24	30
1,2-Dichlorobenzene	0.557	0.586		5.21	30
1,2-Dibromo-3-Chloropropane	0.033	0.040		21.21	30
1,2,4-Trichlorobenzene	0.346	0.381		10.12	30
Hexachlorobutadiene	0.197	0.206		4.57	30
Naphthalene	0.621	0.687		10.63	30
1,2,3-Trichlorobenzene	0.320	0.357		11.56	30

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date/Time:	07/17/2025 09:25
Lab File ID:	VU063519.D	Init. Calib. Date(s):	07/16/2025 07/16/2025
Heated Purge: (Y/N)	N	Init. Calib. Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

COMPOUND	RRF	RRF010	MIN RRF	%D	MAX%D
Nitrobenzene	0.004	0.005		25	30
1,2-Dichlorobenzene-d4	0.350	0.339		-3.14	30
4-Bromofluorobenzene	0.379	0.365		-3.69	30
Iodomethane	0.314	0.350		11.47	30
Allyl Chloride	0.375	0.371		-1.07	30
t-1,4-Dichloro-2-butene	0.055	0.052		-5.45	30
Methacrylonitrile	0.109	0.101		-7.34	30
Ethyl methacrylate	0.229	0.249		8.73	30
Isopropyl Ether	0.825	0.805		-2.42	30
Methyl methacrylate	0.120	0.125		4.17	30

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063519.D
 Acq On : 17 Jul 2025 09:25
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTDCCC010

Quant Time: Jul 18 04:09:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.100	96	27500	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	10050	0.965	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	
68) 1,2-Dichlorobenzene-d4	12.183	152	9321	0.968	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	78194	9.643	ug/l	99
3) Chloromethane	1.518	50	74637	9.902	ug/l	99
4) Vinyl Chloride	1.599	62	93296	9.718	ug/l	100
5) Bromomethane	1.840	94	66515	9.188	ug/l	99
6) Chloroethane	1.923	64	56651	9.774	ug/l	98
7) Trichlorofluoromethane	2.126	101	132982	9.648	ug/l	100
8) 1,1,2-Trichloro-1,2,2-...	2.570	101	71124	9.874	ug/l	99
9) 1,1-Dichloroethene	2.567	96	70211	9.834	ug/l	99
10) Iodomethane	2.708	142	96119	9.096	ug/l	99
11) Allyl Chloride	2.907	41	102152	9.904	ug/l	99
12) Acrylonitrile	3.303	53	34689	19.426	ug/l	99
13) Acetone	2.618	43	109552	76.573	ug/l	98
14) Carbon Disulfide	2.779	76	221309	9.597	ug/l	100
15) Methylene Chloride	3.030	84	78569	9.347	ug/l	99
16) trans-1,2-Dichloroethene	3.335	96	77415	9.547	ug/l	98
17) 1,1-Dichloroethane	3.849	63	147481	9.813	ug/l	98
18) 2-Butanone	4.708	43	137001	61.835	ug/l	100
19) Cyclohexane	5.364	56	120216	9.447	ug/l	97
20) Methylcyclohexane	6.740	83	128329	10.376	ug/l	97
21) 2,2-Dichloropropane	4.647	77	125291	9.790	ug/l	99
22) cis-1,2-Dichloroethene	4.647	96	85795	9.751	ug/l	99
23) Diethyl Ether	2.367	59	54743	10.062	ug/l	99
24) tert-Butyl Alcohol	3.184	59	63328	96.429	ug/l	100
25) Methyl tert-Butyl Ether	3.357	73	187363	10.052	ug/l	100
26) Bromochloromethane	4.955	128	37081	10.094	ug/l	98
27) Chloroform	5.071	83	149276	9.734	ug/l	100
28) 1,1,1-Trichloroethane	5.296	97	128095	9.841	ug/l	99
29) 1,1-Dichloropropene	5.505	75	116999	9.703	ug/l	98
30) Carbon Tetrachloride	5.502	117	106784	10.193	ug/l	96
31) Isopropyl Ether	3.991	45	221350	9.757	ug/l	98
32) Ethyl-t-butyl ether	4.502	59	204582	9.745	ug/l	98
33) Tert-Amyl methyl ether	5.939	73	181869	9.982	ug/l	100
34) Propionitrile	4.772	54	31784	47.084	ug/l	# 94
35) Benzene	5.756	78	326804	10.088	ug/l	98
36) 1,2-Dichloroethane	5.782	62	101239	10.057	ug/l	99
37) Trichloroethene	6.525	130	87532	10.590	ug/l	97
38) 1,2-Dichloropropane	6.779	63	84731	11.175	ug/l	100
39) Methacrylonitrile	4.968	41	27645	9.213	ug/l	99
40) Methyl acrylate	4.846	55	40963	9.339	ug/l	96
41) Tetrahydrofuran	5.058	42	28312	17.936	ug/l	99
42) 1-Chlorobutane	5.438	56	159543	9.953	ug/l	100
43) Dibromomethane	6.904	93	39541	10.067	ug/l	95
44) Bromodichloromethane	7.094	83	89050	10.053	ug/l	# 98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063519.D
 Acq On : 17 Jul 2025 09:25
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTDCCC010

Quant Time: Jul 18 04:09:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.795	43	211583	52.266	ug/l	100
46) t-1,4-Dichloro-2-butene	10.823	75	28706m	18.890	ug/l	
47) Methyl methacrylate	6.962	69	68946	20.900	ug/l	97
48) Ethyl methacrylate	8.332	69	68373	10.861	ug/l	98
49) Toluene	7.959	92	179669	10.158	ug/l	99
50) t-1,3-Dichloropropene	8.203	75	76515	11.010	ug/l	99
51) cis-1,3-Dichloropropene	7.598	75	98787	10.590	ug/l	99
52) 1,1,2-Trichloroethane	8.393	97	54808	10.365	ug/l	97
53) 1,3-Dichloropropane	8.566	76	91688	10.044	ug/l	99
54) 2-Hexanone	8.685	43	162869	60.570	ug/l	100
55) Dibromochloromethane	8.801	129	62870	11.250	ug/l	100
56) 1,2-Dibromoethane	8.917	107	48870	10.326	ug/l	99
58) Tetrachloroethene	8.541	164	73468	9.712	ug/l	99
59) Chlorobenzene	9.438	112	208332	10.255	ug/l	99
60) 1,1,1,2-Tetrachloroethane	9.524	131	67746	10.370	ug/l	99
61) Pentachloroethane	11.418	117	49738	10.774	ug/l	100
62) Hexachloroethane	12.466	117	50359	11.016	ug/l	100
63) Ethyl Benzene	9.563	91	354702	10.146	ug/l	100
64) m/p-Xylenes	9.685	106	280366	20.632	ug/l	99
65) o-Xylene	10.090	106	137219	10.509	ug/l	99
66) Styrene	10.106	104	224585	10.792	ug/l	100
67) Bromoform	10.283	173	31862	11.101	ug/l	99
69) Isopropylbenzene	10.476	105	331800	10.511	ug/l	99
70) 1,1,2,2-Tetrachloroethane	10.775	83	67383	10.472	ug/l	99
71) 1,2,3-Trichloropropane	10.814	75	53509m	10.239	ug/l	
72) Bromobenzene	10.775	156	85460	10.490	ug/l	98
73) n-propylbenzene	10.897	120	100342	10.559	ug/l	98
74) 2-Chlorotoluene	10.978	126	87826	10.457	ug/l	99
75) 1,3,5-Trimethylbenzene	11.081	105	319519	10.596	ug/l	99
76) 4-Chlorotoluene	11.090	126	91522	10.731	ug/l	96
77) tert-Butylbenzene	11.412	119	303113	10.518	ug/l	100
78) 1,2,4-Trimethylbenzene	11.460	105	319824	10.690	ug/l	100
79) sec-Butylbenzene	11.634	105	407802	10.493	ug/l	100
80) Nitrobenzene	13.203	77	6990	48.829	ug/l	98
81) p-Isopropyltoluene	11.785	119	347537	10.712	ug/l	99
82) 1,3-Dichlorobenzene	11.737	146	170997	10.490	ug/l	100
83) 1,4-Dichlorobenzene	11.830	146	171995	10.541	ug/l	99
84) n-Butylbenzene	12.200	91	331771	11.026	ug/l	100
85) 1,2-Dichlorobenzene	12.203	146	161014	10.514	ug/l	99
86) 1,2-Dibromo-3-Chloropr...	12.987	75	11077	10.149	ug/l	96
87) 1,2,4-Trichlorobenzene	13.833	180	104878	11.013	ug/l	100
88) Hexachlorobutadiene	14.013	225	56592	10.464	ug/l	99
89) Naphthalene	14.081	128	188918	11.071	ug/l	100
90) 1,2,3-Trichlorobenzene	14.322	180	98222	11.161	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063519.D
Acq On : 17 Jul 2025 09:25
Operator : MD/SY
Sample : VSTDCCC010
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1


Quant Time: Jul 18 04:09:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

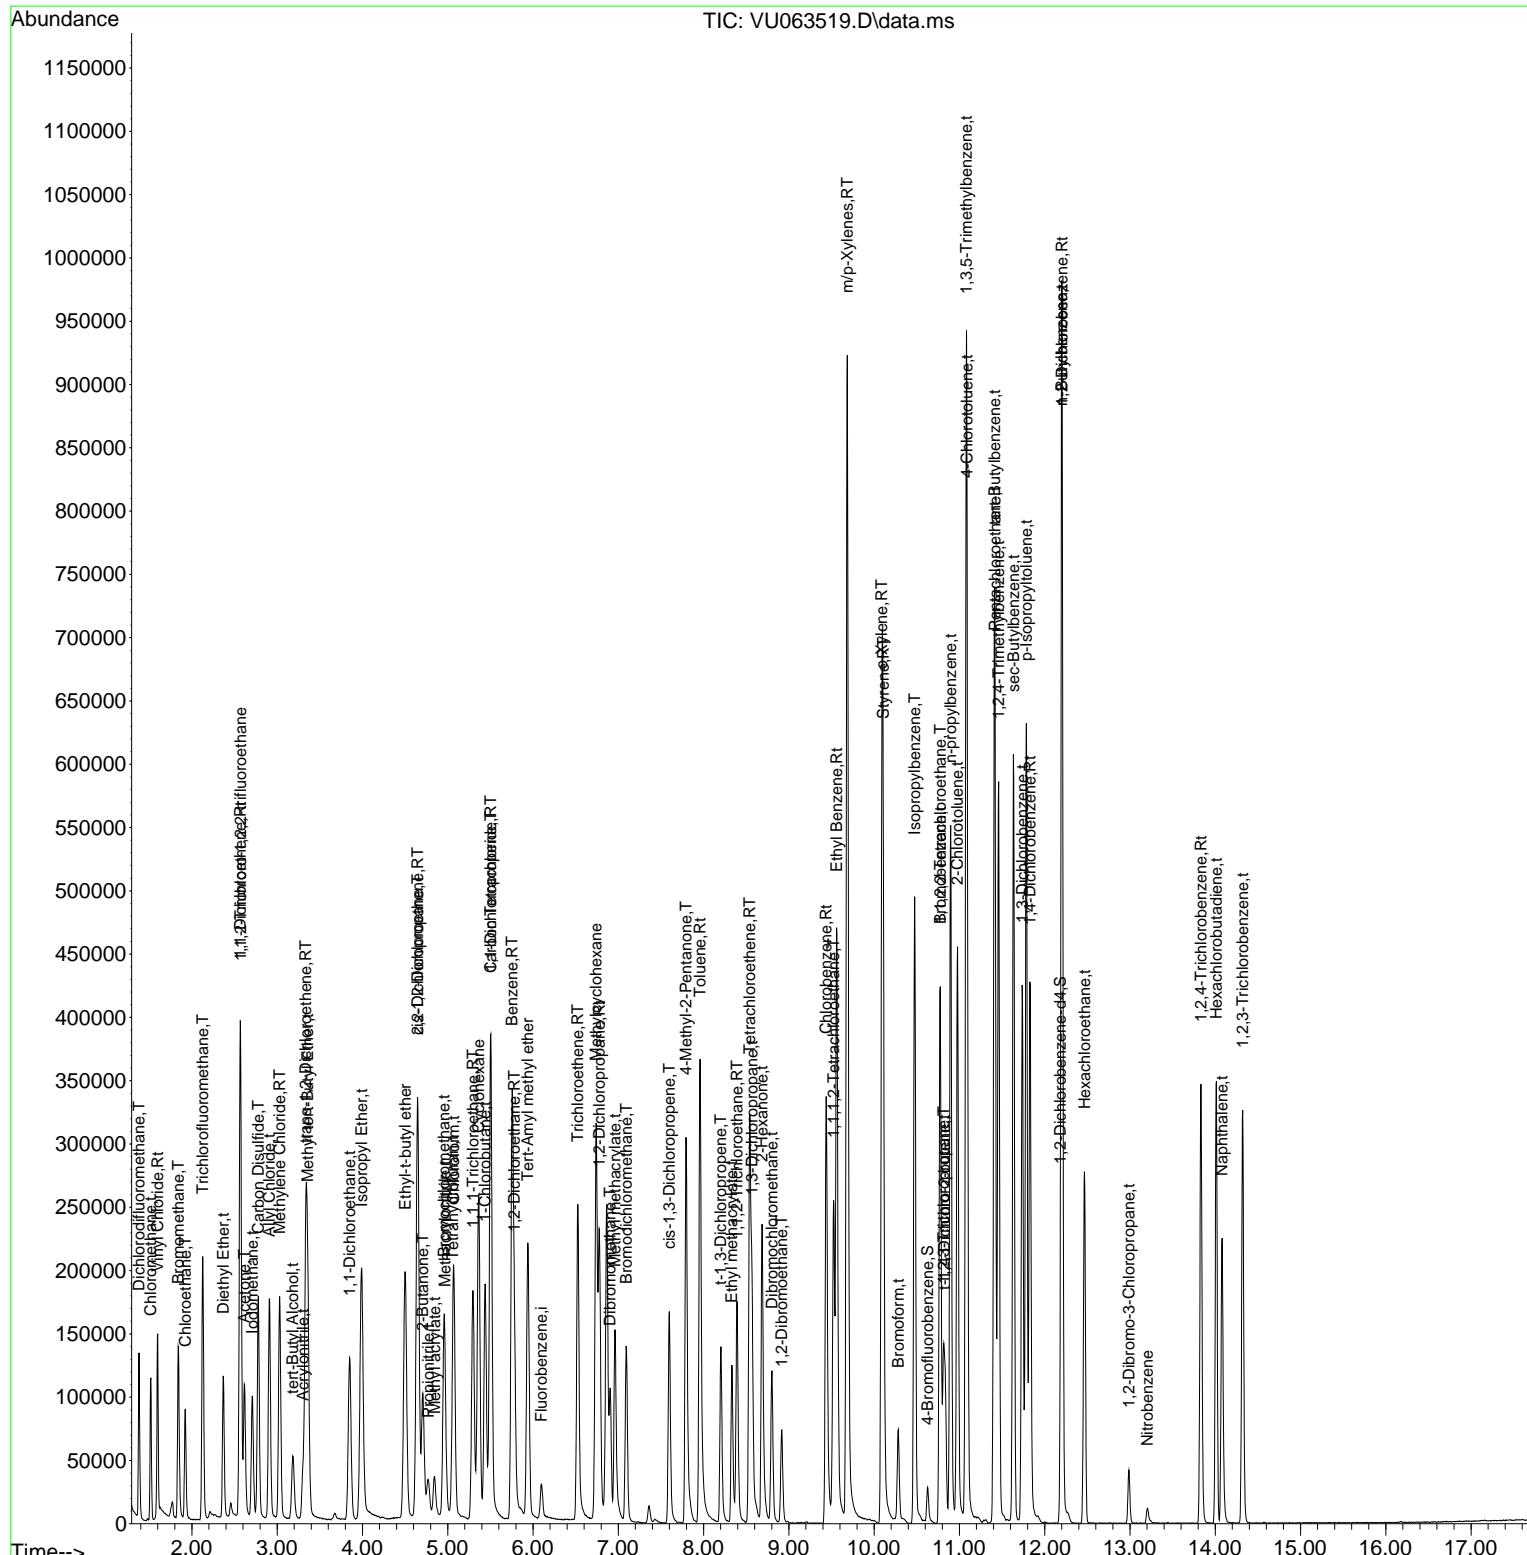



#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 96 Resp: 27500
Ion Ratio Lower Upper
96 100
70 17.1 15.0 22.4
95 7.3 7.4 11.0
97 0.0 0.0 0.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


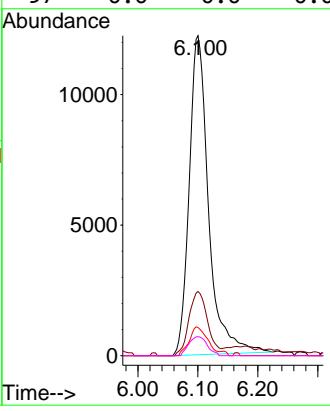
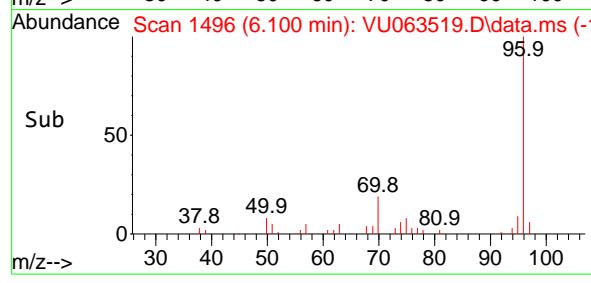


#2
Dichlorodifluoromethane
Concen: 9.643 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25



Tgt Ion: 85 Resp: 78194
Ion Ratio Lower Upper
85 100
87 31.5 16.0 47.9

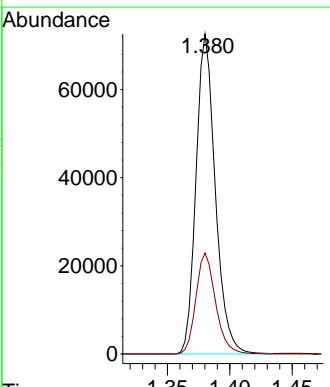



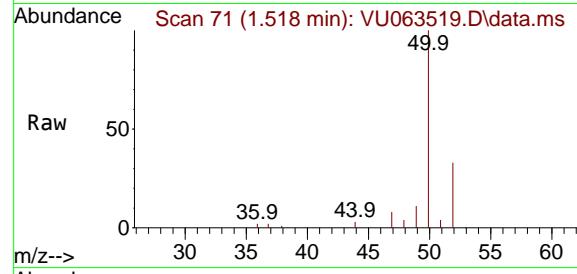



#3
Chloromethane
Concen: 9.902 ug/l
RT: 1.518 min Scan# 7
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument :
MSVOA_U
ClientSampleId :
VSTDCCC010


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#4
Vinyl Chloride
Concen: 9.718 ug/l
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion: 62 Resp: 93296
Ion Ratio Lower Upper
62 100
64 32.1 25.7 38.5

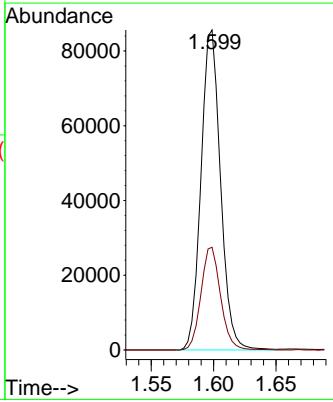







#5
Bromomethane
Concen: 9.188 ug/l
RT: 1.840 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#6
Chloroethane
Concen: 9.774 ug/l
RT: 1.923 min Scan# 197
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25


Tgt Ion: 64 Resp: 56651
Ion Ratio Lower Upper
64 100
66 31.7 26.2 39.4

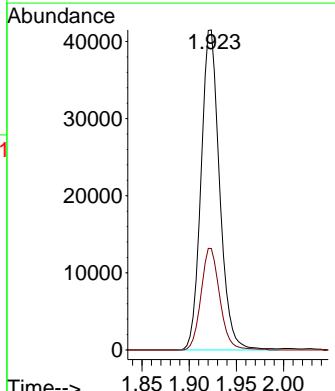



#7
Trichlorofluoromethane
Concen: 9.648 ug/l
RT: 2.126 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

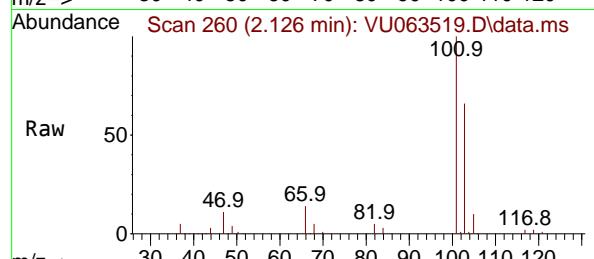


Tgt Ion:101 Resp: 132982
Ion Ratio Lower Upper
101 100
103 65.5 52.2 78.4

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

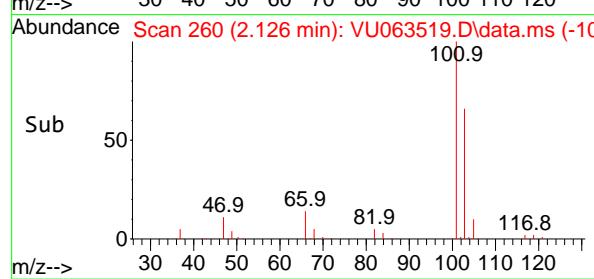


#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 9.874 ug/l
RT: 2.570 min Scan# 398
Delta R.T. 0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Tgt Ion:101 Resp: 71124
Ion Ratio Lower Upper
101 100
85 46.4 37.8 56.6
151 74.9 59.2 88.8

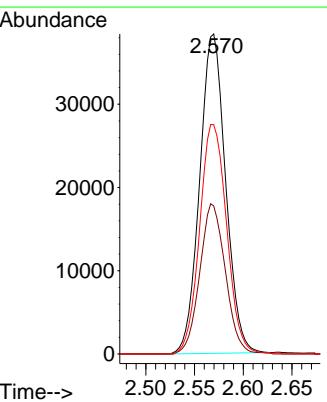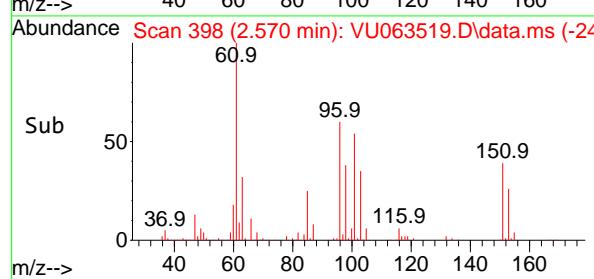



#9
1,1-Dichloroethene
Concen: 9.834 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 96 Resp: 7021:
Ion Ratio Lower Upper
96 100
61 168.0 0.0 504.3
98 61.7 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

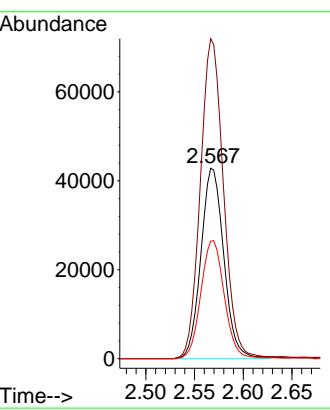


#10
Iodomethane
Concen: 9.096 ug/l
RT: 2.708 min Scan# 441
Delta R.T. -0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Tgt Ion:142 Resp: 96119
Ion Ratio Lower Upper
142 100
127 48.0 37.9 56.9

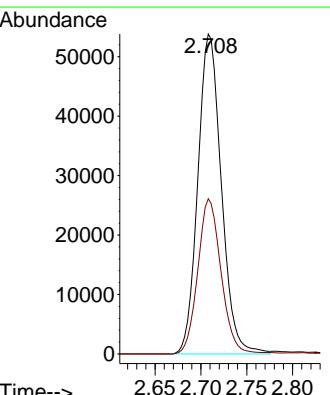



#11
 Allyl Chloride
 Concen: 9.904 ug/l
 RT: 2.907 min Scan# 5
 Delta R.T. 0.000 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
 ClientSampleId : VSTDCCC010




Tgt Ion: 41 Resp: 10215
 Ion Ratio Lower Upper
 41 100
 39 76.2 61.5 92.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

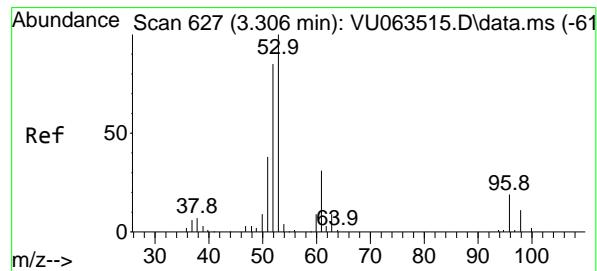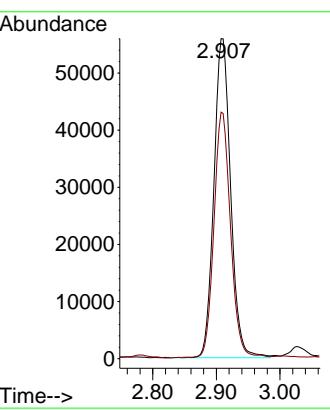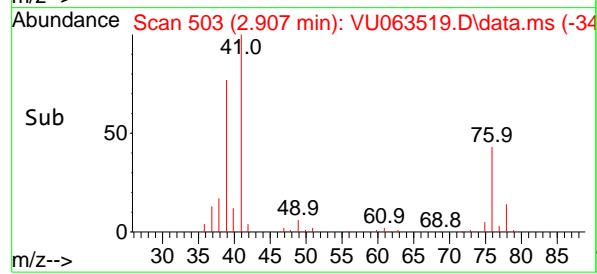


#12
 Acrylonitrile
 Concen: 19.426 ug/l
 RT: 3.303 min Scan# 626
 Delta R.T. -0.003 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25

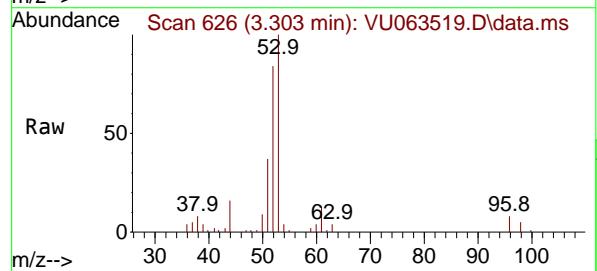


Tgt Ion: 53 Resp: 34689
 Ion Ratio Lower Upper
 53 100
 52 81.5 64.3 96.5
 51 36.0 27.8 41.8

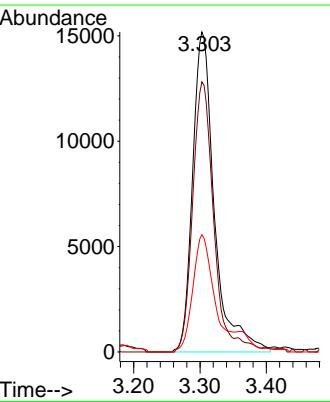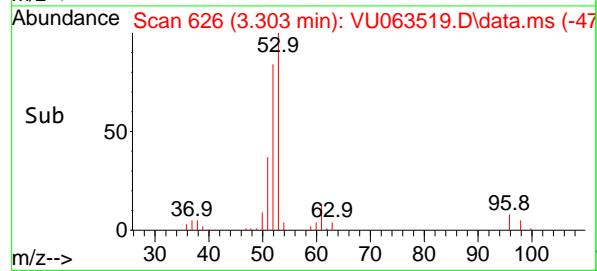



#13
Acetone
Concen: 76.573 ug/l
RT: 2.618 min Scan# 4
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25



Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

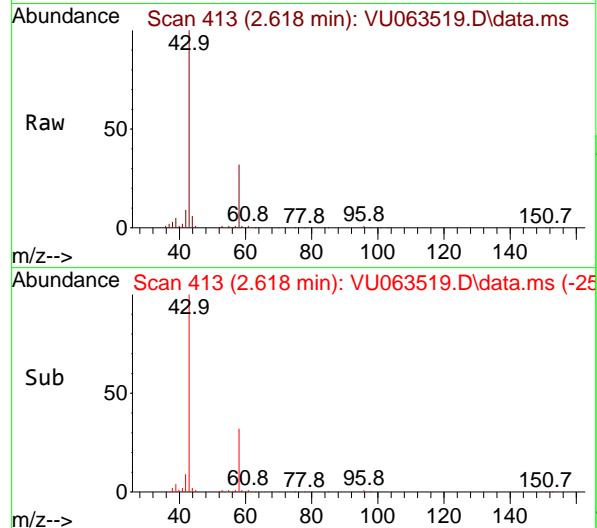


Tgt Ion: 43 Resp: 109555
Ion Ratio Lower Upper
43 100
58 32.7 25.4 38.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025









#14
Carbon Disulfide
Concen: 9.597 ug/l
RT: 2.779 min Scan# 463
Delta R.T. 0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25



Tgt Ion: 76 Resp: 221309
Ion Ratio Lower Upper
76 100
78 8.7 7.0 10.6





#15

Methylene Chloride

Concen: 9.347 ug/l

RT: 3.030 min Scan# 541

Delta R.T. 0.000 min


Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U

ClientSampleId :

VSTDCCC010

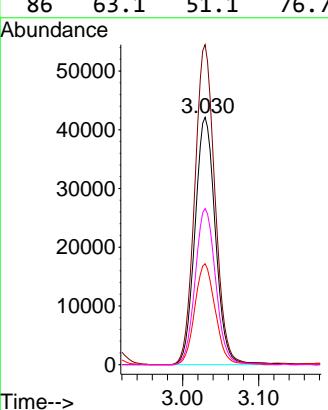**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#16

trans-1,2-Dichloroethene

Concen: 9.547 ug/l

RT: 3.335 min Scan# 636


Delta R.T. 0.000 min




Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Tgt Ion: 96 Resp: 77415

Ion	Ratio	Lower	Upper
96	100		
61	144.5	117.2	175.8
98	62.6	51.4	77.2

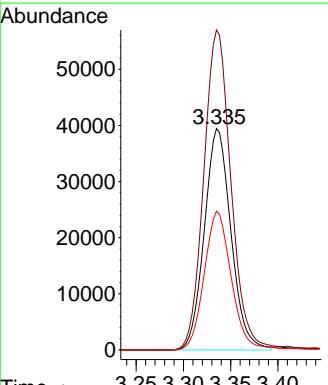

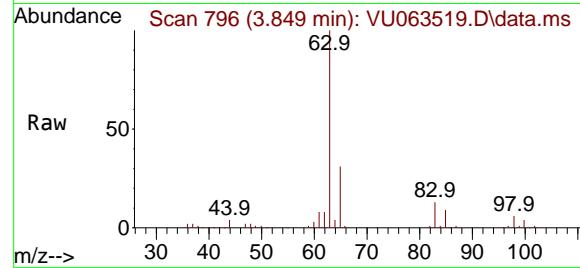

#17

1,1-Dichloroethane

Concen: 9.813 ug/l

RT: 3.849 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#18

2-Butanone

Concen: 61.835 ug/l

RT: 4.708 min Scan# 1063

Delta R.T. -0.003 min

Lab File: VU063519.D


Acq: 17 Jul 2025 09:25


Tgt Ion: 43 Resp: 137001

Ion Ratio Lower Upper

43 100

57 8.3 0.0 16.4

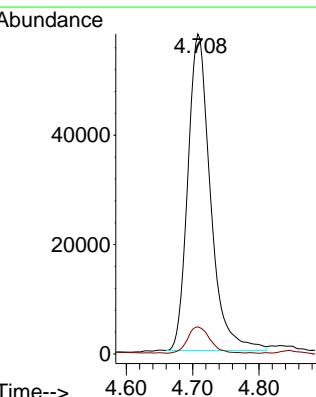



#19

Cyclohexane

Concen: 9.447 ug/l

RT: 5.364 min Scan# 1


Delta R.T. 0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U

ClientSampleId : VSTDCCC010



Tgt Ion: 56 Resp: 120210

Ion Ratio Lower Upper

56 100




69 34.3 26.6 39.8

84 91.3 71.0 106.4


**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025



Supervised By :Semsettin Yesilyurt 07/21/2025

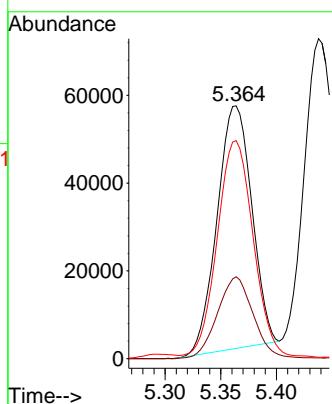


#20
Methylcyclohexane
Concen: 10.376 ug/l
RT: 6.740 min Scan# 1695
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Tgt Ion: 83 Resp: 128329
Ion Ratio Lower Upper
83 100
55 77.8 60.6 90.8
98 47.0 35.8 53.8

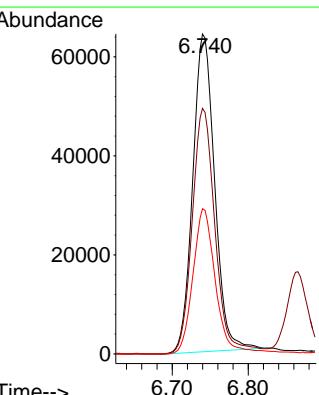



#21
2,2-Dichloropropane
Concen: 9.790 ug/l
RT: 4.647 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 77 Resp: 12529
Ion Ratio Lower Upper
77 100
97 22.0 17.8 26.8

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


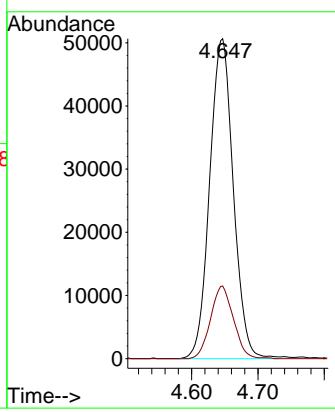



#22
cis-1,2-Dichloroethene
Concen: 9.751 ug/l
RT: 4.647 min Scan# 1044
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25



Tgt Ion: 96 Resp: 85795
Ion Ratio Lower Upper
96 100
61 154.9 0.0 384.7
98 64.2 32.1 96.3

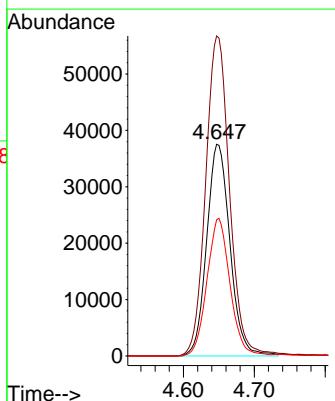

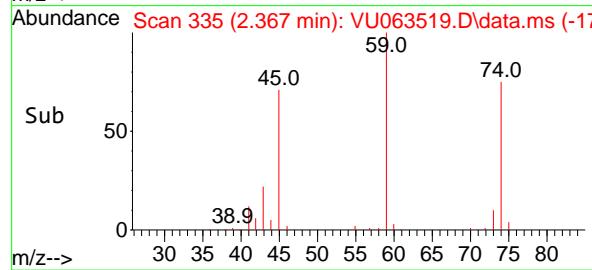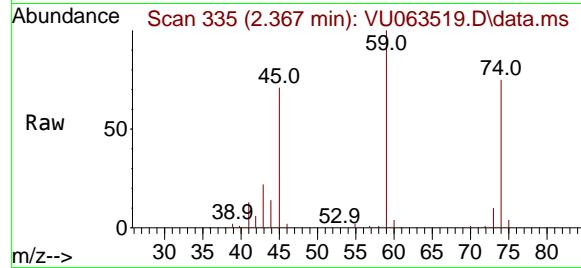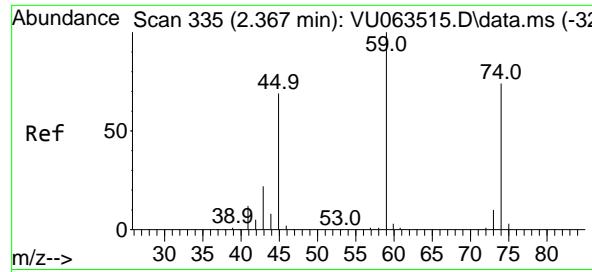

#23

Diethyl Ether

Concen: 10.062 ug/l

RT: 2.367 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

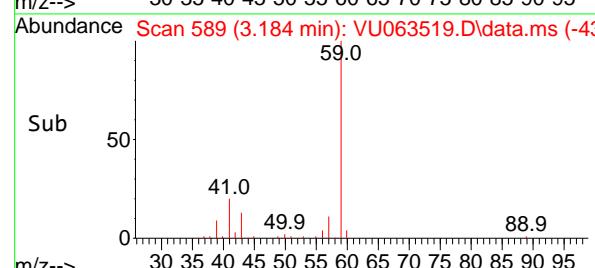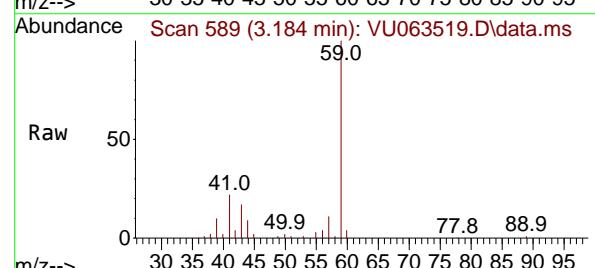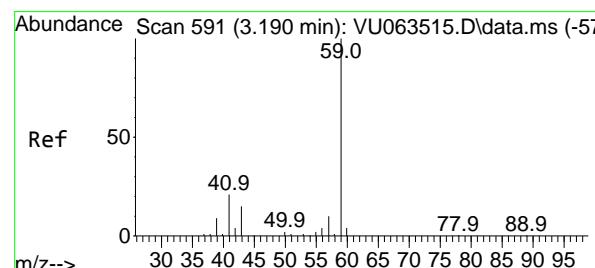

#24

tert-Butyl Alcohol

Concen: 96.429 ug/l

RT: 3.184 min Scan# 589

Delta R.T. -0.006 min

Lab File: VU063519.D


Acq: 17 Jul 2025 09:25


Tgt Ion: 59 Resp: 63328

Ion Ratio Lower Upper

59 100

57 10.6 8.6 12.8

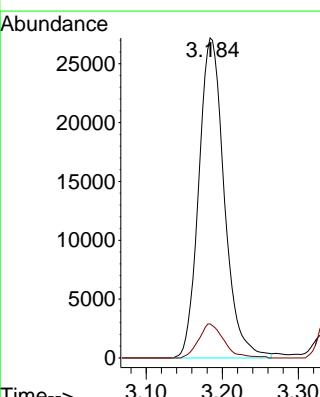


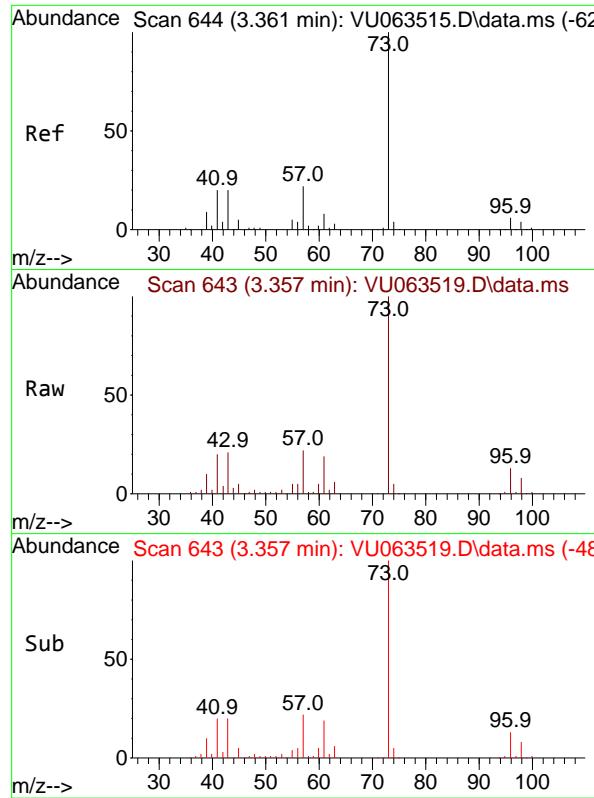


#25
Methyl tert-Butyl Ether
Concen: 10.052 ug/l
RT: 3.357 min Scan# 6
Delta R.T. -0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

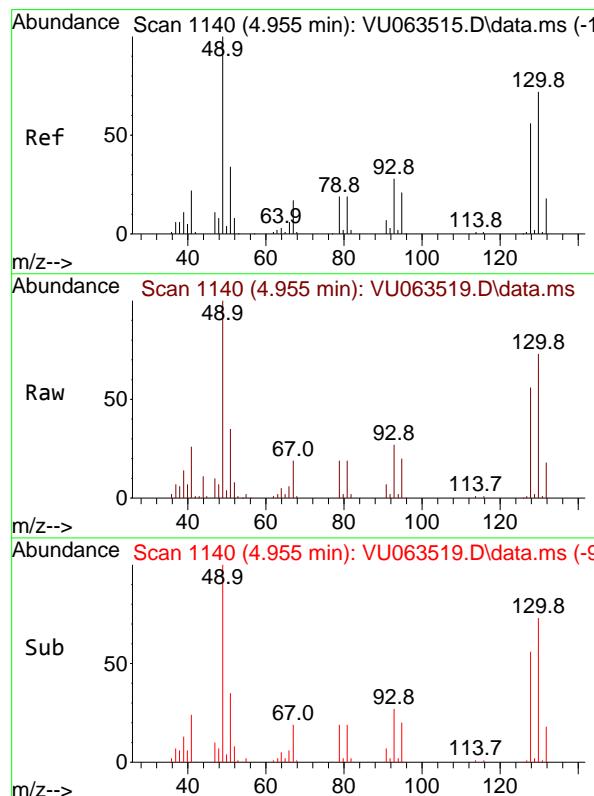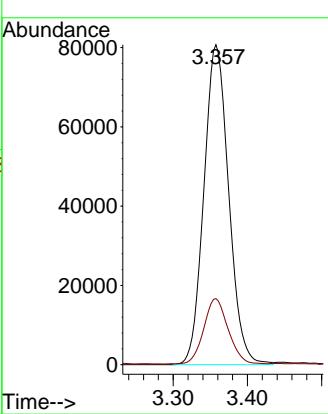

#26
Bromochloromethane
Concen: 10.094 ug/l
RT: 4.955 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25


Tgt Ion:128 Resp: 37081
Ion Ratio Lower Upper
128 100
49 173.8 0.0 340.8
130 126.8 100.5 150.7





#27
 Chloroform
 Concen: 9.734 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
 ClientSampleId : VSTDCCC010




Tgt Ion: 83 Resp: 149270
 Ion Ratio Lower Upper
 83 100
 85 65.2 0.0 130.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

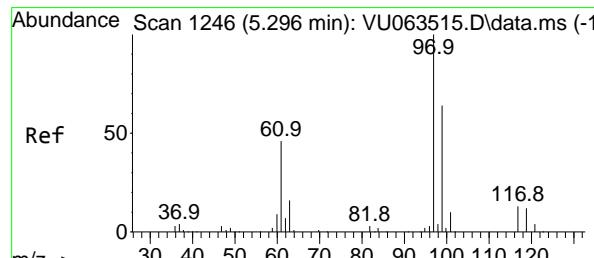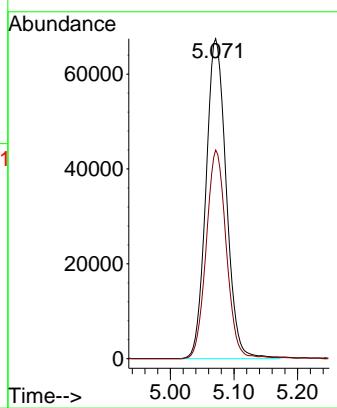


#28
 1,1,1-Trichloroethane
 Concen: 9.841 ug/l
 RT: 5.296 min Scan# 1246
 Delta R.T. 0.000 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25

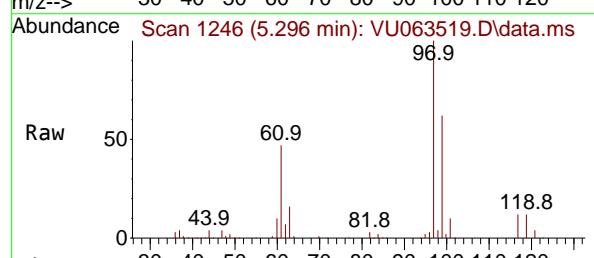

Tgt Ion: 97 Resp: 128095
 Ion Ratio Lower Upper
 97 100
 99 64.3 31.8 95.3
 61 47.5 23.3 69.9

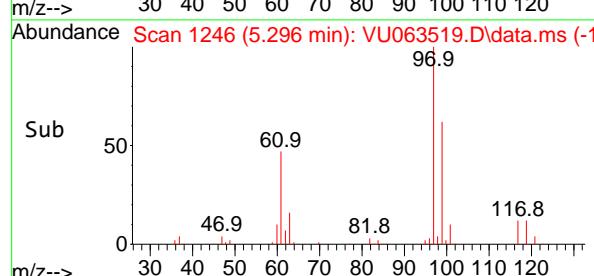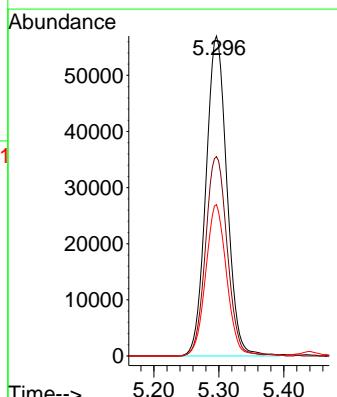



#29

1,1-Dichloropropene


Concen: 9.703 ug/l

RT: 5.505 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25



Tgt Ion: 75 Resp: 11699

Ion Ratio Lower Upper

75 100

110 34.1 17.8 53.4

77 29.9 24.6 37.0

Instrument:

MSVOA_U




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

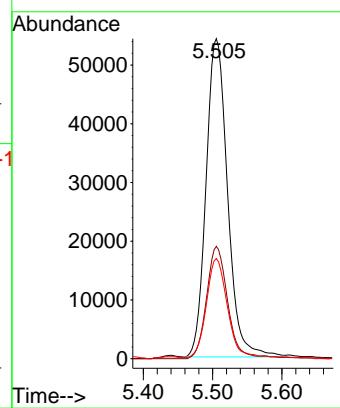

#30

Carbon Tetrachloride





Concen: 10.193 ug/l




RT: 5.502 min Scan# 1310

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

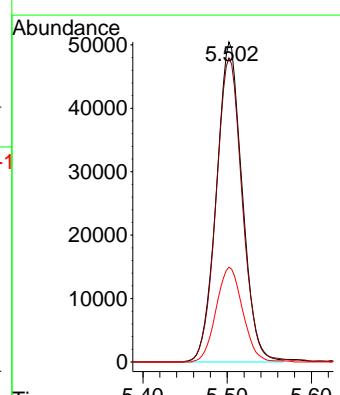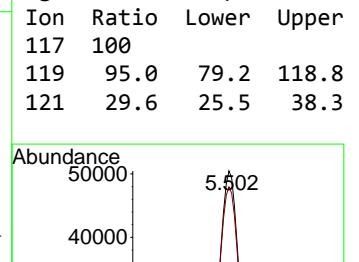



#31

Isopropyl Ether

Concen: 9.757 ug/l

RT: 3.991 min Scan# 8

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25






Instrument :


MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

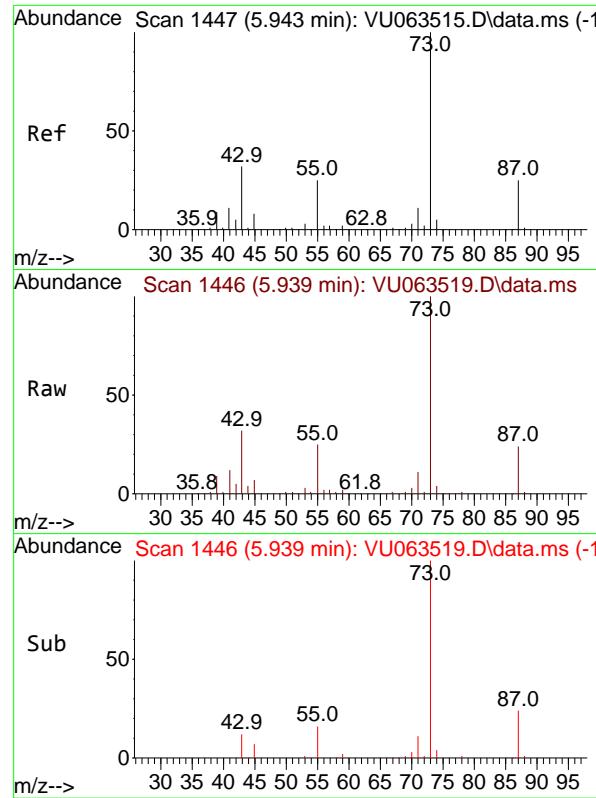 #32
 Ethyl-t-butyl ether
 Concen: 9.745 ug/l
 RT: 4.502 min Scan# 999
 Delta R.T. 0.000 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25

 Tgt Ion: 59 Resp: 204582
 Ion Ratio Lower Upper
 59 100
 87 41.9 32.6 49.0




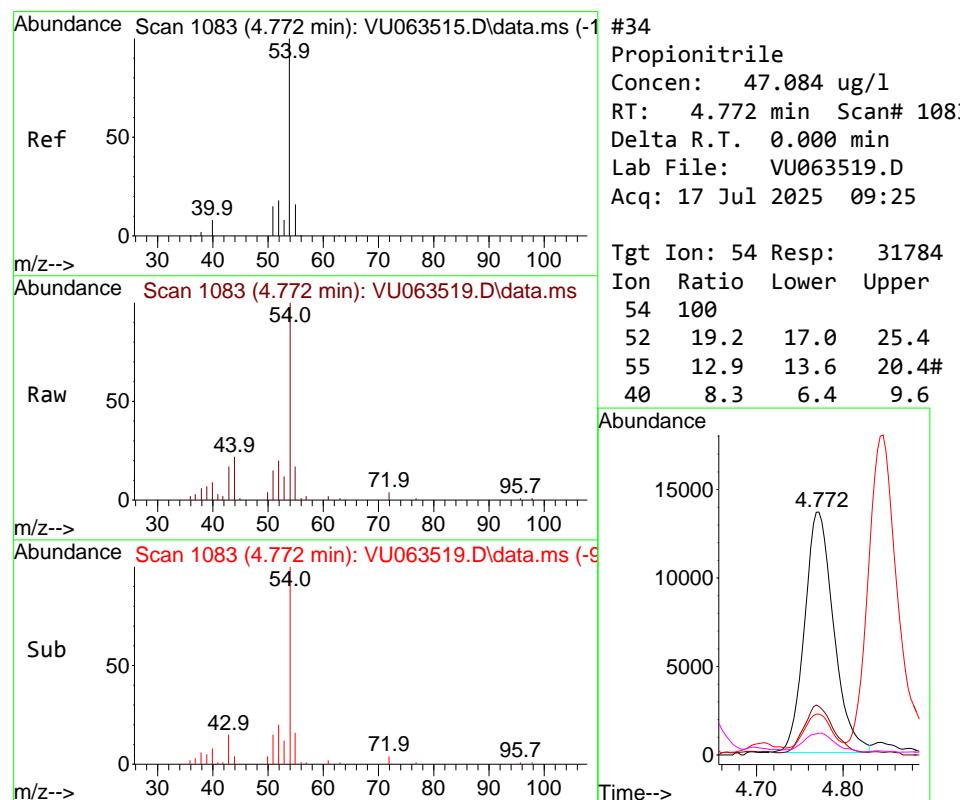
#33

Tert-Amyl methyl ether
Concen: 9.982 ug/l
RT: 5.939 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#34

Propionitrile
Concen: 47.084 ug/l
RT: 4.772 min Scan# 1083
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion: 54 Resp: 31784
Ion Ratio Lower Upper
54 100
52 19.2 17.0 25.4
55 12.9 13.6 20.4#
40 8.3 6.4 9.6

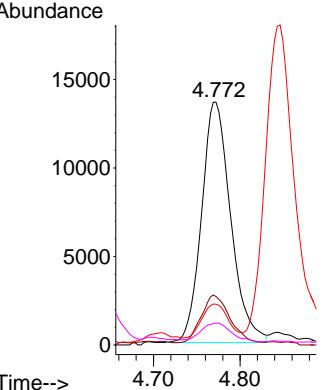



#35

Benzene

Concen: 10.088 ug/l

RT: 5.756 min Scan# 1389

Delta R.T. 0.000 min

Lab File: VU063519.D




Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

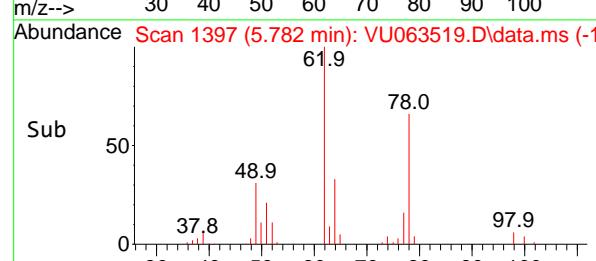**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#36

1,2-Dichloroethane

Concen: 10.057 ug/l

RT: 5.782 min Scan# 1397

Delta R.T. 0.000 min

Lab File: VU063519.D


Acq: 17 Jul 2025 09:25


Tgt Ion: 62 Resp: 101239

Ion Ratio Lower Upper

62 100


98 8.4 6.4 9.6

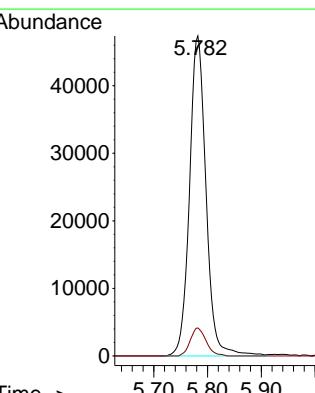



#37
Trichloroethene
Concen: 10.590 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion:130 Resp: 8753
Ion Ratio Lower Upper
130 100
95 103.2 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



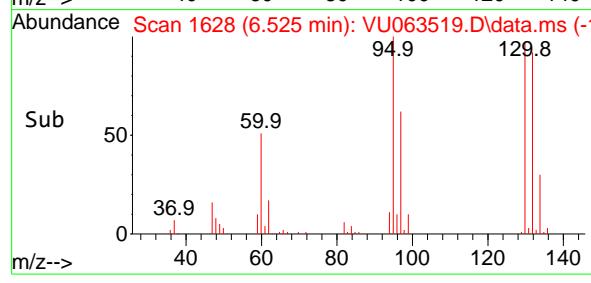


#38
1,2-Dichloropropane
Concen: 11.175 ug/l
RT: 6.779 min Scan# 1707
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25



Tgt Ion: 63 Resp: 84731
Ion Ratio Lower Upper
63 100
65 30.8 24.6 36.8

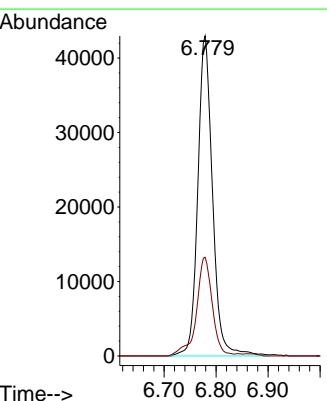

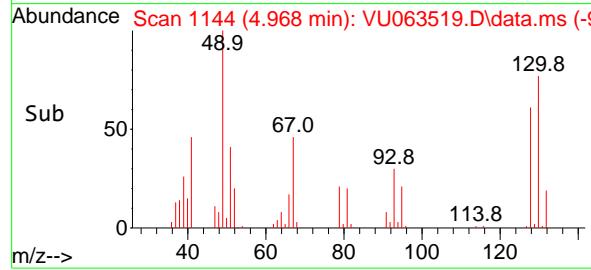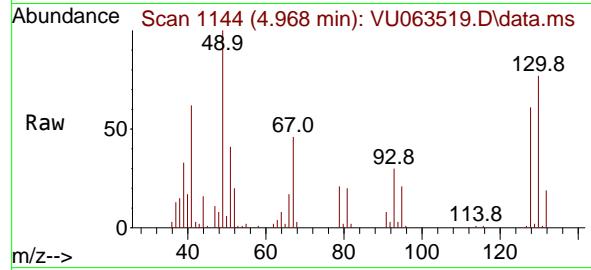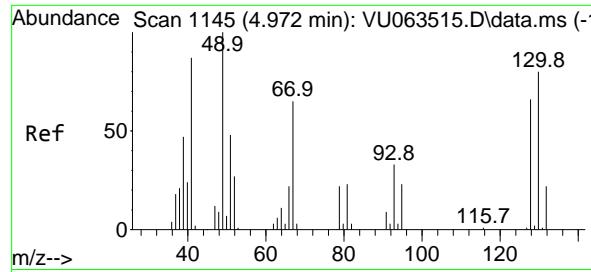

#39

Methacrylonitrile

Concen: 9.213 ug/l

RT: 4.968 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U

ClientSampleId :





VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

 Tgt Ion: 41 Resp: 2764
 Ion Ratio Lower Upper

	100		
41	100		
67	77.2	62.7	94.1
39	54.1	43.1	64.7
52	34.3	27.4	41.0

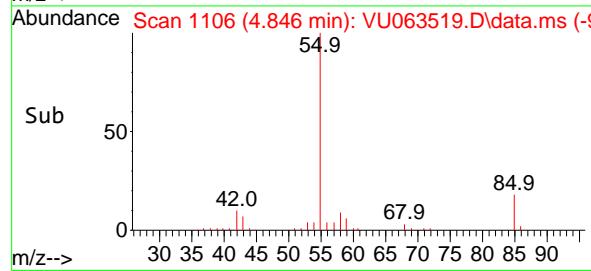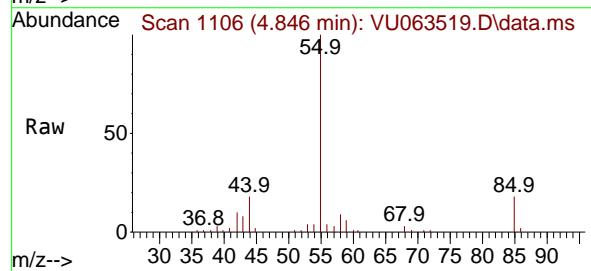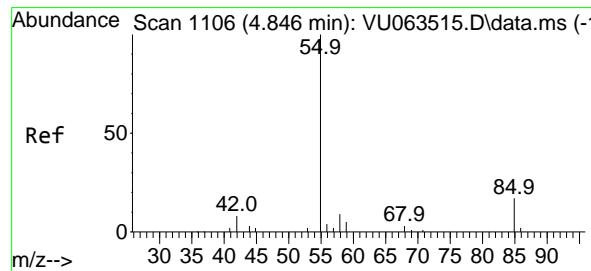

#40

Methyl acrylate

Concen: 9.339 ug/l

RT: 4.846 min Scan# 1106


Delta R.T. 0.000 min




Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

 Tgt Ion: 55 Resp: 40963
 Ion Ratio Lower Upper

	100		
55	100		
85	19.0	12.8	19.2
58	9.3	7.0	10.4
42	8.8	7.0	10.4





#41

Tetrahydrofuran

Concen: 17.936 ug/l

RT: 5.058 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

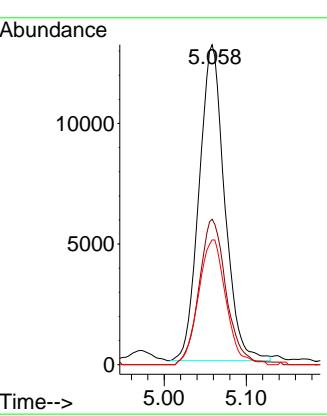 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#42

1-Chlorobutane


Concen: 9.953 ug/l


RT: 5.438 min Scan# 1290

Delta R.T. 0.000 min

Lab File: VU063519.D


Acq: 17 Jul 2025 09:25

 Tgt Ion: 56 Resp: 159543
 Ion Ratio Lower Upper
 56 100
 41 53.3 26.7 80.0

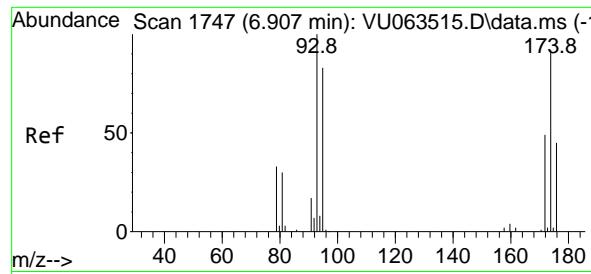


#43
Dibromomethane
Concen: 10.067 ug/l
RT: 6.904 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 93 Resp: 3954:
Ion Ratio Lower Upper
93 100
95 83.3 67.9 101.9
174 84.7 74.6 111.8

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

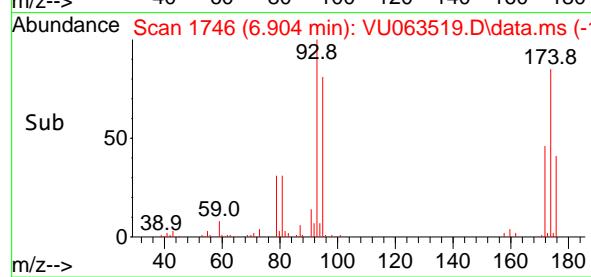


#44
Bromodichloromethane
Concen: 10.053 ug/l
RT: 7.094 min Scan# 1805
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Tgt Ion: 83 Resp: 89050
Ion Ratio Lower Upper
83 100
85 65.0 52.7 79.1
127 7.9 8.1 12.1#


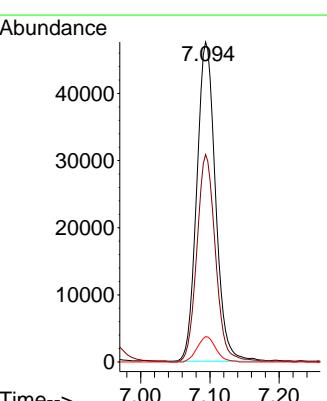





Abundance Scan 2023 (7.795 min): VU063519.D\data.ms

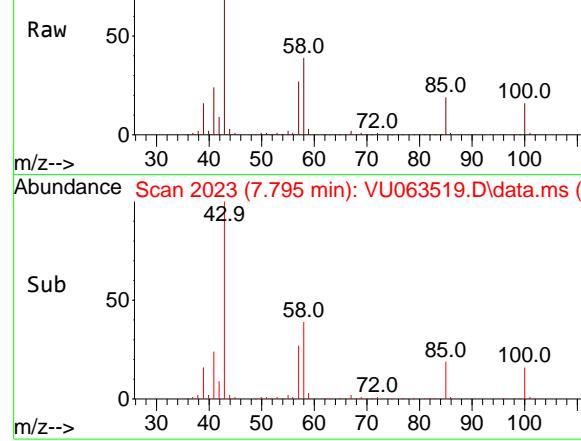


Abundance Scan 2023 (7.795 min): VU063519.D\data.ms (-1)

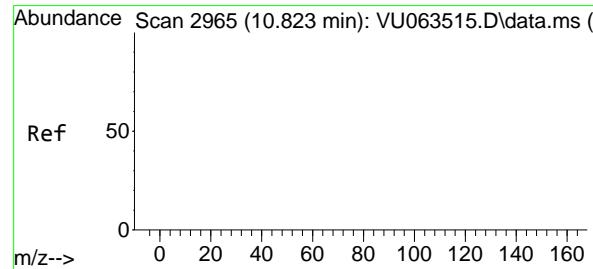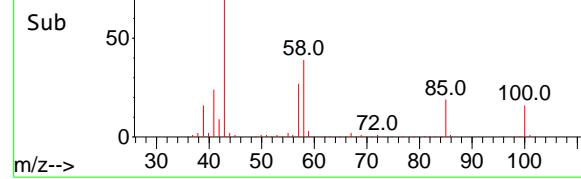

Abundance Scan 2965 (10.823 min): VU063519.D\data.ms

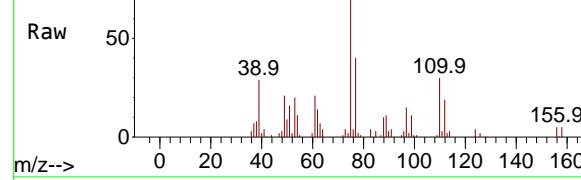

Abundance Scan 2965 (10.823 min): VU063519.D\data.ms (-1)

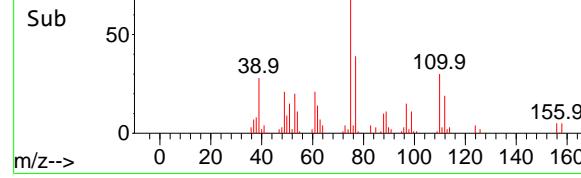

#45

4-Methyl-2-Pentanone

Concen: 52.266 ug/l

RT: 7.795 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

Tgt Ion: 43 Resp: 21158

Ion Ratio Lower Upper

43 100


58 39.9 20.0 60.0

85 19.4 15.4 23.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

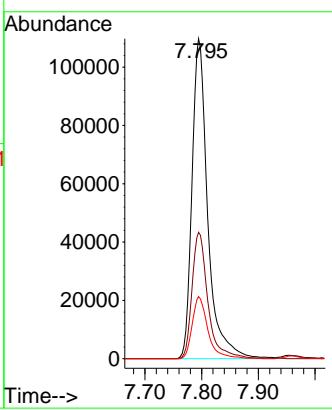

#46
t-1,4-Dichloro-2-butene
Concen: 18.890 ug/l m
RT: 10.823 min Scan# 2965
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion: 75 Resp: 28706


Ion Ratio Lower Upper




75 100

53 63.1 48.4 72.6

89 38.6 30.6 45.8

88 32.7 25.3 37.9

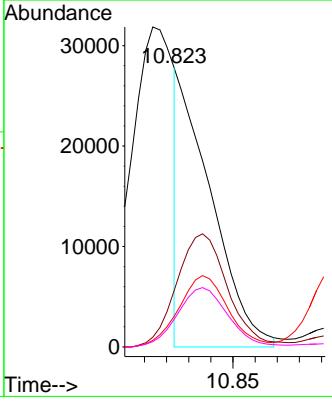



#47

Methyl methacrylate

Concen: 20.900 ug/l

RT: 6.962 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#48

Ethyl methacrylate

Concen: 10.861 ug/l

RT: 8.332 min Scan# 2190

Delta R.T. -0.003 min

Lab File: VU063519.D


Acq: 17 Jul 2025 09:25


Tgt Ion: 69 Resp: 68373

Ion Ratio Lower Upper

69 100


41 62.8 30.8 92.4





#49
Toluene
Concen: 10.158 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 92 Resp: 179669
Ion Ratio Lower Upper
92 100
91 176.8 140.4 210.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025




#50
t-1,3-Dichloropropene
Concen: 11.010 ug/l
RT: 8.203 min Scan# 2150
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25




Tgt Ion: 75 Resp: 76515
Ion Ratio Lower Upper
75 100
77 31.6 24.9 37.3

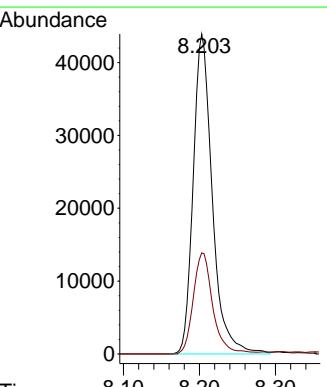



#51
cis-1,3-Dichloropropene
 Concen: 10.590 ug/l
 RT: 7.598 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25




Instrument : MSVOA_U
 ClientSampleId : VSTDCCC010

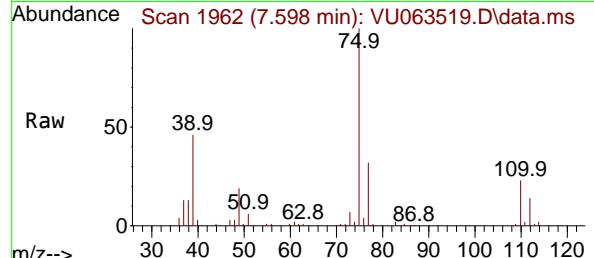


Tgt Ion: 75 Resp: 98781
 Ion Ratio Lower Upper
 75 100
 77 31.5 25.1 37.7
 39 46.0 37.8 56.6

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

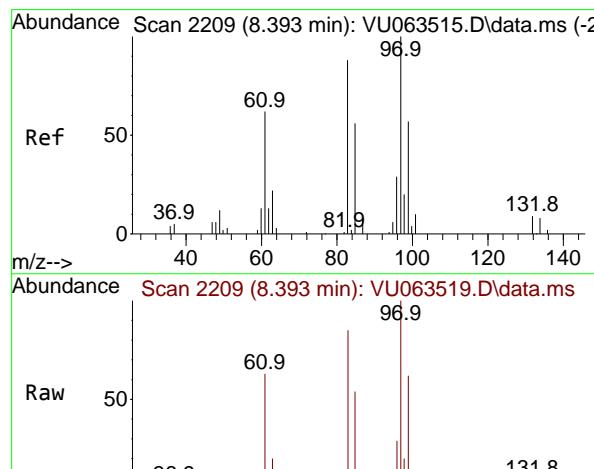
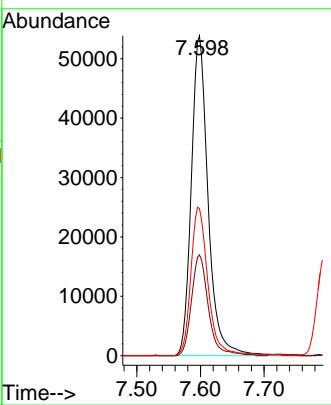
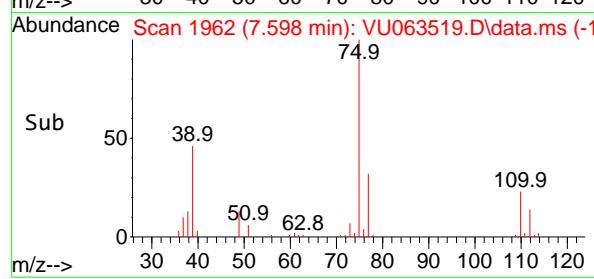


#52
 1,1,2-Trichloroethane
 Concen: 10.365 ug/l
 RT: 8.393 min Scan# 2209
 Delta R.T. 0.000 min
 Lab File: VU063519.D
 Acq: 17 Jul 2025 09:25

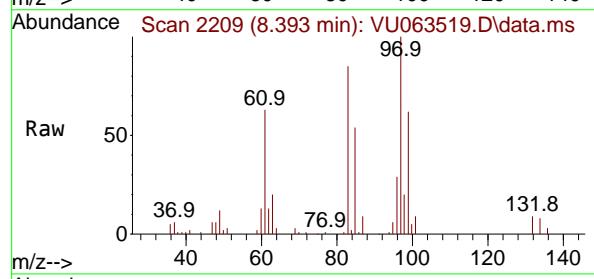

Tgt Ion: 97 Resp: 54808
 Ion Ratio Lower Upper
 97 100
 83 85.1 70.2 105.2
 85 53.8 45.2 67.8
 99 61.6 50.1 75.1

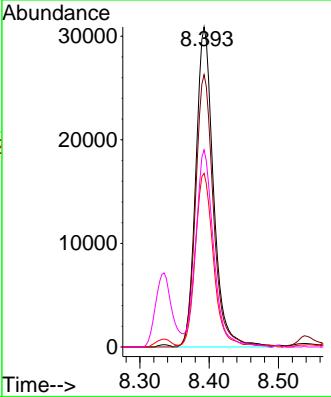



#53

1,3-Dichloropropane

Concen: 10.044 ug/l

RT: 8.566 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063519.D





Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

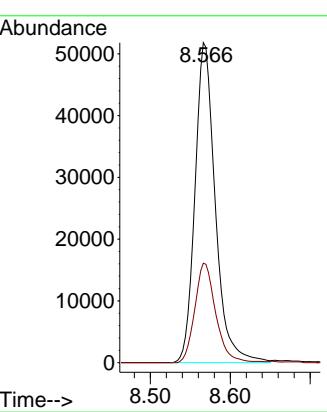**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#54

2-Hexanone

Concen: 60.570 ug/l


RT: 8.685 min Scan# 2300




Delta R.T. -0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Tgt Ion: 43 Resp: 162869
Ion Ratio Lower Upper
43 100
58 55.1 34.8 74.8
57 19.4 0.0 39.5

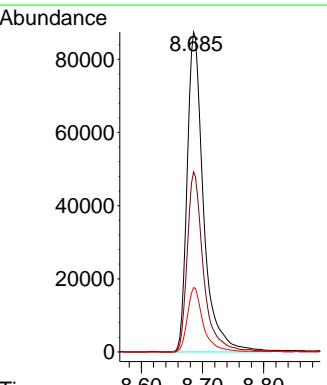






#55

Dibromochloromethane
Concen: 11.250 ug/l
RT: 8.801 min Scan# 2336
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#56

1,2-Dibromoethane
Concen: 10.326 ug/l
RT: 8.917 min Scan# 2372
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion:107 Resp: 48870
Ion Ratio Lower Upper
107 100
109 93.8 0.0 186.4

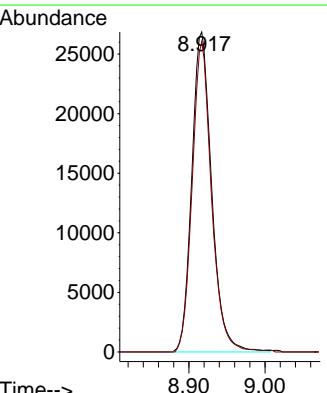

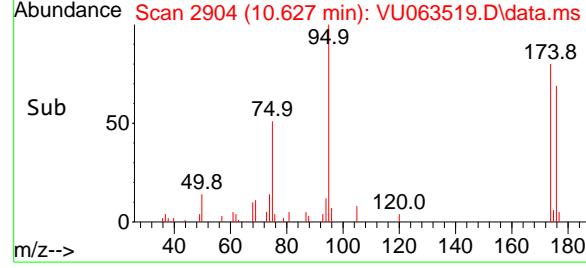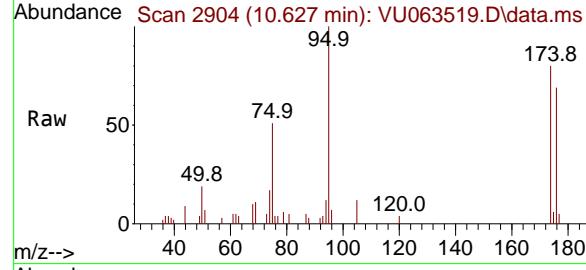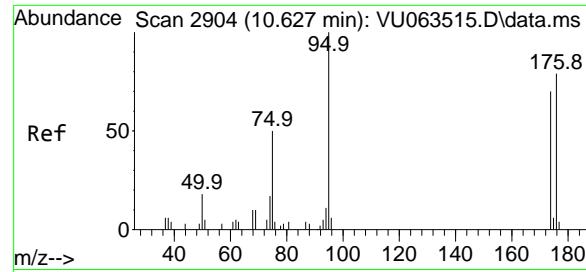

#57

4-Bromofluorobenzene

Concen: 0.965 ug/l

RT: 10.627 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25





Instrument :

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

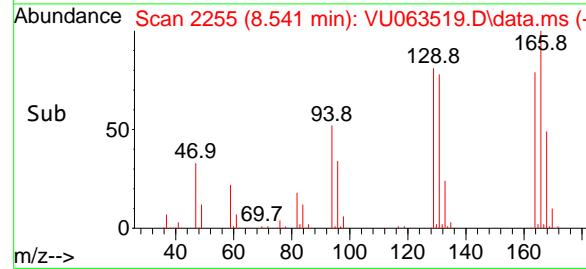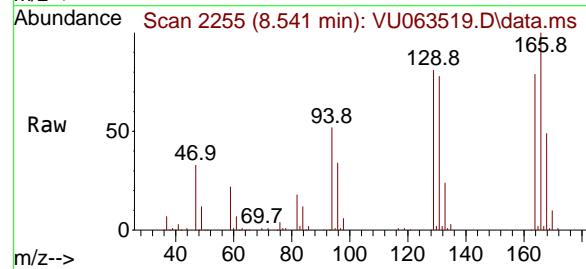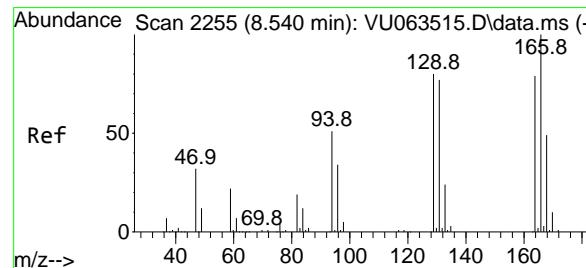 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#58

Tetrachloroethene

Concen: 9.712 ug/l


RT: 8.541 min Scan# 2255


Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Tgt	Ion:164	Resp:	73468
Ion	Ratio	Lower	Upper
164	100		
166	126.2	100.7	151.1
129	102.5	80.6	120.8
131	98.5	77.3	115.9


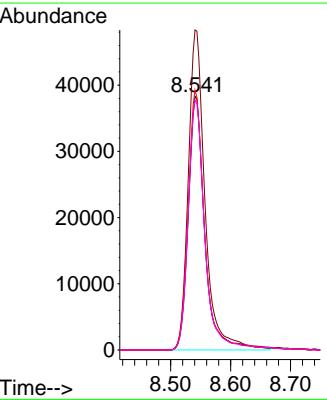


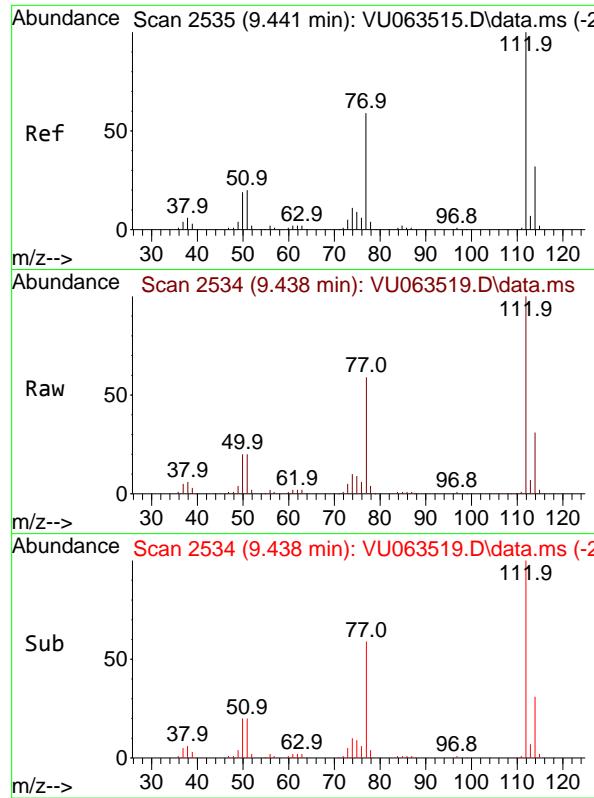

#59
Chlorobenzene
Concen: 10.255 ug/l
RT: 9.438 min Scan# 2
Instrument : MSVOA_U
Delta R.T. -0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

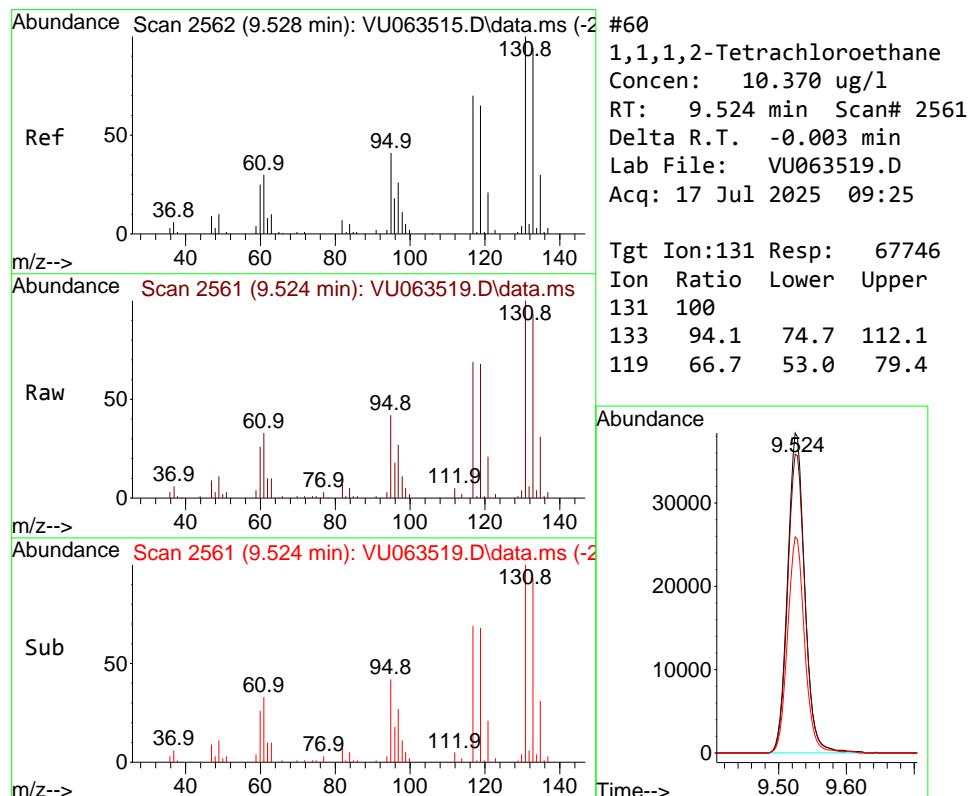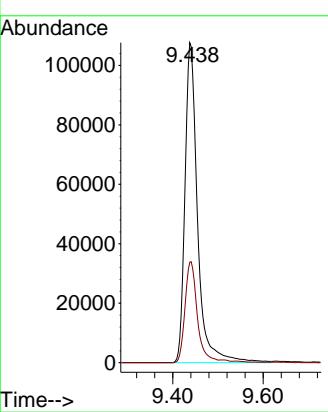

#60
1,1,1,2-Tetrachloroethane
Concen: 10.370 ug/l
RT: 9.524 min Scan# 2561
Delta R.T. -0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion:131 Resp: 67746
Ion Ratio Lower Upper
131 100
133 94.1 74.7 112.1
119 66.7 53.0 79.4

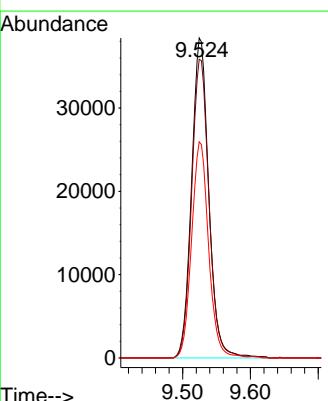



#61

Pentachloroethane

Concen: 10.774 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument :

MSVOA_U





ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

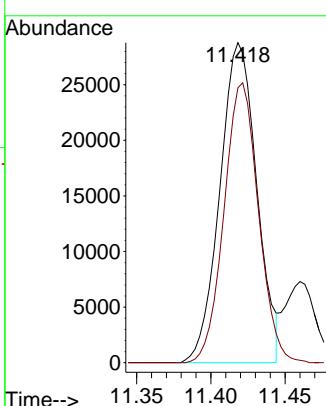

#62

Hexachloroethane


Concen: 11.016 ug/l




RT: 12.466 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

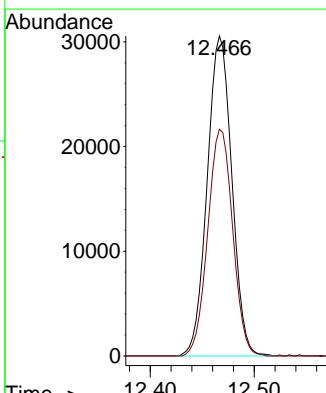Tgt Ion:117 Resp: 50359
Ion Ratio Lower Upper
117 100
201 71.6 57.4 86.0




#63

Ethyl Benzene

Concen: 10.146 ug/l

RT: 9.563 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#64

m/p-Xylenes


Concen: 20.632 ug/l




RT: 9.685 min Scan# 2611

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

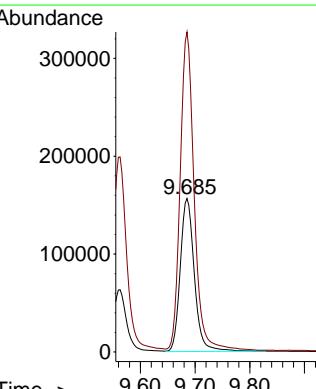 Tgt Ion:106 Resp: 280366
 Ion Ratio Lower Upper
 106 100
 91 206.6 163.6 245.4



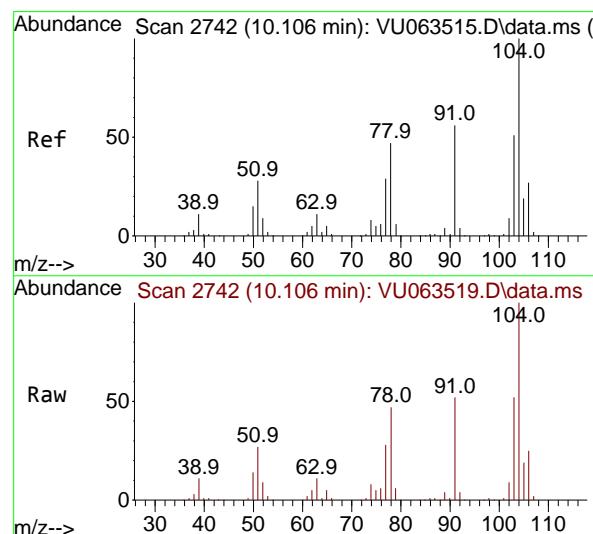


#65
o-Xylene
Concen: 10.509 ug/l
RT: 10.090 min Scan# 2
Instrument : MSVOA_U
Delta R.T. -0.003 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

ClientSampleId : VSTDCCC010



Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#66
Styrene
Concen: 10.792 ug/l
RT: 10.106 min Scan# 2742
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion:104 Resp: 224585
Ion Ratio Lower Upper
104 100
78 51.7 41.3 61.9
103 55.1 43.6 65.4

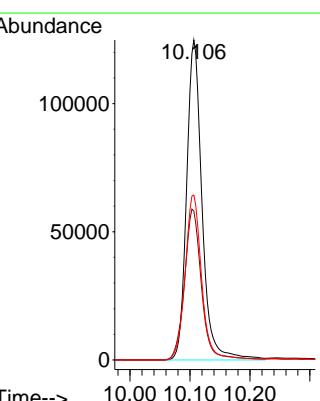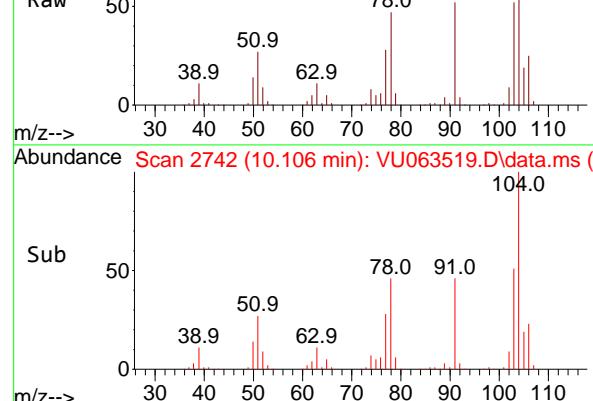



#67

Bromoform

Concen: 11.101 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25





Instrument :

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

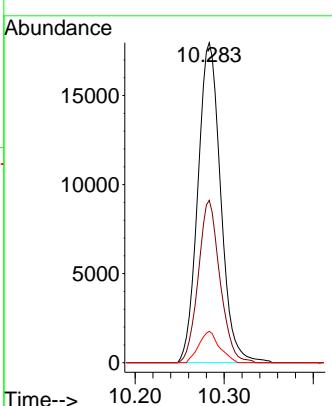 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#68

1,2-Dichlorobenzene-d4

Concen: 0.968 ug/l


RT: 12.183 min Scan# 3388




Delta R.T. -0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Tgt	Ion:152	Resp:	9321
Ion	Ratio	Lower	Upper
152	100		
115	136.9	0.0	262.2
150	338.6	0.0	651.2

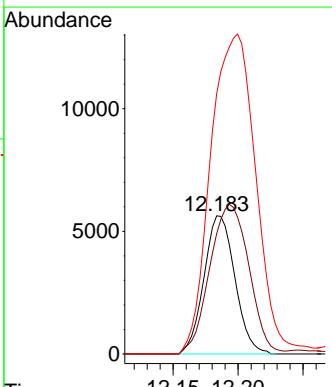



#69

Isopropylbenzene

Concen: 10.511 ug/l

RT: 10.476 min Scan# 2

Instrument :

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 10.472 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25



Tgt Ion: 83 Resp: 67383




Ion Ratio Lower Upper

83 100

131 9.8 8.4 12.6

85 66.0 51.9 77.9

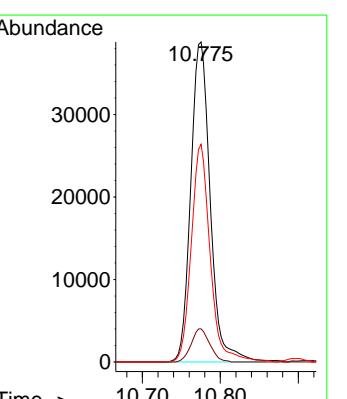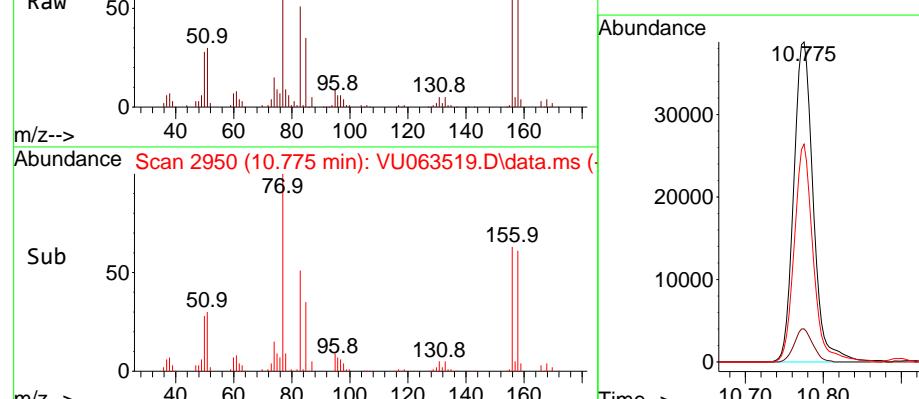

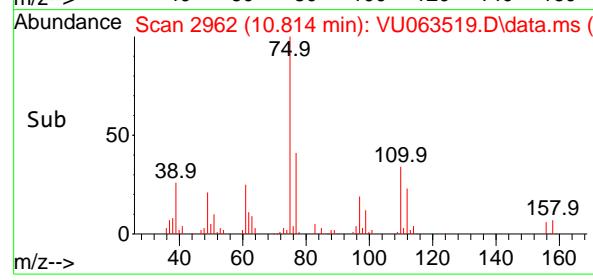

#71

1,2,3-Trichloropropane

Concen: 10.239 ug/l m

RT: 10.814 min Scan# 2962

Delta R.T. -0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#72

Bromobenzene

Concen: 10.490 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25


Tgt Ion:156 Resp: 85460


Ion Ratio Lower Upper

156 100

77 155.6 0.0 315.2


158 95.5 0.0 195.4

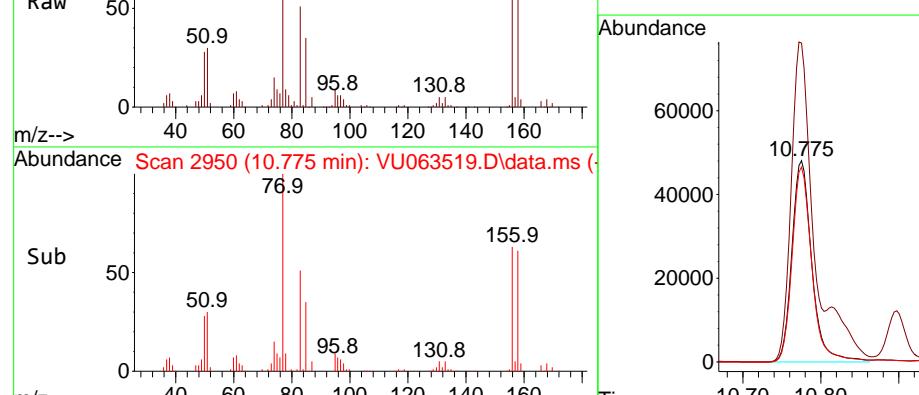



#73
n-propylbenzene
Concen: 10.559 ug/l
RT: 10.897 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25



Instrument : MSVOA_U
ClientSampleId : VSTDCCC010



Tgt Ion:120 Resp: 100342
Ion Ratio Lower Upper
120 100
91 434.4 343.1 514.7



Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

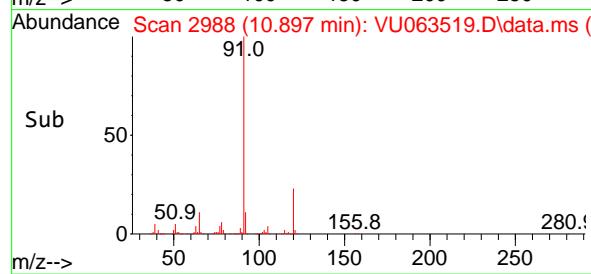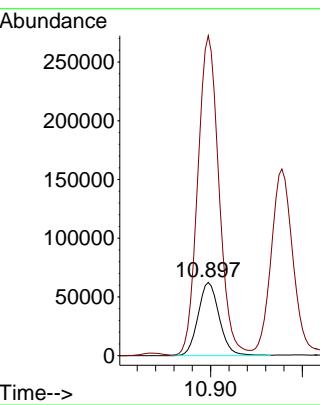


#74
2-Chlorotoluene
Concen: 10.457 ug/l
RT: 10.978 min Scan# 3013
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25


Tgt Ion:126 Resp: 87826
Ion Ratio Lower Upper
126 100
91 300.6 0.0 606.0


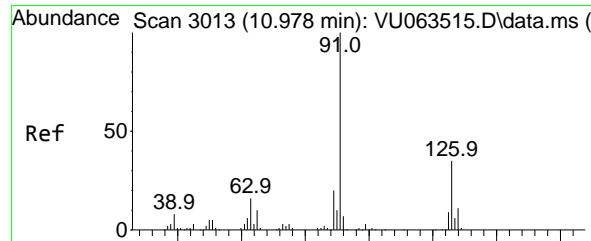
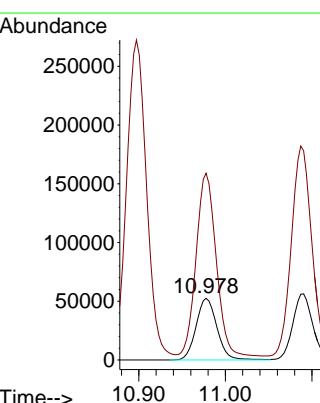


10.978



10.978









#75
1,3,5-Trimethylbenzene
Concen: 10.596 ug/l
RT: 11.081 min Scan# 3045
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#76
4-Chlorotoluene
Concen: 10.731 ug/l
RT: 11.090 min Scan# 3048
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion:126 Resp: 91522
Ion Ratio Lower Upper
126 100
91 333.4 0.0 682.2

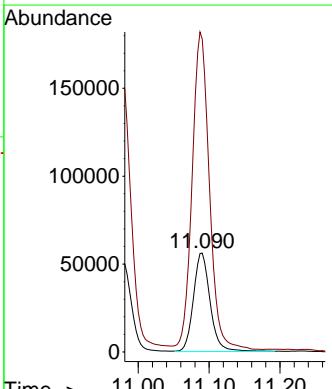

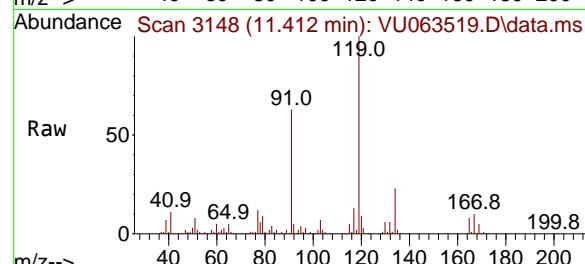

#77

tert-Butylbenzene

Concen: 10.518 ug/l

RT: 11.412 min Scan# 3148

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25





Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

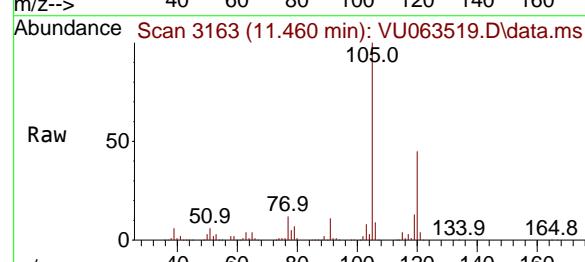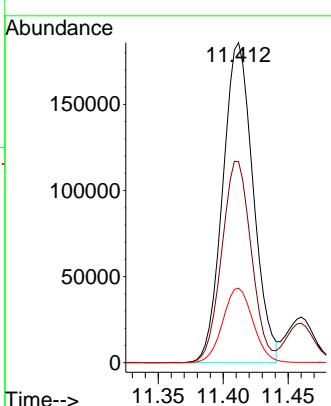 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#78

1,2,4-Trimethylbenzene


Concen: 10.690 ug/l




RT: 11.460 min Scan# 3163

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

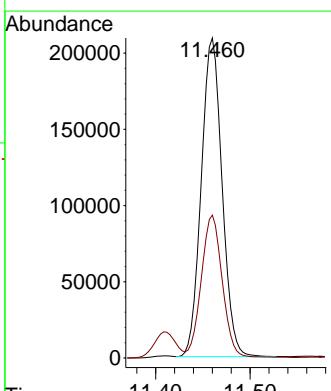 Tgt Ion:105 Resp: 319824
 Ion Ratio Lower Upper
 105 100
 120 45.1 22.7 68.0

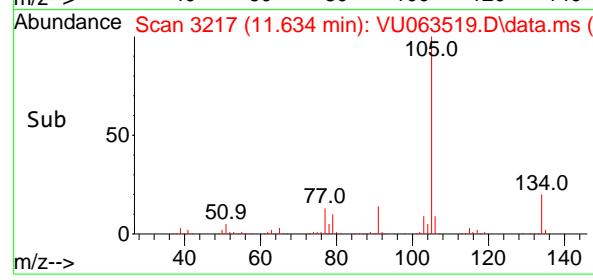


#79

sec-Butylbenzene

Concen: 10.493 ug/l

RT: 11.634 min Scan# 3

Instrument:

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#80

Nitrobenzene

Concen: 48.829 ug/l

RT: 13.203 min Scan# 3705

Delta R.T. -0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25


Tgt Ion: 77 Resp: 6990



Ion Ratio Lower Upper

77 100

123 39.6 16.9 59.7

65 17.5 16.5 20.9

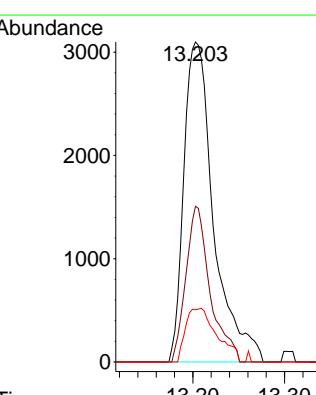



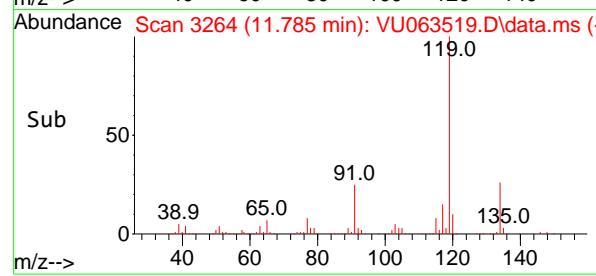



#81
p-Isopropyltoluene
Concen: 10.712 ug/l
RT: 11.785 min Scan# 3264
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

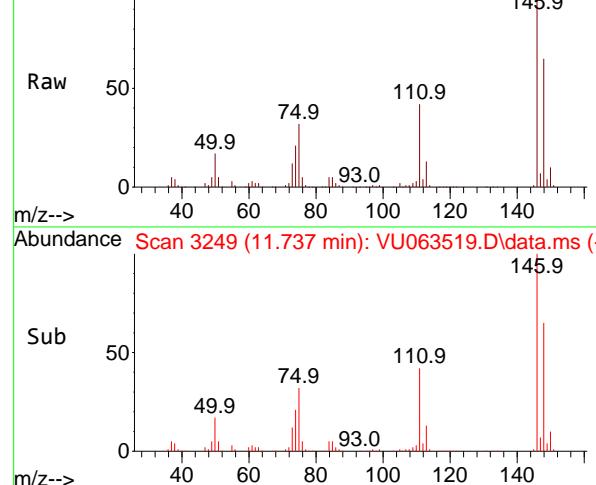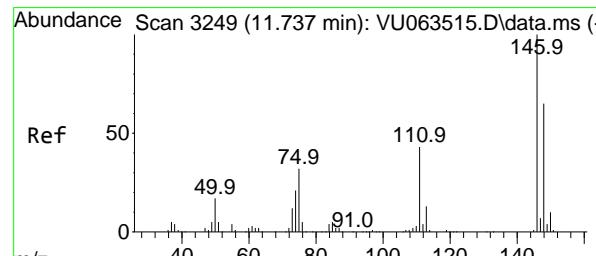

#82
1,3-Dichlorobenzene
Concen: 10.490 ug/l
RT: 11.737 min Scan# 3249
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion:146 Resp: 170997
Ion Ratio Lower Upper
146 100
111 41.8 33.8 50.6
148 64.3 51.5 77.3



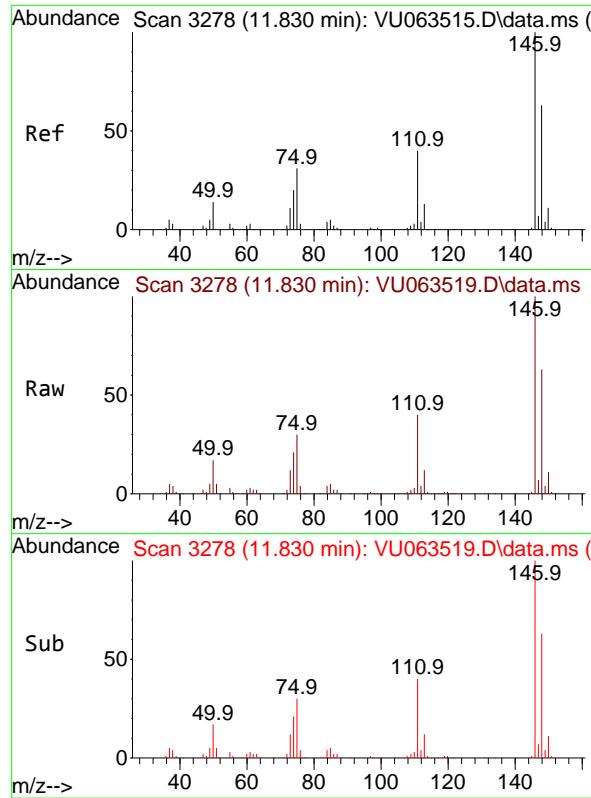

#83

1,4-Dichlorobenzene

Concen: 10.541 ug/l

RT: 11.830 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument :

MSVOA_U

ClientSampleId :

VSTDCCC010

Tgt Ion:146 Resp: 17199

Ion Ratio Lower Upper

146 100



111 40.2 32.0 48.0

148 63.7 50.2 75.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

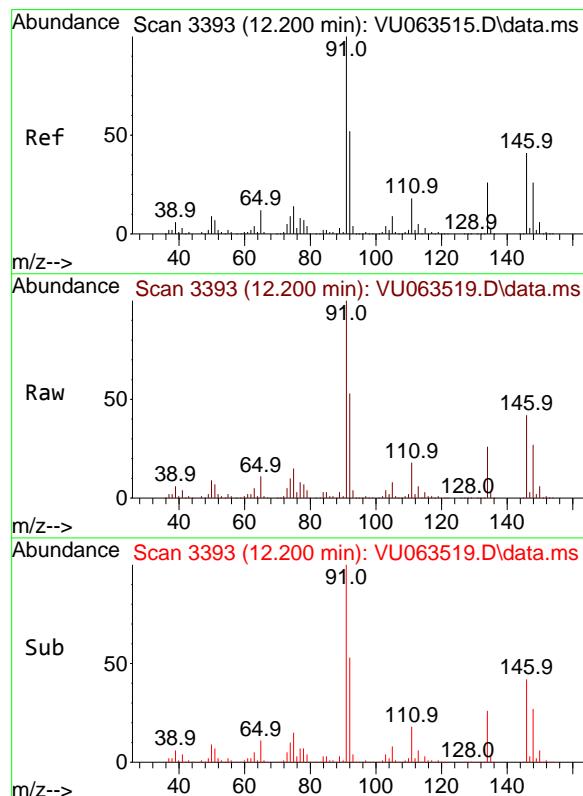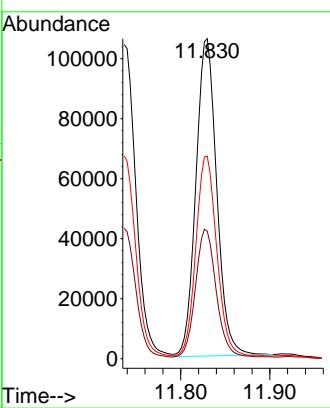

#84

n-Butylbenzene

Concen: 11.026 ug/l

RT: 12.200 min Scan# 3393

Delta R.T. -0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25


Tgt Ion: 91 Resp: 331771




Ion Ratio Lower Upper

91 100

92 52.0 41.5 62.3

134 25.6 20.6 30.8

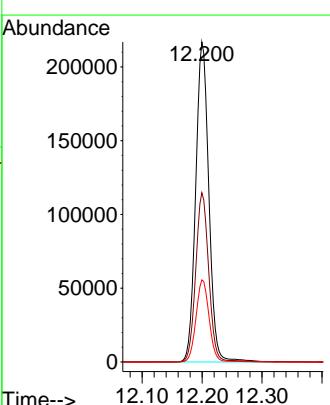



#85

1,2-Dichlorobenzene

Concen: 10.514 ug/l

RT: 12.203 min Scan# 3

Delta R.T. -0.003 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Instrument:

MSVOA_U




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**


Reviewed By :Mahesh Dadoda 07/18/2025


Supervised By :Semsettin Yesilyurt 07/21/2025



#86
1,2-Dibromo-3-Chloropropane
Concen: 10.149 ug/l
RT: 12.987 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion: 75 Resp: 11077
Ion Ratio Lower Upper
75 100
155 78.1 65.8 98.6
157 98.7 81.4 122.2




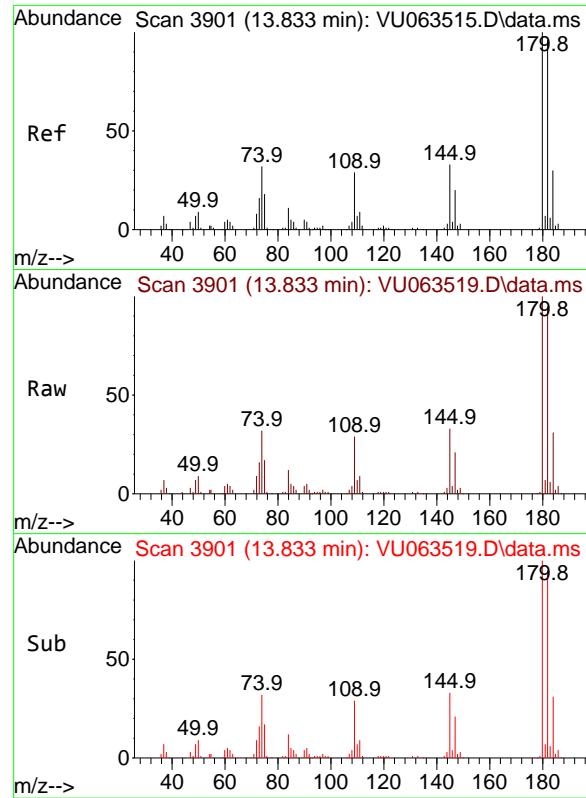


#87
1,2,4-Trichlorobenzene
Concen: 11.013 ug/l
RT: 13.833 min Scan# 3901
Delta R.T. -0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Instrument: MSVOA_U
ClientSampleId: VSTDCCC010


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

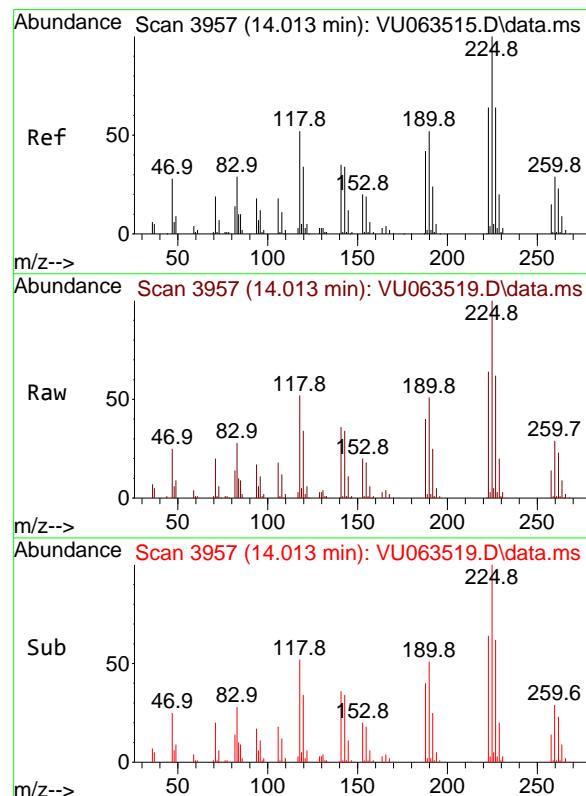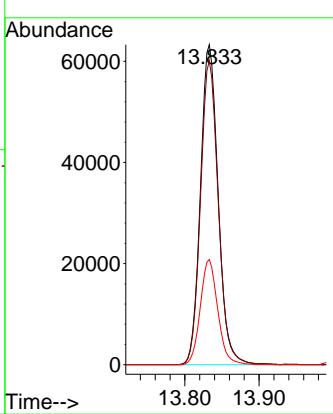

#88
Hexachlorobutadiene
Concen: 10.464 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063519.D
Acq: 17 Jul 2025 09:25

Tgt Ion:225 Resp: 56592
Ion Ratio Lower Upper
225 100
223 63.3 50.8 76.2
227 63.1 51.0 76.6



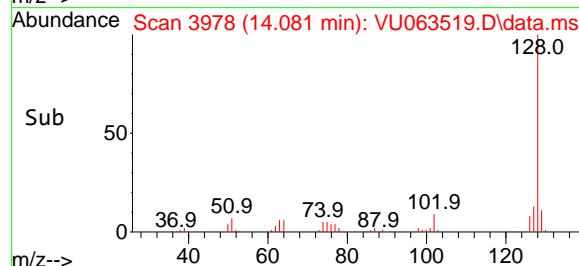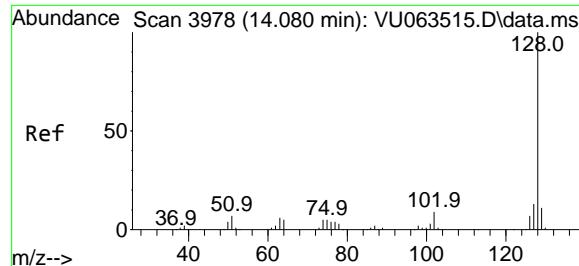

#89

Naphthalene

Concen: 11.071 ug/l





RT: 14.081 min Scan# 3

Instrument : MSVOA_U

Delta R.T. 0.001 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

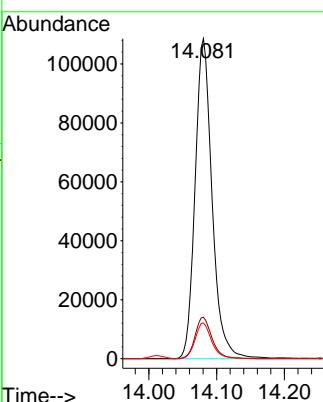**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#90

1,2,3-Trichlorobenzene

Concen: 11.161 ug/l

RT: 14.322 min Scan# 4053


Delta R.T. 0.000 min

Lab File: VU063519.D

Acq: 17 Jul 2025 09:25

Tgt Ion:180 Resp: 98222

	Ion Ratio	Lower	Upper
180	100		
182	95.3	78.0	117.0
145	33.4	27.3	40.9

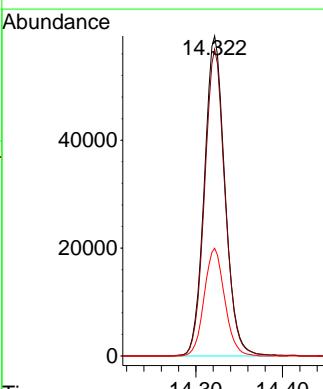

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063519.D
 Acq On : 17 Jul 2025 09:25
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 04:09:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 i	Fluorobenzene	1.000	1.000	0.0	108	0.00
2 T	Dichlorodifluoromethane	0.295	0.284	3.7	103	0.00
3 t	Chloromethane	0.274	0.271	1.1	109	0.00
4 Rt	Vinyl Chloride	0.349	0.339	2.9	103	0.00
5 T	Bromomethane	0.263	0.242	8.0	107	0.00
6 T	Chloroethane	0.211	0.206	2.4	104	0.00
7 T	Trichlorofluoromethane	0.501	0.484	3.4	102	0.00
8	1,1,2-Trichloro-1,2,2-trifl	0.262	0.259	1.1	105	0.00
9 Rt	1,1-Dichloroethene	0.260	0.255	1.9	104	0.00
10 t	Iodomethane	0.314	0.350	-11.5	102	0.00
11 t	Allyl Chloride	0.375	0.371	1.1	105	0.00
12 t	Acrylonitrile	0.065	0.063	3.1	107	0.00
13 T	Acetone	0.052	0.080	-53.8#	172	0.00
14 T	Carbon Disulfide	0.839	0.805	4.1	101	0.00
15 RT	Methylene Chloride	0.306	0.286	6.5	105	0.00
16 RT	trans-1,2-Dichloroethene	0.295	0.282	4.4	102	0.00
17 t	1,1-Dichloroethane	0.546	0.536	1.8	105	0.00
18 T	2-Butanone	0.081	0.100	-23.5	135	0.00
19	Cyclohexane	0.463	0.437	5.6	102	0.00
20	Methylcyclohexane	0.450	0.467	-3.8	103	0.00
21 T	2,2-Dichloropropane	0.465	0.456	1.9	108	0.00
22 RT	cis-1,2-Dichloroethene	0.320	0.312	2.5	105	0.00
23 t	Diethyl Ether	0.198	0.199	-0.5	104	0.00
24 t	tert-Butyl Alcohol	0.024	0.023	4.2	104	0.00
25 t	Methyl tert-Butyl Ether	0.678	0.681	-0.4	106	0.00
26 t	Bromoform	0.134	0.135	-0.7	106	0.00
27 t	Chloroform	0.558	0.543	2.7	107	0.00
28 RT	1,1,1-Trichloroethane	0.473	0.466	1.5	104	0.00
29 T	1,1-Dichloropropene	0.438	0.425	3.0	106	0.00
30 RT	Carbon Tetrachloride	0.381	0.388	-1.8	107	0.00
31 t	Isopropyl Ether	0.825	0.805	2.4	104	0.00
32	Ethyl-t-butyl ether	0.763	0.744	2.5	104	0.00
33	Tert-Amyl methyl ether	0.663	0.661	0.3	107	0.00
34 t	Propionitrile	0.025	0.023	8.0	108	0.00
35 RT	Benzene	1.178	1.188	-0.8	107	0.00
36 RT	1,2-Dichloroethane	0.366	0.368	-0.5	105	0.00
37 RT	Trichloroethene	0.301	0.318	-5.6	106	0.00
38 Rt	1,2-Dichloropropane	0.276	0.308	-11.6	105	0.00
39 t	Methacrylonitrile	0.109	0.101	7.3	107	0.00
40 t	Methyl acrylate	0.159	0.149	6.3	95	0.00
41 t	Tetrahydrofuran	0.057	0.051	10.5	106	0.00
42 t	1-Chlorobutane	0.583	0.580	0.5	106	0.00
43 T	Dibromomethane	0.143	0.144	-0.7	101	0.00
44 T	Bromodichloromethane	0.322	0.324	-0.6	107	0.00
45 T	4-Methyl-2-Pentanone	0.147	0.154	-4.8	109	0.00
46 t	t-1,4-Dichloro-2-butene	0.055	0.052	5.5	90	0.00
47 t	Methyl methacrylate	0.120	0.125	-4.2	106	0.00
48 t	Ethyl methacrylate	0.229	0.249	-8.7	106	0.00
49 Rt	Toluene	0.643	0.653	-1.6	105	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063519.D
 Acq On : 17 Jul 2025 09:25
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 04:09:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
50 T	t-1,3-Dichloropropene	0.253	0.278	-9.9	105	0.00
51 T	cis-1,3-Dichloropropene	0.339	0.359	-5.9	107	0.00
52 RT	1,1,2-Trichloroethane	0.192	0.199	-3.6	106	0.00
53 t	1,3-Dichloropropane	0.332	0.333	-0.3	105	0.00
54 t	2-Hexanone	0.098	0.118	-20.4	124	0.00
55 t	Dibromochloromethane	0.203	0.229	-12.8	106	0.00
56 T	1,2-Dibromoethane	0.172	0.178	-3.5	107	0.00
57 S	4-Bromofluorobenzene	0.379	0.365	3.7	107	0.00
58 RT	Tetrachloroethene	0.275	0.267	2.9	101	0.00
59 Rt	Chlorobenzene	0.739	0.758	-2.6	106	0.00
60 T	1,1,1,2-Tetrachloroethane	0.238	0.246	-3.4	104	0.00
61 t	Pentachloroethane	0.168	0.181	-7.7	105	0.00
62 t	Hexachloroethane	0.166	0.183	-10.2	103	0.00
63 Rt	Ethyl Benzene	1.271	1.290	-1.5	106	0.00
64 RT	m/p-Xylenes	0.494	0.510	-3.2	106	0.00
65 RT	o-Xylene	0.475	0.499	-5.1	107	0.00
66 RT	Styrene	0.757	0.817	-7.9	107	0.00
67 t	Bromoform	0.104	0.116	-11.5	106	0.00
68 S	1,2-Dichlorobenzene-d4	0.350	0.339	3.1	102	0.00
69 T	Isopropylbenzene	1.148	1.207	-5.1	106	0.00
70 T	1,1,2,2-Tetrachloroethane	0.234	0.245	-4.7	109	0.00
71 T	1,2,3-Trichloropropane	0.190	0.195	-2.6	101	0.00
72 t	Bromobenzene	0.296	0.311	-5.1	108	0.00
73 t	n-propylbenzene	0.346	0.365	-5.5	105	0.00
74 t	2-Chlorotoluene	0.305	0.319	-4.6	107	0.00
75 t	1,3,5-Trimethylbenzene	1.097	1.162	-5.9	106	0.00
76 t	4-Chlorotoluene	0.310	0.333	-7.4	109	0.00
77 t	tert-Butylbenzene	1.048	1.102	-5.2	106	0.00
78 t	1,2,4-Trimethylbenzene	1.088	1.163	-6.9	106	0.00
79 t	sec-Butylbenzene	1.413	1.483	-5.0	105	0.00
80	Nitrobenzene	0.004	0.005	-25.0	102	0.00
81 t	p-Isopropyltoluene	1.180	1.264	-7.1	107	0.00
82 t	1,3-Dichlorobenzene	0.593	0.622	-4.9	107	0.00
83 Rt	1,4-Dichlorobenzene	0.593	0.625	-5.4	106	0.00
84 t	n-Butylbenzene	1.094	1.206	-10.2	107	0.00
85 Rt	1,2-Dichlorobenzene	0.557	0.586	-5.2	106	0.00
86 t	1,2-Dibromo-3-Chloropropane	0.033	0.040	-21.2	109	0.00
87 Rt	1,2,4-Trichlorobenzene	0.346	0.381	-10.1	107	0.00
88 t	Hexachlorobutadiene	0.197	0.206	-4.6	105	0.00
89 t	Naphthalene	0.621	0.687	-10.6	109	0.00
90 t	1,2,3-Trichlorobenzene	0.320	0.357	-11.6	109	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063519.D
 Acq On : 17 Jul 2025 09:25
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 04:09:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 i	Fluorobenzene	1.000	1.000	0.0	108	0.00
2 T	Dichlorodifluoromethane	10.000	9.643	3.6	103	0.00
3 t	Chloromethane	10.000	9.902	1.0	109	0.00
4 Rt	Vinyl Chloride	10.000	9.718	2.8	103	0.00
5 T	Bromomethane	10.000	9.188	8.1	107	0.00
6 T	Chloroethane	10.000	9.774	2.3	104	0.00
7 T	Trichlorofluoromethane	10.000	9.648	3.5	102	0.00
8	1,1,2-Trichloro-1,2,2-trifl	10.000	9.874	1.3	105	0.00
9 Rt	1,1-Dichloroethene	10.000	9.834	1.7	104	0.00
10 t	Iodomethane	10.000	9.096	9.0	102	0.00
11 t	Allyl Chloride	10.000	9.904	1.0	105	0.00
12 t	Acrylonitrile	20.000	19.426	2.9	107	0.00
13 T	Acetone	50.000	76.573	-53.1#	172	0.00
14 T	Carbon Disulfide	10.000	9.597	4.0	101	0.00
15 RT	Methylene Chloride	10.000	9.347	6.5	105	0.00
16 RT	trans-1,2-Dichloroethene	10.000	9.547	4.5	102	0.00
17 t	1,1-Dichloroethane	10.000	9.813	1.9	105	0.00
18 T	2-Butanone	50.000	61.835	-23.7	135	0.00
19	Cyclohexane	10.000	9.447	5.5	102	0.00
20	Methylcyclohexane	10.000	10.376	-3.8	103	0.00
21 T	2,2-Dichloropropane	10.000	9.790	2.1	108	0.00
22 RT	cis-1,2-Dichloroethene	10.000	9.751	2.5	105	0.00
23 t	Diethyl Ether	10.000	10.062	-0.6	104	0.00
24 t	tert-Butyl Alcohol	100.000	96.429	3.6	104	0.00
25 t	Methyl tert-Butyl Ether	10.000	10.052	-0.5	106	0.00
26 t	Bromochloromethane	10.000	10.094	-0.9	106	0.00
27 t	Chloroform	10.000	9.734	2.7	107	0.00
28 RT	1,1,1-Trichloroethane	10.000	9.841	1.6	104	0.00
29 T	1,1-Dichloropropene	10.000	9.703	3.0	106	0.00
30 RT	Carbon Tetrachloride	10.000	10.193	-1.9	107	0.00
31 t	Isopropyl Ether	10.000	9.757	2.4	104	0.00
32	Ethyl-t-butyl ether	10.000	9.745	2.6	104	0.00
33	Tert-Amyl methyl ether	10.000	9.982	0.2	107	0.00
34 t	Propionitrile	50.000	47.084	5.8	108	0.00
35 RT	Benzene	10.000	10.088	-0.9	107	0.00
36 RT	1,2-Dichloroethane	10.000	10.057	-0.6	105	0.00
37 RT	Trichloroethene	10.000	10.590	-5.9	106	0.00
38 Rt	1,2-Dichloropropane	10.000	11.175	-11.8	105	0.00
39 t	Methacrylonitrile	10.000	9.213	7.9	107	0.00
40 t	Methyl acrylate	10.000	9.339	6.6	95	0.00
41 t	Tetrahydrofuran	20.000	17.936	10.3	106	0.00
42 t	1-Chlorobutane	10.000	9.953	0.5	106	0.00
43 T	Dibromomethane	10.000	10.067	-0.7	101	0.00
44 T	Bromodichloromethane	10.000	10.053	-0.5	107	0.00
45 T	4-Methyl-2-Pentanone	50.000	52.266	-4.5	109	0.00
46 t	t-1,4-Dichloro-2-butene	20.000	18.890	5.5	90	0.00
47 t	Methyl methacrylate	20.000	20.900	-4.5	106	0.00
48 t	Ethyl methacrylate	10.000	10.861	-8.6	106	0.00
49 Rt	Toluene	10.000	10.158	-1.6	105	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063519.D
 Acq On : 17 Jul 2025 09:25
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 04:09:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
50 T	t-1,3-Dichloropropene	10.000	11.010	-10.1	105	0.00
51 T	cis-1,3-Dichloropropene	10.000	10.590	-5.9	107	0.00
52 RT	1,1,2-Trichloroethane	10.000	10.365	-3.7	106	0.00
53 t	1,3-Dichloropropane	10.000	10.044	-0.4	105	0.00
54 t	2-Hexanone	50.000	60.570	-21.1	124	0.00
55 t	Dibromochloromethane	10.000	11.250	-12.5	106	0.00
56 T	1,2-Dibromoethane	10.000	10.326	-3.3	107	0.00
57 S	4-Bromofluorobenzene	1.000	0.965	3.5	107	0.00
58 RT	Tetrachloroethene	10.000	9.712	2.9	101	0.00
59 Rt	Chlorobenzene	10.000	10.255	-2.6	106	0.00
60 T	1,1,1,2-Tetrachloroethane	10.000	10.370	-3.7	104	0.00
61 t	Pentachloroethane	10.000	10.774	-7.7	105	0.00
62 t	Hexachloroethane	10.000	11.016	-10.2	103	0.00
63 Rt	Ethyl Benzene	10.000	10.146	-1.5	106	0.00
64 RT	m/p-Xylenes	20.000	20.632	-3.2	106	0.00
65 RT	o-Xylene	10.000	10.509	-5.1	107	0.00
66 RT	Styrene	10.000	10.792	-7.9	107	0.00
67 t	Bromoform	10.000	11.101	-11.0	106	0.00
68 S	1,2-Dichlorobenzene-d4	1.000	0.968	3.2	102	0.00
69 T	Isopropylbenzene	10.000	10.511	-5.1	106	0.00
70 T	1,1,2,2-Tetrachloroethane	10.000	10.472	-4.7	109	0.00
71 T	1,2,3-Trichloropropane	10.000	10.239	-2.4	101	0.00
72 t	Bromobenzene	10.000	10.490	-4.9	108	0.00
73 t	n-propylbenzene	10.000	10.559	-5.6	105	0.00
74 t	2-Chlorotoluene	10.000	10.457	-4.6	107	0.00
75 t	1,3,5-Trimethylbenzene	10.000	10.596	-6.0	106	0.00
76 t	4-Chlorotoluene	10.000	10.731	-7.3	109	0.00
77 t	tert-Butylbenzene	10.000	10.518	-5.2	106	0.00
78 t	1,2,4-Trimethylbenzene	10.000	10.690	-6.9	106	0.00
79 t	sec-Butylbenzene	10.000	10.493	-4.9	105	0.00
80	Nitrobenzene	50.000	48.829	2.3	102	0.00
81 t	p-Isopropyltoluene	10.000	10.712	-7.1	107	0.00
82 t	1,3-Dichlorobenzene	10.000	10.490	-4.9	107	0.00
83 Rt	1,4-Dichlorobenzene	10.000	10.541	-5.4	106	0.00
84 t	n-Butylbenzene	10.000	11.026	-10.3	107	0.00
85 Rt	1,2-Dichlorobenzene	10.000	10.514	-5.1	106	0.00
86 t	1,2-Dibromo-3-Chloropropane	10.000	10.149	-1.5	109	0.00
87 Rt	1,2,4-Trichlorobenzene	10.000	11.013	-10.1	107	0.00
88 t	Hexachlorobutadiene	10.000	10.464	-4.6	105	0.00
89 t	Naphthalene	10.000	11.071	-10.7	109	0.00
90 t	1,2,3-Trichlorobenzene	10.000	11.161	-11.6	109	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date/Time:	07/18/2025 09:11
Lab File ID:	VU063532.D	Init. Calib. Date(s):	07/16/2025 07/16/2025
Heated Purge: (Y/N)	N	Init. Calib. Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

COMPOUND	RRF	RRF010	MIN RRF	%D	MAX%D
Dichlorodifluoromethane	0.295	0.285		-3.39	30
Chloromethane	0.274	0.271		-1.1	30
Vinyl Chloride	0.349	0.339		-2.87	30
Bromomethane	0.263	0.257		-2.28	30
Chloroethane	0.211	0.211		0	30
Tetrahydrofuran	0.057	0.054		-5.26	30
Trichlorofluoromethane	0.501	0.508		1.4	30
1,1,2-Trichloro-1,2,2-trifluoroethane	0.262	0.269		2.67	30
tert-Butyl Alcohol	0.024	0.024		0	30
Diethyl Ether	0.198	0.207		4.55	30
1,1-Dichloroethene	0.260	0.260		0	30
Acrylonitrile	0.065	0.066		1.54	30
Acetone	0.052	0.090		73.08	30
Carbon Disulfide	0.839	0.746		-11.09	30
Methyl tert-Butyl Ether	0.678	0.701		3.39	30
Methyl acrylate	0.160	0.155		-3.13	30
Methylene Chloride	0.306	0.304		-0.65	30
trans-1,2-Dichloroethene	0.295	0.292		-1.02	30
1,1-Dichloroethane	0.546	0.553		1.28	30
Cyclohexane	0.463	0.463		0	30
2-Butanone	0.081	0.108		33.33	30
Carbon Tetrachloride	0.381	0.391		2.63	30
2,2-Dichloropropane	0.465	0.465		0	30
cis-1,2-Dichloroethene	0.320	0.322		0.63	30
Bromochloromethane	0.134	0.137		2.24	30
Chloroform	0.558	0.577		3.4	30
1,1,1-Trichloroethane	0.473	0.486		2.75	30
Methylcyclohexane	0.450	0.407		-9.56	30
1,1-Dichloropropene	0.438	0.442		0.91	30
Propionitrile	0.025	0.024		-4	30
Benzene	1.178	1.246		5.77	30
1,2-Dichloroethane	0.366	0.390		6.56	30
Trichloroethene	0.301	0.269		-10.63	30
1,2-Dichloropropane	0.276	0.267		-3.26	30
1-Chlorobutane	0.583	0.602		3.26	30
Dibromomethane	0.143	0.142		-0.7	30
Bromodichloromethane	0.322	0.316		-1.86	30
4-Methyl-2-Pentanone	0.147	0.154		4.76	30

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date/Time:	07/18/2025 09:11
Lab File ID:	VU063532.D	Init. Calib. Date(s):	07/16/2025 07/16/2025
Heated Purge: (Y/N)	N	Init. Calib. Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

COMPOUND	RRF	RRF010	MIN RRF	%D	MAX%D
Toluene	0.643	0.658		2.33	30
t-1,3-Dichloropropene	0.253	0.260		2.77	30
cis-1,3-Dichloropropene	0.339	0.343		1.18	30
1,1,2-Trichloroethane	0.192	0.199		3.65	30
1,3-Dichloropropane	0.332	0.343		3.31	30
2-Hexanone	0.098	0.120		22.45	30
Dibromochloromethane	0.203	0.211		3.94	30
1,2-Dibromoethane	0.172	0.176		2.33	30
Tetrachloroethene	0.275	0.263		-4.36	30
Chlorobenzene	0.739	0.757		2.44	30
1,1,1,2-Tetrachloroethane	0.238	0.239		0.42	30
Hexachloroethane	0.166	0.176		6.02	30
Ethyl Benzene	1.271	1.307		2.83	30
m/p-Xylenes	0.494	0.516		4.45	30
o-Xylene	0.475	0.505		6.32	30
Styrene	0.757	0.823		8.72	30
Bromoform	0.104	0.103		-0.96	30
Isopropylbenzene	1.148	1.225		6.71	30
1,1,2,2-Tetrachloroethane	0.234	0.249		6.41	30
1,2,3-Trichloropropane	0.190	0.194		2.11	30
Bromobenzene	0.296	0.303		2.37	30
n-propylbenzene	0.346	0.377		8.96	30
2-Chlorotoluene	0.305	0.322		5.57	30
1,3,5-Trimethylbenzene	1.097	1.189		8.39	30
4-Chlorotoluene	0.310	0.337		8.71	30
tert-Butylbenzene	1.048	1.124		7.25	30
1,2,4-Trimethylbenzene	1.088	1.184		8.82	30
sec-Butylbenzene	1.413	1.542		9.13	30
p-Isopropyltoluene	1.180	1.299		10.09	30
1,3-Dichlorobenzene	0.593	0.633		6.74	30
1,4-Dichlorobenzene	0.593	0.639		7.76	30
n-Butylbenzene	1.094	1.250		14.26	30
1,2-Dichlorobenzene	0.557	0.605		8.62	30
1,2-Dibromo-3-Chloropropane	0.033	0.037		12.12	30
1,2,4-Trichlorobenzene	0.346	0.373		7.8	30
Hexachlorobutadiene	0.197	0.204		3.55	30
Naphthalene	0.621	0.682		9.82	30
1,2,3-Trichlorobenzene	0.320	0.344		7.5	30

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	Alliance	Contract:	ALLI03
Lab Code:	ACE	SDG No.:	Q2552
Instrument ID:	MSVOA_U	Calibration Date/Time:	07/18/2025 09:11
Lab File ID:	VU063532.D	Init. Calib. Date(s):	07/16/2025 07/16/2025
Heated Purge: (Y/N)	N	Init. Calib. Time(s):	09:24 12:11
GC Column:	DB-624UI	ID:	0.18 (mm)

COMPOUND	RRF	RRF010	MIN RRF	%D	MAX%D
Nitrobenzene	0.004	0.004		0	30
1,2-Dichlorobenzene-d4	0.350	0.381		8.86	30
4-Bromofluorobenzene	0.379	0.425		12.14	30
Iodomethane	0.314	0.333		6.05	30
Allyl Chloride	0.375	0.378		0.8	30
t-1,4-Dichloro-2-butene	0.055	0.055		0	30
Methacrylonitrile	0.109	0.102		-6.42	30
Ethyl methacrylate	0.229	0.243		6.11	30
Isopropyl Ether	0.825	0.824		-0.12	30
Methyl methacrylate	0.120	0.123		2.5	30

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063532.D
 Acq On : 18 Jul 2025 09:11
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTDCCC010

Quant Time: Jul 18 23:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	22137	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.624	95	9400	1.121	ug/l	0.00
Spiked Amount 1.000			Recovery	=	112.000%	
68) 1,2-Dichlorobenzene-d4	12.184	152	8443	1.089	ug/l	0.00
Spiked Amount 1.000			Recovery	=	109.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	63177	9.679	ug/l	99
3) Chloromethane	1.518	50	59882	9.869	ug/l	99
4) Vinyl Chloride	1.596	62	75063	9.713	ug/l	99
5) Bromomethane	1.843	94	56979	9.778	ug/l	99
6) Chloroethane	1.924	64	46809	10.032	ug/l	100
7) Trichlorofluoromethane	2.126	101	112398	10.130	ug/l	97
8) 1,1,2-Trichloro-1,2,2-...	2.567	101	59594	10.278	ug/l	99
9) 1,1-Dichloroethene	2.567	96	57624	10.027	ug/l	99
10) Iodomethane	2.708	142	73635	8.700	ug/l	99
11) Allyl Chloride	2.907	41	83570	10.065	ug/l	99
12) Acrylonitrile	3.303	53	29248	20.347	ug/l	98
13) Acetone	2.615	43	99900	86.744	ug/l	99
14) Carbon Disulfide	2.779	76	165060	8.892	ug/l	99
15) Methylene Chloride	3.026	84	67208	9.932	ug/l	99
16) trans-1,2-Dichloroethene	3.335	96	64633	9.902	ug/l	98
17) 1,1-Dichloroethane	3.850	63	122501	10.126	ug/l	99
18) 2-Butanone	4.708	43	119694	67.111	ug/l	100
19) Cyclohexane	5.361	56	102519	10.008	ug/l	99
20) Methylcyclohexane	6.743	83	90134	9.053	ug/l	97
21) 2,2-Dichloropropane	4.644	77	102934	9.992	ug/l	99
22) cis-1,2-Dichloroethene	4.647	96	71370	10.076	ug/l	98
23) Diethyl Ether	2.367	59	45906	10.482	ug/l	99
24) tert-Butyl Alcohol	3.184	59	52532	99.368	ug/l	99
25) Methyl tert-Butyl Ether	3.358	73	155262	10.348	ug/l	100
26) Bromochloromethane	4.952	128	30399	10.279	ug/l	93
27) Chloroform	5.071	83	127644	10.340	ug/l	99
28) 1,1,1-Trichloroethane	5.293	97	107685	10.278	ug/l	100
29) 1,1-Dichloropropene	5.502	75	97809	10.077	ug/l	98
30) Carbon Tetrachloride	5.499	117	86562	10.264	ug/l	96
31) Isopropyl Ether	3.988	45	182312	9.983	ug/l	96
32) Ethyl-t-butyl ether	4.499	59	170978	10.117	ug/l	100
33) Tert-Amyl methyl ether	5.939	73	149469	10.191	ug/l	99
34) Propionitrile	4.772	54	26069	47.974	ug/l	97
35) Benzene	5.753	78	275788	10.575	ug/l	100
36) 1,2-Dichloroethane	5.779	62	86224	10.641	ug/l	99
37) Trichloroethene	6.525	130	59552	8.950	ug/l	96
38) 1,2-Dichloropropane	6.779	63	59104	9.683	ug/l	99
39) Methacrylonitrile	4.968	41	22645	9.375	ug/l	98
40) Methyl acrylate	4.843	55	34325	9.721	ug/l	98
41) Tetrahydrofuran	5.055	42	23866	18.783	ug/l	98
42) 1-Chlorobutane	5.438	56	133351	10.334	ug/l	100
43) Dibromomethane	6.904	93	31338	9.911	ug/l	95
44) Bromodichloromethane	7.094	83	69921	9.806	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063532.D
 Acq On : 18 Jul 2025 09:11
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTDCCC010

Quant Time: Jul 18 23:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.795	43	170568	52.342	ug/l	100
46) t-1,4-Dichloro-2-butene	10.820	75	24249m	19.823	ug/l	
47) Methyl methacrylate	6.962	69	54529	20.535	ug/l	97
48) Ethyl methacrylate	8.332	69	53751	10.607	ug/l	97
49) Toluene	7.959	92	145734	10.235	ug/l	100
50) t-1,3-Dichloropropene	8.203	75	57571	10.291	ug/l	98
51) cis-1,3-Dichloropropene	7.599	75	75837	10.099	ug/l	98
52) 1,1,2-Trichloroethane	8.393	97	43960	10.327	ug/l	98
53) 1,3-Dichloropropane	8.566	76	75937	10.333	ug/l	99
54) 2-Hexanone	8.685	43	132800	61.353	ug/l	97
55) Dibromochloromethane	8.801	129	46798	10.403	ug/l	99
56) 1,2-Dibromoethane	8.917	107	39027	10.244	ug/l	99
58) Tetrachloroethene	8.541	164	58247	9.565	ug/l	97
59) Chlorobenzene	9.438	112	167611	10.249	ug/l	98
60) 1,1,1,2-Tetrachloroethane	9.525	131	52907	10.060	ug/l	98
61) Pentachloroethane	11.418	117	40119	10.796	ug/l	96
62) Hexachloroethane	12.467	117	39030	10.606	ug/l	99
63) Ethyl Benzene	9.560	91	289339	10.281	ug/l	100
64) m/p-Xylenes	9.685	106	228441	20.884	ug/l	98
65) o-Xylene	10.090	106	111689	10.626	ug/l	99
66) Styrene	10.107	104	182214	10.877	ug/l	99
67) Bromoform	10.283	173	22764	9.853	ug/l	99
69) Isopropylbenzene	10.476	105	271215	10.673	ug/l	100
70) 1,1,2,2-Tetrachloroethane	10.772	83	55200	10.657	ug/l	99
71) 1,2,3-Trichloropropane	10.814	75	42901m	10.198	ug/l	
72) Bromobenzene	10.775	156	67162	10.241	ug/l	95
73) n-propylbenzene	10.898	120	83463	10.911	ug/l	99
74) 2-Chlorotoluene	10.978	126	71241	10.538	ug/l	99
75) 1,3,5-Trimethylbenzene	11.078	105	263117	10.839	ug/l	100
76) 4-Chlorotoluene	11.090	126	74500	10.851	ug/l	99
77) tert-Butylbenzene	11.412	119	248774	10.723	ug/l	99
78) 1,2,4-Trimethylbenzene	11.460	105	262116	10.884	ug/l	100
79) sec-Butylbenzene	11.634	105	341350	10.911	ug/l	99
80) Nitrobenzene	13.203	77	4689	42.376	ug/l	97
81) p-Isopropyltoluene	11.785	119	287611	11.013	ug/l	99
82) 1,3-Dichlorobenzene	11.737	146	140019	10.671	ug/l	99
83) 1,4-Dichlorobenzene	11.827	146	141444	10.769	ug/l	98
84) n-Butylbenzene	12.200	91	276678	11.423	ug/l	99
85) 1,2-Dichlorobenzene	12.203	146	133976	10.868	ug/l	99
86) 1,2-Dibromo-3-Chloropr...	12.987	75	8081	9.368	ug/l	97
87) 1,2,4-Trichlorobenzene	13.833	180	82660	10.783	ug/l	100
88) Hexachlorobutadiene	14.013	225	45081	10.355	ug/l	99
89) Naphthalene	14.081	128	150983	10.991	ug/l	100
90) 1,2,3-Trichlorobenzene	14.322	180	76164	10.751	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063532.D
Acq On : 18 Jul 2025 09:11
Operator : MD/SY
Sample : VSTDCCC010
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1


Quant Time: Jul 18 23:43:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

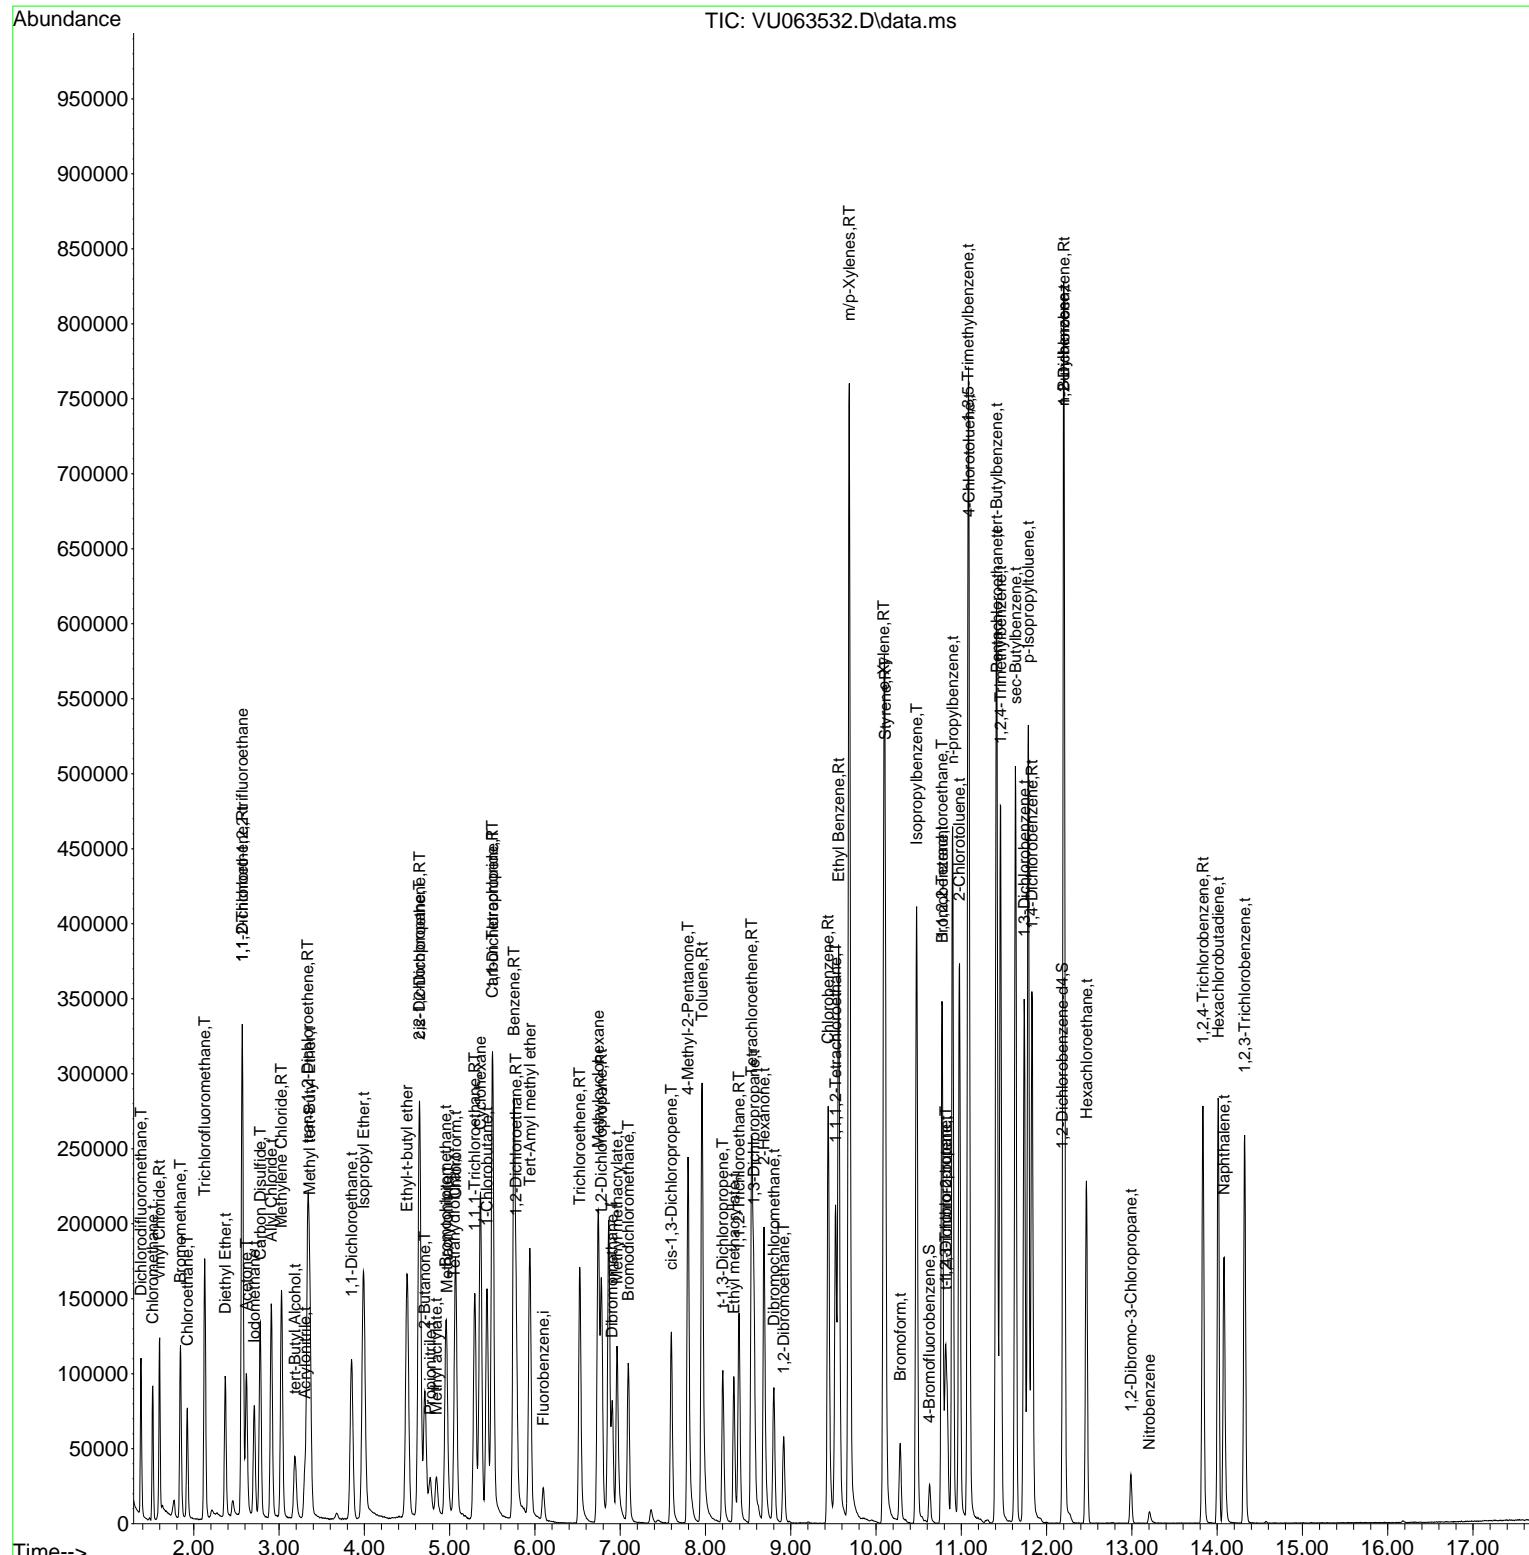



#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 96 Resp: 2213
Ion Ratio Lower Upper
96 100
70 18.9 15.0 22.4
95 8.2 7.4 11.0
97 0.0 0.0 0.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

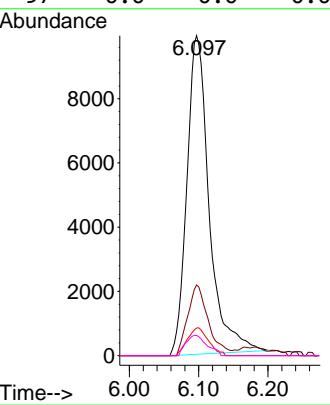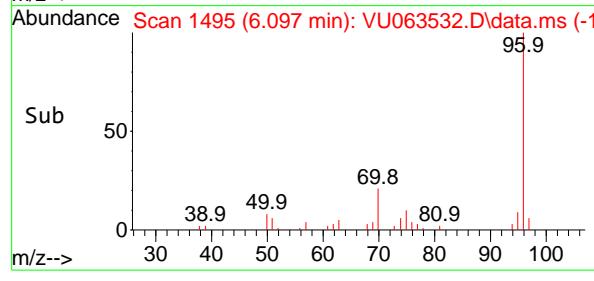


#2
Dichlorodifluoromethane
Concen: 9.679 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11





Tgt Ion: 85 Resp: 63177
Ion Ratio Lower Upper
85 100
87 32.2 16.0 47.9

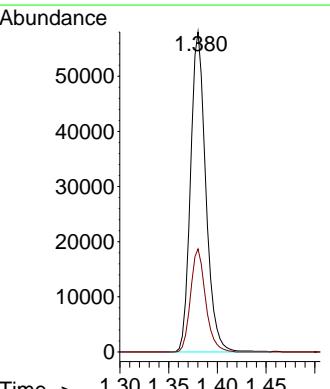




Abundance Scan 71 (1.518 min): VU063532.D\data.ms

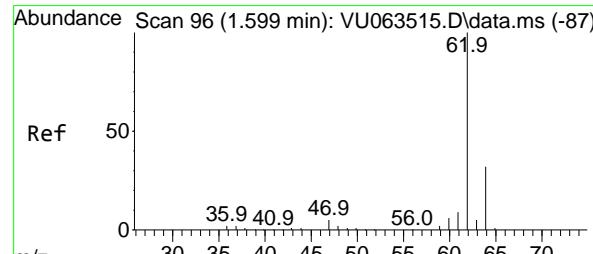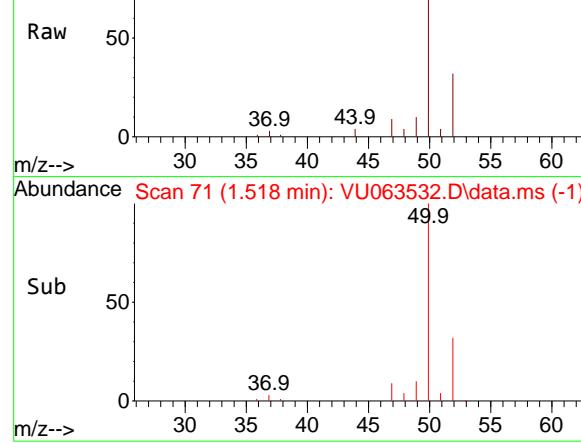

Abundance Scan 95 (1.596 min): VU063532.D\data.ms

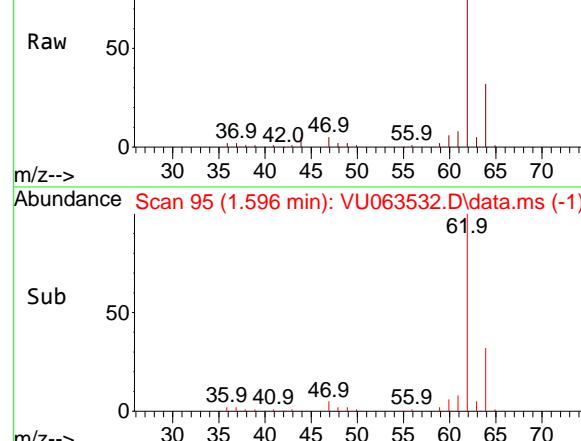

#3

Chloromethane

Concen: 9.869 ug/l

RT: 1.518 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

Tgt Ion: 50 Resp: 5988

Ion Ratio Lower Upper


50 100

52 32.4 26.3 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

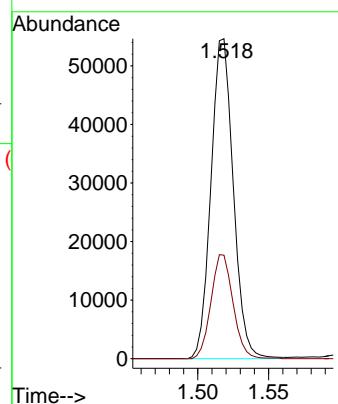

#4

Vinyl Chloride

Concen: 9.713 ug/l

RT: 1.596 min Scan# 95

Delta R.T. -0.003 min

Lab File: VU063532.D


Acq: 18 Jul 2025 09:11


Tgt Ion: 62 Resp: 75063

Ion Ratio Lower Upper

62 100


64 31.7 25.7 38.5

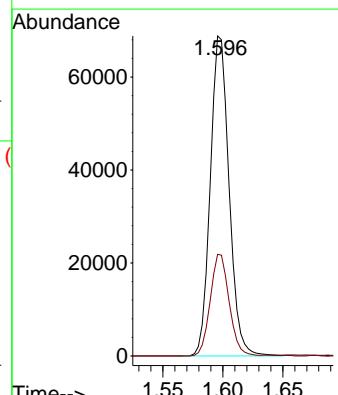

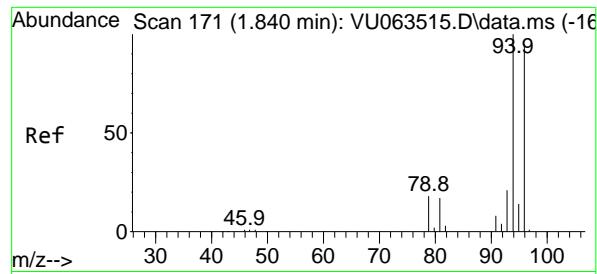

#5
Bromomethane
Concen: 9.778 ug/l
RT: 1.843 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

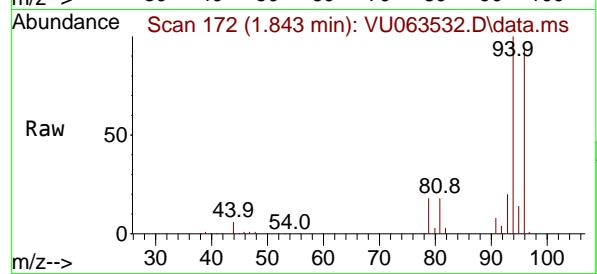


Tgt Ion: 94 Resp: 56975
Ion Ratio Lower Upper
94 100
96 94.2 75.8 113.6

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

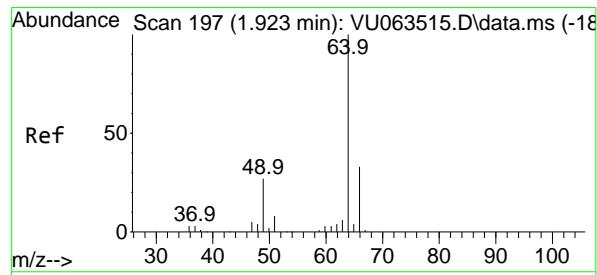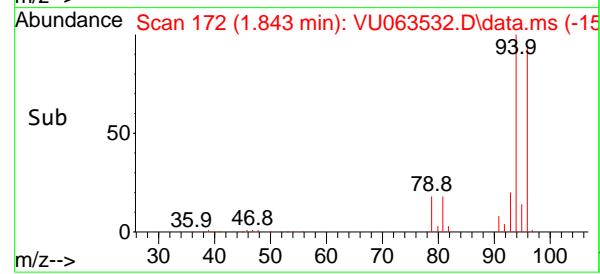


#6
Chloroethane
Concen: 10.032 ug/l
RT: 1.924 min Scan# 197
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

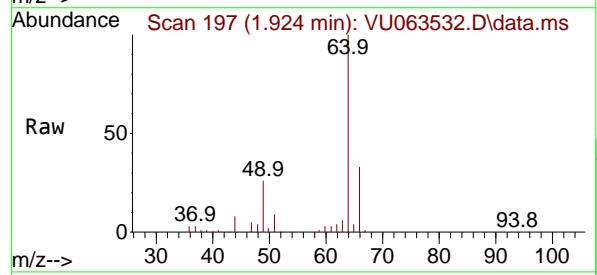


Tgt Ion: 64 Resp: 46809
Ion Ratio Lower Upper
64 100
66 32.6 26.2 39.4

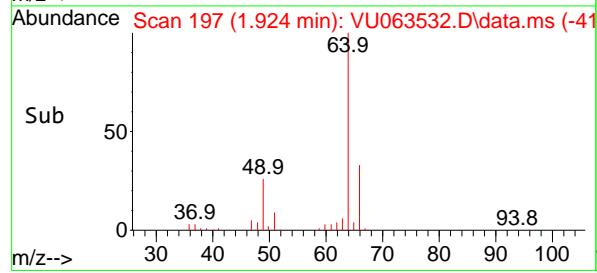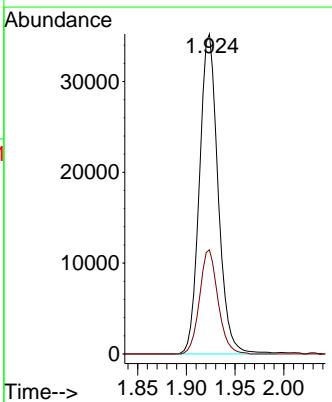



#7
Trichlorofluoromethane
Concen: 10.130 ug/l
RT: 2.126 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion:101 Resp: 112392
Ion Ratio Lower Upper
101 100
103 63.0 52.2 78.4

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

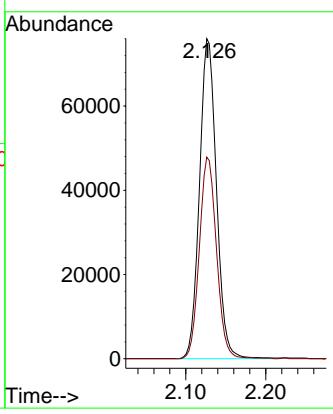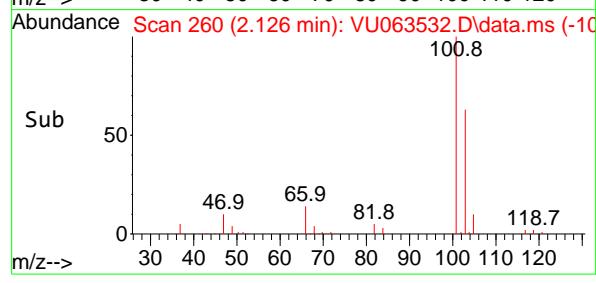


#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 10.278 ug/l
RT: 2.567 min Scan# 397
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Tgt Ion:101 Resp: 59594
Ion Ratio Lower Upper
101 100
85 46.6 37.8 56.6
151 75.3 59.2 88.8

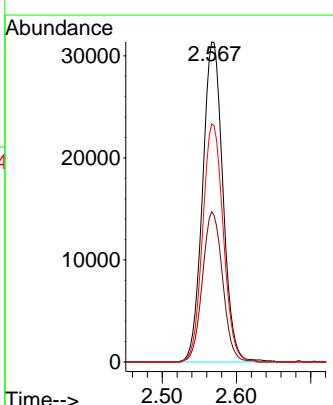



#9
1,1-Dichloroethene
Concen: 10.027 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 96 Resp: 5762
Ion Ratio Lower Upper
96 100
61 170.2 0.0 504.3
98 62.7 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

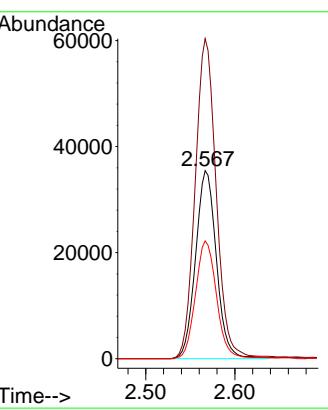


#10
Iodomethane
Concen: 8.700 ug/l
RT: 2.708 min Scan# 441
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Tgt Ion:142 Resp: 73635
Ion Ratio Lower Upper
142 100
127 48.3 37.9 56.9

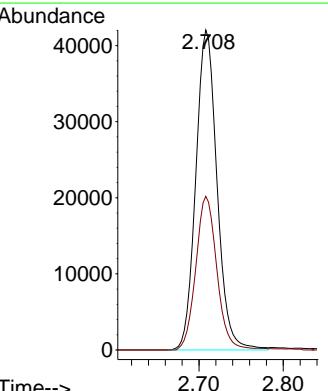



#11
Allyl Chloride
Concen: 10.065 ug/l
RT: 2.907 min Scan# 5
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 41 Resp: 83570
Ion Ratio Lower Upper
41 100
39 77.7 61.5 92.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

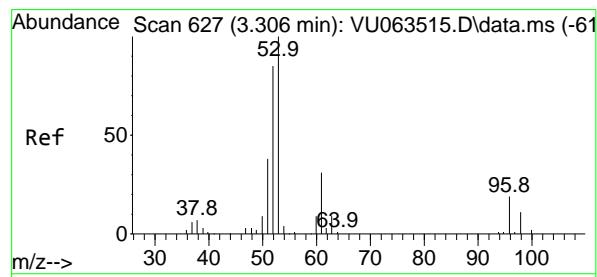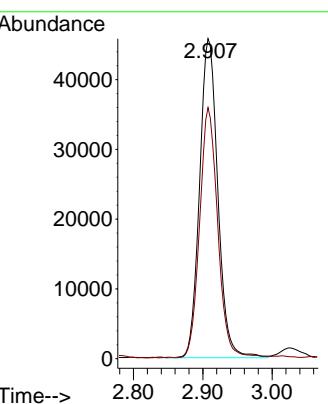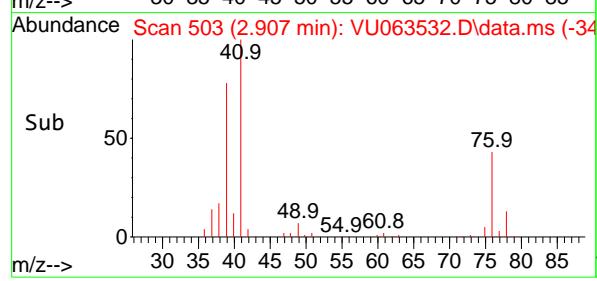


#12
Acrylonitrile
Concen: 20.347 ug/l
RT: 3.303 min Scan# 626
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Tgt Ion: 53 Resp: 29248
Ion Ratio Lower Upper
53 100
52 79.2 64.3 96.5
51 36.5 27.8 41.8

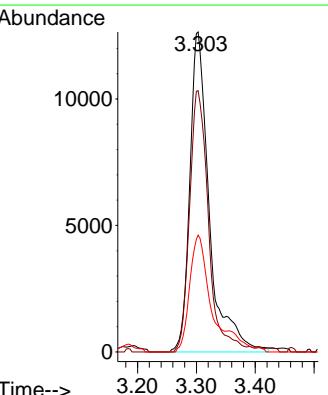



#13
Acetone
Concen: 86.744 ug/l
RT: 2.615 min Scan# 4
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument :
MSVOA_U
ClientSampleId :
VSTDCCC010

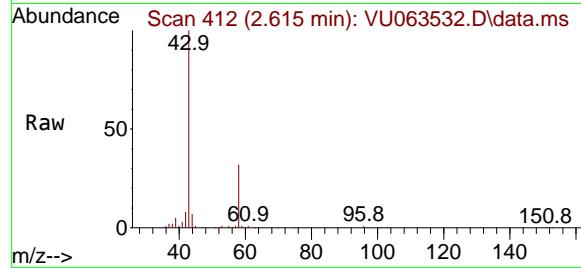


Tgt Ion: 43 Resp: 99900
Ion Ratio Lower Upper
43 100
58 32.5 25.4 38.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025









#14
Carbon Disulfide
Concen: 8.892 ug/l
RT: 2.779 min Scan# 463
Delta R.T. 0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Tgt Ion: 76 Resp: 165060
Ion Ratio Lower Upper
76 100
78 9.2 7.0 10.6





#15

Methylene Chloride

Concen: 9.932 ug/l

RT: 3.026 min Scan# 540

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

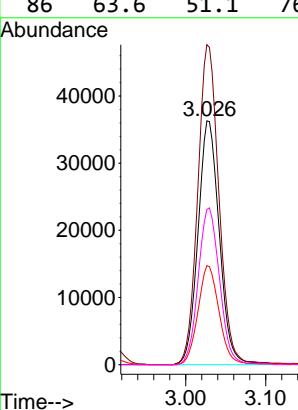 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#16

trans-1,2-Dichloroethene

Concen: 9.902 ug/l


RT: 3.335 min Scan# 636




Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt	Ion	Ion Ratio	Lower	Upper
	96	100		
Tgt	96	100		
	61	149.8	117.2	175.8
	98	64.1	51.4	77.2

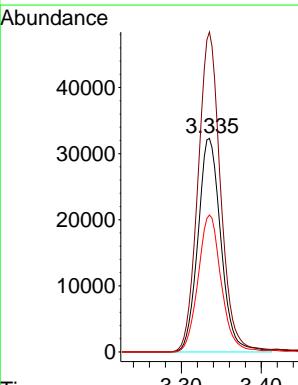






#17

1,1-Dichloroethane
Concen: 10.126 ug/l
RT: 3.850 min Scan# 7
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument :
MSVOA_U
ClientSampleId :
VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

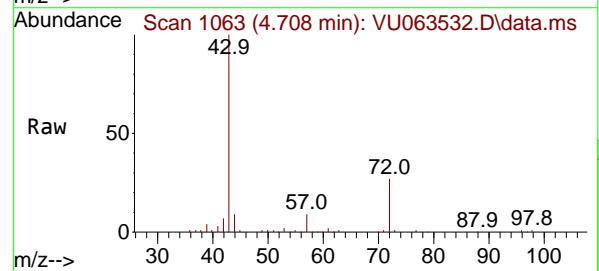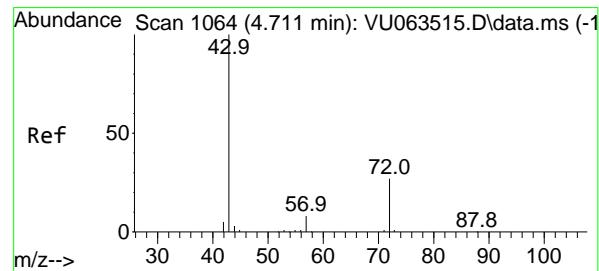


#18

2-Butanone
Concen: 67.111 ug/l
RT: 4.708 min Scan# 1063
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion: 43 Resp: 119694
Ion Ratio Lower Upper
43 100
57 8.1 0.0 16.4

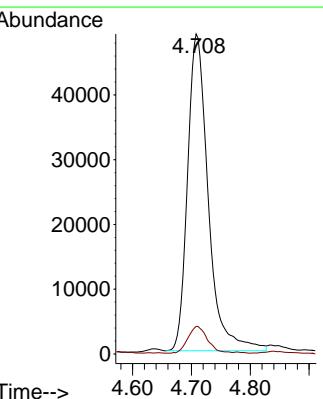



#19

Cyclohexane

Concen: 10.008 ug/l

RT: 5.361 min Scan# 1

Delta R.T. 0.000 min


Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U

ClientSampleId :



VSTDCCC010

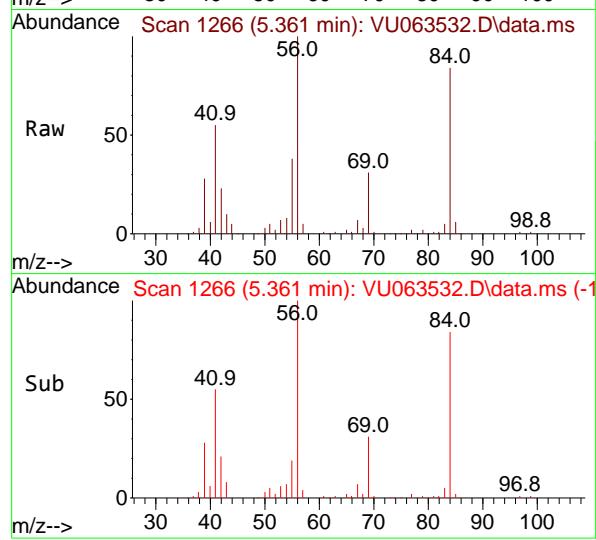

Tgt	Ion:	56	Ion	Ratio:	100	Resp:	102519
		69		33.3	26.6	Lower	
		84		87.7	71.0	Upper	


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

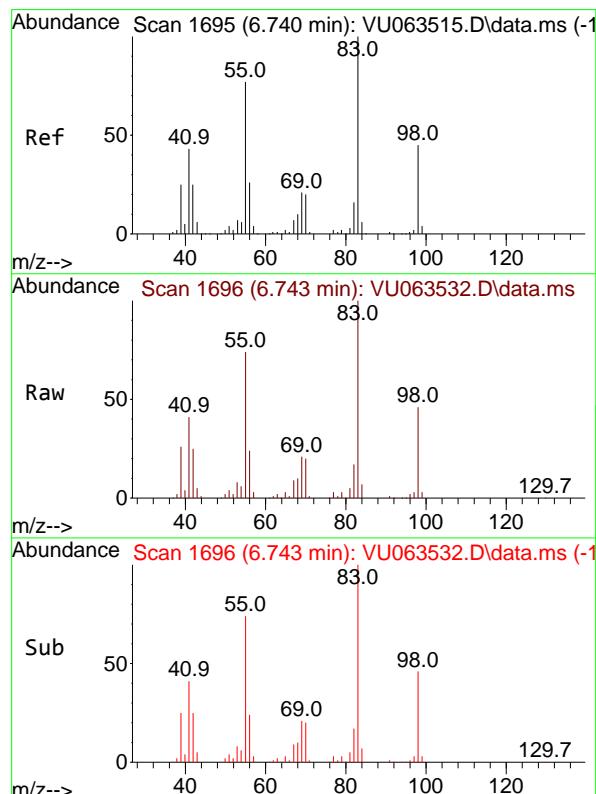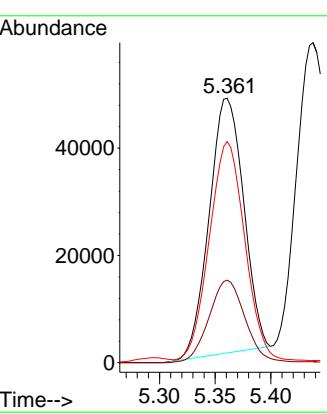

#20
Methylcyclohexane
Concen: 9.053 ug/l
RT: 6.743 min Scan# 1696
Delta R.T. 0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt	Ion:	83	Ion	Ratio:	100	Resp:	90134
		55		73.0	60.6	Lower	
		98		46.8	35.8	Upper	

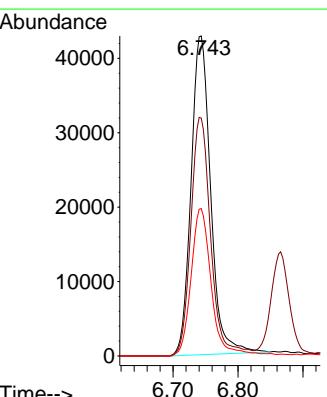

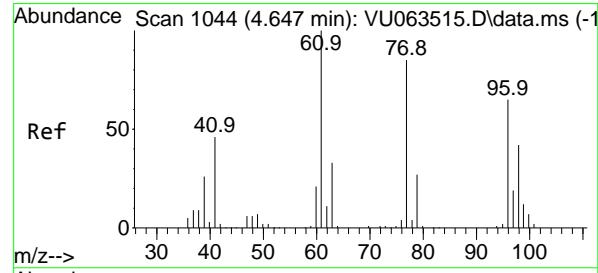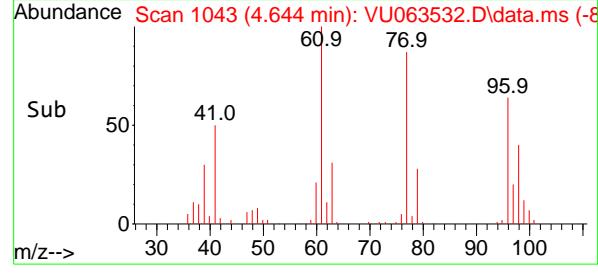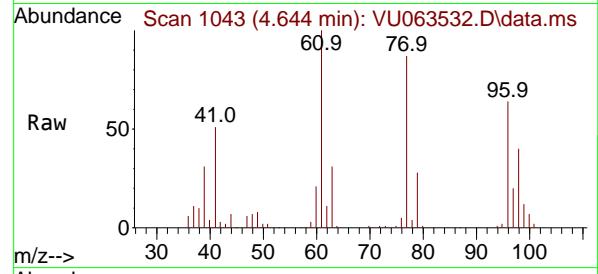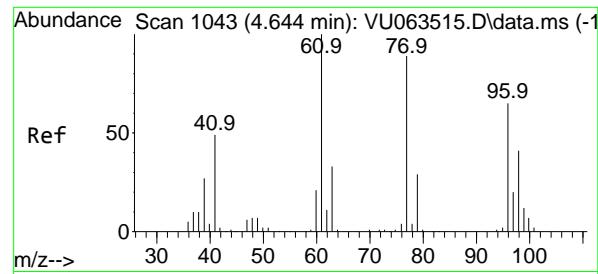

#21

2,2-Dichloropropane

Concen: 9.992 ug/l

RT: 4.644 min Scan# 10293

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

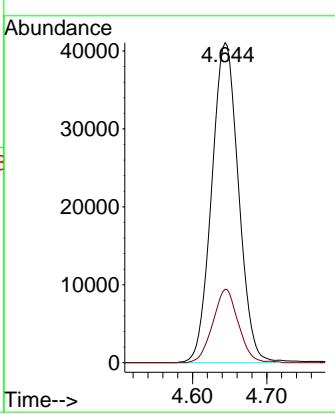 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#22

cis-1,2-Dichloroethene

Concen: 10.076 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Tgt Ion: 96 Resp: 71370




Ion Ratio Lower Upper

96 100

61 157.8 0.0 384.7

98 64.1 32.1 96.3

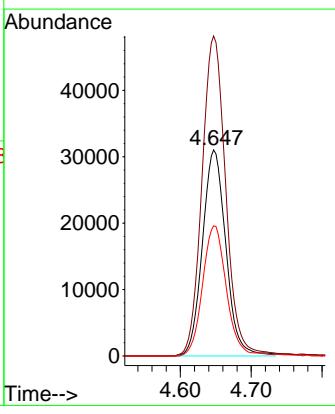

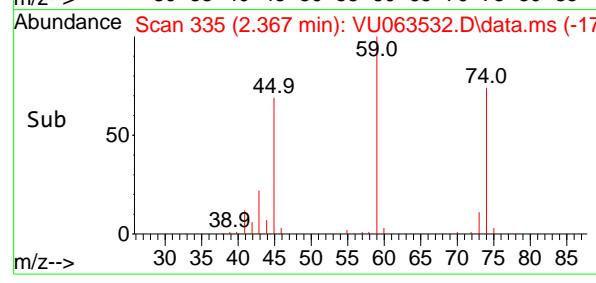

#23

Diethyl Ether

Concen: 10.482 ug/l

RT: 2.367 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U





ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

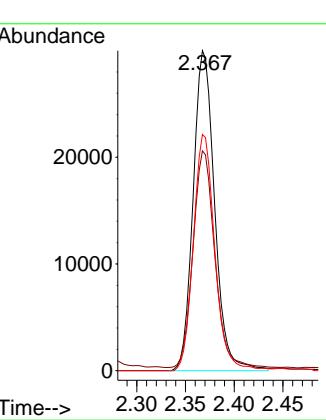

#24

tert-Butyl Alcohol

Concen: 99.368 ug/l


RT: 3.184 min Scan# 589


Delta R.T. -0.006 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt Ion:	59	Resp:	52532
Ion Ratio	100	Lower	Upper
59	100		
57	10.4	8.6	12.8

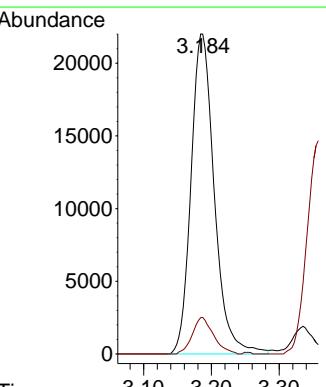

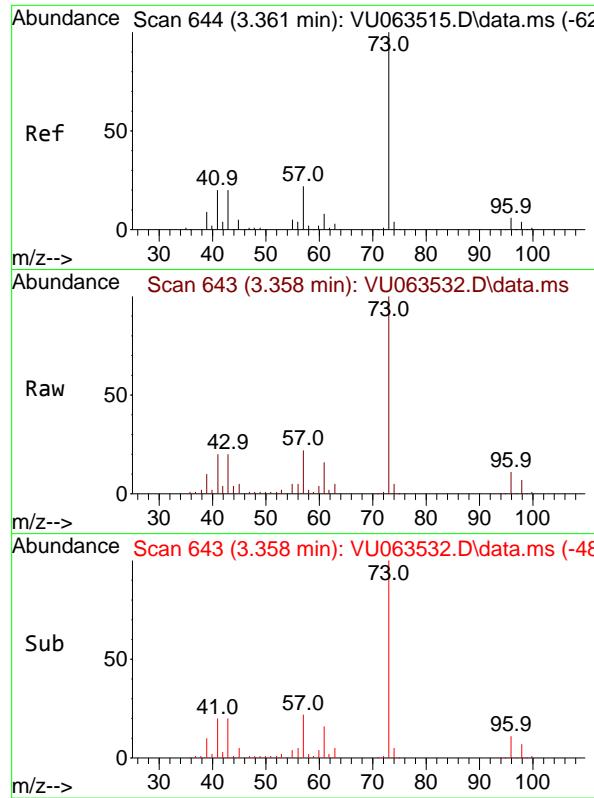



#25

Methyl tert-Butyl Ether
Concen: 10.348 ug/l
RT: 3.358 min Scan# 6
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

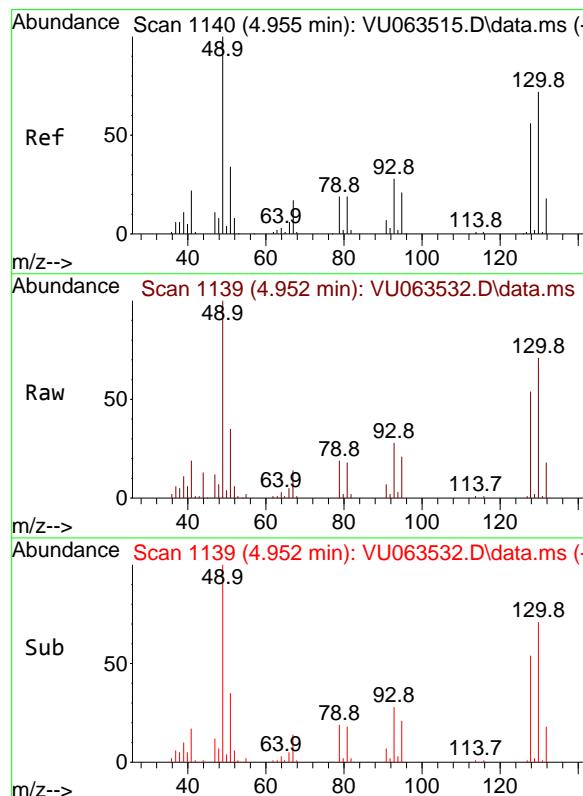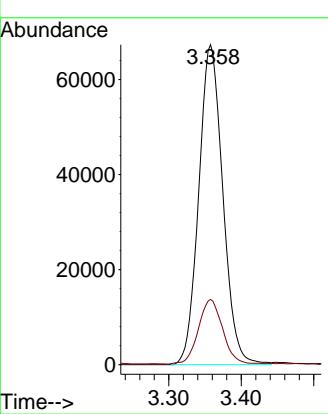


#26

Bromochloromethane
Concen: 10.279 ug/l
RT: 4.952 min Scan# 1139
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11


Tgt Ion:128 Resp: 30399
Ion Ratio Lower Upper
128 100
49 179.2 0.0 340.8
130 133.3 100.5 150.7





#27
 Chloroform
 Concen: 10.340 ug/l
 RT: 5.071 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063532.D
 Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
 ClientSampleId : VSTDCCC010




Tgt Ion: 83 Resp: 127644
 Ion Ratio Lower Upper
 83 100
 85 64.6 0.0 130.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

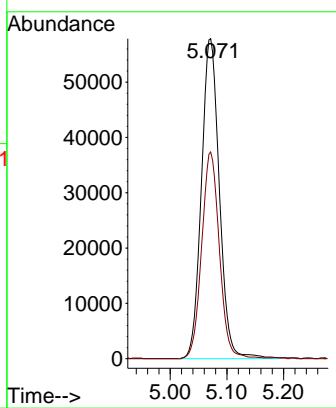


#28
 1,1,1-Trichloroethane
 Concen: 10.278 ug/l
 RT: 5.293 min Scan# 1245
 Delta R.T. -0.003 min
 Lab File: VU063532.D
 Acq: 18 Jul 2025 09:11



Tgt Ion: 97 Resp: 107685
 Ion Ratio Lower Upper
 97 100
 99 63.4 31.8 95.3
 61 47.2 23.3 69.9

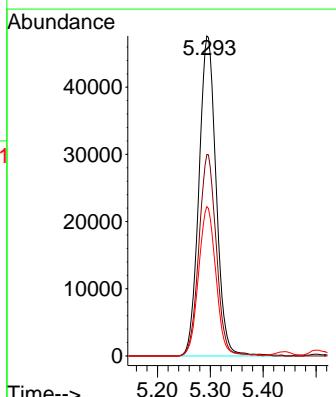



#29

1,1-Dichloropropene

Concen: 10.077 ug/l

RT: 5.502 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063532.D


Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010



Tgt Ion: 75 Resp: 97809

Ion Ratio Lower Upper

75 100




110 34.0 17.8 53.4

77 30.4 24.6 37.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025
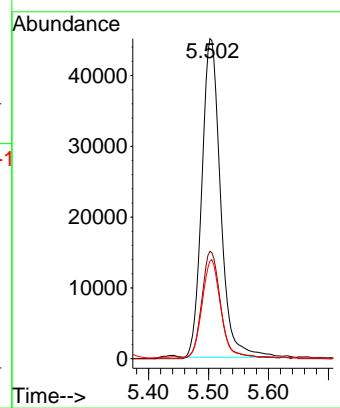
#30
Carbon Tetrachloride
Concen: 10.264 ug/l
RT: 5.499 min Scan# 1309
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Tgt Ion:117 Resp: 86562




Ion Ratio Lower Upper

117 100

119 94.6 79.2 118.8

121 30.7 25.5 38.3

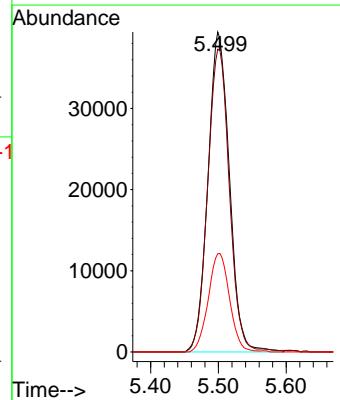

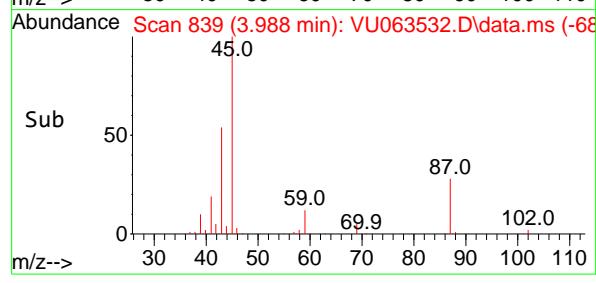

#31

Isopropyl Ether

Concen: 9.983 ug/l

RT: 3.988 min Scan# 8

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11





Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#32

Ethyl-t-butyl ether


Concen: 10.117 ug/l







RT: 4.499 min Scan# 998

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

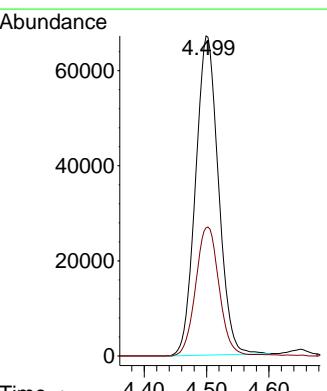 Tgt Ion: 59 Resp: 170978
 Ion Ratio Lower Upper
 59 100
 87 40.7 32.6 49.0

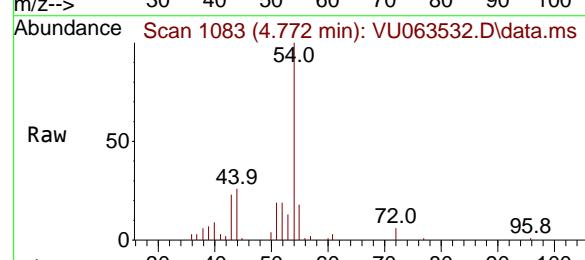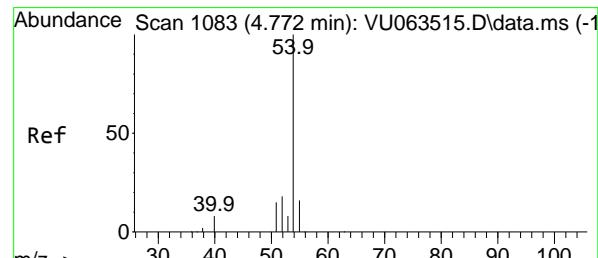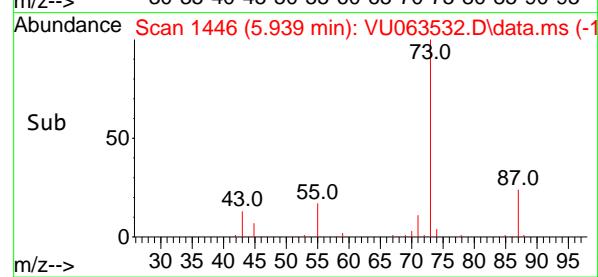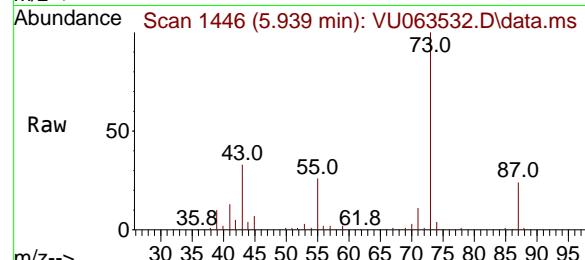


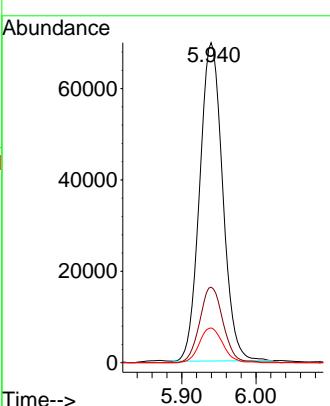
#33

Tert-Amyl methyl ether
Concen: 10.191 ug/l
RT: 5.939 min Scan# 14469
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025




#34

Propionitrile
Concen: 47.974 ug/l
RT: 4.772 min Scan# 1083
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11


Tgt Ion: 54 Resp: 26069
Ion Ratio Lower Upper
54 100
52 19.2 17.0 25.4
55 16.2 13.6 20.4
40 7.4 6.4 9.6

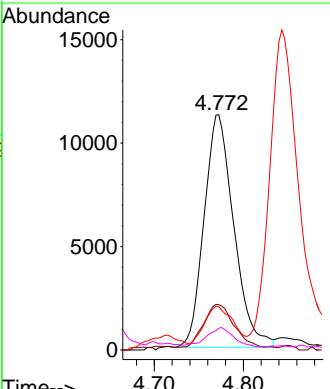



#35
Benzene
Concen: 10.575 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 78 Resp: 275788
Ion Ratio Lower Upper
78 100
77 24.3 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

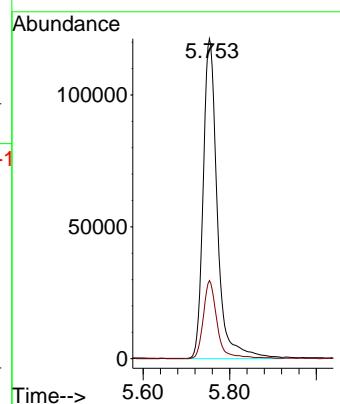


#36
1,2-Dichloroethane
Concen: 10.641 ug/l
RT: 5.779 min Scan# 1396
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Tgt Ion: 62 Resp: 86224
Ion Ratio Lower Upper
62 100
98 8.2 6.4 9.6

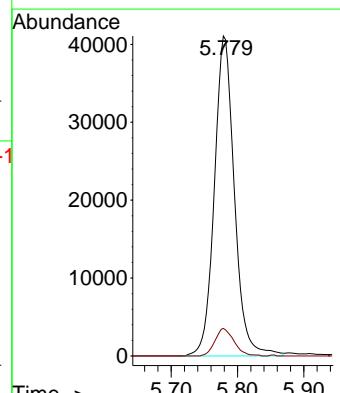



#37
Trichloroethene
Concen: 8.950 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion:130 Resp: 5955
Ion Ratio Lower Upper
130 100
95 104.6 80.3 120.5

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#38
1,2-Dichloropropane
Concen: 9.683 ug/l
RT: 6.779 min Scan# 1707
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Tgt Ion: 63 Resp: 59104
Ion Ratio Lower Upper
63 100
65 31.1 24.6 36.8

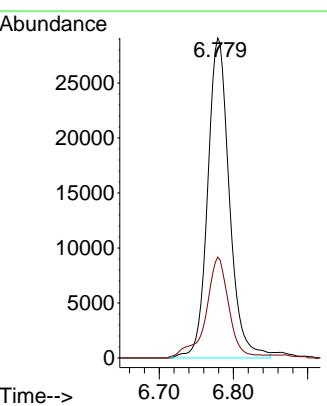



#39

Methacrylonitrile

Concen: 9.375 ug/l

RT: 4.968 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#40

Methyl acrylate

Concen: 9.721 ug/l

RT: 4.843 min Scan# 1105

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt Ion: 55 Resp: 34325




Ion Ratio Lower Upper

55 100

85 17.6 12.8 19.2

58 8.9 7.0 10.4

42 9.4 7.0 10.4

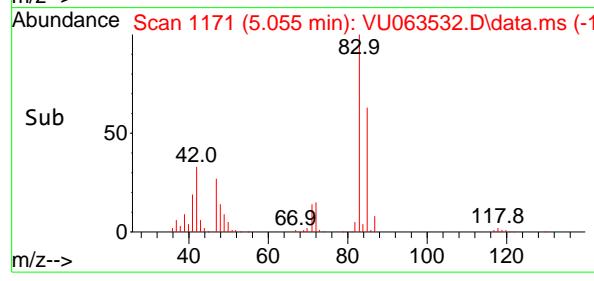

#41

Tetrahydrofuran

Concen: 18.783 ug/l

RT: 5.055 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U





ClientSampleId :

VSTDCCC010

Tgt	Ion:	42	Resp:	23860
Ion	Ratio	Lower	Upper	
42	100			
72	47.3	39.2	58.8	
71	43.7	34.8	52.2	

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

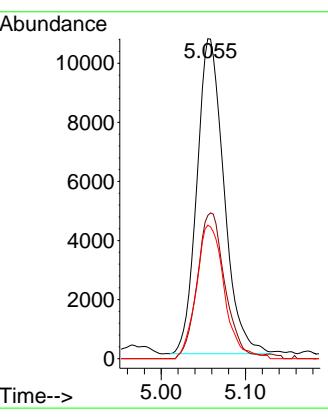

#42

1-Chlorobutane

Concen: 10.334 ug/l


RT: 5.438 min Scan# 1290


Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Tgt	Ion:	56	Resp:	133351
Ion	Ratio	Lower	Upper	
56	100			
41	53.4	26.7	80.0	

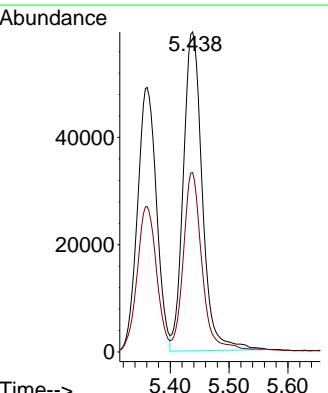



#43
Dibromomethane
Concen: 9.911 ug/l
RT: 6.904 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11




Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 93 Resp: 31333
Ion Ratio Lower Upper
93 100
95 84.9 67.9 101.9
174 83.8 74.6 111.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


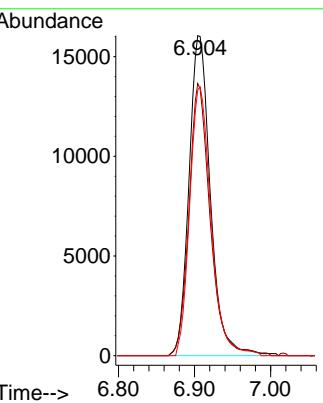



#44
Bromodichloromethane
Concen: 9.806 ug/l
RT: 7.094 min Scan# 1805
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Tgt Ion: 83 Resp: 69921
Ion Ratio Lower Upper
83 100
85 63.9 52.7 79.1
127 9.0 8.1 12.1

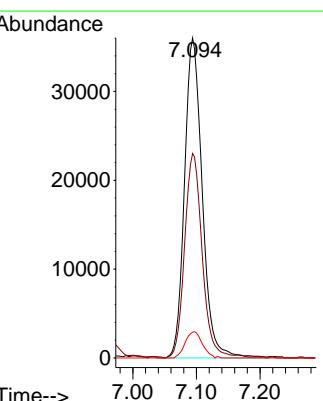



#45

4-Methyl-2-Pentanone

Concen: 52.342 ug/l

RT: 7.795 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U





ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Tgt Ion:	Ion Ratio	Lower	Upper
43	100		
58	40.0	20.0	60.0
85	19.3	15.4	23.0

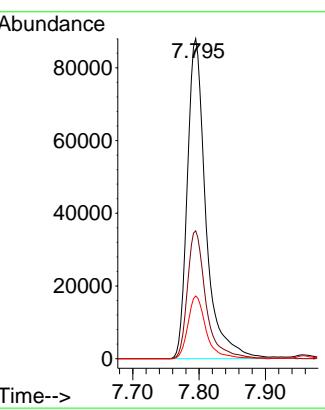

#46

t-1,4-Dichloro-2-butene

Concen: 19.823 ug/l


RT: 10.820 min Scan# 2964







Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt Ion:	Ion Ratio	Lower	Upper
75	100		
53	57.7	48.4	72.6
89	33.1	30.6	45.8
88	25.9	25.3	37.9

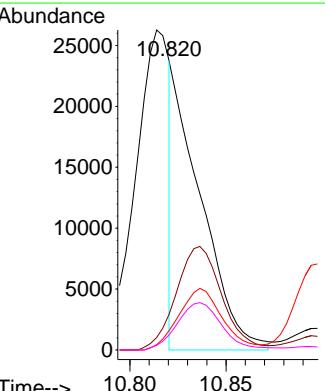



#47

Methyl methacrylate

Concen: 20.535 ug/l

RT: 6.962 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:


MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
69	100			
41	109.1	0.0	224.0	
39	66.6	55.3	82.9	
100	35.2	29.0	43.6	

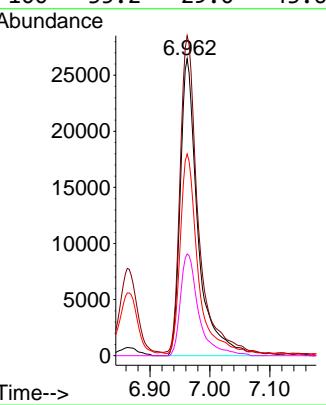

#48

Ethyl methacrylate

Concen: 10.607 ug/l


RT: 8.332 min Scan# 2190


Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11



Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
69	100			
41	64.1	30.8	92.4	

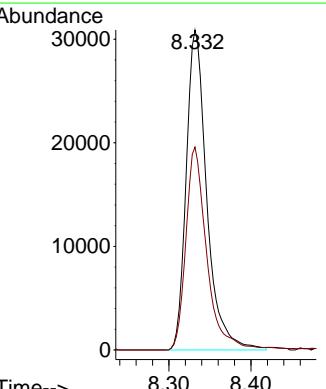



#49
Toluene
Concen: 10.235 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Instrument : MSVOA_U
ClientSampleId : VSTDCCC010




Tgt Ion: 92 Resp: 145734
Ion Ratio Lower Upper
92 100
91 175.5 140.4 210.6

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#50
t-1,3-Dichloropropene
Concen: 10.291 ug/l
RT: 8.203 min Scan# 2150
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Tgt Ion: 75 Resp: 57571
Ion Ratio Lower Upper
75 100
77 32.3 24.9 37.3








#51
cis-1,3-Dichloropropene
Concen: 10.099 ug/l
RT: 7.599 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#52
1,1,2-Trichloroethane
Concen: 10.327 ug/l
RT: 8.393 min Scan# 2209
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion: 97 Resp: 43960
Ion Ratio Lower Upper
97 100
83 89.5 70.2 105.2
85 57.8 45.2 67.8
99 63.2 50.1 75.1

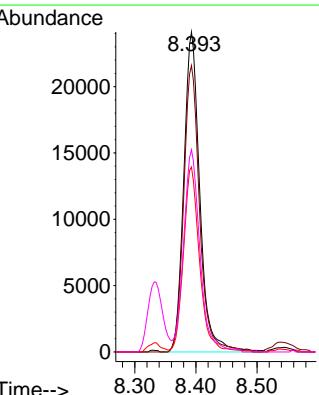

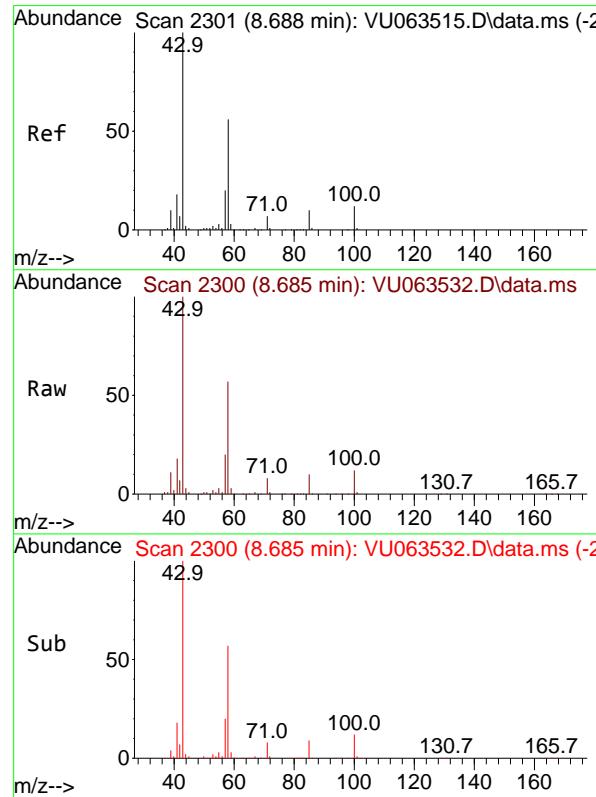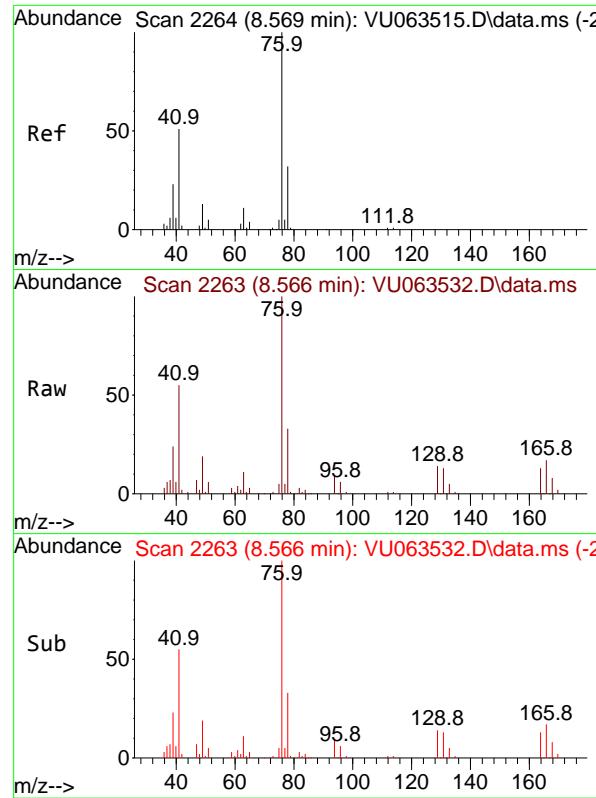

#53

1,3-Dichloropropane

Concen: 10.333 ug/l

RT: 8.566 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

Tgt Ion: 76 Resp: 7593

Ion Ratio Lower Upper

76 100

78 33.2


26.0

39.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

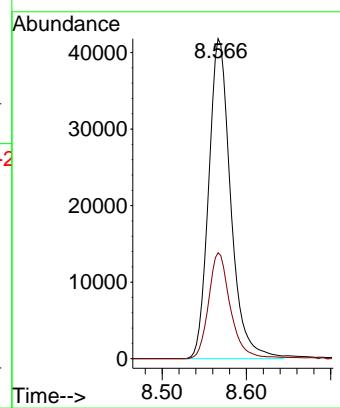

#54

2-Hexanone

Concen: 61.353 ug/l

RT: 8.685 min Scan# 2300

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt Ion: 43 Resp: 132800

Ion Ratio Lower Upper

43 100

58 56.9


34.8




74.8

57 20.2

0.0

39.5

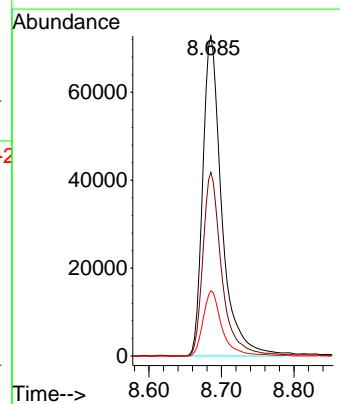






#55

Dibromochloromethane
Concen: 10.403 ug/l
RT: 8.801 min Scan# 2336
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#56

1,2-Dibromoethane
Concen: 10.244 ug/l
RT: 8.917 min Scan# 2372
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion:107 Resp: 39027
Ion Ratio Lower Upper
107 100
109 92.6 0.0 186.4

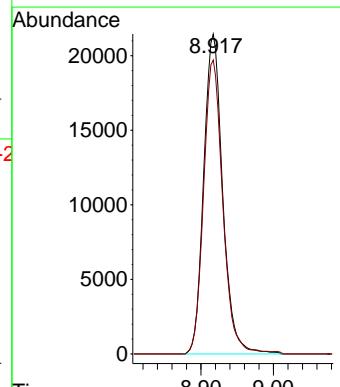

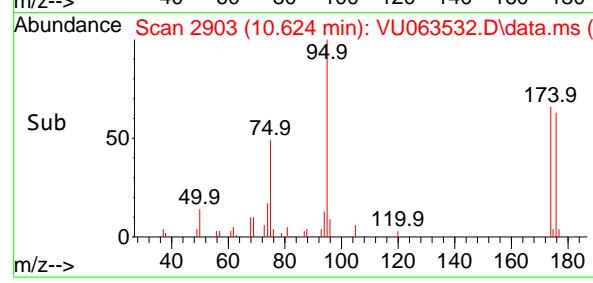

#57

4-Bromofluorobenzene

Concen: 1.121 ug/l

RT: 10.624 min Scan# 2903

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

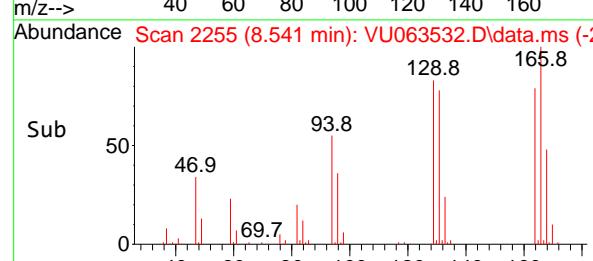 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#58

Tetrachloroethene

Concen: 9.565 ug/l


RT: 8.541 min Scan# 2255




Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt	Ion:164	Resp:	58247
Ion	Ratio	Lower	Upper
164	100		
166	127.2	100.7	151.1
129	105.9	80.6	120.8
131	98.6	77.3	115.9

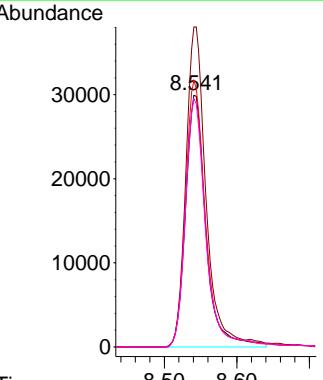

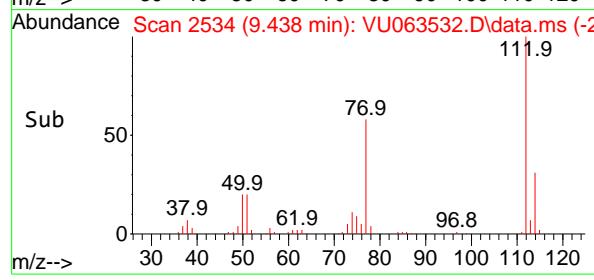

#59

Chlorobenzene

Concen: 10.249 ug/l

RT: 9.438 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11




Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#60

1,1,1,2-Tetrachloroethane

Concen: 10.060 ug/l

RT: 9.525 min Scan# 2561

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11



Tgt Ion:131 Resp: 52907




Ion Ratio Lower Upper

131 100

133 95.9 74.7 112.1

119 65.9 53.0 79.4

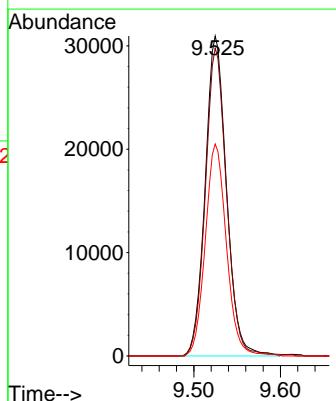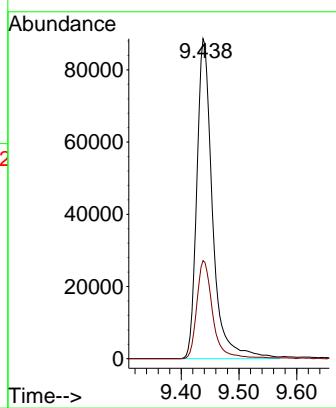

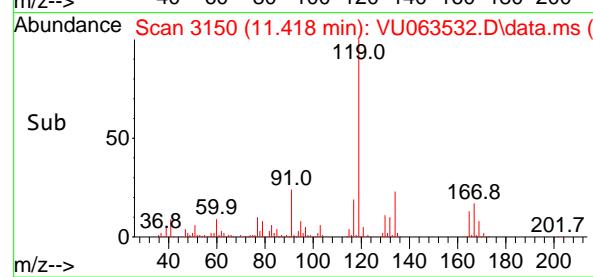

#61

Pentachloroethane

Concen: 10.796 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument :

MSVOA_U




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#62

Hexachloroethane

Concen: 10.606 ug/l


RT: 12.467 min Scan# 3476







Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
117	100				
201	71.1	57.4	39030	86.0	

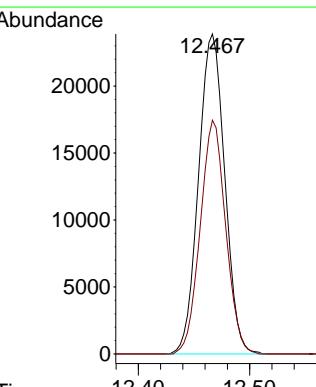



#63

Ethyl Benzene

Concen: 10.281 ug/l

RT: 9.560 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#64

m/p-Xylenes

Concen: 20.884 ug/l

RT: 9.685 min Scan# 2611

Delta R.T. 0.000 min

Lab File: VU063532.D


Acq: 18 Jul 2025 09:11


Tgt Ion:106 Resp: 228441

Ion Ratio Lower Upper

106 100

91 207.6 163.6 245.4

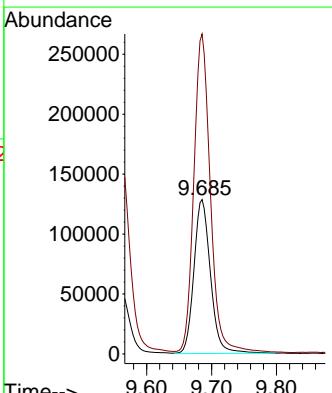


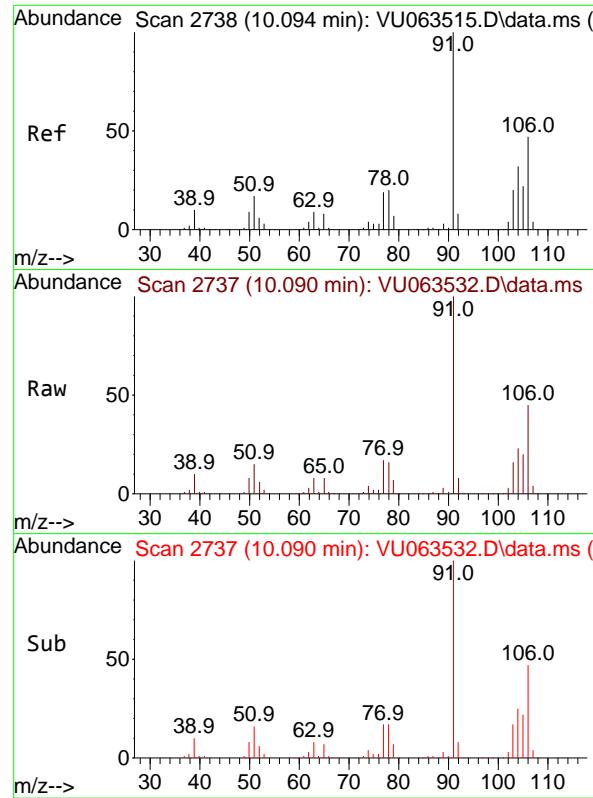


#65
o-Xylene
Concen: 10.626 ug/l
RT: 10.090 min Scan# 2
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

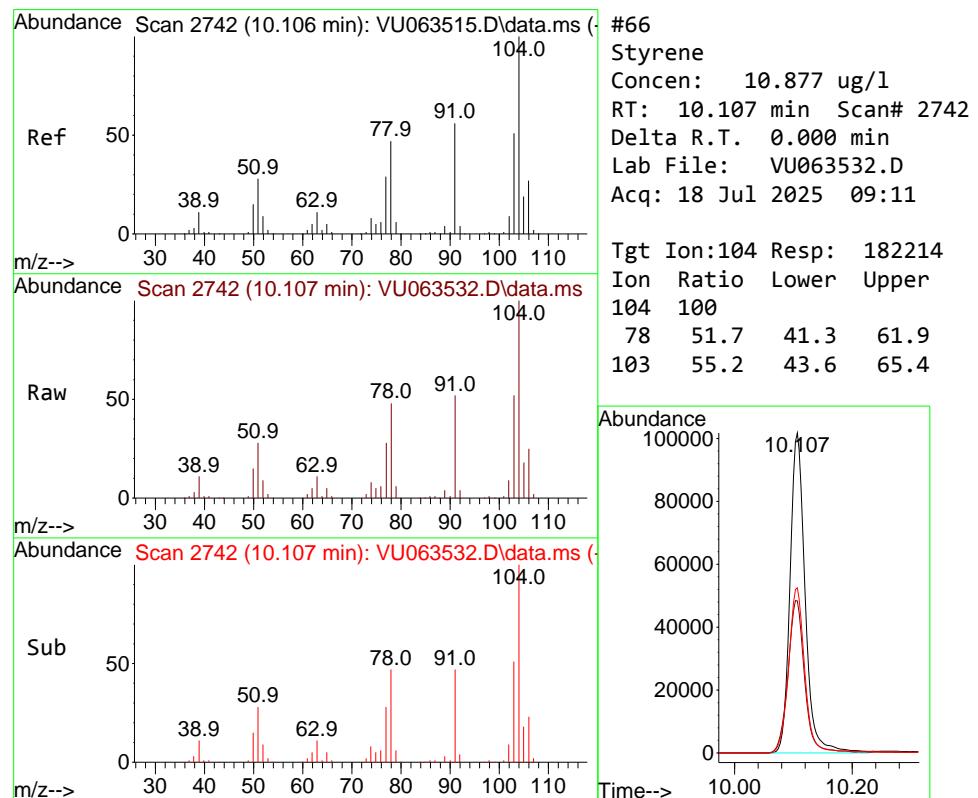

#66
Styrene
Concen: 10.877 ug/l
RT: 10.107 min Scan# 2742
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion:104 Resp: 182214
Ion Ratio Lower Upper
104 100
78 51.7 41.3 61.9
103 55.2 43.6 65.4

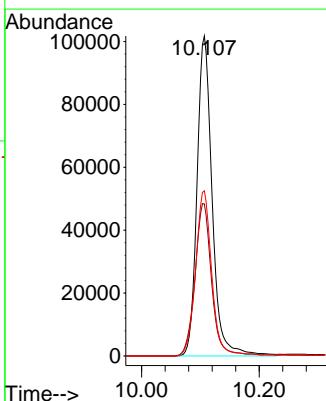



#67

Bromoform

Concen: 9.853 ug/l

RT: 10.283 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11





Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

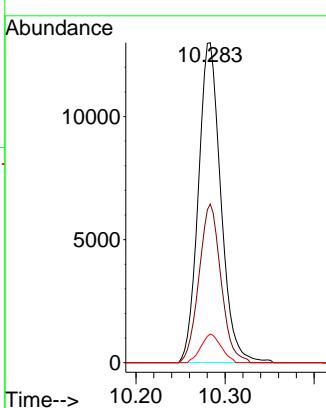 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.089 ug/l


RT: 12.184 min Scan# 3388




Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt	Ion:152	Resp:	8443
Ion	Ratio	Lower	Upper
152	100		
115	134.3	0.0	262.2
150	327.1	0.0	651.2

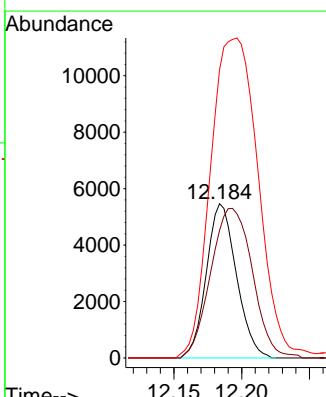



#69

Isopropylbenzene

Concen: 10.673 ug/l

RT: 10.476 min Scan# 2

Instrument :

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11




ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 10.657 ug/l

RT: 10.772 min Scan# 2949

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Tgt Ion: 83 Resp: 55200




Ion Ratio Lower Upper

83 100

131 9.7 8.4 12.6

85 64.4 51.9 77.9



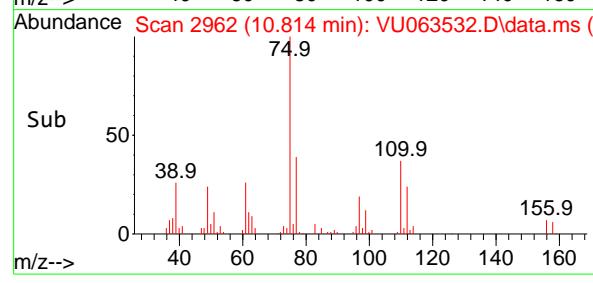

#71

1,2,3-Trichloropropane

Concen: 10.198 ug/l m

RT: 10.814 min Scan# 2962

Delta R.T. -0.003 min

Lab File: VU063532.D




Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#72

Bromobenzene

Concen: 10.241 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Tgt Ion:156 Resp: 67162




Ion Ratio Lower Upper

156 100

77 166.6 0.0 315.2

158 96.7 0.0 195.4

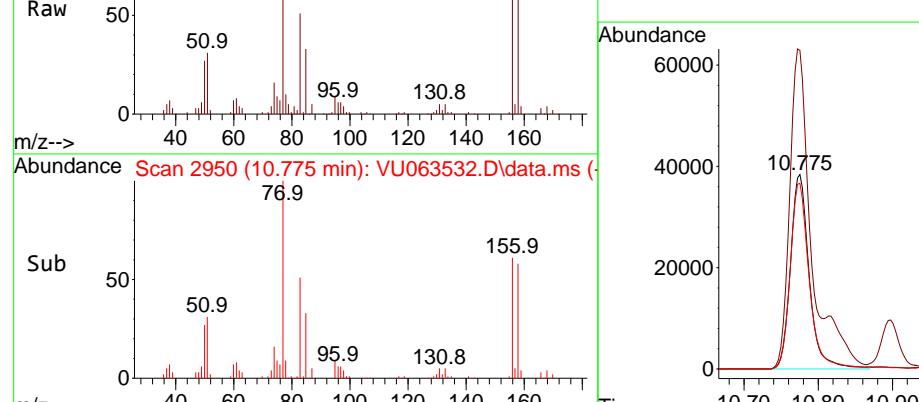



#73

n-propylbenzene

Concen: 10.911 ug/l

RT: 10.898 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11





Instrument :

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

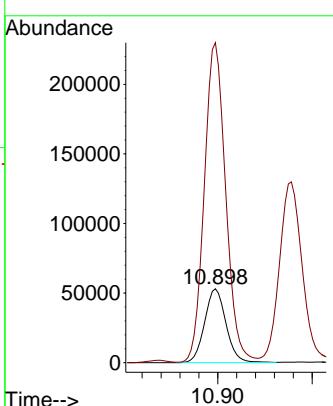 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#74

2-Chlorotoluene

Concen: 10.538 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063532.D


Acq: 18 Jul 2025 09:11




Tgt Ion:126 Resp: 71241

Ion Ratio Lower Upper

126 100

91 305.8 0.0 606.0









#75
1,3,5-Trimethylbenzene
Concen: 10.839 ug/l
RT: 11.078 min Scan# 3044
Delta R.T. -0.003 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

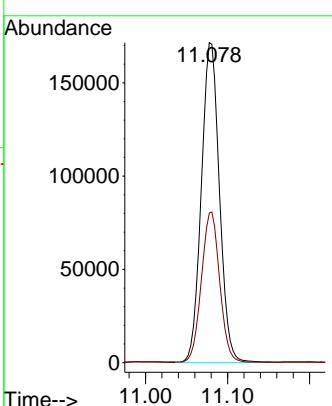

#76
4-Chlorotoluene
Concen: 10.851 ug/l
RT: 11.090 min Scan# 3048
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion:126 Resp: 74500
Ion Ratio Lower Upper
126 100
91 339.7 0.0 682.2

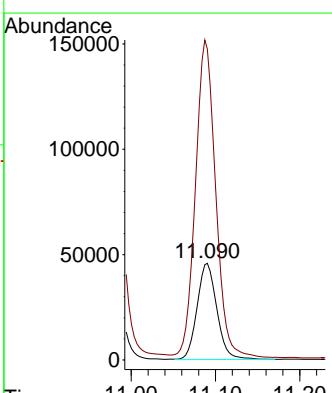

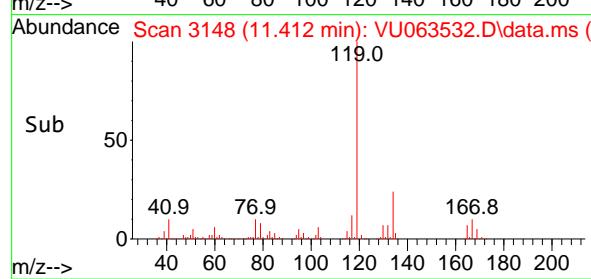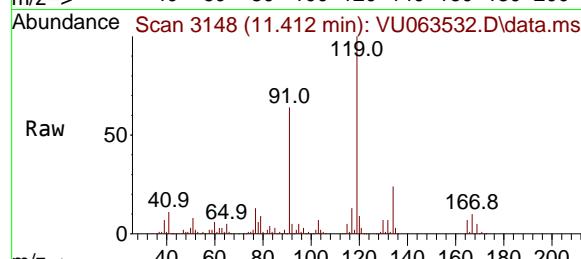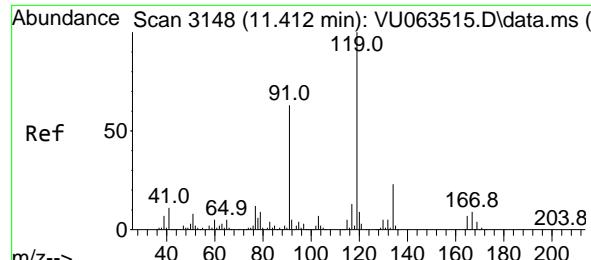

#77

tert-Butylbenzene

Concen: 10.723 ug/l

RT: 11.412 min Scan# 3148

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11





Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

**Manual Integrations
APPROVED**

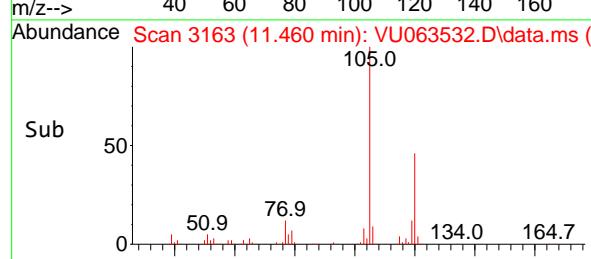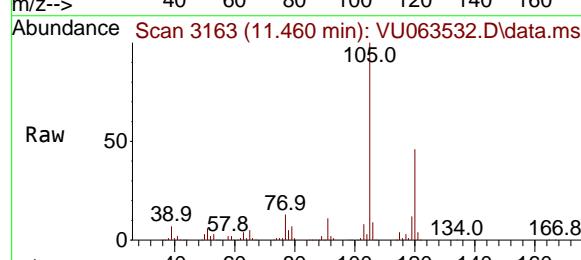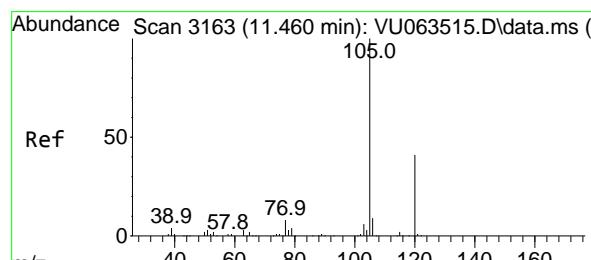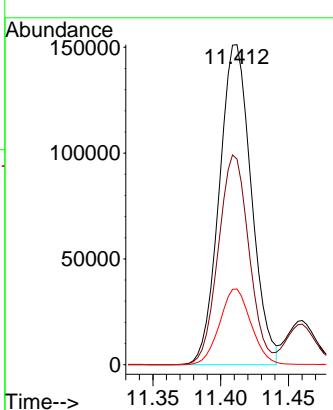 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#78

1,2,4-Trimethylbenzene

Concen: 10.884 ug/l


RT: 11.460 min Scan# 3163




Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt	Ion:105	Resp:	262116
Ion	Ratio	Lower	Upper
105	100		
120	45.6	22.7	68.0

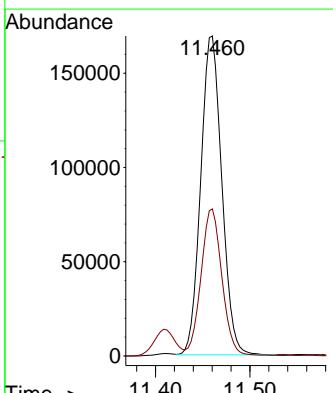







#79
sec-Butylbenzene
Concen: 10.911 ug/l
RT: 11.634 min Scan# 341350
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

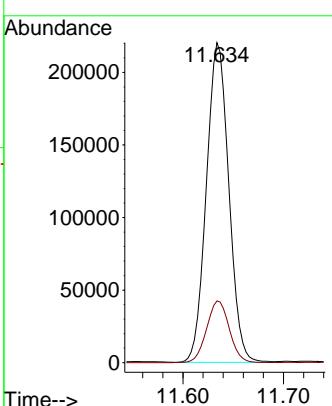

#80
Nitrobenzene
Concen: 42.376 ug/l
RT: 13.203 min Scan# 3705
Delta R.T. -0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11


Tgt Ion: 77 Resp: 4689
Ion Ratio Lower Upper
77 100
123 36.7 16.9 59.7
65 17.3 16.5 20.9

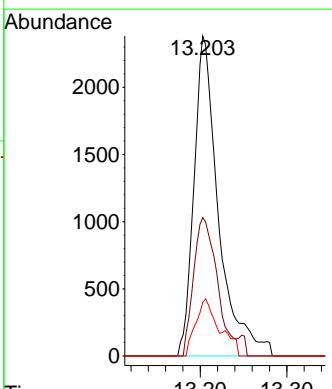



#81
p-Isopropyltoluene
Concen: 11.013 ug/l
RT: 11.785 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11



Instrument : MSVOA_U
ClientSampleId : VSTDCCC010



Tgt Ion:119 Resp: 28761:
Ion Ratio Lower Upper
119 100
134 25.9 21.1 31.7
91 25.1 19.8 29.8




Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

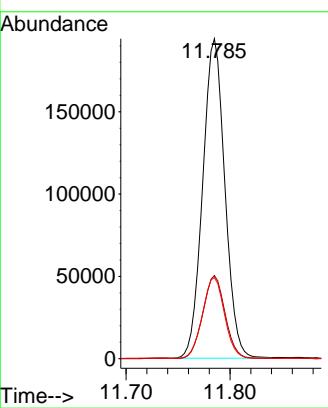

#82
1,3-Dichlorobenzene
Concen: 10.671 ug/l
RT: 11.737 min Scan# 3249
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion:146 Resp: 140019
Ion Ratio Lower Upper
146 100
111 41.4 33.8 50.6
148 63.8 51.5 77.3

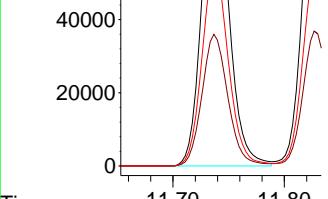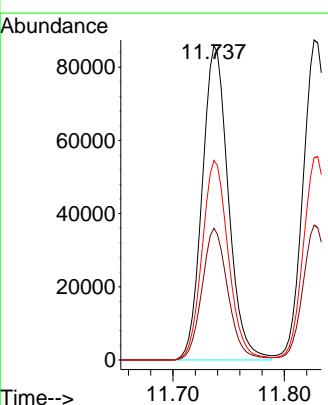

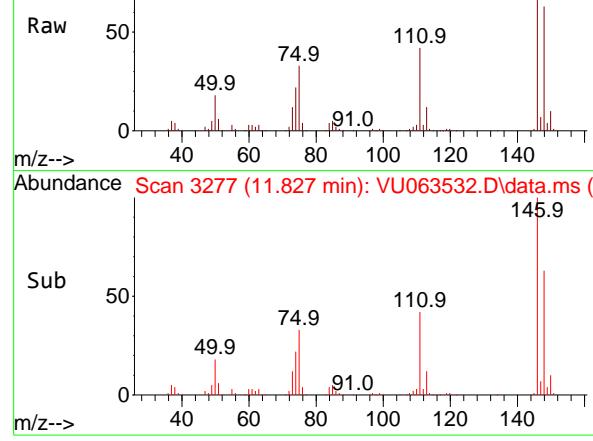

#83

1,4-Dichlorobenzene

Concen: 10.769 ug/l

RT: 11.827 min Scan# 3

Instrument:

MSVOA_U

Delta R.T. -0.003 min

ClientSampleId :

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

VSTDCCC010

Tgt Ion:146 Resp: 141444

Ion Ratio Lower Upper

146 100




111 41.7 32.0 48.0

148 63.4 50.2 75.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#84

n-Butylbenzene

Concen: 11.423 ug/l

RT: 12.200 min Scan# 3393

Delta R.T. -0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Tgt Ion: 91 Resp: 276678







Ion Ratio Lower Upper

91 100

92 52.5 41.5 62.3

134 25.4 20.6 30.8

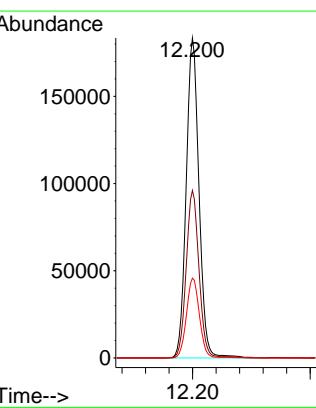



#85

1,2-Dichlorobenzene

Concen: 10.868 ug/l

RT: 12.203 min Scan# 3

Delta R.T. -0.003 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Instrument:

MSVOA_U

ClientSampleId :

VSTDCCC010

Tgt Ion:146 Resp: 133970

Ion Ratio Lower Upper

146 100


111 42.9 21.7 65.1

148 64.0 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

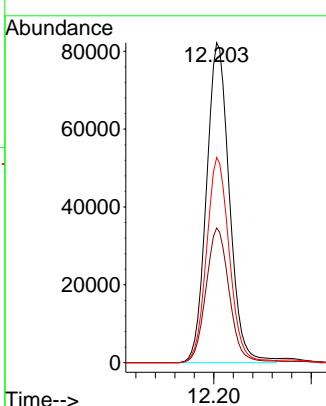

#86

1,2-Dibromo-3-Chloropropane

Concen: 9.368 ug/l

RT: 12.987 min Scan# 3638

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11


Tgt Ion: 75 Resp: 8081


Ion Ratio Lower Upper

75 100

155 79.6 65.8 98.6

157 104.5 81.4 122.2

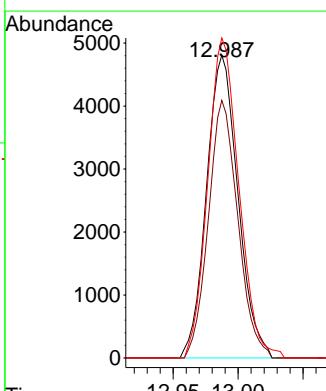


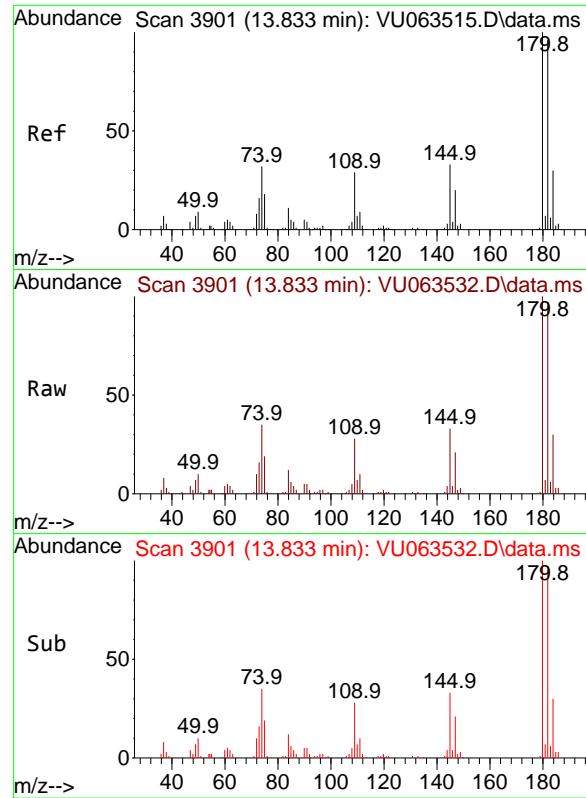


#87
1,2,4-Trichlorobenzene
Concen: 10.783 ug/l
RT: 13.833 min Scan# 3901
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Instrument : MSVOA_U
ClientSampleId : VSTDCCC010


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

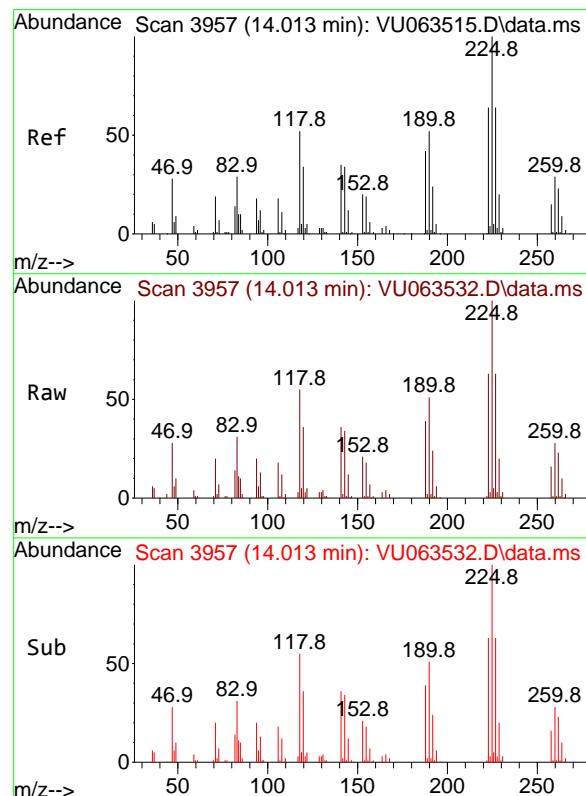

#88
Hexachlorobutadiene
Concen: 10.355 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063532.D
Acq: 18 Jul 2025 09:11

Tgt Ion:225 Resp: 45081
Ion Ratio Lower Upper
225 100
223 64.6 50.8 76.2
227 63.6 51.0 76.6

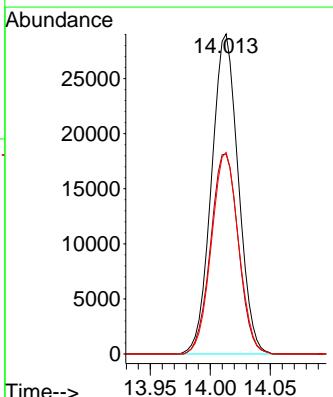

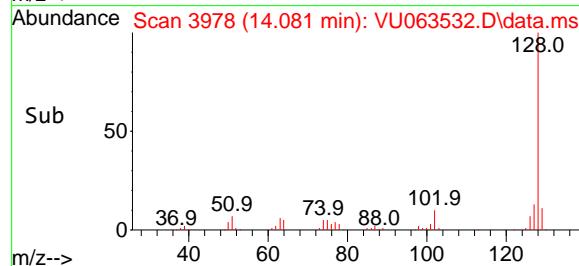

#89

Naphthalene

Concen: 10.991 ug/l

RT: 14.081 min Scan# 3

Instrument : MSVOA_U





Delta R.T. 0.001 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

ClientSampleId : VSTDCCC010

**Manual Integrations
APPROVED**

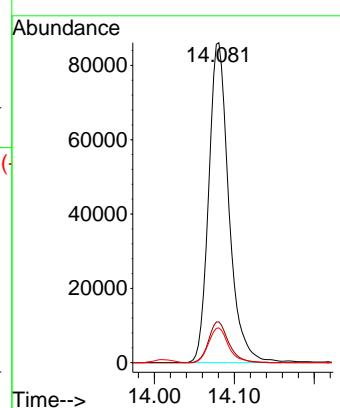 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#90

1,2,3-Trichlorobenzene

Concen: 10.751 ug/l


RT: 14.322 min Scan# 4053

Delta R.T. 0.000 min

Lab File: VU063532.D

Acq: 18 Jul 2025 09:11

Tgt	Ion:180	Resp:	76164
Ion	Ratio	Lower	Upper
180	100		
182	95.9	78.0	117.0
145	34.4	27.3	40.9

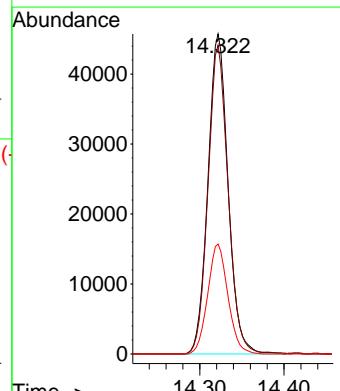

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063532.D
 Acq On : 18 Jul 2025 09:11
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25ML/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 23:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 i	Fluorobenzene	1.000	1.000	0.0	87	0.00
2 T	Dichlorodifluoromethane	0.295	0.285	3.4	84	0.00
3 t	Chloromethane	0.274	0.271	1.1	88	0.00
4 Rt	Vinyl Chloride	0.349	0.339	2.9	83	0.00
5 T	Bromomethane	0.263	0.257	2.3	92	0.00
6 T	Chloroethane	0.211	0.211	0.0	86	0.00
7 T	Trichlorofluoromethane	0.501	0.508	-1.4	87	0.00
8	1,1,2-Trichloro-1,2,2-trifl	0.262	0.269	-2.7	88	0.00
9 Rt	1,1-Dichloroethene	0.260	0.260	0.0	85	0.00
10 t	Iodomethane	0.314	0.333	-6.1	78	0.00
11 t	Allyl Chloride	0.375	0.378	-0.8	86	0.00
12 t	Acrylonitrile	0.065	0.066	-1.5	91	0.00
13 T	Acetone	0.052	0.090	-73.1#	157	0.00
14 T	Carbon Disulfide	0.839	0.746	11.1	75	0.00
15 RT	Methylene Chloride	0.306	0.304	0.7	90	0.00
16 RT	trans-1,2-Dichloroethene	0.295	0.292	1.0	85	0.00
17 t	1,1-Dichloroethane	0.546	0.553	-1.3	88	0.00
18 T	2-Butanone	0.081	0.108	-33.3#	118	0.00
19	Cyclohexane	0.463	0.463	0.0	87	0.00
20	Methylcyclohexane	0.450	0.407	9.6	72	0.00
21 T	2,2-Dichloropropane	0.465	0.465	0.0	89	0.00
22 RT	cis-1,2-Dichloroethene	0.320	0.322	-0.6	87	0.00
23 t	Diethyl Ether	0.198	0.207	-4.5	87	0.00
24 t	tert-Butyl Alcohol	0.024	0.024	0.0	86	0.00
25 t	Methyl tert-Butyl Ether	0.678	0.701	-3.4	88	0.00
26 t	Bromochloromethane	0.134	0.137	-2.2	87	0.00
27 t	Chloroform	0.558	0.577	-3.4	92	0.00
28 RT	1,1,1-Trichloroethane	0.473	0.486	-2.7	88	0.00
29 T	1,1-Dichloropropene	0.438	0.442	-0.9	88	0.00
30 RT	Carbon Tetrachloride	0.381	0.391	-2.6	87	0.00
31 t	Isopropyl Ether	0.825	0.824	0.1	86	0.00
32	Ethyl-t-butyl ether	0.763	0.772	-1.2	87	0.00
33	Tert-Amyl methyl ether	0.663	0.675	-1.8	88	0.00
34 t	Propionitrile	0.025	0.024	4.0	89	0.00
35 RT	Benzene	1.178	1.246	-5.8	90	0.00
36 RT	1,2-Dichloroethane	0.366	0.390	-6.6	90	0.00
37 RT	Trichloroethene	0.301	0.269	10.6	72	0.00
38 Rt	1,2-Dichloropropane	0.276	0.267	3.3	73	0.00
39 t	Methacrylonitrile	0.109	0.102	6.4	88	0.00
40 t	Methyl acrylate	0.159	0.155	2.5	80	0.00
41 t	Tetrahydrofuran	0.057	0.054	5.3	89	0.00
42 t	1-Chlorobutane	0.583	0.602	-3.3	88	0.00
43 T	Dibromomethane	0.143	0.142	0.7	80	0.00
44 T	Bromodichloromethane	0.322	0.316	1.9	84	0.00
45 T	4-Methyl-2-Pentanone	0.147	0.154	-4.8	88	0.00
46 t	t-1,4-Dichloro-2-butene	0.055	0.055	0.0	76	0.00
47 t	Methyl methacrylate	0.120	0.123	-2.5	84	0.00
48 t	Ethyl methacrylate	0.229	0.243	-6.1	84	0.00
49 Rt	Toluene	0.643	0.658	-2.3	85	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063532.D
 Acq On : 18 Jul 2025 09:11
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 23:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
50 T	t-1,3-Dichloropropene	0.253	0.260	-2.8	79	0.00
51 T	cis-1,3-Dichloropropene	0.339	0.343	-1.2	82	0.00
52 RT	1,1,2-Trichloroethane	0.192	0.199	-3.6	85	0.00
53 t	1,3-Dichloropropane	0.332	0.343	-3.3	87	0.00
54 t	2-Hexanone	0.098	0.120	-22.4	101	0.00
55 t	Dibromochloromethane	0.203	0.211	-3.9	79	0.00
56 T	1,2-Dibromoethane	0.172	0.176	-2.3	86	0.00
57 S	4-Bromofluorobenzene	0.379	0.425	-12.1	100	0.00
58 RT	Tetrachloroethene	0.275	0.263	4.4	80	0.00
59 Rt	Chlorobenzene	0.739	0.757	-2.4	85	0.00
60 T	1,1,1,2-Tetrachloroethane	0.238	0.239	-0.4	82	0.00
61 t	Pentachloroethane	0.168	0.181	-7.7	84	0.00
62 t	Hexachloroethane	0.166	0.176	-6.0	80	0.00
63 Rt	Ethyl Benzene	1.271	1.307	-2.8	86	0.00
64 RT	m/p-Xylenes	0.494	0.516	-4.5	86	0.00
65 RT	o-Xylene	0.475	0.505	-6.3	87	0.00
66 RT	Styrene	0.757	0.823	-8.7	87	0.00
67 t	Bromoform	0.104	0.103	1.0	76	0.00
68 S	1,2-Dichlorobenzene-d4	0.350	0.381	-8.9	92	0.00
69 T	Isopropylbenzene	1.148	1.225	-6.7	86	0.00
70 T	1,1,2,2-Tetrachloroethane	0.234	0.249	-6.4	89	0.00
71 T	1,2,3-Trichloropropane	0.190	0.194	-2.1	81	0.00
72 t	Bromobenzene	0.296	0.303	-2.4	85	0.00
73 t	n-propylbenzene	0.346	0.377	-9.0	87	0.00
74 t	2-Chlorotoluene	0.305	0.322	-5.6	87	0.00
75 t	1,3,5-Trimethylbenzene	1.097	1.189	-8.4	87	0.00
76 t	4-Chlorotoluene	0.310	0.337	-8.7	89	0.00
77 t	tert-Butylbenzene	1.048	1.124	-7.3	87	0.00
78 t	1,2,4-Trimethylbenzene	1.088	1.184	-8.8	87	0.00
79 t	sec-Butylbenzene	1.413	1.542	-9.1	88	0.00
80	Nitrobenzene	0.004	0.004	0.0	69	0.00
81 t	p-Isopropyltoluene	1.180	1.299	-10.1	88	0.00
82 t	1,3-Dichlorobenzene	0.593	0.633	-6.7	87	0.00
83 Rt	1,4-Dichlorobenzene	0.593	0.639	-7.8	87	0.00
84 t	n-Butylbenzene	1.094	1.250	-14.3	90	0.00
85 Rt	1,2-Dichlorobenzene	0.557	0.605	-8.6	88	0.00
86 t	1,2-Dibromo-3-Chloropropane	0.033	0.037	-12.1	79	0.00
87 Rt	1,2,4-Trichlorobenzene	0.346	0.373	-7.8	84	0.00
88 t	Hexachlorobutadiene	0.197	0.204	-3.6	84	0.00
89 t	Naphthalene	0.621	0.682	-9.8	87	0.00
90 t	1,2,3-Trichlorobenzene	0.320	0.344	-7.5	85	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063532.D
 Acq On : 18 Jul 2025 09:11
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 23:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 i	Fluorobenzene	1.000	1.000	0.0	87	0.00
2 T	Dichlorodifluoromethane	10.000	9.679	3.2	84	0.00
3 t	Chloromethane	10.000	9.869	1.3	88	0.00
4 Rt	Vinyl Chloride	10.000	9.713	2.9	83	0.00
5 T	Bromomethane	10.000	9.778	2.2	92	0.00
6 T	Chloroethane	10.000	10.032	-0.3	86	0.00
7 T	Trichlorofluoromethane	10.000	10.130	-1.3	87	0.00
8	1,1,2-Trichloro-1,2,2-trifl	10.000	10.278	-2.8	88	0.00
9 Rt	1,1-Dichloroethene	10.000	10.027	-0.3	85	0.00
10 t	Iodomethane	10.000	8.700	13.0	78	0.00
11 t	Allyl Chloride	10.000	10.065	-0.6	86	0.00
12 t	Acrylonitrile	20.000	20.347	-1.7	91	0.00
13 T	Acetone	50.000	86.744	-73.5#	157	0.00
14 T	Carbon Disulfide	10.000	8.892	11.1	75	0.00
15 RT	Methylene Chloride	10.000	9.932	0.7	90	0.00
16 RT	trans-1,2-Dichloroethene	10.000	9.902	1.0	85	0.00
17 t	1,1-Dichloroethane	10.000	10.126	-1.3	88	0.00
18 T	2-Butanone	50.000	67.111	-34.2#	118	0.00
19	Cyclohexane	10.000	10.008	-0.1	87	0.00
20	Methylcyclohexane	10.000	9.053	9.5	72	0.00
21 T	2,2-Dichloropropane	10.000	9.992	0.1	89	0.00
22 RT	cis-1,2-Dichloroethene	10.000	10.076	-0.8	87	0.00
23 t	Diethyl Ether	10.000	10.482	-4.8	87	0.00
24 t	tert-Butyl Alcohol	100.000	99.368	0.6	86	0.00
25 t	Methyl tert-Butyl Ether	10.000	10.348	-3.5	88	0.00
26 t	Bromochloromethane	10.000	10.279	-2.8	87	0.00
27 t	Chloroform	10.000	10.340	-3.4	92	0.00
28 RT	1,1,1-Trichloroethane	10.000	10.278	-2.8	88	0.00
29 T	1,1-Dichloropropene	10.000	10.077	-0.8	88	0.00
30 RT	Carbon Tetrachloride	10.000	10.264	-2.6	87	0.00
31 t	Isopropyl Ether	10.000	9.983	0.2	86	0.00
32	Ethyl-t-butyl ether	10.000	10.117	-1.2	87	0.00
33	Tert-Amyl methyl ether	10.000	10.191	-1.9	88	0.00
34 t	Propionitrile	50.000	47.974	4.1	89	0.00
35 RT	Benzene	10.000	10.575	-5.7	90	0.00
36 RT	1,2-Dichloroethane	10.000	10.641	-6.4	90	0.00
37 RT	Trichloroethene	10.000	8.950	10.5	72	0.00
38 Rt	1,2-Dichloropropane	10.000	9.683	3.2	73	0.00
39 t	Methacrylonitrile	10.000	9.375	6.3	88	0.00
40 t	Methyl acrylate	10.000	9.721	2.8	80	0.00
41 t	Tetrahydrofuran	20.000	18.783	6.1	89	0.00
42 t	1-Chlorobutane	10.000	10.334	-3.3	88	0.00
43 T	Dibromomethane	10.000	9.911	0.9	80	0.00
44 T	Bromodichloromethane	10.000	9.806	1.9	84	0.00
45 T	4-Methyl-2-Pentanone	50.000	52.342	-4.7	88	0.00
46 t	t-1,4-Dichloro-2-butene	20.000	19.823	0.9	76	0.00
47 t	Methyl methacrylate	20.000	20.535	-2.7	84	0.00
48 t	Ethyl methacrylate	10.000	10.607	-6.1	84	0.00
49 Rt	Toluene	10.000	10.235	-2.3	85	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063532.D
 Acq On : 18 Jul 2025 09:11
 Operator : MD/SY
 Sample : VSTDCCC010
 Misc : 25ML/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTDCCC010

Quant Time: Jul 18 23:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
50 T	t-1,3-Dichloropropene	10.000	10.291	-2.9	79	0.00
51 T	cis-1,3-Dichloropropene	10.000	10.099	-1.0	82	0.00
52 RT	1,1,2-Trichloroethane	10.000	10.327	-3.3	85	0.00
53 t	1,3-Dichloropropane	10.000	10.333	-3.3	87	0.00
54 t	2-Hexanone	50.000	61.353	-22.7	101	0.00
55 t	Dibromochloromethane	10.000	10.403	-4.0	79	0.00
56 T	1,2-Dibromoethane	10.000	10.244	-2.4	86	0.00
57 S	4-Bromofluorobenzene	1.000	1.121	-12.1	100	0.00
58 RT	Tetrachloroethene	10.000	9.565	4.4	80	0.00
59 Rt	Chlorobenzene	10.000	10.249	-2.5	85	0.00
60 T	1,1,1,2-Tetrachloroethane	10.000	10.060	-0.6	82	0.00
61 t	Pentachloroethane	10.000	10.796	-8.0	84	0.00
62 t	Hexachloroethane	10.000	10.606	-6.1	80	0.00
63 Rt	Ethyl Benzene	10.000	10.281	-2.8	86	0.00
64 RT	m/p-Xylenes	20.000	20.884	-4.4	86	0.00
65 RT	o-Xylene	10.000	10.626	-6.3	87	0.00
66 RT	Styrene	10.000	10.877	-8.8	87	0.00
67 t	Bromoform	10.000	9.853	1.5	76	0.00
68 S	1,2-Dichlorobenzene-d4	1.000	1.089	-8.9	92	0.00
69 T	Isopropylbenzene	10.000	10.673	-6.7	86	0.00
70 T	1,1,2,2-Tetrachloroethane	10.000	10.657	-6.6	89	0.00
71 T	1,2,3-Trichloropropane	10.000	10.198	-2.0	81	0.00
72 t	Bromobenzene	10.000	10.241	-2.4	85	0.00
73 t	n-propylbenzene	10.000	10.911	-9.1	87	0.00
74 t	2-Chlorotoluene	10.000	10.538	-5.4	87	0.00
75 t	1,3,5-Trimethylbenzene	10.000	10.839	-8.4	87	0.00
76 t	4-Chlorotoluene	10.000	10.851	-8.5	89	0.00
77 t	tert-Butylbenzene	10.000	10.723	-7.2	87	0.00
78 t	1,2,4-Trimethylbenzene	10.000	10.884	-8.8	87	0.00
79 t	sec-Butylbenzene	10.000	10.911	-9.1	88	0.00
80	Nitrobenzene	50.000	42.376	15.2	69	0.00
81 t	p-Isopropyltoluene	10.000	11.013	-10.1	88	0.00
82 t	1,3-Dichlorobenzene	10.000	10.671	-6.7	87	0.00
83 Rt	1,4-Dichlorobenzene	10.000	10.769	-7.7	87	0.00
84 t	n-Butylbenzene	10.000	11.423	-14.2	90	0.00
85 Rt	1,2-Dichlorobenzene	10.000	10.868	-8.7	88	0.00
86 t	1,2-Dibromo-3-Chloropropane	10.000	9.368	6.3	79	0.00
87 Rt	1,2,4-Trichlorobenzene	10.000	10.783	-7.8	84	0.00
88 t	Hexachlorobutadiene	10.000	10.355	-3.6	84	0.00
89 t	Naphthalene	10.000	10.991	-9.9	87	0.00
90 t	1,2,3-Trichlorobenzene	10.000	10.751	-7.5	85	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



QC SAMPLE


DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071625\
 Data File : VU063510.D
 Acq On : 16 Jul 2025 08:13
 Operator : MD/SY
 Sample : BFB
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Jul 17 03:49:40 2025

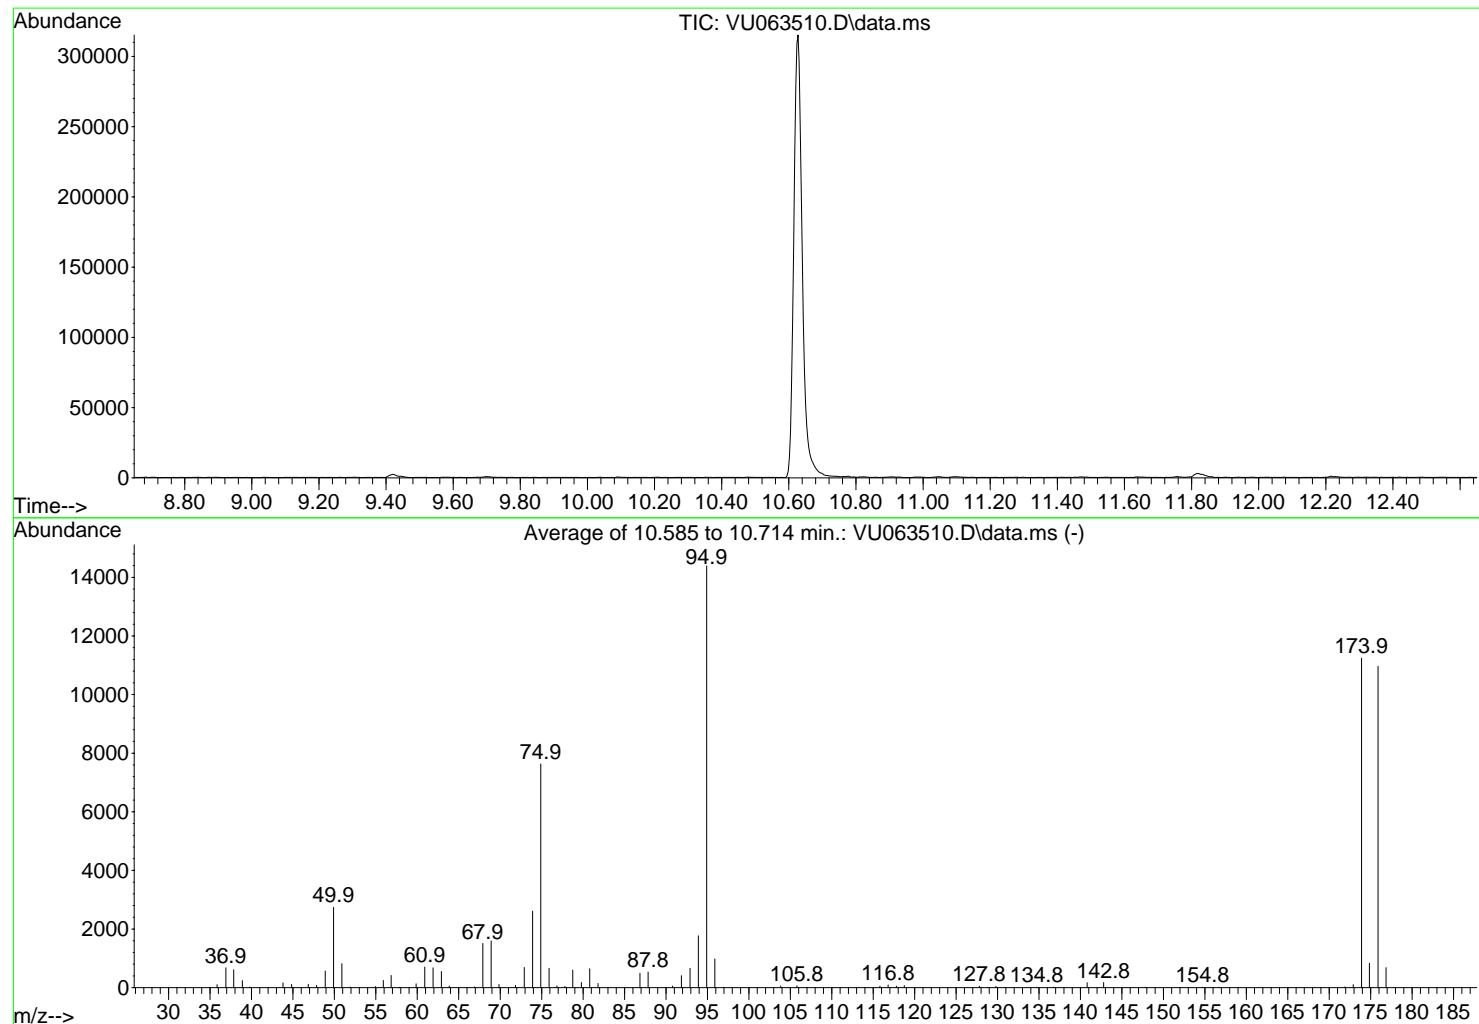

AutoFind: Averaged scan 2891 to 2931; Bkg corrected with scan 2890


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	2743	PASS
75	95	30	60	53.0	7631	PASS
95	95	100	100	100.0	14392	PASS
96	95	5	9	6.8	984	PASS
173	174	0.00	2	0.9	104	PASS
174	95	50	100	78.1	11242	PASS
175	174	5	9	7.4	829	PASS
176	174	95	101	97.5	10965	PASS
177	176	5	9	6.2	681	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063518.D
 Acq On : 17 Jul 2025 08:10
 Operator : MD/SY
 Sample : BFB
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Jul 17 03:49:40 2025

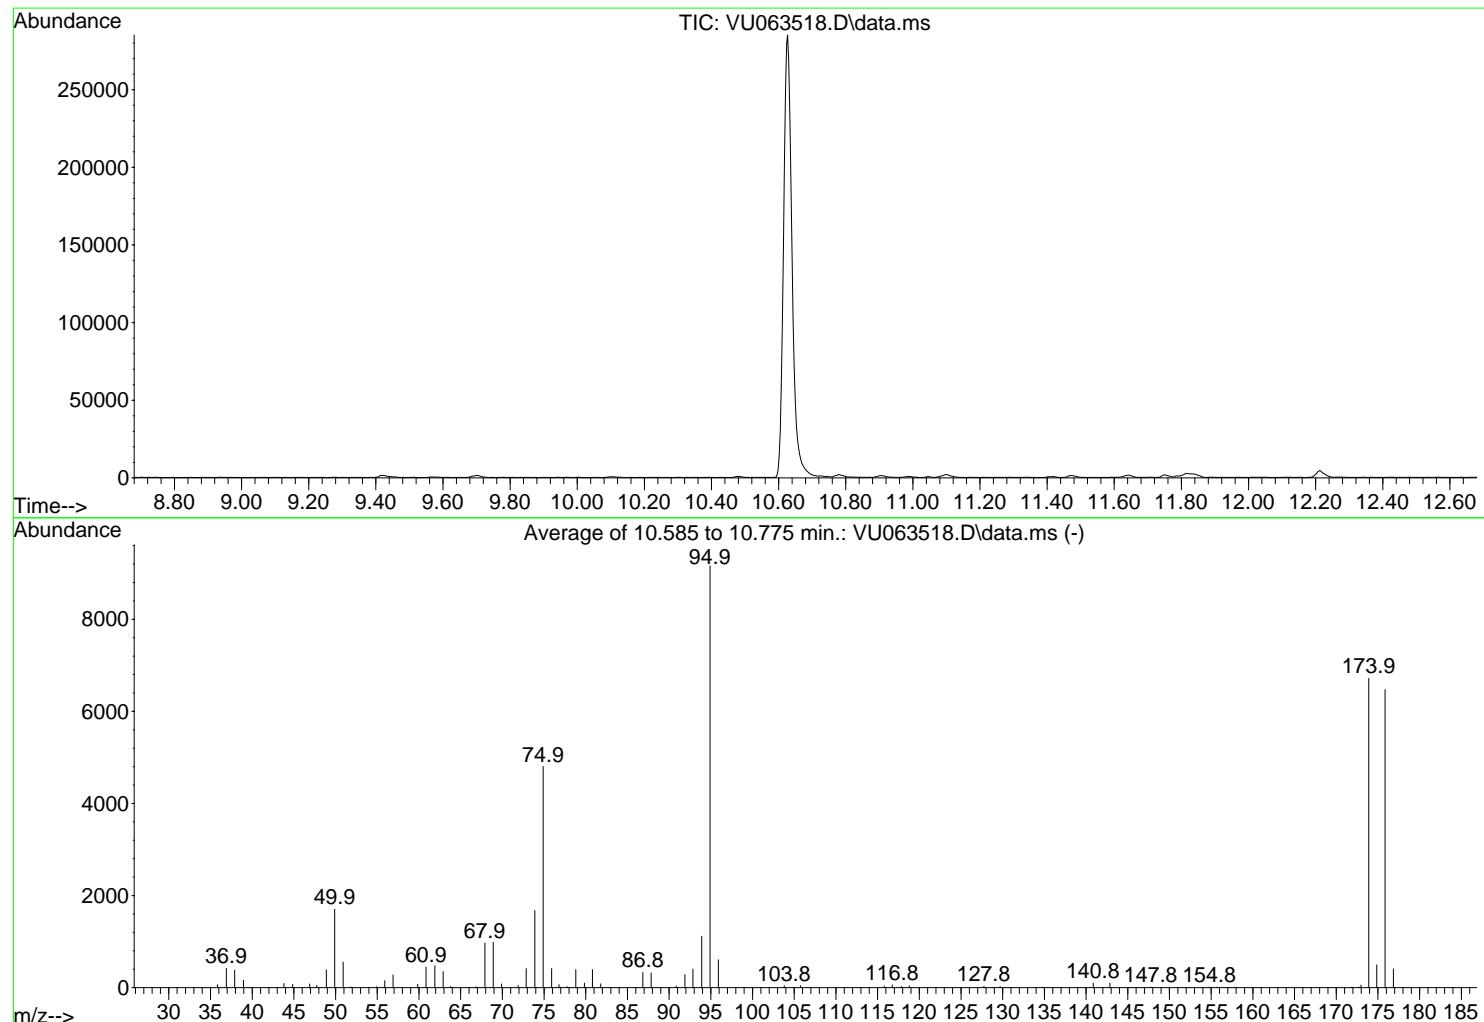

AutoFind: Averaged scan 2891 to 2950; Bkg corrected with scan 2890


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	1703	PASS
75	95	30	60	52.4	4803	PASS
95	95	100	100	100.0	9161	PASS
96	95	5	9	6.6	606	PASS
173	174	0.00	2	0.8	56	PASS
174	95	50	100	73.3	6718	PASS
175	174	5	9	7.3	493	PASS
176	174	95	101	96.4	6474	PASS
177	176	5	9	6.3	405	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063531.D
 Acq On : 18 Jul 2025 08:07
 Operator : MD/SY
 Sample : BFB
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Jul 17 03:49:40 2025

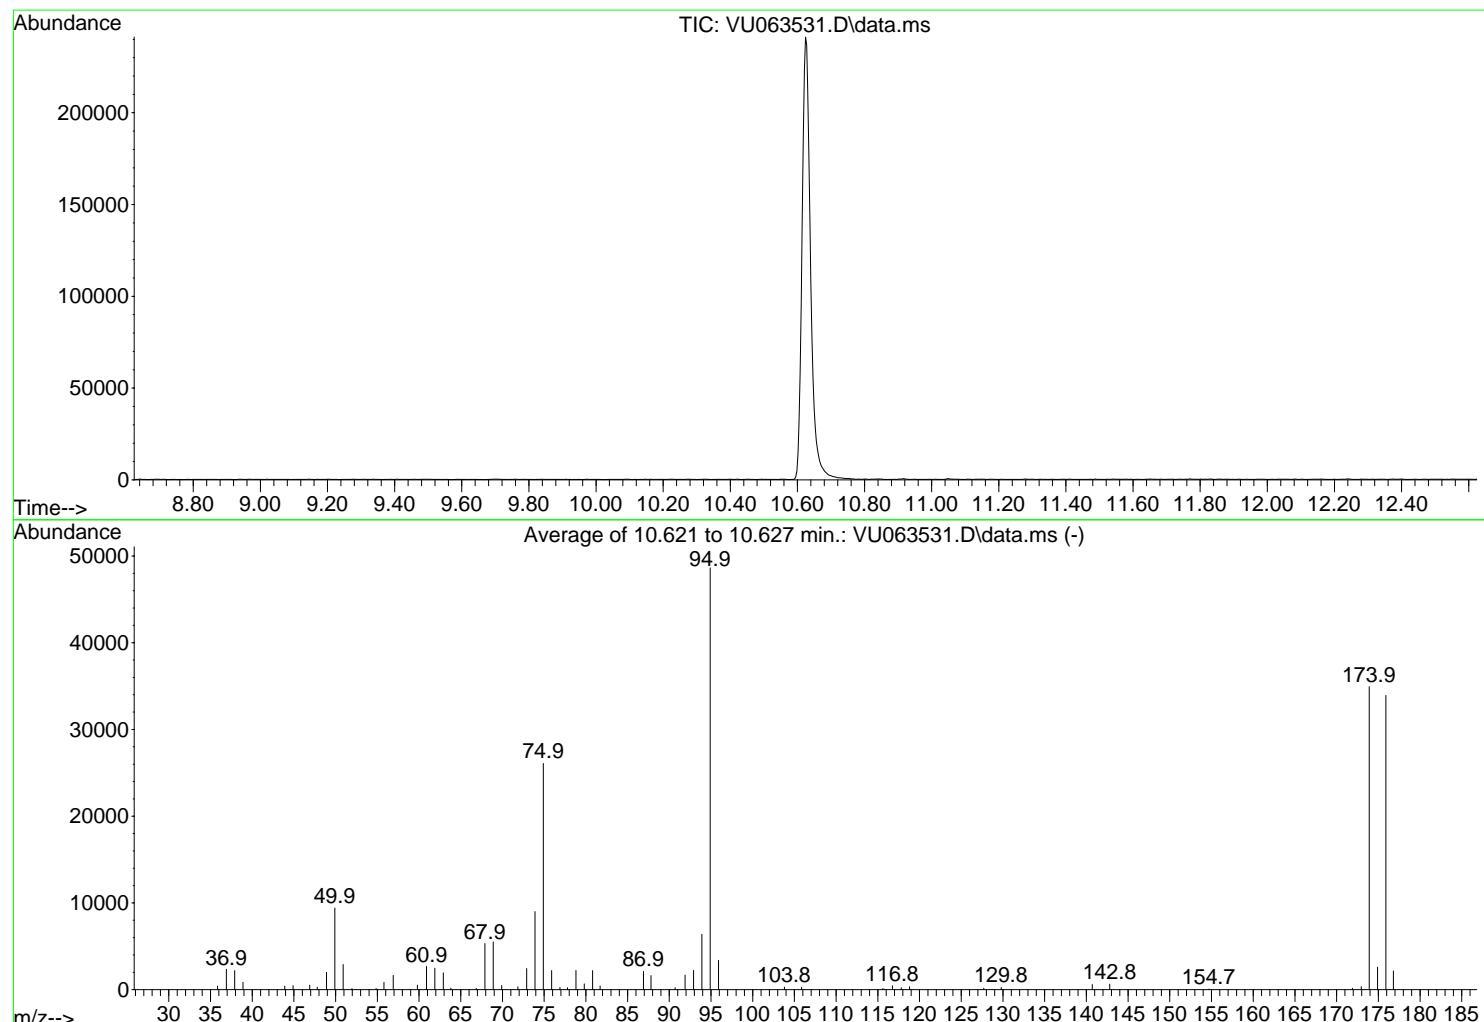

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	9408	PASS
75	95	30	60	53.6	26088	PASS
95	95	100	100	100.0	48635	PASS
96	95	5	9	7.0	3383	PASS
173	174	0.00	2	1.0	361	PASS
174	95	50	100	71.8	34936	PASS
175	174	5	9	7.4	2590	PASS
176	174	95	101	97.1	33925	PASS
177	176	5	9	6.4	2161	PASS



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBL01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBL01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063520.D	1	07/17/25 11:31	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	0.12	U	0.12	0.50	ug/L
74-87-3	Chloromethane	0.13	U	0.13	0.50	ug/L
75-01-4	Vinyl Chloride	0.12	U	0.12	0.50	ug/L
74-83-9	Bromomethane	0.15	U	0.15	0.50	ug/L
75-00-3	Chloroethane	0.14	U	0.14	0.50	ug/L
109-99-9	Tetrahydrofuran	0.42	U	0.42	1.00	ug/L
75-69-4	Trichlorofluoromethane	0.20	U	0.20	0.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	0.11	U	0.11	0.50	ug/L
75-65-0	tert-Butyl Alcohol	3.60	U	3.60	10.0	ug/L
60-29-7	Diethyl Ether	0.13	U	0.13	0.50	ug/L
75-35-4	1,1-Dichloroethene	0.13	U	0.13	0.50	ug/L
107-13-1	Acrylonitrile	0.44	U	0.44	1.00	ug/L
67-64-1	Acetone	0.97	U	0.97	2.50	ug/L
75-15-0	Carbon Disulfide	0.12	U	0.12	0.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	0.11	U	0.11	0.50	ug/L
96-33-3	Methyl acrylate	0.33	U	0.33	0.50	ug/L
75-09-2	Methylene Chloride	0.44	U	0.44	0.50	ug/L
156-60-5	trans-1,2-Dichloroethene	0.14	U	0.14	0.50	ug/L
75-34-3	1,1-Dichloroethane	0.13	U	0.13	0.50	ug/L
110-82-7	Cyclohexane	0.14	U	0.14	0.50	ug/L
78-93-3	2-Butanone	0.72	U	0.72	2.50	ug/L
56-23-5	Carbon Tetrachloride	0.13	U	0.13	0.50	ug/L
594-20-7	2,2-Dichloropropane	0.12	U	0.12	0.50	ug/L
156-59-2	cis-1,2-Dichloroethene	0.13	U	0.13	0.50	ug/L
74-97-5	Bromoform	0.17	U	0.17	0.50	ug/L
67-66-3	Chloroform	0.17	U	0.17	0.50	ug/L
71-55-6	1,1,1-Trichloroethane	0.12	U	0.12	0.50	ug/L
108-87-2	Methylcyclohexane	0.090	U	0.090	0.50	ug/L
563-58-6	1,1-Dichloropropene	0.11	U	0.11	0.50	ug/L
107-12-0	Propionitrile	1.20	U	1.20	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBL01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBL01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063520.D	1	07/17/25 11:31	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	0.11	U	0.11	0.50	ug/L
107-06-2	1,2-Dichloroethane	0.14	U	0.14	0.50	ug/L
79-01-6	Trichloroethene	0.13	U	0.13	0.50	ug/L
78-87-5	1,2-Dichloropropane	0.13	U	0.13	0.50	ug/L
109-69-3	1-Chlorobutane	0.12	U	0.12	0.50	ug/L
74-95-3	Dibromomethane	0.15	U	0.15	0.50	ug/L
75-27-4	Bromodichloromethane	0.13	U	0.13	0.50	ug/L
108-10-1	4-Methyl-2-Pentanone	0.63	U	0.63	2.50	ug/L
108-88-3	Toluene	0.11	U	0.11	0.50	ug/L
10061-02-6	t-1,3-Dichloropropene	0.11	U	0.11	0.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	0.11	U	0.11	0.50	ug/L
79-00-5	1,1,2-Trichloroethane	0.13	U	0.13	0.50	ug/L
142-28-9	1,3-Dichloropropane	0.12	U	0.12	0.50	ug/L
591-78-6	2-Hexanone	0.65	U	0.65	2.50	ug/L
124-48-1	Dibromochloromethane	0.20	U	0.20	0.50	ug/L
106-93-4	1,2-Dibromoethane	0.13	U	0.13	0.50	ug/L
127-18-4	Tetrachloroethene	0.14	U	0.14	0.50	ug/L
108-90-7	Chlorobenzene	0.11	U	0.11	0.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	0.13	U	0.13	0.50	ug/L
67-72-1	Hexachloroethane	0.12	U	0.12	0.50	ug/L
100-41-4	Ethyl Benzene	0.41	U	0.41	0.50	ug/L
179601-23-1	m/p-Xylenes	0.73	U	0.73	1.00	ug/L
1330-20-7	Total Xylenes	1.09	U	1.09	1.50	ug/L
95-47-6	o-Xylene	0.36	U	0.36	0.50	ug/L
100-42-5	Styrene	0.38	U	0.38	0.50	ug/L
75-25-2	Bromoform	0.31	U	0.31	0.50	ug/L
98-82-8	Isopropylbenzene	0.38	U	0.38	0.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	0.13	U	0.13	0.50	ug/L
96-18-4	1,2,3-Trichloropropane	0.19	U	0.19	0.50	ug/L
108-86-1	Bromobenzene	0.13	U	0.13	0.50	ug/L
103-65-1	n-propylbenzene	0.42	U	0.42	0.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBL01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBL01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063520.D	1	07/17/25 11:31	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	0.27	U	0.27	0.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	0.37	U	0.37	0.50	ug/L
106-43-4	4-Chlorotoluene	0.27	U	0.27	0.50	ug/L
98-06-6	tert-Butylbenzene	0.37	U	0.37	0.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	0.40	U	0.40	0.50	ug/L
135-98-8	sec-Butylbenzene	0.36	U	0.36	0.50	ug/L
99-87-6	p-Isopropyltoluene	0.42	U	0.42	0.50	ug/L
541-73-1	1,3-Dichlorobenzene	0.13	U	0.13	0.50	ug/L
106-46-7	1,4-Dichlorobenzene	0.13	U	0.13	0.50	ug/L
104-51-8	n-Butylbenzene	0.43	U	0.43	0.50	ug/L
95-50-1	1,2-Dichlorobenzene	0.14	U	0.14	0.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	0.24	U	0.24	0.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	0.21	U	0.21	0.50	ug/L
87-68-3	Hexachlorobutadiene	0.14	U	0.14	0.50	ug/L
91-20-3	Naphthalene	0.33	U	0.33	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	0.31	U	0.31	0.50	ug/L
98-95-3	Nitrobenzene	1.80	U	1.80	5.00	ug/L
363-72-4	Pentachloroethane	0.16	U	0.16	0.50	ug/L
74-88-4	Iodomethane	0.090	U	0.090	1.00	ug/L
107-05-1	Allyl Chloride	0.13	U	0.13	0.50	ug/L
126-98-7	Methacrylonitrile	0.24	U	0.24	0.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	0.21	U	0.21	1.00	ug/L
97-63-2	Ethyl methacrylate	0.12	U	0.12	0.50	ug/L
108-20-3	Isopropyl Ether	0.14	U	0.14	0.50	ug/L
80-62-6	Methyl methacrylate	0.24	U	0.24	1.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	0.94		70 - 130	94%	SPK: 1
460-00-4	4-Bromofluorobenzene	1.10		70 - 130	107%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	23000	6.1			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBL01	SDG No.:	Q2552	
Lab Sample ID:	VU0717WBL01	Matrix:	Water	
Analytical Method:	E524.2	% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol: 25000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063520.D	1	07/17/25 11:31	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063520.D
 Acq On : 17 Jul 2025 11:31
 Operator : MD/SY
 Sample : VU0717WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBL01

Quant Time: Jul 18 04:10:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<hr/>						
Internal Standards						
1) Fluorobenzene	6.100	96	22965	1.000	ug/l	# 0.00
<hr/>						
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	9320	1.072	ug/l	0.00
Spiked Amount	1.000		Recovery	=	107.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	7520	0.935	ug/l	0.00
Spiked Amount	1.000		Recovery	=	94.000%	


Target Compounds	Qvalue
<hr/>	


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063520.D
Acq On : 17 Jul 2025 11:31
Operator : MD/SY
Sample : VU0717WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBL01

Quant Time: Jul 18 04:10:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration


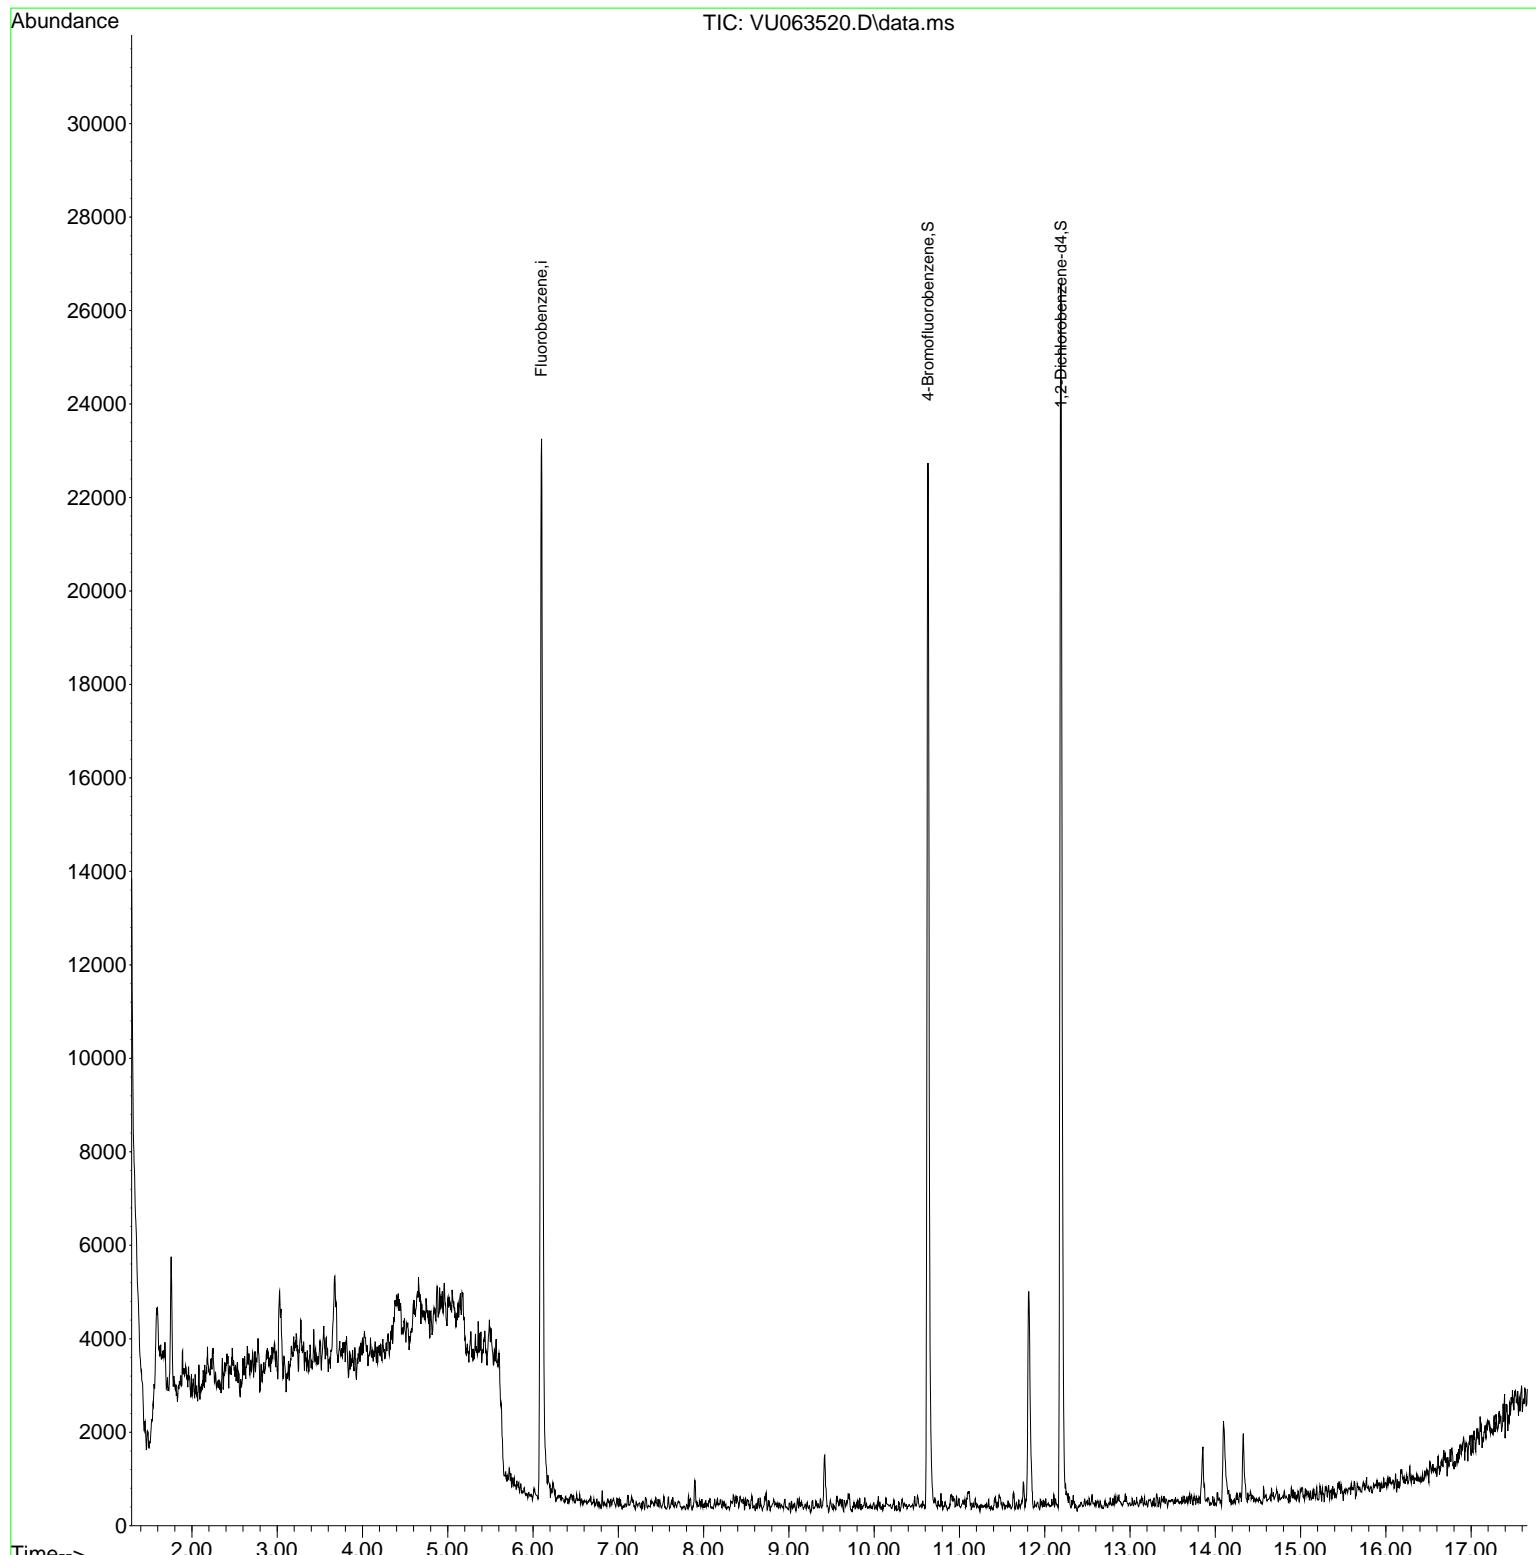


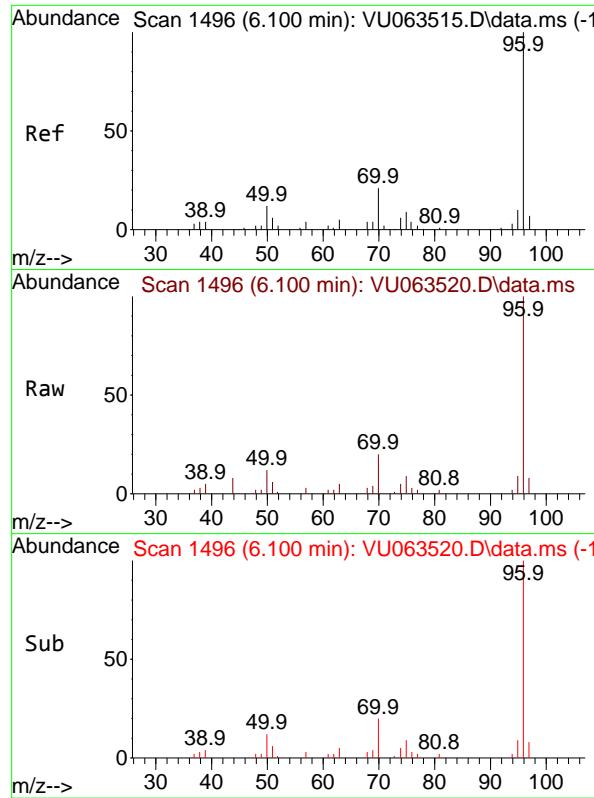

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063520.D
Acq: 17 Jul 2025 11:31


Instrument : MSVOA_U
ClientSampleId : VU0717WBL01


Tgt Ion: 96 Resp: 22965
Ion Ratio Lower Upper
96 100
70 17.1 15.0 22.4
95 8.2 7.4 11.0
97 6.1 0.0 0.0#

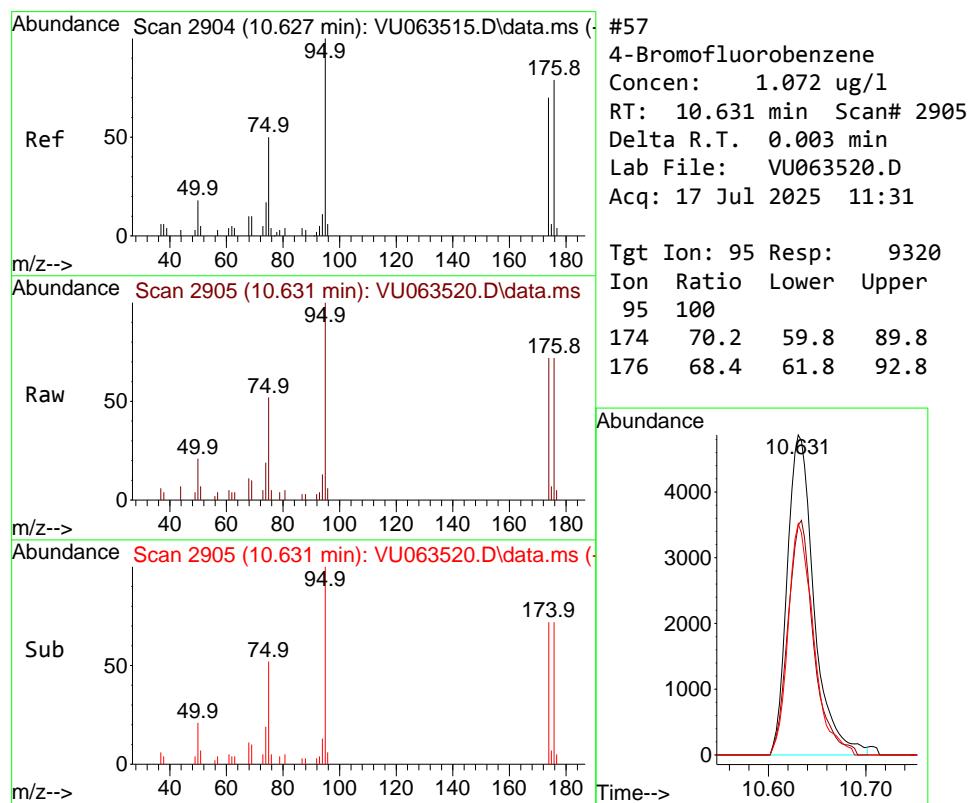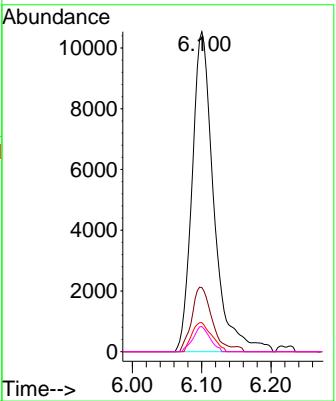

#57
4-Bromofluorobenzene
Concen: 1.072 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063520.D
Acq: 17 Jul 2025 11:31

Tgt Ion: 95 Resp: 9320
Ion Ratio Lower Upper
95 100
174 70.2 59.8 89.8
176 68.4 61.8 92.8

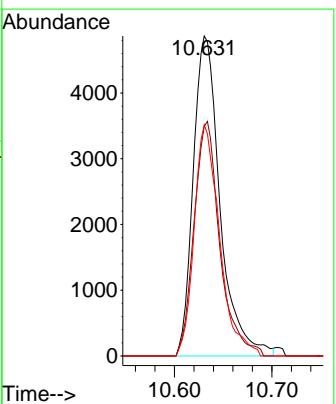

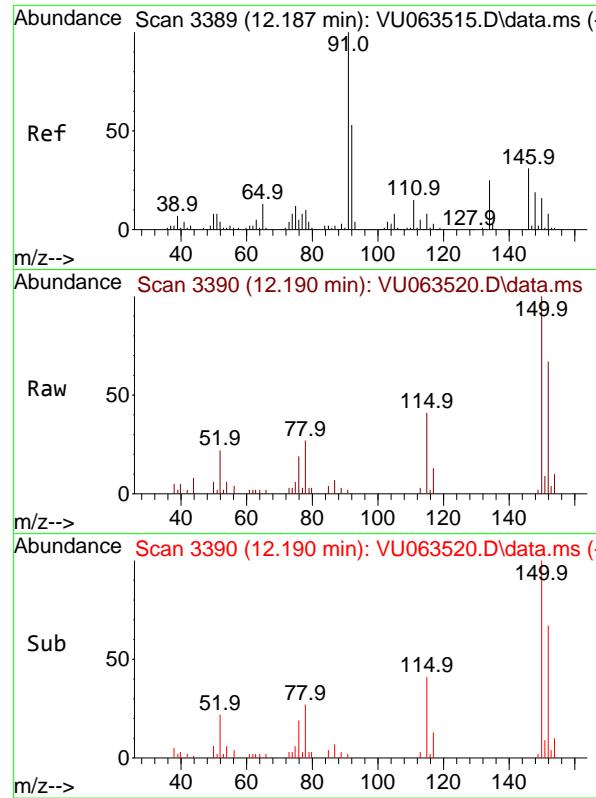

#68

1,2-Dichlorobenzene-d4

Concen: 0.935 ug/l

RT: 12.190 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063520.D

Acq: 17 Jul 2025 11:31

Instrument :

MSVOA_U

ClientSampleId :

VU0717WBL01


Tgt Ion:152 Resp: 7520

Ion Ratio Lower Upper

152 100

115 66.9 0.0 262.2

150 155.8 0.0 651.2

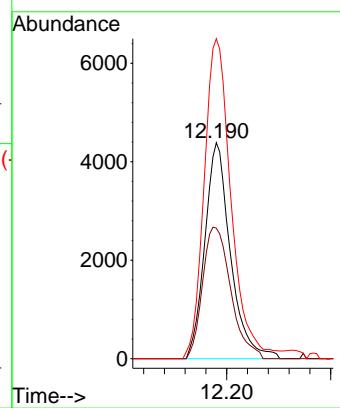



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBL01		SDG No.:	Q2552
Lab Sample ID:	VU0718WBL01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063533.D	1	07/18/25 10:49	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	0.12	U	0.12	0.50	ug/L
74-87-3	Chloromethane	0.13	U	0.13	0.50	ug/L
75-01-4	Vinyl Chloride	0.12	U	0.12	0.50	ug/L
74-83-9	Bromomethane	0.15	U	0.15	0.50	ug/L
75-00-3	Chloroethane	0.14	U	0.14	0.50	ug/L
109-99-9	Tetrahydrofuran	0.42	U	0.42	1.00	ug/L
75-69-4	Trichlorofluoromethane	0.20	U	0.20	0.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	0.11	U	0.11	0.50	ug/L
75-65-0	tert-Butyl Alcohol	3.60	U	3.60	10.0	ug/L
60-29-7	Diethyl Ether	0.13	U	0.13	0.50	ug/L
75-35-4	1,1-Dichloroethene	0.13	U	0.13	0.50	ug/L
107-13-1	Acrylonitrile	0.44	U	0.44	1.00	ug/L
67-64-1	Acetone	0.97	U	0.97	2.50	ug/L
75-15-0	Carbon Disulfide	0.12	U	0.12	0.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	0.11	U	0.11	0.50	ug/L
96-33-3	Methyl acrylate	0.33	U	0.33	0.50	ug/L
75-09-2	Methylene Chloride	0.44	U	0.44	0.50	ug/L
156-60-5	trans-1,2-Dichloroethene	0.14	U	0.14	0.50	ug/L
75-34-3	1,1-Dichloroethane	0.13	U	0.13	0.50	ug/L
110-82-7	Cyclohexane	0.14	U	0.14	0.50	ug/L
78-93-3	2-Butanone	0.72	U	0.72	2.50	ug/L
56-23-5	Carbon Tetrachloride	0.13	U	0.13	0.50	ug/L
594-20-7	2,2-Dichloropropane	0.12	U	0.12	0.50	ug/L
156-59-2	cis-1,2-Dichloroethene	0.13	U	0.13	0.50	ug/L
74-97-5	Bromoform	0.17	U	0.17	0.50	ug/L
67-66-3	Chloroform	0.17	U	0.17	0.50	ug/L
71-55-6	1,1,1-Trichloroethane	0.12	U	0.12	0.50	ug/L
108-87-2	Methylcyclohexane	0.090	U	0.090	0.50	ug/L
563-58-6	1,1-Dichloropropene	0.11	U	0.11	0.50	ug/L
107-12-0	Propionitrile	1.20	U	1.20	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBL01		SDG No.:	Q2552
Lab Sample ID:	VU0718WBL01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063533.D	1	07/18/25 10:49	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	0.11	U	0.11	0.50	ug/L
107-06-2	1,2-Dichloroethane	0.14	U	0.14	0.50	ug/L
79-01-6	Trichloroethene	0.13	U	0.13	0.50	ug/L
78-87-5	1,2-Dichloropropane	0.13	U	0.13	0.50	ug/L
109-69-3	1-Chlorobutane	0.12	U	0.12	0.50	ug/L
74-95-3	Dibromomethane	0.15	U	0.15	0.50	ug/L
75-27-4	Bromodichloromethane	0.13	U	0.13	0.50	ug/L
108-10-1	4-Methyl-2-Pentanone	0.63	U	0.63	2.50	ug/L
108-88-3	Toluene	0.11	U	0.11	0.50	ug/L
10061-02-6	t-1,3-Dichloropropene	0.11	U	0.11	0.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	0.11	U	0.11	0.50	ug/L
79-00-5	1,1,2-Trichloroethane	0.13	U	0.13	0.50	ug/L
142-28-9	1,3-Dichloropropane	0.12	U	0.12	0.50	ug/L
591-78-6	2-Hexanone	0.65	U	0.65	2.50	ug/L
124-48-1	Dibromochloromethane	0.20	U	0.20	0.50	ug/L
106-93-4	1,2-Dibromoethane	0.13	U	0.13	0.50	ug/L
127-18-4	Tetrachloroethene	0.14	U	0.14	0.50	ug/L
108-90-7	Chlorobenzene	0.11	U	0.11	0.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	0.13	U	0.13	0.50	ug/L
67-72-1	Hexachloroethane	0.12	U	0.12	0.50	ug/L
100-41-4	Ethyl Benzene	0.41	U	0.41	0.50	ug/L
179601-23-1	m/p-Xylenes	0.73	U	0.73	1.00	ug/L
1330-20-7	Total Xylenes	1.09	U	1.09	1.50	ug/L
95-47-6	o-Xylene	0.36	U	0.36	0.50	ug/L
100-42-5	Styrene	0.38	U	0.38	0.50	ug/L
75-25-2	Bromoform	0.31	U	0.31	0.50	ug/L
98-82-8	Isopropylbenzene	0.38	U	0.38	0.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	0.13	U	0.13	0.50	ug/L
96-18-4	1,2,3-Trichloropropane	0.19	U	0.19	0.50	ug/L
108-86-1	Bromobenzene	0.13	U	0.13	0.50	ug/L
103-65-1	n-propylbenzene	0.42	U	0.42	0.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBL01		SDG No.:	Q2552
Lab Sample ID:	VU0718WBL01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063533.D	1	07/18/25 10:49	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	0.27	U	0.27	0.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	0.37	U	0.37	0.50	ug/L
106-43-4	4-Chlorotoluene	0.27	U	0.27	0.50	ug/L
98-06-6	tert-Butylbenzene	0.37	U	0.37	0.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	0.40	U	0.40	0.50	ug/L
135-98-8	sec-Butylbenzene	0.36	U	0.36	0.50	ug/L
99-87-6	p-Isopropyltoluene	0.42	U	0.42	0.50	ug/L
541-73-1	1,3-Dichlorobenzene	0.13	U	0.13	0.50	ug/L
106-46-7	1,4-Dichlorobenzene	0.13	U	0.13	0.50	ug/L
104-51-8	n-Butylbenzene	0.43	U	0.43	0.50	ug/L
95-50-1	1,2-Dichlorobenzene	0.14	U	0.14	0.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	0.24	U	0.24	0.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	0.21	U	0.21	0.50	ug/L
87-68-3	Hexachlorobutadiene	0.14	U	0.14	0.50	ug/L
91-20-3	Naphthalene	0.33	U	0.33	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	0.31	U	0.31	0.50	ug/L
98-95-3	Nitrobenzene	1.80	U	1.80	5.00	ug/L
363-72-4	Pentachloroethane	0.16	U	0.16	0.50	ug/L
74-88-4	Iodomethane	0.090	U	0.090	1.00	ug/L
107-05-1	Allyl Chloride	0.13	U	0.13	0.50	ug/L
126-98-7	Methacrylonitrile	0.24	U	0.24	0.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	0.21	U	0.21	1.00	ug/L
97-63-2	Ethyl methacrylate	0.12	U	0.12	0.50	ug/L
108-20-3	Isopropyl Ether	0.14	U	0.14	0.50	ug/L
80-62-6	Methyl methacrylate	0.24	U	0.24	1.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	0.72		70 - 130	72%	SPK: 1
460-00-4	4-Bromofluorobenzene	0.79		70 - 130	79%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	25300	6.1			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBL01	SDG No.:	Q2552	
Lab Sample ID:	VU0718WBL01	Matrix:	Water	
Analytical Method:	E524.2	% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol: 25000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063533.D	1	07/18/25 10:49	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063533.D
 Acq On : 18 Jul 2025 10:49
 Operator : MD/SY
 Sample : VU0718WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01

Quant Time: Jul 18 23:47:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<hr/>						
Internal Standards						
1) Fluorobenzene	6.100	96	25256	1.000	ug/l	# 0.00
<hr/>						
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	7573	0.792	ug/l	0.00
Spiked Amount	1.000		Recovery	=	79.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	6388	0.722	ug/l	0.00
Spiked Amount	1.000		Recovery	=	72.000%	


Target Compounds	Qvalue
<hr/>	


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063533.D
Acq On : 18 Jul 2025 10:49
Operator : MD/SY
Sample : VU0718WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBL01

Quant Time: Jul 18 23:47:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration


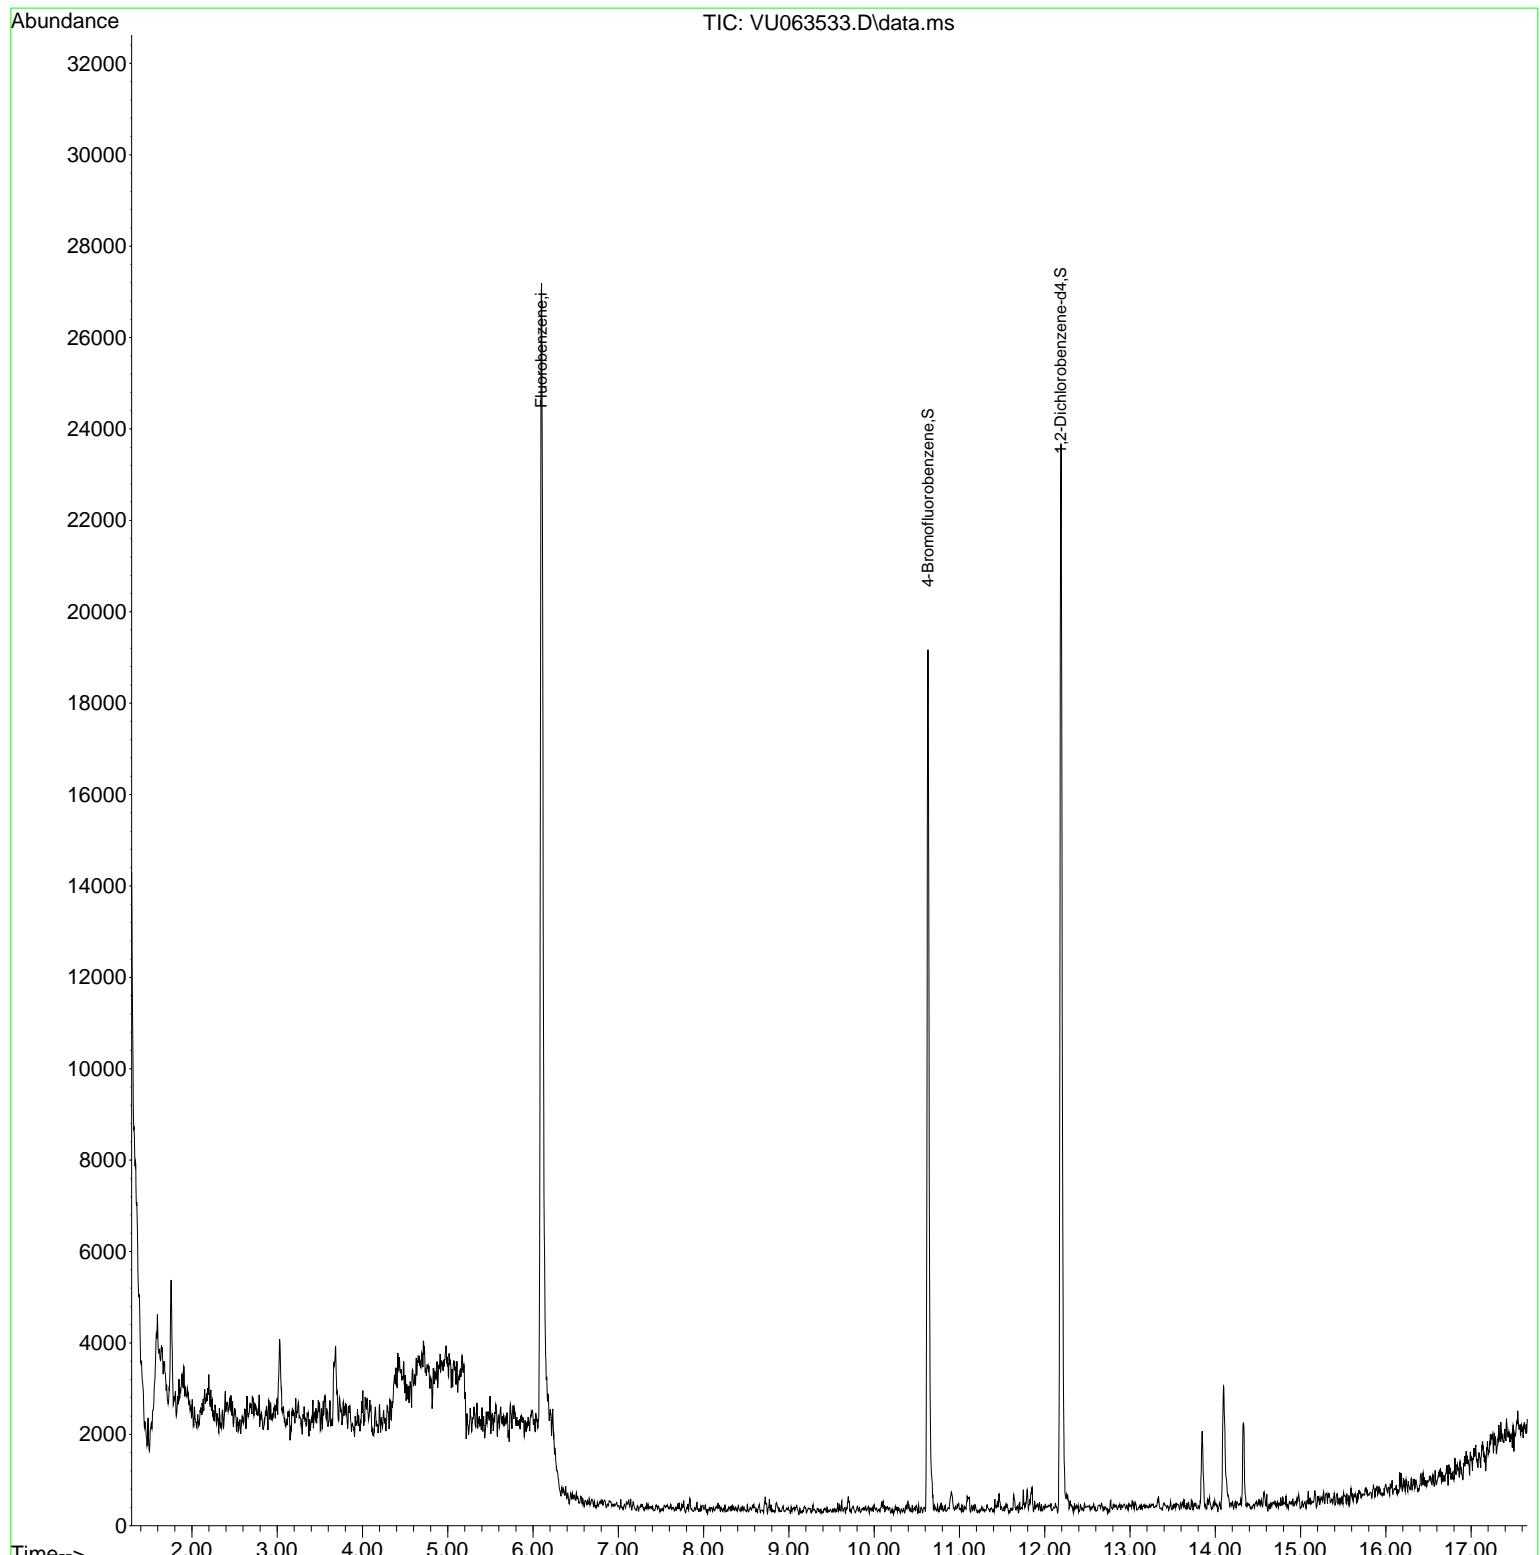


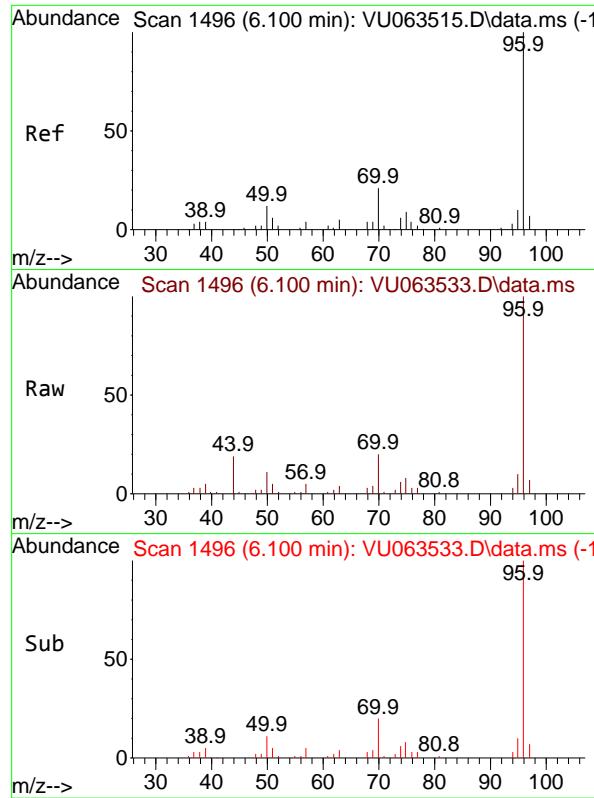

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063533.D
Acq: 18 Jul 2025 10:49


Instrument : MSVOA_U
ClientSampleId : VU0718WBL01


Tgt Ion: 96 Resp: 25256
Ion Ratio Lower Upper
96 100
70 17.9 15.0 22.4
95 8.9 7.4 11.0
97 5.1 0.0 0.0#

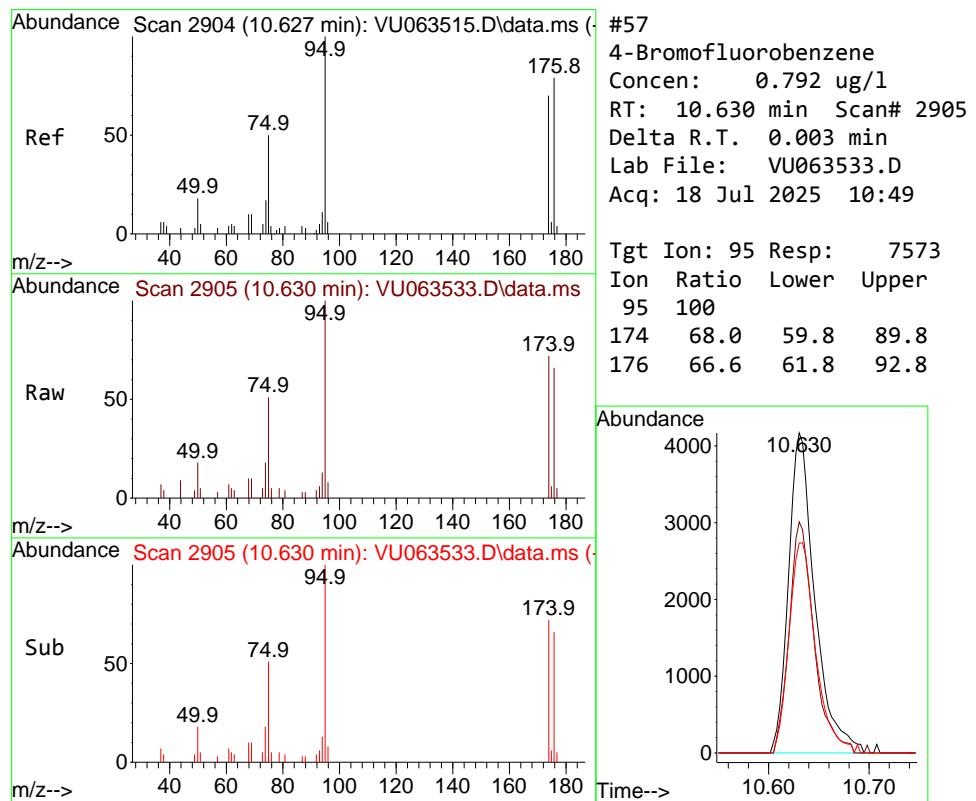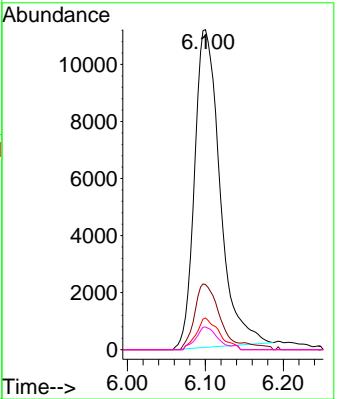

#57
4-Bromofluorobenzene
Concen: 0.792 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063533.D
Acq: 18 Jul 2025 10:49

Tgt Ion: 95 Resp: 7573
Ion Ratio Lower Upper
95 100
174 68.0 59.8 89.8
176 66.6 61.8 92.8

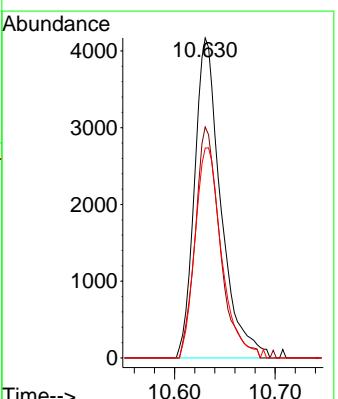

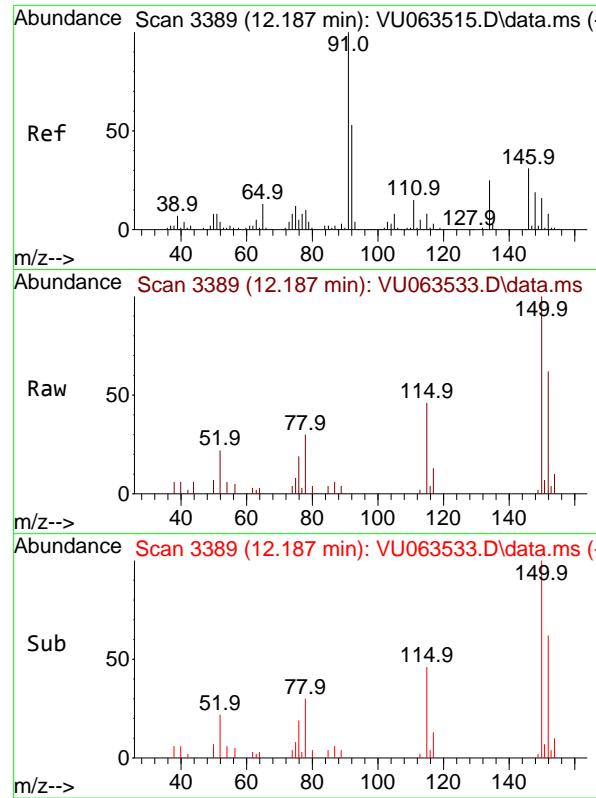

#68

1,2-Dichlorobenzene-d4

Concen: 0.722 ug/l

RT: 12.187 min Scan# 3

Instrument:

MSVOA_U

Delta R.T. 0.000 min

ClientSampleId :

Lab File: VU063533.D

Acq: 18 Jul 2025 10:49

VU0718WBL01


Tgt Ion:152 Resp: 6388

Ion Ratio Lower Upper

152 100

115 71.0 0.0 262.2

150 165.4 0.0 651.2

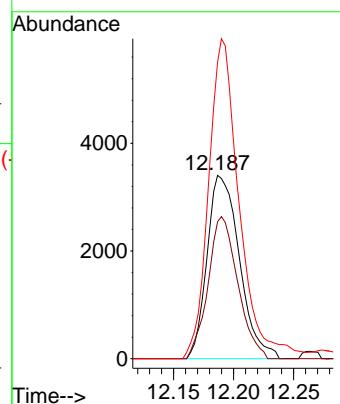



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBS01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBS01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063521.D	1	07/17/25 12:43	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	1.90		0.12	0.50	ug/L
74-87-3	Chloromethane	2.20		0.13	0.50	ug/L
75-01-4	Vinyl Chloride	2.00		0.12	0.50	ug/L
74-83-9	Bromomethane	2.30		0.15	0.50	ug/L
75-00-3	Chloroethane	2.00		0.14	0.50	ug/L
109-99-9	Tetrahydrofuran	4.70		0.42	1.00	ug/L
75-69-4	Trichlorofluoromethane	2.10		0.20	0.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	2.00		0.11	0.50	ug/L
75-65-0	tert-Butyl Alcohol	20.3		3.60	10.0	ug/L
60-29-7	Diethyl Ether	2.10		0.13	0.50	ug/L
75-35-4	1,1-Dichloroethene	2.10		0.13	0.50	ug/L
107-13-1	Acrylonitrile	4.00		0.44	1.00	ug/L
67-64-1	Acetone	12.8		0.97	2.50	ug/L
75-15-0	Carbon Disulfide	1.80		0.12	0.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	2.10		0.11	0.50	ug/L
96-33-3	Methyl acrylate	1.90		0.33	0.50	ug/L
75-09-2	Methylene Chloride	2.30		0.44	0.50	ug/L
156-60-5	trans-1,2-Dichloroethene	2.00		0.14	0.50	ug/L
75-34-3	1,1-Dichloroethane	2.10		0.13	0.50	ug/L
110-82-7	Cyclohexane	2.10		0.14	0.50	ug/L
78-93-3	2-Butanone	11.2		0.72	2.50	ug/L
56-23-5	Carbon Tetrachloride	1.90		0.13	0.50	ug/L
594-20-7	2,2-Dichloropropane	2.00		0.12	0.50	ug/L
156-59-2	cis-1,2-Dichloroethene	2.10		0.13	0.50	ug/L
74-97-5	Bromoform	2.10		0.17	0.50	ug/L
67-66-3	Chloroform	2.10		0.17	0.50	ug/L
71-55-6	1,1,1-Trichloroethane	2.00		0.12	0.50	ug/L
108-87-2	Methylcyclohexane	1.80		0.090	0.50	ug/L
563-58-6	1,1-Dichloropropene	2.10		0.11	0.50	ug/L
107-12-0	Propionitrile	10.4		1.20	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBS01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBS01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063521.D	1	07/17/25 12:43	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	2.20		0.11	0.50	ug/L
107-06-2	1,2-Dichloroethane	2.20		0.14	0.50	ug/L
79-01-6	Trichloroethene	1.80		0.13	0.50	ug/L
78-87-5	1,2-Dichloropropane	1.90		0.13	0.50	ug/L
109-69-3	1-Chlorobutane	2.10		0.12	0.50	ug/L
74-95-3	Dibromomethane	1.80		0.15	0.50	ug/L
75-27-4	Bromodichloromethane	1.80		0.13	0.50	ug/L
108-10-1	4-Methyl-2-Pentanone	9.70		0.63	2.50	ug/L
108-88-3	Toluene	1.90		0.11	0.50	ug/L
10061-02-6	t-1,3-Dichloropropene	1.60		0.11	0.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	1.70		0.11	0.50	ug/L
79-00-5	1,1,2-Trichloroethane	2.00		0.13	0.50	ug/L
142-28-9	1,3-Dichloropropane	2.00		0.12	0.50	ug/L
591-78-6	2-Hexanone	10.2		0.65	2.50	ug/L
124-48-1	Dibromochloromethane	1.80		0.20	0.50	ug/L
106-93-4	1,2-Dibromoethane	1.90		0.13	0.50	ug/L
127-18-4	Tetrachloroethene	1.90		0.14	0.50	ug/L
108-90-7	Chlorobenzene	1.90		0.11	0.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	1.70		0.13	0.50	ug/L
67-72-1	Hexachloroethane	1.60		0.12	0.50	ug/L
100-41-4	Ethyl Benzene	1.90		0.41	0.50	ug/L
179601-23-1	m/p-Xylenes	3.80		0.73	1.00	ug/L
1330-20-7	Total Xylenes	5.80		1.09	1.50	ug/L
95-47-6	o-Xylene	2.00		0.36	0.50	ug/L
100-42-5	Styrene	1.90		0.38	0.50	ug/L
75-25-2	Bromoform	1.60		0.31	0.50	ug/L
98-82-8	Isopropylbenzene	2.00		0.38	0.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	1.90		0.13	0.50	ug/L
96-18-4	1,2,3-Trichloropropane	1.90		0.19	0.50	ug/L
108-86-1	Bromobenzene	1.90		0.13	0.50	ug/L
103-65-1	n-propylbenzene	2.00		0.42	0.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBS01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBS01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063521.D	1	07/17/25 12:43	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	2.00		0.27	0.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	1.90		0.37	0.50	ug/L
106-43-4	4-Chlorotoluene	2.00		0.27	0.50	ug/L
98-06-6	tert-Butylbenzene	1.90		0.37	0.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	1.90		0.40	0.50	ug/L
135-98-8	sec-Butylbenzene	2.00		0.36	0.50	ug/L
99-87-6	p-Isopropyltoluene	2.00		0.42	0.50	ug/L
541-73-1	1,3-Dichlorobenzene	1.90		0.13	0.50	ug/L
106-46-7	1,4-Dichlorobenzene	1.90		0.13	0.50	ug/L
104-51-8	n-Butylbenzene	2.00		0.43	0.50	ug/L
95-50-1	1,2-Dichlorobenzene	1.90		0.14	0.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	1.70		0.24	0.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	1.90		0.21	0.50	ug/L
87-68-3	Hexachlorobutadiene	1.90		0.14	0.50	ug/L
91-20-3	Naphthalene	1.80		0.33	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	1.80		0.31	0.50	ug/L
98-95-3	Nitrobenzene	11.7		1.80	5.00	ug/L
363-72-4	Pentachloroethane	1.70		0.16	0.50	ug/L
74-88-4	Iodomethane	1.80		0.090	1.00	ug/L
107-05-1	Allyl Chloride	2.00		0.13	0.50	ug/L
126-98-7	Methacrylonitrile	1.90		0.24	0.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	3.40		0.21	1.00	ug/L
97-63-2	Ethyl methacrylate	1.90		0.12	0.50	ug/L
108-20-3	Isopropyl Ether	2.10		0.14	0.50	ug/L
80-62-6	Methyl methacrylate	3.50		0.24	1.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	0.94		70 - 130	94%	SPK: 1
460-00-4	4-Bromofluorobenzene	1.00		70 - 130	100%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	21900	6.097			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBS01	SDG No.:		Q2552
Lab Sample ID:	VU0717WBS01	Matrix:	Water	
Analytical Method:	E524.2	% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol: 25000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063521.D	1	07/17/25 12:43	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063521.D
 Acq On : 17 Jul 2025 12:43
 Operator : MD/SY
 Sample : VU0717WBS01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0717WBS01

Quant Time: Jul 18 04:10:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	21864	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.628	95	8236	0.995	ug/l	0.00
Spiked Amount 1.000			Recovery	=	99.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	7166	0.936	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.381	85	12281	1.905	ug/l	98
3) Chloromethane	1.519	50	12925	2.157	ug/l	98
4) Vinyl Chloride	1.599	62	15376	2.015	ug/l	100
5) Bromomethane	1.847	94	13111	2.278	ug/l	94
6) Chloroethane	1.927	64	9342	2.027	ug/l	100
7) Trichlorofluoromethane	2.130	101	22634	2.065	ug/l	100
8) 1,1,2-Trichloro-1,2,2-...	2.570	101	11730	2.048	ug/l	99
9) 1,1-Dichloroethene	2.567	96	11724	2.065	ug/l	97
10) Iodomethane	2.708	142	8006	1.773	ug/l	97
11) Allyl Chloride	2.908	41	16576	2.021	ug/l	98
12) Acrylonitrile	3.306	53	5711	4.023	ug/l	98
13) Acetone	2.622	43	14599	12.835	ug/l	98
14) Carbon Disulfide	2.779	76	33865	1.847	ug/l	98
15) Methylene Chloride	3.030	84	15114	2.262	ug/l	97
16) trans-1,2-Dichloroethene	3.335	96	12801	1.986	ug/l	96
17) 1,1-Dichloroethane	3.850	63	24869	2.081	ug/l	99
18) 2-Butanone	4.718	43	19663	11.163	ug/l	95
19) Cyclohexane	5.358	56	20801	2.056	ug/l	99
20) Methylcyclohexane	6.740	83	17274	1.757	ug/l	98
21) 2,2-Dichloropropane	4.641	77	20379	2.003	ug/l	99
22) cis-1,2-Dichloroethene	4.647	96	14565	2.082	ug/l	99
23) Diethyl Ether	2.371	59	9050	2.092	ug/l	96
24) tert-Butyl Alcohol	3.197	59	10601	20.303	ug/l	100
25) Methyl tert-Butyl Ether	3.361	73	31377	2.117	ug/l	99
26) Bromochloromethane	4.956	128	6000	2.054	ug/l	93
27) Chloroform	5.072	83	25113	2.060	ug/l	99
28) 1,1,1-Trichloroethane	5.294	97	20838	2.014	ug/l	99
29) 1,1-Dichloropropene	5.506	75	20417	2.130	ug/l	97
30) Carbon Tetrachloride	5.499	117	16009	1.922	ug/l	95
31) Isopropyl Ether	3.995	45	38467	2.133	ug/l	97
32) Ethyl-t-butyl ether	4.506	59	35330	2.117	ug/l	98
33) Tert-Amyl methyl ether	5.943	73	30771	2.124	ug/l	99
34) Propionitrile	4.782	54	5569	10.376	ug/l	# 92
35) Benzene	5.753	78	55862	2.169	ug/l	94
36) 1,2-Dichloroethane	5.779	62	17638	2.204	ug/l	100
37) Trichloroethene	6.525	130	11954	1.819	ug/l	99
38) 1,2-Dichloropropane	6.779	63	11421	1.895	ug/l	99
39) Methacrylonitrile	4.972	41	4514	1.892	ug/l	95
40) Methyl acrylate	4.850	55	6649	1.907	ug/l	# 97
41) Tetrahydrofuran	5.062	42	5866	4.674	ug/l	90
42) 1-Chlorobutane	5.438	56	26277	2.062	ug/l	96
43) Dibromomethane	6.908	93	5740	1.838	ug/l	96
44) Bromodichloromethane	7.097	83	12690	1.802	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063521.D
 Acq On : 17 Jul 2025 12:43
 Operator : MD/SY
 Sample : VU0717WBS01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0717WBS01

Quant Time: Jul 18 04:10:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	31264	9.714	ug/1	99
46) t-1,4-Dichloro-2-butene	10.824	75	4116m	3.407	ug/1	
47) Methyl methacrylate	6.969	69	9287	3.541	ug/1	92
48) Ethyl methacrylate	8.338	69	9397	1.877	ug/1	96
49) Toluene	7.962	92	26503	1.885	ug/1	97
50) t-1,3-Dichloropropene	8.207	75	9090	1.645	ug/1	98
51) cis-1,3-Dichloropropene	7.602	75	12550	1.692	ug/1	96
52) 1,1,2-Trichloroethane	8.393	97	8229	1.957	ug/1	95
53) 1,3-Dichloropropane	8.570	76	14200	1.956	ug/1	99
54) 2-Hexanone	8.692	43	21798	10.196	ug/1	99
55) Dibromochloromethane	8.801	129	7818	1.760	ug/1	100
56) 1,2-Dibromoethane	8.917	107	7165	1.904	ug/1	100
58) Tetrachloroethene	8.541	164	11402	1.896	ug/1	98
59) Chlorobenzene	9.441	112	30941	1.916	ug/1	97
60) 1,1,1,2-Tetrachloroethane	9.525	131	8917	1.717	ug/1	92
61) Pentachloroethane	11.419	117	6375	1.737	ug/1	88
62) Hexachloroethane	12.467	117	5976	1.644	ug/1	99
63) Ethyl Benzene	9.563	91	53621	1.929	ug/1	99
64) m/p-Xylenes	9.686	106	40731	3.770	ug/1	98
65) o-Xylene	10.094	106	20319	1.957	ug/1	97
66) Styrene	10.110	104	31561	1.908	ug/1	98
67) Bromoform	10.284	173	3644	1.597	ug/1	99
69) Isopropylbenzene	10.477	105	48988	1.952	ug/1	100
70) 1,1,2,2-Tetrachloroethane	10.776	83	9968	1.948	ug/1	98
71) 1,2,3-Trichloropropane	10.814	75	7776m	1.871	ug/1	
72) Bromobenzene	10.776	156	12098	1.868	ug/1	92
73) n-propylbenzene	10.898	120	14781	1.956	ug/1	93
74) 2-Chlorotoluene	10.978	126	13064	1.957	ug/1	91
75) 1,3,5-Trimethylbenzene	11.081	105	46460	1.938	ug/1	100
76) 4-Chlorotoluene	11.091	126	13377	1.973	ug/1	97
77) tert-Butylbenzene	11.412	119	43549	1.901	ug/1	96
78) 1,2,4-Trimethylbenzene	11.460	105	46303	1.947	ug/1	96
79) sec-Butylbenzene	11.634	105	61626	1.994	ug/1	98
80) Nitrobenzene	13.219	77	968m	11.740	ug/1	
81) p-Isopropyltoluene	11.785	119	50943	1.975	ug/1	99
82) 1,3-Dichlorobenzene	11.740	146	24826	1.916	ug/1	99
83) 1,4-Dichlorobenzene	11.830	146	25218	1.944	ug/1	98
84) n-Butylbenzene	12.203	91	48117	2.011	ug/1	98
85) 1,2-Dichlorobenzene	12.206	146	23502	1.930	ug/1	97
86) 1,2-Dibromo-3-Chloropr...	12.988	75	1114	1.706	ug/1	94
87) 1,2,4-Trichlorobenzene	13.837	180	14007	1.850	ug/1	98
88) Hexachlorobutadiene	14.013	225	8260	1.921	ug/1	97
89) Naphthalene	14.087	128	24449	1.802	ug/1	98
90) 1,2,3-Trichlorobenzene	14.325	180	12843	1.836	ug/1	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063521.D
Acq On : 17 Jul 2025 12:43
Operator : MD/SY
Sample : VU0717WBS01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1


Quant Time: Jul 18 04:10:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBS01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

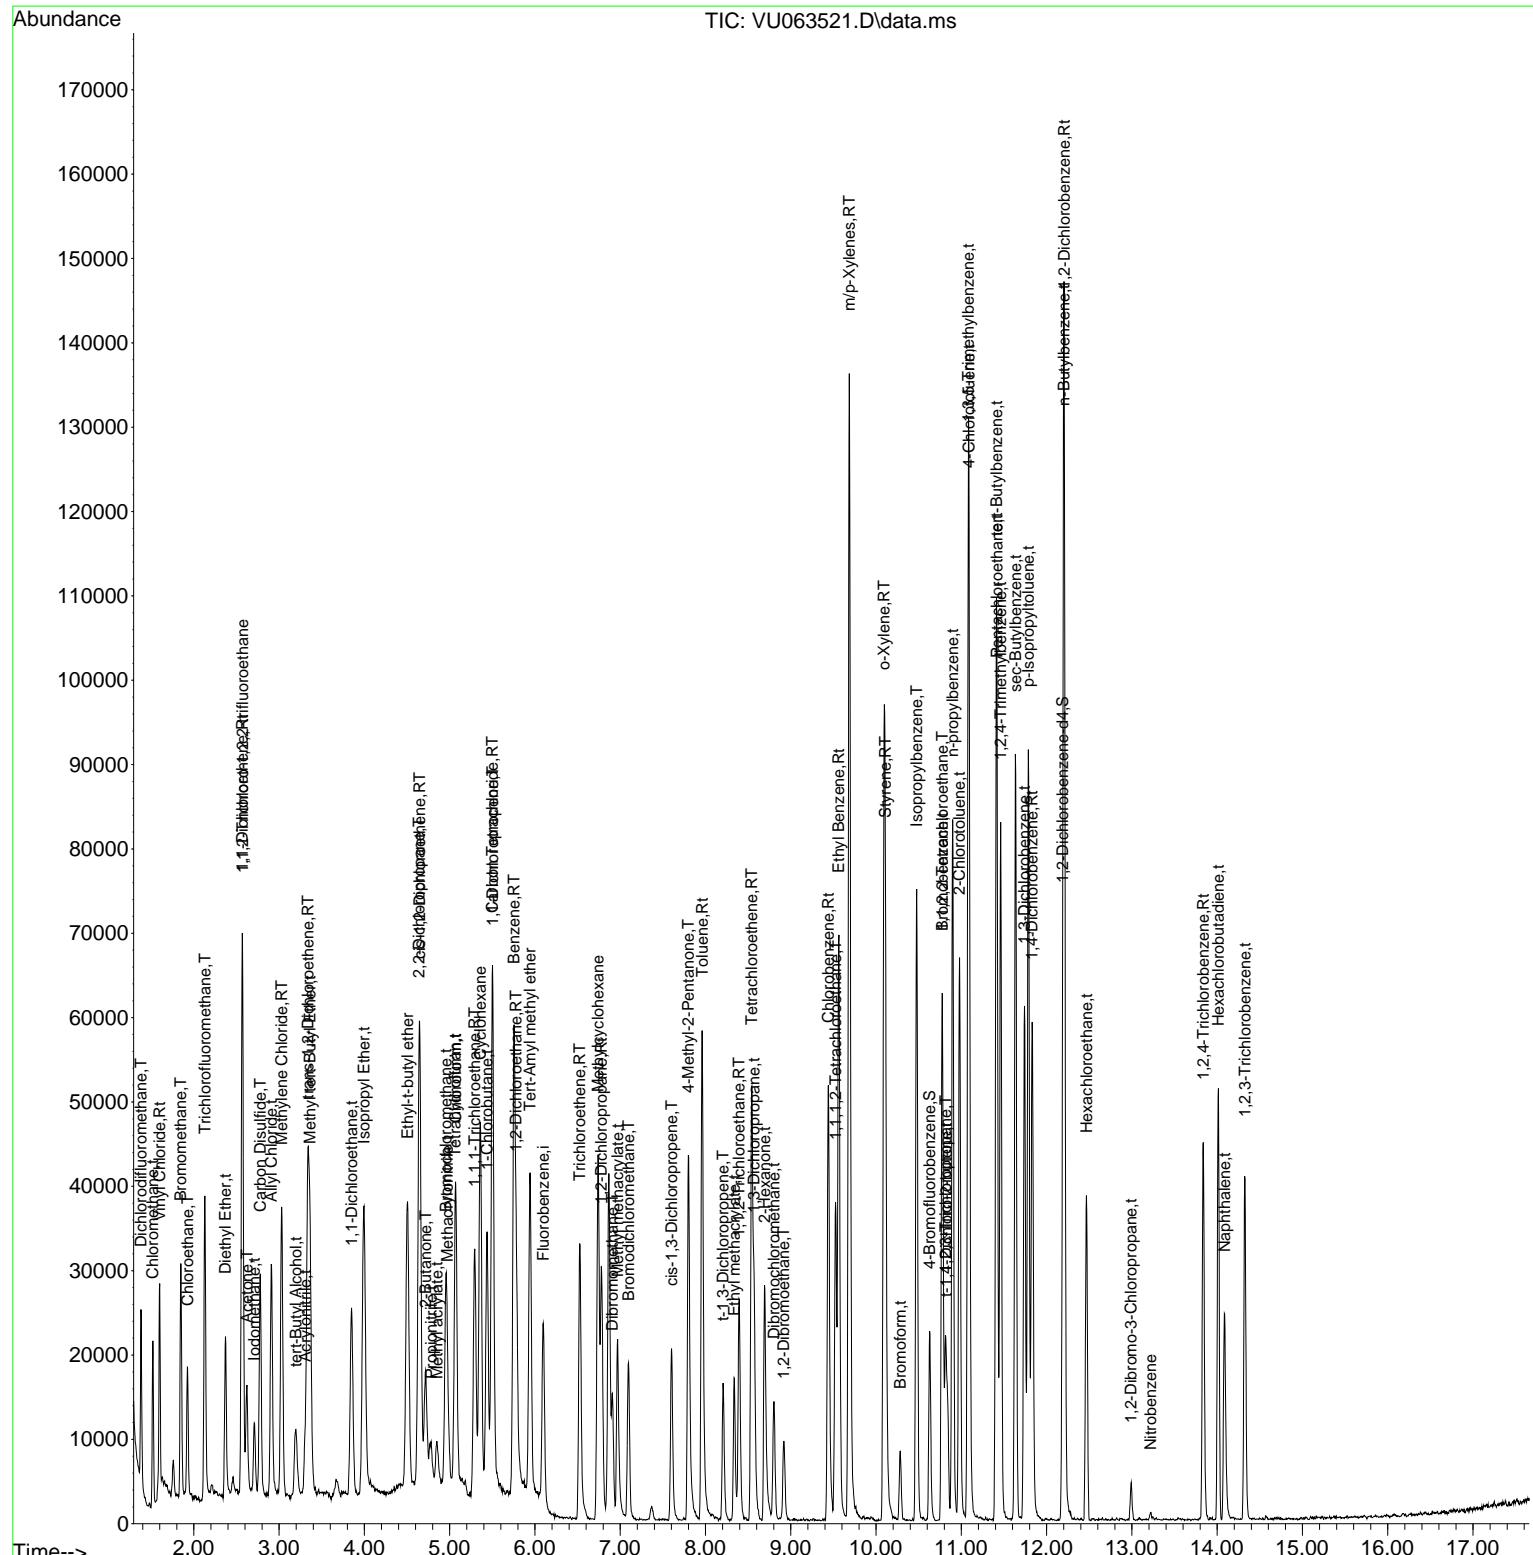



#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01




Tgt Ion: 96 Resp: 21864
Ion Ratio Lower Upper

96	100
70	20.9
95	8.5
97	6.4
	0.0
	0.0

#

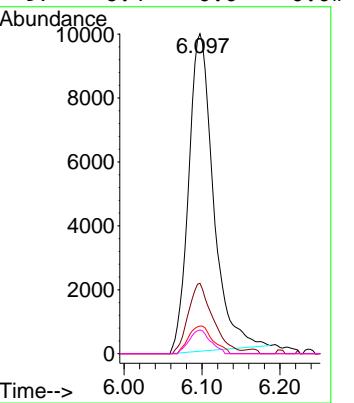
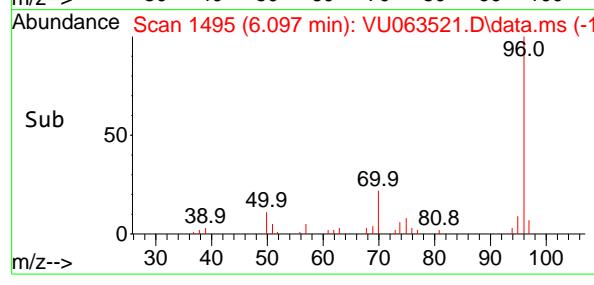



#2
Dichlorodifluoromethane
Concen: 1.905 ug/l
RT: 1.381 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43





Tgt Ion: 85 Resp: 12281
Ion Ratio Lower Upper

85	100
87	30.9
	16.0
	47.9

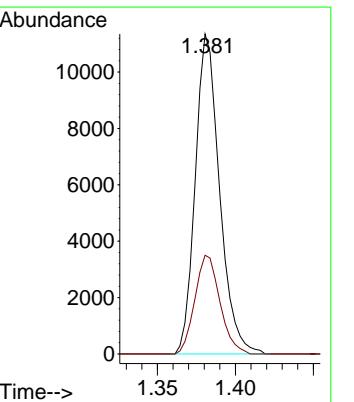




Abundance Scan 71 (1.519 min): VU063521.D\data.ms

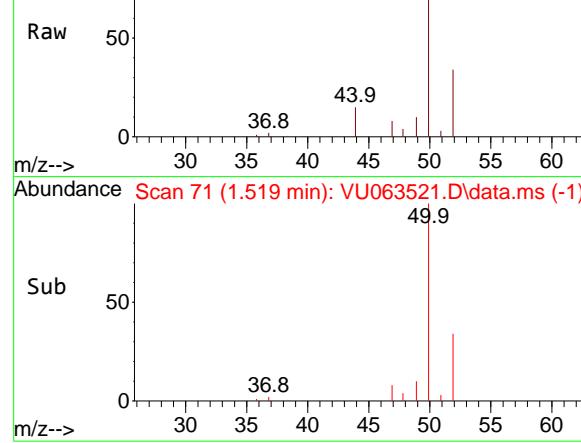

Abundance Scan 96 (1.599 min): VU063521.D\data.ms

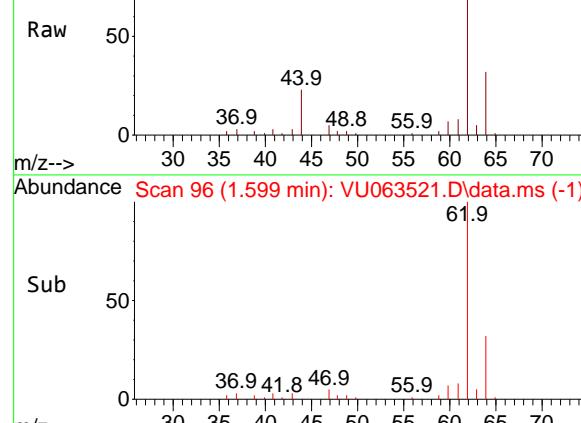

Abundance Scan 96 (1.599 min): VU063521.D\data.ms (-1)

#3

Chloromethane

Concen: 2.157 ug/l

RT: 1.519 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

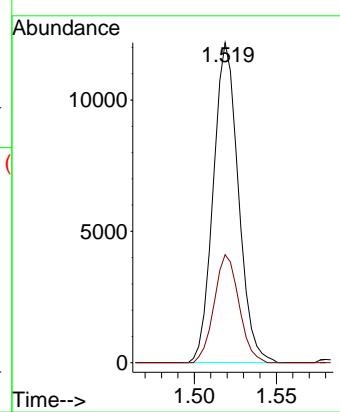 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#4

Vinyl Chloride


Concen: 2.015 ug/l




RT: 1.599 min Scan# 96

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

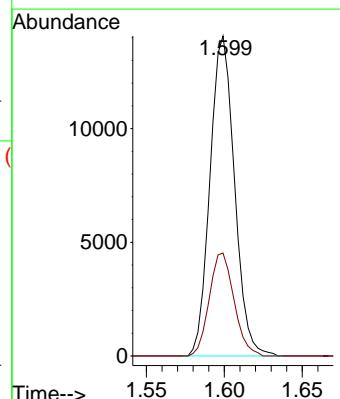 Tgt Ion: 62 Resp: 15376
 Ion Ratio Lower Upper
 62 100
 64 32.2 25.7 38.5

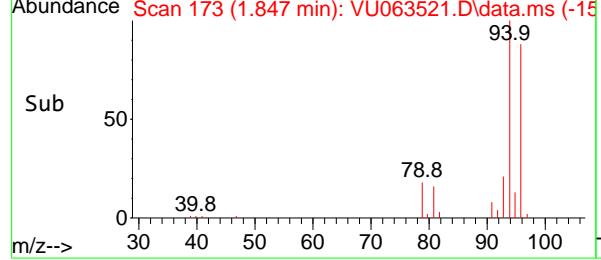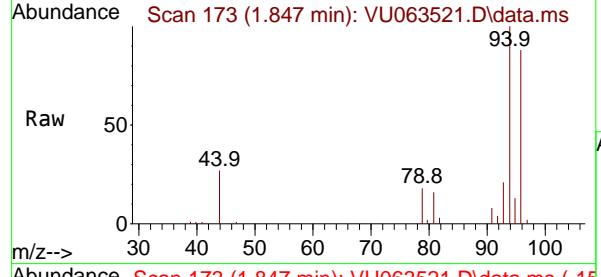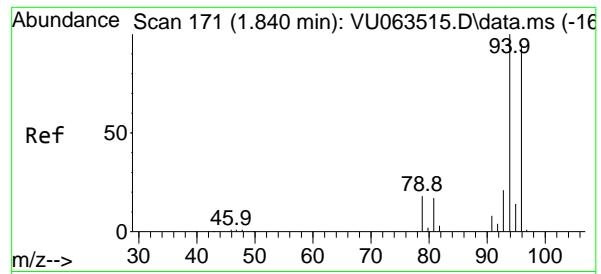
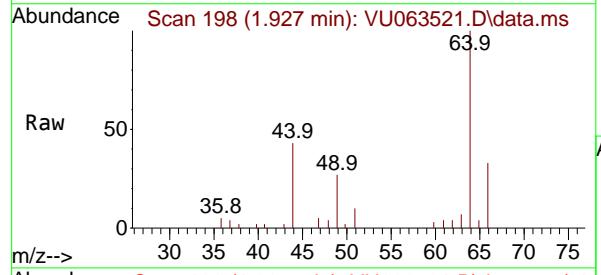
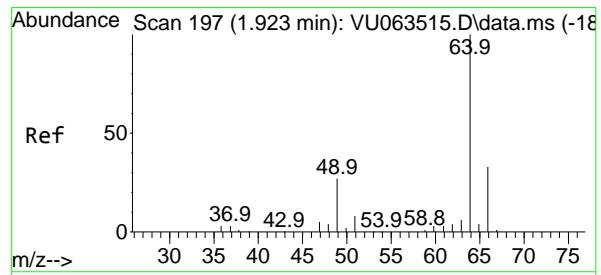
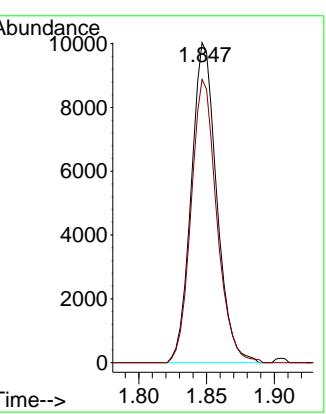


#5
 Bromomethane
 Concen: 2.278 ug/l
 RT: 1.847 min Scan# 1
 Delta R.T. 0.007 min
 Lab File: VU063521.D
 Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
 ClientSampleId : VU0717WBS01



Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025



#6
 Chloroethane
 Concen: 2.027 ug/l
 RT: 1.927 min Scan# 198
 Delta R.T. 0.004 min
 Lab File: VU063521.D
 Acq: 17 Jul 2025 12:43

Tgt Ion: 64 Resp: 9342
 Ion Ratio Lower Upper
 64 100
 66 32.9 26.2 39.4

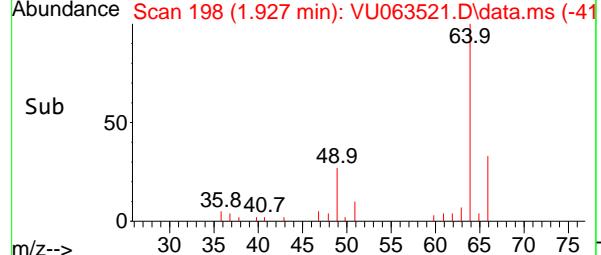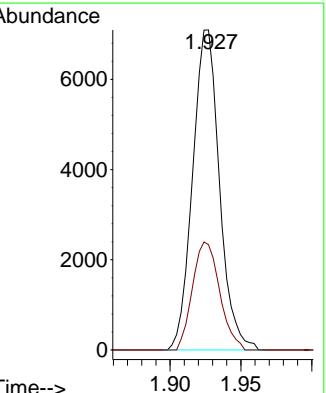

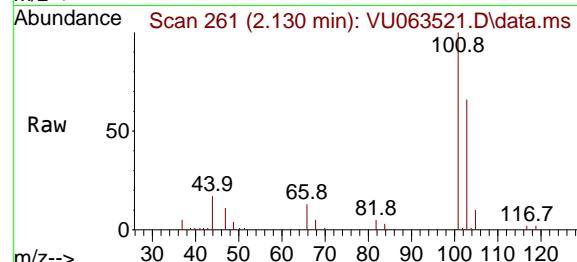


#7

Trichlorofluoromethane
Concen: 2.065 ug/l
RT: 2.130 min Scan# 2
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

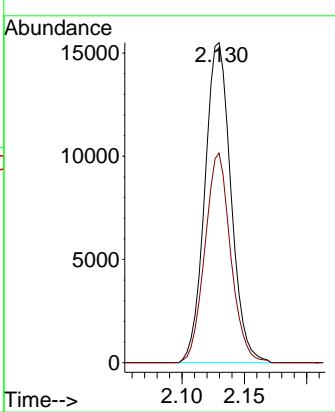


#8

1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 2.048 ug/l
RT: 2.570 min Scan# 398
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43


Tgt Ion:101 Resp: 11730
Ion Ratio Lower Upper
101 100
85 47.0 37.8 56.6
151 75.9 59.2 88.8

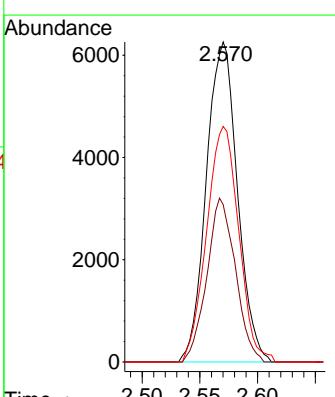



#9
1,1-Dichloroethene
Concen: 2.065 ug/l
RT: 2.567 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01




Tgt Ion: 96 Resp: 11724
Ion Ratio Lower Upper
96 100
61 173.6 0.0 504.3
98 64.2 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

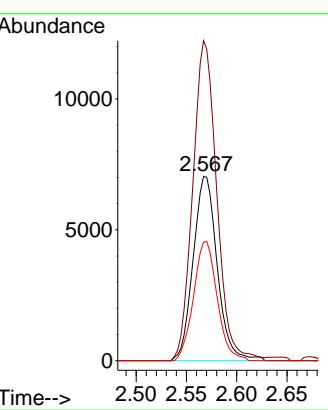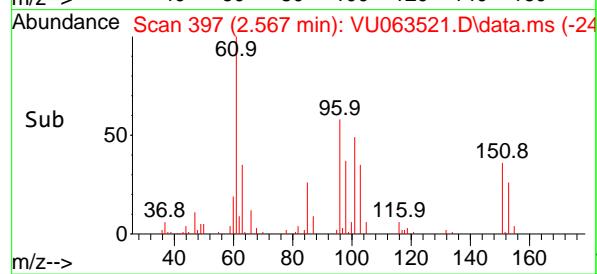


#10
Iodomethane
Concen: 1.773 ug/l
RT: 2.708 min Scan# 441
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Tgt Ion:142 Resp: 8006
Ion Ratio Lower Upper
142 100
127 49.2 37.9 56.9

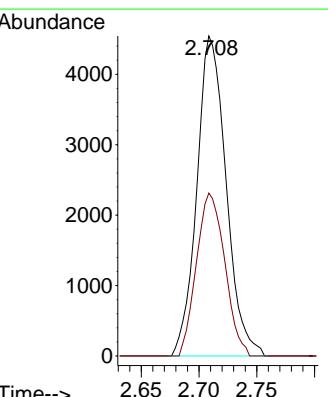



#11
Allyl Chloride
Concen: 2.021 ug/l
RT: 2.908 min Scan# 5
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

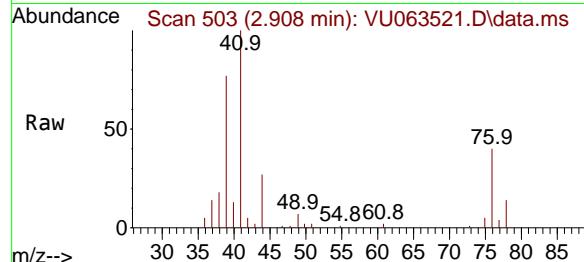


Tgt Ion: 41 Resp: 16570
Ion Ratio Lower Upper
41 100
39 75.4 61.5 92.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

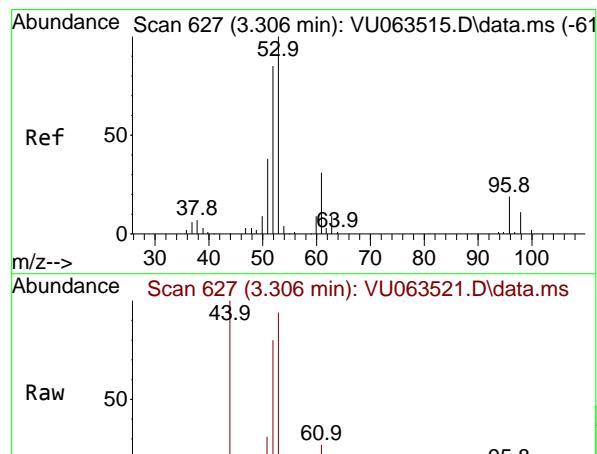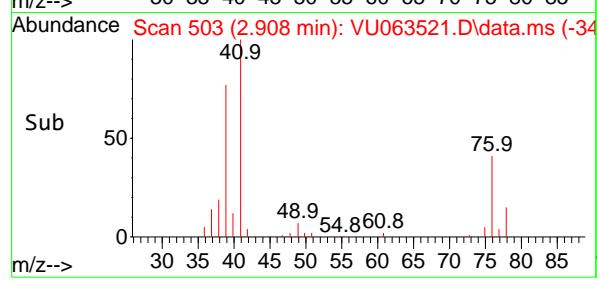


#12
Acrylonitrile
Concen: 4.023 ug/l
RT: 3.306 min Scan# 627
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Tgt Ion: 53 Resp: 5711
Ion Ratio Lower Upper
53 100
52 82.6 64.3 96.5
51 36.1 27.8 41.8

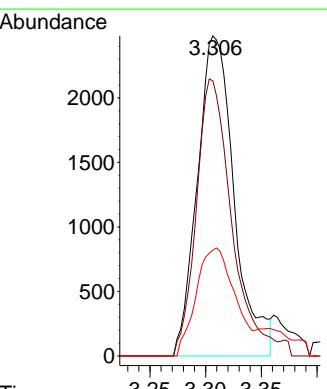



#13
Acetone
Concen: 12.835 ug/l
RT: 2.622 min Scan# 4
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01




Tgt Ion: 43 Resp: 14599
Ion Ratio Lower Upper
43 100
58 32.7 25.4 38.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025





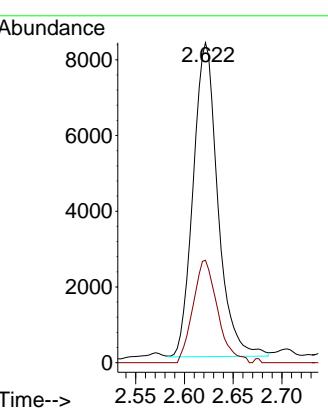



#14
Carbon Disulfide
Concen: 1.847 ug/l
RT: 2.779 min Scan# 463
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43



Tgt Ion: 76 Resp: 33865
Ion Ratio Lower Upper
76 100
78 8.2 7.0 10.6



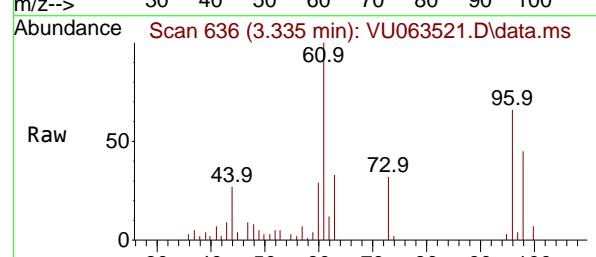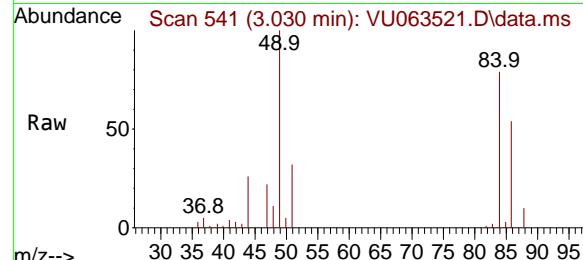

#15

Methylene Chloride

Concen: 2.262 ug/l

RT: 3.030 min Scan# 5

Delta R.T. 0.000 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43

Instrument :

MSVOA_U

ClientSampleId :

VU0717WBS01

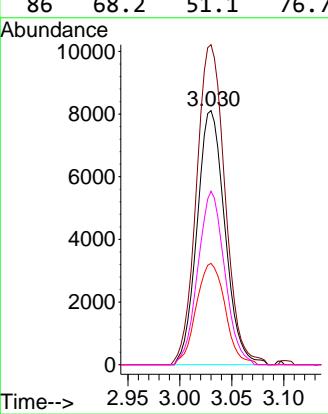**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#16

trans-1,2-Dichloroethene

Concen: 1.986 ug/l

RT: 3.335 min Scan# 636


Delta R.T. 0.000 min




Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Tgt Ion: 96 Resp: 12801

Ion	Ratio	Lower	Upper
96	100		
61	151.1	117.2	175.8
98	68.7	51.4	77.2

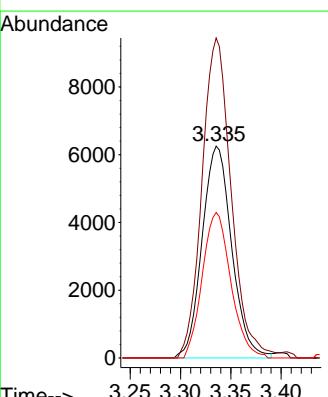



#17

1,1-Dichloroethane

Concen: 2.081 ug/l

RT: 3.850 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43




Instrument:

MSVOA_U

ClientSampleId :


VU0717WBS01


**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#18
2-Butanone
Concen: 11.163 ug/l
RT: 4.718 min Scan# 1066
Delta R.T. 0.007 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion: 43 Resp: 19663
Ion Ratio Lower Upper
43 100
57 10.1 0.0 16.4

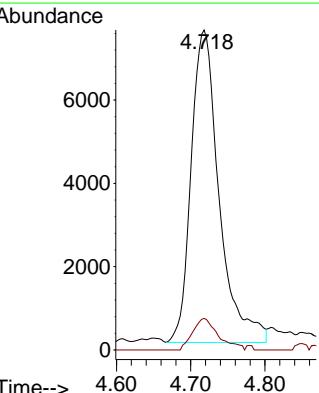

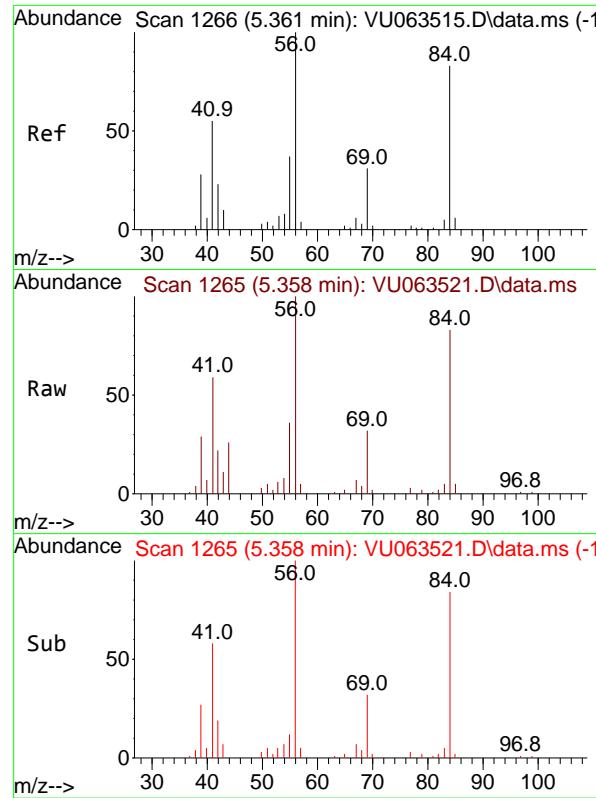

#19

Cyclohexane

Concen: 2.056 ug/l

RT: 5.358 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

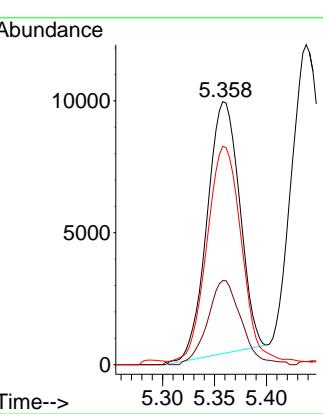 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#20

Methylcyclohexane



Concen: 1.757 ug/l







RT: 6.740 min Scan# 1695

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

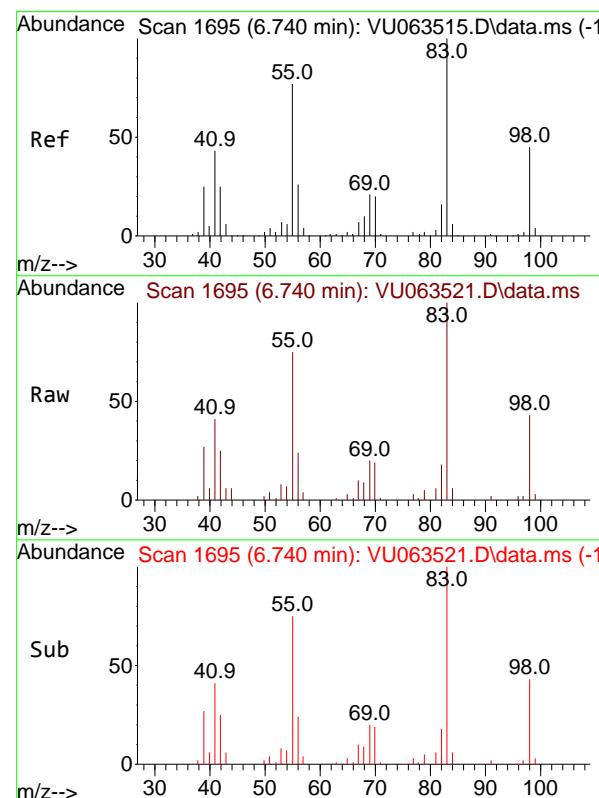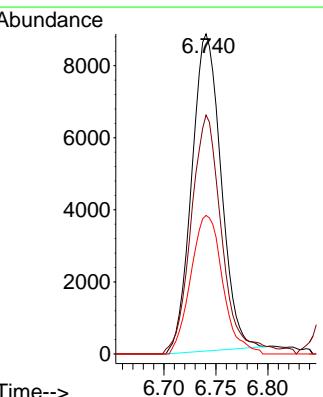 Tgt Ion: 83 Resp: 17274
 Ion Ratio Lower Upper
 83 100
 55 76.1 60.6 90.8
 98 47.5 35.8 53.8

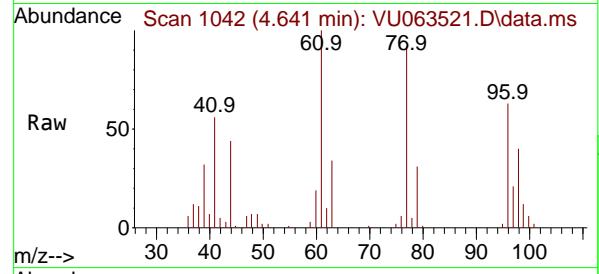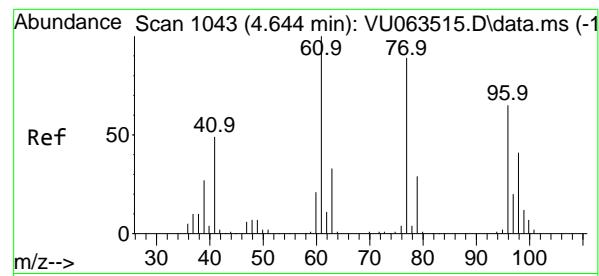


#21

2,2-Dichloropropane

Concen: 2.003 ug/l

RT: 4.641 min Scan# 1042

Delta R.T. -0.003 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43

Instrument :

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#22

cis-1,2-Dichloroethene

Concen: 2.082 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Tgt Ion: 96 Resp: 14565




Ion Ratio Lower Upper

96 100

61 152.8 0.0 384.7

98 63.5 32.1 96.3

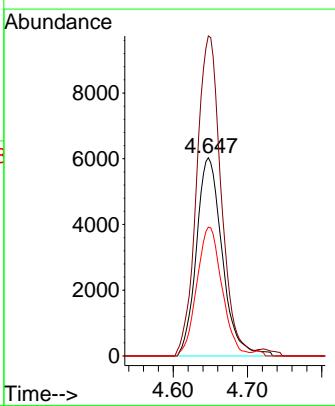

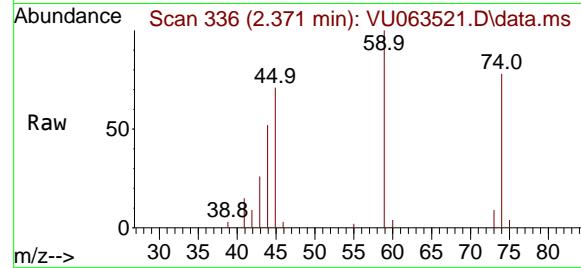

#23

Diethyl Ether

Concen: 2.092 ug/l

RT: 2.371 min Scan# 3

Delta R.T. 0.004 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43




Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#24

tert-Butyl Alcohol

Concen: 20.303 ug/l

RT: 3.197 min Scan# 593

Delta R.T. 0.007 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43







Tgt Ion: 59 Resp: 10601

Ion Ratio Lower Upper

59 100

57 10.5 8.6 12.8






#25

Methyl tert-Butyl Ether
Concen: 2.117 ug/l
RT: 3.361 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#26

Bromochloromethane
Concen: 2.054 ug/l
RT: 4.956 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion:128 Resp: 6000
Ion Ratio Lower Upper
128 100
49 183.5 0.0 340.8
130 130.4 100.5 150.7

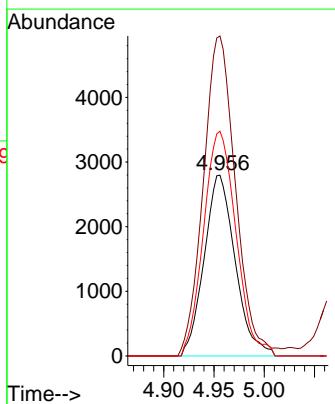






#27
 Chloroform
 Concen: 2.060 ug/l
 RT: 5.072 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU063521.D
 Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
 ClientSampleId : VU0717WBS01


Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025



#28
 1,1,1-Trichloroethane
 Concen: 2.014 ug/l
 RT: 5.294 min Scan# 1245
 Delta R.T. -0.003 min
 Lab File: VU063521.D
 Acq: 17 Jul 2025 12:43

Tgt Ion: 97 Resp: 20838
 Ion Ratio Lower Upper
 97 100
 99 63.5 31.8 95.3
 61 47.6 23.3 69.9




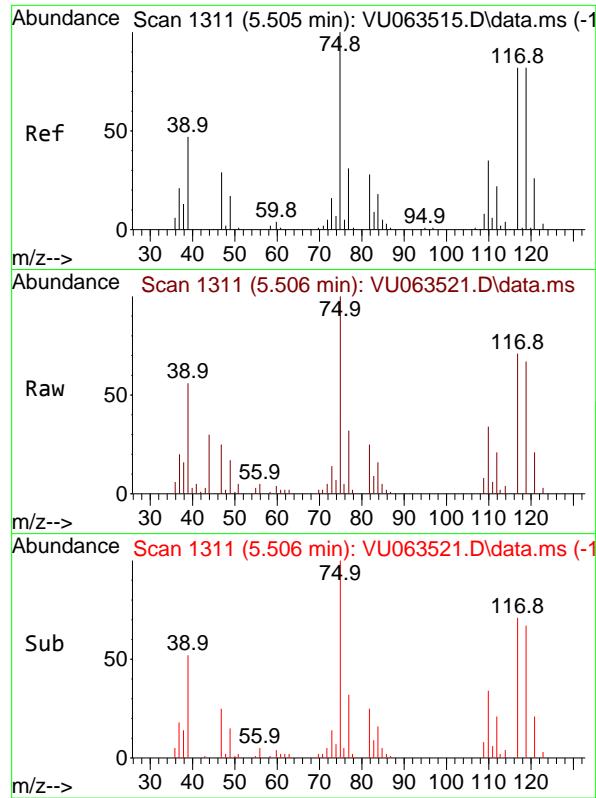


#29
1,1-Dichloropropene
Concen: 2.130 ug/l
RT: 5.506 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

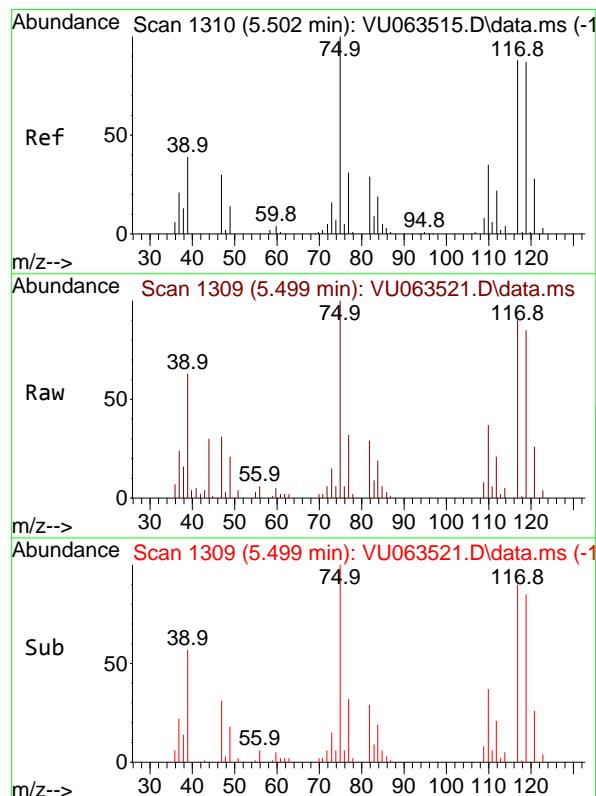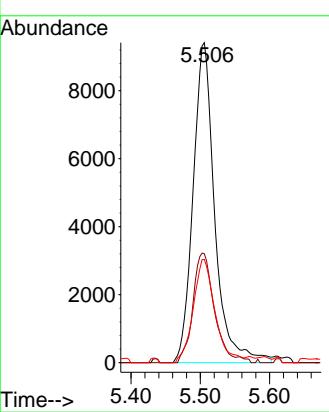

#30
Carbon Tetrachloride
Concen: 1.922 ug/l
RT: 5.499 min Scan# 1309
Delta R.T. -0.003 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion:117 Resp: 16009
Ion Ratio Lower Upper
117 100
119 94.6 79.2 118.8
121 28.9 25.5 38.3

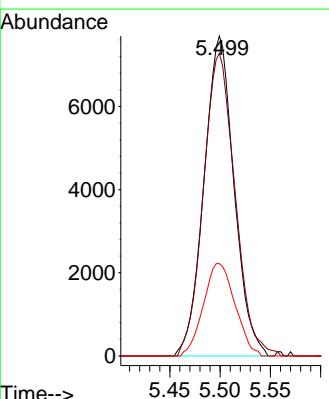



#31

Isopropyl Ether

Concen: 2.133 ug/l

RT: 3.995 min Scan# 8

Instrument:

Delta R.T. 0.004 min

MSVOA_U

Lab File: VU063521.D


ClientSampleId :

Acq: 17 Jul 2025 12:43

VU0717WBS01

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

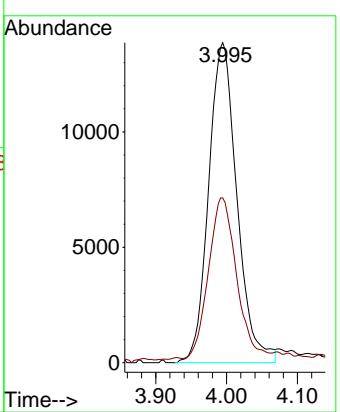**Manual Integrations
APPROVED**


#32

Ethyl-t-butyl ether

Concen: 2.117 ug/l

RT: 4.506 min Scan# 1000

Delta R.T. 0.004 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43




Tgt Ion: 59 Resp: 35330

Ion Ratio Lower Upper

59 100

87 41.9 32.6 49.0

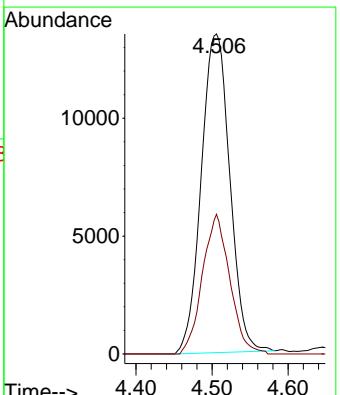

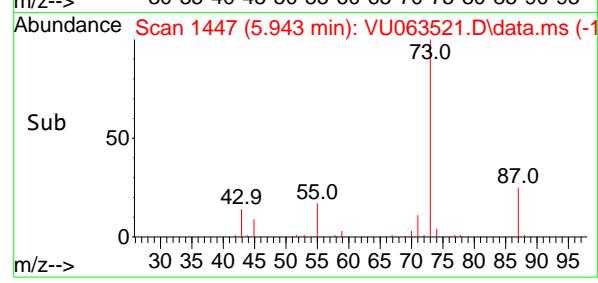




#33

Tert-Amyl methyl ether
Concen: 2.124 ug/l
RT: 5.943 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025




#34

Propionitrile
Concen: 10.376 ug/l
RT: 4.782 min Scan# 1086
Delta R.T. 0.010 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43


Tgt Ion: 54 Resp: 5569
Ion Ratio Lower Upper
54 100
52 18.3 17.0 25.4
55 13.2 13.6 20.4#
40 3.4 6.4 9.6#

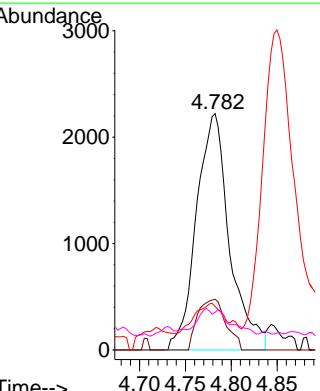



#35
Benzene
Concen: 2.169 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01




Tgt Ion: 78 Resp: 5586
Ion Ratio Lower Upper
78 100
77 27.1 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

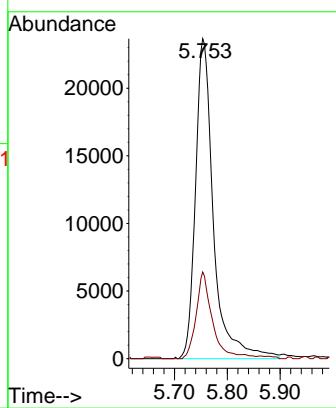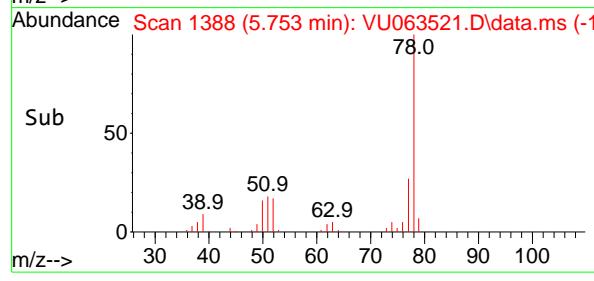


#36
1,2-Dichloroethane
Concen: 2.204 ug/l
RT: 5.779 min Scan# 1396
Delta R.T. -0.003 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Tgt Ion: 62 Resp: 17638
Ion Ratio Lower Upper
62 100
98 8.1 6.4 9.6

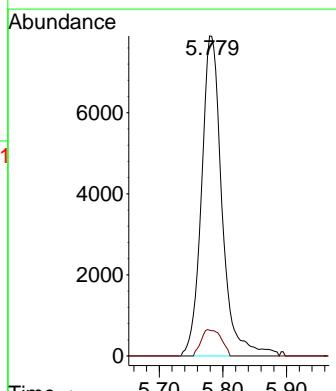



#37
Trichloroethene
Concen: 1.819 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01




Tgt Ion:130 Resp: 11954
Ion Ratio Lower Upper
130 100
95 101.2 80.3 120.5

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


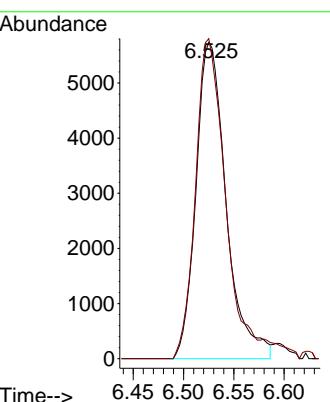
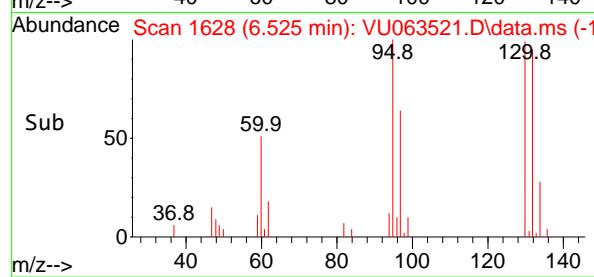


#38
1,2-Dichloropropane
Concen: 1.895 ug/l
RT: 6.779 min Scan# 1707
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43



Tgt Ion: 63 Resp: 11421
Ion Ratio Lower Upper
63 100
65 31.3 24.6 36.8

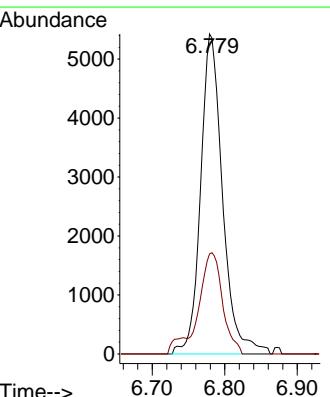

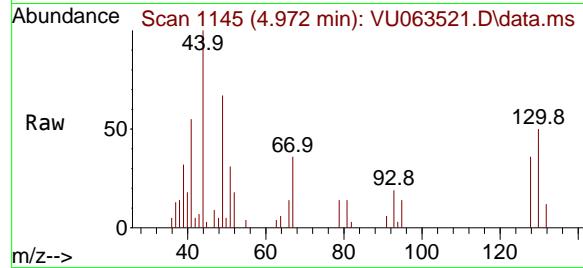

#39

Methacrylonitrile

Concen: 1.892 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43




Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

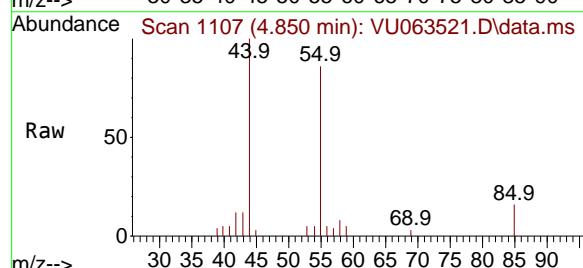 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#40

Methyl acrylate

Concen: 1.907 ug/l

RT: 4.850 min Scan# 1107

Delta R.T. 0.004 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Tgt Ion: 55 Resp: 6649


Ion Ratio Lower Upper




55 100

85 16.7 12.8 19.2

58 9.2 7.0 10.4

42 10.9 7.0 10.4#

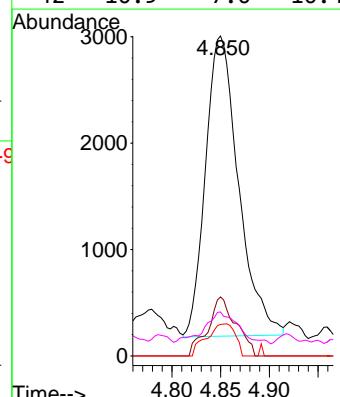

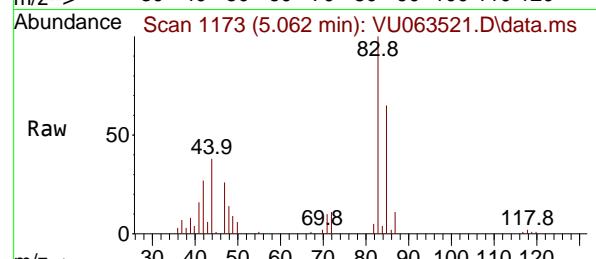

#41

Tetrahydrofuran

Concen: 4.674 ug/l

RT: 5.062 min Scan# 1

Delta R.T. 0.004 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43




Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

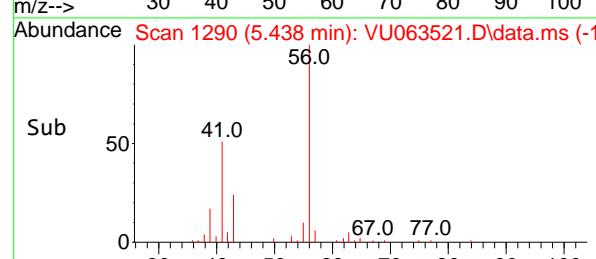 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#42

1-Chlorobutane

Concen: 2.062 ug/l

RT: 5.438 min Scan# 1290

Delta R.T. 0.000 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43


Tgt Ion: 56 Resp: 26277

Ion Ratio Lower Upper

56 100


41 50.5 26.7 80.0



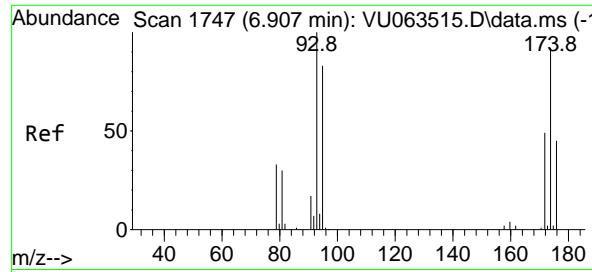

#43
Dibromomethane
Concen: 1.838 ug/l
RT: 6.908 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

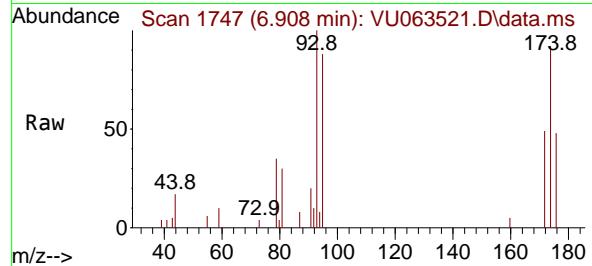

Tgt Ion: 93 Resp: 5740
Ion Ratio Lower Upper
93 100
95 87.8 67.9 101.9
174 88.9 74.6 111.8




Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

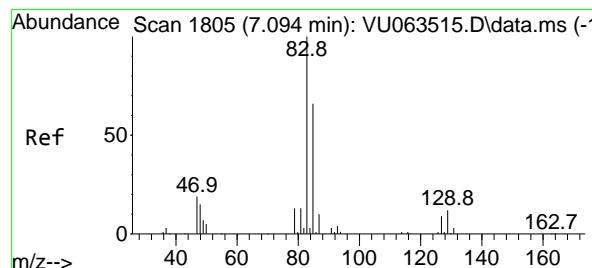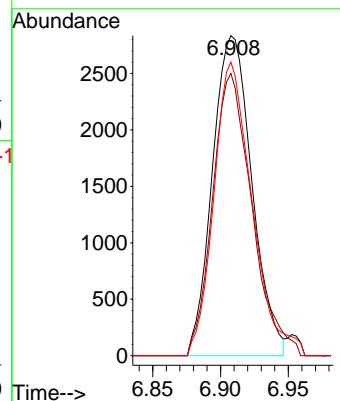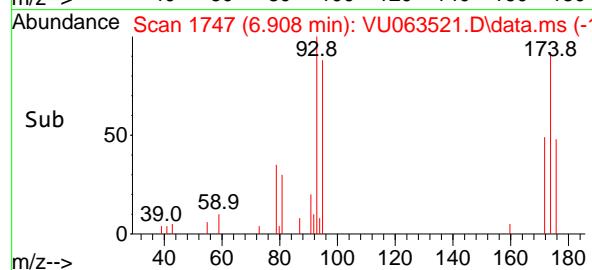

#44
Bromodichloromethane
Concen: 1.802 ug/l
RT: 7.097 min Scan# 1806
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion: 83 Resp: 12690
Ion Ratio Lower Upper
83 100
85 65.2 52.7 79.1
127 9.6 8.1 12.1

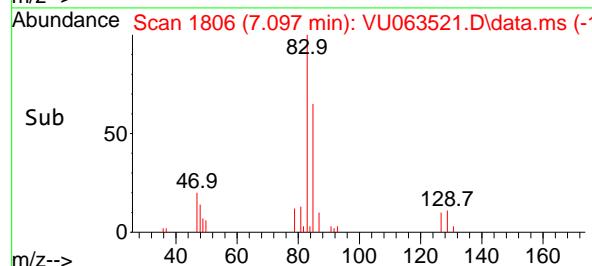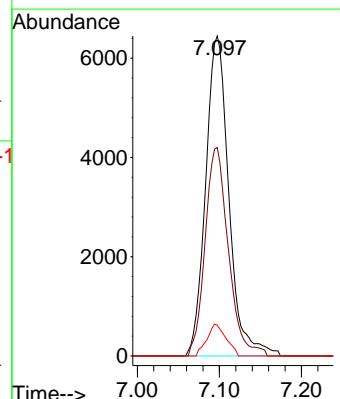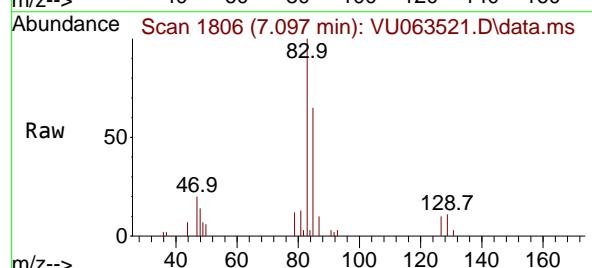



#45

4-Methyl-2-Pentanone

Concen: 9.714 ug/l

RT: 7.798 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43




Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#46

t-1,4-Dichloro-2-butene

Concen: 3.407 ug/l

RT: 10.824 min Scan# 2965

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Tgt Ion: 75 Resp: 4116


Ion Ratio Lower Upper




75 100

53 70.0 48.4 72.6

89 33.8 30.6 45.8

88 28.7 25.3 37.9

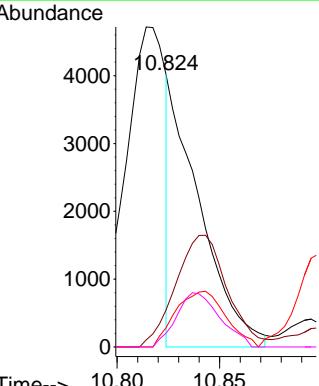






#47

Methyl methacrylate
Concen: 3.541 ug/l
RT: 6.969 min Scan# 1
Delta R.T. 0.007 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBS01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


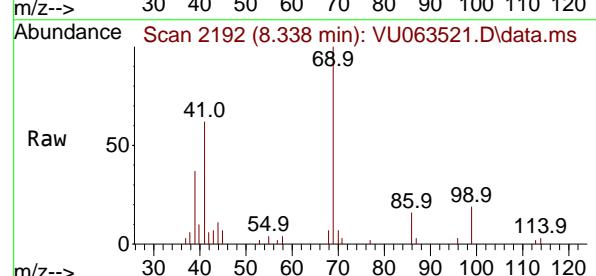



#48

Ethyl methacrylate
Concen: 1.877 ug/l
RT: 8.338 min Scan# 2192
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion: 69 Resp: 9397
Ion Ratio Lower Upper
69 100
41 64.9 30.8 92.4

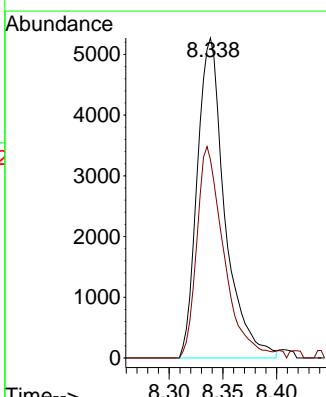







#49

Toluene
Concen: 1.885 ug/l
RT: 7.962 min Scan# 2150
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

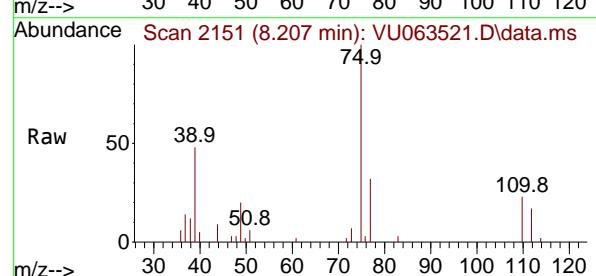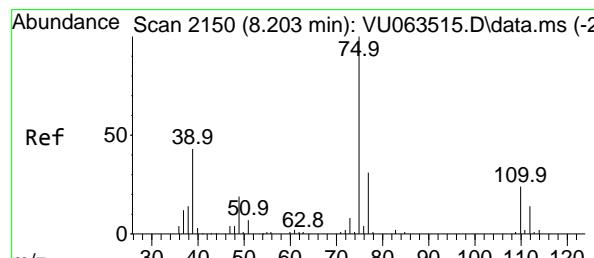


#50


t-1,3-Dichloropropene
Concen: 1.645 ug/l
RT: 8.207 min Scan# 2151
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion: 75 Resp: 9090
Ion Ratio Lower Upper
75 100
77 32.2 24.9 37.3








#51
cis-1,3-Dichloropropene
Concen: 1.692 ug/l
RT: 7.602 min Scan# 1
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43




Tgt Ion: 75 Resp: 12550
Ion Ratio Lower Upper
75 100
77 29.1 25.1 37.7
39 50.0 37.8 56.6

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025




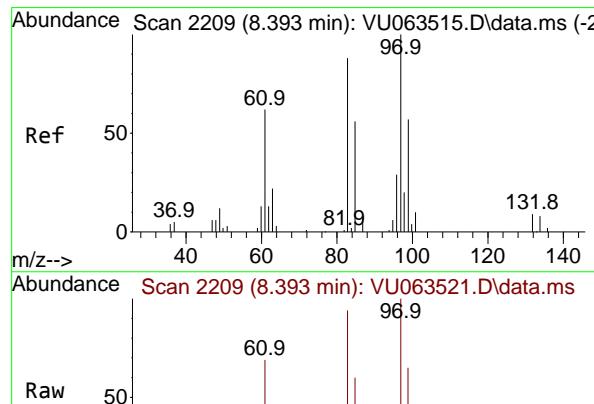
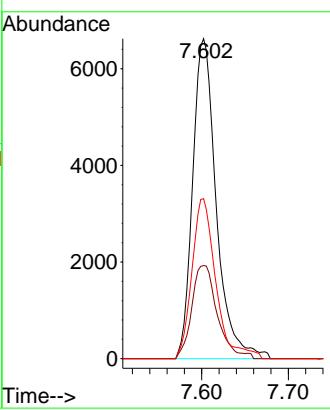



#52
1,1,2-Trichloroethane
Concen: 1.957 ug/l
RT: 8.393 min Scan# 2209
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43



Tgt Ion: 97 Resp: 8229
Ion Ratio Lower Upper
97 100
83 93.6 70.2 105.2
85 59.8 45.2 67.8
99 65.3 50.1 75.1

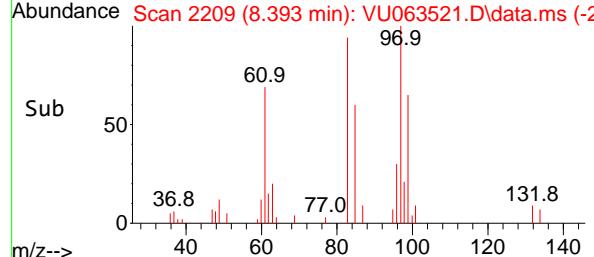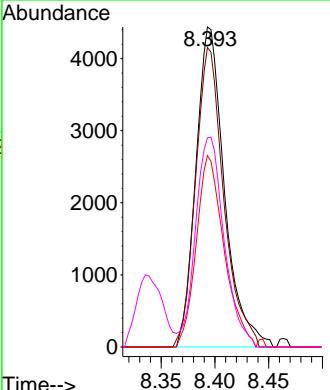



#53




1,3-Dichloropropane
Concen: 1.956 ug/l
RT: 8.570 min Scan# 2




Instrument :
MSVOA_U
ClientSampleId :
VU0717WBS01

Tgt Ion: 76 Resp: 14200
Ion Ratio Lower Upper
76 100
78 32.2 26.0 39.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

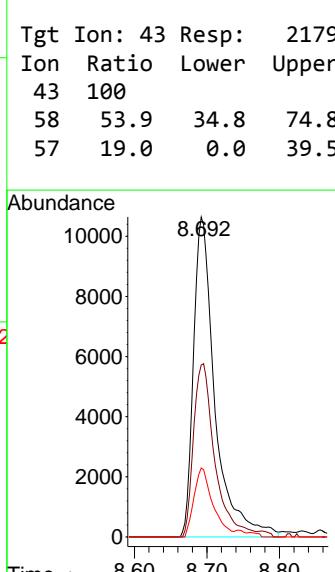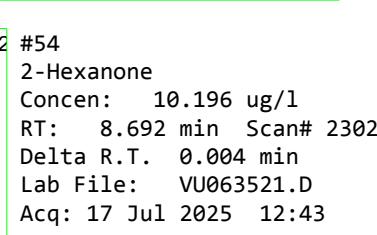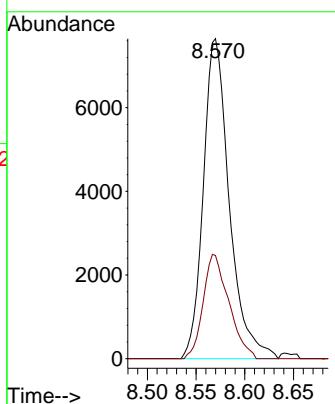



#55

Dibromochloromethane

Concen: 1.760 ug/l

RT: 8.801 min Scan# 2336

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43




Instrument :

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#56

1,2-Dibromoethane

Concen: 1.904 ug/l

RT: 8.917 min Scan# 2372

Delta R.T. 0.000 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43




Tgt Ion:107 Resp: 7165

Ion Ratio Lower Upper

107 100

109 93.4 0.0 186.4

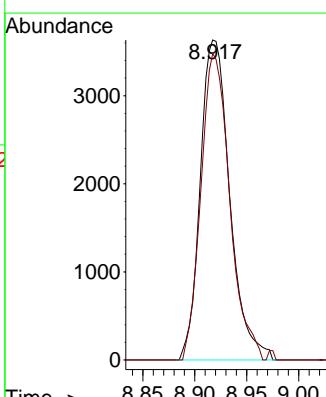



#57

4-Bromofluorobenzene

Concen: 0.995 ug/l

RT: 10.628 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43





Instrument :

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#58

Tetrachloroethene

Concen: 1.896 ug/l


RT: 8.541 min Scan# 2255


Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Tgt	Ion:164	Resp:	11402
Ion	Ratio	Lower	Upper
164	100		
166	125.3	100.7	151.1
129	105.5	80.6	120.8
131	97.9	77.3	115.9





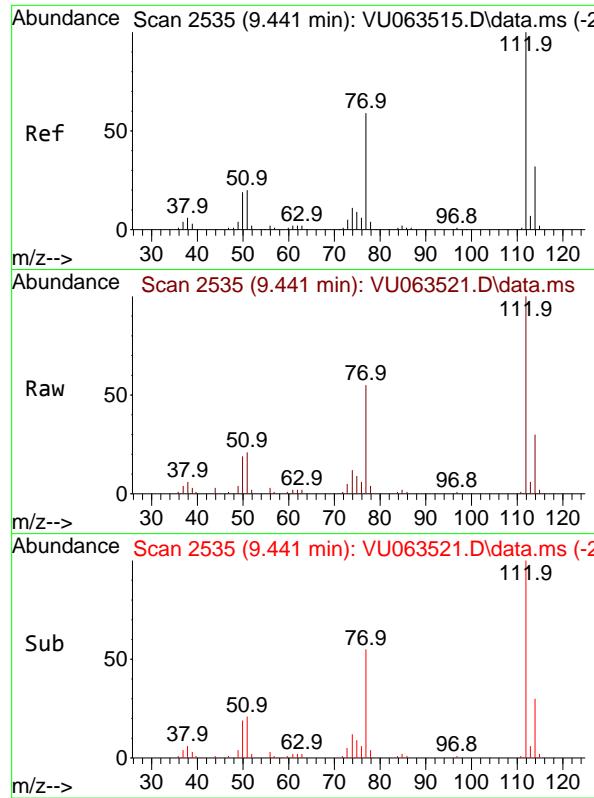

#59
Chlorobenzene
Concen: 1.916 ug/l
RT: 9.441 min Scan# 2
Instrument : MSVOA_U
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43
ClientSampleId : VU0717WBS01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

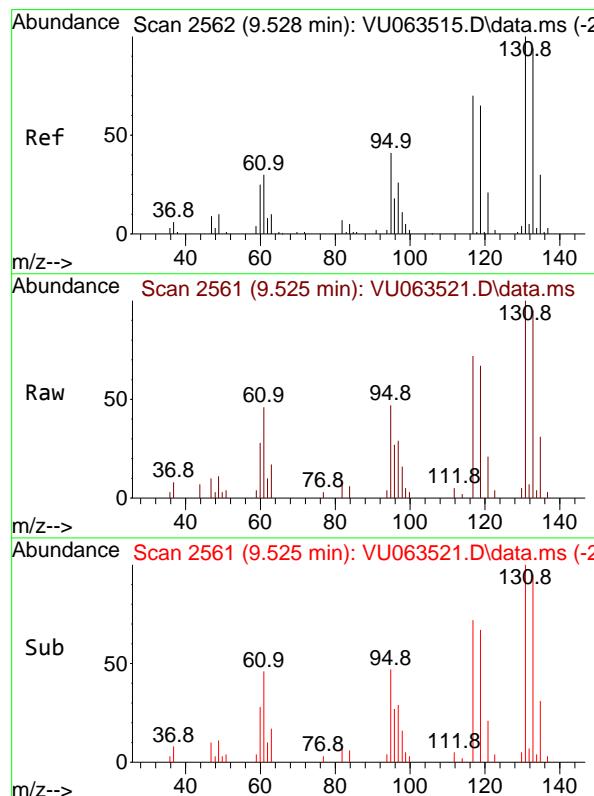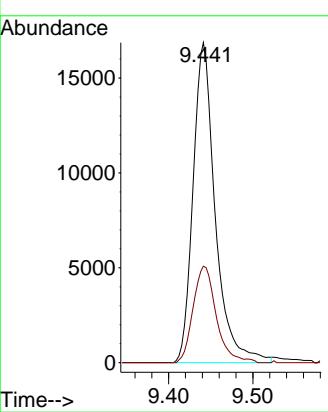

#60
1,1,1,2-Tetrachloroethane
Concen: 1.717 ug/l
RT: 9.525 min Scan# 2561
Delta R.T. -0.003 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion:131 Resp: 8917
Ion Ratio Lower Upper
131 100
133 101.3 74.7 112.1
119 71.6 53.0 79.4





#61

Pentachloroethane

Concen: 1.737 ug/l

RT: 11.419 min Scan# 3150

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43





Instrument :

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#62

Hexachloroethane


Concen: 1.644 ug/l




RT: 12.467 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

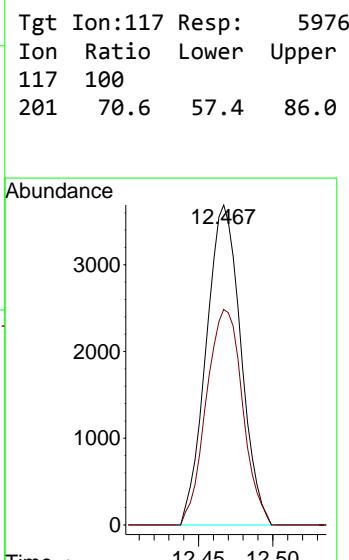



#63

Ethyl Benzene

Concen: 1.929 ug/l

RT: 9.563 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Instrument:

MSVOA_U





ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#64

m/p-Xylenes

Concen: 3.770 ug/l


RT: 9.686 min Scan# 2611


Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Tgt Ion:106 Resp: 40731
 Ion Ratio Lower Upper
 106 100
 91 207.2 163.6 245.4

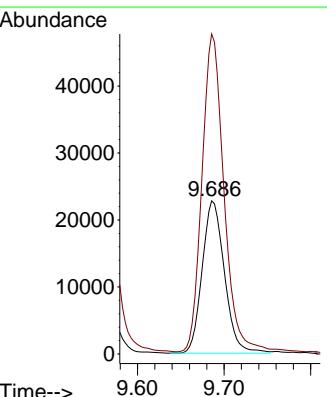


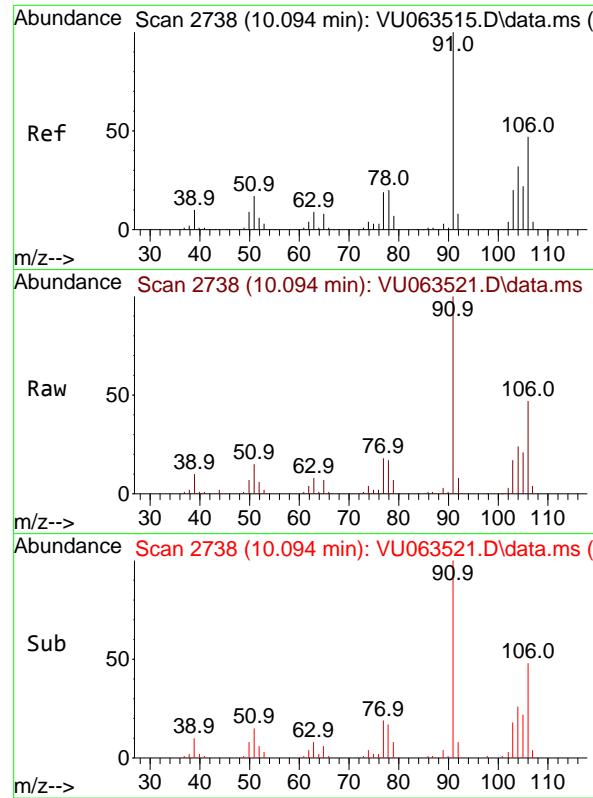


#65
o-Xylene
Concen: 1.957 ug/l
RT: 10.094 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

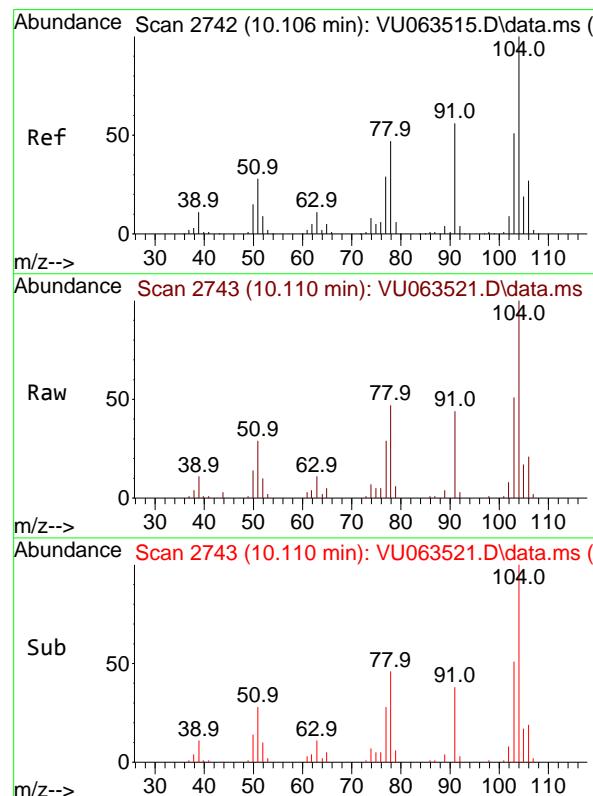

#66
Styrene
Concen: 1.908 ug/l
RT: 10.110 min Scan# 2743
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion:104 Resp: 31561
Ion Ratio Lower Upper
104 100
78 53.4 41.3 61.9
103 55.2 43.6 65.4





#67

Bromoform

Concen: 1.597 ug/l

RT: 10.284 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43





Instrument :

MSVOA_U

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

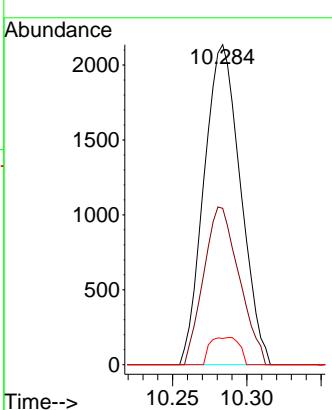 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#68

1,2-Dichlorobenzene-d4

Concen: 0.936 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Tgt	Ion:152	Resp:	7166
Ion	Ratio	Lower	Upper
152	100		
115	84.6	0.0	262.2
150	204.2	0.0	651.2

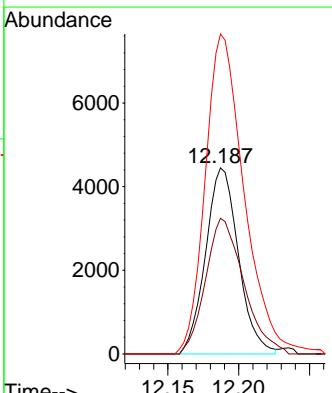



#69

Isopropylbenzene

Concen: 1.952 ug/l

RT: 10.477 min Scan# 2

Instrument :

Delta R.T. 0.000 min

MSVOA_U

Lab File: VU063521.D

ClientSampleId :

Acq: 17 Jul 2025 12:43

VU0717WBS01

Tgt Ion:105 Resp: 4898

Ion Ratio Lower Upper




105 100

120 26.5 13.2 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 1.948 ug/l

RT: 10.776 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Tgt Ion: 83 Resp: 9968

Ion Ratio Lower Upper

83 100

131 10.4 8.4 12.6

85 62.7 51.9 77.9



#71

1,2,3-Trichloropropane

Concen: 1.871 ug/l m

RT: 10.814 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063521.D




Acq: 17 Jul 2025 12:43

Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

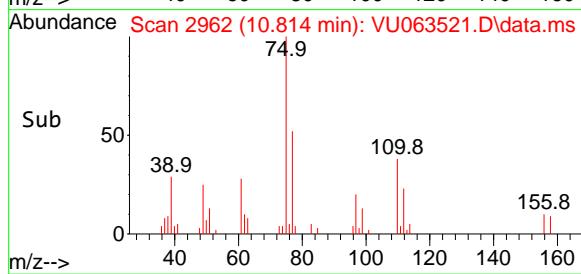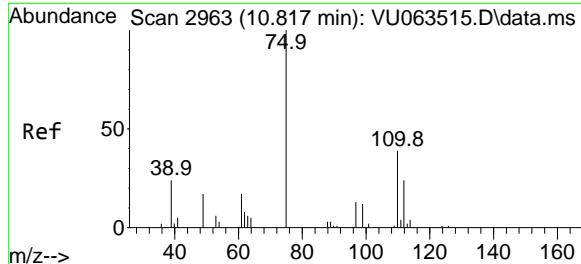

Tgt Ion: 75 Resp: 7770

Ion Ratio Lower Upper

75 100

77 0.0 0.0 0.0





110 38.8 0.0 73.2

97 19.9 0.0 37.6

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

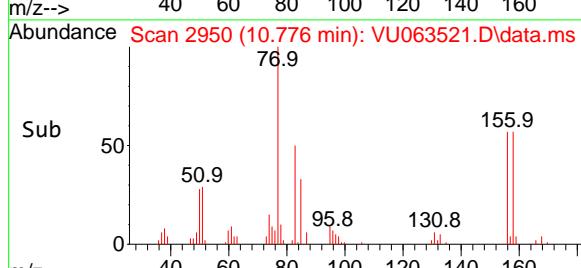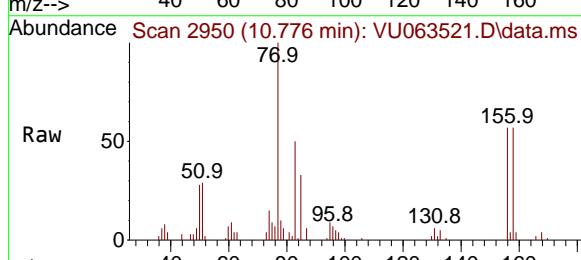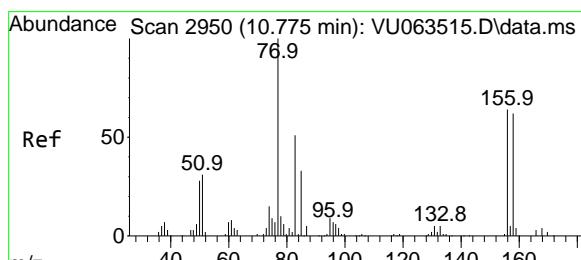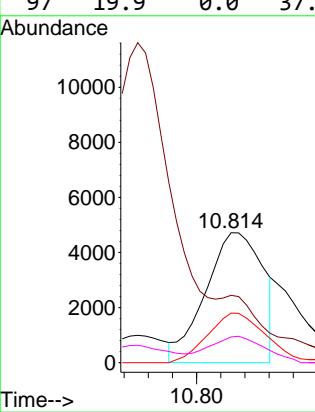

#72
Bromobenzene
Concen: 1.868 ug/l
RT: 10.776 min Scan# 2950
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43


Tgt Ion:156 Resp: 12098




Ion Ratio Lower Upper

156 100

77 174.0 0.0 315.2

158 98.3 0.0 195.4

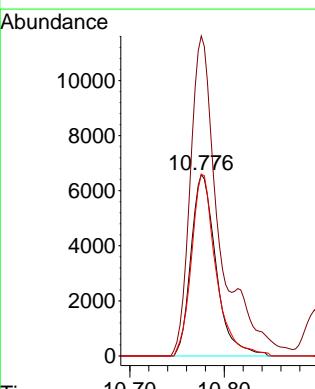



#73

n-propylbenzene

Concen: 1.956 ug/l

RT: 10.898 min Scan# 2

Instrument :

MSVOA_U

Delta R.T. 0.000 min




Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#74

2-Chlorotoluene

Concen: 1.957 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063521.D


Acq: 17 Jul 2025 12:43




Tgt Ion:126 Resp: 13064

Ion Ratio Lower Upper

126 100

91 285.4 0.0 606.0

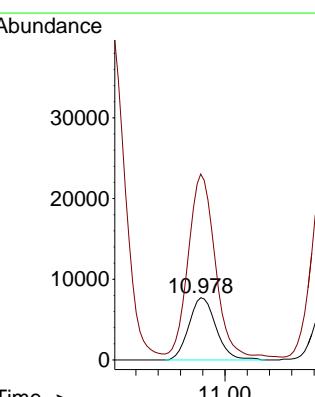







#75
1,3,5-Trimethylbenzene
Concen: 1.938 ug/l
RT: 11.081 min Scan# 3045
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#76
4-Chlorotoluene
Concen: 1.973 ug/l
RT: 11.091 min Scan# 3048
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43


Tgt Ion:126 Resp: 13377
Ion Ratio Lower Upper
126 100
91 334.9 0.0 682.2



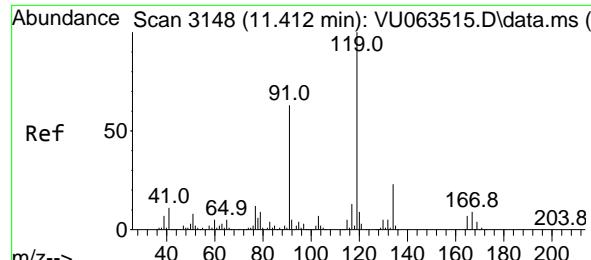

#77
tert-Butylbenzene
Concen: 1.901 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43



Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

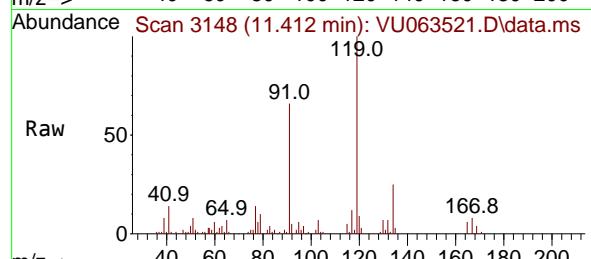


Tgt Ion:119 Resp: 43549
Ion Ratio Lower Upper
119 100
91 64.8 30.7 92.1
134 23.9 18.5 27.7

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


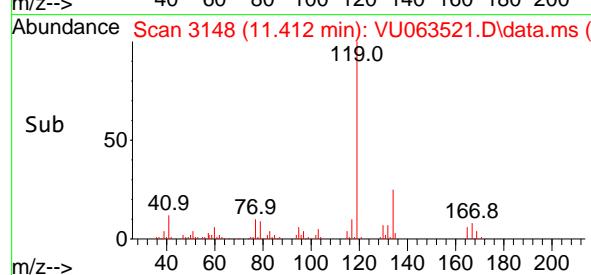



#78
1,2,4-Trimethylbenzene
Concen: 1.947 ug/l
RT: 11.460 min Scan# 3163
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

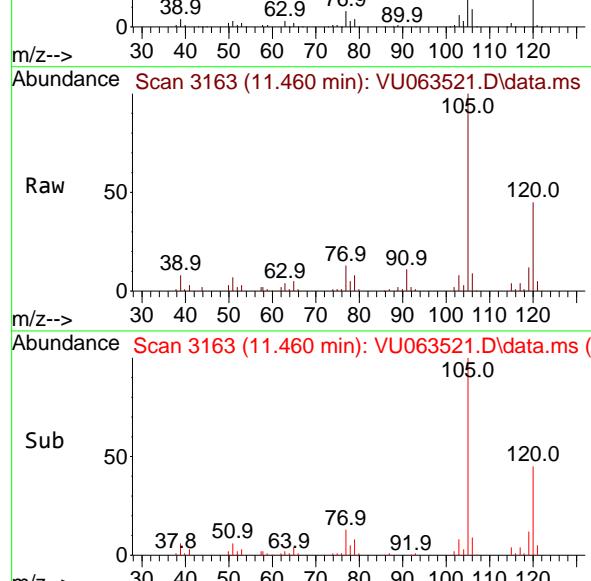

Tgt Ion:105 Resp: 46303
Ion Ratio Lower Upper
105 100
120 42.6 22.7 68.0

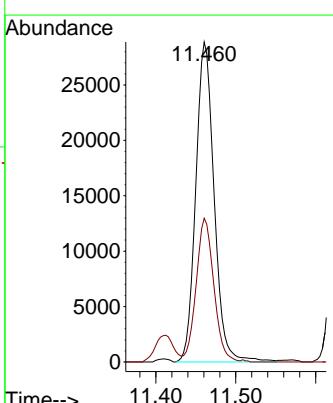




#79
sec-Butylbenzene
Concen: 1.994 ug/l
RT: 11.634 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBS01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

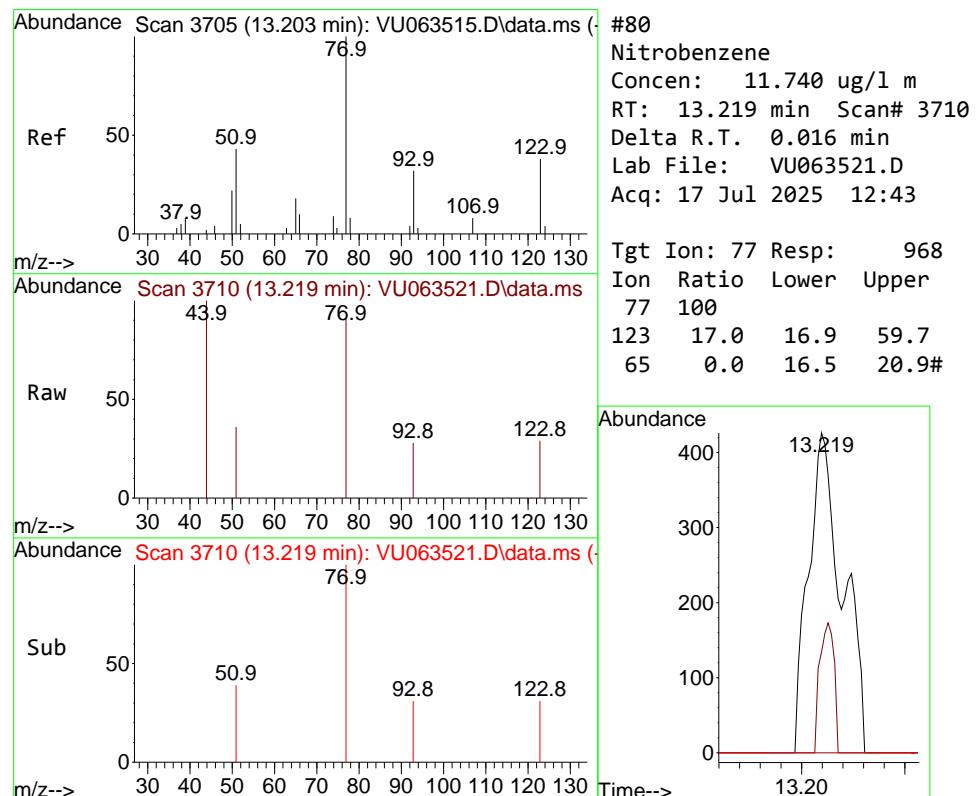

#80
Nitrobenzene
Concen: 11.740 ug/l m
RT: 13.219 min Scan# 3710
Delta R.T. 0.016 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion: 77 Resp: 968
Ion Ratio Lower Upper
77 100
123 17.0 16.9 59.7
65 0.0 16.5 20.9#

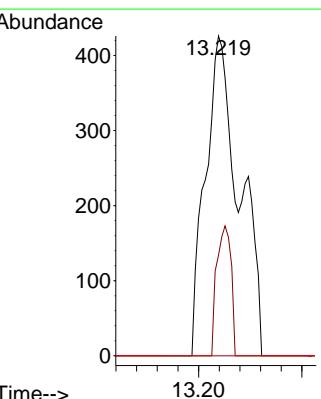






#81
p-Isopropyltoluene
Concen: 1.975 ug/l
RT: 11.785 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01

Tgt	Ion	Ion Ratio	Resp:	5094:
	119	100		
	134	26.0	Lower	21.1
	91	25.1	Upper	31.7
				29.8


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#82
1,3-Dichlorobenzene
Concen: 1.916 ug/l
RT: 11.740 min Scan# 3250
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt	Ion	Ion Ratio	Resp:	24826
	146	100		
	111	44.3	Lower	33.8
	148	64.5	Upper	50.6
				77.3

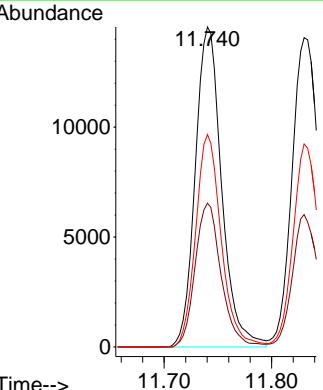

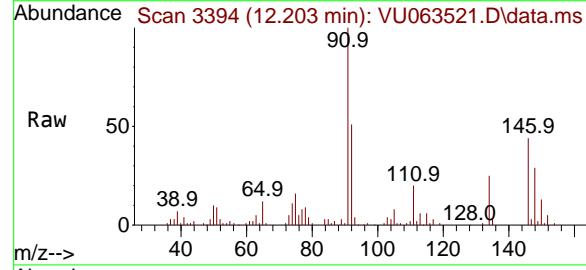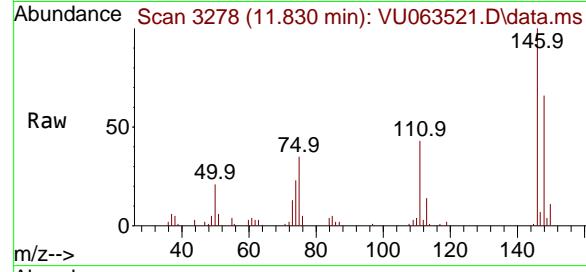

#83

1,4-Dichlorobenzene

Concen: 1.944 ug/l

RT: 11.830 min Scan# 3

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Instrument :

MSVOA_U


ClientSampleId :

VU0717WBS01

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

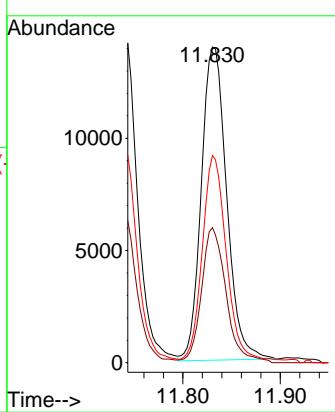

#84

n-Butylbenzene

Concen: 2.011 ug/l

RT: 12.203 min Scan# 3394

Delta R.T. 0.003 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Tgt Ion: 91 Resp: 48117




Ion Ratio Lower Upper

91 100

92 51.1 41.5 62.3

134 24.2 20.6 30.8

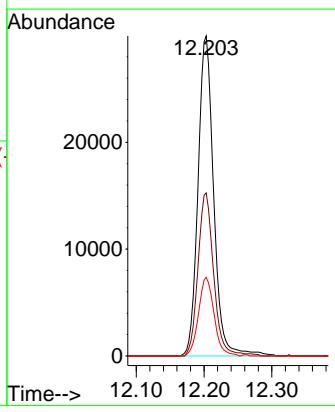



#85

1,2-Dichlorobenzene

Concen: 1.930 ug/l

RT: 12.206 min Scan# 3395

Delta R.T. 0.000 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Instrument:

MSVOA_U

ClientSampleId :

VU0717WBS01

Tgt Ion:146 Resp: 2350

Ion Ratio Lower Upper

146 100




111 45.8 21.7 65.1

148 65.4 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#86

1,2-Dibromo-3-Chloropropane

Concen: 1.706 ug/l

RT: 12.988 min Scan# 3638

Delta R.T. 0.001 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Tgt Ion: 75 Resp: 1114


Ion Ratio Lower Upper

75 100

155 83.8 65.8 98.6

157 110.8 81.4 122.2




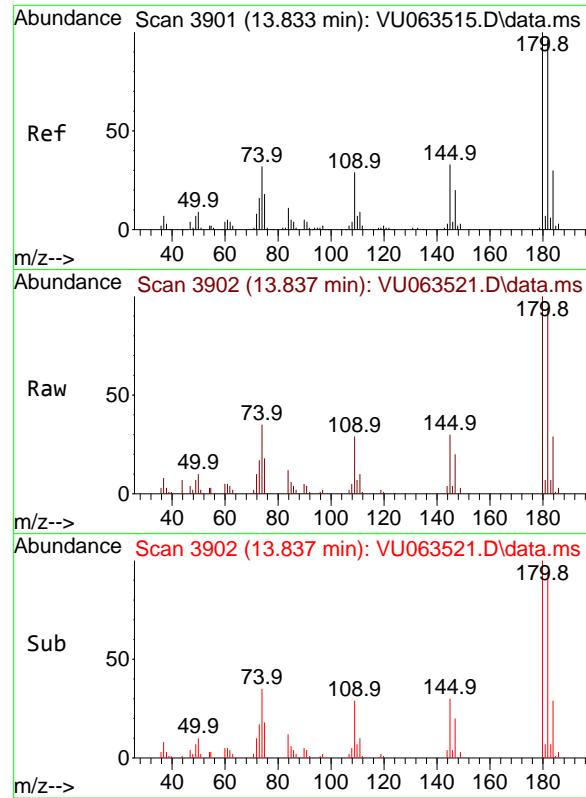


#87
1,2,4-Trichlorobenzene
Concen: 1.850 ug/l
RT: 13.837 min Scan# 3902
Delta R.T. 0.004 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Instrument : MSVOA_U
ClientSampleId : VU0717WBS01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

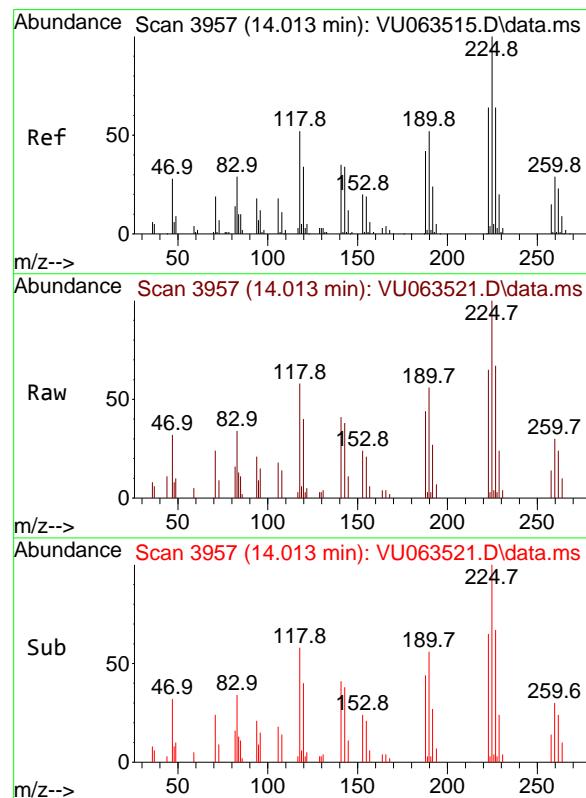

#88
Hexachlorobutadiene
Concen: 1.921 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063521.D
Acq: 17 Jul 2025 12:43

Tgt Ion:225 Resp: 8260
Ion Ratio Lower Upper
225 100
223 60.6 50.8 76.2
227 66.2 51.0 76.6



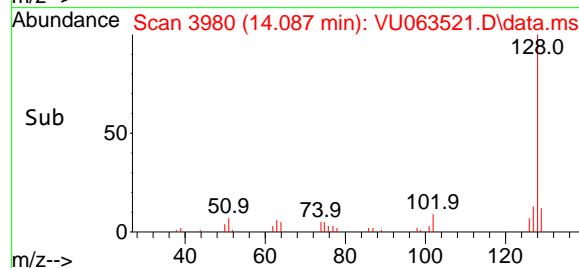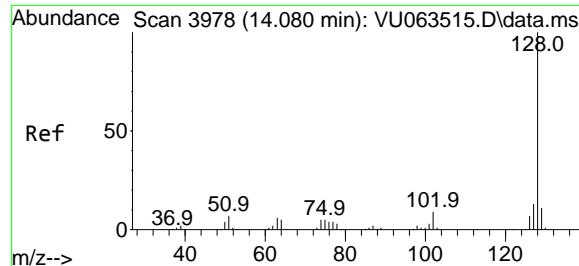

#89

Naphthalene

Concen: 1.802 ug/l

RT: 14.087 min Scan# 3

Delta R.T. 0.007 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43

Instrument :

MSVOA_U




ClientSampleId :

VU0717WBS01

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

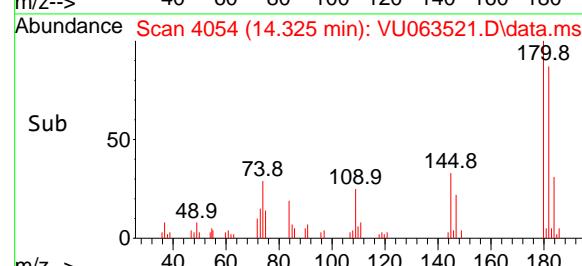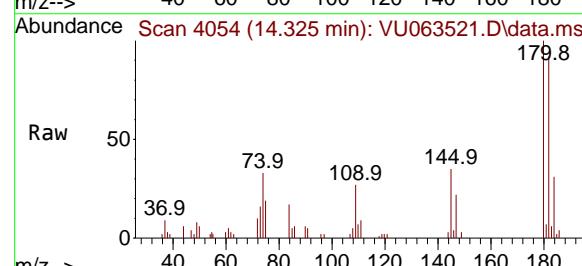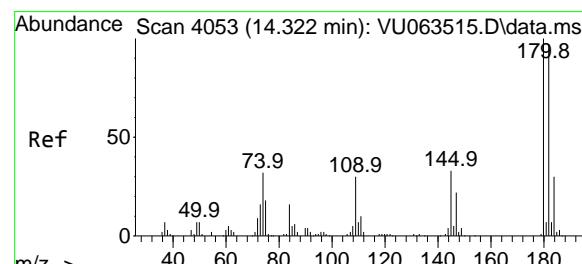

#90

1,2,3-Trichlorobenzene

Concen: 1.836 ug/l

RT: 14.325 min Scan# 4054

Delta R.T. 0.004 min

Lab File: VU063521.D

Acq: 17 Jul 2025 12:43


Tgt Ion:180 Resp: 12843

Ion Ratio Lower Upper

180 100

182 93.4 78.0 117.0

145 34.0 27.3 40.9

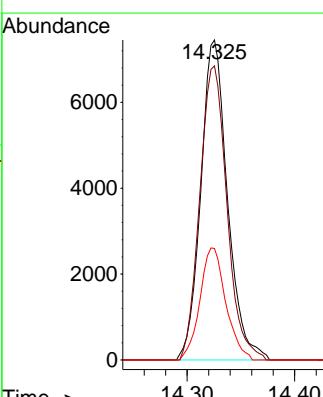



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBS02		SDG No.:	Q2552
Lab Sample ID:	VU0718WBS02		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063535.D	1	07/18/25 11:50	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	1.90		0.12	0.50	ug/L
74-87-3	Chloromethane	2.10		0.13	0.50	ug/L
75-01-4	Vinyl Chloride	2.10		0.12	0.50	ug/L
74-83-9	Bromomethane	2.30		0.15	0.50	ug/L
75-00-3	Chloroethane	2.20		0.14	0.50	ug/L
109-99-9	Tetrahydrofuran	4.80		0.42	1.00	ug/L
75-69-4	Trichlorofluoromethane	2.20		0.20	0.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	2.20		0.11	0.50	ug/L
75-65-0	tert-Butyl Alcohol	20.7		3.60	10.0	ug/L
60-29-7	Diethyl Ether	2.30		0.13	0.50	ug/L
75-35-4	1,1-Dichloroethene	2.20		0.13	0.50	ug/L
107-13-1	Acrylonitrile	4.00		0.44	1.00	ug/L
67-64-1	Acetone	10.2		0.97	2.50	ug/L
75-15-0	Carbon Disulfide	1.80		0.12	0.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	2.20		0.11	0.50	ug/L
96-33-3	Methyl acrylate	2.10		0.33	0.50	ug/L
75-09-2	Methylene Chloride	2.20		0.44	0.50	ug/L
156-60-5	trans-1,2-Dichloroethene	2.10		0.14	0.50	ug/L
75-34-3	1,1-Dichloroethane	2.20		0.13	0.50	ug/L
110-82-7	Cyclohexane	2.20		0.14	0.50	ug/L
78-93-3	2-Butanone	11.0		0.72	2.50	ug/L
56-23-5	Carbon Tetrachloride	2.00		0.13	0.50	ug/L
594-20-7	2,2-Dichloropropane	2.00		0.12	0.50	ug/L
156-59-2	cis-1,2-Dichloroethene	2.20		0.13	0.50	ug/L
74-97-5	Bromoform	2.20		0.17	0.50	ug/L
67-66-3	Chloroform	2.30		0.17	0.50	ug/L
71-55-6	1,1,1-Trichloroethane	2.10		0.12	0.50	ug/L
108-87-2	Methylcyclohexane	1.80		0.090	0.50	ug/L
563-58-6	1,1-Dichloropropene	2.20		0.11	0.50	ug/L
107-12-0	Propionitrile	11.1		1.20	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBS02		SDG No.:	Q2552
Lab Sample ID:	VU0718WBS02		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063535.D	1	07/18/25 11:50	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	1.80		0.11	0.50	ug/L
107-06-2	1,2-Dichloroethane	1.80		0.14	0.50	ug/L
79-01-6	Trichloroethene	1.90		0.13	0.50	ug/L
78-87-5	1,2-Dichloropropane	1.90		0.13	0.50	ug/L
109-69-3	1-Chlorobutane	2.00		0.12	0.50	ug/L
74-95-3	Dibromomethane	2.00		0.15	0.50	ug/L
75-27-4	Bromodichloromethane	1.80		0.13	0.50	ug/L
108-10-1	4-Methyl-2-Pentanone	10.5		0.63	2.50	ug/L
108-88-3	Toluene	2.00		0.11	0.50	ug/L
10061-02-6	t-1,3-Dichloropropene	1.50		0.11	0.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	1.60		0.11	0.50	ug/L
79-00-5	1,1,2-Trichloroethane	2.10		0.13	0.50	ug/L
142-28-9	1,3-Dichloropropane	2.10		0.12	0.50	ug/L
591-78-6	2-Hexanone	10.0		0.65	2.50	ug/L
124-48-1	Dibromochloromethane	1.60		0.20	0.50	ug/L
106-93-4	1,2-Dibromoethane	1.90		0.13	0.50	ug/L
127-18-4	Tetrachloroethene	1.90		0.14	0.50	ug/L
108-90-7	Chlorobenzene	2.00		0.11	0.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	1.70		0.13	0.50	ug/L
67-72-1	Hexachloroethane	1.50		0.12	0.50	ug/L
100-41-4	Ethyl Benzene	1.90		0.41	0.50	ug/L
179601-23-1	m/p-Xylenes	3.90		0.73	1.00	ug/L
1330-20-7	Total Xylenes	5.90		1.09	1.50	ug/L
95-47-6	o-Xylene	2.00		0.36	0.50	ug/L
100-42-5	Styrene	2.00		0.38	0.50	ug/L
75-25-2	Bromoform	1.40		0.31	0.50	ug/L
98-82-8	Isopropylbenzene	2.00		0.38	0.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	2.00		0.13	0.50	ug/L
96-18-4	1,2,3-Trichloropropane	2.00		0.19	0.50	ug/L
108-86-1	Bromobenzene	1.90		0.13	0.50	ug/L
103-65-1	n-propylbenzene	2.00		0.42	0.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBS02		SDG No.:	Q2552
Lab Sample ID:	VU0718WBS02		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063535.D	1	07/18/25 11:50	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	1.90		0.27	0.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	1.90		0.37	0.50	ug/L
106-43-4	4-Chlorotoluene	2.00		0.27	0.50	ug/L
98-06-6	tert-Butylbenzene	2.00		0.37	0.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	2.00		0.40	0.50	ug/L
135-98-8	sec-Butylbenzene	2.00		0.36	0.50	ug/L
99-87-6	p-Isopropyltoluene	2.00		0.42	0.50	ug/L
541-73-1	1,3-Dichlorobenzene	2.00		0.13	0.50	ug/L
106-46-7	1,4-Dichlorobenzene	2.00		0.13	0.50	ug/L
104-51-8	n-Butylbenzene	2.00		0.43	0.50	ug/L
95-50-1	1,2-Dichlorobenzene	2.00		0.14	0.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	1.90		0.24	0.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	1.90		0.21	0.50	ug/L
87-68-3	Hexachlorobutadiene	1.90		0.14	0.50	ug/L
91-20-3	Naphthalene	2.00		0.33	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	2.00		0.31	0.50	ug/L
98-95-3	Nitrobenzene	8.60		1.80	5.00	ug/L
363-72-4	Pentachloroethane	1.80		0.16	0.50	ug/L
74-88-4	Iodomethane	1.90		0.090	1.00	ug/L
107-05-1	Allyl Chloride	2.00		0.13	0.50	ug/L
126-98-7	Methacrylonitrile	2.00		0.24	0.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	4.60		0.21	1.00	ug/L
97-63-2	Ethyl methacrylate	2.00		0.12	0.50	ug/L
108-20-3	Isopropyl Ether	2.30		0.14	0.50	ug/L
80-62-6	Methyl methacrylate	3.70		0.24	1.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	1.00		70 - 130	105%	SPK: 1
460-00-4	4-Bromofluorobenzene	1.00		70 - 130	103%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	20200	6.1			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0718WBS02	SDG No.:	Q2552	
Lab Sample ID:	VU0718WBS02	Matrix:	Water	
Analytical Method:	E524.2	% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol: 25000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063535.D	1	07/18/25 11:50	VU071825

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063535.D
 Acq On : 18 Jul 2025 11:50
 Operator : MD/SY
 Sample : VU0718WBS02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0718WBS02

Quant Time: Jul 18 23:49:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.100	96	20233	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	7909	1.032	ug/l	0.00
Spiked Amount 1.000			Recovery	=	103.000%	
68) 1,2-Dichlorobenzene-d4	12.183	152	7416	1.047	ug/l	0.00
Spiked Amount 1.000			Recovery	=	105.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	11517	1.930	ug/l	97
3) Chloromethane	1.518	50	11598	2.091	ug/l	99
4) Vinyl Chloride	1.599	62	14856	2.103	ug/l	99
5) Bromomethane	1.846	94	12510	2.349	ug/l	98
6) Chloroethane	1.923	64	9455	2.217	ug/l	98
7) Trichlorofluoromethane	2.129	101	21982	2.168	ug/l	96
8) 1,1,2-Trichloro-1,2,2-...	2.570	101	11650	2.198	ug/l	99
9) 1,1-Dichloroethene	2.570	96	11469	2.183	ug/l	99
10) Iodomethane	2.711	142	8386	1.886	ug/l	97
11) Allyl Chloride	2.910	41	15179	2.000	ug/l	92
12) Acrylonitrile	3.306	53	5284	4.022	ug/l	97
13) Acetone	2.618	43	10707	10.172	ug/l	99
14) Carbon Disulfide	2.779	76	29884	1.761	ug/l	97
15) Methylene Chloride	3.029	84	13588	2.197	ug/l	97
16) trans-1,2-Dichloroethene	3.335	96	12679	2.125	ug/l	96
17) 1,1-Dichloroethane	3.849	63	24826	2.245	ug/l	98
18) 2-Butanone	4.717	43	17869	10.962	ug/l	100
19) Cyclohexane	5.357	56	20151	2.152	ug/l	99
20) Methylcyclohexane	6.743	83	16656	1.830	ug/l	99
21) 2,2-Dichloropropane	4.644	77	19201	2.039	ug/l	100
22) cis-1,2-Dichloroethene	4.647	96	14551	2.248	ug/l	99
23) Diethyl Ether	2.370	59	9066	2.265	ug/l	94
24) tert-Butyl Alcohol	3.190	59	9981	20.656	ug/l	98
25) Methyl tert-Butyl Ether	3.361	73	30621	2.233	ug/l	95
26) Bromochloromethane	4.952	128	6006	2.222	ug/l	93
27) Chloroform	5.068	83	25415	2.252	ug/l	95
28) 1,1,1-Trichloroethane	5.293	97	19854	2.073	ug/l	96
29) 1,1-Dichloropropene	5.502	75	19114	2.155	ug/l	98
30) Carbon Tetrachloride	5.496	117	15127	1.963	ug/l	96
31) Isopropyl Ether	3.988	45	38568	2.311	ug/l	97
32) Ethyl-t-butyl ether	4.502	59	33853	2.192	ug/l	99
33) Tert-Amyl methyl ether	5.942	73	23163	1.728	ug/l	98
34) Propionitrile	4.775	54	5508	11.090	ug/l	# 95
35) Benzene	5.756	78	43678	1.832	ug/l	96
36) 1,2-Dichloroethane	5.779	62	13615	1.838	ug/l	100
37) Trichloroethene	6.528	130	11322	1.862	ug/l	90
38) 1,2-Dichloropropane	6.782	63	10377	1.860	ug/l	91
39) Methacrylonitrile	4.975	41	4501	2.039	ug/l	99
40) Methyl acrylate	4.853	55	6736	2.087	ug/l	98
41) Tetrahydrofuran	5.058	42	5573	4.799	ug/l	88
42) 1-Chlorobutane	5.438	56	23868	2.024	ug/l	99
43) Dibromomethane	6.910	93	5720	1.979	ug/l	92
44) Bromodichloromethane	7.097	83	11850	1.818	ug/l	90

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
 Data File : VU063535.D
 Acq On : 18 Jul 2025 11:50
 Operator : MD/SY
 Sample : VU0718WBS02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0718WBS02

Quant Time: Jul 18 23:49:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	31197	10.474	ug/1	97
46) t-1,4-Dichloro-2-butene	10.817	75	5188m	4.640	ug/1	
47) Methyl methacrylate	6.968	69	8996	3.707	ug/1	93
48) Ethyl methacrylate	8.335	69	9290	2.006	ug/1	99
49) Toluene	7.958	92	25746	1.978	ug/1	98
50) t-1,3-Dichloropropene	8.206	75	7896	1.544	ug/1	99
51) cis-1,3-Dichloropropene	7.602	75	11136	1.623	ug/1	95
52) 1,1,2-Trichloroethane	8.393	97	8183	2.103	ug/1	97
53) 1,3-Dichloropropane	8.569	76	13909	2.071	ug/1	99
54) 2-Hexanone	8.692	43	19855	10.036	ug/1	98
55) Dibromochloromethane	8.801	129	6602	1.606	ug/1	99
56) 1,2-Dibromoethane	8.917	107	6737	1.935	ug/1	99
58) Tetrachloroethene	8.540	164	10524	1.891	ug/1	94
59) Chlorobenzene	9.441	112	29416	1.968	ug/1	99
60) 1,1,1,2-Tetrachloroethane	9.528	131	8208	1.708	ug/1	97
61) Pentachloroethane	11.418	117	6154	1.812	ug/1	89
62) Hexachloroethane	12.466	117	5086	1.512	ug/1	93
63) Ethyl Benzene	9.560	91	50124	1.949	ug/1	97
64) m/p-Xylenes	9.685	106	38644	3.865	ug/1	94
65) o-Xylene	10.090	106	18729	1.950	ug/1	96
66) Styrene	10.110	104	30077	1.964	ug/1	98
67) Bromoform	10.283	173	3032	1.436	ug/1 #	94
69) Isopropylbenzene	10.476	105	46030	1.982	ug/1	100
70) 1,1,2,2-Tetrachloroethane	10.775	83	9398	1.985	ug/1	98
71) 1,2,3-Trichloropropane	10.817	75	7499m	1.950	ug/1	
72) Bromobenzene	10.775	156	11376	1.898	ug/1	78
73) n-propylbenzene	10.897	120	13872	1.984	ug/1	94
74) 2-Chlorotoluene	10.978	126	11750	1.902	ug/1	99
75) 1,3,5-Trimethylbenzene	11.081	105	42877	1.933	ug/1	99
76) 4-Chlorotoluene	11.090	126	12663	2.018	ug/1	99
77) tert-Butylbenzene	11.412	119	41361	1.951	ug/1	97
78) 1,2,4-Trimethylbenzene	11.460	105	43519	1.977	ug/1	98
79) sec-Butylbenzene	11.634	105	57444	2.009	ug/1	98
80) Nitrobenzene	13.219	77	614	8.625	ug/1 #	52
81) p-Isopropyltoluene	11.785	119	47010	1.969	ug/1	98
82) 1,3-Dichlorobenzene	11.740	146	23706	1.977	ug/1	99
83) 1,4-Dichlorobenzene	11.830	146	24286	2.023	ug/1	99
84) n-Butylbenzene	12.203	91	44796	2.024	ug/1	97
85) 1,2-Dichlorobenzene	12.206	146	23077	2.048	ug/1	98
86) 1,2-Dibromo-3-Chloropr...	12.987	75	1197	1.944	ug/1	86
87) 1,2,4-Trichlorobenzene	13.836	180	13513	1.929	ug/1	97
88) Hexachlorobutadiene	14.013	225	7537	1.894	ug/1	96
89) Naphthalene	14.084	128	25302	2.015	ug/1	98
90) 1,2,3-Trichlorobenzene	14.322	180	12842	1.983	ug/1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063535.D
Acq On : 18 Jul 2025 11:50
Operator : MD/SY
Sample : VU0718WBS02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1




Quant Time: Jul 18 23:49:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBS02

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

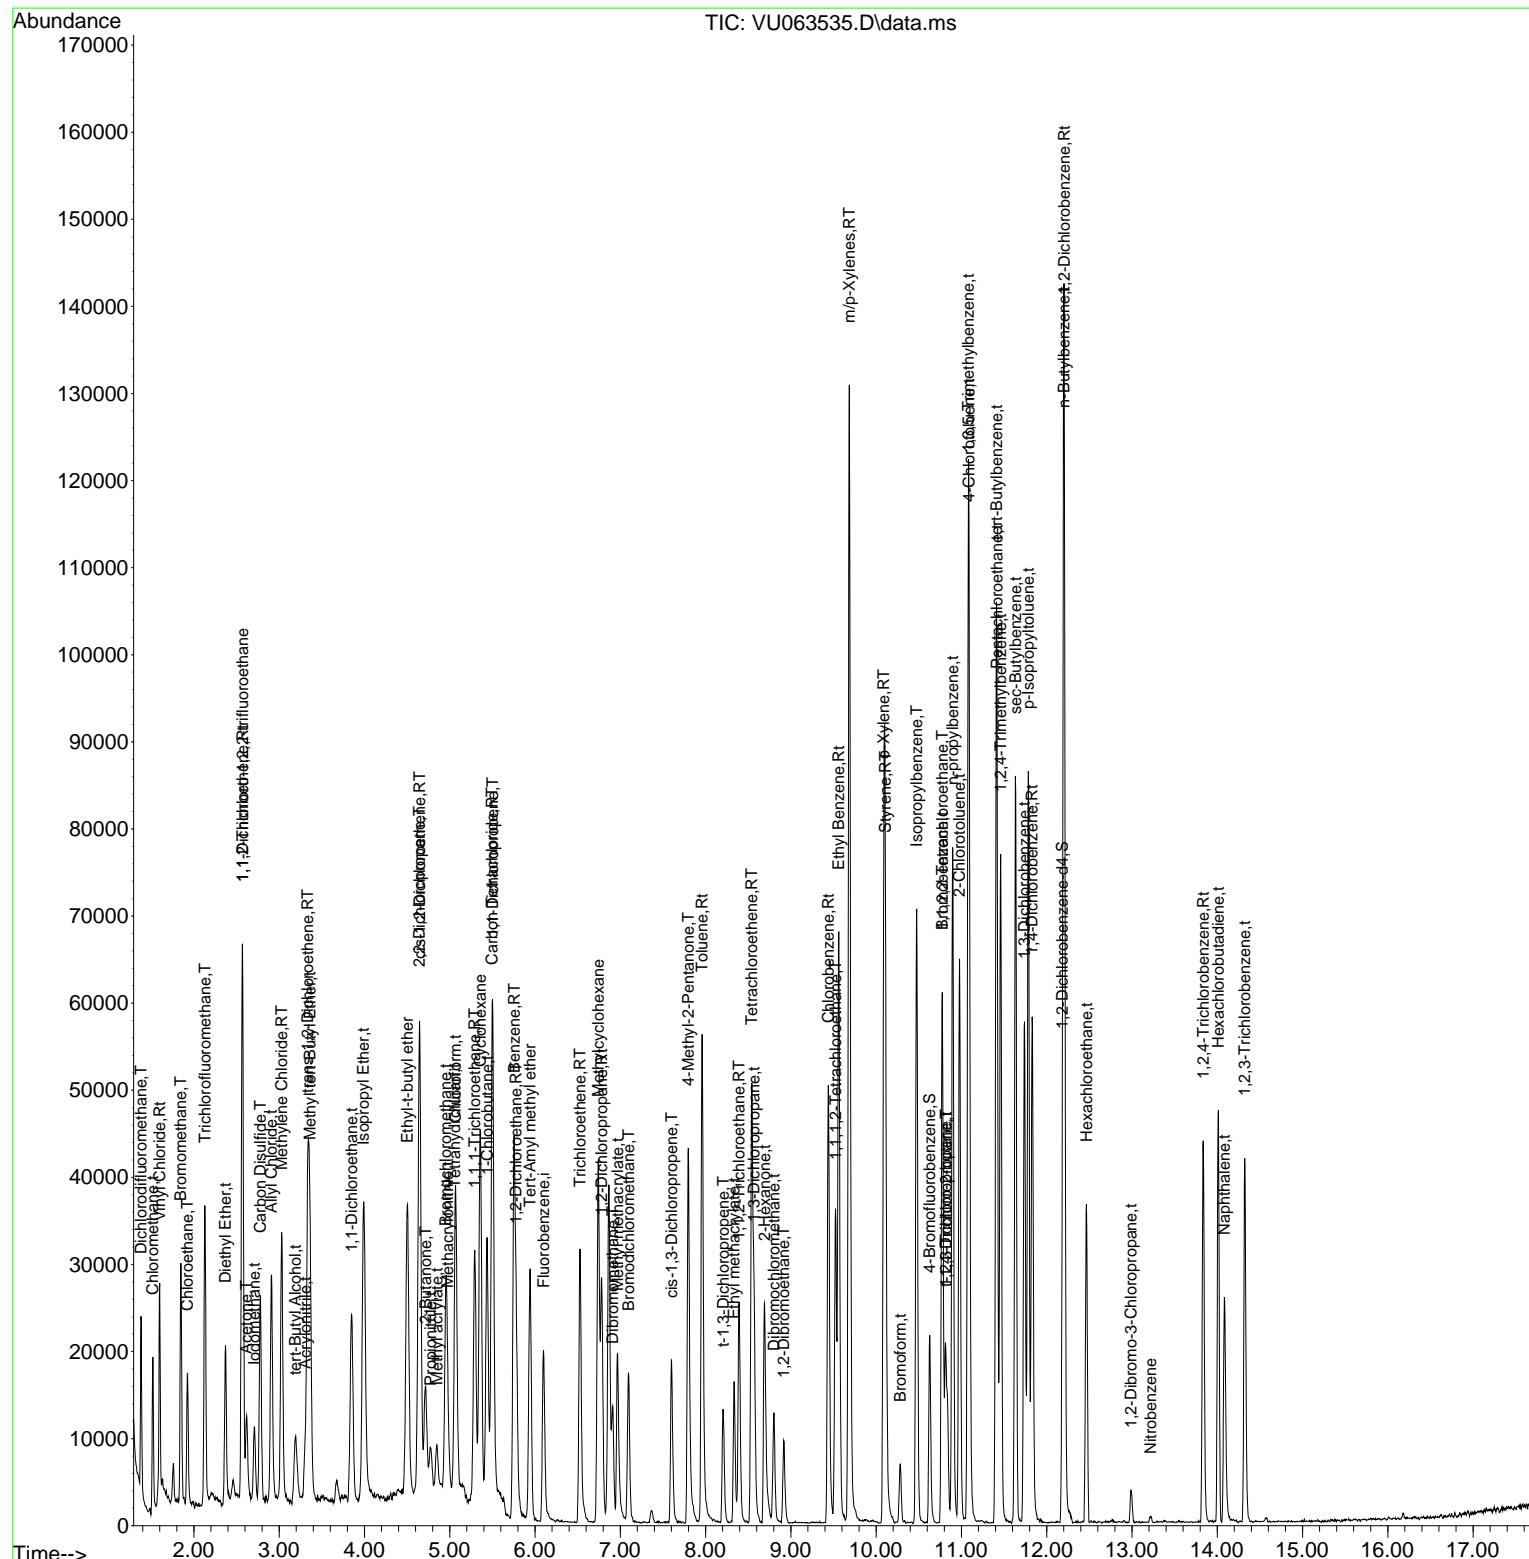







#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

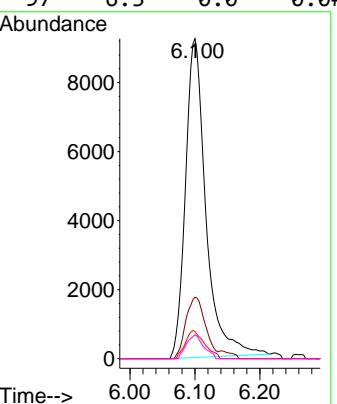

#2
Dichlorodifluoromethane
Concen: 1.930 ug/l
RT: 1.380 min Scan# 28
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 85 Resp: 11517
Ion Ratio Lower Upper
85 100
87 33.5 16.0 47.9

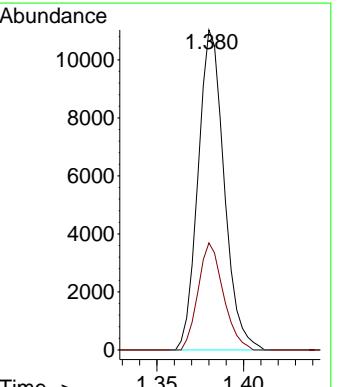



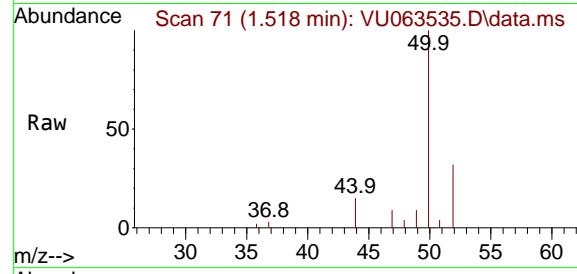



#3
Chloromethane
Concen: 2.091 ug/l
RT: 1.518 min Scan# 7
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

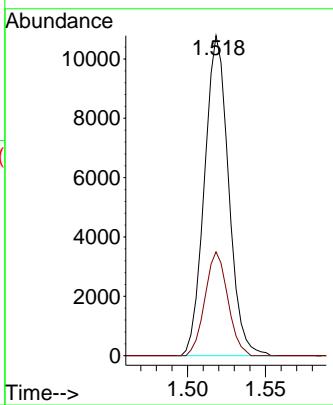

#4
Vinyl Chloride
Concen: 2.103 ug/l
RT: 1.599 min Scan# 96
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 62 Resp: 14856
Ion Ratio Lower Upper
62 100
64 32.4 25.7 38.5



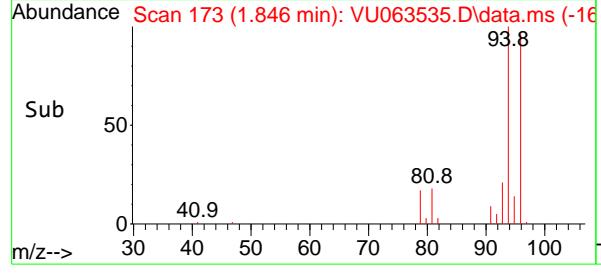
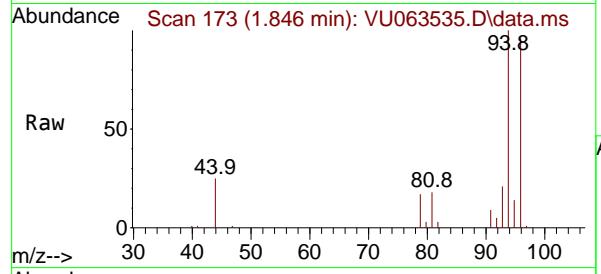
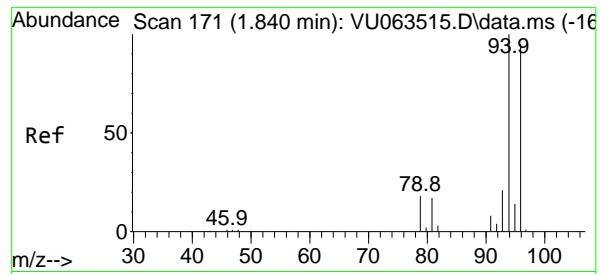


#5
Bromomethane
Concen: 2.349 ug/l
RT: 1.846 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02



Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

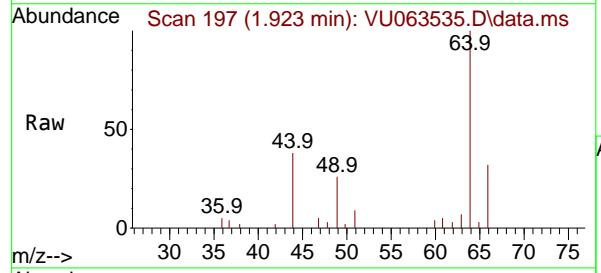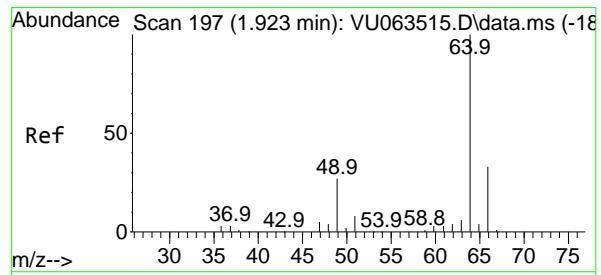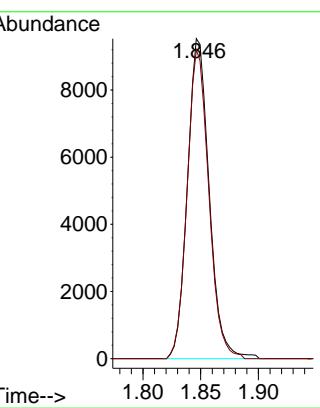

#6
Chloroethane
Concen: 2.217 ug/l
RT: 1.923 min Scan# 197
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 64 Resp: 9455
Ion Ratio Lower Upper
64 100
66 31.6 26.2 39.4

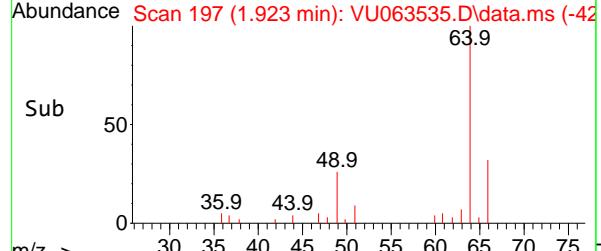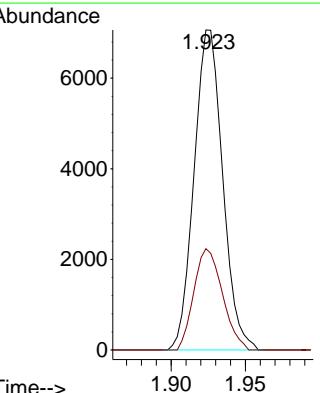

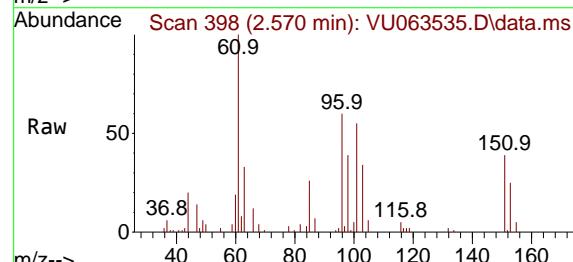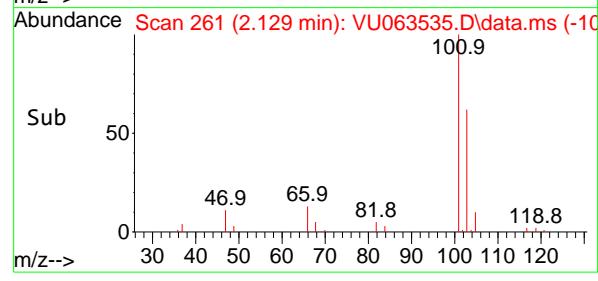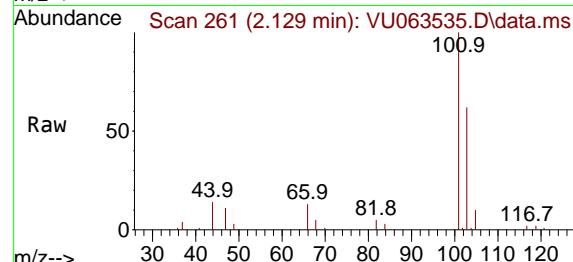

#7

Trichlorofluoromethane

Concen: 2.168 ug/l

RT: 2.129 min Scan# 2

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

Tgt Ion:101 Resp: 2198

Ion Ratio Lower Upper


101 100

103 62.4 52.2 78.4

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

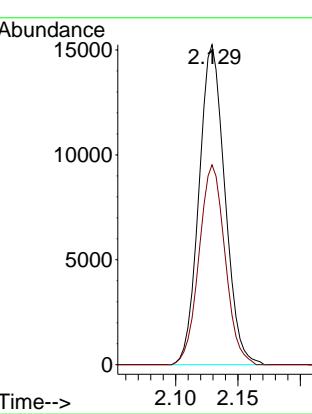

#8

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 2.198 ug/l

RT: 2.570 min Scan# 398

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Tgt Ion:101 Resp: 11650


Ion Ratio Lower Upper

101 100

85 47.7 37.8 56.6


151 72.7 59.2 88.8

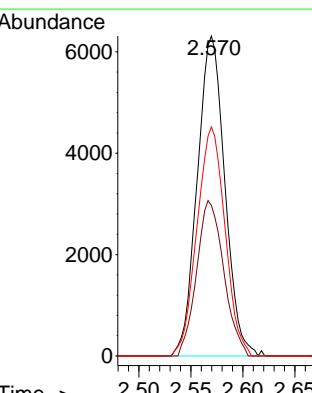



#9
1,1-Dichloroethene
Concen: 2.183 ug/l
RT: 2.570 min Scan# 3
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50




Instrument : MSVOA_U
ClientSampleId : VU0718WBS02




Tgt Ion: 96 Resp: 11469
Ion Ratio Lower Upper
96 100
61 167.6 0.0 504.3
98 64.7 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

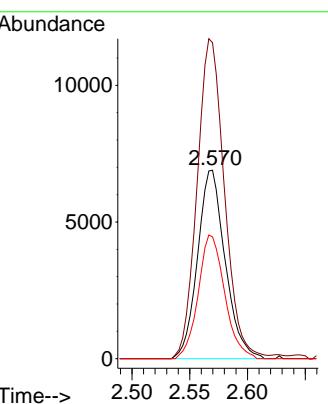


#10
Iodomethane
Concen: 1.886 ug/l
RT: 2.711 min Scan# 442
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50




Tgt Ion:142 Resp: 8386
Ion Ratio Lower Upper
142 100
127 45.2 37.9 56.9

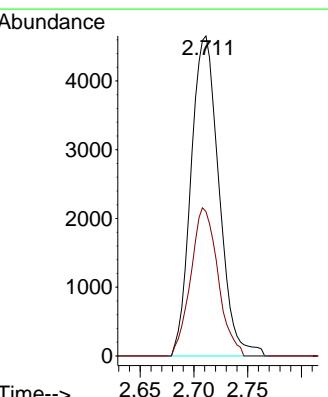



#11
Allyl Chloride
Concen: 2.000 ug/l
RT: 2.910 min Scan# 5
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50




Instrument : MSVOA_U
ClientSampleId : VU0718WBS02




Tgt Ion: 41 Resp: 15179
Ion Ratio Lower Upper
41 100
39 84.0 61.5 92.3

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

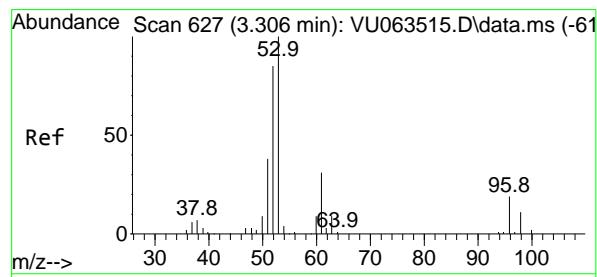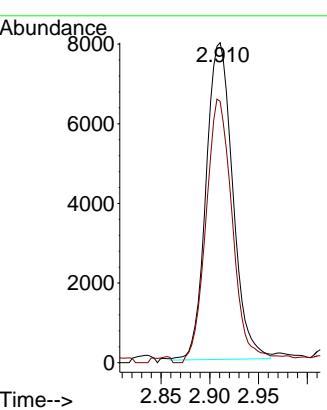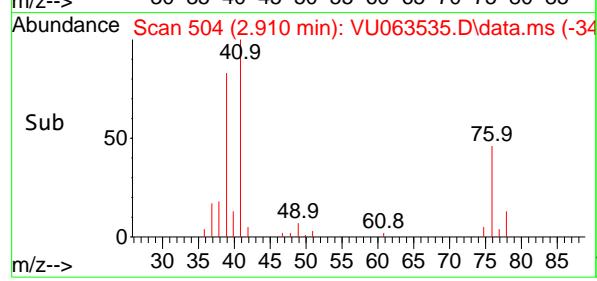


#12
Acrylonitrile
Concen: 4.022 ug/l
RT: 3.306 min Scan# 627
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

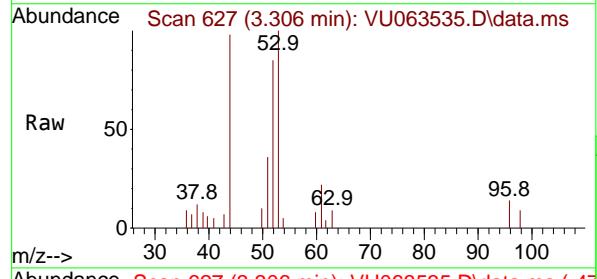


Tgt Ion: 53 Resp: 5284
Ion Ratio Lower Upper
53 100
52 82.2 64.3 96.5
51 37.2 27.8 41.8

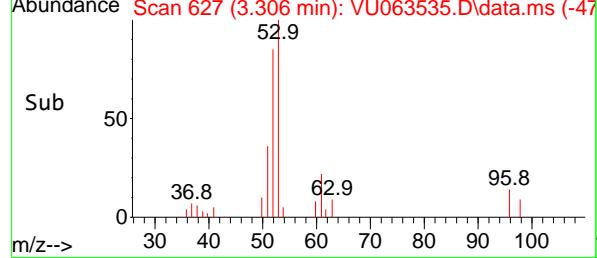



#13
Acetone
Concen: 10.172 ug/l
RT: 2.618 min Scan# 4
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50




Instrument :
MSVOA_U
ClientSampleId :
VU0718WBS02




Tgt Ion: 43 Resp: 1070
Ion Ratio Lower Upper
43 100
58 31.2 25.4 38.0

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025





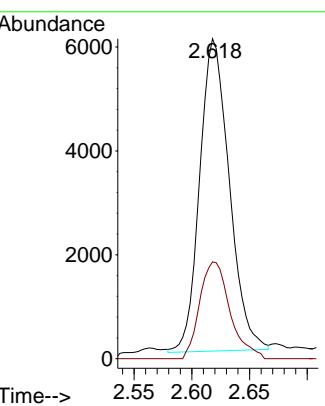



#14
Carbon Disulfide
Concen: 1.761 ug/l
RT: 2.779 min Scan# 463
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50



Tgt Ion: 76 Resp: 29884
Ion Ratio Lower Upper
76 100
78 9.8 7.0 10.6

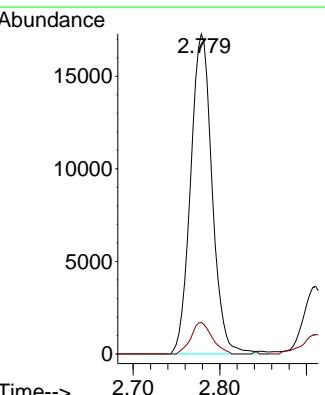



#15

Methylene Chloride

Concen: 2.197 ug/l

RT: 3.029 min Scan# 541

Delta R.T. -0.000 min


Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
 ClientSampleId : VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

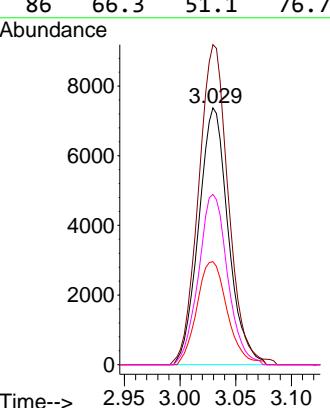

#16
 trans-1,2-Dichloroethene
 Concen: 2.125 ug/l
 RT: 3.335 min Scan# 636
 Delta R.T. -0.000 min
 Lab File: VU063535.D
 Acq: 18 Jul 2025 11:50

Tgt Ion: 96 Resp: 12679
 Ion Ratio Lower Upper
 96 100
 61 153.3 117.2 175.8
 98 65.4 51.4 77.2

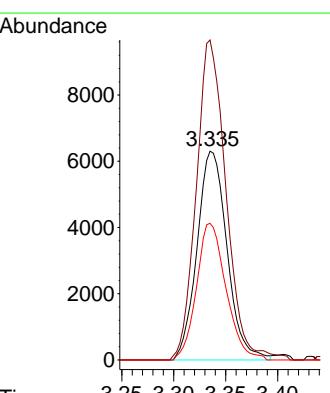






#17

1,1-Dichloroethane
Concen: 2.245 ug/l
RT: 3.849 min Scan# 796
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025









#18

2-Butanone
Concen: 10.962 ug/l
RT: 4.717 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 43 Resp: 17869
Ion Ratio Lower Upper
43 100
57 8.3 0.0 16.4

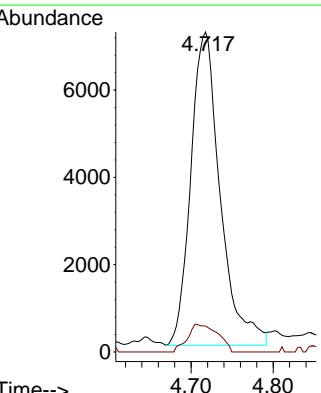

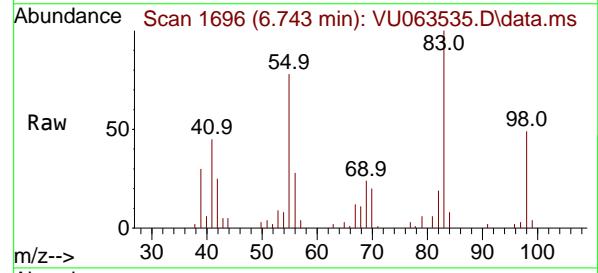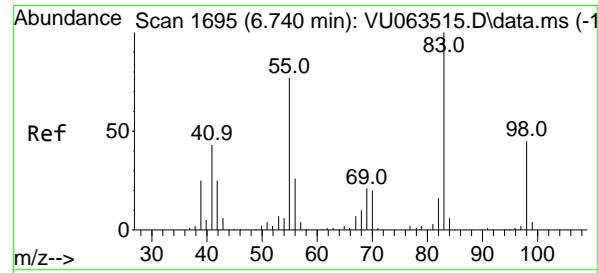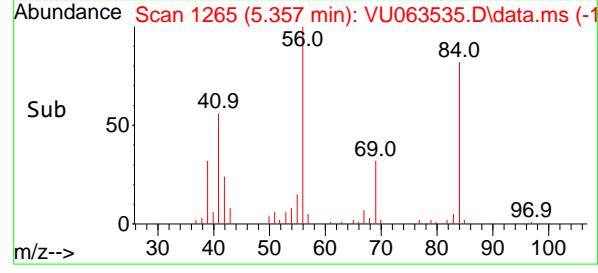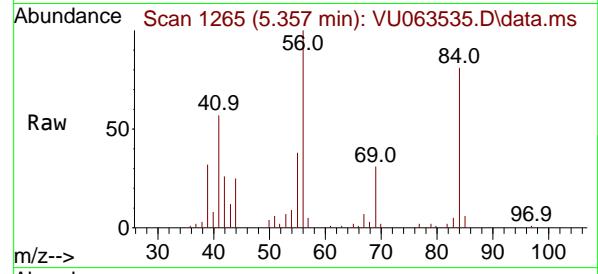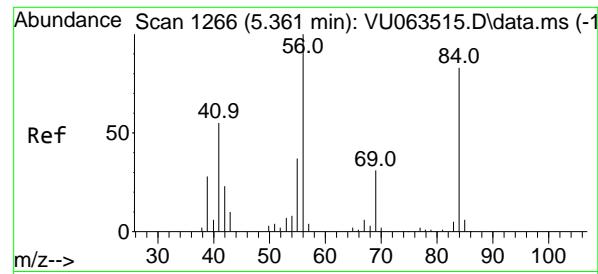

#19

Cyclohexane

Concen: 2.152 ug/l

RT: 5.357 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U


ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

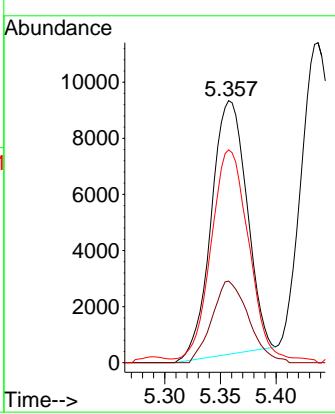

#20

Methylcyclohexane

Concen: 1.830 ug/l


RT: 6.743 min Scan# 1696




Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt	Ion	Resp:	16656
Ion	Ratio	Lower	Upper
83	100		
55	75.8	60.6	90.8
98	46.4	35.8	53.8





#21

2,2-Dichloropropane

Concen: 2.039 ug/l

RT: 4.644 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50




Instrument :

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

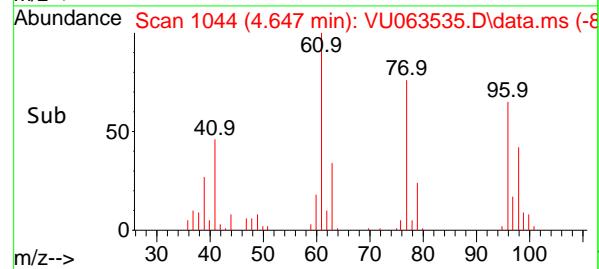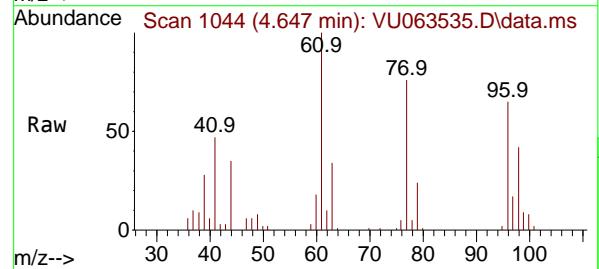 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#22

cis-1,2-Dichloroethene

Concen: 2.248 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Tgt Ion: 96 Resp: 14551




Ion Ratio Lower Upper

96 100

61 153.3 0.0 384.7

98 62.8 32.1 96.3

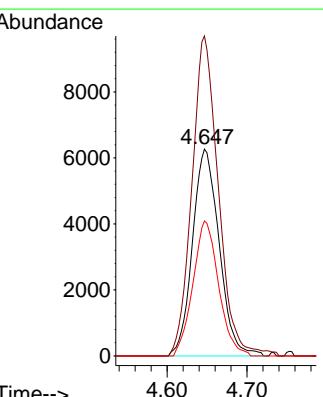

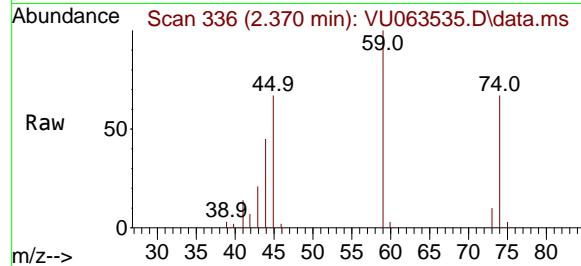

#23

Diethyl Ether

Concen: 2.265 ug/l

RT: 2.370 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument :

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025





Tgt Ion: 59 Resp: 9060

Ion Ratio Lower Upper

59 100

45 74.1 55.1 82.7

74 68.5 58.2 87.4



#24

tert-Butyl Alcohol

Concen: 20.656 ug/l

RT: 3.190 min Scan# 591

Delta R.T. -0.000 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50



Tgt Ion: 59 Resp: 9981

Ion Ratio Lower Upper

59 100

57 11.6 8.6 12.8



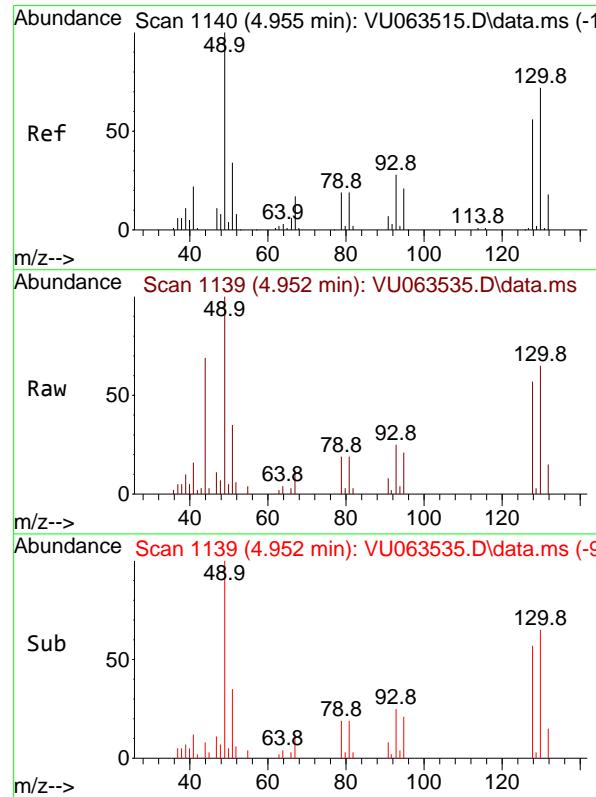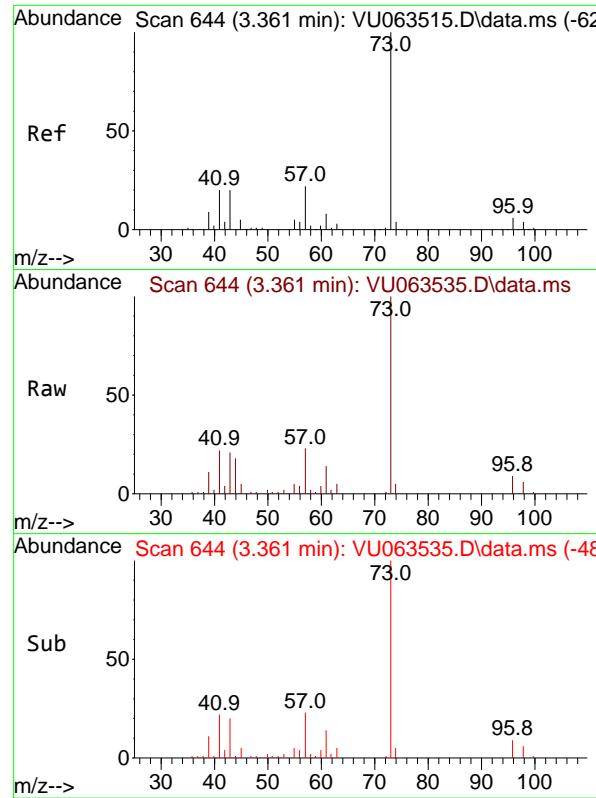


#25

Methyl tert-Butyl Ether
Concen: 2.233 ug/l
RT: 3.361 min Scan# 6
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#26
Bromochloromethane
Concen: 2.222 ug/l
RT: 4.952 min Scan# 1139
Delta R.T. -0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:128 Resp: 6006
Ion Ratio Lower Upper
128 100
49 181.8 0.0 340.8
130 119.6 100.5 150.7





#27

Chloroform

Concen: 2.252 ug/l

RT: 5.068 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

Tgt Ion: 83 Resp: 2541

Ion Ratio Lower Upper

83 100


85 61.1

0.0 130.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

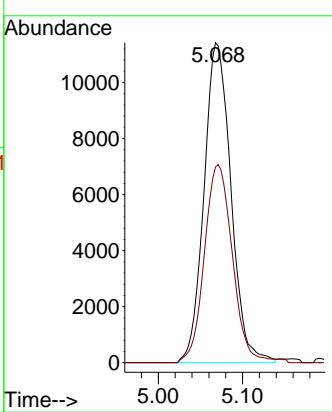

#28

1,1,1-Trichloroethane

Concen: 2.073 ug/l

RT: 5.293 min Scan# 1245

Delta R.T. -0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt Ion: 97 Resp: 19854

Ion Ratio Lower Upper


97 100




99 65.2

31.8 95.3

61 50.8

23.3 69.9

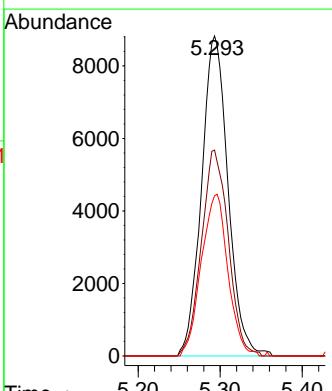







#29

1,1-Dichloropropene
Concen: 2.155 ug/l
RT: 5.502 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



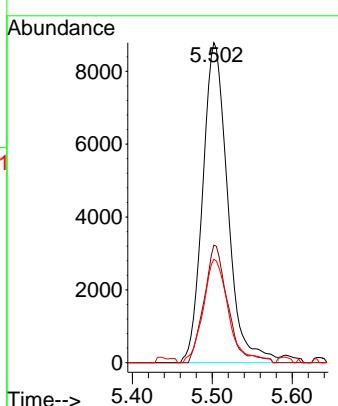


#30

Carbon Tetrachloride
Concen: 1.963 ug/l
RT: 5.496 min Scan# 1308
Delta R.T. -0.006 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:117 Resp: 15127
Ion Ratio Lower Upper
117 100
119 95.0 79.2 118.8
121 30.1 25.5 38.3

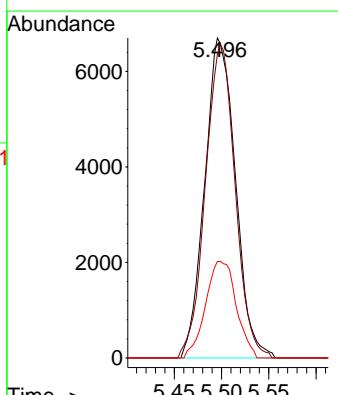

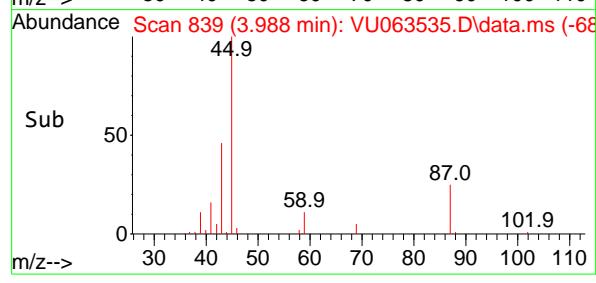

#31

Isopropyl Ether

Concen: 2.311 ug/l

RT: 3.988 min Scan# 8

Instrument:

Delta R.T. -0.003 min

MSVOA_U

Lab File: VU063535.D

ClientSampleId :

Acq: 18 Jul 2025 11:50

VU0718WBS02

Tgt Ion: 45 Resp: 38563

Ion Ratio Lower Upper





45 100

43 49.0 25.7 77.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

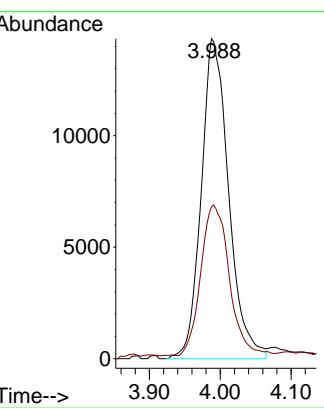

#32

Ethyl-t-butyl ether

Concen: 2.192 ug/l

RT: 4.502 min Scan# 999

Delta R.T. -0.000 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50


Tgt Ion: 59 Resp: 33853

Ion Ratio Lower Upper

59 100

87 41.5 32.6 49.0

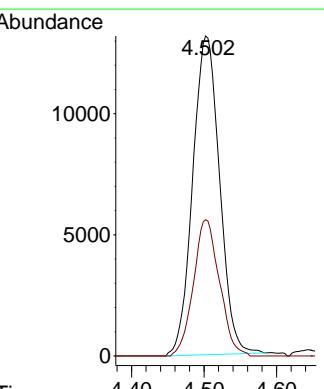

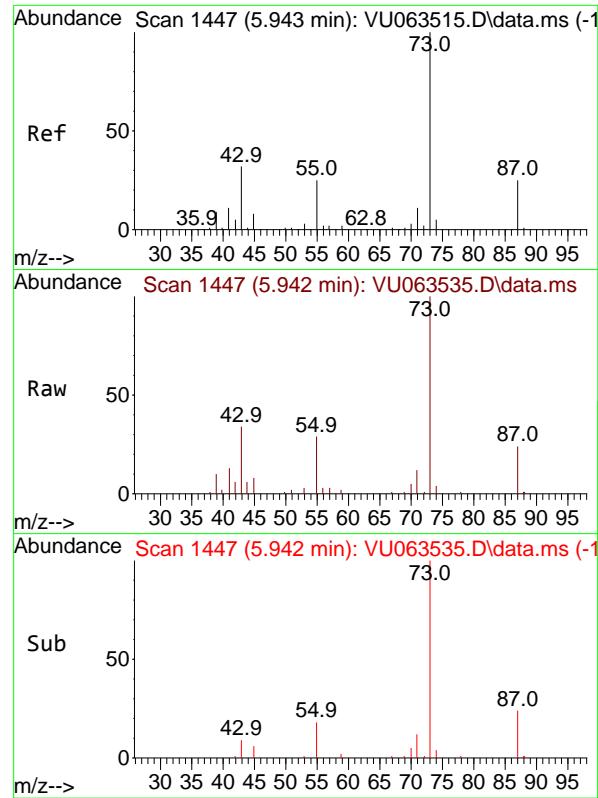


#33

Tert-Amyl methyl ether
Concen: 1.728 ug/l
RT: 5.942 min Scan# 1447
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



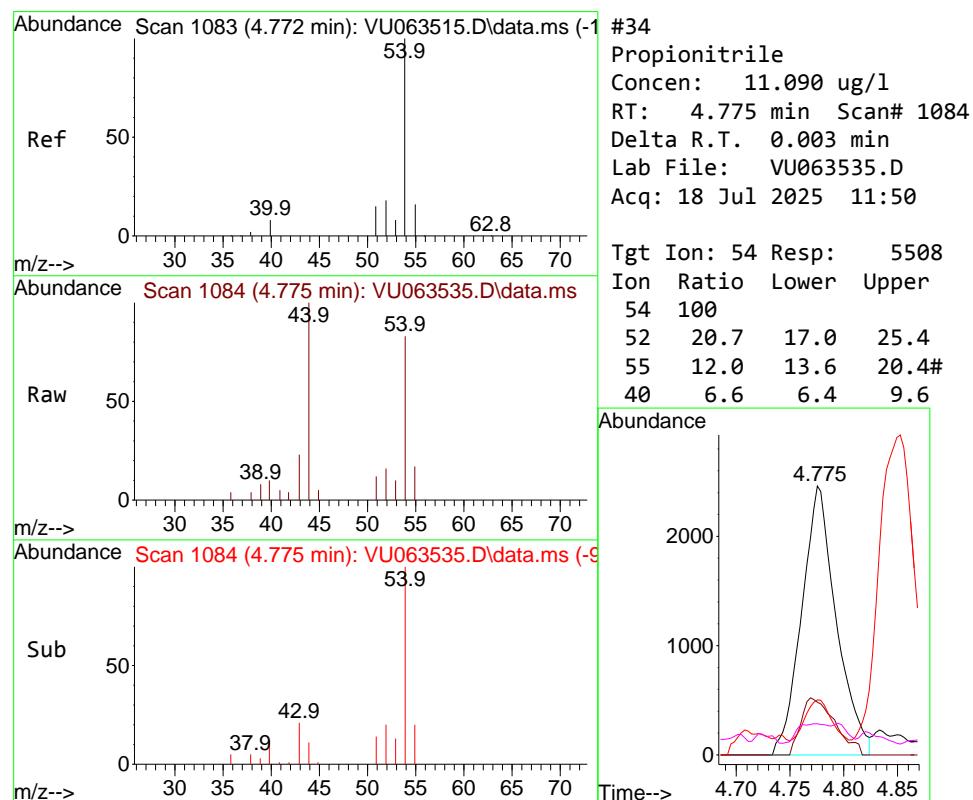


#34

Propionitrile
Concen: 11.090 ug/l
RT: 4.775 min Scan# 1084
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 54 Resp: 5508
Ion Ratio Lower Upper
54 100
52 20.7 17.0 25.4
55 12.0 13.6 20.4#
40 6.6 6.4 9.6

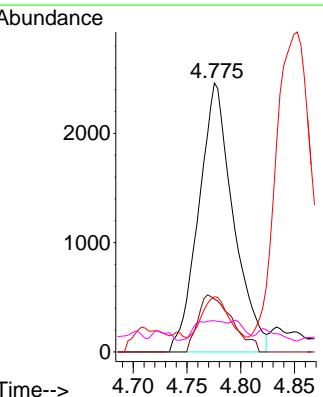



#35

Benzene

Concen: 1.832 ug/l

RT: 5.756 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

Tgt Ion: 78 Resp: 4367

Ion Ratio Lower Upper





78 100

77 22.5 19.4 29.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

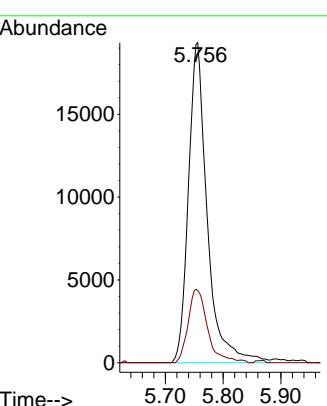

#36

1,2-Dichloroethane

Concen: 1.838 ug/l

RT: 5.779 min Scan# 1396

Delta R.T. -0.003 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50


Tgt Ion: 62 Resp: 13615

Ion Ratio Lower Upper

62 100


98 7.8 6.4 9.6

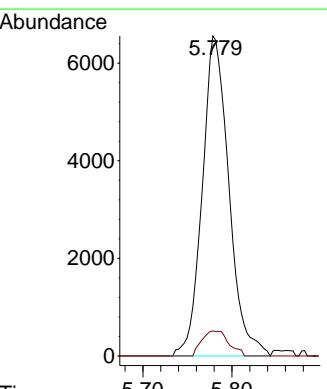



#37
Trichloroethene
Concen: 1.862 ug/l
RT: 6.528 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50



Instrument : MSVOA_U
ClientSampleId : VU0718WBS02




Tgt Ion:130 Resp: 11322
Ion Ratio Lower Upper
130 100
95 110.6 80.3 120.5

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#38
1,2-Dichloropropane
Concen: 1.860 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50



Tgt Ion: 63 Resp: 10377
Ion Ratio Lower Upper
63 100
65 35.4 24.6 36.8

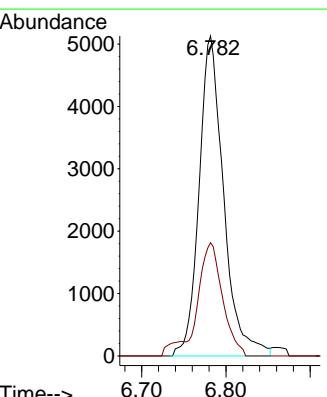



#39

Methacrylonitrile

Concen: 2.039 ug/l

RT: 4.975 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50




Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#40

Methyl acrylate

Concen: 2.087 ug/l

RT: 4.853 min Scan# 1108

Delta R.T. 0.006 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt Ion: 55 Resp: 6736




Ion Ratio Lower Upper

55 100

85 15.8 12.8 19.2

58 7.7 7.0 10.4

42 7.8 7.0 10.4

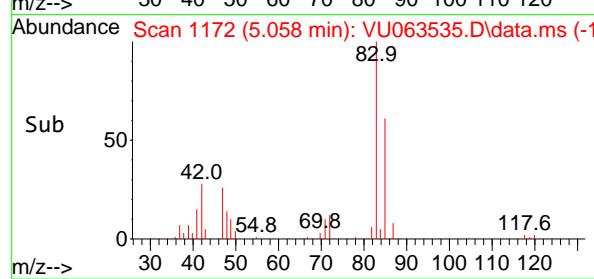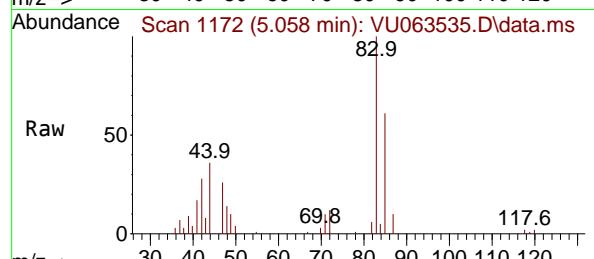

#41

Tetrahydrofuran

Concen: 4.799 ug/l

RT: 5.058 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50





Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

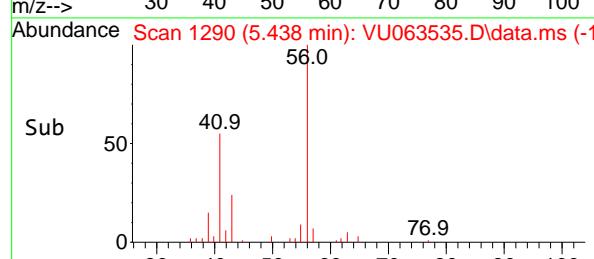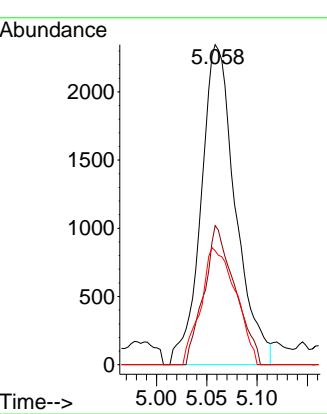 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#42

1-Chlorobutane


Concen: 2.024 ug/l


RT: 5.438 min Scan# 1290

Delta R.T. -0.000 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50

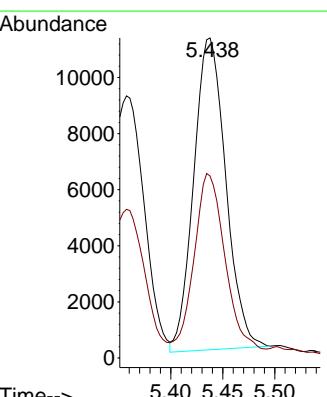 Tgt Ion: 56 Resp: 23868
 Ion Ratio Lower Upper
 56 100
 41 53.9 26.7 80.0

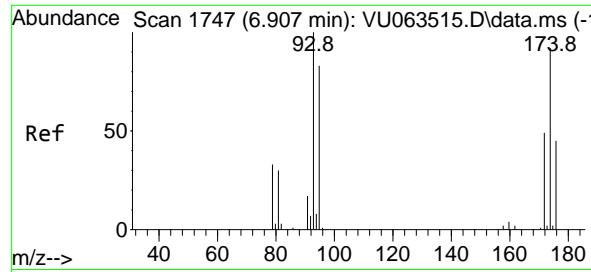


#43
Dibromomethane
Concen: 1.979 ug/l
RT: 6.910 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50




Instrument : MSVOA_U
ClientSampleId : VU0718WBS02



Tgt Ion: 93 Resp: 5720
Ion Ratio Lower Upper
93 100
95 80.8 67.9 101.9
174 82.6 74.6 111.8




Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

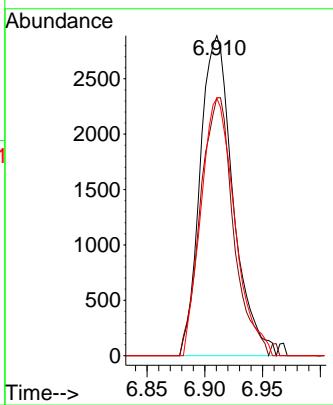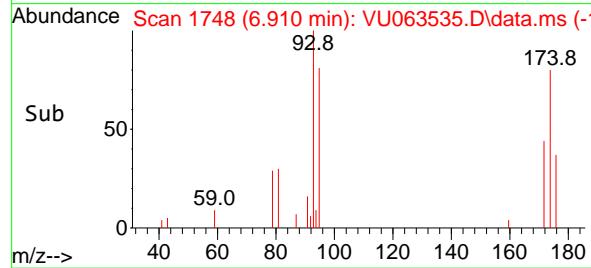

#44
Bromodichloromethane
Concen: 1.818 ug/l
RT: 7.097 min Scan# 1806
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 83 Resp: 11850
Ion Ratio Lower Upper
83 100
85 57.7 52.7 79.1
127 8.1 8.1 12.1

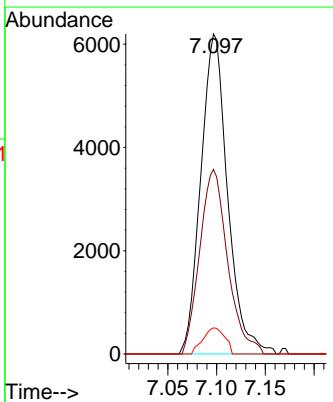

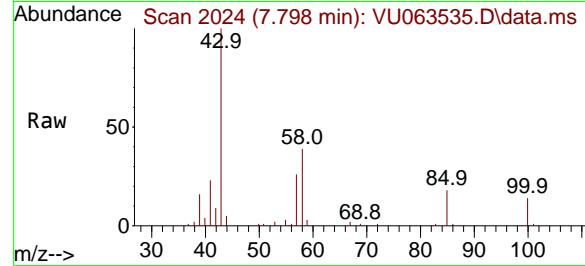

#45

4-Methyl-2-Pentanone

Concen: 10.474 ug/l

RT: 7.798 min Scan# 2

Instrument :

Delta R.T. -0.000 min

MSVOA_U




Lab File: VU063535.D

ClientSampleId :

Acq: 18 Jul 2025 11:50

VU0718WBS02

**Manual Integrations
APPROVED**

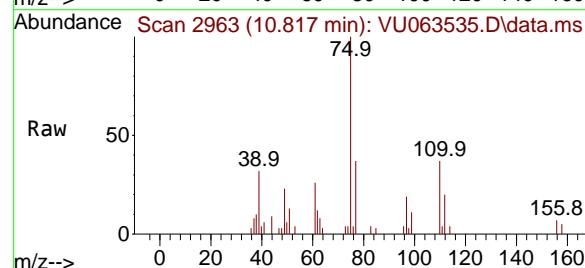 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#46

t-1,4-Dichloro-2-butene

Concen: 4.640 ug/l

RT: 10.817 min Scan# 2963

Delta R.T. -0.006 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt Ion: 75 Resp: 5188


Ion Ratio Lower Upper


75 100

53 50.1 48.4 72.6

89 21.9 30.6 45.8#

88 18.6 25.3 37.9#


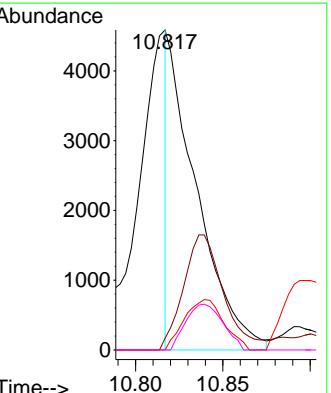




#47

Methyl methacrylate
Concen: 3.707 ug/l
RT: 6.968 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02





Tgt Ion: 69 Resp: 8990

Ion Ratio	Lower	Upper
69 100		
41 118.1	0.0	224.0
39 74.7	55.3	82.9
100 30.8	29.0	43.6




Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

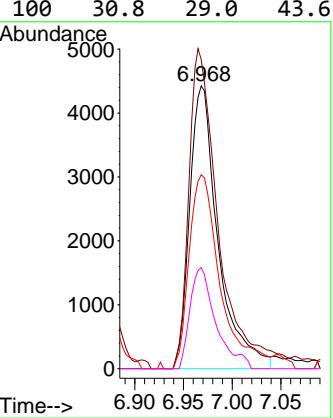

#48
Ethyl methacrylate
Concen: 2.006 ug/l
RT: 8.335 min Scan# 2191
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 69 Resp: 9290
Ion Ratio Lower Upper
69 100
41 62.7 30.8 92.4



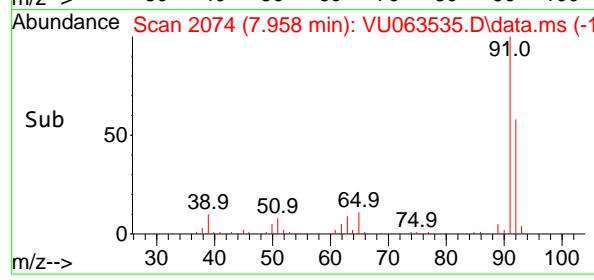

#49

Toluene

Concen: 1.978 ug/l

RT: 7.958 min Scan# 2

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50






Instrument:







MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

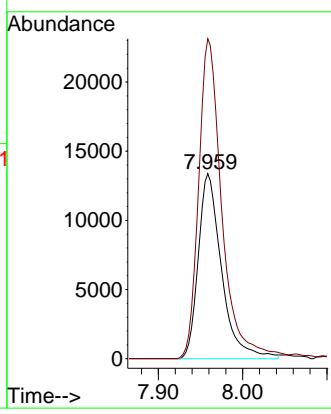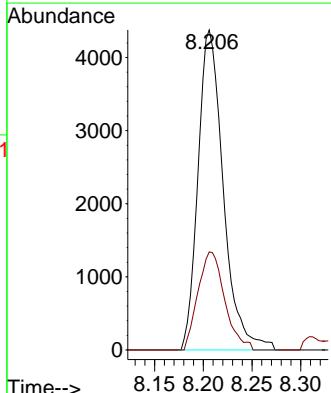 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

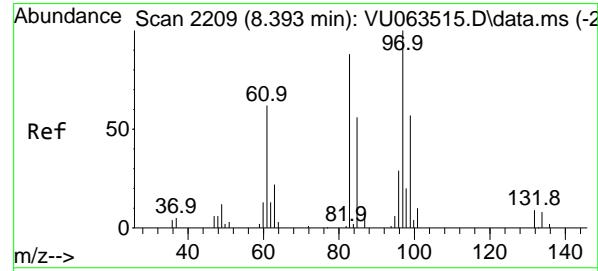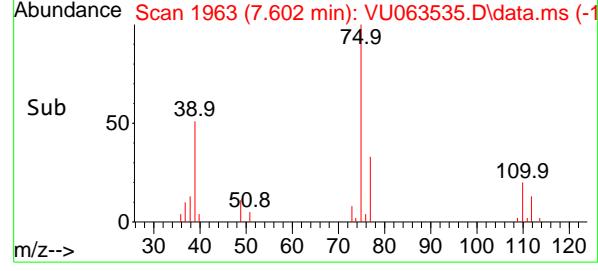 #50
 t-1,3-Dichloropropene
 Concen: 1.544 ug/l
 RT: 8.206 min Scan# 2151
 Delta R.T. 0.003 min
 Lab File: VU063535.D
 Acq: 18 Jul 2025 11:50

 Tgt Ion: 75 Resp: 7896
 Ion Ratio Lower Upper
 75 100
 77 30.7 24.9 37.3




#51

cis-1,3-Dichloropropene

Concen: 1.623 ug/l

RT: 7.602 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Instrument :

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

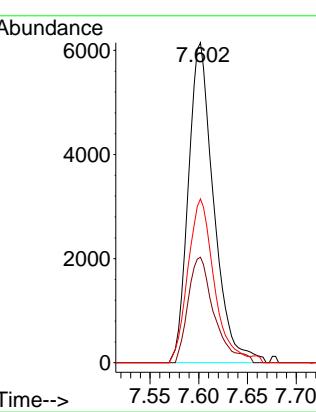 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#52

1,1,2-Trichloroethane

Concen: 2.103 ug/l

RT: 8.393 min Scan# 2209

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt Ion: 97 Resp: 8183


Ion Ratio Lower Upper







97 100

83 91.6 70.2 105.2

85 57.3 45.2 67.8

99 60.2 50.1 75.1

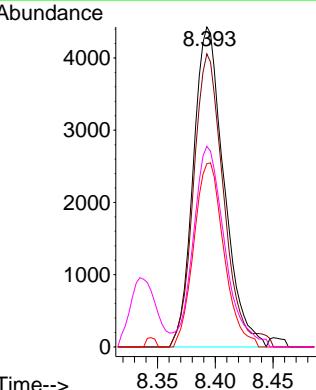



#53

1,3-Dichloropropane

Concen: 2.071 ug/l

RT: 8.569 min Scan# 2

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

Tgt Ion: 76 Resp: 13909

Ion Ratio Lower Upper


76 100

78 32.8 26.0 39.0

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

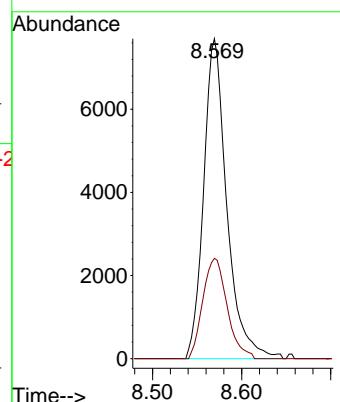

#54
2-Hexanone
Concen: 10.036 ug/l
RT: 8.692 min Scan# 2302
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50


Tgt Ion: 43 Resp: 19855




Ion Ratio Lower Upper

43 100

58 56.5 34.8 74.8

57 19.3 0.0 39.5

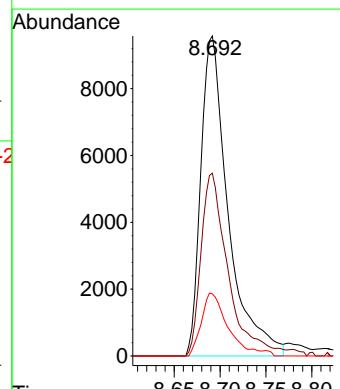



#55

Dibromochloromethane

Concen: 1.606 ug/l

RT: 8.801 min Scan# 2336

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50




Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#56

1,2-Dibromoethane

Concen: 1.935 ug/l

RT: 8.917 min Scan# 2372

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Tgt Ion:107 Resp: 6737


Ion Ratio Lower Upper

107 100

109 92.4 0.0 186.4

Abundance

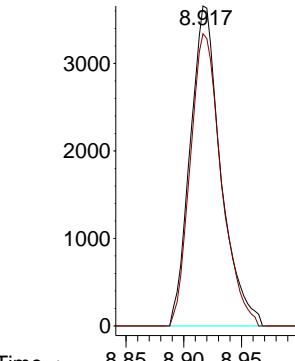

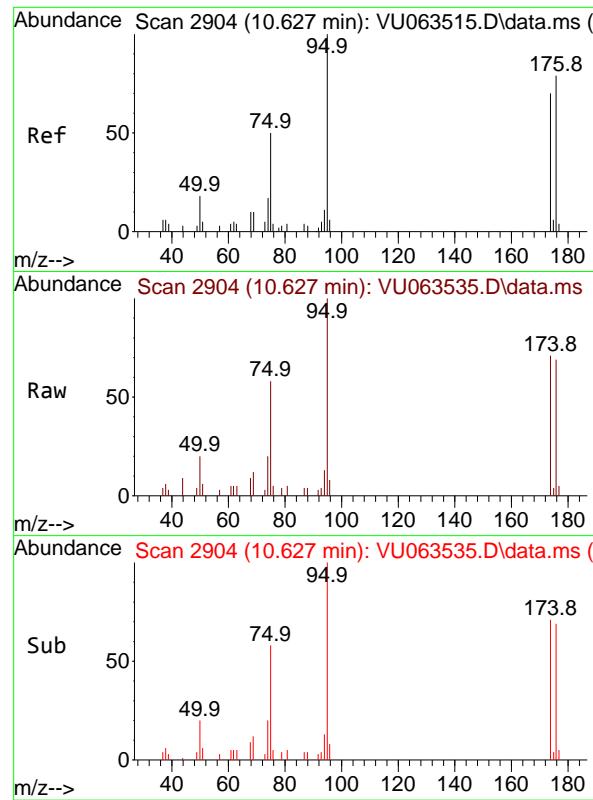

#57

4-Bromofluorobenzene

Concen: 1.032 ug/l

RT: 10.627 min Scan# 2

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:



MSVOA_U

ClientSampleId :

VU0718WBS02

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

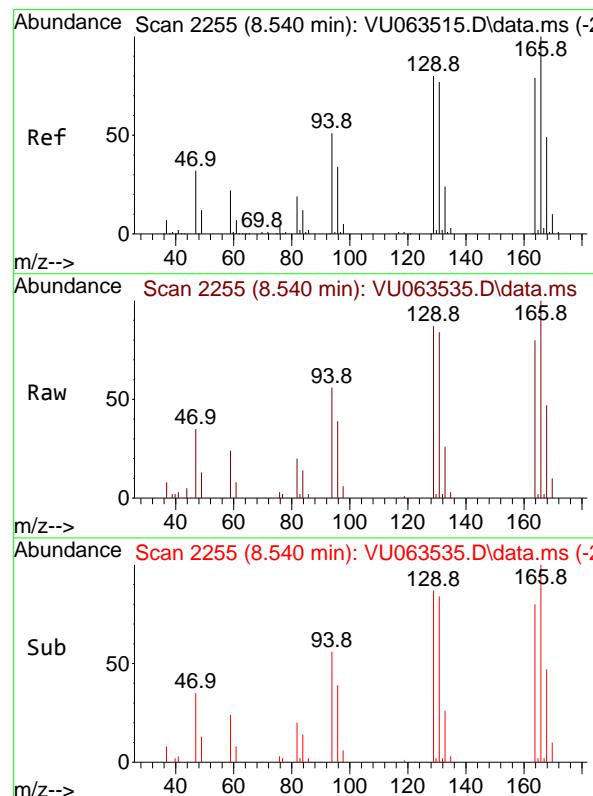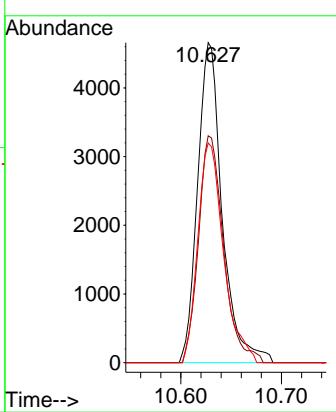

#58

Tetrachloroethene


Concen: 1.891 ug/l


RT: 8.540 min Scan# 2255

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


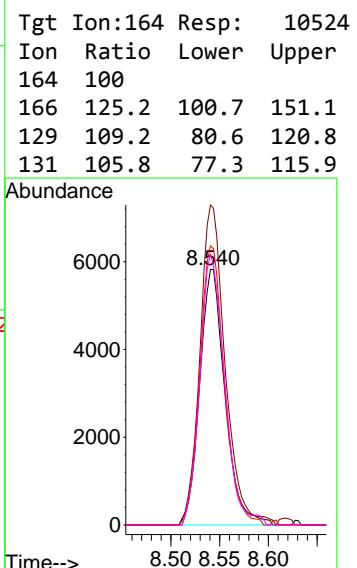


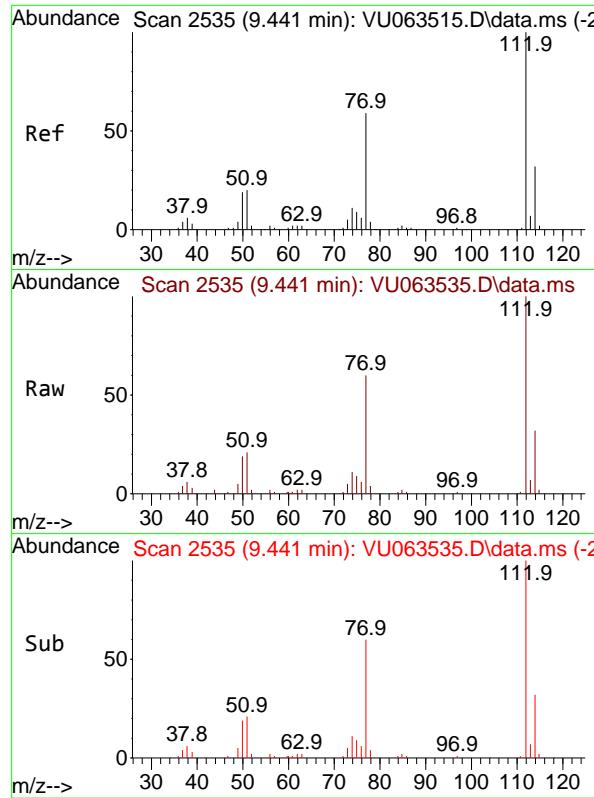

#59
Chlorobenzene
Concen: 1.968 ug/l
RT: 9.441 min Scan# 2
Instrument: MSVOA_U
Delta R.T. -0.000 min
Lab File: VU063535.D
Client SampleId : VU0718WBS02
Acq: 18 Jul 2025 11:50


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

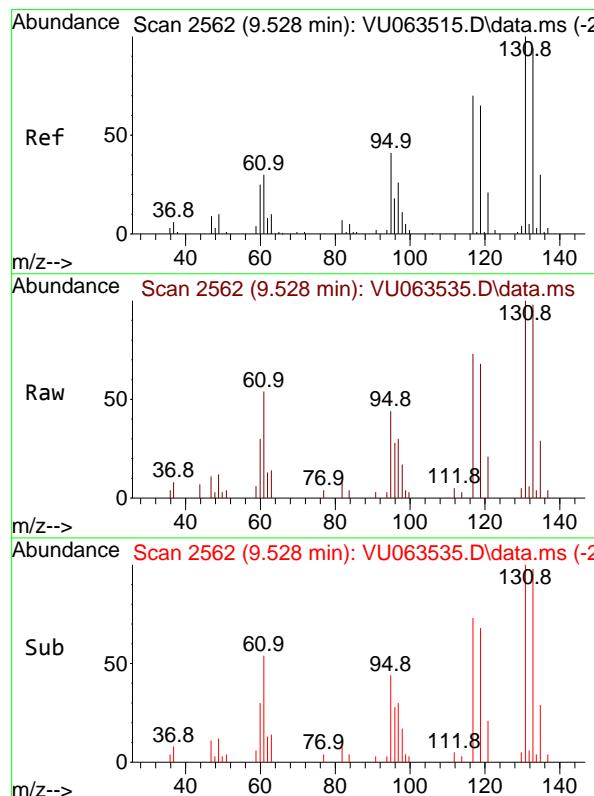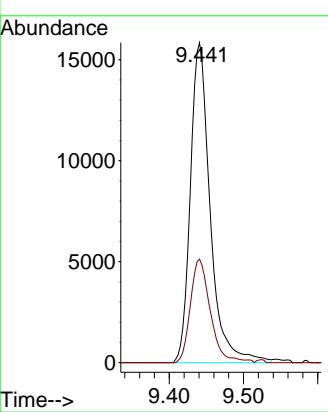

#60
1,1,1,2-Tetrachloroethane
Concen: 1.708 ug/l
RT: 9.528 min Scan# 2562
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:131 Resp: 8208
Ion Ratio Lower Upper
131 100
133 96.5 74.7 112.1
119 68.6 53.0 79.4

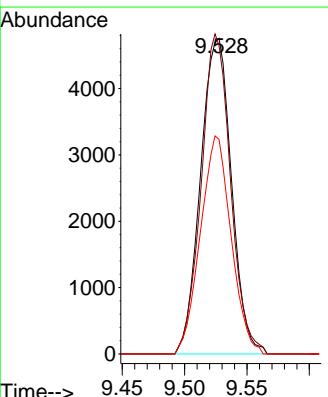



#61

Pentachloroethane

Concen: 1.812 ug/l

RT: 11.418 min Scan# 3150

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U




ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#62

Hexachloroethane

Concen: 1.512 ug/l



RT: 12.466 min Scan# 3476

Delta R.T. -0.000 min


Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
117	100				
201	65.6	57.4	5086	86.0	




Time-->

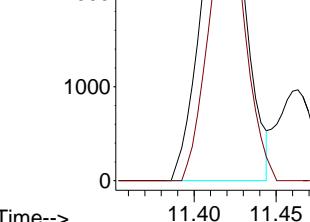

Time-->

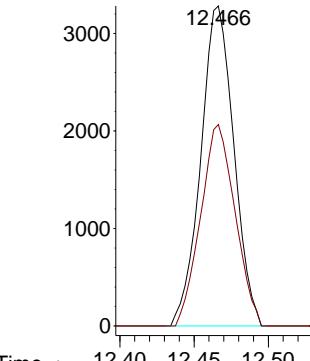

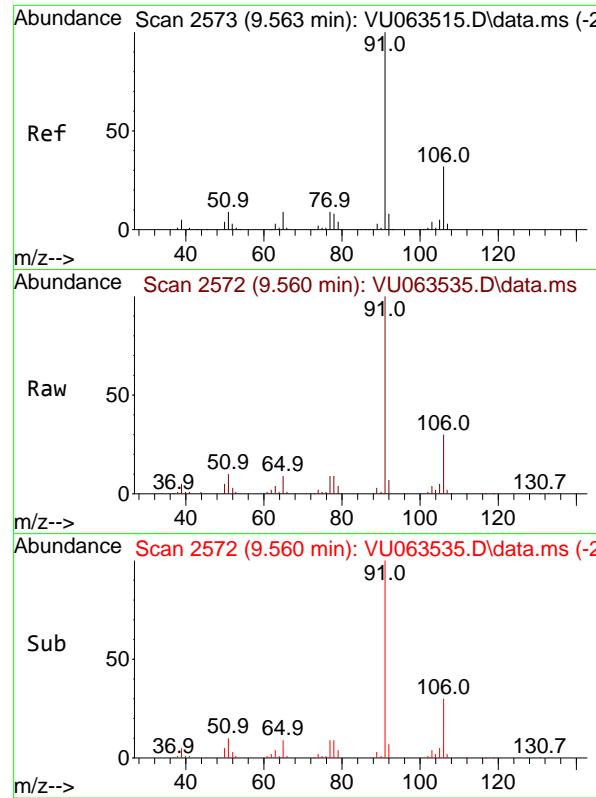

#63

Ethyl Benzene

Concen: 1.949 ug/l

RT: 9.560 min Scan# 2

Delta R.T. -0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U


ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

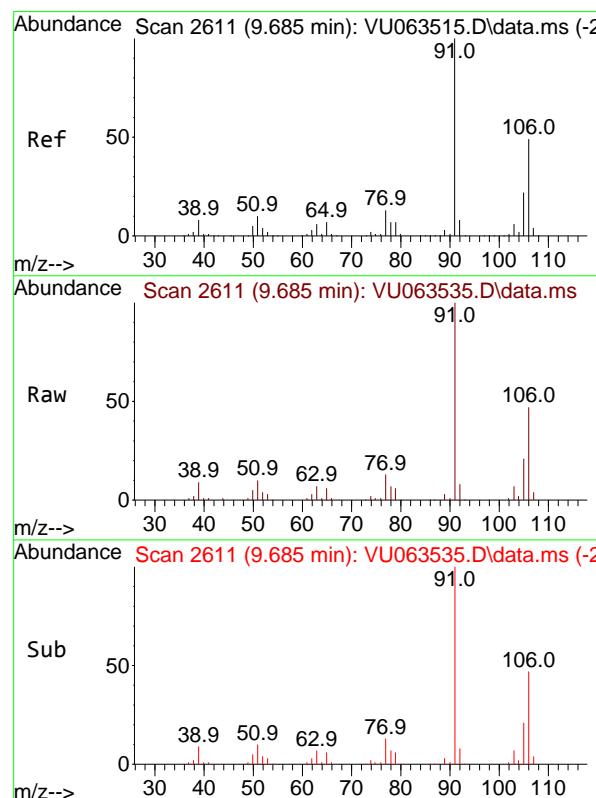

#64

m/p-Xylenes

Concen: 3.865 ug/l

RT: 9.685 min Scan# 2611

Delta R.T. -0.000 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50




Tgt Ion:106 Resp: 38644

Ion Ratio Lower Upper

106 100

91 213.0 163.6 245.4

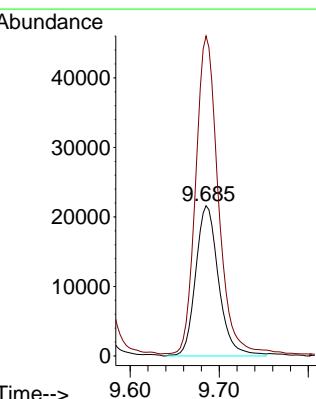







#65
o-Xylene
Concen: 1.950 ug/l
RT: 10.090 min Scan# 2
Delta R.T. -0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument :
MSVOA_U
ClientSampleId :
VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#66
Styrene
Concen: 1.964 ug/l
RT: 10.110 min Scan# 2743
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:104 Resp: 30077
Ion Ratio Lower Upper
104 100
78 53.0 41.3 61.9
103 56.0 43.6 65.4

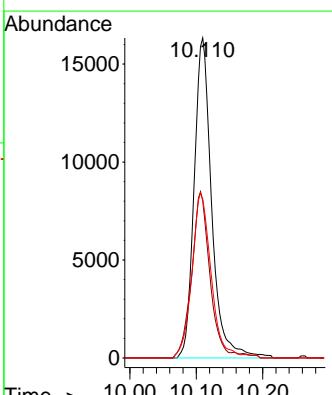



#67

Bromoform

Concen: 1.436 ug/l

RT: 10.283 min Scan# 2

Instrument:

MSVOA_U

Delta R.T. -0.000 min





Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.047 ug/l


RT: 12.183 min Scan# 3388




Delta R.T. -0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt	Ion:152	Resp:	7416
Ion	Ratio	Lower	Upper
152	100		
115	79.8	0.0	262.2
150	191.8	0.0	651.2





#69

Isopropylbenzene

Concen: 1.982 ug/l

RT: 10.476 min Scan# 2

Instrument :

Delta R.T. -0.000 min

MSVOA_U

Lab File: VU063535.D

ClientSampleId :

Acq: 18 Jul 2025 11:50

VU0718WBS02

Tgt Ion:105 Resp: 46030

Ion Ratio Lower Upper




105 100

120 26.3 13.2 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 1.985 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Tgt Ion: 83 Resp: 9398




Ion Ratio Lower Upper

83 100

131 10.5 8.4 12.6

85 66.4 51.9 77.9





#71

1,2,3-Trichloropropane

Concen: 1.950 ug/l m

RT: 10.817 min Scan# 2

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:




MSVOA_U

ClientSampleId :

VU0718WBS02

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

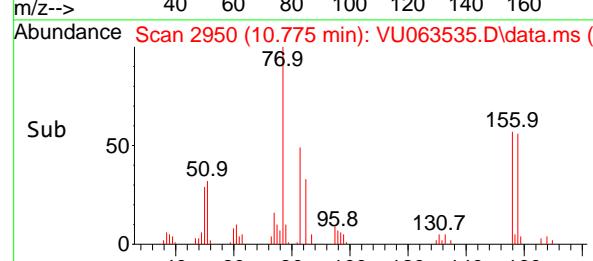

#72

Bromobenzene

Concen: 1.898 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50



Tgt Ion:156 Resp: 11376




Ion Ratio Lower Upper

156 100

77 202.7 0.0 315.2

158 98.5 0.0 195.4

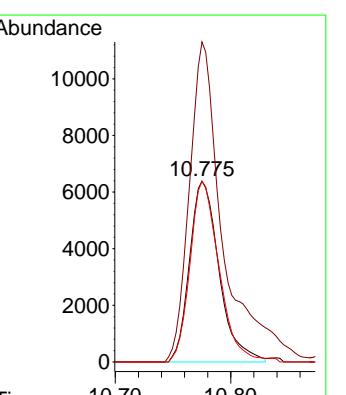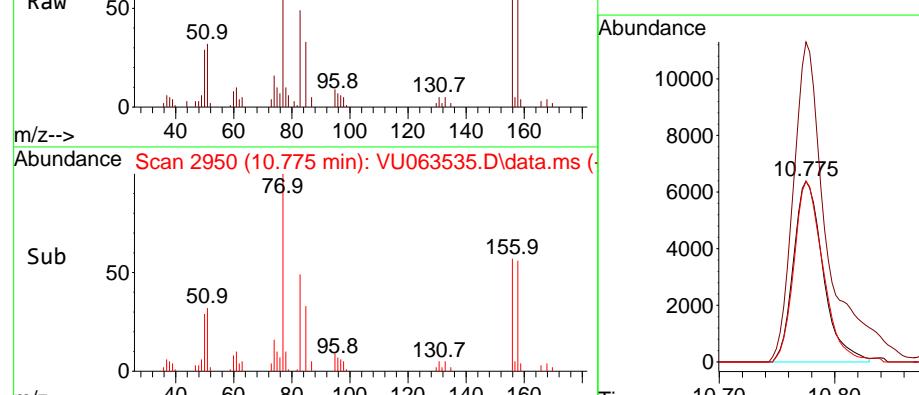



#73

n-propylbenzene

Concen: 1.984 ug/l

RT: 10.897 min Scan# 2

Instrument :

Delta R.T. -0.000 min

MSVOA_U

Lab File: VU063535.D

ClientSampleId :

Acq: 18 Jul 2025 11:50

VU0718WBS02

Tgt Ion:120 Resp: 1387:

Ion Ratio Lower Upper




120 100

91 443.3 343.1 514.7

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/21/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#74

2-Chlorotoluene

Concen: 1.902 ug/l

RT: 10.978 min Scan# 3013

Delta R.T. -0.000 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50




Tgt Ion:126 Resp: 11750

Ion Ratio Lower Upper

126 100

91 304.0 0.0 606.0

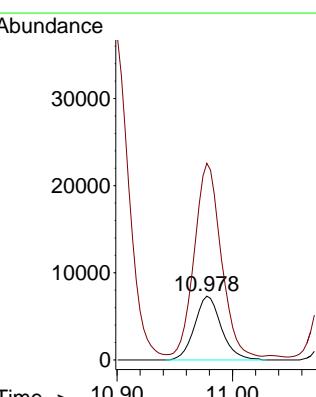







#75
1,3,5-Trimethylbenzene
Concen: 1.933 ug/l
RT: 11.081 min Scan# 3
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#76
4-Chlorotoluene
Concen: 2.018 ug/l
RT: 11.090 min Scan# 3048
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:126 Resp: 12663
Ion Ratio Lower Upper
126 100
91 338.0 0.0 682.2




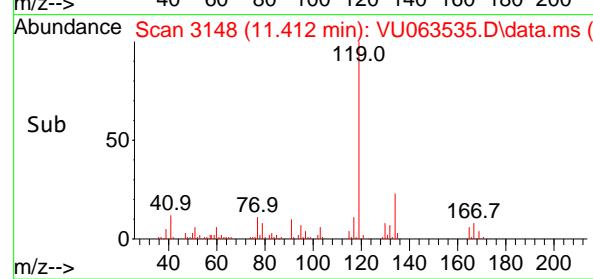
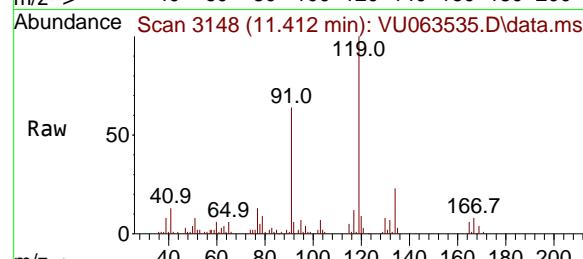



#77
tert-Butylbenzene
Concen: 1.951 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

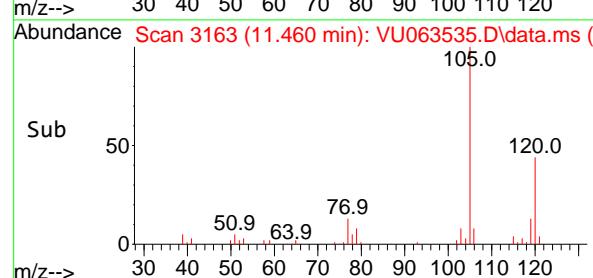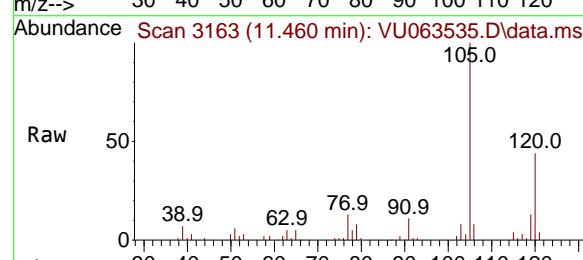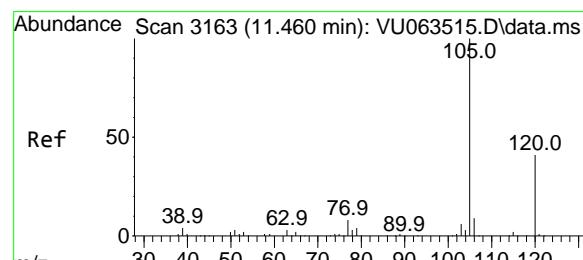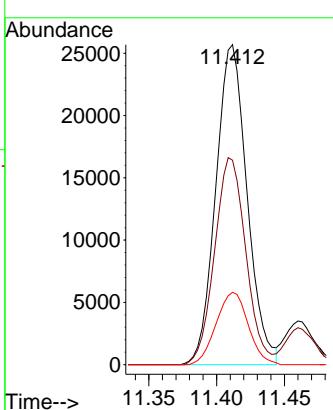

#78
1,2,4-Trimethylbenzene
Concen: 1.977 ug/l
RT: 11.460 min Scan# 3163
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:105 Resp: 43519
Ion Ratio Lower Upper
105 100
120 44.0 22.7 68.0








#79
sec-Butylbenzene
Concen: 2.009 ug/l
RT: 11.634 min Scan# 319
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02



Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

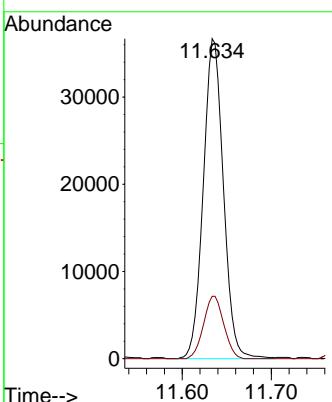

#80
Nitrobenzene
Concen: 8.625 ug/l
RT: 13.219 min Scan# 3710
Delta R.T. 0.016 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion: 77 Resp: 614
Ion Ratio Lower Upper
77 100
123 7.0 16.9 59.7#
65 0.0 16.5 20.9#

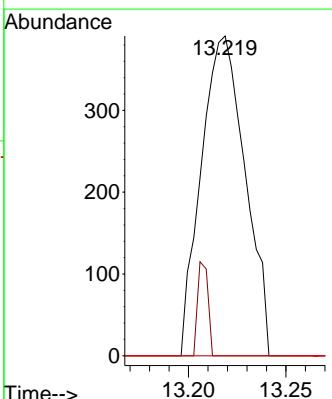






#81
p-Isopropyltoluene
Concen: 1.969 ug/l
RT: 11.785 min Scan# 3264
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Instrument : MSVOA_U
ClientSampleId : VU0718WBS02


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

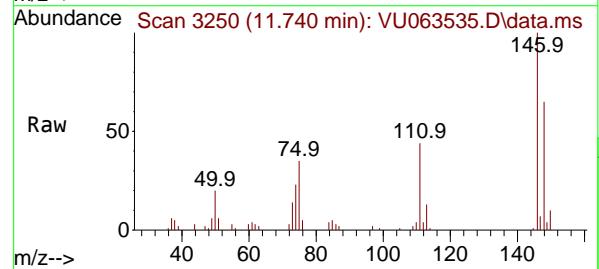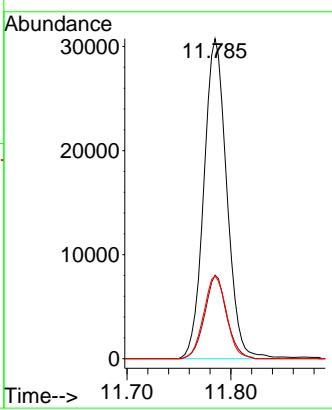

#82
1,3-Dichlorobenzene
Concen: 1.977 ug/l
RT: 11.740 min Scan# 3250
Delta R.T. 0.003 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:146 Resp: 23706
Ion Ratio Lower Upper
146 100
111 42.7 33.8 50.6
148 64.7 51.5 77.3

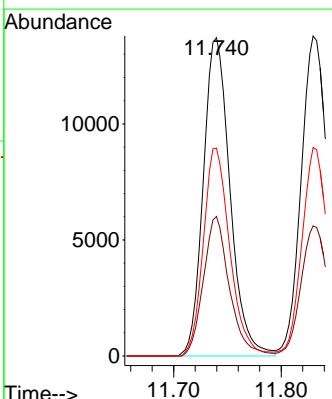



#83

1,4-Dichlorobenzene

Concen: 2.023 ug/l

RT: 11.830 min Scan# 3278

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50




Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#84

n-Butylbenzene

Concen: 2.024 ug/l

RT: 12.203 min Scan# 3394

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50




Tgt Ion: 91 Resp: 44796




Ion Ratio Lower Upper

91 100

92 54.4 41.5 62.3

134 24.6 20.6 30.8

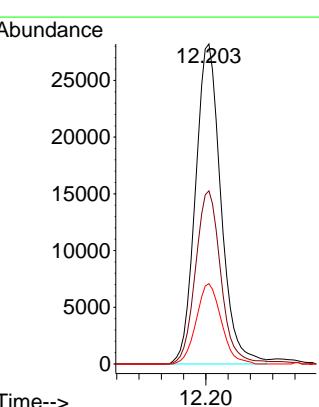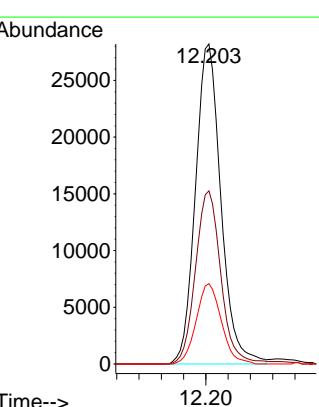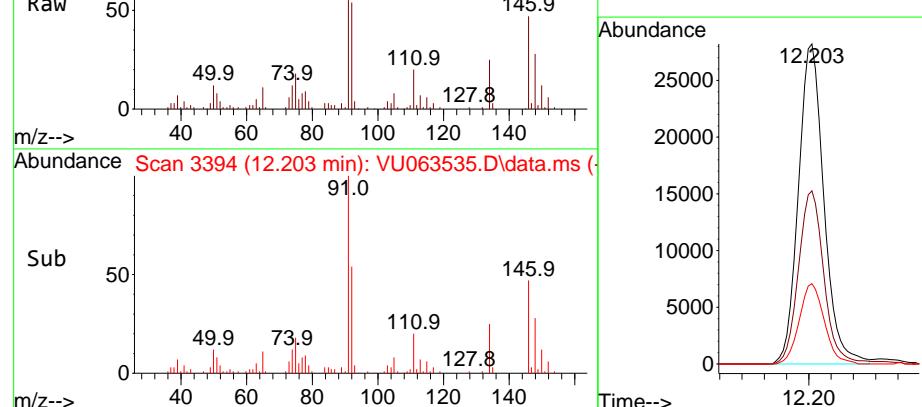



#85

1,2-Dichlorobenzene

Concen: 2.048 ug/l

RT: 12.206 min Scan# 3

Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02




Tgt Ion:146 Resp: 2307

Ion Ratio Lower Upper

146 100

111 44.7 21.7 65.1

148 62.3 31.8 95.3

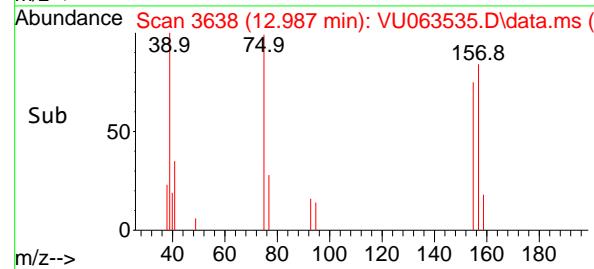**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#86

1,2-Dibromo-3-Chloropropane

Concen: 1.944 ug/l

RT: 12.987 min Scan# 3638

Delta R.T. 0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50


Tgt Ion: 75 Resp: 1197


Ion Ratio Lower Upper

75 100

155 72.5 65.8 98.6

157 85.3 81.4 122.2

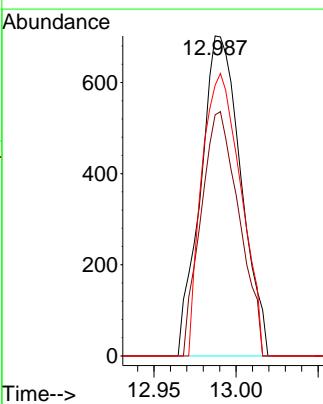

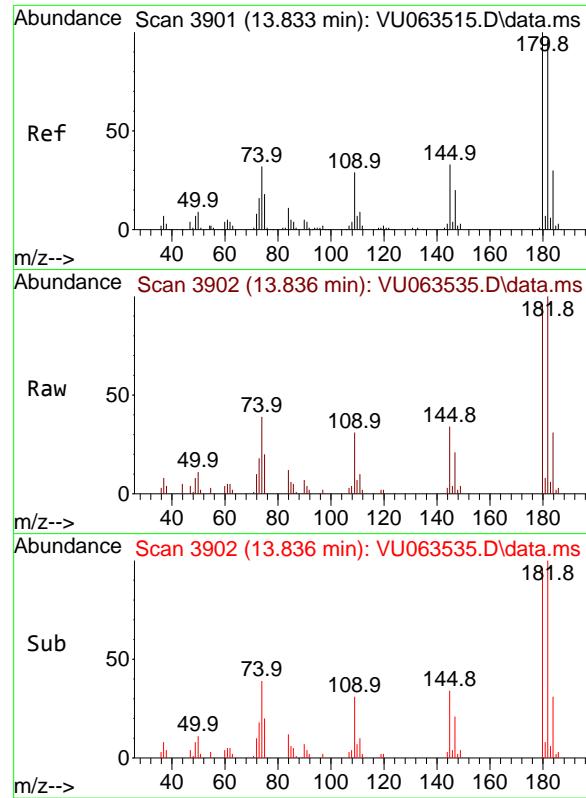

#87

1,2,4-Trichlorobenzene

Concen: 1.929 ug/l

RT: 13.836 min Scan# 3901

Delta R.T. 0.003 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50



Instrument:

MSVOA_U

ClientSampleId :

VU0718WBS02

**Manual Integrations
APPROVED**

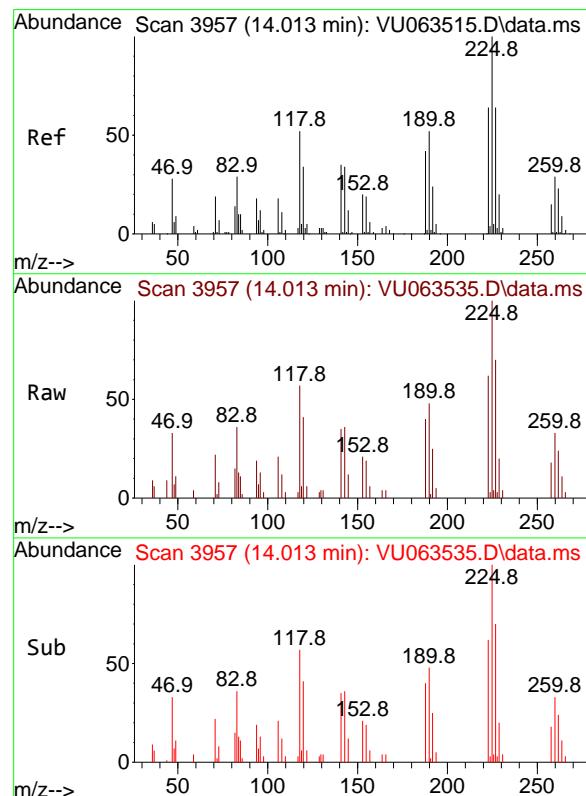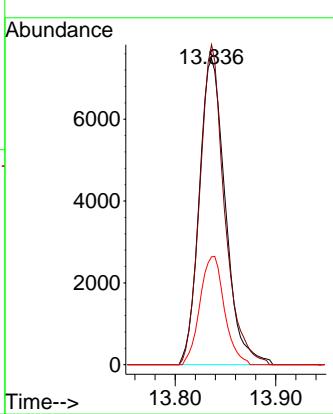 Reviewed By :Mahesh Dadoda 07/21/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#88

Hexachlorobutadiene

Concen: 1.894 ug/l


RT: 14.013 min Scan# 3957






Delta R.T. -0.000 min

Lab File: VU063535.D

Acq: 18 Jul 2025 11:50

Tgt	Ion:225	Resp:	7537
Ion	Ratio	Lower	Upper
225	100		
223	61.2	50.8	76.2
227	67.5	51.0	76.6

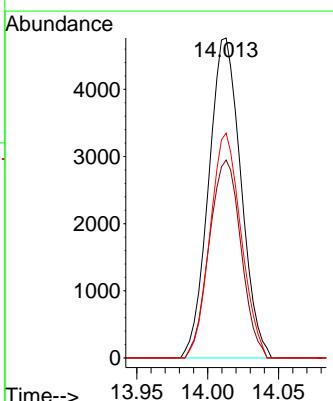

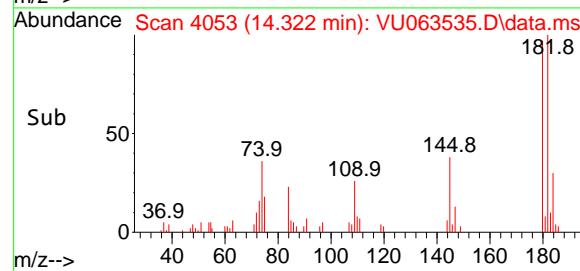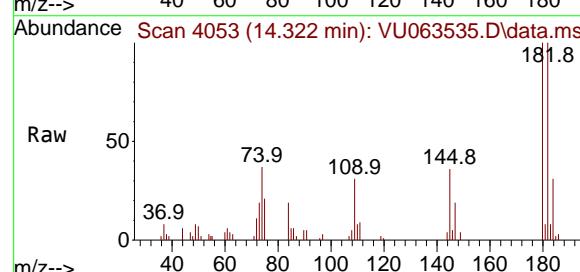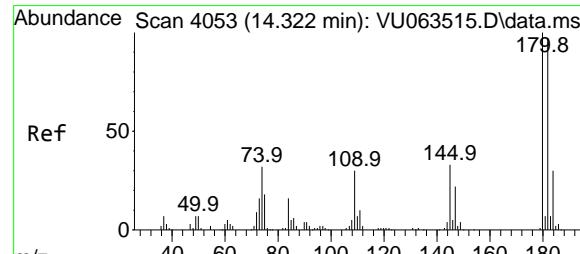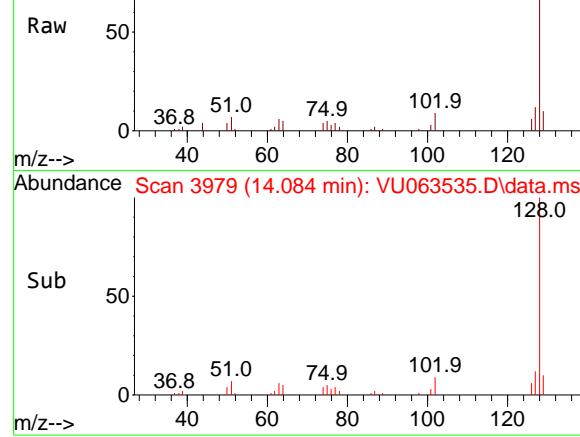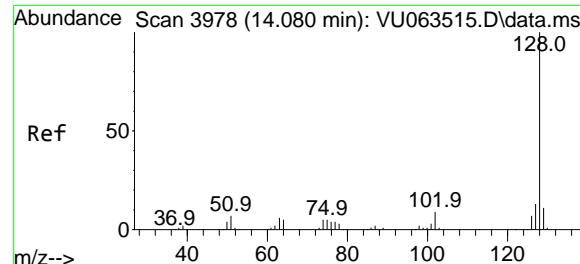

#89

Naphthalene

Concen: 2.015 ug/l

RT: 14.084 min Scan# 3

Delta R.T. 0.004 min

Lab File: VU063535.D


Acq: 18 Jul 2025 11:50

Instrument:

MSVOA_U


ClientSampleId :

VU0718WBS02

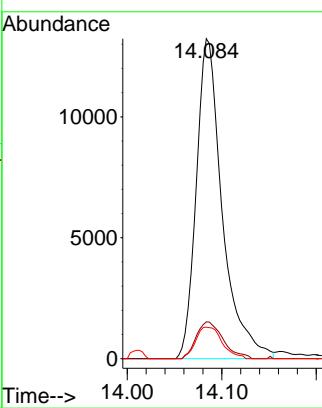**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/21/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#90
1,2,3-Trichlorobenzene
Concen: 1.983 ug/l
RT: 14.322 min Scan# 4053
Delta R.T. -0.000 min
Lab File: VU063535.D
Acq: 18 Jul 2025 11:50

Tgt Ion:180 Resp: 12842
Ion Ratio Lower Upper
180 100
182 96.7 78.0 117.0
145 33.0 27.3 40.9

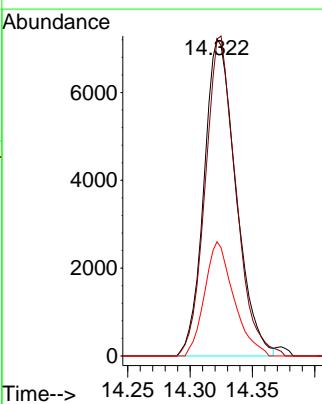



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBSD01	SDG No.:	Q2552	
Lab Sample ID:	VU0717WBSD01	Matrix:	Water	
Analytical Method:	E524.2	% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol: 25000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063522.D	1	07/17/25 13:13	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	2.00		0.12	0.50	ug/L
74-87-3	Chloromethane	2.20		0.13	0.50	ug/L
75-01-4	Vinyl Chloride	2.10		0.12	0.50	ug/L
74-83-9	Bromomethane	2.30		0.15	0.50	ug/L
75-00-3	Chloroethane	2.10		0.14	0.50	ug/L
109-99-9	Tetrahydrofuran	4.10		0.42	1.00	ug/L
75-69-4	Trichlorofluoromethane	2.10		0.20	0.50	ug/L
76-13-1	1,1,2-Trichloro-1,2,2-trifluoroethane	2.20		0.11	0.50	ug/L
75-65-0	tert-Butyl Alcohol	21.0		3.60	10.0	ug/L
60-29-7	Diethyl Ether	2.20		0.13	0.50	ug/L
75-35-4	1,1-Dichloroethene	2.10		0.13	0.50	ug/L
107-13-1	Acrylonitrile	4.20		0.44	1.00	ug/L
67-64-1	Acetone	10.4		0.97	2.50	ug/L
75-15-0	Carbon Disulfide	1.90		0.12	0.50	ug/L
1634-04-4	Methyl tert-Butyl Ether	2.20		0.11	0.50	ug/L
96-33-3	Methyl acrylate	2.00		0.33	0.50	ug/L
75-09-2	Methylene Chloride	2.30		0.44	0.50	ug/L
156-60-5	trans-1,2-Dichloroethene	2.10		0.14	0.50	ug/L
75-34-3	1,1-Dichloroethane	2.20		0.13	0.50	ug/L
110-82-7	Cyclohexane	2.20		0.14	0.50	ug/L
78-93-3	2-Butanone	10.5		0.72	2.50	ug/L
56-23-5	Carbon Tetrachloride	2.00		0.13	0.50	ug/L
594-20-7	2,2-Dichloropropane	2.00		0.12	0.50	ug/L
156-59-2	cis-1,2-Dichloroethene	2.10		0.13	0.50	ug/L
74-97-5	Bromoform	2.10		0.17	0.50	ug/L
67-66-3	Chloroform	2.20		0.17	0.50	ug/L
71-55-6	1,1,1-Trichloroethane	2.10		0.12	0.50	ug/L
108-87-2	Methylcyclohexane	1.90		0.090	0.50	ug/L
563-58-6	1,1-Dichloropropene	2.20		0.11	0.50	ug/L
107-12-0	Propionitrile	11.4		1.20	2.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBSD01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBSD01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063522.D	1	07/17/25 13:13	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
71-43-2	Benzene	1.80		0.11	0.50	ug/L
107-06-2	1,2-Dichloroethane	1.80		0.14	0.50	ug/L
79-01-6	Trichloroethene	1.90		0.13	0.50	ug/L
78-87-5	1,2-Dichloropropane	2.00		0.13	0.50	ug/L
109-69-3	1-Chlorobutane	2.00		0.12	0.50	ug/L
74-95-3	Dibromomethane	2.00		0.15	0.50	ug/L
75-27-4	Bromodichloromethane	1.80		0.13	0.50	ug/L
108-10-1	4-Methyl-2-Pentanone	10.1		0.63	2.50	ug/L
108-88-3	Toluene	2.00		0.11	0.50	ug/L
10061-02-6	t-1,3-Dichloropropene	1.70		0.11	0.50	ug/L
10061-01-5	cis-1,3-Dichloropropene	1.80		0.11	0.50	ug/L
79-00-5	1,1,2-Trichloroethane	2.10		0.13	0.50	ug/L
142-28-9	1,3-Dichloropropane	2.10		0.12	0.50	ug/L
591-78-6	2-Hexanone	10.3		0.65	2.50	ug/L
124-48-1	Dibromochloromethane	1.80		0.20	0.50	ug/L
106-93-4	1,2-Dibromoethane	2.00		0.13	0.50	ug/L
127-18-4	Tetrachloroethene	2.00		0.14	0.50	ug/L
108-90-7	Chlorobenzene	2.00		0.11	0.50	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	1.80		0.13	0.50	ug/L
67-72-1	Hexachloroethane	1.70		0.12	0.50	ug/L
100-41-4	Ethyl Benzene	2.00		0.41	0.50	ug/L
179601-23-1	m/p-Xylenes	4.00		0.73	1.00	ug/L
1330-20-7	Total Xylenes	6.00		1.09	1.50	ug/L
95-47-6	o-Xylene	2.00		0.36	0.50	ug/L
100-42-5	Styrene	2.00		0.38	0.50	ug/L
75-25-2	Bromoform	1.60		0.31	0.50	ug/L
98-82-8	Isopropylbenzene	2.10		0.38	0.50	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	2.00		0.13	0.50	ug/L
96-18-4	1,2,3-Trichloropropane	1.70		0.19	0.50	ug/L
108-86-1	Bromobenzene	2.00		0.13	0.50	ug/L
103-65-1	n-propylbenzene	2.00		0.42	0.50	ug/L



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBSD01		SDG No.:	Q2552
Lab Sample ID:	VU0717WBSD01		Matrix:	Water
Analytical Method:	E524.2		% Solid:	0
Sample Wt/Vol:	25	Units: mL	Final Vol:	25000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063522.D	1	07/17/25 13:13	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
95-49-8	2-Chlorotoluene	2.00		0.27	0.50	ug/L
108-67-8	1,3,5-Trimethylbenzene	2.00		0.37	0.50	ug/L
106-43-4	4-Chlorotoluene	2.00		0.27	0.50	ug/L
98-06-6	tert-Butylbenzene	2.00		0.37	0.50	ug/L
95-63-6	1,2,4-Trimethylbenzene	2.00		0.40	0.50	ug/L
135-98-8	sec-Butylbenzene	2.00		0.36	0.50	ug/L
99-87-6	p-Isopropyltoluene	2.00		0.42	0.50	ug/L
541-73-1	1,3-Dichlorobenzene	2.00		0.13	0.50	ug/L
106-46-7	1,4-Dichlorobenzene	2.00		0.13	0.50	ug/L
104-51-8	n-Butylbenzene	2.10		0.43	0.50	ug/L
95-50-1	1,2-Dichlorobenzene	2.00		0.14	0.50	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	2.00		0.24	0.50	ug/L
120-82-1	1,2,4-Trichlorobenzene	2.00		0.21	0.50	ug/L
87-68-3	Hexachlorobutadiene	2.00		0.14	0.50	ug/L
91-20-3	Naphthalene	2.10		0.33	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	2.00		0.31	0.50	ug/L
98-95-3	Nitrobenzene	10.3		1.80	5.00	ug/L
363-72-4	Pentachloroethane	1.80		0.16	0.50	ug/L
74-88-4	Iodomethane	1.90		0.090	1.00	ug/L
107-05-1	Allyl Chloride	2.10		0.13	0.50	ug/L
126-98-7	Methacrylonitrile	2.00		0.24	0.50	ug/L
110-57-6	t-1,4-Dichloro-2-butene	3.60		0.21	1.00	ug/L
97-63-2	Ethyl methacrylate	2.00		0.12	0.50	ug/L
108-20-3	Isopropyl Ether	2.20		0.14	0.50	ug/L
80-62-6	Methyl methacrylate	3.70		0.24	1.00	ug/L
SURROGATES						
2199-69-1	1,2-Dichlorobenzene-d4	1.10		70 - 130	110%	SPK: 1
460-00-4	4-Bromofluorobenzene	1.00		70 - 130	103%	SPK: 1
INTERNAL STANDARDS						
462-06-6	Fluorobenzene	21700	6.097			



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Drinking Water PT			Date Received:
Client Sample ID:	VU0717WBSD01	SDG No.:		Q2552
Lab Sample ID:	VU0717WBSD01	Matrix:	Water	
Analytical Method:	E524.2	% Solid:	0	
Sample Wt/Vol:	25	Units:	mL	Final Vol: 25000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Date Analyzed	Prep Batch ID
VU063522.D	1	07/17/25 13:13	VU071725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
------------	-----------	-------	-----------	-----	------------	-------

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063522.D
 Acq On : 17 Jul 2025 13:13
 Operator : MD/SY
 Sample : VU0717WBSD01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0717WBSD01

Quant Time: Jul 18 04:11:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Fluorobenzene	6.097	96	21661	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	8475	1.033	ug/l	0.00
Spiked Amount 1.000			Recovery	=	103.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	8367	1.103	ug/l	0.00
Spiked Amount 1.000			Recovery	=	110.000%	
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	12499	1.957	ug/l	98
3) Chloromethane	1.518	50	13003	2.190	ug/l	99
4) Vinyl Chloride	1.599	62	15770	2.086	ug/l	97
5) Bromomethane	1.846	94	13288	2.330	ug/l	98
6) Chloroethane	1.923	64	9681	2.120	ug/l	99
7) Trichlorofluoromethane	2.126	101	23147	2.132	ug/l	98
8) 1,1,2-Trichloro-1,2,2-...	2.570	101	12255	2.160	ug/l	99
9) 1,1-Dichloroethene	2.566	96	11828	2.103	ug/l	95
10) Iodomethane	2.708	142	8884	1.876	ug/l	99
11) Allyl Chloride	2.907	41	16934	2.084	ug/l	90
12) Acrylonitrile	3.309	53	5855	4.163	ug/l	94
13) Acetone	2.618	43	11698	10.381	ug/l	97
14) Carbon Disulfide	2.779	76	34405	1.894	ug/l	97
15) Methylene Chloride	3.026	84	15282	2.308	ug/l	94
16) trans-1,2-Dichloroethene	3.335	96	13484	2.111	ug/l	98
17) 1,1-Dichloroethane	3.849	63	25505	2.155	ug/l	99
18) 2-Butanone	4.718	43	18247	10.456	ug/l	95
19) Cyclohexane	5.357	56	21549	2.150	ug/l	98
20) Methylcyclohexane	6.740	83	18558	1.905	ug/l	98
21) 2,2-Dichloropropane	4.644	77	20534	2.037	ug/l	100
22) cis-1,2-Dichloroethene	4.647	96	14692	2.120	ug/l	98
23) Diethyl Ether	2.370	59	9212	2.150	ug/l	95
24) tert-Butyl Alcohol	3.197	59	10881	21.035	ug/l	96
25) Methyl tert-Butyl Ether	3.361	73	31736	2.162	ug/l	97
26) Bromochloromethane	4.955	128	6089	2.104	ug/l	92
27) Chloroform	5.068	83	26421	2.187	ug/l	98
28) 1,1,1-Trichloroethane	5.293	97	21787	2.125	ug/l	99
29) 1,1-Dichloropropene	5.502	75	21238	2.236	ug/l	99
30) Carbon Tetrachloride	5.499	117	16882	2.046	ug/l	94
31) Isopropyl Ether	3.994	45	39443	2.207	ug/l	100
32) Ethyl-t-butyl ether	4.505	59	35419	2.142	ug/l	96
33) Tert-Amyl methyl ether	5.943	73	25195	1.756	ug/l	99
34) Propionitrile	4.782	54	6040	11.359	ug/l	# 95
35) Benzene	5.753	78	45875	1.798	ug/l	99
36) 1,2-Dichloroethane	5.782	62	14343	1.809	ug/l	99
37) Trichloroethene	6.525	130	12117	1.861	ug/l	99
38) 1,2-Dichloropropane	6.782	63	11764	1.970	ug/l	96
39) Methacrylonitrile	4.972	41	4816	2.038	ug/l	94
40) Methyl acrylate	4.853	55	6941	2.009	ug/l	# 95
41) Tetrahydrofuran	5.062	42	5070	4.078	ug/l	98
42) 1-Chlorobutane	5.435	56	25415	2.013	ug/l	95
43) Dibromomethane	6.910	93	6168	1.994	ug/l	93
44) Bromodichloromethane	7.097	83	12700	1.820	ug/l	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
 Data File : VU063522.D
 Acq On : 17 Jul 2025 13:13
 Operator : MD/SY
 Sample : VU0717WBSD01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0717WBSD01

Quant Time: Jul 18 04:11:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 4-Methyl-2-Pentanone	7.798	43	32113	10.071	ug/1	100
46) t-1,4-Dichloro-2-butene	10.823	75	4288m	3.582	ug/1	
47) Methyl methacrylate	6.968	69	9711	3.737	ug/1	98
48) Ethyl methacrylate	8.335	69	9783	1.973	ug/1	100
49) Toluene	7.959	92	27325	1.961	ug/1	100
50) t-1,3-Dichloropropene	8.206	75	9349	1.708	ug/1	99
51) cis-1,3-Dichloropropene	7.602	75	12871	1.752	ug/1	99
52) 1,1,2-Trichloroethane	8.393	97	8548	2.052	ug/1	97
53) 1,3-Dichloropropane	8.569	76	14962	2.081	ug/1	99
54) 2-Hexanone	8.692	43	21753	10.271	ug/1	99
55) Dibromochloromethane	8.801	129	7756	1.762	ug/1	96
56) 1,2-Dibromoethane	8.917	107	7538	2.022	ug/1	99
58) Tetrachloroethene	8.544	164	11718	1.967	ug/1	96
59) Chlorobenzene	9.441	112	31422	1.964	ug/1	98
60) 1,1,1,2-Tetrachloroethane	9.524	131	9309	1.809	ug/1	98
61) Pentachloroethane	11.415	117	6595	1.814	ug/1	94
62) Hexachloroethane	12.466	117	6118	1.699	ug/1	98
63) Ethyl Benzene	9.563	91	54379	1.975	ug/1	97
64) m/p-Xylenes	9.685	106	42437	3.965	ug/1	99
65) o-Xylene	10.094	106	20286	1.972	ug/1	96
66) Styrene	10.110	104	32779	2.000	ug/1	99
67) Bromoform	10.283	173	3723	1.647	ug/1 #	97
69) Isopropylbenzene	10.476	105	51101	2.055	ug/1	100
70) 1,1,2,2-Tetrachloroethane	10.775	83	10327	2.038	ug/1	97
71) 1,2,3-Trichloropropane	10.817	75	7171m	1.742	ug/1	
72) Bromobenzene	10.778	156	12879	2.007	ug/1	95
73) n-propylbenzene	10.897	120	15141	2.023	ug/1	95
74) 2-Chlorotoluene	10.978	126	13109	1.982	ug/1	95
75) 1,3,5-Trimethylbenzene	11.081	105	47178	1.986	ug/1	99
76) 4-Chlorotoluene	11.090	126	13659	2.033	ug/1	99
77) tert-Butylbenzene	11.412	119	45406	2.000	ug/1	98
78) 1,2,4-Trimethylbenzene	11.460	105	47334	2.009	ug/1	97
79) sec-Butylbenzene	11.634	105	62131	2.030	ug/1	98
80) Nitrobenzene	13.219	77	815m	10.269	ug/1	
81) p-Isopropyltoluene	11.785	119	51424	2.012	ug/1	98
82) 1,3-Dichlorobenzene	11.740	146	26072	2.031	ug/1	99
83) 1,4-Dichlorobenzene	11.830	146	25409	1.977	ug/1	95
84) n-Butylbenzene	12.203	91	49653	2.095	ug/1	98
85) 1,2-Dichlorobenzene	12.206	146	23948	1.985	ug/1	100
86) 1,2-Dibromo-3-Chloropr...	12.991	75	1326	2.003	ug/1	97
87) 1,2,4-Trichlorobenzene	13.836	180	15210	2.028	ug/1	98
88) Hexachlorobutadiene	14.013	225	8359	1.962	ug/1	100
89) Naphthalene	14.087	128	28386	2.112	ug/1	99
90) 1,2,3-Trichlorobenzene	14.322	180	14091	2.033	ug/1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063522.D
Acq On : 17 Jul 2025 13:13
Operator : MD/SY
Sample : VU0717WBSD01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1


Quant Time: Jul 18 04:11:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBSD01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

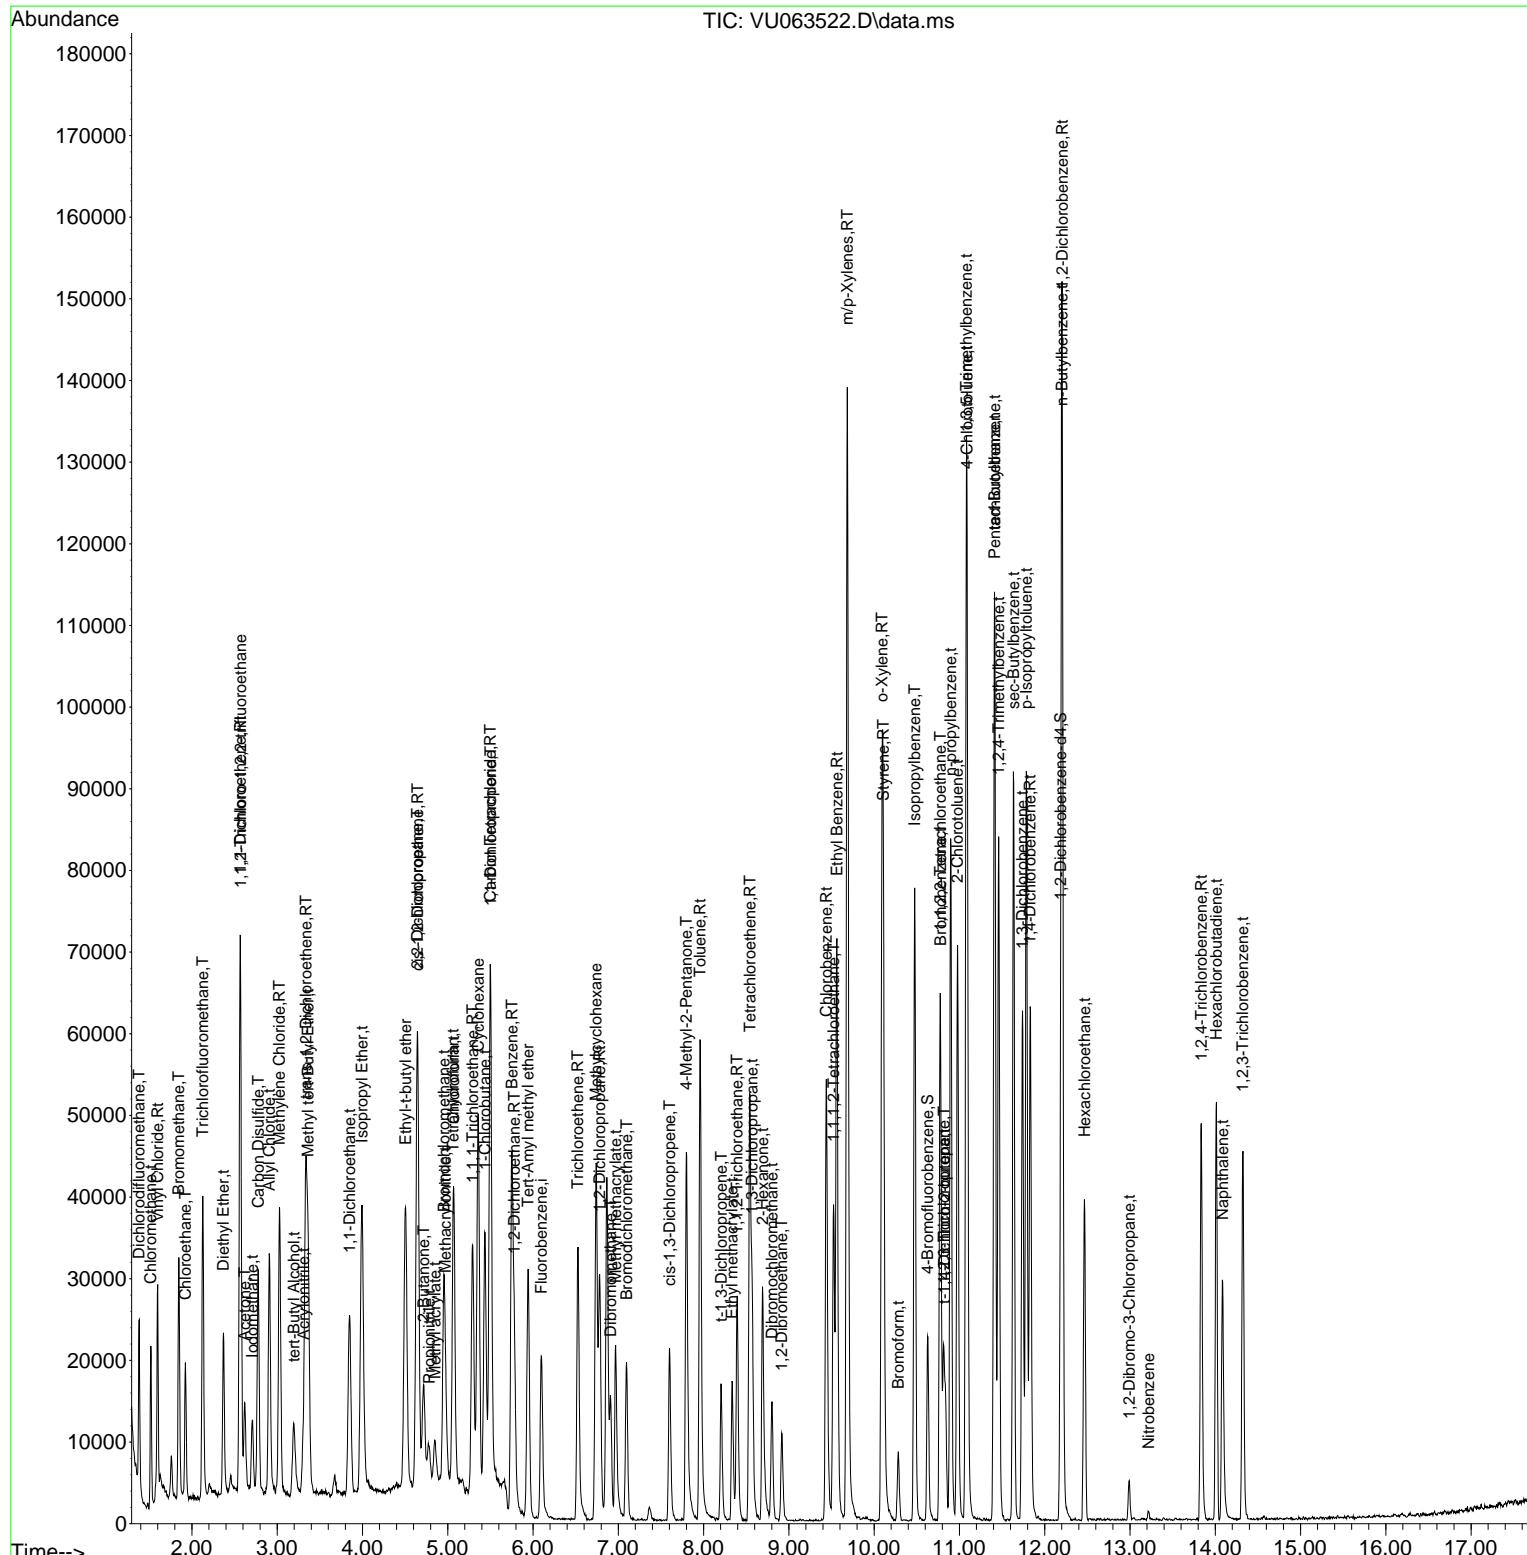



#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01





Tgt Ion: 96 Resp: 21661
Ion Ratio Lower Upper


96	100
70	17.3
95	8.0
97	5.4
	0.0
	0.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#2
Dichlorodifluoromethane
Concen: 1.957 ug/l
RT: 1.380 min Scan# 28
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13





Tgt Ion: 85 Resp: 12499
Ion Ratio Lower Upper

85	100
87	30.7
	16.0
	47.9






Abundance Scan 71 (1.518 min): VU063522.D\data.ms

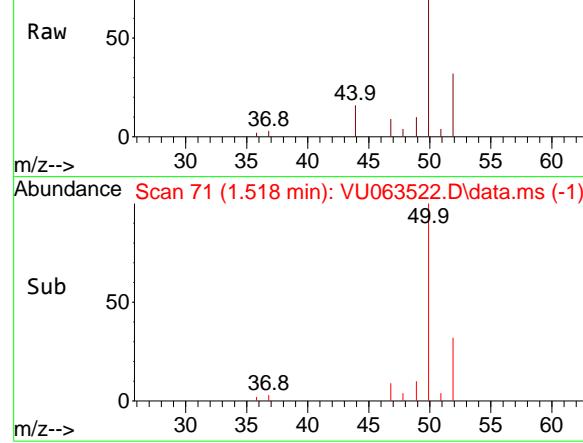

Abundance Scan 96 (1.599 min): VU063522.D\data.ms

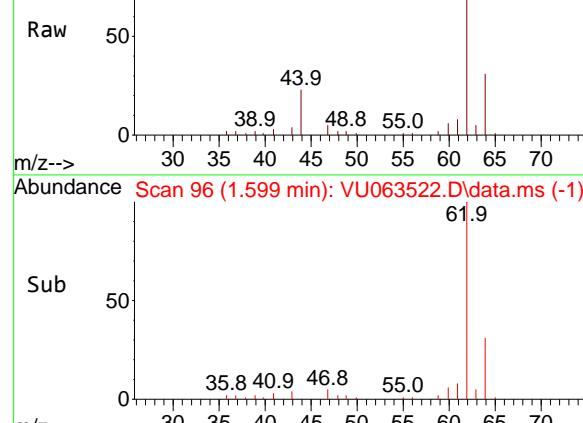

Abundance Scan 96 (1.599 min): VU063522.D\data.ms (-1)

#3

Chloromethane

Concen: 2.190 ug/l

RT: 1.518 min Scan# 7

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

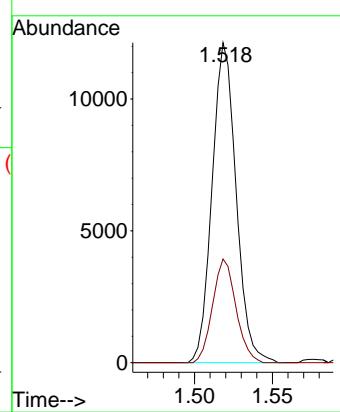 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#4

Vinyl Chloride


Concen: 2.086 ug/l




RT: 1.599 min Scan# 96

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

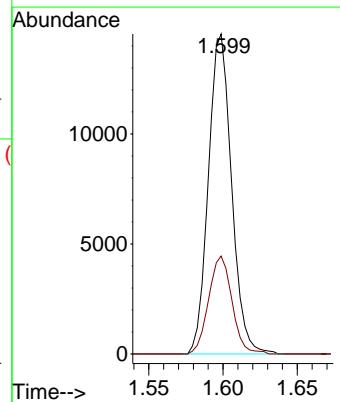 Tgt Ion: 62 Resp: 15770
 Ion Ratio Lower Upper
 62 100
 64 30.6 25.7 38.5

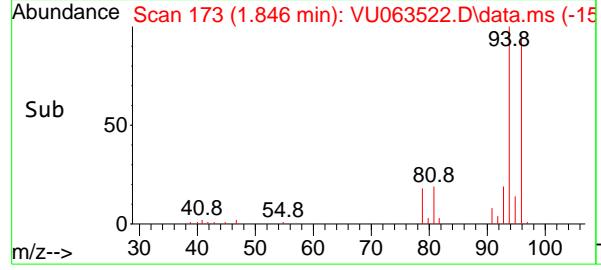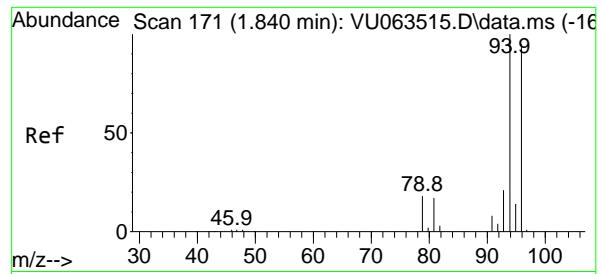
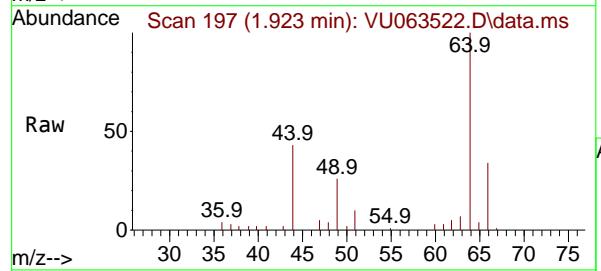
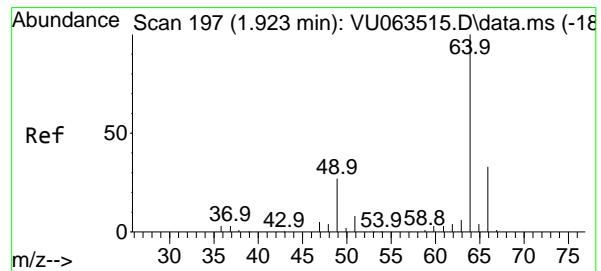
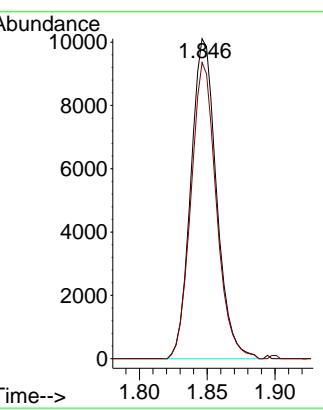


#5
 Bromomethane
 Concen: 2.330 ug/l
 RT: 1.846 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: VU063522.D
 Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
 ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025



#6
 Chloroethane
 Concen: 2.120 ug/l
 RT: 1.923 min Scan# 197
 Delta R.T. 0.000 min
 Lab File: VU063522.D
 Acq: 17 Jul 2025 13:13


Tgt Ion: 64 Resp: 9681
 Ion Ratio Lower Upper
 64 100
 66 33.5 26.2 39.4

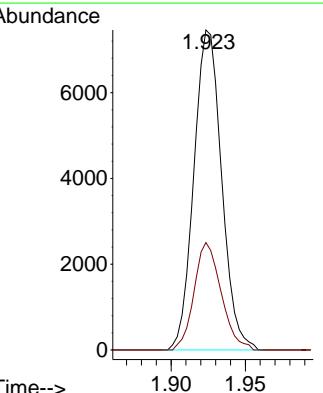



#7
Trichlorofluoromethane
Concen: 2.132 ug/l
RT: 2.126 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01




Tgt Ion:101 Resp: 2314
Ion Ratio Lower Upper
101 100
103 63.7 52.2 78.4

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

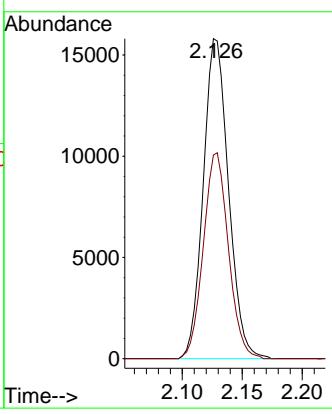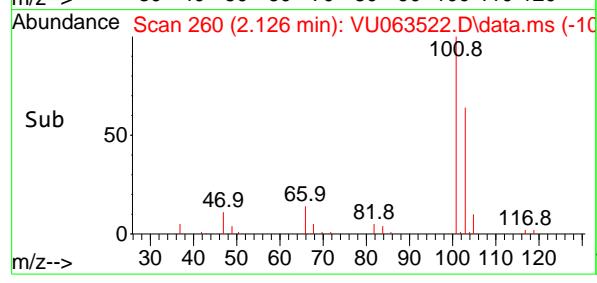


#8
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 2.160 ug/l
RT: 2.570 min Scan# 398
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Tgt Ion:101 Resp: 12255
Ion Ratio Lower Upper
101 100
85 47.0 37.8 56.6
151 75.8 59.2 88.8

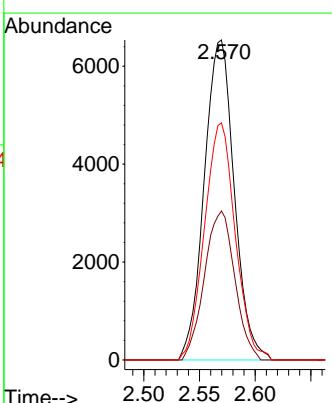



#9
1,1-Dichloroethene
Concen: 2.103 ug/l
RT: 2.566 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01




Tgt Ion: 96 Resp: 11823
Ion Ratio Lower Upper
96 100
61 174.9 0.0 504.3
98 66.0 0.0 126.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

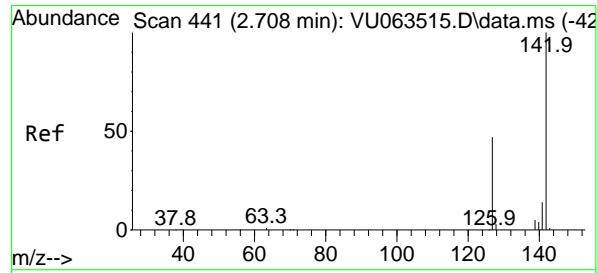
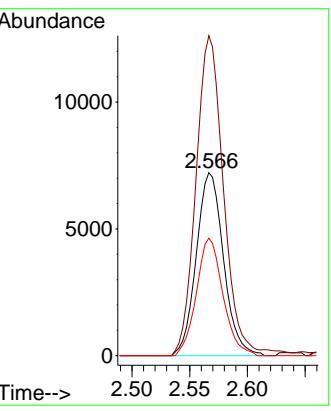



#10
Iodomethane
Concen: 1.876 ug/l
RT: 2.708 min Scan# 441
Delta R.T. -0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

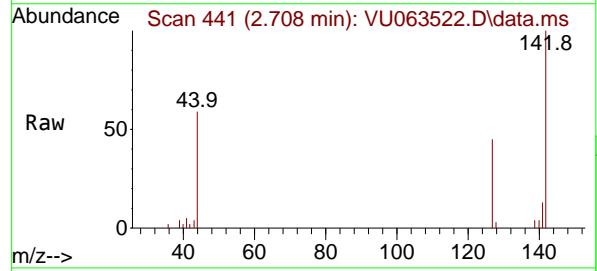

Tgt Ion:142 Resp: 8884
Ion Ratio Lower Upper
142 100
127 46.8 37.9 56.9

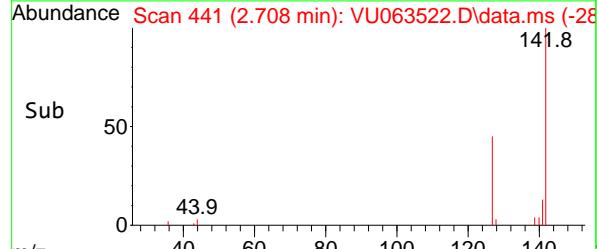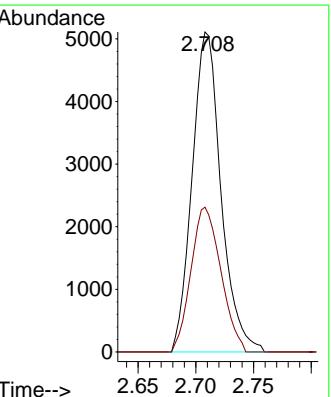

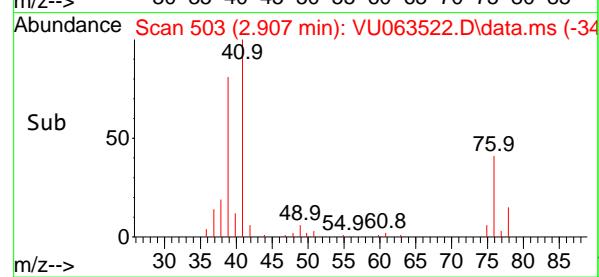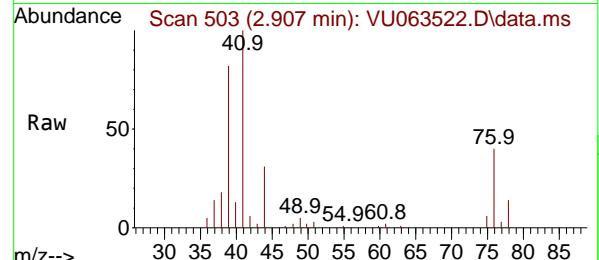

#11

Allyl Chloride

Concen: 2.084 ug/l

RT: 2.907 min Scan# 5

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U

ClientSampleId :




VU0717WBSD01

Tgt Ion: 41 Resp: 16934

Ion Ratio Lower Upper

41 100

39 85.5 61.5 92.3

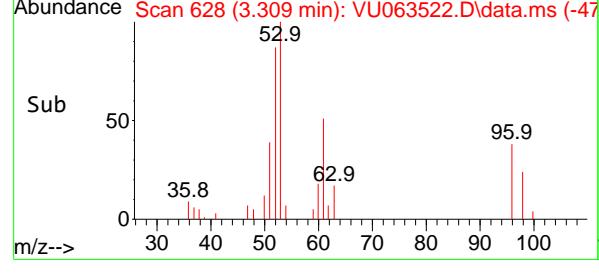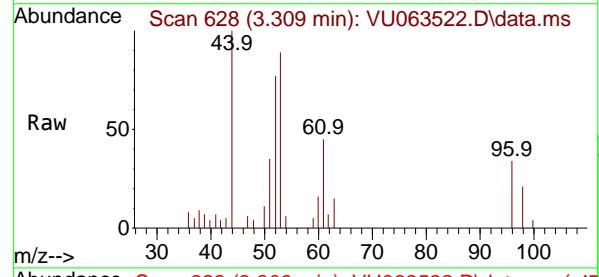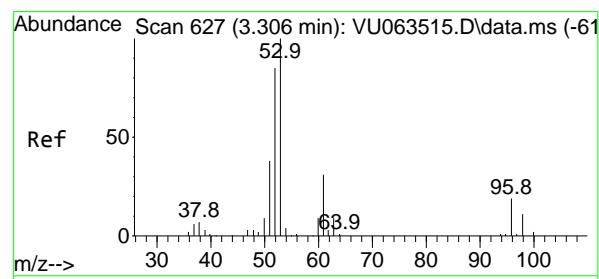**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#12

Acrylonitrile

Concen: 4.163 ug/l

RT: 3.309 min Scan# 628

Delta R.T. 0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 53 Resp: 5855




Ion Ratio Lower Upper

53 100

52 85.0 64.3 96.5

51 38.5 27.8 41.8

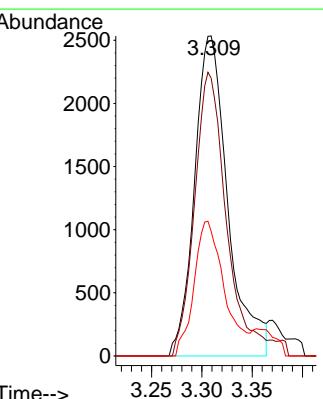


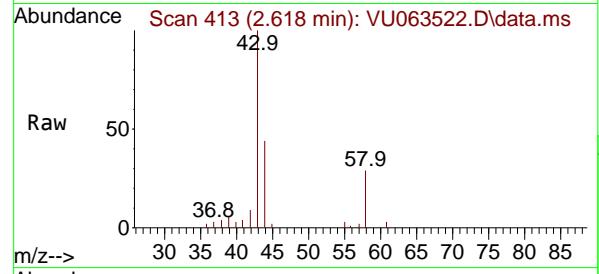
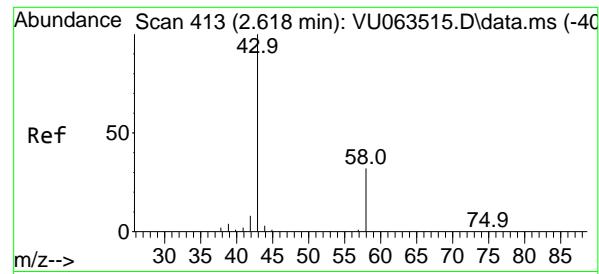


#13
Acetone
Concen: 10.381 ug/l
RT: 2.618 min Scan# 413
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#14
Carbon Disulfide
Concen: 1.894 ug/l
RT: 2.779 min Scan# 463
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 76 Resp: 34405
Ion Ratio Lower Upper
76 100
78 9.8 7.0 10.6

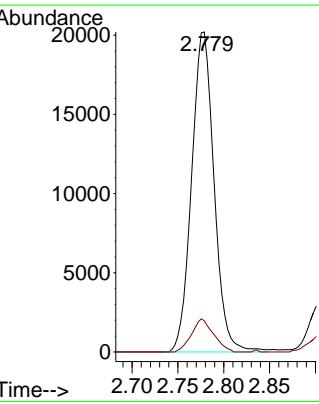



#15

Methylene Chloride

Concen: 2.308 ug/l

RT: 3.026 min Scan# 541

Delta R.T. -0.003 min

Lab File: VU063522.D


Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U


ClientSampleId :







VU0717WBSD01

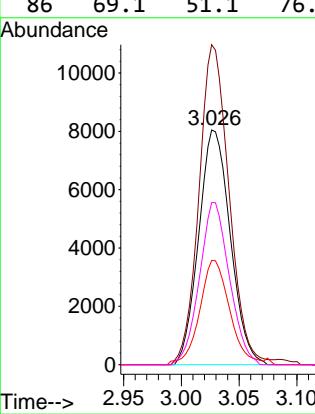**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#16
trans-1,2-Dichloroethene
Concen: 2.111 ug/l
RT: 3.335 min Scan# 636
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 96 Resp: 13484
Ion Ratio Lower Upper
96 100
61 147.7 117.2 175.8
98 67.3 51.4 77.2

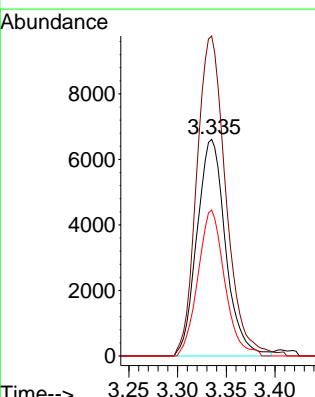

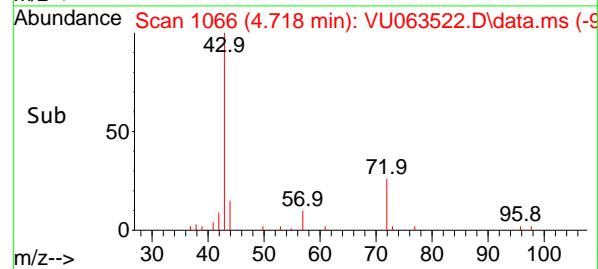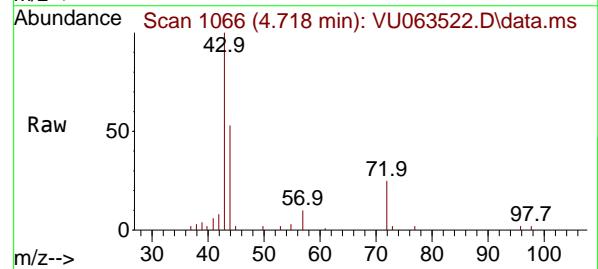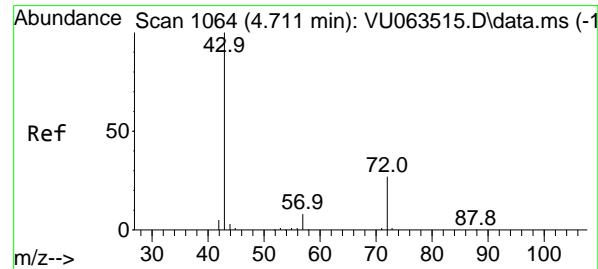


#17

1,1-Dichloroethane
Concen: 2.155 ug/l
RT: 3.849 min Scan# 7
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBSD01


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#18
2-Butanone
Concen: 10.456 ug/l
RT: 4.718 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 43 Resp: 18247
Ion Ratio Lower Upper
43 100
57 9.9 0.0 16.4

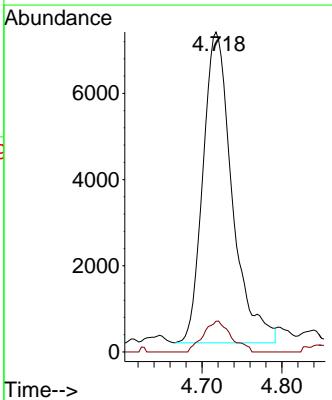



#19

Cyclohexane

Concen: 2.150 ug/l

RT: 5.357 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063522.D


Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

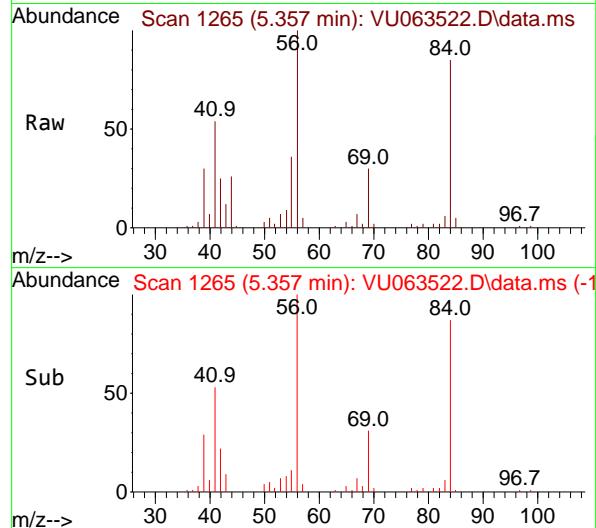

Tgt Ion: 56 Resp: 21549

Ion Ratio Lower Upper

56 100



69 33.0 26.6 39.8

84 85.8 71.0 106.4

**Manual Integrations
APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

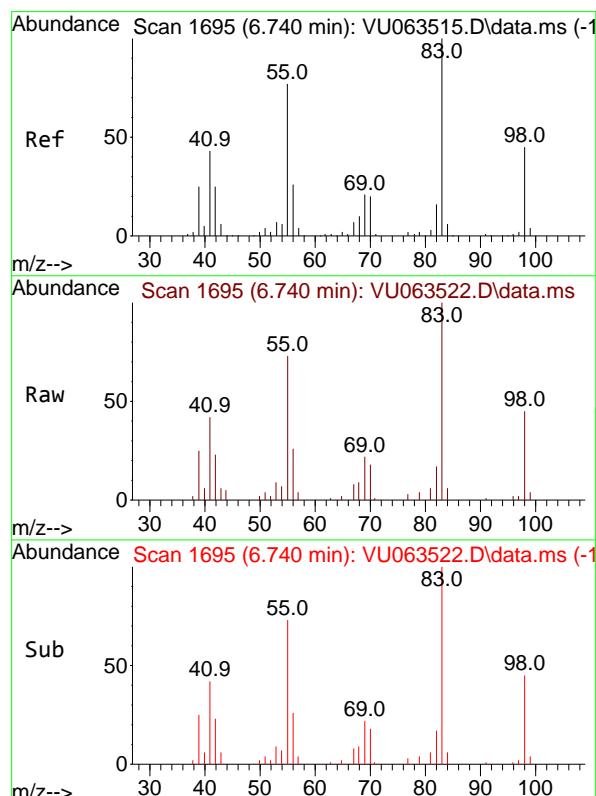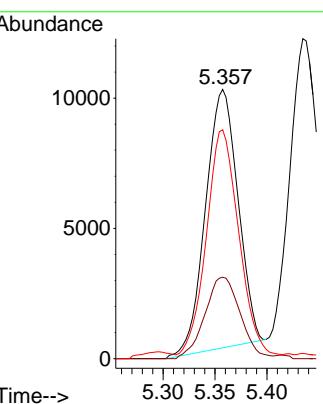

#20

Methylcyclohexane

Concen: 1.905 ug/l

RT: 6.740 min Scan# 1695

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 83 Resp: 18558







Ion Ratio Lower Upper

83 100

55 75.2 60.6 90.8

98 42.3 35.8 53.8

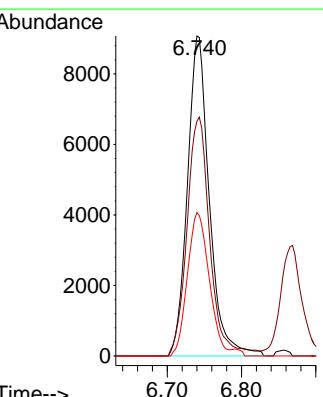

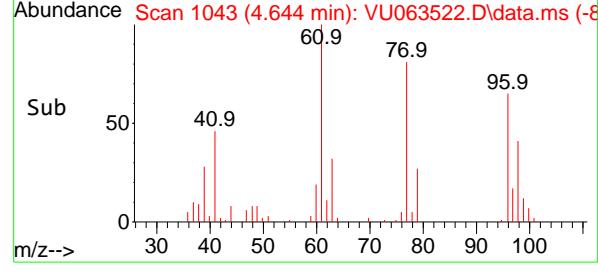

#21

2,2-Dichloropropane

Concen: 2.037 ug/l

RT: 4.644 min Scan# 1043

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

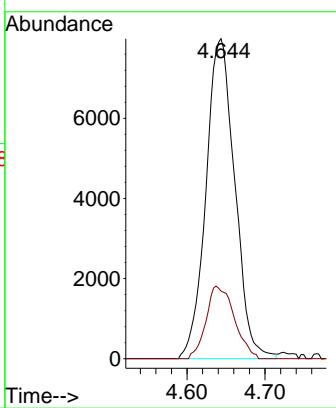 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#22

cis-1,2-Dichloroethene

Concen: 2.120 ug/l

RT: 4.647 min Scan# 1044

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 96 Resp: 14692







Ion Ratio Lower Upper

96 100

61 156.5 0.0 384.7

98 65.0 32.1 96.3

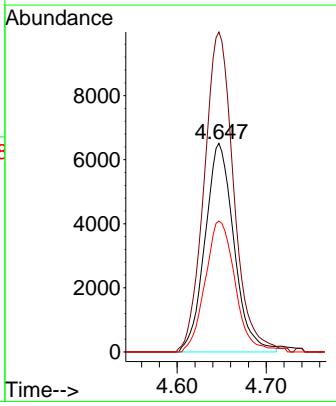

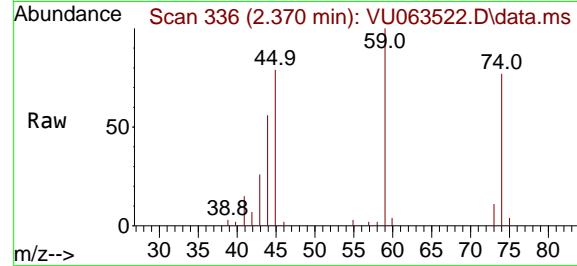

#23

Diethyl Ether

Concen: 2.150 ug/l

RT: 2.370 min Scan# 3

Delta R.T. 0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Instrument :

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

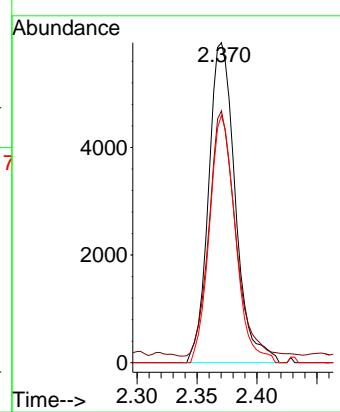 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#24

tert-Butyl Alcohol

Concen: 21.035 ug/l

RT: 3.197 min Scan# 593

Delta R.T. 0.006 min

Lab File: VU063522.D


Acq: 17 Jul 2025 13:13







Tgt Ion: 59 Resp: 10881

Ion Ratio Lower Upper

59 100

57 12.3 8.6 12.8

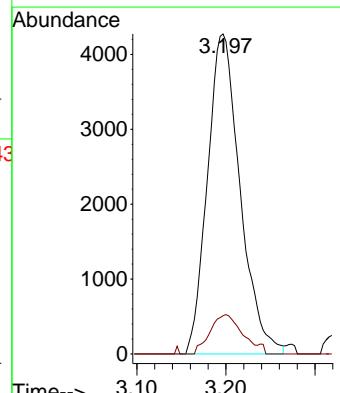




#25

Methyl tert-Butyl Ether
Concen: 2.162 ug/l
RT: 3.361 min Scan# 6
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025









#26

Bromochloromethane
Concen: 2.104 ug/l
RT: 4.955 min Scan# 1140
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:128 Resp: 6089
Ion Ratio Lower Upper
128 100
49 181.5 0.0 340.8
130 134.7 100.5 150.7

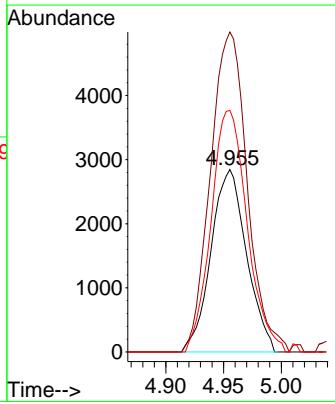

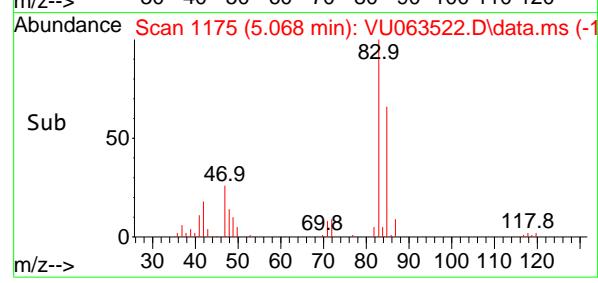

#27

Chloroform

Concen: 2.187 ug/l

RT: 5.068 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

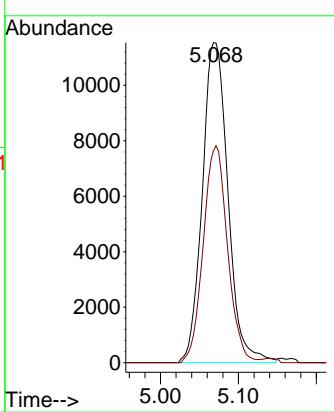 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#28

1,1,1-Trichloroethane

Concen: 2.125 ug/l

RT: 5.293 min Scan# 1245

Delta R.T. -0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 97 Resp: 21787


Ion Ratio Lower Upper

97 100

99 64.1 31.8 95.3

61 48.2 23.3 69.9

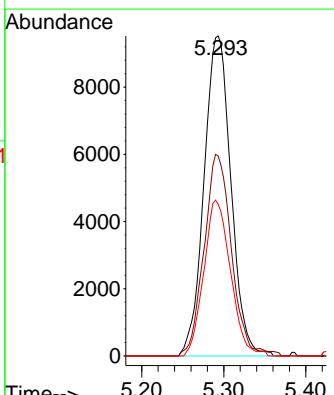


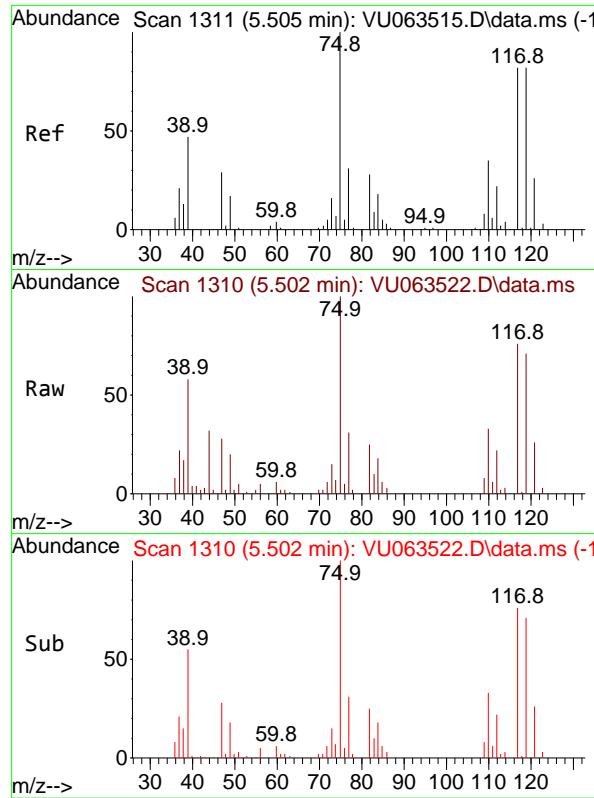


#29
1,1-Dichloropropene
Concen: 2.236 ug/l
RT: 5.502 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations
APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

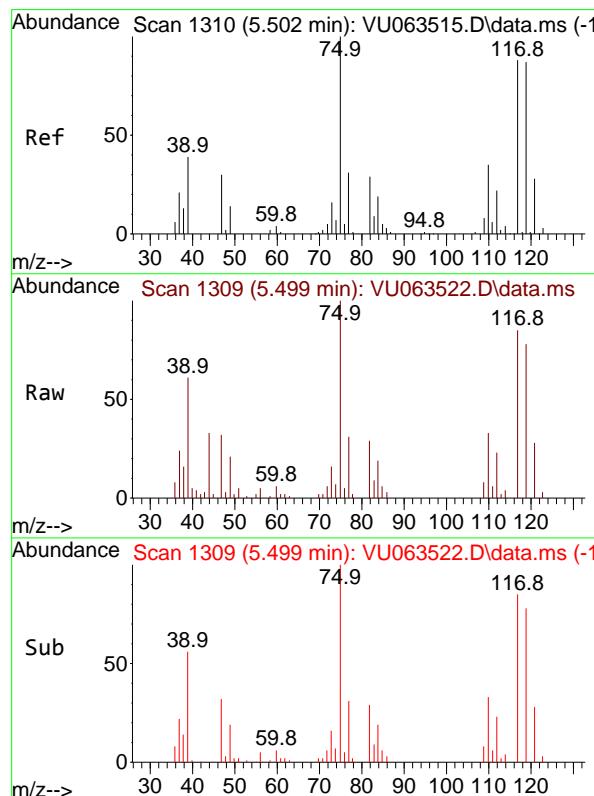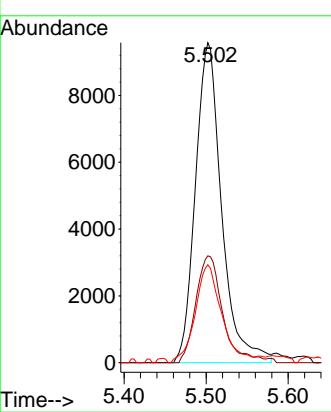

#30
Carbon Tetrachloride
Concen: 2.046 ug/l
RT: 5.499 min Scan# 1309
Delta R.T. -0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:117 Resp: 16882
Ion Ratio Lower Upper
117 100
119 92.0 79.2 118.8
121 33.1 25.5 38.3

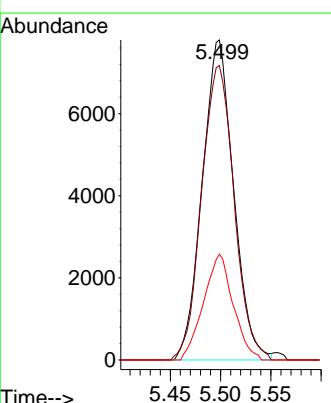



#31

Isopropyl Ether

Concen: 2.207 ug/l

RT: 3.994 min Scan# 8

Instrument :

Delta R.T. 0.003 min







MSVOA_U

Lab File: VU063522.D

ClientSampleId :

Acq: 17 Jul 2025 13:13

VU0717WBSD01



#33

Tert-Amyl methyl ether

Concen: 1.756 ug/l

RT: 5.943 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

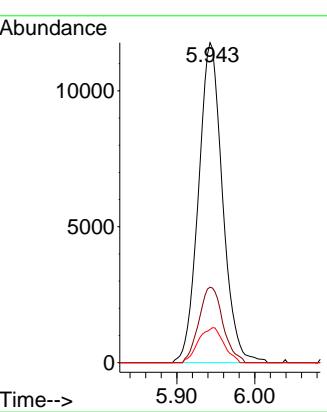 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#34

Propionitrile

Concen: 11.359 ug/l

RT: 4.782 min Scan# 1086

Delta R.T. 0.010 min


Lab File: VU063522.D


Acq: 17 Jul 2025 13:13

Tgt Ion: 54 Resp: 6040


Ion Ratio Lower Upper

	100		
54	100		
52	18.9	17.0	25.4
55	15.6	13.6	20.4
40	5.6	6.4	9.6#

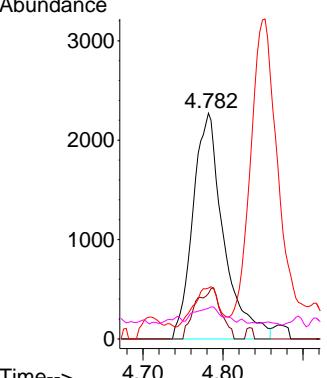






#35
Benzene
Concen: 1.798 ug/l
RT: 5.753 min Scan# 1
Delta R.T. -0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Tgt Ion: 78 Resp: 4587
Ion Ratio Lower Upper
78 100
77 23.7 19.4 29.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

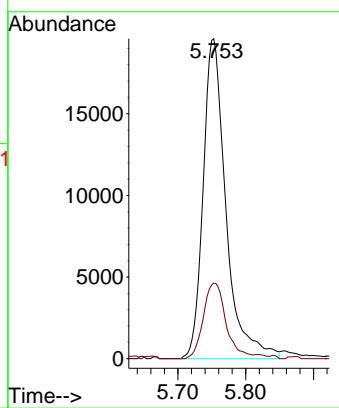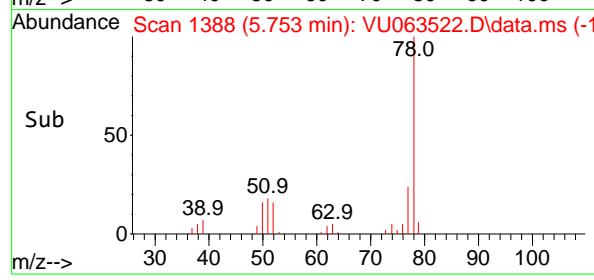


#36
1,2-Dichloroethane
Concen: 1.809 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Tgt Ion: 62 Resp: 14343
Ion Ratio Lower Upper
62 100
98 7.5 6.4 9.6

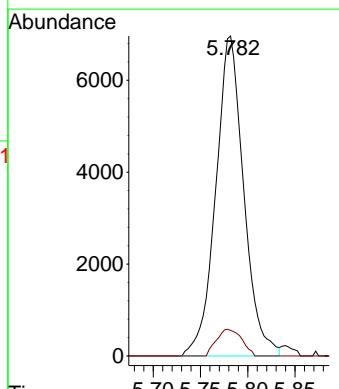



#37
Trichloroethene
Concen: 1.861 ug/l
RT: 6.525 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01




Tgt Ion:130 Resp: 12111
Ion Ratio Lower Upper
130 100
95 99.2 80.3 120.5

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


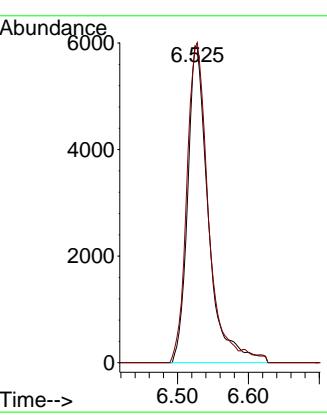



#38
1,2-Dichloropropane
Concen: 1.970 ug/l
RT: 6.782 min Scan# 1708
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13



Tgt Ion: 63 Resp: 11764
Ion Ratio Lower Upper
63 100
65 33.0 24.6 36.8

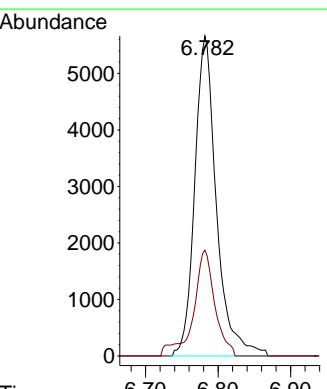

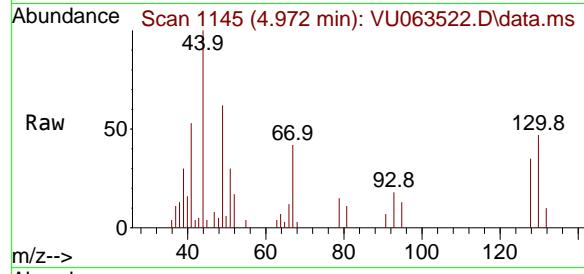

#39

Methacrylonitrile

Concen: 2.038 ug/l

RT: 4.972 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U





ClientSampleId :

VU0717WBSD01

Tgt	Ion	Ion Ratio	Resp:	4810
	41	100		
	67	89.7	Lower	62.7
	39	53.8	Upper	94.1
	52	34.7		27.4
				41.0

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

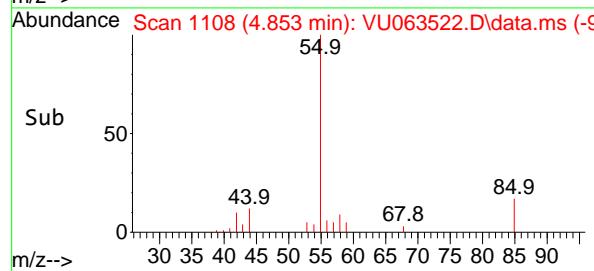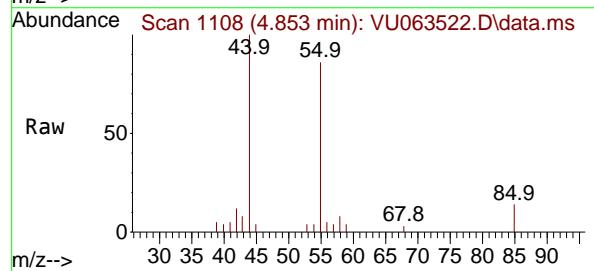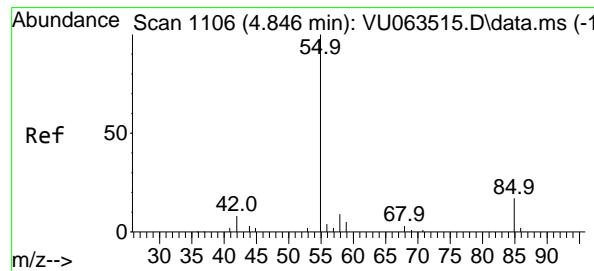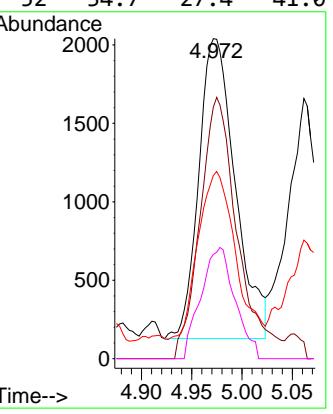

#40

Methyl acrylate

Concen: 2.009 ug/l


RT: 4.853 min Scan# 1108


Delta R.T. 0.006 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Tgt	Ion	Ion Ratio	Resp:	6941
	55	100		
	85	19.6	Lower	12.8
	58	9.4	Upper	19.2#
	42	10.0		7.0
				10.4

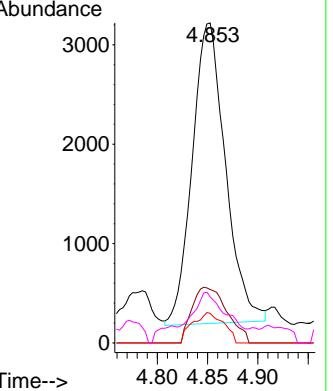



#41

Tetrahydrofuran

Concen: 4.078 ug/l

RT: 5.062 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU063522.D


Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U

ClientSampleId :




VU0717WBSD01

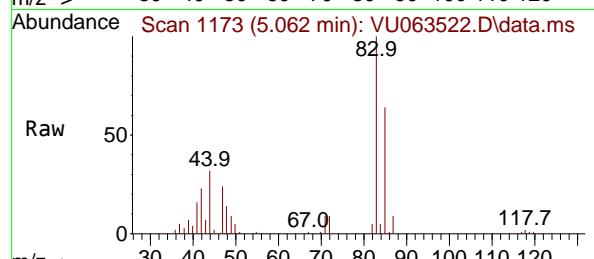


Tgt Ion:	Ion Ratio	Resp:	5070
Ion	Lower	Upper	
42	100		
72	46.8	39.2	58.8
71	43.1	34.8	52.2

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

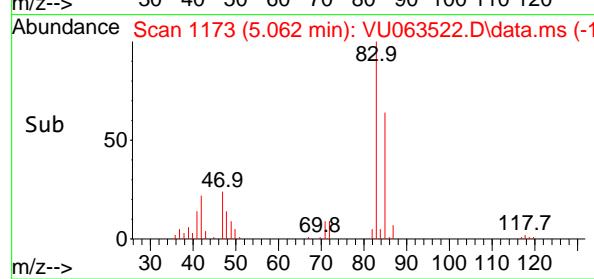


#42
1-Chlorobutane
Concen: 2.013 ug/l
RT: 5.435 min Scan# 1289
Delta R.T. -0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Tgt Ion:	Ion Ratio	Resp:	25415
Ion	Lower	Upper	
56	100		
41	57.0	26.7	80.0

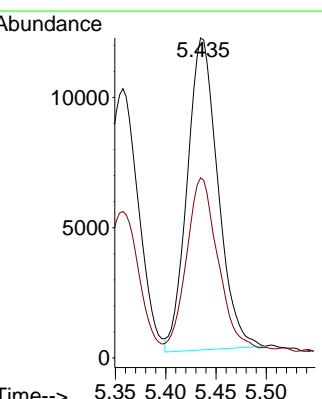



#43
Dibromomethane
Concen: 1.994 ug/l
RT: 6.910 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13




Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01




Tgt Ion: 93 Resp: 6163
Ion Ratio Lower Upper
93 100
95 81.1 67.9 101.9
174 84.5 74.6 111.8

Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


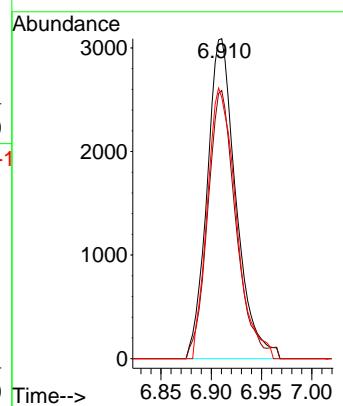
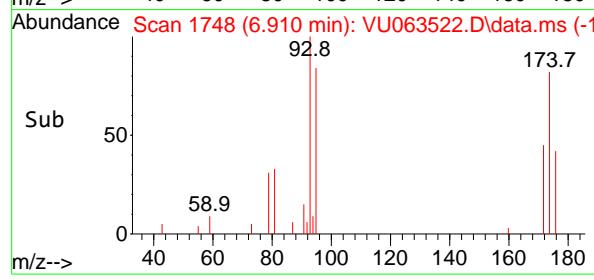


#44
Bromodichloromethane
Concen: 1.820 ug/l
RT: 7.097 min Scan# 1806
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

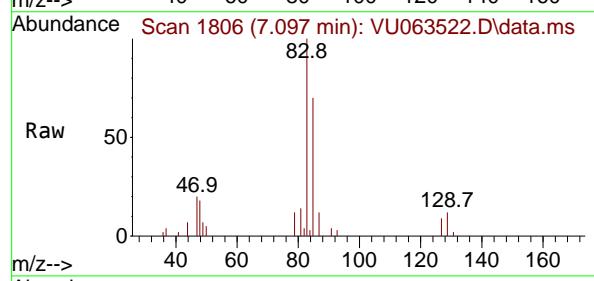

Tgt Ion: 83 Resp: 12700
Ion Ratio Lower Upper
83 100
85 69.8 52.7 79.1
127 9.1 8.1 12.1

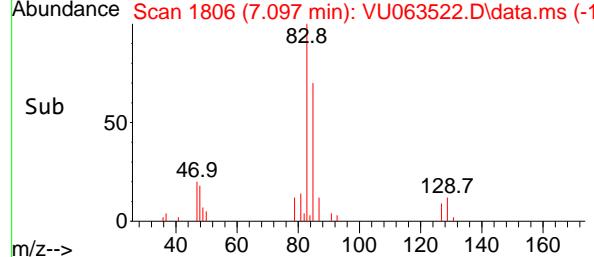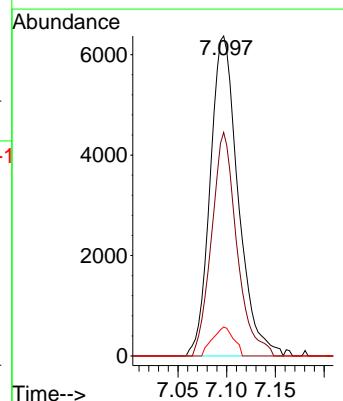



#45

4-Methyl-2-Pentanone

Concen: 10.071 ug/l

RT: 7.798 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13




Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#46

t-1,4-Dichloro-2-butene

Concen: 3.582 ug/l

RT: 10.823 min Scan# 2965

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Tgt Ion: 75 Resp: 4288


Ion Ratio Lower Upper




75 100

53 68.6 48.4 72.6

89 32.0 30.6 45.8

88 26.1 25.3 37.9

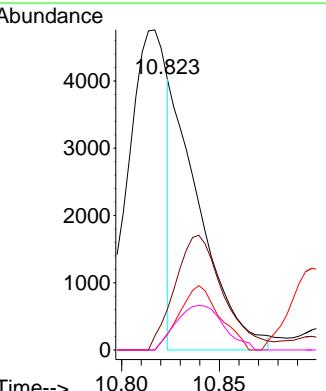






#47

Methyl methacrylate
Concen: 3.737 ug/l
RT: 6.968 min Scan# 1
Delta R.T. 0.006 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025






#48

Ethyl methacrylate
Concen: 1.973 ug/l
RT: 8.335 min Scan# 2191
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 69 Resp: 9783
Ion Ratio Lower Upper
69 100
41 61.8 30.8 92.4

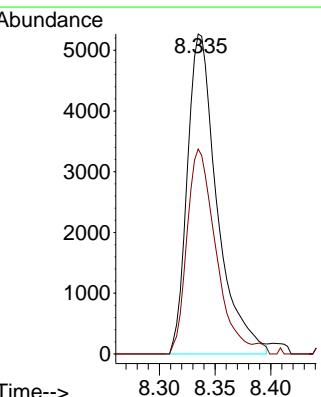






#49
Toluene
Concen: 1.961 ug/l
RT: 7.959 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

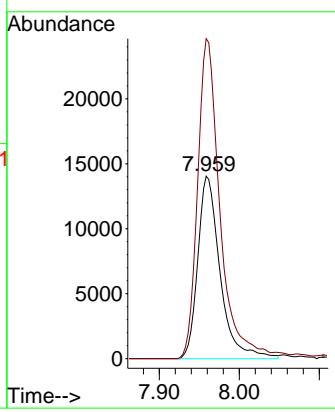

#50
t-1,3-Dichloropropene
Concen: 1.708 ug/l
RT: 8.206 min Scan# 2151
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 75 Resp: 9349
Ion Ratio Lower Upper
75 100
77 30.5 24.9 37.3

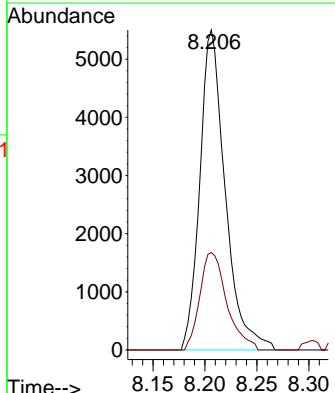




#51
cis-1,3-Dichloropropene
Concen: 1.752 ug/l
RT: 7.602 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13



Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01




Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

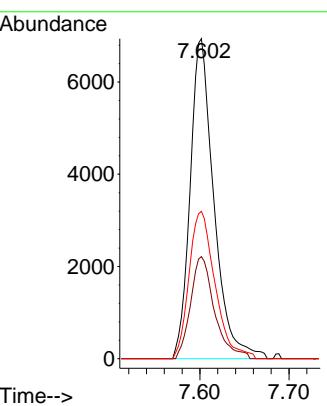

#52
1,1,2-Trichloroethane
Concen: 2.052 ug/l
RT: 8.393 min Scan# 2209
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

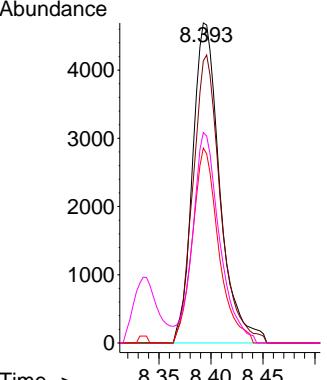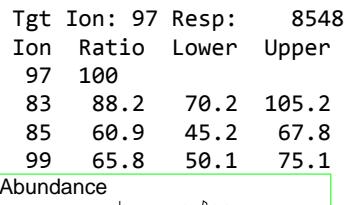



#53

1,3-Dichloropropane

Concen: 2.081 ug/l

RT: 8.569 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063522.D




Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#54

2-Hexanone

Concen: 10.271 ug/l

RT: 8.692 min Scan# 2302

Delta R.T. 0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 43 Resp: 21753







Ion Ratio Lower Upper

43 100

58 54.8 34.8 74.8

57 17.5 0.0 39.5

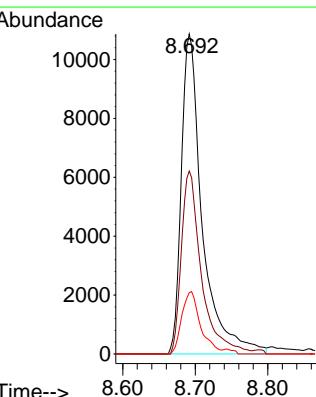



#55

Dibromochloromethane

Concen: 1.762 ug/l

RT: 8.801 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Instrument:


MSVOA_U

ClientSampleId :

VU0717WBSD01

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

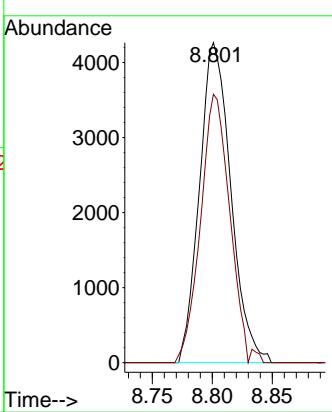

#56

1,2-Dibromoethane

Concen: 2.022 ug/l

RT: 8.917 min Scan# 2372

Delta R.T. 0.000 min

Lab File: VU063522.D


Acq: 17 Jul 2025 13:13


Tgt Ion:107 Resp: 7538

Ion Ratio Lower Upper

107 100

109 92.6 0.0 186.4

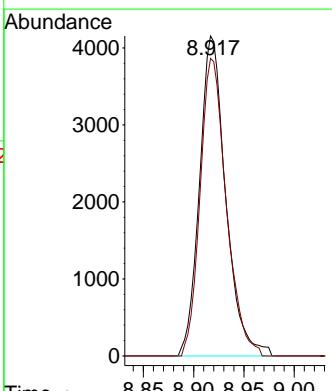


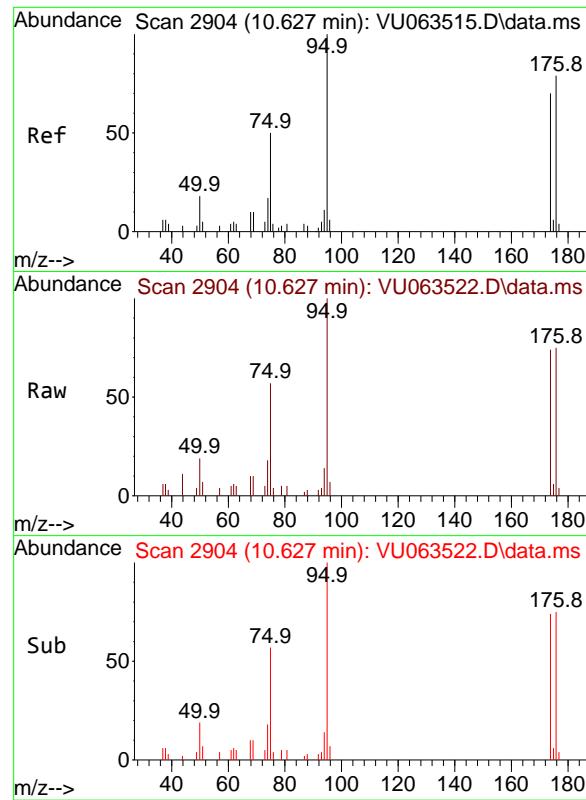


#57
4-Bromofluorobenzene
Concen: 1.033 ug/l
RT: 10.627 min Scan# 2255
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13


Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

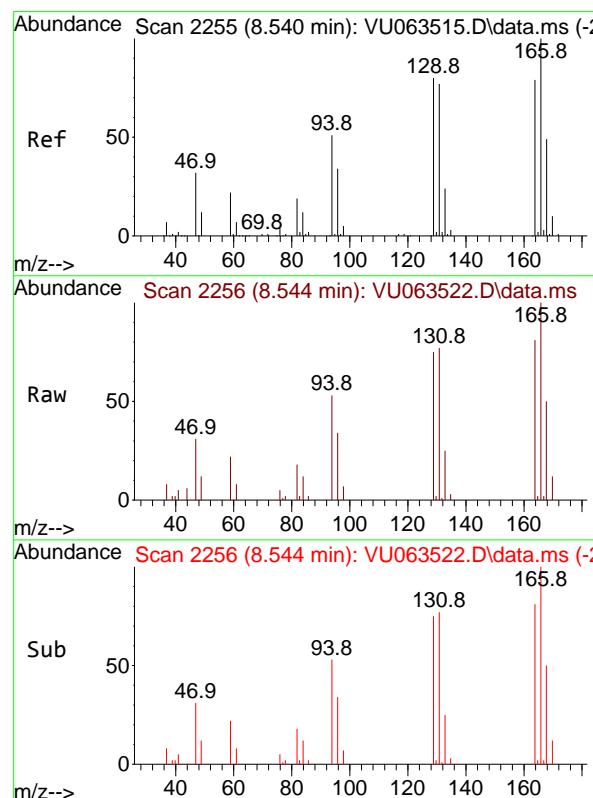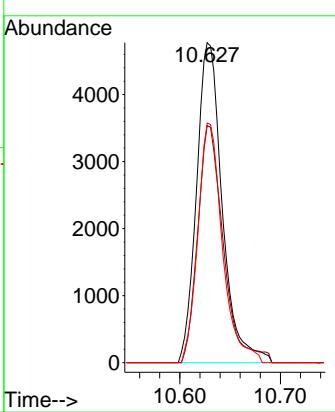

#58
Tetrachloroethene
Concen: 1.967 ug/l
RT: 8.544 min Scan# 2256
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

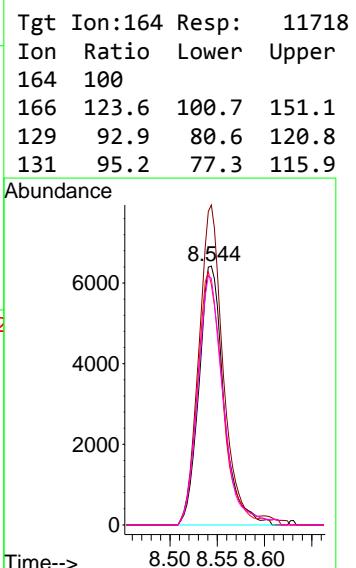

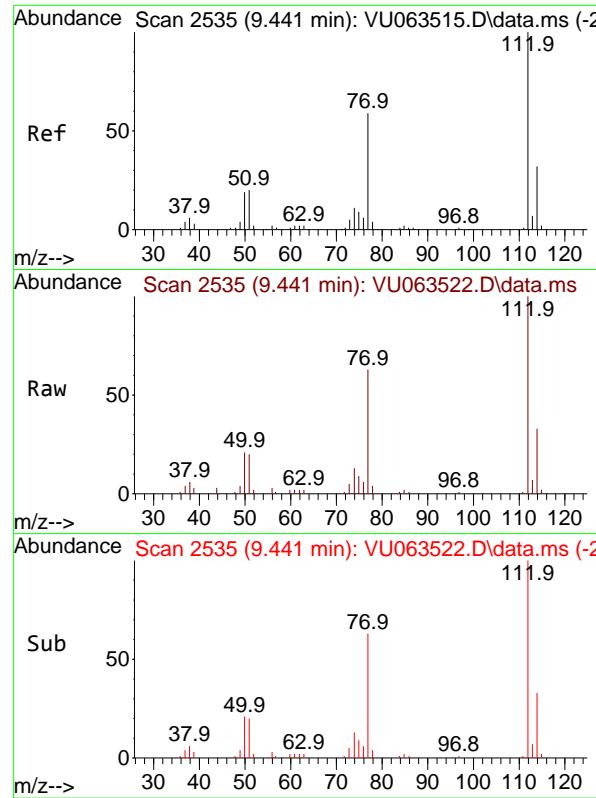


#59
Chlorobenzene
Concen: 1.964 ug/l
RT: 9.441 min Scan# 2
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

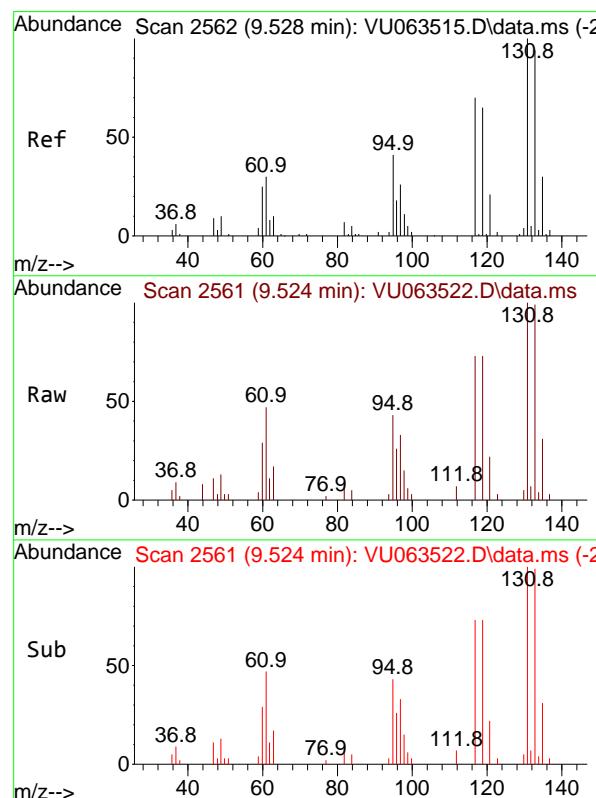

#60
1,1,1,2-Tetrachloroethane
Concen: 1.809 ug/l
RT: 9.524 min Scan# 2561
Delta R.T. -0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:131 Resp: 9309
Ion Ratio Lower Upper
131 100
133 96.1 74.7 112.1
119 67.2 53.0 79.4

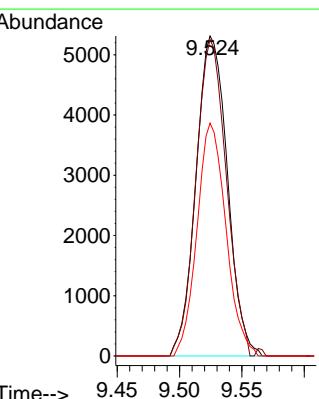



#61

Pentachloroethane

Concen: 1.814 ug/l

RT: 11.415 min Scan# 3149

Delta R.T. -0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13




Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**

 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#62

Hexachloroethane


Concen: 1.699 ug/l


RT: 12.466 min Scan# 3476

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

 Tgt Ion:117 Resp: 6118
 Ion Ratio Lower Upper
 117 100
 201 70.3 57.4 86.0




#63

Ethyl Benzene

Concen: 1.975 ug/l

RT: 9.563 min Scan# 2

Instrument:

Delta R.T. 0.000 min


MSVOA_U

Lab File: VU063522.D

ClientSampleId :

Acq: 17 Jul 2025 13:13



VU0717WBSD01

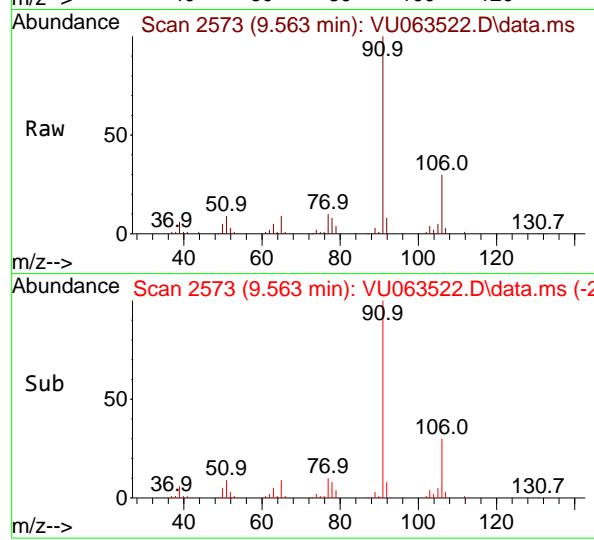

Tgt Ion: 91 Resp: 54379
 Ion Ratio Lower Upper
 91 100
 106 30.3 25.4 38.0


Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025

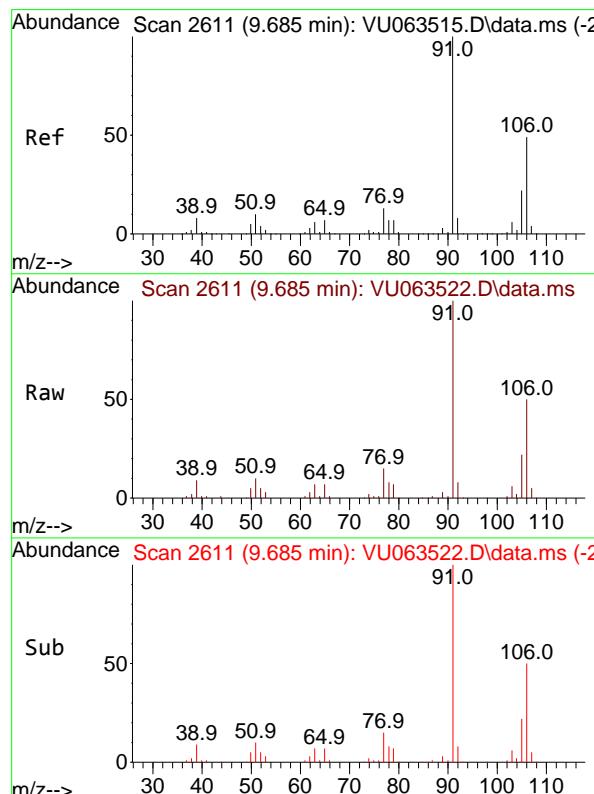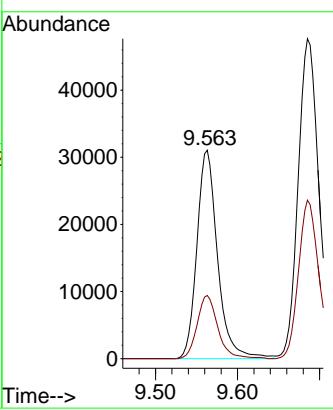

#64
 m/p-Xylenes
 Concen: 3.965 ug/l
 RT: 9.685 min Scan# 2611
 Delta R.T. 0.000 min
 Lab File: VU063522.D
 Acq: 17 Jul 2025 13:13

Tgt Ion:106 Resp: 42437
 Ion Ratio Lower Upper
 106 100
 91 203.4 163.6 245.4

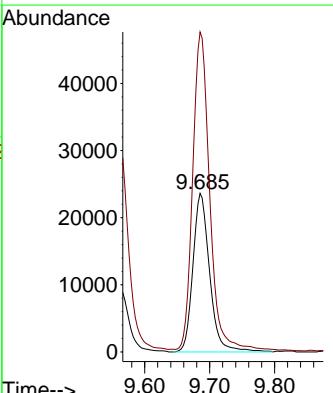


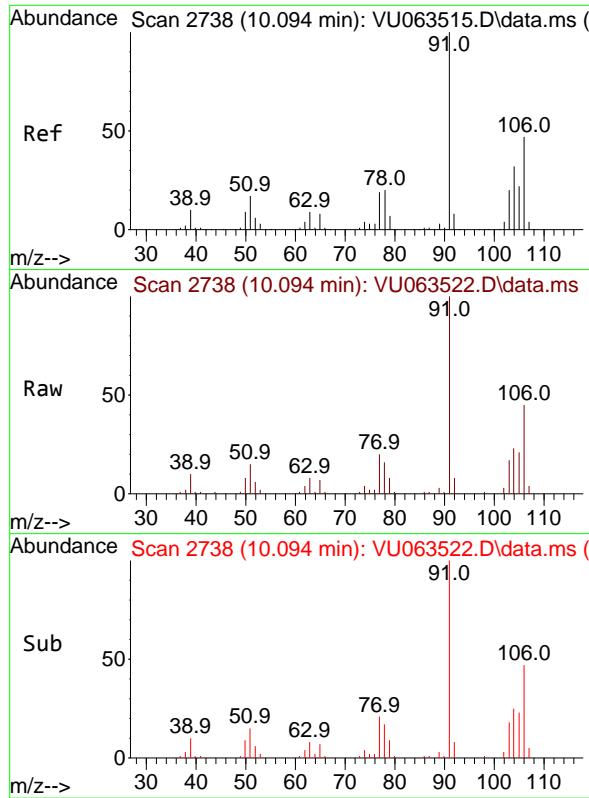


```
#65
o-Xylene
Concen: 1.972 ug/l
RT: 10.094 min Scan# 2 Instrument :
Delta R.T. 0.000 min MSVOA_U
Lab File: VU063522.D ClientSampleId :
Acq: 17 Jul 2025 13:13 VU0717WBSD01
```

Instrument :
SVOA_U
ClientSampleId :
U0717WBSD01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

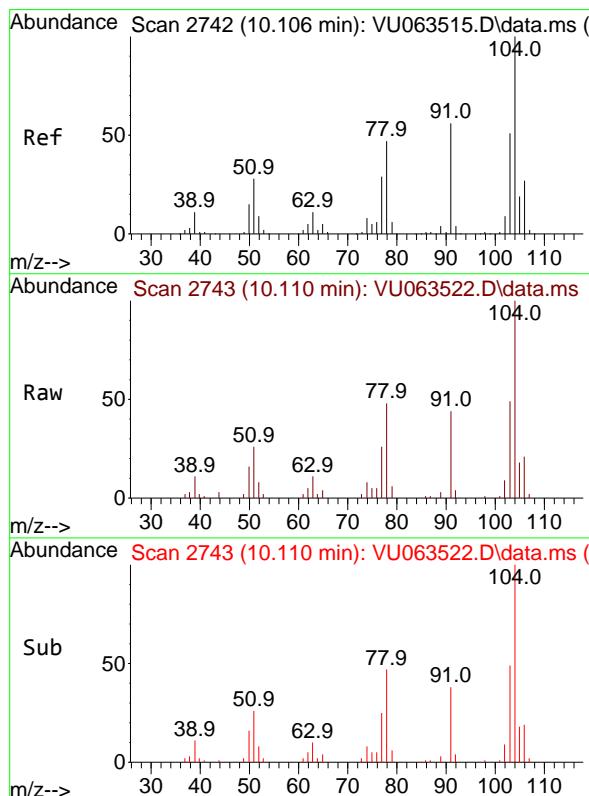

```
#66  
Styrene  
Concen: 2.000 ug/l  
RT: 10.110 min Scan# 2743  
Delta R.T. 0.003 min  
Lab File: VU063522.D  
Acq: 17 Jul 2025 13:13
```

Tgt	Ion:104	Resp:	32779
Ion	Ratio	Lower	Upper
104	100		
78	53.1	41.3	61.9
103	54.9	43.6	65.4

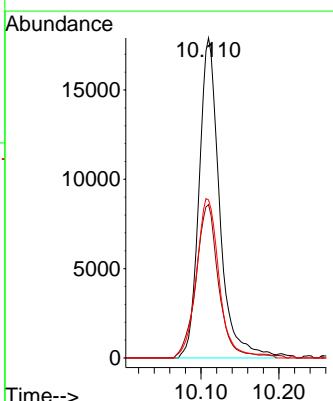



#67

Bromoform

Concen: 1.647 ug/l

RT: 10.283 min Scan# 2

Instrument:

Delta R.T. 0.000 min

MSVOA_U





Lab File: VU063522.D

ClientSampleId :

Acq: 17 Jul 2025 13:13

VU0717WBSD01

**Manual Integrations
APPROVED**

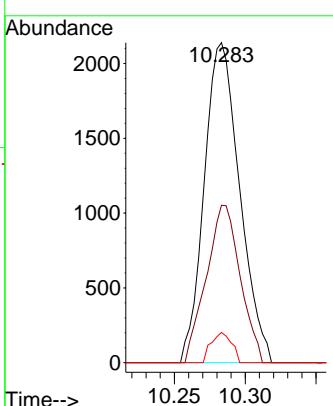 Reviewed By :Mahesh Dadoda 07/18/2025
 Supervised By :Semsettin Yesilyurt 07/21/2025


#68

1,2-Dichlorobenzene-d4

Concen: 1.103 ug/l


RT: 12.187 min Scan# 3389




Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Tgt	Ion:152	Resp:	8367
Ion	Ratio	Lower	Upper
152	100		
115	76.3	0.0	262.2
150	177.3	0.0	651.2





#69

Isopropylbenzene

Concen: 2.055 ug/l

RT: 10.476 min Scan# 2

Instrument:

Delta R.T. 0.000 min

MSVOA_U

Lab File: VU063522.D

ClientSampleId :

Acq: 17 Jul 2025 13:13

VU0717WBSD01

Tgt Ion:105 Resp: 5110

Ion Ratio Lower Upper




105 100

120 26.4 13.2 39.5

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025



#70

1,1,2,2-Tetrachloroethane

Concen: 2.038 ug/l

RT: 10.775 min Scan# 2950

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 83 Resp: 10327




Ion Ratio Lower Upper

83 100

131 9.3 8.4 12.6

85 62.8 51.9 77.9

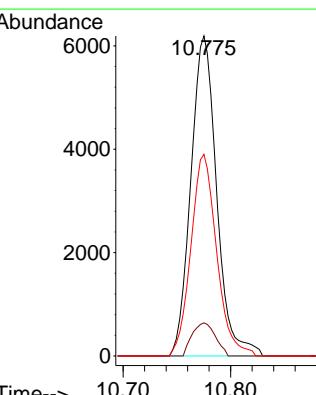



#71

1,2,3-Trichloropropane

Concen: 1.742 ug/l m

RT: 10.817 min Scan# 2963

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Instrument:




MSVOA_U

ClientSampleId :

VU0717WBSD01

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#72

Bromobenzene

Concen: 2.007 ug/l

RT: 10.778 min Scan# 2951

Delta R.T. 0.003 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion:156 Resp: 12879




Ion Ratio Lower Upper

156 100

77 162.7 0.0 315.2

158 91.3 0.0 195.4

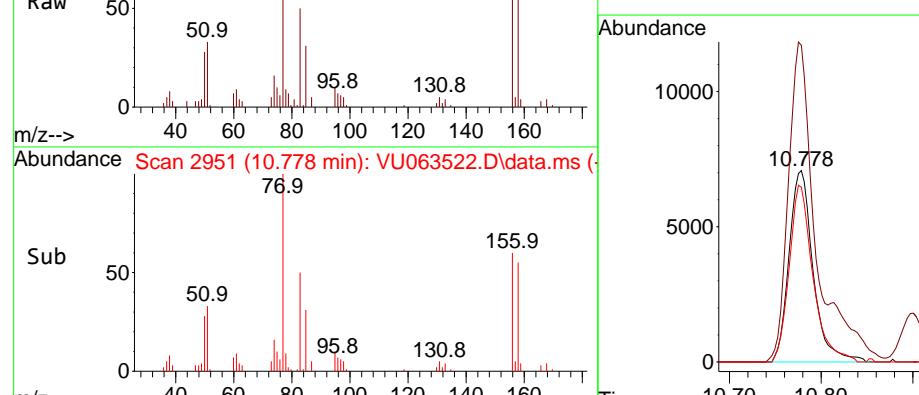



#73

n-propylbenzene

Concen: 2.023 ug/l

RT: 10.897 min Scan# 2

Delta R.T. 0.000 min

Lab File: VU063522.D





Acq: 17 Jul 2025 13:13

Instrument :

MSVOA_U

ClientSampleId :

VU0717WBSD01

**Manual Integrations
APPROVED**
Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

#74

2-Chlorotoluene


Concen: 1.982 ug/l




RT: 10.978 min Scan# 3013

Delta R.T. 0.000 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

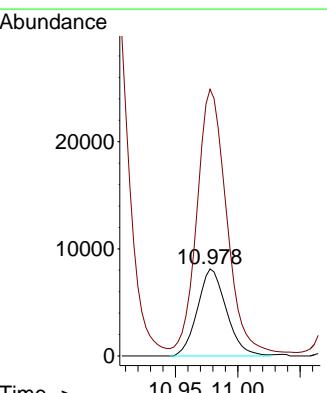Tgt Ion:126 Resp: 13109
Ion Ratio Lower Upper
126 100
91 313.6 0.0 606.0







#75
1,3,5-Trimethylbenzene
Concen: 1.986 ug/l
RT: 11.081 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#76
4-Chlorotoluene
Concen: 2.033 ug/l
RT: 11.090 min Scan# 3048
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:126 Resp: 13659
Ion Ratio Lower Upper
126 100
91 339.0 0.0 682.2




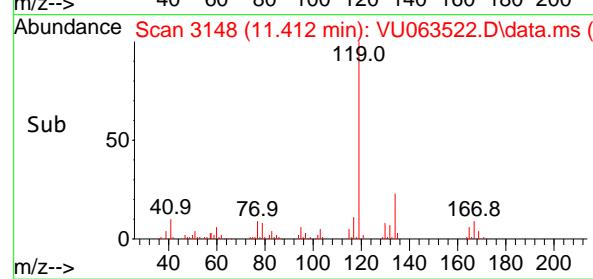
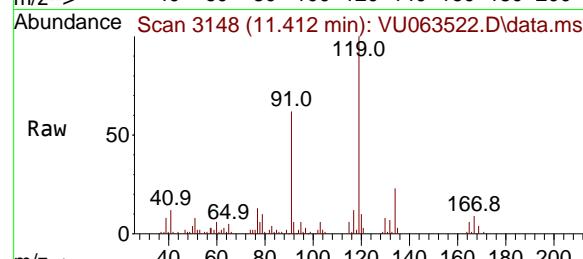



#77
tert-Butylbenzene
Concen: 2.000 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

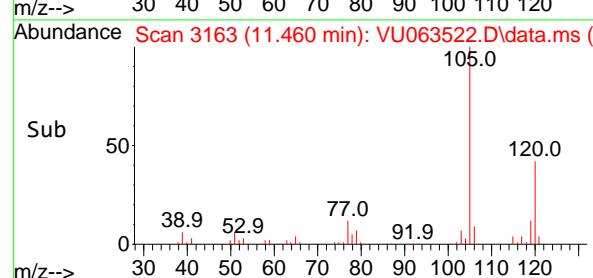

#78
1,2,4-Trimethylbenzene
Concen: 2.009 ug/l
RT: 11.460 min Scan# 3163
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:105 Resp: 47334
Ion Ratio Lower Upper
105 100
120 43.6 22.7 68.0








#79
sec-Butylbenzene
Concen: 2.030 ug/l
RT: 11.634 min Scan# 319
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025



#80
Nitrobenzene
Concen: 10.269 ug/l m
RT: 13.219 min Scan# 3710
Delta R.T. 0.016 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 77 Resp: 815
Ion Ratio Lower Upper
77 100
123 19.3 16.9 59.7
65 2.5 16.5 20.9#

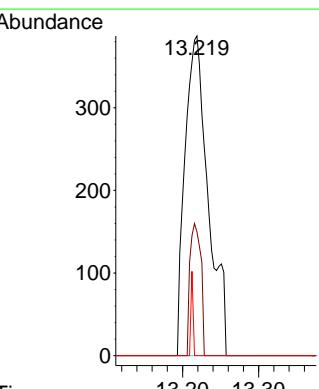






#81
p-Isopropyltoluene
Concen: 2.012 ug/l
RT: 11.785 min Scan# 3
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

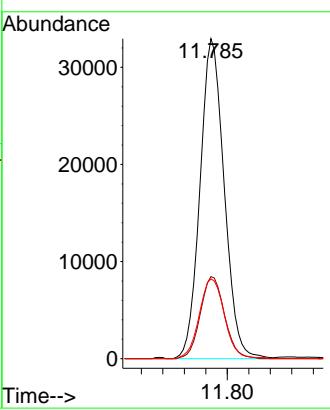

#82
1,3-Dichlorobenzene
Concen: 2.031 ug/l
RT: 11.740 min Scan# 3250
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:146 Resp: 26072
Ion Ratio Lower Upper
146 100
111 41.5 33.8 50.6
148 63.3 51.5 77.3

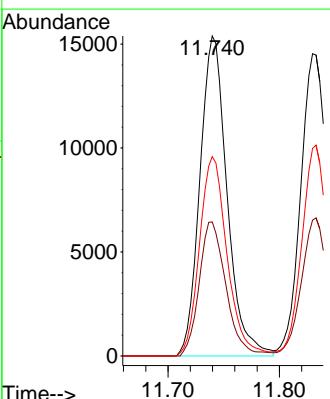

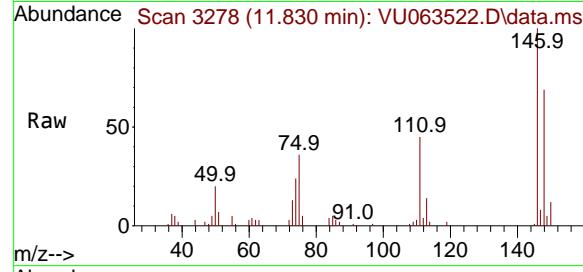




#83

1,4-Dichlorobenzene
Concen: 1.977 ug/l
RT: 11.830 min Scan# 3278
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument :
MSVOA_U
ClientSampleId :
VU0717WBSD01

Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025


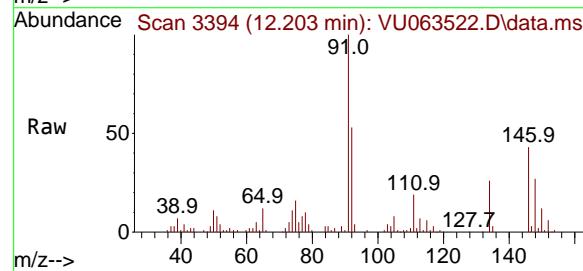



#84

n-Butylbenzene
Concen: 2.095 ug/l
RT: 12.203 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion: 91 Resp: 49653
Ion Ratio Lower Upper
91 100
92 50.8 41.5 62.3
134 24.7 20.6 30.8

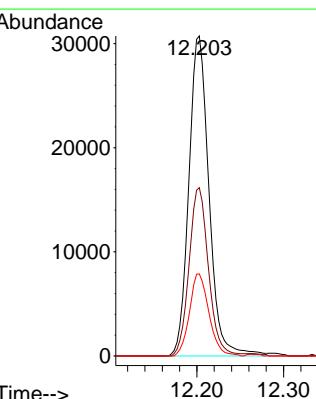

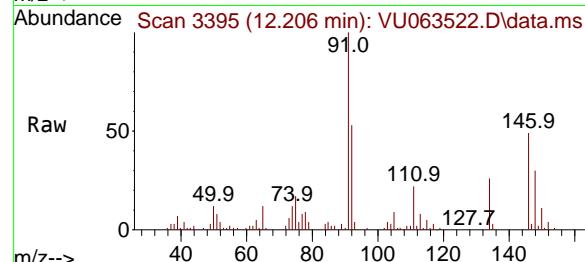

#85

1,2-Dichlorobenzene

Concen: 1.985 ug/l

RT: 12.206 min Scan# 3

Instrument:

MSVOA_U

Delta R.T. 0.000 min

Lab File: VU063522.D

ClientSampleId :

Acq: 17 Jul 2025 13:13

VU0717WBSD01

Tgt Ion:146 Resp: 23943

Ion Ratio Lower Upper

146 100




111 43.6 21.7 65.1

148 63.8 31.8 95.3

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

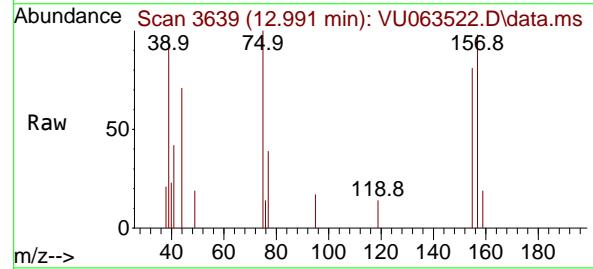

#86

1,2-Dibromo-3-Chloropropane

Concen: 2.003 ug/l

RT: 12.991 min Scan# 3639

Delta R.T. 0.004 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13


Tgt Ion: 75 Resp: 1326


Ion Ratio Lower Upper

75 100

155 82.9 65.8 98.6

157 97.0 81.4 122.2

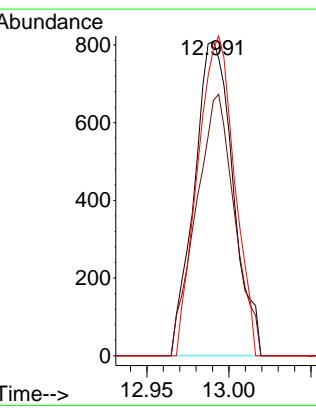


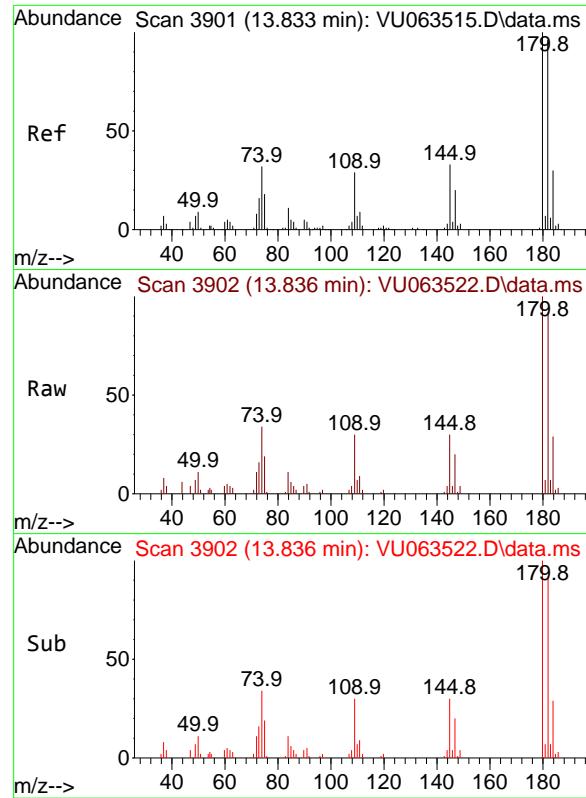


#87
1,2,4-Trichlorobenzene
Concen: 2.028 ug/l
RT: 13.836 min Scan# 3902
Delta R.T. 0.003 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Instrument : MSVOA_U
ClientSampleId : VU0717WBSD01


Manual Integrations
APPROVED







Reviewed By :Mahesh Dadoda 07/18/2025
Supervised By :Semsettin Yesilyurt 07/21/2025

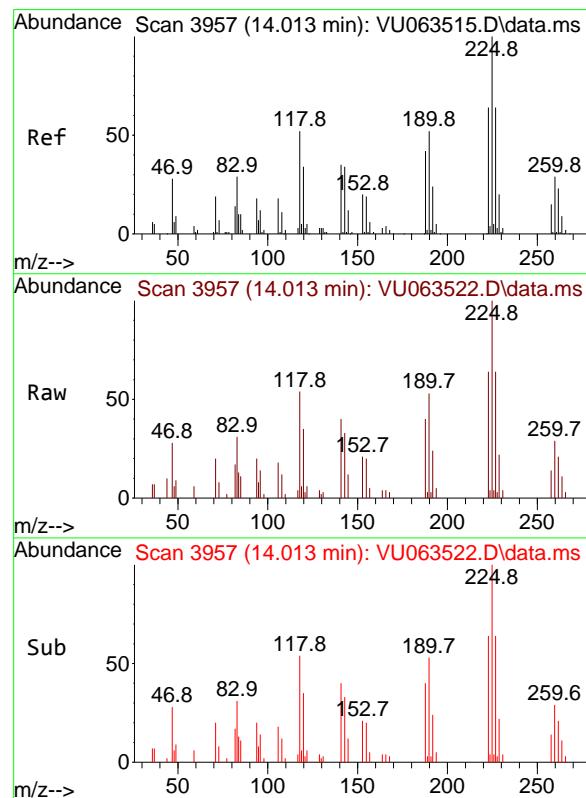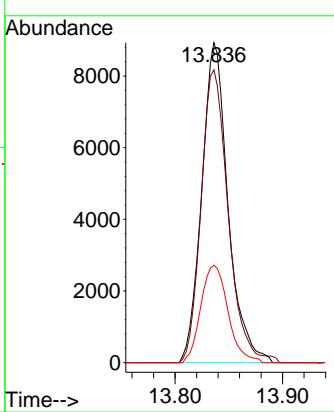

#88
Hexachlorobutadiene
Concen: 1.962 ug/l
RT: 14.013 min Scan# 3957
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13

Tgt Ion:225 Resp: 8359
Ion Ratio Lower Upper
225 100
223 64.0 50.8 76.2
227 63.9 51.0 76.6

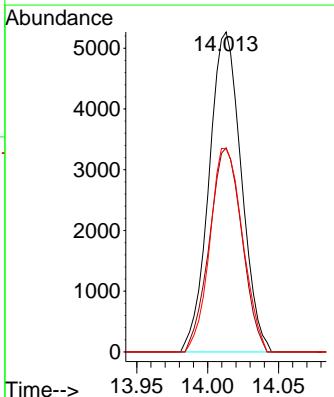

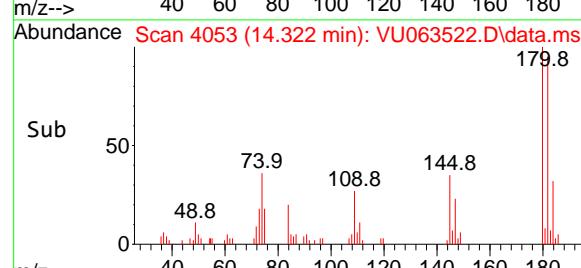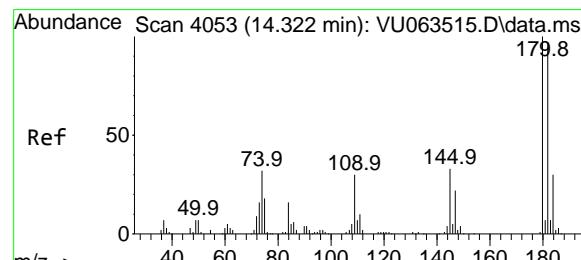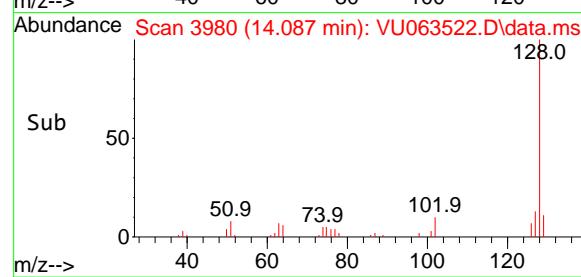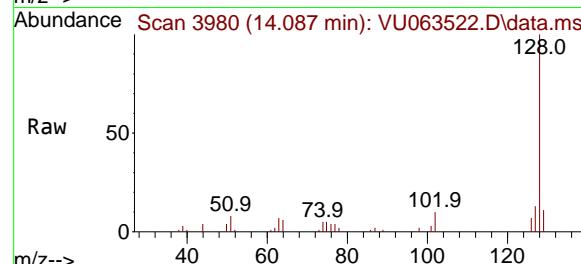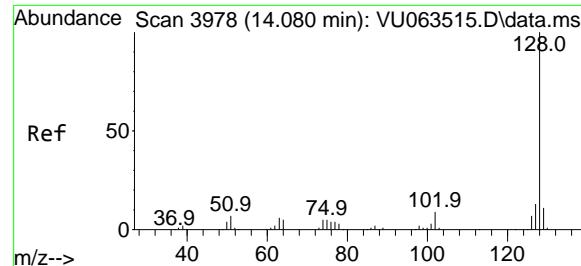

#89

Naphthalene

Concen: 2.112 ug/l

RT: 14.087 min Scan# 3

Delta R.T. 0.007 min

Lab File: VU063522.D

Acq: 17 Jul 2025 13:13

Instrument:

MSVOA_U

ClientSampleId :

VU0717WBSD01

Tgt Ion:128 Resp: 28380

Ion Ratio Lower Upper

128 100


127 12.6 10.2 15.4

129 10.1 8.8 13.2

Manual Integrations**APPROVED**

Reviewed By :Mahesh Dadoda 07/18/2025

Supervised By :Semsettin Yesilyurt 07/21/2025

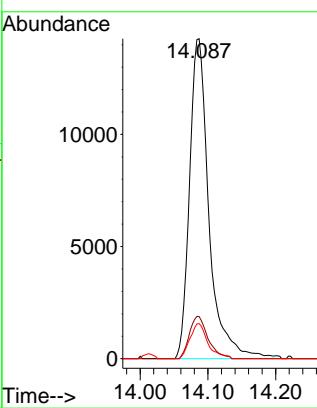

#90
1,2,3-Trichlorobenzene
Concen: 2.033 ug/l
RT: 14.322 min Scan# 4053
Delta R.T. 0.000 min
Lab File: VU063522.D
Acq: 17 Jul 2025 13:13


Tgt Ion:180 Resp: 14091

Ion Ratio Lower Upper

180 100

182 95.5 78.0 117.0

145 33.4 27.3 40.9

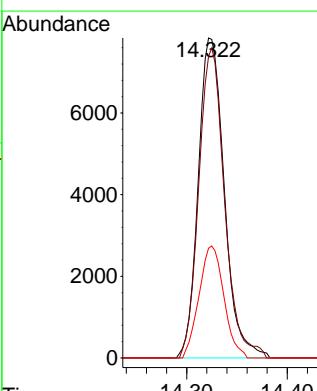



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VU071625	Instrument	MSVOA_u
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICC0.5	VU063511.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:34 AM	Sam	7/17/2025 8:26:15 AM	Peak Integrated by Software
VSTDICC0.5	VU063511.D	Acrylonitrile	MMDadod a	7/17/2025 8:18:34 AM	Sam	7/17/2025 8:26:15 AM	Peak Integrated by Software
VSTDICC0.5	VU063511.D	Methacrylonitrile	MMDadod a	7/17/2025 8:18:34 AM	Sam	7/17/2025 8:26:15 AM	Peak Integrated by Software
VSTDICC0.5	VU063511.D	Propionitrile	MMDadod a	7/17/2025 8:18:34 AM	Sam	7/17/2025 8:26:15 AM	Peak Integrated by Software
VSTDICC0.5	VU063511.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:34 AM	Sam	7/17/2025 8:26:15 AM	Peak Integrated by Software
VSTDICC001	VU063512.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:32 AM	Sam	7/17/2025 8:26:16 AM	Peak Integrated by Software
VSTDICC001	VU063512.D	Nitrobenzene	MMDadod a	7/17/2025 8:18:32 AM	Sam	7/17/2025 8:26:16 AM	Peak Integrated by Software
VSTDICC001	VU063512.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:32 AM	Sam	7/17/2025 8:26:16 AM	Peak Integrated by Software
VSTDICC002	VU063513.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:40 AM	Sam	7/17/2025 8:26:28 AM	Peak Integrated by Software
VSTDICC002	VU063513.D	Acrylonitrile	MMDadod a	7/17/2025 8:18:40 AM	Sam	7/17/2025 8:26:28 AM	Peak Integrated by Software
VSTDICC002	VU063513.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:40 AM	Sam	7/17/2025 8:26:28 AM	Peak Integrated by Software
VSTDICC005	VU063514.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:42 AM	Sam	7/17/2025 8:26:34 AM	Peak Integrated by Software
VSTDICC005	VU063514.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:42 AM	Sam	7/17/2025 8:26:34 AM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VU071625	Instrument	MSVOA_u
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICCC010	VU063515.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:43 AM	Sam	7/17/2025 8:26:27 AM	Peak Integrated by Software
VSTDICCC010	VU063515.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:43 AM	Sam	7/17/2025 8:26:27 AM	Peak Integrated by Software
VSTDICC015	VU063516.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:44 AM	Sam	7/17/2025 8:26:29 AM	Peak Integrated by Software
VSTDICC015	VU063516.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:44 AM	Sam	7/17/2025 8:26:29 AM	Peak Integrated by Software
VSTDICV010	VU063517.D	1,2,3-Trichloropropane	MMDadod a	7/17/2025 8:18:46 AM	Sam	7/17/2025 8:26:29 AM	Peak Integrated by Software
VSTDICV010	VU063517.D	Nitrobenzene	MMDadod a	7/17/2025 8:18:46 AM	Sam	7/17/2025 8:26:29 AM	Peak Integrated by Software
VSTDICV010	VU063517.D	t-1,4-Dichloro-2-butene	MMDadod a	7/17/2025 8:18:46 AM	Sam	7/17/2025 8:26:29 AM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VU071725	Instrument	MSVOA_u
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC010	VU063519.D	1,2,3-Trichloropropane	MMDadod a	7/18/2025 3:02:41 PM	Sam	7/21/2025 9:37:37 PM	Peak Integrated by Software
VSTDCCC010	VU063519.D	t-1,4-Dichloro-2-butene	MMDadod a	7/18/2025 3:02:41 PM	Sam	7/21/2025 9:37:37 PM	Peak Integrated by Software
VU0717WBS01	VU063521.D	1,2,3-Trichloropropane	MMDadod a	7/18/2025 3:02:42 PM	Sam	7/21/2025 9:37:50 PM	Peak Integrated by Software
VU0717WBS01	VU063521.D	Nitrobenzene	MMDadod a	7/18/2025 3:02:42 PM	Sam	7/21/2025 9:37:50 PM	Peak Integrated by Software
VU0717WBS01	VU063521.D	t-1,4-Dichloro-2-butene	MMDadod a	7/18/2025 3:02:42 PM	Sam	7/21/2025 9:37:50 PM	Peak Integrated by Software
VU0717WBSD0 1	VU063522.D	1,2,3-Trichloropropane	MMDadod a	7/18/2025 3:02:43 PM	Sam	7/21/2025 9:37:57 PM	Peak Integrated by Software
VU0717WBSD0 1	VU063522.D	Nitrobenzene	MMDadod a	7/18/2025 3:02:43 PM	Sam	7/21/2025 9:37:57 PM	Peak Integrated by Software
VU0717WBSD0 1	VU063522.D	t-1,4-Dichloro-2-butene	MMDadod a	7/18/2025 3:02:43 PM	Sam	7/21/2025 9:37:57 PM	Peak Integrated by Software
Q2552-07	VU063529.D	Fluorobenzene	MMDadod a	7/18/2025 3:02:47 PM	Sam	7/21/2025 9:38:21 PM	Peak Integrated by Software
VSTDCCC010	VU063530.D	1,2,3-Trichloropropane	MMDadod a	7/18/2025 3:02:48 PM	Sam	7/21/2025 9:38:30 PM	Peak Integrated by Software
VSTDCCC010	VU063530.D	t-1,4-Dichloro-2-butene	MMDadod a	7/18/2025 3:02:48 PM	Sam	7/21/2025 9:38:30 PM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VU071825	Instrument	MSVOA_u
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC010	VU063532.D	1,2,3-Trichloropropane	MMDadoda	7/21/2025 1:56:28 PM	SAM	7/21/2025 2:01:31 PM	Peak Integrated by Software
VSTDCCC010	VU063532.D	t-1,4-Dichloro-2-butene	MMDadoda	7/21/2025 1:56:28 PM	SAM	7/21/2025 2:01:31 PM	Peak Integrated by Software
VU0718WBS02	VU063535.D	1,2,3-Trichloropropane	MMDadoda	7/21/2025 1:56:29 PM	SAM	7/21/2025 2:01:27 PM	Peak Integrated by Software
VU0718WBS02	VU063535.D	t-1,4-Dichloro-2-butene	MMDadoda	7/21/2025 1:56:29 PM	SAM	7/21/2025 2:01:27 PM	Peak Integrated by Software
VSTDCCC010	VU063544.D	1,2,3-Trichloropropane	SAM	7/21/2025 2:01:33 PM	MMDadoda	7/21/2025 9:33:11 PM	Peak Integrated by Software
VSTDCCC010	VU063544.D	t-1,4-Dichloro-2-butene	SAM	7/21/2025 2:01:33 PM	MMDadoda	7/21/2025 9:33:11 PM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_U

Daily Analysis Runlog For Sequence/QCBatch ID # VU071625

Review By	Mahesh Dadoda	Review On	7/17/2025 8:19:30 AM
Supervise By	Semsettin Yesilyurt	Supervise On	7/17/2025 8:26:51 AM
SubDirectory	VU071625	HP Acquire Method	MSVOA_U
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134776 VP134778,VP134779,VP134780,VP134781,VP134782,VP134783 VP134722 VP134784		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VU063510.D	16 Jul 2025 08:13	MD/SY	Ok
2	VSTDICCC0.5	VU063511.D	16 Jul 2025 09:24	MD/SY	Ok,M
3	VSTDICCC001	VU063512.D	16 Jul 2025 09:54	MD/SY	Ok,M
4	VSTDICCC002	VU063513.D	16 Jul 2025 10:27	MD/SY	Ok,M
5	VSTDICCC005	VU063514.D	16 Jul 2025 11:00	MD/SY	Ok,M
6	VSTDICCC010	VU063515.D	16 Jul 2025 11:37	MD/SY	Ok,M
7	VSTDICCC015	VU063516.D	16 Jul 2025 12:11	MD/SY	Ok,M
8	VSTDICCV010	VU063517.D	16 Jul 2025 14:19	MD/SY	Ok,M

M : Manual Integration

Instrument ID: MSVOA_U

Daily Analysis Runlog For Sequence/QCBatch ID # VU071725

Review By	Mahesh Dadoda	Review On	7/18/2025 3:02:54 PM
Supervise By	Semsettin Yesilyurt	Supervise On	7/21/2025 9:38:41 PM
SubDirectory	VU071725	HP Acquire Method	HP Processing Method
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134805		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134806,VP134807 VP134722		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VU063518.D	17 Jul 2025 08:10	MD/SY	Ok
2	VSTDCCC010	VU063519.D	17 Jul 2025 09:25	MD/SY	Ok,M
3	VU0717WBL01	VU063520.D	17 Jul 2025 11:31	MD/SY	Ok
4	VU0717WBS01	VU063521.D	17 Jul 2025 12:43	MD/SY	Ok,M
5	VU0717WBSD01	VU063522.D	17 Jul 2025 13:13	MD/SY	Ok,M
6	Q2552-09	VU063523.D	17 Jul 2025 14:16	MD/SY	Dilution
7	Q2552-09DL	VU063524.D	17 Jul 2025 14:47	MD/SY	Ok
8	Q2552-10	VU063525.D	17 Jul 2025 15:17	MD/SY	Dilution
9	Q2552-10DL	VU063526.D	17 Jul 2025 15:48	MD/SY	Ok
10	RL-CHECK	VU063527.D	17 Jul 2025 16:18	MD/SY	Ok,M
11	RL-CHECK	VU063528.D	17 Jul 2025 16:49	MD/SY	Ok,M
12	Q2552-07	VU063529.D	17 Jul 2025 17:20	MD/SY	Dilution
13	VSTDCCC010	VU063530.D	17 Jul 2025 18:21	MD/SY	Ok,M

M : Manual Integration

Instrument ID: MSVOA_U

Daily Analysis Runlog For Sequence/QCBatch ID # VU071825

Review By	Mahesh Dadoda	Review On	7/21/2025 1:56:39 PM
Supervise By	Semsettin Yesilyurt	Supervise On	7/21/2025 9:34:13 PM
SubDirectory	VU071825	HP Acquire Method	MSVOA_U
HP Processing Method	524u071625dw.m		
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134835		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134836,VP134837,RL-VP134838,VP134839		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VU063531.D	18 Jul 2025 08:07	MD/SY	Ok
2	VSTDCCC010	VU063532.D	18 Jul 2025 09:11	MD/SY	Ok,M
3	VU0718WBL01	VU063533.D	18 Jul 2025 10:49	MD/SY	Ok
4	VU0718WBS01	VU063534.D	18 Jul 2025 11:20	MD/SY	Not Ok
5	VU0718WBS02	VU063535.D	18 Jul 2025 11:50	MD/SY	Ok,M
6	VU0718WBSD02	VU063536.D	18 Jul 2025 13:28	MD/SY	Ok,M
7	Q2552-11	VU063537.D	18 Jul 2025 15:24	MD/SY	Not Ok
8	Q2552-08	VU063538.D	18 Jul 2025 15:54	MD/SY	Dilution
9	Q2552-08DL	VU063539.D	18 Jul 2025 16:24	MD/SY	Ok
10	VIBLK	VU063540.D	18 Jul 2025 16:55	MD/SY	Ok
11	Q2552-07DL	VU063541.D	18 Jul 2025 17:25	MD/SY	Ok
12	RL-CHECK	VU063542.D	18 Jul 2025 17:56	MD/SY	Ok,M
13	RL-CHECK	VU063543.D	18 Jul 2025 18:26	MD/SY	Ok,M
14	VSTDCCC010	VU063544.D	18 Jul 2025 18:56	MD/SY	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_U

Daily Analysis Runlog For Sequence/QCBatch ID # VU071625

Review By	Mahesh Dadoda	Review On	7/17/2025 8:19:30 AM		
Supervise By	Semsettin Yesilyurt	Supervise On	7/17/2025 8:26:51 AM		
SubDirectory	VU071625	HP Acquire Method	MSVOA_U	HP Processing Method	524u071625dw.m
STD. NAME	STD REF.#				
Tune/Reschk	VP134776				
Initial Calibration Stds	VP134778,VP134779,VP134780,VP134781,VP134782,VP134783				
CCC					
Internal Standard/PEM	VP134722				
ICV/I.BLK	VP134784				
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VU063510.D	16 Jul 2025 08:13		MD/SY	Ok
2	VSTDICCC0.5	VSTDICCC0.5	VU063511.D	16 Jul 2025 09:24		MD/SY	Ok,M
3	VSTDICCC001	VSTDICCC001	VU063512.D	16 Jul 2025 09:54	LR - 10 And QR - 80,86	MD/SY	Ok,M
4	VSTDICCC002	VSTDICCC002	VU063513.D	16 Jul 2025 10:27		MD/SY	Ok,M
5	VSTDICCC005	VSTDICCC005	VU063514.D	16 Jul 2025 11:00		MD/SY	Ok,M
6	VSTDICCC010	VSTDICCC010	VU063515.D	16 Jul 2025 11:37		MD/SY	Ok,M
7	VSTDICCC015	VSTDICCC015	VU063516.D	16 Jul 2025 12:11		MD/SY	Ok,M
8	VSTDICCV010	ICVVU071625	VU063517.D	16 Jul 2025 14:19	ICV failed for com.#13,69,80	MD/SY	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_U

Daily Analysis Runlog For Sequence/QCBatch ID # VU071725

Review By	Mahesh Dadoda	Review On	7/18/2025 3:02:54 PM
Supervise By	Semsettin Yesilyurt	Supervise On	7/21/2025 9:38:41 PM
SubDirectory	VU071725	HP Acquire Method	HP Processing Method
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134805		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134806,VP134807 VP134722		

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VU063518.D	17 Jul 2025 08:10		MD/SY	Ok
2	VSTDCCC010	VSTDCCC010	VU063519.D	17 Jul 2025 09:25	524.2 PT study	MD/SY	Ok,M
3	VU0717WBL01	VU0717WBL01	VU063520.D	17 Jul 2025 11:31		MD/SY	Ok
4	VU0717WBS01	VU0717WBS01	VU063521.D	17 Jul 2025 12:43		MD/SY	Ok,M
5	VU0717WBSD01	VU0717WBSD01	VU063522.D	17 Jul 2025 13:13		MD/SY	Ok,M
6	Q2552-09	WS0725-PT-THM-WS	VU063523.D	17 Jul 2025 14:16	Need 5X(THM)	MD/SY	Dilution
7	Q2552-09DL	WS0725-PT-THM-WSD	VU063524.D	17 Jul 2025 14:47		MD/SY	Ok
8	Q2552-10	WS0725-PT-ADD-WS	VU063525.D	17 Jul 2025 15:17	Need 4X(ADD-WS)	MD/SY	Dilution
9	Q2552-10DL	WS0725-PT-ADD-WSD	VU063526.D	17 Jul 2025 15:48		MD/SY	Ok
10	RL-CHECK	RL-CHECK	VU063527.D	17 Jul 2025 16:18	RL-0.5 ppb	MD/SY	Ok,M
11	RL-CHECK	RL-CHECK	VU063528.D	17 Jul 2025 16:49	RL-1.0 ppb	MD/SY	Ok,M
12	Q2552-07	WS0725-PT-RVOA-WS	VU063529.D	17 Jul 2025 17:20	Need 4X(RVOA)	MD/SY	Dilution
13	VSTDCCC010	VSTDCCC010EC	VU063530.D	17 Jul 2025 18:21		MD/SY	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_U

Daily Analysis Runlog For Sequence/QCBatch ID # VU071825

Review By	Mahesh Dadoda	Review On	7/21/2025 1:56:39 PM		
Supervise By	Semsettin Yesilyurt	Supervise On	7/21/2025 9:34:13 PM		
SubDirectory	VU071825	HP Acquire Method	MSVOA_U	HP Processing Method	524u071625dw.m
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds	VP134835				
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134836,VP134837,RL-VP134838,VP134839				

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VU063531.D	18 Jul 2025 08:07		MD/SY	Ok
2	VSTDCCC010	VSTDCCC010	VU063532.D	18 Jul 2025 09:11		MD/SY	Ok,M
3	VU0718WBL01	VU0718WBL01	VU063533.D	18 Jul 2025 10:49		MD/SY	Ok
4	VU0718WBS01	VU0718WBS01	VU063534.D	18 Jul 2025 11:20	Recovery failed	MD/SY	Not Ok
5	VU0718WBS02	VU0718WBS02	VU063535.D	18 Jul 2025 11:50		MD/SY	Ok,M
6	VU0718WBSD02	VU0718WBSD02	VU063536.D	18 Jul 2025 13:28		MD/SY	Ok,M
7	Q2552-11	WS0725-PT-EDBCP-W	VU063537.D	18 Jul 2025 15:24	prep error	MD/SY	Not Ok
8	Q2552-08	WS0725-PT-UNROVA-	VU063538.D	18 Jul 2025 15:54	Need 4X(UNROVA)	MD/SY	Dilution
9	Q2552-08DL	WS0725-PT-UNROVA-	VU063539.D	18 Jul 2025 16:24		MD/SY	Ok
10	VIBLK	VIBLK	VU063540.D	18 Jul 2025 16:55		MD/SY	Ok
11	Q2552-07DL	WS0725-PT-RVOA-WS	VU063541.D	18 Jul 2025 17:25	RVOA	MD/SY	Ok
12	RL-CHECK	RL-CHECK	VU063542.D	18 Jul 2025 17:56	RL-0.5 ppb	MD/SY	Ok,M
13	RL-CHECK	RL-CHECK	VU063543.D	18 Jul 2025 18:26	RL-1.0 ppb	MD/SY	Ok,M
14	VSTDCCC010	VSTDCCC010EC	VU063544.D	18 Jul 2025 18:56		MD/SY	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789
8900, Fax : 908 789 8922

Prep Standard - Chemical Standard Summary

Order ID : Q2552

Test : VOCMS Group1

Prepbatch ID :

Sequence ID/Qc Batch ID: VU071725,VU071825,

Standard ID :

VP133953,VP134722,VP134723,VP134805,VP134806,VP134807,VP134835,VP134836,VP134837,VP134839,

Chemical ID :

RL-VP134838,V13391,V13880,V14419,V14626,V14629,V14710,V14747,V14838,V15045,W3112,



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
218	BFB, 25PPM	VP133953	05/19/2025	11/09/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 05/21/2025

FROM 0.25000ml of V13391 + 24.75000ml of V14626 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
552	524 Internal STD and Surrogate Mix, 5 PPM	VP134722	07/11/2025	12/31/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 07/23/2025

FROM 0.02500ml of V15045 + 9.97500ml of V14629 = Final Quantity: 10.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
553	524 Calibration CC Mix Working STD, 25 PPM	VP134723	07/11/2025	09/30/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 07/23/2025

FROM 0.12500ml of V13880 + 0.12500ml of V14419 + 0.12500ml of V14747 + 0.12500ml of V14838 + 0.25000ml of V14710 + 9.24500ml of V14629 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1736	BFB	VP134805	07/17/2025	07/18/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP133953 = Final Quantity: 40.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1131	10 PPB CCC, 524.2	VP134806	07/17/2025	07/18/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.97600ml of W3112 + 0.00800ml of VP134722 + 0.01600ml of VP134723 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
589	BFB TUNE CHECK	VP134807	07/17/2025	07/18/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP133953 = Final Quantity: 40.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1736	BFB	VP134835	07/18/2025	07/19/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP133953 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1131	10 PPB CCC, 524.2	VP134836	07/18/2025	07/19/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.97600ml of W3112 + 0.00800ml of VP134722 + 0.01600ml of VP134723 = Final Quantity: 40.000 ml

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1131	10 PPB CCC, 524.2	VP134837	07/18/2025	07/19/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.97600ml of W3112 + 0.00800ml of VP134722 + 0.01600ml of VP134723 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1898	524 LOD LOQ, 1PPB	VP134839	07/18/2025	07/19/2025	Mahesh Dadoda	None	None	Semsettin Yesilyurt 07/23/2025

FROM 39.99000ml of W3112 + 0.00160ml of VP134723 + 0.00800ml of VP134722 = Final Quantity: 40.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30067 / BFB tuneing solution	A0191805	11/22/2025	11/22/2024 / SAM	01/13/2023 / SAM	V13391
Restek	564323 / Custom Oxygenates Standard	A0199211	06/16/2026	06/16/2025 / SAM	06/30/2023 / SAM	V13880
Restek	30601 / VOA Mega Mix, Drinking Water VOA Mega Mix, 524.2 Rev 4.1, 1mL, 2000ug/mL P&TM	A0204639	10/17/2025	10/17/2024 / SAM	06/04/2024 / SAM	V14419
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	23I0762004	11/09/2025	05/09/2025 / SAM	11/26/2024 / SAM	V14626
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	23I0762004	01/09/2026	07/07/2025 / SAM	11/26/2024 / SAM	V14629
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	12/16/2025	06/16/2025 / SAM	12/17/2024 / SAM	V14710



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	12/16/2025	06/16/2025 / SAM	12/17/2024 / SAM	V14747
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	560065 / Custom Standard, 524 Std w/ COC [CS 8005]	A0220861	01/31/2026	06/16/2025 / SAM	01/16/2025 / SAM	V14838
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30201 / VOA Mix,500 series method, 524 Internal Std., 2000ug/mL. P&TM, 1mL/ampul	A0223883	07/11/2026	07/11/2025 / SAM	07/01/2025 / SAM	V15045
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 23I0762004
Manufactured Date: 2023-08-11
Expiration Date: 2026-08-10
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.5 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.01
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink.

Ken Koehnlein
Sr. Manager, Quality Assurance

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 23I0762004
Manufactured Date: 2023-08-11
Expiration Date: 2026-08-10
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.5 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.01
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink.

Ken Koehnlein
Sr. Manager, Quality Assurance



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30067

Lot No.: A0191805

Description : 4-Bromofluorobenzene Standard

4-Bromofluorobenzene Standard 2,500 μ g/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : November 30, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	2,483.9 μ g/mL	+/- 139.5488

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:


40 ml/min

Inj. Vol


1 μ l

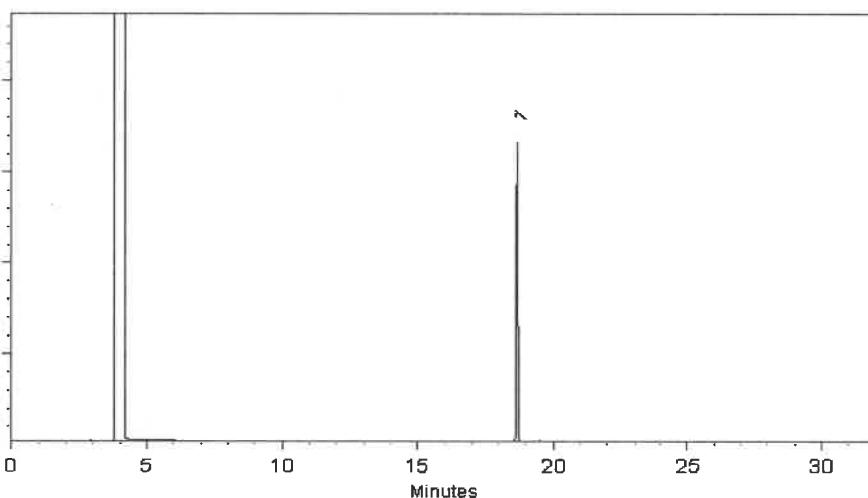

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Alicia Leathers - Operation Technician I

Date Mixed: 17-Nov-2022 Balance Serial #: B251644995


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Nov-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/pECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Certificate of Analysis

chromatographic



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 564323

Lot No.: A0199211

Description : Custom Oxygenates Standard

Custom Oxygenates Standard 2,000-10,000µg/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : June 30, 2028

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	tert-Butanol (TBA)	75-65-0	101619K21F-1	99%	10,093.2 µg/mL	+/- 125.6116
2	Diisopropyl ether (DIPE)	108-20-3	STBK3450	99%	2,011.0 µg/mL	+/- 25.0950
3	Ethyl-tert-butyl ether (ETBE)	637-92-3	MKCP5997	99%	2,009.8 µg/mL	+/- 25.0800
4	tert-Amyl methyl ether (TAME)	994-05-8	HMBJ0825	99%	2,009.2 µg/mL	+/- 25.0726
5	tert-Amyl ethyl ether (TAEE)	919-94-8	IKVYB	97%	2,010.4 µg/mL	+/- 25.0878

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

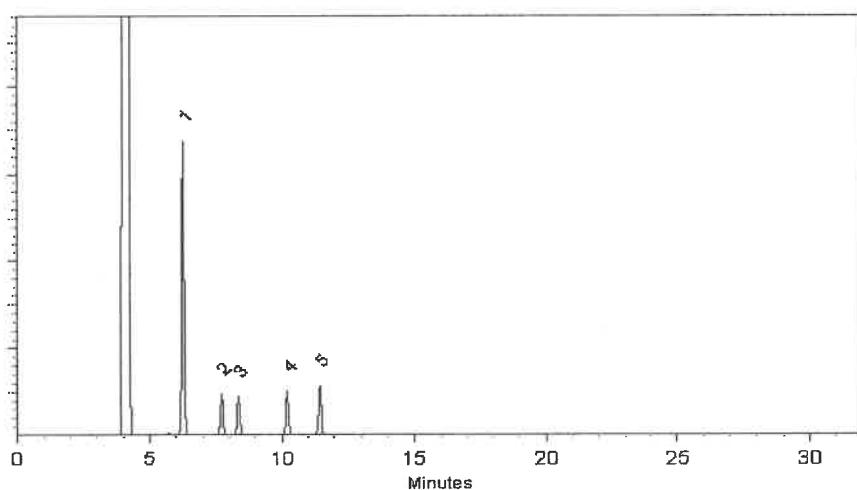

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Bryan Snyder
Bryan Snyder - Operations Tech I

Date Mixed: 22-Jun-2023 Balance Serial #: 1128342314

Jennifer Polino
Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 23-Jun-2023



Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ILAC
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30601

Lot No.: A0204639

Description : Drinking Water VOA MegaMix™, 524.2 Rev 4.1

Drinking Water VOA Mega Mix 524.2 Rev 4.1, 2000 μ g/mL, P&T
Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : November 30, 2026

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Diethyl ether (ethyl ether)	60-29-7	SHBQ1495	99%	2,016.9 μ g/mL	+/- 70.1908
2	1,1-dichloroethene	75-35-4	SHBG8609V	99%	2,009.6 μ g/mL	+/- 69.9229
3	Iodomethane (methyl iodide)	74-88-4	MKCN8012	99%	2,016.5 μ g/mL	+/- 70.1787
4	Allyl chloride (3-chloropropene)	107-05-1	RD221118RSR	99%	2,017.0 μ g/mL	+/- 69.7168
5	Methylene chloride (dichloromethane)	75-09-2	231383	99%	2,013.2 μ g/mL	+/- 70.0499
6	Carbon disulfide	75-15-0	N28F701	99%	2,017.0 μ g/mL	+/- 70.1961
7	Acrylonitrile	107-13-1	102466R02E	99%	2,017.1 μ g/mL	+/- 70.1995
8	Methyl-tert-butyl ether (MTBE)	1634-04-4	SHBP0179	99%	2,017.0 μ g/mL	+/- 69.7168
9	trans-1,2-Dichloroethene	156-60-5	MKCP9516	99%	2,011.9 μ g/mL	+/- 70.0038
10	1,1-Dichloroethane	75-34-3	852900	99%	2,010.5 μ g/mL	+/- 69.9560
11	Propionitrile	107-12-0	BCCH7430	99%	2,017.0 μ g/mL	+/- 70.1943
12	2,2-Dichloropropane	594-20-7	RD230426	99%	2,013.2 μ g/mL	+/- 70.0652
13	cis-1,2-Dichloroethene	156-59-2	MKCP7830	99%	2,014.0 μ g/mL	+/- 70.0903
14	Methacrylonitrile	126-98-7	1012014	99%	2,015.7 μ g/mL	+/- 70.1491
15	Methyl acrylate	96-33-3	SHBG6616V	99%	2,019.0 μ g/mL	+/- 70.2639
16	chloroform	67-66-3	SHBN8469	99%	2,009.7 μ g/mL	+/- 69.9273

17	Bromochloromethane	74-97-5	230810JLM	99%	2,016.0	µg/mL	+/-	70.1613
18	Tetrahydrofuran	109-99-9	SHBQ0910	99%	2,019.6	µg/mL	+/-	70.2865
19	1,1,1-trichloroethane	71-55-6	RD230728RSR	99%	2,011.1	µg/mL	+/-	69.9769
20	1-Chlorobutane (Butyl chloride)	109-69-3	SHBC2651V	99%	2,015.0	µg/mL	+/-	69.6476
21	1,1-Dichloropropene	563-58-6	230825JLM	99%	2,018.9	µg/mL	+/-	70.2629
22	carbon tetrachloride	56-23-5	SHBP4875	99%	2,011.5	µg/mL	+/-	69.9890
23	1,2-Dichloroethane	107-06-2	SHBQ0693	99%	2,008.7	µg/mL	+/-	69.8916
24	Benzene	71-43-2	MKCS3357	99%	2,017.4	µg/mL	+/-	70.2100
25	Trichloroethene	79-01-6	SHBN3720	99%	2,008.3	µg/mL	+/-	69.8786
26	1,2-Dichloropropane	78-87-5	BCBR0882V	99%	2,012.1	µg/mL	+/-	70.0117
27	Methyl methacrylate	80-62-6	MKCQ2756	99%	2,017.7	µg/mL	+/-	70.2204
28	Chloroacetonitrile	107-14-2	MKBG6249V	99%	2,006.0	µg/mL	+/-	69.3366
29	bromodichloromethane	75-27-4	MKCF8470	99%	2,012.6	µg/mL	+/-	70.0273
30	Dibromomethane	74-95-3	10233302	99%	2,014.7	µg/mL	+/-	70.1153
31	2-Nitropropane	79-46-9	BCCB9352	97%	2,015.9	µg/mL	+/-	70.1562
32	cis-1,3-Dichloropropene	10061-01-5	RD230406RSR	99%	2,005.0	µg/mL	+/-	69.7655
33	Toluene	108-88-3	MKCS9989	99%	2,019.0	µg/mL	+/-	70.2643
34	Ethyl methacrylate	97-63-2	MKCN6206	97%	2,015.4	µg/mL	+/-	70.1393
35	trans-1,3-Dichloropropene	10061-02-6	RD230727RSR	99%	2,011.3	µg/mL	+/-	69.9838
36	1,1,2-Trichloroethane	79-00-5	FGB01	99%	2,013.2	µg/mL	+/-	70.0491
37	1,3-Dichloropropane	142-28-9	BCCH5357	99%	2,017.1	µg/mL	+/-	70.2002
38	Tetrachloroethene	127-18-4	SHBQ0051	99%	2,011.5	µg/mL	+/-	69.9908
39	dibromochloromethane	124-48-1	MKCQ4517	99%	2,006.6	µg/mL	+/-	69.8185
40	1,2-Dibromoethane (EDB)	106-93-4	BCCH7113	99%	2,009.0	µg/mL	+/-	69.9176
41	Chlorobenzene	108-90-7	SHBN6640	99%	2,009.8	µg/mL	+/-	69.9299
42	1,1,1,2-Tetrachloroethane	630-20-6	GC01	99%	2,013.8	µg/mL	+/-	70.0833
43	Ethylbenzene	100-41-4	094632L21G	99%	2,006.8	µg/mL	+/-	69.8411
44	m-Xylene	108-38-3	SHBN6673	99%	2,018.7	µg/mL	+/-	70.2559
45	p-Xylene	106-42-3	SHBP5191	99%	2,008.0	µg/mL	+/-	69.8828
46	o-Xylene	95-47-6	SHBN5105	99%	2,016.3	µg/mL	+/-	70.1724
47	Styrene	100-42-5	MKCQ3390	99%	2,014.8	µg/mL	+/-	70.1209
48	Isopropylbenzene (cumene)	98-82-8	Z20D022	99%	2,011.4	µg/mL	+/-	70.0026
49	bromoform	75-25-2	050494L04R	99%	2,009.6	µg/mL	+/-	69.9255
50	1,1,2,2-Tetrachloroethane	79-34-5	OXACF	99%	2,011.7	µg/mL	+/-	69.9986
51	1,2,3-Trichloropropane	96-18-4	Q91-34	98%	2,013.8	µg/mL	+/-	70.0841
52	trans-1,4-dichloro-2-butene	110-57-6	RP231113CTH	94%	2,017.2	µg/mL	+/-	69.7251

53	n-Propylbenzene	103-65-1	095067T18C	99%	2,018.4	µg/mL	+/-	70.2434
54	Bromobenzene	108-86-1	MKCQ7174	99%	2,016.9	µg/mL	+/-	70.1919
55	1,3,5-Trimethylbenzene	108-67-8	BCCF4166	99%	2,017.0	µg/mL	+/-	70.1961
56	2-Chlorotoluene	95-49-8	235783M23T	99%	2,017.8	µg/mL	+/-	70.2253
57	4-Chlorotoluene	106-43-4	BCCG9286	99%	2,014.1	µg/mL	+/-	70.0958
58	tert-Butylbenzene	98-06-6	STBJ1937	99%	2,005.2	µg/mL	+/-	69.7868
59	1,2,4-Trimethylbenzene	95-63-6	MKCS3775	99%	2,015.9	µg/mL	+/-	70.1571
60	Pentachloroethane	76-01-7	13550700	97%	2,012.8	µg/mL	+/-	69.5699
61	sec-Butylbenzene	135-98-8	MKCP2266	99%	2,011.0	µg/mL	+/-	69.9872
62	p-Isopropyltoluene (p-Cymene)	99-87-6	MKCR6143	99%	2,014.6	µg/mL	+/-	70.1111
63	1,3-Dichlorobenzene	541-73-1	BCCD5315	99%	2,003.2	µg/mL	+/-	69.7020
64	1,4-Dichlorobenzene	106-46-7	MKBS7929V	99%	2,015.0	µg/mL	+/-	70.1108
65	n-Butylbenzene	104-51-8	09418JJ	99%	2,005.3	µg/mL	+/-	69.7882
66	1,2-Dichlorobenzene	95-50-1	SHBN3835	99%	2,009.0	µg/mL	+/-	69.9020
67	Hexachloroethane	67-72-1	QTORH	99%	2,016.0	µg/mL	+/-	69.6822
68	1,2-Dibromo-3-chloropropane	96-12-8	HBMVB	97%	2,005.1	µg/mL	+/-	69.7821
69	Nitrobenzene	98-95-3	10224044	99%	2,017.9	µg/mL	+/-	70.2256
70	1,2,4-Trichlorobenzene	120-82-1	SHBP5900	99%	2,015.0	µg/mL	+/-	70.1251
71	Hexachlorobutadiene	87-68-3	RP230823RSR	98%	2,001.7	µg/mL	+/-	69.6639
72	Naphthalene	91-20-3	STBL1057	99%	2,008.9	µg/mL	+/-	69.9149
73	1,2,3-Trichlorobenzene	87-61-6	MKBX7627V	99%	2,012.3	µg/mL	+/-	70.0318

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4 μ m
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant pressure 30 psi

Temp. Program:

40°C (hold 6 min.) to 240°C
@ 6°C/min. (hold 10 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

20.0 ml/min.

Inj. Vol

1 μ l

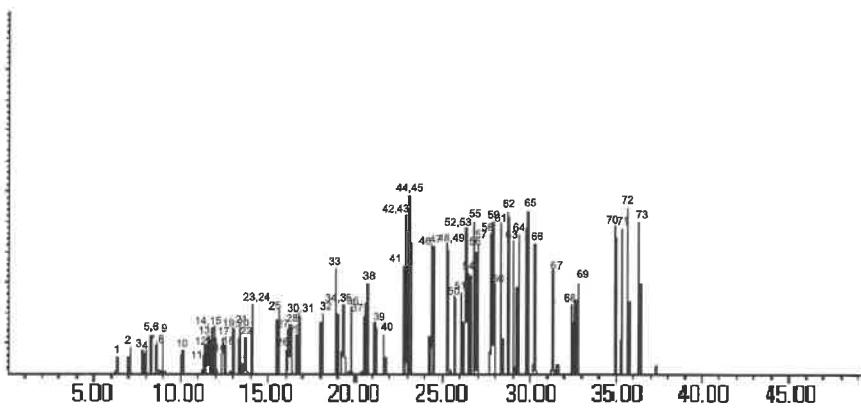

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

John Friedline - Operations Technician I

Date Mixed: 20-Nov-2023 Balance Serial #: 1128342314

Dillon Murphy - Operations Technician I

Date Passed: 29-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

Certificate of Analysis

chromatographic plus

V14697-to-14726



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006

Lot No.: A0210618

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 μ g/mL, P&T Methanol/Water(90:10),
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 μ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 μ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 μ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 μ g/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)

CAS # 67-56-1/7732-18-5

Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol


1 μ l

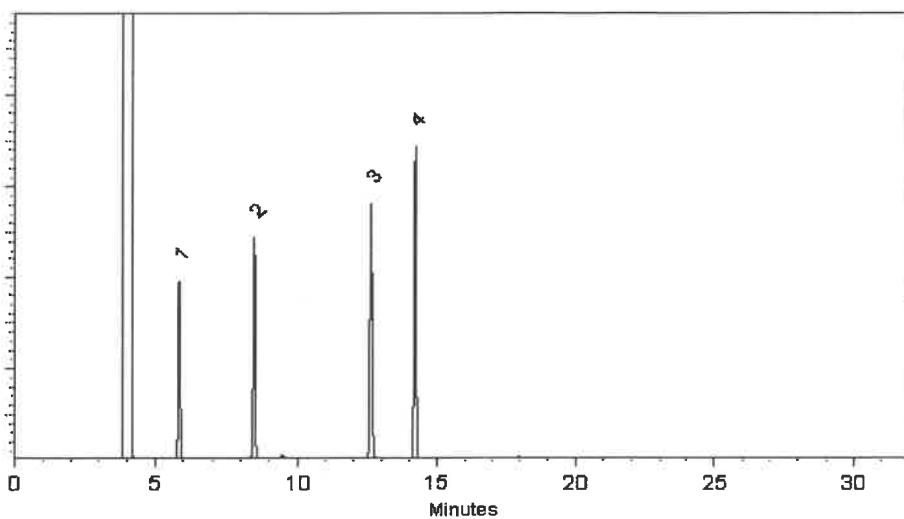

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024 Balance Serial #: B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rev 12/17/24
CERTIFIED REFERENCE MATERIAL
30 μL

Certificate of Analysis
chromatographic plus

*V14727 +
V14756*



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222-01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222-02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30042

Lot No.: A0216826

Description : 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000μg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : May 31, 2031

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 μg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 μg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 μg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 μg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 μg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 μg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4 μ m
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1 μ l

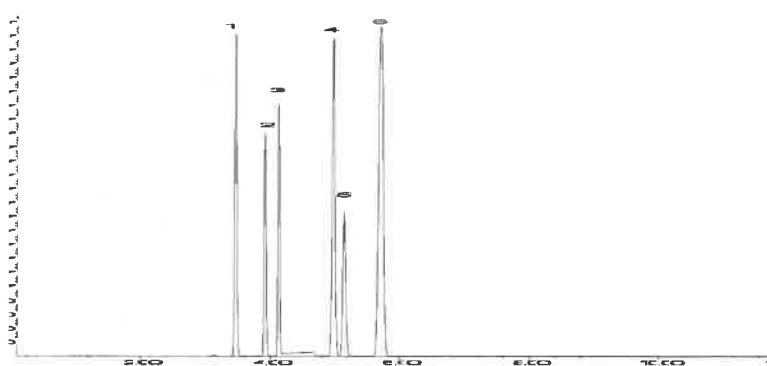

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL

Rec 01/16/25

5 vial



ILAC
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis

chromatographic

✓ 14837 to
J 14841

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 560065

Lot No.: A0220861

Description : Custom 524 Standard

Custom 524 Standard 2,000-10,000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2026

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,1,2-Trichlorotrifluoroethane (CFC-113)	76-13-1	00022779	99%	2,009.0 μ g/mL	+/- 69.4402
2	tert-Butanol (TBA)	75-65-0	SHBR5545	99%	10,036.0 μ g/mL	+/- 346.8674
3	Acrylonitrile	107-13-1	102466R02E	99%	2,015.0 μ g/mL	+/- 69.6476
4	Propionitrile	107-12-0	BCCL0691	99%	8,074.0 μ g/mL	+/- 279.0744
5	Tetrahydrofuran	109-99-9	SHBR7392	99%	2,009.0 μ g/mL	+/- 69.4402
6	Cyclohexane	110-82-7	SHBS0091	99%	2,014.0 μ g/mL	+/- 69.6131
7	Methylcyclohexane	108-87-2	SHBR3777	99%	2,015.0 μ g/mL	+/- 69.6476
8	Methyl methacrylate	80-62-6	MKCQ2756	99%	2,011.0 μ g/mL	+/- 69.5094
9	trans-1,4-dichloro-2-butene	110-57-6	RD240719ECSB	97%	2,013.7 μ g/mL	+/- 69.6034
10	Nitrobenzene	98-95-3	10224044	99%	8,026.0 μ g/mL	+/- 277.4153

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Quality Confirmation Test

Column:
60m x 0.25mm x 1.4 μ m
Rtx-502.2 (cat.#10916)

Carrier Gas:
helium-constant pressure 30 psi

Temp. Program:
40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)


Inj. Temp:
200°C

Det. Temp:
250°C

Det. Type:
MSD

Split Vent:
25.0 ml/min.


Inj. Vol
1 μ l

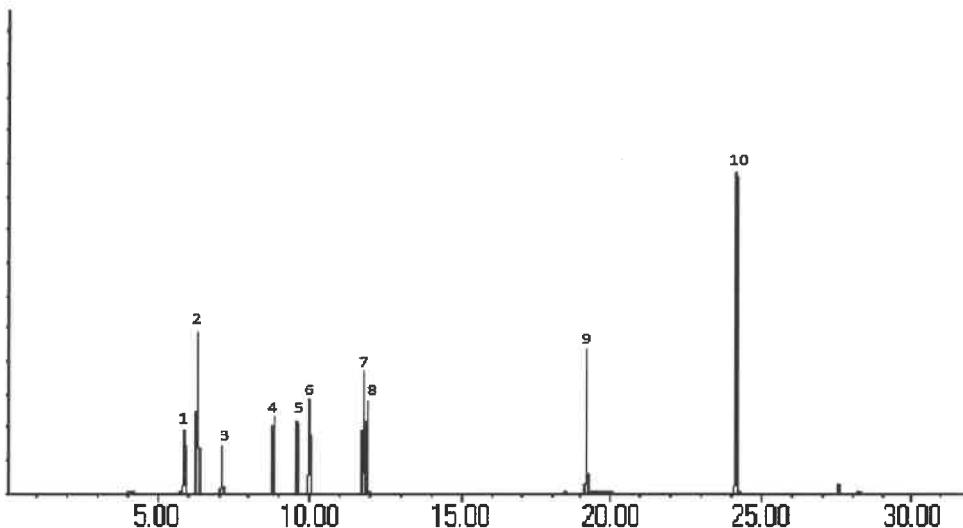

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Morgan Craighead - Mix Technician

Date Mixed: 07-Jan-2025 Balance Serial #: 1128342314


Dillon Murphy - Operations Technician |

Date Passed: 10-Jan-2025 

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis *chromatographic plus*

V15045 to V15049



ILAC
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30201

Lot No.: A0223883

Description: 524 Internal Std / Surrogate Mix

524 Internal Std/Surrogate Mix 2000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: March 31, 2032

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Fluorobenzene	462-06-6	BCBZ5549	99%	2,002.0 μ g/mL	+/- 112.4750
2	1-Bromo-4-fluorobenzene (BFB)	460-00-4	0000268853	99%	2,003.3 μ g/mL	+/- 112.5499
3	1,2-Dichlorobenzene-d4	2199-69-1	PR-32597	99%	2,006.0 μ g/mL	+/- 112.6997

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%



SHIPPING DOCUMENTS



A Phenomenex®
Company

22552

Packing List

Date	Order #
07/07/2025	333292

6390 Joyce Dr., #100
Golden, CO 80403

Tel: +1-303-940-0033
Fax: +1-303-940-0043
info@phenova.com
www.phenova.com

For terms and conditions of your order, please visit:
www.phenova.com/home/termsofsale

Ship To

Alliance Tech Group - Newark
ATTN: Sohil Jodhani
284 Sheffield St., #1
Mountainside, NJ 07092
USA



7/9/25 10:00

Customer PO #	Terms	PT Acct #	Customer #	Ship Via	F.O.B.
PO2-2553	Net 30	ZCM-100	1500470	FedEx Collect 2nd Day	Golden, CO

Qty Ordered	Qty Shipped	Qty Backorder	Part Number	Part Description	Study Number	Lot Number
1	1	0	PT-TM-WS	WS Trace Metals 1	WS0725	9101-04
1	1	0	PT-HG-WS	WS Trace Metals Mercury	WS0725	9101-05
1	1	0	PT-MIN-WS	WS Minerals Only	WS0725	9101-51
1	1	0	PT-TURB-WS	WS Turbidity	WS0725	9101-13
1	1	0	PT-SIO2-WS	WS Silica	WS0725	9101-17
1	1	0	PT-RVOA-WS	WS Regulated Volatiles	WS0725	9101-21
1	1	0	PT-UNRVOA-WS	WS Unregulated Volatiles	WS0725	9101-22
1	1	0	PT-THM-WS	WS Trihalomethanes	WS0725	9101-23
1	1	0	PT-EDBCP-WS	WS EDB/DBCP/TCP	WS0725	9101-27
1	1	0	PT-ADD-WS	WS Gasoline Additives	WS0725	9101-36

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488