


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071825\
Data File : VU063531.D
Acq On : 18 Jul 2025 08:07
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 17 03:49:40 2025

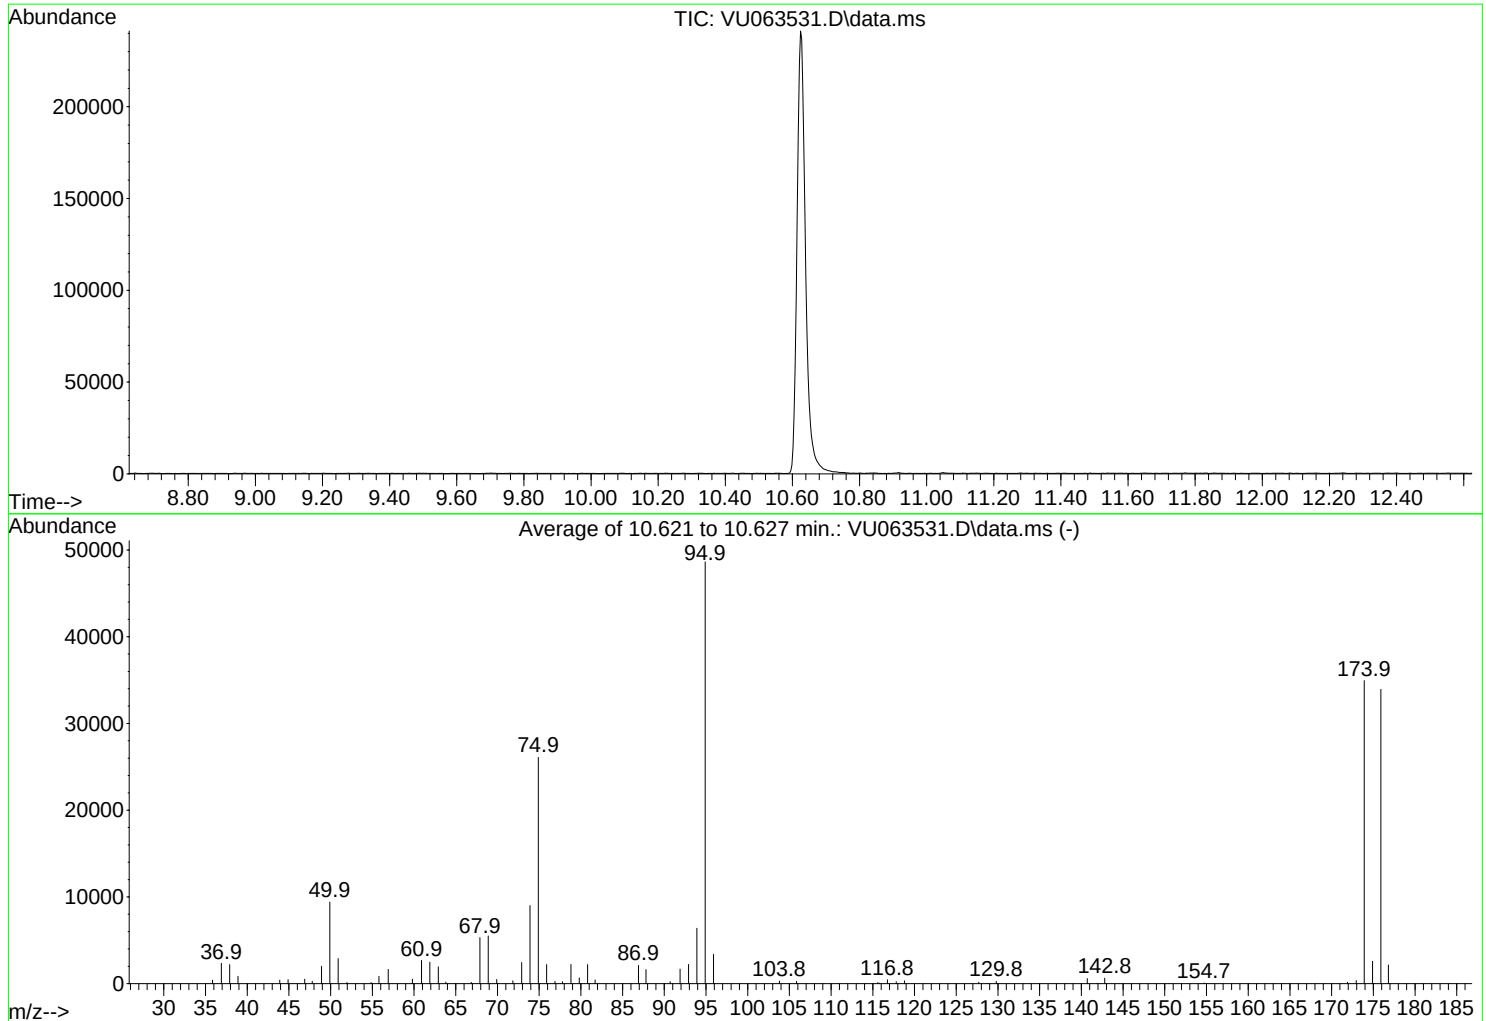

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	9408	PASS
75	95	30	60	53.6	26088	PASS
95	95	100	100	100.0	48635	PASS
96	95	5	9	7.0	3383	PASS
173	174	0.00	2	1.0	361	PASS
174	95	50	100	71.8	34936	PASS
175	174	5	9	7.4	2590	PASS
176	174	95	101	97.1	33925	PASS
177	176	5	9	6.4	2161	PASS