
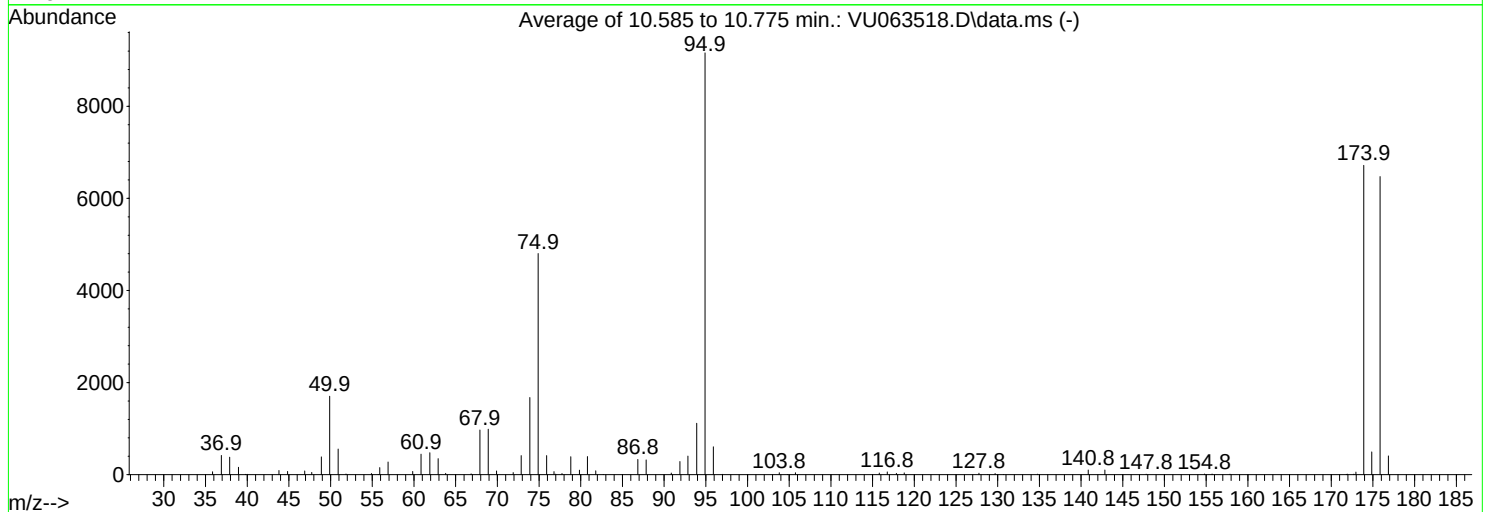


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071725\
Data File : VU063518.D
Acq On : 17 Jul 2025 08:10
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 17 03:49:40 2025

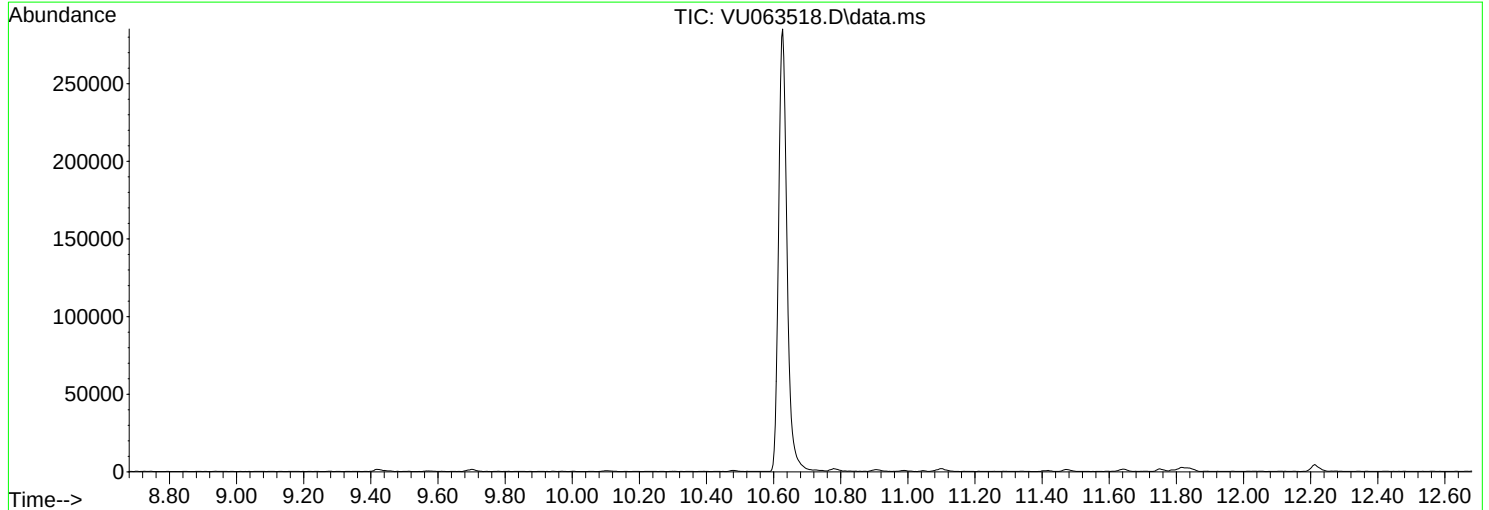

AutoFind: Averaged scan 2891 to 2950; Bkg corrected with scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	1703	PASS
75	95	30	60	52.4	4803	PASS
95	95	100	100	100.0	9161	PASS
96	95	5	9	6.6	606	PASS
173	174	0.00	2	0.8	56	PASS
174	95	50	100	73.3	6718	PASS
175	174	5	9	7.3	493	PASS
176	174	95	101	96.4	6474	PASS
177	176	5	9	6.3	405	PASS