


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072125\
Data File : VU063545.D
Acq On : 21 Jul 2025 08:14
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Jul 17 03:49:40 2025

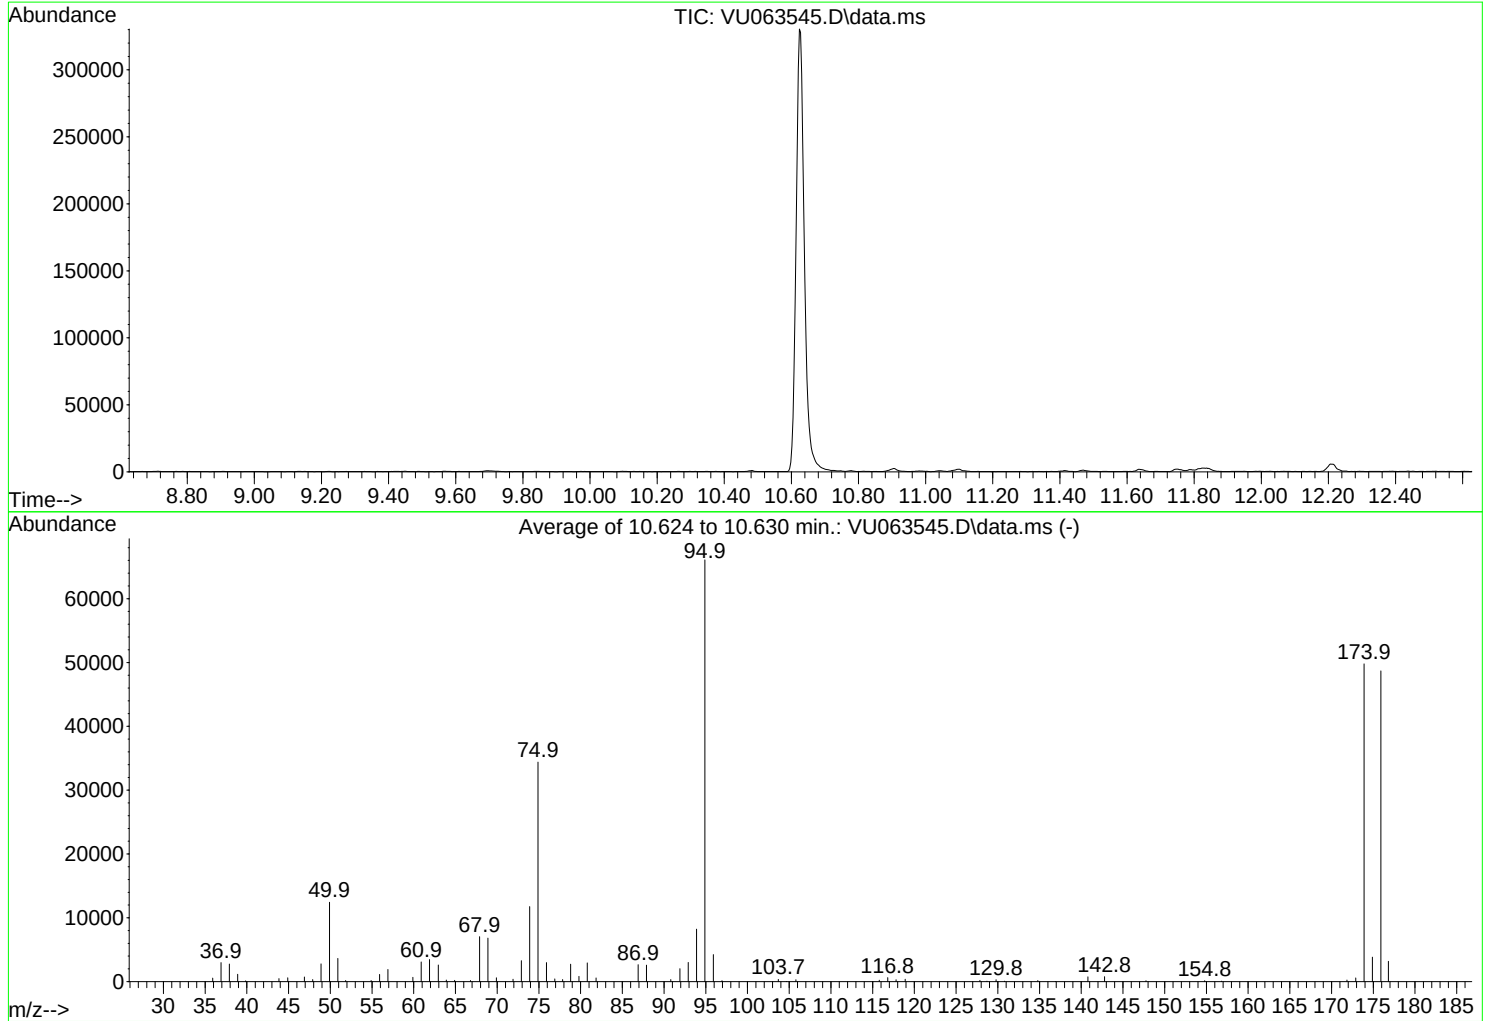

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	12431	PASS
75	95	30	60	52.1	34408	PASS
95	95	100	100	100.0	66088	PASS
96	95	5	9	6.4	4238	PASS
173	174	0.00	2	1.2	583	PASS
174	95	50	100	75.3	49781	PASS
175	174	5	9	7.7	3833	PASS
176	174	95	101	97.8	48677	PASS
177	176	5	9	6.6	3192	PASS