

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072125\
 Data File : VU063547.D
 Acq On : 21 Jul 2025 11:13
 Operator : MD/SY
 Sample : VU0721WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0721WBL01

Quant Time: Jul 22 04:07:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Jul 17 03:49:40 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.100	96	22148	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	6425	0.766	ug/l	0.00
Spiked Amount 1.000			Recovery	=	77.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	5521	0.712	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072125\
Data File : VU063547.D
Acq On : 21 Jul 2025 11:13
Operator : MD/SY
Sample : VU0721WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0721WBL01


Quant Time: Jul 22 04:07:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071625DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Jul 17 03:49:40 2025
Response via : Initial Calibration

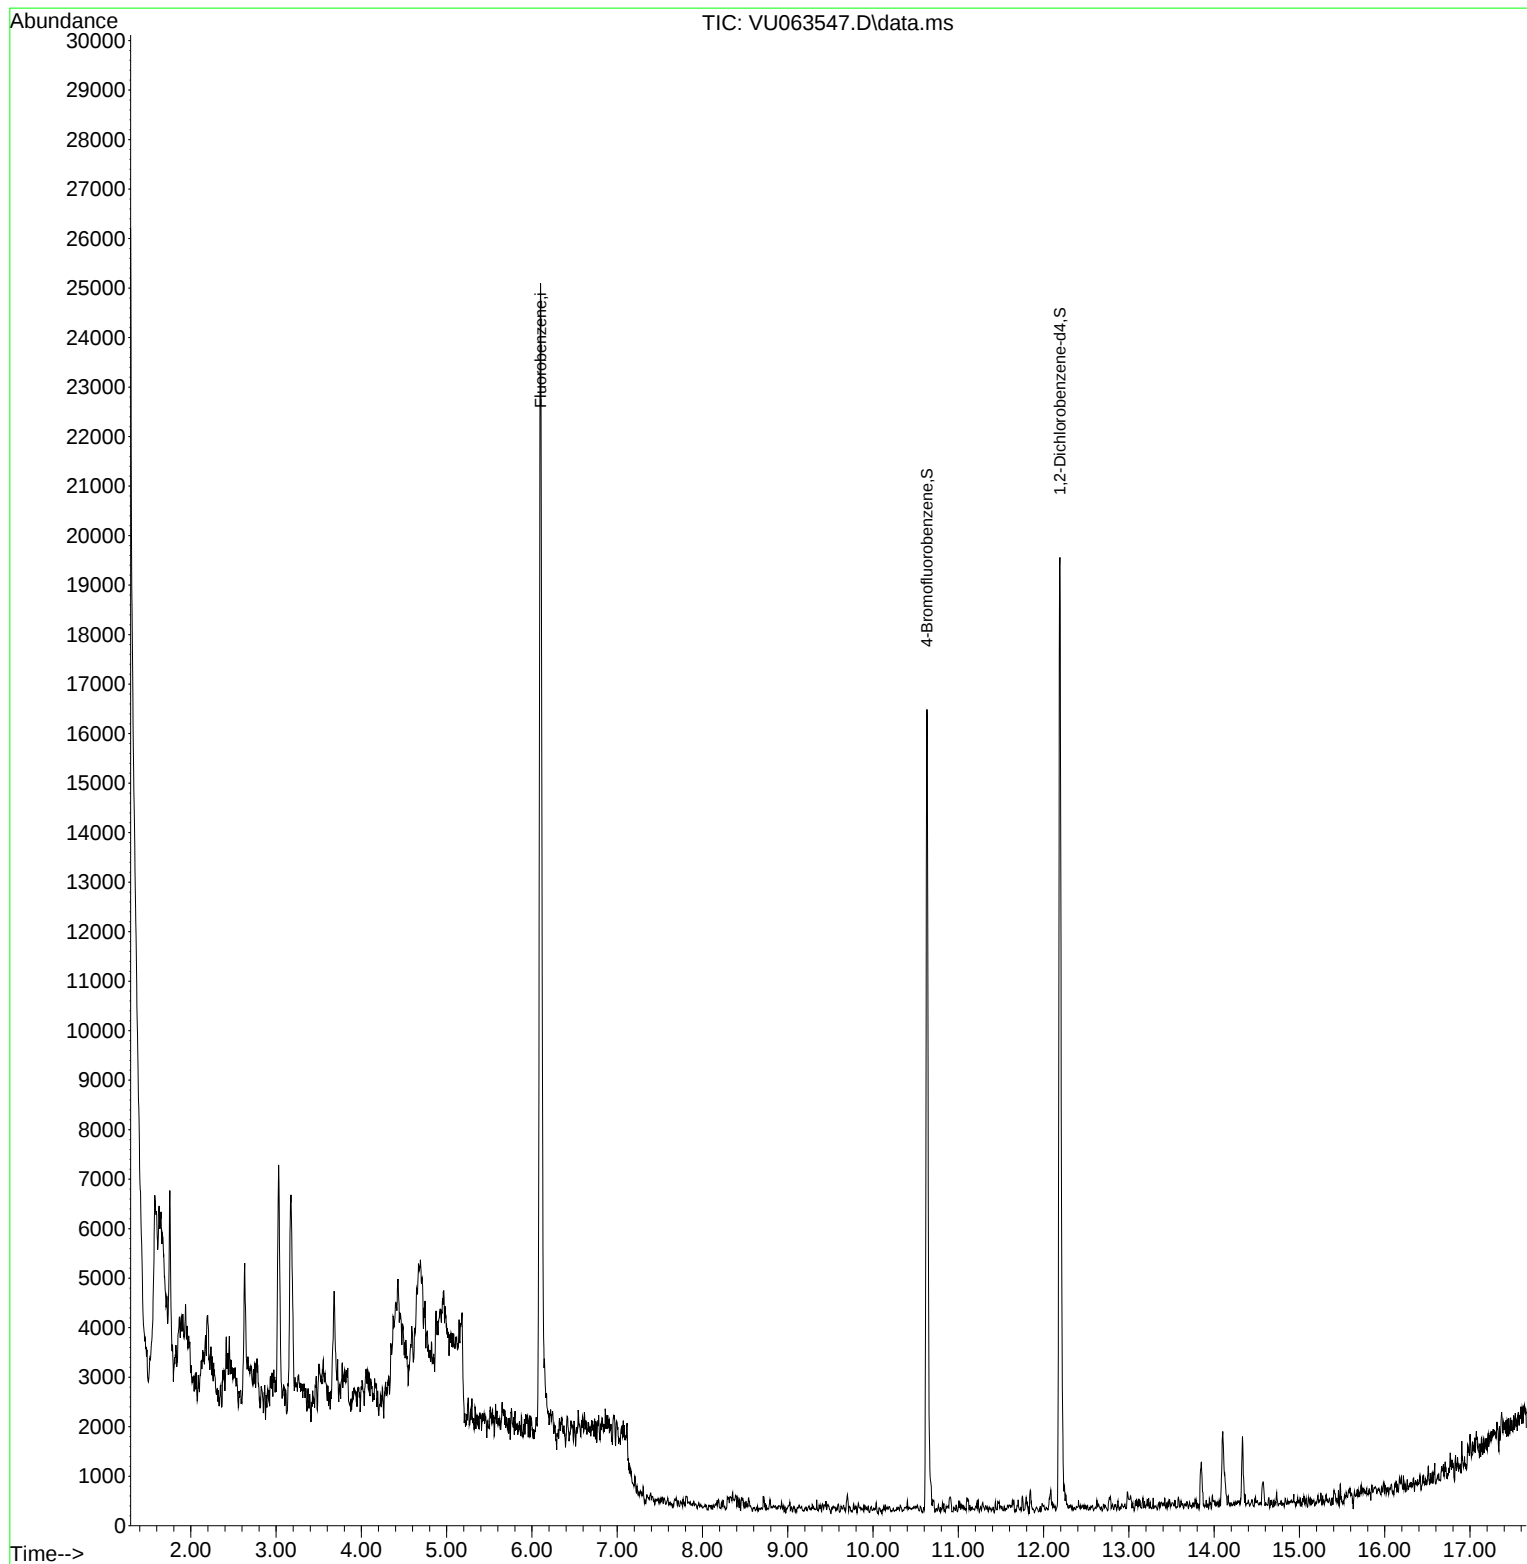



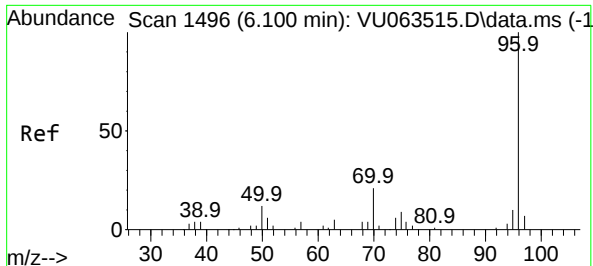


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.100 min Scan# 1496
Delta R.T. 0.000 min
Lab File: VU063547.D
Acq: 21 Jul 2025 11:13


Instrument :
MSVOA_U
ClientSampleId :
VU0721WBL01

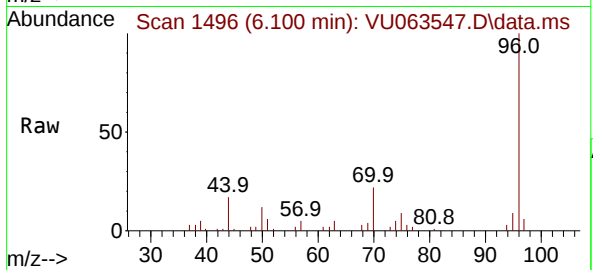



Tgt Ion:	96	Resp:	22148
Ion	Ratio	Lower	Upper
96	100		
70	19.4	15.0	22.4
95	9.0	7.4	11.0
97	6.1	0.0	0.0

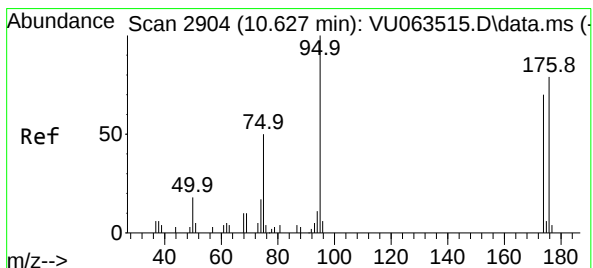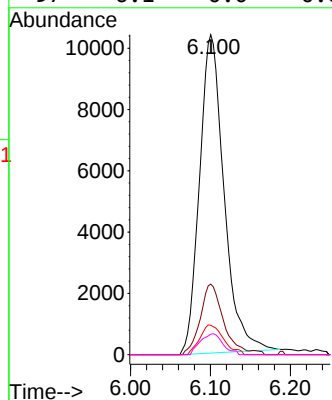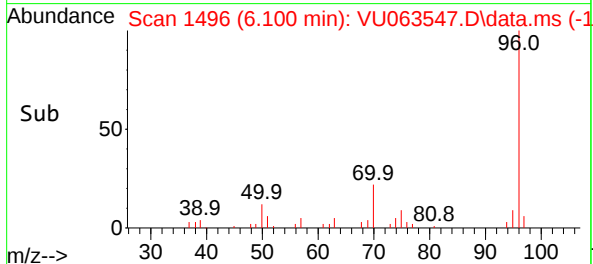


#57
4-Bromofluorobenzene
Concen: 0.766 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.003 min
Lab File: VU063547.D
Acq: 21 Jul 2025 11:13

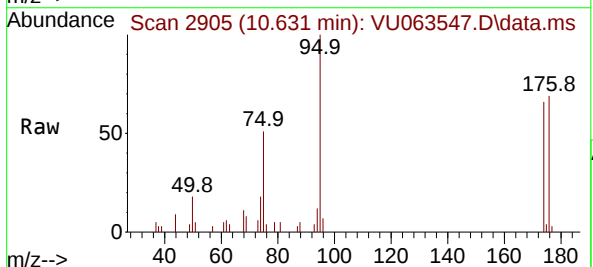

Tgt Ion:	95	Resp:	6425
Ion	Ratio	Lower	Upper
95	100		
174	68.9	59.8	89.8
176	72.3	61.8	92.8

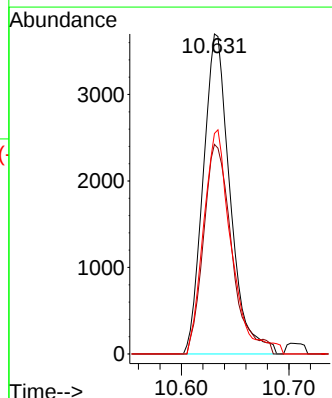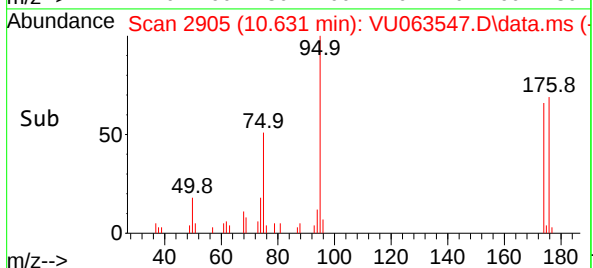

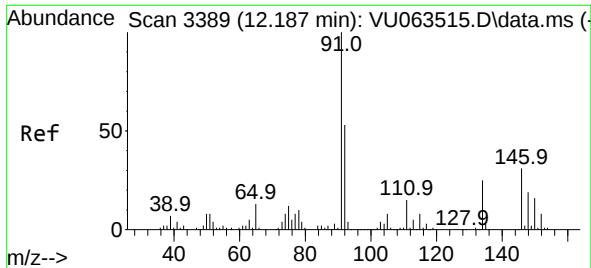

#68

1,2-Dichlorobenzene-d4

Concen: 0.712 ug/l

RT: 12.190 min Scan# 31

Delta R.T. 0.003 min

Lab File: VU063547.D


Acq: 21 Jul 2025 11:13

Instrument :

MSVOA_U

ClientSampleId :

VU0721WBL01

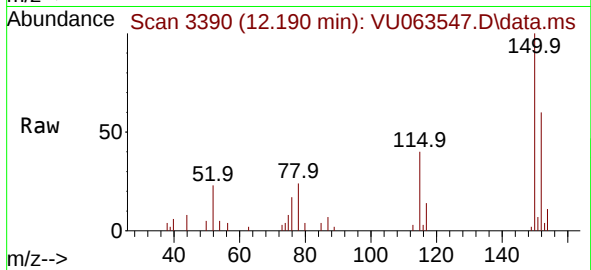

Tgt Ion:152 Resp: 5521

Ion Ratio Lower Upper

152 100

115 70.2 0.0 262.2

150 171.0 0.0 651.2

